

ATTACHMENT Q – DIPOLE VALIDATION

■ Validation Data (1900MHz Brain)

Dipole 1900 MHz

SAM II Phantom; Flat Section; Position: (90°,90°); Frequency: 1900 MHz

Probe: ET3DV6 - SN1609; ConvF(5.34,5.34,5.34); Crest factor: 1.0; Brain 1900 MHz: $s = 1.42$

mho/m $\epsilon_r = 39.6$ $\rho = 1.00$ g/cm³

Cubes (2): SAR (1g): 41.7 mW/g ± 0.01 dB, SAR (10g): 20.8 mW/g ± 0.02 dB

Coarse: Dx = 20.0, Dy = 20.0, Dz = 10.0

Powerdrift: 0.00 dB

Comment:


1900 MHz Brain Dipole Validation (D1900V2/ S.N: 5d032)

Antenna Input Power: 30 dBm (1 W)

HCT Co., Ltd. Brain Tissue Simulating Liquid

Liquid Temperature: 21.9°C

Date Tested : February 1, 2005

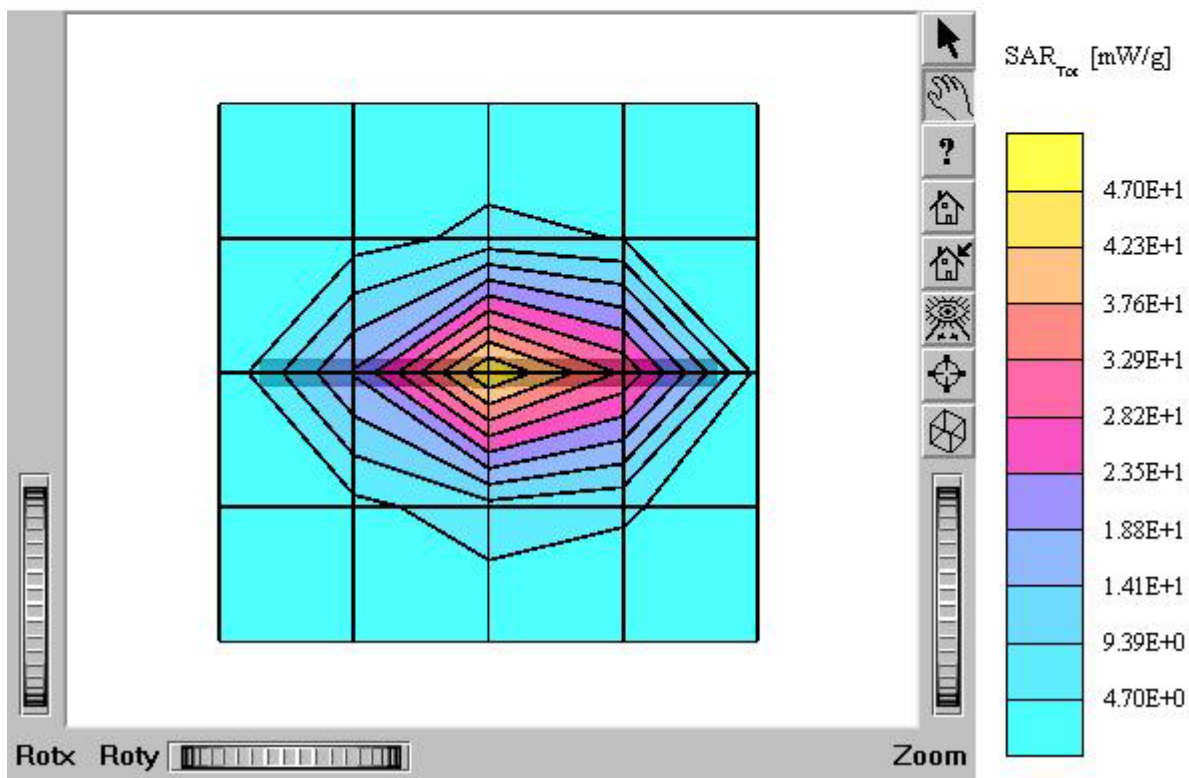

Dipole 1900 MHz

SAM II Phantom; Section; Position; ; Frequency: 1900 MHz

Probe: ET3DV6 - SN1609; ConvF(5.34,5.34,5.34); Crest factor: 1.0; Brain 1900 MHz: $s = 1.42$
 ρ_{ho}/m , $\epsilon_r = 39.6$, $r = 1.00$ g/cm³

:

Z-Axis: $D_x = 0.0$, $D_y = 0.0$, $D_z = 5.0$

Comment:


1900 MHz Brain Dipole Validation (D1900V2/ S.N: 5d032)

Antenna Input Power: 30 dBm (1 W)

HCT Co., Ltd. Brain Tissue Simulating Liquid

Liquid Temperature: 21.9°C

Date Tested : February 1, 2005

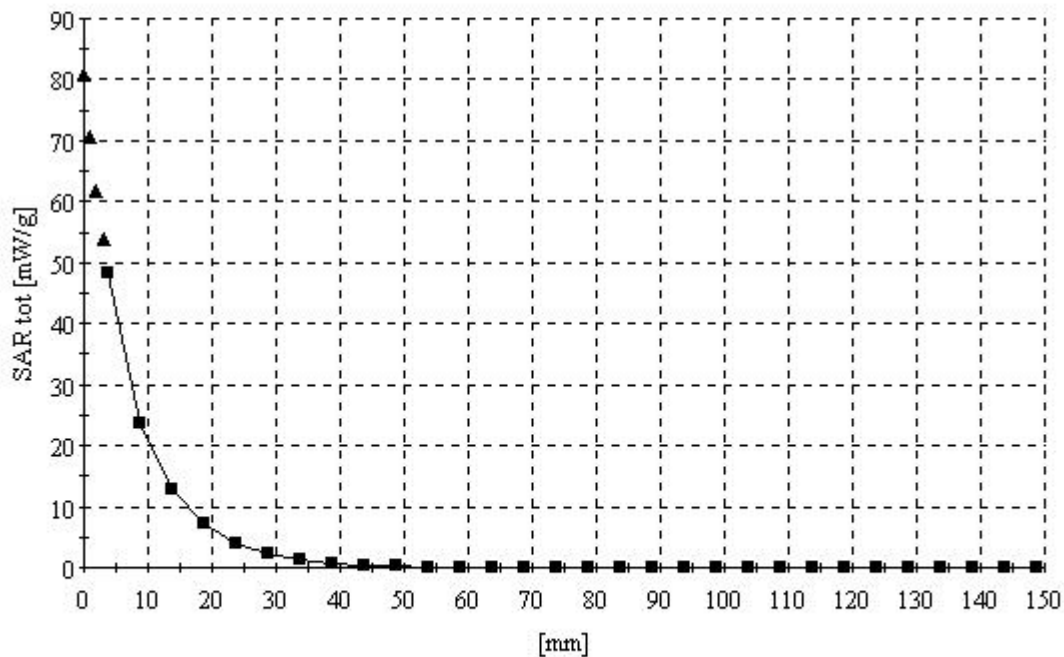

■ Dielectric Parameter (1900MHz Brain)**Title : TDG-320TME****SubTitle : GSM1900**

February 01, 2005 09:12 AM

Frequency	e'	e''
1.800000000 GHz	40.0488	12.9887
1.806666667 GHz	40.0164	13.0255
1.813333333 GHz	39.9434	13.0693
1.820000000 GHz	39.9255	13.1124
1.826666667 GHz	39.8978	13.1827
1.833333333 GHz	39.8908	13.2219
1.840000000 GHz	39.9134	13.2879
1.846666667 GHz	39.9240	13.3338
1.853333333 GHz	39.9301	13.3522
1.860000000 GHz	39.9501	13.3917
1.866666667 GHz	39.9060	13.4386
1.873333333 GHz	39.8997	13.4254
1.880000000 GHz	39.8606	13.4121
1.886666667 GHz	39.8083	13.4195
1.893333333 GHz	39.7429	13.4057
1.900000000 GHz	39.6368	13.4065
1.906666667 GHz	39.5816	13.3928
1.913333333 GHz	39.5009	13.4078
1.920000000 GHz	39.4199	13.3938
1.926666667 GHz	39.3719	13.4208
1.933333333 GHz	39.2690	13.4395
1.940000000 GHz	39.2560	13.5002
1.946666667 GHz	39.2047	13.5328
1.953333333 GHz	39.2096	13.6141
1.960000000 GHz	39.2130	13.6610

■ Dielectric Parameter (1900MHz Muscle)**Title : TDG-320TME****SubTitle : GSM1900 BODY**

February 01, 2005 02:03 PM

Frequency	e'	e''
1.800000000 GHz	51.3270	14.5885
1.810000000 GHz	51.2933	14.6305
1.820000000 GHz	51.2675	14.6838
1.830000000 GHz	51.2361	14.7491
1.840000000 GHz	51.2418	14.7798
1.850000000 GHz	51.2099	14.8351
1.860000000 GHz	51.1707	14.8754
1.870000000 GHz	51.1189	14.8985
1.880000000 GHz	51.0925	14.9036
1.890000000 GHz	51.0048	14.8770
1.900000000 GHz	50.9328	14.8873
1.910000000 GHz	50.8631	14.8821
1.920000000 GHz	50.8095	14.9095
1.930000000 GHz	50.7874	14.9307
1.940000000 GHz	50.7254	14.9806
1.950000000 GHz	50.6849	15.0364
1.960000000 GHz	50.6612	15.1129
1.970000000 GHz	50.6325	15.1342
1.980000000 GHz	50.6251	15.1929
1.990000000 GHz	50.6020	15.2167
2.000000000 GHz	50.5588	15.2204

ATTACHMENT S – DIPOLE CALIBRATION DATA

Calibration Laboratory of
Schmid & Partner
Engineering AG
Zeughausstrasse 43, 8004 Zurich, Switzerland

Client **H-CT (Dymstec)**

CALIBRATION CERTIFICATE

Object(s) D1900V2 - SN:5d032

Calibration procedure(s) QA CAL-05.v2
Calibration procedure for dipole validation kits

Calibration date: April 26, 2004

Condition of the calibrated item In Tolerance (according to the specific calibration document)


This calibration statement documents traceability of M&TE used in the calibration procedures and conformity of the procedures with the ISO/IEC 17025 international standard.

All calibrations have been conducted in the closed laboratory facility: environment temperature 22 +/- 2 degrees Celsius and humidity < 75%.

Calibration Equipment used (M&TE critical for calibration)

Model Type	ID #	Cal Date (Calibrated by, Certificate No.)	Scheduled Calibration
Power meter EPM E442	GB37480704	6-Nov-03 (METAS, No. 252-0254)	Nov-04
Power sensor HP 8481A	US37292783	6-Nov-03 (METAS, No. 252-0254)	Nov-04
Power sensor HP 8481A	MY41092317	18-Oct-02 (Agilent, No. 20021018)	Oct-04
RF generator R&S SML-03	100698	27-Mar-2002 (R&S, No. 20-92389)	In house check: Mar-05
Network Analyzer HP 8753E	US37390585	18-Oct-01 (SPEAG, in house check Nov-03)	In house check: Oct 05

Calibrated by: Name Function Signature
Judith Mueller Technician 

Approved by: Katja Pokovic Laboratory Director 

Date issued: April 27, 2004

This calibration certificate is issued as an intermediate solution until the accreditation process (based on ISO/IEC 17025 International Standard) for Calibration Laboratory of Schmid & Partner Engineering AG is completed.

Schmid & Partner Engineering AG

s p e a gZeughausstrasse 43, 8004 Zurich, Switzerland
Phone +41 1 245 9700, Fax +41 1 245 9779
info@speag.com, <http://www.speag.com>

DASY

Dipole Validation Kit

Type: D1900V2

Serial: 5d032

Manufactured: March 17, 2003
Calibrated: April 26, 2004

1. Measurement Conditions

The measurements were performed in the flat section of the SAM twin phantom filled with **head simulating solution** of the following electrical parameters at 1900 MHz:

Relative Dielectricity	40.1	$\pm 5\%$
Conductivity	1.45 mho/m	$\pm 5\%$

The DASY4 System with a dosimetric E-field probe ET3DV6 (SN:1507, Conversion factor 4.96 at 1900 MHz) was used for the measurements.

The dipole was mounted on the small tripod so that the dipole feedpoint was positioned below the center marking of the flat phantom section and the dipole was oriented parallel to the body axis (the long side of the phantom). The standard measuring distance was 10mm from dipole center to the solution surface. The included distance spacer was used during measurements for accurate distance positioning.

The coarse grid with a grid spacing of 15mm was aligned with the dipole. The 7x7x7 fine cube was chosen for cube integration.

The dipole input power (forward power) was 250 mW $\pm 3\%$. The results are normalized to 1W input power.

2. SAR Measurement with DASY4 System

Standard SAR-measurements were performed according to the measurement conditions described in section 1. The results (see figure supplied) have been normalized to a dipole input power of 1W (forward power). The resulting averaged SAR-values measured with the dosimetric probe ET3DV6 SN:1507 and applying the advanced extrapolation are:

averaged over 1 cm ³ (1 g) of tissue:	40.0 mW/g $\pm 16.8\%$ (k=2)¹
averaged over 10 cm ³ (10 g) of tissue:	21.0 mW/g $\pm 16.2\%$ (k=2)¹

¹ validation uncertainty

3. Dipole Impedance and Return Loss

The impedance was measured at the SMA-connector with a network analyzer and numerically transformed to the dipole feedpoint. The transformation parameters from the SMA-connector to the dipole feedpoint are:

Electrical delay:	1.192 ns	(one direction)
Transmission factor:	0.999	(voltage transmission, one direction)

The dipole was positioned at the flat phantom sections according to section 1 and the distance spacer was in place during impedance measurements.

Feedpoint impedance at 1900 MHz:	$\text{Re}\{Z\} = $ 49.8 Ω
	$\text{Im}\{Z\} = $ 3.4 Ω
Return Loss at 1900 MHz	-29.5 dB

4. Handling

Do not apply excessive force to the dipole arms, because they might bend. Bending of the dipole arms stresses the soldered connections near the feedpoint leading to a damage of the dipole.

5. Design

The dipole is made of standard semirigid coaxial cable. The center conductor of the feeding line is directly connected to the second arm of the dipole. The antenna is therefore short-circuited for DC-signals.

Small end caps have been added to the dipole arms in order to improve matching when loaded according to the position as explained in Section 1. The SAR data are not affected by this change. The overall dipole length is still according to the Standard.

6. Power Test

After long term use with 40W radiated power, only a slight warming of the dipole near the feedpoint can be measured.

Test Laboratory: SPEAG, Zurich, Switzerland

DUT: Dipole 1900 MHz; Type: D1900V2; Serial: D1900V2 - SN5d032

Communication System: CW-1900; Frequency: 1900 MHz; Duty Cycle: 1:1

Medium: HSL 1900 MHz;

Medium parameters used: $f = 1900$ MHz; $\sigma = 1.45$ mho/m; $\epsilon_r = 40.1$; $\rho = 1000$ kg/m³

Phantom section: Flat Section

Measurement Standard: DASY4 (High Precision Assessment)

DASY4 Configuration:

- Probe: ET3DV6 - SN1507; ConvF(4.96, 4.96, 4.96); Calibrated: 1/23/2004
- Sensor-Surface: 4mm (Mechanical Surface Detection)
- Electronics: DAE3 Sn411; Calibrated: 11/6/2003
- Phantom: SAM with CRP - TP1006; Type: SAM 4.0; Serial: TP:1006;
- Measurement SW: DASY4, V4.2 Build 44; Postprocessing SW: SEMCAD, V1.8 Build 112

Pin = 250 mW; d = 10 mm/Area Scan (81x81x1): Measurement grid: dx=15mm, dy=15mm

Reference Value = 92 V/m; Power Drift = 0.0 dB

Maximum value of SAR (interpolated) = 11.4 mW/g


Pin = 250 mW; d = 10 mm/Zoom Scan (7x7x7)/Cube 0: Measurement grid: dx=5mm, dy=5mm, dz=5mm

Reference Value = 92 V/m; Power Drift = 0.0 dB

Maximum value of SAR (measured) = 11.2 mW/g

Peak SAR (extrapolated) = 17.8 W/kg

SAR(1 g) = 10 mW/g; SAR(10 g) = 5.25 mW/g

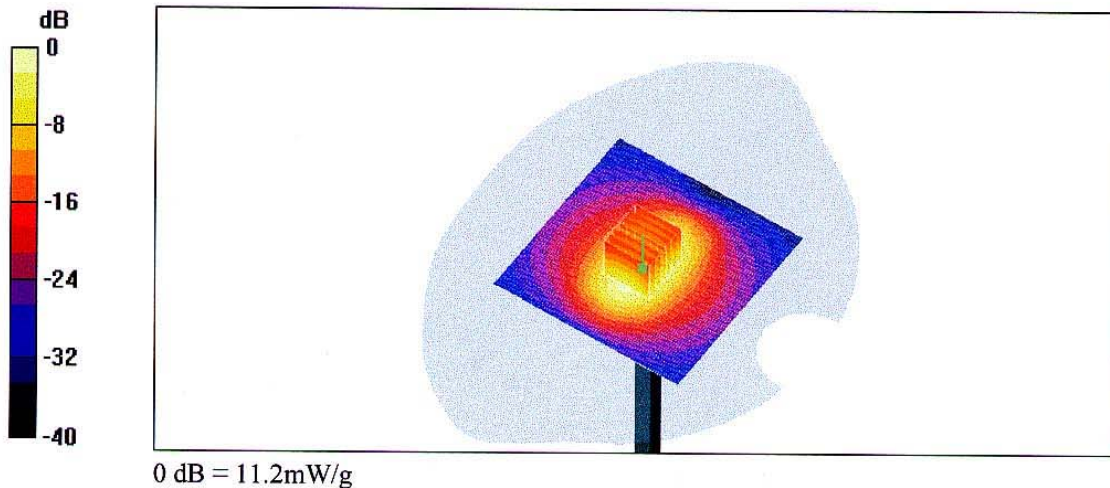

5d032

