

Test Laboratory: Compliance Certification Services
 File Name: [D2450V2SN706_Probe 1577_082903.da4](#)

DUT: Dipole 2450 MHz; Type: D2450V2; Serial: D2450V2 - SN:706
Program: System Performance Check at 2450 MHz
Ambient Temperature: 24.5 deg C; Liquid Temperature: 23.0 deg C


Communication System: CW - 2450 MHz; Frequency: 2450 MHz; Duty Cycle: 1:1
 Medium: Head 2450 MHz ($\sigma = 1.8877$ mho/m, $\epsilon_r = 39.5663$, $\rho = 1000$ kg/m³)
 Phantom section: Flat Section

DASY4 Configuration:

- Probe: ET3DV6 - SN1577; ConvF(5.1, 5.1, 5.1); Calibrated: 2/7/2003
- Sensor-Surface: 4mm (Mechanical Surface Detection)
- Electronics: DAE3 Sn427; Calibrated: 2/4/2003
- Phantom: SAM 1; Type: SAM 1; Serial: 1185
- Measurement SW: DASY4, V4.1 Build 47; Postprocessing SW: SEMCAD, V1.6 Build 115

d=10mm, Pin=250mW/Area Scan (61x61x1): Measurement grid: dx=15mm, dy=15mm
 Reference Value = 93.6 V/m
 Power Drift = 0.04 dB
 Maximum value of SAR = 14.9 mW/g

d=10mm, Pin=250mW/Zoom Scan (5x5x7)/Cube 0: Measurement grid: dx=7.5mm, dy=7.5mm, dz=5mm
 Peak SAR (extrapolated) = 27.8 W/kg
SAR(1 g) = 13.3 mW/g; SAR(10 g) = 6.06 mW/g
 Reference Value = 93.6 V/m
 Power Drift = 0.04 dB
 Maximum value of SAR = 14.8 mW/g

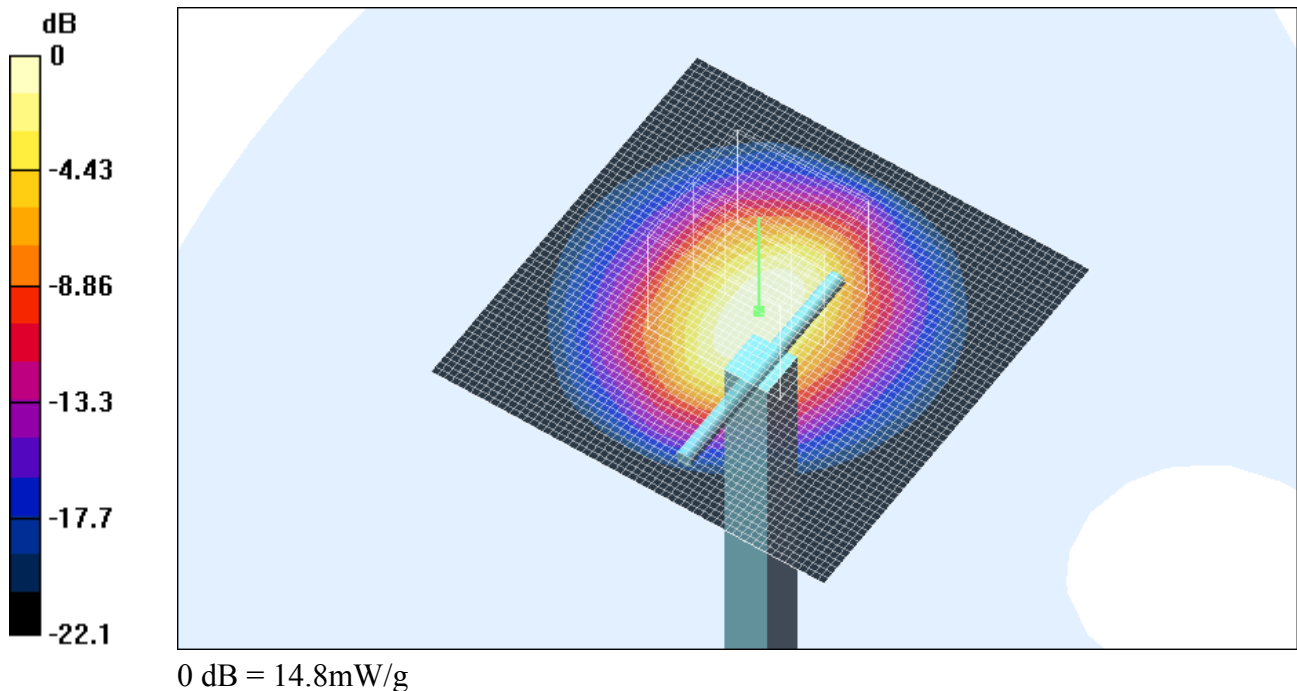

Test Laboratory: Compliance Certification Services
 File Name: [D2450V2SN706_Probe 1577_082903.da4](#)

DUT: Dipole 2450 MHz; Type: D2450V2; Serial: D2450V2 - SN:706
Program: System Performance Check at 2450 MHz

Communication System: CW - 2450 MHz; Frequency: 2450 MHz; Duty Cycle: 1:1

Medium: Head 2450 MHz ($\sigma = 1.8877$ mho/m, $\epsilon_r = 39.5663$, $\rho = 1000$ kg/m³)

Phantom section: Flat Section

DASY4 Configuration:


- Probe: ET3DV6 - SN1577; ConvF(5.1, 5.1, 5.1); Calibrated: 2/7/2003
- Sensor-Surface: 0mm (Fix Surface)
- Electronics: DAE3 Sn427; Calibrated: 2/4/2003
- Phantom: SAM 1; Type: SAM 1; Serial: 1185
- Measurement SW: DASY4, V4.1 Build 47; Postprocessing SW: SEMCAD, V1.6 Build 115

d=10mm, Pin=250mW/Z Scan (1x1x51): Measurement grid: dx=20mm, dy=20mm, dz=2mm

Reference Value = 93.6 V/m

Power Drift = 0.03 dB

Maximum value of SAR = 16.8 mW/g

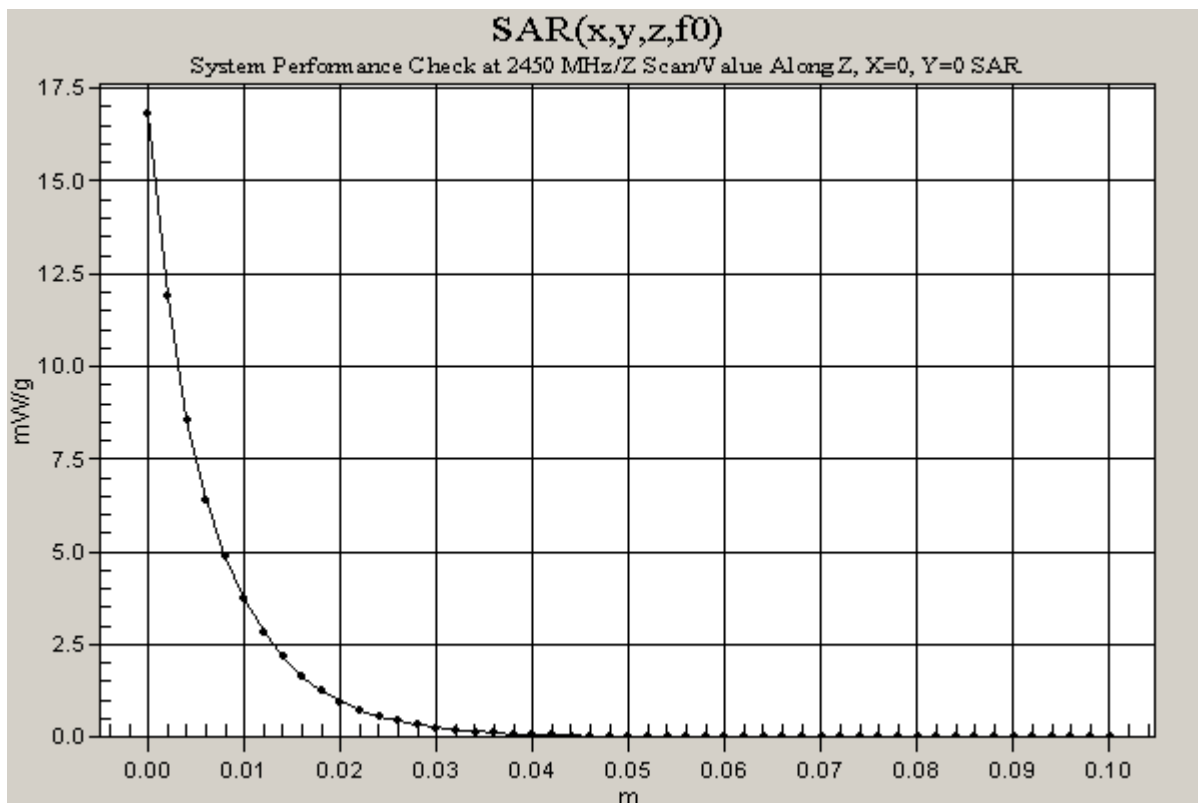

Test Laboratory: Compliance Certification Services
 File Name: [D2450V2SN706_Probe 1577_083103.da4](#)

DUT: Dipole 2450 MHz; Type: D2450V2; Serial: D2450V2 - SN:706
Program: System Performance Check at 2450 MHz
Ambient Temperature: 24.5 deg C; Liquid Temperature: 23.0 deg C


Communication System: CW - 2450 MHz; Frequency: 2450 MHz; Duty Cycle: 1:1
 Medium: Head 2450 MHz ($\sigma = 1.885$ mho/m, $\epsilon_r = 39.3783$, $\rho = 1000$ kg/m³)
 Phantom section: Flat Section

DASY4 Configuration:

- Probe: ET3DV6 - SN1577; ConvF(5.1, 5.1, 5.1); Calibrated: 2/7/2003
- Sensor-Surface: 4mm (Mechanical Surface Detection)
- Electronics: DAE3 Sn427; Calibrated: 2/4/2003
- Phantom: SAM 1; Type: SAM 1; Serial: 1185
- Measurement SW: DASY4, V4.1 Build 47; Postprocessing SW: SEMCAD, V1.6 Build 115

d=10mm, Pin=250mW/Area Scan (61x61x1): Measurement grid: dx=15mm, dy=15mm
 Reference Value = 92.9 V/m
 Power Drift = 0.04 dB
 Maximum value of SAR = 14.8 mW/g

d=10mm, Pin=250mW/Zoom Scan (5x5x7)/Cube 0: Measurement grid: dx=7.5mm, dy=7.5mm, dz=5mm
 Peak SAR (extrapolated) = 27.7 W/kg
[SAR\(1 g\) = 13.3 mW/g](#); SAR(10 g) = 6.05 mW/g
 Reference Value = 92.9 V/m
 Power Drift = 0.04 dB
 Maximum value of SAR = 14.7 mW/g

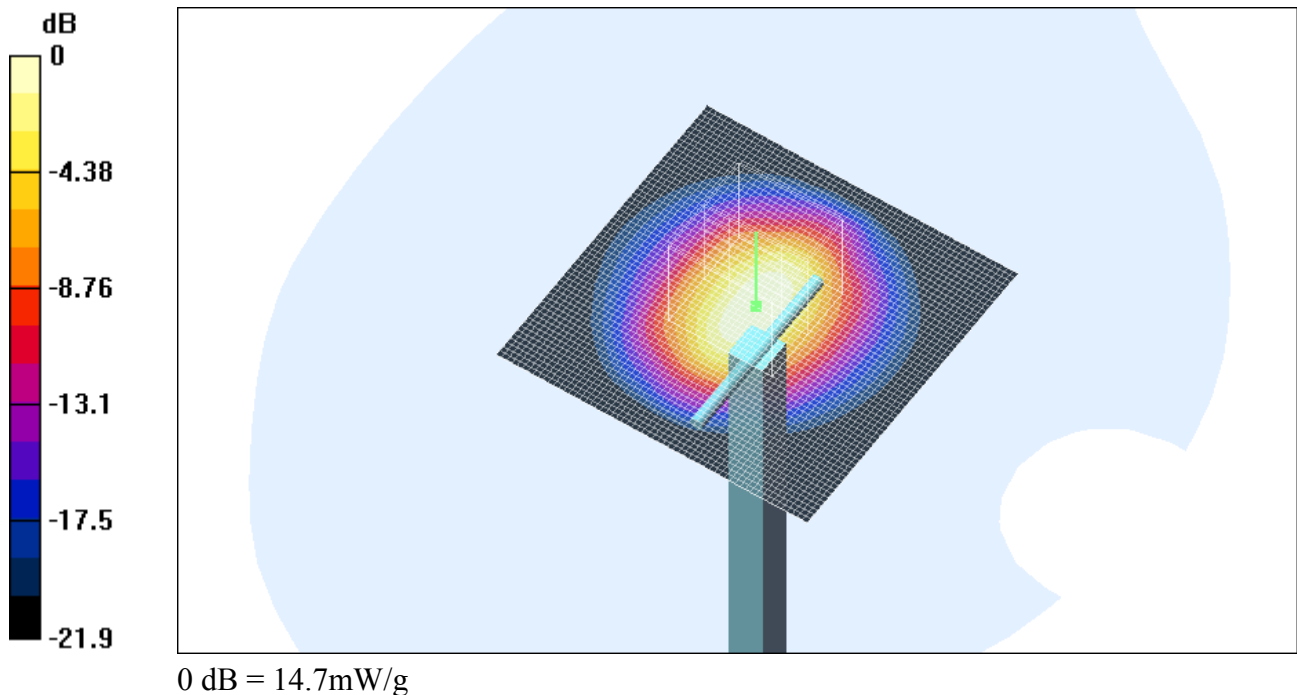

Test Laboratory: Compliance Certification Services
 File Name: [D2450V2SN706_Probe 1577_083103.da4](#)

DUT: Dipole 2450 MHz; Type: D2450V2; Serial: D2450V2 - SN:706
Program: System Performance Check at 2450 MHz

Communication System: CW - 2450 MHz; Frequency: 2450 MHz; Duty Cycle: 1:1

Medium: Head 2450 MHz ($\sigma = 1.885$ mho/m, $\epsilon_r = 39.3783$, $\rho = 1000$ kg/m³)

Phantom section: Flat Section

DASY4 Configuration:


- Probe: ET3DV6 - SN1577; ConvF(5.1, 5.1, 5.1); Calibrated: 2/7/2003
- Sensor-Surface: 0mm (Fix Surface)
- Electronics: DAE3 Sn427; Calibrated: 2/4/2003
- Phantom: SAM 1; Type: SAM 1; Serial: 1185
- Measurement SW: DASY4, V4.1 Build 47; Postprocessing SW: SEMCAD, V1.6 Build 115

d=10mm, Pin=250mW/Z Scan (1x1x51): Measurement grid: dx=20mm, dy=20mm, dz=2mm

Reference Value = 92.9 V/m

Power Drift = 0.03 dB

Maximum value of SAR = 17 mW/g

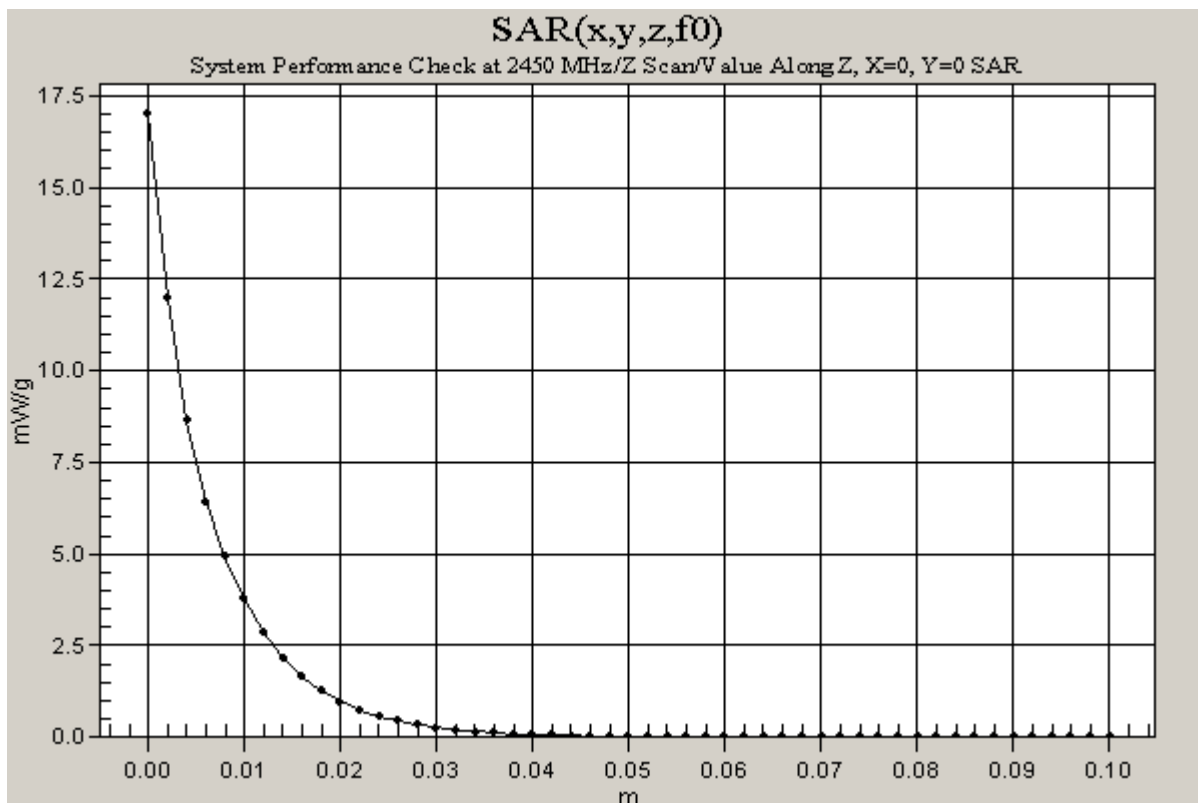

Test Laboratory: Compliance Certification Services
 File Name: [D2450V2SN706_Probe 1577_091903.da4](#)

DUT: Dipole 2450 MHz; Type: D2450V2; Serial: D2450V2 - SN:706
Program: System Performance Check at 2450 MHz
Ambient Temperature: 24.5 deg C; Liquid Temperature: 23.0 deg C


Communication System: CW - 2450 MHz; Frequency: 2450 MHz; Duty Cycle: 1:1
 Medium: Head 2450 MHz ($\sigma = 1.8864$ mho/m, $\epsilon_r = 39.4907$, $\rho = 1000$ kg/m³)
 Phantom section: Flat Section

DASY4 Configuration:

- Probe: ET3DV6 - SN1577; ConvF(5.1, 5.1, 5.1); Calibrated: 2/7/2003
- Sensor-Surface: 4mm (Mechanical Surface Detection)
- Electronics: DAE3 Sn427; Calibrated: 2/4/2003
- Phantom: SAM 1; Type: SAM 1; Serial: 1185
- Measurement SW: DASY4, V4.1 Build 47; Postprocessing SW: SEMCAD, V1.6 Build 115

d=10mm, Pin=250mW/Area Scan (61x61x1): Measurement grid: dx=15mm, dy=15mm
 Reference Value = 93.1 V/m
 Power Drift = -0.02 dB
 Maximum value of SAR = 14.4 mW/g

d=10mm, Pin=250mW/Zoom Scan (5x5x7)/Cube 0: Measurement grid: dx=7.5mm, dy=7.5mm, dz=5mm
 Peak SAR (extrapolated) = 27.3 W/kg
SAR(1 g) = 13.1 mW/g; SAR(10 g) = 5.93 mW/g
 Reference Value = 93.1 V/m
 Power Drift = -0.02 dB
 Maximum value of SAR = 14.6 mW/g

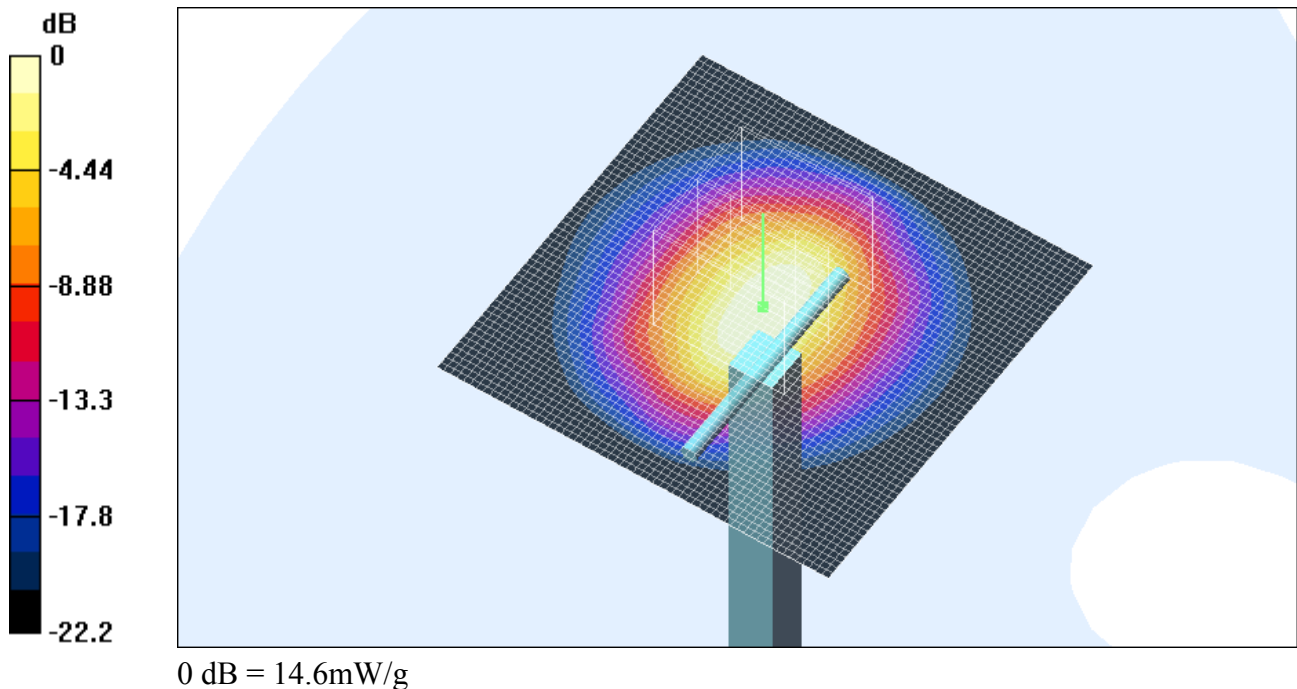

Test Laboratory: Compliance Certification Services
 File Name: [D2450V2SN706_Probe 1577_091903.da4](#)

DUT: Dipole 2450 MHz; Type: D2450V2; Serial: D2450V2 - SN:706
Program: System Performance Check at 2450 MHz

Communication System: CW - 2450 MHz; Frequency: 2450 MHz; Duty Cycle: 1:1

Medium: Head 2450 MHz ($\sigma = 1.8864$ mho/m, $\epsilon_r = 39.4907$, $\rho = 1000$ kg/m³)

Phantom section: Flat Section

DASY4 Configuration:

- Probe: ET3DV6 - SN1577; ConvF(5.1, 5.1, 5.1); Calibrated: 2/7/2003
- Sensor-Surface: 0mm (Fix Surface)
- Electronics: DAE3 Sn427; Calibrated: 2/4/2003
- Phantom: SAM 1; Type: SAM 1; Serial: 1185
- Measurement SW: DASY4, V4.1 Build 47; Postprocessing SW: SEMCAD, V1.6 Build 115

d=10mm, Pin=250mW/Z Scan (1x1x51): Measurement grid: dx=20mm, dy=20mm, dz=2mm

Reference Value = 93.1 V/m

Power Drift = -0.03 dB

Maximum value of SAR = 16.5 mW/g

