

Appendix B – System Check Plots

Test Date : 2025-02-19 | Ambient Temp : 22.1 °C | Tissue Temp : 21.7 °C

System Performance Check**System Performance Check at 2450 MHz****Verification Source Properties**

Manufacturer	Model No.	Serial No.	Input Power [dBm]
SPEAG	D2450V2	1087	17.0

Exposure Conditions

Phantom Section	Group	Frequency [MHz]	Conversion Factor	TSL Conductivity [S/m]	TSL Permittivity
Flat	CW	2450.000	7.25	1.87	39.5

Hardware Setup


Phantom	Tissue Simulating Liquid	Probe Calibration Date	DAE Calibration Date
ELI V8.0 (20deg probe tilt) - 2180	HBBL-600-10000	EX3DV4 - SN7737 / 2024-07-31	DAE4 Sn1741 / 2024-07-16
Measurement Software Version		16.4.0.5005	

Scan Setup

	Area Scan	Zoom Scan
Grid Extents [mm]	40.0 x 80.0	30.0 x 30.0 x 30.0
Grid Steps [mm]	10.0 x 10.0	5.0 x 5.0 x 1.5
Sensor Surface [mm]	3.0	1.4
Graded Grid	N/A	Yes
Grading Ratio	N/A	1.5

Measurement Results

	Area Scan	Zoom Scan
psSAR-1g [W/kg]	2.77	2.71
psSAR-10g [W/kg]	1.27	1.26
Power Drift [dB]		0.02
TSL Correction	Positive only	Positive only

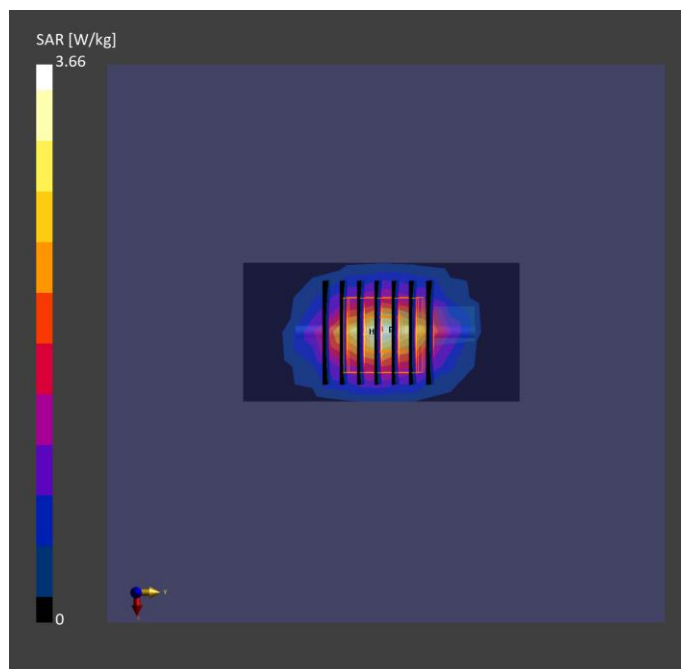

Test Date : 2025-02-20 | Ambient Temp : 22.5 °C | Tissue Temp : 21.7 °C

System Performance Check**System Performance Check at 2450 MHz****Verification Source Properties**

Manufacturer	Model No.	Serial No.	Input Power [dBm]
SPEAG	D2450V2	1087	17.0

Exposure Conditions

Phantom Section	Group	Frequency [MHz]	Conversion Factor	TSL Conductivity [S/m]	TSL Permittivity
Flat	CW	2450.000	7.25	1.74	37.1

Hardware Setup


Phantom	Tissue Simulating Liquid	Probe Calibration Date	DAE Calibration Date
ELI V8.0 (20deg probe tilt) - 2180	HBBL-600-10000	EX3DV4 - SN7737 / 2024-07-31	DAE4 Sn1741 / 2024-07-16
Measurement Software Version		16.4.0.5005	

Scan Setup

	Area Scan	Zoom Scan
Grid Extents [mm]	40.0 x 80.0	30.0 x 30.0 x 30.0
Grid Steps [mm]	10.0 x 10.0	5.0 x 5.0 x 1.5
Sensor Surface [mm]	3.0	1.4
Graded Grid	N/A	Yes
Grading Ratio	N/A	1.5

Measurement Results

	Area Scan	Zoom Scan
psSAR-1g [W/kg]	2.58	2.52
psSAR-10g [W/kg]	1.18	1.17
Power Drift [dB]		-0.01
TSL Correction	Positive only	Positive only

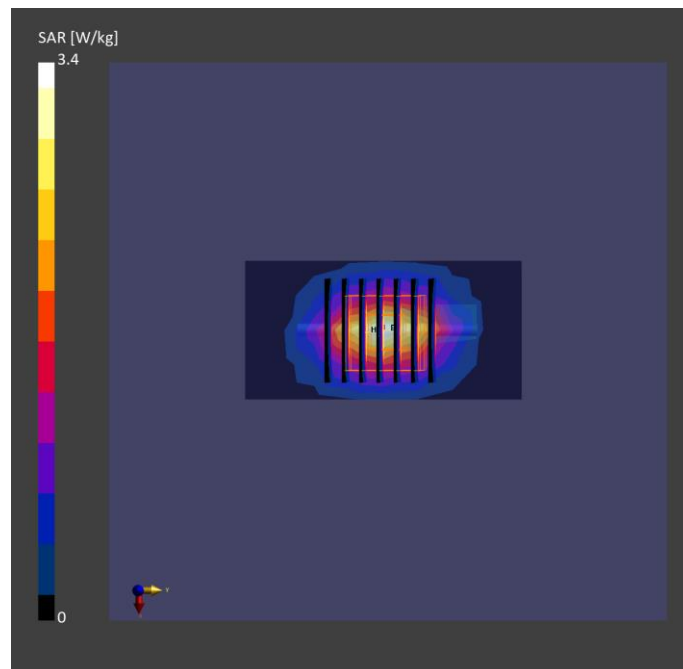

Test Date : 2025-02-21 | Ambient Temp : 22.9 °C | Tissue Temp : 22.1 °C

System Performance Check**System Performance Check at 5250 MHz****Verification Source Properties**

Manufacturer	Model No.	Serial No.	Input Power [dBm]
SPEAG	D5GHzV2	1358	17.0

Exposure Conditions

Phantom Section	Group	Frequency [MHz]	Conversion Factor	TSL Conductivity [S/m]	TSL Permittivity
Flat	CW	5250.000	5.56	4.62	35.1

Hardware Setup


Phantom	Tissue Simulating Liquid	Probe Calibration Date	DAE Calibration Date
ELI V8.0 (20deg probe tilt) - 2180	HBBL-600-10000	EX3DV4 - SN7737 / 2024-07-31	DAE4 Sn1741 / 2024-07-16
Measurement Software Version		16.4.0.5005	

Scan Setup

	Area Scan	Zoom Scan
Grid Extents [mm]	40.0 x 80.0	22.0 x 22.0 x 22.0
Grid Steps [mm]	10.0 x 10.0	4.0 x 4.0 x 1.4
Sensor Surface [mm]	3.0	1.4
Graded Grid	N/A	Yes
Grading Ratio	N/A	1.4

Measurement Results

	Area Scan	Zoom Scan
psSAR-1g [W/kg]	3.66	3.77
psSAR-10g [W/kg]	1.04	1.09
Power Drift [dB]		-0.08
TSL Correction	Positive only	Positive only

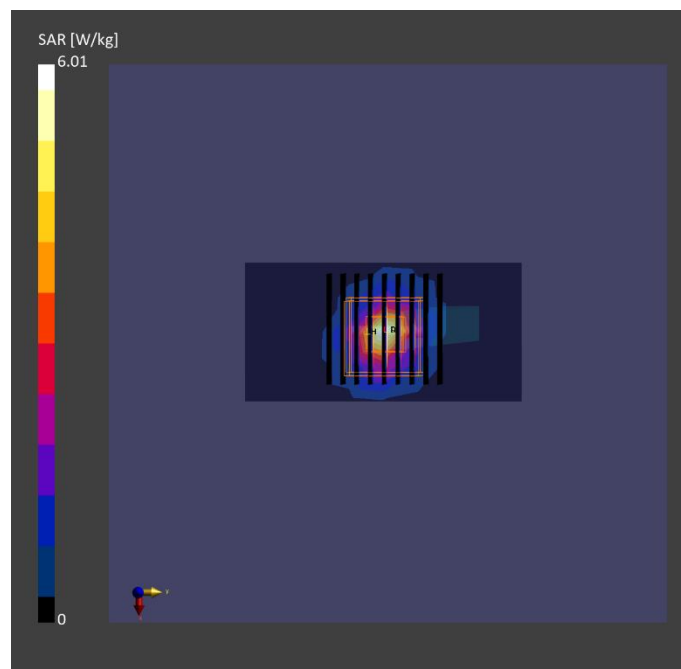

Test Date : 2025-02-21 | Ambient Temp : 22.9 °C | Tissue Temp : 22.1 °C

System Performance Check**System Performance Check at 5600 MHz****Verification Source Properties**

Manufacturer	Model No.	Serial No.	Input Power [dBm]
SPEAG	D5GHzV2	1358	17.0

Exposure Conditions

Phantom Section	Group	Frequency [MHz]	Conversion Factor	TSL Conductivity [S/m]	TSL Permittivity
Flat	CW	5600.000	5.07	4.99	34.4

Hardware Setup


Phantom	Tissue Simulating Liquid	Probe Calibration Date	DAE Calibration Date
ELI V8.0 (20deg probe tilt) - 2180	HBBL-600-10000	EX3DV4 - SN7737 / 2024-07-31	DAE4 Sn1741 / 2024-07-16
Measurement Software Version		16.4.0.5005	

Scan Setup

	Area Scan	Zoom Scan
Grid Extents [mm]	40.0 x 80.0	22.0 x 22.0 x 22.0
Grid Steps [mm]	10.0 x 10.0	4.0 x 4.0 x 1.4
Sensor Surface [mm]	3.0	1.4
Graded Grid	N/A	Yes
Grading Ratio	N/A	1.4

Measurement Results

	Area Scan	Zoom Scan
psSAR-1g [W/kg]	3.85	4.14
psSAR-10g [W/kg]	1.08	1.18
Power Drift [dB]		-0.03
TSL Correction	Positive only	Positive only

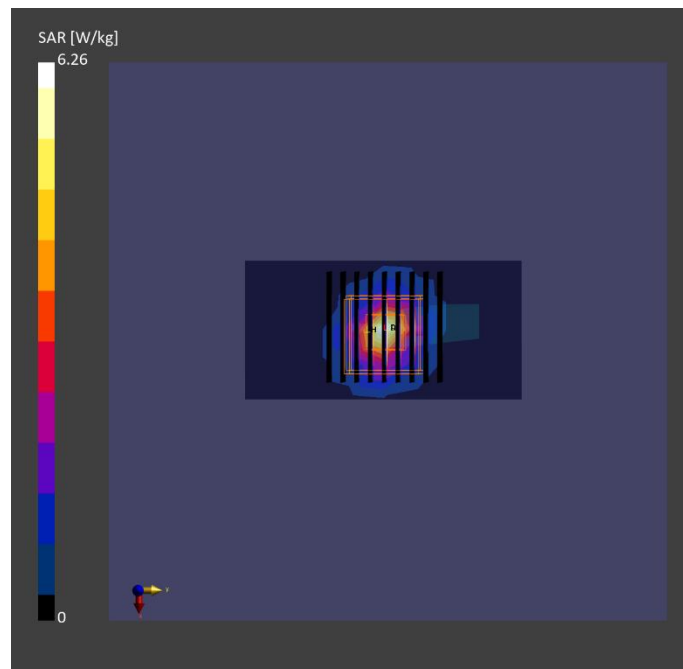

Test Date : 2025-02-24 | Ambient Temp : 21.8 °C | Tissue Temp : 21.1 °C

System Performance Check**System Performance Check at 5800 MHz****Verification Source Properties**

Manufacturer	Model No.	Serial No.	Input Power [dBm]
SPEAG	D5GHzV2	1358	17.0

Exposure Conditions

Phantom Section	Group	Frequency [MHz]	Conversion Factor	TSL Conductivity [S/m]	TSL Permittivity
Flat	CW	5800.000	5.01	5.21	34.0

Hardware Setup


Phantom	Tissue Simulating Liquid	Probe Calibration Date	DAE Calibration Date
ELI V8.0 (20deg probe tilt) - 2180	HBBL-600-10000	EX3DV4 - SN7737 / 2024-07-31	DAE4 Sn1741 / 2024-07-16
Measurement Software Version		16.4.0.5005	

Scan Setup

	Area Scan	Zoom Scan
Grid Extents [mm]	40.0 x 80.0	22.0 x 22.0 x 22.0
Grid Steps [mm]	10.0 x 10.0	4.0 x 4.0 x 1.4
Sensor Surface [mm]	3.0	1.4
Graded Grid	N/A	Yes
Grading Ratio	N/A	1.4

Measurement Results

	Area Scan	Zoom Scan
psSAR-1g [W/kg]	3.69	3.83
psSAR-10g [W/kg]	1.04	1.09
Power Drift [dB]		-0.01
TSL Correction	Positive only	Positive only

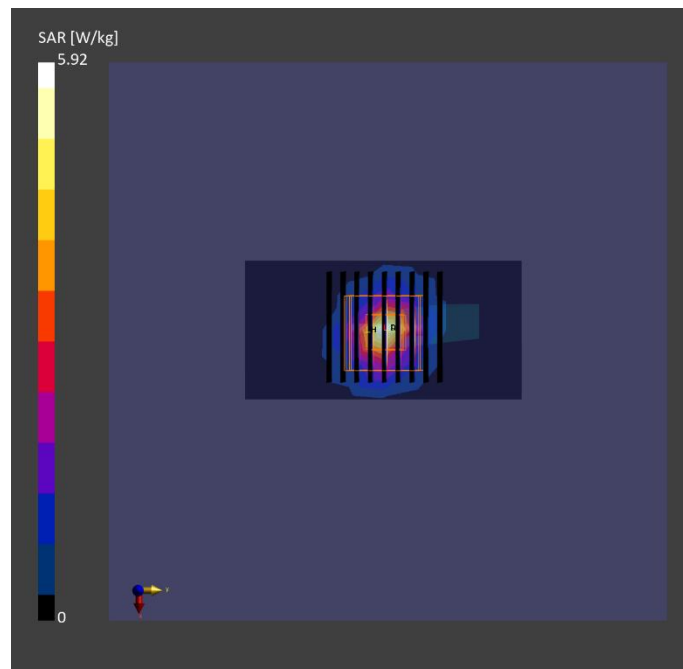

Test Date : 2025-02-25 | Ambient Temp : 21.5 °C | Tissue Temp : 21.1 °C

System Performance Check**System Performance Check at 6500 MHz****Verification Source Properties**

Manufacturer	Model No.	Serial No.	Input Power [dBm]
SPEAG	D6.5GHzV2	1081	20.0

Exposure Conditions

Phantom Section	Group	Frequency [MHz]	Conversion Factor	TSL Conductivity [S/m]	TSL Permittivity
Flat	CW	6500.000	5.25	6.01	32.8

Hardware Setup


Phantom	Tissue Simulating Liquid	Probe Calibration Date	DAE Calibration Date
ELI V8.0 (20deg probe tilt) - 2180	HBBL-600-10000	EX3DV4 - SN7737 / 2024-07-31	DAE4 Sn1741 / 2024-07-16
Measurement Software Version		16.4.0.5005	

Scan Setup

	Area Scan	Zoom Scan
Grid Extents [mm]	51.0 x 85.0	22.0 x 22.0 x 22.0
Grid Steps [mm]	8.5 x 8.5	3.4 x 3.4 x 1.4
Sensor Surface [mm]	3.0	1.4
Graded Grid	N/A	Yes
Grading Ratio	N/A	1.4

Measurement Results

	Area Scan	Zoom Scan
psSAR-1g [W/kg]	24.5	29.9
psSAR-8g [W/kg]	6.15	6.69
psSAR-10g [W/kg]	5.10	5.54
psAPD (1.0 cm ² , sq) [W/m ²]		299
psAPD (4.0 cm ² , sq) [W/m ²]		134
Power Drift [dB]		-0.01
TSL Correction	Positive only	Positive only

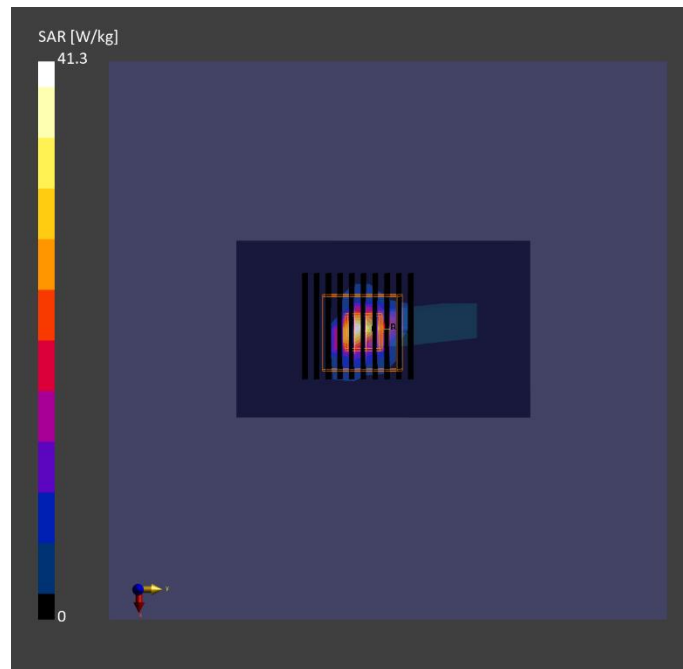

Test Date : 2025-02-26 | Ambient Temp : 22.3 °C

System Performance Check**System Performance Check at 10 GHz****Verification Source Properties**

Manufacturer	Model No.	Serial No.
SPEAG	5G Verification Source 10GHz	1060

Exposure Conditions

Phantom Section	Group	Frequency [MHz]	Conversion Factor
5G	CW	10000.0	1.0

Hardware Setup


Phantom	Medium	Probe Calibration Date	DAE Calibration Date
mmWave - 1102	Air	EUmmWV4 - SN9639_F1- 55GHz / 2024-09-16	DAE4 Sn1742 / 2024-08-15
Measurement Software Version		V3.2.0.1840	

Scan Setup

	5G Scan
Grid Extents [mm]	60.0 x 60.0
Grid Steps [mm]	0.125 x 0.125
Sensor Surface [mm]	10.0

Measurement Results

	5G Scan
Avg. Area [cm ²]	4.00
psPD n+ [W/m ²]	52.3
psPD tot+ [W/m ²]	52.6
psPD mod+ [W/m ²]	53.1
E max [V/m]	149
Power Drift [dB]	0.02

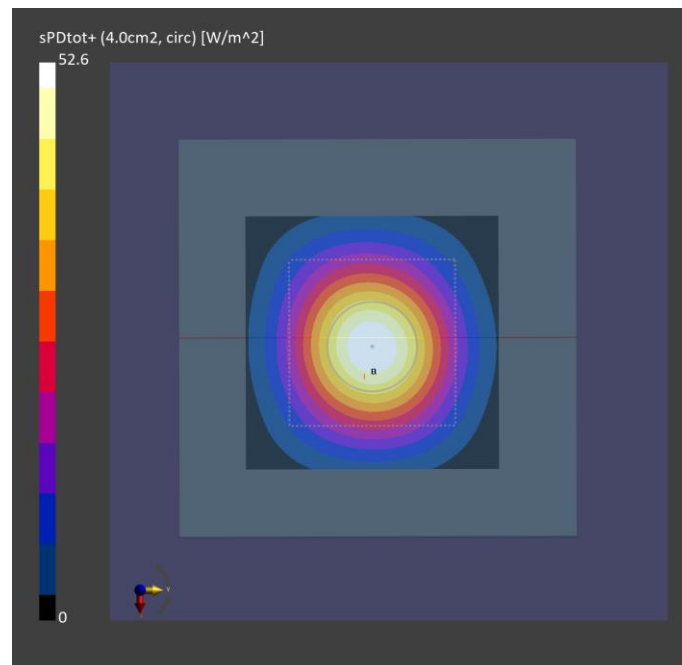

Test Date : 2025-02-27 | Ambient Temp : 22.1 °C

System Performance Check**System Performance Check at 10 GHz****Verification Source Properties**

Manufacturer	Model No.	Serial No.
SPEAG	5G Verification Source 10GHz	1060

Exposure Conditions

Phantom Section	Group	Frequency [MHz]	Conversion Factor
5G	CW	10000.0	1.0

Hardware Setup


Phantom	Medium	Probe Calibration Date	DAE Calibration Date
mmWave - 1102	Air	EUmmWV4 - SN9639_F1- 55GHz / 2024-09-16	DAE4 Sn1742 / 2024-08-15
Measurement Software Version		V3.2.0.1840	

Scan Setup

	5G Scan
Grid Extents [mm]	60.0 x 60.0
Grid Steps [mm]	0.125 x 0.125
Sensor Surface [mm]	10.0

Measurement Results

	5G Scan
Avg. Area [cm ²]	4.00
psPD n+ [W/m ²]	52.0
psPD tot+ [W/m ²]	52.2
psPD mod+ [W/m ²]	52.7
E max [V/m]	147
Power Drift [dB]	0.03

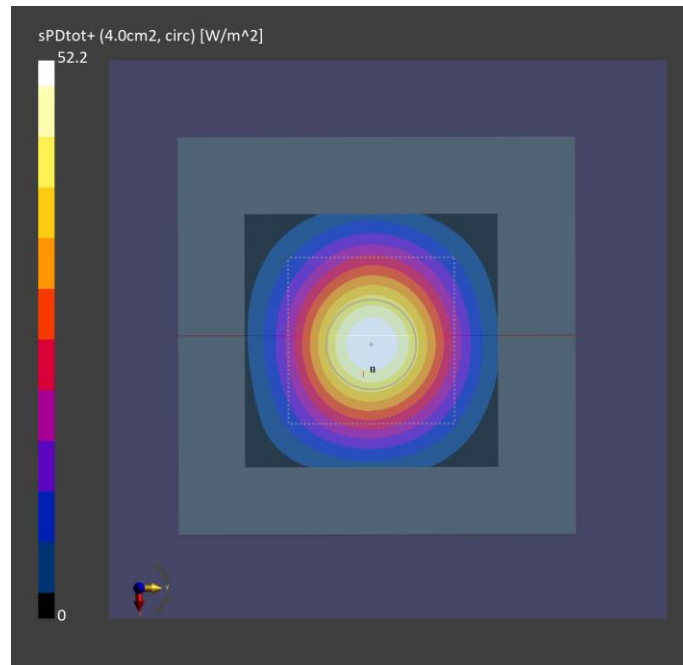

Test Date : 2025-03-01 | Ambient Temp : 22.5 °C

System Performance Check**System Performance Check at 10 GHz****Verification Source Properties**

Manufacturer	Model No.	Serial No.
SPEAG	5G Verification Source 10GHz	1060

Exposure Conditions

Phantom Section	Group	Frequency [MHz]	Conversion Factor
5G	CW	10000.0	1.0

Hardware Setup


Phantom	Medium	Probe Calibration Date	DAE Calibration Date
mmWave - 1102	Air	EUmmWV4 - SN9639_F1- 55GHz / 2024-09-16	DAE4 Sn1742 / 2024-08-15
Measurement Software Version		V3.2.0.1840	

Scan Setup

	5G Scan
Grid Extents [mm]	60.0 x 60.0
Grid Steps [mm]	0.125 x 0.125
Sensor Surface [mm]	10.0

Measurement Results

	5G Scan
Avg. Area [cm ²]	4.00
psPD n+ [W/m ²]	59.8
psPD tot+ [W/m ²]	60.1
psPD mod+ [W/m ²]	60.4
E max [V/m]	159
Power Drift [dB]	-0.16

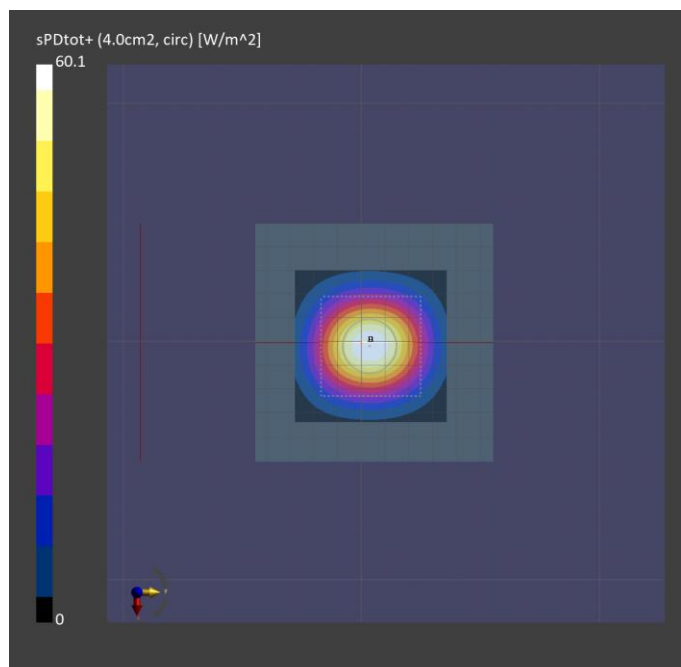

Test Date : 2025-03-02 | Ambient Temp : 22.7 °C

System Performance Check**System Performance Check at 10 GHz****Verification Source Properties**

Manufacturer	Model No.	Serial No.
SPEAG	5G Verification Source 10GHz	1060

Exposure Conditions

Phantom Section	Group	Frequency [MHz]	Conversion Factor
5G	CW	10000.0	1.0

Hardware Setup

Phantom	Medium	Probe Calibration Date	DAE Calibration Date
mmWave - 1102	Air	EUmmWV4 - SN9639_F1- 55GHz / 2024-09-16	DAE4 Sn1742 / 2024-08-15
Measurement Software Version		V3.2.0.1840	

Scan Setup

	5G Scan
Grid Extents [mm]	60.0 x 60.0
Grid Steps [mm]	0.125 x 0.125
Sensor Surface [mm]	10.0

Measurement Results

	5G Scan
Avg. Area [cm ²]	4.00
psPD n+ [W/m ²]	56.3
psPD tot+ [W/m ²]	56.6
psPD mod+ [W/m ²]	57.0
E max [V/m]	154
Power Drift [dB]	0.01

