

Appendix B – System Check Plots

Test Date : 2025-02-27 | Ambient Temp : 22.5 °C | Tissue Temp : 21.2 °C

System Performance Check**System Performance Check at 2450 MHz****Verification Source Properties**

Manufacturer	Model No.	Serial No.	Input Power [dBm]
SPEAG	D2450	1087	17.0

Exposure Conditions

Phantom Section	Group	Frequency [MHz]	Conversion Factor	TSL Conductivity [S/m]	TSL Permittivity
Flat	CW	2450.000	6.96	1.82	38.7

Hardware Setup


Phantom	Tissue Simulating Liquid	Probe / Calibration Date	DAE / Calibration Date
ELI V8.0 (20deg probe tilt) - 2179	HBBL-600-10000	EX3DV4 - SN7650 / 2024-06-04	DAE4 Sn1742 / 2024-08-15
Measurement Software Version		16.2.4.2524	

Scan Setup

	Area Scan	Zoom Scan
Grid Extents [mm]	40.0 x 80.0	30.0 x 30.0 x 30.0
Grid Steps [mm]	10.0 x 10.0	5.0 x 5.0 x 1.5
Sensor Surface [mm]	3.0	1.4
Graded Grid	N/A	Yes
Grading Ratio	N/A	1.5

Measurement Results

	Area Scan	Zoom Scan
psSAR-1g [W/kg]	2.39	2.41
psSAR-10g [W/kg]	1.11	1.13
Power Drift [dB]		0.01
TSL Correction	Positive only	Positive only

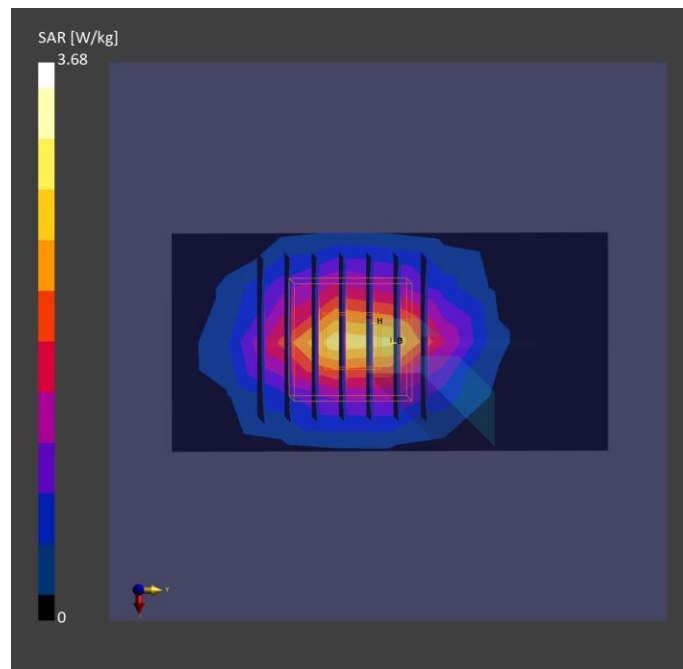

Test Date : 2025-02-28 | Ambient Temp : 22.6 °C | Tissue Temp : 21.1 °C

System Performance Check**System Performance Check at 5250 MHz****Verification Source Properties**

Manufacturer	Model No.	Serial No.	Input Power [dBm]
SPEAG	D5GHzV2	1358	17.0

Exposure Conditions

Phantom Section	Group	Frequency [MHz]	Conversion Factor	TSL Conductivity [S/m]	TSL Permittivity
Flat	CW	5250.000	5.45	4.63	34.5

Hardware Setup


Phantom	Tissue Simulating Liquid	Probe / Calibration Date	DAE / Calibration Date
ELI V8.0 (20deg probe tilt) - 2179	HBBL-600-10000	EX3DV4 - SN7650 / 2024-06-04	DAE4 Sn1742 / 2024-08-15
Measurement Software Version		16.2.4.2524	

Scan Setup

	Area Scan	Zoom Scan
Grid Extents [mm]	40.0 x 80.0	22.0 x 22.0 x 22.0
Grid Steps [mm]	10.0 x 10.0	4.0 x 4.0 x 1.4
Sensor Surface [mm]	3.0	1.4
Graded Grid	N/A	Yes
Grading Ratio	N/A	1.4

Measurement Results

	Area Scan	Zoom Scan
psSAR-1g [W/kg]	3.45	3.66
psSAR-10g [W/kg]	1.05	1.09
Power Drift [dB]		-0.01
TSL Correction	Positive only	Positive only

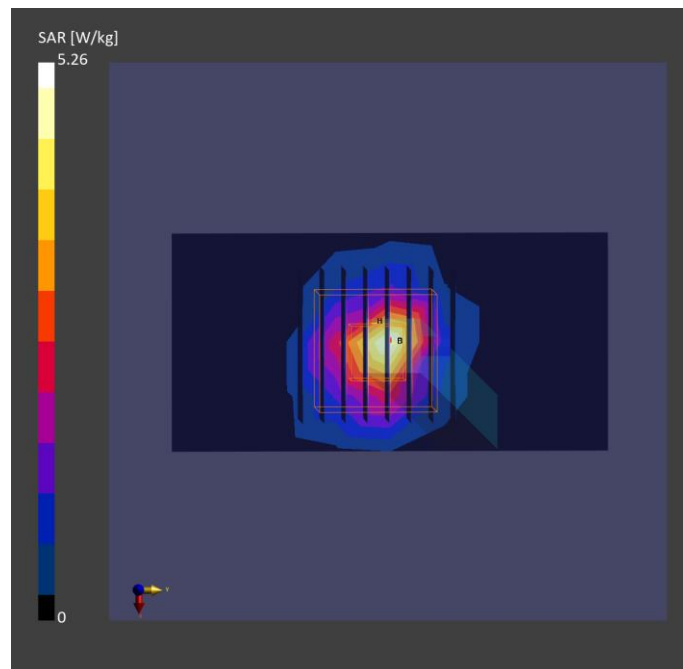

Test Date : 2025-03-01 | Ambient Temp : 22.8 °C | Tissue Temp : 21.4 °C

System Performance Check**System Performance Check at 5600 MHz****Verification Source Properties**

Manufacturer	Model No.	Serial No.	Input Power [dBm]
SPEAG	D5GHzV2	1358	17.0

Exposure Conditions

Phantom Section	Group	Frequency [MHz]	Conversion Factor	TSL Conductivity [S/m]	TSL Permittivity
Flat	CW	5600.000	4.88	5.11	33.9

Hardware Setup


Phantom	Tissue Simulating Liquid	Probe / Calibration Date	DAE / Calibration Date
ELI V8.0 (20deg probe tilt) - 2179	HBBL-600-10000	EX3DV4 - SN7650 / 2024-06-04	DAE4 Sn1742 / 2024-08-15
Measurement Software Version		16.4.0.5005	

Scan Setup

	Area Scan	Zoom Scan
Grid Extents [mm]	40.0 x 80.0	22.0 x 22.0 x 22.0
Grid Steps [mm]	10.0 x 10.0	4.0 x 4.0 x 1.4
Sensor Surface [mm]	3.0	1.4
Graded Grid	N/A	Yes
Grading Ratio	N/A	1.4

Measurement Results

	Area Scan	Zoom Scan
psSAR-1g [W/kg]	4.02	4.45
psSAR-10g [W/kg]	1.17	1.26
Power Drift [dB]		0.04
TSL Correction	Positive only	Positive only

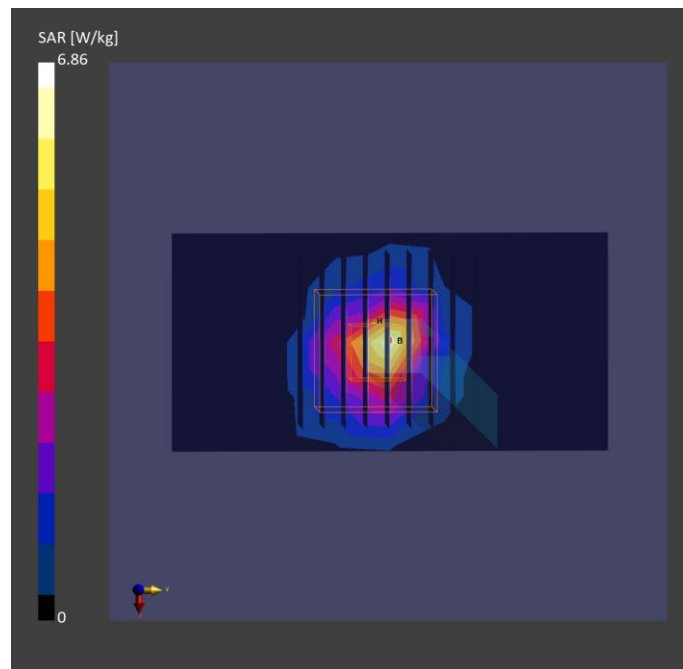

Test Date : 2025-03-02 | Ambient Temp : 22.3 °C | Tissue Temp : 21.3 °C

System Performance Check**System Performance Check at 5800 MHz****Verification Source Properties**

Manufacturer	Model No.	Serial No.	Input Power [dBm]
SPEAG	D5GHzV2	1358	17.0

Exposure Conditions

Phantom Section	Group	Frequency [MHz]	Conversion Factor	TSL Conductivity [S/m]	TSL Permittivity
Flat	CW	5800.000	5.01	5.09	35.0

Hardware Setup


Phantom	Tissue Simulating Liquid	Probe / Calibration Date	DAE / Calibration Date
ELI V8.0 (20deg probe tilt) - 2179	HBBL-600-10000	EX3DV4 - SN7650 / 2024-06-04	DAE4 Sn1742 / 2024-08-15
Measurement Software Version		16.4.0.5005	

Scan Setup

	Area Scan	Zoom Scan
Grid Extents [mm]	40.0 x 80.0	22.0 x 22.0 x 22.0
Grid Steps [mm]	10.0 x 10.0	4.0 x 4.0 x 1.4
Sensor Surface [mm]	3.0	1.4
Graded Grid	N/A	Yes
Grading Ratio	N/A	1.4

Measurement Results

	Area Scan	Zoom Scan
psSAR-1g [W/kg]	3.47	3.83
psSAR-10g [W/kg]	1.01	1.09
Power Drift [dB]		0.01
TSL Correction	Positive only	Positive only

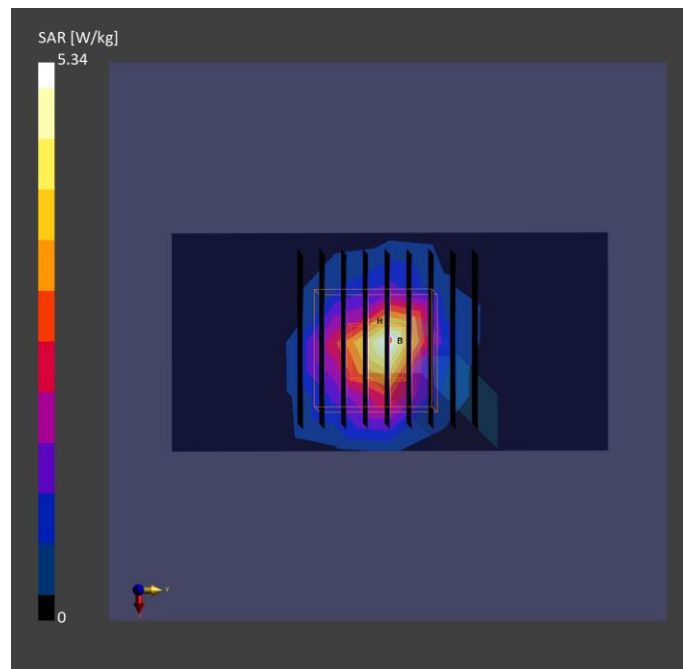

Test Date : 2025-03-04 | Ambient Temp : 22.4 °C | Tissue Temp : 21.7 °C

System Performance Check**System Performance Check at 6500 MHz****Verification Source Properties**

Manufacturer	Model No.	Serial No.	Input Power [dBm]
SPEAG	D6.5GHzV2	1081	20.0

Exposure Conditions

Phantom Section	Group	Frequency [MHz]	Conversion Factor	TSL Conductivity [S/m]	TSL Permittivity
Flat	CW	6500.000	5.37	5.98	32.8

Hardware Setup


Phantom	Tissue Simulating Liquid	Probe / Calibration Date	DAE / Calibration Date
ELI V8.0 (20deg probe tilt) - 2179	HBBL-600-10000	EX3DV4 - SN7650 / 2024-06-04	DAE4 Sn1742 / 2024-08-15
Measurement Software Version		16.4.0.5005	

Scan Setup

	Area Scan	Zoom Scan
Grid Extents [mm]	51.0 x 85.0	22.0 x 22.0 x 22.0
Grid Steps [mm]	8.5 x 8.5	3.4 x 3.4 x 1.4
Sensor Surface [mm]	3.0	1.4
Graded Grid	N/A	Yes
Grading Ratio	N/A	1.4

Measurement Results

	Area Scan	Zoom Scan
psSAR-1g [W/kg]	22.4	27.6
psSAR-8g [W/kg]	5.68	6.23
psSAR-10g [W/kg]	4.71	5.17
psAPD (1.0 cm ² , sq) [W/m ²]		275
psAPD (4.0 cm ² , sq) [W/m ²]		125
Power Drift [dB]		0.01
TSL Correction	Positive only	Positive only

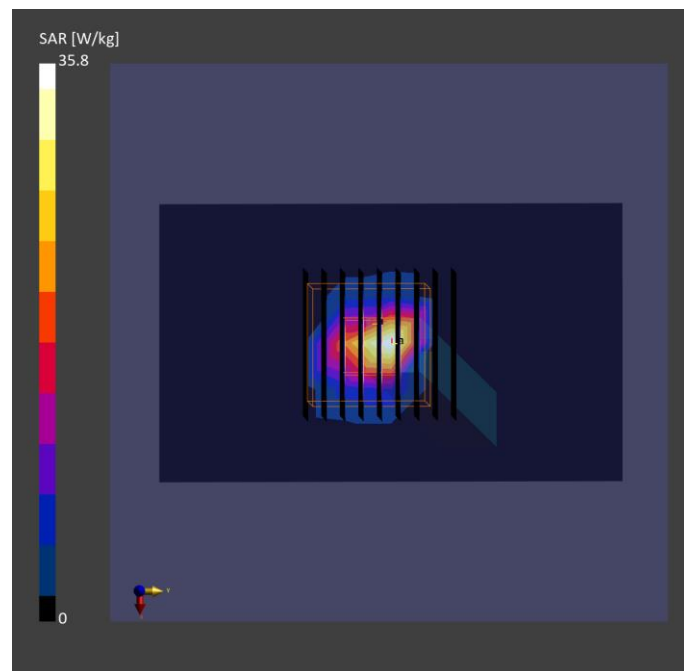

Test Date : 2025-03-05 | Ambient Temp : 22.3 °C

System Performance Check**System Performance Check at 10GHz****Verification Source Properties**

Manufacturer	Model No.	Serial No.
SPEAG	5G Verification Source 10GHz	1060

Exposure Conditions

Phantom Section	Group	Frequency [MHz]	Conversion Factor
5G	CW	10000.0	1.0

Hardware Setup


Phantom	Medium	Probe Calibration Date	DAE Calibration Date
mmWave - 1102	Air	EUmmWV4 - SN9639_F1- 55GHz / 2024-09-16	DAE4 Sn1742 / 2024-08-15
Measurement Software Version		v3.2.2.2358	

Scan Setup

	5G Scan
Grid Extents [mm]	60.0 x 60.0
Grid Steps [mm]	0.125 x 0.125
Sensor Surface [mm]	2.0

Measurement Results

	5G Scan
Avg. Area [cm ²]	4.00
psPD n+ [W/m ²]	60.9
psPD tot+ [W/m ²]	61.1
psPD mod+ [W/m ²]	61.3
E max [V/m]	160
Power Drift [dB]	0.01

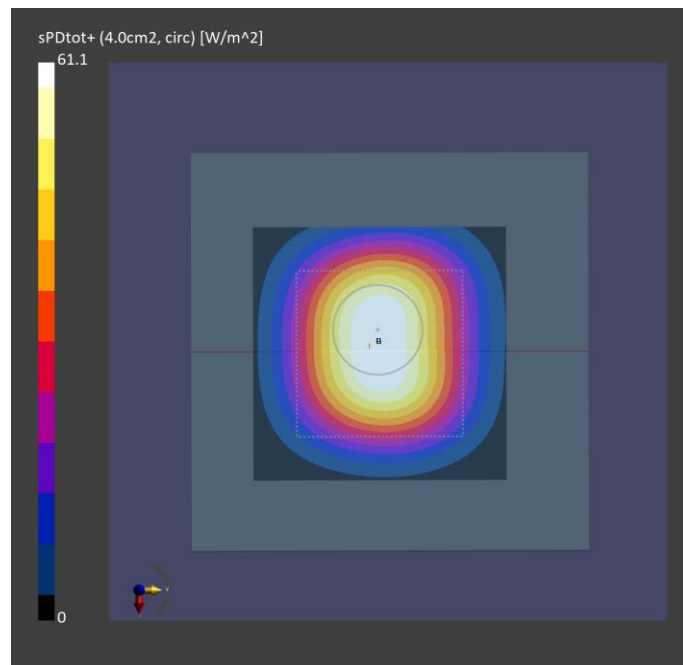

Test Date : 2025-03-06 | Ambient Temp : 22.7 °C

System Performance Check**System Performance Check at 10GHz****Verification Source Properties**

Manufacturer	Model No.	Serial No.
SPEAG	5G Verification Source 10GHz	1060

Exposure Conditions

Phantom Section	Group	Frequency [MHz]	Conversion Factor
5G	CW	10000.0	1.0

Hardware Setup


Phantom	Medium	Probe Calibration Date	DAE Calibration Date
mmWave - 1102	Air	EUmmWV4 - SN9639_F1- 55GHz / 2024-09-16	DAE4 Sn1742 / 2024-08-15
Measurement Software Version		v3.2.2.2358	

Scan Setup

	5G Scan
Grid Extents [mm]	60.0 x 60.0
Grid Steps [mm]	0.125 x 0.125
Sensor Surface [mm]	2.0

Measurement Results

	5G Scan
Avg. Area [cm ²]	4.00
psPD n+ [W/m ²]	54.2
psPD tot+ [W/m ²]	54.6
psPD mod+ [W/m ²]	55.1
E max [V/m]	159
Power Drift [dB]	0.01

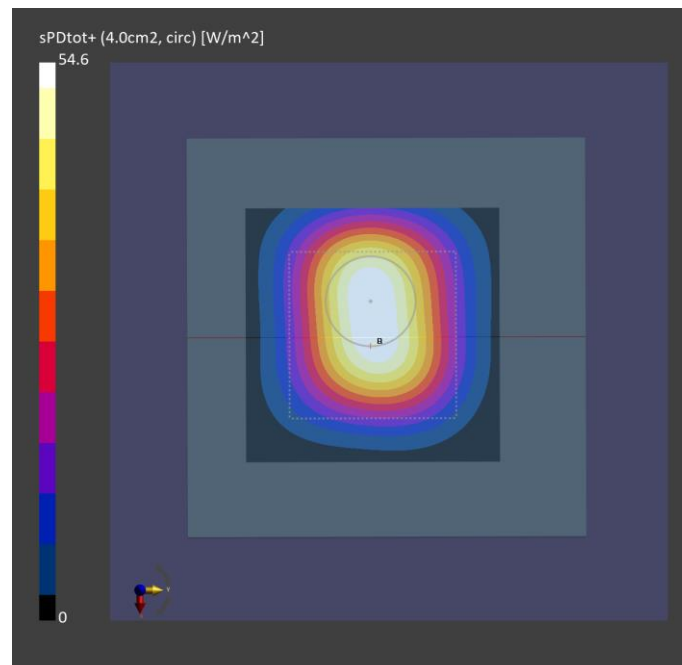

Test Date : 2025-03-07 | Ambient Temp : 22.5 °C

System Performance Check**System Performance Check at 10GHz****Verification Source Properties**

Manufacturer	Model No.	Serial No.
SPEAG	5G Verification Source 10GHz	1060

Exposure Conditions

Phantom Section	Group	Frequency [MHz]	Conversion Factor
5G	CW	10000.0	1.0

Hardware Setup


Phantom	Medium	Probe Calibration Date	DAE Calibration Date
mmWave - 1102	Air	EUmmWV4 - SN9639_F1- 55GHz / 2024-09-16	DAE4 Sn1742 / 2024-08-15
Measurement Software Version		v3.2.2.2358	

Scan Setup

	5G Scan
Grid Extents [mm]	60.0 x 60.0
Grid Steps [mm]	0.125 x 0.125
Sensor Surface [mm]	2.0

Measurement Results

	5G Scan
Avg. Area [cm ²]	4.00
psPD n+ [W/m ²]	56.3
psPD tot+ [W/m ²]	56.3
psPD mod+ [W/m ²]	56.4
E max [V/m]	153
Power Drift [dB]	0.06

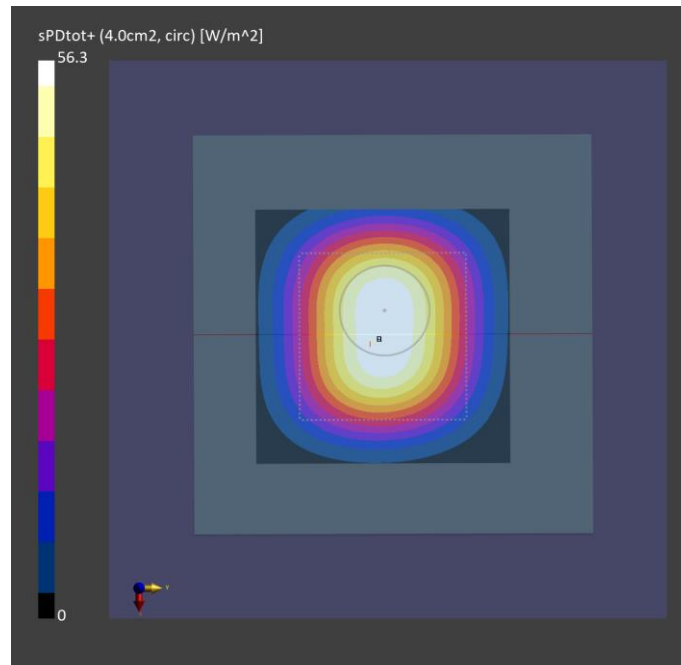

Test Date : 2025-03-08 | Ambient Temp : 22.2 °C

System Performance Check**System Performance Check at 10GHz****Verification Source Properties**

Manufacturer	Model No.	Serial No.
SPEAG	5G Verification Source 10GHz	1060

Exposure Conditions

Phantom Section	Group	Frequency [MHz]	Conversion Factor
5G	CW	10000.0	1.0

Hardware Setup

Phantom	Medium	Probe Calibration Date	DAE Calibration Date
mmWave - 1102	Air	EUmmWV4 - SN9639_F1- 55GHz / 2024-09-16	DAE4 Sn1742 / 2024-08-15
Measurement Software Version		v3.2.2.2358	

Scan Setup

	5G Scan
Grid Extents [mm]	60.0 x 60.0
Grid Steps [mm]	0.125 x 0.125
Sensor Surface [mm]	2.0

Measurement Results

	5G Scan
Avg. Area [cm ²]	4.00
psPD n+ [W/m ²]	58.3
psPD tot+ [W/m ²]	58.7
psPD mod+ [W/m ²]	58.9
E max [V/m]	160
Power Drift [dB]	0.04

