

Appendix B – System Check Plots

Test Date : 2025-03-08 | Ambient Temp : 21.8 °C | Tissue Temp : 21.5 °C

System Performance Check

System Performance Check at 2450 MHz

Verification Source Properties

Manufacturer	Model No.	Serial No.	Input Power [dBm]
SPEAG	D2450	1087	17.0

Exposure Conditions

Phantom Section	Group	Frequency [MHz]	Conversion Factor	TSL Conductivity [S/m]	TSL Permittivity
Flat	CW	2450.000	7.09	1.88	38.6

Hardware Setup


Phantom	Tissue Simulating Liquid	Probe Calibration Date	DAE Calibration Date
ELI V8.0 (20deg probe tilt) - 2141	HBBL-600-10000	EX3DV4 - SN7756 / 2024-09-04	DAE4 Sn1669 / 2024-05-16
Measurement Software Version		16.4.0.5005	

Scan Setup

	Area Scan	Zoom Scan
Grid Extents [mm]	40.0 x 80.0	30.0 x 30.0 x 30.0
Grid Steps [mm]	10.0 x 10.0	5.0 x 5.0 x 1.5
Sensor Surface [mm]	3.0	1.4
Graded Grid	N/A	Yes
Grading Ratio	N/A	1.5

Measurement Results

	Area Scan	Zoom Scan
psSAR-1g [W/kg]	2.62	2.58
psSAR-10g [W/kg]	1.20	1.20
Power Drift [dB]		0.02
TSL Correction	Positive only	Positive only

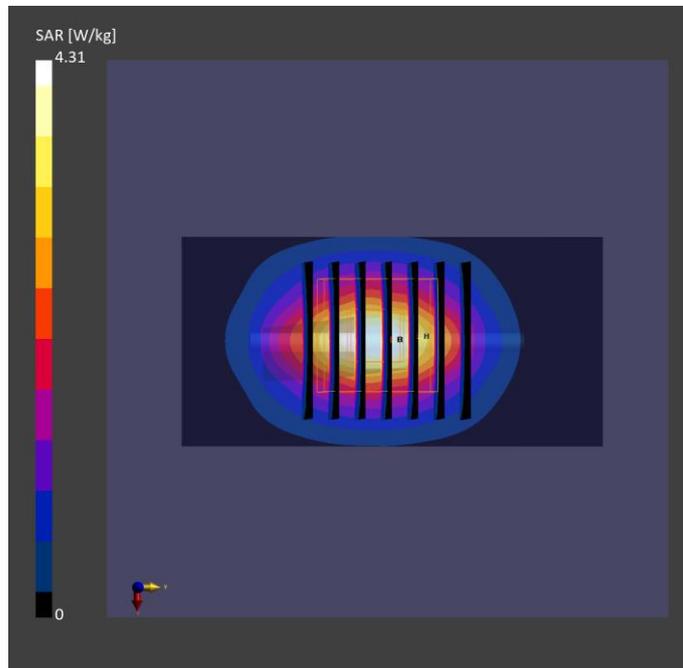

Test Date : 2025-03-09 | Ambient Temp : 22.0 °C | Tissue Temp : 21.8 °C

System Performance Check

System Performance Check at 5250 MHz

Verification Source Properties

Manufacturer	Model No.	Serial No.	Input Power [dBm]
SPEAG	D5GHz	1358	17.0

Exposure Conditions

Phantom Section	Group	Frequency [MHz]	Conversion Factor	TSL Conductivity [S/m]	TSL Permittivity
Flat	CW	5250.000	5.27	4.39	35.3

Hardware Setup


Phantom	Tissue Simulating Liquid	Probe Calibration Date	DAE Calibration Date
ELI V8.0 (20deg probe tilt) - 2141	HBBL-600-10000	EX3DV4 - SN7756 / 2024-09-04	DAE4 Sn1669 / 2024-05-16
Measurement Software Version		16.4.0.5005	

Scan Setup

	Area Scan	Zoom Scan
Grid Extents [mm]	40.0 x 80.0	22.0 x 22.0 x 22.0
Grid Steps [mm]	10.0 x 10.0	4.0 x 4.0 x 1.4
Sensor Surface [mm]	3.0	1.4
Graded Grid	N/A	Yes
Grading Ratio	N/A	1.4

Measurement Results

	Area Scan	Zoom Scan
psSAR-1g [W/kg]	3.28	3.69
psSAR-10g [W/kg]	1.00	1.05
Power Drift [dB]		0.04
TSL Correction	Positive only	Positive only

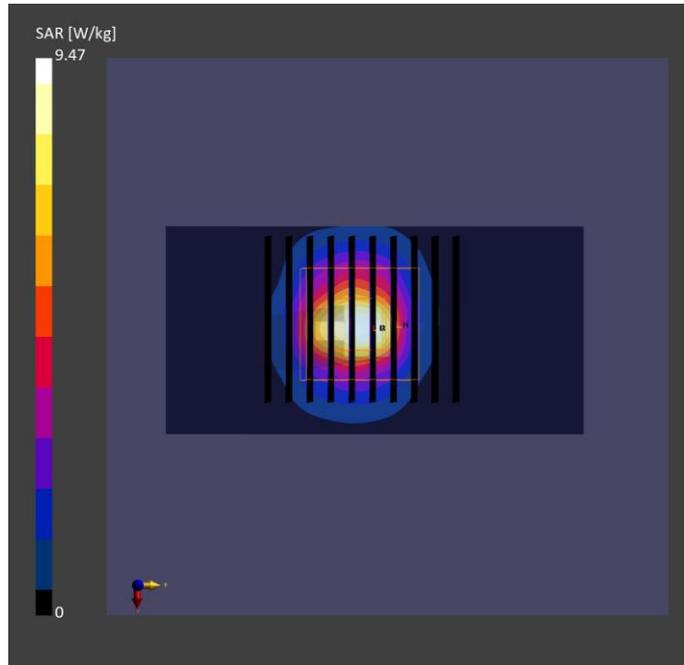

Test Date : 2025-03-09 | Ambient Temp : 22.0 °C | Tissue Temp : 21.8 °C

System Performance Check

System Performance Check at 5600 MHz

Verification Source Properties

Manufacturer	Model No.	Serial No.	Input Power [dBm]
SPEAG	D5GHz	1358	17.0

Exposure Conditions

Phantom Section	Group	Frequency [MHz]	Conversion Factor	TSL Conductivity [S/m]	TSL Permittivity
Flat	CW	5600.000	4.7	4.75	34.7

Hardware Setup


Phantom	Tissue Simulating Liquid	Probe Calibration Date	DAE Calibration Date
ELI V8.0 (20deg probe tilt) - 2141	HBBL-600-10000	EX3DV4 - SN7756 / 2024-09-04	DAE4 Sn1669 / 2024-05-16
Measurement Software Version		16.4.0.5005	

Scan Setup

	Area Scan	Zoom Scan
Grid Extents [mm]	40.0 x 80.0	22.0 x 22.0 x 22.0
Grid Steps [mm]	10.0 x 10.0	4.0 x 4.0 x 1.4
Sensor Surface [mm]	3.0	1.4
Graded Grid	N/A	Yes
Grading Ratio	N/A	1.4

Measurement Results

	Area Scan	Zoom Scan
psSAR-1g [W/kg]	3.53	4.03
psSAR-10g [W/kg]	1.06	1.14
Power Drift [dB]		-0.01
TSL Correction	Positive only	Positive only

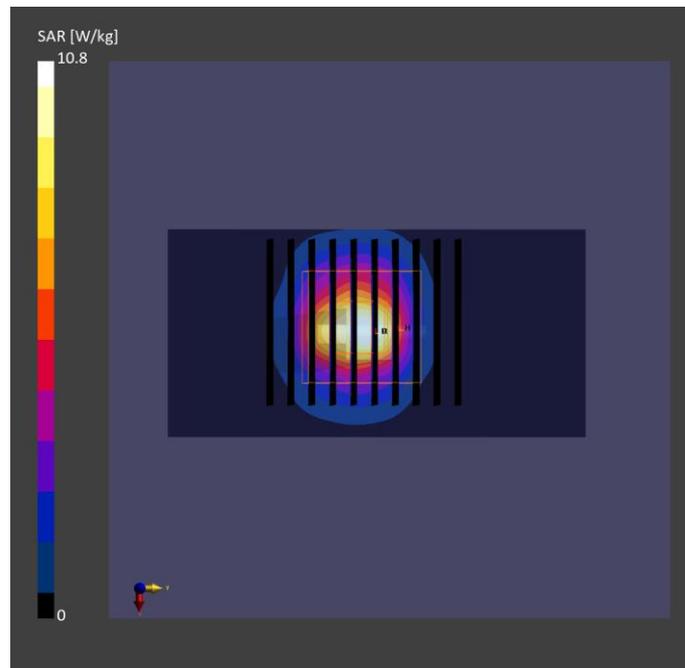

Test Date : 2025-03-09 | Ambient Temp : 22.0 °C | Tissue Temp : 21.8 °C

System Performance Check

System Performance Check at 5800 MHz

Verification Source Properties

Manufacturer	Model No.	Serial No.	Input Power [dBm]
SPEAG	D5GHz	1358	17.0

Exposure Conditions

Phantom Section	Group	Frequency [MHz]	Conversion Factor	TSL Conductivity [S/m]	TSL Permittivity
Flat	CW	5800.000	4.73	4.97	34.4

Hardware Setup


Phantom	Tissue Simulating Liquid	Probe Calibration Date	DAE Calibration Date
ELI V8.0 (20deg probe tilt) - 2141	HBBL-600-10000	EX3DV4 - SN7756 / 2024-09-04	DAE4 Sn1669 / 2024-05-16
Measurement Software Version		16.4.0.5005	

Scan Setup

	Area Scan	Zoom Scan
Grid Extents [mm]	40.0 x 80.0	22.0 x 22.0 x 22.0
Grid Steps [mm]	10.0 x 10.0	4.0 x 4.0 x 1.4
Sensor Surface [mm]	3.0	1.4
Graded Grid	N/A	Yes
Grading Ratio	N/A	1.4

Measurement Results

	Area Scan	Zoom Scan
psSAR-1g [W/kg]	3.35	3.59
psSAR-10g [W/kg]	0.985	1.12
Power Drift [dB]		-0.11
TSL Correction	Positive only	Positive only

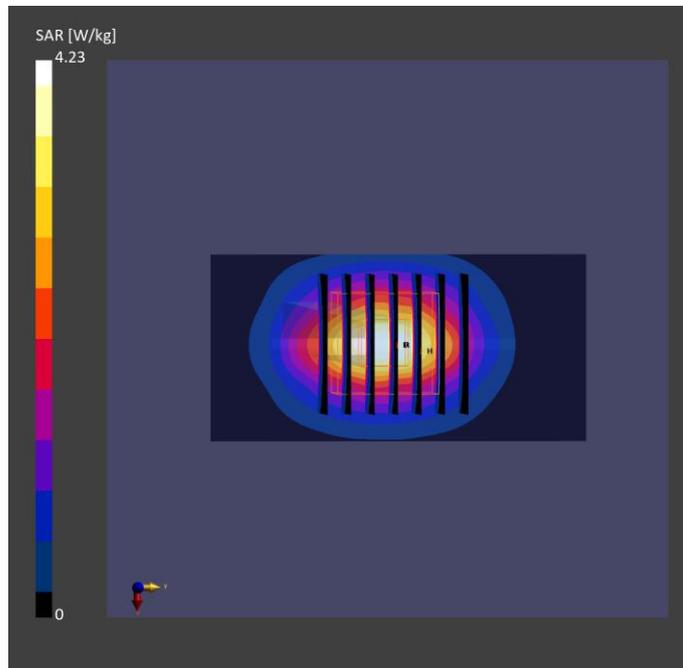

Test Date : 2025-03-08 | Ambient Temp : 21.8 °C | Tissue Temp : 21.5 °C

System Performance Check

System Performance Check at 6500 MHz

Verification Source Properties

Manufacturer	Model No.	Serial No.	Input Power [dBm]
SPEAG	D6.5GHz	1081	20.0

Exposure Conditions

Phantom Section	Group	Frequency [MHz]	Conversion Factor	TSL Conductivity [S/m]	TSL Permittivity
Flat	CW	6500.000	4.64	6.1	33.7

Hardware Setup

Phantom	Tissue Simulating Liquid	Probe Calibration Date	DAE Calibration Date
ELI V8.0 (20deg probe tilt) - 2141	HBBL-600-10000	EX3DV4 - SN7756 / 2024-09-04	DAE4 Sn1669 / 2024-05-16


Measurement Software Version
16.2.4.2524

Scan Setup

	Area Scan	Zoom Scan
Grid Extents [mm]	51.0 x 85.0	22.0 x 22.0 x 22.0
Grid Steps [mm]	8.5 x 8.5	3.4 x 3.4 x 1.4
Sensor Surface [mm]	3.0	1.4
Graded Grid	N/A	Yes
Grading Ratio	N/A	1.4

Measurement Results

	Area Scan	Zoom Scan
psSAR-1g [W/kg]	19.9	26.8
psSAR-8g [W/kg]	5.39	6.02
psSAR-10g [W/kg]	4.47	4.95
psAPD (1.0 cm ² , sq) [W/m ²]		268
psAPD (4.0 cm ² , sq) [W/m ²]		120
Power Drift [dB]		-0.02
TSL Correction	Positive only	Positive only

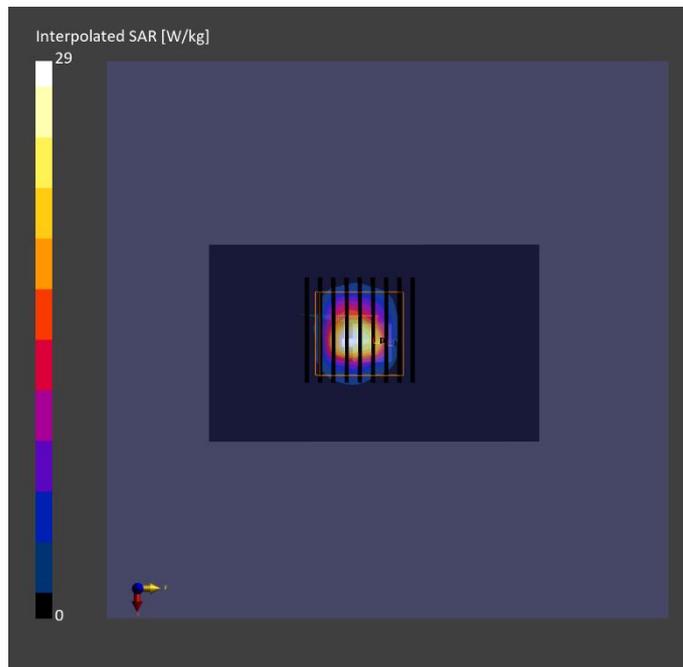

Test Date : 2025-03-14 | Ambient Temp : 22.2 °C

System Performance Check

System Performance Check at 10GHz

Verification Source Properties

Manufacturer	Model No.	Serial No.
SPEAG	5G Verification Source 10GHz	1060

Exposure Conditions

Phantom Section	Group	Frequency [MHz]	Conversion Factor
5G	CW	10000.0	1.0

Hardware Setup


Phantom	Medium	Probe Calibration Date	DAE Calibration Date
mmWave - 1102	Air	EUmmWV4 - SN9639_F1-55GHz / 2024-09-16	DAE4 Sn1742 / 2024-08-15
Measurement Software Version		V3.2.2.2358	

Scan Setup

	5G Scan
Grid Extents [mm]	60.0 x 60.0
Grid Steps [mm]	0.125 x 0.125
Sensor Surface [mm]	10.0

Measurement Results

	5G Scan
Avg. Area [cm ²]	4.00
psPD n+ [W/m ²]	56.3
psPD tot+ [W/m ²]	56.3
psPD mod+ [W/m ²]	56.4
E max [V/m]	153
Power Drift [dB]	0.06

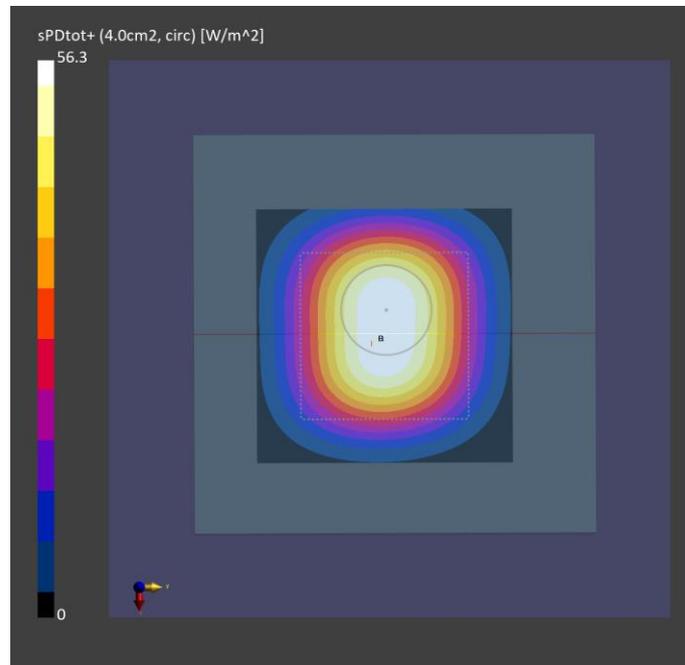

Test Date : 2025-03-15 | Ambient Temp : 22.1 °C

System Performance Check

System Performance Check at 10GHz

Verification Source Properties

Manufacturer	Model No.	Serial No.
SPEAG	5G Verification Source 10GHz	1060

Exposure Conditions

Phantom Section	Group	Frequency [MHz]	Conversion Factor
5G	CW	10000.0	1.0

Hardware Setup

Phantom	Medium	Probe Calibration Date	DAE Calibration Date
mmWave - 1102	Air	EUmmWV4 - SN9639_F1-55GHz / 2024-09-16	DAE4 Sn1742 / 2024-08-15


Measurement Software Version
V3.2.2.2358

Scan Setup

	5G Scan
Grid Extents [mm]	60.0 x 60.0
Grid Steps [mm]	0.125 x 0.125
Sensor Surface [mm]	10.0

Measurement Results

	5G Scan
Avg. Area [cm ²]	4.00
psPD n+ [W/m ²]	62.1
psPD tot+ [W/m ²]	62.2
psPD mod+ [W/m ²]	62.4
E max [V/m]	164
Power Drift [dB]	0.02

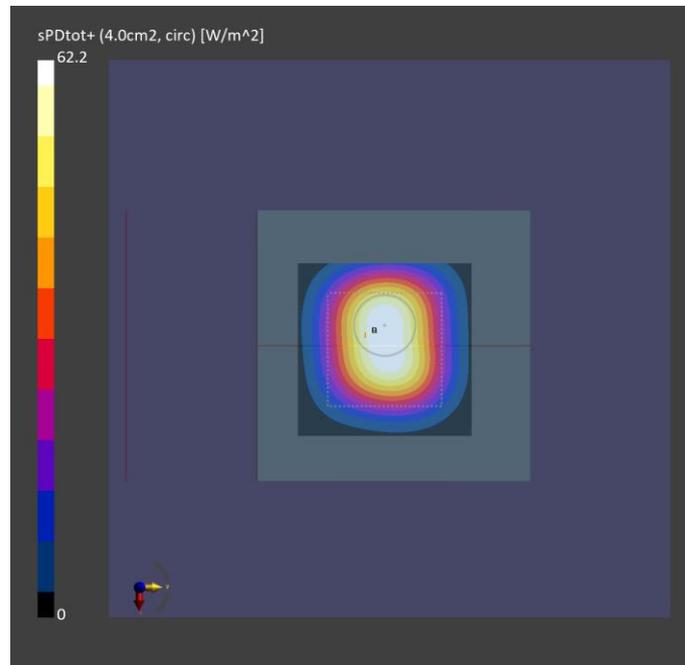

Test Date : 2025-03-16 | Ambient Temp : 22.2 °C

System Performance Check

System Performance Check at 10GHz

Verification Source Properties

Manufacturer	Model No.	Serial No.
SPEAG	5G Verification Source 10GHz	1060

Exposure Conditions

Phantom Section	Group	Frequency [MHz]	Conversion Factor
5G	CW	10000.0	1.0

Hardware Setup

Phantom	Medium	Probe Calibration Date	DAE Calibration Date
mmWave - 1102	Air	EUmmWV4 - SN9639_F1-55GHz / 2024-09-16	DAE4 Sn1742 / 2024-08-15
Measurement Software Version		V3.2.2.2358	

Scan Setup

	5G Scan
Grid Extents [mm]	60.0 x 60.0
Grid Steps [mm]	0.125 x 0.125
Sensor Surface [mm]	10.0

Measurement Results

	5G Scan
Avg. Area [cm ²]	4.00
psPD n+ [W/m ²]	58.3
psPD tot+ [W/m ²]	58.7
psPD mod+ [W/m ²]	58.9
E max [V/m]	160
Power Drift [dB]	0.04

