



PCTEST ENGINEERING LABORATORY, INC.

6660-B Dobbin Road, Columbia, MD 21045 USA
Tel. +1.410.290.6652 / Fax +1.410.290.6654
<http://www.pctestlab.com>



SAR EVALUATION REPORT

Applicant Name:

Sierra Wireless, Inc.
13811 Wireless Way
Richmond, BC V6V 3A4
Canada

Date of Testing:

05/15/12 - 05/21/12

Test Site/Location:

PCTEST Lab, Columbia, MD, USA

Document Serial No.:

0Y1206280879.N7N

FCC ID: **N7NMC8355 (Integrated in Panasonic CF-19mk6)**

APPLICANT: **SIERRA WIRELESS, INC.**

DUT Type:

Module in Portable Convertible Tablet Laptop Computer

FCC Rule Part(s):

CFR §2.1093

Test Device Serial No.:

Pre-Production [S/N: 2CKSA00021]

| Band & Mode | Tx Frequency | Conducted Power [dBm] | SAR | |
|-----------------|-----------------------|-----------------------|------------------|--|
| | | | 1 gm Body (W/kg) | |
| GPRS/EDGE 850 | 824.20 - 848.80 MHz | 32.95 | 0.62 | |
| WCDMA/HSPA 850 | 826.40 - 846.60 MHz | 24.41 | 0.38 | |
| Cell. CDMA/EVDO | 824.70 - 848.31 MHz | 24.33 | 0.43 | |
| AWS WCDMA/HSPA | 1712.4 - 1752.5 MHz | 24.43 | 0.62 | |
| GPRS/EDGE 1900 | 1850.20 - 1909.80 MHz | 29.80 | 0.42 | |
| WCDMA/HSPA 1900 | 1852.4 - 1907.6 MHz | 24.81 | 0.72 | |
| PCS CDMA/EVDO | 1851.25 - 1908.75 MHz | 24.14 | 0.66 | |

Note: Powers in the above table represent output powers for the SAR test configurations and may not represent the highest output powers for all configurations for each mode.

This model portable tablet computer also includes a transmitter using FCC ID ACJ9TGWL12A.

This wireless portable device has been shown to be capable of compliance for localized specific absorption rate (SAR) for uncontrolled environment/general population exposure limits specified in ANSI/IEEE C95.1-1992 and has been tested in accordance with the measurement procedures specified in FCC/OET Bulletin 65 Supplement C (2001), IEEE 1528-2003 and in applicable Industry Canada Radio Standards Specifications (RSS); for 850/1900 GSM/GPRS/EDGE/WCDMA/HSPA/CDMA/EVDO and AWS WCDMA/HSPA operations mentioned in this report only.

I attest to the accuracy of data. All measurements reported herein were performed by me or were made under my supervision and are correct to the best of my knowledge and belief. I assume full responsibility for the completeness of these measurements and vouch for the qualifications of all persons taking them. Test results reported herein relate only to the item(s) tested.

PCTEST certifies that no party to this application has been subject to a denial of Federal benefits that includes FCC benefits pursuant to Section 5301 of the Anti-Drug Abuse Act of 1988, 21 U.S.C. 862..



Randy Ortanez
President



| | | | |
|---|------------------------------------|--|---|
| IC Cert No: N7NMC8355 (Integrated in Panasonic CF-19mk6) | | SAR EVALUATION REPORT | |
| Document S/N: 0Y1206280879.N7N | Test Dates: 05/15/12 - 05/21/12 | DUT Type: Module in Portable Convertible Tablet Laptop Computer | Reviewed by: Quality Manager Page 1 of 25 |

T A B L E O F C O N T E N T S

| | | |
|----|---------------------------------|----|
| 1 | DEVICE UNDER TEST | 3 |
| 2 | INTRODUCTION | 5 |
| 3 | SAR MEASUREMENT SETUP | 6 |
| 4 | DOSIMETRIC ASSESSMENT | 7 |
| 5 | FCC RF EXPOSURE LIMITS..... | 8 |
| 6 | SAR TABLET TESTING | 9 |
| 7 | FCC MEASUREMENT PROCEDURES..... | 10 |
| 8 | RF CONDUCTED POWERS..... | 13 |
| 9 | SYSTEM VERIFICATION..... | 16 |
| 10 | SAR DATA SUMMARY | 18 |
| 11 | EQUIPMENT LIST..... | 21 |
| 12 | MEASUREMENT UNCERTAINTIES | 22 |
| 13 | CONCLUSION..... | 23 |
| 14 | REFERENCES | 24 |

| | | | |
|---|--|--|---------------------------------|
| IC Cert No: N7NMC8355 (Integrated in Panasonic CF-19mk6) |  PCTEST Environmental Engineering Inc. | SAR EVALUATION REPORT | Reviewed by: Quality Manager |
| Document S/N: 0Y1206280879.N7N | Test Dates: 05/15/12 - 05/21/12 | DUT Type: Module in Portable Convertible Tablet Laptop Computer | Page 2 of 25 |

1 DEVICE UNDER TEST

1.1 Device Overview

| Band & Mode | Tx Frequency |
|-----------------|-----------------------|
| GPRS/EDGE 850 | 824.20 - 848.80 MHz |
| WCDMA/HSPA 850 | 826.40 - 846.60 MHz |
| Cell. CDMA/EVDO | 824.70 - 848.31 MHz |
| AWS WCDMA/HSPA | 1712.4 - 1752.5 MHz |
| GPRS/EDGE 1900 | 1850.20 - 1909.80 MHz |
| WCDMA/HSPA 1900 | 1852.4 - 1907.6 MHz |
| PCS CDMA/EVDO | 1851.25 - 1908.75 MHz |

1.2 DUT Antenna Locations

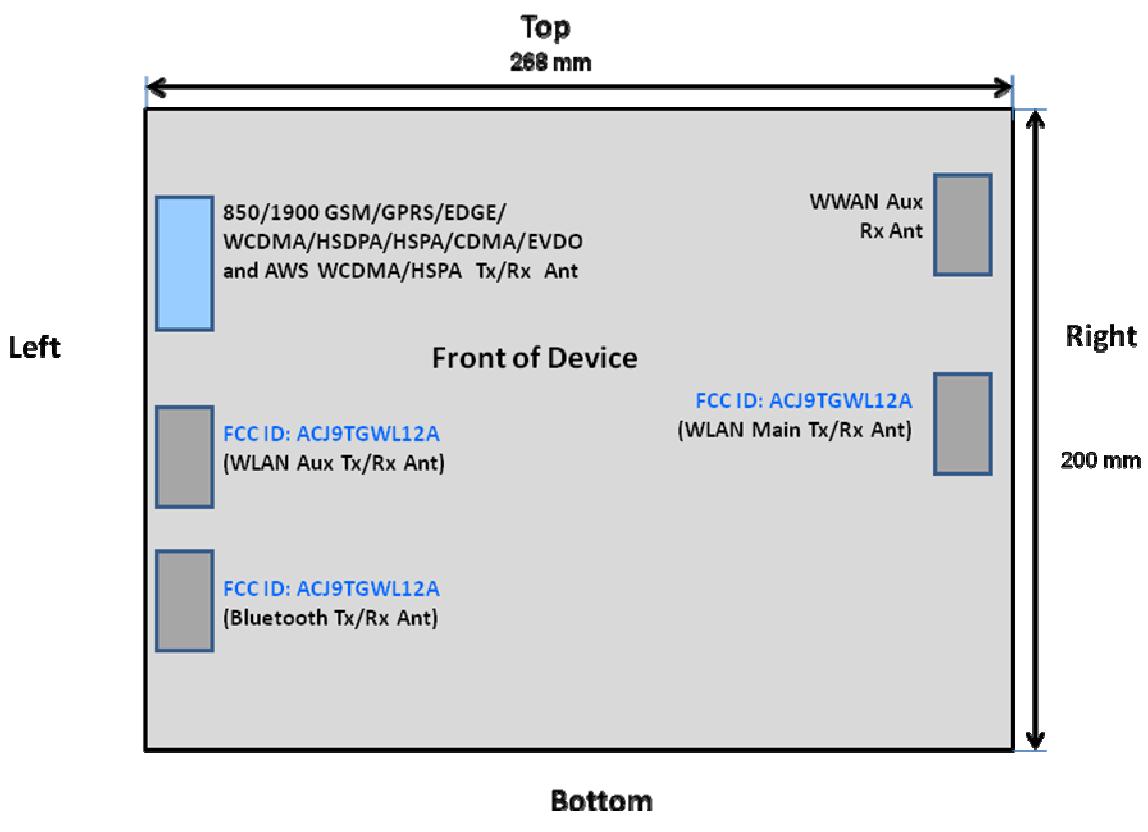


Figure 1-1
DUT Antenna Locations

| | | | |
|---|---|--|---------------------------------|
| IC Cert No: N7NMC8355 (Integrated in Panasonic CF-19mk6) |  | SAR EVALUATION REPORT | Reviewed by: Quality Manager |
| Document S/N: 0Y1206280879.N7N | Test Dates: 05/15/12 - 05/21/12 | DUT Type: Module in Portable Convertible Tablet Laptop Computer | Page 3 of 25 |

1.3 SAR Test Exclusions Applied

(A) Licensed Transmitter(s)

This model does not support Simultaneous Voice and Data for the licensed transmitter in any modes except in WCDMA that allows Multi-RAB transmissions that share voice and data operations on a single physical channel.

This device is only capable of QPSK HSUPA in the uplink, but is capable of HSPA+ in the downlink. Therefore, no additional SAR tests are required beyond that described for devices with HSUPA in KDB 941225 D01.

1.4 Power Reduction for SAR

There is no power reduction for any band/mode implemented in this device for SAR purposes.

1.5 Guidance Applied

- IEEE 1528-2003
- FCC OET Bulletin 65 Supplement C [June 2001]
- FCC KDB 941225 (2G/3G and Hotspot)
- FCC KDB 447498 (Tablet SAR Considerations)

| | | | |
|---|--|--|---|
| IC Cert No: N7NMC8355 (Integrated in Panasonic CF-19mk6) |  PCTEST Engineering Laboratory, Inc. | SAR EVALUATION REPORT | |
| Document S/N: 0Y1206280879.N7N | Test Dates: 05/15/12 - 05/21/12 | DUT Type: Module in Portable Convertible Tablet Laptop Computer | Reviewed by: Quality Manager Page 4 of 25 |

2 INTRODUCTION

The FCC has adopted the guidelines for evaluating the environmental effects of radio frequency (RF) radiation in ET Docket 93-62 on Aug. 6, 1996 to protect the public and workers from the potential hazards of RF emissions due to FCC-regulated portable devices. [1]

The safety limits used for the environmental evaluation measurements are based on the criteria published by the American National Standards Institute (ANSI) for localized specific absorption rate (SAR) in IEEE/ANSI C95.1-1992 Standard for Safety Levels with Respect to Human Exposure to Radio Frequency Electromagnetic Fields, 3 kHz to 300 GHz [3] and Health Canada RF Exposure Guidelines Safety Code 6 [24]. The measurement procedure described in IEEE/ANSI C95.3-2002 Recommended Practice for the Measurement of Potentially Hazardous Electromagnetic Fields - RF and Microwave [4] is used for guidance in measuring the Specific Absorption Rate (SAR) due to the RF radiation exposure from the Equipment Under Test (EUT). These criteria for SAR evaluation are similar to those recommended by the International Committee for Non-Ionizing Radiation Protection (ICNIRP) in Biological Effects and Exposure Criteria for Radiofrequency Electromagnetic Fields," Report No. Vol 74. SAR is a measure of the rate of energy absorption due to exposure to an RF transmitting source. SAR values have been related to threshold levels for potential biological hazards.

2.1 SAR Definition

Specific Absorption Rate is defined as the time derivative (rate) of the incremental energy (dU) absorbed by (dissipated in) an incremental mass (dm) contained in a volume element (dV) of a given density (ρ). It is also defined as the rate of RF energy absorption per unit mass at a point in an absorbing body (see Equation 2-1).

Equation 2-1
SAR Mathematical Equation

$$S A R = \frac{d}{d t} \left(\frac{d U}{d m} \right) = \frac{d}{d t} \left(\frac{d U}{\rho d v} \right)$$

SAR is expressed in units of Watts per Kilogram (W/kg).

$$S A R = \frac{\sigma \cdot E^2}{\rho}$$

where:

σ = conductivity of the tissue-simulating material (S/m)

ρ = mass density of the tissue-simulating material (kg/m³)

E = Total RMS electric field strength (V/m)

NOTE: The primary factors that control rate of energy absorption were found to be the wavelength of the incident field in relation to the dimensions and geometry of the irradiated organism, the orientation of the organism in relation to the polarity of field vectors, the presence of reflecting surfaces, and whether conductive contact is made by the organism with a ground plane.[6]

| | | | |
|---|---|--|---------------------------------|
| IC Cert No: N7NMC8355 (Integrated in Panasonic CF-19mk6) |  PCTEST Environmental Engineering | SAR EVALUATION REPORT | Reviewed by: Quality Manager |
| Document S/N: 0Y1206280879.N7N | Test Dates: 05/15/12 - 05/21/12 | DUT Type: Module in Portable Convertible Tablet Laptop Computer | Page 5 of 25 |

3 SAR MEASUREMENT SETUP

3.1 Automated SAR Measurement System

Measurements are performed using the DASY automated dosimetric SAR assessment system. The DASY is made by Schmid & Partner Engineering AG (SPEAG) in Zurich, Switzerland and consists of a high precision robotics system (Staubli), robot controller, desktop computer, near-field probe, probe alignment sensor, and the SAM phantom containing the head or body equivalent material. The robot is a six-axis industrial robot, performing precise movements to position the probe to the location (points) of maximum electromagnetic field (EMF). See www.speag.com for more information about the specification of the SAR assessment system.



Figure 3-1
SAR Measurement System



Figure 3-2
Near-Field Probe

Table 3-1
Composition of the Tissue Equivalent Matter

| Frequency (MHz) | 835 | 1750 | 1900 |
|---------------------------|-------|------|-------|
| Tissue | Body | Body | Body |
| Ingredients (% by weight) | | | |
| Bactericide | 0.1 | | |
| DGBE | | 31 | 29.44 |
| HEC | 1 | | |
| NaCl | 0.94 | 0.2 | 0.39 |
| Sucrose | 44.9 | | |
| Water | 53.06 | 68.8 | 70.17 |

| | | | |
|---|---|--|---------------------------------|
| IC Cert No: N7NMC8355 (Integrated in Panasonic CF-19mk6) |  PCTEST [®] ENVIRONMENTAL LABORATORY, INC. | SAR EVALUATION REPORT | Reviewed by: Quality Manager |
| Document S/N: 0Y1206280879.N7N | Test Dates: 05/15/12 - 05/21/12 | DUT Type: Module in Portable Convertible Tablet Laptop Computer | Page 6 of 25 |

4 DOSIMETRIC ASSESSMENT

4.1 Measurement Procedure

The evaluation was performed using the following procedure:

1. The SAR distribution at the exposed side of the body was measured at a distance no greater than 5.0 mm from the inner surface of the shell. The area covered the entire dimension of the device-head interface and the horizontal grid resolution was 15mm and 15mm for frequencies < 3 GHz in the x and y directions respectively. When applicable, for frequencies above 3 GHz, a 10 mm by 10 mm resolution was used.
2. The point SAR measurement was taken at the maximum SAR region determined from Step 1 to enable the monitoring of SAR fluctuations/drifts during the 1 gram cube evaluation. SAR at this fixed point was measured and used as a reference value.
3. Based on the area scan data, the peak area of the maximum absorption was determined by spline interpolation. Around this point, a volume of 32mm x 32mm x 30mm (fine resolution volume scan, zoom scan) was assessed by measuring at least 5 x 5 x 7 points. On this basis of this data set, the spatial peak SAR value was evaluated with the following procedure (see references or the DASY manual online for more details):
 - a. The data was extrapolated to the surface of the outer-shell of the phantom. The combined distance extrapolated was the combined distance from the center of the dipoles 2.7mm away from the tip of the probe housing plus the 1.2 mm distance between the surface and the lowest measuring point. The extrapolation was based on a least-squares algorithm. A polynomial of the fourth order was calculated through the points in the z-axis (normal to the phantom shell).
 - b. After the maximum interpolated values were calculated between the points in the cube, the SAR was averaged over the spatial volume (1g or 10g) using a 3D-Spline interpolation algorithm. The 3D-spline is composed of three one-dimensional splines with the "Not a knot" condition (in x, y, and z directions). The volume was then integrated with the trapezoidal algorithm. One thousand points (10 x 10 x 10) were obtained through interpolation, in order to calculate the averaged SAR.
 - c. All neighboring volumes were evaluated until no neighboring volume with a higher average value was found.
4. The SAR reference value, at the same location as step 2, was re-measured after the zoom scan was complete to calculate the SAR drift. If the drift deviated by more than 5%, the SAR test and drift measurements were repeated.

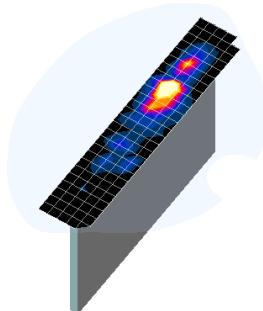


Figure 4-1
Sample SAR Area Scan

| | | | |
|---|---|--|---|
| IC Cert No: N7NMC8355 (Integrated in Panasonic CF-19mk6) |  PCTEST Environmental Engineering | SAR EVALUATION REPORT | Reviewed by: Quality Manager |
| Document S/N: 0Y1206280879.N7N | Test Dates: 05/15/12 - 05/21/12 | DUT Type: Module in Portable Convertible Tablet Laptop Computer | Page 7 of 25 REV. 11.3 M 04/23/2012 |

5 FCC RF EXPOSURE LIMITS

5.1 Uncontrolled Environment

UNCONTROLLED ENVIRONMENTS are defined as locations where there is the exposure of individuals who have no knowledge or control of their exposure. The general population/uncontrolled exposure limits are applicable to situations in which the general public may be exposed or in which persons who are exposed as a consequence of their employment may not be made fully aware of the potential for exposure or cannot exercise control over their exposure. Members of the general public would come under this category when exposure is not employment-related; for example, in the case of a wireless transmitter that exposes persons in its vicinity.

5.2 Controlled Environment

CONTROLLED ENVIRONMENTS are defined as locations where there is exposure that may be incurred by persons who are aware of the potential for exposure, (i.e. as a result of employment or occupation). In general, occupational/controlled exposure limits are applicable to situations in which persons are exposed as a consequence of their employment, who have been made fully aware of the potential for exposure and can exercise control over their exposure. This exposure category is also applicable when the exposure is of a transient nature due to incidental passage through a location where the exposure levels may be higher than the general population/uncontrolled limits, but the exposed person is fully aware of the potential for exposure and can exercise control over his or her exposure by leaving the area or by some other appropriate means.

Table 5-1
SAR Human Exposure Specified in ANSI/IEEE C95.1-1992 and Health Canada Safety Code 6

| HUMAN EXPOSURE LIMITS | | |
|---|---|---|
| | UNCONTROLLED ENVIRONMENT <i>General Population</i> (W/kg) or (mW/g) | CONTROLLED ENVIRONMENT <i>Occupational</i> (W/kg) or (mW/g) |
| SPATIAL PEAK SAR Brain | 1.6 | 8.0 |
| SPATIAL AVERAGE SAR Whole Body | 0.08 | 0.4 |
| SPATIAL PEAK SAR Hands, Feet, Ankles, Wrists | 4.0 | 20 |

1. The Spatial Peak value of the SAR averaged over any 1 gram of tissue (defined as a tissue volume in the shape of a cube) and over the appropriate averaging time.
2. The Spatial Average value of the SAR averaged over the whole body.
3. The Spatial Peak value of the SAR averaged over any 10 grams of tissue (defined as a tissue volume in the shape of a cube) and over the appropriate averaging time.

| | | | |
|---|---|--|---------------------------------|
| IC Cert No: N7NMC8355 (Integrated in Panasonic CF-19mk6) |  | SAR EVALUATION REPORT | Reviewed by: Quality Manager |
| Document S/N: 0Y1206280879.N7N | Test Dates: 05/15/12 - 05/21/12 | DUT Type: Module in Portable Convertible Tablet Laptop Computer | Page 8 of 25 |

6 SAR TABLET TESTING

6.1 SAR Testing for Tablet per KDB Publication 447498 Section 4

Lap-touching devices that have transmitting antennas located less than 20 cm from the body of the user require routine SAR evaluation. Such devices are considered portable, and are capable of being held to the body. Devices are to be setup according to KDB publication 447498 requirements and are configured with maximum output power during SAR assessment for a worst-case SAR evaluation.

Per KDB 447498 4) b) i), the bottom face (back of the device) is required to be tested touching the flat phantom.

Per KDB Publication 447498 4) b) ii) (2), SAR testing applies for the tablet edges with antennas located within 5 cm of each tablet edge closest to the user. According to KDB Publication 447498 4) b) ii) (2), for each antenna, SAR is only required for the edge with the most conservative exposure condition. Since the diagonal dimension of the device is more than 20 cm (33.4 cm), this device is a tablet.

6.2 Display Orientation Capabilities

This device is capable of multiple display orientations supporting both portrait and landscape positions. Therefore per KDB 447498 4) b) ii) (2), SAR testing applies for the tablet edges with antennas located within 5 cm of each tablet edge closest to the user. According to KDB 447498 4) b) ii) (2), for each antenna, SAR is only required for the edge with the most conservative exposure condition.

| | | | |
|---|--|--|---|
| IC Cert No: N7NMC8355 (Integrated in Panasonic CF-19mk6) |  PCTEST Environmental Engineering Inc. | SAR EVALUATION REPORT | |
| Document S/N: 0Y1206280879.N7N | Test Dates: 05/15/12 - 05/21/12 | DUT Type: Module in Portable Convertible Tablet Laptop Computer | Reviewed by: Quality Manager Page 9 of 25 |

Power measurements were performed using a base station simulator under digital average power.

7.1 Procedures Used to Establish RF Signal for SAR

The following procedures are according to FCC KDB Publication 941225 D01 "SAR Measurement Procedures for 3G Devices" v02, October 2007.

The device was placed into a simulated call using a base station simulator in a RF shielded chamber. Establishing connections in this manner ensure a consistent means for testing SAR and are recommended for evaluating SAR [4]. Devices under test were evaluated prior to testing, with a fully charged battery and were configured to operate at maximum output power. In order to verify that the device was tested throughout the SAR test at maximum output power, the SAR measurement system measures a "point SAR" at an arbitrary reference point at the start and end of the 1 gram SAR evaluation, to assess for any power drifts during the evaluation. If the power drift deviated by more than 5%, the SAR test and drift measurements were repeated.

7.2 SAR Measurement Conditions for CDMA2000

The following procedures were performed according to FCC KDB Publication 941225 D01 "SAR Measurement Procedures for 3G Devices" v02, October 2007.

7.2.1 Output Power Verification

See 3GPP2 C.S0011/TIA-98-E as recommended by "SAR Measurement Procedures for 3G Devices" v02, October 2007. Maximum output power is verified on the High, Middle and Low channels according to procedures in section 4.4.5.2 of 3GPP2 C.S0011/TIA-98-E. SO55 tests were measured with power control bits in the "All Up" condition.

1. If the mobile station (MS) supports Reverse TCH RC 1 and Forward TCH RC 1, set up a call using Fundamental Channel Test Mode 1 (RC=1/1) with 9600 bps data rate only.
2. Under RC1, C.S0011 Table 4.4.5.2-1, Table 7-1 parameters were applied.
3. If the MS supports the RC 3 Reverse FCH, RC3 Reverse SCH₀ and demodulation of RC 3,4, or 5, set up a call using Supplemental Channel Test Mode 3 (RC 3/3) with 9600 bps Fundamental Channel and 9600 bps SCH₀ data rate.
4. Under RC3, C.S0011 Table 4.4.5.2-2, Table 7-2 was applied.
5. FCHs were configured at full rate for maximum SAR with "All Up" power control bits.

Table 7-1
Parameters for Max. Power for RC1

| Parameter | Units | Value |
|--------------------------------------|--------------|-------|
| $\frac{I_{or}}{I_{or}}$ | dBm/1.23 MHz | -104 |
| $\frac{\text{Pilot } E_c}{I_{or}}$ | dB | -7 |
| $\frac{\text{Traffic } E_c}{I_{or}}$ | dB | -7.4 |

Table 7-2
Parameters for Max. Power for RC3

| Parameter | Units | Value |
|--------------------------------------|--------------|-------|
| $\frac{I_{or}}{I_{or}}$ | dBm/1.23 MHz | -86 |
| $\frac{\text{Pilot } E_c}{I_{or}}$ | dB | -7 |
| $\frac{\text{Traffic } E_c}{I_{or}}$ | dB | -7.4 |

7.2.2 Body SAR Measurements for EVDO Data Devices

Body SAR is measured using Subtype 0/1 Physical Layer configurations for Rev. 0. SAR for Subtype 2 Physical layer configurations is not required for Rev. A when the maximum average output of each RF channels is less than that measured in Subtype 0/1 Physical layer configurations. Otherwise, SAR is measured on the maximum output channel for Rev. A using the exposure configuration that results in the highest SAR for the RF channels in Rev. 0. The AT is

| | | | |
|---|---|--|---------------------------------|
| IC Cert No: N7NMC8355 (Integrated in Panasonic CF-19mk6) |  | SAR EVALUATION REPORT | Reviewed by: Quality Manager |
| Document S/N: 0Y1206280879.N7N | Test Dates: 05/15/12 - 05/21/12 | DUT Type: Module in Portable Convertible Tablet Laptop Computer | Page 10 of 25 |

tested with a Reverse Data Channel rate of 153.6 kbps in Subtype 0/1 Physical Layer configurations; and a Reverse Data Channel payload size of 4096 bits and Termination Target of 16 slots in Subtype 2 Physical Layer configurations. Both FTAP and FETAP are configured with a Forward Traffic Channel data rate corresponding to the 2-slot version of 307.2 kbps with the ACK Channel transmitting in all slots. AT power control should be in "All Bits Up" conditions for TAP/ETAP. For Ev-Do devices that also support 1x RTT data operations, SAR is not required for 1x RTT when the maximum average output of each channel is less than 1/4 dB higher than that measured in Subtype 0/1 Physical Layer configurations for Rev.0. Otherwise, the body SAR measurements procedures for CDMA Handsets should be applied (See Sections 7.2.3).

7.2.3 Body SAR Measurements for CDMA2000 1x

SAR for body exposure configurations is measured in RC3 with the DUT configured to transmit at full rate on FCH with all other code channels disabled using TDSO / SO32. SAR for multiple code channels (FCH + SCHn) is not required when the maximum average output of each RF channel is less than 1/4 dB higher than that measured with FCH only. Otherwise, SAR is measured on the maximum output channel (FCH + SCHn) with FCH at full rate and SCH0 enabled at 9600 bps using the exposure configuration that results in the highest SAR for that channel with FCH only. When multiple code channels are enabled, the DUT output may shift by more than 0.5 dB and lead to higher SAR drifts and SCH dropouts. Body SAR was measured using TDSO / SO32 with power control bits in the "All Up." Body SAR in RC1 is not required when the maximum average output of each channel is less than 1/4 dB higher than that measured in RC3.

7.3 SAR Measurement Conditions for WCDMA

7.3.1 Output Power Verification

Maximum output power is measured on the High, Middle and Low channels for each applicable transmission band according to the general descriptions in section 5.2 of 3GPP TS 34.121, using the appropriate RMC or AMR with TPC (transmit power control) set to all "1s".

Maximum output power is verified on the High, Middle and Low channels according to the general descriptions in section 5.2 of 3GPP TS 34.121 (release 5), using the appropriate RMC with TPC (transmit power control) set to all "1s". Results for all applicable physical channel configurations (DPCCH, DPDCHn and spreading codes, HS-DPCCH) are tabulated in the test report. All configurations that are not supported by the DUT or cannot be measured due to technical or equipment limitations is identified.

7.3.2 Body SAR Measurements

SAR for body exposure configurations is measured using the 12.2 kbps RMC with the TPC bits all "1s".

7.3.3 Procedures Used to Establish RF Signal for SAR HSDPA Data Devices

The following procedures are applicable to HSDPA data devices operating under 3GPP Release 5. Body exposure conditions are typically applicable to these devices, including handsets and data modems operating in various electronic devices. HSDPA operates in conjunction with WCDMA and requires an active DPCCH. The default test configuration is to measure SAR in WCDMA without HSDPA, with an established radio link between the DUT and a communication test set with 12.2 kbps RMC mode configured in Test Loop Mode 1; and tested with HSDPA with FRC and a 12.2 kbps RMC using the highest SAR configuration in WCDMA. SAR is selectively confirmed for other

| | | | |
|---|--|--|---------------------------------|
| IC Cert No: N7NMC8355 (Integrated in Panasonic CF-19mk6) |  PCTEST Engineering Laboratory, Inc. | SAR EVALUATION REPORT | Reviewed by: Quality Manager |
| Document S/N: 0Y1206280879.N7N | Test Dates: 05/15/12 - 05/21/12 | DUT Type: Module in Portable Convertible Tablet Laptop Computer | Page 11 of 25 |

physical channel configurations according to output power, exposure conditions and device operating capabilities. Maximum output power is verified according to 3GPP TS 23.121 (Release 5) and SAR must be measured according to these maximum output conditions.

7.3.4 SAR Measurement Conditions for HSUPA Data Devices

SAR for body exposure configurations are measured according to the 'Body SAR Measurements' procedures in the 'WCDMA Handsets' section of the KDB 941225 D01 FCC 3G document. In addition, Body SAR is also measured for HSPA when the maximum average output of each RF channel with HSPA active is at least $\frac{1}{4}$ dB higher of that measured without HSPA in 12.2 kbps RMC mode or the maximum SAR for 12.2 kbps RMC is above 75% of the SAR limit. Body SAR for HSPA is measured with E-DCH Sub-test 5, using H-Set 1 and QPSK for FRC and a 12.2 kbps RMC configured in Test Loop Mode 1 with power control algorithm 2, according to the highest body SAR configuration in 12.2 kbps RMC without HSPA. When VOIP is applicable for head exposure, SAR is not required when the maximum output of each RF channel with HSPA is less than $\frac{1}{4}$ dB higher than that measured using 12.2 kbps RMC; otherwise, the same HSPA configuration used for body measurements should be used to test for head exposure.

Due to inner loop power control requirements in HSPA, a commercial communication test set should be used for the output power and SAR tests. The 12.2 kbps RMC, FRC H-set 1 and EDCH configurations for HSPA should be configured according to the β values indicated below as well as other applicable procedures described in the 'WCDMA Handset' and 'Release 5 HSDPA Data Devices' sections of the FCC 3G document.

| Sub-test | β_c | β_d | β_d (SF) | β_c/β_d | $\beta_{hs}^{(1)}$ | β_{ec} | β_{ed} | β_{ed} (SF) | β_{ed} (codes) | CM ⁽²⁾ (dB) | MPR (dB) | AG ⁽⁴⁾ Index | E-TFCI |
|----------|----------------------|----------------------|-------------------|----------------------|--------------------|--------------|--|----------------------|-------------------------|---------------------------|-------------|----------------------------|--------|
| 1 | 11/15 ⁽³⁾ | 15/15 ⁽³⁾ | 64 | 11/15 ⁽³⁾ | 22/15 | 209/225 | 1039/225 | 4 | 1 | 1.0 | 0.0 | 20 | 75 |
| 2 | 6/15 | 15/15 | 64 | 6/15 | 12/15 | 12/15 | 94/75 | 4 | 1 | 3.0 | 2.0 | 12 | 67 |
| 3 | 15/15 | 9/15 | 64 | 15/9 | 30/15 | 30/15 | $\beta_{ed1}: 47/15$ $\beta_{ed2}: 47/15$ | 4 | 2 | 2.0 | 1.0 | 15 | 92 |
| 4 | 2/15 | 15/15 | 64 | 2/15 | 4/15 | 2/15 | 56/75 | 4 | 1 | 3.0 | 2.0 | 17 | 71 |
| 5 | 15/15 ⁽⁴⁾ | 15/15 ⁽⁴⁾ | 64 | 15/15 ⁽⁴⁾ | 30/15 | 24/15 | 134/15 | 4 | 1 | 1.0 | 0.0 | 21 | 81 |

Note 1: Δ_{ACK} , Δ_{NACK} and $\Delta_{CQI} = 8 \Leftrightarrow \beta_{hs} = \beta_c/\beta_d = 30/15 \Leftrightarrow \beta_{hs} = 30/15 * \beta_c$.
 Note 2: CM = 1 for $\beta_c/\beta_d = 12/15$, $\beta_c/\beta_d = 24/15$. For all other combinations of DPDCH, DPCCH, HS-DPCCH, E-DPDCH and E-DPCCH the MPR is based on the relative CM difference.
 Note 3: For subtest 1 the β_c/β_d ratio of 11/15 for the TFC during the measurement period (TF1, TF0) is achieved by setting the signaled gain factors for the reference TFC (TF1, TF1) to $\beta_c = 10/15$ and $\beta_d = 15/15$.
 Note 4: For subtest 5 the β_c/β_d ratio of 15/15 for the TFC during the measurement period (TF1, TF0) is achieved by setting the signaled gain factors for the reference TFC (TF1, TF1) to $\beta_c = 14/15$ and $\beta_d = 15/15$.
 Note 5: Testing UE using E-DPDCH Physical Layer category 1 Sub-test 3 is not required according to TS 25.306 Table 5.1g.
 Note 6: β_{ed} can not be set directly; it is set by Absolute Grant Value.

| | | | | | | |
|---|---|--|--|--|--|---------------------------------|
| IC Cert No: N7NMC8355 (Integrated in Panasonic CF-19mk6) |  PCTEST Engineering Laboratory Inc. | SAR EVALUATION REPORT | | | | Reviewed by: Quality Manager |
| Document S/N: 0Y1206280879.N7N | Test Dates: 05/15/12 - 05/21/12 | DUT Type: Module in Portable Convertible Tablet Laptop Computer | | | | |

8 RF CONDUCTED POWERS

8.1 CDMA Conducted Powers

| Band | Channel | Frequency | TDSO SO32 [dBm] | TDSO SO32 [dBm] | 1x EvDO Rev. 0 [dBm] | 1x EvDO Rev. A [dBm] |
|----------|---------|-----------|-----------------|-----------------|----------------------|----------------------|
| | F-RC | MHz | FCH+SCH | FCH | (RTAP) | (RETAP) |
| Cellular | 1013 | 824.7 | 24.16 | 24.17 | 24.22 | 24.21 |
| | 384 | 836.52 | 24.08 | 24.09 | 24.33 | 24.31 |
| | 777 | 848.31 | 23.83 | 23.84 | 24.02 | 24.01 |
| PCS | 25 | 1851.25 | 24.10 | 24.21 | 24.36 | 24.34 |
| | 600 | 1880 | 24.06 | 24.13 | 24.14 | 24.13 |
| | 1175 | 1908.75 | 24.12 | 24.14 | 24.28 | 24.22 |

Per KDB Publication 941225 D01:

1. Body SAR was evaluated with EVDO Rev 0. SAR was not required for 1x RTT, because the maximum average output of each channel is less than 1/4 dB higher than that measured in Subtype 0/1 Physical Layer configurations for Rev. 0. SAR for Subtype 2 Physical layer configurations was not required for Rev. A because the maximum average output of each RF channel is less than that measured in Subtype 0/1 Physical layer configurations
2. The bolded modes were tested for SAR.




Figure 8-1
Power Measurement Setup

| | | | | |
|---|---|--|--|---------------------------------|
| IC Cert No: N7NMC8355 (Integrated in Panasonic CF-19mk6) |  | SAR EVALUATION REPORT | | Reviewed by: Quality Manager |
| Document S/N: 0Y1206280879.N7N | Test Dates: 05/15/12 - 05/21/12 | DUT Type: Module in Portable Convertible Tablet Laptop Computer | | Page 13 of 25 |

8.2 GSM Conducted Powers

| | | Maximum Burst-Averaged Output Power | | | |
|----------|---------|--|-------------------------|-------------------------|-------------------------|
| | | GPRS/EDGE Data (GMSK) | | EDGE Data (8-PSK) | |
| Band | Channel | GPRS [dBm] 1 Tx Slot | GPRS [dBm] 2 Tx Slot | EDGE [dBm] 1 Tx Slot | EDGE [dBm] 2 Tx Slot |
| Cellular | 128 | 32.93 | 32.84 | 27.00 | 26.86 |
| | 190 | 33.02 | 32.95 | 27.14 | 27.01 |
| | 251 | 33.11 | 33.05 | 27.20 | 27.10 |
| PCS | 512 | 30.05 | 29.84 | 26.11 | 26.06 |
| | 661 | 29.95 | 29.80 | 26.10 | 26.03 |
| | 810 | 30.07 | 30.00 | 26.23 | 26.12 |
| | | Calculated Maximum Frame-Averaged Output Power | | | |
| | | GPRS/EDGE Data (GMSK) | | EDGE Data (8-PSK) | |
| Band | Channel | GPRS [dBm] 1 Tx Slot | GPRS [dBm] 2 Tx Slot | EDGE [dBm] 1 Tx Slot | EDGE [dBm] 2 Tx Slot |
| Cellular | 128 | 23.90 | 26.82 | 17.97 | 20.84 |
| | 190 | 23.99 | 26.93 | 18.11 | 20.99 |
| | 251 | 24.08 | 27.03 | 18.17 | 21.08 |
| PCS | 512 | 21.02 | 23.82 | 17.08 | 20.04 |
| | 661 | 20.92 | 23.78 | 17.07 | 20.01 |
| | 810 | 21.04 | 23.98 | 17.20 | 20.10 |

Notes:

1. Both burst-averaged and calculated frame-averaged powers are included. Frame-averaged power was calculated from the measured burst-averaged power by converting the slot powers into linear units and calculating the energy over 8 timeslots.
2. The bolded GPRS modes were selected according to the highest frame-averaged output power table according to KDB 941225 D03.
3. CS1 coding scheme was used in GPRS output power measurements and SAR Testing, as a condition where GMSK modulation was ensured. It was investigated that CS1 - CS4 settings do not have any impact on the output levels in the GPRS modes.
4. MCS7 coding scheme was used to measure the output powers for EDGE since it was investigated that choosing MCS7 coding scheme will ensure 8-PSK modulation, MCS levels that produce 8PSK modulation do not have an impact on output power.

GSM Class: C (Data Only)
GPRS Multislot class: 10 (max 2 Tx Uplink slots)
EDGE Multislot class: 10 (max 2Tx Uplink slots)
DTM Multislot Class: N/A



Figure 8-2
Power Measurement Setup

| | | | |
|---|---|--|---------------------------------|
| IC Cert No: N7NMC8355 (Integrated in Panasonic CF-19mk6) |  | SAR EVALUATION REPORT | Reviewed by: Quality Manager |
| Document S/N: 0Y1206280879.N7N | Test Dates: 05/15/12 - 05/21/12 | DUT Type: Module in Portable Convertible Tablet Laptop Computer | Page 14 of 25 |

8.3 HSPA Conducted Powers

| 3GPP Release Version | Mode | 3GPP 34.121 Subtest | Cellular Band [dBm] | | | AWS Band [dBm] | | | PCS Band [dBm] | | | MPR [dB] |
|----------------------|-------|---------------------|---------------------|-------|-------|----------------|-------|-------|----------------|-------|-------|----------|
| | | | 4132 | 4183 | 4233 | 1312 | 1412 | 1862 | 9262 | 9400 | 9538 | |
| 99 | WCDMA | 12.2 kbps RMC | 24.39 | 24.41 | 24.38 | 24.63 | 24.43 | 24.45 | 24.53 | 24.81 | 24.50 | - |
| 6 | HSDPA | Subtest 1 | 23.85 | 23.85 | 23.77 | 24.02 | 23.91 | 23.94 | 24.15 | 24.31 | 23.96 | 0 |
| 6 | | Subtest 2 | 23.86 | 23.92 | 23.90 | 24.00 | 23.97 | 23.87 | 24.17 | 24.35 | 24.05 | 0 |
| 6 | | Subtest 3 | 23.37 | 23.42 | 23.38 | 23.51 | 23.48 | 23.37 | 23.72 | 23.84 | 23.50 | 0.5 |
| 6 | | Subtest 4 | 23.34 | 23.37 | 23.32 | 23.63 | 23.58 | 23.42 | 23.74 | 23.90 | 23.65 | 0.5 |
| 6 | HSUPA | Subtest 1 | 23.50 | 23.57 | 23.70 | 24.11 | 23.69 | 23.73 | 23.88 | 24.15 | 23.55 | 0 |
| 6 | | Subtest 2 | 22.16 | 22.17 | 22.18 | 22.45 | 22.37 | 22.35 | 22.60 | 22.80 | 22.55 | 2 |
| 6 | | Subtest 3 | 22.70 | 22.44 | 22.80 | 22.86 | 22.67 | 22.62 | 22.90 | 23.10 | 22.87 | 1 |
| 6 | | Subtest 4 | 22.46 | 22.53 | 22.60 | 22.62 | 22.89 | 22.47 | 22.96 | 23.20 | 22.63 | 2 |
| 6 | | Subtest 5 | 23.60 | 23.69 | 23.62 | 23.78 | 23.70 | 23.95 | 23.93 | 24.30 | 23.80 | 0 |

WCDMA SAR was tested under RMC 12.2 kbps with HSPA Inactive per KDB Publication 941225 D01.

HSPA SAR was not required since the average output power of the HSPA subtests was not more than 0.25 dB higher than the RMC level and SAR was less than 1.2 W/kg.

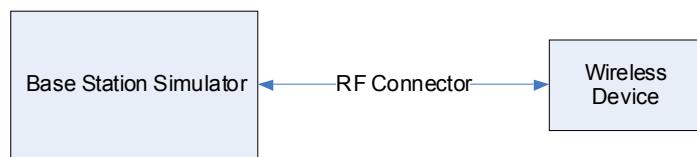


Figure 8-3
Power Measurement Setup

| | | | | | |
|---|--|--|--|--|---------------------------------|
| IC Cert No: N7NMC8355 (Integrated in Panasonic CF-19mk6) |  PCTEST Engineering Laboratory, Inc. | SAR EVALUATION REPORT | | | Reviewed by: Quality Manager |
| Document S/N: 0Y1206280879.N7N | Test Dates: 05/15/12 - 05/21/12 | DUT Type: Module in Portable Convertible Tablet Laptop Computer | | | |

9 SYSTEM VERIFICATION

9.1 Tissue Verification

Table 9-1
Measured Tissue Properties

| Calibrated for Tests Performed on: | Tissue Type | Tissue Temp During Calibration (C°) | Measured Frequency (MHz) | Measured Conductivity, σ (S/m) | Measured Dielectric Constant, ϵ | TARGET Conductivity, σ (S/m) | TARGET Dielectric Constant, ϵ | % dev σ | % dev ϵ |
|------------------------------------|-------------|-------------------------------------|--------------------------|---------------------------------------|--|-------------------------------------|--|----------------|------------------|
| 05/21/2012 | 835B | 22.8 | 820 | 0.955 | 53.19 | 0.97 | 55.28 | -1.44% | -3.79% |
| | | | 835 | 0.972 | 52.99 | 0.97 | 55.20 | 0.21% | -4.00% |
| | | | 850 | 0.986 | 52.95 | 0.99 | 55.15 | -0.20% | -4.00% |
| 05/21/2012 | 1750B | 22.6 | 1710 | 1.465 | 52.85 | 1.46 | 53.54 | 0.34% | -1.29% |
| | | | 1750 | 1.508 | 52.56 | 1.49 | 53.43 | 1.21% | -1.63% |
| | | | 1790 | 1.564 | 52.20 | 1.51 | 53.33 | 3.58% | -2.12% |
| 05/15/2012 | 1900B | 23.0 | 1850 | 1.475 | 51.89 | 1.52 | 53.30 | -2.96% | -2.65% |
| | | | 1880 | 1.511 | 51.79 | 1.52 | 53.30 | -0.59% | -2.83% |
| | | | 1910 | 1.538 | 51.77 | 1.52 | 53.30 | 1.18% | -2.87% |
| 05/16/2012 | 1900B | 22.5 | 1850 | 1.466 | 51.09 | 1.52 | 53.30 | -3.55% | -4.15% |
| | | | 1880 | 1.502 | 50.96 | 1.52 | 53.30 | -1.18% | -4.39% |
| | | | 1910 | 1.534 | 50.88 | 1.52 | 53.30 | 0.92% | -4.54% |

Note: KDB Publication 450824 was ensured to be applied for probe calibration frequencies greater than or equal to 50 MHz of the DUT frequencies.

The above measured tissue parameters were used in the DASY software to perform interpolation via the DASY software to determine actual dielectric parameters at the test frequencies (per IEEE 1528 6.6.1.2). The SAR test plots may slightly differ from the table above since the DASY software rounds to three significant digits.

9.2 Measurement Procedure for Tissue verification

- 1) The network analyzer and probe system was configured and calibrated.
- 2) The probe was immersed in the sample which was placed in a nonmetallic container. Trapped air bubbles beneath the flange were minimized by placing the probe at a slight angle.
- 3) The complex admittance with respect to the probe aperture was measured
- 4) The complex relative permittivity ϵ can be calculated from the below equation (Pournaropoulos and Misra):

$$Y = \frac{j2\omega\epsilon_r\epsilon_0}{[\ln(b/a)]^2} \int_a^b \int_a^b \int_0^\pi \cos\phi' \frac{\exp[-j\omega r(\mu_0\epsilon_r\epsilon_0)^{1/2}]}{r} d\phi' d\rho' d\rho$$

where Y is the admittance of the probe in contact with the sample, the primed and unprimed coordinates refer to source and observation points, respectively, $r^2 = \rho^2 + \rho'^2 - 2\rho\rho'\cos\phi'$, ω is the angular frequency, and $j = \sqrt{-1}$.

| | | | | |
|---|--|--|--|---------------------------------|
| IC Cert No: N7NMC8355 (Integrated in Panasonic CF-19mk6) |  PCTEST [®] ENVIRONMENTAL LABORATORY INC. | SAR EVALUATION REPORT | | Reviewed by: Quality Manager |
| Document S/N: 0Y1206280879.N7N | Test Dates: 05/15/12 - 05/21/12 | DUT Type: Module in Portable Convertible Tablet Laptop Computer | | Page 16 of 25 |

9.3 Test System Verification

Prior to assessment, the system is verified to $\pm 10\%$ of the manufacturer SAR measurement on the reference dipole at the time of calibration.

Table 9-2
System Verification Results

| System Verification TARGET & MEASURED | | | | | | | | | | | |
|--|-------------|------------|----------------|------------------|-----------------|-----------|----------|----------------------------|------------------------------|----------------------------------|---------------|
| Tissue Frequency (MHz) | Tissue Type | Date: | Amb. Temp (°C) | Liquid Temp (°C) | Input Power (W) | Dipole SN | Probe SN | Measured SAR_{1g} (W/kg) | 1 W Target SAR_{1g} (W/kg) | 1 W Normalized SAR_{1g} (W/kg) | Deviation (%) |
| 835 | Body | 05/21/2012 | 23.9 | 22.4 | 0.250 | 4d047 | 3561 | 2.47 | 9.410 | 9.880 | 4.99% |
| 1750 | Body | 05/21/2012 | 23.4 | 22.2 | 0.100 | 1051 | 3022 | 3.72 | 37.600 | 37.200 | -1.06% |
| 1900 | Body | 05/15/2012 | 24.2 | 22.7 | 0.100 | 5d080 | 3209 | 4.17 | 40.900 | 41.700 | 1.96% |
| 1900 | Body | 05/16/2012 | 24.3 | 23.2 | 0.100 | 5d149 | 3561 | 4.18 | 39.300 | 41.800 | 6.36% |

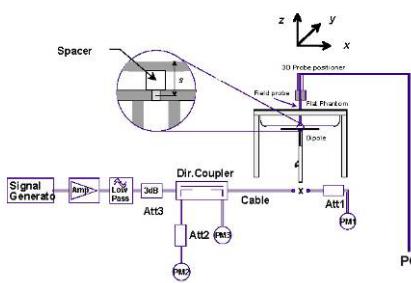


Figure 9-1
System Verification Setup Diagram



Figure 9-2
System Verification Setup Photo

| | | | |
|---|--|--|---------------------------------|
| IC Cert No: N7NMC8355 (Integrated in Panasonic CF-19mk6) |  PCTEST [®] ENVIRONMENTAL LABORATORY INC. | SAR EVALUATION REPORT | Reviewed by: Quality Manager |
| Document S/N: 0Y1206280879.N7N | Test Dates: 05/15/12 - 05/21/12 | DUT Type: Module in Portable Convertible Tablet Laptop Computer | Page 17 of 25 |

10 SAR DATA SUMMARY

10.1 Standalone Body SAR Data

Table 10-1
Licensed Transmitter Body SAR Results

| MEASUREMENT RESULTS | | | | | | | | | | |
|--|------|------------|-------------|-----------------------|------------------|---------|----------------------|-----------------|------|--------------------|
| FREQUENCY | | Mode | Service | Conducted Power [dBm] | Power Drift [dB] | Spacing | Device Serial Number | # of GPRS Slots | Side | SAR (1g) (W/kg) |
| MHz | Ch. | | | | | | | | | |
| 836.60 | 190 | GSM 850 | GPRS | 32.95 | 0.15 | 0.0 cm | 2CKSA00021 | 2 | back | 0.093 |
| 836.60 | 190 | GSM 850 | GPRS | 32.95 | 0.09 | 0.0 cm | 2CKSA00021 | 2 | top | 0.172 |
| 836.60 | 190 | GSM 850 | GPRS | 32.95 | -0.01 | 0.0 cm | 2CKSA00021 | 2 | left | 0.620 |
| 836.60 | 4183 | WCDMA 850 | RMC | 24.41 | -0.12 | 0.0 cm | 2CKSA00021 | N/A | back | 0.050 |
| 836.60 | 4183 | WCDMA 850 | RMC | 24.41 | -0.03 | 0.0 cm | 2CKSA00021 | N/A | top | 0.105 |
| 836.60 | 4183 | WCDMA 850 | RMC | 24.41 | 0.08 | 0.0 cm | 2CKSA00021 | N/A | left | 0.376 |
| 836.52 | 384 | Cell. CDMA | EVDO Rev. 0 | 24.33 | -0.06 | 0.0 cm | 2CKSA00021 | N/A | back | 0.049 |
| 836.52 | 384 | Cell. CDMA | EVDO Rev. 0 | 24.33 | 0.19 | 0.0 cm | 2CKSA00021 | N/A | top | 0.071 |
| 836.52 | 384 | Cell. CDMA | EVDO Rev. 0 | 24.33 | -0.14 | 0.0 cm | 2CKSA00021 | N/A | left | 0.434 |
| 1730.40 | 1412 | AWS WCDMA | RMC | 24.43 | -0.15 | 0.0 cm | 2CKSA00021 | N/A | back | 0.058 |
| 1730.40 | 1412 | AWS WCDMA | RMC | 24.43 | 0.00 | 0.0 cm | 2CKSA00021 | N/A | top | 0.421 |
| 1730.40 | 1412 | AWS WCDMA | RMC | 24.43 | -0.06 | 0.0 cm | 2CKSA00021 | N/A | left | 0.617 |
| 1880.00 | 661 | GSM 1900 | GPRS | 29.80 | 0.04 | 0.0 cm | 2CKSA00021 | 2 | back | 0.055 |
| 1880.00 | 661 | GSM 1900 | GPRS | 29.80 | -0.12 | 0.0 cm | 2CKSA00021 | 2 | top | 0.163 |
| 1880.00 | 661 | GSM 1900 | GPRS | 29.80 | -0.18 | 0.0 cm | 2CKSA00021 | 2 | left | 0.424 |
| 1880.00 | 9400 | WCDMA 1900 | RMC | 24.81 | 0.21 | 0.0 cm | 2CKSA00021 | N/A | back | 0.096 |
| 1880.00 | 9400 | WCDMA 1900 | RMC | 24.81 | -0.05 | 0.0 cm | 2CKSA00021 | N/A | top | 0.286 |
| 1880.00 | 9400 | WCDMA 1900 | RMC | 24.81 | 0.18 | 0.0 cm | 2CKSA00021 | N/A | left | 0.717 |
| 1880.00 | 600 | PCS CDMA | EVDO Rev. 0 | 24.14 | 0.17 | 0.0 cm | 2CKSA00021 | N/A | back | 0.105 |
| 1880.00 | 600 | PCS CDMA | EVDO Rev. 0 | 24.14 | -0.20 | 0.0 cm | 2CKSA00021 | N/A | top | 0.259 |
| 1880.00 | 600 | PCS CDMA | EVDO Rev. 0 | 24.14 | -0.01 | 0.0 cm | 2CKSA00021 | N/A | left | 0.662 |
| ANSI / IEEE C95.1 1992 - SAFETY LIMIT | | | | | | | Body | | | |
| Spatial Peak | | | | | | | 1.6 W/kg (mW/g) | | | |
| Uncontrolled Exposure/General Population | | | | | | | averaged over 1 gram | | | |

| | | | | | | |
|---|---|--|--|--|--|---------------------------------|
| IC Cert No: N7NMC8355 (Integrated in Panasonic CF-19mk6) |  | SAR EVALUATION REPORT | | | | Reviewed by: Quality Manager |
| Document S/N: 0Y1206280879.N7N | Test Dates: 05/15/12 - 05/21/12 | DUT Type: Module in Portable Convertible Tablet Laptop Computer | | | | Page 18 of 25 |

10.2 SAR Test Notes

General Notes:

1. The test data reported are the worst-case SAR value with the position of the device configured for SAR testing according to KDB 447498 Section 4.
2. Batteries are fully charged for all readings.
3. Tissue parameters and temperatures are listed on the SAR plots.
4. The manufacturer has confirmed that the device(s) tested have the same physical, mechanical and thermal characteristics and are within operational tolerances expected for production units.
5. Per FCC KDB Publication 447498, if the SAR measured at the middle channel for each test configuration is at least 3.0 dB lower than the SAR limit, testing at the high and low channels is optional for such test configuration(s).
6. Liquid tissue depth was at least 15.0 cm. To confirm the proper SAR liquid depth, the z-axis plots from the system verifications were included since the system verifications were performed using the same liquid, probe and DAE as the SAR tests in the same time period.
7. Per KDB Publication 447498 4) b) i) the back side is required to be tested touching the flat phantom for large sized tablet devices.
8. This device is capable of multiple display orientations supporting both portrait and landscape positions. Therefore per KDB 447498 4) b) ii) (2), SAR testing applies for the tablet edges with antennas located within 5 cm of each tablet edge closest to the user. According to KDB 447498 4) b) ii) (2), for each antenna, SAR is required for the edge with the most conservative exposure condition.

GSM Notes:

1. Justification for reduced test configurations per KDB Publication 941225 D03: The source-based time-averaged output power was evaluated for all multi-slot operations. Worst case was tested.

WCDMA Notes:

1. WCDMA mode was tested under RMC 12.2 kbps with HSPA Inactive per KDB Publication 941225 D01. HSPA SAR for the body was not required since the average output power of the HSPA subtests was not more than 0.25 dB higher than the RMC level and SAR was less than 1.2 W/kg.
2. AWS WCDMA SAR was measured with a probe calibrated at 1750 MHz and is valid for measuring SAR from \pm 50 MHz. The 1750MHz specific liquid was verified with specific probe calibration factors as required per FCC KDB Publication 450824 D01.

CDMA Notes:

1. CDMA Body SAR is measured using Subtype 0/1 Physical Layer configurations for Rev. 0 according to KDB 941225 D01 procedures for data devices. Since the average output power of Subtype 2 for Rev. A is less than the Rev. 0 power levels, then Rev. A SAR is not required. SAR was not required for 1x RTT for Ev-Do data devices since the maximum average output of each channel is less than 1/4 dB higher than that measured in Subtype 0/1 Physical Layer configurations for Rev. 0.

| | | | |
|---|---|--|---------------------------------|
| IC Cert No: N7NMC8355 (Integrated in Panasonic CF-19mk6) |  PCTEST Environmental Engineering | SAR EVALUATION REPORT | Reviewed by: Quality Manager |
| Document S/N: 0Y1206280879.N7N | Test Dates: 05/15/12 - 05/21/12 | DUT Type: Module in Portable Convertible Tablet Laptop Computer | Page 19 of 25 |

11 SIMULTANEOUS TRANSMISSION SAR ANALYSIS: WWAN+2.4 GHZ WIFI

This device uses a separate module for the WLAN/Bluetooth Transmitter. Please refer to the following WLAN and Bluetooth reports submitted under FCCID: ACJ9TGWL12A. It has been confirmed that the installation of this module provides more than 14 mm from the antenna to the user in this computer; therefore, the maximum SAR value from the original certification [0.399 W/kg] is used for simultaneous transmission purposes.

The separation between the WWAN antenna and the WLAN main and auxiliary WLAN antenna is 282 mm and 35 mm, respectively.

The maximum peak RF conducted power of Bluetooth is 4.00 mW.
The maximum average RF conducted power of WLAN is 49.00 mW.

Per KDB Publication 447498 Bluetooth SAR testing is not required based on the maximum conducted power, the Bluetooth to WWAN and Bluetooth to WLAN antenna separation distance and the Body SAR of the WWAN and WLAN antennas.

| Simult Tx | Configuration | GPRS 850 SAR (W/kg) | WLAN SAR (W/kg) | Σ SAR (W/kg) | Simult Tx | Configuration | WCDMA 850 SAR (W/kg) | WLAN SAR (W/kg) | Σ SAR (W/kg) |
|-----------|---------------|-----------------------|-----------------|---------------------|-----------------|---------------------|-----------------------|-----------------|---------------------|
| Body SAR | Back | 0.093 | 0.399 | 0.492 | Body SAR | Back | 0.050 | 0.399 | 0.449 |
| | Top | 0.172 | 0.399 | 0.571 | | Top | 0.105 | 0.399 | 0.504 |
| | Bottom | - | 0.399 | 0.399 | | Bottom | - | 0.399 | 0.399 |
| | Right | - | 0.399 | 0.399 | | Right | - | 0.399 | 0.399 |
| | Left | 0.620 | 0.390 | 1.010 | | Left | 0.376 | 0.390 | 0.766 |
| Simult Tx | Configuration | Cell. EVDO SAR (W/kg) | WLAN SAR (W/kg) | Σ SAR (W/kg) | Simult Tx | Configuration | AWS WCDMA SAR (W/kg) | WLAN SAR (W/kg) | Σ SAR (W/kg) |
| Body SAR | Back | 0.049 | 0.399 | 0.448 | Body SAR | Back | 0.058 | 0.399 | 0.457 |
| | Top | 0.071 | 0.399 | 0.470 | | Top | 0.421 | 0.399 | 0.820 |
| | Bottom | - | 0.399 | 0.399 | | Bottom | - | 0.399 | 0.399 |
| | Right | - | 0.399 | 0.399 | | Right | - | 0.399 | 0.399 |
| | Left | 0.434 | 0.390 | 0.824 | | Left | 0.617 | 0.390 | 1.007 |
| Simult Tx | Configuration | GPRS 1900 SAR (W/kg) | WLAN SAR (W/kg) | Σ SAR (W/kg) | Simult Tx | Configuration | WCDMA 1900 SAR (W/kg) | WLAN SAR (W/kg) | Σ SAR (W/kg) |
| Body SAR | Back | 0.055 | 0.399 | 0.454 | Body SAR | Back | 0.096 | 0.399 | 0.495 |
| | Top | 0.163 | 0.399 | 0.562 | | Top | 0.286 | 0.399 | 0.685 |
| | Bottom | - | 0.399 | 0.399 | | Bottom | - | 0.399 | 0.399 |
| | Right | - | 0.399 | 0.399 | | Right | - | 0.399 | 0.399 |
| | Left | 0.424 | 0.390 | 0.814 | | Left | 0.717 | 0.390 | 1.107 |
| | | Simult Tx | Configuration | PCS EVDO SAR (W/kg) | WLAN SAR (W/kg) | Σ SAR (W/kg) | | | |
| | | Body SAR | Back | 0.105 | 0.399 | 0.504 | | | |
| | | | Top | 0.259 | 0.399 | 0.658 | | | |
| | | | Bottom | - | 0.399 | 0.399 | | | |
| | | | Right | - | 0.399 | 0.399 | | | |
| | | | Left | 0.662 | 0.390 | 1.052 | | | |

| | | | | | |
|---|---|--|--|--|---------------------------------|
| IC Cert No: N7NMC8355 (Integrated in Panasonic CF-19mk6) |  | SAR EVALUATION REPORT | | | Reviewed by: Quality Manager |
| Document S/N: 0Y1206280879.N7N | Test Dates: 05/15/12 - 05/21/12 | DUT Type: Module in Portable Convertible Tablet Laptop Computer | | | Page 20 of 25 |

12 EQUIPMENT LIST

| Manufacturer | Model | Description | Cal Date | Cal Interval | Cal Due | Serial Number |
|--------------------|-----------------|---|------------|--------------|------------|---------------|
| Agilent | 85070E | Dielectric Probe Kit | 3/8/2012 | Annual | 3/8/2013 | MY44300633 |
| Agilent | 8594A | (9kHz-2.9GHz) Spectrum Analyzer | N/A | | N/A | 3051A00187 |
| Agilent | 8648D | (9kHz-4GHz) Signal Generator | 10/10/2011 | Annual | 10/10/2012 | 3613A00315 |
| Agilent | 8648D | Signal Generator | 4/3/2012 | Annual | 4/3/2013 | 3629U00687 |
| Agilent | 8753E | (30kHz-6GHz) Network Analyzer | 4/4/2012 | Annual | 4/4/2013 | JP38020182 |
| Agilent | 8753E | (30kHz-6GHz) Network Analyzer | 4/3/2012 | Annual | 4/3/2013 | US37390350 |
| Agilent | E5515C | Wireless Communications Test Set | 2/14/2012 | Annual | 2/14/2013 | GB43304447 |
| Agilent | E5515C | Wireless Communications Test Set | 2/12/2012 | Annual | 2/12/2013 | GB45360985 |
| Agilent | E5515C | Wireless Communications Test Set | 2/9/2012 | Annual | 2/9/2013 | GB43460554 |
| Agilent | E8257D | (250kHz-20GHz) Signal Generator | 4/5/2012 | Annual | 4/5/2013 | MY45470194 |
| Amplifier Research | 551G4 | 5W, 800MHz-4.2GHz | CBT | N/A | CBT | 21910 |
| Anritsu | MA2481A | Power Sensor | 2/14/2012 | Annual | 2/14/2013 | 5318 |
| Anritsu | MA2481A | Power Sensor | 2/14/2012 | Annual | 2/14/2013 | 5442 |
| Anritsu | MA2481A | Power Sensor | 2/14/2012 | Annual | 2/14/2013 | 5821 |
| Anritsu | MA2481A | Power Sensor | 2/14/2012 | Annual | 2/14/2013 | 8013 |
| Anritsu | ML2438A | Power Meter | 2/14/2012 | Annual | 2/14/2013 | 98150041 |
| Anritsu | ML2438A | Power Meter | 10/13/2011 | Annual | 10/13/2012 | 1070030 |
| Anritsu | MT8820C | Radio Communication Tester | 11/11/2011 | Annual | 11/11/2012 | 6200901190 |
| COMTECH | AR85729-5/5759B | Solid State Amplifier | CBT | N/A | CBT | M3W1A00-1002 |
| Control Company | 36934-158 | Wall-Mounted Thermometer | 1/4/2012 | Biennial | 1/4/2014 | 122014497 |
| Control Company | 61220-416 | Long-Stem Thermometer | 2/15/2011 | Biennial | 2/15/2013 | 111331322 |
| Control Company | 61220-416 | Long-Stem Thermometer | 7/1/2011 | Biennial | 7/1/2013 | 111642941 |
| Control Company | 61220-416 | Long-Stem Thermometer | 10/12/2011 | Biennial | 10/12/2013 | 111860820 |
| Gigatronics | 80701A | (0.05-18GHz) Power Sensor | 10/12/2011 | Annual | 10/12/2012 | 1833460 |
| Gigatronics | 8651A | Universal Power Meter | 10/12/2011 | Annual | 10/12/2012 | 8650319 |
| Intelligent Weigh | PD-3000 | Electronic Balance | 3/27/2012 | Annual | 3/27/2013 | 11081534 |
| MCL | BW-N6W5+ | 6dB Attenuator | CBT | N/A | CBT | 1139 |
| MiniCircuits | SLP-2400+ | Low Pass Filter | CBT | N/A | CBT | R8979500903 |
| Mini-Circuits | BW-N20W5+ | DC to 18 GHz Precision Fixed 20 dB Attenuator | CBT | N/A | CBT | N/A |
| Mini-Circuits | NLP-1200+ | Low Pass Filter DC to 1000 MHz | CBT | N/A | CBT | N/A |
| Mini-Circuits | NLP-2950+ | Low Pass Filter DC to 2700 MHz | CBT | N/A | CBT | N/A |
| Narda | 4014C-6 | 4 - 8 GHz SMA 6 dB Directional Coupler | CBT | N/A | CBT | N/A |
| Narda | 4772-3 | Attenuator (3dB) | CBT | N/A | CBT | 9406 |
| Narda | BW-S3W2 | Attenuator (3dB) | CBT | N/A | CBT | 120 |
| Pasternack | PE2208-6 | Bidirectional Coupler | 6/3/2011 | Annual | 6/3/2012 | N/A |
| Pasternack | PE2209-10 | Bidirectional Coupler | 6/3/2011 | Annual | 6/3/2012 | N/A |
| Rohde & Schwarz | NRVD | Dual Channel Power Meter | 4/8/2011 | Biennial | 4/8/2013 | 101695 |
| Rohde & Schwarz | SMIQ03B | Signal Generator | 4/5/2012 | Annual | 4/5/2013 | DE27259 |
| Seekonk | NC-100 | Torque Wrench (8" lb) | 11/29/2011 | Triennial | 11/29/2014 | 21053 |
| Seekonk | NC-100 | Torque Wrench (8" lb) | 3/5/2012 | Triennial | 3/5/2015 | N/A |
| Seekonk | NC-100 | Torque Wrench (8" lb) | 3/5/2012 | Triennial | 3/5/2015 | N/A |
| SPEAG | D1750V2 | 1750 MHz SAR Dipole | 4/24/2012 | Annual | 4/24/2013 | 1051 |
| SPEAG | D1900V2 | 1900 MHz SAR Dipole | 7/22/2011 | Annual | 7/22/2012 | 5d080 |
| SPEAG | D1900V2 | 1900 MHz SAR Dipole | 2/22/2012 | Annual | 2/22/2013 | 5d149 |
| SPEAG | D835V2 | 835 MHz SAR Dipole | 1/25/2012 | Annual | 1/25/2013 | 4d047 |
| SPEAG | DAE4 | Dasy Data Acquisition Electronics | 4/19/2012 | Annual | 4/19/2013 | 665 |
| SPEAG | DAE4 | Dasy Data Acquisition Electronics | 2/15/2012 | Annual | 2/15/2013 | 1323 |
| SPEAG | DAE4 | Dasy Data Acquisition Electronics | 4/12/2012 | Annual | 4/12/2013 | 1333 |
| Speag | DAK-3.5 | Dielectric Assessment Kit | 12/1/2011 | Annual | 12/1/2012 | 1031 |
| SPEAG | ES3DV2 | SAR Probe | 8/25/2011 | Annual | 8/25/2012 | 3022 |
| SPEAG | ES3DV3 | SAR Probe | 3/16/2012 | Annual | 3/16/2013 | 3209 |
| SPEAG | EX3DV4 | SAR Probe | 7/27/2011 | Annual | 7/27/2012 | 3561 |
| Tektronix | RSA-6114A | Real Time Spectrum Analyzer | 4/5/2012 | Annual | 4/5/2013 | B010177 |
| VWR | 36934-158 | Wall-Mounted Thermometer | 1/21/2011 | Biennial | 1/21/2013 | 111286445 |
| VWR | 36934-158 | Wall-Mounted Thermometer | 1/21/2011 | Biennial | 1/21/2013 | 111286454 |
| VWR | 36934-158 | Wall-Mounted Thermometer | 9/30/2011 | Biennial | 9/30/2013 | 111859323 |

Note: CBT (Calibrated Before Testing). Prior to testing, the measurement paths containing a cable, attenuator, coupler, amplifier or filter were connected to a calibrated source (i.e. a signal generator) to determine the losses of the measurement path. The power meter offset was then adjusted to compensate for the measurement system losses. This level offset is stored within the power meter before measurements are made. This calibration verification procedure applies to the system verification and output power measurements. The calibrated reading is then taken directly from the power meter after compensation of the losses for all final power measurements.

| IC Cert No: N7NMC8355 (Integrated in Panasonic CF-19mk6) | SAR EVALUATION REPORT | | Reviewed by: Quality Manager |
|---|------------------------------------|--|---------------------------------|
| Document S/N: 0Y1206280879.N7N | Test Dates: 05/15/12 - 05/21/12 | DUT Type: Module in Portable Convertible Tablet Laptop Computer | Page 21 of 25 |
| © 2012 PCTEST Engineering Laboratory, Inc. | | | REV. 11.3 M 04/23/2012 |

13 MEASUREMENT UNCERTAINTIES

| a | b | c | d | e= f(d,k) | f | g | h = c x f/e | i = c x g/e | k |
|---|----------------|------------|-------------|-----------|----------------|----------------|-------------|-------------|----------------|
| Uncertainty Component | IEEE 1528 Sec. | Tol. (± %) | Prob. Dist. | Div. | c _i | c _i | 1gm | 10gms | v _i |
| Measurement System | | | | | | | | | |
| Probe Calibration | E.2.1 | 6.0 | N | 1 | 1.0 | 1.0 | 6.0 | 6.0 | ∞ |
| Axial Isotropy | E.2.2 | 0.25 | N | 1 | 0.7 | 0.7 | 0.2 | 0.2 | ∞ |
| Hemispherical Isotropy | E.2.2 | 1.3 | N | 1 | 1.0 | 1.0 | 1.3 | 1.3 | ∞ |
| Boundary Effect | E.2.3 | 0.4 | N | 1 | 1.0 | 1.0 | 0.4 | 0.4 | ∞ |
| Linearity | E.2.4 | 0.3 | N | 1 | 1.0 | 1.0 | 0.3 | 0.3 | ∞ |
| System Detection Limits | E.2.5 | 5.1 | N | 1 | 1.0 | 1.0 | 5.1 | 5.1 | ∞ |
| Readout Electronics | E.2.6 | 1.0 | N | 1 | 1.0 | 1.0 | 1.0 | 1.0 | ∞ |
| Response Time | E.2.7 | 0.8 | R | 1.73 | 1.0 | 1.0 | 0.5 | 0.5 | ∞ |
| Integration Time | E.2.8 | 2.6 | R | 1.73 | 1.0 | 1.0 | 1.5 | 1.5 | ∞ |
| RF Ambient Conditions | E.6.1 | 3.0 | R | 1.73 | 1.0 | 1.0 | 1.7 | 1.7 | ∞ |
| Probe Positioner Mechanical Tolerance | E.6.2 | 0.4 | R | 1.73 | 1.0 | 1.0 | 0.2 | 0.2 | ∞ |
| Probe Positioning w/ respect to Phantom | E.6.3 | 2.9 | R | 1.73 | 1.0 | 1.0 | 1.7 | 1.7 | ∞ |
| Extrapolation, Interpolation & Integration algorithms for Max. SAR Evaluation | E.5 | 1.0 | R | 1.73 | 1.0 | 1.0 | 0.6 | 0.6 | ∞ |
| Test Sample Related | | | | | | | | | |
| Test Sample Positioning | E.4.2 | 6.0 | N | 1 | 1.0 | 1.0 | 6.0 | 6.0 | 287 |
| Device Holder Uncertainty | E.4.1 | 3.32 | R | 1.73 | 1.0 | 1.0 | 1.9 | 1.9 | ∞ |
| Output Power Variation - SAR drift measurement | 6.6.2 | 5.0 | R | 1.73 | 1.0 | 1.0 | 2.9 | 2.9 | ∞ |
| Phantom & Tissue Parameters | | | | | | | | | |
| Phantom Uncertainty (Shape & Thickness tolerances) | E.3.1 | 4.0 | R | 1.73 | 1.0 | 1.0 | 2.3 | 2.3 | ∞ |
| Liquid Conductivity - deviation from target values | E.3.2 | 5.0 | R | 1.73 | 0.64 | 0.43 | 1.8 | 1.2 | ∞ |
| Liquid Conductivity - measurement uncertainty | E.3.3 | 3.8 | N | 1 | 0.64 | 0.43 | 2.4 | 1.6 | 6 |
| Liquid Permittivity - deviation from target values | E.3.2 | 5.0 | R | 1.73 | 0.60 | 0.49 | 1.7 | 1.4 | ∞ |
| Liquid Permittivity - measurement uncertainty | E.3.3 | 4.5 | N | 1 | 0.60 | 0.49 | 2.7 | 2.2 | 6 |
| Combined Standard Uncertainty (k=1) | | | | | | | 12.1 | 11.7 | 299 |
| Expanded Uncertainty (95% CONFIDENCE LEVEL) | | | | | | | 24.2 | 23.5 | |

The above measurement uncertainties are according to IEEE Std. 1528-2003

| | | | | | | |
|---|---|--|--|--|--|---------------------------------|
| IC Cert No: N7NMC8355 (Integrated in Panasonic CF-19mk6) |  | SAR EVALUATION REPORT | | | | Reviewed by: Quality Manager |
| Document S/N: 0Y1206280879.N7N | Test Dates: 05/15/12 - 05/21/12 | DUT Type: Module in Portable Convertible Tablet Laptop Computer | | | | Page 22 of 25 |

14 CONCLUSION

14.1 Measurement Conclusion

The SAR evaluation indicates that the EUT complies with the RF radiation exposure limits of the FCC and Industry Canada for the 850/1900 GSM/GPRS/EDGE/WCDMA/HSPA/CDMA/EVDO and AWS WCDMA/HSPA operations only, with respect to all parameters subject to this test. These measurements were taken to simulate the RF effects of RF exposure under worst-case conditions. Precise laboratory measures were taken to assure repeatability of the tests. The results and statements relate only to the item(s) tested. The test results in this report do not demonstrate compliance with the other capabilities of this EUT.

Please note that the absorption and distribution of electromagnetic energy in the body are very complex phenomena that depend on the mass, shape, and size of the body, the orientation of the body with respect to the field vectors, and the electrical properties of both the body and the environment. Other variables that may play a substantial role in possible biological effects are those that characterize the environment (e.g. ambient temperature, air velocity, relative humidity, and body insulation) and those that characterize the individual (e.g. age, gender, activity level, debilitation, or disease). Because various factors may interact with one another to vary the specific biological outcome of an exposure to electromagnetic fields, any protection guide should consider maximal amplification of biological effects as a result of field-body interactions, environmental conditions, and physiological variables. [3]

| | | | |
|---|---|--|---------------------------------|
| IC Cert No: N7NMC8355 (Integrated in Panasonic CF-19mk6) |  PCTEST Environmental Engineering, Inc. | SAR EVALUATION REPORT | Reviewed by: Quality Manager |
| Document S/N: 0Y1206280879.N7N | Test Dates: 05/15/12 - 05/21/12 | DUT Type: Module in Portable Convertible Tablet Laptop Computer | Page 23 of 25 |

15 REFERENCES

- [1] Federal Communications Commission, ET Docket 93-62, Guidelines for Evaluating the Environmental Effects of Radiofrequency Radiation, Aug. 1996.
- [2] ANSI/IEEE C95.1-2005, American National Standard safety levels with respect to human exposure to radio frequency electromagnetic fields, 3kHz to 300GHz, New York: IEEE, 2006.
- [3] ANSI/IEEE C95.1-1992, American National Standard safety levels with respect to human exposure to radio frequency electromagnetic fields, 3kHz to 300GHz, New York: IEEE, Sept. 1992.
- [4] ANSI/IEEE C95.3-2002, IEEE Recommended Practice for the Measurement of Potentially Hazardous Electromagnetic Fields - RF and Microwave, New York: IEEE, December 2002.
- [5] Federal Communications Commission, OET Bulletin 65 (Edition 97-01), Supplement C (Edition 01-01), Evaluating Compliance with FCC Guidelines for Human Exposure to Radiofrequency Electromagnetic Fields, June 2001.
- [6] IEEE Standards Coordinating Committee 34 – IEEE Std. 1528-2003, Recommended Practice for Determining the Peak Spatial-Average Specific Absorption Rate (SAR) in the Human Body Due to Wireless Communications Devices.
- [7] NCRP, National Council on Radiation Protection and Measurements, Biological Effects and Exposure Criteria for RadioFrequency Electromagnetic Fields, NCRP Report No. 86, 1986. Reprinted Feb. 1995.
- [8] T. Schmid, O. Egger, N. Kuster, Automated E-field scanning system for dosimetric assessments, IEEE Transaction on Microwave Theory and Techniques, vol. 44, Jan. 1996, pp. 105-113.
- [9] K. Pokovic, T. Schmid, N. Kuster, Robust setup for precise calibration of E-field probes in tissue simulating liquids at mobile communications frequencies, ICECOM97, Oct. 1997, pp. 120-124.
- [10] K. Pokovic, T. Schmid, and N. Kuster, E-field Probe with improved isotropy in brain simulating liquids, Proceedings of the ELMAR, Zadar, Croatia, June 23-25, 1996, pp. 172-175.
- [11] Schmid & Partner Engineering AG, Application Note: Data Storage and Evaluation, June 1998, p2.
- [12] V. Hombach, K. Meier, M. Burkhardt, E. Kuhn, N. Kuster, The Dependence of EM Energy Absorption upon Human Head Modeling at 900 MHz, IEEE Transaction on Microwave Theory and Techniques, vol. 44 no. 10, Oct. 1996, pp. 1865-1873.
- [13] N. Kuster and Q. Balzano, Energy absorption mechanism by biological bodies in the near field of dipole antennas above 300MHz, IEEE Transaction on Vehicular Technology, vol. 41, no. 1, Feb. 1992, pp. 17-23.
- [14] G. Hartsgrove, A. Kraszewski, A. Surowiec, Simulated Biological Materials for Electromagnetic Radiation Absorption Studies, University of Ottawa, Bioelectromagnetics, Canada: 1987, pp. 29-36.
- [15] Q. Balzano, O. Garay, T. Manning Jr., Electromagnetic Energy Exposure of Simulated Users of Portable Cellular Telephones, IEEE Transactions on Vehicular Technology, vol. 44, no.3, Aug. 1995.
- [16] W. Gander, Computermathematick, Birkhaeuser, Basel, 1992.
- [17] W.H. Press, S.A. Teukolsky, W.T. Vetterling, and B.P. Flannery, Numerical Recipes in C, The Art of Scientific Computing, Second edition, Cambridge University Press, 1992.

| | | |
|---|--|--|
| IC Cert No: N7NMC8355 (Integrated in Panasonic CF-19mk6) |  SAR EVALUATION REPORT | Reviewed by: Quality Manager |
| Document S/N: 0Y1206280879.N7N | Test Dates: 05/15/12 - 05/21/12 | DUT Type: Module in Portable Convertible Tablet Laptop Computer |

- [18] Federal Communications Commission, OET Bulletin 65, Evaluating Compliance with FCC Guidelines for Human Exposure to Radiofrequency Electromagnetic Fields. Supplement C, Dec. 1997.
- [19] N. Kuster, R. Kastle, T. Schmid, Dosimetric evaluation of mobile communications equipment with known precision, IEEE Transaction on Communications, vol. E80-B, no. 5, May 1997, pp. 645-652.
- [20] CENELEC CLC/SC111B, European Prestandard (prENV 50166-2), Human Exposure to Electromagnetic Fields High-frequency: 10kHz-300GHz, Jan. 1995.
- [21] Prof. Dr. Niels Kuster, ETH, Eidgenössische Technische Hochschule Zürich, Dosimetric Evaluation of the Cellular Phone.
- [22] IEC 62209-1, Human exposure to radio frequency fields from hand-held and body-mounted wireless communication devices - Human models, instrumentation, and procedures - Part 1: Procedure to determine the specific absorption rate (SAR) for hand-held devices used in close proximity to the ear (frequency range of 300 MHz to 3 GHz), Feb. 2005.
- [23] Industry Canada RSS-102 Radio Frequency Exposure Compliance of Radiocommunication Apparatus (All Frequency Bands) Issue 4, March 2010.
- [24] Health Canada Safety Code 6 Limits of Human Exposure to Radio Frequency Electromagnetic Fields in the Frequency Range from 3 kHz – 300 GHz, 2009
- [25] FCC Public Notice DA-02-1438. Office of Engineering and Technology Announces a Transition Period for the Phantom Requirements of Supplement C to OET Bulletin 65, June 19, 2002
- [26] FCC SAR Measurement Procedures for 3G Devices KDB Publication 941225
- [27] SAR Measurement procedures for IEEE 802.11a/b/g KDB Publication 248227
- [28] FCC SAR Considerations for Handsets with Multiple Transmitters and Antennas, KDB Publication 648474
- [29] FCC Application Note for SAR Probe Calibration and System Verification Consideration for Measurements at 150 MHz – 3 GHz, KDB Publication 450824
- [30] FCC SAR Evaluation Considerations for Laptop Computers with Antennas Built-in on Display Screens, KDB Publication 616217
- [31] FCC SAR Measurement Requirements for 3 – 6 GHz, KDB Publication 865664
- [32] FCC Mobile Portable RF Exposure Procedure, KDB Publication 447498
- [33] FCC SAR Procedures for Dongle Transmitters, KDB Publication 447498
- [34] Anexo à Resolução No. 533, de 10 de Setembro de 2009.
- [35] FCC SAR Test Considerations for LTE Handsets and Data Modems, KDB Publication 941225.
- [36] IEC 62209-2, Human exposure to radio frequency fields from hand-held and body-mounted wireless communication devices - Human models, instrumentation, and procedures - Part 2: Procedure to determine the specific absorption rate (SAR) for wireless communication devices used in close proximity to the human body (frequency range of 30 MHz to 6 GHz), Mar. 2010.
- [37] FCC Hot Spot SAR v01, KDB Publication 941225 D06.

| | | | |
|---|---|--|--|
| IC Cert No: N7NMC8355 (Integrated in Panasonic CF-19mk6) |  | SAR EVALUATION REPORT | |
| Document S/N: 0Y1206280879.N7N | Test Dates: 05/15/12 - 05/21/12 | DUT Type: Module in Portable Convertible Tablet Laptop Computer | Reviewed by: Quality Manager Page 25 of 25 |

APPENDIX D: SAR TEST SETUP PHOTOGRAPHS

| | | |
|---|--|---------------------------------|
| IC Cert No: N7NMC8355 (Integrated in Panasonic CF-19mk6) |  SAR EVALUATION REPORT | Reviewed by: Quality Manager |
| Test Dates: 05/15/12 - 05/21/12 | DUT Type: Module in Portable Convertible Tablet Laptop Computer | Page D1 of D3 |




SAR Test Setup Photo 1: Back at 0.0 cm



SAR Test Setup Photo 2: Top at 0.0 cm

| | | | |
|---|---|-----------------------|---------------------------------|
| IC Cert No: N7NMC8355 (Integrated in Panasonic CF-19mk6) |  PCTEST [®] | SAR EVALUATION REPORT | Reviewed by: Quality Manager |
| Test Dates: 05/15/12 - 05/21/12 | DUT Type: Module in Portable Convertible Tablet Laptop Computer | | Page D2 of D3 |

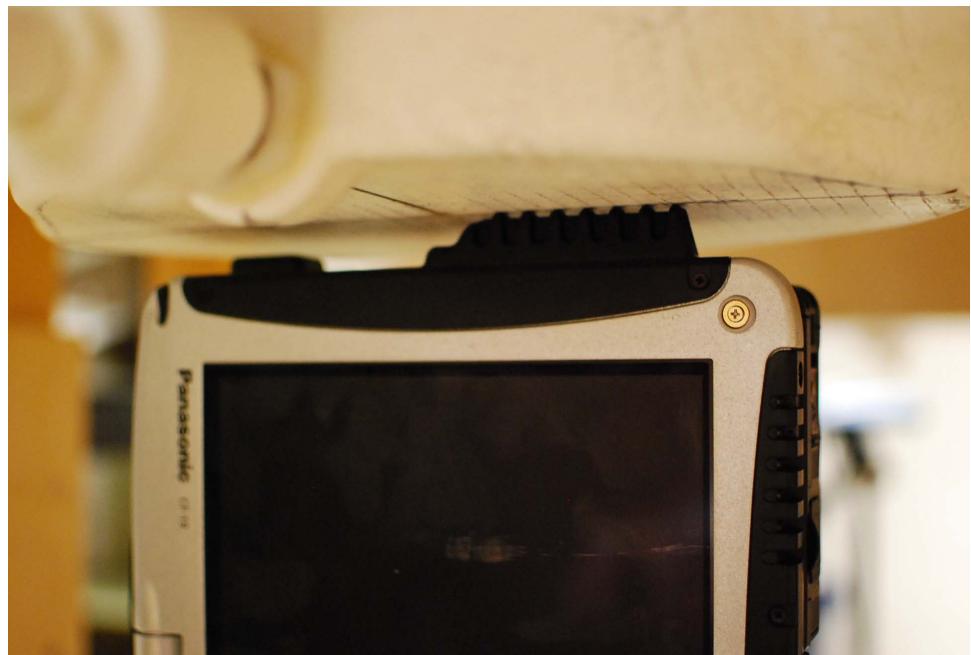

SAR Test Setup Photo 3: Left at 0.0 cm

| | | |
|---|--|---------------------------------|
| IC Cert No: N7NMC8355 (Integrated in Panasonic CF-19mk6) |  SAR EVALUATION REPORT | Reviewed by: Quality Manager |
| Test Dates: 05/15/12 - 05/21/12 | DUT Type: Module in Portable Convertible Tablet Laptop Computer | Page D3 of D3 |

APPENDIX A: SAR TEST DATA

PCTEST ENGINEERING LABORATORY, INC.

DUT: CF-19 mk6; Type: Portable Tablet Computer; Serial: 2CKSA00021

Communication System: GSM GPRS; 2 Tx slots; Frequency: 836.6 MHz; Duty Cycle: 1:4.15

Medium: 835 Body Medium parameters used (interpolated):

$f = 836.6$ MHz; $\sigma = 0.973$ mho/m; $\epsilon_r = 52.986$; $\rho = 1000$ kg/m³

Phantom section: Flat Section; Space: 0.0 cm

Test Date: 05-21-2012; Ambient Temp: 23.9°C; Tissue Temp: 22.4°C

Probe: EX3DV4 - SN3561; ConvF(8.25, 8.25, 8.25); Calibrated: 7/27/2011;

Sensor-Surface: 4mm (Mechanical Surface Detection)

Electronics: DAE4 Sn1333; Calibrated: 4/12/2012

Phantom: SAM 5.0 front; Type: QD000P40CD; Serial: TP:-1648

Measurement SW: DASY52, Version 52.8 (1); SEMCAD X Version 14.6.5 (6469)

Mode: GPRS 850, Body SAR, Back side, Mid.ch, 2 Tx Slots


Area Scan (11x21x1): Measurement grid: dx=15mm, dy=15mm

Zoom Scan (5x5x7)/Cube 0: Measurement grid: dx=8mm, dy=8mm, dz=5mm

Reference Value = 1.672 V/m; Power Drift = 0.149 dB

Peak SAR (extrapolated) = 0.141 mW/g

SAR(1 g) = 0.093 mW/g; SAR(10 g) = 0.067 mW/g

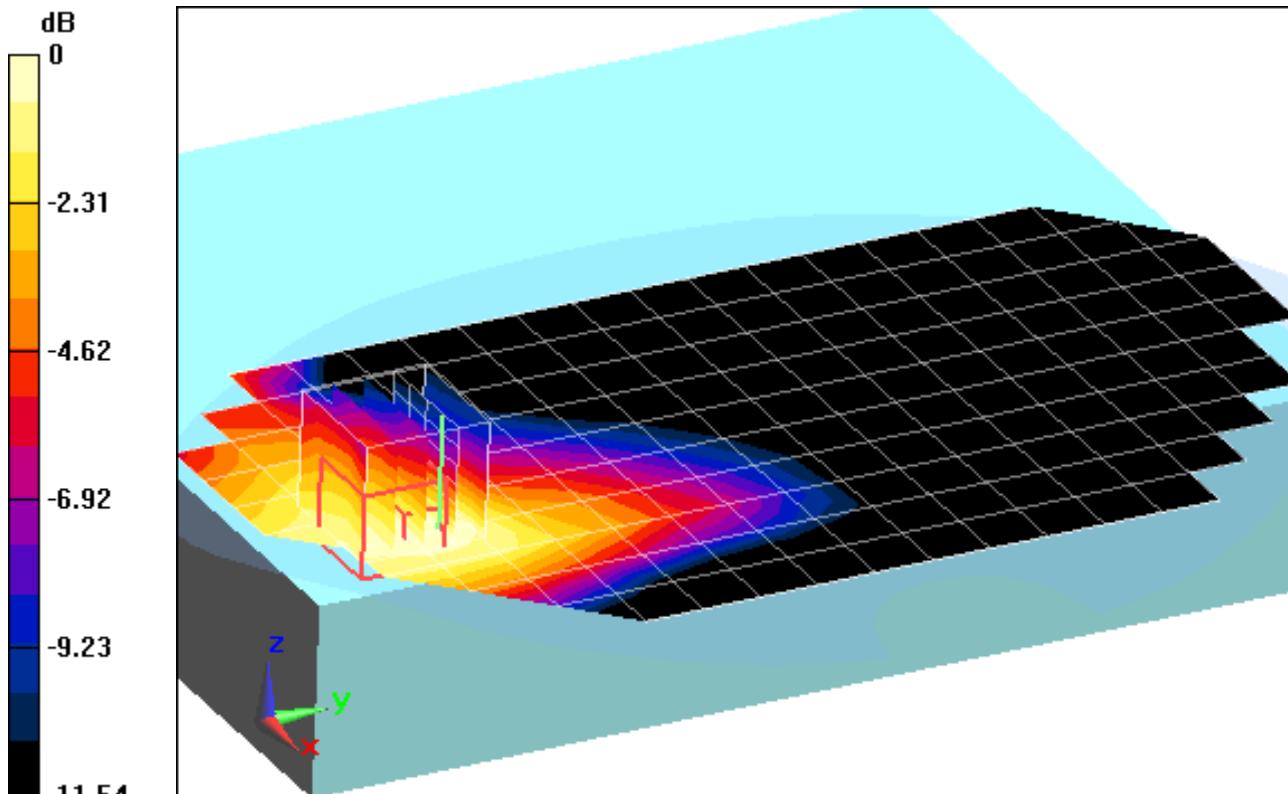

PCTEST ENGINEERING LABORATORY, INC.

DUT: CF-19 mk6; Type: Portable Tablet Computer; Serial: 2CKSA00021

Communication System: GSM GPRS; 2 Tx slots; Frequency: 836.6 MHz; Duty Cycle: 1:4.15

Medium: 835 Body Medium parameters used (interpolated):

$f = 836.6$ MHz; $\sigma = 0.973$ mho/m; $\epsilon_r = 52.986$; $\rho = 1000$ kg/m³

Phantom section: Flat Section; Space: 0.0 cm

Test Date: 05-21-2012; Ambient Temp: 23.9°C; Tissue Temp: 22.4°C

Probe: EX3DV4 - SN3561; ConvF(8.25, 8.25, 8.25); Calibrated: 7/27/2011;

Sensor-Surface: 4mm (Mechanical Surface Detection)

Electronics: DAE4 Sn1333; Calibrated: 4/12/2012

Phantom: SAM 5.0 front; Type: QD000P40CD; Serial: TP:-1648

Measurement SW: DASY52, Version 52.8 (1); SEMCAD X Version 14.6.5 (6469)

Mode: GPRS 850, Body SAR, Top Edge, Mid.ch, 2 Tx Slots


Area Scan (9x21x1): Measurement grid: dx=15mm, dy=15mm

Zoom Scan (5x5x7)/Cube 0: Measurement grid: dx=8mm, dy=8mm, dz=5mm

Reference Value = 13.732 V/m; Power Drift = 0.089 dB

Peak SAR (extrapolated) = 0.304 mW/g

SAR(1 g) = 0.172 mW/g; SAR(10 g) = 0.109 mW/g

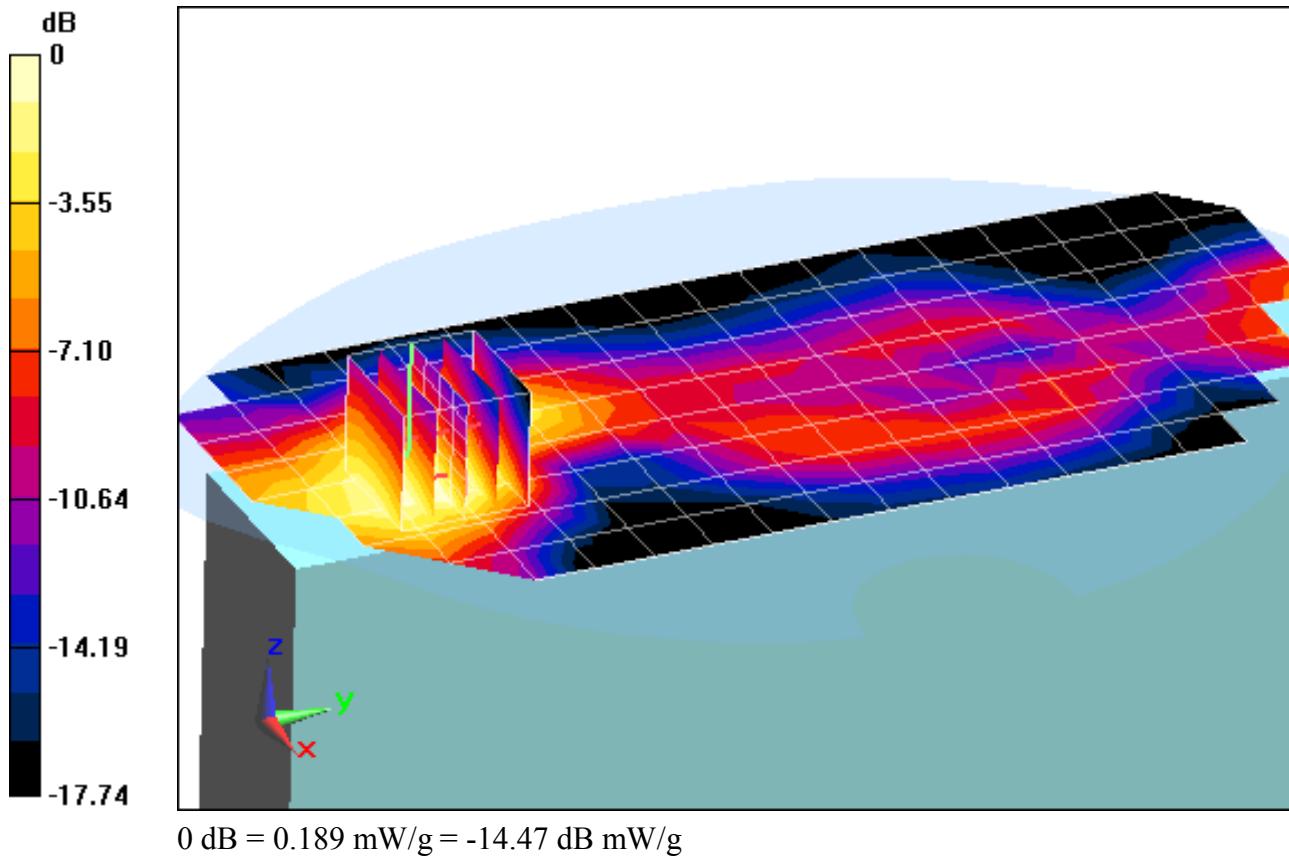

PCTEST ENGINEERING LABORATORY, INC.

DUT: CF-19 mk6; Type: Portable Tablet Computer; Serial: 2CKSA00021

Communication System: GSM GPRS; 2 Tx slots; Frequency: 836.6 MHz; Duty Cycle: 1:4.15

Medium: 835 Body Medium parameters used (interpolated):

$f = 836.6$ MHz; $\sigma = 0.973$ mho/m; $\epsilon_r = 52.986$; $\rho = 1000$ kg/m³

Phantom section: Flat Section; Space: 0.0 cm

Test Date: 05-21-2012; Ambient Temp: 23.9°C; Tissue Temp: 22.4°C

Probe: EX3DV4 - SN3561; ConvF(8.25, 8.25, 8.25); Calibrated: 7/27/2011;

Sensor-Surface: 4mm (Mechanical Surface Detection)

Electronics: DAE4 Sn1333; Calibrated: 4/12/2012

Phantom: SAM 5.0 front; Type: QD000P40CD; Serial: TP:-1648

Measurement SW: DASY52, Version 52.8 (1); SEMCAD X Version 14.6.5 (6469)

Mode: GPRS 850, Body SAR, Left Edge, Mid.ch, 2 Tx Slots


Area Scan (9x21x1): Measurement grid: dx=15mm, dy=15mm

Zoom Scan (5x5x7)/Cube 0: Measurement grid: dx=8mm, dy=8mm, dz=5mm

Reference Value = 25.885 V/m; Power Drift = -0.01 dB

Peak SAR (extrapolated) = 0.929 mW/g

SAR(1 g) = 0.620 mW/g; SAR(10 g) = 0.386 mW/g

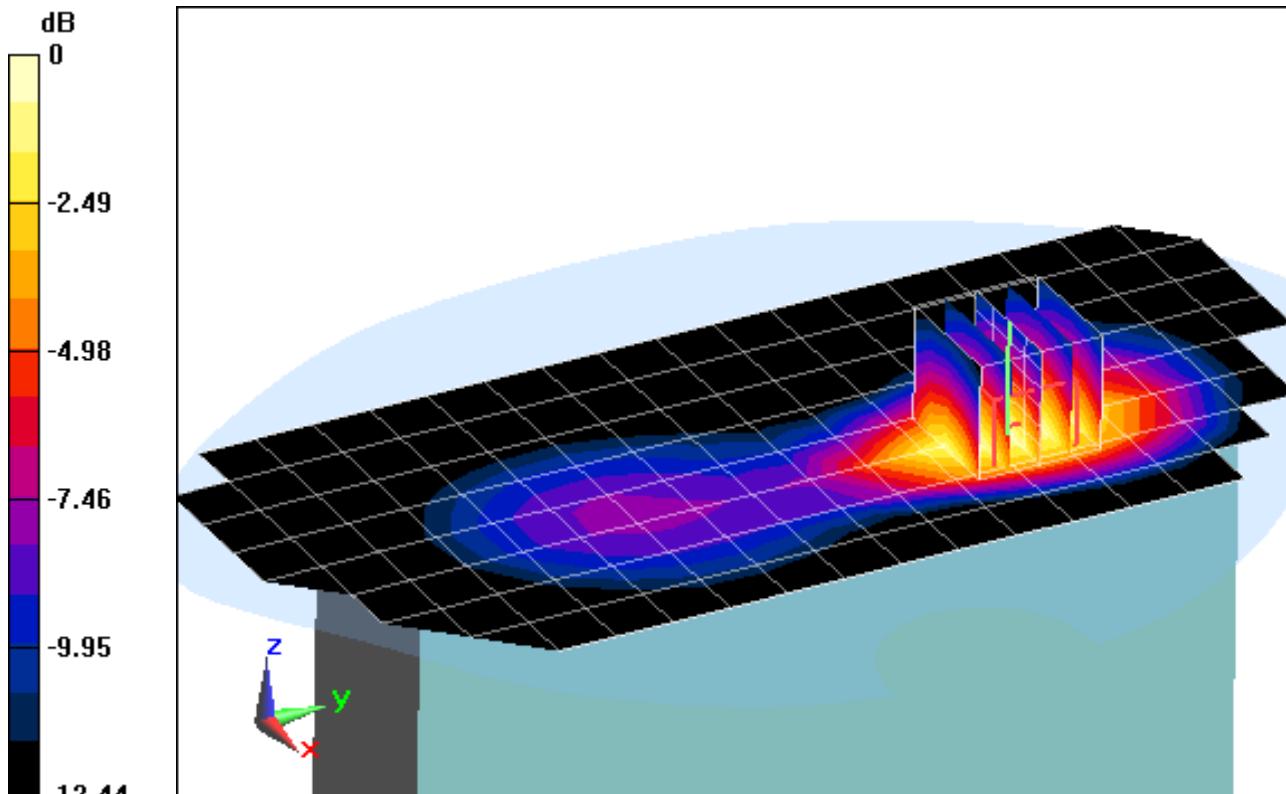

0 dB = 0.680 mW/g = -3.35 dB mW/g

PCTEST ENGINEERING LABORATORY, INC.

DUT: CF-19 mk6; Type: Portable Tablet Computer; Serial: 2CKSA00021

Communication System: WCDMA; Frequency: 836.6 MHz; Duty Cycle: 1:1

Medium: 835 Body Medium parameters used (interpolated):

$f = 836.6$ MHz; $\sigma = 0.973$ mho/m; $\epsilon_r = 52.986$; $\rho = 1000$ kg/m³

Phantom section: Flat Section; Space: 0.0 cm

Test Date: 05-21-2012; Ambient Temp: 23.9°C; Tissue Temp: 22.4°C

Probe: EX3DV4 - SN3561; ConvF(8.25, 8.25, 8.25); Calibrated: 7/27/2011;

Sensor-Surface: 4mm (Mechanical Surface Detection)

Electronics: DAE4 Sn1333; Calibrated: 4/12/2012

Phantom: SAM 5.0 front; Type: QD000P40CD; Serial: TP:-1648

Measurement SW: DASY52, Version 52.8 (1); SEMCAD X Version 14.6.5 (6469)

Mode: WCDMA 850, Body SAR, Back side, Mid.ch


Area Scan (11x21x1): Measurement grid: dx=15mm, dy=15mm

Zoom Scan (5x5x7)/Cube 0: Measurement grid: dx=8mm, dy=8mm, dz=5mm

Reference Value = 7.361 V/m; Power Drift = -0.12 dB

Peak SAR (extrapolated) = 0.077 mW/g

SAR(1 g) = 0.050 mW/g; SAR(10 g) = 0.033 mW/g

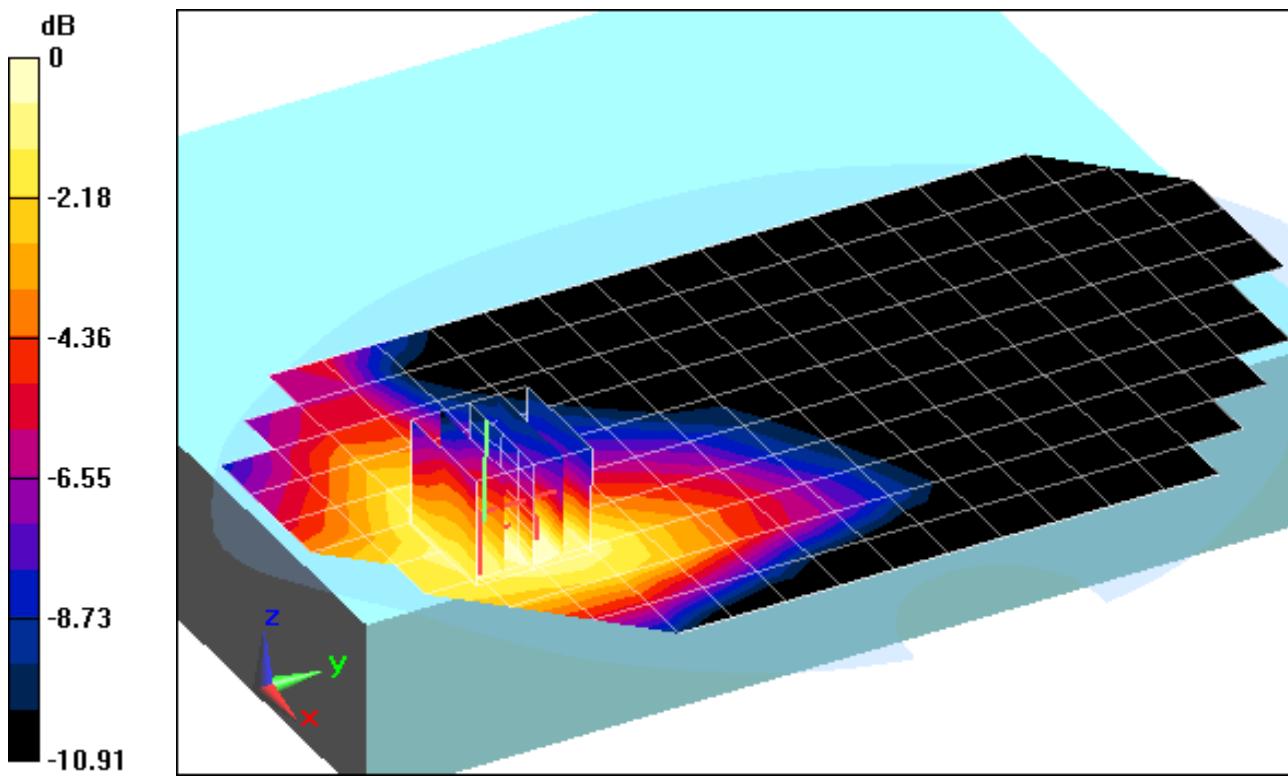

PCTEST ENGINEERING LABORATORY, INC.

DUT: CF-19 mk6; Type: Portable Tablet Computer; Serial: 2CKSA00021

Communication System: WCDMA; Frequency: 836.6 MHz; Duty Cycle: 1:1

Medium: 835 Body Medium parameters used (interpolated):

$f = 836.6$ MHz; $\sigma = 0.973$ mho/m; $\epsilon_r = 52.986$; $\rho = 1000$ kg/m³

Phantom section: Flat Section; Space: 0.0 cm

Test Date: 05-21-2012; Ambient Temp: 23.9°C; Tissue Temp: 22.4°C

Probe: EX3DV4 - SN3561; ConvF(8.25, 8.25, 8.25); Calibrated: 7/27/2011;

Sensor-Surface: 4mm (Mechanical Surface Detection)

Electronics: DAE4 Sn1333; Calibrated: 4/12/2012

Phantom: SAM 5.0 front; Type: QD000P40CD; Serial: TP:-1648

Measurement SW: DASY52, Version 52.8 (1); SEMCAD X Version 14.6.5 (6469)

Mode: WCDMA 850, Body SAR, Top Edge, Mid.ch


Area Scan (9x21x1): Measurement grid: dx=15mm, dy=15mm

Zoom Scan (5x5x7)/Cube 0: Measurement grid: dx=8mm, dy=8mm, dz=5mm

Reference Value = 10.647 V/m; Power Drift = -0.03 dB

Peak SAR (extrapolated) = 0.183 mW/g

SAR(1 g) = 0.105 mW/g; SAR(10 g) = 0.066 mW/g

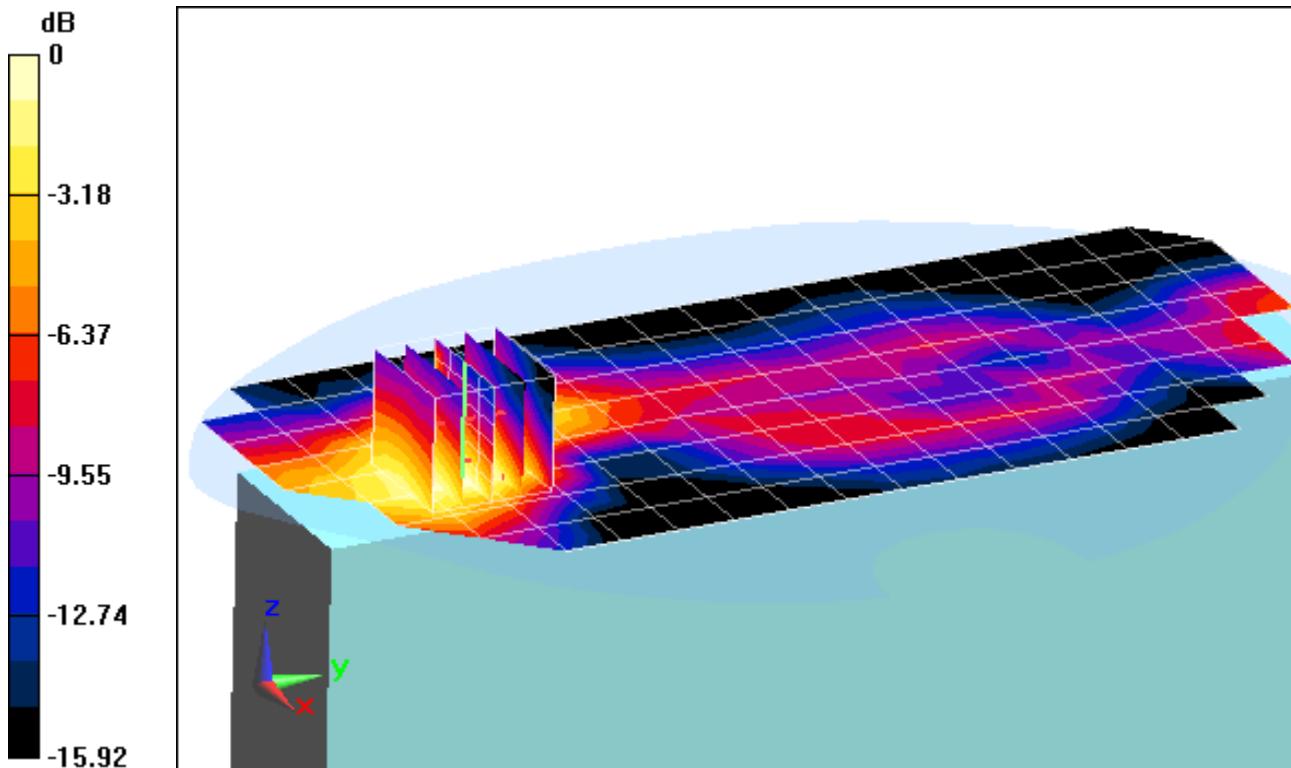

0 dB = 0.113 mW/g = -18.94 dB mW/g

PCTEST ENGINEERING LABORATORY, INC.

DUT: CF-19 mk6; Type: Portable Tablet Computer; Serial: 2CKSA00021

Communication System: WCDMA; Frequency: 836.6 MHz; Duty Cycle: 1:1

Medium: 835 Body Medium parameters used (interpolated):

$f = 836.6$ MHz; $\sigma = 0.973$ mho/m; $\epsilon_r = 52.986$; $\rho = 1000$ kg/m³

Phantom section: Flat Section; Space: 0.0 cm

Test Date: 05-21-2012; Ambient Temp: 23.9°C; Tissue Temp: 22.4°C

Probe: EX3DV4 - SN3561; ConvF(8.25, 8.25, 8.25); Calibrated: 7/27/2011;

Sensor-Surface: 4mm (Mechanical Surface Detection)

Electronics: DAE4 Sn1333; Calibrated: 4/12/2012

Phantom: SAM 5.0 front; Type: QD000P40CD; Serial: TP:-1648

Measurement SW: DASY52, Version 52.8 (1); SEMCAD X Version 14.6.5 (6469)

Mode: WCDMA 850, Body SAR, Left Edge, Mid.ch


Area Scan (9x21x1): Measurement grid: dx=15mm, dy=15mm

Zoom Scan (5x5x7)/Cube 0: Measurement grid: dx=8mm, dy=8mm, dz=5mm

Reference Value = 19.853 V/m; Power Drift = 0.08 dB

Peak SAR (extrapolated) = 0.582 mW/g

SAR(1 g) = 0.376 mW/g; SAR(10 g) = 0.232 mW/g

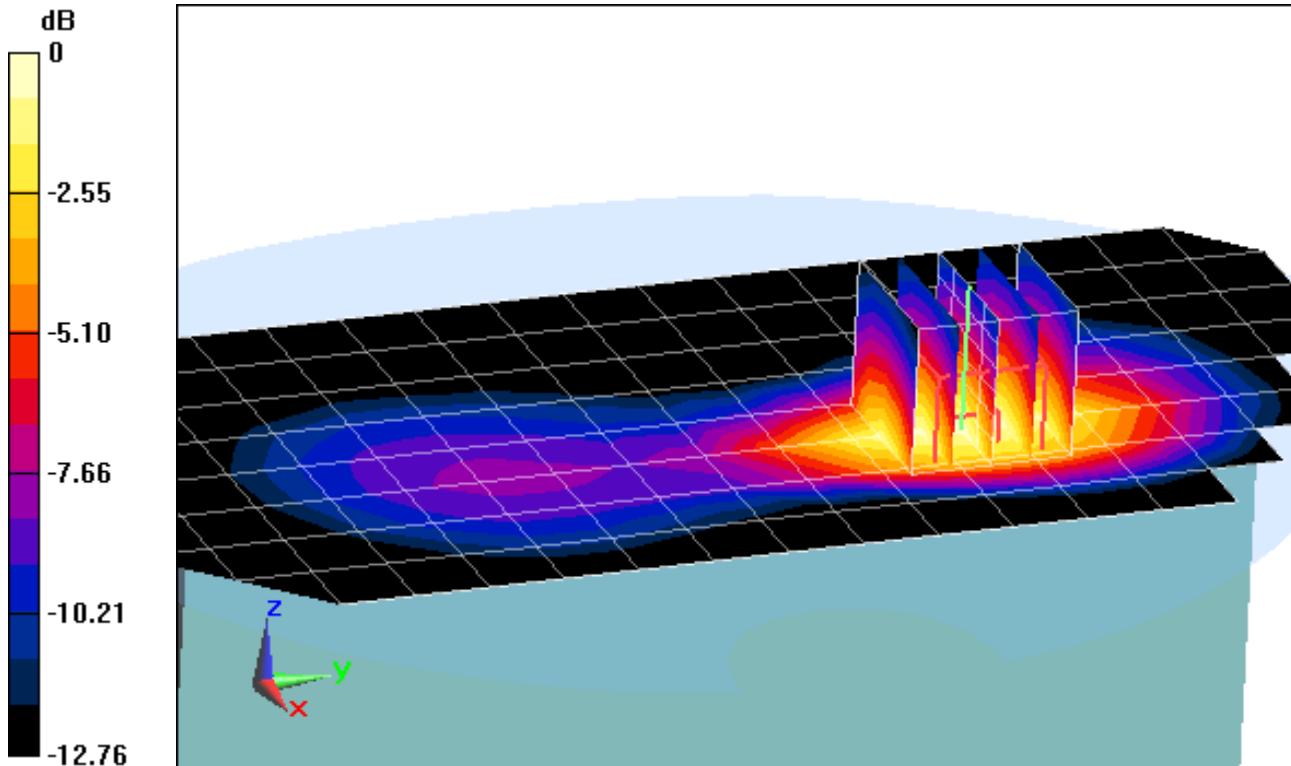

0 dB = 0.413 mW/g = -7.68 dB mW/g

PCTEST ENGINEERING LABORATORY, INC.

DUT: CF-19 mk6; Type: Portable Tablet Computer; Serial: 2CKSA00021

Communication System: CDMA; Frequency: 836.52 MHz; Duty Cycle: 1:1

Medium: 835 Body Medium parameters used (interpolated):

$f = 836.52$ MHz; $\sigma = 0.973$ mho/m; $\epsilon_r = 52.986$; $\rho = 1000$ kg/m³

Phantom section: Flat Section; Space: 0.0 cm

Test Date: 05-21-2012; Ambient Temp: 23.9°C; Tissue Temp: 22.4°C

Probe: EX3DV4 - SN3561; ConvF(8.25, 8.25, 8.25); Calibrated: 7/27/2011;

Sensor-Surface: 4mm (Mechanical Surface Detection)

Electronics: DAE4 Sn1333; Calibrated: 4/12/2012

Phantom: SAM 5.0 front; Type: QD000P40CD; Serial: TP:-1648

Measurement SW: DASY52, Version 52.8 (1); SEMCAD X Version 14.6.5 (6469)

Mode: Cell. EVDO, Body SAR, Back side, Mid.ch


Area Scan (9x21x1): Measurement grid: dx=15mm, dy=15mm

Zoom Scan (5x5x7)/Cube 0: Measurement grid: dx=8mm, dy=8mm, dz=5mm

Reference Value = 2.659 V/m; Power Drift = -0.06 dB

Peak SAR (extrapolated) = 0.089 mW/g

SAR(1 g) = 0.049 mW/g; SAR(10 g) = 0.033 mW/g

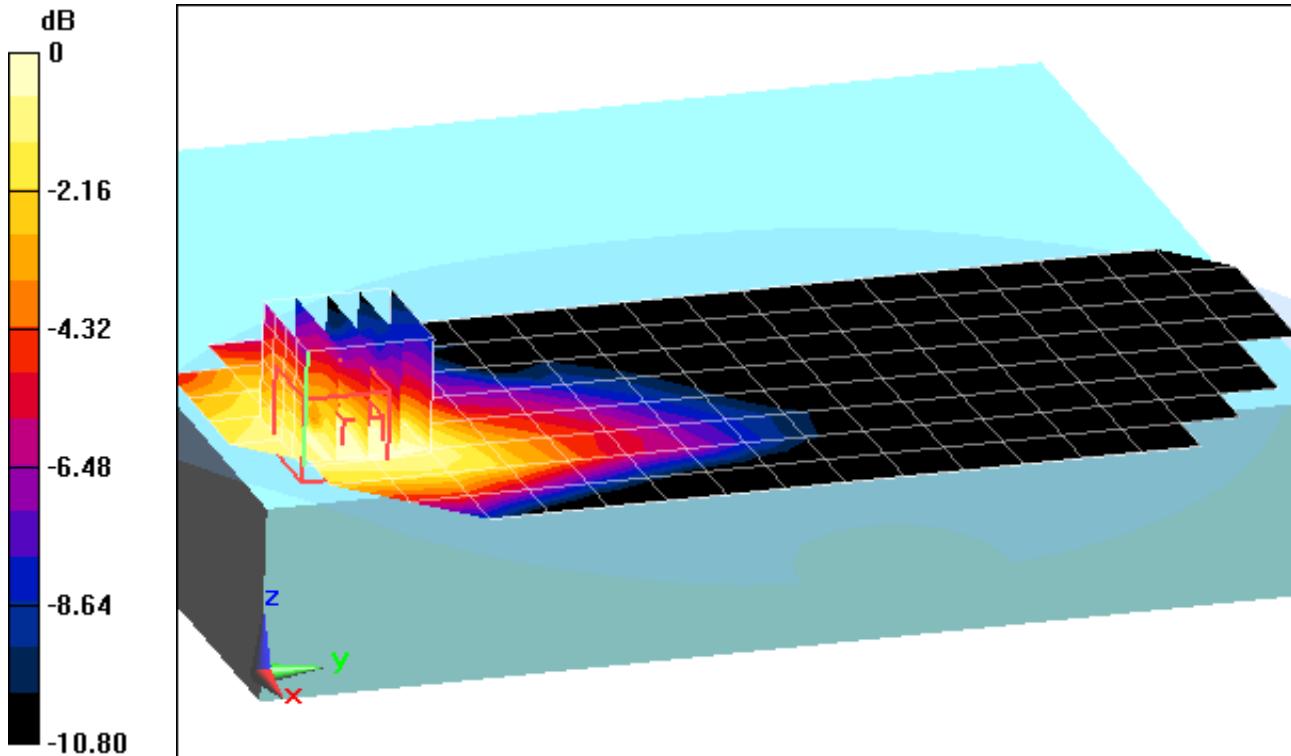

0 dB = 0.0504 mW/g = -25.96 dB mW/g

PCTEST ENGINEERING LABORATORY, INC.

DUT: CF-19 mk6; Type: Portable Tablet Computer; Serial: 2CKSA00021

Communication System: CDMA; Frequency: 836.52 MHz; Duty Cycle: 1:1

Medium: 835 Body Medium parameters used (interpolated):

$f = 836.52$ MHz; $\sigma = 0.973$ mho/m; $\epsilon_r = 52.986$; $\rho = 1000$ kg/m³

Phantom section: Flat Section; Space: 0.0 cm

Test Date: 05-21-2012; Ambient Temp: 23.9°C; Tissue Temp: 22.4°C

Probe: EX3DV4 - SN3561; ConvF(8.25, 8.25, 8.25); Calibrated: 7/27/2011;

Sensor-Surface: 4mm (Mechanical Surface Detection)

Electronics: DAE4 Sn1333; Calibrated: 4/12/2012

Phantom: SAM 5.0 front; Type: QD000P40CD; Serial: TP:-1648

Measurement SW: DASY52, Version 52.8 (1); SEMCAD X Version 14.6.5 (6469)

Mode: Cell. EVDO, Body SAR, Top Edge, Mid.ch


Area Scan (7x21x1): Measurement grid: dx=15mm, dy=15mm

Zoom Scan (5x5x7)/Cube 0: Measurement grid: dx=8mm, dy=8mm, dz=5mm

Reference Value = 5.727 V/m; Power Drift = 0.19 dB

Peak SAR (extrapolated) = 0.112 mW/g

SAR(1 g) = 0.071 mW/g; SAR(10 g) = 0.041 mW/g

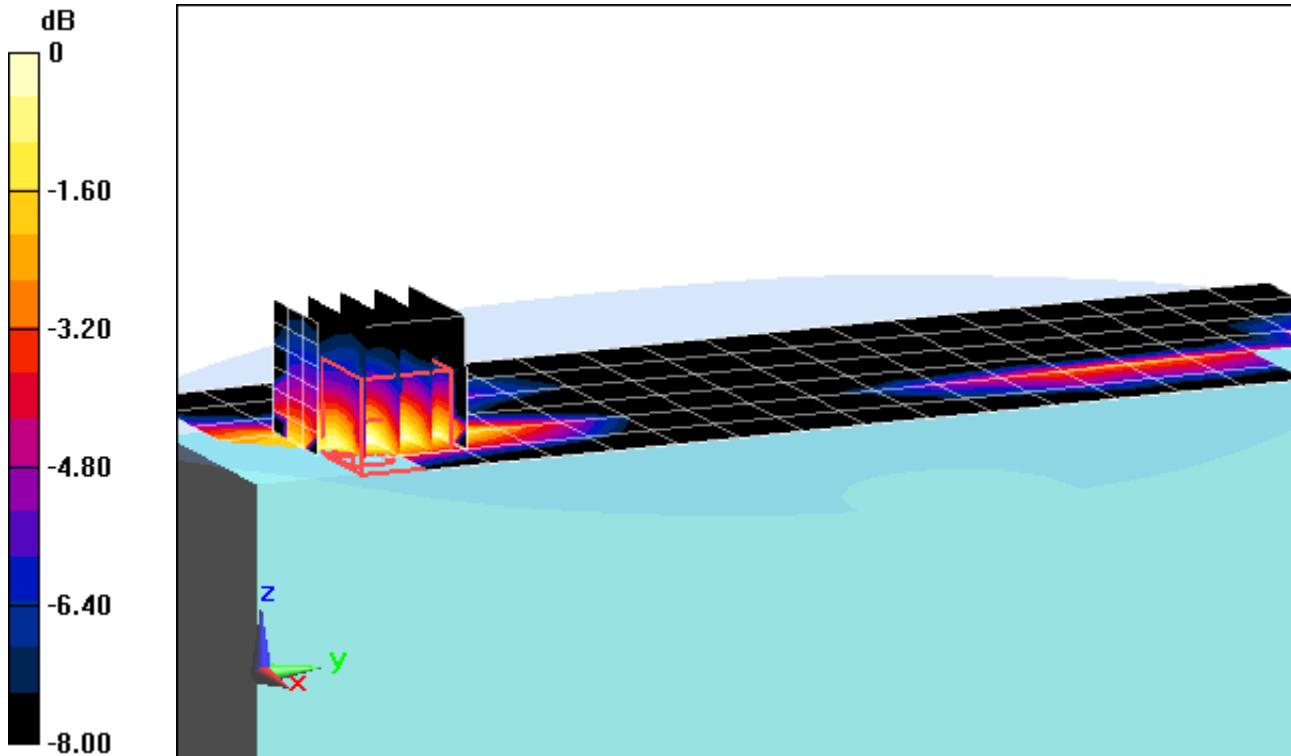

PCTEST ENGINEERING LABORATORY, INC.

DUT: CF-19 mk6; Type: Portable Tablet Computer; Serial: 2CKSA00021

Communication System: CDMA; Frequency: 836.52 MHz; Duty Cycle: 1:1

Medium: 835 Body Medium parameters used (interpolated):

$f = 836.52$ MHz; $\sigma = 0.973$ mho/m; $\epsilon_r = 52.986$; $\rho = 1000$ kg/m³

Phantom section: Flat Section; Space: 0.0 cm

Test Date: 05-21-2012; Ambient Temp: 23.9°C; Tissue Temp: 22.4°C

Probe: EX3DV4 - SN3561; ConvF(8.25, 8.25, 8.25); Calibrated: 7/27/2011;

Sensor-Surface: 4mm (Mechanical Surface Detection)

Electronics: DAE4 Sn1333; Calibrated: 4/12/2012

Phantom: SAM 5.0 front; Type: QD000P40CD; Serial: TP:-1648

Measurement SW: DASY52, Version 52.8 (1); SEMCAD X Version 14.6.5 (6469)

Mode: Cell. EVDO, Body SAR, Left Edge, Mid.ch


Area Scan (7x21x1): Measurement grid: dx=15mm, dy=15mm

Zoom Scan (5x5x7)/Cube 0: Measurement grid: dx=8mm, dy=8mm, dz=5mm

Reference Value = 20.923 V/m; Power Drift = -0.14 dB

Peak SAR (extrapolated) = 0.716 mW/g

SAR(1 g) = 0.434 mW/g; SAR(10 g) = 0.269 mW/g

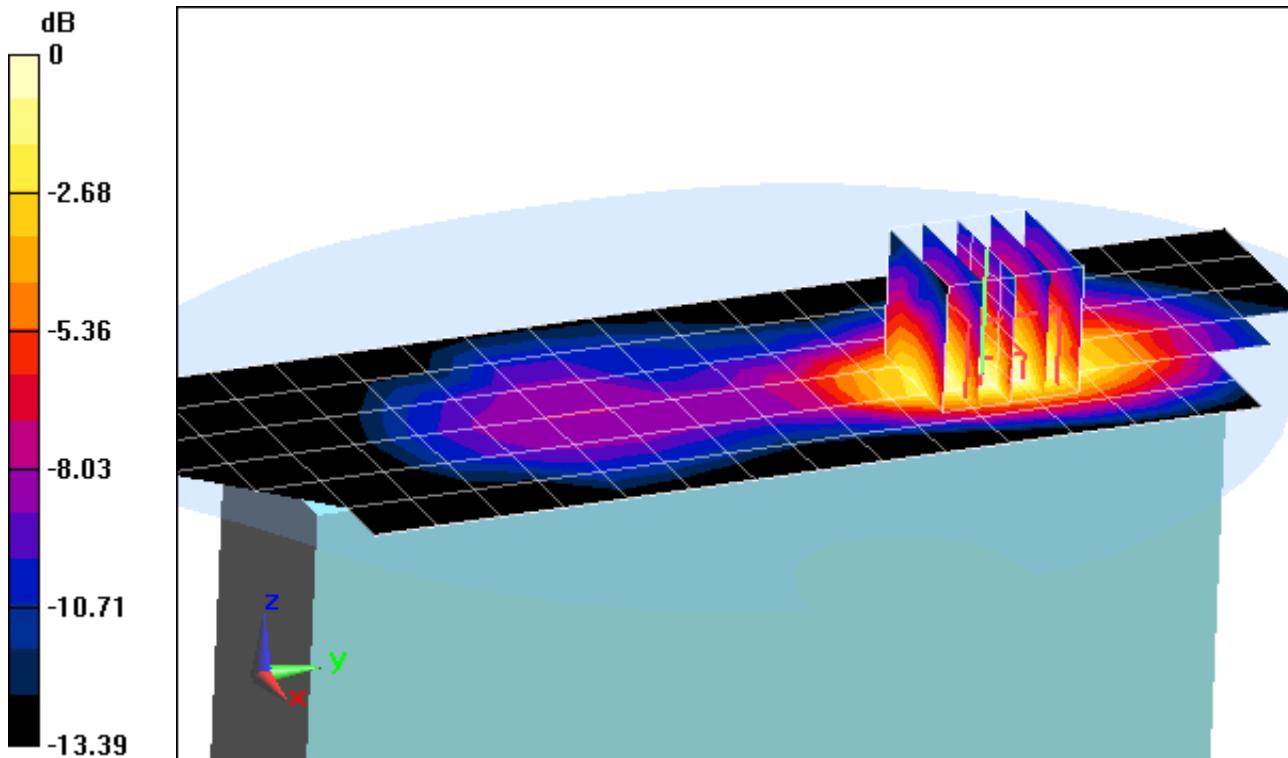

PCTEST ENGINEERING LABORATORY, INC.

DUT: CF-19 mk6; Type: Portable Tablet Computer; Serial: 2CKSA00021

Communication System: AWS WCDMA; Frequency: 1730.4 MHz; Duty Cycle: 1:1

Medium: 1750 Body Medium parameters used (interpolated):

$f = 1730.4$ MHz; $\sigma = 1.487$ mho/m; $\epsilon_r = 52.702$; $\rho = 1000$ kg/m³

Phantom section: Flat Section; Space: 0.0 cm

Test Date: 05-21-2012; Ambient Temp: 23.4°C; Tissue Temp: 22.2°C

Probe: ES3DV2 - SN3022; ConvF(4.64, 4.64, 4.64); Calibrated: 8/25/2011;

Sensor-Surface: 4mm (Mechanical Surface Detection)

Electronics: DAE4 Sn665; Calibrated: 4/19/2012

Phantom: SAM Sub Dasy B; Type: SAM 5.0; Serial: TP-1626

Measurement SW: DASY4, Version 4.7 (80); SEMCAD X Version 14.6.5 (6469)

Mode: AWS WCDMA, Body SAR, Back side, Mid.ch


Area Scan (10x18x1): Measurement grid: dx=15mm, dy=15mm

Zoom Scan (5x5x7)/Cube 0: Measurement grid: dx=8mm, dy=8mm, dz=5mm

Reference Value = 6.749 V/m; Power Drift = -0.15 dB

Peak SAR (extrapolated) = 0.093 mW/g

SAR(1 g) = 0.058 mW/g; SAR(10 g) = 0.037 mW/g

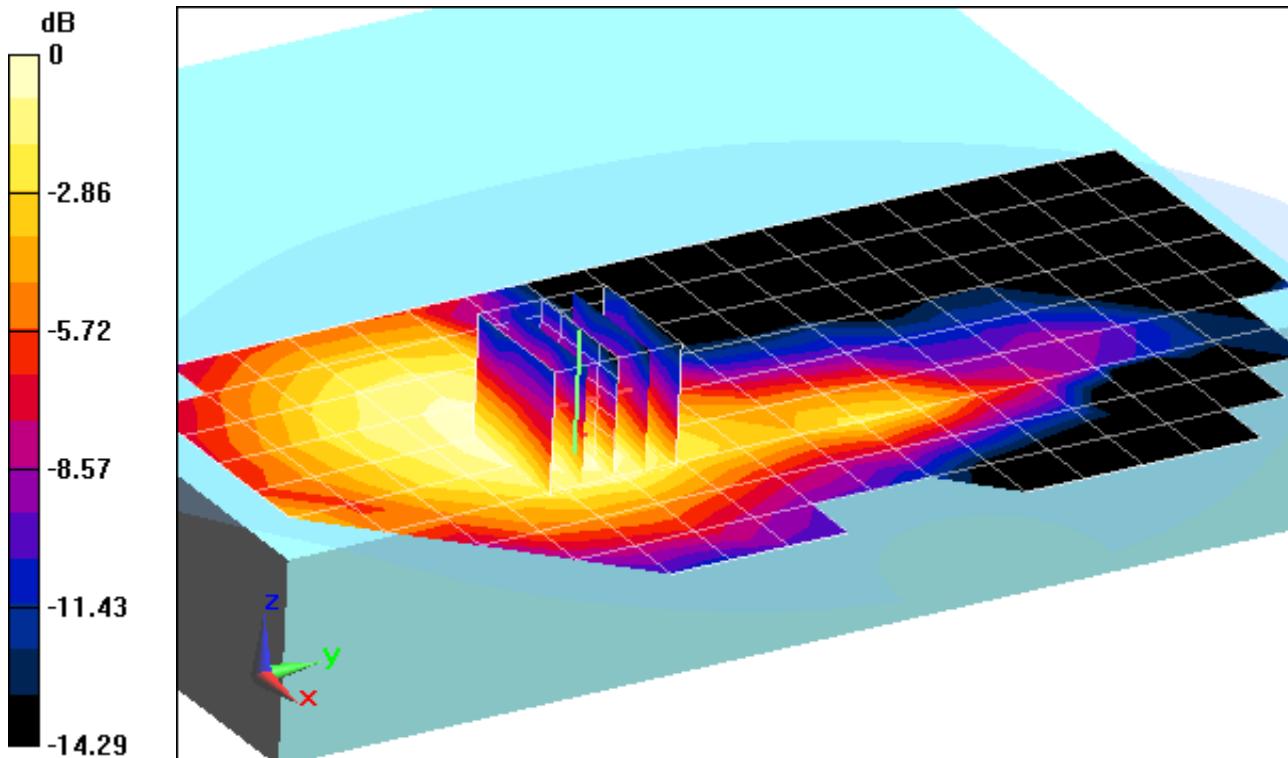

PCTEST ENGINEERING LABORATORY, INC.

DUT: CF-19 mk6; Type: Portable Tablet Computer; Serial: 2CKSA00021

Communication System: AWS WCDMA; Frequency: 1730.4 MHz; Duty Cycle: 1:1

Medium: 1750 Body Medium parameters used (interpolated):

$f = 1730.4$ MHz; $\sigma = 1.487$ mho/m; $\epsilon_r = 52.702$; $\rho = 1000$ kg/m³

Phantom section: Flat Section; Space: 0.0 cm

Test Date: 05-21-2012; Ambient Temp: 23.4°C; Tissue Temp: 22.2°C

Probe: ES3DV2 - SN3022; ConvF(4.64, 4.64, 4.64); Calibrated: 8/25/2011;

Sensor-Surface: 4mm (Mechanical Surface Detection)

Electronics: DAE4 Sn665; Calibrated: 4/19/2012

Phantom: SAM Sub Dasy B; Type: SAM 5.0; Serial: TP-1626

Measurement SW: DASY4, Version 4.7 (80); SEMCAD X Version 14.6.5 (6469)

Mode: AWS WCDMA, Body SAR, Top Edge, Mid.ch


Area Scan (10x18x1): Measurement grid: dx=15mm, dy=15mm

Zoom Scan (5x5x7)/Cube 0: Measurement grid: dx=8mm, dy=8mm, dz=5mm

Reference Value = 17.634 V/m; Power Drift = 0.00 dB

Peak SAR (extrapolated) = 0.704 mW/g

SAR(1 g) = 0.421 mW/g; SAR(10 g) = 0.253 mW/g

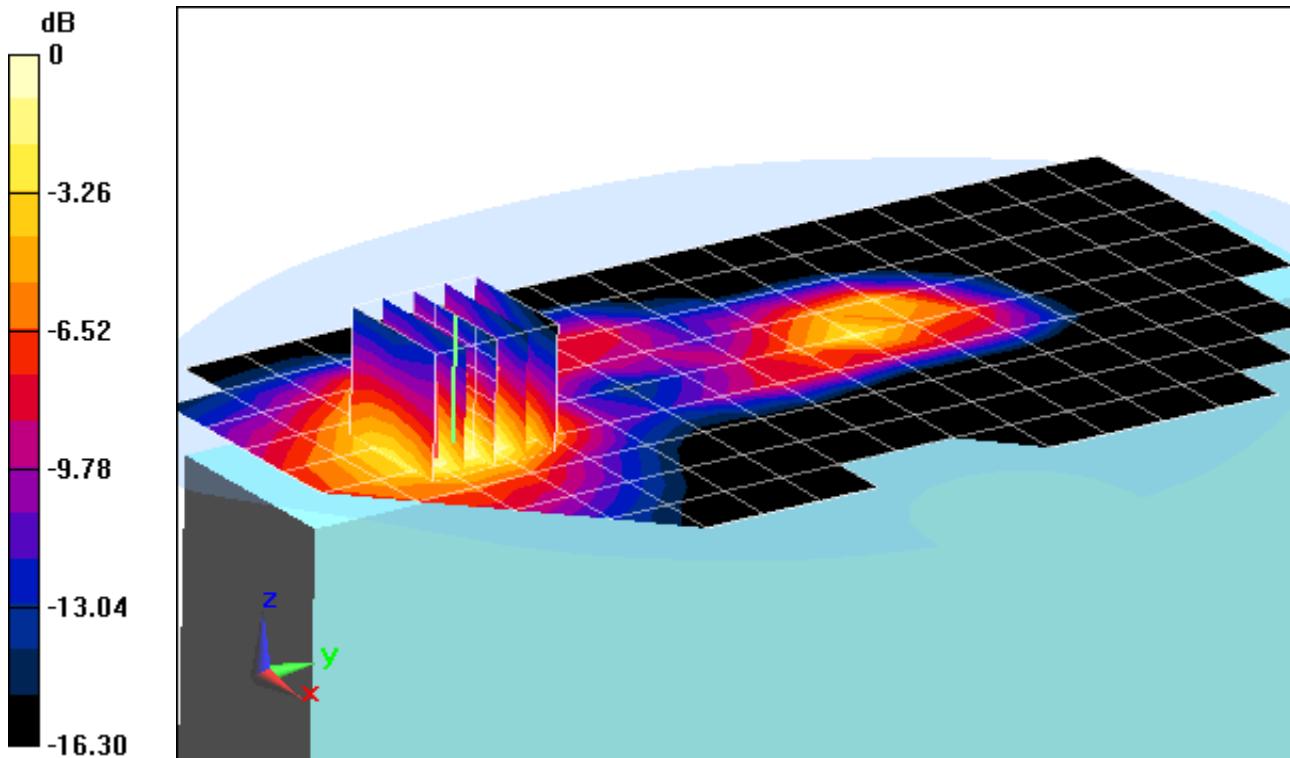

0 dB = 0.456 mW/g = -6.82 dB mW/g

PCTEST ENGINEERING LABORATORY, INC.

DUT: CF-19 mk6; Type: Portable Tablet Computer; Serial: 2CKSA00021

Communication System: AWS WCDMA; Frequency: 1730.4 MHz; Duty Cycle: 1:1

Medium: 1750 Body Medium parameters used (interpolated):

$f = 1730.4$ MHz; $\sigma = 1.487$ mho/m; $\epsilon_r = 52.702$; $\rho = 1000$ kg/m³

Phantom section: Flat Section; Space: 0.0 cm

Test Date: 05-21-2012; Ambient Temp: 23.4°C; Tissue Temp: 22.2°C

Probe: ES3DV2 - SN3022; ConvF(4.64, 4.64, 4.64); Calibrated: 8/25/2011;

Sensor-Surface: 4mm (Mechanical Surface Detection)

Electronics: DAE4 Sn665; Calibrated: 4/19/2012

Phantom: SAM Sub Dasy B; Type: SAM 5.0; Serial: TP-1626

Measurement SW: DASY4, Version 4.7 (80); SEMCAD X Version 14.6.5 (6469)

Mode: AWS WCDMA, Body SAR, Left Edge, Mid.ch


Area Scan (7x18x1): Measurement grid: dx=15mm, dy=15mm

Zoom Scan (5x5x7)/Cube 0: Measurement grid: dx=8mm, dy=8mm, dz=5mm

Reference Value = 20.854 V/m; Power Drift = -0.06 dB

Peak SAR (extrapolated) = 1.004 mW/g

SAR(1 g) = 0.617 mW/g; SAR(10 g) = 0.364 mW/g

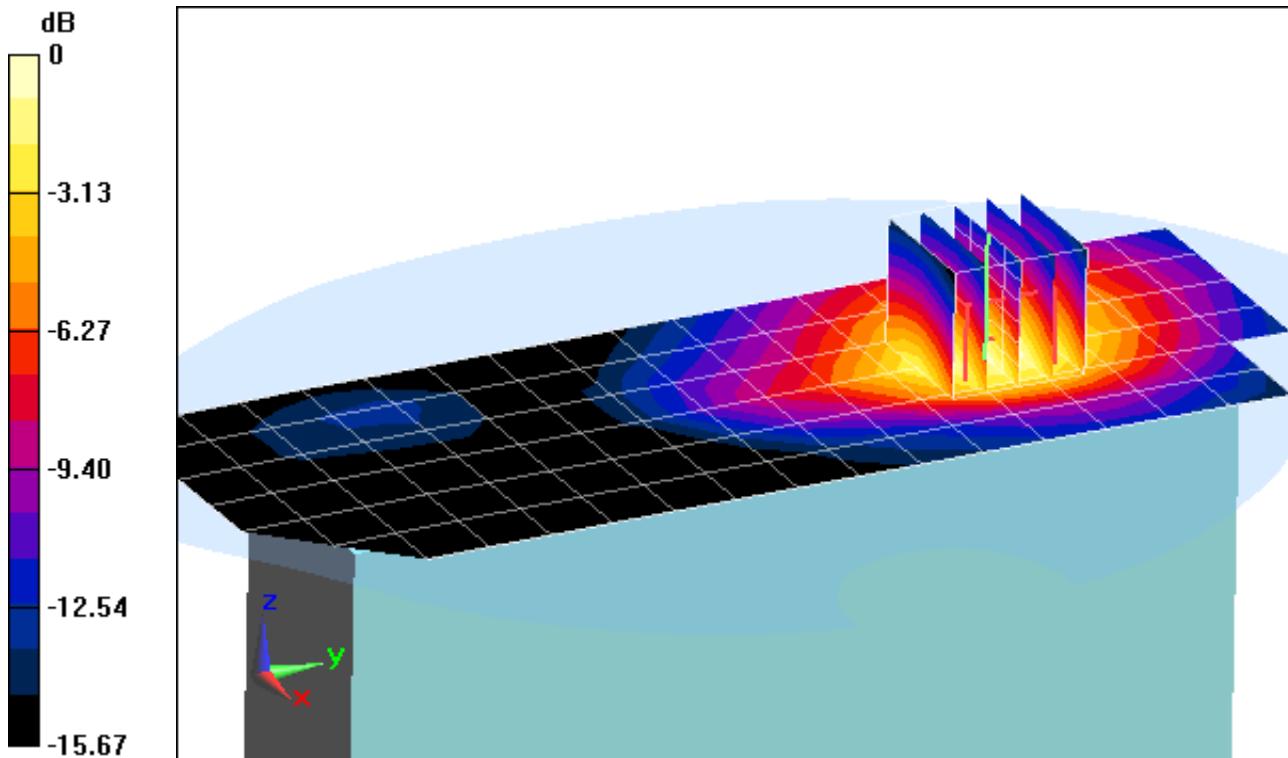

0 dB = 0.680 mW/g = -3.35 dB mW/g

PCTEST ENGINEERING LABORATORY, INC.

DUT: CF-19 mk6; Type: Portable Tablet Computer; Serial: 2CKSA00021

Communication System: GSM1900 GPRS; 2 Tx slots; Frequency: 1880 MHz; Duty Cycle: 1:4.15

Medium: 1900 Body Medium parameters used:

$f = 1880 \text{ MHz}$; $\sigma = 1.511 \text{ mho/m}$; $\epsilon_r = 51.79$; $\rho = 1000 \text{ kg/m}^3$

Phantom section: Flat Section; Space: 0.0 cm

Test Date: 05-15-2012; Ambient Temp: 24.2°C; Tissue Temp: 22.7°C

Probe: ES3DV3 - SN3209; ConvF(4.63, 4.63, 4.63); Calibrated: 3/16/2012;

Sensor-Surface: 4mm (Mechanical Surface Detection)

Electronics: DAE4 Sn1323; Calibrated: 2/15/2012

Phantom: SAM Sub; Type: SAM 4.0; Serial: TP-1357

Measurement SW: DASY4, Version 4.7 (80); SEMCAD X Version 14.6.5 (6469)

Mode: GPRS 1900, Body SAR, Back side, Mid.ch, 2 Tx Slots


Area Scan (13x21x1): Measurement grid: $dx=15\text{mm}$, $dy=15\text{mm}$

Zoom Scan (5x5x7)/Cube 0: Measurement grid: $dx=8\text{mm}$, $dy=8\text{mm}$, $dz=5\text{mm}$

Reference Value = 6.073 V/m; Power Drift = 0.04 dB

Peak SAR (extrapolated) = 0.085 mW/g

SAR(1 g) = 0.055 mW/g; SAR(10 g) = 0.033 mW/g

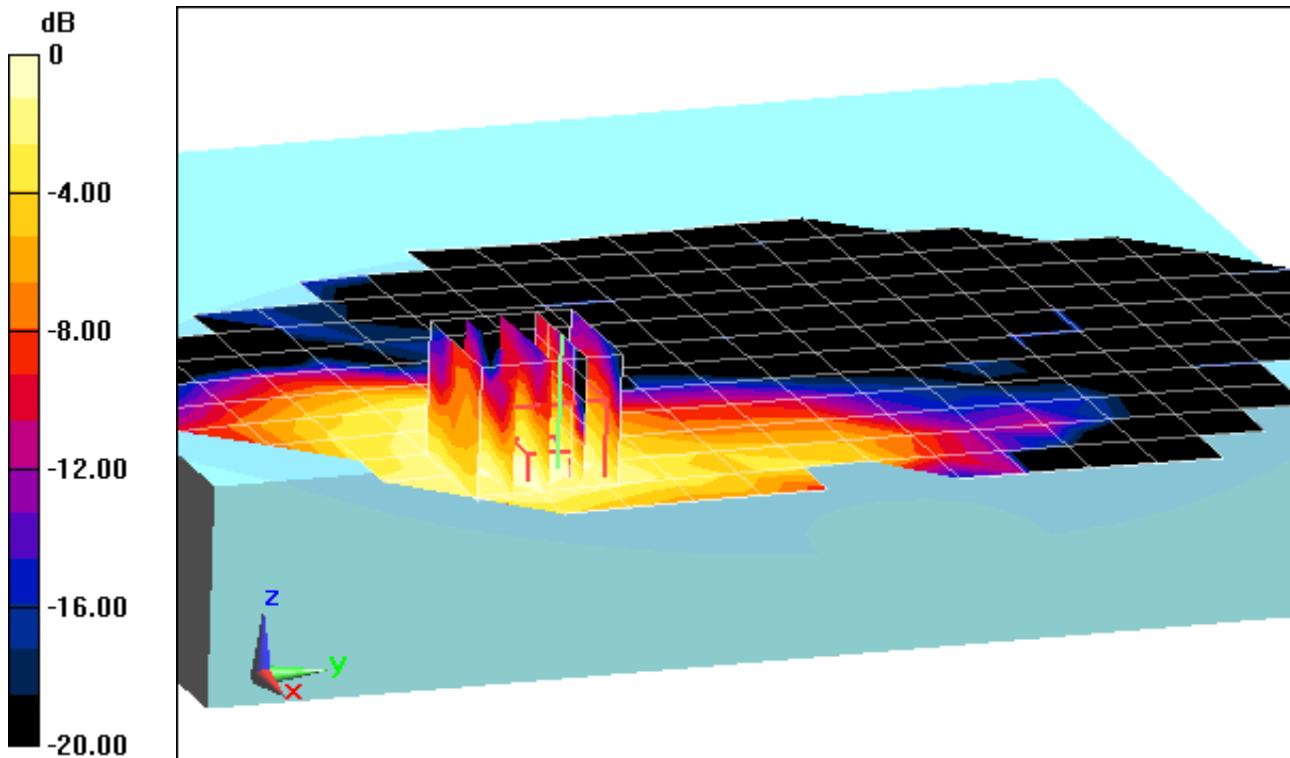

PCTEST ENGINEERING LABORATORY, INC.

DUT: CF-19 mk6; Type: Portable Tablet Computer; Serial: 2CKSA00021

Communication System: GSM1900 GPRS; 2 Tx slots; Frequency: 1880 MHz; Duty Cycle: 1:4.15

Medium: 1900 Body Medium parameters used:

$$f = 1880 \text{ MHz}; \sigma = 1.511 \text{ mho/m}; \epsilon_r = 51.79; \rho = 1000 \text{ kg/m}^3$$

Phantom section: Flat Section; Space: 0.0 cm

Test Date: 05-15-2012; Ambient Temp: 24.2°C; Tissue Temp: 22.7°C

Probe: ES3DV3 - SN3209; ConvF(4.63, 4.63, 4.63); Calibrated: 3/16/2012;

Sensor-Surface: 4mm (Mechanical Surface Detection)

Electronics: DAE4 Sn1323; Calibrated: 2/15/2012

Phantom: SAM Sub; Type: SAM 4.0; Serial: TP-1357

Measurement SW: DASY4, Version 4.7 (80); SEMCAD X Version 14.6.5 (6469)

Mode: GPRS 1900, Body SAR, Top Edge, Mid.ch, 2 Tx Slots


Area Scan (8x21x1): Measurement grid: dx=15mm, dy=15mm

Zoom Scan 2 (5x5x7)/Cube 0: Measurement grid: dx=8mm, dy=8mm, dz=5mm

Reference Value = 10.511 V/m; Power Drift = -0.12 dB

Peak SAR (extrapolated) = 0.275 mW/g

SAR(1 g) = 0.163 mW/g; SAR(10 g) = 0.098 mW/g

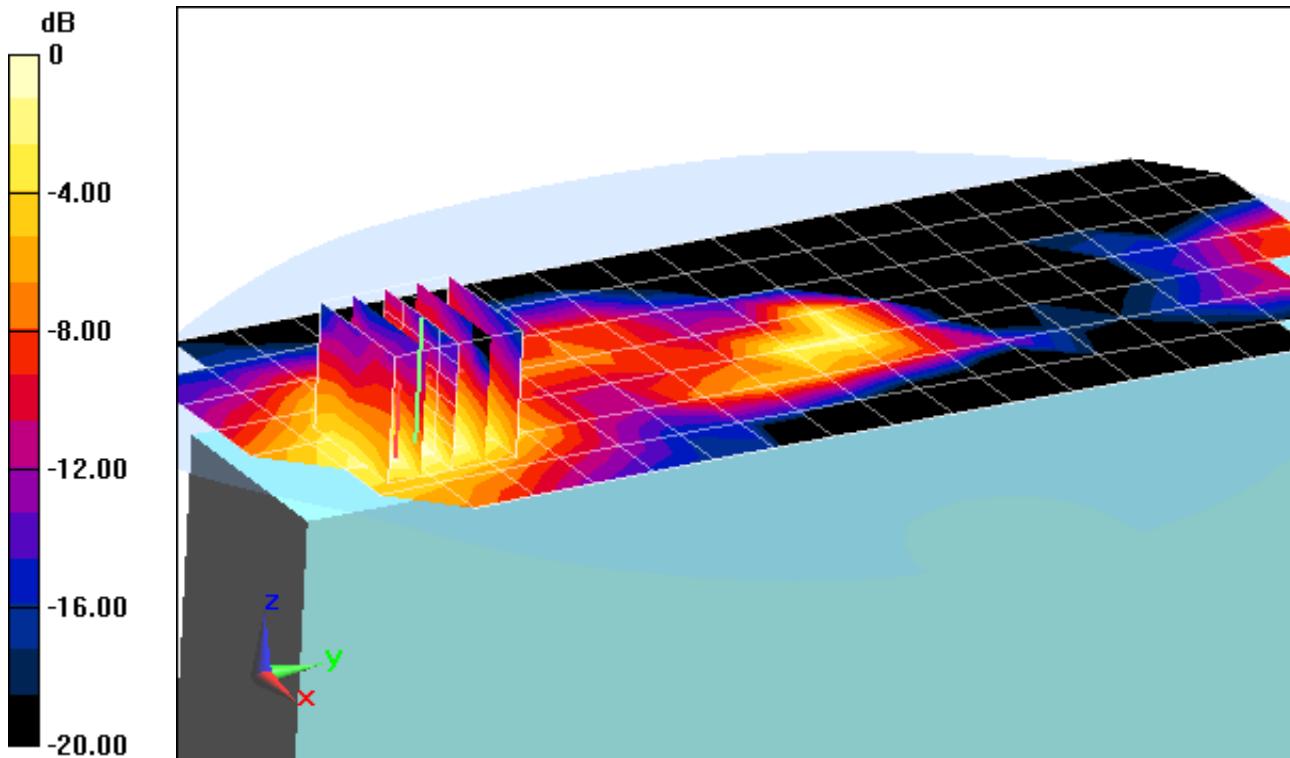

$$0 \text{ dB} = 0.178 \text{ mW/g} = -14.99 \text{ dB mW/g}$$

PCTEST ENGINEERING LABORATORY, INC.

DUT: CF-19 mk6; Type: Portable Tablet Computer; Serial: 2CKSA00021

Communication System: GSM1900 GPRS; 2 Tx slots; Frequency: 1880 MHz; Duty Cycle: 1:4.15

Medium: 1900 Body Medium parameters used:

$$f = 1880 \text{ MHz}; \sigma = 1.511 \text{ mho/m}; \epsilon_r = 51.79; \rho = 1000 \text{ kg/m}^3$$

Phantom section: Flat Section; Space: 0.0 cm

Test Date: 05-15-2012; Ambient Temp: 24.2°C; Tissue Temp: 22.7°C

Probe: ES3DV3 - SN3209; ConvF(4.63, 4.63, 4.63); Calibrated: 3/16/2012;

Sensor-Surface: 4mm (Mechanical Surface Detection)

Electronics: DAE4 Sn1323; Calibrated: 2/15/2012

Phantom: SAM Sub; Type: SAM 4.0; Serial: TP-1357

Measurement SW: DASY4, Version 4.7 (80); SEMCAD X Version 14.6.5 (6469)

Mode: GPRS 1900, Body SAR, Left Edge, Mid.ch, 2 Tx Slots


Area Scan (7x19x1): Measurement grid: dx=15mm, dy=15mm

Zoom Scan (5x5x7)/Cube 0: Measurement grid: dx=8mm, dy=8mm, dz=5mm

Reference Value = 17.814 V/m; Power Drift = -0.18 dB

Peak SAR (extrapolated) = 0.688 mW/g

SAR(1 g) = 0.424 mW/g; SAR(10 g) = 0.246 mW/g

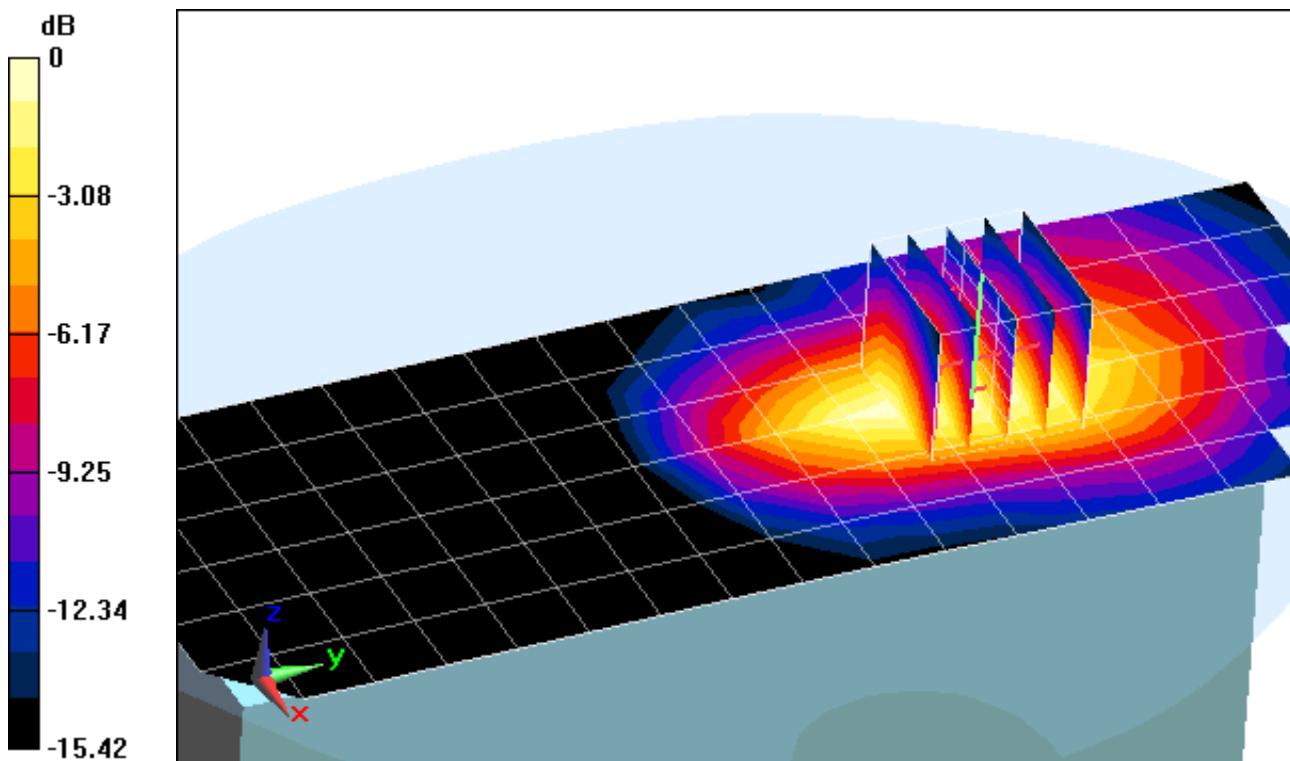

0 dB = 0.475 mW/g = -6.47 dB mW/g

PCTEST ENGINEERING LABORATORY, INC.

DUT: CF-19 mk6; Type: Portable Tablet Computer; Serial: 2CKSA00021

Communication System: WCDMA1900; Frequency: 1880 MHz; Duty Cycle: 1:1

Medium: 1900 Body Medium parameters used:

$f = 1880 \text{ MHz}$; $\sigma = 1.511 \text{ mho/m}$; $\epsilon_r = 51.79$; $\rho = 1000 \text{ kg/m}^3$

Phantom section: Flat Section; Space: 0.0 cm

Test Date: 05-15-2012; Ambient Temp: 24.2°C; Tissue Temp: 22.7°C

Probe: ES3DV3 - SN3209; ConvF(4.63, 4.63, 4.63); Calibrated: 3/16/2012;

Sensor-Surface: 4mm (Mechanical Surface Detection)

Electronics: DAE4 Sn1323; Calibrated: 2/15/2012

Phantom: SAM Sub; Type: SAM 4.0; Serial: TP-1357

Measurement SW: DASY4, Version 4.7 (80); SEMCAD X Version 14.6.5 (6469)

Mode: WCDMA 1900, Body SAR, Back side, Mid.ch


Area Scan (13x21x1): Measurement grid: $dx=15\text{mm}$, $dy=15\text{mm}$

Zoom Scan (5x5x7)/Cube 0: Measurement grid: $dx=8\text{mm}$, $dy=8\text{mm}$, $dz=5\text{mm}$

Reference Value = 5.359 V/m; Power Drift = 0.21 dB

Peak SAR (extrapolated) = 0.154 mW/g

SAR(1 g) = 0.096 mW/g; SAR(10 g) = 0.058 mW/g

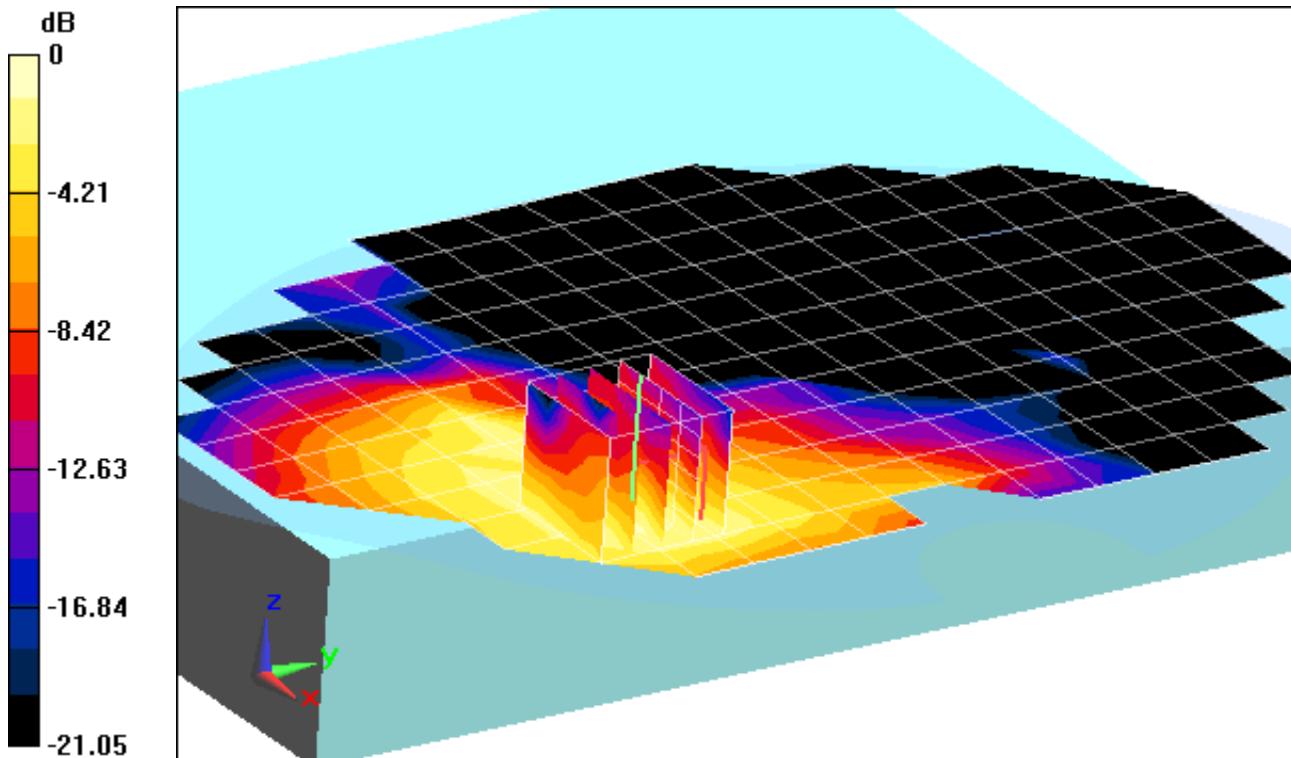

PCTEST ENGINEERING LABORATORY, INC.

DUT: CF-19 mk6; Type: Portable Tablet Computer; Serial: 2CKSA00021

Communication System: WCDMA1900; Frequency: 1880 MHz; Duty Cycle: 1:1

Medium: 1900 Body Medium parameters used:

$f = 1880 \text{ MHz}$; $\sigma = 1.511 \text{ mho/m}$; $\epsilon_r = 51.79$; $\rho = 1000 \text{ kg/m}^3$

Phantom section: Flat Section; Space: 0.0 cm

Test Date: 05-15-2012; Ambient Temp: 24.2°C; Tissue Temp: 22.7°C

Probe: ES3DV3 - SN3209; ConvF(4.63, 4.63, 4.63); Calibrated: 3/16/2012;

Sensor-Surface: 4mm (Mechanical Surface Detection)

Electronics: DAE4 Sn1323; Calibrated: 2/15/2012

Phantom: SAM Sub; Type: SAM 4.0; Serial: TP-1357

Measurement SW: DASY4, Version 4.7 (80); SEMCAD X Version 14.6.5 (6469)

Mode: WCDMA 1900, Body SAR, Top Edge, Mid.ch


Area Scan (8x21x1): Measurement grid: $dx=15\text{mm}$, $dy=15\text{mm}$

Zoom Scan (5x5x7)/Cube 0: Measurement grid: $dx=8\text{mm}$, $dy=8\text{mm}$, $dz=5\text{mm}$

Reference Value = 13.823 V/m; Power Drift = -0.05 dB

Peak SAR (extrapolated) = 0.479 mW/g

SAR(1 g) = 0.286 mW/g; SAR(10 g) = 0.175 mW/g

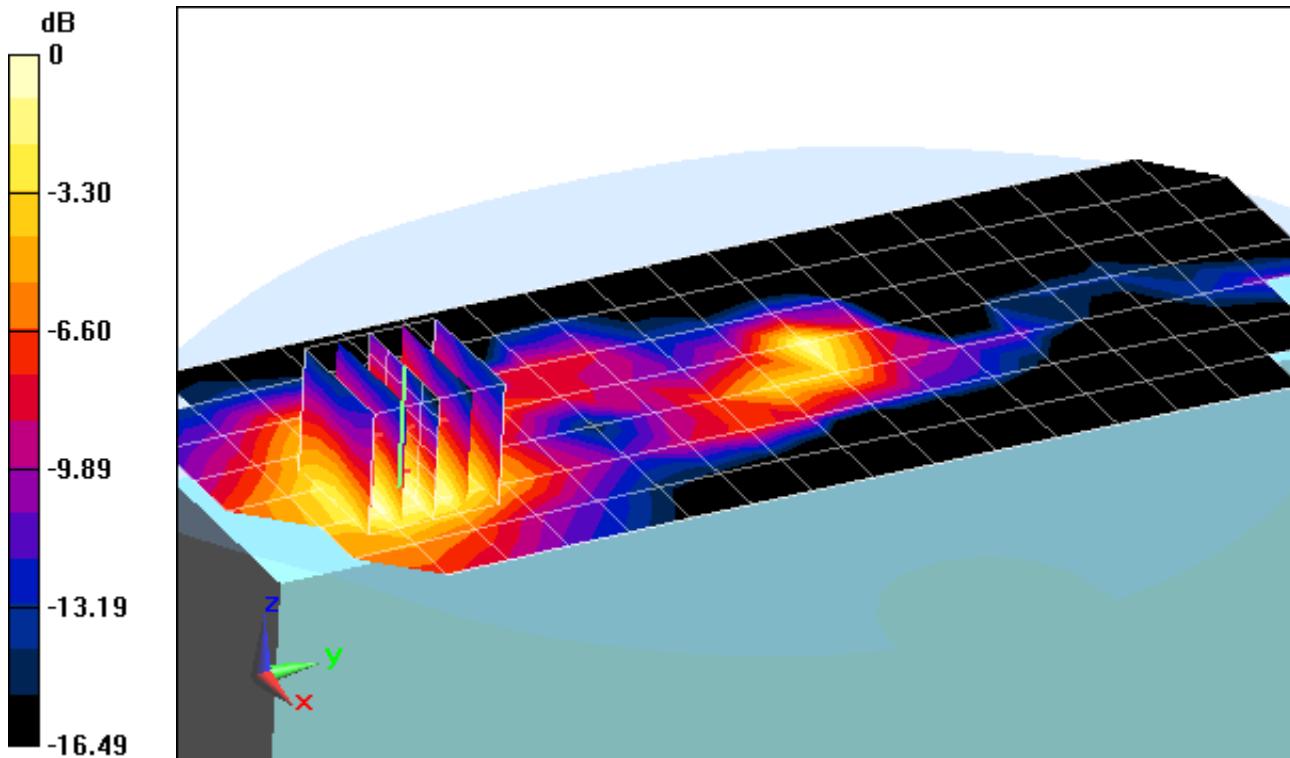

PCTEST ENGINEERING LABORATORY, INC.

DUT: CF-19 mk6; Type: Portable Tablet Computer; Serial: 2CKSA00021

Communication System: WCDMA1900; Frequency: 1880 MHz; Duty Cycle: 1:1

Medium: 1900 Body Medium parameters used:

$f = 1880 \text{ MHz}$; $\sigma = 1.511 \text{ mho/m}$; $\epsilon_r = 51.79$; $\rho = 1000 \text{ kg/m}^3$

Phantom section: Flat Section; Space: 0.0 cm

Test Date: 05-15-2012; Ambient Temp: 24.2°C; Tissue Temp: 22.7°C

Probe: ES3DV3 - SN3209; ConvF(4.63, 4.63, 4.63); Calibrated: 3/16/2012;

Sensor-Surface: 4mm (Mechanical Surface Detection)

Electronics: DAE4 Sn1323; Calibrated: 2/15/2012

Phantom: SAM Sub; Type: SAM 4.0; Serial: TP-1357

Measurement SW: DASY4, Version 4.7 (80); SEMCAD X Version 14.6.5 (6469)

Mode: WCDMA 1900, Body SAR, Left Edge, Mid.ch


Area Scan (7x19x1): Measurement grid: $dx=15\text{mm}$, $dy=15\text{mm}$

Zoom Scan (5x5x7)/Cube 0: Measurement grid: $dx=8\text{mm}$, $dy=8\text{mm}$, $dz=5\text{mm}$

Reference Value = 21.419 V/m; Power Drift = 0.18 dB

Peak SAR (extrapolated) = 1.166 mW/g

SAR(1 g) = 0.717 mW/g; SAR(10 g) = 0.418 mW/g

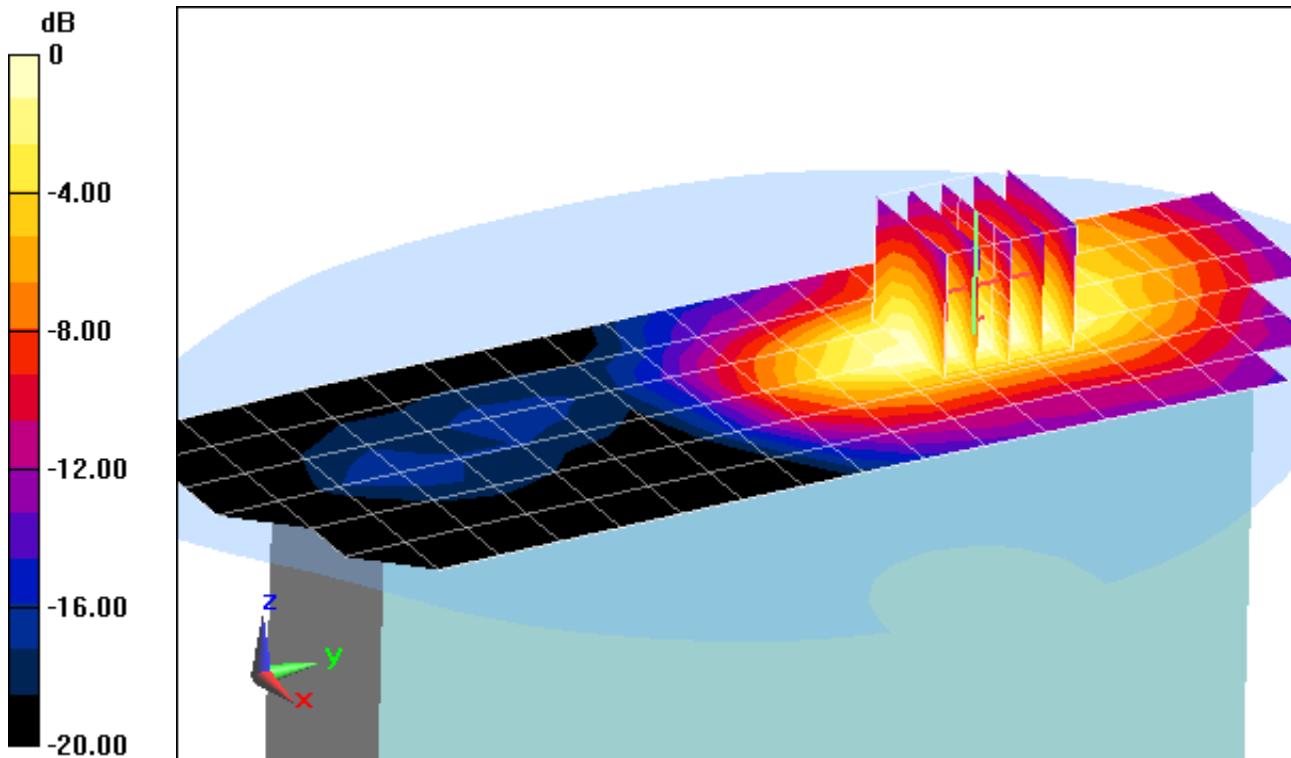

0 dB = 0.642 mW/g = -3.85 dB mW/g

PCTEST ENGINEERING LABORATORY, INC.

DUT: CF-19 mk6; Type: Portable Tablet Computer; Serial: 2CKSA00021

Communication System: CDMA; Frequency: 1880 MHz; Duty Cycle: 1:1

Medium: 1900 Body Medium parameters used:

$f = 1880$ MHz; $\sigma = 1.502$ mho/m; $\epsilon_r = 50.96$; $\rho = 1000$ kg/m³

Phantom section: Flat Section; Space: 0.0 cm

Test Date: 05-16-2012; Ambient Temp: 24.3°C; Tissue Temp: 23.2°C

Probe: EX3DV4 - SN3561; ConvF(6.58, 6.58, 6.58); Calibrated: 7/27/2011;

Sensor-Surface: 4mm (Mechanical Surface Detection)

Electronics: DAE4 Sn1333; Calibrated: 4/12/2012

Phantom: SAM 5.0 front; Type: QD000P40CD; Serial: TP:-1648

Measurement SW: DASY52, Version 52.8 (0); SEMCAD X Version 14.6.5 (6469)

Mode: PCS EVDO, Body SAR, Back side, Mid.ch


Area Scan (9x21x1): Measurement grid: dx=15mm, dy=15mm

Zoom Scan (5x5x7)/Cube 0: Measurement grid: dx=8mm, dy=8mm, dz=5mm

Reference Value = 6.025 V/m; Power Drift = 0.17 dB

Peak SAR (extrapolated) = 0.166 mW/g

SAR(1 g) = 0.105 mW/g; SAR(10 g) = 0.061 mW/g

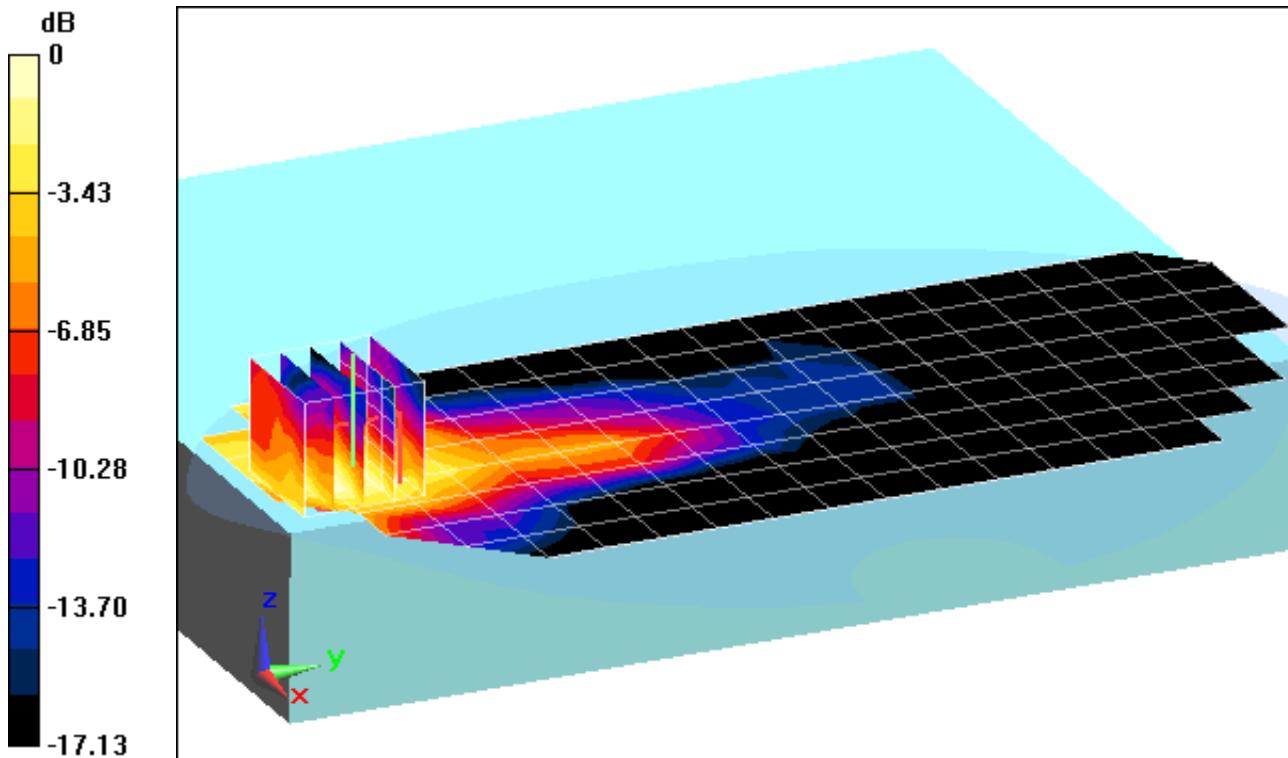

0 dB = 0.116 mW/g = -18.71 dB mW/g

PCTEST ENGINEERING LABORATORY, INC.

DUT: CF-19 mk6; Type: Portable Tablet Computer; Serial: 2CKSA00021

Communication System: CDMA; Frequency: 1880 MHz; Duty Cycle: 1:1

Medium: 1900 Body Medium parameters used:

$f = 1880$ MHz; $\sigma = 1.502$ mho/m; $\epsilon_r = 50.96$; $\rho = 1000$ kg/m³

Phantom section: Flat Section; Space: 0.0 cm

Test Date: 05-16-2012; Ambient Temp: 24.3°C; Tissue Temp: 23.2°C

Probe: EX3DV4 - SN3561; ConvF(6.58, 6.58, 6.58); Calibrated: 7/27/2011;

Sensor-Surface: 4mm (Mechanical Surface Detection)

Electronics: DAE4 Sn1333; Calibrated: 4/12/2012

Phantom: SAM 5.0 front; Type: QD000P40CD; Serial: TP:-1648

Measurement SW: DASY52, Version 52.8 (0); SEMCAD X Version 14.6.5 (6469)

Mode: PCS EVDO, Body SAR, Top Edge, Mid.ch


Area Scan (9x21x1): Measurement grid: dx=15mm, dy=15mm

Zoom Scan (5x5x7)/Cube 0: Measurement grid: dx=8mm, dy=8mm, dz=5mm

Reference Value = 13.516 V/m; Power Drift = -0.20 dB

Peak SAR (extrapolated) = 0.462 mW/g

SAR(1 g) = 0.259 mW/g; SAR(10 g) = 0.142 mW/g

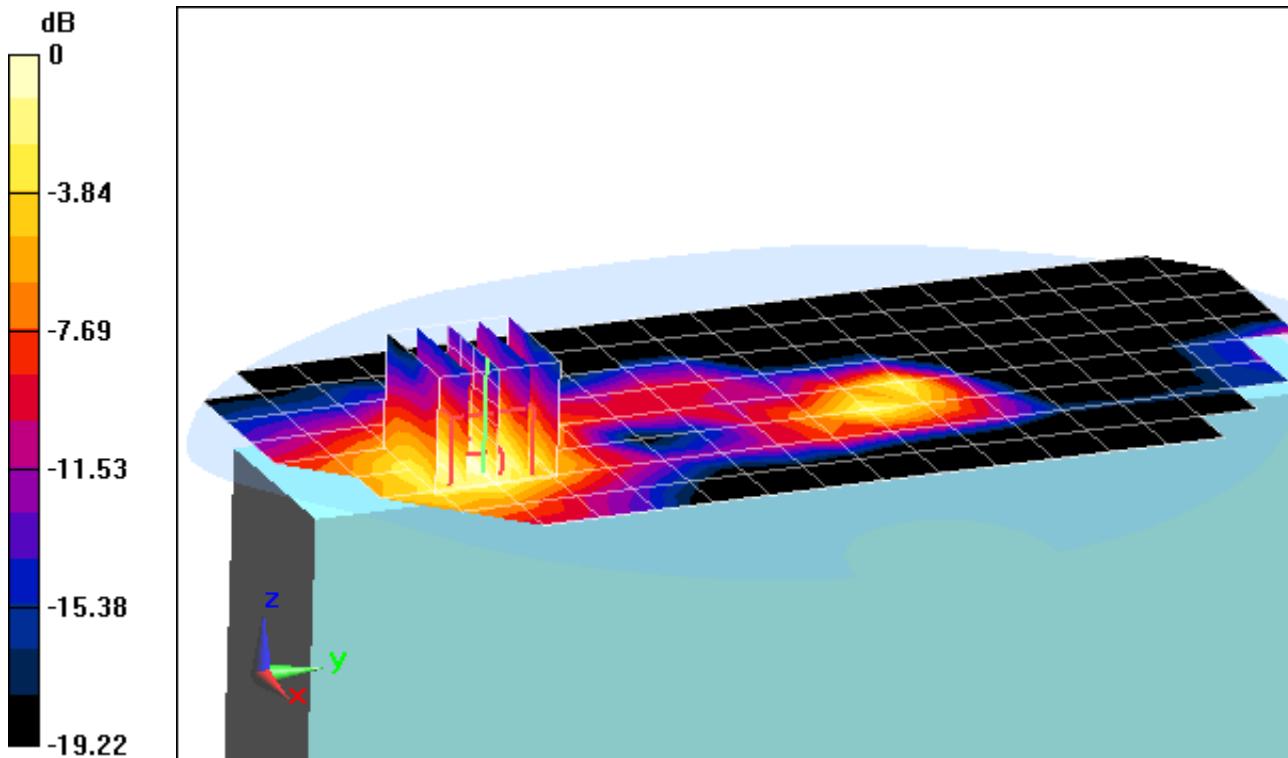

PCTEST ENGINEERING LABORATORY, INC.

DUT: CF-19 mk6; Type: Portable Tablet Computer; Serial: 2CKSA00021

Communication System: CDMA; Frequency: 1880 MHz; Duty Cycle: 1:1

Medium: 1900 Body Medium parameters used:

$f = 1880$ MHz; $\sigma = 1.502$ mho/m; $\epsilon_r = 50.96$; $\rho = 1000$ kg/m³

Phantom section: Flat Section; Space: 0.0 cm

Test Date: 05-16-2012; Ambient Temp: 24.3°C; Tissue Temp: 23.2°C

Probe: EX3DV4 - SN3561; ConvF(6.58, 6.58, 6.58); Calibrated: 7/27/2011;

Sensor-Surface: 4mm (Mechanical Surface Detection)

Electronics: DAE4 Sn1333; Calibrated: 4/12/2012

Phantom: SAM 5.0 front; Type: QD000P40CD; Serial: TP:-1648

Measurement SW: DASY52, Version 52.8 (0); SEMCAD X Version 14.6.5 (6469)

Mode: PCS EVDO, Body SAR, Left Edge, Mid.ch


Area Scan (9x19x1): Measurement grid: dx=15mm, dy=15mm

Zoom Scan (5x5x7)/Cube 0: Measurement grid: dx=8mm, dy=8mm, dz=5mm

Reference Value = 20.281 V/m; Power Drift = -0.01 dB

Peak SAR (extrapolated) = 1.068 mW/g

SAR(1 g) = 0.662 mW/g; SAR(10 g) = 0.387 mW/g

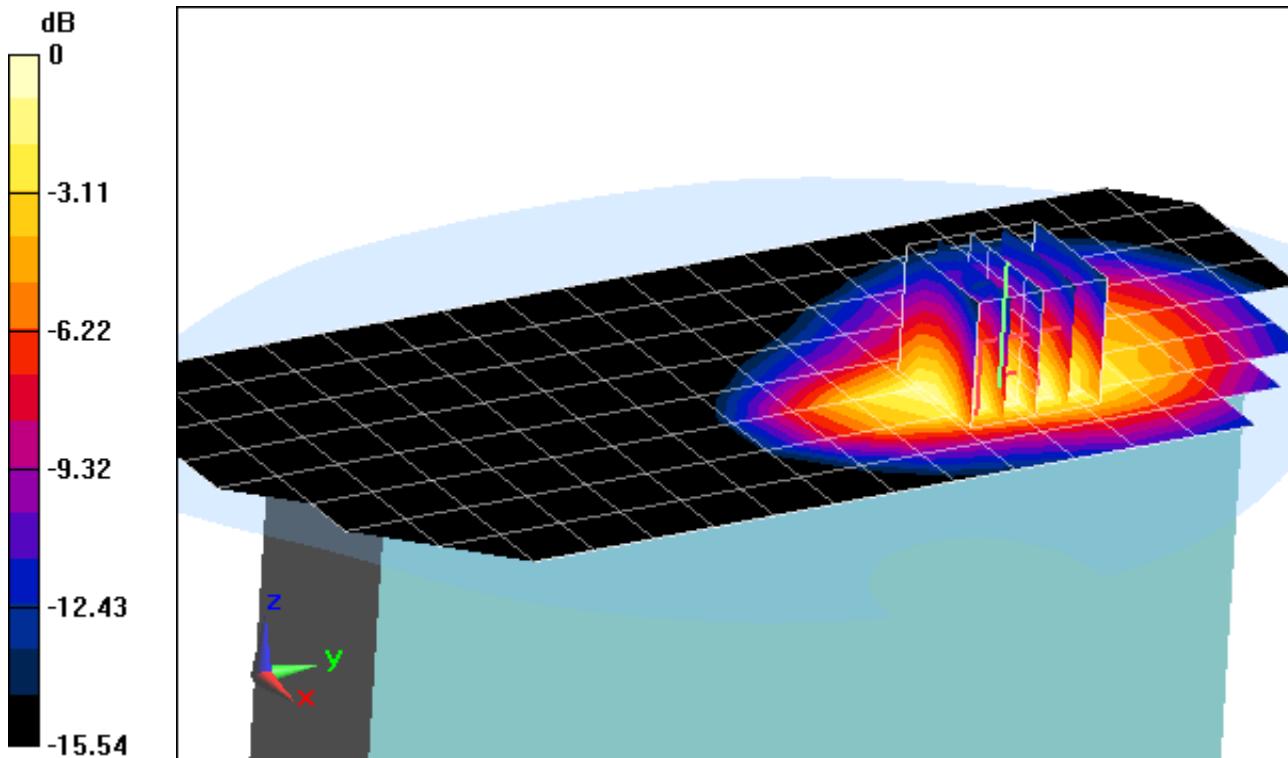

0 dB = 0.731 mW/g = -2.72 dB mW/g

APPENDIX B: SYSTEM VERIFICATION

PCTEST ENGINEERING LABORATORY, INC.

DUT: SAR Dipole 835 MHz; Type: D835V2; Serial: 4d047

Communication System: CW; Frequency: 835 MHz; Duty Cycle: 1:1

Medium: 835 Body Medium parameters used:

$f = 835 \text{ MHz}$; $\sigma = 0.972 \text{ mho/m}$; $\epsilon_r = 52.99$; $\rho = 1000 \text{ kg/m}^3$

Phantom section: Flat Section; Space: 1.5 cm

Test Date: 05-21-2012; Ambient Temp: 23.9°C; Tissue Temp: 22.4°C

Probe: EX3DV4 - SN3561; ConvF(8.25, 8.25, 8.25); Calibrated: 7/27/2011

Sensor-Surface: 4mm (Mechanical Surface Detection)

Electronics: DAE4 Sn1333; Calibrated: 4/12/2012

Phantom: SAM 5.0 front; Type: QD000P40CD; Serial: TP:-1648

Measurement SW: DASY52, Version 52.8 (3); SEMCAD X Version 14.6.7 (868);)

835 MHz System Verification


Area Scan (7x14x1): Measurement grid: $dx=15\text{mm}$, $dy=15\text{mm}$

Zoom Scan (5x5x7)/Cube 0: Measurement grid: $dx=8\text{mm}$, $dy=8\text{mm}$, $dz=5\text{mm}$

Input Power = 24.0 dBm (250 mW)

SAR(1 g) = 2.47 mW/g; SAR(10 g) = 1.63 mW/g

Deviation = 4.99 %

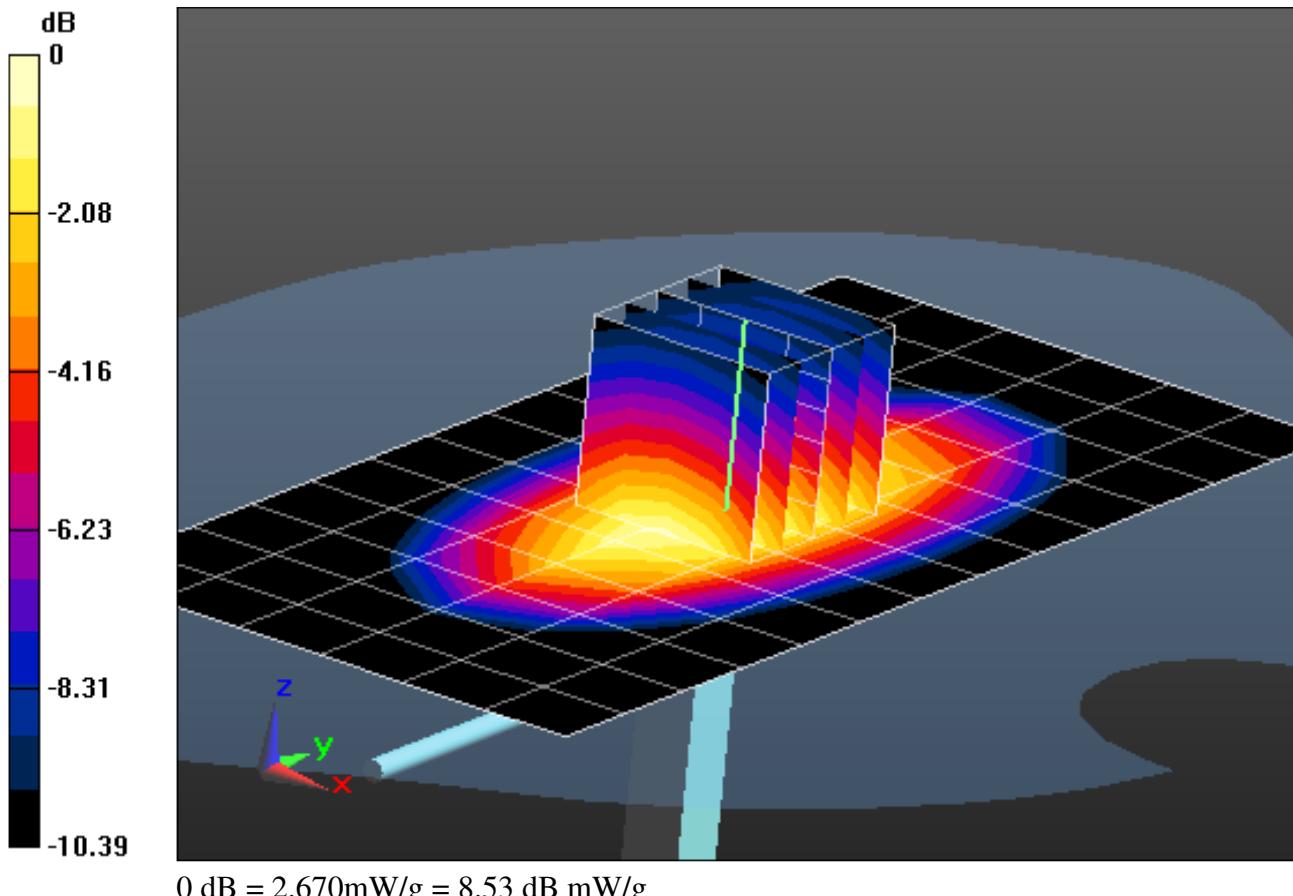

PCTEST ENGINEERING LABORATORY, INC.

DUT: SAR Dipole 835 MHz; Type: D835V2; Serial: 4d047

Communication System: CW; Frequency: 835 MHz; Duty Cycle: 1:1

Medium: 835 Body Medium parameters used:

$f = 835$ MHz; $\sigma = 0.972$ mho/m; $\epsilon_r = 52.99$; $\rho = 1000$ kg/m³

Phantom section: Flat Section; Space: 1.5 cm

Test Date: 05-21-2012; Ambient Temp: 23.9°C; Tissue Temp: 22.4°C

Probe: EX3DV4 - SN3561; ConvF(8.25, 8.25, 8.25); Calibrated: 7/27/2011

Sensor-Surface: 4mm (Mechanical Surface Detection)

Electronics: DAE4 Sn1333; Calibrated: 4/12/2012

Phantom: SAM 5.0 front; Type: QD000P40CD; Serial: TP:-1648

Measurement SW: DASY52, Version 52.8 (3); SEMCAD X Version 14.6.7 (868;)

835 MHz System Verification


Area Scan (7x14x1): Measurement grid: dx=15mm, dy=15mm

Zoom Scan (5x5x7)/Cube 0: Measurement grid: dx=8mm, dy=8mm, dz=5mm

Input Power = 24.0 dBm (250 mW)

SAR(1 g) = 2.47 mW/g; SAR(10 g) = 1.63 mW/g

Deviation = 4.99 %

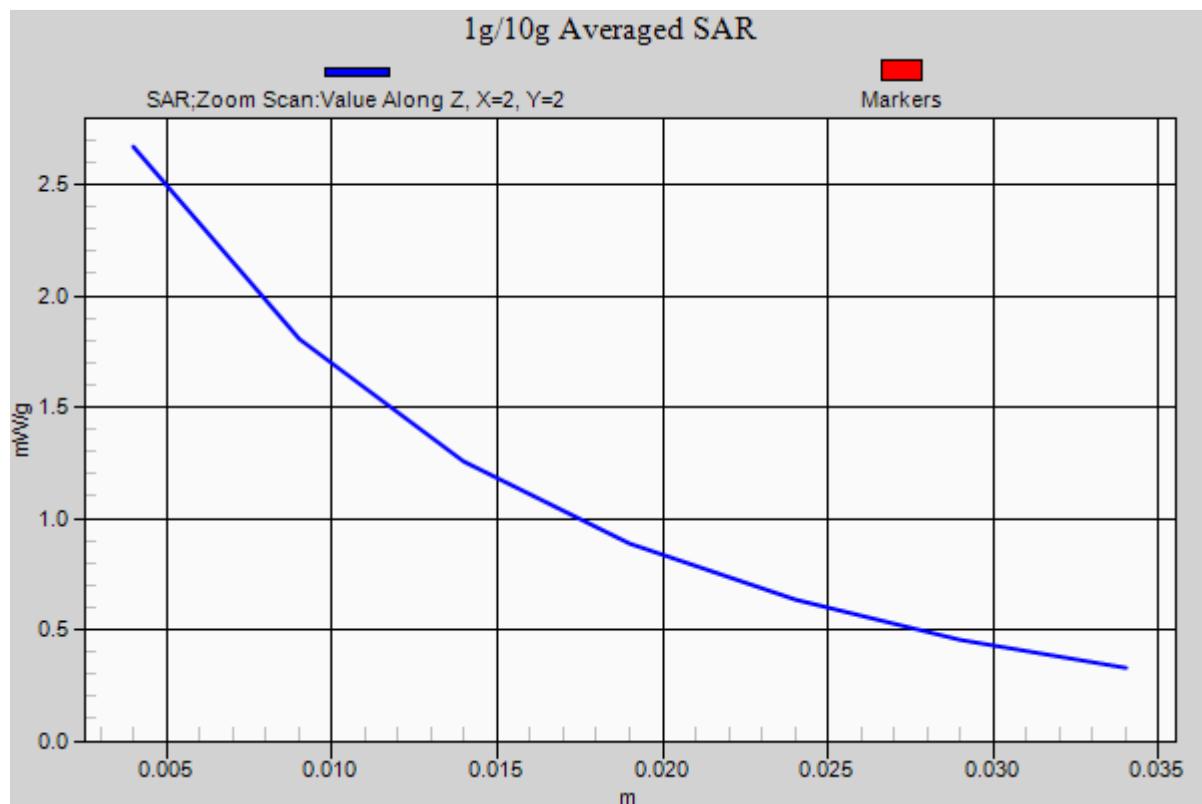

PCTEST ENGINEERING LABORATORY, INC.

DUT: Dipole 1750 MHz; Type: D1750V2; Serial: 1051

Communication System: CW; Frequency: 1750 MHz; Duty Cycle: 1:1

Medium: 1750 Body Medium parameters used:

$f = 1750 \text{ MHz}$; $\sigma = 1.508 \text{ mho/m}$; $\epsilon_r = 52.56$; $\rho = 1000 \text{ kg/m}^3$

Phantom section: Flat Section; Space: 1.0 cm

Test Date: 05-21-2012; Ambient Temp: 23.4°C; Tissue Temp: 22.2°C

Probe: ES3DV2 - SN3022; ConvF(4.64, 4.64, 4.64); Calibrated: 8/25/2011

Sensor-Surface: 4mm (Mechanical Surface Detection)

Electronics: DAE4 Sn665; Calibrated: 4/19/2012

Phantom: SAM Sub Dasy B; Type: SAM 5.0; Serial: TP-1626

Measurement SW: DASY4, Version 4.7 (80); SEMCAD X Version 14.6.7 (868);)

1750 MHz System Verification


Area Scan (6x6x1): Measurement grid: $dx=15\text{mm}$, $dy=15\text{mm}$

Zoom Scan (5x5x7)/Cube 0: Measurement grid: $dx=8\text{mm}$, $dy=8\text{mm}$, $dz=5\text{mm}$

Input Power = 20 dBm (100 mW)

SAR(1 g) = 3.72 mW/g; SAR(10 g) = 1.95 mW/g

Deviation = -1.06%

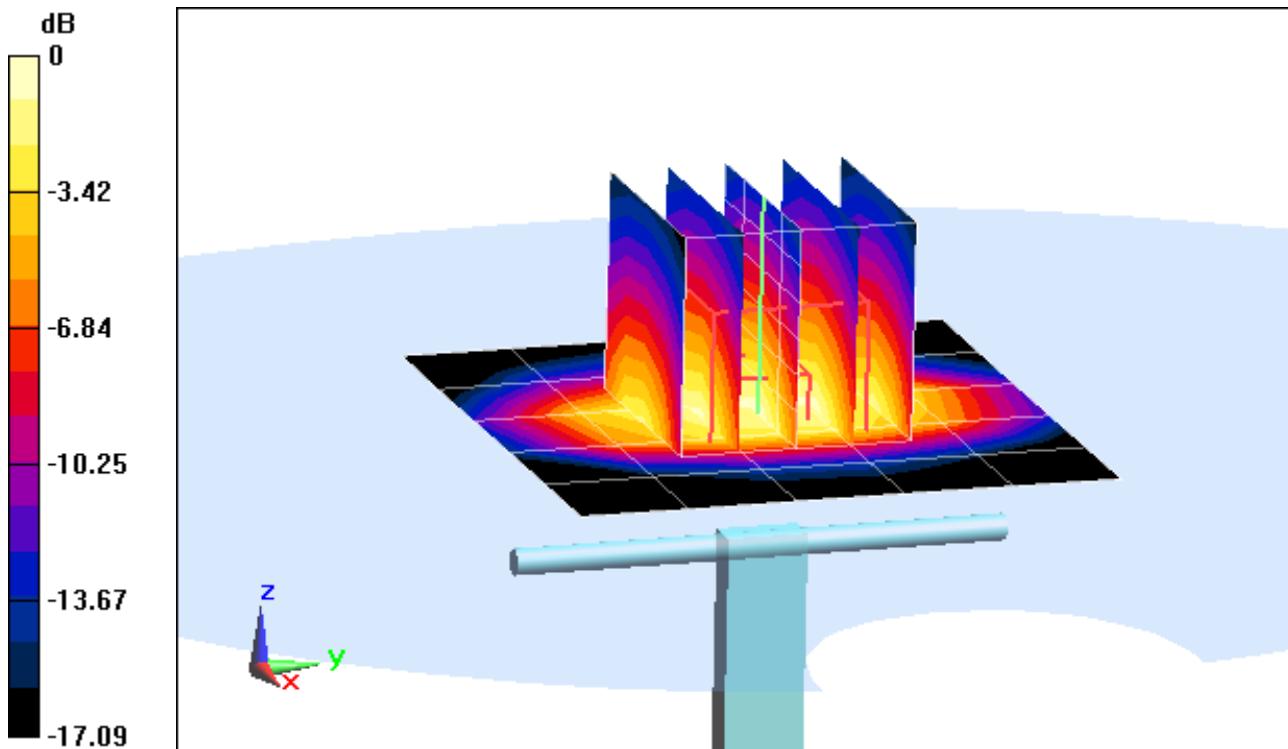

PCTEST ENGINEERING LABORATORY, INC.

DUT: Dipole 1750 MHz; Type: D1750V2; Serial: 1051

Communication System: CW; Frequency: 1750 MHz; Duty Cycle: 1:1

Medium: 1750 Body Medium parameters used:

$f = 1750 \text{ MHz}$; $\sigma = 1.508 \text{ mho/m}$; $\epsilon_r = 52.56$; $\rho = 1000 \text{ kg/m}^3$

Phantom section: Flat Section; Space: 1.0 cm

Test Date: 05-21-2012; Ambient Temp: 23.4°C; Tissue Temp: 22.2°C

Probe: ES3DV2 - SN3022; ConvF(4.64, 4.64, 4.64); Calibrated: 8/25/2011

Sensor-Surface: 4mm (Mechanical Surface Detection)

Electronics: DAE4 Sn665; Calibrated: 4/19/2012

Phantom: SAM Sub Dasy B; Type: SAM 5.0; Serial: TP-1626

Measurement SW: DASY4, Version 4.7 (80); SEMCAD X Version 14.6.5 (6469)

1750 MHz System Verification


Area Scan (6x6x1): Measurement grid: $dx=15\text{mm}$, $dy=15\text{mm}$

Zoom Scan (5x5x7)/Cube 0: Measurement grid: $dx=8\text{mm}$, $dy=8\text{mm}$, $dz=5\text{mm}$

Input Power = 20 dBm (100 mW)

SAR(1 g) = 3.72 mW/g; SAR(10 g) = 1.95 mW/g

Deviation = -1.06%

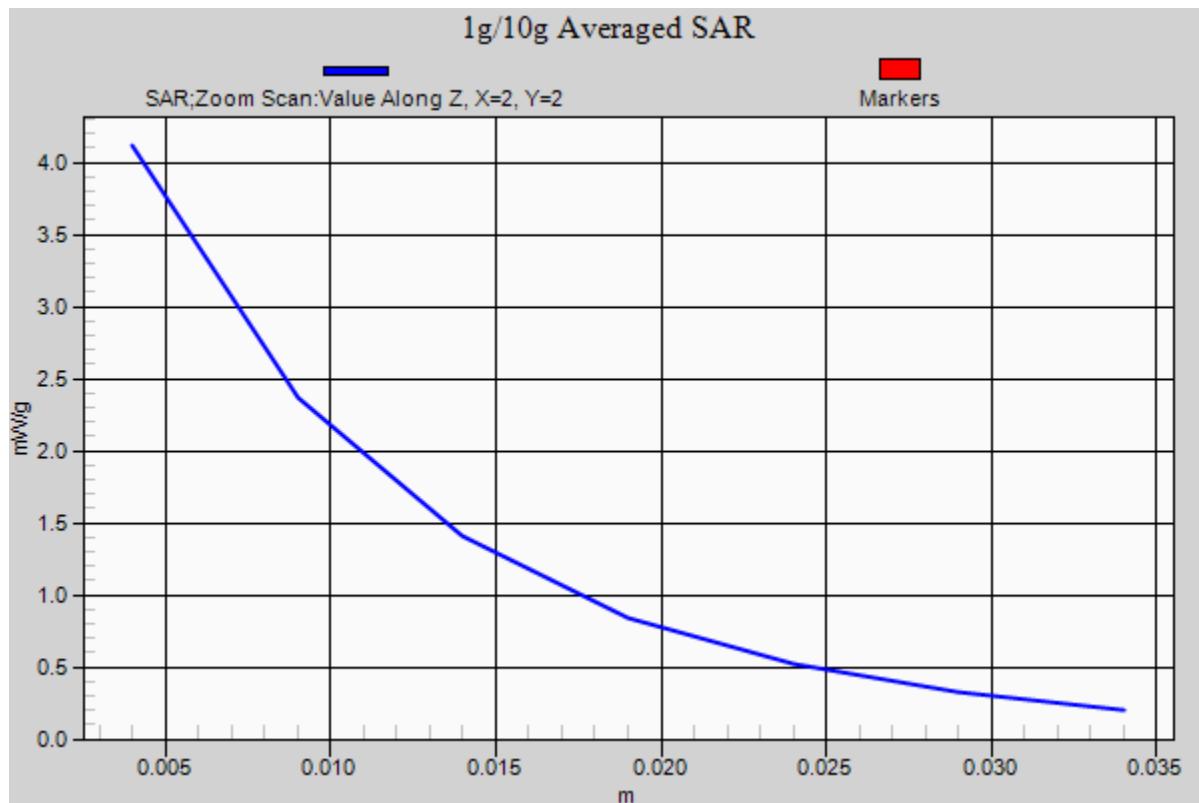

PCTEST ENGINEERING LABORATORY, INC.

DUT: SAR Dipole 1900 MHz; Type: D1900V2; Serial: 5d080

Communication System: CW; Frequency: 1900 MHz; Duty Cycle: 1:1

Medium: 1900 Body Medium parameters used (interpolated):

$f = 1900$ MHz; $\sigma = 1.529$ mho/m; $\epsilon_r = 51.777$; $\rho = 1000$ kg/m³

Phantom section: Flat Section; Space: 1.0 cm

Test Date: 05-15-2012; Ambient Temp: 24.2°C; Tissue Temp: 22.7°C

Probe: ES3DV3 - SN3209; ConvF(4.63, 4.63, 4.63); Calibrated: 3/16/2012;

Sensor-Surface: 4mm (Mechanical Surface Detection)

Electronics: DAE4 Sn1323; Calibrated: 2/15/2012

Phantom: SAM Sub; Type: SAM 4.0; Serial: TP-1357

Measurement SW: DASY4, Version 4.7 (80); SEMCAD X Version 14.6.5 (6469)

1900MHz System Verification


Area Scan (5x7x1): Measurement grid: dx=15mm, dy=15mm

Zoom Scan (5x5x7)/Cube 0: Measurement grid: dx=8mm, dy=8mm, dz=5mm

Input Power = 20 dBm (100 mW)

SAR(1 g) = 4.17 mW/g; SAR(10 g) = 2.16 mW/g

Deviation = 1.96%

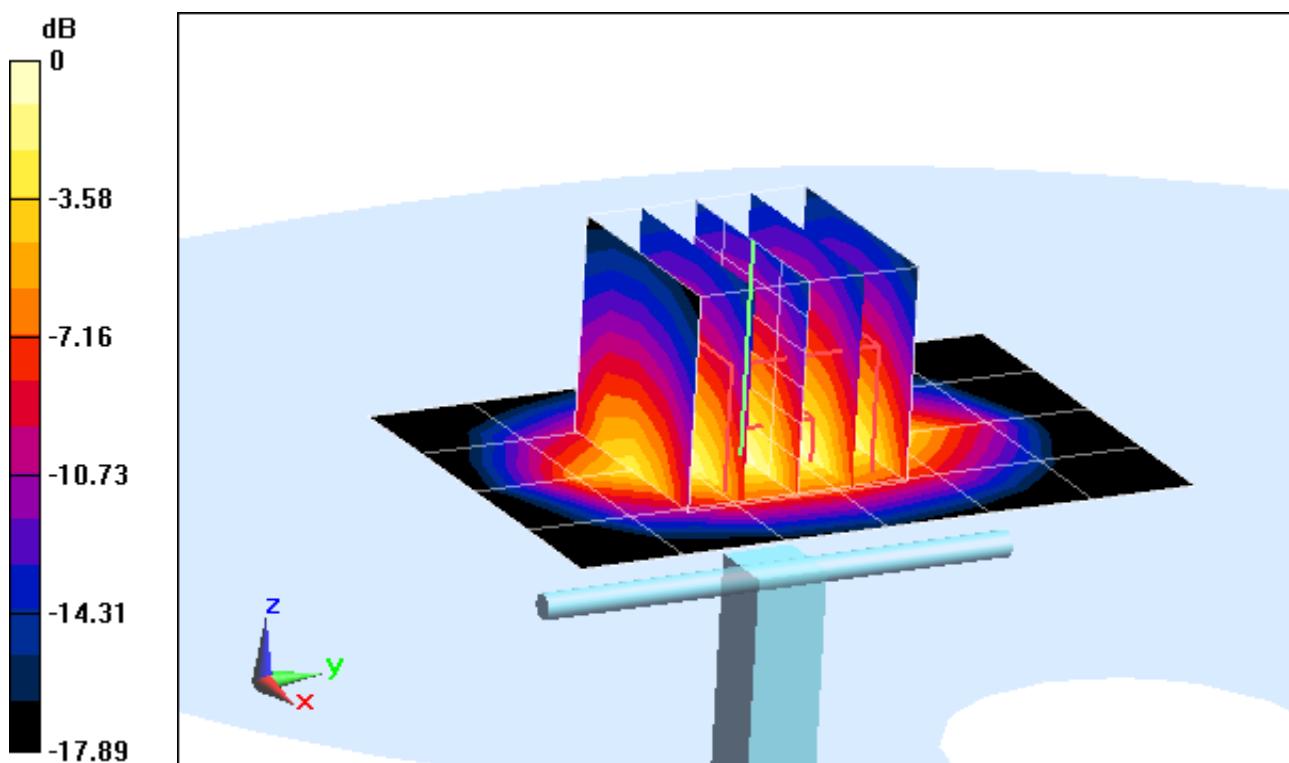

0 dB = 4.66 mW/g = 13.37 dB mW/g

PCTEST ENGINEERING LABORATORY, INC.

DUT: SAR Dipole 1900 MHz; Type: D1900V2; Serial: 5d080

Communication System: CW; Frequency: 1900 MHz; Duty Cycle: 1:1

Medium: 1900 Body Medium parameters used (interpolated):

$f = 1900$ MHz; $\sigma = 1.529$ mho/m; $\epsilon_r = 51.777$; $\rho = 1000$ kg/m³

Phantom section: Flat Section; Space: 1.0 cm

Test Date: 05-15-2012; Ambient Temp: 24.2°C; Tissue Temp: 22.7°C

Probe: ES3DV3 - SN3209; ConvF(4.63, 4.63, 4.63); Calibrated: 3/16/2012;

Sensor-Surface: 4mm (Mechanical Surface Detection)

Electronics: DAE4 Sn1323; Calibrated: 2/15/2012

Phantom: SAM Sub; Type: SAM 4.0; Serial: TP-1357

Measurement SW: DASY4, Version 4.7 (80); SEMCAD X Version 14.6.5 (6469)

1900MHz System Verification


Area Scan (5x7x1): Measurement grid: dx=15mm, dy=15mm

Zoom Scan (5x5x7)/Cube 0: Measurement grid: dx=8mm, dy=8mm, dz=5mm

Input Power = 20 dBm (100 mW)

SAR(1 g) = 4.17 mW/g; SAR(10 g) = 2.16 mW/g

Deviation = 1.96%

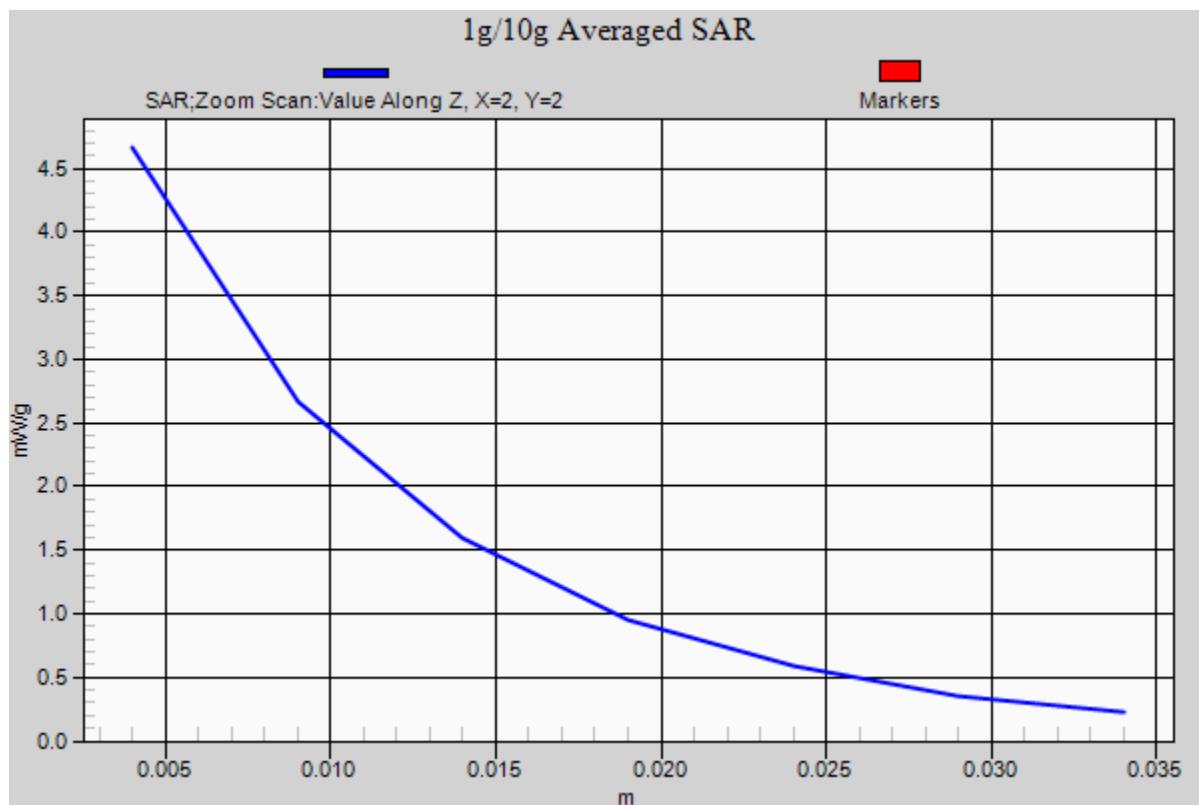

PCTEST ENGINEERING LABORATORY, INC.

DUT: SAR Dipole 1900 MHz; Type: D1900V2; Serial: 5d149

Communication System: CW; Frequency: 1900 MHz; Duty Cycle: 1:1

Medium: 1900 Body; Medium parameters used (interpolated):

$f = 1900$ MHz; $\sigma = 1.523$ mho/m; $\epsilon_r = 50.907$; $\rho = 1000$ kg/m³

Phantom section: Flat Section; Space: 1.0 cm

Test Date: 05-16-2012; Ambient Temp: 24.3°C; Tissue Temp: 23.2°C

Probe: EX3DV4 - SN3561; ConvF(6.58, 6.58, 6.58); Calibrated: 7/27/2011

Sensor-Surface: 4mm (Mechanical Surface Detection)

Electronics: DAE4 Sn1333; Calibrated: 4/12/2012

Phantom: SAM 5.0 front; Type: SAM v5.0; Serial: TP:-1648

Measurement SW: DASY52, Version 52.8 (0); SEMCAD X Version 14.6.5 (6469)

1900 MHz System Verification


Area Scan (7x9x1): Measurement grid: dx=15mm, dy=15mm

Zoom Scan (5x5x7)/Cube 0: Measurement grid: dx=8mm, dy=8mm, dz=5mm

Input Power = 20.0 dB (100 mW)

SAR(1 g) = 4.18 mW/g; SAR(10 g) = 2.21 mW/g

Deviation = 6.36%

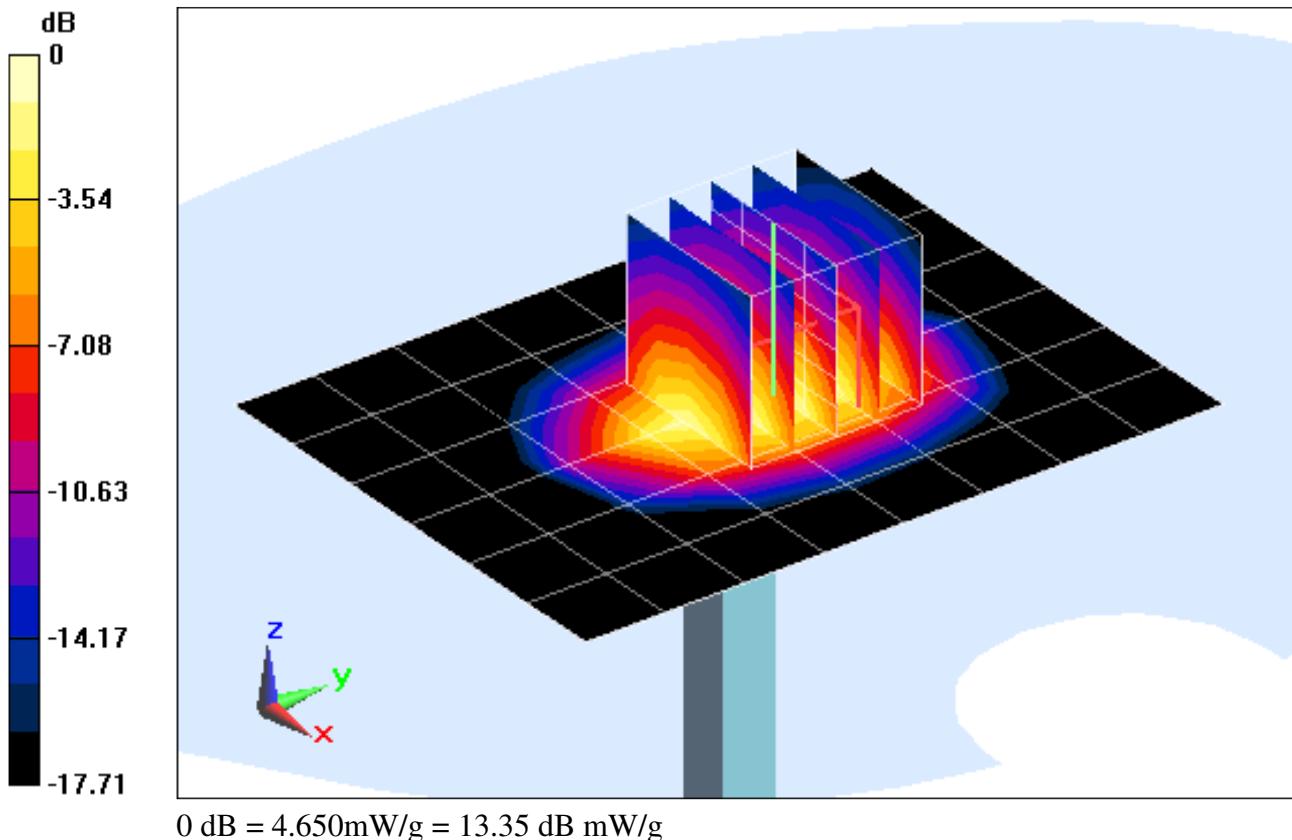

PCTEST ENGINEERING LABORATORY, INC.

DUT: SAR Dipole 1900 MHz; Type: D1900V2; Serial: 5d149

Communication System: CW; Frequency: 1900 MHz; Duty Cycle: 1:1

Medium: 1900 Body; Medium parameters used (interpolated):

$f = 1900 \text{ MHz}$; $\sigma = 1.523 \text{ mho/m}$; $\epsilon_r = 50.907$; $\rho = 1000 \text{ kg/m}^3$

Phantom section: Flat Section; Space: 1.0 cm

Test Date: 05-16-2012; Ambient Temp: 24.3°C; Tissue Temp: 23.2°C

Probe: EX3DV4 - SN3561; ConvF(6.58, 6.58, 6.58); Calibrated: 7/27/2011

Sensor-Surface: 4mm (Mechanical Surface Detection)

Electronics: DAE4 Sn1333; Calibrated: 4/12/2012

Phantom: SAM 5.0 front; Type: SAM v5.0; Serial: TP:-1648

Measurement SW: DASY52, Version 52.8 (0); SEMCAD X Version 14.6.5 (6469)

1900 MHz System Verification


Area Scan (7x9x1): Measurement grid: $dx=15\text{mm}$, $dy=15\text{mm}$

Zoom Scan (5x5x7)/Cube 0: Measurement grid: $dx=8\text{mm}$, $dy=8\text{mm}$, $dz=5\text{mm}$

Input Power = 20.0 dB (100 mW)

SAR(1 g) = 4.18 mW/g; SAR(10 g) = 2.21 mW/g

Deviation = 6.36%

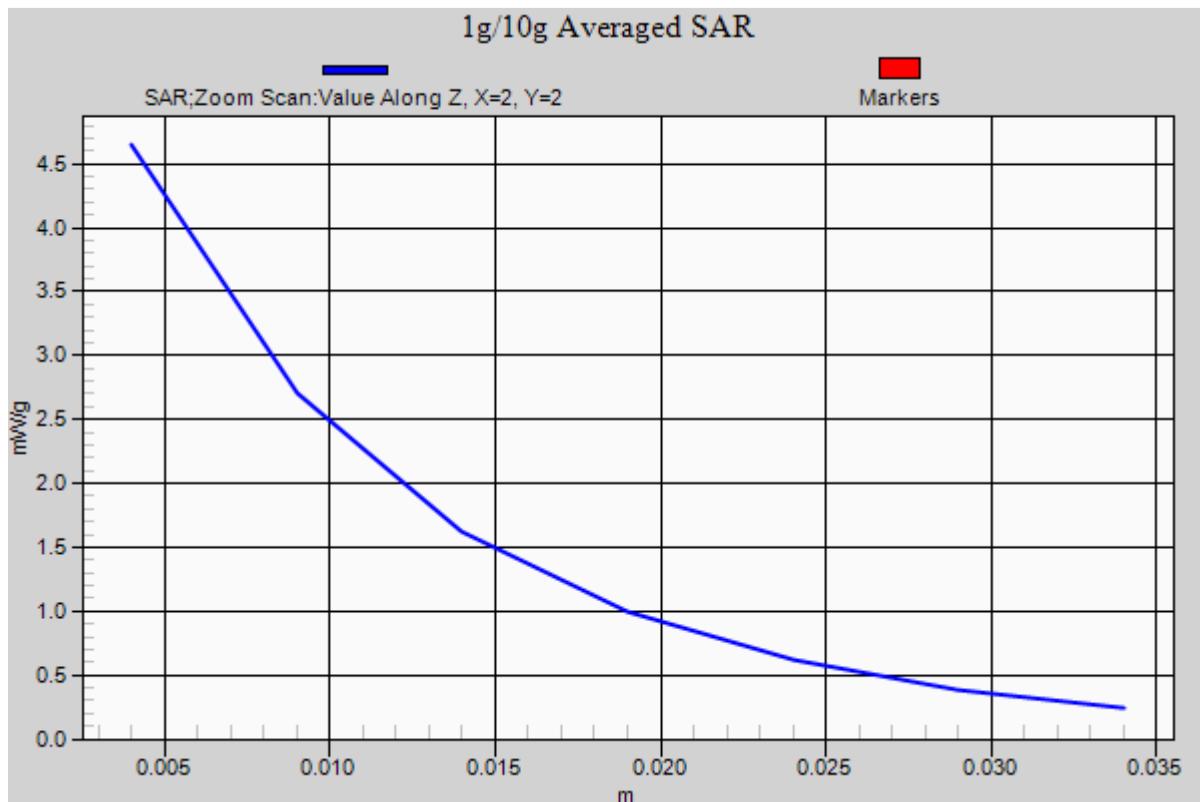

APPENDIX C: PROBE CALIBRATION



Accredited by the Swiss Accreditation Service (SAS)

Accreditation No.: SCS 108

The Swiss Accreditation Service is one of the signatories to the EA
Multilateral Agreement for the recognition of calibration certificates

Client PC Test

Certificate No: D835V2-4d047_Jan12

CALIBRATION CERTIFICATE

Object D835V2 - SN: 4d047

Calibration procedure(s)
QA CAL-05.v8
Calibration procedure for dipole validation kits above 700 MHz

Calibration date: January 25, 2012

✓ KOK
2/6/12

This calibration certificate documents the traceability to national standards, which realize the physical units of measurements (SI). The measurements and the uncertainties with confidence probability are given on the following pages and are part of the certificate.

All calibrations have been conducted in the closed laboratory facility: environment temperature (22 ± 3)°C and humidity < 70%.

Calibration Equipment used (M&TE critical for calibration)

| Primary Standards | ID # | Cal Date (Certificate No.) | Scheduled Calibration |
|-----------------------------|--------------------|-----------------------------------|------------------------|
| Power meter EPM-442A | GB37480704 | 05-Oct-11 (No. 217-01451) | Oct-12 |
| Power sensor HP 8481A | US37292783 | 05-Oct-11 (No. 217-01451) | Oct-12 |
| Reference 20 dB Attenuator | SN: 5086 (20g) | 29-Mar-11 (No. 217-01368) | Apr-12 |
| Type-N mismatch combination | SN: 5047.2 / 06327 | 29-Mar-11 (No. 217-01371) | Apr-12 |
| Reference Probe ES3DV3 | SN: 3205 | 30-Dec-11 (No. ES3-3205_Dec11) | Dec-12 |
| DAE4 | SN: 601 | 04-Jul-11 (No. DAE4-601_Jul11) | Jul-12 |
| Secondary Standards | ID # | Check Date (in house) | Scheduled Check |
| Power sensor HP 8481A | MY41092317 | 18-Oct-02 (in house check Oct-11) | In house check: Oct-13 |
| RF generator R&S SMT-06 | 100005 | 04-Aug-99 (in house check Oct-11) | In house check: Oct-13 |
| Network Analyzer HP 8753E | US37390585 S4206 | 18-Oct-01 (in house check Oct-11) | In house check: Oct-12 |

| Calibrated by: | Name | Function | Signature |
|----------------|----------------|-----------------------|-----------|
| | Israe El-Naouq | Laboratory Technician | |
| Approved by: | Katja Pokovic | Technical Manager | |

Issued: January 25, 2012

This calibration certificate shall not be reproduced except in full without written approval of the laboratory.



Accredited by the Swiss Accreditation Service (SAS)

Accreditation No.: SCS 108

The Swiss Accreditation Service is one of the signatories to the EA
Multilateral Agreement for the recognition of calibration certificates

Glossary:

| | |
|-------|---------------------------------|
| TSL | tissue simulating liquid |
| ConvF | sensitivity in TSL / NORM x,y,z |
| N/A | not applicable or not measured |

Calibration is Performed According to the Following Standards:

- a) IEEE Std 1528-2003, "IEEE Recommended Practice for Determining the Peak Spatial-Averaged Specific Absorption Rate (SAR) in the Human Head from Wireless Communications Devices: Measurement Techniques", December 2003
- b) IEC 62209-1, "Procedure to measure the Specific Absorption Rate (SAR) for hand-held devices used in close proximity to the ear (frequency range of 300 MHz to 3 GHz)", February 2005
- c) Federal Communications Commission Office of Engineering & Technology (FCC OET), "Evaluating Compliance with FCC Guidelines for Human Exposure to Radiofrequency Electromagnetic Fields; Additional Information for Evaluating Compliance of Mobile and Portable Devices with FCC Limits for Human Exposure to Radiofrequency Emissions", Supplement C (Edition 01-01) to Bulletin 65

Additional Documentation:

- d) DASY4/5 System Handbook

Methods Applied and Interpretation of Parameters:

- *Measurement Conditions:* Further details are available from the Validation Report at the end of the certificate. All figures stated in the certificate are valid at the frequency indicated.
- *Antenna Parameters with TSL:* The dipole is mounted with the spacer to position its feed point exactly below the center marking of the flat phantom section, with the arms oriented parallel to the body axis.
- *Feed Point Impedance and Return Loss:* These parameters are measured with the dipole positioned under the liquid filled phantom. The impedance stated is transformed from the measurement at the SMA connector to the feed point. The Return Loss ensures low reflected power. No uncertainty required.
- *Electrical Delay:* One-way delay between the SMA connector and the antenna feed point. No uncertainty required.
- *SAR measured:* SAR measured at the stated antenna input power.
- *SAR normalized:* SAR as measured, normalized to an input power of 1 W at the antenna connector.
- *SAR for nominal TSL parameters:* The measured TSL parameters are used to calculate the nominal SAR result.

Measurement Conditions

DASY system configuration, as far as not given on page 1.

| | | |
|------------------------------|------------------------|-------------|
| DASY Version | DASY5 | V52.8.0 |
| Extrapolation | Advanced Extrapolation | |
| Phantom | Modular Flat Phantom | |
| Distance Dipole Center - TSL | 15 mm | with Spacer |
| Zoom Scan Resolution | dx, dy, dz = 5 mm | |
| Frequency | 835 MHz \pm 1 MHz | |

Head TSL parameters

The following parameters and calculations were applied.

| | Temperature | Permittivity | Conductivity |
|---|---------------------|----------------|----------------------|
| Nominal Head TSL parameters | 22.0 °C | 41.5 | 0.90 mho/m |
| Measured Head TSL parameters | (22.0 \pm 0.2) °C | 41.8 \pm 6 % | 0.89 mho/m \pm 6 % |
| Head TSL temperature change during test | < 0.5 °C | ---- | ---- |

SAR result with Head TSL

| | | |
|---|--------------------|--------------------------------|
| SAR averaged over 1 cm ³ (1 g) of Head TSL | Condition | |
| SAR measured | 250 mW input power | 2.33 mW / g |
| SAR for nominal Head TSL parameters | normalized to 1W | 9.41 mW / g \pm 17.0 % (k=2) |

| | | |
|---|--------------------|--------------------------------|
| SAR averaged over 10 cm ³ (10 g) of Head TSL | Condition | |
| SAR measured | 250 mW input power | 1.53 mW / g |
| SAR for nominal Head TSL parameters | normalized to 1W | 6.17 mW / g \pm 16.5 % (k=2) |

Body TSL parameters

The following parameters and calculations were applied.

| | Temperature | Permittivity | Conductivity |
|---|---------------------|----------------|----------------------|
| Nominal Body TSL parameters | 22.0 °C | 55.2 | 0.97 mho/m |
| Measured Body TSL parameters | (22.0 \pm 0.2) °C | 53.3 \pm 6 % | 0.98 mho/m \pm 6 % |
| Body TSL temperature change during test | < 0.5 °C | ---- | ---- |

SAR result with Body TSL

| | | |
|---|--------------------|--------------------------------|
| SAR averaged over 1 cm ³ (1 g) of Body TSL | Condition | |
| SAR measured | 250 mW input power | 2.39 mW / g |
| SAR for nominal Body TSL parameters | normalized to 1W | 9.41 mW / g \pm 17.0 % (k=2) |

| | | |
|---|--------------------|--------------------------------|
| SAR averaged over 10 cm ³ (10 g) of Body TSL | Condition | |
| SAR measured | 250 mW input power | 1.57 mW / g |
| SAR for nominal Body TSL parameters | normalized to 1W | 6.21 mW / g \pm 16.5 % (k=2) |

Appendix

Antenna Parameters with Head TSL

| | |
|--------------------------------------|-------------------------------|
| Impedance, transformed to feed point | 51.7 Ω - 3.0 $j\Omega$ |
| Return Loss | - 29.4 dB |

Antenna Parameters with Body TSL

| | |
|--------------------------------------|-------------------------------|
| Impedance, transformed to feed point | 47.8 Ω - 5.0 $j\Omega$ |
| Return Loss | - 25.0 dB |

General Antenna Parameters and Design

| | |
|----------------------------------|----------|
| Electrical Delay (one direction) | 1.386 ns |
|----------------------------------|----------|

After long term use with 100W radiated power, only a slight warming of the dipole near the feedpoint can be measured.

The dipole is made of standard semirigid coaxial cable. The center conductor of the feeding line is directly connected to the second arm of the dipole. The antenna is therefore short-circuited for DC-signals. On some of the dipoles, small end caps are added to the dipole arms in order to improve matching when loaded according to the position as explained in the "Measurement Conditions" paragraph. The SAR data are not affected by this change. The overall dipole length is still according to the Standard.

No excessive force must be applied to the dipole arms, because they might bend or the soldered connections near the feedpoint may be damaged.

Additional EUT Data

| | |
|-----------------|-----------------|
| Manufactured by | SPEAG |
| Manufactured on | August 16, 2006 |

DASY5 Validation Report for Head TSL

Date: 25.01.2012

Test Laboratory: SPEAG, Zurich, Switzerland

DUT: Dipole 835 MHz; Type: D835V2; Serial: D835V2 - SN: 4d047

Communication System: CW; Frequency: 835 MHz

Medium parameters used: $f = 835$ MHz; $\sigma = 0.89$ mho/m; $\epsilon_r = 41.8$; $\rho = 1000$ kg/m³

Phantom section: Flat Section

Measurement Standard: DASY5 (IEEE/IEC/ANSI C63.19-2007)

DASY52 Configuration:

- Probe: ES3DV3 - SN3205; ConvF(6.07, 6.07, 6.07); Calibrated: 30.12.2011
- Sensor-Surface: 3mm (Mechanical Surface Detection)
- Electronics: DAE4 Sn601; Calibrated: 04.07.2011
- Phantom: Flat Phantom 4.9L; Type: QD000P49AA; Serial: 1001
- DASY52 52.8.0(692); SEMCAD X 14.6.4(4989)

Dipole Calibration for Head Tissue/Pin=250 mW, d=15mm/Zoom Scan (7x7x7)/Cube 0:


Measurement grid: dx=5mm, dy=5mm, dz=5mm

Reference Value = 56.752 V/m; Power Drift = 0.02 dB


Peak SAR (extrapolated) = 3.4130

SAR(1 g) = 2.33 mW/g; SAR(10 g) = 1.53 mW/g

Maximum value of SAR (measured) = 2.709 mW/g

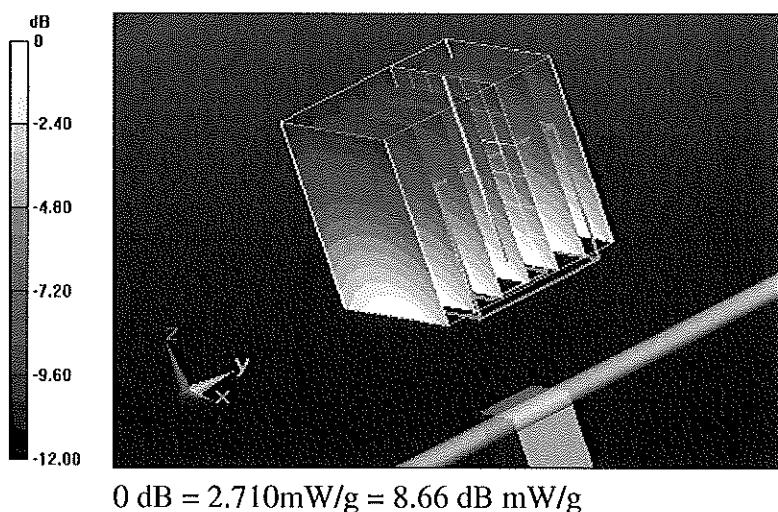

Impedance Measurement Plot for Head TSL

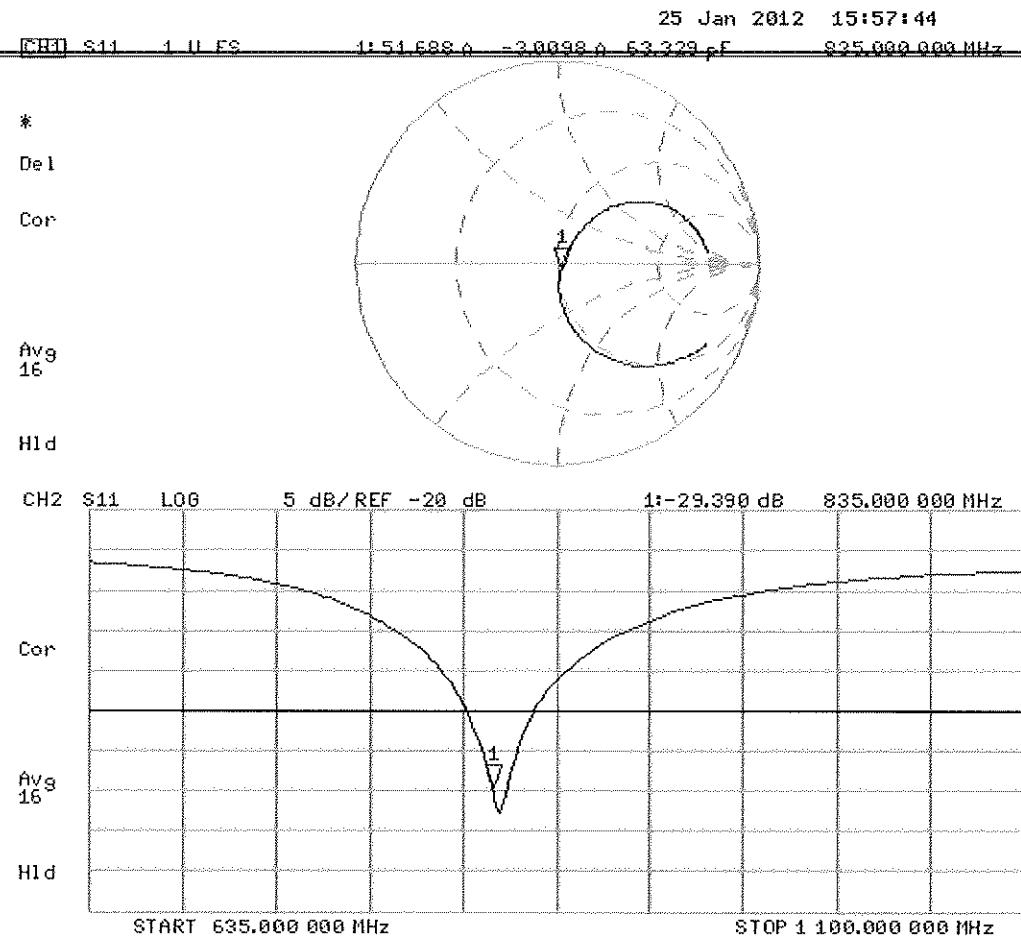

DASY5 Validation Report for Body TSL

Date: 25.01.2012

Test Laboratory: SPEAG, Zurich, Switzerland

DUT: Dipole 835 MHz; Type: D835V2; Serial: D835V2 - SN: 4d047

Communication System: CW; Frequency: 835 MHz

Medium parameters used: $f = 835$ MHz; $\sigma = 0.98$ mho/m; $\epsilon_r = 53.3$; $\rho = 1000$ kg/m³

Phantom section: Flat Section

Measurement Standard: DASY5 (IEEE/IEC/ANSI C63.19-2007)

DASY52 Configuration:

- Probe: ES3DV3 - SN3205; ConvF(6.02, 6.02, 6.02); Calibrated: 30.12.2011
- Sensor-Surface: 3mm (Mechanical Surface Detection)
- Electronics: DAE4 Sn601; Calibrated: 04.07.2011
- Phantom: Flat Phantom 4.9L; Type: QD000P49AA; Serial: 1001
- DASY52 52.8.0(692); SEMCAD X 14.6.4(4989)

Dipole Calibration for Body Tissue/Pin=250 mW, d=15mm/Zoom Scan (7x7x7)/Cube 0:


Measurement grid: $dx=5$ mm, $dy=5$ mm, $dz=5$ mm

Reference Value = 54.995 V/m; Power Drift = 0.02 dB


Peak SAR (extrapolated) = 3.4790

SAR(1 g) = 2.39 mW/g; SAR(10 g) = 1.57 mW/g

Maximum value of SAR (measured) = 2.767 mW/g

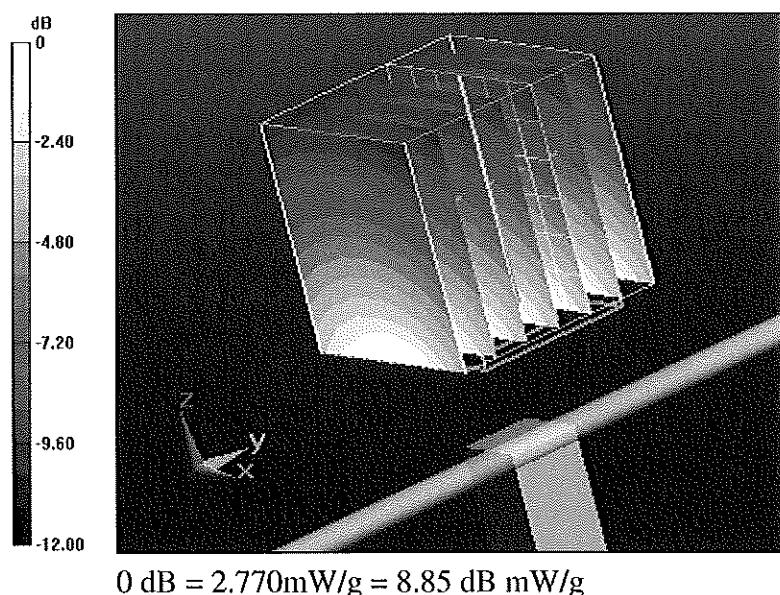

Impedance Measurement Plot for Body TSL

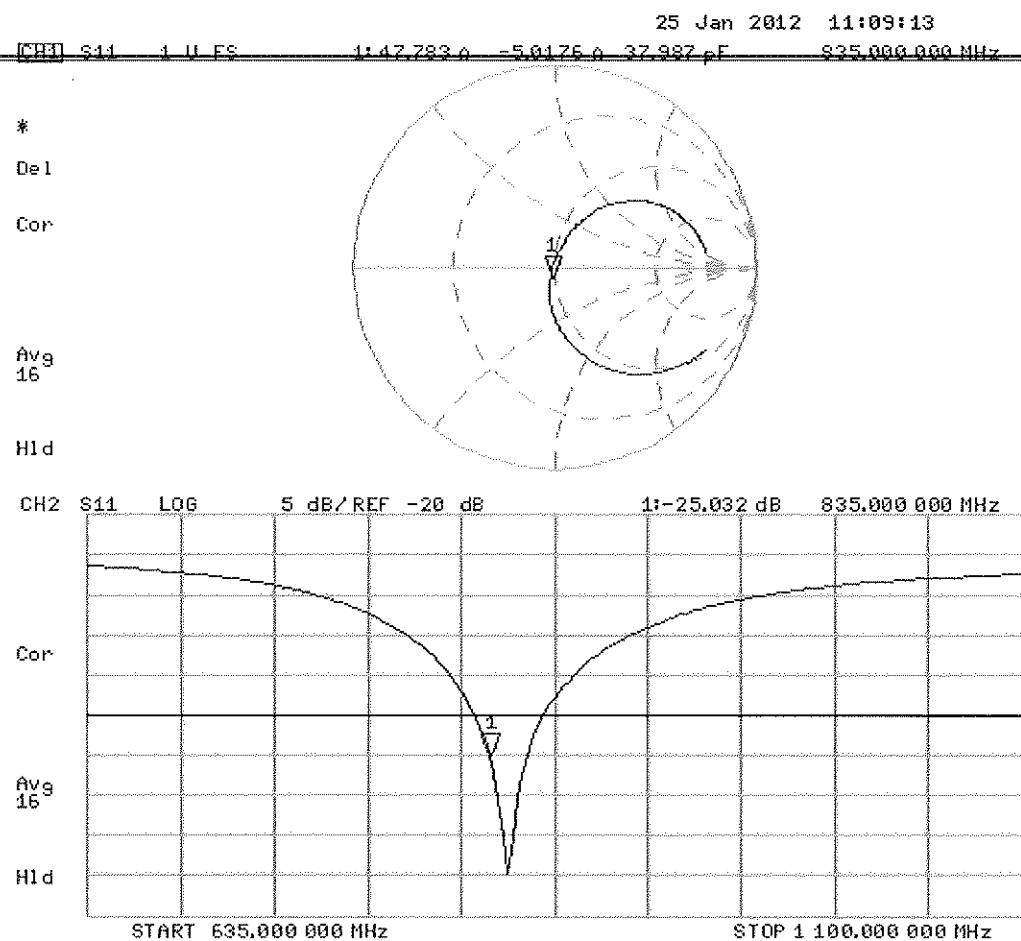



Accredited by the Swiss Accreditation Service (SAS)

Accreditation No.: **SCS 108**

The Swiss Accreditation Service is one of the signatories to the EA
 Multilateral Agreement for the recognition of calibration certificates

Client **PC Test**

Certificate No: **D1900V2-5d080_Jul11**

CALIBRATION CERTIFICATE

Object **D1900V2 - SN: 5d080**

Calibration procedure(s) **QA CAL-05.v8**
 Calibration procedure for dipole validation kits above 700 MHz

Calibration date: **July 22, 2011**

✓ KOK
 9/6/11

This calibration certificate documents the traceability to national standards, which realize the physical units of measurements (SI).
 The measurements and the uncertainties with confidence probability are given on the following pages and are part of the certificate.

All calibrations have been conducted in the closed laboratory facility: environment temperature $(22 \pm 3)^\circ\text{C}$ and humidity $< 70\%$.

Calibration Equipment used (M&TE critical for calibration)

| Primary Standards | ID # | Cal Date (Certificate No.) | Scheduled Calibration |
|-----------------------------|--------------------|-----------------------------------|------------------------|
| Power meter EPM-442A | GB37480704 | 06-Oct-10 (No. 217-01266) | Oct-11 |
| Power sensor HP 8481A | US37292783 | 06-Oct-10 (No. 217-01266) | Oct-11 |
| Reference 20 dB Attenuator | SN: S5086 (20b) | 29-Mar-11 (No. 217-01367) | Apr-12 |
| Type-N mismatch combination | SN: 5047.2 / 06327 | 29-Mar-11 (No. 217-01371) | Apr-12 |
| Reference Probe ES3DV3 | SN: 3205 | 29-Apr-11 (No. ES3-3205_Apr11) | Apr-12 |
| DAE4 | SN: 601 | 04-Jul-11 (No. DAE4-601_Jul11) | Jul-12 |
| Secondary Standards | ID # | Check Date (in house) | Scheduled Check |
| Power sensor HP 8481A | MY41092317 | 18-Oct-02 (in house check Oct-09) | In house check: Oct-11 |
| RF generator R&S SMT-06 | 100005 | 04-Aug-99 (in house check Oct-09) | In house check: Oct-11 |
| Network Analyzer HP 8753E | US37390585 S4206 | 18-Oct-01 (in house check Oct-10) | In house check: Oct-11 |

Calibrated by: **Dimce Iliev** **Laboratory Technician**

Approved by: **Katja Pokovic** **Technical Manager**

Issued: July 22, 2011

This calibration certificate shall not be reproduced except in full without written approval of the laboratory.



Accredited by the Swiss Accreditation Service (SAS)

Accreditation No.: SCS 108

The Swiss Accreditation Service is one of the signatories to the EA
Multilateral Agreement for the recognition of calibration certificates

Glossary:

| | |
|-------|---------------------------------|
| TSL | tissue simulating liquid |
| ConvF | sensitivity in TSL / NORM x,y,z |
| N/A | not applicable or not measured |

Calibration is Performed According to the Following Standards:

- a) IEEE Std 1528-2003, "IEEE Recommended Practice for Determining the Peak Spatial-Averaged Specific Absorption Rate (SAR) in the Human Head from Wireless Communications Devices: Measurement Techniques", December 2003
- b) IEC 62209-1, "Procedure to measure the Specific Absorption Rate (SAR) for hand-held devices used in close proximity to the ear (frequency range of 300 MHz to 3 GHz)", February 2005
- c) Federal Communications Commission Office of Engineering & Technology (FCC OET), "Evaluating Compliance with FCC Guidelines for Human Exposure to Radiofrequency Electromagnetic Fields; Additional Information for Evaluating Compliance of Mobile and Portable Devices with FCC Limits for Human Exposure to Radiofrequency Emissions", Supplement C (Edition 01-01) to Bulletin 65

Additional Documentation:

- d) DASY4/5 System Handbook

Methods Applied and Interpretation of Parameters:

- *Measurement Conditions:* Further details are available from the Validation Report at the end of the certificate. All figures stated in the certificate are valid at the frequency indicated.
- *Antenna Parameters with TSL:* The dipole is mounted with the spacer to position its feed point exactly below the center marking of the flat phantom section, with the arms oriented parallel to the body axis.
- *Feed Point Impedance and Return Loss:* These parameters are measured with the dipole positioned under the liquid filled phantom. The impedance stated is transformed from the measurement at the SMA connector to the feed point. The Return Loss ensures low reflected power. No uncertainty required.
- *Electrical Delay:* One-way delay between the SMA connector and the antenna feed point. No uncertainty required.
- *SAR measured:* SAR measured at the stated antenna input power.
- *SAR normalized:* SAR as measured, normalized to an input power of 1 W at the antenna connector.
- *SAR for nominal TSL parameters:* The measured TSL parameters are used to calculate the nominal SAR result.

Measurement Conditions

DASY system configuration, as far as not given on page 1.

| | | |
|------------------------------|--------------------------------------|-------------|
| DASY Version | DASY5 | V52.6.2 |
| Extrapolation | Advanced Extrapolation | |
| Phantom | Modular Flat Phantom | |
| Distance Dipole Center - TSL | 10 mm | with Spacer |
| Zoom Scan Resolution | $dx, dy, dz = 5 \text{ mm}$ | |
| Frequency | $1900 \text{ MHz} \pm 1 \text{ MHz}$ | |

Head TSL parameters

The following parameters and calculations were applied.

| | Temperature | Permittivity | Conductivity |
|---|-----------------------------|------------------------|--------------------------------------|
| Nominal Head TSL parameters | 22.0 °C | 40.0 | 1.40 mho/m |
| Measured Head TSL parameters | $(22.0 \pm 0.2) \text{ °C}$ | $39.1 \pm 6 \text{ %}$ | $1.42 \text{ mho/m} \pm 6 \text{ %}$ |
| Head TSL temperature change during test | $< 0.5 \text{ °C}$ | ---- | ---- |

SAR result with Head TSL

| | | |
|---|--------------------|--|
| SAR averaged over 1 cm ³ (1 g) of Head TSL | Condition | |
| SAR measured | 250 mW input power | 10.1 mW / g |
| SAR for nominal Head TSL parameters | normalized to 1W | $39.9 \text{ mW / g} \pm 17.0 \text{ % (k=2)}$ |

| | | |
|---|--------------------|--|
| SAR averaged over 10 cm ³ (10 g) of Head TSL | Condition | |
| SAR measured | 250 mW input power | 5.26 mW / g |
| SAR for nominal Head TSL parameters | normalized to 1W | $20.9 \text{ mW / g} \pm 16.5 \text{ % (k=2)}$ |

Body TSL parameters

The following parameters and calculations were applied.

| | Temperature | Permittivity | Conductivity |
|---|-----------------------------|------------------------|--------------------------------------|
| Nominal Body TSL parameters | 22.0 °C | 53.3 | 1.52 mho/m |
| Measured Body TSL parameters | $(22.0 \pm 0.2) \text{ °C}$ | $52.3 \pm 6 \text{ %}$ | $1.53 \text{ mho/m} \pm 6 \text{ %}$ |
| Body TSL temperature change during test | $< 0.5 \text{ °C}$ | ---- | ---- |

SAR result with Body TSL

| | | |
|---|--------------------|--|
| SAR averaged over 1 cm ³ (1 g) of Body TSL | Condition | |
| SAR measured | 250 mW input power | 10.3 mW / g |
| SAR for nominal Body TSL parameters | normalized to 1W | $40.9 \text{ mW / g} \pm 17.0 \text{ % (k=2)}$ |

| | | |
|---|--------------------|--|
| SAR averaged over 10 cm ³ (10 g) of Body TSL | Condition | |
| SAR measured | 250 mW input power | 5.38 mW / g |
| SAR for nominal Body TSL parameters | normalized to 1W | $21.4 \text{ mW / g} \pm 16.5 \text{ % (k=2)}$ |

Appendix

Antenna Parameters with Head TSL

| | |
|--------------------------------------|-----------------------------|
| Impedance, transformed to feed point | $52.5 \Omega + 8.0 j\Omega$ |
| Return Loss | -21.8 dB |

Antenna Parameters with Body TSL

| | |
|--------------------------------------|-----------------------------|
| Impedance, transformed to feed point | $46.7 \Omega + 7.1 j\Omega$ |
| Return Loss | -21.8 dB |

General Antenna Parameters and Design

| | |
|----------------------------------|----------|
| Electrical Delay (one direction) | 1.192 ns |
|----------------------------------|----------|

After long term use with 100W radiated power, only a slight warming of the dipole near the feedpoint can be measured.

The dipole is made of standard semirigid coaxial cable. The center conductor of the feeding line is directly connected to the second arm of the dipole. The antenna is therefore short-circuited for DC-signals.

No excessive force must be applied to the dipole arms, because they might bend or the soldered connections near the feedpoint may be damaged.

Additional EUT Data

| | |
|-----------------|---------------|
| Manufactured by | SPEAG |
| Manufactured on | June 28, 2006 |

DASY5 Validation Report for Head TSL

Date: 20.07.2011

Test Laboratory: SPEAG, Zurich, Switzerland

DUT: Dipole 1900 MHz; Type: D1900V2; Serial: D1900V2 - SN: 5d080

Communication System: CW; Frequency: 1900 MHz

Medium parameters used: $f = 1900$ MHz; $\sigma = 1.42$ mho/m; $\epsilon_r = 39.1$; $\rho = 1000$ kg/m³

Phantom section: Flat Section

Measurement Standard: DASY5 (IEEE/IEC/ANSI C63.19-2007)

DASY52 Configuration:

- Probe: ES3DV3 - SN3205; ConvF(5.01, 5.01, 5.01); Calibrated: 29.04.2011
- Sensor-Surface: 3mm (Mechanical Surface Detection)
- Electronics: DAE4 Sn601; Calibrated: 04.07.2011
- Phantom: Flat Phantom 5.0 (front); Type: QD000P50AA; Serial: 1001
- DASY52 52.6.2(482); SEMCAD X 14.4.5(3634)

Dipole Calibration for Head Tissue/Pin=250 mW, d=10mm/Zoom Scan (7x7x7)/Cube 0:


Measurement grid: dx=5mm, dy=5mm, dz=5mm

Reference Value = 98.443 V/m; Power Drift = 0.03 dB


Peak SAR (extrapolated) = 18.442 W/kg

SAR(1 g) = 10.1 mW/g; SAR(10 g) = 5.26 mW/g

Maximum value of SAR (measured) = 12.731 mW/g

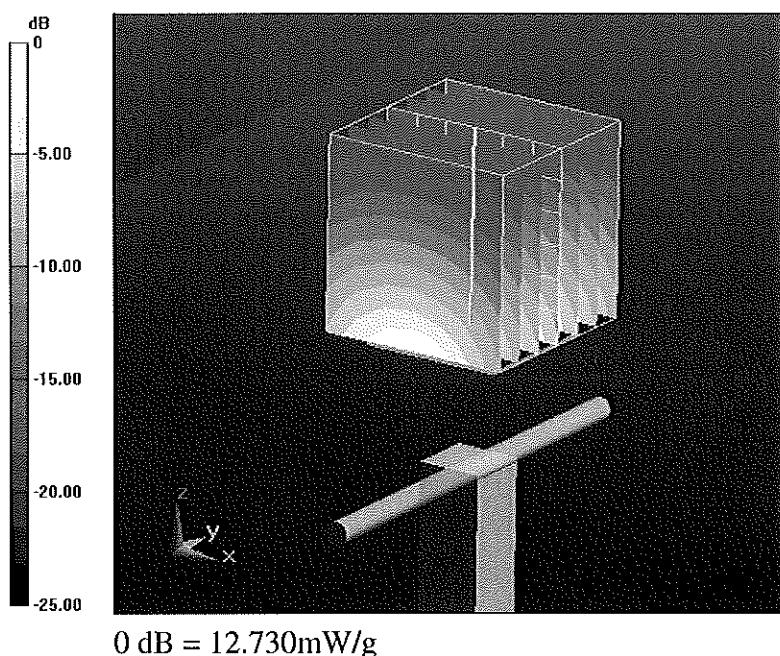

Impedance Measurement Plot for Head TSL

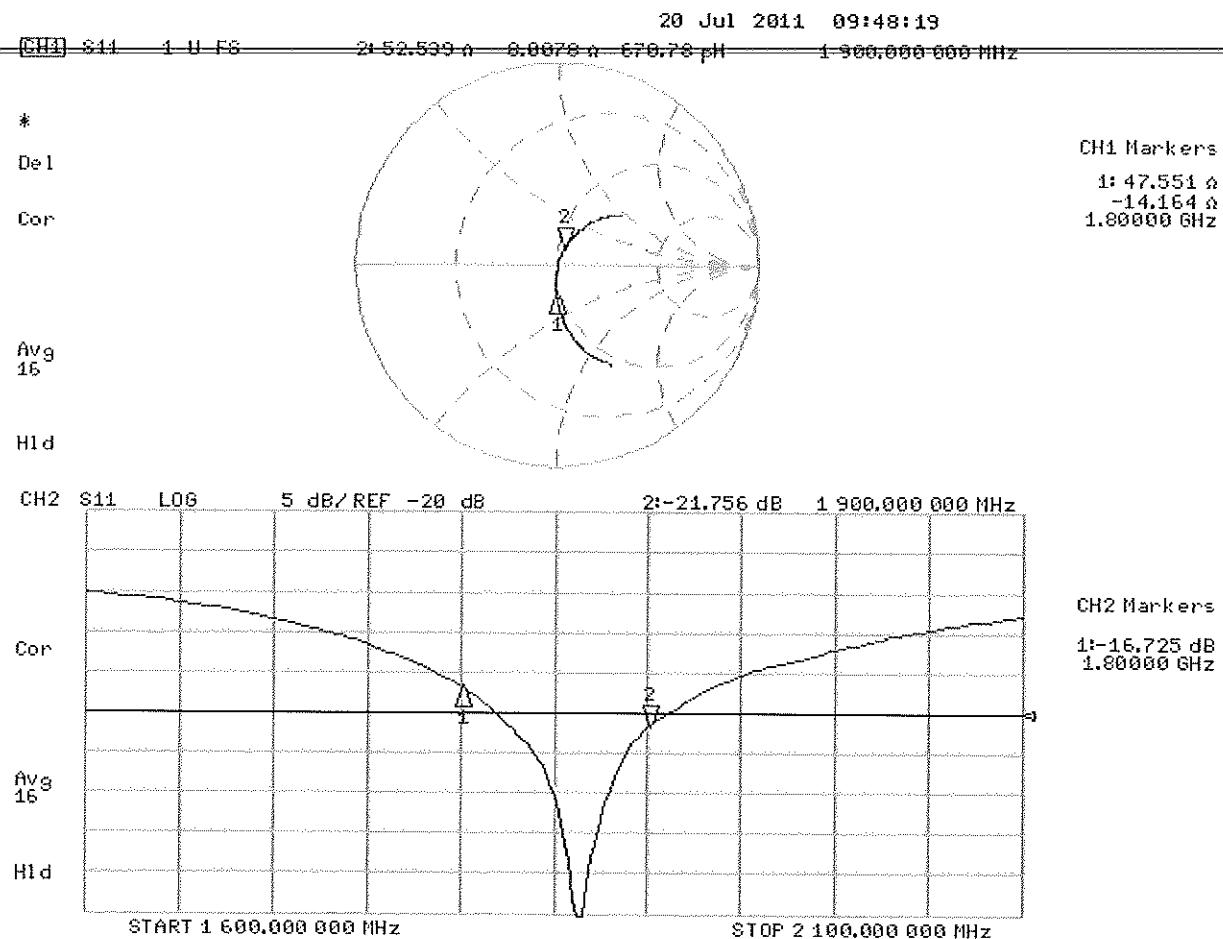

DASY5 Validation Report for Body TSL

Date: 22.07.2011

Test Laboratory: SPEAG, Zurich, Switzerland

~~DUT: Dipole 1900 MHz; Type: D1900V2; Serial: D1900V2 - SN: 5d080~~

Communication System: CW; Frequency: 1900 MHz

Medium parameters used: $f = 1900$ MHz; $\sigma = 1.53$ mho/m; $\epsilon_r = 52.3$; $\rho = 1000$ kg/m³

Phantom section: Flat Section

Measurement Standard: DASY5 (IEEE/IEC/ANSI C63.19-2007)

DASY52 Configuration:

- Probe: ES3DV3 - SN3205; ConvF(4.62, 4.62, 4.62); Calibrated: 29.04.2011
- Sensor-Surface: 3mm (Mechanical Surface Detection)
- Electronics: DAE4 Sn601; Calibrated: 04.07.2011
- Phantom: Flat Phantom 5.0 (back); Type: QD000P50AA; Serial: 1002
- DASY52 52.6.2(482); SEMCAD X 14.4.5(3634)

Dipole Calibration for Body Tissue/Pin=250 mW, d=10mm/Zoom Scan (7x7x7)/Cube 0:


Measurement grid: $dx=5$ mm, $dy=5$ mm, $dz=5$ mm

Reference Value = 96.049 V/m; Power Drift = 0.0018 dB


Peak SAR (extrapolated) = 18.160 W/kg

SAR(1 g) = 10.3 mW/g; SAR(10 g) = 5.38 mW/g

Maximum value of SAR (measured) = 13.017 mW/g

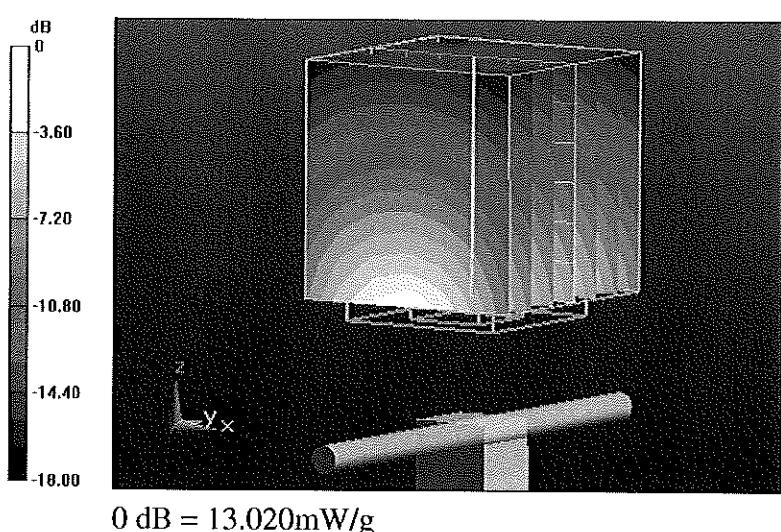

Impedance Measurement Plot for Body TSL

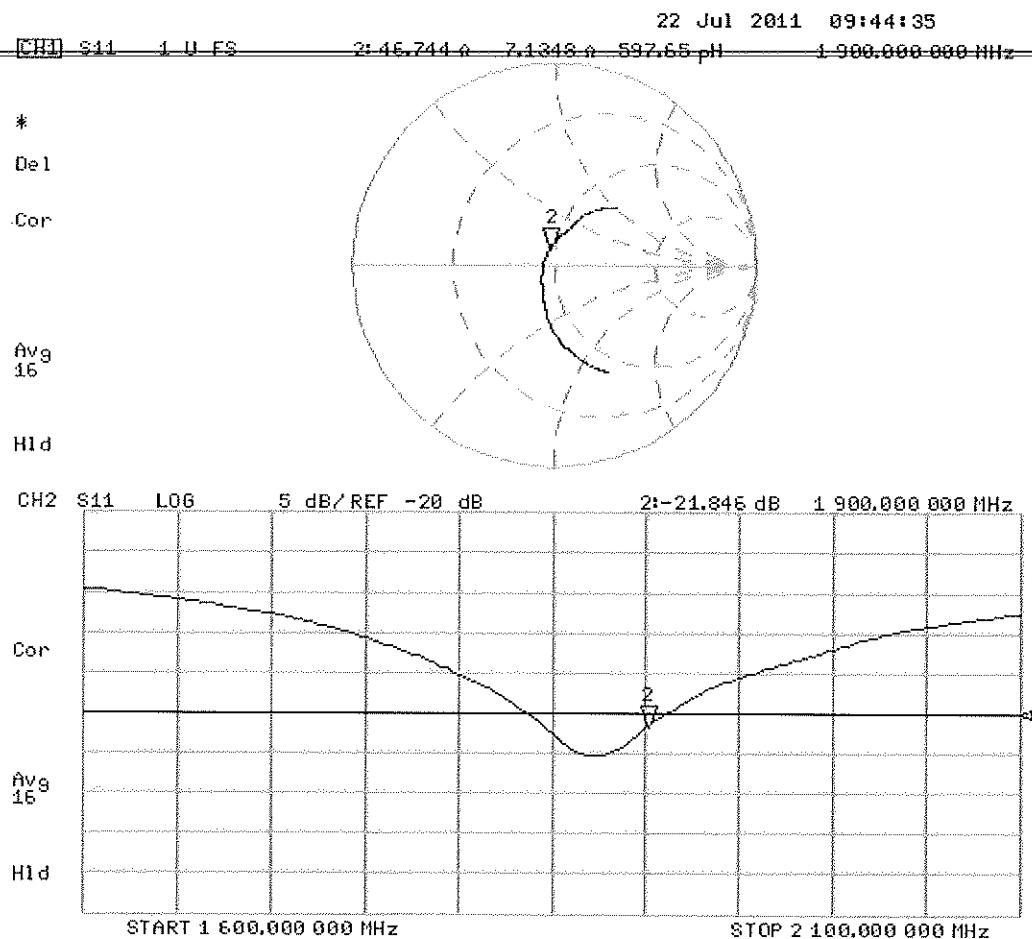



Accredited by the Swiss Accreditation Service (SAS)

The Swiss Accreditation Service is one of the signatories to the EA
 Multilateral Agreement for the recognition of calibration certificates

Accreditation No.: **SCS 108**

Client **PC Test**

Certificate No: **D1900V2-5d149_Feb12**

CALIBRATION CERTIFICATE

Object **D1900V2 - SN: 5d149**

Calibration procedure(s) **QA CAL-05.v8**
 Calibration procedure for dipole validation kits above 700 MHz

Calibration date: **February 22, 2012**

✓
 1/1/12

This calibration certificate documents the traceability to national standards, which realize the physical units of measurements (SI).
 The measurements and the uncertainties with confidence probability are given on the following pages and are part of the certificate.

All calibrations have been conducted in the closed laboratory facility: environment temperature (22 ± 3)°C and humidity < 70%.

Calibration Equipment used (M&TE critical for calibration)

| Primary Standards | ID # | Cal Date (Certificate No.) | Scheduled Calibration |
|-----------------------------|--------------------|-----------------------------------|------------------------|
| Power meter EPM-442A | GB37480704 | 05-Oct-11 (No. 217-01451) | Oct-12 |
| Power sensor HP 8481A | US37292783 | 05-Oct-11 (No. 217-01451) | Oct-12 |
| Reference 20 dB Attenuator | SN: 5086 (20g) | 29-Mar-11 (No. 217-01368) | Apr-12 |
| Type-N mismatch combination | SN: 5047.2 / 06327 | 29-Mar-11 (No. 217-01371) | Apr-12 |
| Reference Probe ES3DV3 | SN: 3205 | 30-Dec-11 (No. ES3-3205_Dec11) | Dec-12 |
| DAE4 | SN: 601 | 04-Jul-11 (No. DAE4-601_Jul11) | Jul-12 |
| Secondary Standards | ID # | Check Date (in house) | Scheduled Check |
| Power sensor HP 8481A | MY41092317 | 18-Oct-02 (in house check Oct-11) | In house check: Oct-13 |
| RF generator R&S SMT-06 | 100005 | 04-Aug-99 (in house check Oct-11) | In house check: Oct-13 |
| Network Analyzer HP 8753E | US37390585 S4206 | 18-Oct-01 (in house check Oct-11) | In house check: Oct-12 |

| | | | |
|----------------|-------------------------------|--|---------------|
| Calibrated by: | Name Israe El-Naouq | Function Laboratory Technician | Signature |
| Approved by: | Katja Pokovic | Technical Manager | |

Issued: February 23, 2012

This calibration certificate shall not be reproduced except in full without written approval of the laboratory.



Accredited by the Swiss Accreditation Service (SAS)
The Swiss Accreditation Service is one of the signatories to the EA
Multilateral Agreement for the recognition of calibration certificates

Accreditation No.: SCS 108

Glossary:

| | |
|-------|---------------------------------|
| TSL | tissue simulating liquid |
| ConvF | sensitivity in TSL / NORM x,y,z |
| N/A | not applicable or not measured |

Calibration is Performed According to the Following Standards:

- a) IEEE Std 1528-2003, "IEEE Recommended Practice for Determining the Peak Spatial-Averaged Specific Absorption Rate (SAR) in the Human Head from Wireless Communications Devices: Measurement Techniques", December 2003
- b) IEC 62209-1, "Procedure to measure the Specific Absorption Rate (SAR) for hand-held devices used in close proximity to the ear (frequency range of 300 MHz to 3 GHz)", February 2005
- c) Federal Communications Commission Office of Engineering & Technology (FCC OET), "Evaluating Compliance with FCC Guidelines for Human Exposure to Radiofrequency Electromagnetic Fields; Additional Information for Evaluating Compliance of Mobile and Portable Devices with FCC Limits for Human Exposure to Radiofrequency Emissions", Supplement C (Edition 01-01) to Bulletin 65

Additional Documentation:

- d) DASY4/5 System Handbook

Methods Applied and Interpretation of Parameters:

- *Measurement Conditions:* Further details are available from the Validation Report at the end of the certificate. All figures stated in the certificate are valid at the frequency indicated.
- *Antenna Parameters with TSL:* The dipole is mounted with the spacer to position its feed point exactly below the center marking of the flat phantom section, with the arms oriented parallel to the body axis.
- *Feed Point Impedance and Return Loss:* These parameters are measured with the dipole positioned under the liquid filled phantom. The impedance stated is transformed from the measurement at the SMA connector to the feed point. The Return Loss ensures low reflected power. No uncertainty required.
- *Electrical Delay:* One-way delay between the SMA connector and the antenna feed point. No uncertainty required.
- *SAR measured:* SAR measured at the stated antenna input power.
- *SAR normalized:* SAR as measured, normalized to an input power of 1 W at the antenna connector.
- *SAR for nominal TSL parameters:* The measured TSL parameters are used to calculate the nominal SAR result.

Measurement Conditions

DASY system configuration, as far as not given on page 1.

| | | |
|------------------------------|------------------------|-------------|
| DASY Version | DASY5 | V52.8.0 |
| Extrapolation | Advanced Extrapolation | |
| Phantom | Modular Flat Phantom | |
| Distance Dipole Center - TSL | 10 mm | with Spacer |
| Zoom Scan Resolution | dx, dy, dz = 5 mm | |
| Frequency | 1900 MHz \pm 1 MHz | |

Head TSL parameters

The following parameters and calculations were applied.

| | Temperature | Permittivity | Conductivity |
|---|---------------------|----------------|----------------------|
| Nominal Head TSL parameters | 22.0 °C | 40.0 | 1.40 mho/m |
| Measured Head TSL parameters | (22.0 \pm 0.2) °C | 40.4 \pm 6 % | 1.40 mho/m \pm 6 % |
| Head TSL temperature change during test | < 0.5 °C | ---- | ---- |

SAR result with Head TSL

| | | |
|---|--------------------|-------------------------------|
| SAR averaged over 1 cm ³ (1 g) of Head TSL | Condition | |
| SAR measured | 250 mW input power | 9.80 mW / g |
| SAR for nominal Head TSL parameters | normalized to 1W | 39.3 mW /g \pm 17.0 % (k=2) |

| | | |
|---|--------------------|-------------------------------|
| SAR averaged over 10 cm ³ (10 g) of Head TSL | condition | |
| SAR measured | 250 mW input power | 5.18 mW / g |
| SAR for nominal Head TSL parameters | normalized to 1W | 20.7 mW /g \pm 16.5 % (k=2) |

Body TSL parameters

The following parameters and calculations were applied.

| | Temperature | Permittivity | Conductivity |
|---|---------------------|----------------|----------------------|
| Nominal Body TSL parameters | 22.0 °C | 53.3 | 1.52 mho/m |
| Measured Body TSL parameters | (22.0 \pm 0.2) °C | 53.0 \pm 6 % | 1.56 mho/m \pm 6 % |
| Body TSL temperature change during test | < 0.5 °C | ---- | ---- |

SAR result with Body TSL

| | | |
|---|--------------------|--------------------------------|
| SAR averaged over 1 cm ³ (1 g) of Body TSL | Condition | |
| SAR measured | 250 mW input power | 9.99 mW / g |
| SAR for nominal Body TSL parameters | normalized to 1W | 39.3 mW / g \pm 17.0 % (k=2) |

| | | |
|---|--------------------|--------------------------------|
| SAR averaged over 10 cm ³ (10 g) of Body TSL | condition | |
| SAR measured | 250 mW input power | 5.23 mW / g |
| SAR for nominal Body TSL parameters | normalized to 1W | 20.7 mW / g \pm 16.5 % (k=2) |

Appendix

Antenna Parameters with Head TSL

| | |
|--------------------------------------|-----------------------------|
| Impedance, transformed to feed point | $52.4 \Omega + 5.5 j\Omega$ |
| Return Loss | - 24.6 dB |

Antenna Parameters with Body TSL

| | |
|--------------------------------------|-----------------------------|
| Impedance, transformed to feed point | $48.0 \Omega + 6.7 j\Omega$ |
| Return Loss | - 23.0 dB |

General Antenna Parameters and Design

| | |
|----------------------------------|----------|
| Electrical Delay (one direction) | 1.199 ns |
|----------------------------------|----------|

After long term use with 100W radiated power, only a slight warming of the dipole near the feedpoint can be measured.

The dipole is made of standard semirigid coaxial cable. The center conductor of the feeding line is directly connected to the second arm of the dipole. The antenna is therefore short-circuited for DC-signals. On some of the dipoles, small end caps are added to the dipole arms in order to improve matching when loaded according to the position as explained in the "Measurement Conditions" paragraph. The SAR data are not affected by this change. The overall dipole length is still according to the Standard.

No excessive force must be applied to the dipole arms, because they might bend or the soldered connections near the feedpoint may be damaged.

Additional EUT Data

| | |
|-----------------|----------------|
| Manufactured by | SPEAG |
| Manufactured on | March 11, 2011 |

DASY5 Validation Report for Head TSL

Date: 22.02.2012

Test Laboratory: SPEAG, Zurich, Switzerland

DUT: Dipole 1900 MHz; Type: D1900V2; Serial: D1900V2 - SN: 5d149

Communication System: CW; Frequency: 1900 MHz

Medium parameters used: $f = 1900$ MHz; $\sigma = 1.4$ mho/m; $\epsilon_r = 40.4$; $\rho = 1000$ kg/m³

Phantom section: Flat Section

Measurement Standard: DASY5 (IEEE/IEC/ANSI C63.19-2007)

DASY52 Configuration:

- Probe: ES3DV3 - SN3205; ConvF(5.01, 5.01, 5.01); Calibrated: 30.12.2011
- Sensor-Surface: 3mm (Mechanical Surface Detection)
- Electronics: DAE4 Sn601; Calibrated: 04.07.2011
- Phantom: Flat Phantom 5.0 (front); Type: QD000P50AA; Serial: 1001
- DASY52 52.8.0(692); SEMCAD X 14.6.4(4989)

Dipole Calibration for Head Tissue/Pin=250 mW, d=10mm/Zoom Scan (7x7x7)/Cube 0:


Measurement grid: dx=5mm, dy=5mm, dz=5mm

Reference Value = 96.685 V/m; Power Drift = 0.04 dB


Peak SAR (extrapolated) = 17.4710

SAR(1 g) = 9.8 mW/g; SAR(10 g) = 5.18 mW/g

Maximum value of SAR (measured) = 12.114 mW/g

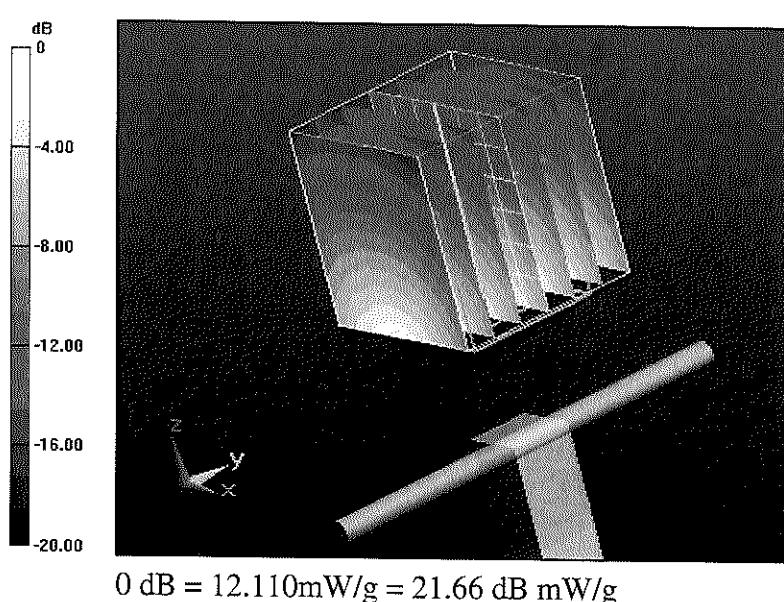

Impedance Measurement Plot for Head TSL

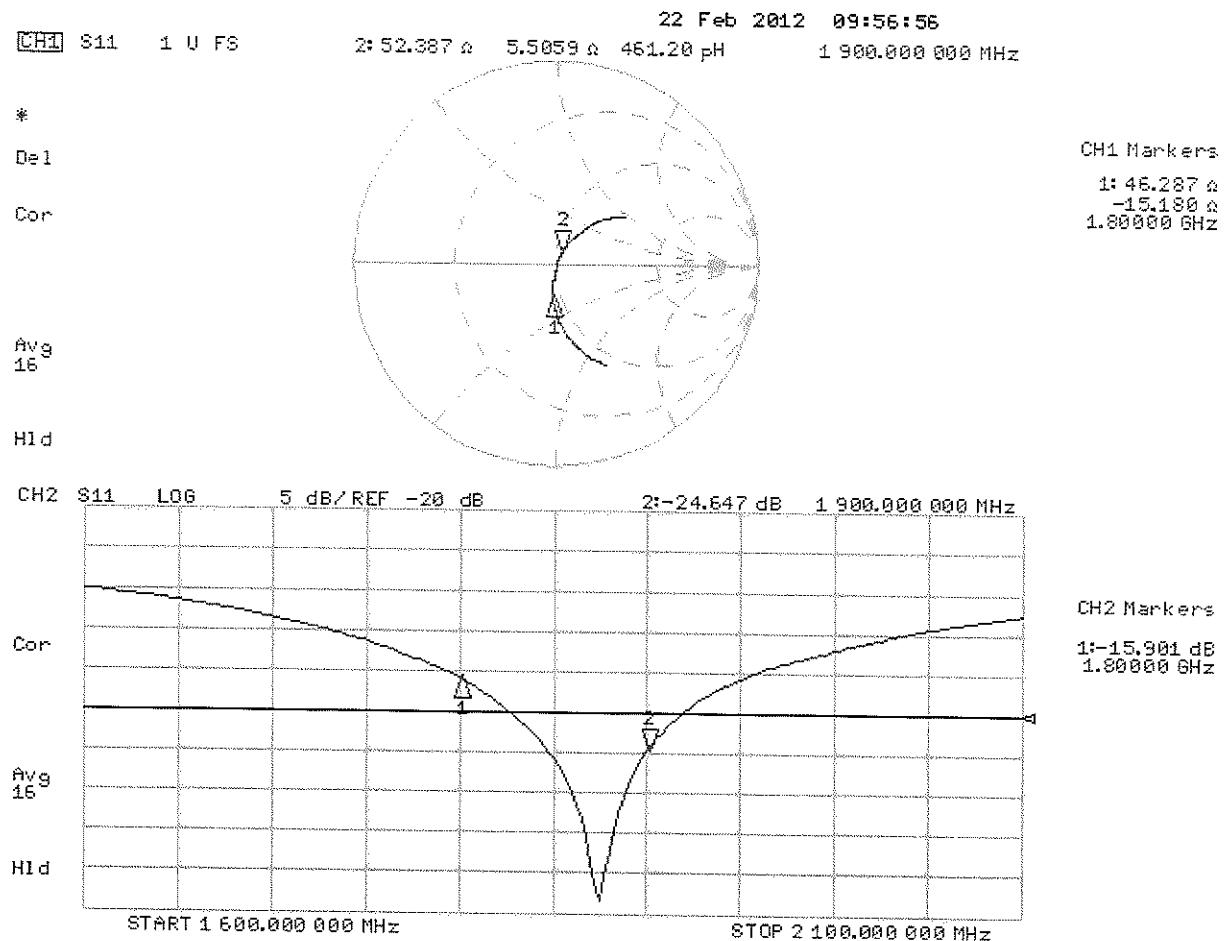

DASY5 Validation Report for Body TSL

Date: 06.02.2012

Test Laboratory: SPEAG, Zurich, Switzerland

DUT: Dipole 1900 MHz; Type: D1900V2; Serial: D1900V2 - SN: 5d149

Communication System: CW; Frequency: 1900 MHz

Medium parameters used: $f = 1900$ MHz; $\sigma = 1.56$ mho/m; $\epsilon_r = 53$; $\rho = 1000$ kg/m³

Phantom section: Flat Section

Measurement Standard: DASY5 (IEEE/IEC/ANSI C63.19-2007)

DASY52 Configuration:

- Probe: ES3DV3 - SN3205; ConvF(4.62, 4.62, 4.62); Calibrated: 30.12.2011
- Sensor-Surface: 3mm (Mechanical Surface Detection)
- Electronics: DAE4 Sn601; Calibrated: 04.07.2011
- Phantom: Flat Phantom 5.0 (back); Type: QD000P50AA; Serial: 1002
- DASY52 52.8.0(692); SEMCAD X 14.6.4(4989)

Dipole Calibration for Body Tissue/Pin=250 mW, d=10mm/Zoom Scan (7x7x7)/Cube 0:


Measurement grid: dx=5mm, dy=5mm, dz=5mm

Reference Value = 94.047 V/m; Power Drift = 0.0017 dB


Peak SAR (extrapolated) = 18.1310

SAR(1 g) = 9.99 mW/g; SAR(10 g) = 5.23 mW/g

Maximum value of SAR (measured) = 12.672 mW/g

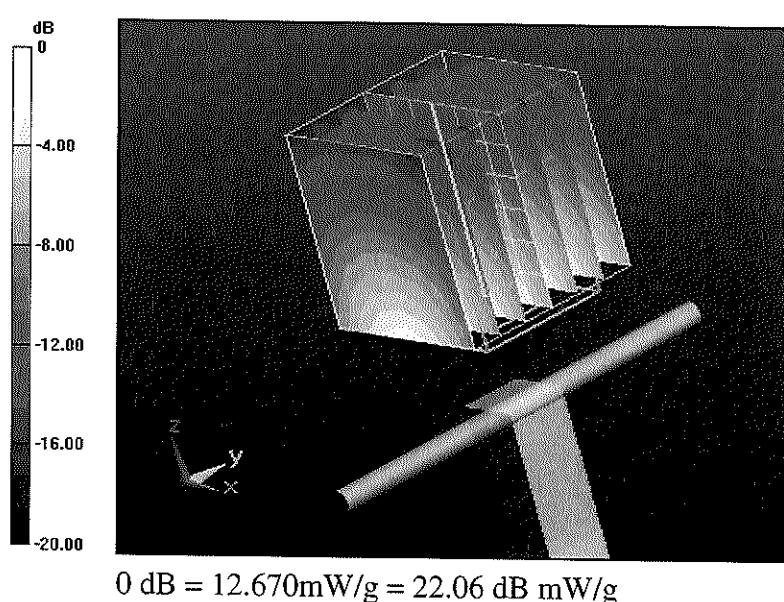

Impedance Measurement Plot for Body TSL

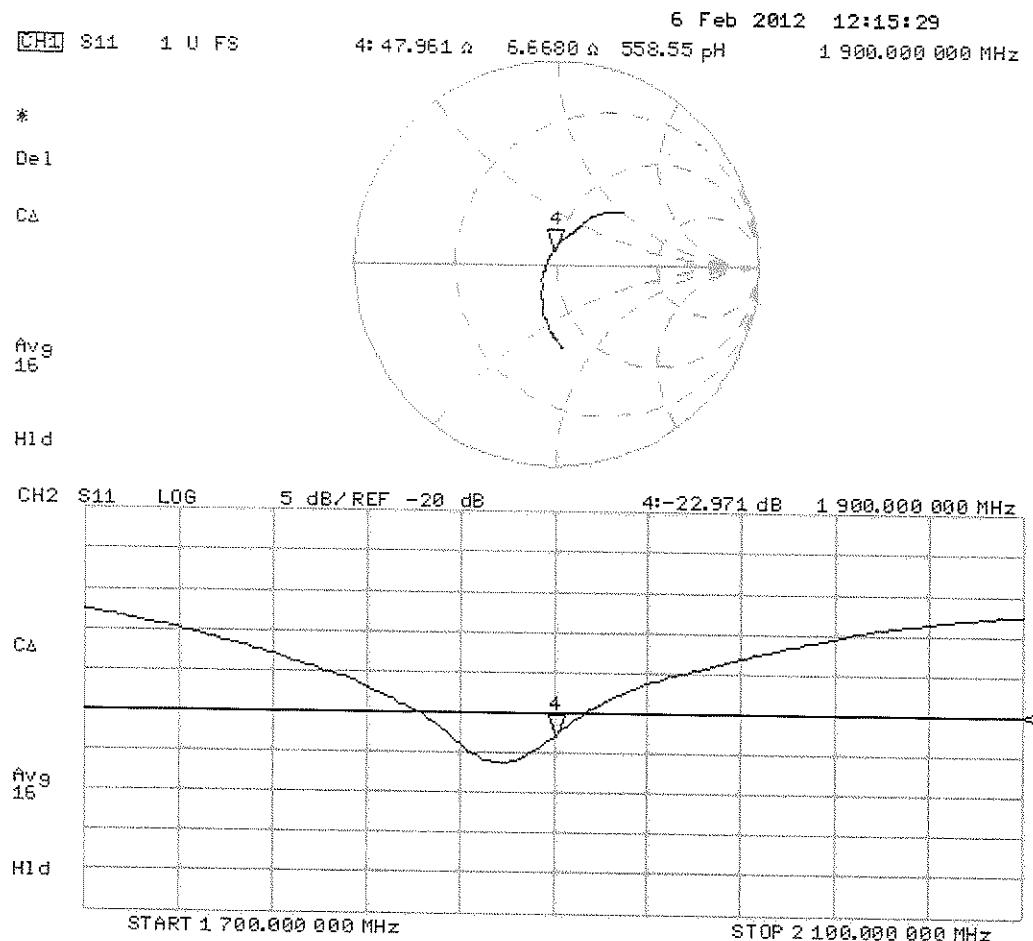



Accredited by the Swiss Accreditation Service (SAS)

Accreditation No.: SCS 108

The Swiss Accreditation Service is one of the signatories to the EA
Multilateral Agreement for the recognition of calibration certificates

Client

PC Test

Certificate No: ES3-3022_Aug11

CALIBRATION CERTIFICATE

Object ES3DV2 - SN:3022

Calibration procedure(s) QA CAL-01.v8, QA CAL-12.v7, QA CAL-23.v4, QA CAL-25.v4
Calibration procedure for dosimetric E-field probes

Calibration date: August 25, 2011

J/KOK
9/6/11

This calibration certificate documents the traceability to national standards, which realize the physical units of measurements (SI).
The measurements and the uncertainties with confidence probability are given on the following pages and are part of the certificate.

All calibrations have been conducted in the closed laboratory facility: environment temperature (22 ± 3)°C and humidity < 70%.

Calibration Equipment used (M&TE critical for calibration)

| Primary Standards | ID | Cal Date (Certificate No.) | Scheduled Calibration |
|----------------------------|-----------------|-----------------------------------|------------------------|
| Power meter E4419B | GB41293874 | 31-Mar-11 (No. 217-01372) | Apr-12 |
| Power sensor E4412A | MY41498087 | 31-Mar-11 (No. 217-01372) | Apr-12 |
| Reference 3 dB Attenuator | SN: S5054 (3c) | 29-Mar-11 (No. 217-01369) | Apr-12 |
| Reference 20 dB Attenuator | SN: S5086 (20b) | 29-Mar-11 (No. 217-01367) | Apr-12 |
| Reference 30 dB Attenuator | SN: S5129 (30b) | 29-Mar-11 (No. 217-01370) | Apr-12 |
| Reference Probe ES3DV2 | SN: 3013 | 29-Dec-10 (No. ES3-3013_Dec10) | Dec-11 |
| DAE4 | SN: 654 | 3-May-11 (No. DAE4-654_May11) | May-12 |
| Secondary Standards | ID | Check Date (in house) | Scheduled Check |
| RF generator HP 8648C | US3642U01700 | 4-Aug-99 (in house check Oct-09) | In house check: Oct-11 |
| Network Analyzer HP 8753E | US37390585 | 18-Oct-01 (in house check Oct-10) | In house check: Oct-11 |

| | | | |
|----------------|-------------------------|-----------------------------------|-----------|
| Calibrated by: | Name Claudio Leubler | Function Laboratory Technician | Signature |
| Approved by: | Katja Pokovic | Technical Manager | |

Issued: August 27, 2011

This calibration certificate shall not be reproduced except in full without written approval of the laboratory.



Accredited by the Swiss Accreditation Service (SAS)

Accreditation No.: SCS 108

The Swiss Accreditation Service is one of the signatories to the EA
 Multilateral Agreement for the recognition of calibration certificates

Glossary:

| | |
|------------------------|--|
| TSL | tissue simulating liquid |
| NORM x,y,z | sensitivity in free space |
| ConvF | sensitivity in TSL / NORM x,y,z |
| DCP | diode compression point |
| CF | crest factor (1/duty_cycle) of the RF signal |
| A, B, C | modulation dependent linearization parameters |
| Polarization φ | φ rotation around probe axis |
| Polarization θ | θ rotation around an axis that is in the plane normal to probe axis (at measurement center), i.e., $\theta = 0$ is normal to probe axis |

Calibration is Performed According to the Following Standards:

- IEEE Std 1528-2003, "IEEE Recommended Practice for Determining the Peak Spatial-Averaged Specific Absorption Rate (SAR) in the Human Head from Wireless Communications Devices: Measurement Techniques", December 2003
- IEC 62209-1, "Procedure to measure the Specific Absorption Rate (SAR) for hand-held devices used in close proximity to the ear (frequency range of 300 MHz to 3 GHz)", February 2005

Methods Applied and Interpretation of Parameters:

- $NORM_{x,y,z}$: Assessed for E-field polarization $\theta = 0$ ($f \leq 900$ MHz in TEM-cell; $f > 1800$ MHz: R22 waveguide). $NORM_{x,y,z}$ are only intermediate values, i.e., the uncertainties of $NORM_{x,y,z}$ does not affect the E^2 -field uncertainty inside TSL (see below ConvF).
- $NORM(f)x,y,z = NORM_{x,y,z} * frequency_response$ (see Frequency Response Chart). This linearization is implemented in DASY4 software versions later than 4.2. The uncertainty of the frequency response is included in the stated uncertainty of ConvF.
- $DCPx,y,z$: DCP are numerical linearization parameters assessed based on the data of power sweep with CW signal (no uncertainty required). DCP does not depend on frequency nor media.
- PAR : PAR is the Peak to Average Ratio that is not calibrated but determined based on the signal characteristics
- $Ax,y,z; Bx,y,z; Cx,y,z; VRx,y,z$: A, B, C are numerical linearization parameters assessed based on the data of power sweep for specific modulation signal. The parameters do not depend on frequency nor media. VR is the maximum calibration range expressed in RMS voltage across the diode.
- ConvF and Boundary Effect Parameters*: Assessed in flat phantom using E-field (or Temperature Transfer Standard for $f \leq 800$ MHz) and inside waveguide using analytical field distributions based on power measurements for $f > 800$ MHz. The same setups are used for assessment of the parameters applied for boundary compensation (alpha, depth) of which typical uncertainty values are given. These parameters are used in DASY4 software to improve probe accuracy close to the boundary. The sensitivity in TSL corresponds to $NORM_{x,y,z} * ConvF$ whereby the uncertainty corresponds to that given for ConvF. A frequency dependent ConvF is used in DASY version 4.4 and higher which allows extending the validity from ± 50 MHz to ± 100 MHz.
- Spherical Isotropy (3D deviation from isotropy)*: in a field of low gradients realized using a flat phantom exposed by a patch antenna.
- Sensor Offset*: The sensor offset corresponds to the offset of virtual measurement center from the probe tip (on probe axis). No tolerance required.

Probe ES3DV2

SN:3022

Manufactured: April 15, 2003
Calibrated: August 25, 2011

Calibrated for DASY/EASY Systems
(Note: non-compatible with DASY2 system!)

DASY/EASY - Parameters of Probe: ES3DV2 - SN:3022

Basic Calibration Parameters

| | Sensor X | Sensor Y | Sensor Z | Unc (k=2) |
|---|----------|----------|----------|---------------|
| Norm ($\mu\text{V}/(\text{V}/\text{m})^2$) ^A | 1.00 | 1.04 | 0.99 | $\pm 10.1 \%$ |
| DCP (mV) ^B | 99.5 | 97.7 | 99.2 | |

Modulation Calibration Parameters

| UID | Communication System Name | PAR | | A dB | B dB | C dB | VR mV | Unc ^E (k=2) |
|-------|---------------------------|------|---|---------|---------|---------|----------|---------------------------|
| 10000 | CW | 0.00 | X | 0.00 | 0.00 | 1.00 | 133.2 | $\pm 2.7 \%$ |
| | | | Y | 0.00 | 0.00 | 1.00 | 130.0 | |
| | | | Z | 0.00 | 0.00 | 1.00 | 133.9 | |

The reported uncertainty of measurement is stated as the standard uncertainty of measurement multiplied by the coverage factor k=2, which for a normal distribution corresponds to a coverage probability of approximately 95%.

^A The uncertainties of NormX,Y,Z do not affect the E²-field uncertainty inside TSL (see Pages 5 and 6).

^B Numerical linearization parameter: uncertainty not required.

^E Uncertainty is determined using the max. deviation from linear response applying rectangular distribution and is expressed for the square of the field value.

DASY/EASY - Parameters of Probe: ES3DV2 - SN:3022

Calibration Parameter Determined in Head Tissue Simulating Media

| f (MHz) ^c | Relative Permittivity ^f | Conductivity (S/m) ^f | ConvF X | ConvF Y | ConvF Z | Alpha | Depth (mm) | Unct. (k=2) |
|----------------------|------------------------------------|---------------------------------|---------|---------|---------|-------|------------|-------------|
| 750 | 41.9 | 0.89 | 6.27 | 6.27 | 6.27 | 0.80 | 1.13 | ± 12.0 % |
| 835 | 41.5 | 0.90 | 6.05 | 6.05 | 6.05 | 0.80 | 1.14 | ± 12.0 % |
| 1750 | 40.1 | 1.37 | 5.20 | 5.20 | 5.20 | 0.59 | 1.39 | ± 12.0 % |
| 1900 | 40.0 | 1.40 | 4.98 | 4.98 | 4.98 | 0.66 | 1.30 | ± 12.0 % |
| 2450 | 39.2 | 1.80 | 4.30 | 4.30 | 4.30 | 0.58 | 1.41 | ± 12.0 % |
| 2600 | 39.0 | 1.96 | 4.20 | 4.20 | 4.20 | 0.58 | 1.43 | ± 12.0 % |

^c Frequency validity of ± 100 MHz only applies for DASY v4.4 and higher (see Page 2), else it is restricted to ± 50 MHz. The uncertainty is the RSS of the ConvF uncertainty at calibration frequency and the uncertainty for the indicated frequency band.

^f At frequencies below 3 GHz, the validity of tissue parameters (ϵ and σ) can be relaxed to ± 10% if liquid compensation formula is applied to measured SAR values. At frequencies above 3 GHz, the validity of tissue parameters (ϵ and σ) is restricted to ± 5%. The uncertainty is the RSS of the ConvF uncertainty for indicated target tissue parameters.

DASY/EASY - Parameters of Probe: ES3DV2- SN:3022

Calibration Parameter Determined in Body Tissue Simulating Media


| f (MHz) ^c | Relative Permittivity ^f | Conductivity (S/m) ^f | ConvF X | ConvF Y | ConvF Z | Alpha | Depth (mm) | Unct. (k=2) |
|----------------------|------------------------------------|---------------------------------|---------|---------|---------|-------|------------|-------------|
| 450 | 56.7 | 0.94 | 6.93 | 6.93 | 6.93 | 0.07 | 1.00 | ± 13.4 % |
| 750 | 55.5 | 0.96 | 6.11 | 6.11 | 6.11 | 0.80 | 1.18 | ± 12.0 % |
| 835 | 55.2 | 0.97 | 6.06 | 6.06 | 6.06 | 0.80 | 1.20 | ± 12.0 % |
| 1640 | 53.8 | 1.40 | 5.07 | 5.07 | 5.07 | 0.70 | 1.32 | ± 12.0 % |
| 1750 | 53.4 | 1.49 | 4.64 | 4.64 | 4.64 | 0.67 | 1.35 | ± 12.0 % |
| 1900 | 53.3 | 1.52 | 4.41 | 4.41 | 4.41 | 0.54 | 1.56 | ± 12.0 % |
| 2450 | 52.7 | 1.95 | 4.01 | 4.01 | 4.01 | 0.66 | 1.19 | ± 12.0 % |
| 2600 | 52.5 | 2.16 | 3.90 | 3.90 | 3.90 | 0.54 | 1.45 | ± 12.0 % |

^c Frequency validity of ± 100 MHz only applies for DASY v4.4 and higher (see Page 2), else it is restricted to ± 50 MHz. The uncertainty is the RSS of the ConvF uncertainty at calibration frequency and the uncertainty for the indicated frequency band.

^f At frequencies below 3 GHz, the validity of tissue parameters (ϵ and σ) can be relaxed to ± 10% if liquid compensation formula is applied to measured SAR values. At frequencies above 3 GHz, the validity of tissue parameters (ϵ and σ) is restricted to ± 5%. The uncertainty is the RSS of the ConvF uncertainty for indicated target tissue parameters.

Frequency Response of E-Field

(TEM-Cell:ifi110 EXX, Waveguide: R22)


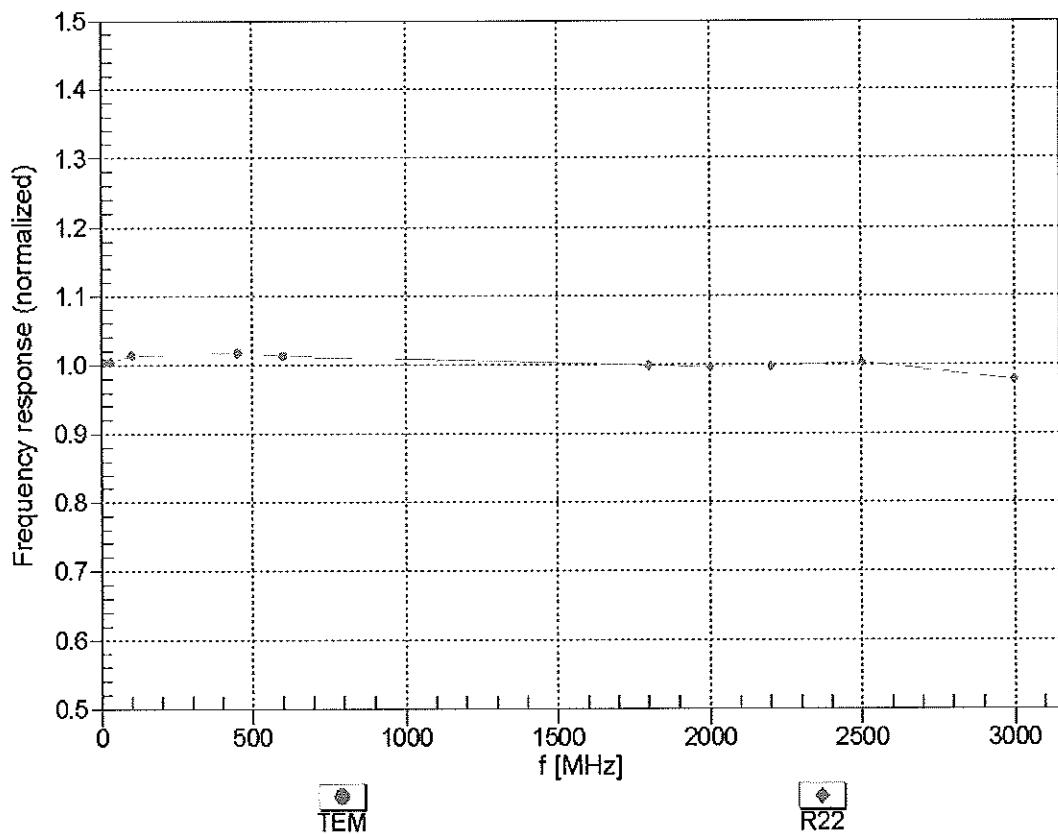


Uncertainty of Frequency Response of E-field: $\pm 6.3\%$ (k=2)

Receiving Pattern (ϕ), $\vartheta = 0^\circ$

f=600 MHz, TEM



f=1800 MHz, R22

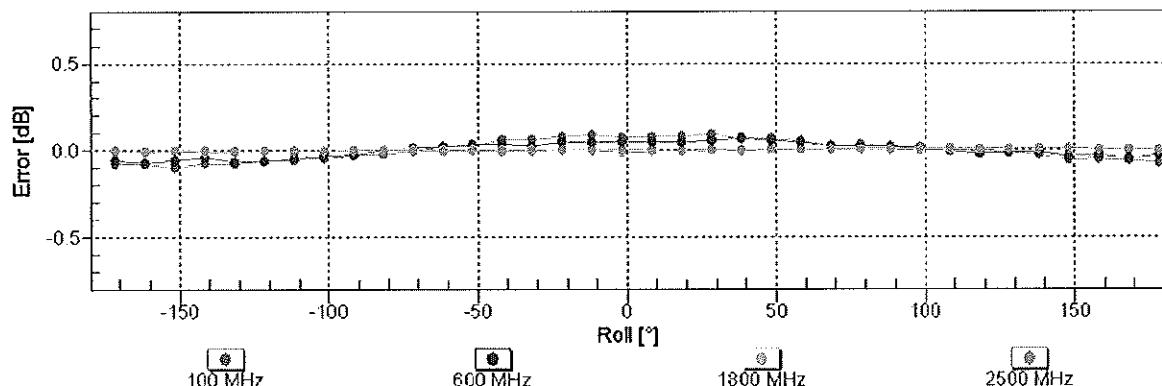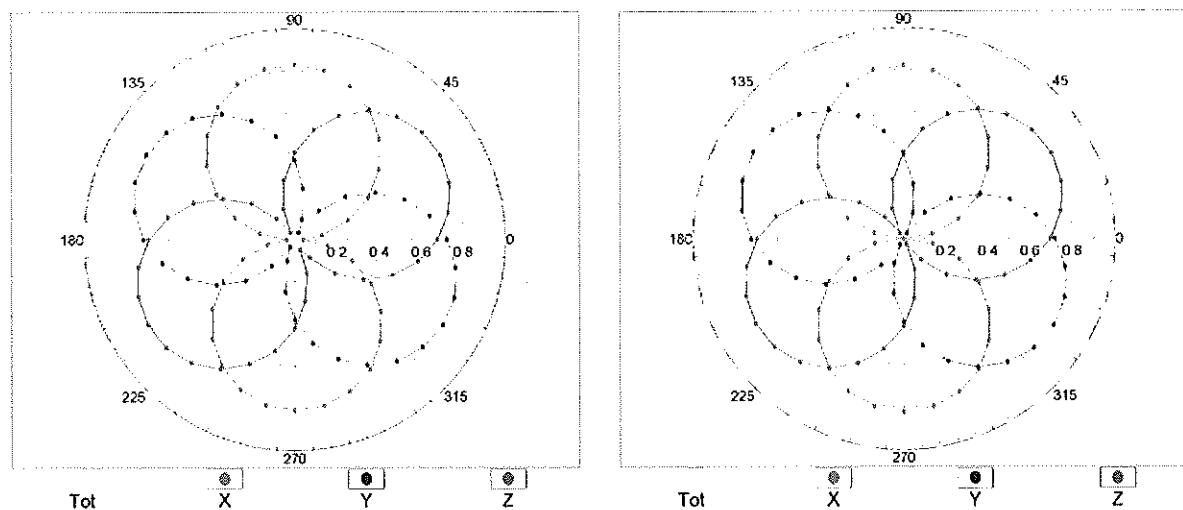

Uncertainty of Axial Isotropy Assessment: $\pm 0.5\%$ (k=2)


Dynamic Range f(SAR_{head})

(TEM cell , f = 900 MHz)

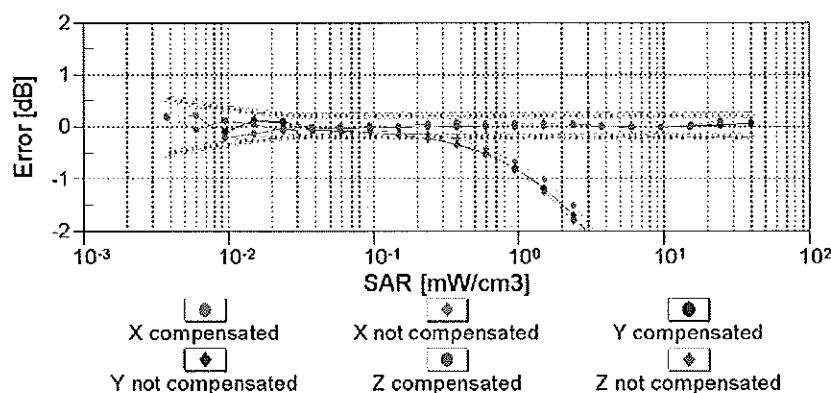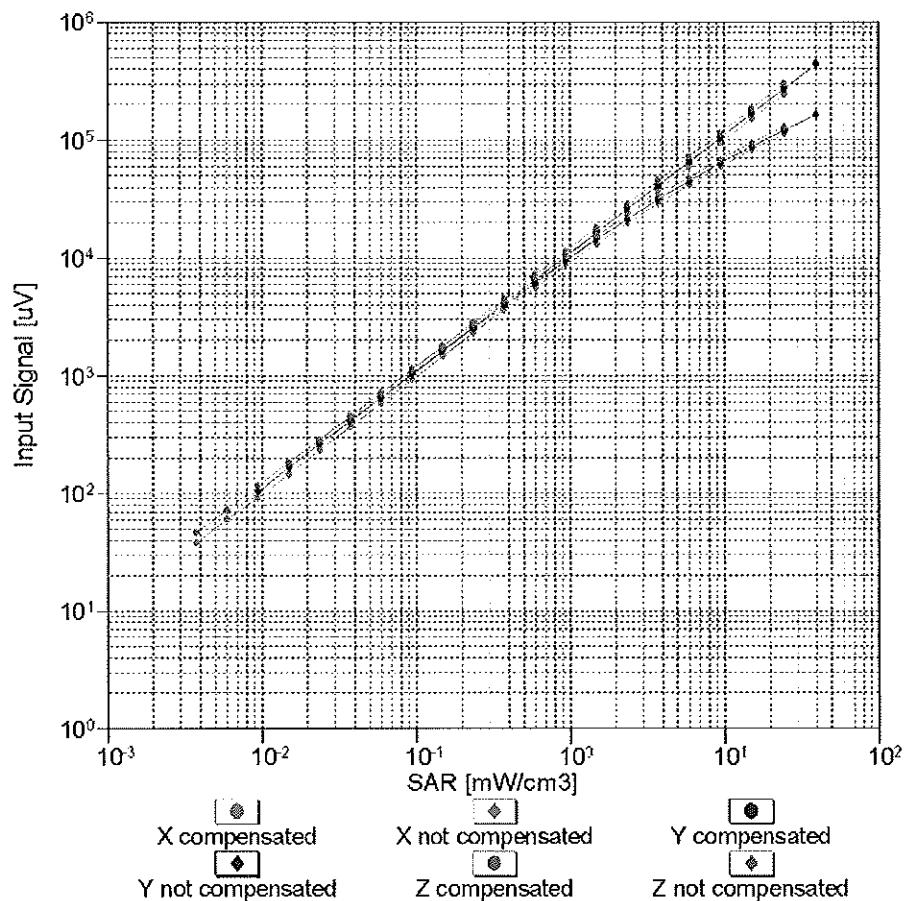


Uncertainty of Linearity Assessment: $\pm 0.6\%$ ($k=2$)

Conversion Factor Assessment

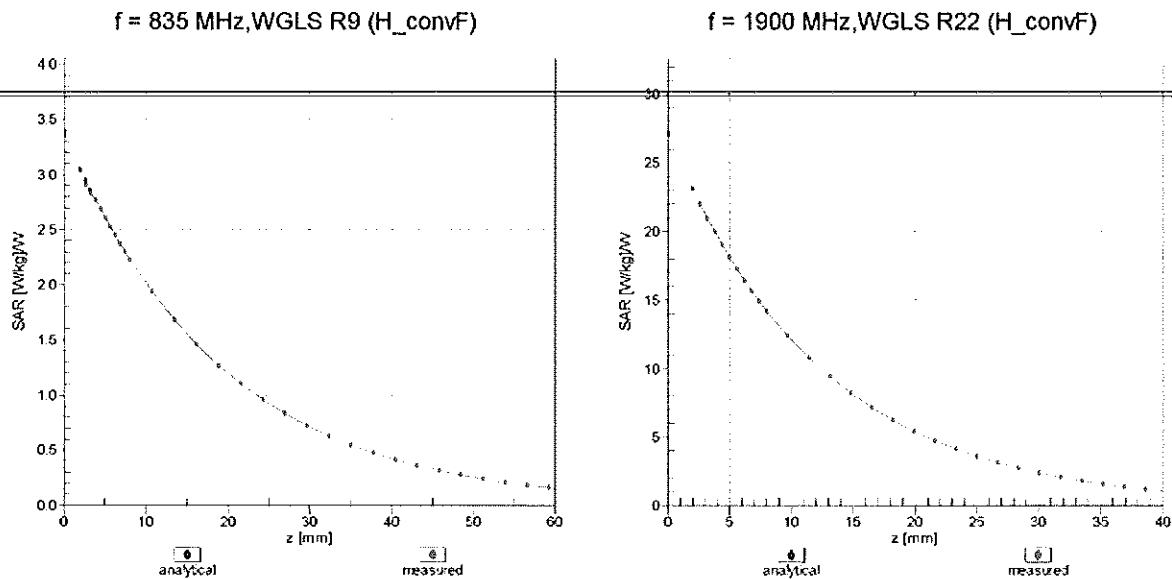

Deviation from Isotropy in Liquid

Error (ϕ, θ), $f = 900 \text{ MHz}$

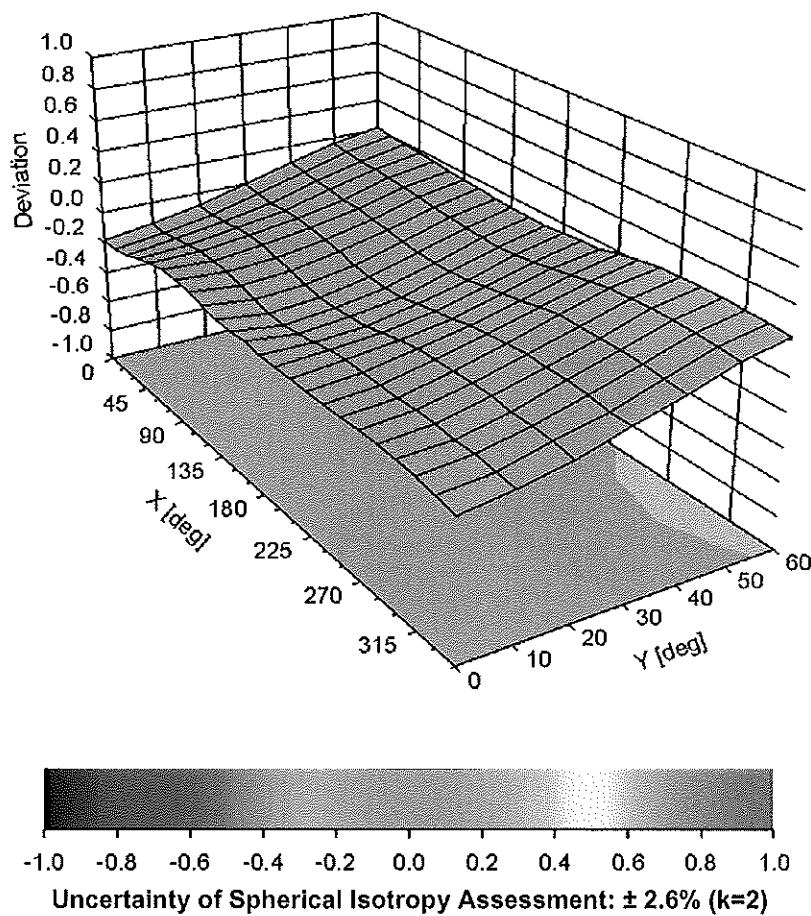

DASY/EASY - Parameters of Probe: ES3DV2 - SN:3022

Other Probe Parameters

| | |
|---|----------------|
| Sensor Arrangement | Triangular |
| Connector Angle (°) | Not applicable |
| Mechanical Surface Detection Mode | enabled |
| Optical Surface Detection Mode | disabled |
| Probe Overall Length | 337 mm |
| Probe Body Diameter | 10 mm |
| Tip Length | 10 mm |
| Tip Diameter | 4 mm |
| Probe Tip to Sensor X Calibration Point | 2 mm |
| Probe Tip to Sensor Y Calibration Point | 2 mm |
| Probe Tip to Sensor Z Calibration Point | 2 mm |
| Recommended Measurement Distance from Surface | 3 mm |

Additional Conversion Factors for Dosimetric E-Field Probe

Type:

ES3DV2

Serial Number:

3022

Place of Assessment:

Zurich

Date of Assessment:

August 29, 2011

Probe Calibration Date:

August 25, 2011

Schmid & Partner Engineering AG hereby certifies that conversion factor(s) of this probe have been evaluated on the date indicated above. The assessment was performed using the FDTD numerical code SEMCAD of Schmid & Partner Engineering AG. The evaluation is coupled with measured conversion factors (probe calibration date indicated above). The uncertainty of the numerical assessment is based on the extrapolation from measured value at 835 MHz or at 1750 MHz.

Assessed by:



Dosimetric E-Field Probe ES3DV2 SN:3022

Conversion factor (\pm standard deviation)

| | | | |
|------------------------------------|--------------|---------------------------------|---|
| 550 \pm 50 MHz | <i>ConvF</i> | 6.57 \pm 7% | $\epsilon_r = 56.3 \pm 5\%$ $\sigma = 0.95 \pm 5\%$ mho/m (body tissue) |
| 650 \pm 50 MHz | <i>ConvF</i> | 6.16 \pm 7% | $\epsilon_r = 55.9 \pm 5\%$ $\sigma = 0.95 \pm 5\%$ mho/m (body tissue) |

Important Note:

For numerically assessed probe conversion factors, parameters Alpha and Delta in the DASY software must have the following entries: Alpha = 0 and Delta = 1.

Please see also DASY Manual.



Accredited by the Swiss Accreditation Service (SAS)
 The Swiss Accreditation Service is one of the signatories to the EA
 Multilateral Agreement for the recognition of calibration certificates

Accreditation No.: **SCS 108**

Client **PC Test**

Certificate No: **ES3-3209_Mar12**

CALIBRATION CERTIFICATE

Object **ES3DV3 - SN:3209**

Calibration procedure(s) **QA CAL-01.v8, QA CAL-12.v7, QA CAL-23.v4, QA CAL-25.v4
 Calibration procedure for dosimetric E-field probes**

Calibration date: **March 16, 2012**

This calibration certificate documents the traceability to national standards, which realize the physical units of measurements (SI).
 The measurements and the uncertainties with confidence probability are given on the following pages and are part of the certificate.

All calibrations have been conducted in the closed laboratory facility: environment temperature (22 ± 3)°C and humidity < 70%.

Calibration Equipment used (M&TE critical for calibration)

KOK
 4/5/12

| Primary Standards | ID | Cal Date (Certificate No.) | Scheduled Calibration |
|----------------------------|-----------------|-----------------------------------|------------------------|
| Power meter E4419B | GB41293874 | 31-Mar-11 (No. 217-01372) | Apr-12 |
| Power sensor E4412A | MY41498087 | 31-Mar-11 (No. 217-01372) | Apr-12 |
| Reference 3 dB Attenuator | SN: S5054 (3c) | 29-Mar-11 (No. 217-01369) | Apr-12 |
| Reference 20 dB Attenuator | SN: S5086 (20b) | 29-Mar-11 (No. 217-01367) | Apr-12 |
| Reference 30 dB Attenuator | SN: S5129 (30b) | 29-Mar-11 (No. 217-01370) | Apr-12 |
| Reference Probe ES3DV2 | SN: 3013 | 29-Dec-11 (No. ES3-3013_Dec11) | Dec-12 |
| DAE4 | SN: 654 | 3-May-11 (No. DAE4-654_May11) | May-12 |
| Secondary Standards | ID | Check Date (in house) | Scheduled Check |
| RF generator HP 8648C | US3642U01700 | 4-Aug-99 (in house check Apr-11) | In house check: Apr-13 |
| Network Analyzer HP 8753E | US37390585 | 18-Oct-01 (in house check Oct-11) | In house check: Oct-12 |

| | | | |
|---|-------------------------------|--|------------------------|
| Calibrated by: | Name Jeton Kastrati | Function Laboratory Technician | Signature |
| Approved by: | Name Katja Pokovic | Function Technical Manager | Signature |
| This calibration certificate shall not be reproduced except in full without written approval of the laboratory. | | | Issued: March 19, 2012 |



Accredited by the Swiss Accreditation Service (SAS)

The Swiss Accreditation Service is one of the signatories to the EA
 Multilateral Agreement for the recognition of calibration certificates

Accreditation No.: **SCS 108**

Glossary:

| | |
|--------------------------|--|
| TSL | tissue simulating liquid |
| NORM x,y,z | sensitivity in free space |
| ConvF | sensitivity in TSL / NORM x,y,z |
| DCP | diode compression point |
| CF | crest factor (1/duty_cycle) of the RF signal |
| A, B, C | modulation dependent linearization parameters |
| Polarization φ | φ rotation around probe axis |
| Polarization ϑ | ϑ rotation around an axis that is in the plane normal to probe axis (at measurement center), i.e., $\vartheta = 0$ is normal to probe axis |

Calibration is Performed According to the Following Standards:

- IEEE Std 1528-2003, "IEEE Recommended Practice for Determining the Peak Spatial-Averaged Specific Absorption Rate (SAR) in the Human Head from Wireless Communications Devices: Measurement Techniques", December 2003
- IEC 62209-1, "Procedure to measure the Specific Absorption Rate (SAR) for hand-held devices used in close proximity to the ear (frequency range of 300 MHz to 3 GHz)", February 2005

Methods Applied and Interpretation of Parameters:

- $NORMx,y,z$: Assessed for E-field polarization $\vartheta = 0$ ($f \leq 900$ MHz in TEM-cell; $f > 1800$ MHz: R22 waveguide). $NORMx,y,z$ are only intermediate values, i.e., the uncertainties of $NORMx,y,z$ does not affect the E^2 -field uncertainty inside TSL (see below $ConvF$).
- $NORM(f)x,y,z = NORMx,y,z * frequency_response$ (see Frequency Response Chart). This linearization is implemented in DASY4 software versions later than 4.2. The uncertainty of the frequency response is included in the stated uncertainty of $ConvF$.
- $DCPx,y,z$: DCP are numerical linearization parameters assessed based on the data of power sweep with CW signal (no uncertainty required). DCP does not depend on frequency nor media.
- PAR : PAR is the Peak to Average Ratio that is not calibrated but determined based on the signal characteristics
- $Ax,y,z; Bx,y,z; Cx,y,z; VRx,y,z; A, B, C$ are numerical linearization parameters assessed based on the data of power sweep for specific modulation signal. The parameters do not depend on frequency nor media. VR is the maximum calibration range expressed in RMS voltage across the diode.
- ConvF and Boundary Effect Parameters*: Assessed in flat phantom using E-field (or Temperature Transfer Standard for $f \leq 800$ MHz) and inside waveguide using analytical field distributions based on power measurements for $f > 800$ MHz. The same setups are used for assessment of the parameters applied for boundary compensation (alpha, depth) of which typical uncertainty values are given. These parameters are used in DASY4 software to improve probe accuracy close to the boundary. The sensitivity in TSL corresponds to $NORMx,y,z * ConvF$ whereby the uncertainty corresponds to that given for $ConvF$. A frequency dependent $ConvF$ is used in DASY version 4.4 and higher which allows extending the validity from ± 50 MHz to ± 100 MHz.
- Spherical isotropy (3D deviation from isotropy)*: in a field of low gradients realized using a flat phantom exposed by a patch antenna.
- Sensor Offset*: The sensor offset corresponds to the offset of virtual measurement center from the probe tip (on probe axis). No tolerance required.

Probe ES3DV3

SN:3209

Manufactured: October 14, 2008
Calibrated: March 16, 2012

Calibrated for DASY/EASY Systems
(Note: non-compatible with DASY2 system!)

DASY/EASY - Parameters of Probe: ES3DV3 - SN:3209

Basic Calibration Parameters

| | Sensor X | Sensor Y | Sensor Z | Unc (k=2) |
|---|----------|----------|----------|--------------|
| Norm ($\mu\text{V}/(\text{V}/\text{m})^2$) ^A | 1.36 | 1.34 | 1.15 | $\pm 10.1\%$ |
| DCP (mV) ^B | 98.2 | 97.4 | 98.7 | |

Modulation Calibration Parameters

| UID | Communication System Name | PAR | | A dB | B dB | C dB | VR mV | Unc ^E (k=2) |
|-------|---------------------------|------|---|---------|---------|---------|----------|---------------------------|
| 10000 | CW | 0.00 | X | 0.00 | 0.00 | 1.00 | 119.2 | $\pm 3.5\%$ |
| | | | Y | 0.00 | 0.00 | 1.00 | 89.3 | |
| | | | Z | 0.00 | 0.00 | 1.00 | 111.5 | |

The reported uncertainty of measurement is stated as the standard uncertainty of measurement multiplied by the coverage factor k=2, which for a normal distribution corresponds to a coverage probability of approximately 95%.

^A The uncertainties of NormX,Y,Z do not affect the E²-field uncertainty inside TSL (see Pages 5 and 6).

^B Numerical linearization parameter: uncertainty not required.

^E Uncertainty is determined using the max. deviation from linear response applying rectangular distribution and is expressed for the square of the field value.

DASY/EASY - Parameters of Probe: ES3DV3 - SN:3209

Calibration Parameter Determined in Head Tissue Simulating Media

| f (MHz) ^C | Relative Permittivity ^F | Conductivity (S/m) ^F | ConvF X | ConvF Y | ConvF Z | Alpha | Depth (mm) | Unct. (k=2) |
|----------------------|------------------------------------|---------------------------------|---------|---------|---------|-------|------------|-------------|
| 750 | 41.9 | 0.89 | 6.47 | 6.47 | 6.47 | 0.37 | 1.61 | ± 12.0 % |
| 835 | 41.5 | 0.90 | 6.22 | 6.22 | 6.22 | 0.24 | 2.24 | ± 12.0 % |
| 1640 | 40.3 | 1.29 | 5.38 | 5.38 | 5.38 | 0.41 | 1.56 | ± 12.0 % |
| 1750 | 40.1 | 1.37 | 5.26 | 5.26 | 5.26 | 0.41 | 1.60 | ± 12.0 % |
| 1900 | 40.0 | 1.40 | 5.15 | 5.15 | 5.15 | 0.80 | 1.16 | ± 12.0 % |
| 2450 | 39.2 | 1.80 | 4.46 | 4.46 | 4.46 | 0.64 | 1.39 | ± 12.0 % |
| 2600 | 39.0 | 1.96 | 4.30 | 4.30 | 4.30 | 0.69 | 1.42 | ± 12.0 % |

^C Frequency validity of ± 100 MHz only applies for DASY v4.4 and higher (see Page 2), else it is restricted to ± 50 MHz. The uncertainty is the RSS of the ConvF uncertainty at calibration frequency and the uncertainty for the indicated frequency band.

^F At frequencies below 3 GHz, the validity of tissue parameters (ϵ and σ) can be relaxed to ± 10% if liquid compensation formula is applied to measured SAR values. At frequencies above 3 GHz, the validity of tissue parameters (ϵ and σ) is restricted to ± 5%. The uncertainty is the RSS of the ConvF uncertainty for indicated target tissue parameters.

DASY/EASY - Parameters of Probe: ES3DV3 - SN:3209

Calibration Parameter Determined in Body Tissue Simulating Media


| f (MHz) ^c | Relative Permittivity ^f | Conductivity (S/m) ^f | ConvF X | ConvF Y | ConvF Z | Alpha | Depth (mm) | Unct. (k=2) |
|----------------------|------------------------------------|---------------------------------|---------|---------|---------|-------|------------|-------------|
| 450 | 56.7 | 0.94 | 7.11 | 7.11 | 7.11 | 0.07 | 1.00 | ± 13.4 % |
| 750 | 55.5 | 0.96 | 6.23 | 6.23 | 6.23 | 0.54 | 1.40 | ± 12.0 % |
| 835 | 55.2 | 0.97 | 6.13 | 6.13 | 6.13 | 0.24 | 2.27 | ± 12.0 % |
| 1640 | 53.8 | 1.40 | 5.21 | 5.21 | 5.21 | 0.72 | 1.29 | ± 12.0 % |
| 1750 | 53.4 | 1.49 | 4.83 | 4.83 | 4.83 | 0.59 | 1.44 | ± 12.0 % |
| 1900 | 53.3 | 1.52 | 4.63 | 4.63 | 4.63 | 0.57 | 1.50 | ± 12.0 % |
| 2450 | 52.7 | 1.95 | 4.23 | 4.23 | 4.23 | 0.80 | 1.00 | ± 12.0 % |
| 2600 | 52.5 | 2.16 | 4.02 | 4.02 | 4.02 | 0.62 | 0.90 | ± 12.0 % |

^c Frequency validity of ± 100 MHz only applies for DASY v4.4 and higher (see Page 2), else it is restricted to ± 50 MHz. The uncertainty is the RSS of the ConvF uncertainty at calibration frequency and the uncertainty for the indicated frequency band.

^f At frequencies below 3 GHz, the validity of tissue parameters (ϵ and σ) can be relaxed to ± 10% if liquid compensation formula is applied to measured SAR values. At frequencies above 3 GHz, the validity of tissue parameters (ϵ and σ) is restricted to ± 5%. The uncertainty is the RSS of the ConvF uncertainty for indicated target tissue parameters.

Frequency Response of E-Field


(TEM-Cell:ifi110 EXX, Waveguide: R22)

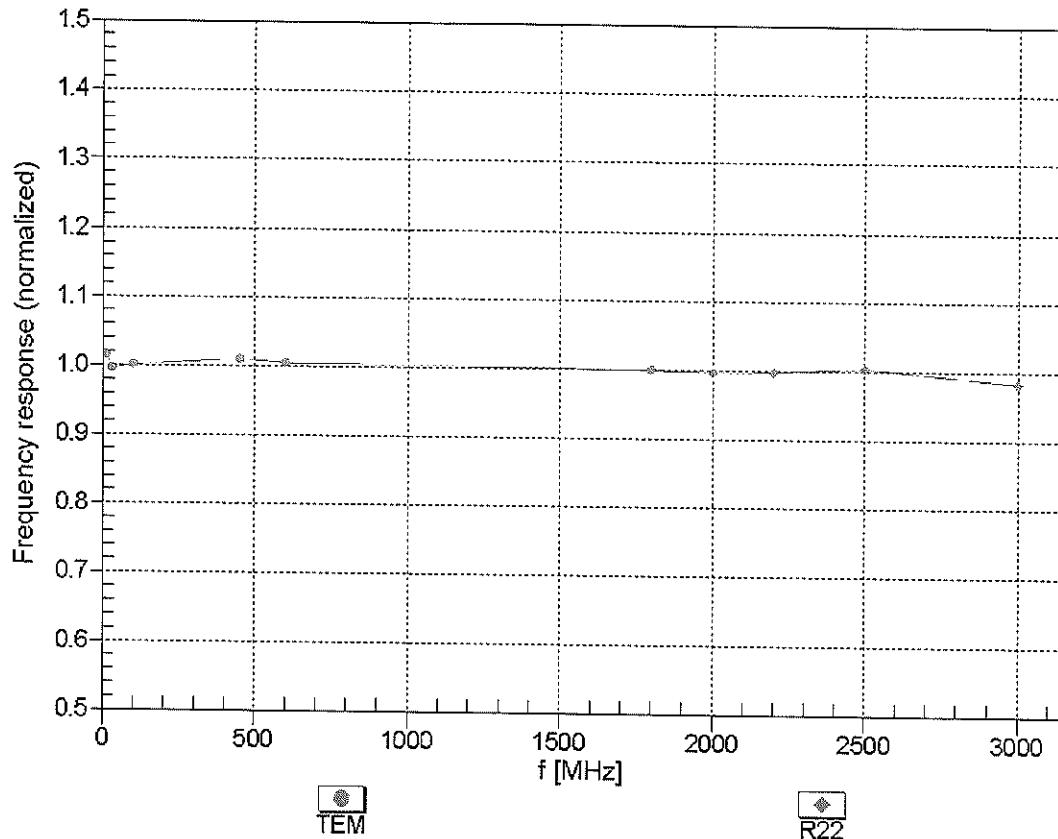



Uncertainty of Frequency Response of E-field: $\pm 6.3\%$ ($k=2$)

Receiving Pattern (ϕ), $\theta = 0^\circ$

$f=600$ MHz, TEM


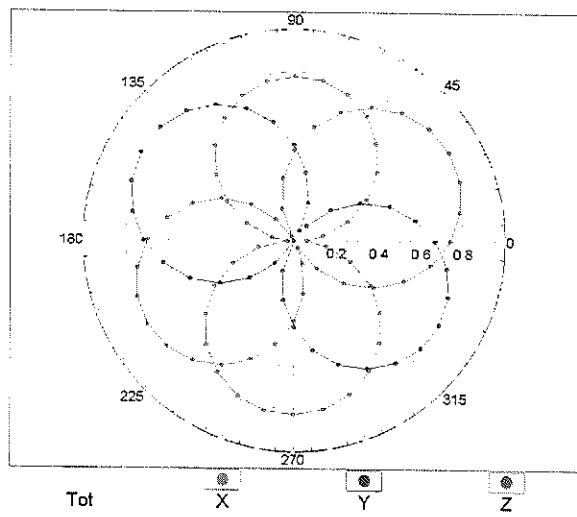


$f=1800$ MHz, R22

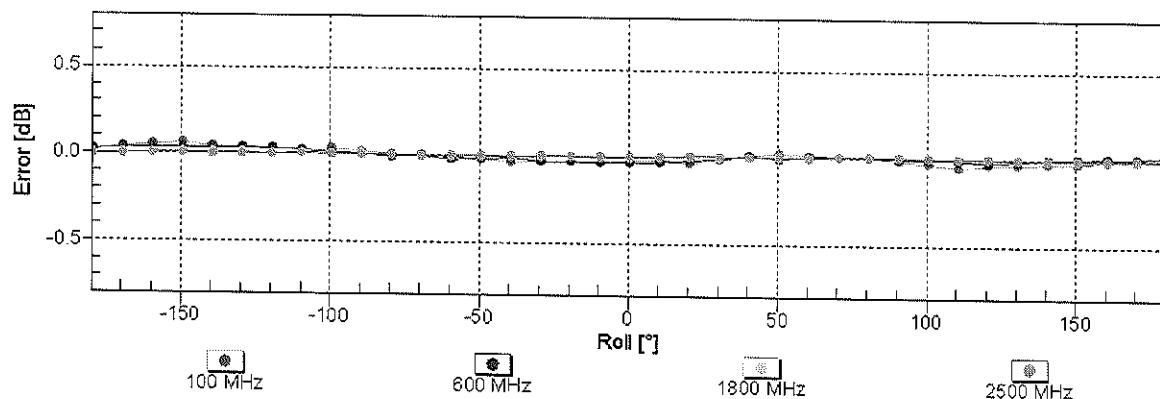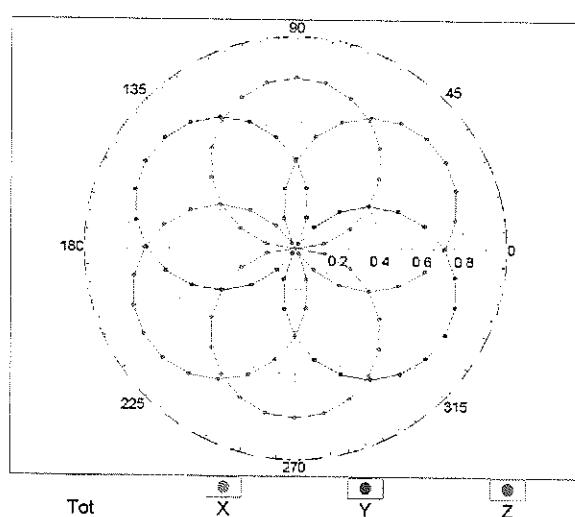


Uncertainty of Axial Isotropy Assessment: $\pm 0.5\%$ ($k=2$)

Dynamic Range $f(\text{SAR}_{\text{head}})$ (TEM cell , $f = 900 \text{ MHz}$)

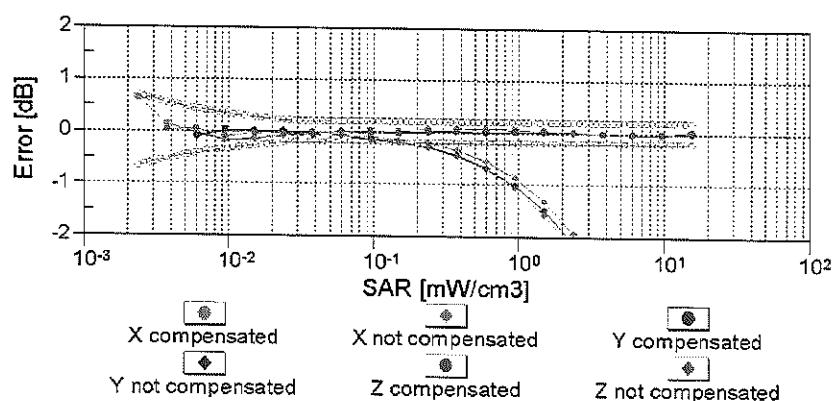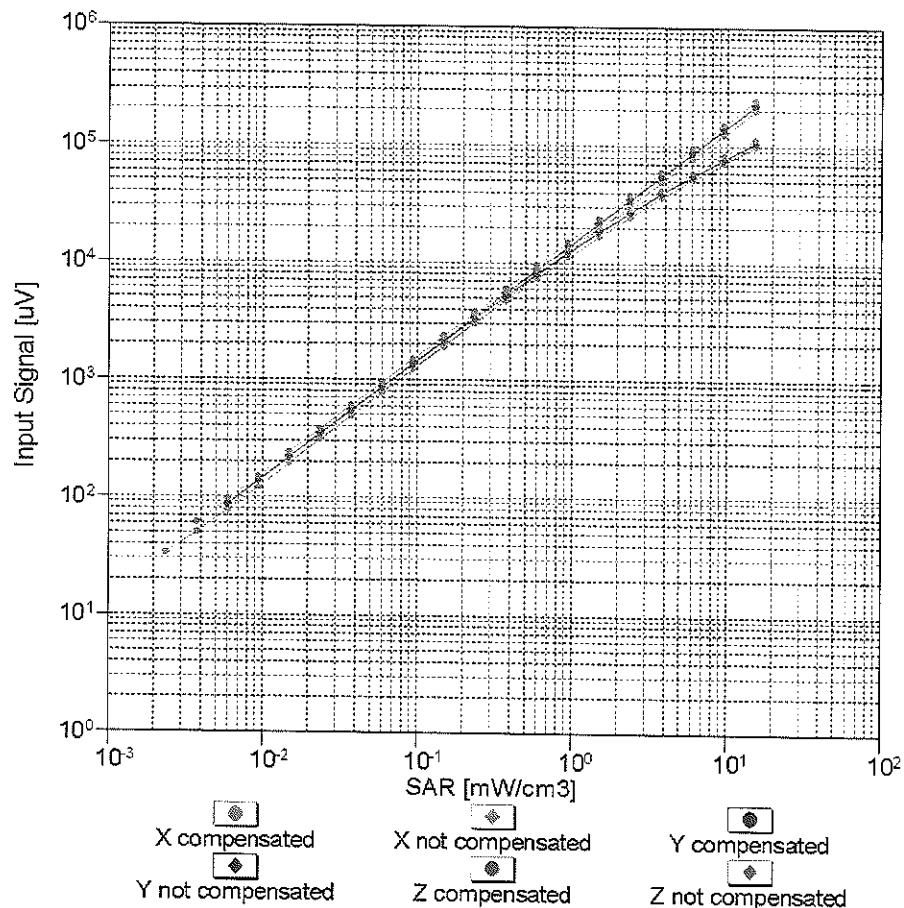



Uncertainty of Linearity Assessment: $\pm 0.6\% (k=2)$

Conversion Factor Assessment

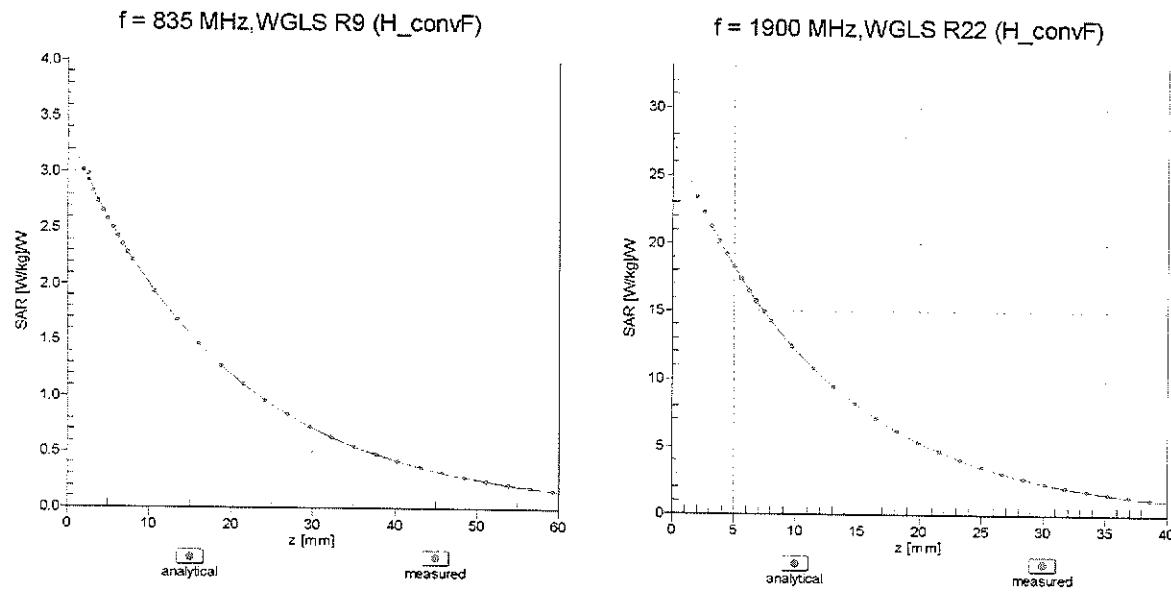

Deviation from Isotropy in Liquid

Error (ϕ, θ), $f = 900$ MHz

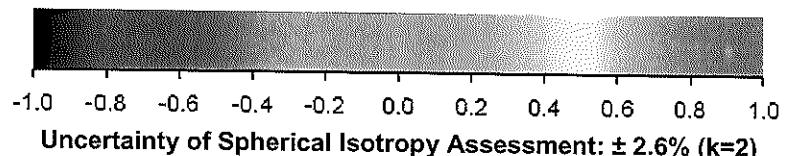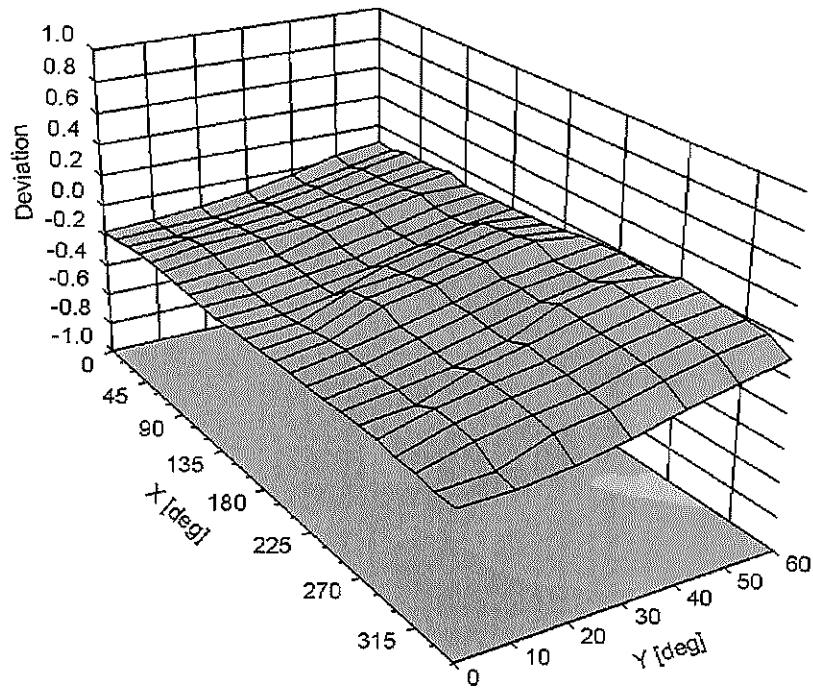

DASY/EASY - Parameters of Probe: ES3DV3 - SN:3209

Other Probe Parameters

| | |
|---|----------------|
| Sensor Arrangement | Triangular |
| Connector Angle (°) | Not applicable |
| Mechanical Surface Detection Mode | enabled |
| Optical Surface Detection Mode | disabled |
| Probe Overall Length | 337 mm |
| Probe Body Diameter | 10 mm |
| Tip Length | 10 mm |
| Tip Diameter | 4 mm |
| Probe Tip to Sensor X Calibration Point | 2 mm |
| Probe Tip to Sensor Y Calibration Point | 2 mm |
| Probe Tip to Sensor Z Calibration Point | 2 mm |
| Recommended Measurement Distance from Surface | 3 mm |



Accredited by the Swiss Accreditation Service (SAS)

Accreditation No.: SCS 108

The Swiss Accreditation Service is one of the signatories to the EA
Multilateral Agreement for the recognition of calibration certificates

Client

PC Test

Certificate No: EX3-3561_Jul11

CALIBRATION CERTIFICATE

Object EX3DV4 - SN:3561

Calibration procedure(s)
QA CAL-01.v8, QA CAL-14.v3, QA CAL-23.v4, QA CAL-25.v4
Calibration procedure for dosimetric E-field probes

Calibration date: July 27, 2011

This calibration certificate documents the traceability to national standards, which realize the physical units of measurements (SI).
The measurements and the uncertainties with confidence probability are given on the following pages and are part of the certificate.

All calibrations have been conducted in the closed laboratory facility: environment temperature $(22 \pm 3)^\circ\text{C}$ and humidity $< 70\%$.

Calibration Equipment used (M&TE critical for calibration)


✓OK
8/23/11

| Primary Standards | ID | Cal Date (Certificate No.) | Scheduled Calibration |
|----------------------------|-----------------|-----------------------------------|------------------------|
| Power meter E4419B | GB41293874 | 31-Mar-11 (No. 217-01372) | Apr-12 |
| Power sensor E4412A | MY41498087 | 31-Mar-11 (No. 217-01372) | Apr-12 |
| Reference 3 dB Attenuator | SN: S5054 (3c) | 29-Mar-11 (No. 217-01369) | Apr-12 |
| Reference 20 dB Attenuator | SN: S5086 (20b) | 29-Mar-11 (No. 217-01367) | Apr-12 |
| Reference 30 dB Attenuator | SN: S5129 (30b) | 29-Mar-11 (No. 217-01370) | Apr-12 |
| Reference Probe ES3DV2 | SN: 3013 | 29-Dec-10 (No. ES3-3013_Dec10) | Dec-11 |
| DAE4 | SN: 654 | 3-May-11 (No. DAE4-654_May11) | May-12 |
| | | | |
| Secondary Standards | ID | Check Date (in house) | Scheduled Check |
| RF generator HP 8648C | US3642U01700 | 4-Aug-99 (in house check Oct-09) | In house check: Oct-11 |
| Network Analyzer HP 8753E | US37390585 | 18-Oct-01 (in house check Oct-10) | In house check: Oct-11 |

| Calibrated by: | Name | Function | Signature |
|----------------|---------------|-------------------|-----------|
| | Katja Pokovic | Technical Manager | |
| Approved by: | Niels Kuster | Quality Manager | |

Issued: July 27, 2011

This calibration certificate shall not be reproduced except in full without written approval of the laboratory.

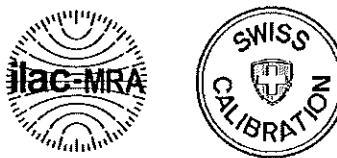

Accredited by the Swiss Accreditation Service (SAS)

The Swiss Accreditation Service is one of the signatories to the EA
 Multilateral Agreement for the recognition of calibration certificates

Accreditation No.: SCS 108

Glossary:

| | |
|------------------------|--|
| TSL | tissue simulating liquid |
| NORM x,y,z | sensitivity in free space |
| ConvF | sensitivity in TSL / NORM x,y,z |
| DCP | diode compression point |
| CF | crest factor (1/duty_cycle) of the RF signal |
| A, B, C | modulation dependent linearization parameters |
| Polarization φ | φ rotation around probe axis |
| Polarization θ | θ rotation around an axis that is in the plane normal to probe axis (at measurement center), i.e., $\theta = 0$ is normal to probe axis |

Calibration is Performed According to the Following Standards:

- IEEE Std 1528-2003, "IEEE Recommended Practice for Determining the Peak Spatial-Averaged Specific Absorption Rate (SAR) in the Human Head from Wireless Communications Devices: Measurement Techniques", December 2003
- IEC 62209-1, "Procedure to measure the Specific Absorption Rate (SAR) for hand-held devices used in close proximity to the ear (frequency range of 300 MHz to 3 GHz)", February 2005

Methods Applied and Interpretation of Parameters:

- $NORM_{x,y,z}$: Assessed for E-field polarization $\theta = 0$ ($f \leq 900$ MHz in TEM-cell; $f > 1800$ MHz: R22 waveguide). $NORM_{x,y,z}$ are only intermediate values, i.e., the uncertainties of $NORM_{x,y,z}$ does not affect the E^2 -field uncertainty inside TSL (see below ConvF).
- $NORM(f)x,y,z = NORM_{x,y,z} * frequency_response$ (see Frequency Response Chart). This linearization is implemented in DASY4 software versions later than 4.2. The uncertainty of the frequency response is included in the stated uncertainty of ConvF.
- $DCPx,y,z$: DCP are numerical linearization parameters assessed based on the data of power sweep with CW signal (no uncertainty required). DCP does not depend on frequency nor media.
- PAR : PAR is the Peak to Average Ratio that is not calibrated but determined based on the signal characteristics
- $Ax,y,z; Bx,y,z; Cx,y,z; VRx,y,z$: A, B, C are numerical linearization parameters assessed based on the data of power sweep for specific modulation signal. The parameters do not depend on frequency nor media. VR is the maximum calibration range expressed in RMS voltage across the diode.
- ConvF and Boundary Effect Parameters*: Assessed in flat phantom using E-field (or Temperature Transfer Standard for $f \leq 800$ MHz) and inside waveguide using analytical field distributions based on power measurements for $f > 800$ MHz. The same setups are used for assessment of the parameters applied for boundary compensation (alpha, depth) of which typical uncertainty values are given. These parameters are used in DASY4 software to improve probe accuracy close to the boundary. The sensitivity in TSL corresponds to $NORM_{x,y,z} * ConvF$ whereby the uncertainty corresponds to that given for ConvF. A frequency dependent ConvF is used in DASY version 4.4 and higher which allows extending the validity from ± 50 MHz to ± 100 MHz.
- Spherical Isotropy (3D deviation from isotropy)*: in a field of low gradients realized using a flat phantom exposed by a patch antenna.
- Sensor Offset*: The sensor offset corresponds to the offset of virtual measurement center from the probe tip (on probe axis). No tolerance required.

Probe EX3DV4

SN:3561

Manufactured: February 14, 2005
Calibrated: July 27, 2011

Calibrated for DASY/EASY Systems
(Note: non-compatible with DASY2 system!)

DASY/EASY - Parameters of Probe: EX3DV4 - SN:3561

Basic Calibration Parameters

| | Sensor X | Sensor Y | Sensor Z | Unc (k=2) |
|--|----------|----------|----------|--------------|
| Norm (μ V/(V/m) ²) ^A | 0.42 | 0.48 | 0.43 | \pm 10.1 % |
| DCP (mV) ^B | 93.4 | 99.3 | 96.6 | |

Modulation Calibration Parameters

| UID | Communication System Name | PAR | | A dB | B dB | C dB | VR mV | Unc ^E (k=2) |
|-------|---------------------------|------|---|---------|---------|---------|----------|---------------------------|
| 10000 | CW | 0.00 | X | 0.00 | 0.00 | 1.00 | 101.6 | \pm 2.7 % |
| | | | Y | 0.00 | 0.00 | 1.00 | 107.1 | |
| | | | Z | 0.00 | 0.00 | 1.00 | 104.3 | |

The reported uncertainty of measurement is stated as the standard uncertainty of measurement multiplied by the coverage factor k=2, which for a normal distribution corresponds to a coverage probability of approximately 95%.

^A The uncertainties of NormX,Y,Z do not affect the E²-field uncertainty inside TSL (see Pages 5 and 6).

^B Numerical linearization parameter: uncertainty not required.

^E Uncertainty is determined using the max. deviation from linear response applying rectangular distribution and is expressed for the square of the field value.

DASY/EASY - Parameters of Probe: EX3DV4 - SN:3561

Calibration Parameter Determined in Head Tissue Simulating Media

| f (MHz) ^c | Relative Permittivity ^f | Conductivity (S/m) ^f | ConvF X | ConvF Y | ConvF Z | Alpha | Depth (mm) | Unct. (k=2) |
|----------------------|------------------------------------|---------------------------------|---------|---------|---------|-------|------------|-------------|
| 750 | 41.9 | 0.89 | 8.38 | 8.38 | 8.38 | 0.80 | 0.70 | ± 12.0 % |
| 835 | 41.5 | 0.90 | 8.07 | 8.07 | 8.07 | 0.80 | 0.69 | ± 12.0 % |
| 1750 | 40.1 | 1.37 | 7.37 | 7.37 | 7.37 | 0.80 | 0.63 | ± 12.0 % |
| 1900 | 40.0 | 1.40 | 7.16 | 7.16 | 7.16 | 0.80 | 0.60 | ± 12.0 % |
| 2450 | 39.2 | 1.80 | 6.42 | 6.42 | 6.42 | 0.69 | 0.65 | ± 12.0 % |
| 2600 | 39.0 | 1.96 | 6.38 | 6.38 | 6.38 | 0.63 | 0.70 | ± 12.0 % |
| 4950 | 36.3 | 4.40 | 4.55 | 4.55 | 4.55 | 0.35 | 1.80 | ± 13.1 % |
| 5200 | 36.0 | 4.66 | 4.27 | 4.27 | 4.27 | 0.45 | 1.80 | ± 13.1 % |
| 5300 | 35.9 | 4.76 | 4.03 | 4.03 | 4.03 | 0.50 | 1.80 | ± 13.1 % |
| 5500 | 35.6 | 4.96 | 4.04 | 4.04 | 4.04 | 0.52 | 1.80 | ± 13.1 % |
| 5600 | 35.5 | 5.07 | 3.72 | 3.72 | 3.72 | 0.55 | 1.80 | ± 13.1 % |
| 5800 | 35.3 | 5.27 | 3.88 | 3.88 | 3.88 | 0.50 | 1.80 | ± 13.1 % |

^c Frequency validity of ± 100 MHz only applies for DASY v4.4 and higher (see Page 2), else it is restricted to ± 50 MHz. The uncertainty is the RSS of the ConvF uncertainty at calibration frequency and the uncertainty for the indicated frequency band.

^f At frequencies below 3 GHz, the validity of tissue parameters (ϵ and σ) can be relaxed to ± 10% if liquid compensation formula is applied to measured SAR values. At frequencies above 3 GHz, the validity of tissue parameters (ϵ and σ) is restricted to ± 5%. The uncertainty is the RSS of the ConvF uncertainty for indicated target tissue parameters.

DASY/EASY - Parameters of Probe: EX3DV4- SN:3561

Calibration Parameter Determined in Body Tissue Simulating Media


| f (MHz) ^c | Relative Permittivity ^f | Conductivity (S/m) ^f | ConvF X | ConvF Y | ConvF Z | Alpha | Depth (mm) | Unct. (k=2) |
|----------------------|------------------------------------|---------------------------------|---------|---------|---------|-------|------------|-------------|
| 750 | 55.5 | 0.96 | 8.34 | 8.34 | 8.34 | 0.80 | 0.77 | ± 12.0 % |
| 835 | 55.2 | 0.97 | 8.25 | 8.25 | 8.25 | 0.80 | 0.76 | ± 12.0 % |
| 1750 | 53.4 | 1.49 | 7.14 | 7.14 | 7.14 | 0.80 | 0.70 | ± 12.0 % |
| 1900 | 53.3 | 1.52 | 6.58 | 6.58 | 6.58 | 0.80 | 0.68 | ± 12.0 % |
| 2450 | 52.7 | 1.95 | 6.26 | 6.26 | 6.26 | 0.80 | 0.63 | ± 12.0 % |
| 2600 | 52.5 | 2.16 | 6.24 | 6.24 | 6.24 | 0.80 | 0.50 | ± 12.0 % |
| 4950 | 49.4 | 5.01 | 3.79 | 3.79 | 3.79 | 0.55 | 1.90 | ± 13.1 % |
| 5200 | 49.0 | 5.30 | 3.70 | 3.70 | 3.70 | 0.55 | 1.90 | ± 13.1 % |
| 5300 | 48.9 | 5.42 | 3.49 | 3.49 | 3.49 | 0.55 | 1.90 | ± 13.1 % |
| 5500 | 48.6 | 5.65 | 3.28 | 3.28 | 3.28 | 0.60 | 1.90 | ± 13.1 % |
| 5600 | 48.5 | 5.77 | 3.16 | 3.16 | 3.16 | 0.60 | 1.90 | ± 13.1 % |
| 5800 | 48.2 | 6.00 | 3.34 | 3.34 | 3.34 | 0.60 | 1.90 | ± 13.1 % |

^c Frequency validity of ± 100 MHz only applies for DASY v4.4 and higher (see Page 2), else it is restricted to ± 50 MHz. The uncertainty is the RSS of the ConvF uncertainty at calibration frequency and the uncertainty for the indicated frequency band.

^f At frequencies below 3 GHz, the validity of tissue parameters (ϵ and σ) can be relaxed to ± 10% if liquid compensation formula is applied to measured SAR values. At frequencies above 3 GHz, the validity of tissue parameters (ϵ and σ) is restricted to ± 5%. The uncertainty is the RSS of the ConvF uncertainty for indicated target tissue parameters.

Frequency Response of E-Field


(TEM-Cell:ifi110 EXX, Waveguide: R22)

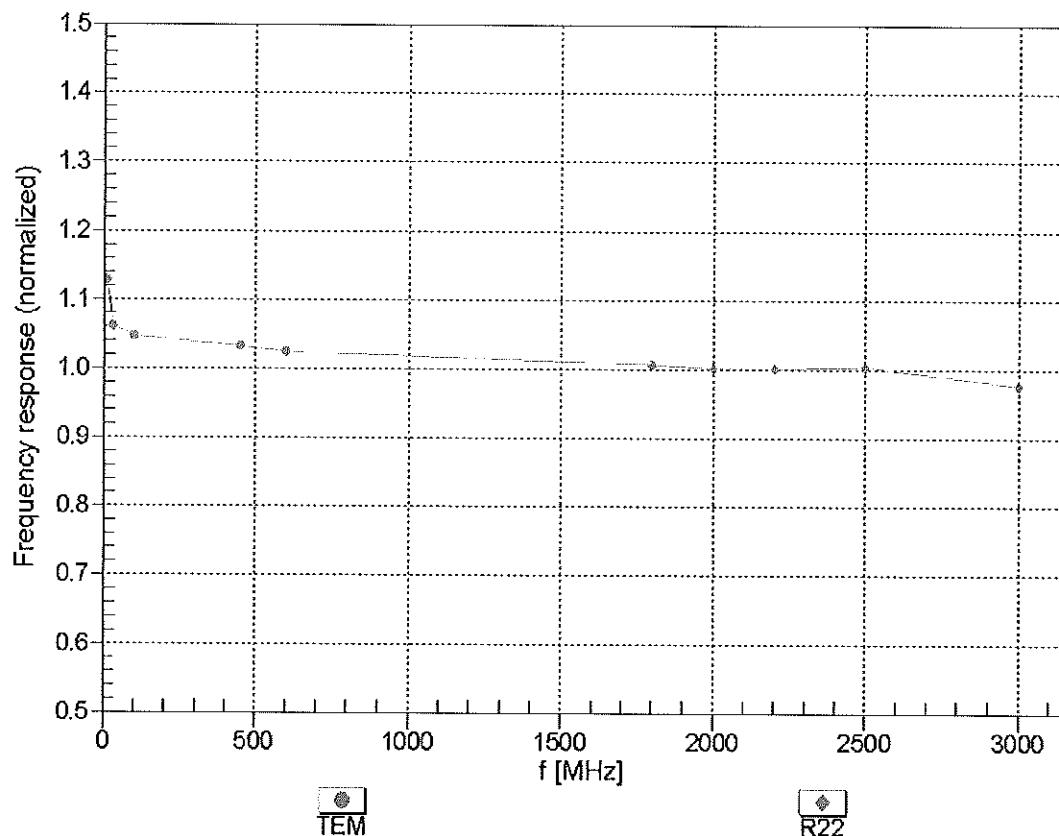



Uncertainty of Frequency Response of E-field: $\pm 6.3\%$ (k=2)

Receiving Pattern (ϕ), $\theta = 0^\circ$

$f=600$ MHz, TEM


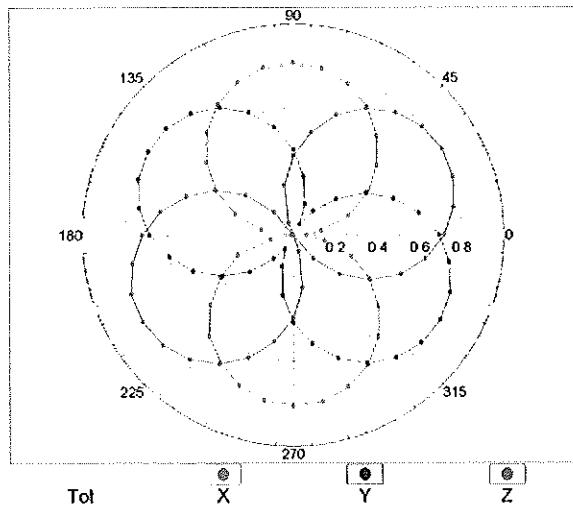


$f=1800$ MHz, R22

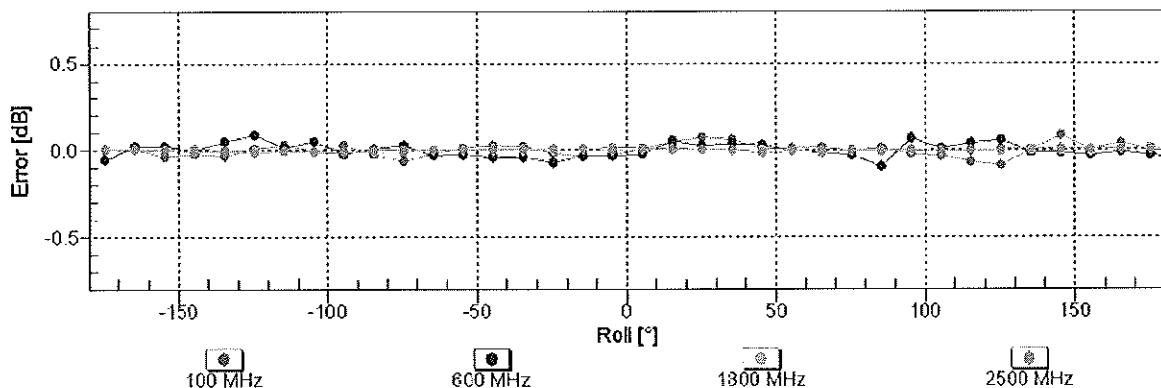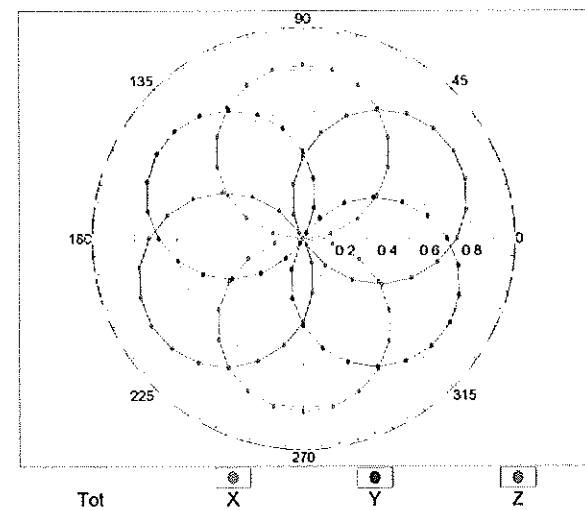

Uncertainty of Axial Isotropy Assessment: $\pm 0.5\%$ ($k=2$)

Dynamic Range $f(\text{SAR}_{\text{head}})$ (TEM cell, $f = 900 \text{ MHz}$)

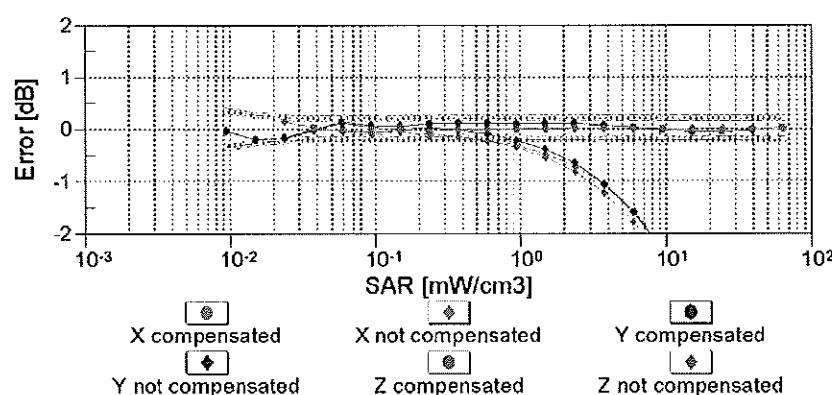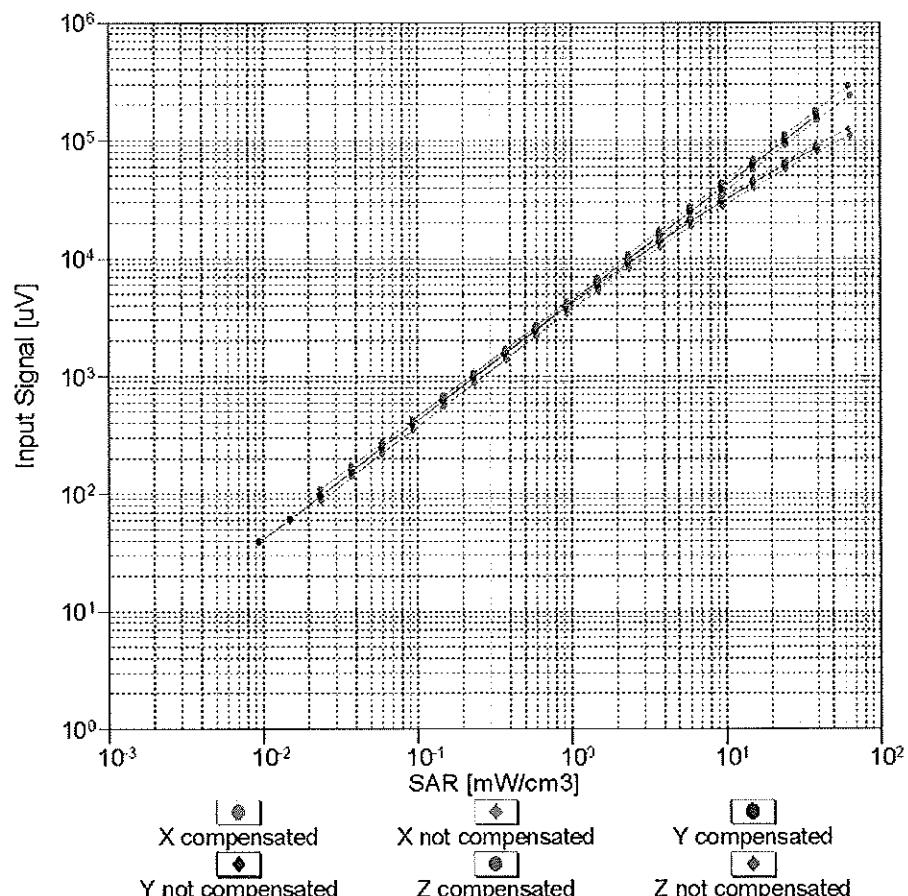


Uncertainty of Linearity Assessment: $\pm 0.6\%$ ($k=2$)

Conversion Factor Assessment


$f = 750 \text{ MHz, WGLS R9 (H_convF)}$

$f = 2600 \text{ MHz, WGLS R22 (H_convF)}$

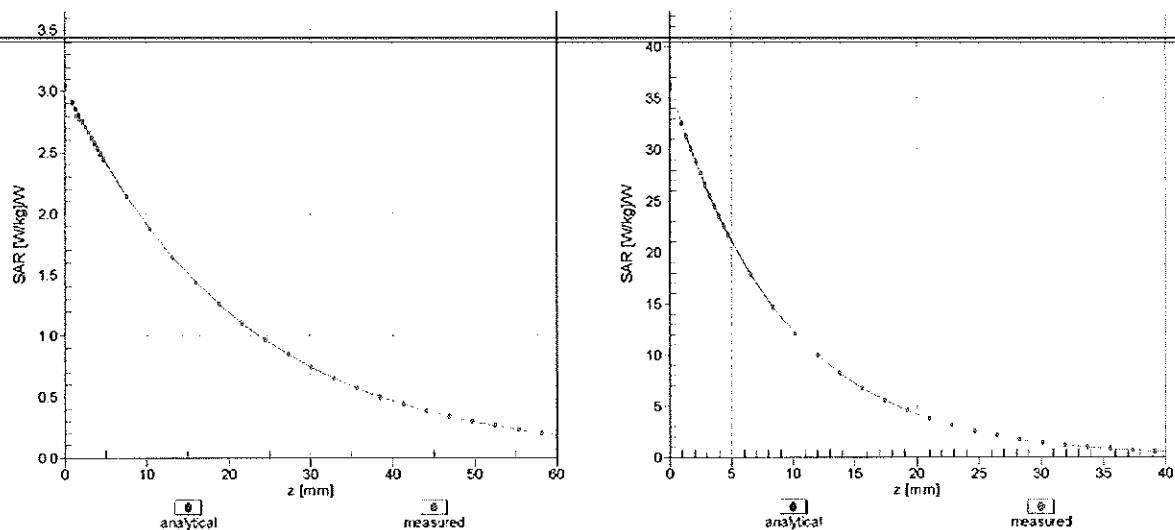

Deviation from Isotropy in Liquid

Error (ϕ, ϑ), $f = 900 \text{ MHz}$

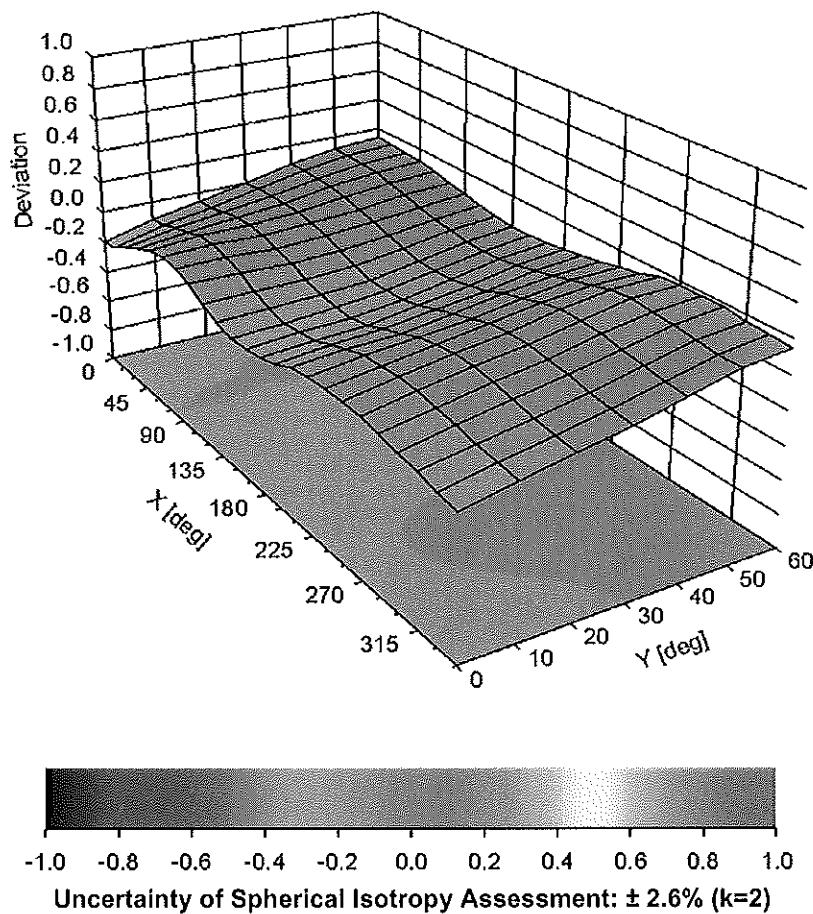

DASY/EASY - Parameters of Probe: EX3DV4 - SN:3561

Other Probe Parameters

| | |
|---|----------------|
| Sensor Arrangement | Triangular |
| Connector Angle (°) | Not applicable |
| Mechanical Surface Detection Mode | enabled |
| Optical Surface Detection Mode | disabled |
| Probe Overall Length | 337 mm |
| Probe Body Diameter | 10 mm |
| Tip Length | 9 mm |
| Tip Diameter | 2.5 mm |
| Probe Tip to Sensor X Calibration Point | 1 mm |
| Probe Tip to Sensor Y Calibration Point | 1 mm |
| Probe Tip to Sensor Z Calibration Point | 1 mm |
| Recommended Measurement Distance from Surface | 2 mm |



Accredited by the Swiss Accreditation Service (SAS)
The Swiss Accreditation Service is one of the signatories to the EA
Multilateral Agreement for the recognition of calibration certificates

Accreditation No.: SCS 108

Client PC Test

Certificate No: D1750V2-1051_Apr12

CALIBRATION CERTIFICATE

Object D1750V2 - SN: 1051

Calibration procedure(s) QA CAL-05.v8
Calibration procedure for dipole validation kits above 700 MHz

Calibration date: April 24, 2012

✓KOF
5/4/12

This calibration certificate documents the traceability to national standards, which realize the physical units of measurements (SI). The measurements and the uncertainties with confidence probability are given on the following pages and are part of the certificate.

All calibrations have been conducted in the closed laboratory facility: environment temperature (22 ± 3)°C and humidity < 70%.

Calibration Equipment used (M&TE critical for calibration)

| Primary Standards | ID # | Cal Date (Certificate No.) | Scheduled Calibration |
|-----------------------------|--------------------|-----------------------------------|------------------------|
| Power meter EPM-442A | GB37480704 | 05-Oct-11 (No. 217-01451) | Oct-12 |
| Power sensor HP 8481A | US37292783 | 05-Oct-11 (No. 217-01451) | Oct-12 |
| Reference 20 dB Attenuator | SN: 5058 (20k) | 27-Mar-12 (No. 217-01530) | Apr-13 |
| Type-N mismatch combination | SN: 5047.2 / 06327 | 27-Mar-12 (No. 217-01533) | Apr-13 |
| Reference Probe ES3DV3 | SN: 3205 | 30-Dec-11 (No. ES3-3205_Dec11) | Dec-12 |
| DAE4 | SN: 601 | 04-Jul-11 (No. DAE4-601_Jul11) | Jul-12 |
| Secondary Standards | ID # | Check Date (in house) | Scheduled Check |
| Power sensor HP 8481A | MY41092317 | 18-Oct-02 (in house check Oct-11) | In house check: Oct-13 |
| RF generator R&S SMT-06 | 100005 | 04-Aug-99 (in house check Oct-11) | In house check: Oct-13 |
| Network Analyzer HP 8753E | US37390585 S4206 | 18-Oct-01 (in house check Oct-11) | In house check: Oct-12 |

Calibrated by: Name Dimce Iliev Function Laboratory Technician Signature

Approved by: Name Katja Pokovic Function Technical Manager Signature

Issued: April 24, 2012

This calibration certificate shall not be reproduced except in full without written approval of the laboratory.



Accredited by the Swiss Accreditation Service (SAS)

The Swiss Accreditation Service is one of the signatories to the EA
Multilateral Agreement for the recognition of calibration certificates

Accreditation No.: SCS 108

Glossary:

| | |
|-------|--------------------------------|
| TS | tissue simulating liquid |
| ConvF | sensitivity in TS / NORM x,y,z |
| N/A | not applicable or not measured |

Calibration is Performed According to the Following Standards:

- a) IEEE Std 1528-2003, "IEEE Recommended Practice for Determining the Peak Spatial-Averaged Specific Absorption Rate (SAR) in the Human Head from Wireless Communications Devices: Measurement Techniques", December 2003
- b) IEC 62209-1, "Procedure to measure the Specific Absorption Rate (SAR) for hand-held devices used in close proximity to the ear (frequency range of 300 MHz to 3 GHz)", February 2005
- c) Federal Communications Commission Office of Engineering & Technology (FCC OET), "Evaluating Compliance with FCC Guidelines for Human Exposure to Radiofrequency Electromagnetic Fields; Additional Information for Evaluating Compliance of Mobile and Portable Devices with FCC Limits for Human Exposure to Radiofrequency Emissions", Supplement C (Edition 01-01) to Bulletin 65

Additional Documentation:

- d) DASY4/5 System Handbook

Methods Applied and Interpretation of Parameters:

- *Measurement Conditions:* Further details are available from the Validation Report at the end of the certificate. All figures stated in the certificate are valid at the frequency indicated.
- *Antenna Parameters with TS:* The dipole is mounted with the spacer to position its feed point exactly below the center marking of the flat phantom section, with the arms oriented parallel to the body axis.
- *Feed Point Impedance and Return Loss:* These parameters are measured with the dipole positioned under the liquid filled phantom. The impedance stated is transformed from the measurement at the SMA connector to the feed point. The Return Loss ensures low reflected power. No uncertainty required.
- *Electrical Delay:* One-way delay between the SMA connector and the antenna feed point. No uncertainty required.
- *SAR measured:* SAR measured at the stated antenna input power.
- *SAR normalized:* SAR as measured, normalized to an input power of 1 W at the antenna connector.
- *SAR for nominal TS parameters:* The measured TS parameters are used to calculate the nominal SAR result.

The reported uncertainty of measurement is stated as the standard uncertainty of measurement multiplied by the coverage factor $k=2$, which for a normal distribution corresponds to a coverage probability of approximately 95%.

Measurement Conditions

DASY system configuration, as far as not given on page 1.

| | | |
|------------------------------|------------------------|-------------|
| DASY Version | DASY5 | V52.8.1 |
| Extrapolation | Advanced Extrapolation | |
| Phantom | Modular Flat Phantom | |
| Distance Dipole Center - TSL | 10 mm | with Spacer |
| Zoom Scan Resolution | dx, dy, dz = 5 mm | |
| Frequency | 1750 MHz \pm 1 MHz | |

Head TSL parameters

The following parameters and calculations were applied.

| | Temperature | Permittivity | Conductivity |
|---|---------------------|----------------|----------------------|
| Nominal Head TSL parameters | 22.0 °C | 40.1 | 1.37 mho/m |
| Measured Head TSL parameters | (22.0 \pm 0.2) °C | 40.6 \pm 6 % | 1.35 mho/m \pm 6 % |
| Head TSL temperature change during test | < 0.5 °C | ---- | ---- |

SAR result with Head TSL

| | | |
|---|--------------------|-------------------------------|
| SAR averaged over 1 cm ³ (1 g) of Head TSL | Condition | |
| SAR measured | 250 mW input power | 9.03 mW / g |
| SAR for nominal Head TSL parameters | normalized to 1W | 36.6 mW /g \pm 17.0 % (k=2) |

| | | |
|---|--------------------|-------------------------------|
| SAR averaged over 10 cm ³ (10 g) of Head TSL | condition | |
| SAR measured | 250 mW input power | 4.83 mW / g |
| SAR for nominal Head TSL parameters | normalized to 1W | 19.5 mW /g \pm 16.5 % (k=2) |

Body TSL parameters

The following parameters and calculations were applied.

| | Temperature | Permittivity | Conductivity |
|---|---------------------|----------------|----------------------|
| Nominal Body TSL parameters | 22.0 °C | 53.4 | 1.49 mho/m |
| Measured Body TSL parameters | (22.0 \pm 0.2) °C | 52.9 \pm 6 % | 1.47 mho/m \pm 6 % |
| Body TSL temperature change during test | < 0.5 °C | ---- | ---- |

SAR result with Body TSL

| | | |
|---|--------------------|--------------------------------|
| SAR averaged over 1 cm ³ (1 g) of Body TSL | Condition | |
| SAR measured | 250 mW input power | 9.33 mW / g |
| SAR for nominal Body TSL parameters | normalized to 1W | 37.6 mW / g \pm 17.0 % (k=2) |

| | | |
|---|--------------------|--------------------------------|
| SAR averaged over 10 cm ³ (10 g) of Body TSL | condition | |
| SAR measured | 250 mW input power | 5.03 mW / g |
| SAR for nominal Body TSL parameters | normalized to 1W | 20.2 mW / g \pm 16.5 % (k=2) |

Appendix

Antenna Parameters with Head TSL

| | |
|--------------------------------------|-------------------------------|
| Impedance, transformed to feed point | 50.7 Ω - 0.2 $j\Omega$ |
| Return Loss | - 42.8 dB |

Antenna Parameters with Body TSL

| | |
|--------------------------------------|-------------------------------|
| Impedance, transformed to feed point | 46.0 Ω + 0.0 $j\Omega$ |
| Return Loss | - 27.5 dB |

General Antenna Parameters and Design

| | |
|----------------------------------|----------|
| Electrical Delay (one direction) | 1.222 ns |
|----------------------------------|----------|

After long term use with 100W radiated power, only a slight warming of the dipole near the feedpoint can be measured.

The dipole is made of standard semirigid coaxial cable. The center conductor of the feeding line is directly connected to the second arm of the dipole. The antenna is therefore short-circuited for DC-signals. On some of the dipoles, small end caps are added to the dipole arms in order to improve matching when loaded according to the position as explained in the "Measurement Conditions" paragraph. The SAR data are not affected by this change. The overall dipole length is still according to the Standard.

No excessive force must be applied to the dipole arms, because they might bend or the soldered connections near the feedpoint may be damaged.

Additional EUT Data

| | |
|-----------------|-------------------|
| Manufactured by | SPEAG |
| Manufactured on | February 19, 2010 |

DASY5 Validation Report for Head TSL

Date: 24.04.2012

Test Laboratory: SPEAG, Zurich, Switzerland

DUT: Dipole 1750 MHz; Type: D1750V2; Serial: D1750V2 - SN: 1051

Communication System: CW; Frequency: 1750 MHz

Medium parameters used: $f = 1750$ MHz; $\sigma = 1.35$ mho/m; $\epsilon_r = 40.6$; $\rho = 1000$ kg/m³

Phantom section: Flat Section

Measurement Standard: DASY5 (IEEE/IEC/ANSI C63.19-2007)

DASY52 Configuration:

- Probe: ES3DV3 - SN3205; ConvF(5.22, 5.22, 5.22); Calibrated: 30.12.2011;
- Sensor-Surface: 3mm (Mechanical Surface Detection)
- Electronics: DAE4 Sn601; Calibrated: 04.07.2011
- Phantom: Flat Phantom 5.0 (front); Type: QD000P50AA; Serial: 1001
- DASY52 52.8.1(838); SEMCAD X 14.6.5(6469)

Dipole Calibration for Head Tissue/Pin=250 mW, d=10mm/Zoom Scan (7x7x7)/Cube 0:


Measurement grid: dx=5mm, dy=5mm, dz=5mm

Reference Value = 93.857 V/m; Power Drift = 0.05 dB


Peak SAR (extrapolated) = 16.022 mW/g

SAR(1 g) = 9.03 mW/g; SAR(10 g) = 4.83 mW/g

Maximum value of SAR (measured) = 11.2 mW/g

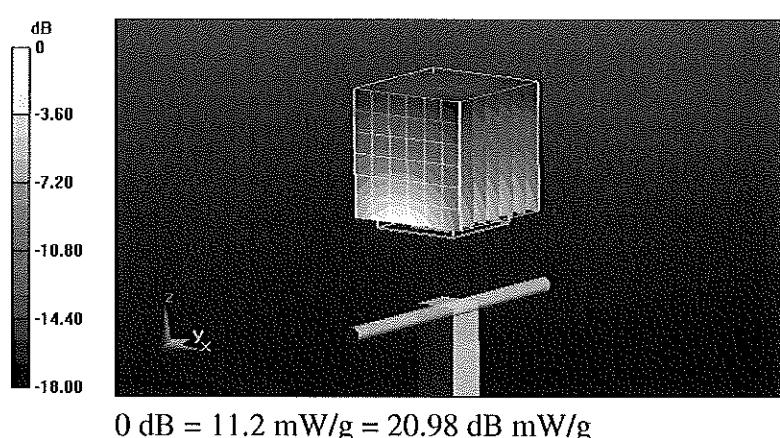

Impedance Measurement Plot for Head TSL

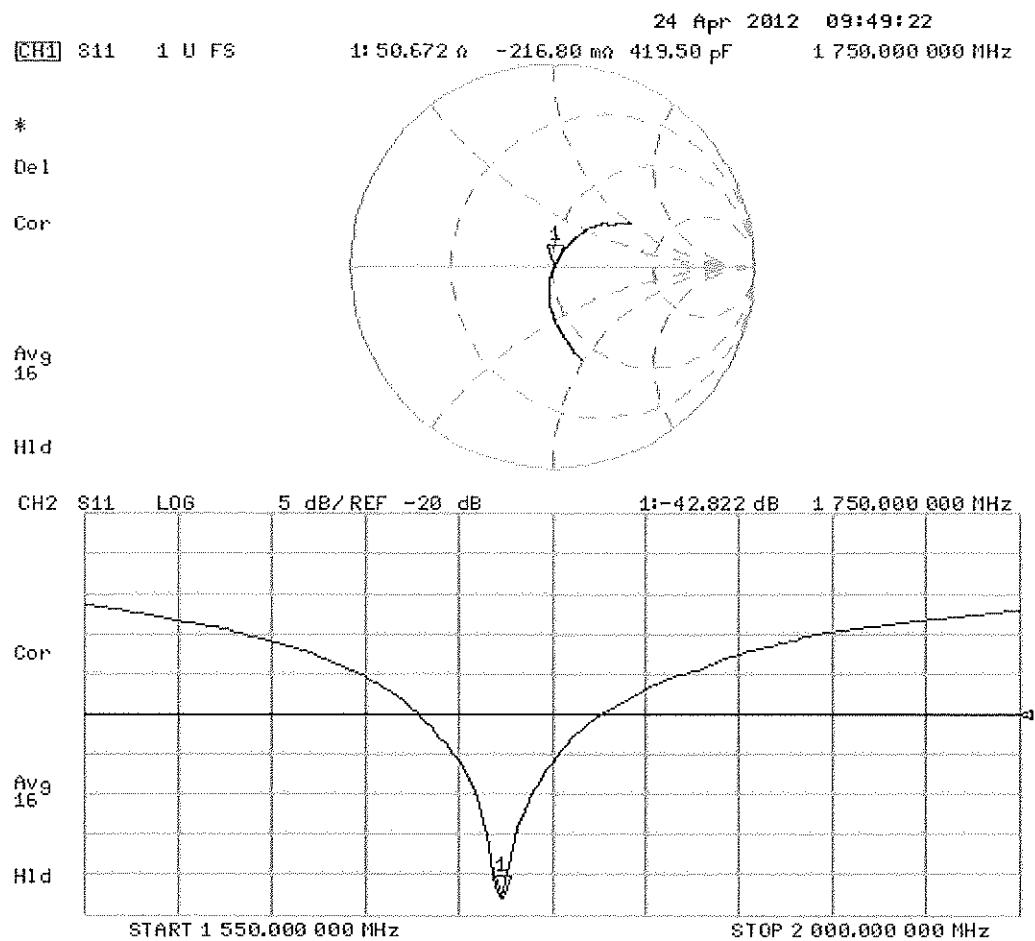

DASY5 Validation Report for Body TSL

Date: 24.04.2012

Test Laboratory: SPEAG, Zurich, Switzerland

DUT: Dipole 1750 MHz; Type: D1750V2; Serial: D1750V2 - SN: 1051

Communication System: CW; Frequency: 1750 MHz

Medium parameters used: $f = 1750$ MHz; $\sigma = 1.47$ mho/m; $\epsilon_r = 52.9$; $\rho = 1000$ kg/m³

Phantom section: Flat Section

Measurement Standard: DASY5 (IEEE/IEC/ANSI C63.19-2007)

DASY52 Configuration:

- Probe: ES3DV3 - SN3205; ConvF(4.85, 4.85, 4.85); Calibrated: 30.12.2011;
- Sensor-Surface: 3mm (Mechanical Surface Detection)
- Electronics: DAE4 Sn601; Calibrated: 04.07.2011
- Phantom: Flat Phantom 5.0 (back); Type: QD000P50AA; Serial: 1002
- DASY52 52.8.1(838); SEMCAD X 14.6.5(6469)

Dipole Calibration for Body Tissue/Pin=250 mW, d=10mm/Zoom Scan (7x7x7)/Cube 0:


Measurement grid: dx=5mm, dy=5mm, dz=5mm

Reference Value = 93.394 V/m; Power Drift = -0.01 dB

Peak SAR (extrapolated) = 15.953 mW/g

SAR(1 g) = 9.33 mW/g; SAR(10 g) = 5.03 mW/g

Maximum value of SAR (measured) = 11.7 mW/g

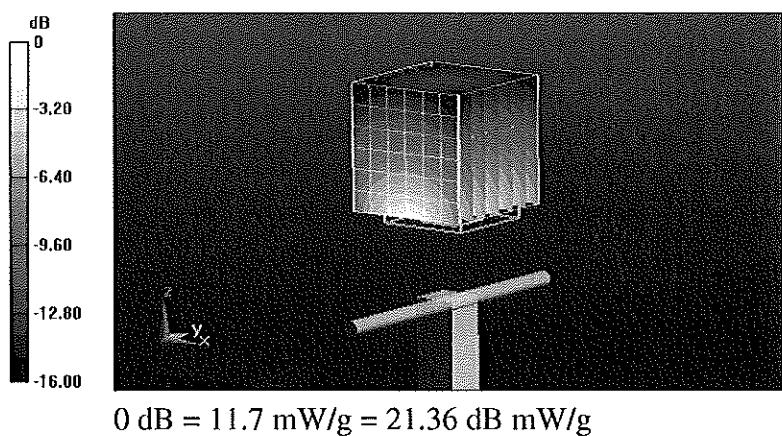

Impedance Measurement Plot for Body TSL

