

Contents

APPENDIX

1. Photographs of Test Setup.....	02
2. Photographs of EUT.....	08
3. Photographs of the Battery.....	13

1. Photographs of Test Setup

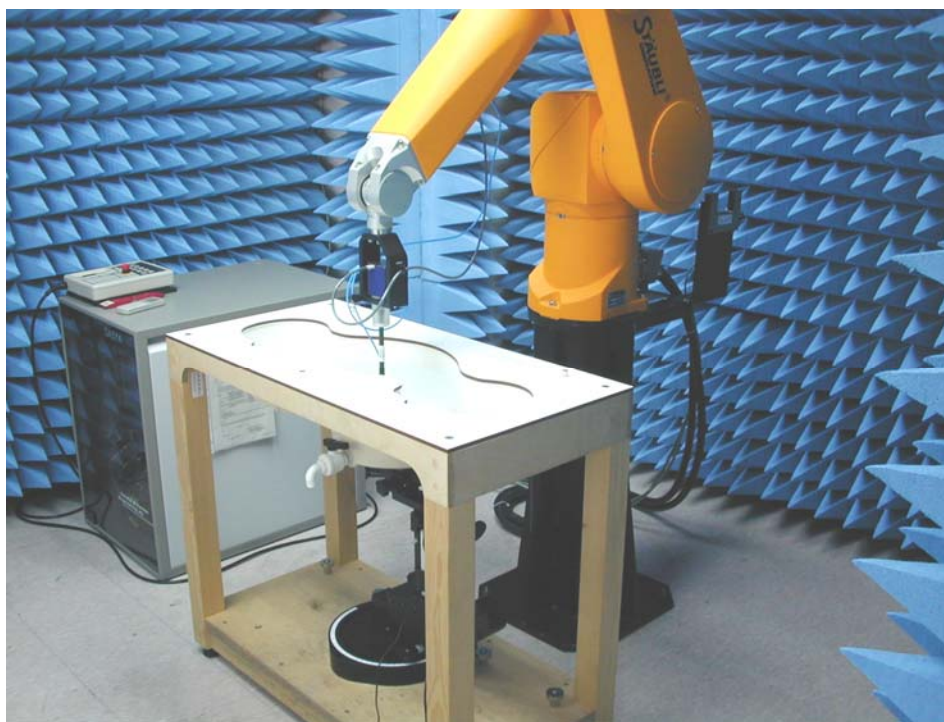


Fig.1 Photograph of the SAR measurement System

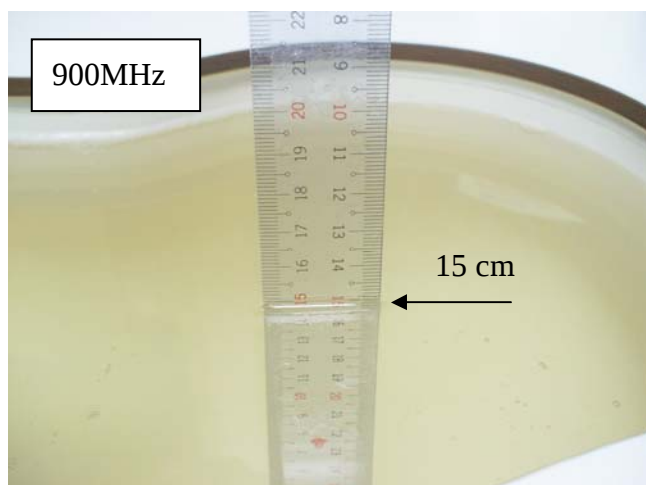


Fig.2.1 Photograph of the Tissue Simulant Fluid liquid depth 15cm for Left-head Side

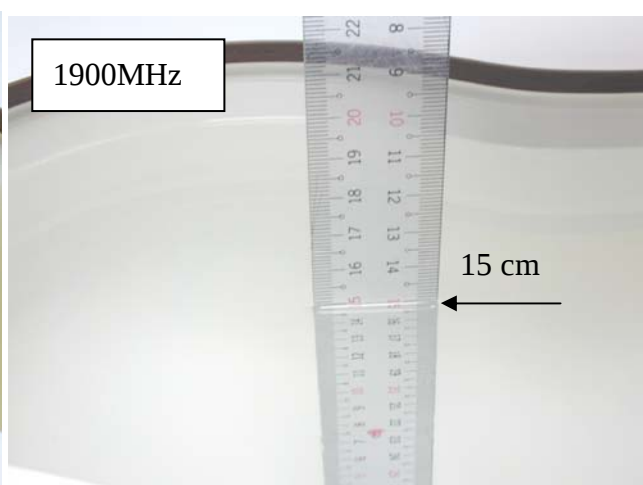


Fig.2.2 Photograph of the Tissue Simulant Fluid liquid depth 15cm for Right-head Side

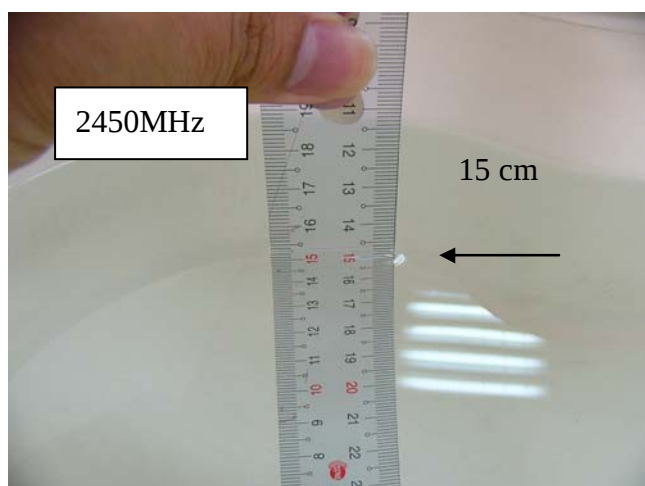


Fig.2.3 Photograph of the Tissue Simulant Fluid liquid depth 15cm for Right-head Side

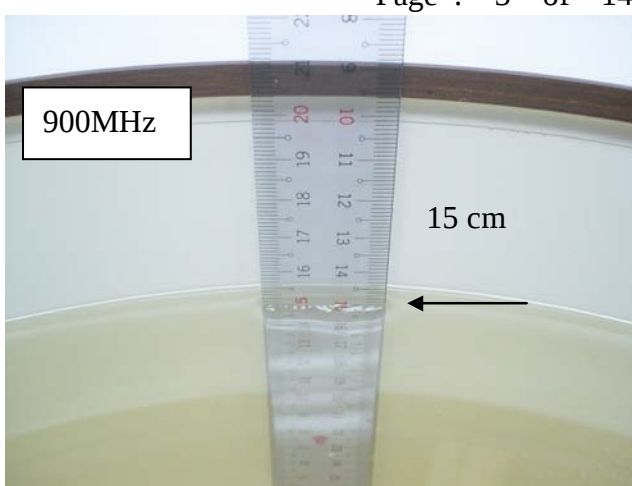


Fig.2.4 Photograph of the Tissue Simulant Fluid liquid depth 15cm for Flat (Body)

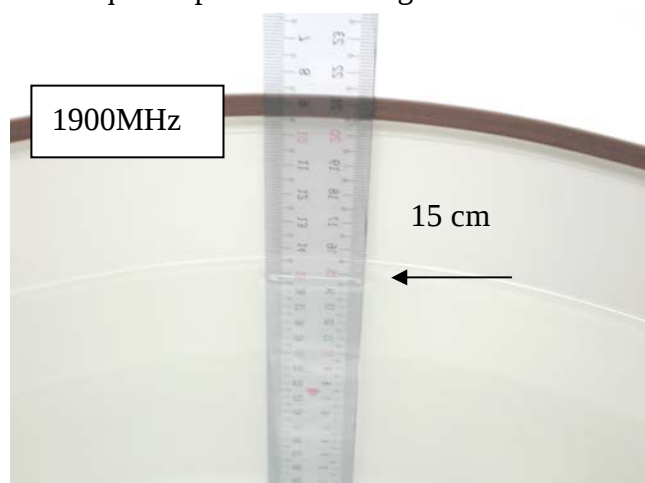


Fig.2.5 Photograph of the Tissue Simulant Fluid liquid depth 15cm for Flat (Body)

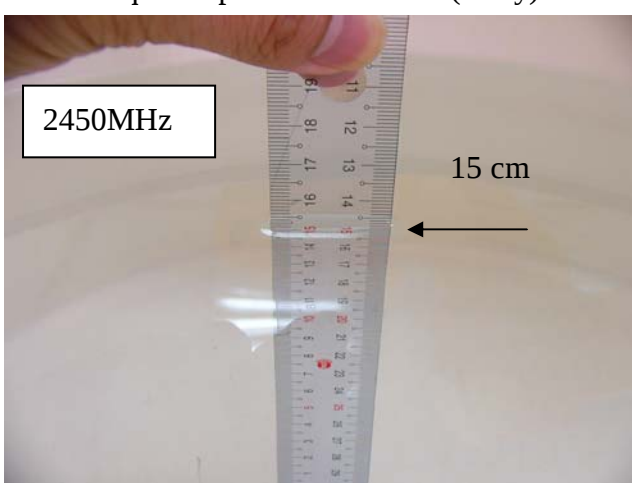


Fig.2.6 Photograph of the Tissue Simulant Fluid liquid depth 15cm for Flat (Body)

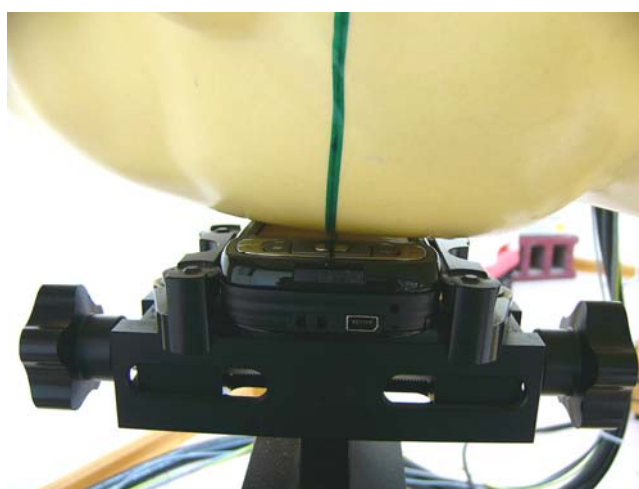
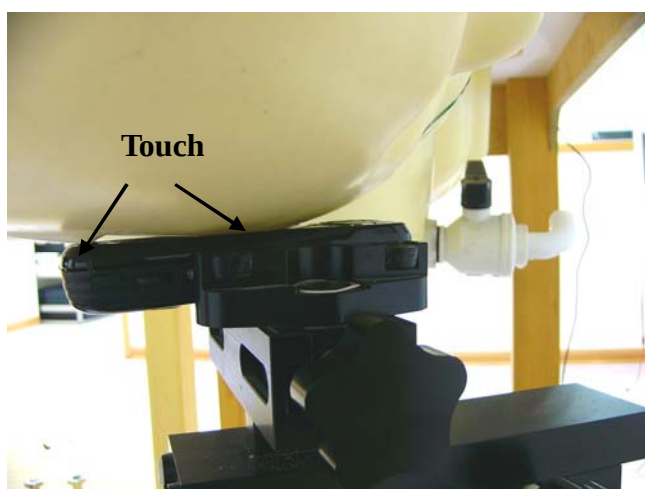


Fig.3 Right Head at Slider-off Section / Cheek-Touch Position

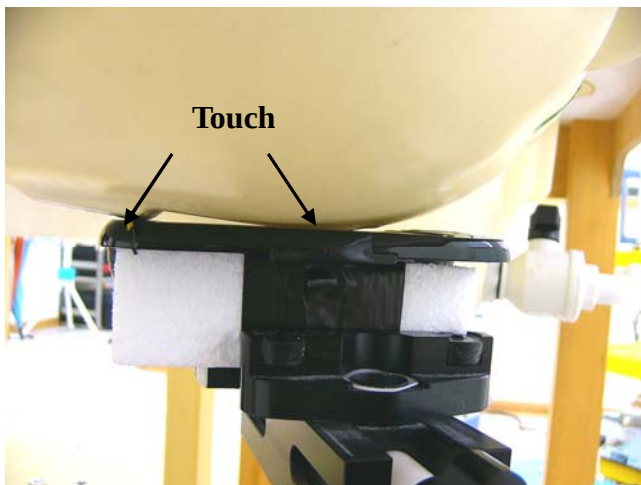


Fig.4 Right Head at Slider-on Section / Cheek-Touch Position

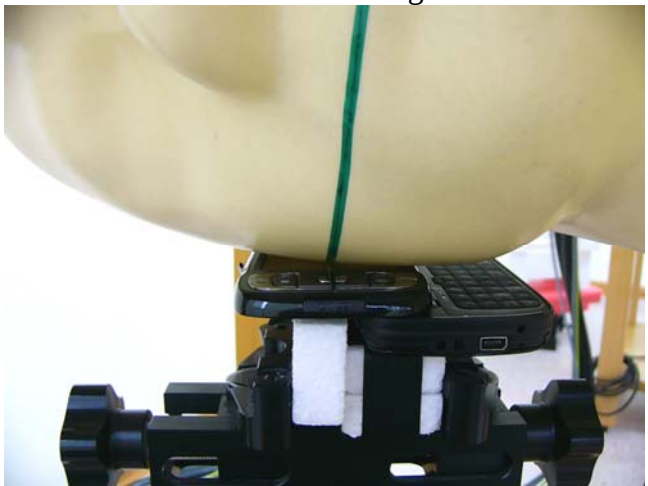


Fig.5 Right Head at Hold up Section / Cheek-Touch Position

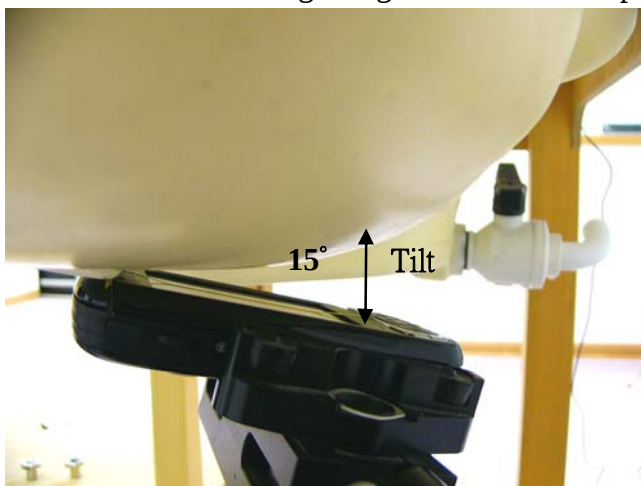
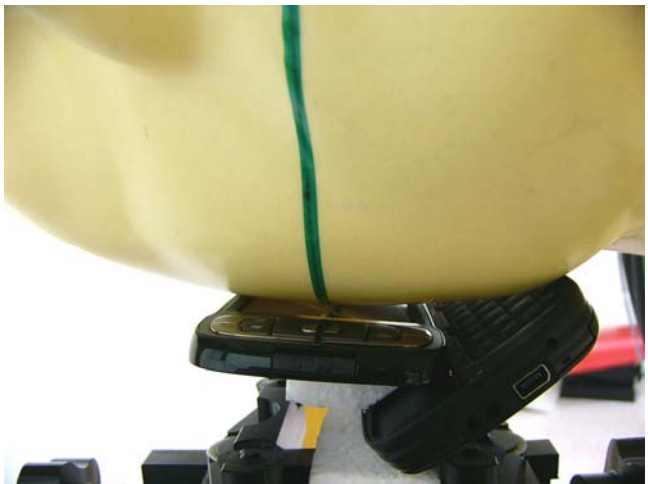


Fig.6 Right Head at Slider-off Section / Ear-Tilt Position(15°)



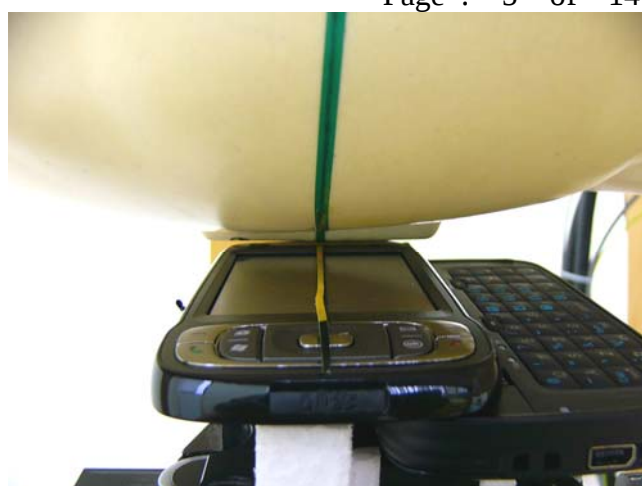
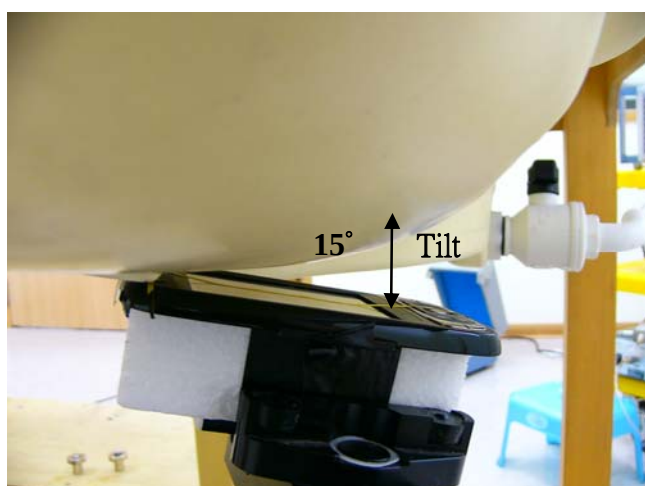


Fig.7 Right Head at Slider-on Section / Ear-Tilt Position(15°)

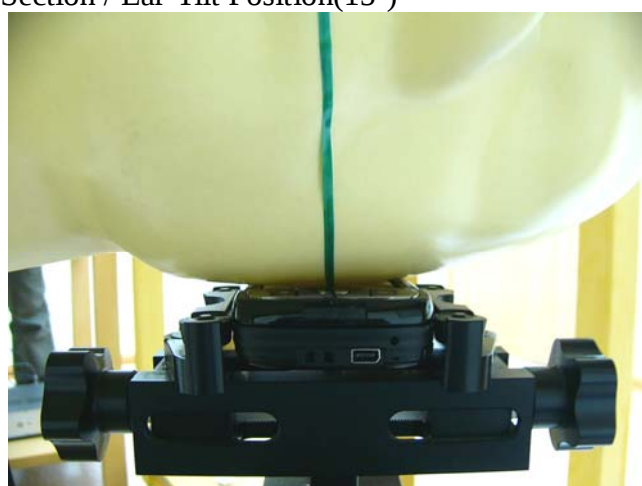
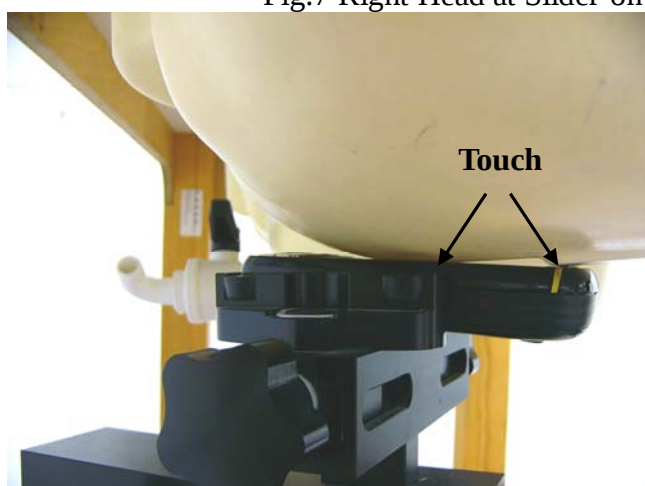


Fig.8 Left Head at Slider-off Section / Cheek-Touch Position

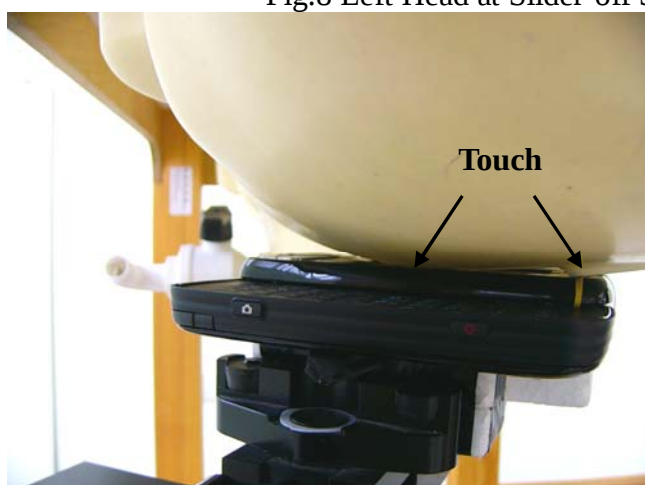


Fig.9 Left Head at Slider-on Section / Cheek-Touch Position



Fig.10 Left Head at Hold up Section / Cheek-Touch Position

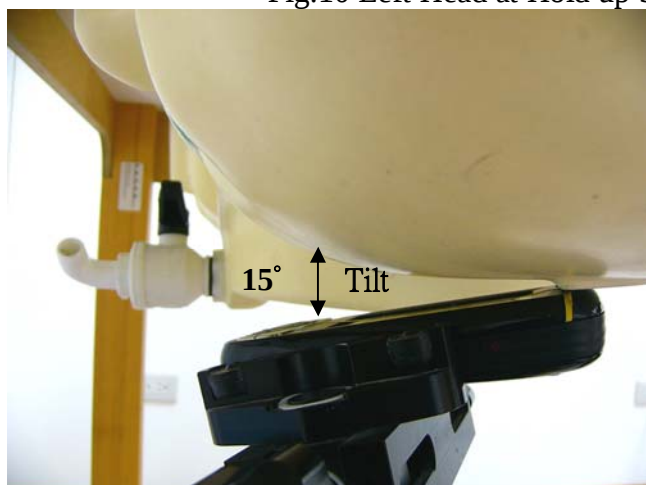
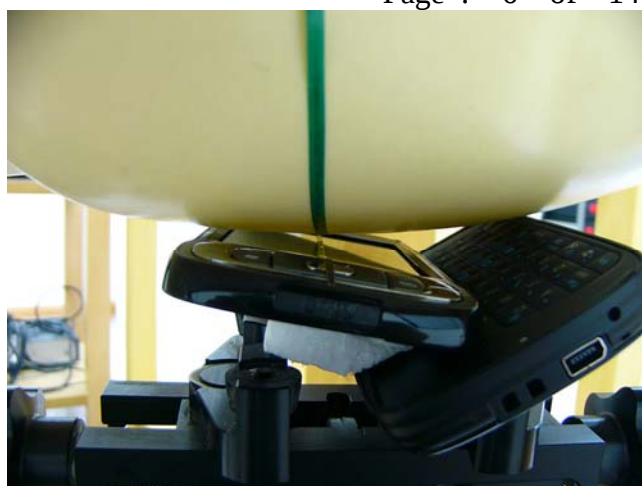


Fig.11 Left Head at Slider-off Section / Ear-Tilt Position(15°)

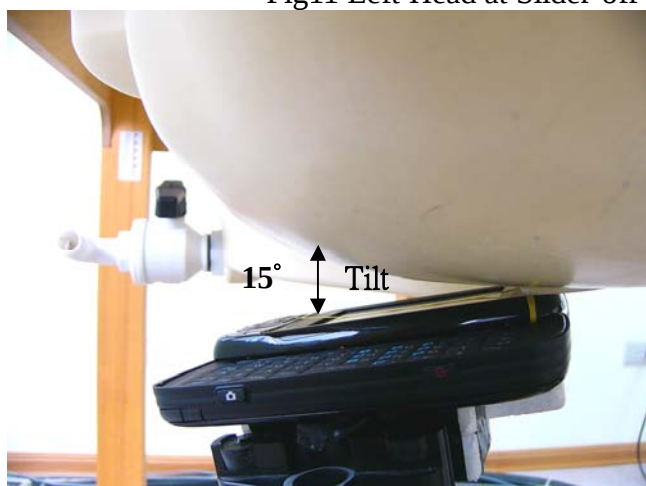
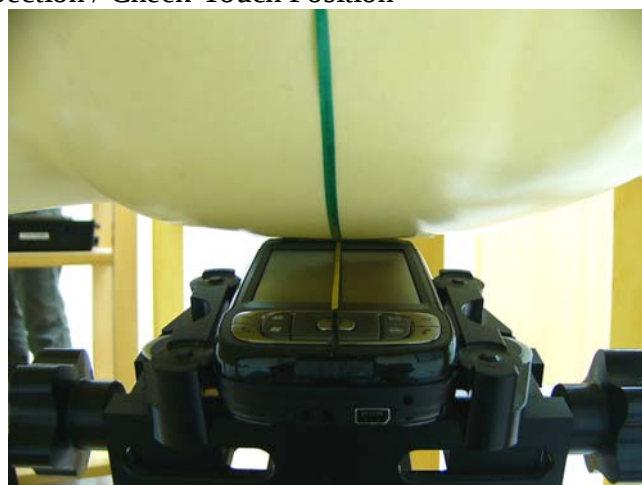


Fig.12 Left Head at Slider-on Section / Ear-Tilt Position(15°)

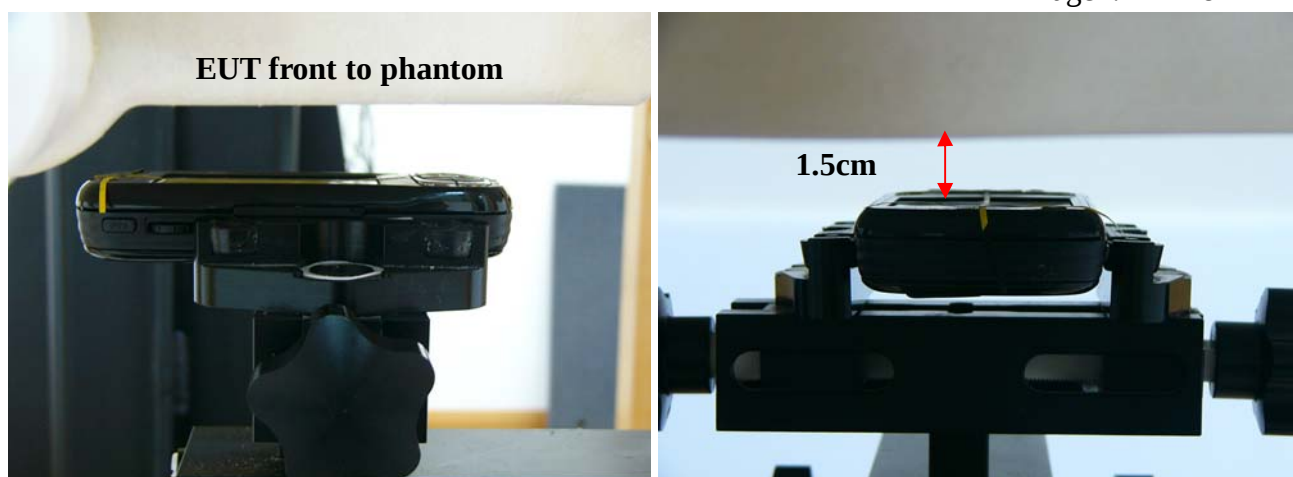


Fig.13 Body worn- EUT front to flat phantom and distance between flat phantom and mobile phone is 1.5 cm

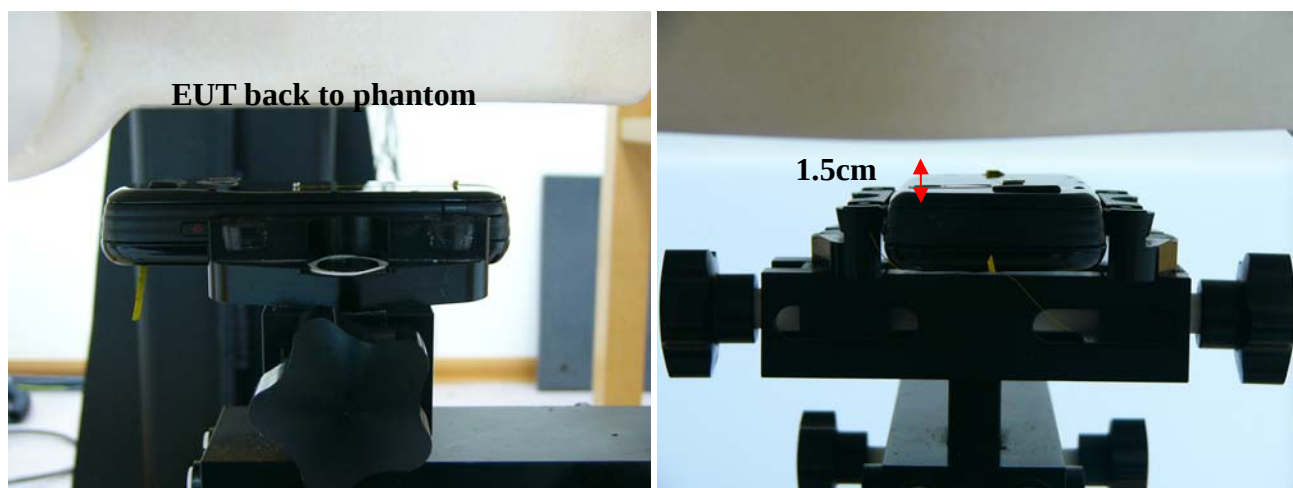


Fig.14 Body worn- EUT back to flat phantom and distance between flat phantom and mobile phone is 1.5 cm