
SAR VALIDATION PLOTS

DIGITAL EMC CO., LTD

DUT: Dipole 835 MHz; Type: D835V2; Serial: D835V2 - SN:464

Communication System: CW; Frequency: 835 MHz; Duty Cycle: 1:1

Medium parameters used: $f = 835 \text{ MHz}$; $\sigma = 0.875 \text{ mho/m}$; $\epsilon_r = 40.1$; $\rho = 1000 \text{ kg/m}^3$

Phantom section: Flat Section

DASY4 Configuration:

Probe: ET3DV6 - SN1703; ConvF(6.51, 6.51, 6.51); Calibrated: 2005-03-24; Electronics: DAE3 Sn520

Phantom: SAM with 835MHz; Type: SAM; Serial: TP-1223

Measurement SW: DASY4, V4.5 Build 19; Postprocessing SW: SEMCAD, V1.8 Build 145

Test Date: 2005-10-11; Ambient Temp: 23.0; Tissue Temp: 22.0

Dipole Validation


Area Scan (51x101x1): Measurement grid: $dx=15\text{mm}$, $dy=15\text{mm}$

Zoom Scan (7x7x7)/Cube 0: Measurement grid: $dx=5\text{mm}$, $dy=5\text{mm}$, $dz=5\text{mm}$

Power Drift = -0.027 dB

Peak SAR (extrapolated) = 3.66 W/kg

SAR(1 g) = 2.42 mW/g; SAR(10 g) = 1.58 mW/g

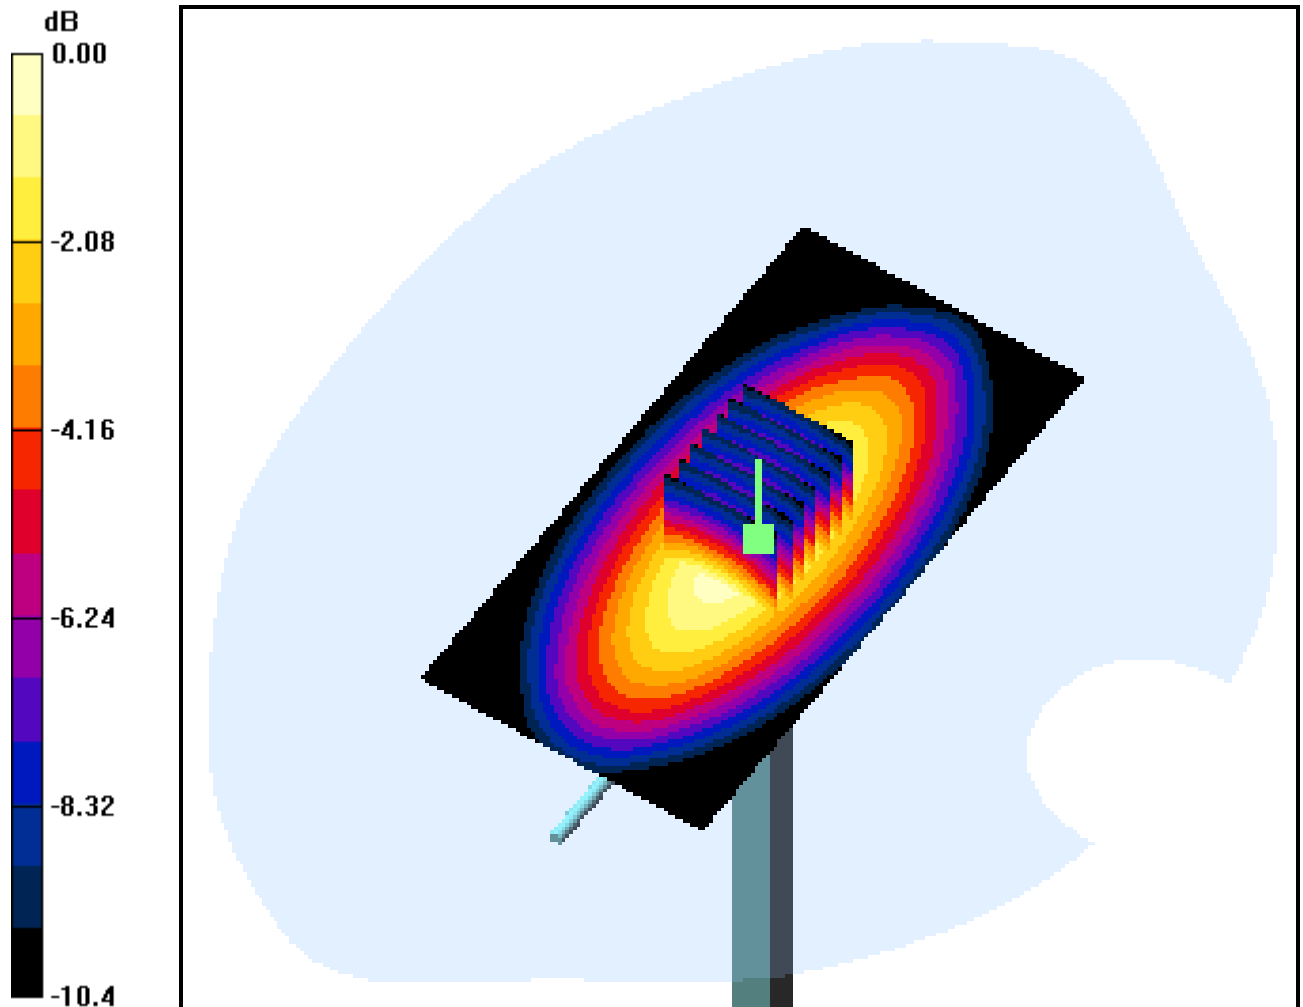

0 dB = 2.61mW/g

DIGITAL EMC CO., LTD

DUT: Dipole 1900 MHz; Type: D1900V2; Serial: D1900V2 - SN:5d029

Communication System: CW; Frequency: 1900 MHz; Duty Cycle: 1:1

Medium parameters used: $f = 1900 \text{ MHz}$; $\sigma = 1.43 \text{ mho/m}$; $\epsilon_r = 38.9$; $\rho = 1000 \text{ kg/m}^3$

Phantom section: Flat Section

DASY4 Configuration:

Probe: ET3DV6 - SN1703; ConvF(5.27, 5.27, 5.27); Calibrated: 2005-03-24; Electronics: DAE3 Sn520

Phantom: SAM 1800/1900 MHz; Type: SAM; Serial: TP-1224

Measurement SW: DASY4, V4.5 Build 19; Postprocessing SW: SEMCAD, V1.8 Build 145

Test Date: 2005-10-12; Ambient Temp: 23.0; Tissue Temp: 21.3

Dipole Validation


Area Scan (51x71x1): Measurement grid: $dx=15\text{mm}$, $dy=15\text{mm}$

Zoom Scan (7x7x7)/Cube 0: Measurement grid: $dx=5\text{mm}$, $dy=5\text{mm}$, $dz=5\text{mm}$

Power Drift = -0.080 dB

Peak SAR (extrapolated) = 17.8 W/kg

SAR(1 g) = 10.3 mW/g; SAR(10 g) = 5.48 mW/g

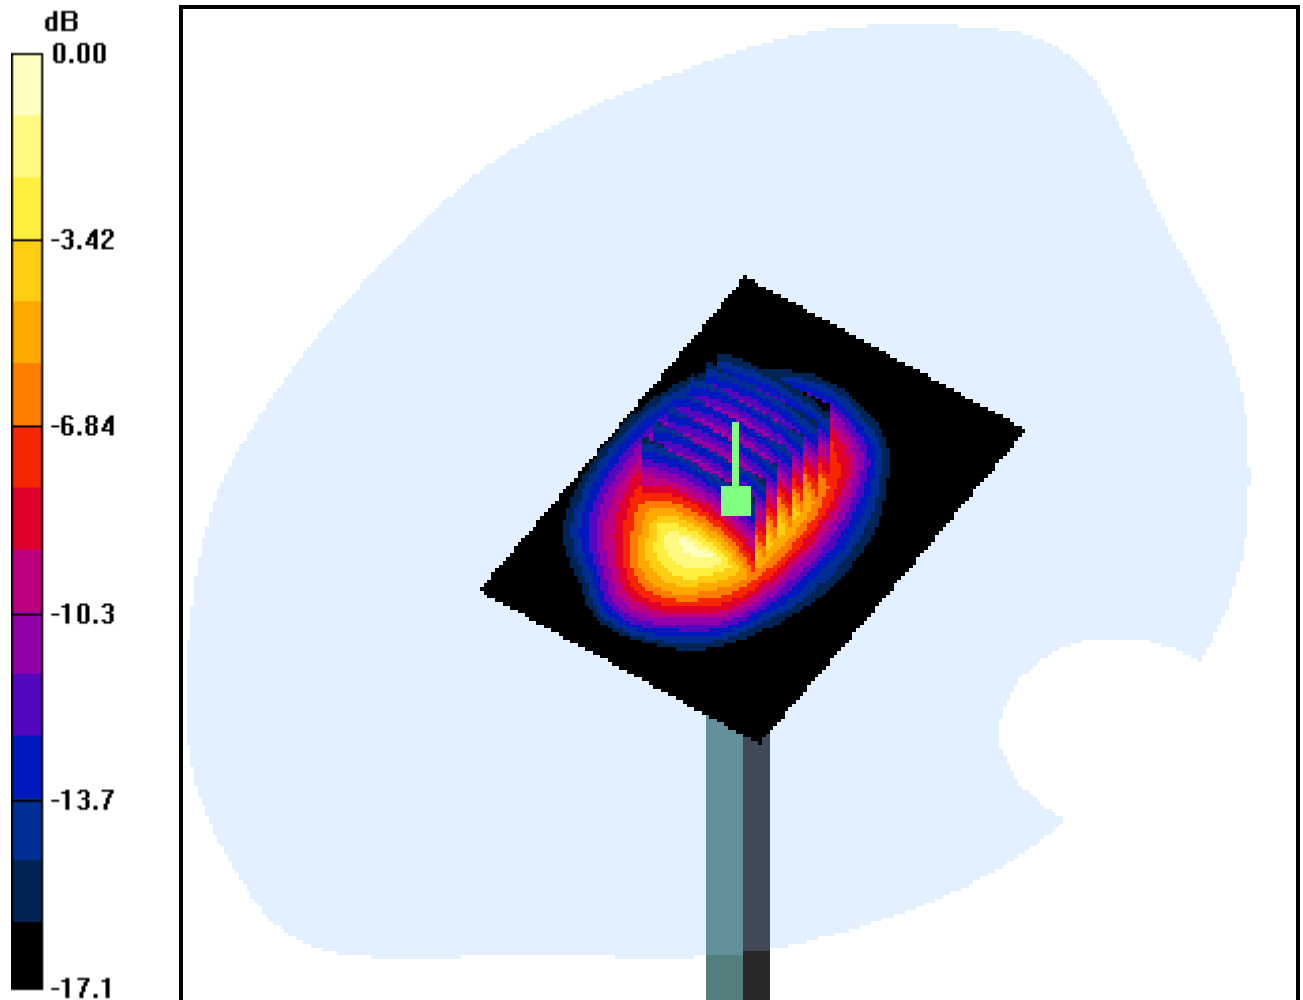

0 dB = 11.5mW/g