

Date: 2025-03-10

System Check_Head_835MHz

DUT: D835V2 - SN4d162

Communication System: CW; Frequency: 835.000 MHz; Duty Cycle: 1:1

Medium: Head Simulating Liquid Medium parameters used: $f = 835.000$ MHz; $\sigma = 0.938$ S/m; $\epsilon_r = 42.4$

Ambient Temperature: 23.2°C; Liquid Temperature: 22.8°C

DASY8 Configuration:

- Probe: EX3DV4 - SN7764; ConvF(9.47, 9.3, 9.4); Calibrated: 2024-09-02
- Sensor-Surface: 1.4 mm
- Electronics: DAE4 Sn1691; Calibrated: 2024-04-19
- Phantom: ELI V8.0 (20deg probe tilt); Serial: 2151
- Measurement Software: 16.4.0.5005
- UID: CW, 0--

Area Scan (40.0 mm x 90.0 mm): Measurement Grid: 10.0 mm x 15.0 mm

SAR (1g) = 0.465 W/kg; SAR (10g) = 0.308 W/kg;


Zoom Scan (32.0 mm x 32.0 mm x 30.0 mm): Measurement Grid: 6.0 mm x 6.0 mm x 1.5 mm

Power Drift = -0.02 dB

SAR (1g) = 0.469 W/kg; SAR (10g) = 0.308 W/kg

Smallest distance from peaks to all points 3 dB below = 17.5 mm

Ratio of SAR at M2 to SAR at M1 = 87.9 %

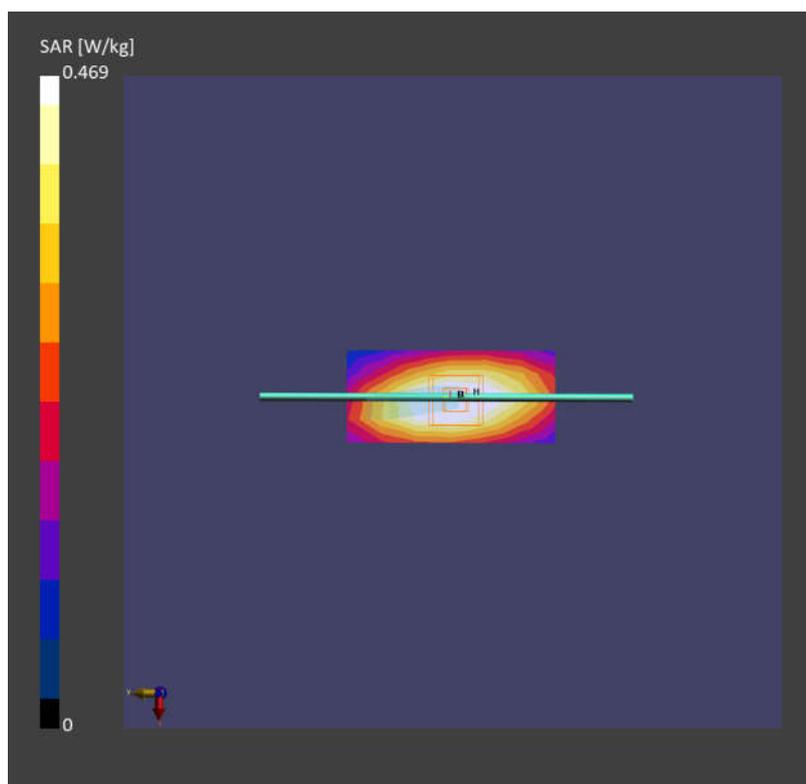

Date: 2025-03-10

System Check_Head_2600MHz**DUT: D2600V2 - SN1112**

Communication System: CW; Frequency: 2600.000 MHz; Duty Cycle: 1:1

Medium: Head Simulating Liquid Medium parameters used: $f = 2600.000$ MHz; $\sigma = 2.01$ S/m; $\epsilon_r = 40.6$

Ambient Temperature: 23.3°C; Liquid Temperature: 22.6°C

DASY8 Configuration:

- Probe: EX3DV4 - SN7764; ConvF(7.96, 7.81, 7.89); Calibrated: 2024-09-02
- Sensor-Surface: 1.4 mm
- Electronics: DAE4 Sn1691; Calibrated: 2024-04-19
- Phantom: ELI V8.0 (20deg probe tilt); Serial: 2151
- Measurement Software: 16.4.0.5005
- UID: CW, 0--

Area Scan (40.0 mm x 80.0 mm): Measurement Grid: 10.0 mm x 10.0 mm

SAR (1g) = 2.70 W/kg; SAR (10g) = 1.24 W/kg;


Zoom Scan (30.0 mm x 30.0 mm x 30.0 mm): Measurement Grid: 5.0 mm x 5.0 mm x 1.5 mm

Power Drift = 0.03 dB

SAR (1g) = 2.79 W/kg; SAR (10g) = 1.27 W/kg

Smallest distance from peaks to all points 3 dB below = 9.0 mm

Ratio of SAR at M2 to SAR at M1 = 80.3 %

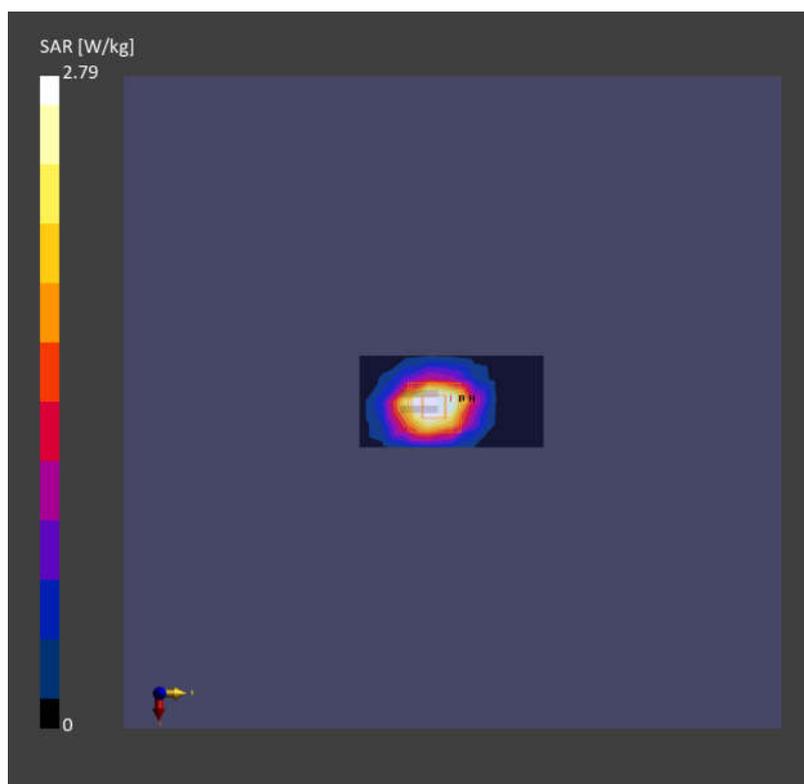

Date: 2025-03-11

System Check_Head_3500MHz**DUT: D3500V2 - SN1037**

Communication System: CW; Frequency: 3500.000 MHz; Duty Cycle: 1:1

Medium: Head Simulating Liquid Medium parameters used: $f = 3500.000$ MHz; $\sigma = 2.83$ S/m; $\epsilon_r = 39.1$

Ambient Temperature: 23.3°C; Liquid Temperature: 22.8°C

DASY8 Configuration:

- Probe: EX3DV4 - SN7764; ConvF(7.13, 7.0, 7.07); Calibrated: 2024-09-02
- Sensor-Surface: 1.4 mm
- Electronics: DAE4 Sn1691; Calibrated: 2024-04-19
- Phantom: ELI V8.0 (20deg probe tilt); Serial: 2151
- Measurement Software: 16.4.0.5005
- UID: CW, 0--

Area Scan (40.0 mm x 80.0 mm): Measurement Grid: 10.0 mm x 10.0 mm

SAR (1g) = 3.40 W/kg; SAR (10g) = 1.32 W/kg;


Zoom Scan (24.0 mm x 24.0 mm x 22.0 mm): Measurement Grid: 4.0 mm x 4.0 mm x 1.4 mm

Power Drift = 0.02 dB

SAR (1g) = 3.43 W/kg; SAR (10g) = 1.33 W/kg

Smallest distance from peaks to all points 3 dB below = 9.0 mm

Ratio of SAR at M2 to SAR at M1 = 77.5 %

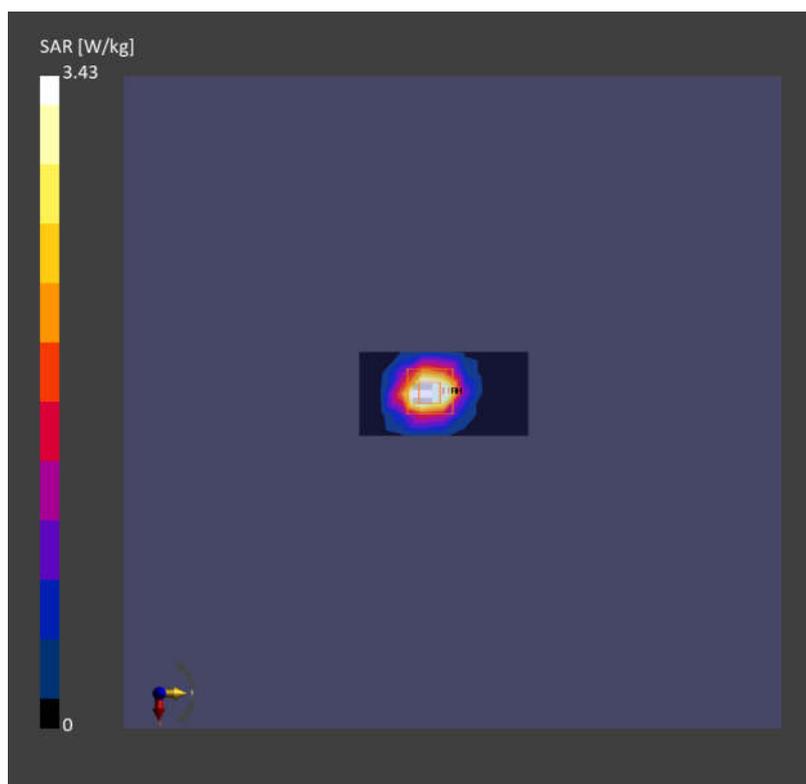

Date: 2025-03-11

System Check_Head_3900MHz**DUT: D3900V2 - SN1048**

Communication System: CW; Frequency: 3900.000 MHz; Duty Cycle: 1:1

Medium: Head Simulating Liquid Medium parameters used: $f = 3900.000$ MHz; $\sigma = 3.23$ S/m; $\epsilon_r = 38.4$

Ambient Temperature: 23.3°C; Liquid Temperature: 22.7°C

DASY8 Configuration:

- Probe: EX3DV4 - SN7764; ConvF(6.97, 6.83, 6.91); Calibrated: 2024-09-02
- Sensor-Surface: 1.4 mm
- Electronics: DAE4 Sn1691; Calibrated: 2024-04-19
- Phantom: ELI V8.0 (20deg probe tilt); Serial: 2151
- Measurement Software: 16.4.0.5005
- UID: CW, 0--

Area Scan (40.0 mm x 80.0 mm): Measurement Grid: 10.0 mm x 10.0 mm

SAR (1g) = 3.45 W/kg; SAR (10g) = 1.31 W/kg;


Zoom Scan (24.0 mm x 24.0 mm x 22.0 mm): Measurement Grid: 4.0 mm x 4.0 mm x 1.4 mm

Power Drift = 0.02 dB

SAR (1g) = 3.45 W/kg; SAR (10g) = 1.29 W/kg

Smallest distance from peaks to all points 3 dB below = 9.0 mm

Ratio of SAR at M2 to SAR at M1 = 77.2 %

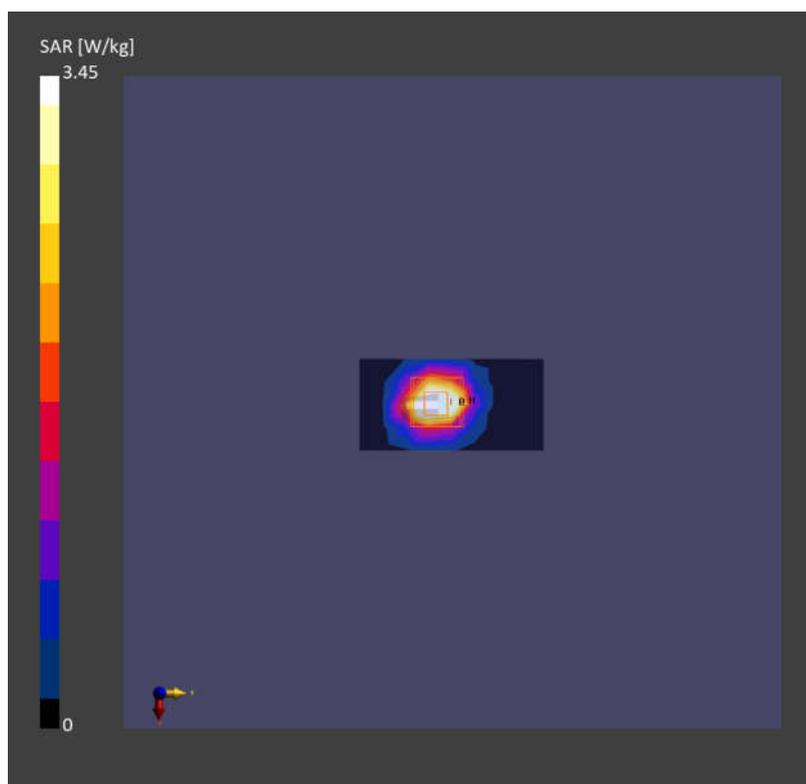

Date: 2025-03-12

System Check_Head_2450MHz**DUT: D2450V2 - SN1095**

Communication System: CW; Frequency: 2450.000 MHz; Duty Cycle: 1:1

Medium: Head Simulating Liquid Medium parameters used: $f = 2450.000$ MHz; $\sigma = 1.84$ S/m; $\epsilon_r = 39.2$

Ambient Temperature: 23.2°C; Liquid Temperature: 22.9°C

DASY8 Configuration:

- Probe: EX3DV4 - SN7764; ConvF(7.87, 7.72, 7.8); Calibrated: 2024-09-02
- Sensor-Surface: 1.4 mm
- Electronics: DAE4 Sn1691; Calibrated: 2024-04-19
- Phantom: ELI V8.0 (20deg probe tilt); Serial: 2151
- Measurement Software: 16.4.0.5005
- UID: CW, 0--

Area Scan (40.0 mm x 80.0 mm): Measurement Grid: 10.0 mm x 10.0 mm

SAR (1g) = 2.66 W/kg; SAR (10g) = 1.26 W/kg;


Zoom Scan (30.0 mm x 30.0 mm x 30.0 mm): Measurement Grid: 5.0 mm x 5.0 mm x 1.5 mm

Power Drift = -0.02 dB

SAR (1g) = 2.67 W/kg; SAR (10g) = 1.27 W/kg

Smallest distance from peaks to all points 3 dB below = 9.0 mm

Ratio of SAR at M2 to SAR at M1 = 82.0 %

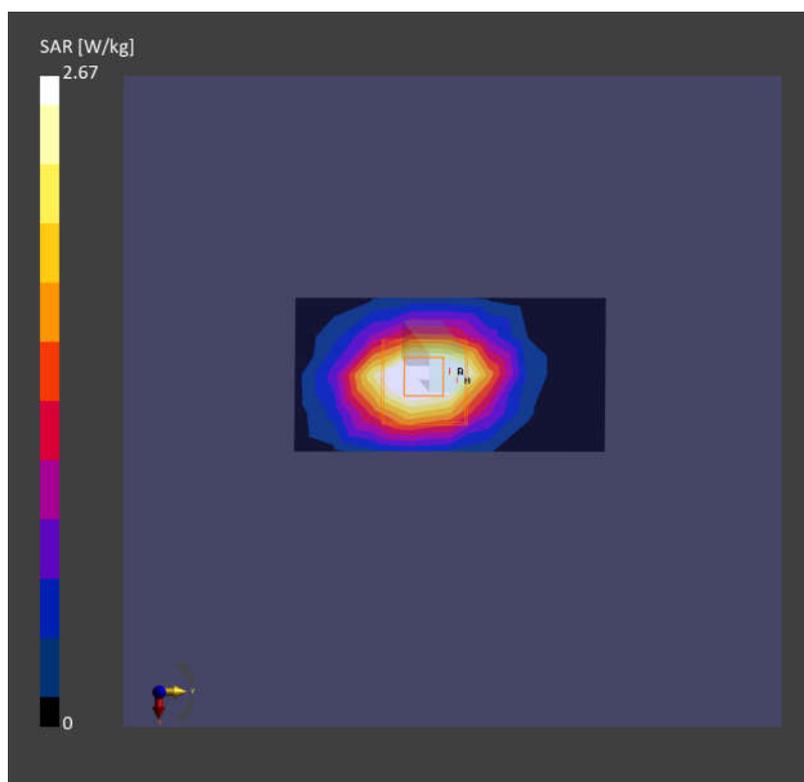

Date: 2025-03-12

System Check_Head_5250MHz**DUT: D5GHzV2 - SN1113**

Communication System: CW; Frequency: 5250.000 MHz; Duty Cycle: 1:1

Medium: Head Simulating Liquid Medium parameters used: $f = 5250.000$ MHz; $\sigma = 4.64$ S/m; $\epsilon_r = 36.5$

Ambient Temperature: 23.1°C; Liquid Temperature: 22.7°C

DASY8 Configuration:

- Probe: EX3DV4 - SN7764; ConvF(5.98, 5.87, 5.93); Calibrated: 2024-09-02
- Sensor-Surface: 1.4 mm
- Electronics: DAE4 Sn1691; Calibrated: 2024-04-19
- Phantom: ELI V8.0 (20deg probe tilt); Serial: 2151
- Measurement Software: 16.4.0.5005
- UID: CW, 0--

Area Scan (40.0 mm x 80.0 mm): Measurement Grid: 10.0 mm x 10.0 mm

SAR (1g) = 3.69 W/kg; SAR (10g) = 1.13 W/kg;


Zoom Scan (24.0 mm x 24.0 mm x 22.0 mm): Measurement Grid: 4.0 mm x 4.0 mm x 1.4 mm

Power Drift = -0.04 dB

SAR (1g) = 4.10 W/kg; SAR (10g) = 1.21 W/kg

Smallest distance from peaks to all points 3 dB below = 7.4 mm

Ratio of SAR at M2 to SAR at M1 = 64.3 %

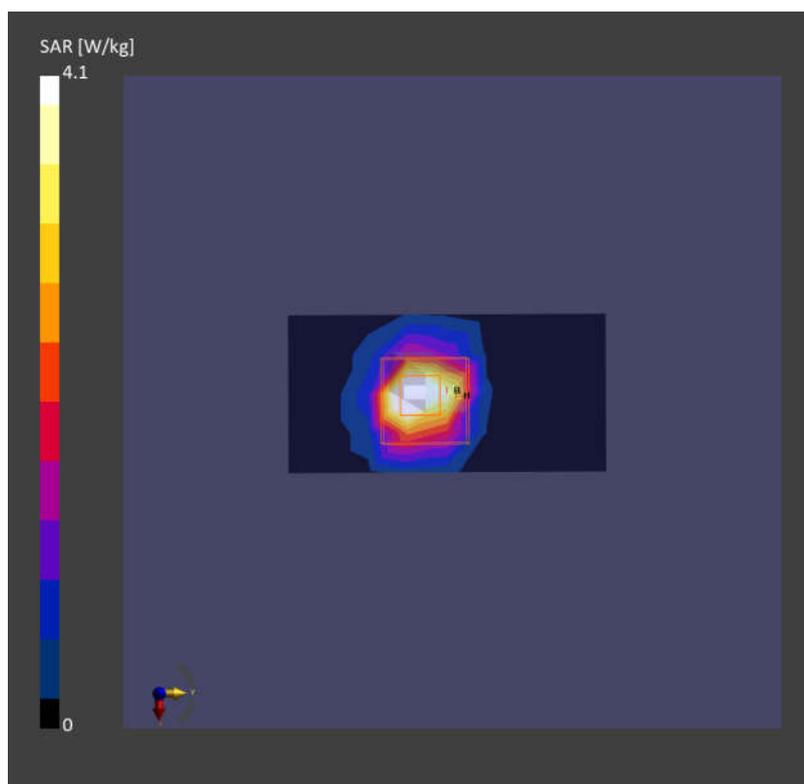

Date: 2025-03-12

System Check_Head_5600MHz**DUT: D5GHzV2 - SN1113**

Communication System: CW; Frequency: 5600.000 MHz; Duty Cycle: 1:1

Medium: Head Simulating Liquid Medium parameters used: $f = 5600.000$ MHz; $\sigma = 4.99$ S/m; $\epsilon_r = 35.9$

Ambient Temperature: 23.2°C; Liquid Temperature: 22.6°C

DASY8 Configuration:

- Probe: EX3DV4 - SN7764; ConvF(5.36, 5.26, 5.32); Calibrated: 2024-09-02
- Sensor-Surface: 1.4 mm
- Electronics: DAE4 Sn1691; Calibrated: 2024-04-19
- Phantom: ELI V8.0 (20deg probe tilt); Serial: 2151
- Measurement Software: 16.4.0.5005
- UID: CW, 0--

Area Scan (40.0 mm x 80.0 mm): Measurement Grid: 10.0 mm x 10.0 mm

SAR (1g) = 3.88 W/kg; SAR (10g) = 1.17 W/kg;


Zoom Scan (24.0 mm x 24.0 mm x 22.0 mm): Measurement Grid: 4.0 mm x 4.0 mm x 1.4 mm

Power Drift = 0.05 dB

SAR (1g) = 4.42 W/kg; SAR (10g) = 1.27 W/kg

Smallest distance from peaks to all points 3 dB below = 7.2 mm

Ratio of SAR at M2 to SAR at M1 = 60.0 %

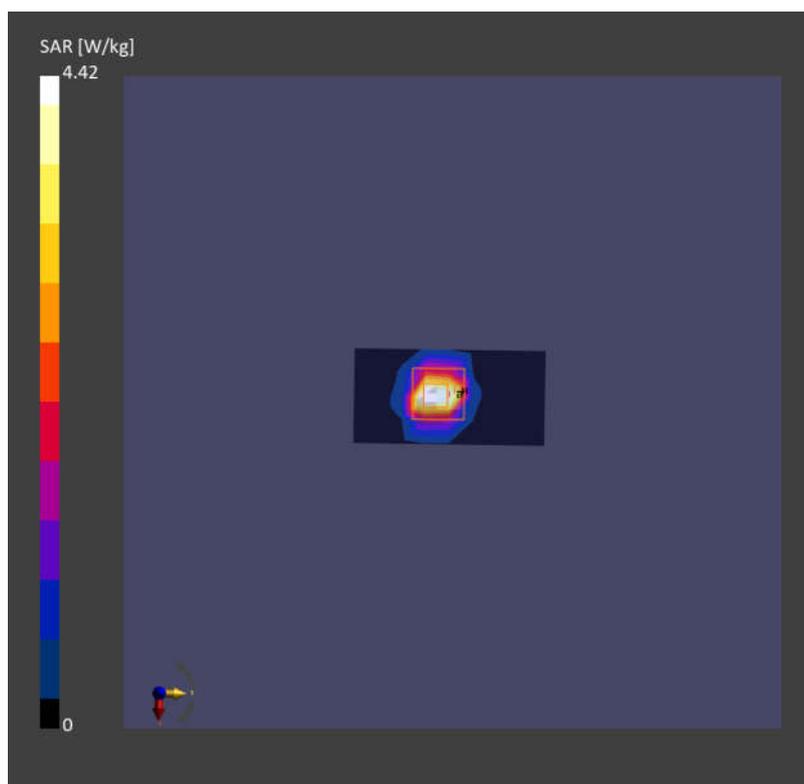

Date: 2025-03-12

System Check_Head_5750MHz**DUT: D5GHzV2 - SN1113**

Communication System: CW; Frequency: 5750.000 MHz; Duty Cycle: 1:1

Medium: Head Simulating Liquid Medium parameters used: $f = 5750.000$ MHz; $\sigma = 5.22$ S/m; $\epsilon_r = 35.6$

Ambient Temperature: 23.4°C; Liquid Temperature: 22.7°C

DASY8 Configuration:

- Probe: EX3DV4 - SN7764; ConvF(5.44, 5.34, 5.4); Calibrated: 2024-09-02
- Sensor-Surface: 1.4 mm
- Electronics: DAE4 Sn1691; Calibrated: 2024-04-19
- Phantom: ELI V8.0 (20deg probe tilt); Serial: 2151
- Measurement Software: 16.4.0.5005
- UID: CW, 0--

Area Scan (40.0 mm x 80.0 mm): Measurement Grid: 10.0 mm x 10.0 mm

SAR (1g) = 3.74 W/kg; SAR (10g) = 1.13 W/kg;

Zoom Scan (24.0 mm x 24.0 mm x 22.0 mm): Measurement Grid: 4.0 mm x 4.0 mm x 1.4 mm

Power Drift = 0.01 dB

SAR (1g) = 4.23 W/kg; SAR (10g) = 1.23 W/kg

Smallest distance from peaks to all points 3 dB below = 7.6 mm

Ratio of SAR at M2 to SAR at M1 = 59.5 %

