

System Check_Head_2450MHz

DUT:D2450V2 - SN:1095

Communication System: ; Frequency: 2450.000

Medium: HSL. Medium parameters used: $f = 2450.000$ MHz; $\sigma = 1.74$ S/m; $\epsilon_r = 39.3$

Ambient Temperature: 23.4°C; Liquid Temperature: 22.8°C

DASY6 Configuration:

- Probe: EX3DV4 - SN7706; ConvF(7.47, 8.61, 7.55); Calibrated: 2024-01-24
- Sensor-Surface: 1.4 mm
- Electronics: DAE4 Sn1691; Calibrated: 2024-04-19
- Phantom: ELI V8.0 (20deg probe tilt); Serial: 2134
- Measurement Software: cDASY6 V6.6.0.13926

Area Scan (40.0 mm x 90.0 mm): Measurement Grid: 10.0 mm x 10.0 mm


SAR (1g) = 2.47 W/kg; SAR (10g) = 1.18 W/kg;

Zoom Scan (30.0 mm x 30.0 mm x 30.0 mm): Measurement Grid: 5.0 mm x 5.0 mm x 1.5 mm

Power Drift = 0.07 dB

SAR (1g) = 2.66 W/kg; SAR (10g) = 1.27 W/kg;

Smallest distance from peaks to all points 3dB below is 7.7 mm Ratio of SAR at M2 to SAR at M1 = 73.5 %

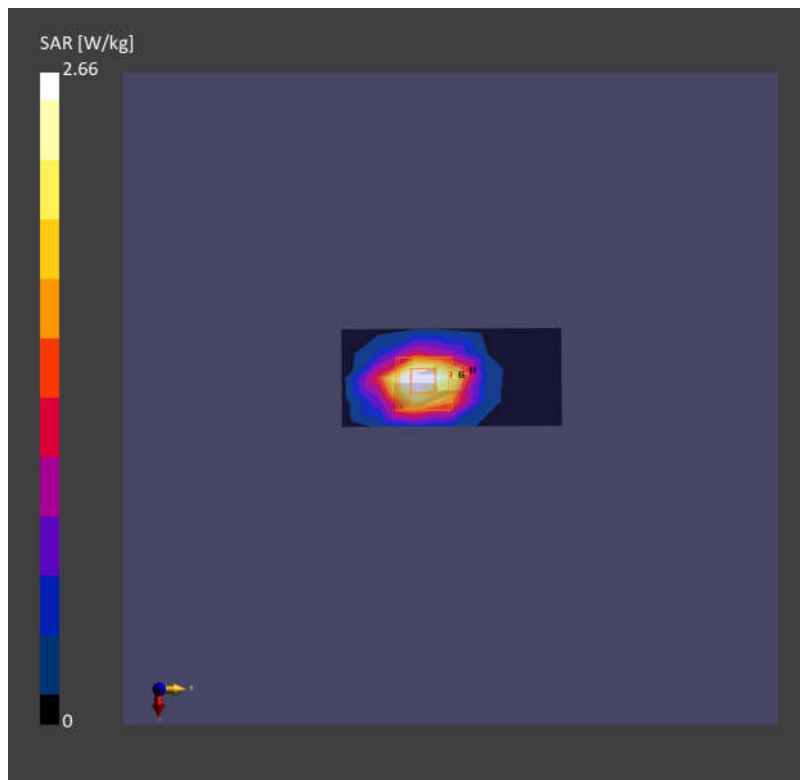

System Check_Head_5250MHz

DUT:D5GHzV2 - SN:1113

Communication System: ; Frequency: 5250.000

Medium: HSL. Medium parameters used: $f = 5250.000$ MHz; $\sigma = 4.57$ S/m; $\epsilon_r = 35.7$

Ambient Temperature: 23.3°C; Liquid Temperature: 22.7°C

DASY6 Configuration:

- Probe: EX3DV4 - SN7706; ConvF(5.84, 6.82, 5.88); Calibrated: 2024-01-24
- Sensor-Surface: 1.4 mm
- Electronics: DAE4 Sn1691; Calibrated: 2024-04-19
- Phantom: ELI V8.0 (20deg probe tilt); Serial: 2134
- Measurement Software: cDASY6 V6.6.0.13926

Area Scan (40.0 mm x 80.0 mm): Measurement Grid: 10.0 mm x 10.0 mm


SAR (1g) = 3.84 W/kg; SAR (10g) = 1.11 W/kg;

Zoom Scan (22.0 mm x 22.0 mm x 22.0 mm): Measurement Grid: 4.0 mm x 4.0 mm x 1.4 mm

Power Drift = 0.04 dB

SAR (1g) = 4.17 W/kg; SAR (10g) = 1.22 W/kg;

Smallest distance from peaks to all points 3dB below is 6.6 mm Ratio of SAR at M2 to SAR at M1 = 65.6 %

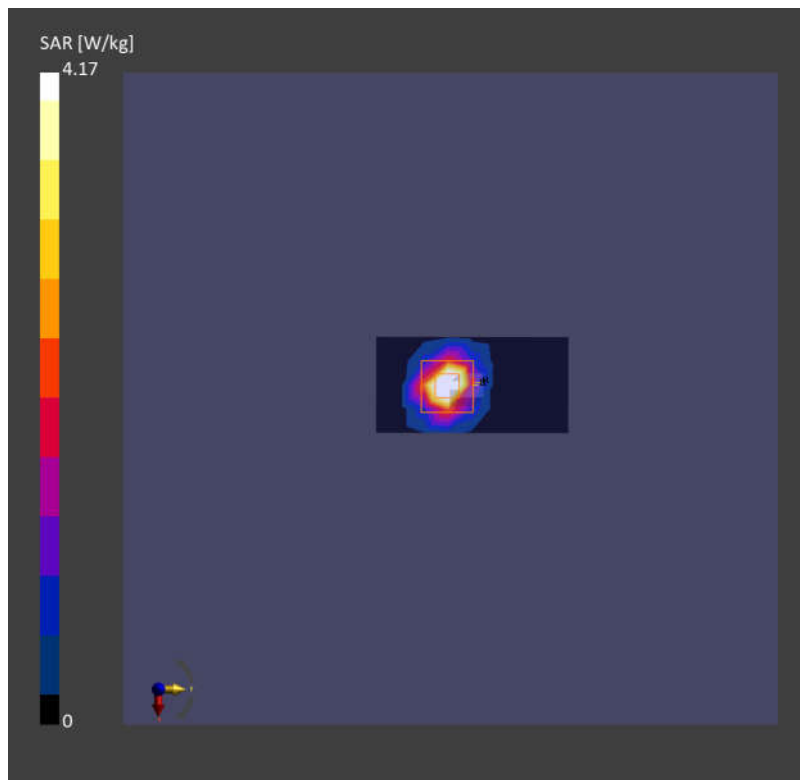

System Check_Head_5600MHz

DUT:D5GHzV2 - SN:1113

Communication System: ; Frequency: 5600.000

Medium: HSL. Medium parameters used: $f = 5600.000$ MHz; $\sigma = 4.95$ S/m; $\epsilon_r = 35.1$

Ambient Temperature: 23.4°C; Liquid Temperature: 22.7°C

DASY6 Configuration:

- Probe: EX3DV4 - SN7706; ConvF(4.83, 5.71, 4.90); Calibrated: 2024-01-24
- Sensor-Surface: 1.4 mm
- Electronics: DAE4 Sn1691; Calibrated: 2024-04-19
- Phantom: ELI V8.0 (20deg probe tilt); Serial: 2134
- Measurement Software: cDASY6 V6.6.0.13926

Area Scan (40.0 mm x 80.0 mm): Measurement Grid: 10.0 mm x 10.0 mm


SAR (1g) = 4.21 W/kg; SAR (10g) = 1.20 W/kg;

Zoom Scan (22.0 mm x 22.0 mm x 22.0 mm): Measurement Grid: 4.0 mm x 4.0 mm x 1.4 mm

Power Drift = -0.06 dB

SAR (1g) = 4.45 W/kg; SAR (10g) = 1.25 W/kg;

Smallest distance from peaks to all points 3dB below is 6.7 mm Ratio of SAR at M2 to SAR at M1 = 63.2 %

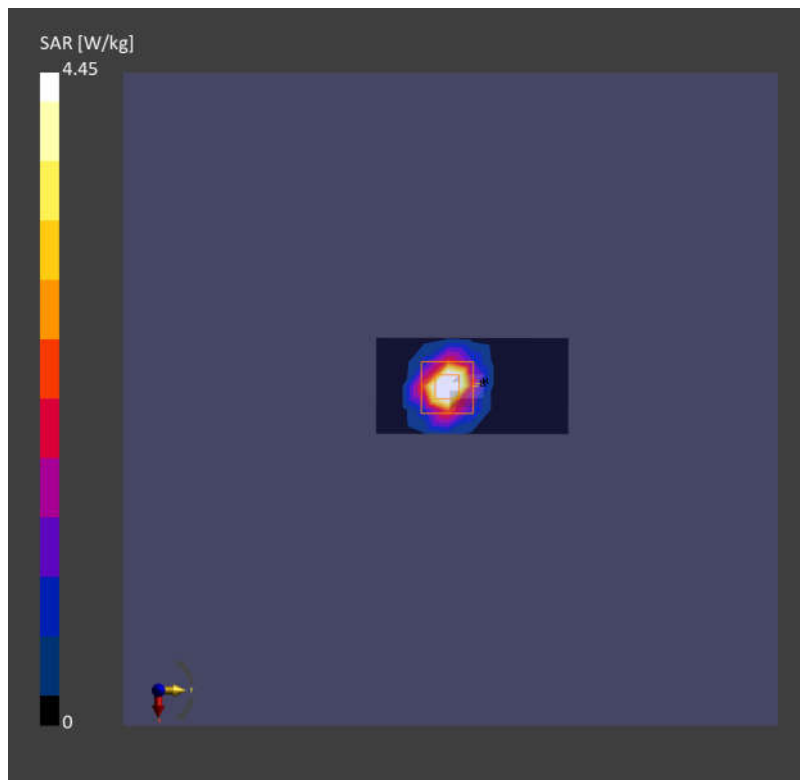

System Check_Head_5750MHz

DUT:D5GHzV2 - SN:1113

Communication System: ; Frequency: 5750.000

Medium: HSL. Medium parameters used: $f = 5750.000$ MHz; $\sigma = 5.11$ S/m; $\epsilon_r = 34.9$

Ambient Temperature: 23.3°C; Liquid Temperature: 22.9°C

DASY6 Configuration:

- Probe: EX3DV4 - SN7706; ConvF(5.03, 5.88, 5.16); Calibrated: 2024-01-24
- Sensor-Surface: 1.4 mm
- Electronics: DAE4 Sn1691; Calibrated: 2024-04-19
- Phantom: ELI V8.0 (20deg probe tilt); Serial: 2134
- Measurement Software: cDASY6 V6.6.0.13926

Area Scan (40.0 mm x 80.0 mm): Measurement Grid: 10.0 mm x 10.0 mm


SAR (1g) = 3.94 W/kg; SAR (10g) = 1.12 W/kg;

Zoom Scan (22.0 mm x 22.0 mm x 22.0 mm): Measurement Grid: 4.0 mm x 4.0 mm x 1.4 mm

Power Drift = 0.02 dB

SAR (1g) = 4.23 W/kg; SAR (10g) = 1.22 W/kg;

Smallest distance from peaks to all points 3dB below is 6.9 mm Ratio of SAR at M2 to SAR at M1 = 62.5 %

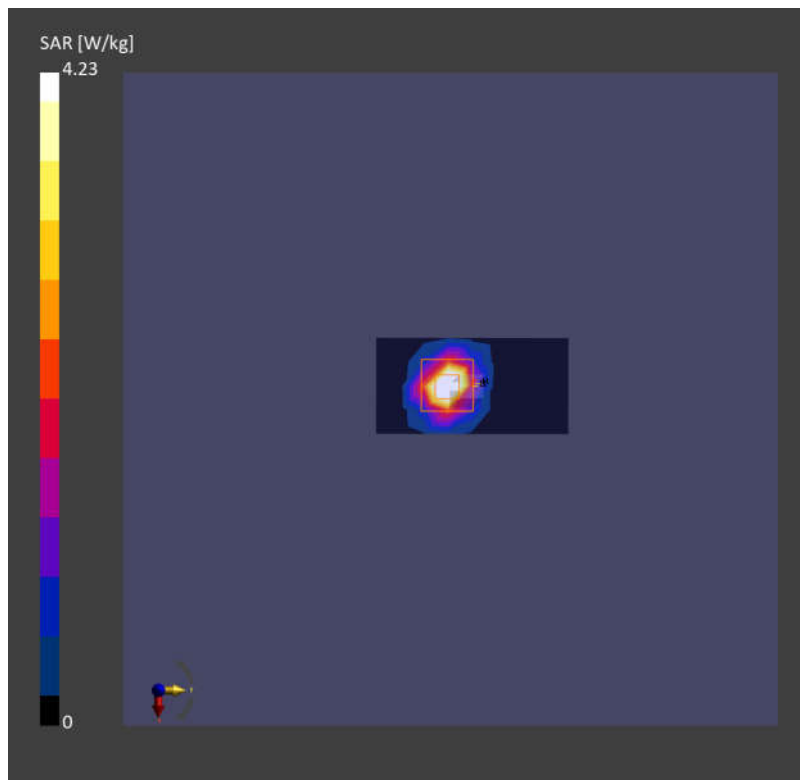

System Check_Head_6500MHz

DUT:D6.5GHzV2 - SN:1031

Communication System: ; Frequency: 6500.0000

Medium: HSL. Medium parameters used: $f = 6500.0000$ MHz; $\sigma = 6.06$ S/m; $\epsilon_r = 34.5$

Ambient Temperature: 23.3°C; Liquid Temperature: 22.8°C

DASY6 Configuration:

- Probe: EX3DV4 - SN7706; ConvF(5.27, 6.32, 5.24); Calibrated: 2024-01-24
- Sensor-Surface: 1.4 mm
- Electronics: DAE4 Sn1691; Calibrated: 2024-04-19
- Phantom: ELI V8.0 (20deg probe tilt); Serial: 2134
- Measurement Software: cDASY6 V6.6.0.13926

Area Scan (51.0 mm x 85.0 mm): Measurement Grid: 8.5 mm x 8.5 mm

SAR (1g) = 14.4 W/kg; SAR (10g) = 2.51 W/kg;


Zoom Scan (22.0 mm x 22.0 mm x 22.0 mm): Measurement Grid: 3.4 mm x 3.4 mm x 1.4 mm;
Graded Ratio: 1.4

Power Drift = 0.05 dB

SAR (1g) = 15.9 W/kg; SAR (10g) = 2.68 W/kg;

Smallest distance from peaks to all points 3dB below is 5.6 mm Ratio of SAR at M2 to SAR at M1 = 58.7 %

psAPD (4.0cm², sq) = 63.4 [W/m²];

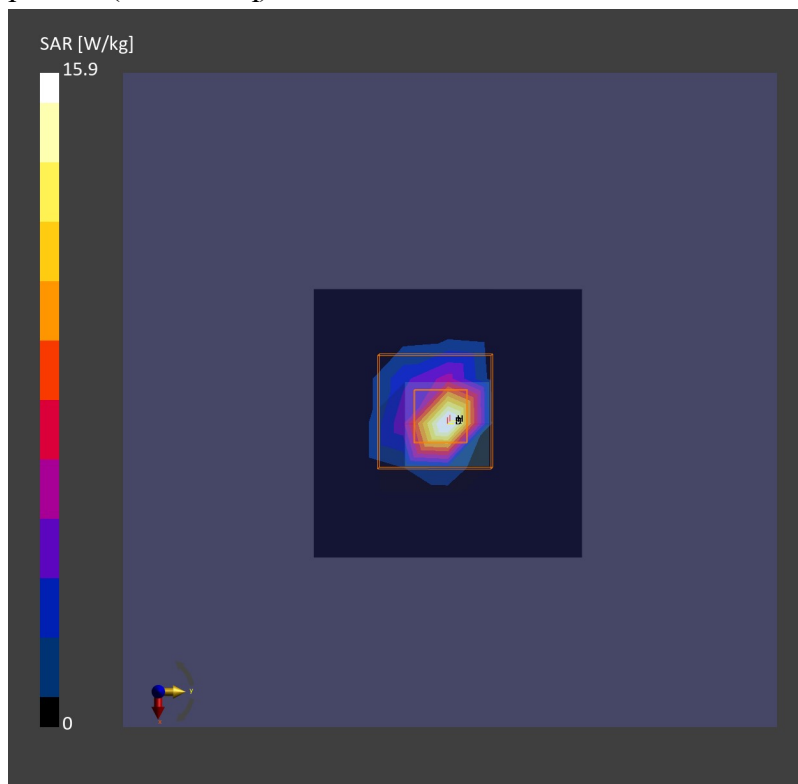

Measurement Report for Device, FRONT, Validation band, CW, Channel 10000 (10000.0 MHz)

Device Under Test Properties

Model, Manufacturer	Dimensions [mm]
Device,	100.0 x 100.0 x 105.0

Exposure Conditions

Phantom Section	Position, Test Distance [mm]	Band	Group, UID	Frequency [MHz], Channel Number	Conversion Factor
5G	FRONT, 10.00	Validation band	CW, 0--	10000.0, 10000	1.0

Hardware Setup

Phantom	Medium	Probe, Calibration Date	DAE, Calibration Date
mmWave – 1065	Air –	EUmmWV4 – SN9553_F1–55GHz, 2023–10–18	DAE4 Sn1303, 2023–11–20

Scans Setup

Scan Type	5G Scan
Grid Extents [mm]	60.0 x 60.0
Grid Steps [lambda]	0.125 x 0.125
Sensor Surface [mm]	10.0
MAIA	N/A

Measurement Results

Scan Type	5G Scan
Date	2024–05–30
Avg. Area [cm ²]	4.00
psPDn+ [W/m ²]	64.2
psPDtot+ [W/m ²]	64.7
psPDmod+ [W/m ²]	66.8
E _{max} [V/m]	183
Power Drift [dB]	–0.01

