

Medtronic MiniMed

ADDENDUM TO TEST REPORT 95094-9A

Carelink USB 2.4
Model: MMT-7306CL

Tested To The Following Standards:

FCC Part 15 Subpart C Sections 15.207 and 15.247

Report No.: 95094-9B

Date of issue: February 10, 2015



This test report bears the accreditation symbol indicating that the testing performed herein meets the test and reporting requirements of ISO/IEC 17025 under the applicable scope of EMC testing for CKC Laboratories, Inc.

We strive to create long-term, trust based relationships by providing sound, adaptive, customer first testing services. We embrace each of our customers' unique EMC challenges, not as an interruption to set processes, but rather as the reason we are in business.

TABLE OF CONTENTS

Administrative Information	3
Test Report Information	3
Revision History	3
Report Authorization	3
Test Facility Information	4
Software Versions	4
Site Registration & Accreditation Information	4
Summary of Results	5
Conditions During Testing	5
Equipment Under Test	6
Peripheral Devices	6
FCC Part 15 Subpart C	7
15.207 AC Conducted Emissions	7
15.247(a)(2) 6dB Occupied Bandwidth	15
15.247(b)(3) Maximum Output Power	19
15.247(d) Radiated Spurious Emissions	23
15.247(e) Power Spectral Density	32
Supplemental Information	36
Measurement Uncertainty	36
Emissions Test Details	36

ADMINISTRATIVE INFORMATION

Test Report Information

REPORT PREPARED FOR:

Medtronic MiniMed
18000 Devonshire Street
Northridge, CA 91325-1219

Representative: Bob Vitti
Customer Reference Number: 4500091834

DATE OF EQUIPMENT RECEIPT:**DATE(S) OF TESTING:****REPORT PREPARED BY:**

Dianne Dudley
CKC Laboratories, Inc.
5046 Sierra Pines Drive
Mariposa, CA 95338

Project Number: 95094

November 4, 2013

November 4-6, 2013

Revision History

Original: Testing of Carelink USB 2.4, Model: MMT-7306CL to FCC Part 15 Subpart C Sections 15.207 and 15.247.

Addendum A: To correct the labels in the Power Output 15.247(b)(3) table by removing the word "bandwidth" in the "Corrections due to bandwidth, cables, amplifiers & antennas (dB)" header and correcting the last column header from "ERP Watts" to "Conducted Power (Watts)".

Addendum B: To correct an error in the value description of LISN, Asset # 01311. The value listed was 5uH and it should have been 50uH.

Report Authorization

The test data contained in this report documents the observed testing parameters pertaining to and are relevant for only the sample equipment tested in the agreed upon operational mode(s) and configuration(s) as identified herein. Compliance assessment remains the client's responsibility. This report may not be used to claim product endorsement by A2LA or any government agencies. This test report has been authorized for release under quality control from CKC Laboratories, Inc.



Steve Behm
Director of Quality Assurance & Engineering Services
CKC Laboratories, Inc.

Test Facility Information



Our laboratories are configured to effectively test a wide variety of product types. CKC utilizes first class test equipment, anechoic chambers, data acquisition and information services to create accurate, repeatable and affordable test results.

TEST LOCATION(S):
CKC Laboratories, Inc.
22116 23rd Drive S.E., Suite A
Bothell, WA 98021-4413

Software Versions

CKC Laboratories Proprietary Software	Version
EMITest Emissions	5.00.14
Immunity	5.00.07

Site Registration & Accreditation Information

Location	CB #	TAIWAN	CANADA	FCC	JAPAN
Brea A	US0060	SL2-IN-E-1146R	3082D-1	90473	A-0147

SUMMARY OF RESULTS

Standard / Specification: FCC Part 15 Subpart C

Description	Test Procedure/Method	Results
Conducted Emissions	FCC Part 15 Subpart C Section 15.207 / ANSI C63.4	Pass
6dB Occupied Bandwidth	FCC Part 15 Subpart C Section 15.247(a)(2) / FHSS – DA00-705 / DTS – KDB 558074/ ANSI C63.4	Pass
Maximum Output Power	FCC Part 15 Subpart C Section 15.247(b)(3) / FHSS – DA00-705 / DTS – KDB 558074 / ANSI C63.4	Pass
Radiated Spurious Emissions / Bandedge	FCC Part 15 Subpart C Section 15.247(d) / FHSS – DA00-705 / DTS – KDB 558074 / ANSI C63.4	Pass
Power Spectral Density	FCC Part 15 Subpart C 15.247(e) / FHSS – DA00-705 / DTS – KDB 558074 / ANSI C63.4	Pass

Conditions During Testing

This list is a summary of the conditions noted for or modifications made to the equipment during testing.

Summary of Conditions
None

EQUIPMENT UNDER TEST (EUT)

EQUIPMENT UNDER TEST

Carelink USB 2.4

Manuf: Medtronic MiniMed
Model: MMT-7306CL
Serial: PC0002898F

PERIPHERAL DEVICES

The EUT was tested with the following peripheral device(s):

Mouse

Manuf: Microsoft
Model: X800898
Serial: NA

Headphones

Manuf: Monster
Model: DNA
Serial: 5W64574YRF

Laptop

Manuf: Dell
Model: Latitude E6320
Serial:

AC/DC Adaptor

Manuf: Dell
Model: DA90PE3-00
Serial: NA

FCC PART 15 SUBPART C

This report contains EMC emissions test results under United States Federal Communications Commission (FCC) 47 CFR 15C requirements for Unlicensed Radio Frequency Devices, Subpart C - Intentional Radiators.

15.207 AC Conducted Emissions

Test Data Sheets

Test Location: CKC Laboratories, Inc. • 22116 23rd Drive SE, Suite A • Bothell, WA 98021 • (425) 402-1717

Customer: **Medtronic MiniMed**
 Specification: **15.207 AC Mains - Quasi-peak**
 Work Order #: **95094**
 Test Type: **Conducted Emissions**
 Equipment: **Carelink USB 2.4**
 Manufacturer: **Medtronic MiniMed**
 Model: **MMT-7306CL**
 S/N: **PC0002898F**

Date: 11/4/2013
 Time: 12:08:08
 Sequence#: 10
 Tested By: Steven Pittsford
 120V 60Hz

Test Equipment:

ID	Asset #	Description	Model	Calibration Date	Cal Due Date
T1	ANP05435	Attenuator	PE7015-10	10/5/2012	10/5/2014
T2	ANP05546	Cable	HeliAx	3/27/2013	3/27/2015
T3	ANP05547	Cable	HeliAx	9/7/2012	9/7/2014
T4	AN01311	50uH LISN-Line	3816/2	12/9/2011	12/9/2013
	AN01311	50uH LISN-Neutral	3816/2	12/9/2011	12/9/2013
T5	AN02871	Spectrum Analyzer	E4440A	4/11/2013	4/11/2015
T6	AN02611	High Pass Filter	HE9615-150K-50-720B	4/18/2012	4/18/2014

Equipment Under Test (* = EUT):

Function	Manufacturer	Model #	S/N
Carelink USB 2.4*	Medtronic MiniMed	MMT-7306CL	PC0002898F

Support Devices:

Function	Manufacturer	Model #	S/N
Mouse	Microsoft	X800898	NA
Headphones	Monster	DNA	5W64574YRF
Laptop	Dell	Latitude E6320	NA
AC/DC Adaptor	Dell	DA90PE3-00	NA

Test Conditions / Notes:

Temperature: 21°C
Pressure: 102.7kPa
Humidity: 32%
Frequency: 150k-30MHz

EUT is located on the top of the test table 80cm over the ground plane.
EUT is connected to support laptop via a 6 foot long USB extender.
Ports are filled on the support laptop.
EUT is in Transmitting.

Ext Attn: 0 dB

Measurement Data:


Reading listed by margin.

Test Lead: Line

#	Freq MHz	Rdng dB μ V	T1 T5 dB	T2 T6 dB	T3 dB	T4 dB	Dist Table	Corr dB μ V	Spec dB μ V	Margin dB	Polar Ant
1	194.359k QP	51.7	+9.0 +0.0	+0.0 +0.3	+0.0	+0.1	+0.0	61.1	63.8	-2.7	Line
2	201.631k QP	49.1	+9.0 +0.0	+0.0 +0.2	+0.0	+0.1	+0.0	58.4	63.5	-5.1	Line
3	176.178k QP	49.5	+9.0 +0.0	+0.0 +0.4	+0.0	+0.1	+0.0	59.0	64.7	-5.7	Line
4	17.765M	33.3	+9.0 +0.0	+0.0 +0.1	+0.1	+0.6	+0.0	43.1	50.0	-6.9	Line
5	1.355M	28.3	+9.0 +0.0	+0.0 +0.2	+0.1	+0.1	+0.0	37.7	46.0	-8.3	Line
6	3.691M	28.1	+9.0 +0.0	+0.0 +0.2	+0.1	+0.1	+0.0	37.5	46.0	-8.5	Line
7	280.896k QP	42.3	+9.0 +0.0	+0.0 +0.1	+0.0	+0.1	+0.0	51.5	60.8	-9.3	Line
8	332.530k QP	39.0	+9.0 +0.0	+0.0 +0.1	+0.0	+0.1	+0.0	48.2	59.4	-11.2	Line
9	226.356k QP	42.0	+9.0 +0.0	+0.0 +0.3	+0.0	+0.1	+0.0	51.4	62.6	-11.2	Line
10	14.904M	28.6	+9.0 +0.0	+0.0 +0.0	+0.1	+0.7	+0.0	38.4	50.0	-11.6	Line
11	453.500k QP	35.1	+9.0 +0.0	+0.0 +0.2	+0.0	+0.1	+0.0	44.4	56.8	-12.4	Line
12	10.407M	27.0	+9.0 +0.0	+0.1 +0.0	+0.1	+0.3	+0.0	36.5	50.0	-13.5	Line
13	259.807k QP	37.9	+9.0 +0.0	+0.0 +0.2	+0.0	+0.1	+0.0	47.2	61.4	-14.2	Line
14	591.200k Ave	16.0	+9.0 +0.0	+0.0 +0.2	+0.0	+0.1	+0.0	25.3	46.0	-20.7	Line
^	591.200k	41.4	+9.0 +0.0	+0.0 +0.2	+0.0	+0.1	+0.0	50.7	46.0	+4.7	Line
16	201.631k Ave	23.1	+9.0 +0.0	+0.0 +0.2	+0.0	+0.1	+0.0	32.4	53.5	-21.1	Line
^	201.631k	62.5	+9.0 +0.0	+0.0 +0.2	+0.0	+0.1	+0.0	71.8	53.5	+18.3	Line

18	176.178k Ave	23.3	+9.0 +0.0	+0.0 +0.4	+0.0	+0.1	+0.0	32.8	54.7	-21.9	Line
^	176.178k	61.4	+9.0 +0.0	+0.0 +0.4	+0.0	+0.1	+0.0	70.9	54.7	+16.2	Line
20	30.000M	17.7	+9.1 +0.0	+0.1 +0.2	+0.1	+0.8	+0.0	28.0	50.0	-22.0	Line
21	194.359k Ave	22.4	+9.0 +0.0	+0.0 +0.3	+0.0	+0.1	+0.0	31.8	53.8	-22.0	Line
^	194.359k	63.4	+9.0 +0.0	+0.0 +0.3	+0.0	+0.1	+0.0	72.8	53.8	+19.0	Line
23	453.500k Ave	14.8	+9.0 +0.0	+0.0 +0.2	+0.0	+0.1	+0.0	24.1	46.8	-22.7	Line
^	453.500k	47.7	+9.0 +0.0	+0.0 +0.2	+0.0	+0.1	+0.0	57.0	46.8	+10.2	Line
25	711.900k Ave	13.8	+9.0 +0.0	+0.0 +0.2	+0.0	+0.1	+0.0	23.1	46.0	-22.9	Line
^	711.900k	35.8	+9.0 +0.0	+0.0 +0.2	+0.0	+0.1	+0.0	45.1	46.0	-0.9	Line
27	259.807k Ave	18.9	+9.0 +0.0	+0.0 +0.2	+0.0	+0.1	+0.0	28.2	51.4	-23.2	Line
^	259.807k	57.2	+9.0 +0.0	+0.0 +0.2	+0.0	+0.1	+0.0	66.5	51.4	+15.1	Line
29	400.885k QP	24.8	+9.0 +0.0	+0.0 +0.2	+0.0	+0.1	+0.0	34.1	57.8	-23.7	Line
30	332.530k Ave	16.4	+9.0 +0.0	+0.0 +0.1	+0.0	+0.1	+0.0	25.6	49.4	-23.8	Line
^	332.530k	49.4	+9.0 +0.0	+0.0 +0.1	+0.0	+0.1	+0.0	58.6	49.4	+9.2	Line
32	400.885k Ave	14.1	+9.0 +0.0	+0.0 +0.2	+0.0	+0.1	+0.0	23.4	47.8	-24.4	Line
^	400.885k	48.2	+9.0 +0.0	+0.0 +0.2	+0.0	+0.1	+0.0	57.5	47.8	+9.7	Line
34	226.356k Ave	17.9	+9.0 +0.0	+0.0 +0.3	+0.0	+0.1	+0.0	27.3	52.6	-25.3	Line
^	226.356k	60.2	+9.0 +0.0	+0.0 +0.3	+0.0	+0.1	+0.0	69.6	52.6	+17.0	Line
36	350.000k Ave	14.0	+9.0 +0.0	+0.0 +0.1	+0.0	+0.1	+0.0	23.2	49.0	-25.8	Line
37	671.400k Ave	9.3	+9.0 +0.0	+0.0 +0.2	+0.0	+0.1	+0.0	18.6	46.0	-27.4	Line
^	671.400k	35.9	+9.0 +0.0	+0.0 +0.2	+0.0	+0.1	+0.0	45.2	46.0	-0.8	Line
39	280.896k Ave	12.6	+9.0 +0.0	+0.0 +0.1	+0.0	+0.1	+0.0	21.8	50.8	-29.0	Line
^	280.896k	53.3	+9.0 +0.0	+0.0 +0.1	+0.0	+0.1	+0.0	62.5	50.8	+11.7	Line
41	350.000k QP	20.2	+9.0 +0.0	+0.0 +0.1	+0.0	+0.1	+0.0	29.4	59.0	-29.6	Line

CKC Laboratories, Inc. Date: 11/4/2013 Time: 12:08:08 Medtronic MiniMed WO#: 95094
Test Lead: Line 120V 60Hz Sequence#: 10 Line
Medtronic MiniMed Carelink USB 2.4 P/N: MMT-7306CL

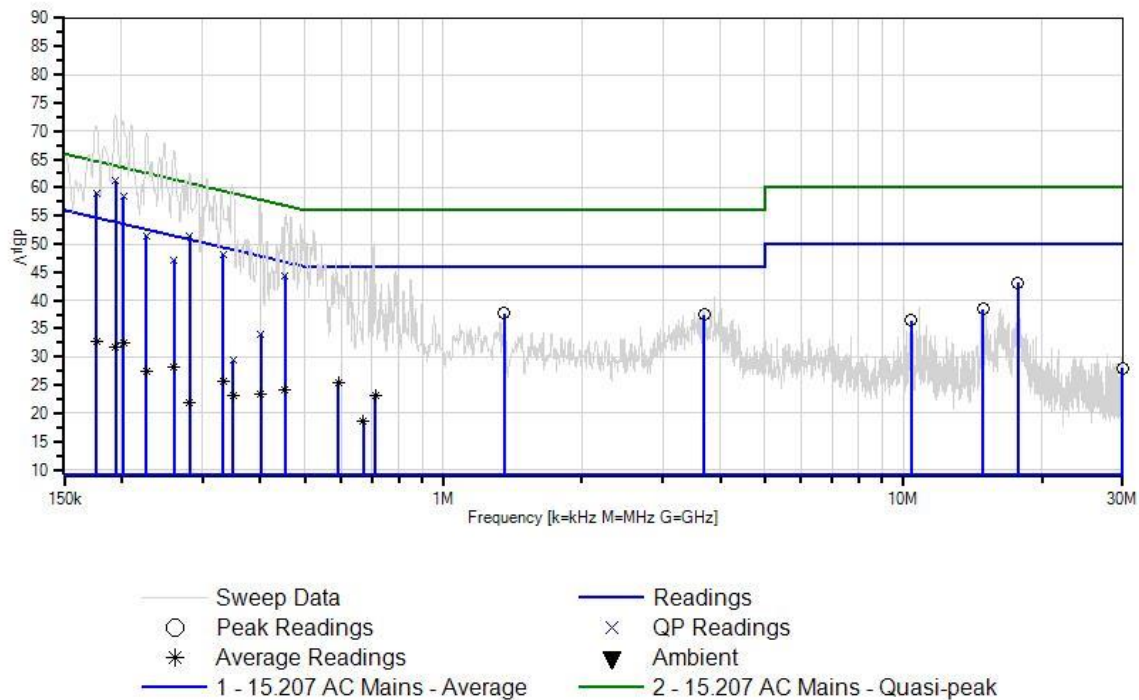

Test Location: CKC Laboratories, Inc. • 22116 23rd Drive SE, Suite A • Bothell, WA 98021 • (425) 402-1717

Customer: **Medtronic MiniMed**
 Specification: **15.207 AC Mains - Average**
 Work Order #: **95094**
 Test Type: **Conducted Emissions**
 Equipment: **Carelink USB 2.4**
 Manufacturer: **Medtronic MiniMed**
 Model: **MMT-7306CL**
 S/N: **PC0002898F**

Date: 11/4/2013
 Time: 12:20:52
 Sequence#: 11
 Tested By: Steven Pittsford
 120V 60Hz

Test Equipment:

ID	Asset #	Description	Model	Calibration Date	Cal Due Date
T1	ANP05435	Attenuator	PE7015-10	10/5/2012	10/5/2014
T2	ANP05546	Cable	Heliac	3/27/2013	3/27/2015
T3	ANP05547	Cable	Heliac	9/7/2012	9/7/2014
	AN01311	50uH LISN-Line	3816/2	12/9/2011	12/9/2013
T4	AN01311	50uH LISN-Neutral	3816/2	12/9/2011	12/9/2013
	AN02871	Spectrum Analyzer	E4440A	4/11/2013	4/11/2015
T5	AN02611	High Pass Filter	HE9615-150K-50-720B	4/18/2012	4/18/2014

Equipment Under Test (* = EUT):

Function	Manufacturer	Model #	S/N
Carelink USB 2.4*	Medtronic MiniMed	MMT-7306CL	PC0002898F

Support Devices:

Function	Manufacturer	Model #	S/N
Mouse	Microsoft	X800898	NA
Headphones	Monster	DNA	5W64574YRF
Laptop	Dell	Latitude E6320	NA
AC/DC Adaptor	Dell	DA90PE3-00	NA

Test Conditions / Notes:

Temperature: 21°C
 Pressure: 102.7kPa
 Humidity: 32%
 Frequency: 150k-30MHz

EUT is located on the top of the test table 80cm over the ground plane.
 EUT is connected to support laptop via a 6 foot long USB extender.
 Ports are filled on the support laptop.
 EUT is in Transmitting.

Ext Attn: 0 dB

Measurement Data:


Reading listed by margin.

Test Lead: Neutral

#	Freq MHz	Rdng dBμV	T1 T5 dB	T2 dB	T3 dB	T4 dB	Dist Table	Corr dBμV	Spec dBμV	Margin dB	Polar Ant
1	174.725k QP	50.9	+9.0 +0.4	+0.0	+0.0	+0.1	+0.0	60.4	64.7	-4.3	Neutr
2	223.448k QP	47.2	+9.0 +0.3	+0.0	+0.0	+0.1	+0.0	56.6	62.7	-6.1	Neutr
3	3.639M	28.0	+9.0 +0.2	+0.0	+0.1	+0.2	+0.0	37.5	46.0	-8.5	Neutr
4	157.999k QP	46.5	+9.0 +0.7	+0.0	+0.0	+0.1	+0.0	56.3	65.6	-9.3	Neutr
5	299.804k QP	40.1	+9.0 +0.1	+0.0	+0.0	+0.1	+0.0	49.3	60.2	-10.9	Neutr
^	299.804k	56.0	+9.0 +0.1	+0.0	+0.0	+0.1	+0.0	65.2	50.2	+15.0	Neutr
7	267.807k QP	40.3	+9.0 +0.2	+0.0	+0.0	+0.1	+0.0	49.6	61.2	-11.6	Neutr
8	17.762M	28.0	+9.0 +0.1	+0.0	+0.1	+0.6	+0.0	37.8	50.0	-12.2	Neutr
9	10.976M	27.1	+9.0 +0.0	+0.1	+0.1	+0.3	+0.0	36.6	50.0	-13.4	Neutr
10	28.376M	21.9	+9.1 +0.2	+0.1	+0.1	+0.8	+0.0	32.2	50.0	-17.8	Neutr
11	560.200k Ave	17.8	+9.0 +0.2	+0.0	+0.0	+0.1	+0.0	27.1	46.0	-18.9	Neutr
^	560.200k	42.8	+9.0 +0.2	+0.0	+0.0	+0.1	+0.0	52.1	46.0	+6.1	Neutr
13	157.999k Ave	26.7	+9.0 +0.7	+0.0	+0.0	+0.1	+0.0	36.5	55.6	-19.1	Neutr
^	157.999k	65.1	+9.0 +0.7	+0.0	+0.0	+0.1	+0.0	74.9	55.6	+19.3	Neutr
15	511.300k Ave	13.4	+9.0 +0.2	+0.0	+0.0	+0.1	+0.0	22.7	46.0	-23.3	Neutr
^	511.300k	40.9	+9.0 +0.2	+0.0	+0.0	+0.1	+0.0	50.2	46.0	+4.2	Neutr
17	223.448k Ave	19.6	+9.0 +0.3	+0.0	+0.0	+0.1	+0.0	29.0	52.7	-23.7	Neutr
^	223.448k	58.3	+9.0 +0.3	+0.0	+0.0	+0.1	+0.0	67.7	52.7	+15.0	Neutr
19	174.725k Ave	21.4	+9.0 +0.4	+0.0	+0.0	+0.1	+0.0	30.9	54.7	-23.8	Neutr
^	174.725k	65.3	+9.0 +0.4	+0.0	+0.0	+0.1	+0.0	74.8	54.7	+20.1	Neutr
21	364.526k QP	22.3	+9.0 +0.1	+0.0	+0.0	+0.1	+0.0	31.5	58.6	-27.1	Neutr
^	364.526k	50.1	+9.0 +0.1	+0.0	+0.0	+0.1	+0.0	59.3	48.6	+10.7	Neutr
23	646.200k Ave	9.3	+9.0 +0.2	+0.0	+0.0	+0.1	+0.0	18.6	46.0	-27.4	Neutr

^	646.200k	40.6	+9.0 +0.2	+0.0	+0.0	+0.1	+0.0	49.9	46.0	+3.9	Neutr
25	422.700k	10.0	+9.0 +0.2	+0.0	+0.0	+0.1	+0.0	19.3	47.4	-28.1	Neutr
Ave											
^	422.700k	44.7	+9.0 +0.2	+0.0	+0.0	+0.1	+0.0	54.0	47.4	+6.6	Neutr
27	707.500k	8.1	+9.0 +0.2	+0.0	+0.0	+0.1	+0.0	17.4	46.0	-28.6	Neutr
Ave											
^	707.500k	37.3	+9.0 +0.2	+0.0	+0.0	+0.1	+0.0	46.6	46.0	+0.6	Neutr
29	267.807k	12.0	+9.0 +0.2	+0.0	+0.0	+0.1	+0.0	21.3	51.2	-29.9	Neutr
Ave											
^	267.807k	54.7	+9.0 +0.2	+0.0	+0.0	+0.1	+0.0	64.0	51.2	+12.8	Neutr

CKC Laboratories, Inc. Date: 11/4/2013 Time: 12:20:52 Medtronic MiniMed WO#: 95094
Test Lead: Neutral 120V 60Hz Sequence#: 11 Neutral
Medtronic MiniMed Carelink USB 2.4 P/N: MMT-7306CL

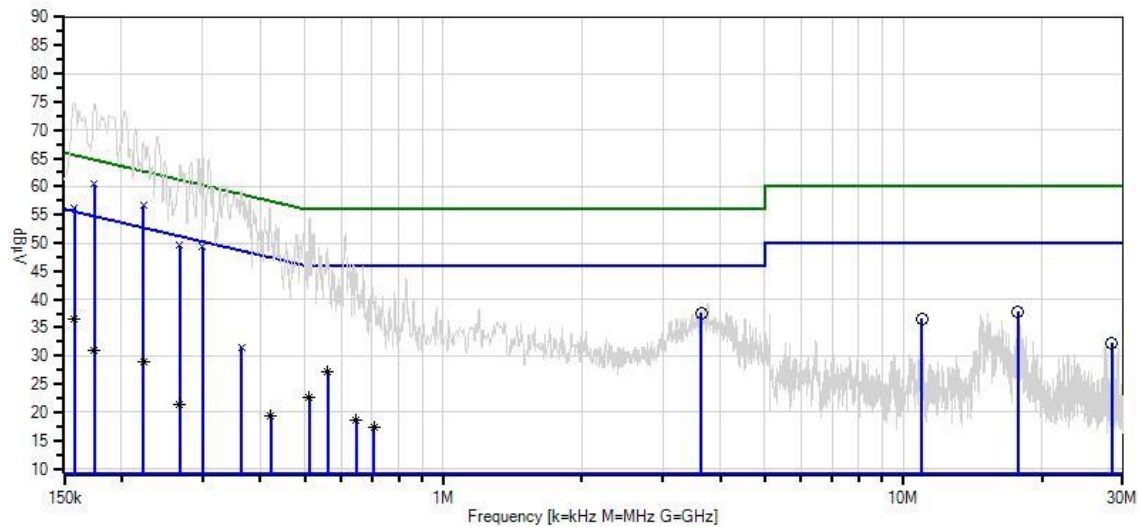

— Sweep Data
○ Peak Readings
* Average Readings
— 1 - 15.207 AC Mains - Average
— Readings
× QP Readings
▼ Ambient
— 2 - 15.207 AC Mains - Quasi-peak

Test Setup Photos



15.247(a)(2) 6dB Occupied Bandwidth

Test Conditions / Setup

The EUT's antenna is non-removable, thus the data will be gathered through radiated measurements. The EUT is located on top of a Styrofoam table, 80cm over the ground plane. The EUT is connected to support laptop via a 6 foot long USB extender. Ports are filled on the support laptop.

Test Conditions:

Temp: 23°C

Humidity: 31%

Pressure: 102.5kPa


Freq: 2400-2483.5MHz

Engineer Name: Steven Pittsford


Test Equipment					
Asset #	Description	Model	Manufacturer	Cal Date	Cal Due
AN01467	Horn Antenna-ANSI C63.5 Calibration	3115	EMCO	9/16/2013	9/16/2015
AN03209	Preamplifier	83051A	Agilent	3/5/2013	3/5/2015
ANP05546	Cable	Helix	Andrews	3/27/2013	3/27/2015
ANP05547	Cable	Helix	Andrews	9/7/2012	9/7/2014
AN02871	Spectrum Analyzer	E4440A	Agilent	4/11/2013	4/11/2015

Test Data


Frequency (MHz)	6dB Bandwidth
2420	1.595MHz
2450	1.520MHz
2480	1.606MHz

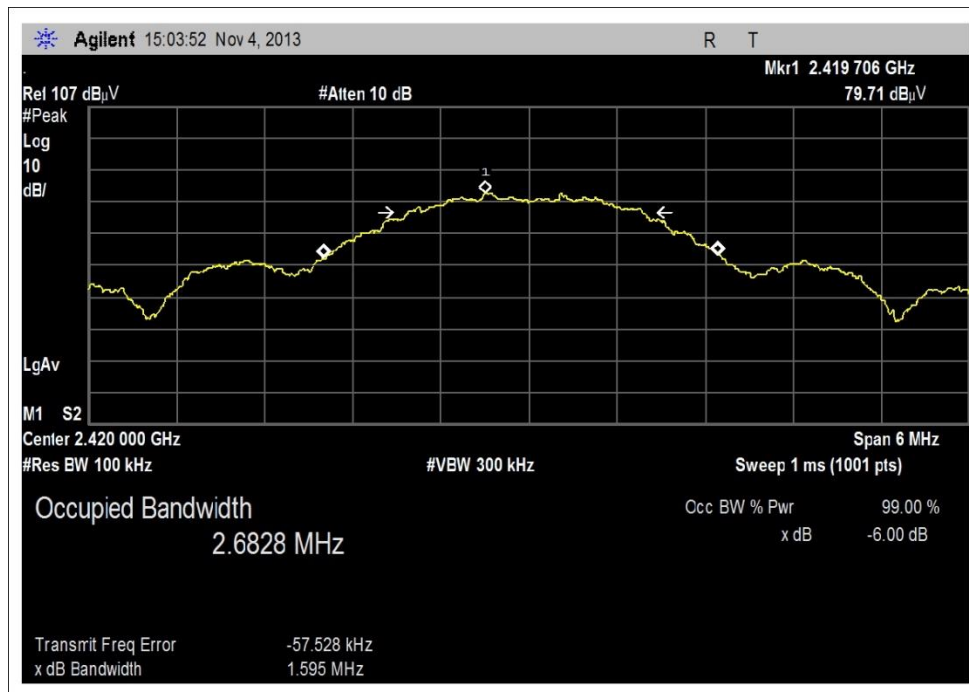

Low

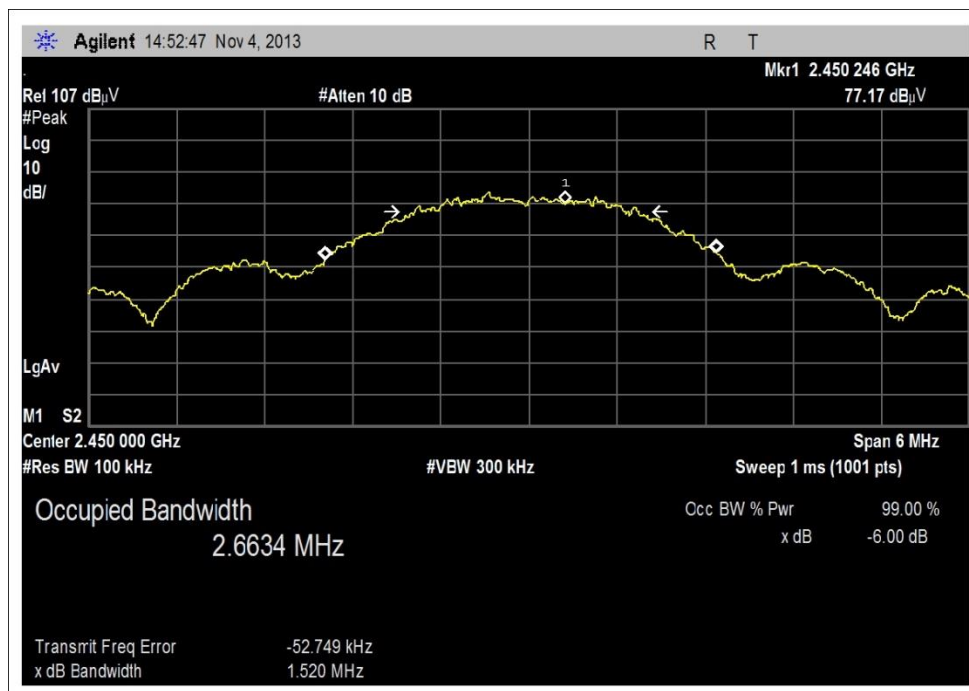

Middle

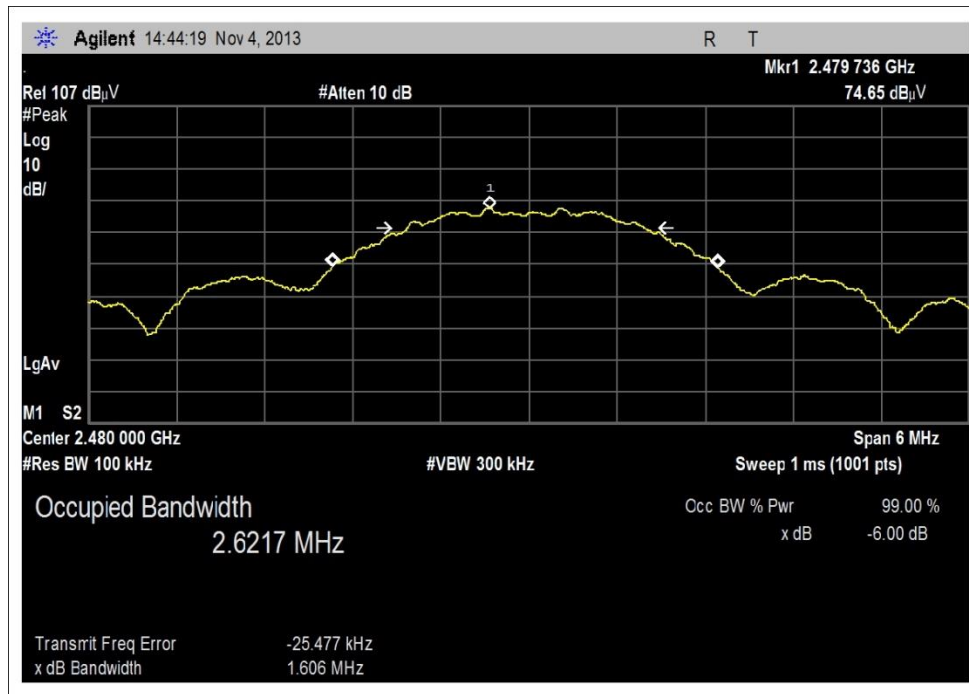

High

Test Setup Photos



15.247(b)(3) Maximum Output Power

Test Conditions / Setup

The EUT's antenna is non-removable, thus the data will be gathered through radiated measurements. The formula shown below will be used to calculate the ERP. The EUT is located on top of a Styrofoam table, 80cm over the ground plane. Voltage on the laptop will be varied per FCC 15.31(e). The EUT is connected to support laptop via a 6 foot long USB extender. Ports are filled on the support laptop.

Test Conditions:

Temp: 21°C

Humidity: 32%

Pressure: 102.6kPa

Freq: 2400-2483.5MHz

$$P = (E_d)^2 / (30 * G)$$

E = Field strength of the measurement converted to V/M

d = Measurement distance in meters

G = Numerical gain of the EUT's antenna relative to an isotropic radiator.


P = The power in watts for which we are solving

Engineer Name: Steven Pittsford


Test Equipment					
Asset #	Description	Model	Manufacturer	Cal Date	Cal Due
AN01467	Horn Antenna-ANSI C63.5 Calibration	3115	EMCO	9/16/2013	9/16/2015
AN03209	Preamplifier	83051A	Agilent	3/5/2013	3/5/2015
ANP05546	Cable	Heliac	Andrews	3/27/2013	3/27/2015
ANP05547	Cable	Heliac	Andrews	9/7/2012	9/7/2014
AN02871	Spectrum Analyzer	E4440A	Agilent	4/11/2013	4/11/2015

Test Data


Frequency (MHz)	Input Voltage	Spectrum Analyzer Measurement (dBuV)	Corrections due to cables, amplifiers, antennas and (dB)	Corrected Reading (dBuV)	Antenna Gain (dBi)	Conducted Power (Watts)
2420	102VAC	88.7	1.5	90.2	0	3.141×10^{-4}
	120VAC	88.7	1.5	90.2	0	3.141×10^{-4}
	138VAC	88.7	1.5	90.2	0	3.141×10^{-4}
2450	102VAC	87.2	1.6	88.8	0	2.276×10^{-4}
	120VAC	87.2	1.6	88.8	0	2.276×10^{-4}
	138VAC	87.2	1.6	88.8	0	2.276×10^{-4}
2480	102VAC	86.6	1.6	88.2	0	1.982×10^{-4}
	120VAC	86.6	1.6	88.2	0	1.982×10^{-4}
	138VAC	86.6	1.6	88.2	0	1.982×10^{-4}

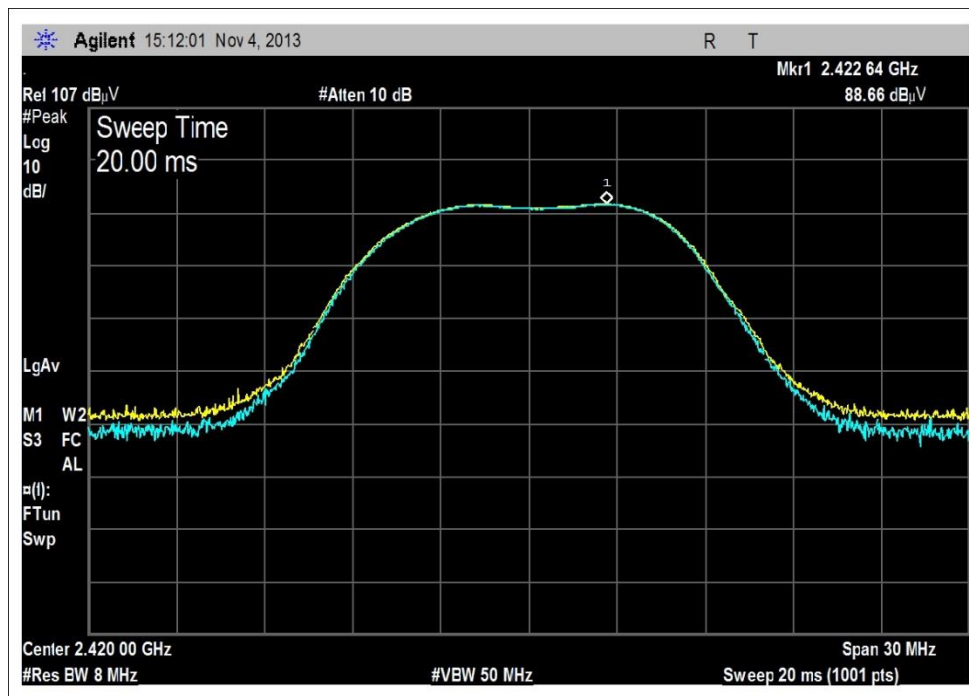

Low

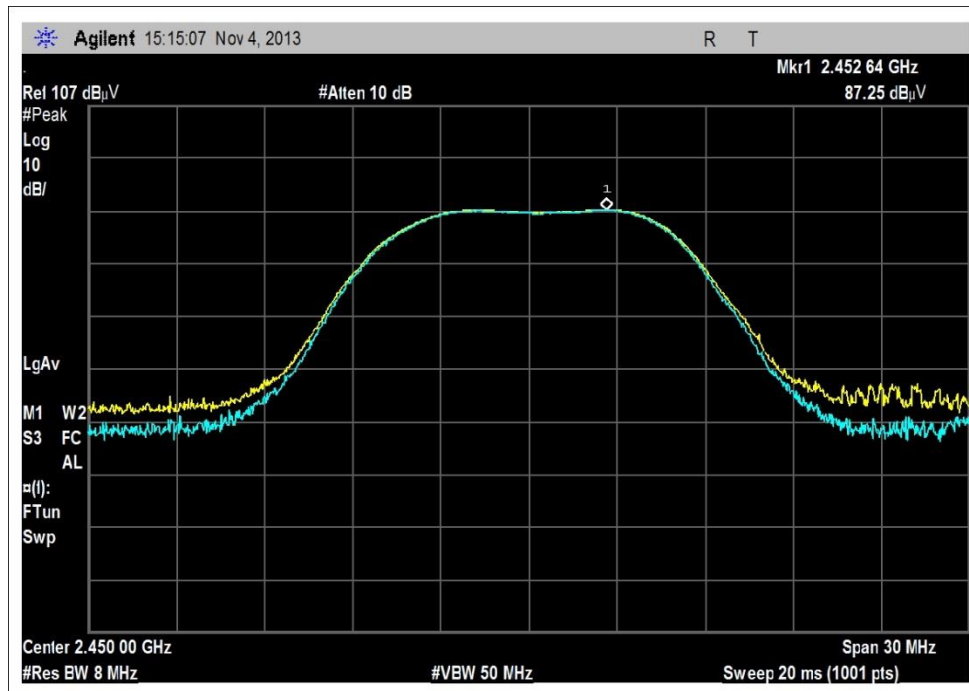

Middle

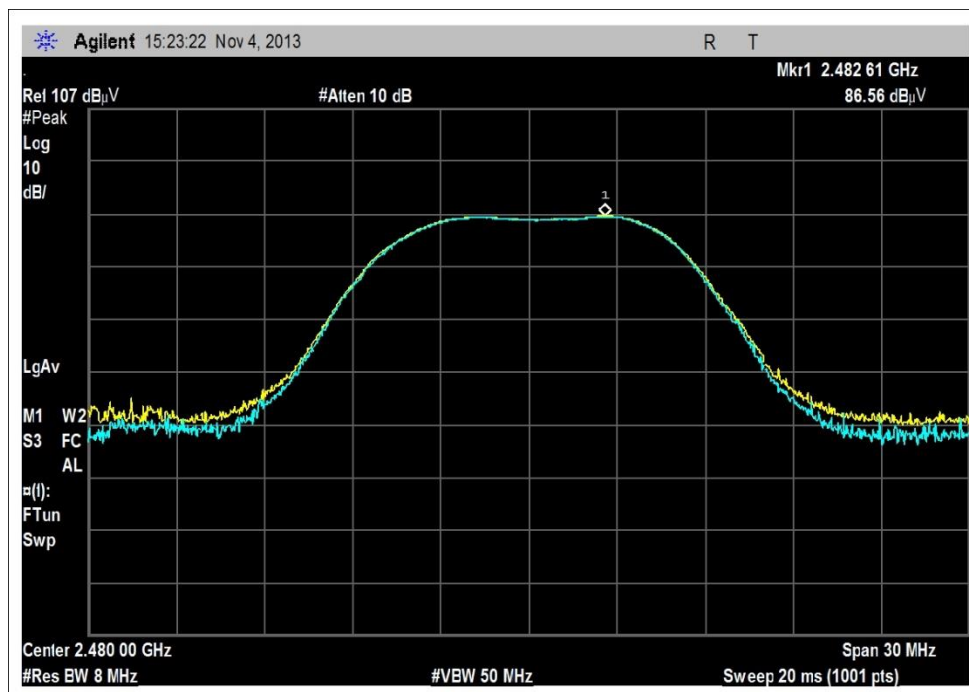

High

Test Setup Photos



15.247(d) Radiated Spurious Emissions

Test Data Sheet

Test Location: CKC Laboratories, Inc. • 22116 23rd Drive SE, Suite A • Bothell, WA 98021 • (425) 402-1717

Customer: **Medtronic MiniMed**
 Specification: **15.247(d) / 15.209 Radiated Spurious Emissions**
 Work Order #: **95094** Date: 11/5/2013
 Test Type: **Maximized Emissions** Time: 18:16:37
 Equipment: **Carelink USB 2.4** Sequence#: 10
 Manufacturer: **Medtronic MiniMed** Tested By: **Steven Pittsford**
 Model: **MMT-7306CL**
 S/N: **PC0002898F**

Test Equipment:

ID	Asset #	Description	Model	Calibration Date	Cal Due Date
T1	AN01467	Horn Antenna-ANSI C63.5 Calibration	3115	9/16/2013	9/16/2015
T2	AN03209	Preamplifier	83051A	3/5/2013	3/5/2015
T3	ANP05546	Cable	Heliac	3/27/2013	3/27/2015
T4	ANP05547	Cable	Heliac	9/7/2012	9/7/2014
T5	AN02871	Spectrum Analyzer	E4440A	4/11/2013	4/11/2015
T6	AN02741	Active Horn Antenna	AMFW-5F-12001800-20-10P	12/18/2012	12/18/2014
T7	AN02742	Active Horn Antenna	AMFW-5F-18002650-20-10P	12/17/2012	12/17/2014
T8	AN02763-69	Waveguide	Multiple	6/7/2012	6/7/2014
T9	ANP05428	Cable	PE35591-60	6/8/2012	6/8/2014
T10	AN02308	Preamplifier	8447D	4/3/2012	4/3/2014
T11	AN01996	Biconilog Antenna	CBL6111C	3/2/2012	3/2/2014
T12	ANP05360	Cable	RG214	12/3/2012	12/3/2014
T13	ANP05541	Cable	Heliac	4/11/2012	4/11/2014
T14	AN00052	Loop Antenna	6502	5/16/2012	5/16/2014
T15	ANP05422	Cable	PE35591-72	6/8/2012	6/8/2014

Equipment Under Test (* = EUT):

Function	Manufacturer	Model #	S/N
Carelink USB 2.4*	Medtronic MiniMed	MMT-7306CL	PC0002898F

Support Devices:

Function	Manufacturer	Model #	S/N
AC/DC Adaptor	Dell	DA90PE3-00	NA
Laptop	Dell	Latitude E6320	NA
Headphones	Monster	DNA	5W64574YRF
Mouse	Microsoft	X800898	NA

Test Conditions / Notes:

Temperature: 23°C
Pressure: 102.5kPa
Humidity: 31%
Frequency: 9k-26GHz

Vertical and Horizontal Polarizations investigated
CISPR Bandwidths Used.

EUT is located on the top of the test table 80cm over the ground plane.

EUT is connected to support laptop via a 6 foot long USB extender. Ports are filled on the support laptop.

EUT is transmitting at Low, Mid and High Channels.

Ext Attn: 0 dB

Measurement Data:

Reading listed by margin.

Test Distance: 3 Meters

#	Freq	Rdng	T1 T5 T9 T13	T2 T6 T10 T14	T3 T7 T11 T15	T4 T8 T12	Dist	Corr	Spec	Margin	Polar
	MHz	dBμV	dB	dB	dB	dB	Table	dBμV/m	dBμV/m	dB	Ant
1	4959.658M	41.4	+32.5 +0.0 +0.0 +0.0	-30.8 +0.0 +0.0 +0.0	+2.3 +0.0 +0.0 +0.0	+3.6 +0.0 +0.0 +0.0	+0.0 -16	49.0	54.0	-5.0	Vert 100
2	144.500M	53.3	+0.0 +0.0 +0.0 +0.4	+0.0 +0.0 -27.6 +0.0	+0.3 +0.0 +11.3 +0.0	+0.0 +0.0 +0.7	+0.0 351	38.4	43.5	-5.1	Horiz 131
3	4960.692M	41.3	+32.5 +0.0 +0.0 +0.0	-30.8 +0.0 +0.0 +0.0	+2.3 +0.0 +0.0 +0.0	+3.6 +0.0 +0.0 +0.0	+0.0	48.9	54.0	-5.1	Horiz
4	4899.905M	41.5	+32.3 +0.0 +0.0 +0.0	-30.8 +0.0 +0.0 +0.0	+2.2 +0.0 +0.0 +0.0	+3.6 +0.0 +0.0 +0.0	+0.0 360	48.8	54.0	-5.2	Horiz 116
5	24800.345 M	44.9	+0.0 +0.0 +6.3 +0.0	+0.0 +0.0 +0.0 +0.0	+0.0 -12.4 +0.0 +8.6	+0.0 +0.2 +0.0	+0.0 304	47.6	54.0	-6.4	Vert 106
6	4840.915M	40.5	+32.2 +0.0 +0.0 +0.0	-30.9 +0.0 +0.0 +0.0	+2.2 +0.0 +0.0 +0.0	+3.5 +0.0 +0.0 +0.0	+0.0 348	47.5	54.0	-6.5	Horiz 112
7	4899.235M	39.7	+32.3 +0.0 +0.0 +0.0	-30.8 +0.0 +0.0 +0.0	+2.2 +0.0 +0.0 +0.0	+3.6 +0.0 +0.0 +0.0	+0.0	47.0	54.0	-7.0	Vert 123
8	4840.000M	39.2	+32.2 +0.0 +0.0 +0.0	-30.9 +0.0 +0.0 +0.0	+2.2 +0.0 +0.0 +0.0	+3.5 +0.0 +0.0 +0.0	+0.0 203	46.2	54.0	-7.8	Vert 101


9	711.900M	41.5	+0.0	+0.0	+0.7	+0.0	+0.0	37.7	46.0	-8.3	Horiz
			+0.0	+0.0	+0.0	+0.0	360				131
			+0.0	-28.2	+20.9	+1.8					
			+1.0	+0.0	+0.0						
10	263.800M	49.9	+0.0	+0.0	+0.4	+0.0	+0.0	37.5	46.0	-8.5	Horiz
			+0.0	+0.0	+0.0	+0.0					99
			+0.0	-27.1	+12.7	+1.0					
			+0.6	+0.0	+0.0						
11	1330.000M	48.4	+24.5	-30.7	+1.3	+1.8	+0.0	45.3	54.0	-8.7	Horiz
			+0.0	+0.0	+0.0	+0.0	102				99
			+0.0	+0.0	+0.0	+0.0					
			+0.0	+0.0	+0.0						
12	24500.050 M	42.8	+0.0	+0.0	+0.0	+0.0	+0.0	45.1	54.0	-8.9	Vert
			+0.0	+0.0	-12.9	+0.1					
			+6.4	+0.0	+0.0	+0.0	360				109
			+0.0	+0.0	+8.7						
13	143.500M	49.3	+0.0	+0.0	+0.3	+0.0	+0.0	34.4	43.5	-9.1	Horiz
			+0.0	+0.0	+0.0	+0.0					99
			+0.0	-27.6	+11.3	+0.7					
			+0.4	+0.0	+0.0						
14	59.100M	52.4	+0.0	+0.0	+0.1	+0.0	+0.0	30.8	40.0	-9.2	Horiz
			+0.0	+0.0	+0.0	+0.0					99
			+0.0	-28.0	+5.5	+0.5					
			+0.3	+0.0	+0.0						
15	52.300M	50.6	+0.0	+0.0	+0.1	+0.0	+0.0	30.7	40.0	-9.3	Horiz
			+0.0	+0.0	+0.0	+0.0	360				131
			+0.0	-28.0	+7.4	+0.4					
			+0.2	+0.0	+0.0						
16	24200.000 M	42.9	+0.0	+0.0	+0.0	+0.0	+0.0	44.5	54.0	-9.5	Vert
			+0.0	+0.0	-13.5	+0.1					
			+6.4	+0.0	+0.0	+0.0					109
			+0.0	+0.0	+8.6						
17	273.500M	48.1	+0.0	+0.0	+0.4	+0.0	+0.0	35.9	46.0	-10.1	Horiz
			+0.0	+0.0	+0.0	+0.0	360				131
			+0.0	-27.1	+12.8	+1.1					
			+0.6	+0.0	+0.0						
18	384.000M	45.4	+0.0	+0.0	+0.4	+0.0	+0.0	35.8	46.0	-10.2	Horiz
			+0.0	+0.0	+0.0	+0.0	360				131
			+0.0	-27.7	+15.8	+1.2					
			+0.7	+0.0	+0.0						
19	19360.000 M	42.2	+0.0	+0.0	+0.0	+0.0	+0.0	43.6	54.0	-10.4	Vert
			+0.0	+0.0	-13.3	+1.5					
			+5.5	+0.0	+0.0	+0.0	360				106
			+0.0	+0.0	+7.7						
20	359.800M	45.7	+0.0	+0.0	+0.4	+0.0	+0.0	35.6	46.0	-10.4	Horiz
			+0.0	+0.0	+0.0	+0.0					99
			+0.0	-27.5	+15.1	+1.2					
			+0.7	+0.0	+0.0						
21	19838.245 M	42.4	+0.0	+0.0	+0.0	+0.0	+0.0	43.5	54.0	-10.5	Vert
			+0.0	+0.0	-13.4	+0.9					
			+5.7	+0.0	+0.0	+0.0					99
			+0.0	+0.0	+7.9						

22	19600.050 M	41.8	+0.0 +0.0 +5.6 +0.0	+0.0 +0.0 +0.0 +0.0	+0.0 -13.3 +0.0 +7.8	+0.0 +1.3 +0.0	+0.0 360	43.2	54.0	-10.8	Vert 109
23	2666.000M	40.8	+28.5 +0.0 +0.0 +0.0	-30.2 +0.0 +0.0 +0.0	+1.4 +0.0 +0.0 +0.0	+2.7 +0.0	+0.0	43.2	54.0	-10.8	Vert 99
24	7440.110M Ave	25.7	+37.5 +0.0 +0.0 +0.0	-28.2 +0.0 +0.0 +0.0	+3.2 +0.0 +0.0 +0.0	+4.4 +0.0 360	+0.0	42.6	54.0	-11.4	Vert 105
^	7440.110M	39.2	+37.5 +0.0 +0.0 +0.0	-28.2 +0.0 +0.0 +0.0	+3.2 +0.0 +0.0 +0.0	+4.4 +0.0 220	+0.0	56.1	54.0	+2.1	Vert 100
26	9681.275M Ave	24.6	+37.5 +0.0 +0.0 +0.0	-27.8 +0.0 +0.0 +0.0	+3.4 +0.0 +0.0 +0.0	+4.8 +0.0 +0.0	+0.0 360	42.5	54.0	-11.5	Vert 105
^	9681.275M	39.5	+37.5 +0.0 +0.0 +0.0	-27.8 +0.0 +0.0 +0.0	+3.4 +0.0 +0.0 +0.0	+4.8 +0.0 360	+0.0	57.4	54.0	+3.4	Vert 100
28	9920.000M Ave	25.1	+37.3 +0.0 +0.0 +0.0	-27.9 +0.0 +0.0 +0.0	+3.1 +0.0 +0.0 +0.0	+4.9 +0.0 360	+0.0	42.5	54.0	-11.5	Horiz 105
^	9920.000M	40.5	+37.3 +0.0 +0.0 +0.0	-27.9 +0.0 +0.0 +0.0	+3.1 +0.0 +0.0 +0.0	+4.9 +0.0 360	+0.0	57.9	54.0	+3.9	Horiz 99
30	9800.642M Ave	24.8	+37.4 +0.0 +0.0 +0.0	-27.8 +0.0 +0.0 +0.0	+3.2 +0.0 +0.0 +0.0	+4.9 +0.0 360	+0.0	42.5	54.0	-11.5	Vert 105
^	9800.642M	39.9	+37.4 +0.0 +0.0 +0.0	-27.8 +0.0 +0.0 +0.0	+3.2 +0.0 +0.0 +0.0	+4.9 +0.0 275	+0.0	57.6	54.0	+3.6	Vert 105
32	171.600M	48.3	+0.0 +0.0 +0.0 +0.5	+0.0 +0.0 -27.4 +0.0	+0.3 +0.0 +9.5 +0.0	+0.0 +0.0 +0.8	+0.0 360	32.0	43.5	-11.5	Horiz 131
33	7349.230M Ave	25.5	+37.1 +0.0 +0.0 +0.0	-28.2 +0.0 +0.0 +0.0	+3.1 +0.0 +0.0 +0.0	+4.3 +0.0 360	+0.0	41.8	54.0	-12.2	Horiz 105
^	7349.230M	40.8	+37.1 +0.0 +0.0 +0.0	-28.2 +0.0 +0.0 +0.0	+3.1 +0.0 +0.0 +0.0	+4.3 +0.0	+0.0	57.1	54.0	+3.1	Horiz 120

35	7262.230M Ave	25.5	+36.8 +0.0 +0.0 +0.0	-28.2 +0.0 +0.0 +0.0	+3.0 +0.0 +0.0 +0.0	+4.3 +0.0 +0.0 +0.0	+0.0 360	41.4	54.0	-12.6	Vert 105
36	7262.230M Ave	25.5	+36.8 +0.0 +0.0 +0.0	-28.2 +0.0 +0.0 +0.0	+3.0 +0.0 +0.0 +0.0	+4.3 +0.0 +0.0 +0.0	+0.0 360	41.4	54.0	-12.6	Horiz 105
^	7262.230M	40.8	+36.8 +0.0 +0.0 +0.0	-28.2 +0.0 +0.0 +0.0	+3.0 +0.0 +0.0 +0.0	+4.3 +0.0 +0.0 +0.0	+0.0	56.7	54.0	+2.7	Horiz 124
38	17359.925 M	41.2	+0.0 +0.0 +0.0 +0.0	+0.0 -12.3 +0.0 +0.0	+4.5 +0.0 +0.0 +0.0	+6.9 +0.0 +0.0 +0.0	+0.0	40.3	54.0	-13.7	Vert 99
39	467.500M	40.0	+0.0 +0.0 +0.0 +0.8	+0.0 +0.0 -28.2 +0.0	+0.5 +0.0 +17.5 +0.0	+0.0 +0.0 +1.4	+0.0 360	32.0	46.0	-14.0	Horiz 131
40	17150.630 M	41.5	+0.0 +0.0 +0.0 +0.0	+0.0 -12.7 +0.0 +0.0	+4.4 +0.0 +0.0 +0.0	+6.7 +0.0 +0.0	+0.0	39.9	54.0	-14.1	Horiz 99
41	22318.860 M	41.9	+0.0 +0.0 +6.0 +0.0	+0.0 +0.0 +0.0 +0.0	+0.0 -16.8 +0.0 +8.3	+0.0 +0.1 +0.0	+0.0 181	39.5	54.0	-14.5	Vert 106
42	22050.050 M	41.3	+0.0 +0.0 +6.1 +0.0	+0.0 +0.0 +0.0 +0.0	+0.0 -16.5 +0.0 +8.3	+0.0 +0.2 +0.0	+0.0 360	39.4	54.0	-14.6	Vert 109
43	468.400M	39.1	+0.0 +0.0 +0.0 +0.8	+0.0 +0.0 -28.2 +0.0	+0.5 +0.0 +17.5 +0.0	+0.0 +0.0 +1.4	+0.0	31.1	46.0	-14.9	Horiz 99
44	81.400M	44.2	+0.0 +0.0 +0.0 +0.3	+0.0 +0.0 -28.0 +0.0	+0.2 +0.0 +7.4 +0.0	+0.0 +0.0 +0.6	+0.0 360	24.7	40.0	-15.3	Horiz 131
45	21780.000 M	40.2	+0.0 +0.0 +6.0 +0.0	+0.0 +0.0 +0.0 +0.0	+0.0 -16.1 +0.0 +8.3	+0.0 +0.2 +0.0	+0.0	38.6	54.0	-15.4	Vert 109
46	16942.270 M	39.9	+0.0 +0.0 +0.0 +0.0	+0.0 -12.9 +0.0 +0.0	+4.4 +0.0 +0.0 +0.0	+6.5 +0.0 +0.0	+0.0	37.9	54.0	-16.1	Vert 99
47	14699.250 M	41.8	+0.0 +0.0 +0.0 +0.0	+0.0 -14.9 +0.0 +0.0	+4.2 +0.0 +0.0 +0.0	+6.3 +0.0 +0.0	+0.0 354	37.4	54.0	-16.6	Horiz 99



48	14879.360 M	40.9	+0.0 +0.0 +0.0 +0.0	+0.0 -14.8 +0.0 +0.0	+4.0 +0.0 +0.0 +0.0	+6.3 +0.0 +0.0 +0.0	+0.0	36.4	54.0	-17.6	Vert 99
49	12398.105 M	40.0	+0.0 +0.0 +0.0 +0.0	+0.0 -14.1 +0.0 +0.0	+3.8 +0.0 +0.0 +0.0	+5.7 +0.0 +0.0 +0.0	+0.0	35.4	54.0	-18.6	Vert 99
50	12100.865 M	39.4	+0.0 +0.0 +0.0 +0.0	+0.0 -13.9 +0.0 +0.0	+3.8 +0.0 +0.0 +0.0	+5.6 +0.0 +0.0 +0.0	+0.0	34.9	54.0	-19.1	Vert 99
51	12250.480 M	38.6	+0.0 +0.0 +0.0 +0.0	+0.0 -13.9 +0.0 +0.0	+3.8 +0.0 +0.0 +0.0	+5.7 +0.0 +0.0 +0.0	+0.0	34.2	54.0	-19.8	Horiz 105
52	24800.000 M Ave	30.7	+0.0 +0.0 +6.3 +0.0	+0.0 +0.0 +0.0 +0.0	+0.0 -12.4 +0.0 +8.6	+0.0 +0.2 +0.0 +0.0	+0.0 298	33.4	54.0	-20.6	Vert 106
53	19.582M	25.3	+0.0 +0.0 +0.0 +0.0	+0.0 +0.0 +0.0 +7.9	+0.0 +0.0 +0.0 +0.0	+0.0 +0.0 +0.0 +0.0	-40.0	-6.8	29.5	-36.3	Paral 99
54	130.500k	43.2	+0.0 +0.0 +0.0 +0.0	+0.0 +0.0 +0.0 +9.5	+0.0 +0.0 +0.0 +0.0	+0.0 +0.0 +0.0 +0.0	-80.0	-27.3	25.3	-52.6	Paral 99
55	135.140k	42.6	+0.0 +0.0 +0.0 +0.0	+0.0 +0.0 +0.0 +9.5	+0.0 +0.0 +0.0 +0.0	+0.0 +0.0 +0.0 +0.0	-80.0	-27.9	25.0	-52.9	Paral 99

CKC Laboratories, Inc. Date: 11/5/2013 Time: 18:16:37 Medtronic MiniMed WO#: 95094
 Test Distance: 3 Meters Sequence#: 10 Horiz
 Medtronic MiniMed Carelink USB 2.4 P/N: MMT-7306CL

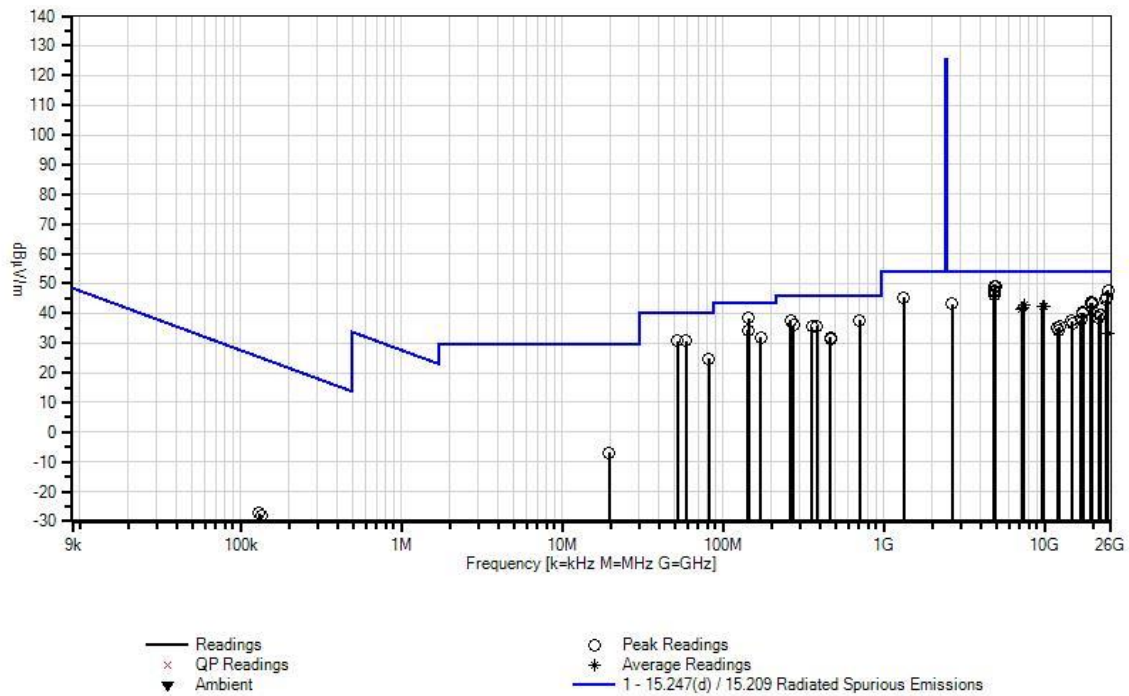

Bandedge

Test Plots

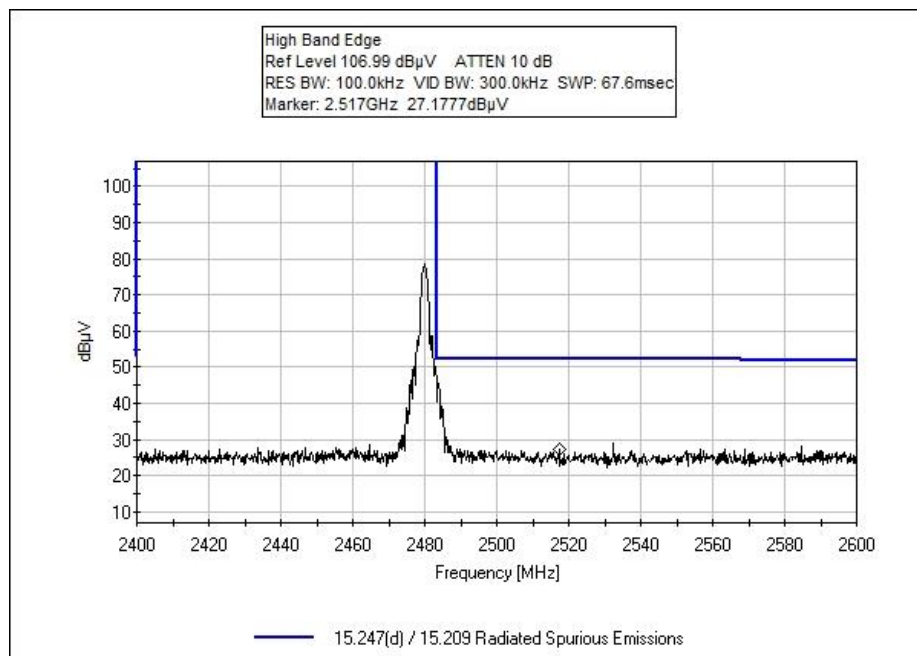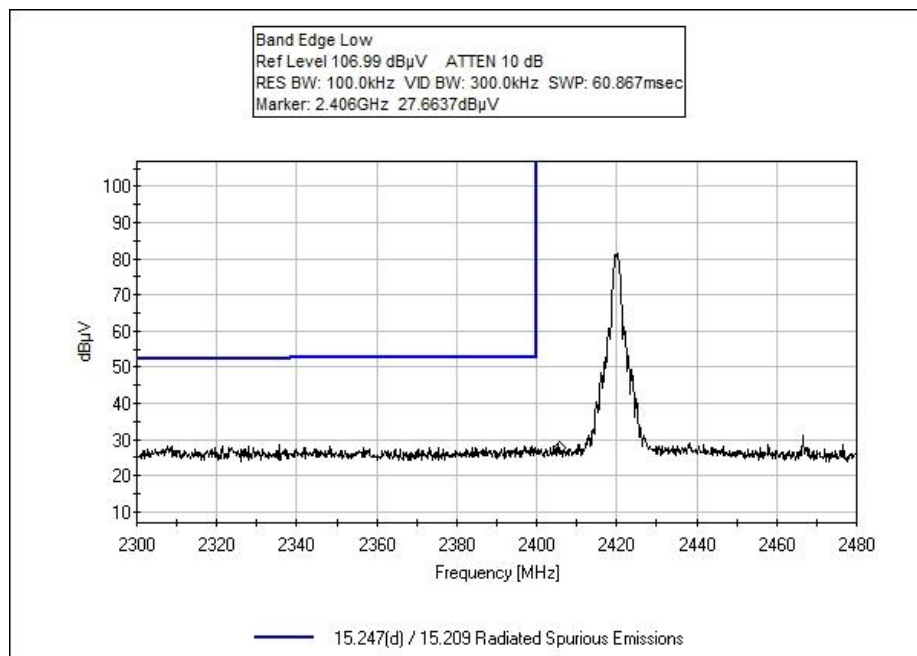

Test Setup Photos



15.247(e) Power Spectral Density

Test Conditions / Setup

The EUT's antenna is non-removable, thus the data will be gathered through radiated measurements. The formula shown below will be used to calculate the Power Spectral Density. The EUT is located on top of a Styrofoam table, 80cm over the ground plane. The EUT is connected to support laptop via a 6 foot long USB extender. Ports are filled on the support laptop.

Test Conditions:

Temp: 21°C

Humidity: 38%

Pressure: 103.1kPa

Freq: 2400-2483.5MHz

$$P = (Ed)^2 / (30 * G)$$

E = Field strength of the measurement converted to V/M.

d = Measurement distance in meters.

G = Numerical gain of the EUT's antenna relative to an isotropic radiator.


P = The power in watts for which we are solving.

Engineer Name: Steven Pittsford


Test Equipment					
Asset #	Description	Model	Manufacturer	Cal Date	Cal Due
AN01467	Horn Antenna-ANSI C63.5 Calibration	3115	EMCO	9/16/2013	9/16/2015
AN03209	Preamplifier	83051A	Agilent	3/5/2013	3/5/2015
ANP05546	Cable	Heliac	Andrews	3/27/2013	3/27/2015
ANP05547	Cable	Heliac	Andrews	9/7/2012	9/7/2014
AN02871	Spectrum Analyzer	E4440A	Agilent	4/11/2013	4/11/2015

Test Data


Frequency (MHz)	Spectrum Analyzer Measurement (dBuV)	Corrections due to cables, amplifiers, antennas and Bandwidth (dB)	Corrected Reading (dBuV)	Antenna Gain (dBi)	Spectral Density (Watts)	Spectral Density (dBm)
2420	78.6	1.5	80.1	0.0	3.070×10^{-5}	-15.129
2450	77.1	1.6	78.7	0.0	2.224×10^{-5}	-16.529
2480	77.1	1.6	78.7	0.0	2.224×10^{-5}	-16.529

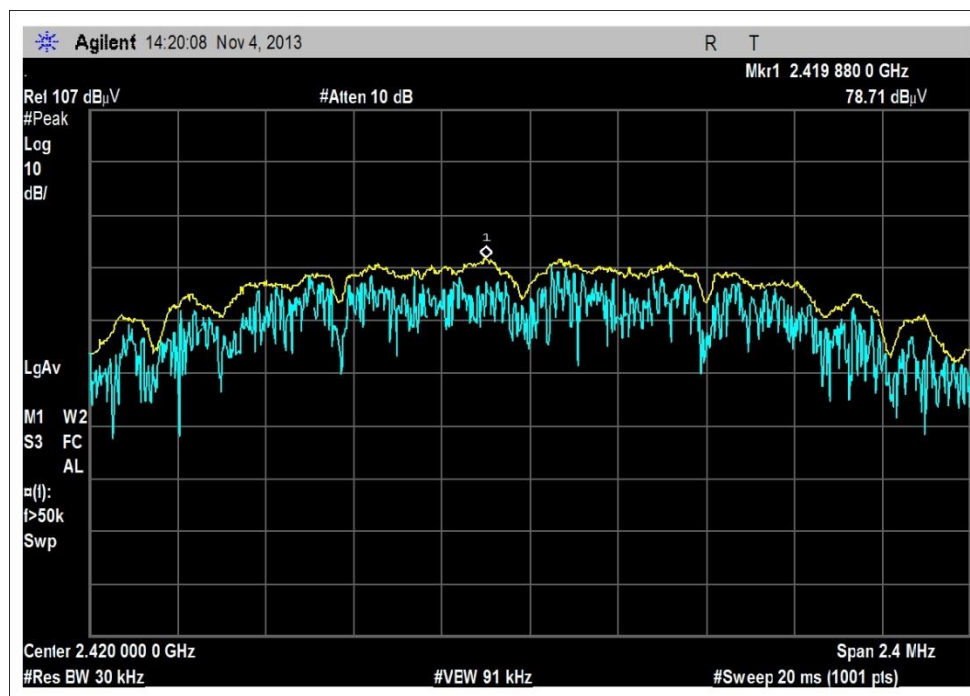

Low

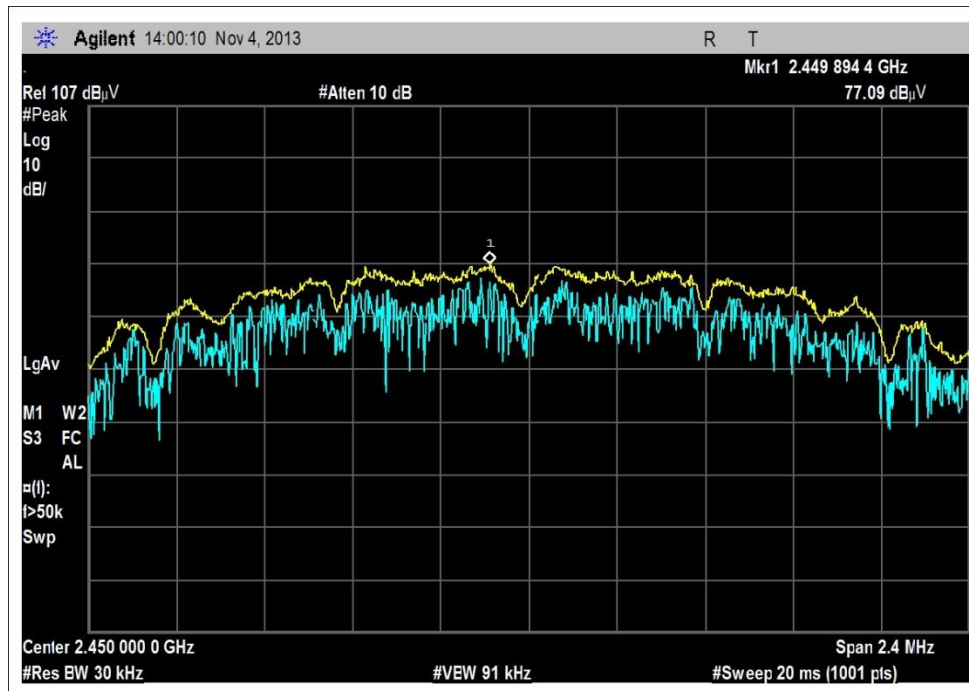

Middle

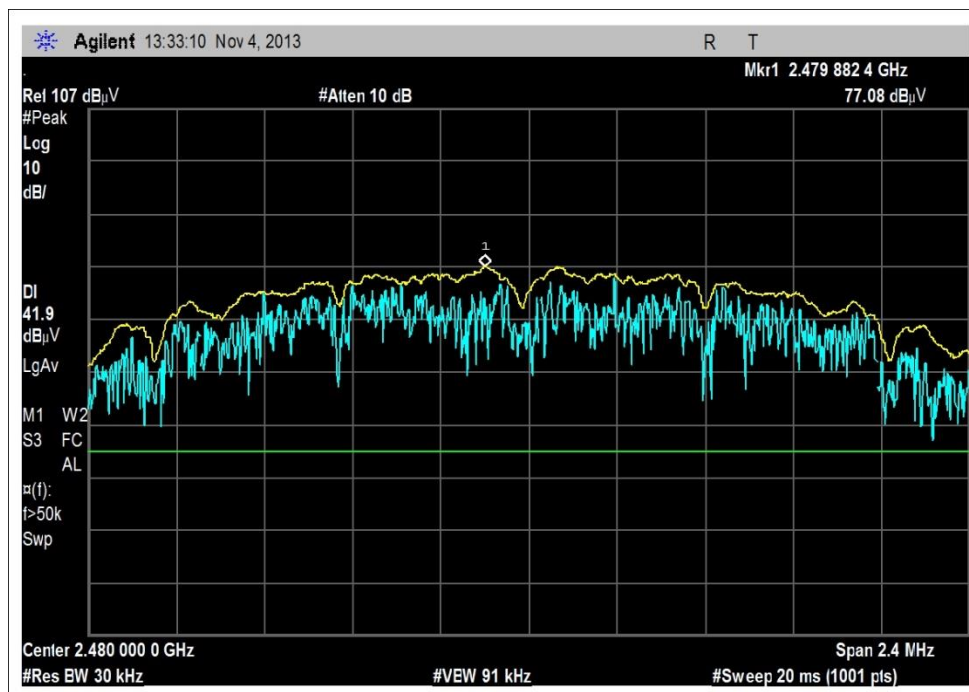

High

Test Setup Photos



SUPPLEMENTAL INFORMATION

Measurement Uncertainty

Uncertainty Value	Parameter
4.73 dB	Radiated Emissions
3.34 dB	Mains Conducted Emissions
3.30 dB	Disturbance Power

The reported measurement uncertainties are calculated based on the worst case of all laboratory environments from CKC Laboratories, Inc. test sites. Only those parameters which require estimation of measurement uncertainty are reported. The reported worst case measurement uncertainty is less than the maximum values derived in CISPR 16-4-2. Reported uncertainties represent expanded uncertainties expressed at approximately the 95% confidence level using a coverage factor of $k=2$. Compliance is deemed to occur provided measurements are below the specified limits.

Emissions Test Details

TESTING PARAMETERS

Unless otherwise indicated, the following configuration parameters are used for equipment setup: The cables were routed consistent with the typical application by varying the configuration of the test sample. Interface cables were connected to the available ports of the test unit. The effect of varying the position of the cables was investigated to find the configuration that produced maximum emissions. Cables were of the type and length specified in the individual requirements. The length of cable that produced maximum emissions was selected.

The equipment under test (EUT) was set up in a manner that represented its normal use, as shown in the setup photographs. Any special conditions required for the EUT to operate normally are identified in the comments that accompany the emissions tables.

The emissions data was taken with a spectrum analyzer or receiver. Incorporating the applicable correction factors for distance, antenna, cable loss and amplifier gain, the data was reduced as shown in the table below. The corrected data was then compared to the applicable emission limits. Preliminary and final measurements were taken in order to ensure that all emissions from the EUT were found and maximized.

CORRECTION FACTORS

The basic spectrum analyzer reading was converted using correction factors as shown in the highest emissions readings in the tables. For radiated emissions in dB μ V/m, the spectrum analyzer reading in dB μ V was corrected by using the following formula. This reading was then compared to the applicable specification limit.

SAMPLE CALCULATIONS		
	Meter reading	(dBμV)
+	Antenna Factor	(dB)
+	Cable Loss	(dB)
-	Distance Correction	(dB)
-	Preamplifier Gain	(dB)
=	Corrected Reading	(dBμV/m)

TEST INSTRUMENTATION AND ANALYZER SETTINGS

The test instrumentation and equipment listed were used to collect the emissions data. A spectrum analyzer or receiver was used for all measurements. Unless otherwise specified, the following table shows the measuring equipment bandwidth settings that were used in designated frequency bands. For testing emissions, an appropriate reference level and a vertical scale size of 10 dB per division were used.

MEASURING EQUIPMENT BANDWIDTH SETTINGS PER FREQUENCY RANGE			
TEST	BEGINNING FREQUENCY	ENDING FREQUENCY	BANDWIDTH SETTING
CONDUCTED EMISSIONS	150 kHz	30 MHz	9 kHz
RADIATED EMISSIONS	9 kHz	150 kHz	200 Hz
RADIATED EMISSIONS	150 kHz	30 MHz	9 kHz
RADIATED EMISSIONS	30 MHz	1000 MHz	120 kHz
RADIATED EMISSIONS	1000 MHz	>1 GHz	1 MHz

SPECTRUM ANALYZER/RECEIVER DETECTOR FUNCTIONS

The notes that accompany the measurements contained in the emissions tables indicate the type of detector function used to obtain the given readings. Unless otherwise noted, all readings were made in the "positive peak" detector mode. Whenever a "quasi-peak" or "average" reading was recorded, the measurement was annotated with a "QP" or an "Ave" on the appropriate rows of the data sheets. In cases where quasi-peak or average limits were employed and data exists for multiple measurement types for the same frequency then the peak measurement was retained in the report for reference, however the numbering for the affected row was removed and an arrow or carrot ("^") was placed in the far left-hand column indicating that the row above takes precedence for comparison to the limit. The following paragraphs describe in more detail the detector functions and when they were used to obtain the emissions data.

Peak

In this mode, the spectrum analyzer or receiver recorded all emissions at their peak value as the frequency band selected was scanned. By combining this function with another feature called "peak hold," the measurement device had the ability to measure intermittent or low duty cycle transient emission peak levels. In this mode the measuring device made a slow scan across the frequency band selected and measured the peak emission value found at each frequency across the band.

Quasi-Peak

Quasi-peak measurements were taken using the quasi-peak detector when the true peak values exceeded or were within 2 dB of a quasi-peak specification limit. Additional QP measurements may have been taken at the discretion of the operator.

Average

Average measurements were taken using the average detector when the true peak values exceeded or were within 2 dB of an average specification limit. Additional average measurements may have been taken at the discretion of the operator. If the specification or test procedure requires trace averaging, then the averaging was performed using 100 samples or as required by the specification. All other average measurements are performed using video bandwidth averaging. To make these measurements, the test engineer reduces the video bandwidth on the measuring device until the modulation of the signal is filtered out. At this point the measuring device is set into the linear mode and the scan time is reduced.