

Nemko Korea CO., Ltd.

300-2, Osan-Ri, Mohyun-Myun, Yongin-City, Kyungki-Do, KOREA

TEL:+82 31 322 2333 FAX:+82 31 322 2332

FCC EVALUATION REPORT FOR CERTIFICATION**Manufacturer :**

Sein Electronics Co., Ltd.
 133-3, Pyungchon-dong, Dongan-gu, Anyang-
 City, Kyunggi-do, Korea
 Attn : Mr. Ha-lyong, Jung

Dates of Issue : May 30, 2002**Test Report No. : NK2CE283****Test Site : Nemko Korea Co., Ltd.****EMC site, Korea****FCC ID****P3VSE-25S****Brand Name****SEIN****Contact Person**

Sein Electronics Co., Ltd.
 133-3, Pyungchon-dong, Dongan-gu, Anyang-city,
 Kyunggi-do, Korea
 Mr. Ha-lyong, Jung
 Telephone No. : +82 31 421 0389

FCC Rule Part(s):

Part 15 & 2

Classification :

FCC Class B Device

EUT Type:

Ambulatory Blood Pressure Monitor

Voltage :

Ni-MH(AA):4.8Vdc, LR6(AA):6.0Vdc

The device bearing the brand name and Fcc ID specified above has been shown to comply with the applicable technical standards as indicated in the measurement report and was tested in accordance with the measurement procedures specified in ANSI C63.4-1992.

I attest to the accuracy of data and all measurements reported herein were performed by me or were made under my supervision and are correct to the best of my knowledge and belief. I assume full responsibility for the completeness of these measurements and vouch for the qualifications of all persons taking them.

Tested By : Sung-hun, Baek
 Engineer

Reviewed By : Hyun-ho, Kim
 Manager & Chief Engineer

TABLE OF CONTENTS

SCOPE	3
INTRODUCTION (Site Description)	4
GENERAL TEST CONDITION	5
DESCRIPTION OF TEST (Conducted Emissions)	6
DESCRIPTION OF TEST (Radiated Emissions)	7
TEST DATA (Conducted Emissions)	8
TEST DATA (Radiated Emissions)	9
PLOTS OF EMISSION	10
Conducted Emissions Diagram	
SAMPLE CALCULATIONS	12
ACCURACY of MEASUREMENT	13
LIST of TEST EQUIPMENT	14
RECOMMENDATION/CONCLUSION	15
APPENDIX A - LABELLING REQUIREMENTS	16
APPENDIX B - CIRCUIT DIAGRAM	17
APPENDIX C - PHOTOGRAPHS of TEST SET-UP	18
APPENDIX D - EUT PHOTOGRAPHS	20
APPENDIX E - USER'S MANUAL	26
APPENDIX F – SCHEMATIC DIAGRAM	27

SCOPE

Measurement and determination of electromagnetic emissions (EME) of radio frequency devices including intentional and/or unintentional radiators for compliance with the technical rules and regulations of the Federal Communications Commission under FCC part 15.

Responsible Party* :	Sein Electronics Co., Ltd.
Contact Person :	Mr. Ha-lyong, Jung Tel : +82 31 421 0389/Fax: +82 31 424 6398 E-mail : hrjsein@unitel.co.kr
Manufacturer :	Title : Assistant Manager Sein Electronics Co., Ltd. 133-3, Pyungchon-dong, Dongan-gu, Anyang-city Kyunggi-do, Korea Tel : +82 31 421 0389/Fax: +82 31 424 6398

- FCC ID: P3VSE-25S
- Brand Name: SEIN
- EUT Type: Ambulatory Blood Pressure Monitor
- Voltage: Ni-MH(AA):4.8Vdc, LR6(AA):6.0Vdc

- Classification: FCC Class B
- Rule Part(s): FCC Part 15 & Part 2
- Test Procedure(s): ANSI C63.4 (1992)
- Dates of Test: May 13, 2002
- Place of Tests: Nemko Korea Co., Ltd. EMC Site
- Test Report No.: NK2CE283

* NOTE: Please refer to the duties and responsibilities of the Responsible Party attached.

INTRODUCTION

The measurement procedure described in American National Standard for Methods of Measurement of Radio-Noise Emissions from Low-Voltage Electrical and Electronic Equipment in the Range of 9kHz to 40GHz (ANSI C63.4-1992) was used in determining radiated and conducted emissions emanating from **Sein Electronics Co., Ltd.**

Fcc ID : **P3VSE-25S, Ambulatory Blood Pressure Monitor.**

These measurement tests were conducted at **Nemko Korea Co., Ltd. EMC Laboratory**.

The site address is 300-2, Osan-Ri, Mohyun-Myun, Yongin-City, Kyungki-Do, KOREA

The area of Nemko Korea Corporation LTD. EMC Test Site is located in a mountain area at 50 kilometers (30 miles) southeast and Seoul International Airport (Kimpo Airport), 30 kilometers (18miles) south-southeast from central Seoul.

It is located in the valley surrounded by mountains in all directions where ambient radio signal conditions are quiet and a favorable area to measure the radio frequency interference on open field test site for the computing and ISM devices manufactures.

The detailed description of the measurement facility was found to be in compliance with the requirements of § 2.948 according to ANSI C63.4 on October 19, 1992.



Nemko Korea Co., Ltd.
OPEN AREA TEST SITE
300-2, Osan-Ri, Mohyun-Myun, Yongin-City Kyungki-Do, KOREA 449-852
Tel)+82-31-322-2333
Fax)+82-31-322-2332

Fig. 1. The map above shows the Seoul in Korea vicinity area.

The map also shows Nemko Korea Co., Ltd. EMC Lab and Kimpo Airport.

GENERAL TEST CONDITIONS

Operating During Test

The EUT was connected to PC and tested at data receiving mode continuously.

Support Equipment

Notebook PC	LG Elec Model: CM2080	S/N: 5Y12FP74KC49
Printer	HP Model: C4562K	S/N: SG74T1C206 1.5m Shield D-sub cable
Mouse	Logitech Model: M-UB48	S/N: LZA71148729 2.0m shield Din cable
Ambulatory Blood Pressure Monitor	Sein Elec. FCC ID:P3VSE-25S	S/N: 998744 1.5m shield D-sub cable

EUT Information

Clock:	4MHz(XT1,XT3), 32.768kHz(XT2)
Chipset	KS3016(U1),
Display	6 digit
Measuring method:	Oscillometric method
Measuring range:	Systole 60-280 mmHg Diastole 30-160 mmHg Pulse rate 40-200 pul/min
Resolution	1 mmHg
Accuracy:	± 3 mmHg (Blood Pressure) ± 5% (Pulse rate)
Memory	512 measurements

DESCRIPTION OF TESTS

Conducted Emissions

The Line conducted emission test facility is located inside a 4 X 7 X 2.5 meter shielded enclosure.

It is manufactured by EM engineering. The shielding effectiveness of the shielded room is in accordance with MIL-STD-285 or NSA 65-6.

A 1mX 1.5M wooden table 0.8m height is placed 0.4m away from the vertical wall and 1.5m away from the side of wall of the shielded room

Rohde & Schwarz LISN and PMM LISN L3-32 50ohm/50uH line impedance stabilization network are bonded to the shielded room.

The EUT is powered from the Rohde & Schwarz LISN and the support equipment is powered from the PMM LISN. Power to the LISN s are filtered by high-current high insertion loss

Power line filters. The purpose of filter is to attenuate ambient signal interference and this filter is also bonded to shielded enclosure. All electrical cables are shielded by tinned copper zipper tubing with inner diameter of 1/2".

If DC power device, power will be derived from the source power supply it normally will be powered from and this supply lines will be connected to the LISNs,

All interconnecting cables more than 1 meter were shortened by non inductive bundling (serpentine fashion) to a 1 meter length.

Sufficient time for EUT, support equipment, and test equipment was allowed in order for them to warm up to their normal operating condition. The RF output of the LISN was connected to the spectrum analyzer to determine the frequency producing the maximum EME from the EUT. The spectrum was scanned from 450KHz to 30MHz with 20msec sweep time.

The frequency producing the maximum level was re-examined using the EMI test receiver. (Rohde & Schwarz ESCS30).

The detector function was set to CISPR quasi-peak mode.

The bandwidth of receiver was set to 9KHz. The EUT, support equipment, and interconnecting cables were arranged and manipulated to maximize each EME emission.

Each EME reported was calibrated using the R&S signal generator.

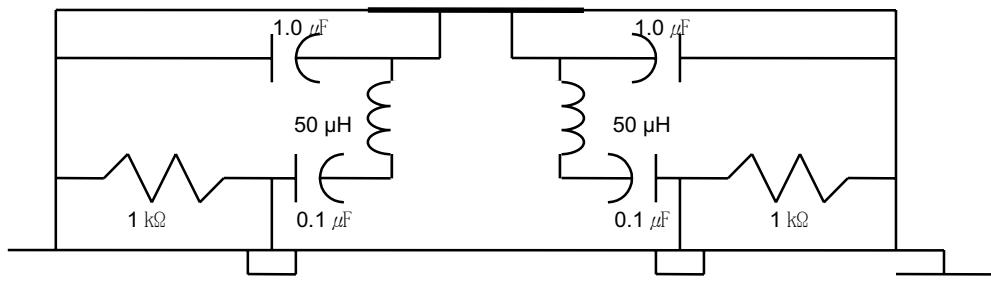


Fig. 2. LISN Schematic Diagram

DESCRIPTION OF TESTS

Radiated Emissions

Preliminary measurement were made indoors at 1 meter using broad band antennas, broadband amplifier, and spectrum analyzer to determine the frequency producing the maximum EME. Appropriate precaution was taken to ensure that all EME from the EUT were maximized and investigated. The system configuration, clock speed, mode of operation or video resolution, turntable azimuth with respect to the antenna was note for each frequency found. The spectrum was scanned from 30 to 1000MHz using Biconical log Antenna(ARA, LPB-2520/A). Above 1GHz, log periodic antenna (Rohde Schwarz HL025:upto 18GHz) was used.

Final Measurements were made outdoors at 3 or 10m test range using Logbicon Super Antenna(Schwarzbeck, VULB9166) or log periodic antenna.(Rohde Schwarz HL025)

The test equipment was placed on a wooden table.

Sufficient time for the EUT, support equipment, and test equipment was allowed in order for them to warm up to their normal operating condition.

Each frequency found during pre-scan measurements was reexamined and investigated using EMI test receiver.(ESCS30)

The detector function was set to CISPR quasi-peak mode and the bandwidth of the receiver was set to 120KHz or 1MHz depending on the frequency or type of signal.

The half wave dipole antenna was tuned to the frequency found during preliminary radiated measurements.

The EUT support equipment and interconnecting cables were re configured to the setup producing the maximum emission for the frequency and were placed on top of a 0.8m high non-metallic 1.0X 1.5 meter table.

The EUT, support equipment and interconnecting cables were re-arranged and manipulated to maximize each EME emission.

The turn table containing the system was rotated; the antenna height was varied 1 to 4meter and stopped at the azimuth or height producing the maximum emission.

Each EME reported was calibrated using the R/S signal generator.

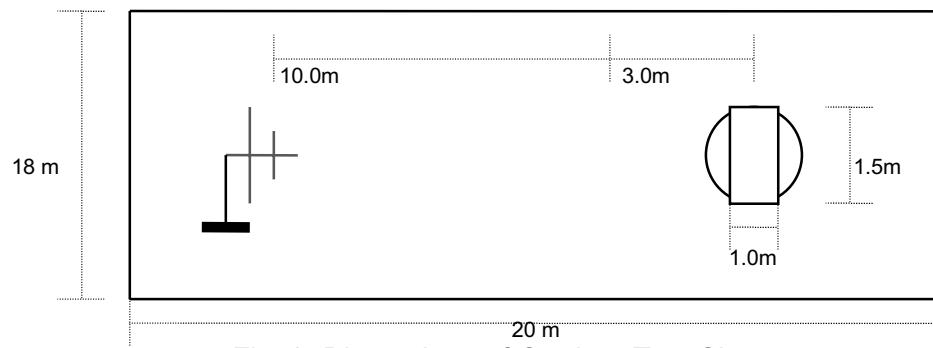


Fig. 3. Dimensions of Outdoor Test Site

TEST DATA

Conducted Emissions

Fcc ID : P3VSE-25S

Test Mode : tested at data receiving mode continuously

FREQ (MHz)	LEVEL(dB μ V)	LINE	LIMIT(μ V)	(μ V)	MARGIN(dB μ V)
1.06	29.7	N	250	30.55	18.3
2.06	28.0	N	250	25.12	20.0
3.52	29.9	N	250	31.26	18.1
5.84	31.4	L	250	37.15	16.6
9.23	33.2	N	250	45.71	14.8
12.41	40.6	N	250	107.15	7.4

Table 1. Line Conducted Emissions Tabulated Data

NOTES:

1. Measurements using CISPR quasi-peak mode
2. All modes of operation were investigated and the worst -case emission are reported. See attached Plots.
- 3.The limit for Class B device is 250 μ V from 450 kHz to 30MHz.
- 4.LINE : L =Line , N = Neutral

Baek Sung-hun

Tested by Sung-hun, Baek

TEST DATA

Radiated Emissions

Fcc ID : P3VSE-25S

Test Mode : tested at data receiving mode continuously

Frequency (MHz)	Reading (dB μ V/m)	Pol* (H/V)	AF+CL+Amp (dB)**	Result (dB μ V/m)	Limit (dB μ V/m)	Margin (dB μ V/m)
53.73	53.5	V	-21.5	32.0	40.0	8.0
139.29	47.5	V	-14.3	33.2	43.5	10.3
163.45	43.2	V	-12.9	30.3	43.5	13.2
248.89	43.7	V	-12.5	31.2	46.0	14.8
622.25	36.5	H	-3.0	33.5	46.0	12.5
748.25	37.6	V	0.3	37.9	46.0	8.1

*) Above 1GHz : Not significant or detectable.

Table 2. Radiated Measurements at 3meters

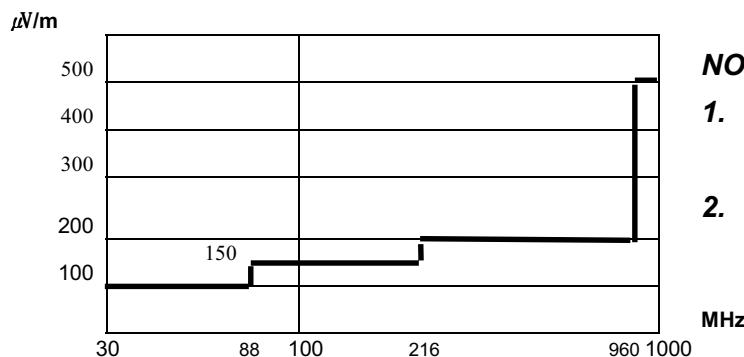


Fig. 3. Limits at 3 meters

NOTES:

1. All modes of operation were investigated the worst-case emission are reported.
2. The radiated limits are shown on Figure 4.
Above 1GHz the limit is 500 μ V/m.

* Pol. H =Horizontal V=Vertical

** AF+CL+Amp. = Antenna Factor + Cable Loss + Amplifier.


*** Measurements using CISPR quasi-peak mode. Above 1GHz, peak detector function mode is used using a resolution bandwidth of 1MHz and a video bandwidth of 1MHz. The peak level complies with the average limit. Peak mode is used with linearly polarized horn antenna and low-loss microwave cable.

Baek Sung-hun

Tested by Sung-hun, Baek


PLOTS OF EMISSIONS

- Conducted Emission at the Mains port(Line)

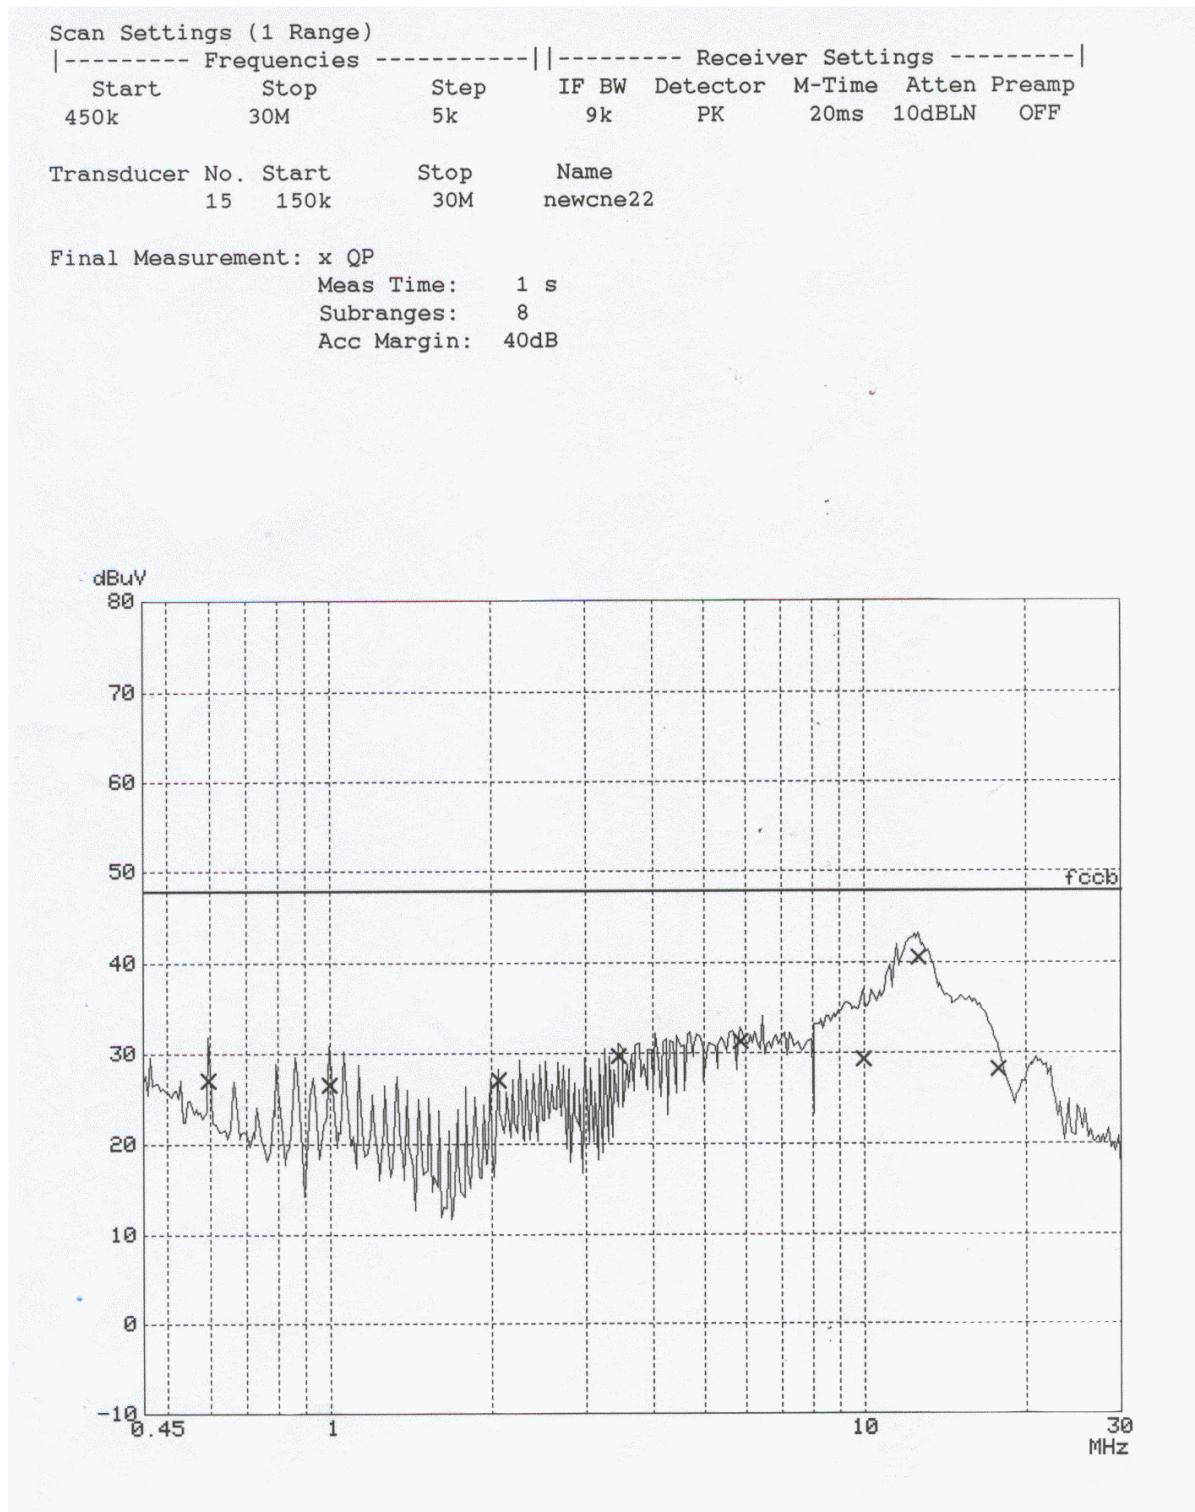

PLOTS OF EMISSIONS

- Conducted Emission at the Mains port(Neutral)

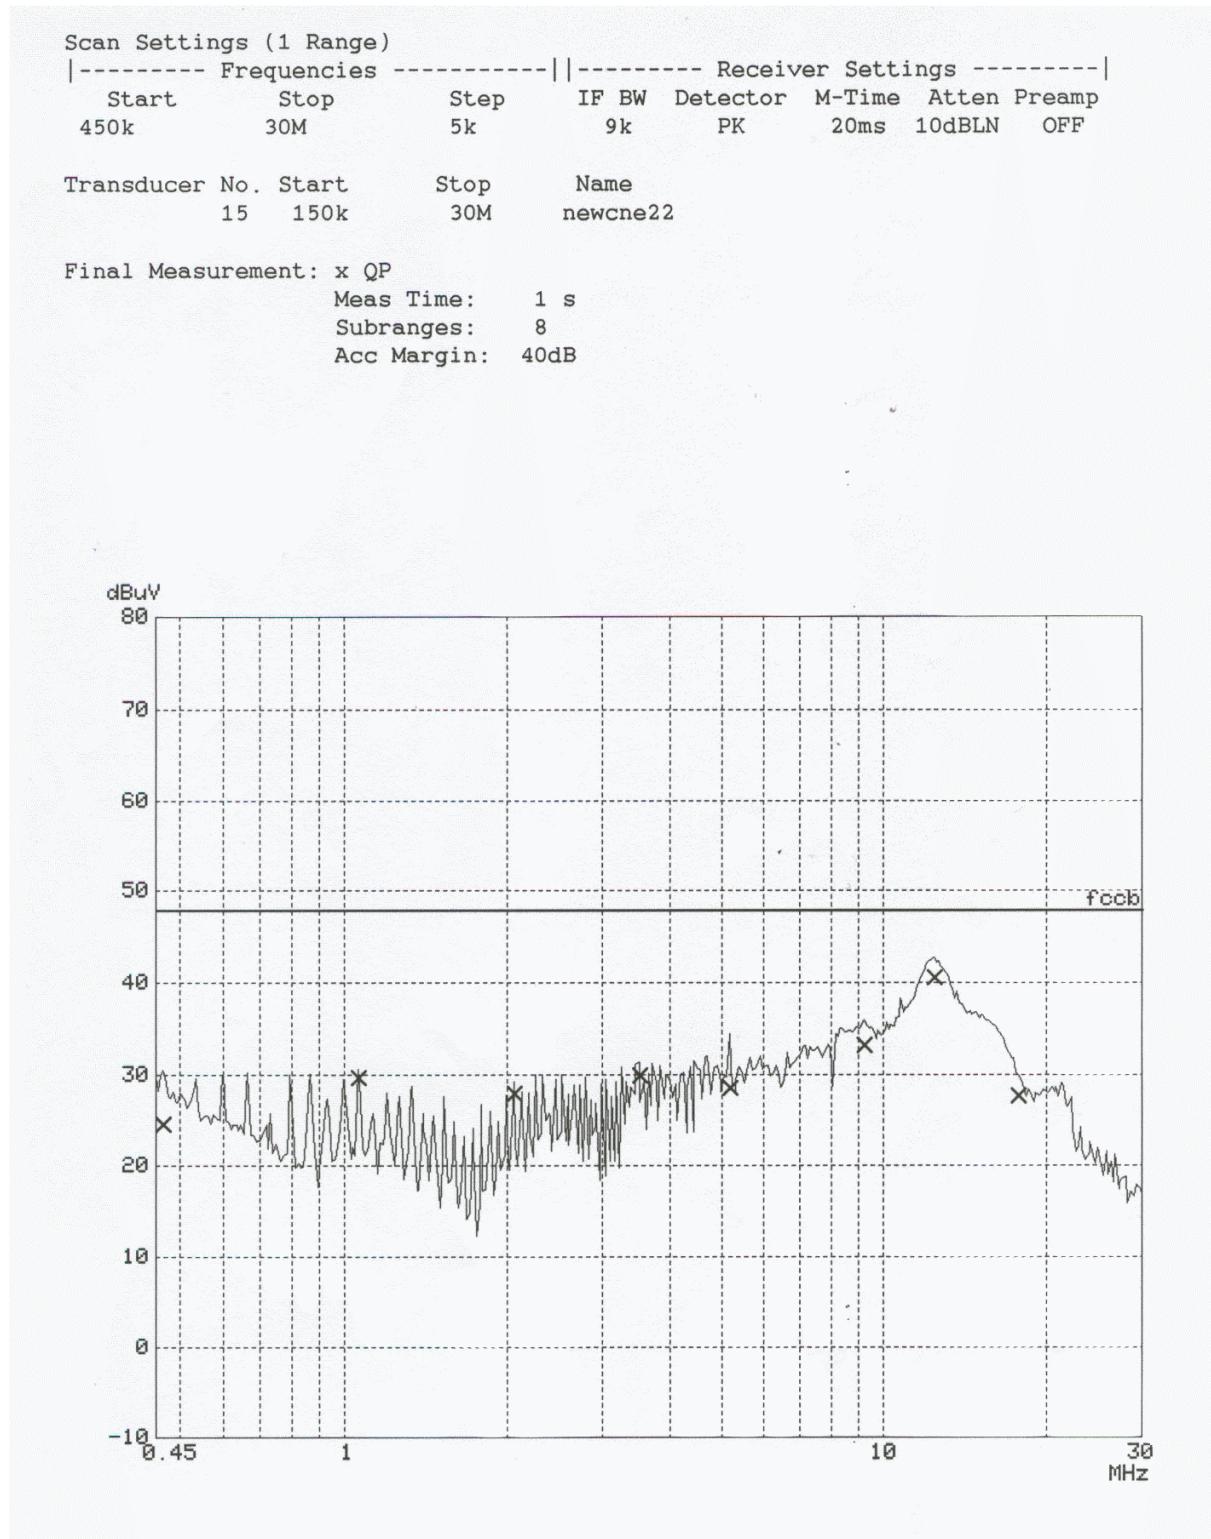

SAMPLE CALCULATIONS

$$\text{dB } \mu\text{V} = 20 \log_{10} (\mu\text{V}/\text{m})$$

$$\mu\text{V} = 10^{(\text{dB } \mu\text{V}/20)}$$

EX. 1.

@20.3 MHz

Class B limit = 250 μV = 48.0 dB μV

Reading = 40.8 dB μV (calibrated level)

$$10^{(40.8/20)} = 109.64 \mu\text{V}$$

$$\text{Margin} = 48.0 - 40.8 = 7.2$$

7.2 dB below limit

EX. 2.

@57.7 MHz

Class B limit = 100 $\mu\text{V}/\text{m}$ = 40.0 dB $\mu\text{V}/\text{m}$

Reading = 19.1 dB μV (calibrated level)

Antenna factor + Cable Loss = 10.12 dB

Total = 29.22 dB $\mu\text{V}/\text{m}$

$$\text{Margin} = 40.0 - 29.22 = 10.78$$

10.78 dB below the limit

ACCURACY OF MEASUREMENT

The Measurement Uncertainties stated were calculated in accordance with the requirements of NIST Technical Note 1297 with the confidence level of 95%

1. Radiation Uncertainty Calculation

<i>Contribution</i>	<i>Probability Distribution</i>	<i>Uncertainty(+/-dB)</i>
Antenna Factor	Normal (k=2)	± 0.5
Cable Loss	Normal (k=2)	± 0.04
Receiver Specification	Rectangular	± 2.0
Antenna directivity	Rectangular	± 1.0
Antenna Factor variation with Height		
Antenna Phase Center Variation		
Antenna Factor Frequency Interpolation		
Measurement Distance Variation		
Site Imperfections	Rectangular	± 2.0
Mismatch: Receiver VRC ri=0.3 Antenna VRC rR=0.1(Bi)0.4(Lp) Uncertainty Limits 20Log(1+/-ri rR)	U-Shaped	+ 0.25 / - 0.26
System Repeatability	Std.deviation	± 0.05
Repeatability of EUT	-	-
Combined Standard Uncertainty	Normal	± 1.77
Expended Uncertainty U	Normal (k=2)	± 3.5

2. Conducted Uncertainty Calculation

<i>Contribution</i>	<i>Probability Distribution</i>	<i>Uncertainty(+/-dB)</i>
Receiver Specification	Normal (k=2)	± 2.0
LISN coupling spec.	Normal (k=2)	± 0.4
Cable and input attenuator cal.	Rectangular	± 0.4
Mismatch: Receiver VRC ri=0.3 LISN vrc rg=0.1 Uncertainty Limits 20Log(1+/-ri rR)	U-Shaped	± 0.26
System Repeatability		
Repeatability of EUT		
Combined Standard Uncertainty		
Expended Uncertainty U		

TEST EQUIPMENT

No.	Instrument	Manufacturer	Model	Calibration Date
1	*Test Receiver	R & S	ESCS 30	2002.02
2	Test Receiver	PMM	PMM9000	2001.06
3	*Amplifier	HP	8447F	2001.11
4	*Amplifier	HP	8447F	2001.11
5	*Spectrum Analyzer	Advantest	R3265A	2002.03
6	*Biconical log Antenna	ARA	LPB-2520/A	2002.01
7	Log-Periodic Antenna	R & S	HL025	2002.01
8	Dipole Antenna	R & S	VHA9103	2001.05
9	Dipole Antenna	R & S	UHA9105	2001.05
11	Biconical Log Antenna	ARA	LPB-2520/A	2002.01
12	Asorbing Clamp	R & S	MDS21	2002.03
13	High Voltage Probe	R & S	ESH2-Z3	2001.09
14	Signal Generater	R & S	SMP02	2001.12
15	Matching Pad	R & S	RAM358.5414.02	2001.05
16	*LISN	R & S	ESH3-Z5	2001.10
17	*LISN	PMM	L3-9103	2001.06
18	*Position Controller	EM Eng.	N/A	N/A
19	*Turn Table	EM Eng.	N/A	N/A
20	*Antenna Mast	EM Eng.	N/A	N/A
21	*Anechoic Chamber	EM Eng.	N/A	N/A
22	*Shielded Room	EM Eng.	N/A	N/A

*) Test equipment used during the test


RECOMMENDATION/CONCLUSION

The data collected shows that the **Sein Electronics Co., Ltd.** Fcc ID : **P3VSE-25S, Ambulatory Blood Pressure Monitor.** complies with § 15.107, § 15.109 of the FCC Rules. The highest emission observed was at **12.41MHz** for conducted emissions with a margin of **7.4dB μ V** and at **53.73MHz** for radiated emissions with a margin of **8dB μ N/m**.

APPENDIX A – SAMPLE LABEL

Labelling Requirements

The sample label shown shall be *permanently affixed* at a conspicuous location on the device and be readily visible to the user at the time of purchase.

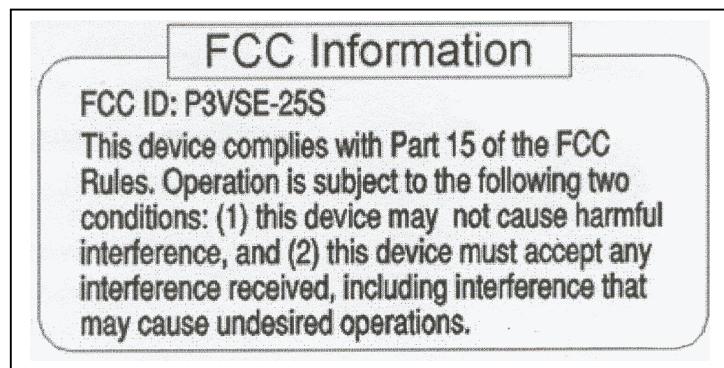

● FCC ID Location



APPENDIX B – CIRCUIT DIAGRAM

APPENDIX E – USER’S MANUAL

APPENDIX F – BLOCK DIAGRAM
