




SAR 장비 중간 점검 SAR Equipment Check		점검자 Prepared by	승인자 Approval by	
		이정호 이정호	Yongjin Jund [Signature]	
점검일자 Date:	2022-05-09			
사용장비 Used Equipment Lists				
자산번호 Assets No.	계측기명 Equipment Name	모델명 Model Name	일련번호 Serial No.	
E4-010002	ENA Network Analyzer	E5071C	MY46212858	
E4-010017	3.5mm Stanard Calibration Kit	85033E	MY39204493	
점검 장비 Equipment for Check				
자산번호 Assets No.	계측기명 Equipment Name	모델명 Model Name	일련번호 Serial No.	
E4-010130	System Validation Dipole	D2450V2	716	
● 점검방법: 해당 대역의 Tissue가 들어있는 Phantom에 Dipole를 인접한 후 점검				
주파수 Frequency[MHz]	입력레벨 Input Level	반사손실 Return Loss	이상유무 Pass / Fail	비고
2450	0	-22.247	PASS	

※ 중간점검을 진행한 장비에 문제가 발생한 경우에는 즉시 기술책임자 및 품질책임자에게 보고한다.

※ In the case when a problem for the result of equipment comes up, report this to Technical manager and Quality manager immediately.


Tr1 S11 Smith (Lin/Phase) Scale 1.000u [F1]

>1 2.4500000 GHz 77.205 mU 174.01 °

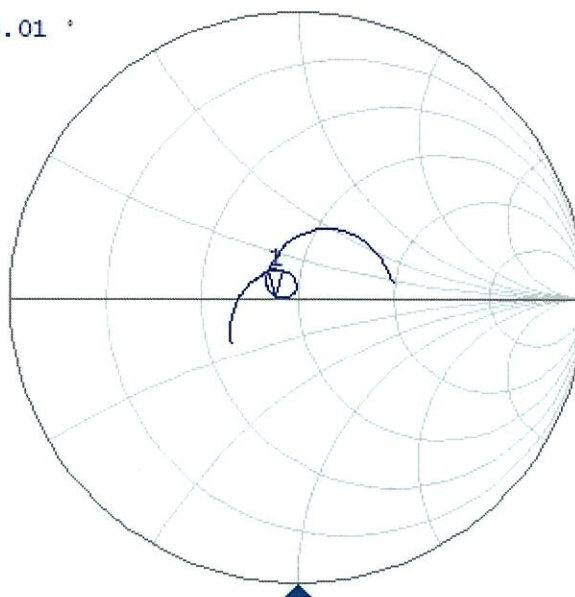

► Tr2 S11 Log Mag 5.000dB/ Ref -15.00dB [F1]

>1 2.4500000 GHz -22.247 dB

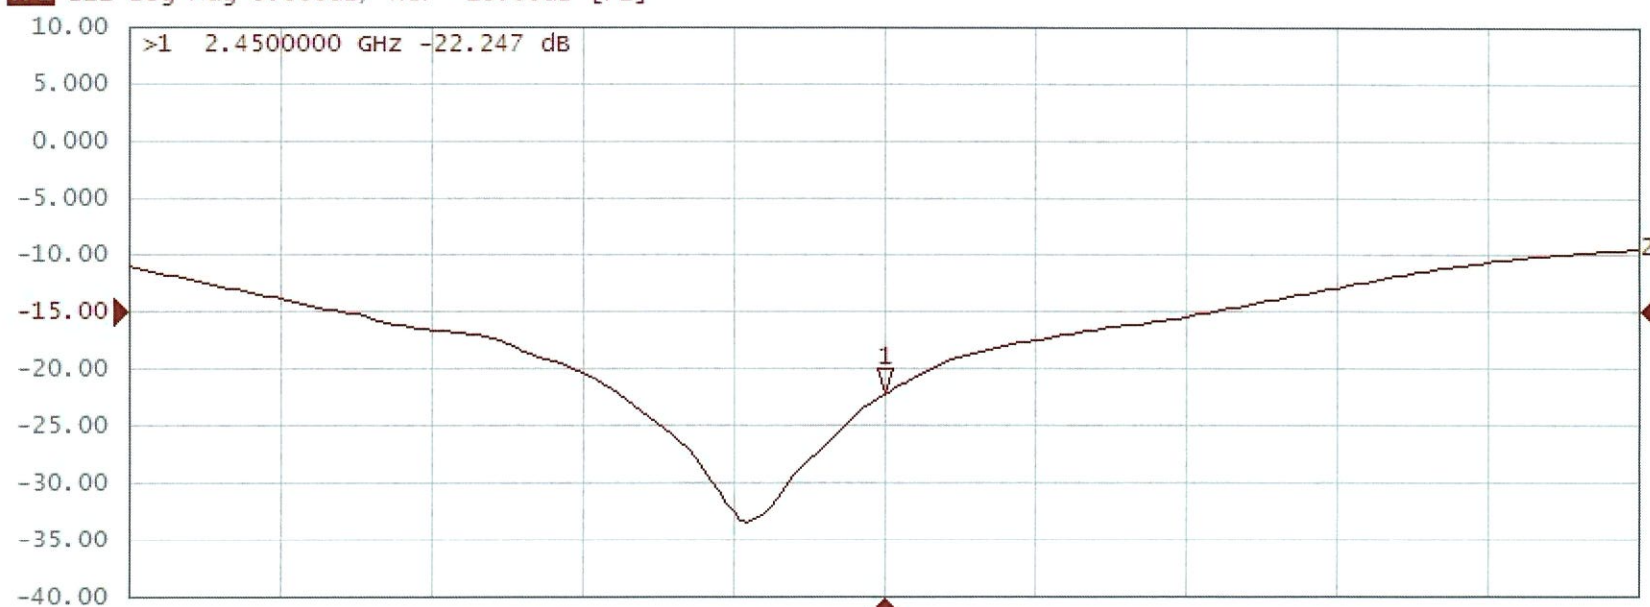

1 Start 2.25 GHz

IFBW 70 kHz

Stop 2.65 GHz Cor |

System

Print

Abort Printing

Printer Setup...

Invert Image

ON

Dump
Screen Image...Multiport Test Set
Setup

Misc Setup

Backlight

ON

Firmware
Revision

Service Menu

Help

Return