


EQUIPMENT TYPE	MFR	MODEL NUMBER	SERIAL NUMBER	LAST CAL	CAL DUE.
Spectrum Analyzer	Agilent	E4446A	MY5110000 3	05/19/2014	05/18/2015
Power meter	Anritsu	ML2495A	1005007	01/13/2014	01/12/2015


BT (Please see test plot in next page)

<i>FCC</i>	<i>by spectrum</i>		<i>unit: dBm</i>
1M	2402	2441	2480
<i>Peak</i>	8.57	8.83	8.71
2M	2402	2441	2480
<i>Peak</i>	7.29	7.68	7.90
3M	2402	2441	2480
<i>Peak</i>	7.65	8.17	8.24

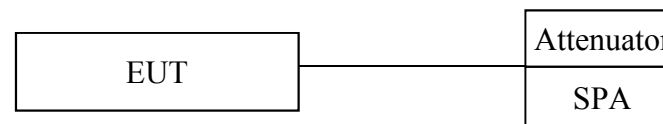


BLE


<i>FCC</i>	<i>by power meter</i>		<i>unit: dBm</i>
1M	2402	2442	2480
<i>Peak</i>	2.31	2.91	3.16
<i>Avg</i>	0.44	0.87	1.13




1M 2402

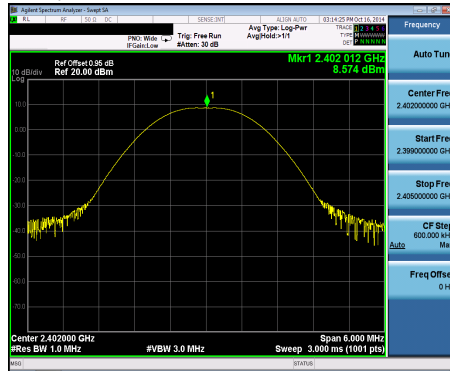


2M 2402

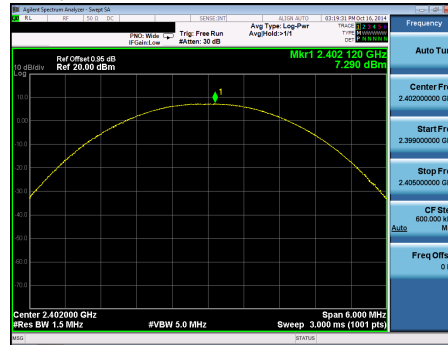


3M 2402

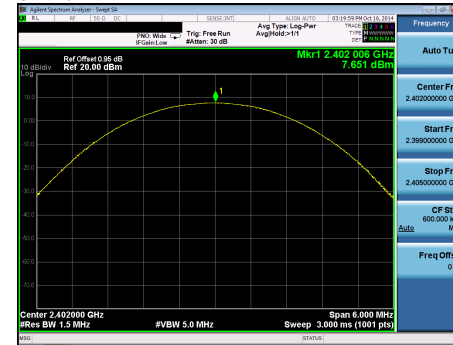

1M 2441

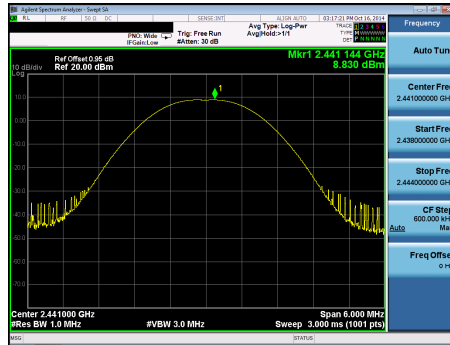


2M 2441

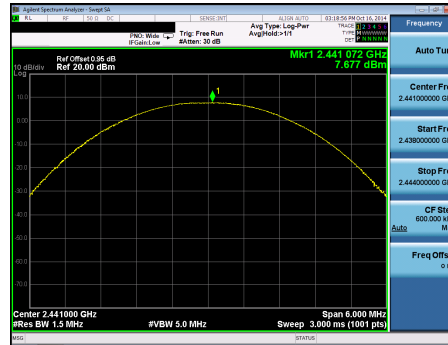


3M 2441



1M 2480

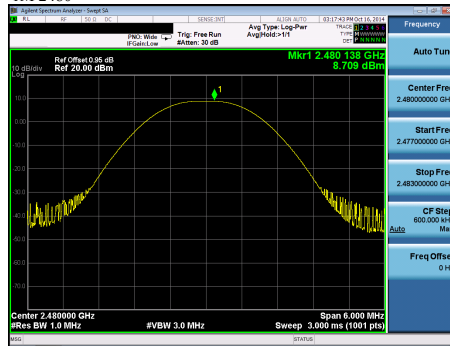

2M 2480

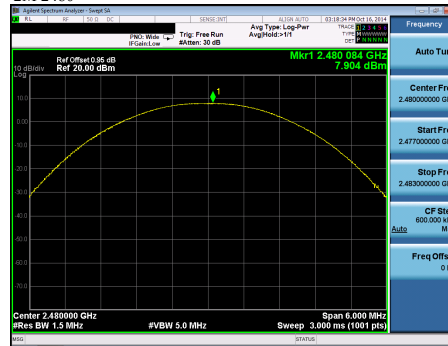

3M 2480

