




Test Setup Photo

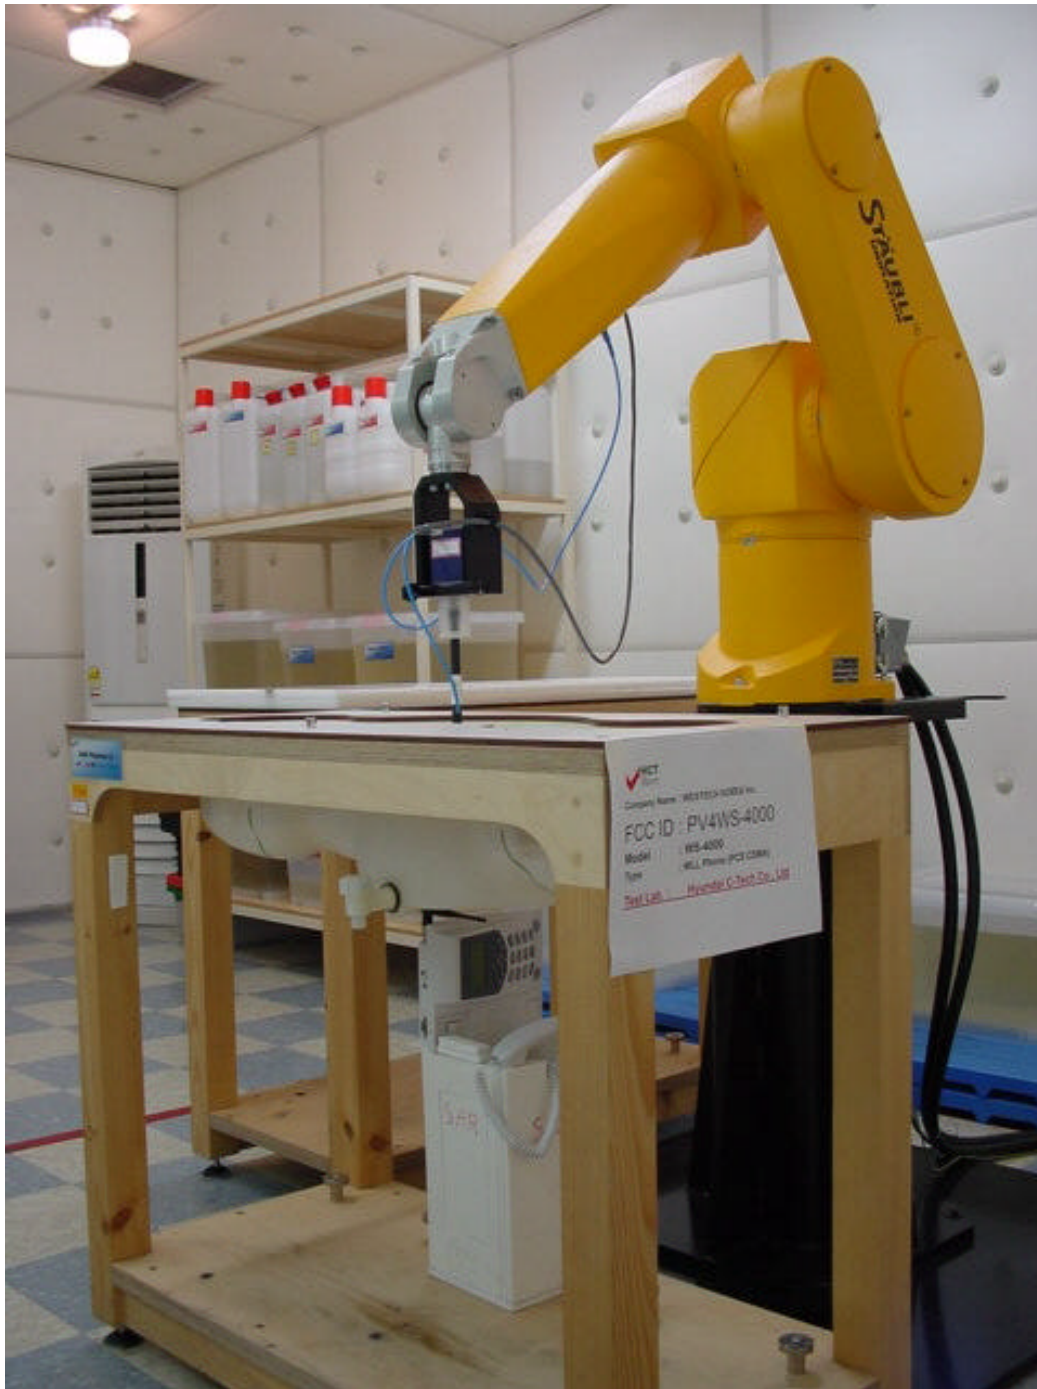

Test Setup Photo

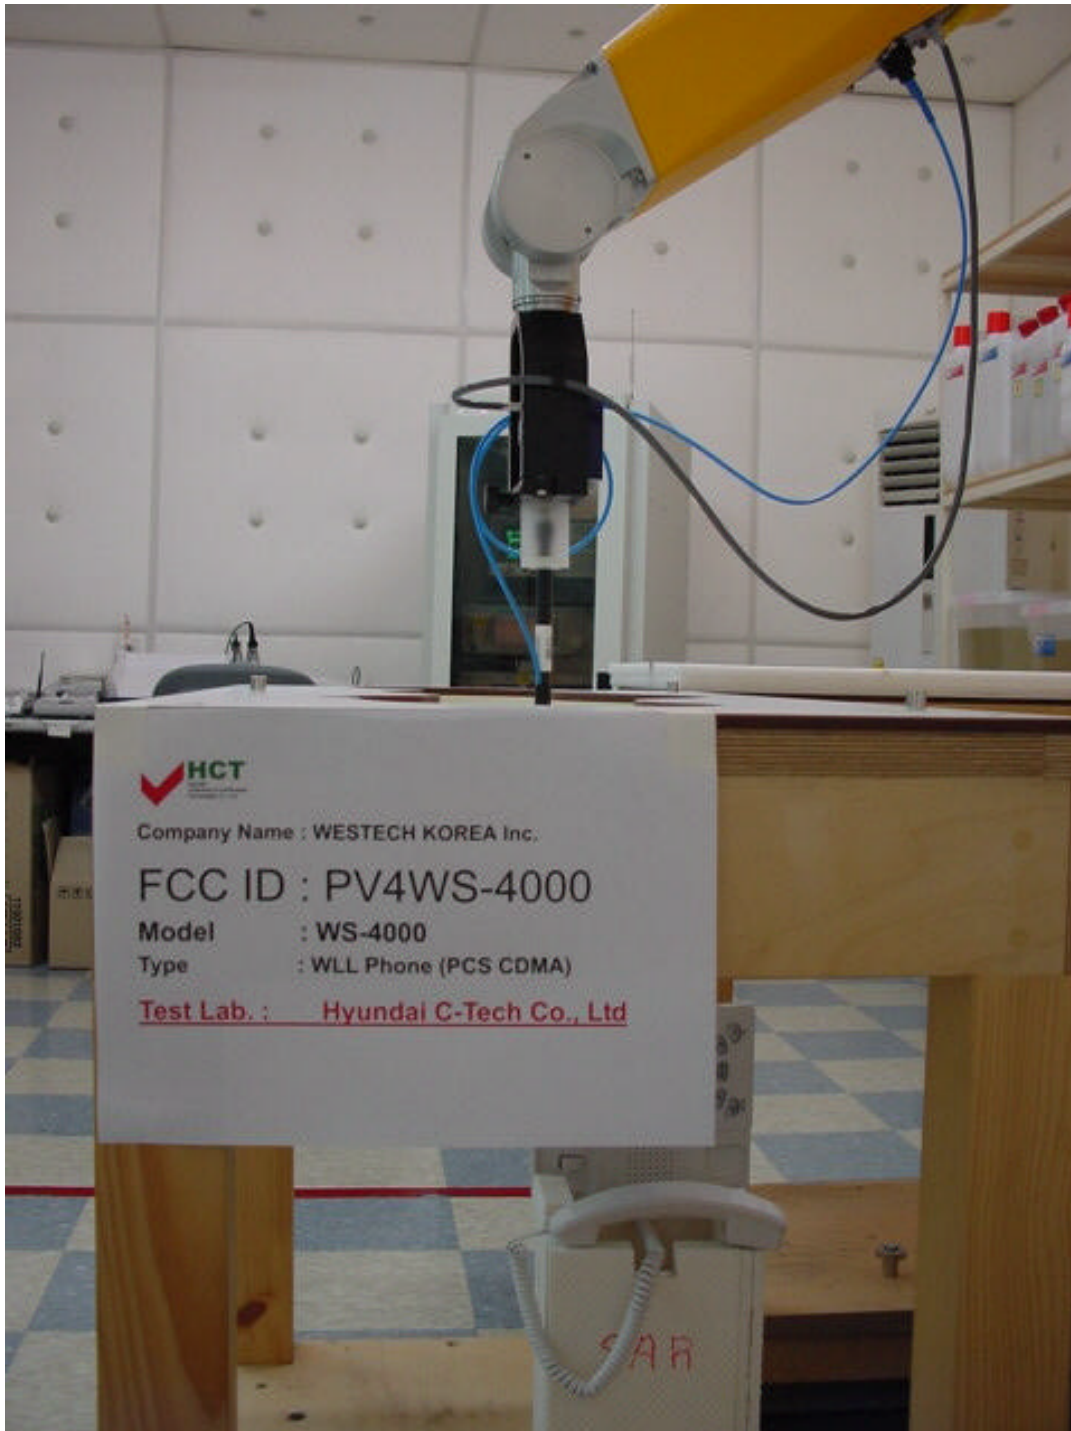


Test Setup Photo

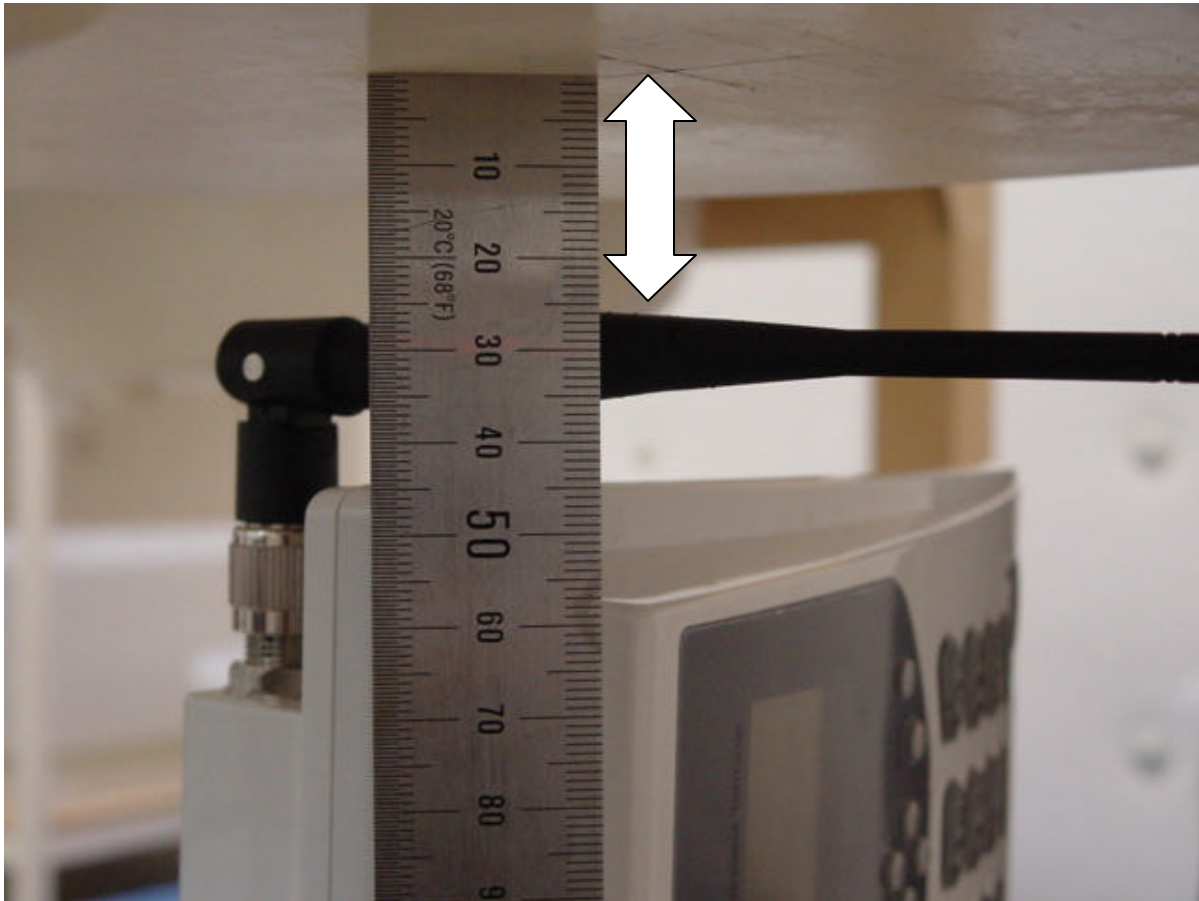

[Distance of 25 mm from the EUT]

Test Setup Photo

[835MHz Body Tissue Liquid Depth : 15cm]

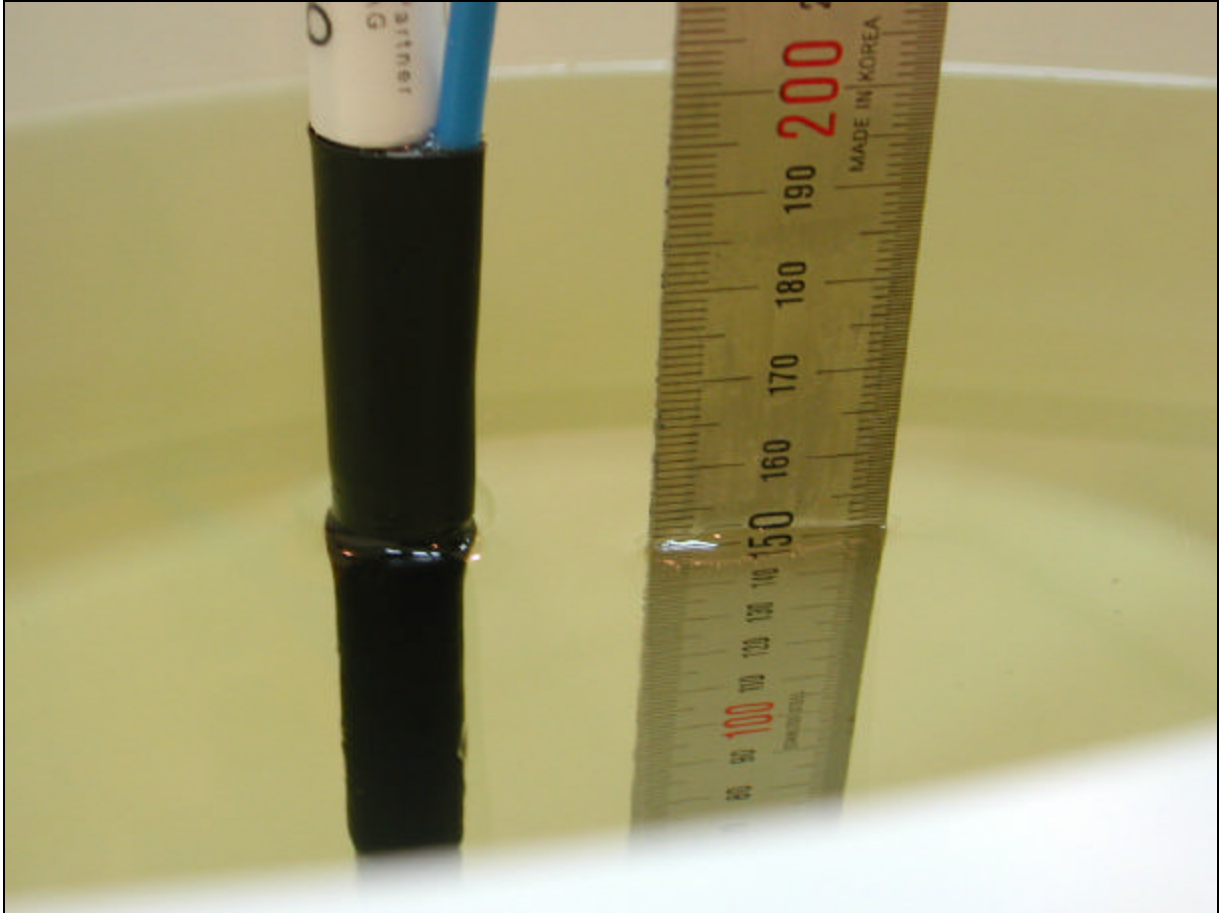

Test Setup Photo (Validation)

