
Calibration Data for the Report

Dosimetric Assessment of the Siemens S46 (FCC ID: PWX-S46) According to the FCC Requirements

November 05, 2001
IMST GmbH
Carl-Friedrich-Gauß-Str. 2
D-47475 Kamp-Lintfort

Customer
Siemens Information and Communication Mobile LLC
16745 West Bernado Drive Suite 400
San Diego-CA 92127

This report shall not be reproduced except in full without the written
approval of the testing laboratory.

Schmid & Partner Engineering AG

Zeughausstrasse 43, 8004 Zurich, Switzerland, Phone +41 1 245 97 00, Fax +41 1 245 97 79

Calibration Certificate

Dosimetric E-Field Probe

Type:

ET3DV6

Serial Number:

1579

Place of Calibration:

Zurich

Date of Calibration:

May 11, 2001

Calibration Interval:

12 months

Schmid & Partner Engineering AG hereby certifies, that this device has been calibrated on the date indicated above. The calibration was performed in accordance with specifications and procedures of Schmid & Partner Engineering AG.

Wherever applicable, the standards used in the calibration process are traceable to international standards. In all other cases the standards of the Laboratory for EMF and Microwave Electronics at the Swiss Federal Institute of Technology (ETH) in Zurich, Switzerland have been applied.

Calibrated by:

Nikolaus Morand

Approved by:

Blaise Khatja

**Schmid & Partner
Engineering AG**

Zeughausstrasse 43, 8004 Zurich, Switzerland, Telephone +41 1 245 97 00, Fax +41 1 245 97 79

Probe ET3DV6

SN:1579

Manufactured: May 7, 2001
Calibrated: May 11, 2001

Calibrated for System DASY3

ET3DV6 SN:1579

DASY3 - Parameters of Probe: ET3DV6 SN:1579

Sensitivity in Free Space

Diode Compression

NormX	1.73 $\mu\text{V}/(\text{V/m})^2$	DCP X	99 mV
NormY	1.72 $\mu\text{V}/(\text{V/m})^2$	DCP Y	99 mV
NormZ	1.94 $\mu\text{V}/(\text{V/m})^2$	DCP Z	99 mV


Sensitivity in Tissue Simulating Liquid

Head	450 MHz	$\epsilon_r = 43.5 \pm 5\%$	$\sigma = 0.87 \pm 10\%$ mho/m
ConvF X	7.38 extrapolated	Boundary effect:	
ConvF Y	7.38 extrapolated	Alpha	0.43
ConvF Z	7.38 extrapolated	Depth	2.18
Head	900 MHz	$\epsilon_r = 42 \pm 5\%$	$\sigma = 0.97 \pm 10\%$ mho/m
ConvF X	6.78 $\pm 7\%$ (k=2)	Boundary effect:	
ConvF Y	6.78 $\pm 7\%$ (k=2)	Alpha	0.47
ConvF Z	6.78 $\pm 7\%$ (k=2)	Depth	2.11
Head	1500 MHz	$\epsilon_r = 40.4 \pm 5\%$	$\sigma = 1.23 \pm 10\%$ mho/m
ConvF X	5.97 interpolated	Boundary effect:	
ConvF Y	5.97 interpolated	Alpha	0.53
ConvF Z	5.97 interpolated	Depth	2.03
Head	1800 MHz	$\epsilon_r = 40 \pm 5\%$	$\sigma = 1.40 \pm 10\%$ mho/m
ConvF X	5.57 $\pm 7\%$ (k=2)	Boundary effect:	
ConvF Y	5.57 $\pm 7\%$ (k=2)	Alpha	0.55
ConvF Z	5.57 $\pm 7\%$ (k=2)	Depth	1.99



Sensor Offset

Probe Tip to Sensor Center	2.7	mm
Optical Surface Detection	1.2 $\pm$ 0.2	mm

ET3DV6 SN:1579

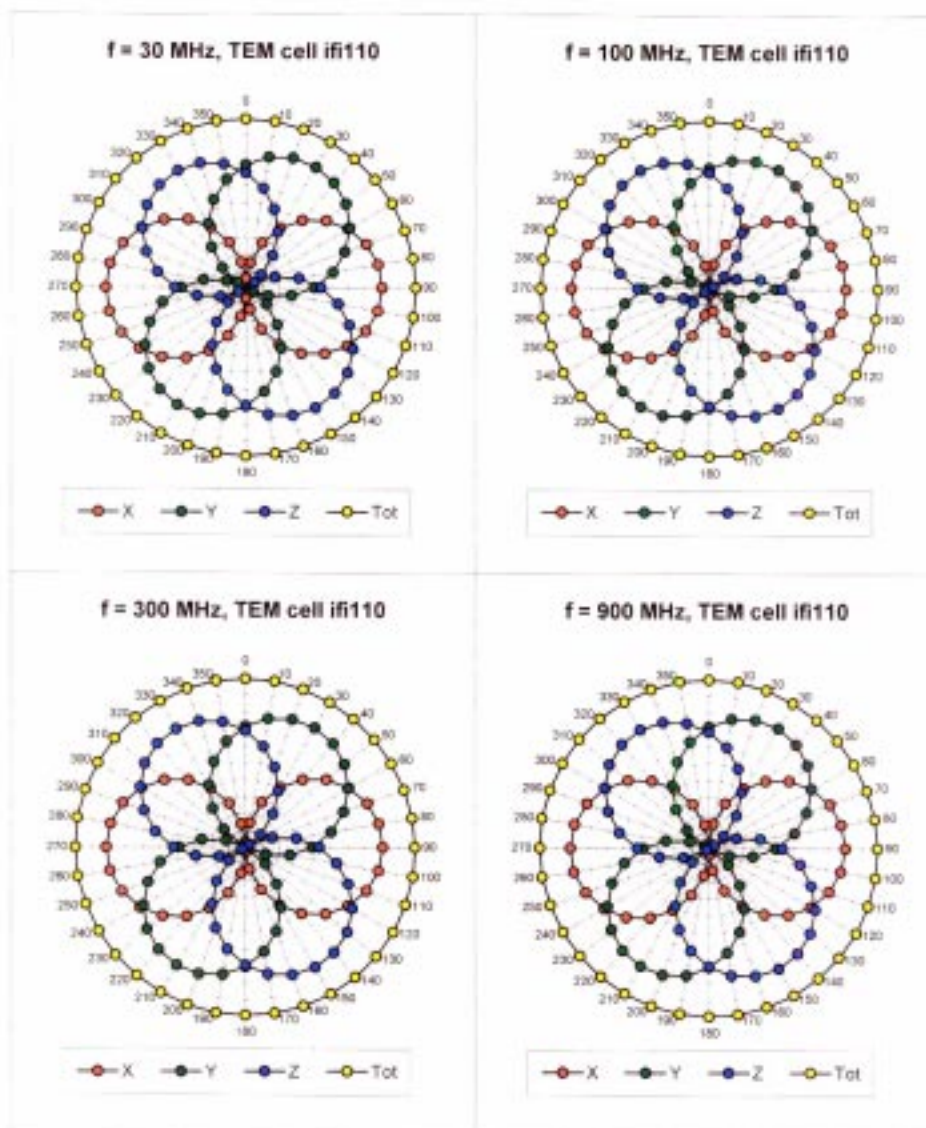Receiving Pattern (ϕ), $\theta = 0^\circ$ 


ET3DV6 SN:1579

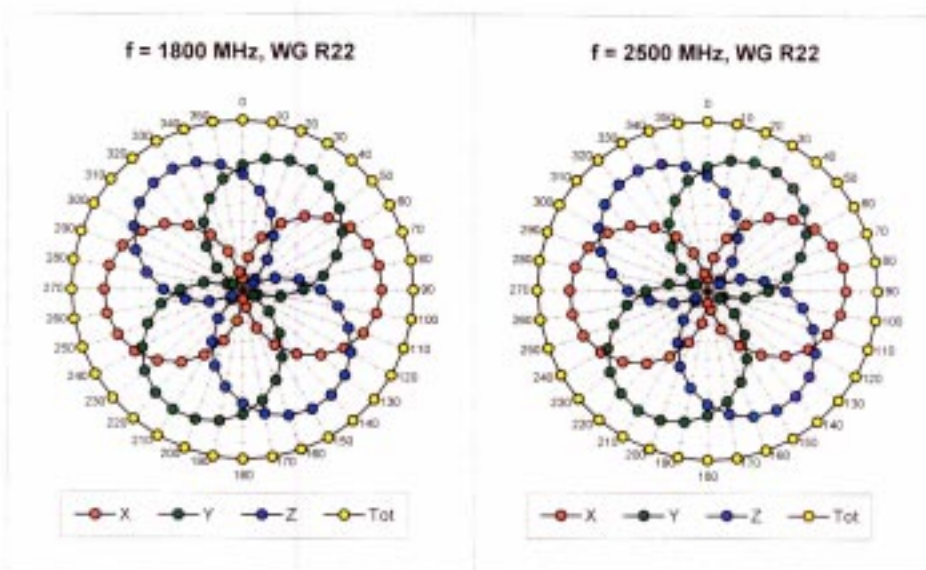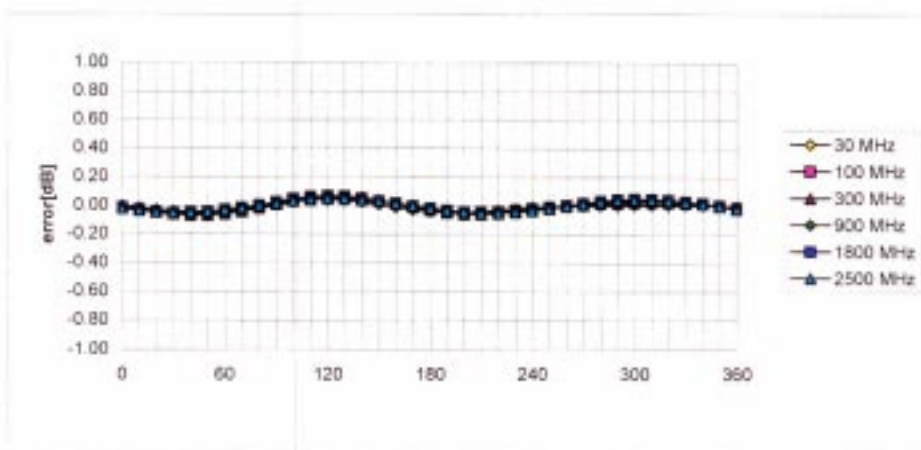Isotropy Error (ϕ), $\theta = 0^\circ$ 

ET3DV6 SN:1579

Frequency Response of E-Field



(TEM-Cell:ifi110, Waveguide R22)

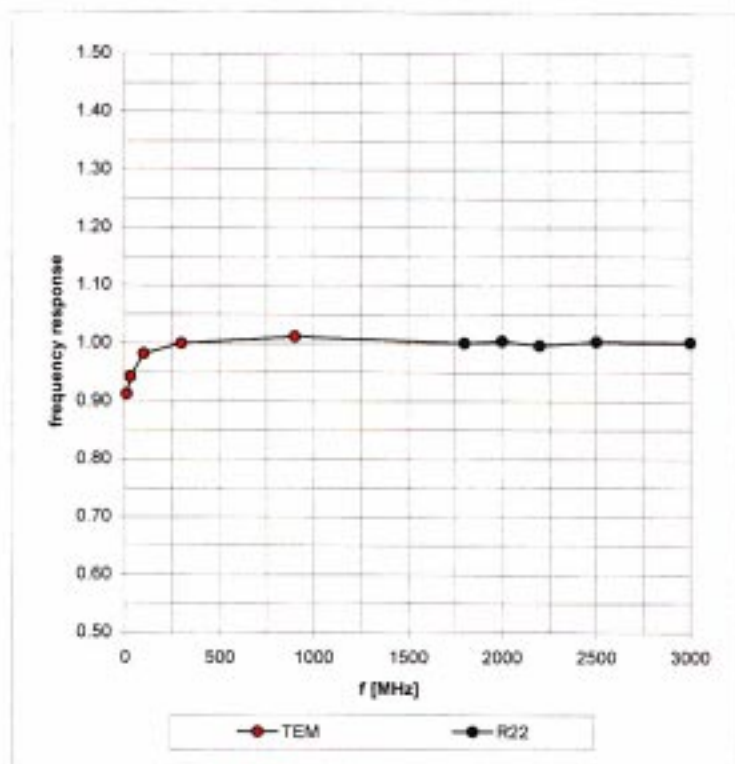

ET3DV6 SN:1579


Dynamic Range $f(\text{SAR}_{\text{brain}})$

(TEM-Cell:ifi110)

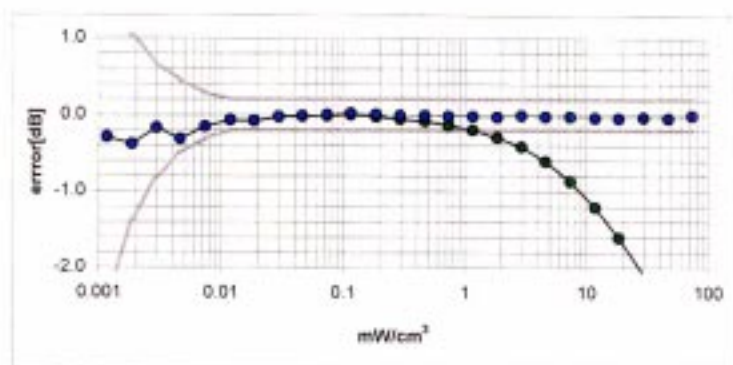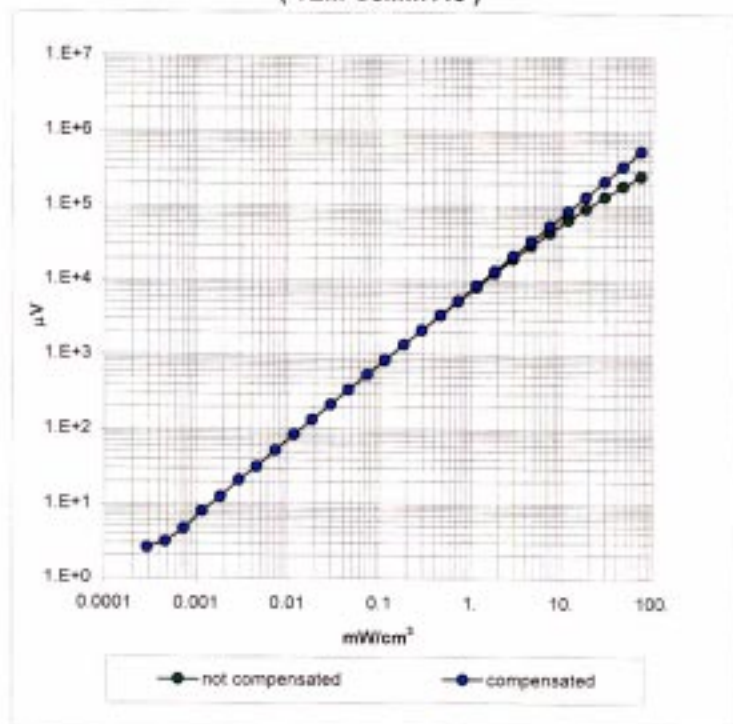


ET3DV6 SN:1579

Conversion Factor Assessment

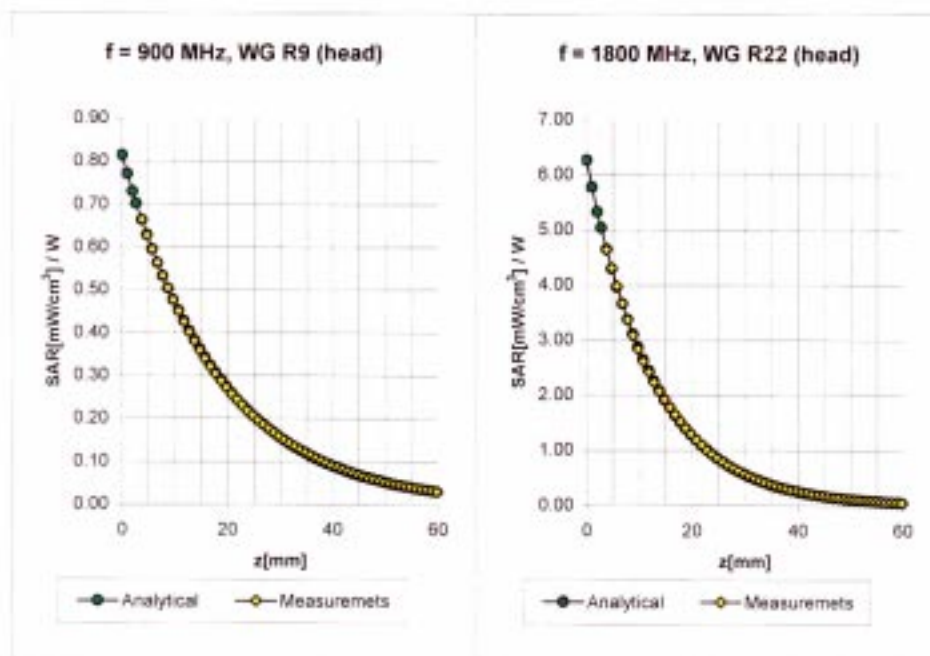

Head	900 MHz	$\epsilon_r = 42 \pm 5\%$	$\sigma = 0.97 \pm 10\% \text{ mho/m}$
ConvF X	6.78 $\pm 7\%$ (k=2)	Boundary effect:	
ConvF Y	6.78 $\pm 7\%$ (k=2)	Alpha	0.47
ConvF Z	6.78 $\pm 7\%$ (k=2)	Depth	2.11
Head	1800 MHz	$\epsilon_r = 40 \pm 5\%$	$\sigma = 1.40 \pm 10\% \text{ mho/m}$
ConvF X	5.57 $\pm 7\%$ (k=2)	Boundary effect:	
ConvF Y	5.57 $\pm 7\%$ (k=2)	Alpha	0.55
ConvF Z	5.57 $\pm 7\%$ (k=2)	Depth	1.99

ET3DV6 SN:1579

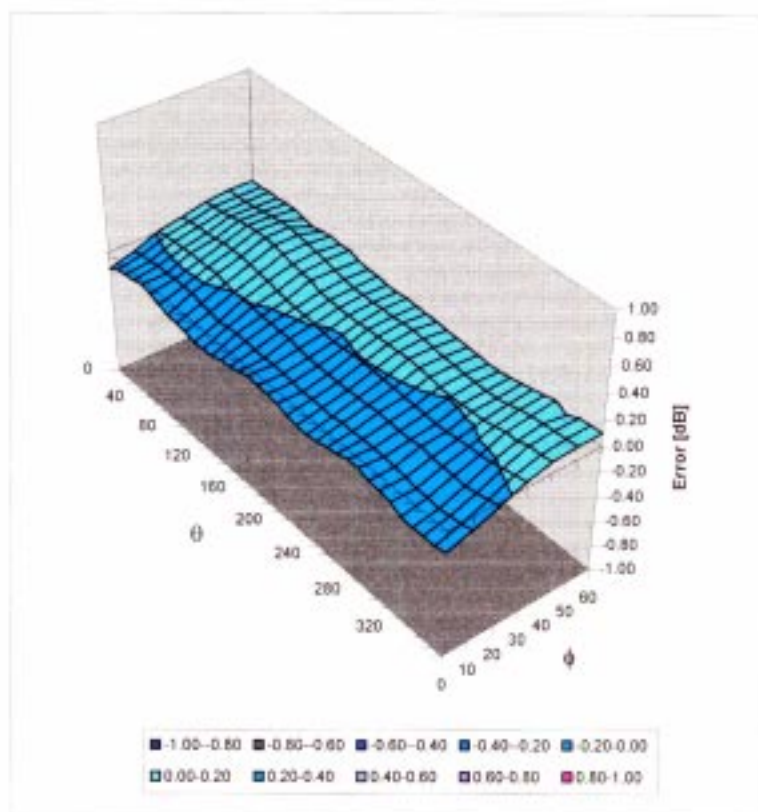Deviation from Isotropy in HSLError (θ, ϕ), $f = 900$ MHz

**Schmid & Partner
Engineering AG**

Zeughausstrasse 43, 8004 Zurich, Switzerland, Phone +41 1 245 97 00, Fax +41 1 245 97 79

Additional Conversion Factors

for Dosimetric E-Field Probe

Type:

ET3DV6

Serial Number:

1579

Place of Assessment:

Zurich

Date of Assessment:


August 22, 2001

Probe Calibration Date:

May 11, 2001

Schmid & Partner Engineering AG hereby certifies that conversion factor(s) of this probe have been evaluated on the date indicated above. The assessment was performed using the FDTD numerical code SEMCAD of Schmid & Partner Engineering AG. Since the evaluation is coupled with measured conversion factors, it has to be recalculated yearly, i.e., following the re-calibration schedule of the probe. The uncertainty of the numerical assessment is based on the extrapolation from measured value at 900 MHz or at 1800 MHz.

Assessed by:



Dosimetric E-Field Probe ET3DV6 SN:1579Conversion factor ($\pm$ standard deviation)

835 MHz	ConvF	$6.9 \pm 8\%$	$\epsilon_r = 41.5 \pm 5\%$ $\sigma = 0.90 \pm 10\%$ mho/m (head tissue)
835 MHz	ConvF	$6.6 \pm 8\%$	$\epsilon_r = 56.1 \pm 5\%$ $\sigma = 0.95 \pm 10\%$ mho/m (body tissue)
1900 MHz	ConvF	$5.4 \pm 8\%$	$\epsilon_r = 40.0 \pm 5\%$ $\sigma = 1.4 \pm 10\%$ mho/m (head tissue)
1900 MHz	ConvF	$4.9 \pm 8\%$	$\epsilon_r = 54.2 \pm 5\%$ $\sigma = 1.5 \pm 10\%$ mho/m (body tissue)

Schmid & Partner Engineering AG

Zeughausstrasse 43, 8004 Zurich, Switzerland, Phone +41 1 245 97 00, Fax +41 1 245 97 79

Calibration Certificate

835 MHz System Validation Dipole

Type:

D835V2

Serial Number:

437

Place of Calibration:

Zurich

Date of Calibration:

April 24, 2001

Calibration Interval:

24 months

Schmid & Partner Engineering AG hereby certifies, that this device has been calibrated on the date indicated above. The calibration was performed in accordance with specifications and procedures of Schmid & Partner Engineering AG.

Wherever applicable, the standards used in the calibration process are traceable to international standards. In all other cases the standards of the Laboratory for EMF and Microwave Electronics at the Swiss Federal Institute of Technology (ETH) in Zurich, Switzerland have been applied.

Calibrated by:

Nikolaus von der

Approved by:

Alain Kappeler

**Schmid & Partner
Engineering AG**

Zeughausstrasse 43, 8004 Zurich, Switzerland, Phone +41 1 245 97 00, Fax +41 1 245 97 79

DASY

Dipole Validation Kit

Type: D835V2

Serial: 437

Manufactured: December 15, 2000
Calibrated: April 24, 2001

1. Measurement Conditions

The measurements were performed in the flat section of the new generic twin phantom filled with head simulating solution of the following electrical parameters at 835 MHz:

Relative Dielectricity	43.0	$\pm 5\%$
Conductivity	0.91 mho/m	$\pm 5\%$

The DASY3 System (Software version 3.1c) with a dosimetric E-field probe ET3DV6 (SN:1507, Conversion factor 6.27 at 900 MHz) was used for the measurements.

The dipole was mounted on the small tripod so that the dipole feedpoint was positioned below the center marking of the flat phantom section and the dipole was oriented parallel to the body axis (the long side of the phantom). The standard measuring distance was 15mm from dipole center to the solution surface. The included distance holder was used during measurements for accurate distance positioning.

The coarse grid with a grid spacing of 15mm was aligned with the dipole. The 5x5x7 fine cube was chosen for cube integration. Probe isotropy errors were cancelled by measuring the SAR with normal and 90° turned probe orientations and averaging.

The dipole input power (forward power) was 250mW $\pm 3\%$. The results are normalized to 1W input power.

2. SAR Measurement

Standard SAR-measurements were performed with the phantom according to the measurement conditions described in section 1. The results have been normalized to a dipole input power of 1W (forward power). The resulting averaged SAR-values are:

averaged over 1 cm ³ (1 g) of tissue:	10.7 mW/g
averaged over 10 cm ³ (10 g) of tissue:	6.84 mW/g

Note: If the liquid parameters for validation are slightly different from the ones used for initial calibration, the SAR-values will be different as well. The estimated sensitivities of SAR-values and penetration depths to the liquid parameters are listed in the DASY Application Note 4: "SAR Sensitivities".

3. Dipole Impedance and Return Loss

The impedance was measured at the SMA-connector with a network analyzer and numerically transformed to the dipole feedpoint. The transformation parameters from the SMA-connector to the dipole feedpoint are:

Electrical delay:	1.458 ns	(one direction)
Transmission factor:	0.985	(voltage transmission, one direction)

The dipole was positioned at the flat phantom sections according to section 1 and the distance holder was in place during impedance measurements.

Feedpoint impedance at 835 MHz:	$\text{Re}\{Z\} = $ 52.8 Ω
---------------------------------	---

	$\text{Im}\{Z\} = $ -0.8 Ω
--	---

Return Loss at 835 MHz	-30.7 dB
------------------------	-----------------

4. Handling

The dipole is made of standard semirigid coaxial cable. The center conductor of the feeding line is directly connected to the second arm of the dipole. The antenna is therefore short-circuited for DC-signals.

Do not apply excessive force to the dipole arms, because they might bend. If the dipole arms have to be bent back, take care to release stress to the soldered connections near the feedpoint; they might come off.


After prolonged use with 100W radiated power, only a slight warming of the dipole near the feedpoint can be measured.


04/24/01

Validation Dipole D835V2 SN:437, d = 15 mm

Frequency: 835 MHz; Antenna Input Power: 250 [mW]
Generic Twin Phantom; Flat Section; Grid Spacing: Dx = 15.0, Dy = 15.0, Dz = 10.0
Probe: ET3DV6 - SN1507; ConvF(6.27 & 27.6 27) at 900 MHz; IEEE1528 835 MHz; $\sigma = 0.51$ mho/m $\epsilon_r = 43.0$ $\rho = 1.00$ g/cm³
Cubes (2): Peak: 4.26 mW/g ± 0.02 dB, SAR (1g): 2.67 mW/g ± 0.01 dB, SAR (10g): 1.71 mW/g ± 0.01 dB. (Worst-case extrapolation)
Penetration depth: 12.0 (10.7, 13.6) [mm]
Powerdrift: 0.02 dB



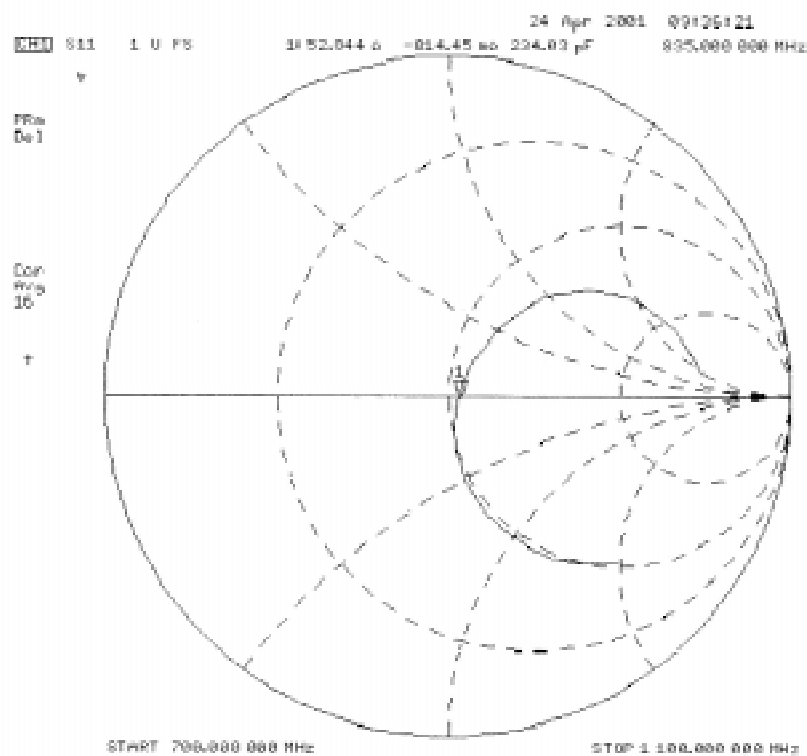

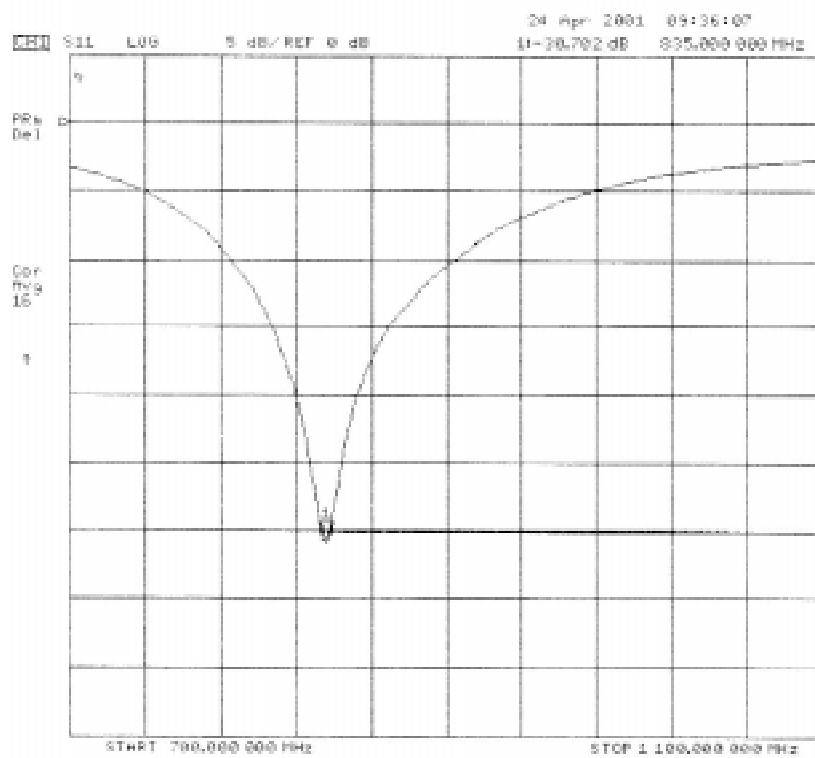

**Schmid & Partner
Engineering AG**

Zeughausstrasse 43, 8004 Zurich, Switzerland, Phone +41 1 245 97 00, Fax +41 1 245 97 79

Calibration Certificate**835 MHz System Validation Dipole (Muscle Tissue)**

Type:

D835V2

Serial Number:

437

Place of Calibration:

Zurich

Date of Calibration:

August 23, 2001

Calibration Interval:

24 months

Schmid & Partner Engineering AG hereby certifies, that this device has been calibrated on the date indicated above. The calibration was performed in accordance with specifications and procedures of Schmid & Partner Engineering AG.

Wherever applicable, the standards used in the calibration process are traceable to international standards. In all other cases the standards of the Laboratory for EMF and Microwave Electronics at the Swiss Federal Institute of Technology (ETH) in Zurich, Switzerland have been applied.

Calibrated by:



Approved by:

