



**Hearing Aid Compatibility (HAC)
RF Emissions Test Report
for
ZTE CORPORATION
on the
ZTE C78 CDMA1X Digital Mobile Phone**

Report No. : HA830102
Trade Name : ZTE
Model Name : ZTE C78
FCC ID : Q78-ZTEC78
Date of Testing : Apr. 02, 2008
Date of Report : Apr. 09, 2008
Date of Review : Apr. 09, 2008

- **Results Summary : M Category = M4**
- The test results refer exclusively to the presented test model/sample only.
- Without written approval of SPORTON International Inc., the test report shall not be reproduced except in full.
- Report Version: Rev.01

SPORTON International Inc.

No.52, Hwa-Ya 1st RD., Hwa Ya Technology Park, Kwei-Shan Hsiang, TaoYuan Hsien, Taiwan, R.O.C.



Table of Contents

- 1. Statement of Compliance 1**
- 2. Administration Data 2**
 - 2.1 Testing Laboratory 2
 - 2.2 Detail of Applicant 2
 - 2.3 Detail of Manufacturer 2
 - 2.4 Application Details 2
- 3. General Information 3**
 - 3.1 Description of Device Under Test (DUT) 3
 - 3.2 Applied Standards: 4
 - 3.4 Test Conditions: 5
 - 3.4.1 Ambient Condition 5
 - 3.4.2 Test Configuration 5
- 4. Hearing Aid Compliance (HAC) 6**
 - 4.1 Introduction 6
- 5. HAC Measurement Setup 7**
 - 5.1 DASY4 E-Field and H-Field Probe System 8
 - 5.2 System Specification 9
 - 5.2.1 ER3DV6 E-Field Probe Description 9
 - 5.2.2 H3DV6 H-Field Probe Description 9
 - 5.2.3 Probe Tip Description 10
 - 5.3 DATA Acquisition Electronics (DAE) 12
 - 5.4 Robot 12
 - 5.5 Measurement Server 12
 - 5.6 Phone Positioner 13
 - 5.6.1 Test Arch Phantom 14
 - 5.7 Data Storage and Evaluation 15
 - 5.7.1 Data Storage 15
 - 5.7.2 Data Evaluation 15
 - 5.8 Test Equipment List 17
- 6. Uncertainty Assessment 18**
- 7. HAC Measurement Evaluation 20**
 - 7.1 Purpose of System Performance check 20
 - 7.2 System Setup 20
 - 7.3 Validation Results 22
- 8. RF Field Probe Modulation Factor 23**
- 9. Description for DUT Testing Position 26**
- 10. RF Emissions Test Procedure 27**
- 11. HAC Test Results 28**
 - 11.1 E-Field Emission 28
 - 11.2 H-Field Emission 28
- 12. References 29**

- Appendix A - System Performance Check Data
- Appendix B - HAC Measurement Data
- Appendix C - Calibration Date
- Appendix D - CDMA2000 1xRTT Test Modes for HAC
- Appendix E - Setup Photographs



1. Statement of Compliance

The Hearing Aid Compliance (HAC) maximum results found during testing for the ZTE CORPORATION ZTE C78 CDMA1X Digital Mobile Phone ZTE C78 are as follows (with expanded uncertainty $\pm 29.4\%$ for E-field and $\pm 21.8\%$ for H-field):

Band	E-Field (V/m)	M Rating	H-Field (A/m)	M Rating
CDMA2000 Cellular	117	M4	0.202	M4
CDMA2000 AWS	54.5	M4	0.157	M4
CDMA2000 PCS	43.9	M4	0.117	M4
Remark : HAC test data for part 27 AWS band are provided for reference only, that they are not part of requirements for equipment authorization under part 20.19.				

They are in compliance with HAC limits specified in guidelines FCC 47CFR §20.19 and ANSI Standard ANSI C63.19 for HAC Rated category M3.

Results Summary : M Category = M4

Approved by

Roy Wu
Manager



2. Administration Data

2.1 Testing Laboratory

Company Name : Sporton International Inc.
Department : Antenna Design/SAR
Address : No.52, Hwa-Ya 1st RD., Hwa Ya Technology Park, Kwei-Shan Hsiang,
TaoYuan Hsien, Taiwan, R.O.C.
Telephone Number : 886-3-327-3456
Fax Number : 886-3-327-0973

2.2 Detail of Applicant

Company Name : ZTE CORPORATION
Address : ZTE Plaza, Keji Road South, Hi-Tech Industrial Park, Nanshan District,
Shenzhen, Guangdong, 518057, P.R.China

2.3 Detail of Manufacturer

Company Name : ZTE CORPORATION
Address: ZTE Plaza, Keji Road South, Hi-Tech Industrial Park, Nanshan District,
Shenzhen, Guangdong, 518057, P.R.China

2.4 Application Details

Date of reception of application: Mar. 01, 2008
Start of test : Apr. 02, 2008
End of test : Apr. 02, 2008



3. General Information

3.1 Description of Device Under Test (DUT)

DUT Type :	ZTE C78 CDMA1X Digital Mobile Phone
Trade Name :	ZTE
Model Name :	ZTE C78
FCC ID :	Q78-ZTEC78
Tx Frequency :	CDMA2000 Cellular : 824 ~ 849 MHz CDMA2000 AWS : 1710 ~ 1755 MHz CDMA2000 PCS : 1850 ~1910 MHz
Rx Frequency :	CDMA2000 Cellular : 869 ~ 894 MHz CDMA2000 AWS : 2110 ~ 2155 MHz CDMA2000 PCS : 1930 ~1990 MHz
Antenna Type :	Fixed Internal
HW Version :	c73B
SW Version :	ZTEC78V1.0.0B02
Maximum Output Power to Antenna :	<for HAC> CDMA2000 Cellular : 23.97 dBm CDMA2000 AWS : 24.41 dBm CDMA2000 PCS : 24.25 dBm <for EMC> CDMA2000 Cellular : 23.95 dBm CDMA2000 AWS : 24.40 dBm CDMA2000 PCS : 24.06 dBm
Type of Modulation :	QPSK



3.2 Applied Standards:

The ANSI Standard ANSI C63.19:2006 represents performance requirements for acceptable interoperability of hearing aids with wireless communications devices. When these parameters are met, a hearing aid operates acceptably in close proximity to a wireless communications device.

The following AWF factors shall be used for the standard transmission protocols:

Standard	Technology	AWF (dB)
TIA/EIA/IS-2000	CDMA	0
TIA/EIA-136	TDMA (50 Hz)	0
J-STD-007	GSM (217)	-5
T1/T1P1/3GPP	UMTS (WCDMA)	0
iDENTM	TDMA (22 and 11 Hz)	0

Table 3.1 Articulation Weighting Factor (AWF)

Category	Telephone RF Parameters				
	Near Field	AWF	E-Field Emissions	H-Field Emissions	
< 960 MHz					
Category M1	0	631.0 – 1122.0	V/m	1.91 – 3.39	A/m
	-5	473.2 – 841.4	V/m	1.43 – 2.54	A/m
Category M2	0	354.8 – 631.0	V/m	1.07 – 1.91	A/m
	-5	266.1 – 473.2	V/m	0.80 – 1.43	A/m
Category M3	0	199.5 – 354.8	V/m	0.6 – 1.07	A/m
	-5	149.6 – 266.1	V/m	0.45 – 0.80	A/m
Category M4	0	< 199.5	V/m	< 0.60	A/m
	-5	< 149.6	V/m	< 0.45	A/m
> 960 MHz					
Category M1	0	199.5 – 354.8	V/m	0.60 – 1.07	A/m
	-5	149.6 – 266.1	V/m	0.45 – 0.80	A/m
Category M2	0	112.2 – 199.5	V/m	0.34 – 0.60	A/m
	-5	84.1 – 149.6	V/m	0.25 – 0.45	A/m
Category M3	0	63.1 – 112.2	V/m	0.19 – 0.34	A/m
	-5	47.3 – 84.1	V/m	0.14 – 0.25	A/m
Category M4	0	< 63.1	V/m	< 0.19	A/m
	-5	< 47.3	V/m	< 0.14	A/m

Table 3.2 Telephone near-field categories in linear units



3.4 Test Conditions:

3.4.1 Ambient Condition

Ambient Temperature (°C)	20-24°C
Humidity (%)	<60%

3.4.2 Test Configuration

The device was controlled by using a base station emulator R&S CMU200. Communication between the device and the emulator was established by air link.

Measurements were performed on the low, middle and high channels of all bands.

The DUT was set from the emulator to radiate maximum output power during all testings.

The worst case for CDMA2000 test modes please refer to Appendix D.



4. Hearing Aid Compliance (HAC)

4.1 Introduction

The federal communication commission (FCC) adopted ANSI C63.19 as HAC test standard.

5. HAC Measurement Setup

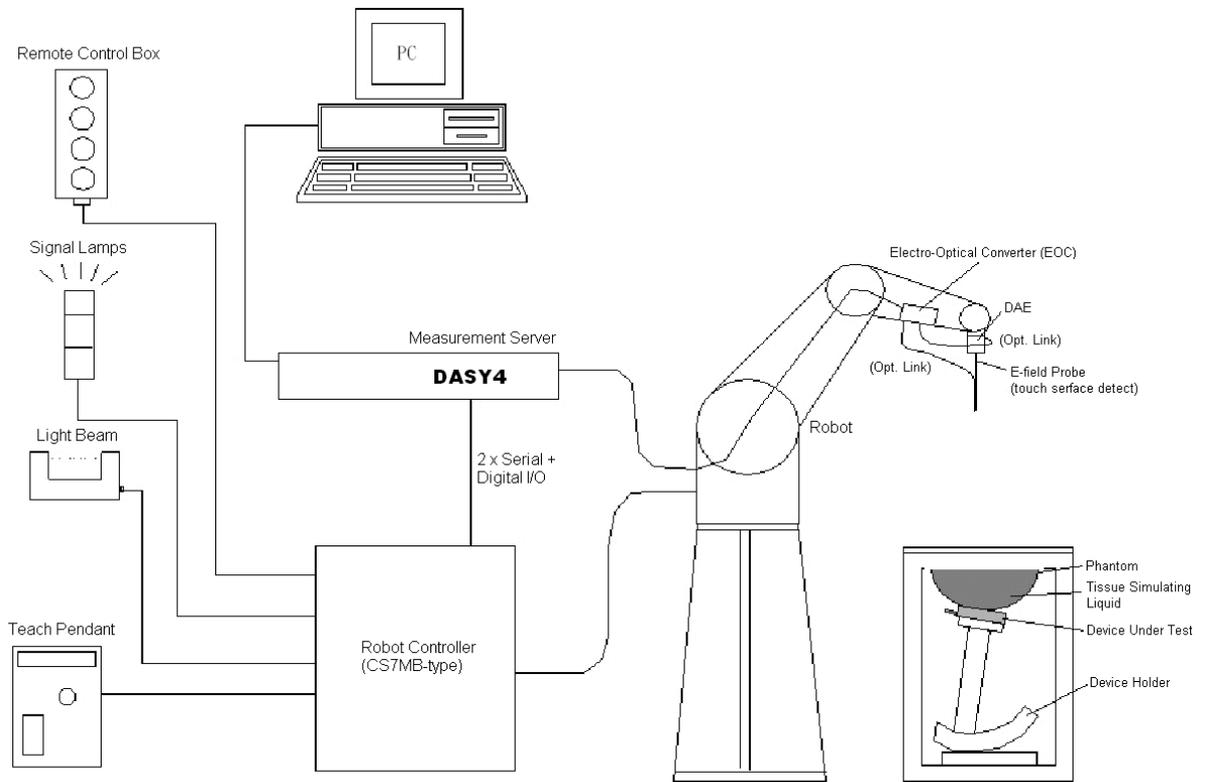


Fig. 5.1 DASY4 system



The DASY4 system for performance compliance tests is illustrated above graphically. This system consists of the following items:

- A standard high precision 6-axis robot with controller, a teach pendant and software
- A data acquisition electronic (DAE) attached to the robot arm extension
- A dosimetric probe equipped with an optical surface detector system
- The electro-optical converter (EOC) performs the conversion between optical and electrical signals
- A measurement server performs the time critical tasks such as signal filtering, control of the robot operation and fast movement interrupts.
- A probe alignment unit which improves the accuracy of the probe positioning
- A computer operating Windows XP
- DASY4 software
- Remove control with teach pendant and additional circuitry for robot safety such as warning lamps, etc.
- The SAM twin phantom
- A device holder
- Dipole for evaluating the proper functioning of the system
- Arch Phantom

Some of the components are described in details in the following sub-sections.

5.1 DASY4 E-Field and H-Field Probe System

The HAC measurement is conducted with the dosimetric probe ER3DV6 and H3DV6 (manufactured by SPEAG). The probe is specially designed and calibrated. This probe has a built in optical surface detection system to prevent from collision with DUT.

5.2 System Specification

5.2.1 ER3DV6 E-Field Probe Description

Construction	One dipole parallel, two dipoles normal to probe axis Built-in shielding against static charges
Calibration	In air from 100 MHz to 3.0 GHz (absolute accuracy $\pm 6.0\%$, $k=2$)
Frequency	100 MHz to 6 GHz; Linearity: ± 2.0 dB (100 MHz to 3 GHz)
Directivity	± 0.2 dB in air (rotation around probe axis) ± 0.4 dB in air (rotation normal to probe axis)
Dynamic Range	2 V/m to 1000 V/m (M3 or better device readings fall well below diode compression point)
Linearity	± 0.2 dB
Dimensions	Overall length: 330 mm (Tip: 16 mm) Tip diameter: 8 mm (Body: 12 mm) Distance from probe tip to dipole centers: 2.5 mm



Fig. 5.2
E-field Free-space Probe

5.2.2 H3DV6 H-Field Probe Description

Construction	Three concentric loop sensors with 3.8 mm loop diameters Resistively loaded detector diodes for linear response Built-in shielding against static charges
Frequency	200 MHz to 3 GHz (absolute accuracy $\pm 6.0\%$, $k=2$); Output linearized
Directivity	± 0.25 dB (spherical isotropy error)
Dynamic Range	10 m A/m to 2 A/m at 1 GHz (M3 or better device readings fall well below diode compression point)
Dimensions	Overall length: 330 mm (Tip: 40 mm) Tip diameter: 6 mm (Body: 12 mm) Distance from probe tip to dipole centers: 3 mm
E-Field Interference	$< 10\%$ at 3 GHz (for plane wave)



Fig. 5.3
H-field Free-space Probe

5.2.3 Probe Tip Description

HAC field measurements take place in the close near field with high gradients. Increasing the measuring distance from the source will generally decrease the measured field values (in case of the validation dipole approx. 10% per mm).

Magnetic field sensors are measuring the integral of the H-field across their sensor area surrounded by the loop. They are calibrated in a precise, homogeneous field. When measuring a gradient field, the result will be very close to the field in the center of the loop which is equivalent to the value of a homogeneous field equivalent to the center value. But it will be different from the field at the field at the border of the loop.

Consequently, two sensors with different loop diameters – both calibrated ideally – would give different results when measuring from the edge of the probe sensor elements. The behavior for electrically small E-field sensors is equivalent. See below for distance plots from a WD which show the conservative nature of field readings at the probe element center vs. measurements at the sensor end:



Fig. 5.4 Z-Axis Scan at maximum point above a typical wireless device for E-field

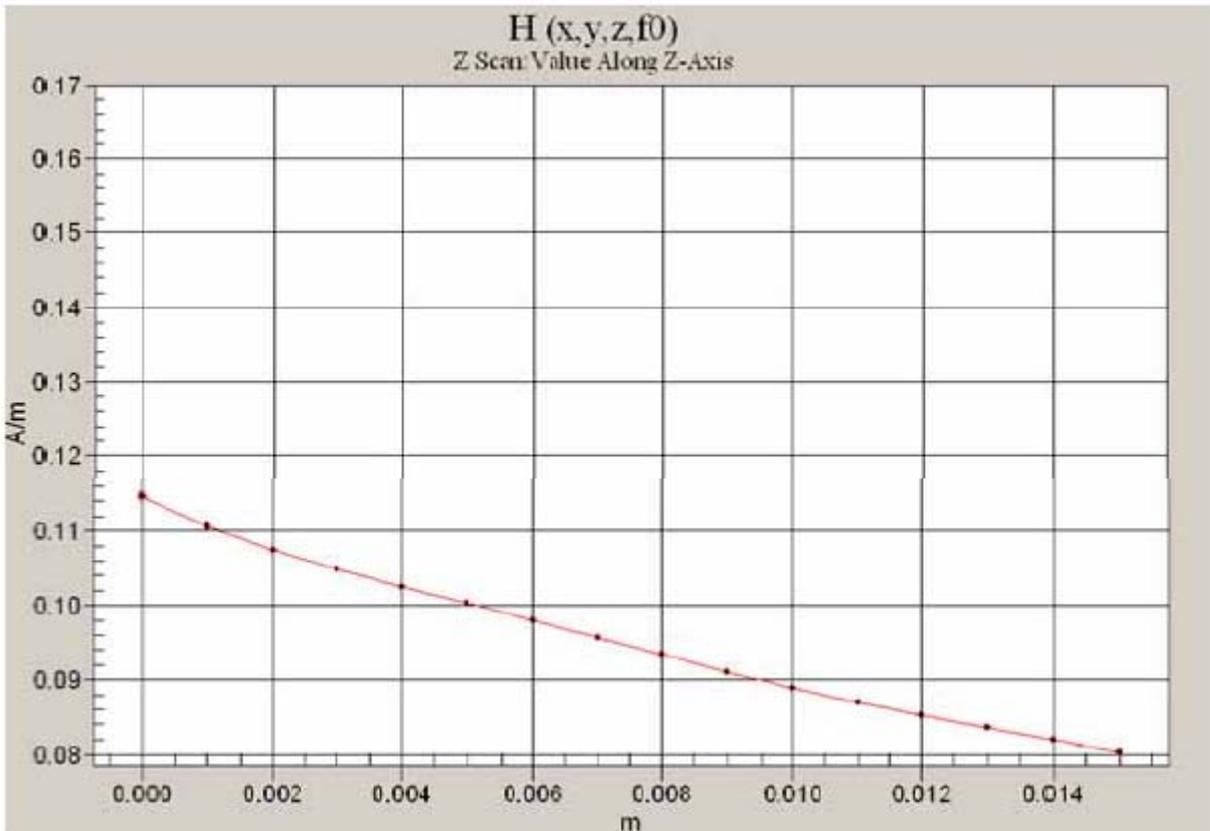


Fig. 5.5 Z-Axis Scan at maximum point above a typical wireless device for H-field

The magnetic field loops of the H3D probes are concentric, with the center 3mm from the tip for H3DV6. Their radius is 1.9 mm.

The electric field probes have a more irregular internal geometry because it is physically not possible to have the 3 orthogonal sensors situated with the same center. The effect of the different sensor centers is accounted for in the HAC uncertainty budget (“sensor displacement”). Their geometric center is at 2.5 mm from the tip, and the element ends are 1.1 mm closer to the tip.

Where:

Peak Field = Peak field (in dB V/m or dB A/m)

Raw = Raw field measurement from the measurement system (in V/m or A/m).

PMF = Probe Modulation Factor (in Linear units). See Chapter 8 of test report.



5.3 DATA Acquisition Electronics (DAE)

The data acquisition electronics (DAE4) consists of a highly sensitive electrometer-grade preamplifier with auto-zeroing, a channel and gain-switching multiplexer, a fast 16 bit AD-converter and a command decoder and control logic unit. Transmission to the measurement server is accomplished through an optical downlink for data and status information as well as an optical uplink for commands and the clock.

The mechanical probe mounting device includes two different sensor systems for frontal and sideways probe contacts. They are used for mechanical surface detection and probe collision detection.

The input impedance of the DAE4 is 200M Ohm; the inputs are symmetrical and floating. Common mode rejection is above 80dB.

5.4 Robot

The DASY4 system uses the high precision robots RX90BL type out of the newer series from Stäubli SA (France). For the 6-axis controller DASY4 system, the CS7MB robot controller version from Stäubli is used. The TX robot series have many features that are important for our application:

- High precision (repeatability 0.02 mm)
- High reliability (industrial design)
- Jerk-free straight movements
- Low ELF interference (the closed metallic construction shields against motor control fields)
- 6-axis controller

5.5 Measurement Server

The DASY4 measurement server is based on a PC/104 CPU board with
166 MHz CPU
32 MB chipset and
64 MB RAM.

Communication with
the DAE4 electronic box
the 16-bit AD-converter system for optical detection and digital I/O interface.

The measurement server performs all the real-time data evaluation for field measurements and surface detection, controls robot movements and handles safety operations.

5.6 Phone Positioner

The phone positioner shown in Fig. 5.8 is used to adjust DUT to the suitable position.



Fig. 5.6 Phone Positioner

5.6.1 Test Arch Phantom

Construction	Enables easy and well defined positioning of the phone and validation dipoles as well as simple teaching of the robot.
Dimensions	370 x 370 x 370 mm

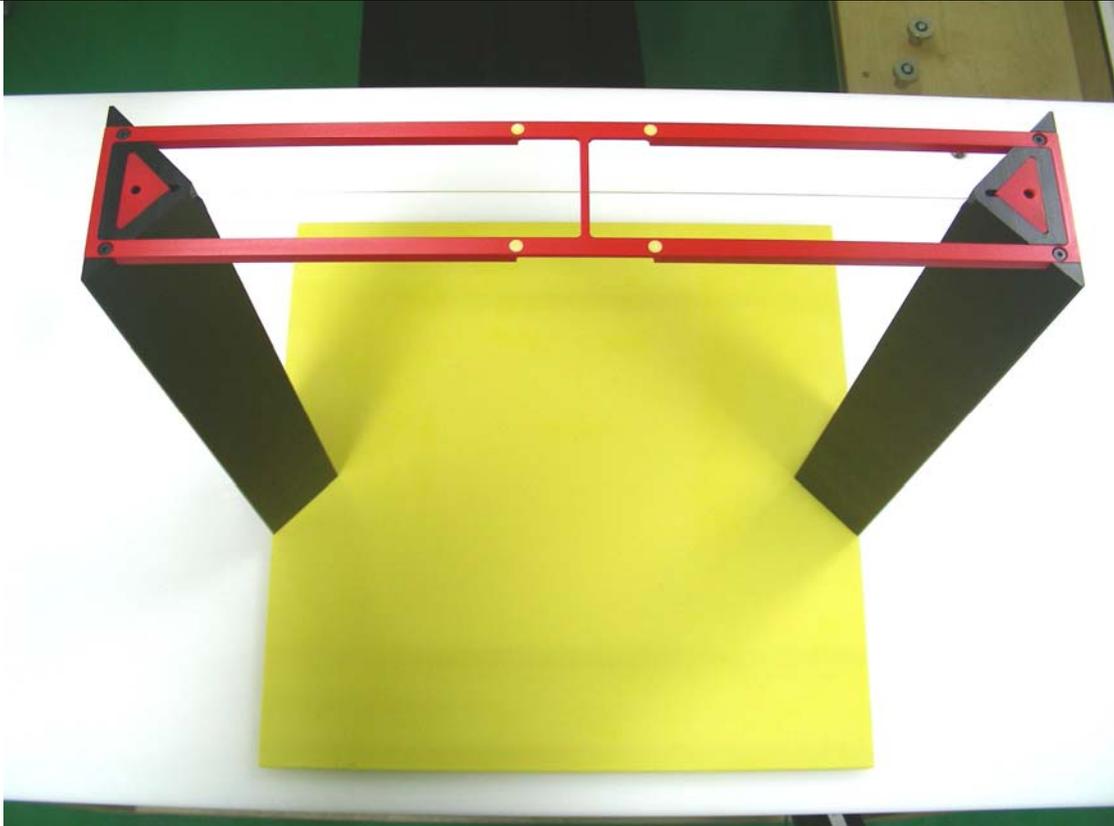


Fig. 5.7 Test Arch Phantom



5.7 Data Storage and Evaluation

5.7.1 Data Storage

The DASY4 software stores the assessed data from the data acquisition electronics as raw data (in microvolt readings from the probe sensors), together with all the necessary software parameters for the data evaluation (probe calibration data, and device frequency and modulation data) in measurement files with the extension .DA4. The postprocessing software evaluates the desired unit and format for output each time the data is visualized or exported. This allows verification of the complete software setup even after the measurement and allows correction of erroneous parameter settings.

5.7.2 Data Evaluation

The DASY4 postprocessing software (SEMCAD) automatically executes the following procedures to calculate the field units from the microvolt readings at the probe connector. The parameters used in the evaluation are stored in the configuration modules of the software :

Probe parameters :	- Sensitivity	Norm _i , a _{i0} , a _{i1} , a _{i2}
	- Conversion factor	ConvF _i
	- Diode compression point	dcp _i
Device parameters :	- Frequency	f
	- Crest factor	cf
Media parameters :	- Conductivity	σ
	- Density	ρ

These parameters must be set correctly in the software. They can be found in the component documents or they can be imported into the software from the configuration files issued for the DASY4 components. In the direct measuring mode of the multimeter option, the parameters of the actual system setup are used. In the scan visualization and export modes, the parameters stored in the corresponding document files are used.

The first step of the evaluation is a linearization of the filtered input signal to account for the compression characteristics of the detector diode. The compensation depends on the input signal, the diode type and the DC-transmission factor from the diode to the evaluation electronics. If the exciting field is pulsed, the crest factor of the signal must be known to correctly compensate for peak power. The formula for each channel can be given as :

$$V_i = U_i + U_i^2 \cdot \frac{cf}{dcp_i}$$

with $V_i =$ compensated signal of channel i ($i = x, y, z$)
 $U_i =$ input signal of channel i ($i = x, y, z$)
 $cf =$ crest factor of exciting field (DASY parameter)
 $dcp_i =$ diode compression point (DASY parameter)

From the compensated input signals, the primary field data for each channel can be evaluated :



E-field probes : $E_i = \sqrt{\frac{V_i}{Norm_i ConvF}}$

H-field probes : $H_i = \sqrt{V_i \frac{a_{i0} + a_{i1}f + a_{i2}f^2}{f}}$

- with
- V_i = compensated signal of channel i ($i = x, y, z$)
 - $Norm_i$ = sensor sensitivity of channel i ($i = x, y, z$)
 $\mu V/(V/m)^2$ for E-field Probes
 - $ConvF$ = sensitivity enhancement in solution
 - a_{ij} = sensor sensitivity factors for H-field probes
 - f = carrier frequency [GHz]
 - E_i = electric field strength of channel i in V/m
 - H_i = magnetic field strength of channel i in A/m

The RSS value of the field components gives the total field strength (Hermitian magnitude) :

$$E_{tot} = \sqrt{E_x^2 + E_y^2 + E_z^2}$$

The primary field data are used to calculate the derived field units.

The power flow density is calculated assuming the excitation field to be a free space field.

$$P_{pwe} = \frac{E_{tot}^2}{3770} \quad \text{or} \quad P_{pwe} = H_{tot}^2 \cdot 37.7$$

- with
- P_{pwe} = equivalent power density of a plane wave in mW/cm²
 - E_{tot} = total electric field strength in V/m
 - H_{tot} = total magnetic field strength in A/m

The measurement/integration time per point, as specified by the system manufacturer is >500 ms.

The signal response time is evaluated as the time required by the system to reach 90% of the expected final value after an on/off switch of the power source with an integration time of 500 ms and a probe response time of <5 ms. In the current implementation, DASY4 waits longer than 100 ms after having reached the grid point before starting a measurement, i.e., the response time uncertainty is negligible.

If the device under test does not emit a CW signal, the integration time applied to measure the electric field at a specific point may introduce additional uncertainties due to the discretization. The tolerances for the different systems had the worst-case of 2.6%.



5.8 Test Equipment List

Manufacture	Name of Equipment	Type/Model	Serial Number	Calibration	
				Last Cal.	Due Date
SPEAG	Isotropic E-Filed Probe	ER3DV6	2358	Jan. 28, 2008	Jan. 27, 2009
SPEAG	Isotropic H-Filed Probe	H3DV6	6184	Jan. 28, 2008	Jan. 27, 2009
SPEAG	835MHz Calibration Dipole	CD835V3	1017	Jul. 12, 2007	Jul. 12, 2008
SPEAG	1880MHz Calibration Dipole	CD1880V3	1036	Jul. 12, 2007	Jul. 12, 2008
SPEAG	Data Acquisition Electronics	DAE4	778	Sep. 17, 2007	Sep. 17, 2008
SPEAG	Phone Positoiner	N/A	N/A	NCR	NCR
SPEAG	Test Arch Phantom	N/A	N/A	NCR	NCR
SPEAG	Phantom	QD 000 P40 C	TP-1150	NCR	NCR
SPEAG	Robot	Staubli RX90BL	F03/5W15A1/A/01	NCR	NCR
SPEAG	Software	DASY4 V4.7 Build 55	N/A	NCR	NCR
SPEAG	Software	SEMCAD V1.8 Build 176	N/A	NCR	NCR
SPEAG	Measurement Server	SE UMS 001 BA	1021	NCR	NCR
Agilent	Dual Directional Coupler	778D	50422	NCR	NCR
Agilent	Power Amplifier	8449B	3008A01917	NCR	NCR
Agilent	Power Meter	E4416A	GB41292344	Feb. 21, 2008	Feb. 20, 2009
Agilent	Power Sensor	E9327A	US40441548	Feb. 21, 2008	Feb. 20, 2009
Agilent	Wireless COM. Test Set	E5515C	GB46311322	Dec. 22, 2006	Dec. 22, 2008
R&S	Universal Radio Communication Tester	CMU200	103937	Oct. 19, 2007	Oct. 19, 2008

Table 5.6 Test Equipment List



6. Uncertainty Assessment

The component of uncertainty may generally be categorized according to the methods used to evaluate them. The evaluation of uncertainty by the statistical analysis of a series of observations is termed a Type A evaluation of uncertainty. The evaluation of uncertainty by means other than the statistical analysis of a series of observation is termed a Type B evaluation of uncertainty. Each component of uncertainty, however evaluated, is represented by an estimated standard deviation, termed standard uncertainty, which is determined by the positive square root of the estimated variance.

A Type A evaluation of standard uncertainty may be based on any valid statistical method for treating data. This includes calculating the standard deviation of the mean of a series of independent observations; using the method of least squares to fit a curve to the data in order to estimate the parameter of the curve and their standard deviations; or carrying out an analysis of variance in order to identify and quantify random effects in certain kinds of measurement.

A type B evaluation of standard uncertainty is typically based on scientific judgment using all of the relevant information available. These may include previous measurement data, experience and knowledge of the behavior and properties of relevant materials and instruments, manufacture’s specification, data provided in calibration reports and uncertainties assigned to reference data taken from handbooks. Broadly speaking, the uncertainty is either obtained from an outdoor source or obtained from an assumed distribution, such as the normal distribution, rectangular or triangular distributions indicated in Table 7.1

Uncertainty Distributions	Normal	Rectangular	Triangular	U-shape
Multiplying factor ^(a)	1/k ^(b)	1/√3	1/√6	1/√2

(a) standard uncertainty is determined as the product of the multiplying factor and the estimated range of variations in the measured quantity
(b) *k* is the coverage factor

Table 6.1

The combined standard uncertainty of the measurement result represents the estimated standard deviation of the result. It is obtained by combining the individual standard uncertainties of both Type A and Type B evaluation using the usual “root-sum-squares” (RSS) methods of combining standard deviations by taking the positive square root of the estimated variances.

Expanded uncertainty is a measure of uncertainty that defines an interval about the measurement result within which the measured value is confidently believed to lie. It is obtained by multiplying the combined standard uncertainty by a coverage factor. Typically, the coverage factor ranges from 2 to 3. Using a coverage factor allows the true value of a measured quantity to be specified with a defined probability within the specified uncertainty range. For purpose of this document, a coverage factor two is used, which corresponds to confidence interval of about 95 %. The DASY4 uncertainty Budget is showed in Table 6.2.



Error Description	Uncertainty Value (\pm %)	Probability Distribution	Divisor	(Ci) E	(Ci) H	Std. Unc. E	Std. Unc. H
Measurement System							
Probe Calibration	± 5.1	Normal	1	1	1	± 5.1	± 5.1
Axial Isotropy	± 4.7	Rectangular	$\sqrt{3}$	1	1	± 2.7	± 2.7
Sensor Displacement	± 16.5	Rectangular	$\sqrt{3}$	1	0.145	± 9.5	± 1.4
Boundary Effect	± 2.4	Rectangular	$\sqrt{3}$	1	1	± 1.4	± 1.4
Linearity	± 4.7	Rectangular	$\sqrt{3}$	1	1	± 2.7	± 2.7
Scaling to Peak Envelope Power	± 2.0	Rectangular	$\sqrt{3}$	1	1	± 1.2	± 1.2
System Detection Limit	± 1.0	Rectangular	$\sqrt{3}$	1	1	± 0.6	± 0.6
Readout Electronics	± 0.3	Normal	1	1	1	± 0.3	± 0.3
Response Time	± 0.8	Rectangular	$\sqrt{3}$	1	1	± 0.5	± 0.5
Integration Time	± 2.6	Rectangular	$\sqrt{3}$	1	1	± 1.5	± 1.5
RF Ambient Conditions	± 3.0	Rectangular	$\sqrt{3}$	1	1	± 1.7	± 1.7
RF Reflections	± 12.0	Rectangular	$\sqrt{3}$	1	1	± 6.9	± 6.9
Probe Positioner	± 1.2	Rectangular	$\sqrt{3}$	1	0.67	± 0.7	± 0.5
Probe Positioning	± 4.7	Rectangular	$\sqrt{3}$	1	0.67	± 2.7	± 1.8
Extrap. and Interpolation	± 1.0	Rectangular	$\sqrt{3}$	1	1	± 0.6	± 0.6
Test Sample Related							
Device Positioning Vertical	± 4.7	Rectangular	$\sqrt{3}$	1	0.67	± 2.7	± 1.8
Device Positioning Lateral	± 1.0	Rectangular	$\sqrt{3}$	1	1	± 0.6	± 0.6
Device Holder and Phantom	± 2.4	Rectangular	$\sqrt{3}$	1	1	± 1.4	± 1.4
Power Drift	± 5.0	Rectangular	$\sqrt{3}$	1	1	± 2.9	± 2.9
Phantom and Setup Related							
Phantom Thickness	± 2.4	Rectangular	$\sqrt{3}$	1	0.67	± 1.4	± 0.9
Combined Standard Uncertainty						± 14.7	± 10.9
Coverage Factor for 95 %		K=2					
Expanded uncertainty (Coverage factor = 2)						± 29.4	± 21.8

Table 6.2 Uncertainty Budget of DASY4

7. HAC Measurement Evaluation

Each DASY4 system is equipped with one or more system validation kits. These units, together with the predefined measurement procedures within the DASY4 software, enable the user to conduct the system performance check and system validation. System validation kit includes a dipole, tripod holder to fix it underneath the test Arch and a corresponding distance holder.

7.1 Purpose of System Performance check

The system performance check verifies that the system operates within its specifications. System and operator errors can be detected and corrected. It is recommended that the system performance check be performed prior to any usage of the system in order to guarantee reproducible results. The system performance check uses normal HAC measurements in a simplified setup with a well characterized source. This setup was selected to give a high sensitivity to all parameters that might fail or vary over time. The system check does not intend to replace the calibration of the components, but indicates situations where the system uncertainty is exceeded due to drift or failure.

7.2 System Setup

In the simplified setup for system evaluation, the DUT is replaced by a calibrated dipole and the power source is replaced by a continuous wave which comes from a signal generator at frequency 835 and 1880 MHz. The calibrated dipole must be placed beneath the flat phantom section of the ARC with the correct distance holder. The equipment setup is shown below:

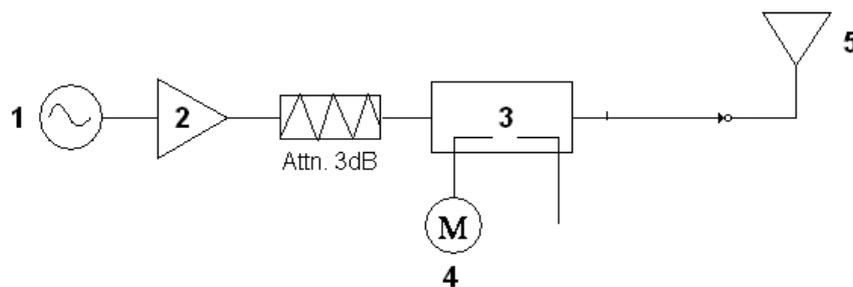


Fig. 7.1 System Setup of System Evaluation



1. Signal Generator
2. Amplifier
3. Directional Coupler
4. Power Meter
5. 835 or 1880 MHz Dipole

The output power on dipole port must be calibrated to 20dBm (100mW) before dipole is connected.

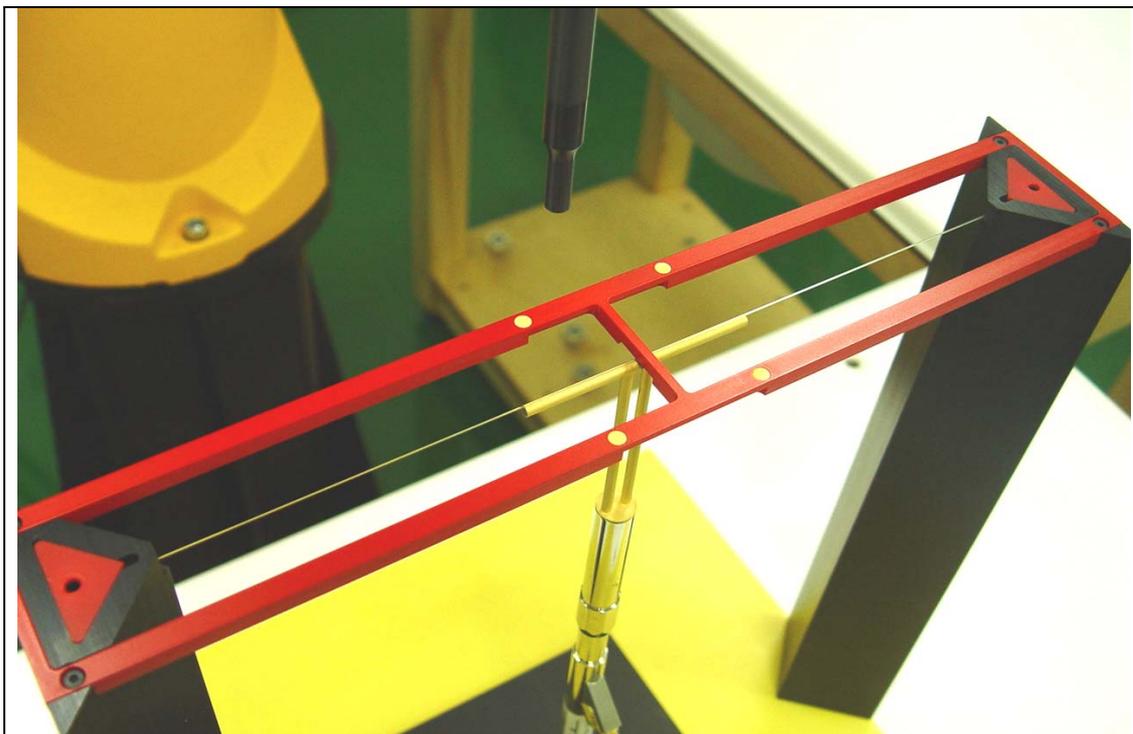


Fig 7.2 Dipole Setup



7.3 Validation Results

Frequency (MHz)	Input Power (dBm)	E-field Result (V/m)	Target Field (V/m)	Deviation (%)
835	20.0	174.95	167.1	4.70
1880	20.0	148.65	138.9	7.02
Frequency (MHz)	Input Power (dBm)	H-field Result (A/m)	Target Field (A/m)	Deviation (%)
835	20.0	0.459	0.453	1.32
1880	20.0	0.498	0.471	5.73

Table 7.1 System Validation

Remark: Deviation = ((E or H-field Result) - (Target field)) / (Target field) * 100%

The table above indicates the system performance check can meet the variation criterion, ±25%.

8. RF Field Probe Modulation Factor

A calibration shall be made of the modulation response of the probe and its instrumentation chain. This calibration shall be performed with the field probe, attached to the instrumentation that is to be used with it during the measurement. The response of the probe system to a CW field at the frequency(s) of interest is compared to its response to a modulated signal with equal peak amplitude. The field level of the test signals shall be more than 10 dB above the ambient level and the noise floor of the instrumentation being used. The ratio of the CW reading to that taken with a modulated field shall be applied to the readings taken of modulated fields of the specified type.

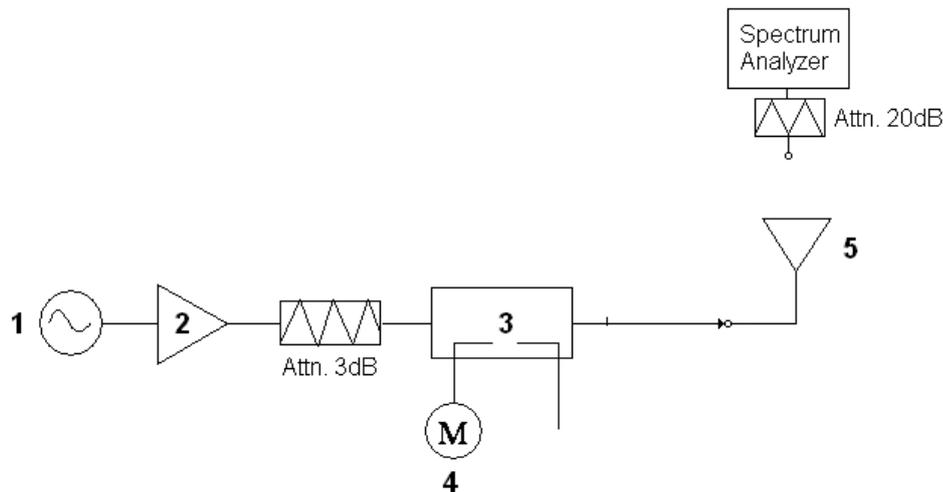


Fig. 8.1 System Calibration

This was done using the following procedure:


1. Fixing the probe in a set location relative to a field generating device.
2. Illuminate the probe with a CW signal at the intended measurement frequency.
3. Record the reading of the probe measurement system of the CW signal.
4. Determine the level of the CW signal being used to drive the field generating device.
5. Substitute a signal using the same modulation as that used by the intended WD for the CW signal.
6. Set the peak amplitude during transmission of the modulated signal to equal the amplitude of the CW signal.
7. Record the reading of the probe measurement system of the modulated signal.
8. The ratio of the CW to modulated signal reading is the modulation factor.
9. Repeat 2~8 steps at intended measurement frequency for both E and H field probe.




PMF Measurement Summary:

Frequency	Functions	E-field	H-field	PMF	
		V/m	A/m	E-field	H-field
835MHz	CW	185.5	0.802	-	-
835MHz	AM	117.8	0.515	1.57	1.56
835MHz	CDMA	191.4	0.817	0.97	0.98
835MHz	CMDA 1/8	66.3	0.287	2.80	2.79
1880MHz	CW	176.4	0.793	-	-
1880MHz	AM	114.5	0.487	1.54	1.63
1880MHz	CDMA	179.9	0.801	0.98	0.99
1880MHz	CMDA 1/8	63.2	0.283	2.79	2.80


Zero span Spectrum Plots for RF Field Probe Modulation Factor

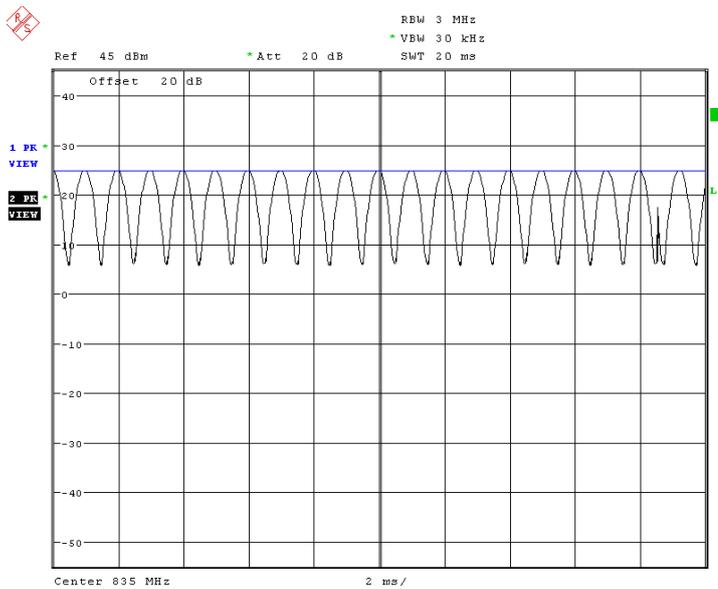


835MHz - CW and 80% AM

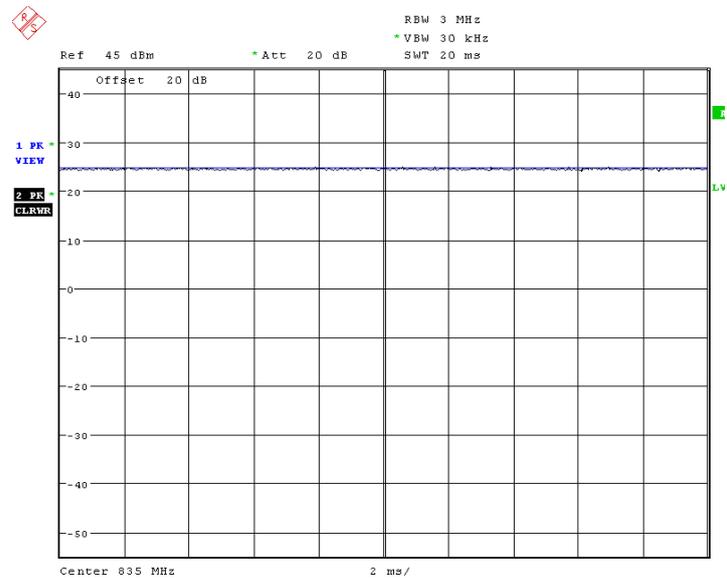


835MHz - CW and CDMA (Full Rate)

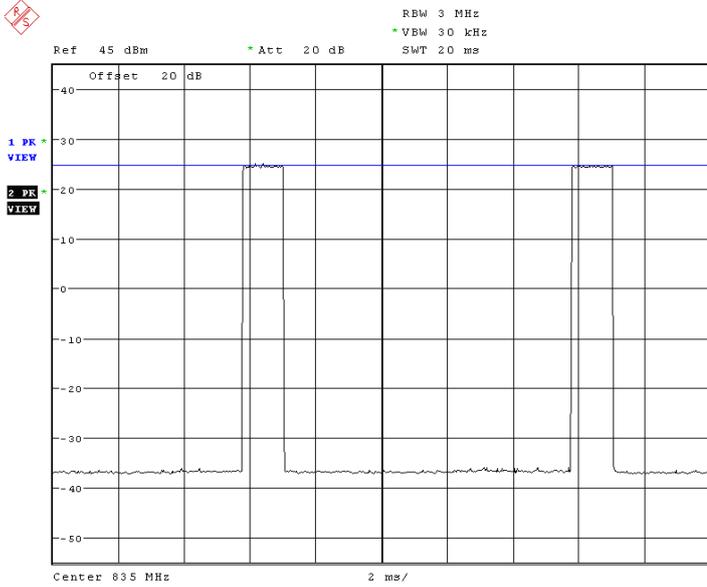


835MHz - CW and CDMA (1/8 Rate)

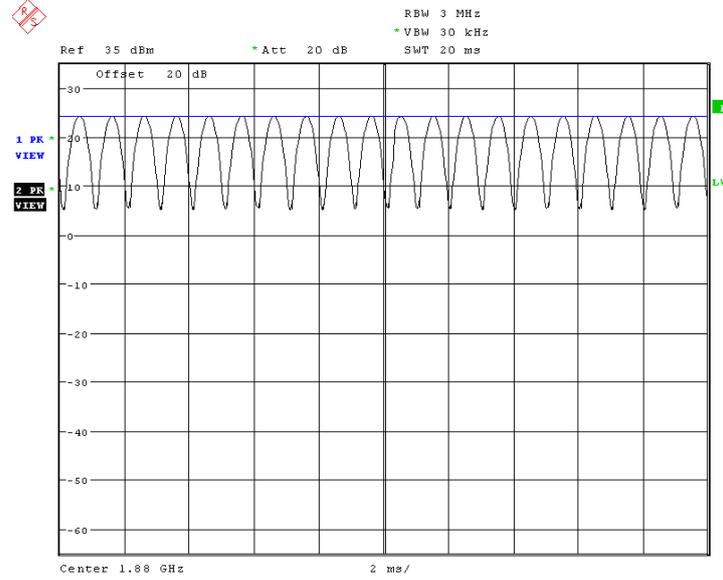

1880MHz - CW and 80% AM

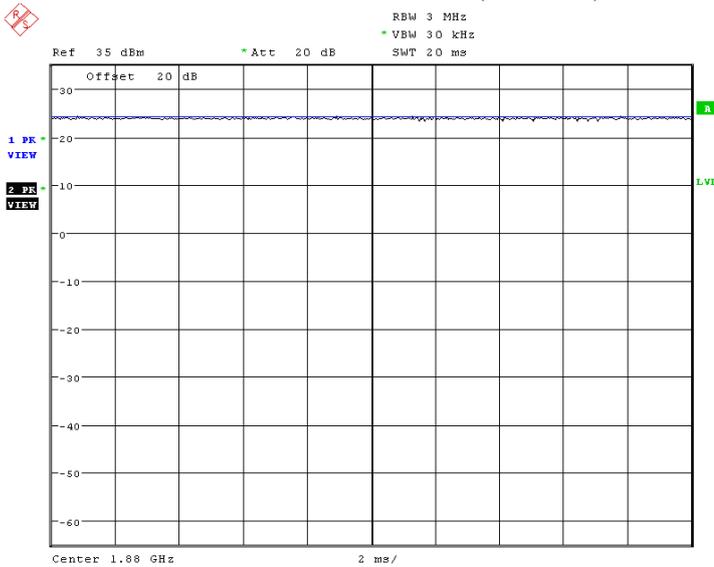

1880MHz - CW and CDMA (Full Rate)

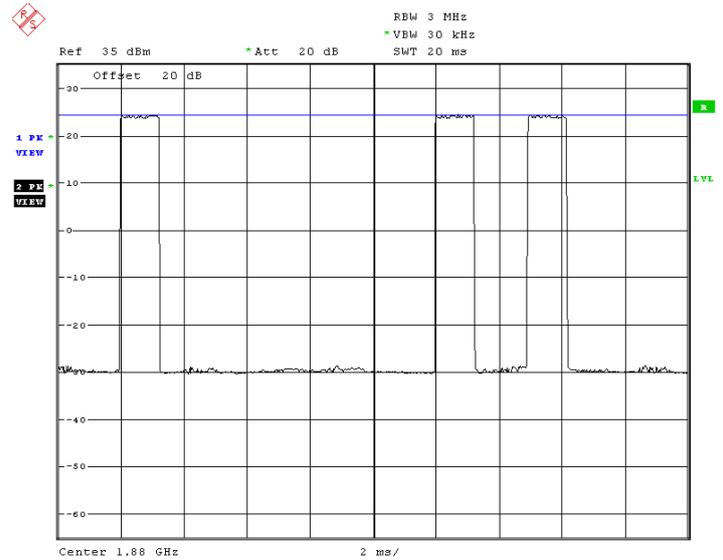

1880MHz - CW and CDMA (1/8 Rate)

9. Description for DUT Testing Position

The DUT was put on device holder and adjusted to the accurate and reliable position. Figure 9.1 illustrate the references and reference plane that shall be used in a typical DUT emissions measurement. The principle of this section is applied to DUT with similar geometry.

- The grid is 5 cm by 5 cm area that is divided into 9 evenly sized blocks or sub-grids.
- The grid is centered on the audio frequency output transducer of the DUT.
- The grid is in a reference plane, which is defined as the planar area that contains the highest point in the area of the phone that normally rests against the user’s ear. It is parallel to the centerline of the receiver area of the phone and is defined by the points of the receiver-end of the DUT handset, which, in normal handset use, rest against the ear.
- The measurement plane is parallel to, and 1.0 cm in front of, the reference plane.



Figure 9.1: A typical DUT reference and plane for HAC measurements

Setup photographs please refer to Appendix E.



10. RF Emissions Test Procedure

The following illustrate a typical RF emissions test scan over a wireless communications device:

1. Proper operation of the field probe, probe measurement system, other instrumentation, and the positioning system was confirmed.
2. DUT is positioned in its intended test position, acoustic output point of the device perpendicular to the field probe.
3. The DUT operation for maximum rated RF output power was configured and confirmed with the base station simulator, at the test channel and other normal operating parameters as intended for the test. The battery was ensured to be fully charged before each test.
4. The center sub-grid was centered over the center of the acoustic output (also audio band magnetic output, if applicable). The DUT audio output was positioned tangent (as physically possible) to the measurement plane.
5. A surface calibration was performed before each setup change to ensure repeatable spacing and proper maintenance of the measurement plane using the test Arch.
6. The measurement system measured the field strength at the reference location.
7. Measurements at 5 mm increments in the 5 x 5 cm region were performed and recorded. A 360° rotation about the azimuth axis at the maximum interpolated position was measured. For the worst-case condition, the peak reading from this rotation was used in re-evaluating the HAC category.
8. The system performed a drift evaluation by measuring the field at the reference location.
9. Steps 1-8 were done for both the E and H-Field measurements.



11. HAC Test Results

11.1 E-Field Emission

Mode	Chan.	Freq. (MHz)	Modulation type	PMF	Conducted Power (dBm)	Power Drift (dB)	Peak Field (V/m)	Backlight	Bluetooth	M-Rating
CDMA2000 Cellular	1013	824.70	QPSK	0.97	23.35	-0.037	96.5	Off	Off	M4
	384	836.52	QPSK	0.97	23.68	0.037	116.4	Off	Off	M4
	384	836.52	QPSK	0.97	23.68	0.028	117	On	Off	M4
	384	836.52	QPSK	0.97	23.68	-0.073	115.4	Off	On	M4
	777	848.31	QPSK	0.97	23.86	0.021	96.6	Off	Off	M4
CDMA2000 AWS	25	1711.25	QPSK	0.98	23.79	-0.075	52.1	Off	Off	M4
	450	1732.50	QPSK	0.98	24.20	-0.059	52.5	Off	Off	M4
	875	1753.75	QPSK	0.98	23.82	-0.088	53.9	Off	Off	M4
	875	1753.75	QPSK	0.98	23.82	0.071	54.5	On	Off	M4
	875	1753.75	QPSK	0.98	23.82	0.007	54.4	Off	On	M4
CDMA2000 PCS	25	1851.25	QPSK	0.98	24.08	0.09	41.5	Off	Off	M4
	600	1880.00	QPSK	0.98	24.15	-0.027	43.9	Off	Off	M4
	600	1880.00	QPSK	0.98	24.15	-0.02	43.5	On	Off	M4
	600	1880.00	QPSK	0.98	24.15	-0.049	43.6	Off	On	M4
	1175	1908.75	QPSK	0.98	23.79	-0.026	37.1	Off	Off	M4

11.2 H-Field Emission

Mode	Chan.	Freq. (MHz)	Modulation type	PMF	Conducted Power (dBm)	Power Drift (dB)	Peak Field (A/m)	Backlight	Bluetooth	M-Rating
CDMA2000 Cellular	1013	824.70	QPSK	0.98	23.35	-0.096	0.171	Off	Off	M4
	384	836.52	QPSK	0.98	23.68	0.007	0.202	Off	Off	M4
	384	836.52	QPSK	0.98	23.68	-0.029	0.202	On	Off	M4
	384	836.52	QPSK	0.98	23.68	0.047	0.202	Off	On	M4
	777	848.31	QPSK	0.98	23.86	-0.054	0.171	Off	Off	M4
CDMA2000 AWS	25	1711.25	QPSK	0.99	23.79	-0.06	0.145	Off	Off	M4
	450	1732.50	QPSK	0.99	24.20	0.117	0.151	Off	Off	M4
	875	1753.75	QPSK	0.99	23.82	-0.09	0.157	Off	Off	M4
	875	1753.75	QPSK	0.99	23.82	0.006	0.155	On	Off	M4
	875	1753.75	QPSK	0.99	23.82	-0.012	0.156	Off	On	M4
CDMA2000 PCS	25	1851.25	QPSK	0.99	24.08	0.139	0.11	Off	Off	M4
	600	1880.00	QPSK	0.99	24.15	0.027	0.116	Off	Off	M4
	600	1880.00	QPSK	0.99	24.15	-0.059	0.117	Off	Off	M4
	600	1880.00	QPSK	0.99	24.15	0.068	0.117	Off	On	M4
	1175	1908.75	QPSK	0.99	23.79	0.054	0.101	Off	Off	M4

Remark :

1. The device was chosen to be tested in the worst case peak E-Field condition under RC3/SO55 Full Rate.
2. The output power is adjusted to maximum level during RF Emission testing.
3. Test Engineer : Eric Huang



12. References

- [1] ANSI C63.19 2006, “American National Standard for Methods of Measurement of Compatibility between Wireless Communications Devices and Hearing Aids”
- [2] DASY4 System Hand book.



Appendix A - System Performance Check Data

Test Laboratory: Sporton International Inc. SAR/HAC Testing Lab

Date:2008/4/2

HAC_E_Dipole_835

DUT: HAC-Dipole 835 MHz; Type: CD835V3

Communication System: CW; Frequency: 835 MHz;Duty Cycle: 1:1

Medium: Air Medium parameters used: $\sigma = 0$ mho/m, $\epsilon_r = 1$; $\rho = 1000$ kg/m³

Ambient Temperature : 22.0 °C

DASY4 Configuration:

- Probe: ER3DV6 - SN2358; ConvF(1, 1, 1); Calibrated: 2008/1/28

- Sensor-Surface: (Fix Surface)

- Electronics: DAE4 Sn778; Calibrated: 2007/9/17

- Phantom: HAC Test Arch 4.6; Type: SD HAC P01 BA;

- Measurement SW: DASY4, V4.7 Build 55; Postprocessing SW: SEMCAD, V1.8 Build 176

E Scan - ER probe center 10mm above CD835 Dipole/Hearing Aid Compatibility Test

(41x361x1): Measurement grid: dx=5mm, dy=5mm

Maximum value of peak Total field = 180.1 V/m

Probe Modulation Factor = 1.00

Device Reference Point: 0.000, 0.000, 353.7 mm

Reference Value = 59.4 V/m; Power Drift = 0.035 dB

Hearing Aid Near-Field Category: M4 (AWF 0 dB)

Peak E-field in V/m


Grid 1	Grid 2	Grid 3
174.5 M4	180.1 M4	173.4 M4
Grid 4	Grid 5	Grid 6
89.0 M4	94.1 M4	92.1 M4
Grid 7	Grid 8	Grid 9
165.4 M4	169.8 M4	164.9 M4

Cursor:

Total = 180.0 V/m

E Category: M4

Location: 0, -79, 363.7 mm

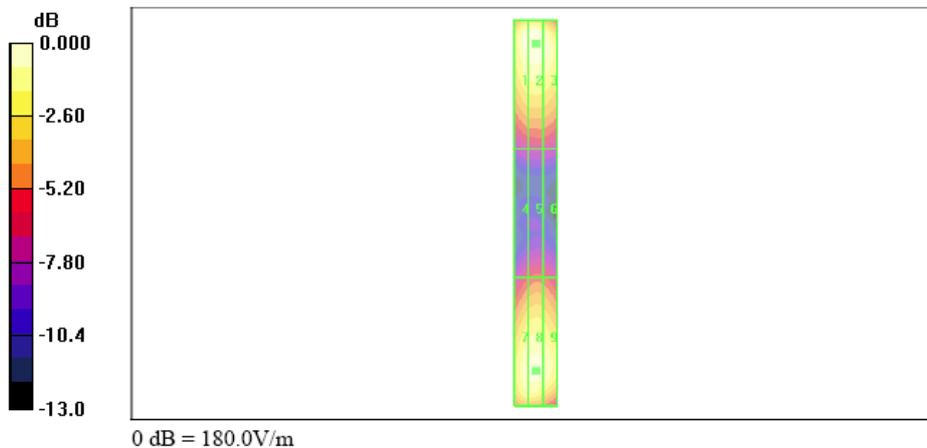



Test Laboratory: Sporton International Inc. SAR/HAC Testing Lab

Date:2008/4/2

HAC_E_Dipole_1880

DUT: HAC Dipole 1880 MHz; Type: CD1880V3

Communication System: CW; Frequency: 1880 MHz;Duty Cycle: 1:1
Medium: Air Medium parameters used: sigma = 0 mho/m, epsilon_r = 1; rho = 1000 kg/m^3
Ambient Temperature : 22.0 C

DASY4 Configuration:

- Probe: ER3DV6 - SN2358; ConvF(1, 1, 1); Calibrated: 2008/1/28
- Sensor-Surface: (Fix Surface)
- Electronics: DAE4 Sn778; Calibrated: 2007/9/17
- Phantom: HAC Test Arch 4.6; Type: SD HAC P01 BA;
- Measurement SW: DASY4, V4.7 Build 55; Postprocessing SW: SEMCAD, V1.8 Build 176

E Scan - ER probe center 10mm above CD1880 Dipole/Hearing Aid Compatibility Test


(41x181x1): Measurement grid: dx=5mm, dy=5mm
Maximum value of peak Total field = 148.8 V/m
Probe Modulation Factor = 1.00
Device Reference Point: 0.000, 0.000, 353.7 mm
Reference Value = 72.1 V/m; Power Drift = 0.004 dB
Hearing Aid Near-Field Category: M2 (AWF 0 dB)

Peak E-field in V/m

Table with 3 columns (Grid 1-3, Grid 4-6, Grid 7-9) and 3 rows of peak E-field values in V/m.

Cursor:

Total = 148.7 V/m
E Category: M2
Location: 0.5, 33, 363.7 mm

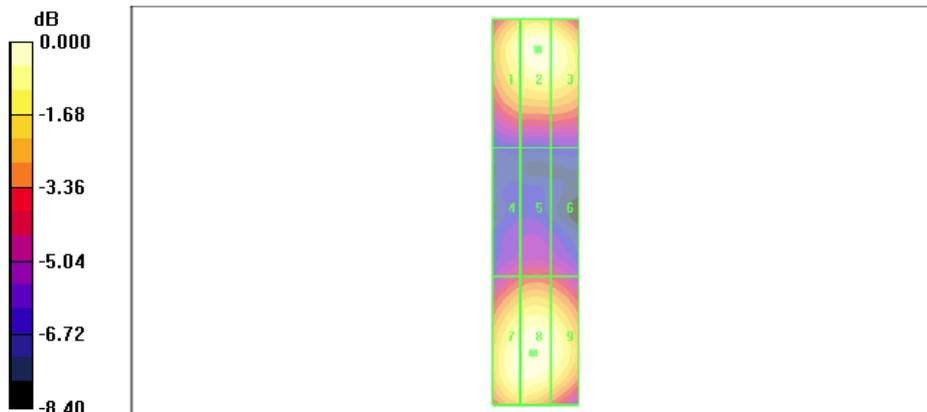

0 dB = 148.7V/m



Test Laboratory: Sporton International Inc. SAR/HAC Testing Lab

Date:2008/4/2

HAC_H_Dipole_835

DUT: HAC-Dipole 835 MHz; Type: CD835V3

Communication System: CW; Frequency: 835 MHz;Duty Cycle: 1:1
Medium: Air Medium parameters used: sigma = 0 mho/m, epsilon = 1; rho = 1 kg/m^3
Ambient Temperature : 22.0 C


- DASY4 Configuration:
- Probe: H3DV6 - SN6184; ; Calibrated: 2008/1/28
- Sensor-Surface: (Fix Surface)
- Electronics: DAE4 Sn778; Calibrated: 2007/9/17
- Phantom: HAC Test Arch 4.6; Type: SD HAC P01 BA;
- Measurement SW: DASY4, V4.7 Build 55; Postprocessing SW: SEMCAD, V1.8 Build 176

H Scan - HSDV6 probe center 10mm above CD835 Dipole/Hearing Aid Compatibility Test
(41x361x1): Measurement grid: dx=5mm, dy=5mm
Maximum value of peak Total field = 0.459 A/m
Probe Modulation Factor = 1.00
Device Reference Point: 0.000, 0.000, 353.7 mm
Reference Value = 0.447 A/m; Power Drift = -0.050 dB
Hearing Aid Near-Field Category: M4 (AWF 0 dB)

Peak H-field in A/m

Table with 3 columns (Grid 1-3, Grid 4-6, Grid 7-9) and 3 rows of peak H-field values in A/m, ranging from 0.375 M4 to 0.459 M4.

Cursor:
Total = 0.459 A/m
H Category: M4
Location: 0.5, -4, 363.7 mm

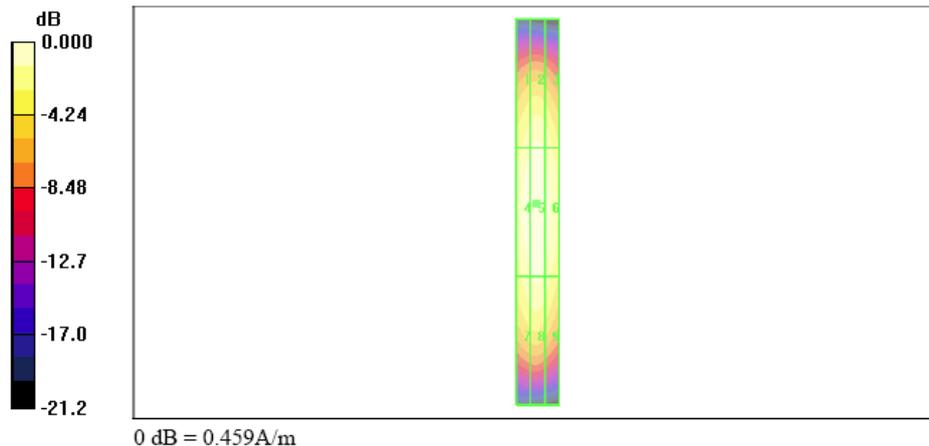



Test Laboratory: Sporton International Inc. SAR/HAC Testing Lab

Date:2008/4/2

HAC_H_Dipole_1880

DUT: HAC Dipole 1880 MHz; Type: CD1880V3

Communication System: CW; Frequency: 1880 MHz;Duty Cycle: 1:1
Medium: Air Medium parameters used: $\sigma = 0$ mho/m, $\epsilon_r = 1$; $\rho = 1$ kg/m³
Ambient Temperature : 22.0 °C

DASY4 Configuration:

- Probe: H3DV6 - SN6184; ; Calibrated: 2008/1/28
- Sensor-Surface: (Fix Surface)
- Electronics: DAE4 Sn778; Calibrated: 2007/9/17
- Phantom: HAC Test Arch 4.6; Type: SD HAC P01 BA;
- Measurement SW: DASY4, V4.7 Build 55; Postprocessing SW: SEMCAD, V1.8 Build 176

H Scan - HSDV6 probe center 10mm above CD1880 Dipole/Hearing Aid Compatibility Test


(41x181x1): Measurement grid: dx=5mm, dy=5mm
Maximum value of peak Total field = 0.498 A/m
Probe Modulation Factor = 1.00
Device Reference Point: 0.000, 0.000, 353.7 mm
Reference Value = 0.485 A/m; Power Drift = 0.004 dB
Hearing Aid Near-Field Category: M2 (AWF 0 dB)

Peak H-field in A/m

Grid 1	Grid 2	Grid 3
0.439 M2	0.459 M2	0.429 M2
Grid 4	Grid 5	Grid 6
0.481 M2	0.498 M2	0.465 M2
Grid 7	Grid 8	Grid 9
0.443 M2	0.461 M2	0.425 M2

Cursor:

Total = 0.498 A/m
H Category: M2
Location: 0.5, 0, 363.7 mm

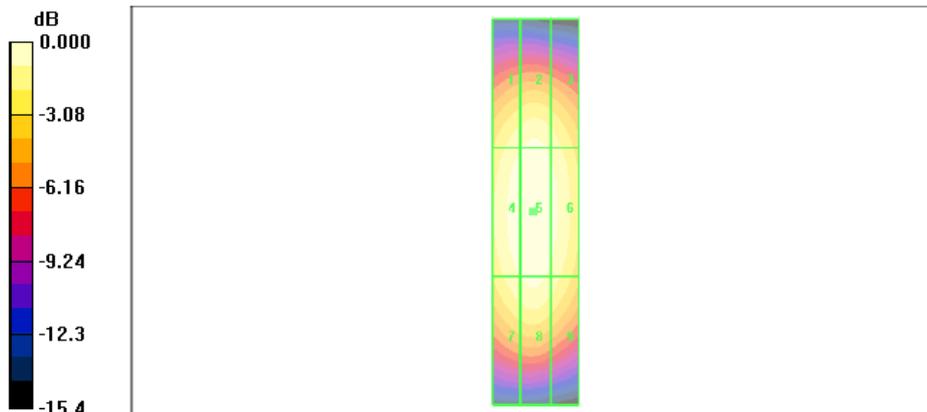

0 dB = 0.498A/m



Appendix B - HAC Measurement Data

Test Laboratory: Sporton International Inc. SAR/HAC Testing Lab

Date:2008/4/2

HAC_E_CDMA850 Ch1013_RC3 SO55_Loop_Full

DUT: 830102

Communication System: CDMA ; Frequency: 824.7 MHz;Duty Cycle: 1:1
Medium: Air Medium parameters used: sigma = 0 mho/m, epsilon_r = 1; rho = 1000 kg/m^3
Ambient Temperature : 22.7 C

DASY4 Configuration:

- Probe: ER3DV6 - SN2358; ConvF(1, 1, 1); Calibrated: 2008/1/28
- Sensor-Surface: (Fix Surface)
- Electronics: DAE4 Sn778; Calibrated: 2007/9/17
- Phantom: HAC Test Arch 4.6; Type: SD HAC P01 BA;
- Measurement SW: DASY4, V4.7 Build 55; Postprocessing SW: SEMCAD, V1.8 Build 176

Ch1013/Hearing Aid Compatibility Test (101x101x1): Measurement grid: dx=5mm, dy=5mm

Maximum value of peak Total field = 96.5 V/m
Probe Modulation Factor = 0.970
Device Reference Point: 0.000, 0.000, 353.7 mm
Reference Value = 107.4 V/m; Power Drift = -0.037 dB


Hearing Aid Near-Field Category: M4 (AWF 0 dB)

Peak E-field in V/m

Table with 3 columns (Grid 1-3, Grid 4-6, Grid 7-9) and 3 rows of peak E-field values in V/m.

Cursor:

Total = 96.5 V/m
E Category: M4
Location: -3, -1.5, 364.8 mm

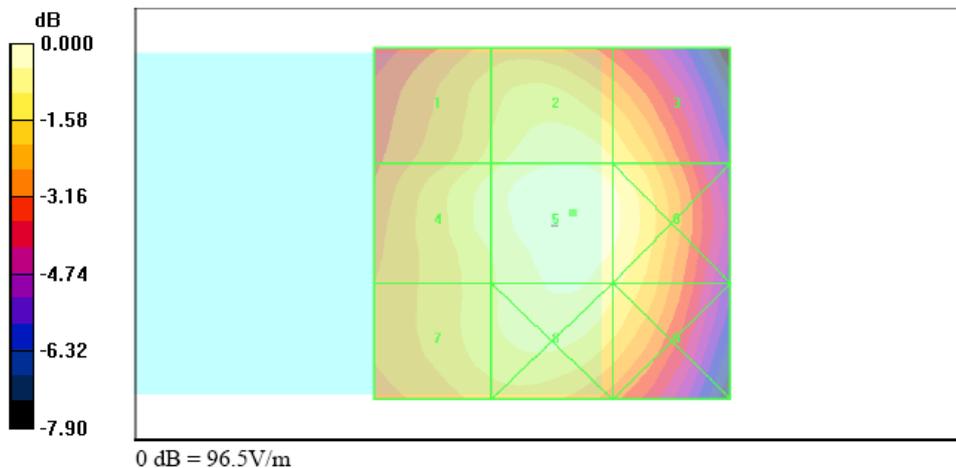



Test Laboratory: Sporton International Inc. SAR/HAC Testing Lab

Date:2008/4/2

HAC_E_CDMA850 Ch384_RC3 SO55_Loop_Full

DUT: 830102

Communication System: CDMA ; Frequency: 836.52 MHz;Duty Cycle: 1:1
Medium: Air Medium parameters used: $\sigma = 0$ mho/m, $\epsilon_r = 1$; $\rho = 1000$ kg/m³
Ambient Temperature : 22.8 °C

DASY4 Configuration:

- Probe: ER3DV6 - SN2358; ConvF(1, 1, 1); Calibrated: 2008/1/28
- Sensor-Surface: (Fix Surface)
- Electronics: DAE4 Sn778; Calibrated: 2007/9/17
- Phantom: HAC Test Arch 4.6; Type: SD HAC P01 BA
- Measurement SW: DASY4, V4.7 Build 55; Postprocessing SW: SEMCAD, V1.8 Build 176

Ch384/Hearing Aid Compatibility Test (101x101x1): Measurement grid: dx=5mm, dy=5mm


Maximum value of peak Total field = 116.4 V/m
Probe Modulation Factor = 0.970
Device Reference Point: 0.000, 0.000, 353.7 mm
Reference Value = 129.7 V/m; Power Drift = 0.037 dB
Hearing Aid Near-Field Category: M4 (AWF 0 dB)

Peak E-field in V/m

Grid 1	Grid 2	Grid 3
100.4 M4	110.1 M4	104.3 M4
Grid 4	Grid 5	Grid 6
107.1 M4	116.4 M4	111.7 M4
Grid 7	Grid 8	Grid 9
102.8 M4	110.3 M4	104.2 M4

Cursor:

Total = 116.4 V/m
E Category: M4
Location: -2, -2, 364.8 mm

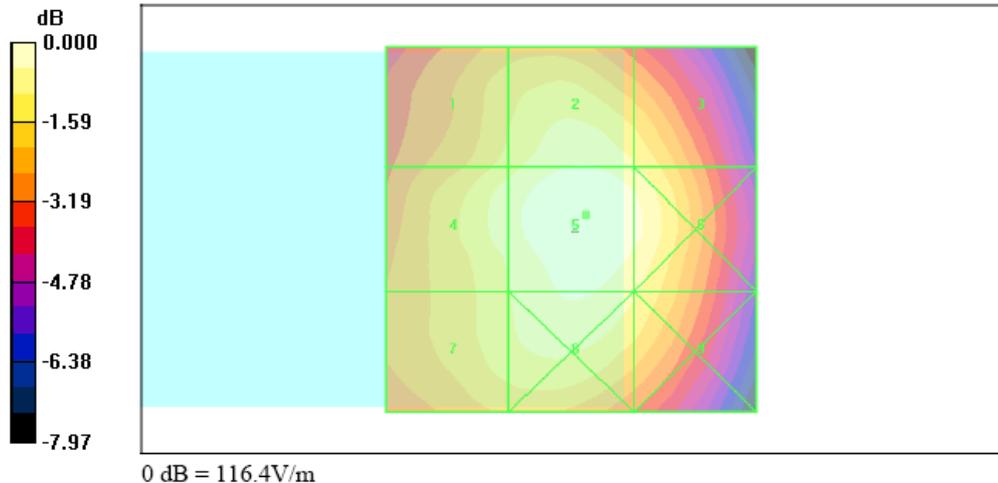



Test Laboratory: Sporton International Inc. SAR/HAC Testing Lab

Date:2008/4/2

HAC_E_CDMA850 Ch384_RC3 SO55_Loop_Full_Backlight On

DUT: 830102

Communication System: CDMA ; Frequency: 836.52 MHz;Duty Cycle: 1:1
Medium: Air Medium parameters used: $\sigma = 0$ mho/m, $\epsilon_r = 1$; $\rho = 1000$ kg/m³
Ambient Temperature : 22.9 °C

DASY4 Configuration:

- Probe: ER3DV6 - SN2358; ConvF(1, 1, 1); Calibrated: 2008/1/28
- Sensor-Surface: (Fix Surface)
- Electronics: DAE4 Sn778; Calibrated: 2007/9/17
- Phantom: HAC Test Arch 4.6; Type: SD HAC P01 BA;
- Measurement SW: DASY4, V4.7 Build 55; Postprocessing SW: SEMCAD, V1.8 Build 176

Ch384/Hearing Aid Compatibility Test (101x101x1): Measurement grid: dx=5mm, dy=5mm

Maximum value of peak Total field = 117.0 V/m

Probe Modulation Factor = 0.980

Device Reference Point: 0.000, 0.000, 353.7 mm

Reference Value = 128.4 V/m; Power Drift = 0.028 dB

Hearing Aid Near-Field Category: M4 (AWF 0 dB)

Peak E-field in V/m


Grid 1	Grid 2	Grid 3
100.6 M4	110.2 M4	104.3 M4
Grid 4	Grid 5	Grid 6
107.1 M4	117.0 M4	111.8 M4
Grid 7	Grid 8	Grid 9
102.9 M4	110.9 M4	104.9 M4

Cursor:

Total = 117.0 V/m

E Category: M4

Location: -3, -1.5, 364.8 mm

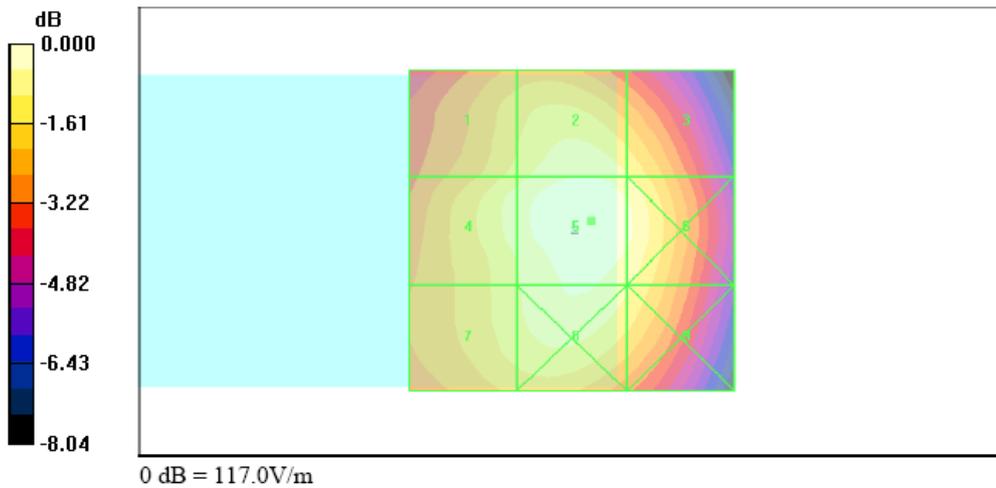



Test Laboratory: Sporton International Inc. SAR/HAC Testing Lab

Date:2008/4/2

HAC_E_CDMA850 Ch384_RC3 SO55_Loop_Full_Bluetooth On

DUT: 830102

Communication System: CDMA ; Frequency: 836.52 MHz;Duty Cycle: 1:1
Medium: Air Medium parameters used: sigma = 0 mho/m, epsilon_r = 1; rho = 1000 kg/m^3
Ambient Temperature : 22.9 C

DASY4 Configuration:

- Probe: ER3DV6 - SN2358; ConvF(1, 1, 1); Calibrated: 2008/1/28
- Sensor-Surface: (Fix Surface)
- Electronics: DAE4 Sn778; Calibrated: 2007/9/17
- Phantom: HAC Test Arch 4.6; Type: SD HAC P01 BA
- Measurement SW: DASY4, V4.7 Build 55; Postprocessing SW: SEMCAD, V1.8 Build 176

Ch384/Hearing Aid Compatibility Test (101x101x1): Measurement grid: dx=5mm, dy=5mm


Maximum value of peak Total field = 115.4 V/m
Probe Modulation Factor = 0.970
Device Reference Point: 0.000, 0.000, 353.7 mm
Reference Value = 129.2 V/m; Power Drift = -0.073 dB
Hearing Aid Near-Field Category: M4 (AWF 0 dB)

Peak E-field in V/m

Table with 3 columns (Grid 1-9) and 3 rows of peak E-field values in V/m, ranging from 100.1 M4 to 115.4 M4.

Cursor:

Total = 115.4 V/m
E Category: M4
Location: -3, -1, 364.8 mm

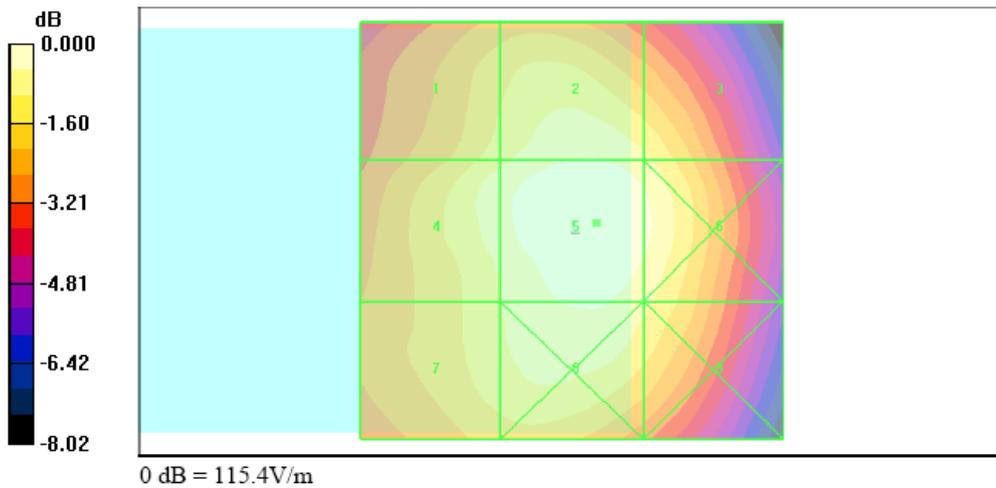



Test Laboratory: Sporton International Inc. SAR/HAC Testing Lab

Date:2008/4/2

HAC_E_CDMA850 Ch777_RC3 SO55_Loop_Full

DUT: 830102

Communication System: CDMA ; Frequency: 848.31 MHz;Duty Cycle: 1:1
Medium: Air Medium parameters used: sigma = 0 mho/m, epsilon_r = 1; rho = 1000 kg/m^3
Ambient Temperature : 22.9 C


- DASY4 Configuration:
- Probe: ER3DV6 - SN2358; ConvF(1, 1, 1); Calibrated: 2008/1/28
- Sensor-Surface: (Fix Surface)
- Electronics: DAE4 Sn778; Calibrated: 2007/9/17
- Phantom: HAC Test Arch 4.6; Type: SD HAC P01 BA
- Measurement SW: DASY4, V4.7 Build 55; Postprocessing SW: SEMCAD, V1.8 Build 176

Ch777/Hearing Aid Compatibility Test (101x101x1): Measurement grid: dx=5mm, dy=5mm
Maximum value of peak Total field = 96.6 V/m
Probe Modulation Factor = 0.970
Device Reference Point: 0.000, 0.000, 353.7 mm
Reference Value = 107.1 V/m; Power Drift = 0.021 dB
Hearing Aid Near-Field Category: M4 (AWF 0 dB)

Peak E-field in V/m

Table with 3 columns (Grid 1-3, Grid 4-6, Grid 7-9) and 3 rows of peak E-field values in V/m (e.g., 83.0 M4, 91.1 M4, 86.2 M4).

Cursor:
Total = 96.6 V/m
E Category: M4
Location: -2.5, -1.5, 364.8 mm

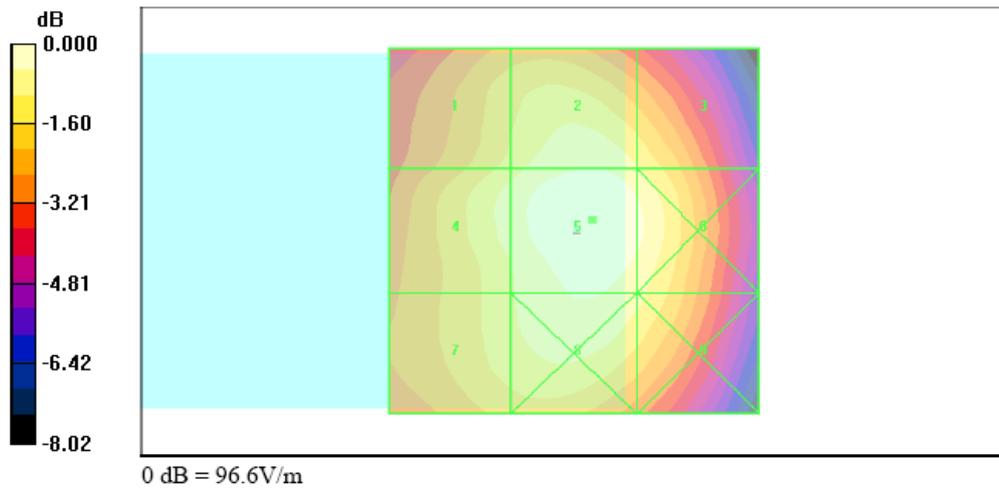



Test Laboratory: Sporton International Inc. SAR/HAC Testing Lab

Date:2008/4/2

HAC_E_CDMA1700 Ch25_RC3 SO55_Loop_Full

DUT: 830102

Communication System: CDMA ; Frequency: 1711.25 MHz;Duty Cycle: 1:1
Medium: Air Medium parameters used: $\sigma = 0$ mho/m, $\epsilon_r = 1$; $\rho = 1000$ kg/m³
Ambient Temperature : 22.7 °C

DASY4 Configuration:

- Probe: ER3DV6 - SN2358; ConvF(1, 1, 1); Calibrated: 2008/1/28
- Sensor-Surface: (Fix Surface)
- Electronics: DAE4 Sn778; Calibrated: 2007/9/17
- Phantom: HAC Test Arch 4.6; Type: SD HAC P01 BA
- Measurement SW: DASY4, V4.7 Build 55; Postprocessing SW: SEMCAD, V1.8 Build 176

Ch25/Hearing Aid Compatibility Test (101x101x1): Measurement grid: dx=5mm, dy=5mm


Maximum value of peak Total field = 52.1 V/m
Probe Modulation Factor = 0.980
Device Reference Point: 0.000, 0.000, 353.7 mm
Reference Value = 53.6 V/m; Power Drift = -0.075 dB
Hearing Aid Near-Field Category: M4 (AWF 0 dB)

Peak E-field in V/m

Grid 1	Grid 2	Grid 3
34.1 M4	42.1 M4	41.6 M4
Grid 4	Grid 5	Grid 6
48.6 M4	52.1 M4	48.8 M4
Grid 7	Grid 8	Grid 9
53.5 M4	54.4 M4	48.8 M4

Cursor:

Total = 54.4 V/m
E Category: M4
Location: 3.5, 17.5, 364.8 mm

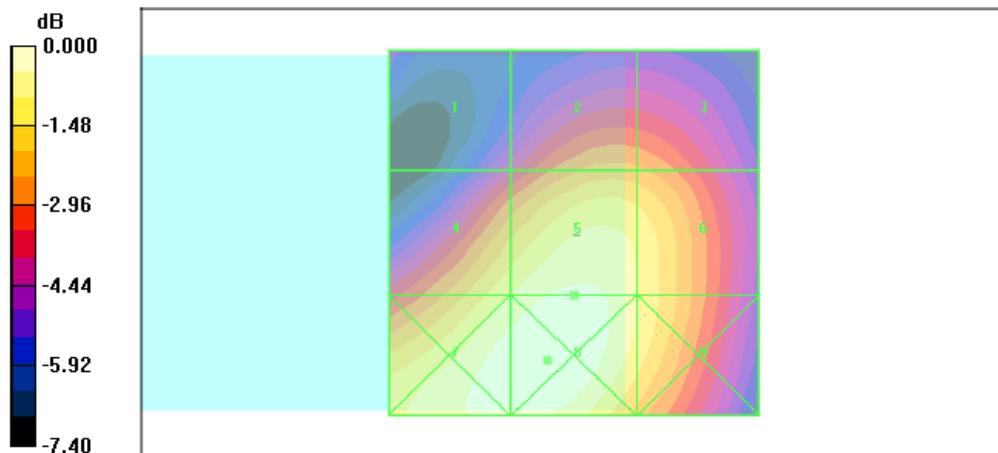

0 dB = 54.4V/m



Test Laboratory: Sporton International Inc. SAR/HAC Testing Lab

Date:2008/4/2

HAC_E_CDMA1700 Ch450_RC3 SO55_Loop_Full

DUT: 830102

Communication System: CDMA ; Frequency: 1732.5 MHz;Duty Cycle: 1:1
Medium: Air Medium parameters used: $\sigma = 0$ mho/m, $\epsilon_r = 1$; $\rho = 1000$ kg/m³
Ambient Temperature : 22.9 °C

DASY4 Configuration:

- Probe: ER3DV6 - SN2358; ConvF(1, 1, 1); Calibrated: 2008/1/28
- Sensor-Surface: (Fix Surface)
- Electronics: DAE4 Sn778; Calibrated: 2007/9/17
- Phantom: HAC Test Arch 4.6; Type: SD HAC P01 BA;
- Measurement SW: DASY4, V4.7 Build 55; Postprocessing SW: SEMCAD, V1.8 Build 176

Ch450/Hearing Aid Compatibility Test (101x101x1): Measurement grid: dx=5mm, dy=5mm

Maximum value of peak Total field = 52.5 V/m

Probe Modulation Factor = 0.980

Device Reference Point: 0.000, 0.000, 353.7 mm

Reference Value = 52.6 V/m; Power Drift = -0.059 dB

Hearing Aid Near-Field Category: M4 (AWF 0 dB)

Peak E-field in V/m


Grid 1	Grid 2	Grid 3
33.6 M4	42.2 M4	42.0 M4
Grid 4	Grid 5	Grid 6
47.2 M4	52.5 M4	50.1 M4
Grid 7	Grid 8	Grid 9
52.9 M4	54.8 M4	50.1 M4

Cursor:

Total = 54.8 V/m

E Category: M4

Location: 1.5, 16.5, 364.8 mm

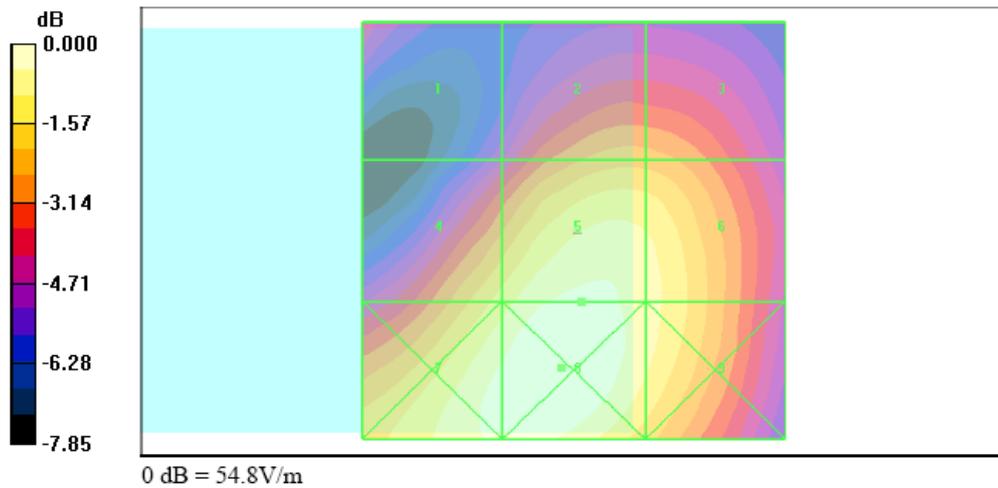



Test Laboratory: Sporton International Inc. SAR/HAC Testing Lab

Date:2008/4/2

HAC_E_CDMA1700 Ch875_RC3 SO55_Loop_Full

DUT: 830102; Type

Communication System: CDMA ; Frequency: 1753.75 MHz;Duty Cycle: 1:1
Medium: Air Medium parameters used: $\sigma = 0$ mho/m, $\epsilon_r = 1$; $\rho = 1000$ kg/m³
Ambient Temperature : 22.7 °C

DASY4 Configuration:

- Probe: ER3DV6 - SN2358; ConvF(1, 1, 1); Calibrated: 2008/1/28
- Sensor-Surface: (Fix Surface)
- Electronics: DAE4 Sn778; Calibrated: 2007/9/17
- Phantom: HAC Test Arch 4.6; Type: SD HAC P01 BA;
- Measurement SW: DASY4, V4.7 Build 55; Postprocessing SW: SEMCAD, V1.8 Build 176

Ch875/Hearing Aid Compatibility Test (101x101x1): Measurement grid: dx=5mm, dy=5mm

Maximum value of peak Total field = 53.9 V/m

Probe Modulation Factor = 0.980

Device Reference Point: 0.000, 0.000, 353.7 mm

Reference Value = 53.1 V/m; Power Drift = -0.088 dB

Hearing Aid Near-Field Category: M4 (AWF 0 dB)

Peak E-field in V/m


Grid 1	Grid 2	Grid 3
37.4 M4	41.9 M4	41.7 M4
Grid 4	Grid 5	Grid 6
48.3 M4	53.9 M4	51.6 M4
Grid 7	Grid 8	Grid 9
55.2 M4	56.6 M4	51.8 M4

Cursor:

Total = 56.6 V/m

E Category: M4

Location: 2, 18, 364.8 mm

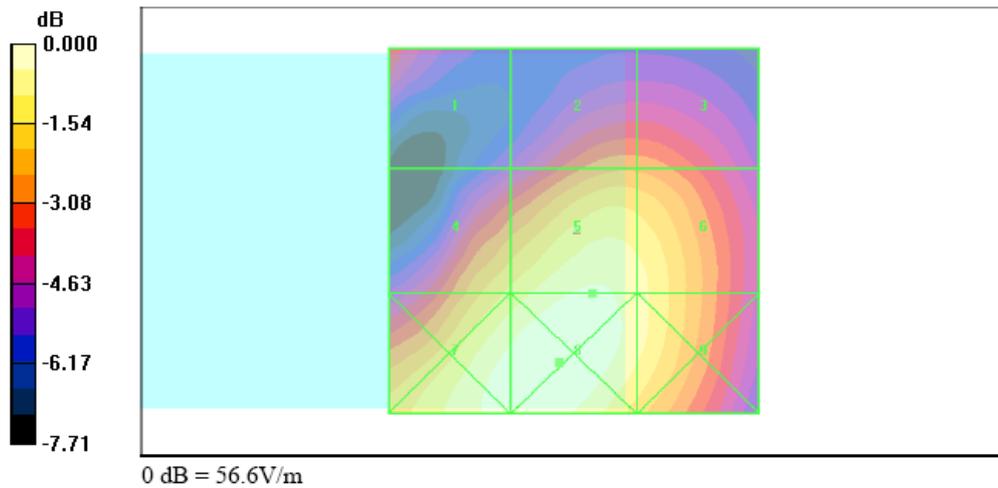



Test Laboratory: Sporton International Inc. SAR/HAC Testing Lab

Date:2008/4/2

HAC_E_CDMA1700 Ch875_RC3 SO55_Loop_Full_Backlight On

DUT: 830102

Communication System: CDMA ; Frequency: 1753.75 MHz;Duty Cycle: 1:1
Medium: Air Medium parameters used: $\sigma = 0$ mho/m, $\epsilon_r = 1$; $\rho = 1000$ kg/m³
Ambient Temperature : 22.7 °C

DASY4 Configuration:

- Probe: ER3DV6 - SN2358; ConvF(1, 1, 1); Calibrated: 2008/1/28
- Sensor-Surface: (Fix Surface)
- Electronics: DAE4 Sn778; Calibrated: 2007/9/17
- Phantom: HAC Test Arch 4.6; Type: SD HAC P01 BA;
- Measurement SW: DASY4, V4.7 Build 55; Postprocessing SW: SEMCAD, V1.8 Build 176

Ch875/Hearing Aid Compatibility Test (101x101x1): Measurement grid: dx=5mm, dy=5mm

Maximum value of peak Total field = 54.5 V/m

Probe Modulation Factor = 0.980

Device Reference Point: 0.000, 0.000, 353.7 mm

Reference Value = 52.8 V/m; Power Drift = 0.071 dB

Hearing Aid Near-Field Category: M4 (AWF 0 dB)

Peak E-field in V/m


Grid 1	Grid 2	Grid 3
37.7 M4	42.2 M4	41.9 M4
Grid 4	Grid 5	Grid 6
48.1 M4	54.5 M4	52.1 M4
Grid 7	Grid 8	Grid 9
55.3 M4	57.3 M4	52.3 M4

Cursor:

Total = 57.3 V/m

E Category: M4

Location: 1.5, 17, 364.8 mm

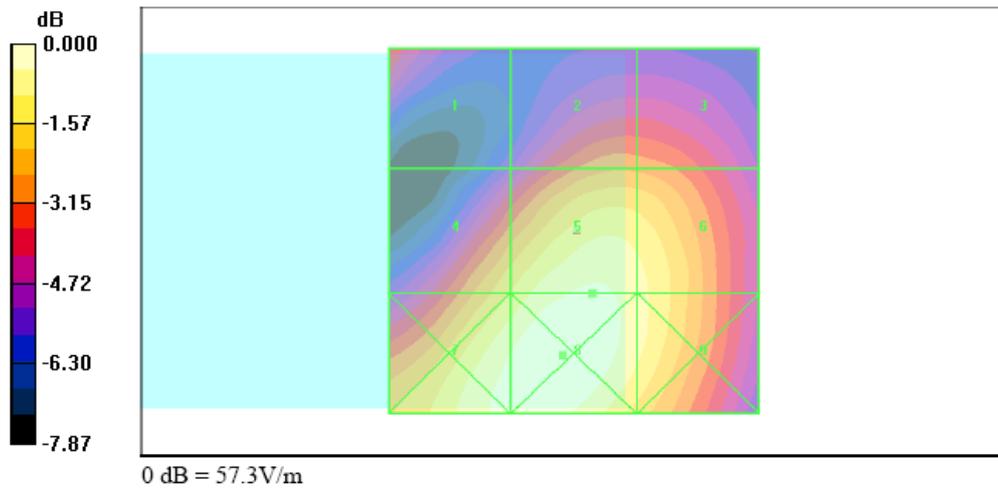



Test Laboratory: Sporton International Inc. SAR/HAC Testing Lab

Date:2008/4/2

HAC_E_CDMA1700 Ch875_RC3 SO55_Loop_Full_Bluetooth On

DUT: 830102

Communication System: CDMA ; Frequency: 1753.75 MHz;Duty Cycle: 1:1
Medium: Air Medium parameters used: sigma = 0 mho/m, epsilon_r = 1; rho = 1000 kg/m^3
Ambient Temperature : 22.7 C

DASY4 Configuration:

- Probe: ER3DV6 - SN2358; ConvF(1, 1, 1); Calibrated: 2008/1/28
- Sensor-Surface: (Fix Surface)
- Electronics: DAE4 Sn778; Calibrated: 2007/9/17
- Phantom: HAC Test Arch 4.6; Type: SD HAC P01 BA
- Measurement SW: DASY4, V4.7 Build 55; Postprocessing SW: SEMCAD, V1.8 Build 176

Ch875/Hearing Aid Compatibility Test (101x101x1): Measurement grid: dx=5mm, dy=5mm

Maximum value of peak Total field = 54.4 V/m

Probe Modulation Factor = 0.980

Device Reference Point: 0.000, 0.000, 353.7 mm

Reference Value = 53.0 V/m; Power Drift = 0.007 dB

Hearing Aid Near-Field Category: M4 (AWF 0 dB)

Peak E-field in V/m


Table with 3 columns (Grid 1-3, Grid 4-6, Grid 7-9) and 3 rows of peak E-field values in V/m, ranging from 37.5 M4 to 56.6 M4.

Cursor:

Total = 56.6 V/m

E Category: M4

Location: 1.5, 17.5, 364.8 mm

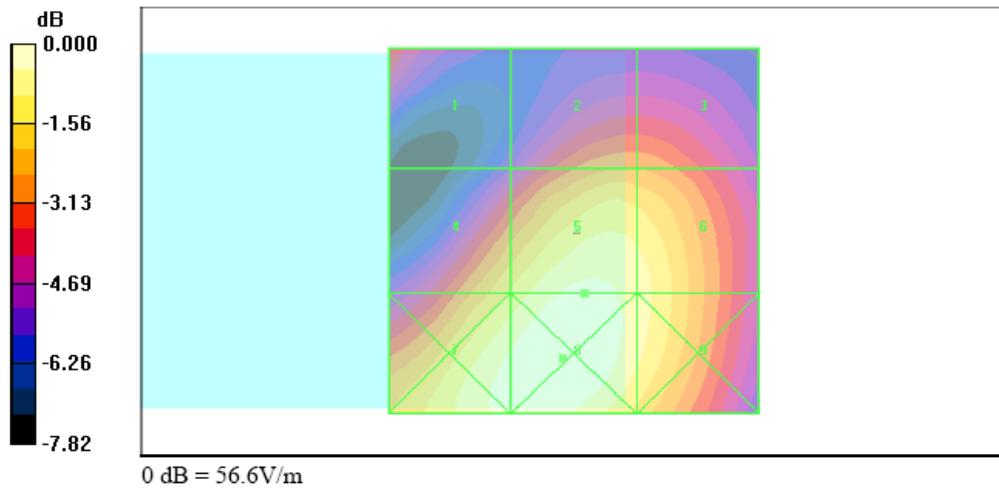



Test Laboratory: Sporton International Inc. SAR/HAC Testing Lab

Date:2008/4/2

HAC_E_CDMA1900 Ch25_RC3 SO55_Loop_Full

DUT: 830102

Communication System: CDMA ; Frequency: 1851.25 MHz;Duty Cycle: 1:1
Medium: Air Medium parameters used: $\sigma = 0$ mho/m, $\epsilon_r = 1$; $\rho = 1000$ kg/m³
Ambient Temperature : 22.0 °C

DASY4 Configuration:

- Probe: ER3DV6 - SN2358; ConvF(1, 1, 1); Calibrated: 2008/1/28
- Sensor-Surface: (Fix Surface)
- Electronics: DAE4 Sn778; Calibrated: 2007/9/17
- Phantom: HAC Test Arch 4.6; Type: SD HAC P01 BA
- Measurement SW: DASY4, V4.7 Build 55; Postprocessing SW: SEMCAD, V1.8 Build 176

Ch25/Hearing Aid Compatibility Test (101x101x1): Measurement grid: dx=5mm, dy=5mm


Maximum value of peak Total field = 41.5 V/m
Probe Modulation Factor = 0.980
Device Reference Point: 0.000, 0.000, 353.7 mm
Reference Value = 39.8 V/m; Power Drift = 0.090 dB
Hearing Aid Near-Field Category: M4 (AWF 0 dB)

Peak E-field in V/m

Grid 1	Grid 2	Grid 3
26.7 M4	31.4 M4	31.3 M4
Grid 4	Grid 5	Grid 6
35.5 M4	41.5 M4	40.2 M4
Grid 7	Grid 8	Grid 9
40.9 M4	43.3 M4	40.3 M4

Cursor:

Total = 43.3 V/m
E Category: M4
Location: 0.5, 18.5, 364.8 mm

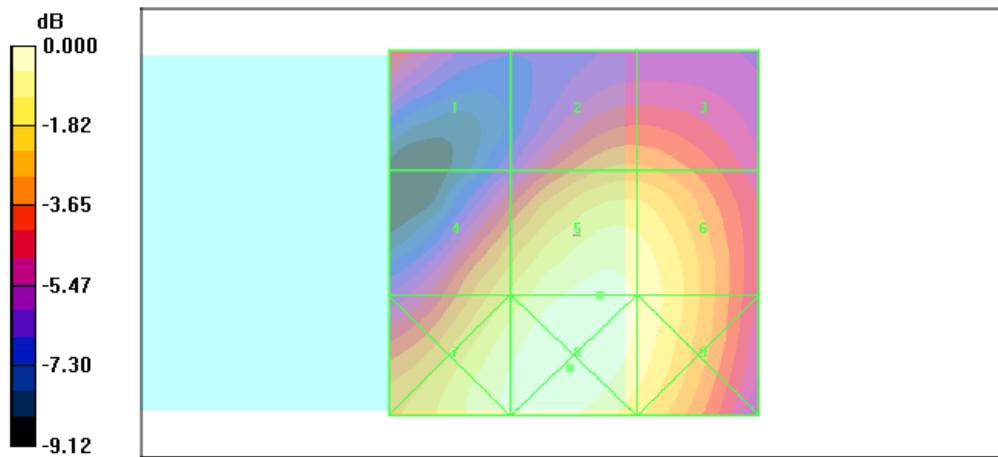

0 dB = 43.3V/m



Test Laboratory: Sporton International Inc. SAR/HAC Testing Lab

Date:2008/4/2

HAC_E_CDMA1900 Ch600_RC3 SO55_Loop_Full

DUT: 830102


Communication System: CDMA ; Frequency: 1880 MHz;Duty Cycle: 1:1
Medium: Air Medium parameters used: sigma = 0 mho/m, epsilon_r = 1; rho = 1000 kg/m^3
Ambient Temperature : 22.7 C

- DASY4 Configuration:
- Probe: ER3DV6 - SN2358; ConvF(1, 1, 1); Calibrated: 2008/1/28
- Sensor-Surface: (Fix Surface)
- Electronics: DAE4 Sn778; Calibrated: 2007/9/17
- Phantom: HAC Test Arch 4.6; Type: SD HAC P01 BA
- Measurement SW: DASY4, V4.7 Build 55; Postprocessing SW: SEMCAD, V1.8 Build 176

Ch600/Hearing Aid Compatibility Test (101x101x1): Measurement grid: dx=5mm, dy=5mm
Maximum value of peak Total field = 43.9 V/m
Probe Modulation Factor = 0.980
Device Reference Point: 0.000, 0.000, 353.7 mm
Reference Value = 40.4 V/m; Power Drift = -0.027 dB
Hearing Aid Near-Field Category: M4 (AWF 0 dB)

Peak E-field in V/m
Table with 3 columns (Grid 1-3, Grid 4-6, Grid 7-9) and 3 rows of values (e.g., 31.2 M4, 31.0 M4, 31.0 M4)

Cursor:
Total = 46.9 V/m
E Category: M4
Location: 1.5, 19, 364.8 mm

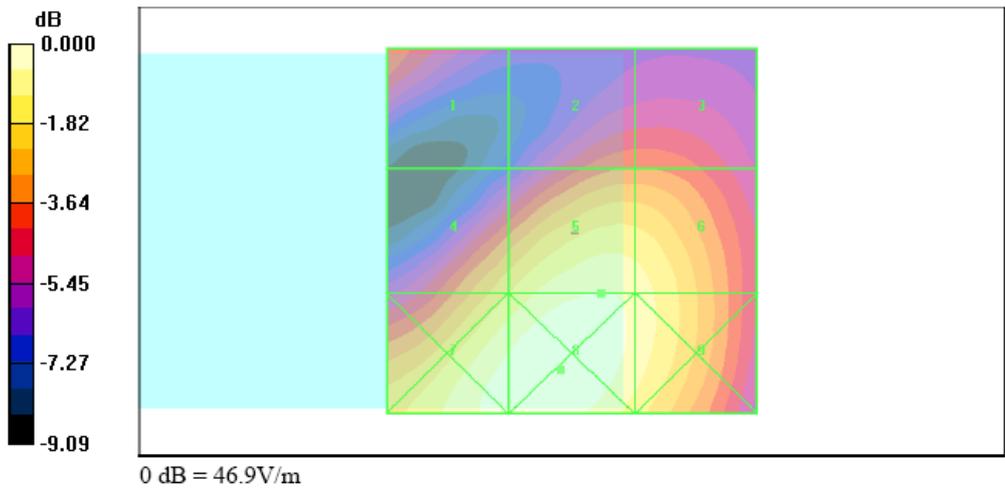



Test Laboratory: Sporton International Inc. SAR/HAC Testing Lab

Date:2008/4/2

HAC_E_CDMA1900 Ch600_RC3 SO55_Loop_Full_Backlight On

DUT: 830102

Communication System: CDMA ; Frequency: 1880 MHz;Duty Cycle: 1:1
Medium: Air Medium parameters used: $\sigma = 0$ mho/m, $\epsilon_r = 1$; $\rho = 1000$ kg/m³
Ambient Temperature : 22.7 °C

DASY4 Configuration:

- Probe: ER3DV6 - SN2358; ConvF(1, 1, 1); Calibrated: 2008/1/28
- Sensor-Surface: (Fix Surface)
- Electronics: DAE4 Sn778; Calibrated: 2007/9/17
- Phantom: HAC Test Arch 4.6; Type: SD HAC P01 BA
- Measurement SW: DASY4, V4.7 Build 55; Postprocessing SW: SEMCAD, V1.8 Build 176

Ch600/Hearing Aid Compatibility Test (101x101x1): Measurement grid: dx=5mm, dy=5mm

Maximum value of peak Total field = 43.5 V/m

Probe Modulation Factor = 0.980

Device Reference Point: 0.000, 0.000, 353.7 mm

Reference Value = 40.0 V/m; Power Drift = -0.020 dB

Hearing Aid Near-Field Category: M4 (AWF 0 dB)

Peak E-field in V/m


Grid 1	Grid 2	Grid 3
31.7 M4	30.7 M4	30.7 M4
Grid 4	Grid 5	Grid 6
37.6 M4	43.5 M4	42.1 M4
Grid 7	Grid 8	Grid 9
45.3 M4	46.7 M4	42.7 M4

Cursor:

Total = 46.7 V/m

E Category: M4

Location: 3, 19.5, 364.8 mm

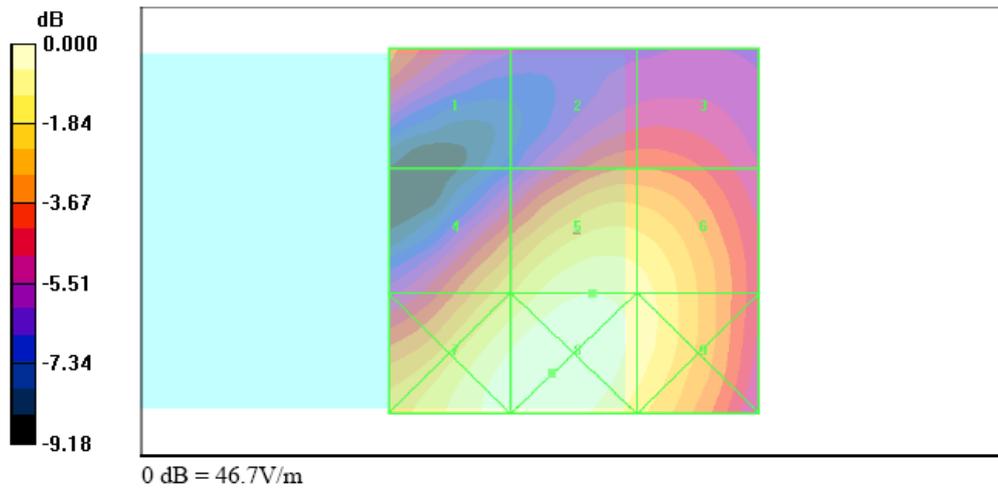



Test Laboratory: Sporton International Inc. SAR/HAC Testing Lab

Date:2008/4/2

HAC_E_CDMA1900 Ch600_RC3 SO55_Loop_Full_Bluetooth On

DUT: 830102

Communication System: CDMA ; Frequency: 1880 MHz;Duty Cycle: 1:1
Medium: Air Medium parameters used: $\sigma = 0$ mho/m, $\epsilon_r = 1$; $\rho = 1000$ kg/m³
Ambient Temperature : 22.7 °C

DASY4 Configuration:

- Probe: ER3DV6 - SN2358; ConvF(1, 1, 1); Calibrated: 2008/1/28
- Sensor-Surface: (Fix Surface)
- Electronics: DAE4 Sn778; Calibrated: 2007/9/17
- Phantom: HAC Test Arch 4.6; Type: SD HAC P01 BA;
- Measurement SW: DASY4, V4.7 Build 55; Postprocessing SW: SEMCAD, V1.8 Build 176

Ch600/Hearing Aid Compatibility Test (101x101x1): Measurement grid: dx=5mm, dy=5mm


Maximum value of peak Total field = 43.6 V/m
Probe Modulation Factor = 0.980
Device Reference Point: 0.000, 0.000, 353.7 mm
Reference Value = 40.3 V/m; Power Drift = -0.049 dB
Hearing Aid Near-Field Category: M4 (AWF 0 dB)

Peak E-field in V/m

Grid 1	Grid 2	Grid 3
31.6 M4	30.8 M4	30.8 M4
Grid 4	Grid 5	Grid 6
37.5 M4	43.6 M4	42.1 M4
Grid 7	Grid 8	Grid 9
45.3 M4	46.7 M4	42.8 M4

Cursor:

Total = 46.7 V/m
E Category: M4
Location: 1.5, 18.5, 364.8 mm

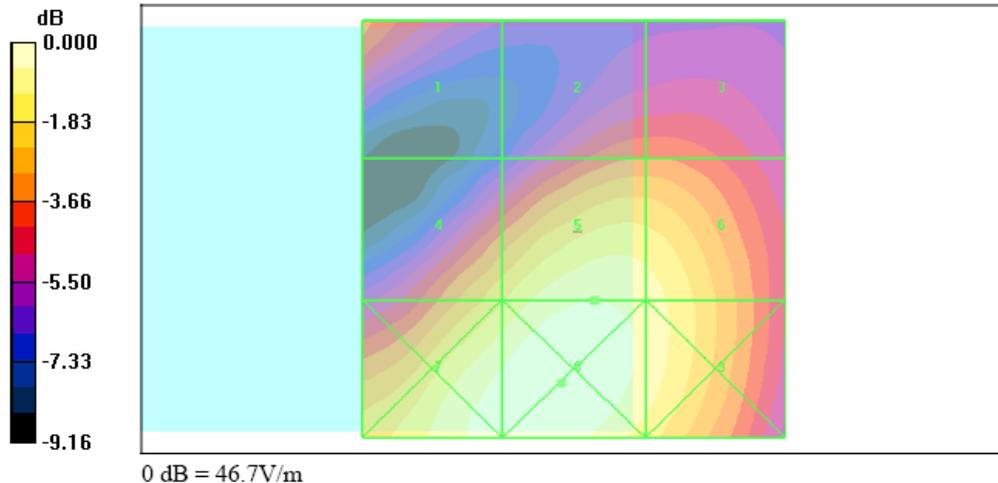



Test Laboratory: Sporton International Inc. SAR/HAC Testing Lab

Date:2008/4/2

HAC_E_CDMA1900 Ch1175_RC3 SO55_Loop_Full

DUT: 830102

Communication System: CDMA ; Frequency: 1908.75 MHz;Duty Cycle: 1:1
Medium: Air Medium parameters used: $\sigma = 0$ mho/m, $\epsilon_r = 1$; $\rho = 1000$ kg/m³
Ambient Temperature : 22.6 °C

DASY4 Configuration:

- Probe: ER3DV6 - SN2358; ConvF(1, 1, 1); Calibrated: 2008/1/28
- Sensor-Surface: (Fix Surface)
- Electronics: DAE4 Sn778; Calibrated: 2007/9/17
- Phantom: HAC Test Arch 4.6; Type: SD HAC P01 BA
- Measurement SW: DASY4, V4.7 Build 55; Postprocessing SW: SEMCAD, V1.8 Build 176

Ch1175/Hearing Aid Compatibility Test (101x101x1): Measurement grid: dx=5mm, dy=5mm


Maximum value of peak Total field = 37.1 V/m
Probe Modulation Factor = 0.980
Device Reference Point: 0.000, 0.000, 353.7 mm
Reference Value = 33.2 V/m; Power Drift = -0.026 dB
Hearing Aid Near-Field Category: M4 (AWF 0 dB)

Peak E-field in V/m

Grid 1	Grid 2	Grid 3
32.0 M4	25.6 M4	25.6 M4
Grid 4	Grid 5	Grid 6
32.3 M4	37.1 M4	35.7 M4
Grid 7	Grid 8	Grid 9
39.8 M4	40.3 M4	36.5 M4

Cursor:

Total = 40.3 V/m
E Category: M4
Location: 3, 20.5, 364.8 mm

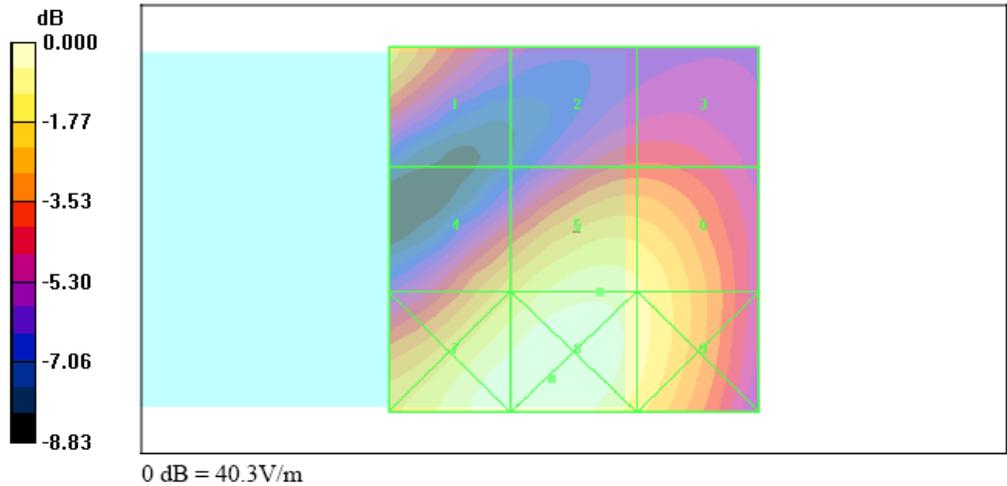



Test Laboratory: Sporton International Inc. SAR/HAC Testing Lab

Date:2008/4/2

HAC_H_CDMA850 Ch1013_RC3 SO55_Loop_Full

DUT: 830102

Communication System: CDMA ; Frequency: 824.7 MHz;Duty Cycle: 1:1

Medium: Air Medium parameters used: $\sigma = 0$ mho/m, $\epsilon_r = 1$; $\rho = 1$ kg/m³

Ambient Temperature : 22.9 °C

DASY4 Configuration:

- Probe: H3DV6 - SN6184; ; Calibrated: 2008/1/28
- Sensor-Surface: (Fix Surface)
- Electronics: DAE4 Sn778; Calibrated: 2007/9/17
- Phantom: HAC Test Arch 4.6; Type: SD HAC P01 BA
- Measurement SW: DASY4, V4.7 Build 55; Postprocessing SW: SEMCAD, V1.8 Build 176

Ch1013/Hearing Aid Compatibility Test (101x101x1): Measurement grid: dx=5mm, dy=5mm

Maximum value of peak Total field = 0.171 A/m

Probe Modulation Factor = 0.980

Device Reference Point: 0.000, 0.000, 353.7 mm

Reference Value = 0.090 A/m; Power Drift = -0.096 dB

Hearing Aid Near-Field Category: M4 (AWF 0 dB)

Peak H-field in A/m


Grid 1	Grid 2	Grid 3
0.171 M4	0.117 M4	0.068 M4
Grid 4	Grid 5	Grid 6
0.169 M4	0.116 M4	0.065 M4
Grid 7	Grid 8	Grid 9
0.163 M4	0.111 M4	0.060 M4

Cursor:

Total = 0.171 A/m

H Category: M4

Location: 25, -18, 365.6 mm

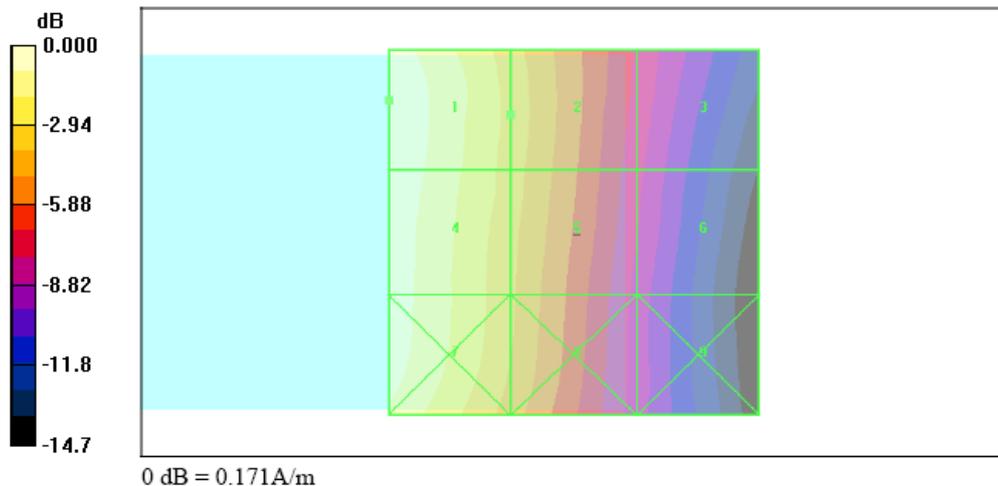



Test Laboratory: Sporton International Inc. SAR/HAC Testing Lab

Date:2008/4/2

HAC_H_CDMA850 Ch384_RC3 SO55_Loop_Full

DUT: 830102

Communication System: CDMA ; Frequency: 836.52 MHz;Duty Cycle: 1:1

Medium: Air Medium parameters used: $\sigma = 0$ mho/m, $\epsilon_r = 1$; $\rho = 1$ kg/m³

Ambient Temperature : 22.9 °C

DASY4 Configuration:

- Probe: H3DV6 - SN6184; ; Calibrated: 2008/1/28
- Sensor-Surface: (Fix Surface)
- Electronics: DAE4 Sn778; Calibrated: 2007/9/17
- Phantom: HAC Test Arch 4.6; Type: SD HAC P01 BA
- Measurement SW: DASY4, V4.7 Build 55; Postprocessing SW: SEMCAD, V1.8 Build 176

Ch384/Hearing Aid Compatibility Test (101x101x1): Measurement grid: dx=5mm, dy=5mm

Maximum value of peak Total field = 0.202 A/m

Probe Modulation Factor = 0.980

Device Reference Point: 0.000, 0.000, 353.7 mm

Reference Value = 0.110 A/m; Power Drift = 0.007 dB

Hearing Aid Near-Field Category: M4 (AWF 0 dB)

Peak H-field in A/m


Grid 1	Grid 2	Grid 3
0.202 M4	0.140 M4	0.082 M4
Grid 4	Grid 5	Grid 6
0.200 M4	0.138 M4	0.078 M4
Grid 7	Grid 8	Grid 9
0.197 M4	0.133 M4	0.073 M4

Cursor:

Total = 0.202 A/m

H Category: M4

Location: 25, -14, 365.6 mm

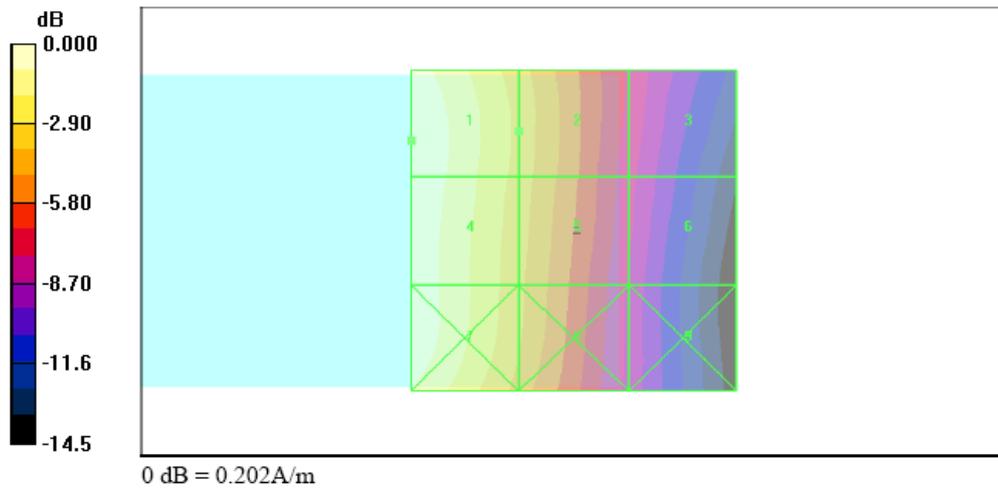



Test Laboratory: Sporton International Inc. SAR/HAC Testing Lab

Date:2008/4/2

HAC_H_CDMA850 Ch384_RC3 SO55_Loop_Full Backlight On

DUT: 830102

Communication System: CDMA ; Frequency: 836.52 MHz;Duty Cycle: 1:1

Medium: Air Medium parameters used: $\sigma = 0$ mho/m, $\epsilon_r = 1$; $\rho = 1$ kg/m³

Ambient Temperature : 22.9 °C

DASY4 Configuration:

- Probe: H3DV6 - SN6184; ; Calibrated: 2008/1/28
- Sensor-Surface: (Fix Surface)
- Electronics: DAE4 Sn778; Calibrated: 2007/9/17
- Phantom: HAC Test Arch 4.6; Type: SD HAC P01 BA
- Measurement SW: DASY4, V4.7 Build 55; Postprocessing SW: SEMCAD, V1.8 Build 176

Ch384/Hearing Aid Compatibility Test (101x101x1): Measurement grid: dx=5mm, dy=5mm

Maximum value of peak Total field = 0.202 A/m

Probe Modulation Factor = 0.980

Device Reference Point: 0.000, 0.000, 353.7 mm

Reference Value = 0.109 A/m; Power Drift = -0.029 dB

Hearing Aid Near-Field Category: M4 (AWF 0 dB)

Peak H-field in A/m


Grid 1	Grid 2	Grid 3
0.202 M4	0.140 M4	0.081 M4
Grid 4	Grid 5	Grid 6
0.199 M4	0.138 M4	0.078 M4
Grid 7	Grid 8	Grid 9
0.196 M4	0.133 M4	0.073 M4

Cursor:

Total = 0.202 A/m

H Category: M4

Location: 25, -14.5, 365.6 mm

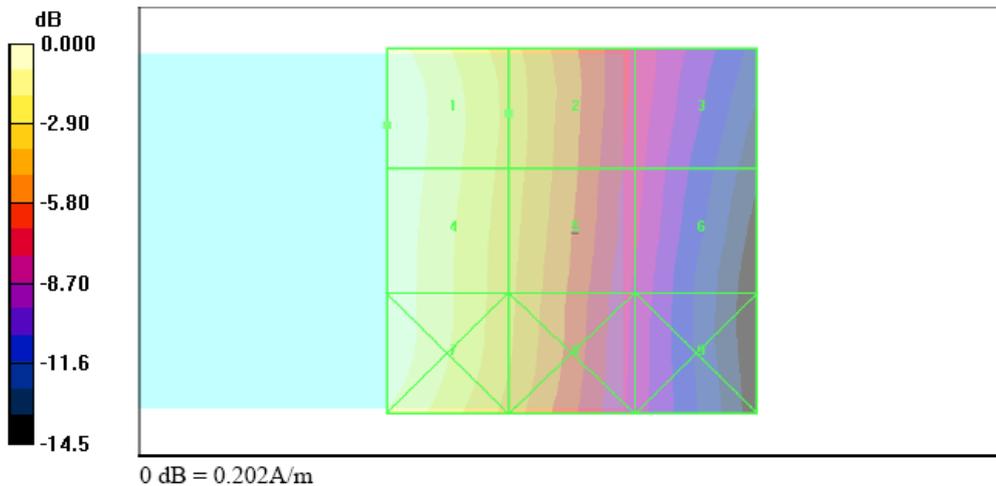



Test Laboratory: Sporton International Inc. SAR/HAC Testing Lab

Date:2008/4/2

HAC_H_CDMA850 Ch384_RC3 SO55_Loop_Full Bluetooth On

DUT: 830102

Communication System: CDMA ; Frequency: 836.52 MHz;Duty Cycle: 1:1

Medium: Air Medium parameters used: $\sigma = 0$ mho/m, $\epsilon_r = 1$; $\rho = 1$ kg/m³

Ambient Temperature : 22.9 °C

DASY4 Configuration:

- Probe: H3DV6 - SN6184; ; Calibrated: 2008/1/28
- Sensor-Surface: (Fix Surface)
- Electronics: DAE4 Sn778; Calibrated: 2007/9/17
- Phantom: HAC Test Arch 4.6; Type: SD HAC P01 BA
- Measurement SW: DASY4, V4.7 Build 55; Postprocessing SW: SEMCAD, V1.8 Build 176

Ch384/Hearing Aid Compatibility Test (101x101x1): Measurement grid: dx=5mm, dy=5mm

Maximum value of peak Total field = 0.202 A/m

Probe Modulation Factor = 0.980

Device Reference Point: 0.000, 0.000, 353.7 mm

Reference Value = 0.108 A/m; Power Drift = 0.047 dB

Hearing Aid Near-Field Category: M4 (AWF 0 dB)

Peak H-field in A/m


Grid 1	Grid 2	Grid 3
0.202 M4	0.140 M4	0.082 M4
Grid 4	Grid 5	Grid 6
0.198 M4	0.138 M4	0.078 M4
Grid 7	Grid 8	Grid 9
0.196 M4	0.133 M4	0.073 M4

Cursor:

Total = 0.202 A/m

H Category: M4

Location: 25, -15, 365.6 mm

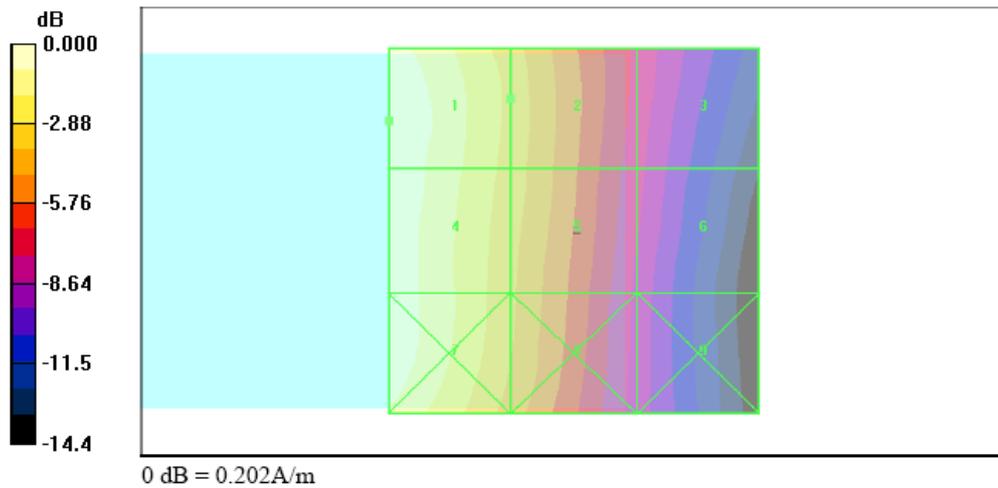



Test Laboratory: Sporton International Inc. SAR/HAC Testing Lab

Date:2008/4/2

HAC_H_CDMA850 Ch777_RC3 SO55_Loop_Full

DUT: 830102

Communication System: CDMA ; Frequency: 848.31 MHz;Duty Cycle: 1:1

Medium: Air Medium parameters used: $\sigma = 0$ mho/m, $\epsilon_r = 1$; $\rho = 1$ kg/m³

Ambient Temperature : 22.9 °C

DASY4 Configuration:

- Probe: H3DV6 - SN6184; ; Calibrated: 2008/1/28
- Sensor-Surface: (Fix Surface)
- Electronics: DAE4 Sn778; Calibrated: 2007/9/17
- Phantom: HAC Test Arch 4.6; Type: SD HAC P01 BA
- Measurement SW: DASY4, V4.7 Build 55; Postprocessing SW: SEMCAD, V1.8 Build 176

Ch777/Hearing Aid Compatibility Test (101x101x1): Measurement grid: dx=5mm, dy=5mm

Maximum value of peak Total field = 0.171 A/m

Probe Modulation Factor = 0.980

Device Reference Point: 0.000, 0.000, 353.7 mm

Reference Value = 0.094 A/m; Power Drift = -0.054 dB

Hearing Aid Near-Field Category: M4 (AWF 0 dB)

Peak H-field in A/m


Grid 1	Grid 2	Grid 3
0.171 M4	0.119 M4	0.069 M4
Grid 4	Grid 5	Grid 6
0.169 M4	0.117 M4	0.066 M4
Grid 7	Grid 8	Grid 9
0.167 M4	0.114 M4	0.063 M4

Cursor:

Total = 0.171 A/m

H Category: M4

Location: 25, -17.5, 365.6 mm

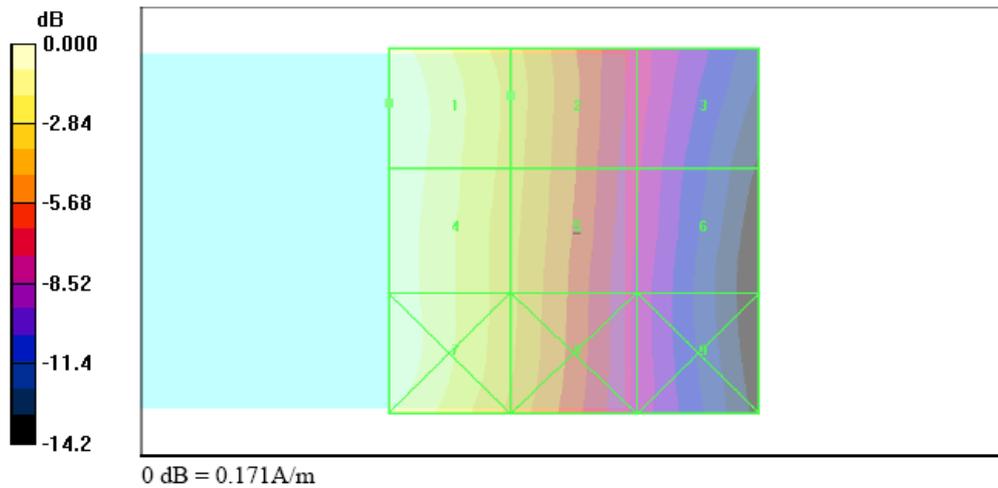



Test Laboratory: Sporton International Inc. SAR/HAC Testing Lab

Date:2008/4/2

HAC_H_CDMA1700 Ch25_RC3 SO55_Loop_Full

DUT: 830102

Communication System: CDMA ; Frequency: 1711.25 MHz;Duty Cycle: 1:1

Medium: Air Medium parameters used: $\sigma = 0$ mho/m, $\epsilon_r = 1$; $\rho = 1$ kg/m³

Ambient Temperature : 22.9 °C

DASY4 Configuration:

- Probe: H3DV6 - SN6184; ; Calibrated: 2008/1/28
- Sensor-Surface: (Fix Surface)
- Electronics: DAE4 Sn778; Calibrated: 2007/9/17
- Phantom: HAC Test Arch 4.6; Type: SD HAC P01 BA;
- Measurement SW: DASY4, V4.7 Build 55; Postprocessing SW: SEMCAD, V1.8 Build 176

Ch25/Hearing Aid Compatibility Test (101x101x1): Measurement grid: dx=5mm, dy=5mm

Maximum value of peak Total field = 0.145 A/m

Probe Modulation Factor = 0.990

Device Reference Point: 0.000, 0.000, 353.7 mm

Reference Value = 0.097 A/m; Power Drift = -0.060 dB

Hearing Aid Near-Field Category: M4 (AWF 0 dB)

Peak H-field in A/m


Grid 1	Grid 2	Grid 3
0.136 M4	0.122 M4	0.095 M4
Grid 4	Grid 5	Grid 6
0.145 M4	0.118 M4	0.087 M4
Grid 7	Grid 8	Grid 9
0.149 M4	0.109 M4	0.067 M4

Cursor:

Total = 0.149 A/m

H Category: M4

Location: 25, 15.5, 365.6 mm

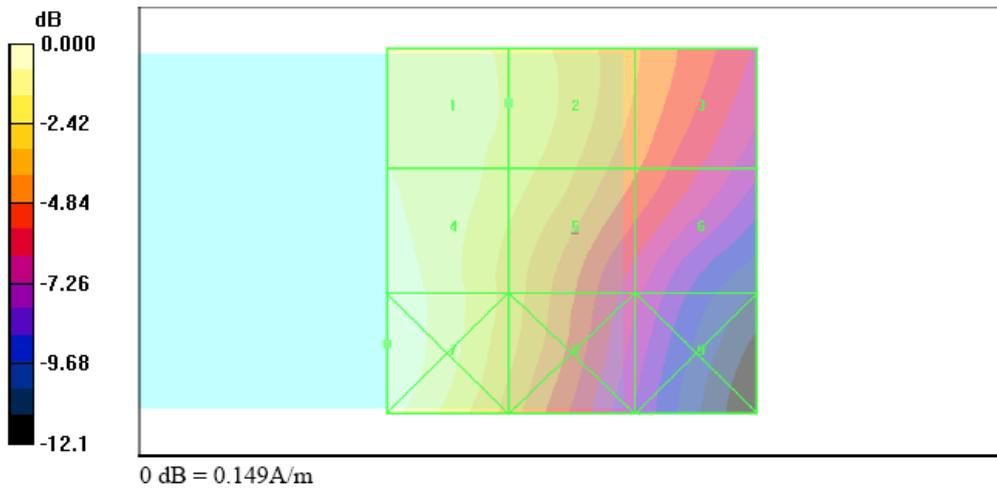



Test Laboratory: Sporton International Inc. SAR/HAC Testing Lab

Date:2008/4/2

HAC_H_CDMA1700 Ch450_RC3 SO55_Loop_Full

DUT: 830102

Communication System: CDMA ; Frequency: 1732.5 MHz;Duty Cycle: 1:1

Medium: Air Medium parameters used: $\sigma = 0$ mho/m, $\epsilon_r = 1$; $\rho = 1$ kg/m³

Ambient Temperature : 22.9 °C

DASY4 Configuration:

- Probe: H3DV6 - SN6184; ; Calibrated: 2008/1/28
- Sensor-Surface: (Fix Surface)
- Electronics: DAE4 Sn778; Calibrated: 2007/9/17
- Phantom: HAC Test Arch 4.6; Type: SD HAC P01 BA;
- Measurement SW: DASY4, V4.7 Build 55; Postprocessing SW: SEMCAD, V1.8 Build 176

Ch450/Hearing Aid Compatibility Test (101x101x1): Measurement grid: dx=5mm, dy=5mm

Maximum value of peak Total field = 0.151 A/m

Probe Modulation Factor = 0.990

Device Reference Point: 0.000, 0.000, 353.7 mm

Reference Value = 0.106 A/m; Power Drift = 0.117 dB

Hearing Aid Near-Field Category: M4 (AWF 0 dB)

Peak H-field in A/m


Grid 1	Grid 2	Grid 3
0.138 M4	0.129 M4	0.102 M4
Grid 4	Grid 5	Grid 6
0.151 M4	0.126 M4	0.095 M4
Grid 7	Grid 8	Grid 9
0.156 M4	0.117 M4	0.073 M4

Cursor:

Total = 0.156 A/m

H Category: M4

Location: 25, 17, 365.6 mm

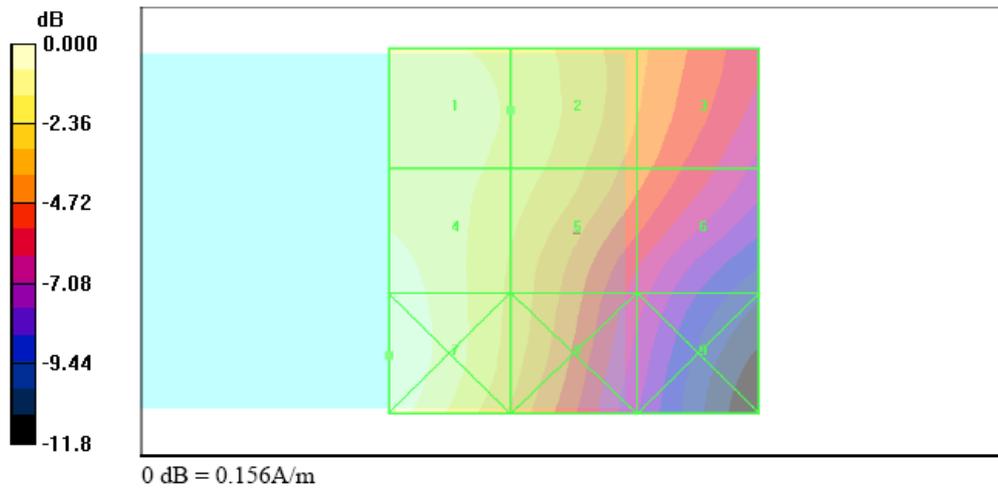



Test Laboratory: Sporton International Inc. SAR/HAC Testing Lab

Date:2008/4/2

HAC_H_CDMA1700 Ch875_RC3 SO55_Loop_Full

DUT: 830102

Communication System: CDMA ; Frequency: 1753.75 MHz;Duty Cycle: 1:1

Medium: Air Medium parameters used: $\sigma = 0$ mho/m, $\epsilon_r = 1$; $\rho = 1$ kg/m³

Ambient Temperature : 22.7 °C

DASY4 Configuration:

- Probe: H3DV6 - SN6184; ; Calibrated: 2008/1/28
- Sensor-Surface: (Fix Surface)
- Electronics: DAE4 Sn778; Calibrated: 2007/9/17
- Phantom: HAC Test Arch 4.6; Type: SD HAC P01 BA
- Measurement SW: DASY4, V4.7 Build 55; Postprocessing SW: SEMCAD, V1.8 Build 176

Ch875/Hearing Aid Compatibility Test (101x101x1): Measurement grid: dx=5mm, dy=5mm

Maximum value of peak Total field = 0.157 A/m

Probe Modulation Factor = 0.990

Device Reference Point: 0.000, 0.000, 353.7 mm

Reference Value = 0.116 A/m; Power Drift = -0.090 dB

Hearing Aid Near-Field Category: M4 (AWF 0 dB)

Peak H-field in A/m


Grid 1	Grid 2	Grid 3
0.140 M4	0.134 M4	0.108 M4
Grid 4	Grid 5	Grid 6
0.157 M4	0.131 M4	0.103 M4
Grid 7	Grid 8	Grid 9
0.164 M4	0.123 M4	0.081 M4

Cursor:

Total = 0.164 A/m

H Category: M4

Location: 25, 17.5, 365.6 mm

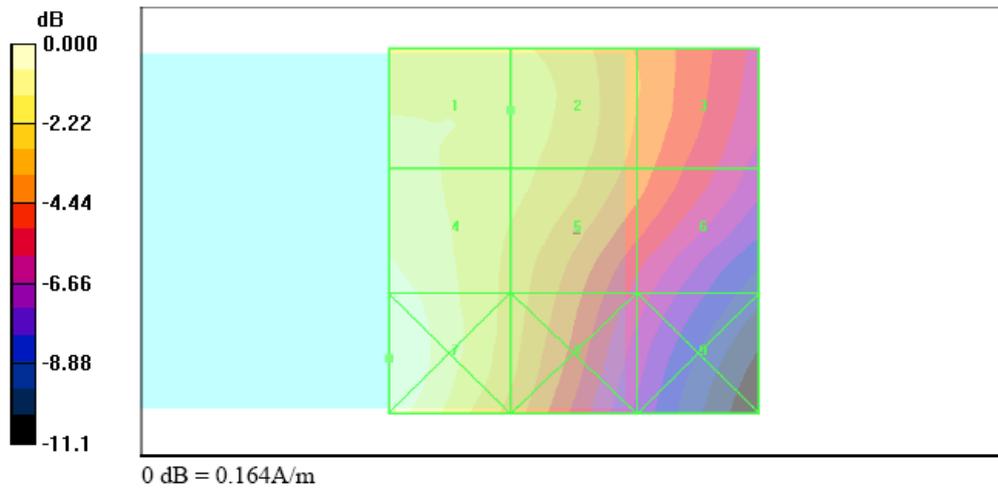



Test Laboratory: Sporton International Inc. SAR/HAC Testing Lab

Date:2008/4/2

HAC_H_CDMA1700 Ch875_RC3 SO55_Loop_Full Backlight On

DUT: 830102

Communication System: CDMA ; Frequency: 1753.75 MHz;Duty Cycle: 1:1

Medium: Air Medium parameters used: $\sigma = 0$ mho/m, $\epsilon_r = 1$; $\rho = 1$ kg/m³

Ambient Temperature : 22.9 °C

DASY4 Configuration:

- Probe: H3DV6 - SN6184; ; Calibrated: 2008/1/28
- Sensor-Surface: (Fix Surface)
- Electronics: DAE4 Sn778; Calibrated: 2007/9/17
- Phantom: HAC Test Arch 4.6; Type: SD HAC P01 BA;
- Measurement SW: DASY4, V4.7 Build 55; Postprocessing SW: SEMCAD, V1.8 Build 176

Ch875/Hearing Aid Compatibility Test (101x101x1): Measurement grid: dx=5mm, dy=5mm

Maximum value of peak Total field = 0.155 A/m

Probe Modulation Factor = 0.990

Device Reference Point: 0.000, 0.000, 353.7 mm

Reference Value = 0.114 A/m; Power Drift = 0.006 dB

Hearing Aid Near-Field Category: M4 (AWF 0 dB)

Peak H-field in A/m


Grid 1	Grid 2	Grid 3
0.140 M4	0.134 M4	0.108 M4
Grid 4	Grid 5	Grid 6
0.155 M4	0.132 M4	0.104 M4
Grid 7	Grid 8	Grid 9
0.162 M4	0.124 M4	0.081 M4

Cursor:

Total = 0.162 A/m

H Category: M4

Location: 25, 18, 365.6 mm

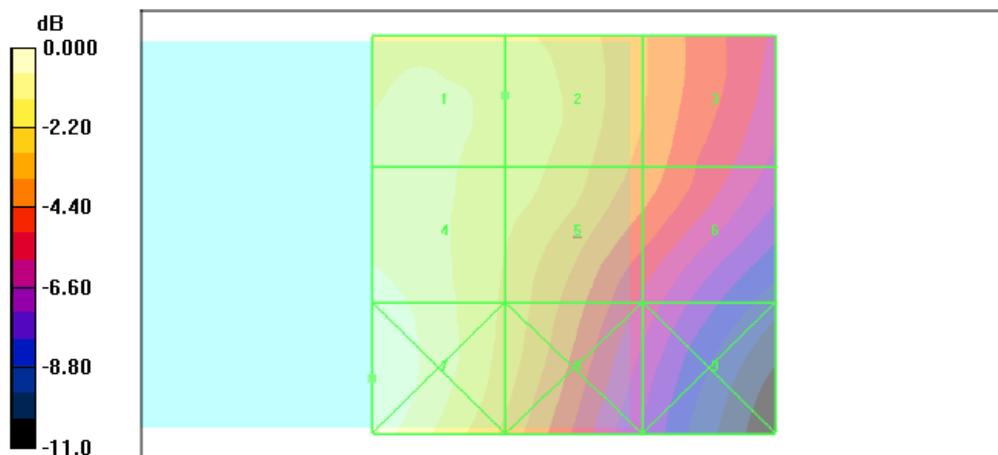



Test Laboratory: Sporton International Inc. SAR/HAC Testing Lab

Date:2008/4/2

HAC_H_CDMA1700 Ch875_RC3 SO55_Loop_Full Bluetooth On

DUT: 830102

Communication System: CDMA ; Frequency: 1753.75 MHz;Duty Cycle: 1:1

Medium: Air Medium parameters used: $\sigma = 0$ mho/m, $\epsilon_r = 1$; $\rho = 1$ kg/m³

Ambient Temperature : 22.9 °C

DASY4 Configuration:

- Probe: H3DV6 - SN6184; ; Calibrated: 2008/1/28
- Sensor-Surface: (Fix Surface)
- Electronics: DAE4 Sn778; Calibrated: 2007/9/17
- Phantom: HAC Test Arch 4.6; Type: SD HAC P01 BA
- Measurement SW: DASY4, V4.7 Build 55; Postprocessing SW: SEMCAD, V1.8 Build 176

Ch875/Hearing Aid Compatibility Test (101x101x1): Measurement grid: dx=5mm, dy=5mm

Maximum value of peak Total field = 0.156 A/m

Probe Modulation Factor = 0.990

Device Reference Point: 0.000, 0.000, 353.7 mm

Reference Value = 0.115 A/m; Power Drift = -0.012 dB

Hearing Aid Near-Field Category: M4 (AWF 0 dB)

Peak H-field in A/m


Grid 1	Grid 2	Grid 3
0.139 M4	0.135 M4	0.108 M4
Grid 4	Grid 5	Grid 6
0.156 M4	0.132 M4	0.104 M4
Grid 7	Grid 8	Grid 9
0.162 M4	0.124 M4	0.080 M4

Cursor:

Total = 0.162 A/m

H Category: M4

Location: 25, 17, 365.6 mm

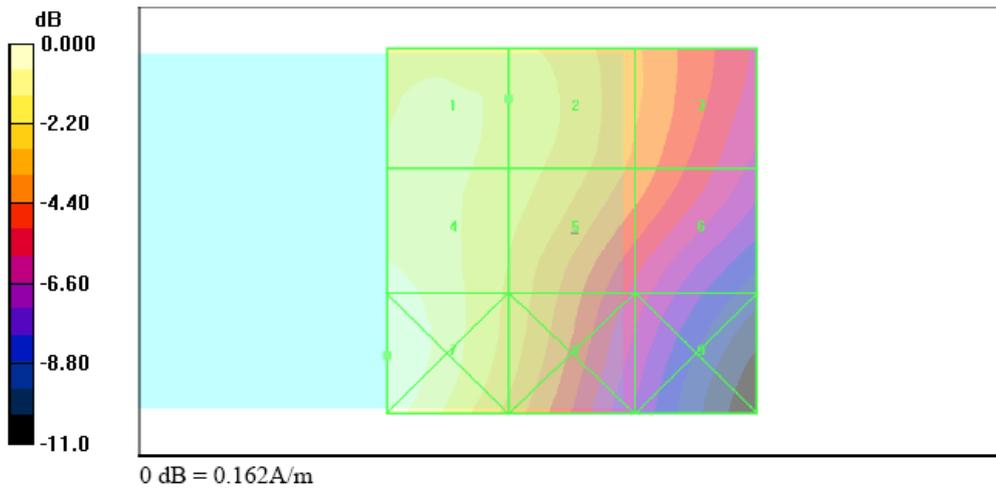



Test Laboratory: Sporton International Inc. SAR/HAC Testing Lab

Date:2008/4/2

HAC_H_CDMA1900 Ch25_RC3 SO55_Loop_Full

DUT: 830102

Communication System: CDMA ; Frequency: 1851.25 MHz;Duty Cycle: 1:1

Medium: Air Medium parameters used: $\sigma = 0$ mho/m, $\epsilon_r = 1$; $\rho = 1$ kg/m³

Ambient Temperature : 22.8 °C

DASY4 Configuration:

- Probe: H3DV6 - SN6184; ; Calibrated: 2008/1/28
- Sensor-Surface: (Fix Surface)
- Electronics: DAE4 Sn778; Calibrated: 2007/9/17
- Phantom: HAC Test Arch 4.6; Type: SD HAC P01 BA
- Measurement SW: DASY4, V4.7 Build 55; Postprocessing SW: SEMCAD, V1.8 Build 176

Ch25/Hearing Aid Compatibility Test (101x101x1): Measurement grid: dx=5mm, dy=5mm

Maximum value of peak Total field = 0.110 A/m

Probe Modulation Factor = 0.990

Device Reference Point: 0.000, 0.000, 353.7 mm

Reference Value = 0.085 A/m; Power Drift = 0.139 dB

Hearing Aid Near-Field Category: M4 (AWF 0 dB)

Peak H-field in A/m


Grid 1	Grid 2	Grid 3
0.096 M4	0.096 M4	0.083 M4
Grid 4	Grid 5	Grid 6
0.110 M4	0.094 M4	0.080 M4
Grid 7	Grid 8	Grid 9
0.121 M4	0.089 M4	0.062 M4

Cursor:

Total = 0.121 A/m

H Category: M4

Location: 25, 19.5, 365.6 mm

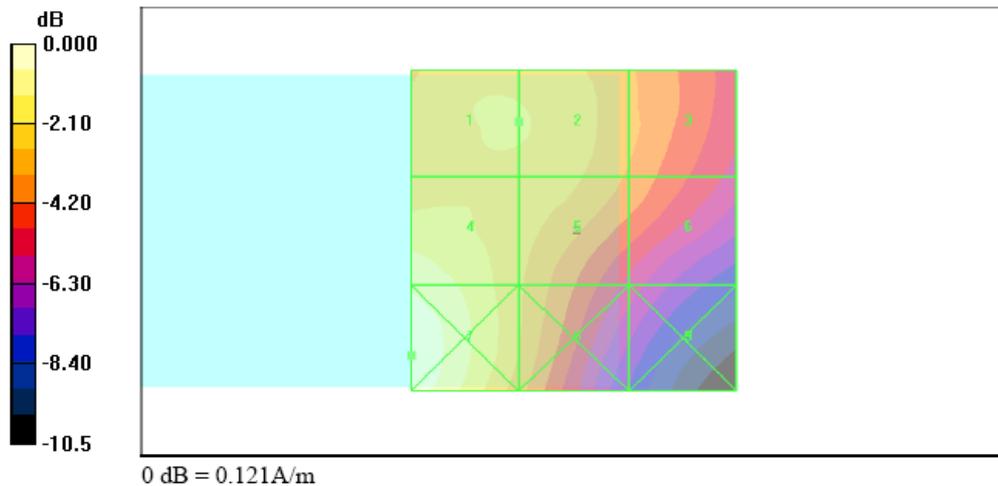



Test Laboratory: Sporton International Inc. SAR/HAC Testing Lab

Date:2008/4/2

HAC_H_CDMA1900 Ch600_RC3 SO55_Loop_Full

DUT: 830102

Communication System: CDMA ; Frequency: 1880 MHz;Duty Cycle: 1:1

Medium: Air Medium parameters used: $\sigma = 0$ mho/m, $\epsilon_r = 1$; $\rho = 1$ kg/m³

Ambient Temperature : 22.7 °C

DASY4 Configuration:

- Probe: H3DV6 - SN6184; ; Calibrated: 2008/1/28
- Sensor-Surface: (Fix Surface)
- Electronics: DAE4 Sn778; Calibrated: 2007/9/17
- Phantom: HAC Test Arch 4.6; Type: SD HAC P01 BA
- Measurement SW: DASY4, V4.7 Build 55; Postprocessing SW: SEMCAD, V1.8 Build 176

Ch600/Hearing Aid Compatibility Test (101x101x1): Measurement grid: dx=5mm, dy=5mm

Maximum value of peak Total field = 0.116 A/m

Probe Modulation Factor = 0.990

Device Reference Point: 0.000, 0.000, 353.7 mm

Reference Value = 0.096 A/m; Power Drift = 0.027 dB

Hearing Aid Near-Field Category: M4 (AWF 0 dB)

Peak H-field in A/m


Grid 1	Grid 2	Grid 3
0.104 M4	0.104 M4	0.094 M4
Grid 4	Grid 5	Grid 6
0.116 M4	0.102 M4	0.092 M4
Grid 7	Grid 8	Grid 9
0.130 M4	0.097 M4	0.072 M4

Cursor:

Total = 0.130 A/m

H Category: M4

Location: 25, 21, 365.6 mm

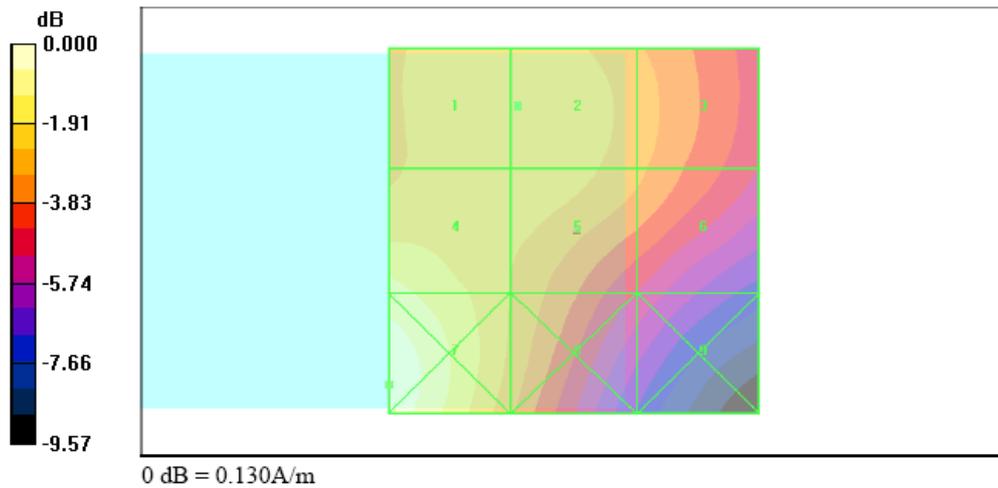



Test Laboratory: Sporton International Inc. SAR/HAC Testing Lab

Date:2008/4/2

HAC_H_CDMA1900 Ch600_RC3 SO55_Loop_Full Backlight On

DUT: 830102

Communication System: CDMA ; Frequency: 1880 MHz;Duty Cycle: 1:1

Medium: Air Medium parameters used: $\sigma = 0$ mho/m, $\epsilon_r = 1$; $\rho = 1$ kg/m³

Ambient Temperature : 23.1 °C

DASY4 Configuration:

- Probe: H3DV6 - SN6184; ; Calibrated: 2008/1/28
- Sensor-Surface: (Fix Surface)
- Electronics: DAE4 Sn778; Calibrated: 2007/9/17
- Phantom: HAC Test Arch 4.6; Type: SD HAC P01 BA;
- Measurement SW: DASY4, V4.7 Build 55; Postprocessing SW: SEMCAD, V1.8 Build 176

Ch600/Hearing Aid Compatibility Test (101x101x1): Measurement grid: dx=5mm, dy=5mm

Maximum value of peak Total field = 0.117 A/m

Probe Modulation Factor = 0.990

Device Reference Point: 0.000, 0.000, 353.7 mm

Reference Value = 0.097 A/m; Power Drift = -0.059 dB

Hearing Aid Near-Field Category: M4 (AWF 0 dB)

Peak H-field in A/m


Grid 1	Grid 2	Grid 3
0.104 M4	0.104 M4	0.094 M4
Grid 4	Grid 5	Grid 6
0.117 M4	0.102 M4	0.092 M4
Grid 7	Grid 8	Grid 9
0.131 M4	0.097 M4	0.072 M4

Cursor:

Total = 0.131 A/m

H Category: M4

Location: 25, 21, 365.6 mm

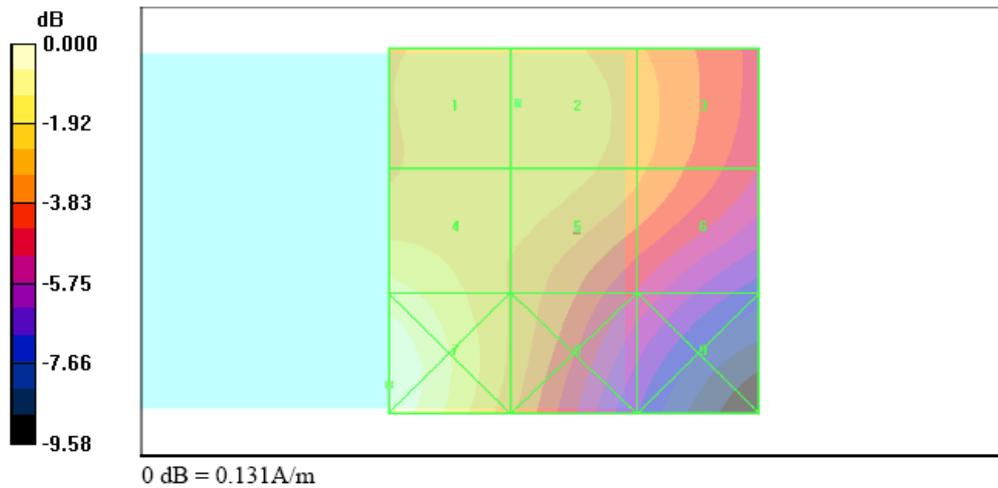



Test Laboratory: Sporton International Inc. SAR/HAC Testing Lab

Date:2008/4/2

HAC_H_CDMA1900 Ch600_RC3 SO55_Loop_Full Bluetooth On

DUT: 830102

Communication System: CDMA ; Frequency: 1880 MHz;Duty Cycle: 1:1

Medium: Air Medium parameters used: $\sigma = 0$ mho/m, $\epsilon_r = 1$; $\rho = 1$ kg/m³

Ambient Temperature : 22.8 °C

DASY4 Configuration:

- Probe: H3DV6 - SN6184; ; Calibrated: 2008/1/28
- Sensor-Surface: (Fix Surface)
- Electronics: DAE4 Sn778; Calibrated: 2007/9/17
- Phantom: HAC Test Arch 4.6; Type: SD HAC P01 BA
- Measurement SW: DASY4, V4.7 Build 55; Postprocessing SW: SEMCAD, V1.8 Build 176

Ch600/Hearing Aid Compatibility Test (101x101x1): Measurement grid: dx=5mm, dy=5mm

Maximum value of peak Total field = 0.117 A/m

Probe Modulation Factor = 0.990

Device Reference Point: 0.000, 0.000, 353.7 mm

Reference Value = 0.096 A/m; Power Drift = 0.068 dB

Hearing Aid Near-Field Category: M4 (AWF 0 dB)

Peak H-field in A/m


Grid 1	Grid 2	Grid 3
0.104 M4	0.105 M4	0.094 M4
Grid 4	Grid 5	Grid 6
0.117 M4	0.103 M4	0.092 M4
Grid 7	Grid 8	Grid 9
0.130 M4	0.097 M4	0.071 M4

Cursor:

Total = 0.130 A/m

H Category: M4

Location: 25, 21, 365.6 mm

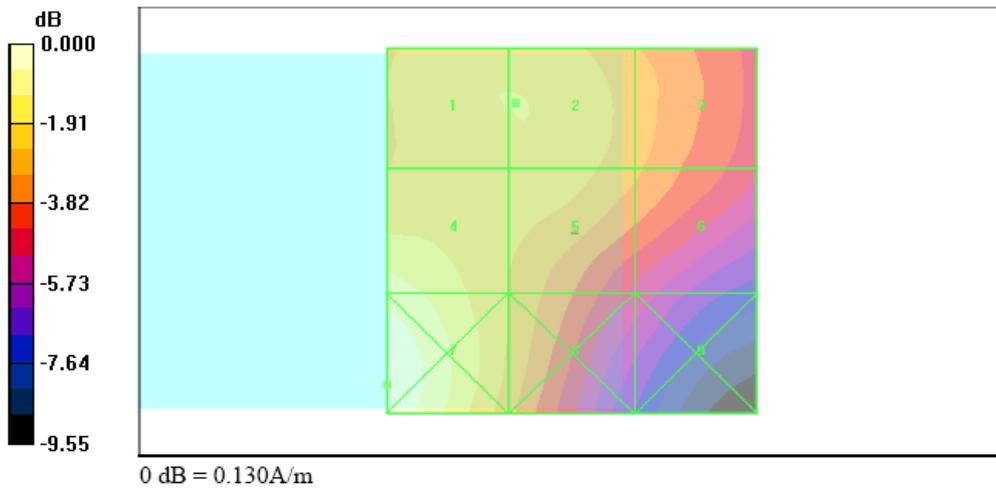



Test Laboratory: Sporton International Inc. SAR/HAC Testing Lab

Date:2008/4/2

HAC_H_CDMA1900 Ch1175_RC3 SO55_Loop_Full

DUT: 830102

Communication System: CDMA ; Frequency: 1908.75 MHz;Duty Cycle: 1:1

Medium: Air Medium parameters used: $\sigma = 0$ mho/m, $\epsilon_r = 1$; $\rho = 1$ kg/m³

Ambient Temperature : 22.5 °C

DASY4 Configuration:

- Probe: H3DV6 - SN6184; ; Calibrated: 2008/1/28
- Sensor-Surface: (Fix Surface)
- Electronics: DAE4 Sn778; Calibrated: 2007/9/17
- Phantom: HAC Test Arch 4.6; Type: SD HAC P01 BA
- Measurement SW: DASY4, V4.7 Build 55; Postprocessing SW: SEMCAD, V1.8 Build 176

Ch1175/Hearing Aid Compatibility Test (101x101x1): Measurement grid: dx=5mm, dy=5mm

Maximum value of peak Total field = 0.101 A/m

Probe Modulation Factor = 0.990

Device Reference Point: 0.000, 0.000, 353.7 mm

Reference Value = 0.087 A/m; Power Drift = 0.054 dB

Hearing Aid Near-Field Category: M4 (AWF 0 dB)

Peak H-field in A/m

Grid 1 0.093 M4	Grid 2 0.093 M4	Grid 3 0.085 M4
Grid 4 0.101 M4	Grid 5 0.092 M4	Grid 6 0.084 M4
Grid 7 0.112 M4	Grid 8 0.086 M4	Grid 9 0.066 M4

Cursor:

Total = 0.112 A/m

H Category: M4

Location: 25, 21, 365.6 mm

