

HEARING AID COMPATIBILITY

Testing Report

<RF-Emission>

Applicant Name	ZTE Corporation
Address of Applicant	ZTE Plaza, Keji Road South, Hi-Tech, Industrial Park, Nanshan District, Shenzhen, Guangdong, P.R. China 518057
EUT Type	Mobile phone
Model Number	ZTE C88
Date of receive	2007.05.30
Date of Test(s)	2007.07.10~2007.07.10
Date of Issue	2007.07.26

Standards:

ANSI PC63.19-2006 v3.12

FCC RULE PART(S): 47 CFR PART 20.19(B)

HAC RATE CATEGORY: M4 (M Category)


In the configuration tested, the EUT complied with the standards specified above.

Remarks:

This report details the results of the testing carried out on one sample, the results contained in this test report do not relate to other samples of the same product. The manufacturer should ensure that all products in series production are in conformity with the product sample detailed in this report.

This report may only be reproduced and distributed in full. If the product in this report is used in any configuration other than that detailed in the report, the manufacturer must ensure the new system complies with all relevant standards. Any mention of SGS Taiwan EC Services or testing done by SGS Taiwan EC Services in connection with distribution or use of the product described in this report must be approved by SGS Taiwan EC Services in writing.

Tested by :



Approved by:



Leo Hsu

Dikin Yang

Testing Engineer

Date: 2007/07/18

Asst. Supervisor

Date: 2007/07/26

Table of Contents

1. Introduction	3
2. Testing Laboratory	3
3. Details of Applicant.....	4
4. Description of EUT	4
5. Test Environment	4
6. System Specifications of DASY4.....	5
7. Measurement Procedure	7
8. System Verification	8
9. Probe Modulation Factor.....	8
10. Test Standards and Limits	11
11. Instruments List.....	12
12. Summary of Results	13
13.Measurement Data.....	14
14. DAE& Probe Calibration certificate.....	54
15. Uncertainty Analysis	72
16. System Validation from Original equipment supplier	73

1. Introduction

The purpose of the Hearing Aid Compatibility extension is to enable measurements of the near electric and magnetic fields generated by wireless communication devices in the region controlled for use by a hearing aid in accordance with ANSI-C63.19-2006

FCC has granted a request for waiver of the HAC rules in section 20.19 for dual band GSM handsets. The waiver has specific conditions, as stated in the order (FCC 05-166) and expires 1 August 2006.

The purpose of this standard is to establish categories for hearing aids and for WD (wireless communications devices) that can indicate to health care practitioners and hearing aid users which hearing aids are compatible with which WD, and to provide tests that can be used to assess the electromagnetic characteristics of hearing aids and WD and assign them to these categories. The various parameters required, in order to demonstrate compatibility and accessibility are measured. The design of the standard is such that when a hearing aid and WD achieve one of the categories specified, as measured by the methodology of this standard, the indicated performance is realized.

In order to provide for the usability of a hearing aid with a WD, several factors must be coordinated:

- a) Radio frequency (RF) measurements of the near-field electric and magnetic fields emitted by a WD to categorize these emissions for correlation with the RF immunity of a hearing aid.

Hence, the following are measurements made for the WD:

- a) RF E-Field emissions
- b) RF H-Field emissions

2. Testing Laboratory

Company Name	SGS Taiwan Ltd. Electronics & Communication Laboratory
Company address	134, Wu Kung Road, Wuku Industrial Zone Taipei, Taiwan, R.O.C.
Telephone	+886-2-2299-3279
Fax	+886-2-2298-0488
Website	http://www.tw.sgs.com/

3. Details of Applicant

Name	ZTE Corporation
Address	ZTE Plaza, Keji Road South, Hi-Tech, Industrial Park, Nanshan District, Shenzhen, Guangdong, P.R. China 518057
Country	China
Telephone	+86-021-68895196
Fax	N/A
Contact Person	li.dz
E-mail	li.dz@zte.com.cn

4. Description of EUT

ESN	0D5A5E88	
Mode(s) of Operation	CDMA Cellular/US PCS	
TX Frequency range (MHz)	Cellular	US PCS
	824.7~848.31	1851.25~1908.75
Channel Number (ARFCN)	1013~777	25~1175
Maximum Output Power Setting (dBm)	24.13	23.97
Duty Cycle	1	1
Battery Type	Li-ion 3.7Vdc 800mAh	
EUT Type	Mobile phone	

5. Test Environment

Ambient Temperature	22.1° C
Relative Humidity	62 %

6. System Specifications of DASY4

6.1 Measurement system Diagram for SPEAG Robotic

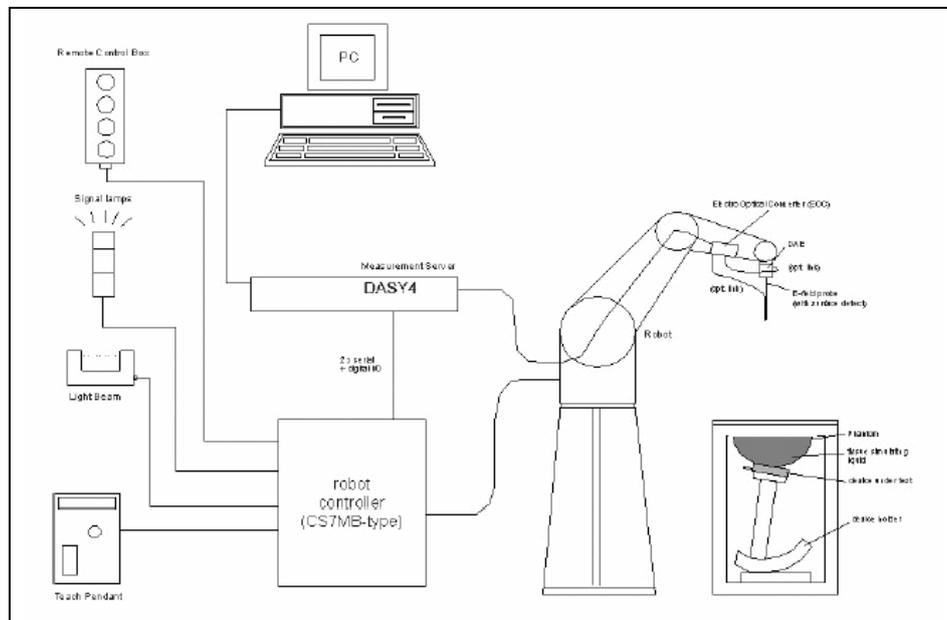


Fig 1. The SPEAG Robotic Diagram

The DASY4 system for performing compliance tests consists of the following items:

- A standard high precision 6-axis robot (Stabile RX family) with controller, teach pendant and software. An arm extension is for accommodating the data acquisition electronics (DAE).
- E and H Field probe.
- A data acquisition electronics (DAE) which performs the signal amplification, signal multiplexing, AD-conversion, offset measurements, mechanical surface detection, collision detection, etc. The unit is battery powered with standard or rechargeable batteries. The signal is optically transmitted to the EOC.
- The Electro-optical converter (EOC) performs the conversion between optical and electrical of the signals for the digital communication to the DAE and for the analog signal from the optical surface detection. The EOC is connected to the measurement server.
- The function of the measurement server is to perform the time critical tasks such as signal filtering, control of the robot operation and fast movement interrupts.
- A probe alignment unit which improves the (absolute) accuracy of the probe positioning.
- A computer operating Windows 2000 or Windows XP.
- DASY4 software.
- Remote control with teach pendant and additional circuitry for robot safety such as warning lamps, etc.
- The Test Arch phantom.

- The device holder for handheld mobile phones.
- Validation dipole kits allowing to validate the proper functioning of the system.


6.2 E and H Field Probe

Construction	One dipole parallel, two dipoles normal to probe axis Built-in shielding against static charges PEEK enclosure material	 <p>ER3DV6 E-Field Probe</p>
Calibration	In air from 100 MHz to 3.0 GHz (absolute accuracy $\pm 6.0\%$, $k=2$)	
Frequency	100 MHz to > 6 GHz (extended to 20 MHz for MRI), Linearity: ± 0.2 dB (100 MHz to 3 GHz)	
Directivity	± 0.2 dB in air (rotation around probe axis) ± 0.4 dB in air (rotation normal to probe axis)	
Dynamic Range	2 V/m to > 1000 V/m; Linearity: ± 0.2 dB	
Dimensions	Overall length: 330 mm (Tip: 16 mm) Tip diameter: 8 mm (Body: 12 mm) Distance from probe tip to dipole centers: 2.5 mm	
Application	General near-field measurements up to 6 GHz Field component measurements Fast automatic scanning in phantoms	

Construction	Three concentric loop sensors with 3.8 mm loop diameters Resistively loaded detector diodes for linear response Built-in shielding against static charges PEEK enclosure material (resistant to organic solvents, e.g., glycoether)	 <p>H3DV6 H-Field Probe</p>
Frequency	200 MHz to 3 GHz (absolute accuracy $\pm 6.0\%$, $k=2$); Output linearized	
Directivity	± 0.2 dB (spherical isotropy error)	
Dynamic Range	10 mA/m to 2 A/m at 1 GHz	
E-Field Interference	< 10% at 3 GHz (for plane wave)	

Dimensions	Overall length: 330 mm (Tip: 40 mm) Tip diameter: 6 mm (Body: 12 mm) Distance from probe tip to dipole centers: 3 mm
Application	General magnetic near-field measurements up to 3 GHz (in air or liquids) Field component measurements Surface current measurements Low interaction with the measured field

6.3 Test Arch

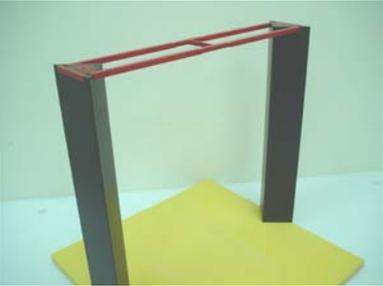Description	Enables easy and well defined positioning of the phone and validation dipoles as well as simple teaching of the robot.	
Dimensions	length: 370 mm width: 370 mm height: 370 mm	

Test Arch

6.4 Phone Holder

Description	Supports accurate and reliable positioning of any phone Effect on near field < +/- 0.5 dB	
-------------	---	--

Phone Holder

7. Measurement Procedure

The following illustrate a typical RF emissions test scan over a wireless communications device:


1. Proper operation of the field probe, probe measurement system, other instrumentation, and the positioning system was confirmed.
2. WD is positioned in its intended test position, acoustic output point of the device perpendicular to the field probe.
3. the WD operation for maximum rated RF output power was configured and confirmed with the base station simulator, at the test channel and other normal operating parameters as intended for the test. The battery was ensured to be fully charged before each test.

4. the center sub-grid was centered over the center of the acoustic output (also audio band magnetic output, if applicable). The WD audio output was positioned tangent (as physically possible) to the measurement plane.
5. A surface calibration was performed before each setup change to ensure repeatable spacing and proper maintenance of the measurement plane using the HAC Phantom.
6. The measurement system measured the field strength at the reference location.
7. Measurements at 2mm increments in the 5×5 cm region were performed and recorded. A 360° rotation about the azimuth axis at the maximum interpolated position was measured. For the worst-case condition, the peak reading from this rotation was used in re-evaluating the HAC category.
8. The system performed a drift evaluation by measuring the field at the reference location.
9. Steps 1-8 were done for both the E and H-Field measurements.

8. System Verification

A dipole antenna meeting the requirements given in PC63.19 was placed in the position normally occupied by the WD.

The length of the dipole was scanned with both E-field and H-field probes and the maximum values for each were recorded.

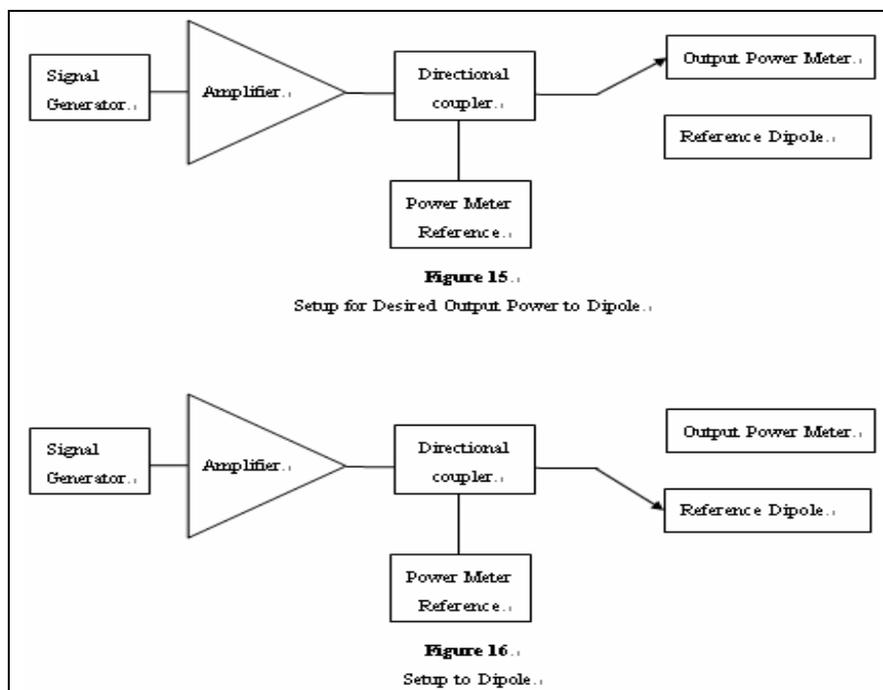

For E-Field Scan

Mode	Frequency (MHz)	Input Power(dBm)	Measured Value(V/m)	Target Value(V/m)	Measured Date
CW	835	20	165.9	166.6	2007/07/16
CW	1880	20	138.5	135.3	2007/07/16

For H-Field Scan

Mode	Frequency	Input Power	Measured Value(V/m)	Target Value(V/m)	Measured Date
CW	835	20	0.47	0.45	2007/07/16
CW	1880	20	0.445	0.457	2007/07/16

9. Probe Modulation Factor

The measurement setup for determination of the PMF is given in DASY4 manual section 28.2. The following points describe the installation, the measurement procedure and the evaluation.

1. Install the field probe in the DASY4 window setup.
2. Mount a validation dipole for the appropriate frequency band under the Test Arch. Move the probe manually to a point of high field strength for the specific field type. The probe may be very close to the dipole and might even touch it. During the fine adjustment of the probe with a signal applied to the dipole, read the x, y and z channel amplitudes in a multimeter job. They should all show a similar amplitude.
3. For comparing the peak amplitudes of modulated and CW signal, the same spectrum analyzer settings are required. The signal path (and setup geometry) between spectrum analyzer and probe must not be changed during the evaluation of the PMF! Only signal type and amplitudes as well as DASY4 settings may be varied.

Spectrum analyzer settings:

- Center Frequency: nominal center frequency of channel
- Span: zero
- Resolution bandwidth \geq emission bandwidth
- Video bandwidth = 20kHz
- Detection: RMS detection
- Trigger: Video or IF trigger, adjusted to give a stable display of the transmission
- Sweep rate: Set to show a complete transmission cycle
- Line max hold may be used temporarily to ease the peak reading.

4. Define a DASY4 document and set the procedure properties (frequency as above, modulation frequency and crest factor for the modulated signal) according to the measured signal. Define a multimeter job (continuous mode) for the field reading. The probe shall not move. A predefined document is available.
5. Define a DASY4 document with a procedure for the evaluation of the CW signal (frequency, modulation frequency = 0, crest factor = 1) with a multimeter job.
The HAC measurement procedure is as follows:
 6. Prepare the evaluation sheet for the installed field probe, frequency and modulation type.
 7. Modulated signal measurement: Connect the modulated signal using the appropriate frequency via the cable to the setup. Do not move the setup between the following measurements.
 8. Run the multimeter job in the procedure with the corresponding modulation setting in continuous mode.
 9. Adjust the signal amplitude to achieve the the desired field level display in the multimeter. (A number of levels over the full dynamic range of the probe in the desired range shall be set, including the values read during the WD scans.)
 10. Read the total field for the modulated signal.
 11. Read the peak envelope signal on the spectrum analyzer.
 12. Repeat these readings for other amplitude settings.
 13. Switch the signal source off and verify that the ambient and instrumentation noise level is at least 10 dB lower (a factor of 3 in field).
 14. CW measurement: Change the signal to CW at the same center frequency, without touching or moving dipole or probe in the setup.
 15. Adjust the CW signal amplitude to a similar range of peak levels on the spectrum analyzer.
 16. Run the multimeter in the CW procedure in continuous mode.
 17. Read the multimeter total field display.
 18. Read the signal on the spectrum analyzer.
 19. Repeat these readings for other amplitude settings.
 20. Select the correct type of predefined Excel calculation sheet and insert the readings into the appropriate measurement columns. Conversion from linear DASY readings to logarithmic will be automatically made. The diagrams contain fitting curves for the logarithmic quantities. CW and E-field values will be fitted by linear trendlines, H-field values by quadratic.

10. Test Standards and Limits

The measurements were performed to ensure compliance to the ANSI PC63.19-2006 rd 3.12 standard,

Category	Telephone RF Parameters < 960 MHz				
	Near Field	AWF	E-Field Emissions		H-Field Emissions
Category M1/T1	0	56 to 61	dB (V/m)	+5.6 to +10.6	dB (A/m)
	-5	53.5 to 58.5	dB (V/m)	+3.1 to +8.1	dB (A/m)
Category M2/T2	0	51 to 56	dB (V/m)	+0.6 to +5.6	dB (A/m)
	-5	48.5 to 53.5	dB (V/m)	-1.9 to +3.1	dB (A/m)
Category M3/T3	0	46 to 51	dB (V/m)	-4.4 to +0.6	dB (A/m)
	-5	43.5 to 48.5	dB (V/m)	-6.9 to -1.9	dB (A/m)
Category M4/T4	0	< 46	dB (V/m)	< -4.4	dB (A/m)
	-5	< 43.5	dB (V/m)	< -6.9	dB (A/m)

Category	Telephone RF Parameters > 960 MHz				
	Near Field	AWF	E-Field Emissions		H-Field Emissions
Category M1/T1	0	46 to 51	dB (V/m)	-4.4 to 0.6	dB (A/m)
	-5	43.5 to 48.5	dB (V/m)	-6.9 to -1.9	dB (A/m)
Category M2/T2	0	41 to 46	dB (V/m)	-9.4 to -4.4	dB (A/m)
	-5	38.5 to 43.5	dB (V/m)	-11.9 to -6.9	dB (A/m)
Category M3/T3	0	36 to 41	dB (V/m)	-14.4 to -9.4	dB (A/m)
	-5	33.5 to 38.5	dB (V/m)	-16.9 to -11.9	dB (A/m)
Category M4/T4	0	<36	dB (V/m)	<-14.4	dB (A/m)
	-5	<33.5	dB (V/m)	<-16.9	dB (A/m)

11. Instruments List

Manufacturer	Device	Type	Serial number	Date of last calibration
Schmid & Partner Engineering AG	E-Field and H-Field Probe	ER3DV6 H3DV6	2306 6142	Apr.20.2007 Apr.20.2007
Schmid & Partner Engineering AG	835/1880 MHz System Validation Dipole In Air	CD835V3 CD1880V3	1052 1044	Jan.16.2007 Jan.16.2007
Schmid & Partner Engineering AG	Data acquisition Electronics	DAE4	547	Mar.21.2007
Schmid & Partner Engineering AG	Software	DASY 4 V4.7 Build 53	N/A	Calibration isn't necessary
Agilent	Dielectric Probe Kit	85070D	US01440168	Calibration isn't necessary
Agilent	Dual-directional coupler	778D	50313	Sep.01.2006
Agilent	RF Signal Generator	8648D	3847M00432	May.22.2007
Agilent	Power Sensor	8481H	MY41091361	Jun.04.2007
Agilent	8960 Series 10 Wireless Communication Tester	8960	GB44051912	Nov.28.2006
Schmid & Partner Engineering AG	Test Arch SD HAC	P01	1047	N/A
Agilent	Spectrum Analyzer	E4404B	MY45111447	Jan.10.2007

12. Summary of Results

E-Field Emission	Band	function	Channel	Modulation Factor	Conducted Power at BS (dBm)	Measured Drift(%)	Time Avg. Field (V/m)	Time Avg. Field dB(V/m)	RESULT	Excl Blocks per 4.3.1.2.2
CDMA	CELLULAR	No Bluetooth	1013	1	23.71	-0.016	73.2	37.29	M4	689
			384	1	24.13	-0.057	77.6	37.80	M4	689
			777	1	24.02	-0.21	85.2	38.61	M4	689
		With Bluetooth active on	777	1	24.02	-0.132	91.6	39.24	M4	689
	US PCS	No Bluetooth	25	1	23.82	0.1	30.8	29.77	M4	789
			600	1	23.95	0.199	39	31.82	M4	689
			1175	1	23.97	0.154	36.9	31.84	M4	369
		With Bluetooth active on	1175	1	23.97	-0.061	38.6	31.73	M4	147

H-Field Emission	Band	function	Channel	Modulation Factor	Conducted Power at BS (dBm)	Measured Drift(%)	Time Avg. Field (V/m)	Time Avg. Field dB(V/m)	RESULT	Excl Blocks per 4.3.1.2.2
CDMA	CELLULAR	No Bluetooth	1013	1	23.71	-0.034	0.186	-14.61	M4	478
			384	1	24.13	0.028	0.186	-14.61	M4	478
			777	1	24.02	-0.005	0.199	-14.02	M4	478
		With Bluetooth active on	777	1	24.02	0.091	0.204	-13.81	M4	236
	US PCS	No Bluetooth	25	1	23.82	0.029	0.108	-19.33	M4	478
			600	1	23.95	0.201	0.139	-17.14	M4	147
			1175	1	23.97	0.189	0.136	-17.33	M4	124
		With Bluetooth active on	600	1	24.02	-0.023	0.145	-16.77	M4	147

13. Measurement Data

Date/Time: 2007/7/16 17:02:52

HAC_E_C88_CDMA Cellular_CH1013

DUT: C88; Type: CDMA;

Communication System: CDMA_850; Frequency: 824.7 MHz; Duty Cycle: 1:1

Medium: Air Medium parameters used: $\sigma = 0$ mho/m, $\epsilon_r = 1$; $\rho = 1000$ kg/m³

Phantom section: E Device Section

DASY4 Configuration:

- Probe: ER3DV6 - SN2306; ConvF(1, 1, 1); Calibrated: 2007/4/20
- Sensor-Surface: (Fix Surface)
- Electronics: DAE4 Sn547; Calibrated: 2007/3/5
- Phantom: HAC Test Arch 4.6; Type: SD HAC P01 BA;
- Measurement SW: DASY4, V4.7 Build 53; Postprocessing SW: SEMCAD, V1.8 Build 172

E Scan - ER probe center 10mm above Device Reference/Hearing Aid Compatibility Test (101x101x1):

Measurement grid: dx=5mm, dy=5mm

Maximum value of peak Total field = 73.2 V/m

Probe Modulation Factor = 1.00

Reference Value = 64.7 V/m; Power Drift = -0.016 dB

Hearing Aid Near-Field Category: M4 (AWF 0 dB)

Peak E-field in V/m

Grid 1	Grid 2	Grid 3
52.5	67.0	66.9
Grid 4	Grid 5	Grid 6
56.5	73.2	71.9
Grid 7	Grid 8	Grid 9
62.7	73.3	70.7


Category	AWF (dB)	Limits for E-Field Emissions dB(V/m) > 960MHz	Limits for H-Field Emissions dB(A/m) > 960MHz
M1	0	56 to 61	5.6 to 10.6
	-5	53.5 to 58.5	3.1 to 8.1
M2	0	51 to 56	0.6 to 5.6
	-5	48.5 to 53.5	-1.9 to 3.1
M3	0	46 to 51	-4.4 to 0.6
	-5	43.5 to 48.5	-6.9 to -1.9
M4	0	<46	<-4.4
	-5	<43.5	<-6.9
Category	AWF (dB)	Limits for E-Field Emissions dB(V/m) < 960MHz	Limits for H-Field Emissions dB(A/m) < 960 MHz
M1	0	46 to 51	-4.4 to 0.6
	-5	43.5 to 48.5	-6.9 to -1.9
M2	0	41 to 46	-9.4 to -4.4
	-5	38.5 to 43.5	-11.9 to -6.9
M3	0	36 to 41	-14.4 to -9.4
	-5	33.5 to 38.5	-16.9 to -11.9
M4	0	<36	<-14.4
	-5	<33.5	<-16.9

Cursor:

Total = 37.29 dB V/m

E Category: M4

Location: -4.5, 9.5, 363.7 mm

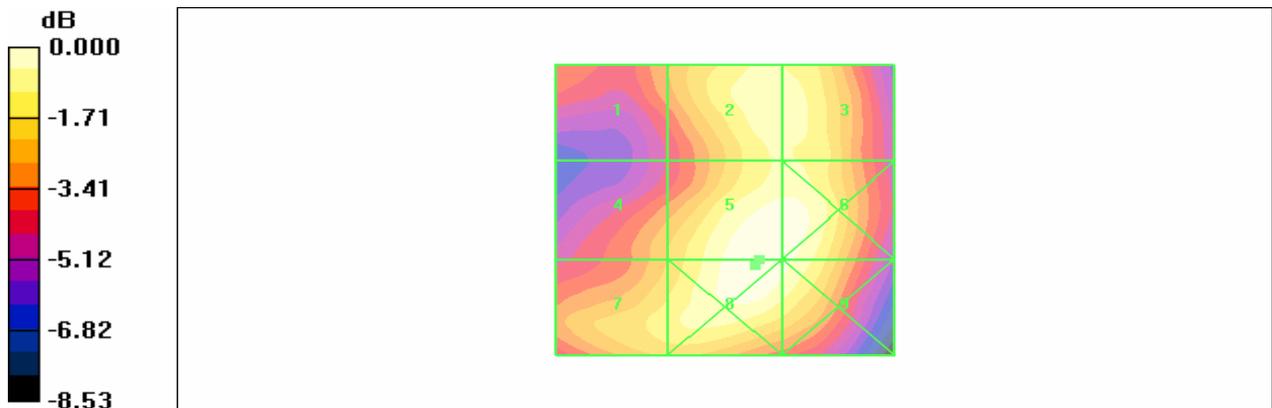

0 dB = 73.3V/m

HAC_E_C88_CDMA Cellular_CH384

DUT: C88; Type: CDMA;

Communication System: CDMA_850; Frequency: 836.52 MHz; Duty Cycle: 1:1

Medium: Air Medium parameters used: $\sigma = 0$ mho/m, $\epsilon_r = 1$; $\rho = 1000$ kg/m³

Phantom section: E Device Section

DASY4 Configuration:

- Probe: ER3DV6 - SN2306; ConvF(1, 1, 1); Calibrated: 2007/4/20
- Sensor-Surface: (Fix Surface)
- Electronics: DAE4 Sn547; Calibrated: 2007/3/5
- Phantom: HAC Test Arch 4.6; Type: SD HAC P01 BA;
- Measurement SW: DASY4, V4.7 Build 53; Postprocessing SW: SEMCAD, V1.8 Build 172

E Scan - ER probe center 10mm above Device Reference/Hearing Aid Compatibility Test

(101x101x1): Measurement grid: dx=5mm, dy=5mm

Maximum value of peak Total field = 77.6 V/m

Probe Modulation Factor = 1.00

Reference Value = 69.6 V/m; Power Drift = -0.057 dB

Hearing Aid Near-Field Category: M4 (AWF 0 dB)

Peak E-field in V/m

Grid 1	Grid 2	Grid 3
54.2	70.2	70.0
Grid 4	Grid 5	Grid 6
59.3	77.6	76.2
Grid 7	Grid 8	Grid 9
66.2	77.6	75.6

Category	AWF (dB)	Limits for E-Field Emissions dB(V/m) > 960MHz	Limits for H-Field Emissions dB(A/m) > 960MHz
M1	0	56 to 61	5.6 to 10.6


	-5	53.5 to 58.5	3.1 to 8.1
M2	0	51 to 56	0.6 to 5.6
	-5	48.5 to 53.5	-1.9 to 3.1
M3	0	46 to 51	-4.4 to 0.6
	-5	43.5 to 48.5	-6.9 to -1.9
M4	0	<46	<-4.4
	-5	<43.5	<-6.9
Category	AWF (dB)	Limits for E-Field Emissions dB(V/m) < 960MHz	Limits for H-Field Emissions dB(A/m) < 960 MHz
M1	0	46 to 51	-4.4 to 0.6
	-5	43.5 to 48.5	-6.9 to -1.9
M2	0	41 to 46	-9.4 to -4.4
	-5	38.5 to 43.5	-11.9 to -6.9
M3	0	36 to 41	-14.4 to -9.4
	-5	33.5 to 38.5	-16.9 to -11.9
M4	0	<36	<-14.4
	-5	<33.5	<-16.9

Cursor:

Total = 37.80 dB V/m

E Category: M4

Location: -5, 8.5, 363.7 mm

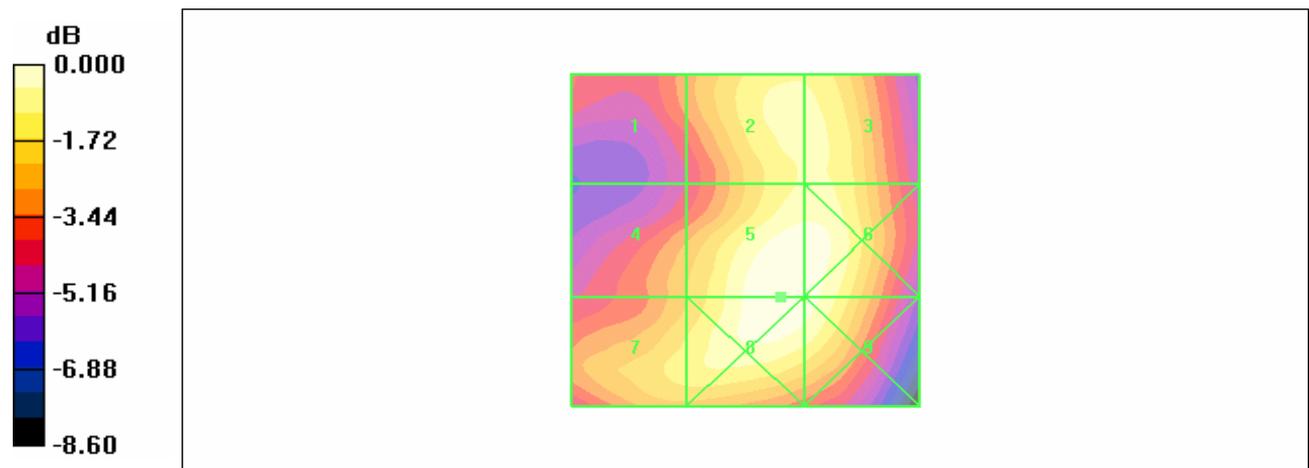

0 dB = 77.6V/m

HAC_E_C88_CDMA Cellular_CH777

DUT: C88; Type: CDMA;

Communication System: CDMA_850; Frequency: 848.31 MHz; Duty Cycle: 1:1

Medium: Air Medium parameters used: $\sigma = 0$ mho/m, $\epsilon_r = 1$; $\rho = 1000$ kg/m³

Phantom section: E Device Section

DASY4 Configuration:

- Probe: ER3DV6 - SN2306; ConvF(1, 1, 1); Calibrated: 2007/4/20
- Sensor-Surface: (Fix Surface)
- Electronics: DAE4 Sn547; Calibrated: 2007/3/5
- Phantom: HAC Test Arch 4.6; Type: SD HAC P01 BA;
- Measurement SW: DASY4, V4.7 Build 53; Postprocessing SW: SEMCAD, V1.8 Build 172

E Scan - ER probe center 10mm above Device Reference/Hearing Aid Compatibility Test

(101x101x1): Measurement grid: dx=5mm, dy=5mm

Maximum value of peak Total field = 85.2 V/m

Probe Modulation Factor = 1.00

Reference Value = 76.0 V/m; Power Drift = 0.210 dB

Hearing Aid Near-Field Category: M4 (AWF 0 dB)

Peak E-field in V/m

Grid 1	Grid 2	Grid 3
58.9	76.3	76.3
Grid 4	Grid 5	Grid 6
65.7	85.2	84.8
Grid 7	Grid 8	Grid 9
73.4	85.1	83.6

Category	AWF (dB)	Limits for E-Field Emissions dB(V/m) > 960MHz	Limits for H-Field Emissions dB(A/m) > 960MHz
M1	0	56 to 61	5.6 to 10.6


	-5	53.5 to 58.5	3.1 to 8.1
M2	0	51 to 56	0.6 to 5.6
	-5	48.5 to 53.5	-1.9 to 3.1
M3	0	46 to 51	-4.4 to 0.6
	-5	43.5 to 48.5	-6.9 to -1.9
M4	0	<46	<-4.4
	-5	<43.5	<-6.9
Category	AWF (dB)	Limits for E-Field Emissions dB(V/m) < 960MHz	Limits for H-Field Emissions dB(A/m) < 960 MHz
M1	0	46 to 51	-4.4 to 0.6
	-5	43.5 to 48.5	-6.9 to -1.9
M2	0	41 to 46	-9.4 to -4.4
	-5	38.5 to 43.5	-11.9 to -6.9
M3	0	36 to 41	-14.4 to -9.4
	-5	33.5 to 38.5	-16.9 to -11.9
M4	0	<36	<-14.4
	-5	<33.5	<-16.9

Cursor:

Total = 38.61 dB V/m

E Category: M4

Location: -5, 7.5, 363.7 mm

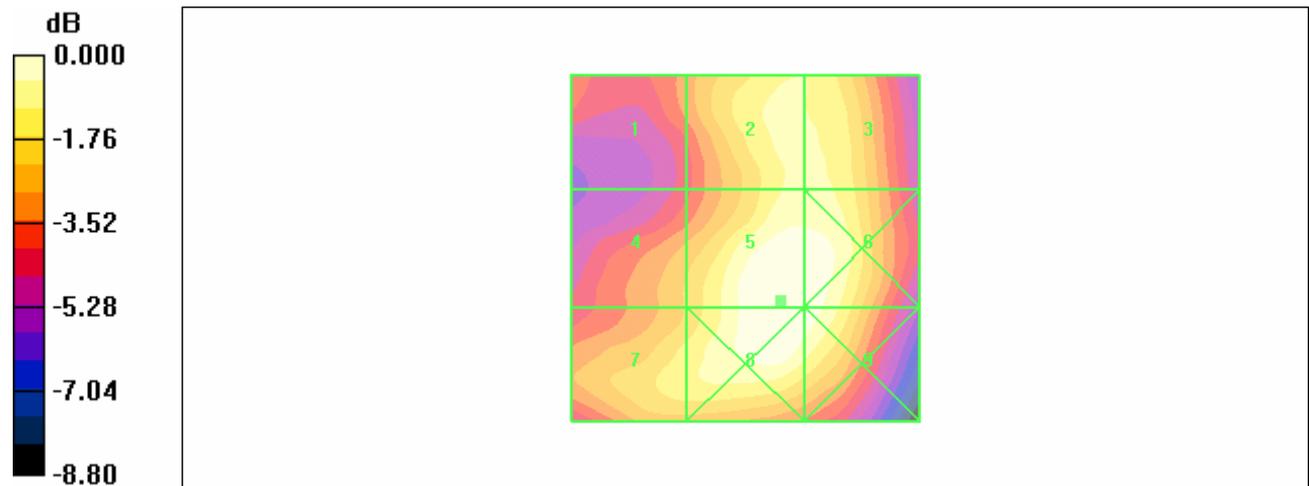

0 dB = 85.2V/m

HAC_E_C88_CDMA Cellular_CH777 (with Bluetooth active)

DUT: C88; Type: CDMA;

Communication System: CDMA_850; Frequency: 848.31 MHz; Duty Cycle: 1:1

Medium: Air Medium parameters used: $\sigma = 0$ mho/m, $\epsilon_r = 1$; $\rho = 1000$ kg/m³

Phantom section: H Device Section

DASY4 Configuration:

- Probe: ER3DV6 - SN2306; ConvF(1, 1, 1); Calibrated: 2007/4/20
- Sensor-Surface: (Fix Surface)
- Electronics: DAE4 Sn547; Calibrated: 2007/3/5
- Phantom: HAC Test Arch 4.6; Type: SD HAC P01 BA;
- Measurement SW: DASY4, V4.7 Build 53; Postprocessing SW: SEMCAD, V1.8 Build 172

E Scan - ER probe center 10mm above Device Reference/Hearing Aid Compatibility Test

(101x101x1): Measurement grid: dx=5mm, dy=5mm

Maximum value of peak Total field = 91.6 V/m

Probe Modulation Factor = 1.00

Reference Value = 70.0 V/m; Power Drift = -0.132 dB

Hearing Aid Near-Field Category: M4 (AWF 0 dB)

Peak E-field in V/m

Grid 1	Grid 2	Grid 3
63.1	80.9	82.0
Grid 4	Grid 5	Grid 6
64.6	91.6	92.0
Grid 7	Grid 8	Grid 9
73.3	91.1	91.4

Category	AWF (dB)	Limits for E-Field Emissions dB(V/m) > 960MHz	Limits for H-Field Emissions dB(A/m) > 960MHz
M1	0	56 to 61	5.6 to 10.6


	-5	53.5 to 58.5	3.1 to 8.1
M2	0	51 to 56	0.6 to 5.6
	-5	48.5 to 53.5	-1.9 to 3.1
M3	0	46 to 51	-4.4 to 0.6
	-5	43.5 to 48.5	-6.9 to -1.9
M4	0	<46	<-4.4
	-5	<43.5	<-6.9
Category	AWF (dB)	Limits for E-Field Emissions dB(V/m) < 960MHz	Limits for H-Field Emissions dB(A/m) < 960 MHz
M1	0	46 to 51	-4.4 to 0.6
	-5	43.5 to 48.5	-6.9 to -1.9
M2	0	41 to 46	-9.4 to -4.4
	-5	38.5 to 43.5	-11.9 to -6.9
M3	0	36 to 41	-14.4 to -9.4
	-5	33.5 to 38.5	-16.9 to -11.9
M4	0	<36	<-14.4
	-5	<33.5	<-16.9

Cursor:

Total = 39.24 dB V/m

E Category: M4

Location: -10, 6, 363.2 mm

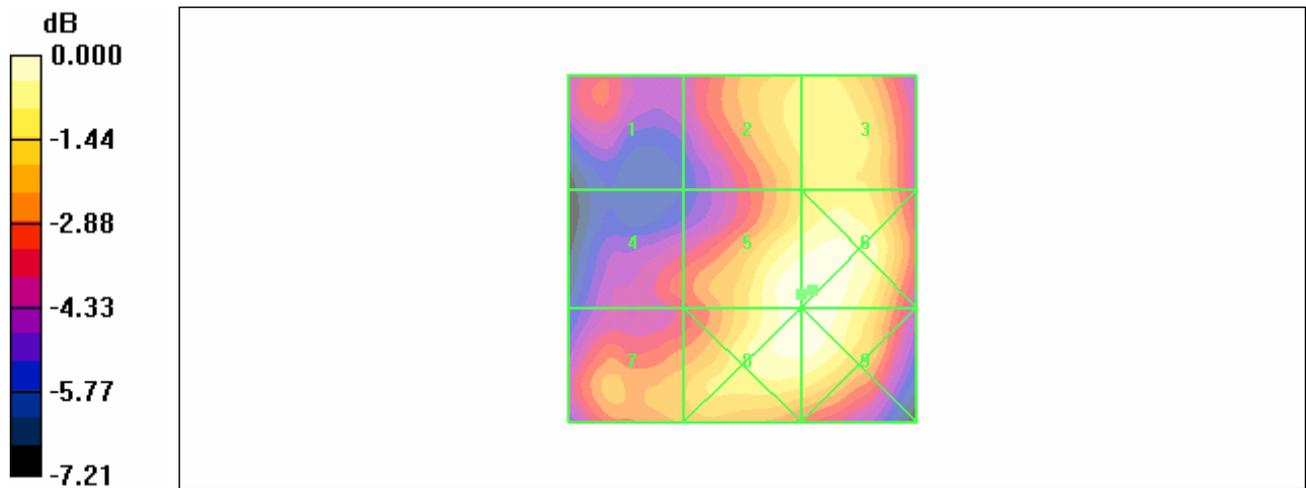

0 dB = 92.0V/m

HAC_E_C88_US PCS_CH25

DUT: C88; Type: CDMA;

Communication System: CDMA2000; Frequency: 1851.25 MHz; Duty Cycle: 1:1

Medium: Air Medium parameters used: $\sigma = 0$ mho/m, $\epsilon_r = 1$; $\rho = 1000$ kg/m³

Phantom section: E Device Section

DASY4 Configuration:

- Probe: ER3DV6 - SN2306; ConvF(1, 1, 1); Calibrated: 2007/4/20
- Sensor-Surface: (Fix Surface)
- Electronics: DAE4 Sn547; Calibrated: 2007/3/5
- Phantom: HAC Test Arch 4.6; Type: SD HAC P01 BA;
- Measurement SW: DASY4, V4.7 Build 53; Postprocessing SW: SEMCAD, V1.8 Build 172

E Scan - ER probe center 10mm above Device Reference/Hearing Aid Compatibility Test

(101x101x1): Measurement grid: dx=5mm, dy=5mm

Maximum value of peak Total field = 30.8 V/m

Probe Modulation Factor = 1.00

Reference Value = 18.4 V/m; Power Drift = 0.100 dB

Hearing Aid Near-Field Category: M4 (AWF 0 dB)

Peak E-field in V/m

Grid 1	Grid 2	Grid 3
29.3	25.1	29.1
Grid 4	Grid 5	Grid 6
23.6	27.1	30.8
Grid 7	Grid 8	Grid 9
32.1	30.7	30.7

Category	AWF (dB)	Limits for E-Field Emissions dB(V/m) > 960MHz	Limits for H-Field Emissions dB(A/m) > 960MHz
M1	0	56 to 61	5.6 to 10.6


	-5	53.5 to 58.5	3.1 to 8.1
M2	0	51 to 56	0.6 to 5.6
	-5	48.5 to 53.5	-1.9 to 3.1
M3	0	46 to 51	-4.4 to 0.6
	-5	43.5 to 48.5	-6.9 to -1.9
M4	0	<46	<-4.4
	-5	<43.5	<-6.9
Category	AWF (dB)	Limits for E-Field Emissions dB(V/m) < 960MHz	Limits for H-Field Emissions dB(A/m) < 960 MHz
M1	0	46 to 51	-4.4 to 0.6
	-5	43.5 to 48.5	-6.9 to -1.9
M2	0	41 to 46	-9.4 to -4.4
	-5	38.5 to 43.5	-11.9 to -6.9
M3	0	36 to 41	-14.4 to -9.4
	-5	33.5 to 38.5	-16.9 to -11.9
M4	0	<36	<-14.4
	-5	<33.5	<-16.9

Cursor:

Total = 29.77 dB V/m

E Category: M4

Location: 25, 25, 363.7 mm

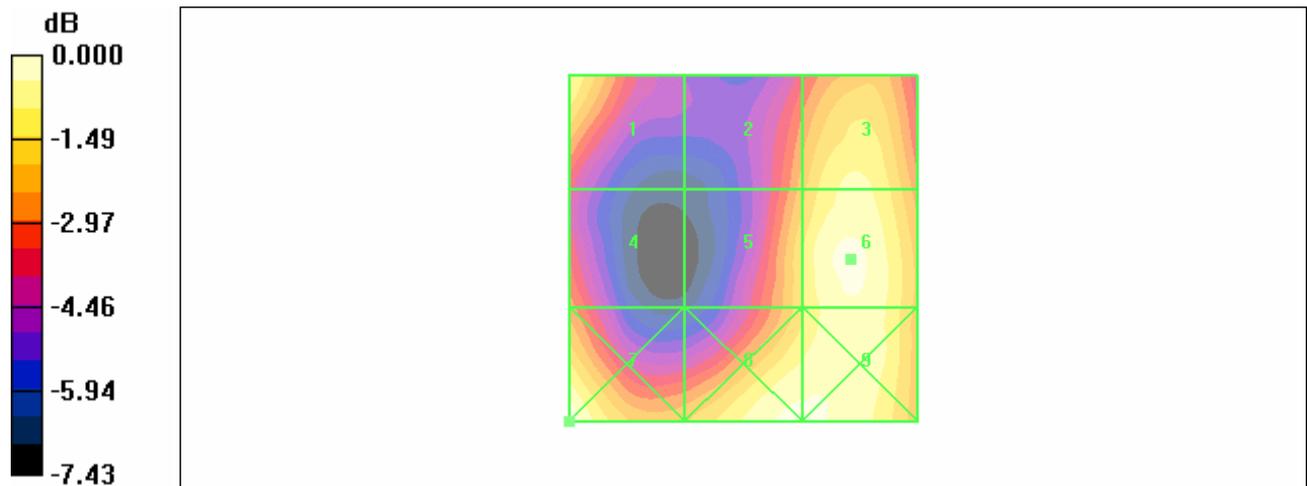

0 dB = 32.1V/m

HAC_E_C88_US PCS_CH600

DUT: C88; Type: CDMA;

Communication System: CDMA2000; Frequency: 1880 MHz; Duty Cycle: 1:1

Medium: Air Medium parameters used: $\sigma = 0$ mho/m, $\epsilon_r = 1$; $\rho = 1000$ kg/m³

Phantom section: E Device Section

DASY4 Configuration:

- Probe: ER3DV6 - SN2306; ConvF(1, 1, 1); Calibrated: 2007/4/20
- Sensor-Surface: (Fix Surface)
- Electronics: DAE4 Sn547; Calibrated: 2007/3/5
- Phantom: HAC Test Arch 4.6; Type: SD HAC P01 BA;
- Measurement SW: DASY4, V4.7 Build 53; Postprocessing SW: SEMCAD, V1.8 Build 172

E Scan - ER probe center 10mm above Device Reference/Hearing Aid Compatibility Test

(101x101x1): Measurement grid: dx=5mm, dy=5mm

Maximum value of peak Total field = 39.0 V/m

Probe Modulation Factor = 1.00

Reference Value = 24.0 V/m; Power Drift = 0.199 dB

Hearing Aid Near-Field Category: M4 (AWF 0 dB)

Peak E-field in V/m

Grid 1	Grid 2	Grid 3
39.0	33.2	36.8
Grid 4	Grid 5	Grid 6
30.7	36.2	40.1
Grid 7	Grid 8	Grid 9
37.9	37.9	38.9

Category	AWF (dB)	Limits for E-Field Emissions dB(V/m) > 960MHz	Limits for H-Field Emissions dB(A/m) > 960MHz
M1	0	56 to 61	5.6 to 10.6


	-5	53.5 to 58.5	3.1 to 8.1
M2	0	51 to 56	0.6 to 5.6
	-5	48.5 to 53.5	-1.9 to 3.1
M3	0	46 to 51	-4.4 to 0.6
	-5	43.5 to 48.5	-6.9 to -1.9
M4	0	<46	<-4.4
	-5	<43.5	<-6.9
Category	AWF (dB)	Limits for E-Field Emissions dB(V/m) < 960MHz	Limits for H-Field Emissions dB(A/m) < 960 MHz
M1	0	46 to 51	-4.4 to 0.6
	-5	43.5 to 48.5	-6.9 to -1.9
M2	0	41 to 46	-9.4 to -4.4
	-5	38.5 to 43.5	-11.9 to -6.9
M3	0	36 to 41	-14.4 to -9.4
	-5	33.5 to 38.5	-16.9 to -11.9
M4	0	<36	<-14.4
	-5	<33.5	<-16.9

Cursor:

Total = 31.82 dB V/m

E Category: M4

Location: -15, 5, 363.7 mm

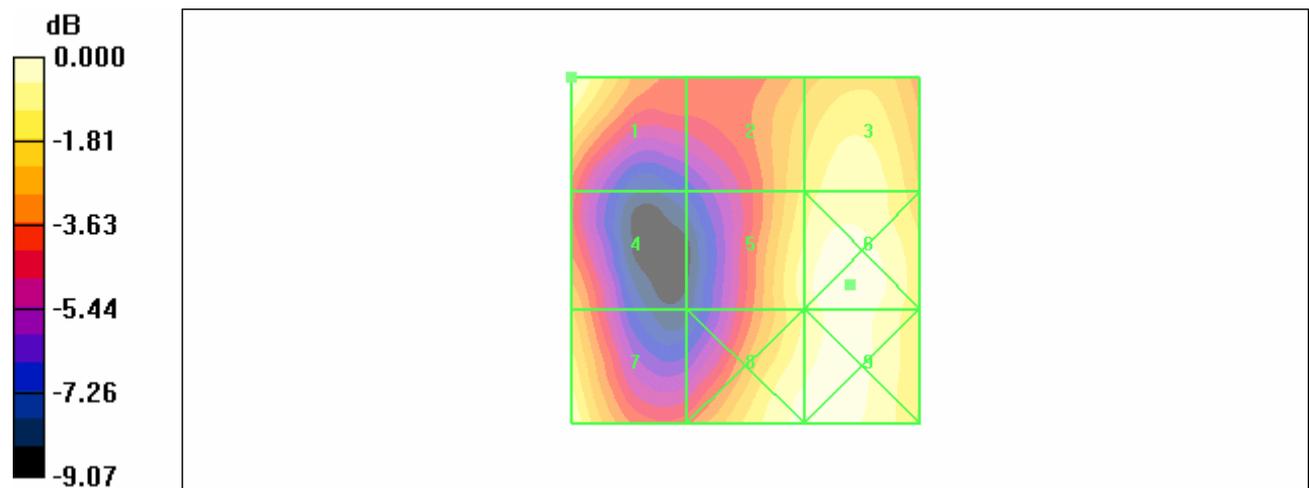

0 dB = 40.1V/m

HAC_E_C88_US PCS_CH1175

DUT: C88; Type: CDMA;

Communication System: CDMA2000; Frequency: 1908.75 MHz; Duty Cycle: 1:1

Medium: Air Medium parameters used: $\sigma = 0$ mho/m, $\epsilon_r = 1$; $\rho = 1000$ kg/m³

Phantom section: E Device Section

DASY4 Configuration:

- Probe: ER3DV6 - SN2306; ConvF(1, 1, 1); Calibrated: 2007/4/20
- Sensor-Surface: (Fix Surface)
- Electronics: DAE4 Sn547; Calibrated: 2007/3/5
- Phantom: HAC Test Arch 4.6; Type: SD HAC P01 BA;
- Measurement SW: DASY4, V4.7 Build 53; Postprocessing SW: SEMCAD, V1.8 Build 172

E Scan - ER probe center 10mm above Device Reference/Hearing Aid Compatibility Test

(101x101x1): Measurement grid: dx=5mm, dy=5mm

Maximum value of peak Total field = 36.9 V/m

Probe Modulation Factor = 1.00

Reference Value = 22.3 V/m; Power Drift = 0.154 dB

Hearing Aid Near-Field Category: M4 (AWF 0 dB)

Peak E-field in V/m

Grid 1	Grid 2	Grid 3
36.4	32.2	35.4
Grid 4	Grid 5	Grid 6
31.5	34.4	37.7
Grid 7	Grid 8	Grid 9
36.9	34.2	36.5

Category	AWF (dB)	Limits for E-Field Emissions dB(V/m) > 960MHz	Limits for H-Field Emissions dB(A/m) > 960MHz
M1	0	56 to 61	5.6 to 10.6


	-5	53.5 to 58.5	3.1 to 8.1
M2	0	51 to 56	0.6 to 5.6
	-5	48.5 to 53.5	-1.9 to 3.1
M3	0	46 to 51	-4.4 to 0.6
	-5	43.5 to 48.5	-6.9 to -1.9
M4	0	<46	<-4.4
	-5	<43.5	<-6.9
Category	AWF (dB)	Limits for E-Field Emissions dB(V/m) < 960MHz	Limits for H-Field Emissions dB(A/m) < 960 MHz
M1	0	46 to 51	-4.4 to 0.6
	-5	43.5 to 48.5	-6.9 to -1.9
M2	0	41 to 46	-9.4 to -4.4
	-5	38.5 to 43.5	-11.9 to -6.9
M3	0	36 to 41	-14.4 to -9.4
	-5	33.5 to 38.5	-16.9 to -11.9
M4	0	<36	<-14.4
	-5	<33.5	<-16.9

Cursor:

Total = 31.84 dB V/m

E Category: M4

Location: -15, 4.5, 363.7 mm

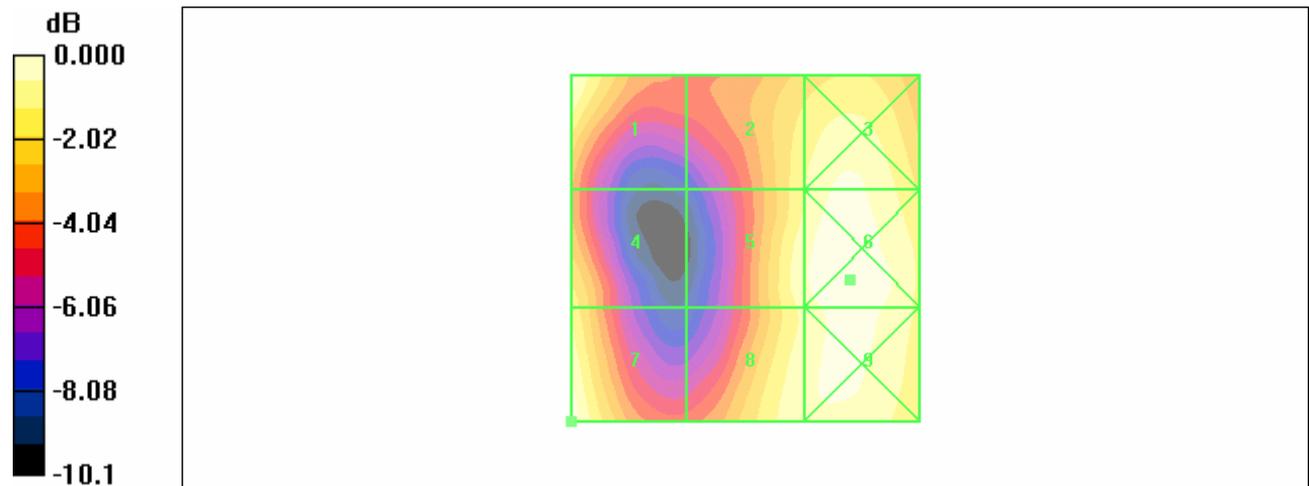

0 dB = 37.7V/m

HAC_E_C88_US PCS_CH1175 (with Bluetooth active)

DUT: C88; Type: CDMA;

Communication System: CDMA2000; Frequency: 1908.75 MHz; Duty Cycle: 1:1

Medium: Air Medium parameters used: $\sigma = 0$ mho/m, $\epsilon_r = 1$; $\rho = 1000$ kg/m³

Phantom section: E Device Section

DASY4 Configuration:

- Probe: ER3DV6 - SN2306; ConvF(1, 1, 1); Calibrated: 2007/4/20
- Sensor-Surface: (Fix Surface)
- Electronics: DAE4 Sn547; Calibrated: 2007/3/5
- Phantom: HAC Test Arch 4.6; Type: SD HAC P01 BA;
- Measurement SW: DASY4, V4.7 Build 53; Postprocessing SW: SEMCAD, V1.8 Build 172

E Scan - ER probe center 10mm above Device Reference/Hearing Aid Compatibility Test

(101x101x1): Measurement grid: dx=5mm, dy=5mm

Maximum value of peak Total field = 38.6 V/m

Probe Modulation Factor = 1.00

Reference Value = 16.1 V/m; Power Drift = -0.061 dB

Hearing Aid Near-Field Category: M4 (AWF 0 dB)

Peak E-field in V/m

Grid 1	Grid 2	Grid 3
40.5	27.2	35.7
Grid 4	Grid 5	Grid 6
36.8	28.3	38.6
Grid 7	Grid 8	Grid 9
42.0	33.4	37.3

Category	AWF (dB)	Limits for E-Field Emissions dB(V/m) > 960MHz	Limits for H-Field Emissions dB(A/m) > 960MHz
M1	0	56 to 61	5.6 to 10.6


	-5	53.5 to 58.5	3.1 to 8.1
M2	0	51 to 56	0.6 to 5.6
	-5	48.5 to 53.5	-1.9 to 3.1
M3	0	46 to 51	-4.4 to 0.6
	-5	43.5 to 48.5	-6.9 to -1.9
M4	0	<46	<-4.4
	-5	<43.5	<-6.9
Category	AWF (dB)	Limits for E-Field Emissions dB(V/m) < 960MHz	Limits for H-Field Emissions dB(A/m) < 960 MHz
M1	0	46 to 51	-4.4 to 0.6
	-5	43.5 to 48.5	-6.9 to -1.9
M2	0	41 to 46	-9.4 to -4.4
	-5	38.5 to 43.5	-11.9 to -6.9
M3	0	36 to 41	-14.4 to -9.4
	-5	33.5 to 38.5	-16.9 to -11.9
M4	0	<36	<-14.4
	-5	<33.5	<-16.9

Cursor:

Total = 31.73 dB V/m

E Category: M4

Location: 24, 25, 363.7 mm

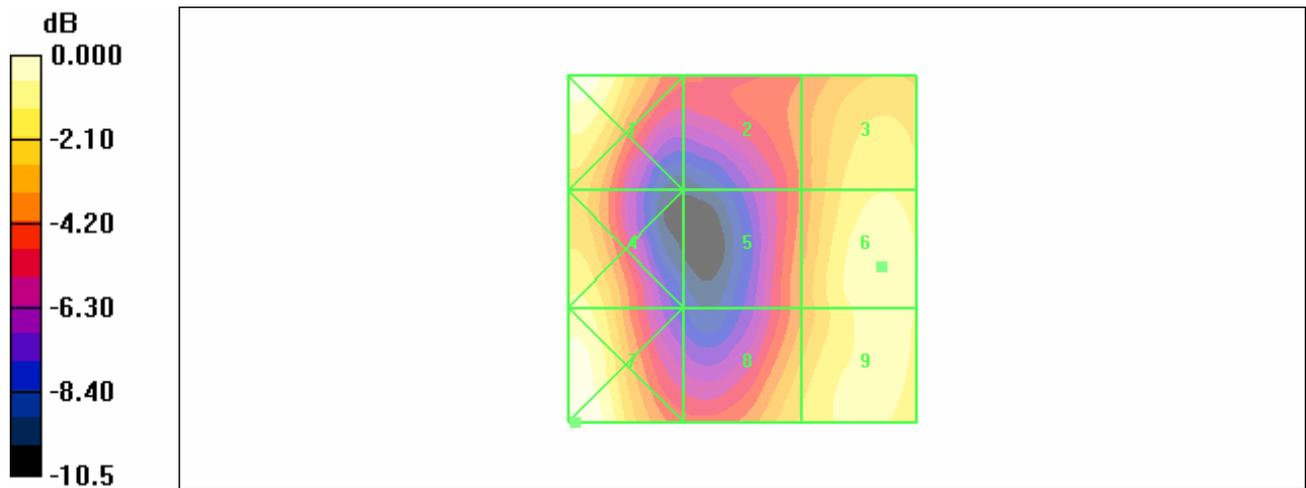

0 dB = 42.0V/m

HAC_H_C88_CDMA Cellular_CH1013

DUT: C88; Type: CDMA;

Communication System: CDMA_850; Frequency: 824.7 MHz; Duty Cycle: 1:1

Medium: Air Medium parameters used: $\sigma = 0$ mho/m, $\epsilon_r = 1$; $\rho = 1$ kg/m³

Phantom section: H Device Section

DASY4 Configuration:

- Probe: H3DV6 - SN6142; ; Calibrated: 2007/4/20
- Sensor-Surface: (Fix Surface)
- Electronics: DAE4 Sn547; Calibrated: 2007/3/5
- Phantom: HAC Test Arch 4.6; Type: SD HAC P01 BA;
- Measurement SW: DASY4, V4.7 Build 53; Postprocessing SW: SEMCAD, V1.8 Build 172

H Scan - H3DV6 probe center 10mm above Device Reference/Hearing Aid Compatibility Test

(101x101x1): Measurement grid: dx=5mm, dy=5mm

Maximum value of peak Total field = 0.186 A/m

Probe Modulation Factor = 1.00

Reference Value = 0.182 A/m; Power Drift = -0.034 dB

Hearing Aid Near-Field Category: M4 (AWF 0 dB)

Peak H-field in A/m

Grid 1	Grid 2	Grid 3
0.148	0.176	0.141
Grid 4	Grid 5	Grid 6
0.165	0.186	0.150
Grid 7	Grid 8	Grid 9
0.164	0.182	0.148

Category	AWF (dB)	Limits for E-Field Emissions dB(V/m) > 960MHz	Limits for H-Field Emissions dB(A/m) > 960MHz
M1	0	56 to 61	5.6 to 10.6


	-5	53.5 to 58.5	3.1 to 8.1
M2	0	51 to 56	0.6 to 5.6
	-5	48.5 to 53.5	-1.9 to 3.1
M3	0	46 to 51	-4.4 to 0.6
	-5	43.5 to 48.5	-6.9 to -1.9
M4	0	<46	<-4.4
	-5	<43.5	<-6.9
Category	AWF (dB)	Limits for E-Field Emissions dB(V/m) < 960MHz	Limits for H-Field Emissions dB(A/m) < 960 MHz
M1	0	46 to 51	-4.4 to 0.6
	-5	43.5 to 48.5	-6.9 to -1.9
M2	0	41 to 46	-9.4 to -4.4
	-5	38.5 to 43.5	-11.9 to -6.9
M3	0	36 to 41	-14.4 to -9.4
	-5	33.5 to 38.5	-16.9 to -11.9
M4	0	<36	<-14.4
	-5	<33.5	<-16.9

Cursor:

Total = -14.61 dB A/m

H Category: M4

Location: 0.5, 4.5, 363.7 mm

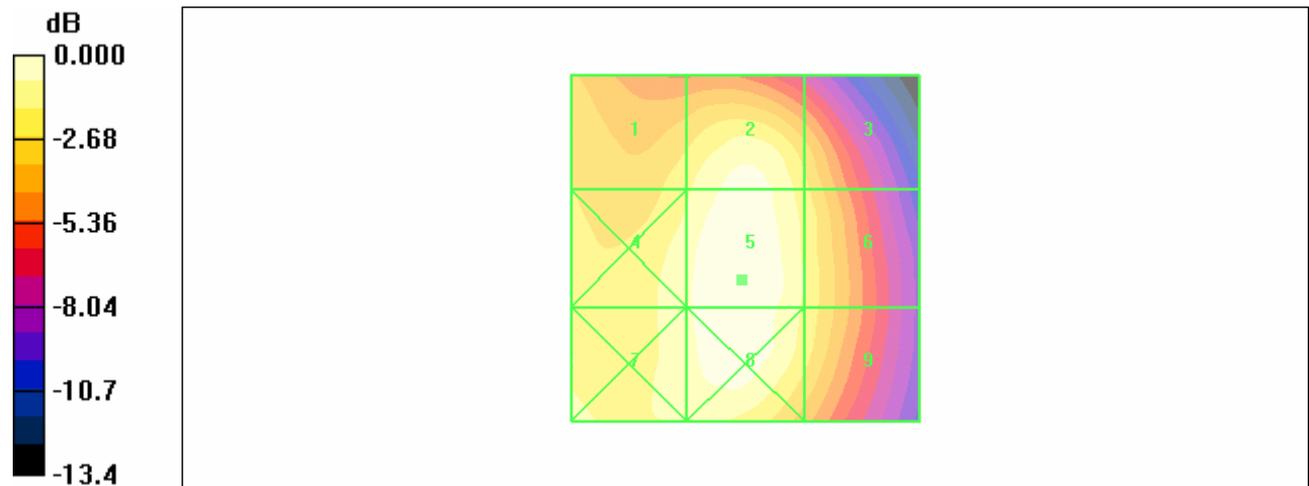

0 dB = 0.186A/m

HAC_H_C88_CDMA Cellular_CH384

DUT: C88; Type: CDMA;

Communication System: CDMA_850; Frequency: 836.52 MHz; Duty Cycle: 1:1

Medium: Air Medium parameters used: $\sigma = 0$ mho/m, $\epsilon_r = 1$; $\rho = 1$ kg/m³

Phantom section: H Device Section

DASY4 Configuration:

- Probe: H3DV6 - SN6142; ; Calibrated: 2007/4/20
- Sensor-Surface: (Fix Surface)
- Electronics: DAE4 Sn547; Calibrated: 2007/3/5
- Phantom: HAC Test Arch 4.6; Type: SD HAC P01 BA;
- Measurement SW: DASY4, V4.7 Build 53; Postprocessing SW: SEMCAD, V1.8 Build 172

H Scan - H3DV6 probe center 10mm above Device Reference/Hearing Aid Compatibility Test

(101x101x1): Measurement grid: dx=5mm, dy=5mm

Maximum value of peak Total field = 0.186 A/m

Probe Modulation Factor = 1.00

Reference Value = 0.179 A/m; Power Drift = 0.028 dB

Hearing Aid Near-Field Category: M4 (AWF 0 dB)

Peak H-field in A/m

Grid 1	Grid 2	Grid 3
0.153	0.178	0.143
0.166	0.186	0.150
0.166	0.184	0.148

Category	AWF (dB)	Limits for E-Field Emissions dB(V/m) > 960MHz	Limits for H-Field Emissions dB(A/m) > 960MHz
M1	0	56 to 61	5.6 to 10.6


	-5	53.5 to 58.5	3.1 to 8.1
M2	0	51 to 56	0.6 to 5.6
	-5	48.5 to 53.5	-1.9 to 3.1
M3	0	46 to 51	-4.4 to 0.6
	-5	43.5 to 48.5	-6.9 to -1.9
M4	0	<46	<-4.4
	-5	<43.5	<-6.9
Category	AWF (dB)	Limits for E-Field Emissions dB(V/m) < 960MHz	Limits for H-Field Emissions dB(A/m) < 960 MHz
M1	0	46 to 51	-4.4 to 0.6
	-5	43.5 to 48.5	-6.9 to -1.9
M2	0	41 to 46	-9.4 to -4.4
	-5	38.5 to 43.5	-11.9 to -6.9
M3	0	36 to 41	-14.4 to -9.4
	-5	33.5 to 38.5	-16.9 to -11.9
M4	0	<36	<-14.4
	-5	<33.5	<-16.9

Cursor:

Total = -14.61 dB A/m

H Category: M4

Location: 1, 4.5, 363.7 mm

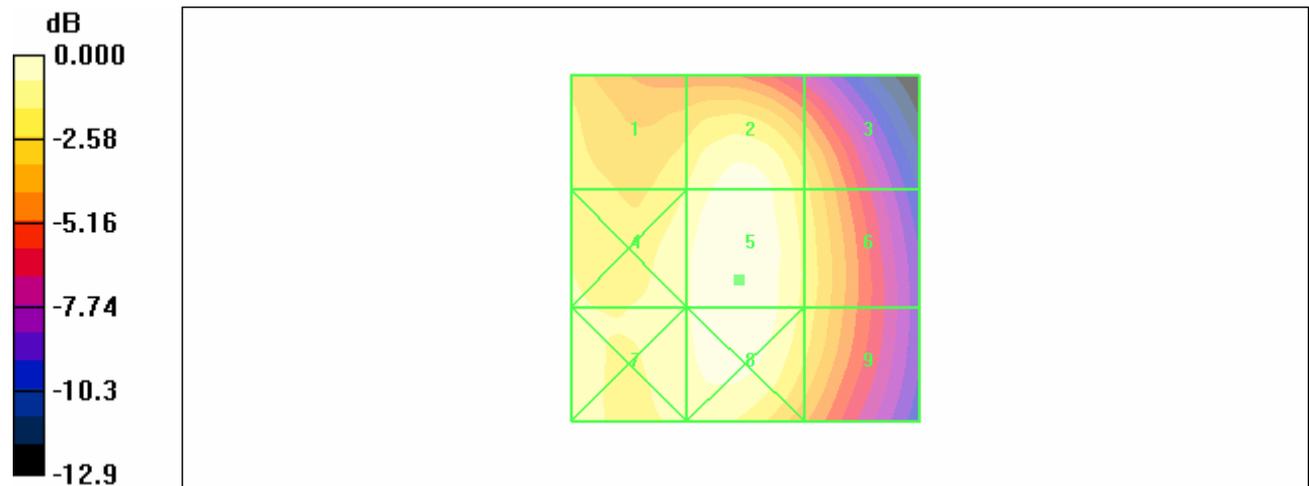

0 dB = 0.186A/m

HAC_H_C88_CDMA Cellular_CH777

DUT: C88; Type: CDMA;

Communication System: CDMA_850; Frequency: 848.31 MHz; Duty Cycle: 1:1

Medium: Air Medium parameters used: $\sigma = 0$ mho/m, $\epsilon_r = 1$; $\rho = 1$ kg/m³

Phantom section: H Device Section

DASY4 Configuration:

- Probe: H3DV6 - SN6142; ; Calibrated: 2007/4/20
- Sensor-Surface: (Fix Surface)
- Electronics: DAE4 Sn547; Calibrated: 2007/3/5
- Phantom: HAC Test Arch 4.6; Type: SD HAC P01 BA;
- Measurement SW: DASY4, V4.7 Build 53; Postprocessing SW: SEMCAD, V1.8 Build 172

H Scan - H3DV6 probe center 10mm above Device Reference/Hearing Aid Compatibility Test

(101x101x1): Measurement grid: dx=5mm, dy=5mm

Maximum value of peak Total field = 0.199 A/m

Probe Modulation Factor = 1.00

Reference Value = 0.192 A/m; Power Drift = -0.005 dB

Hearing Aid Near-Field Category: M4 (AWF 0 dB)

Peak H-field in A/m

Grid 1	Grid 2	Grid 3
0.167	0.190	0.151
Grid 4	Grid 5	Grid 6
0.179	0.199	0.160
Grid 7	Grid 8	Grid 9
0.181	0.193	0.156

Category	AWF (dB)	Limits for E-Field Emissions dB(V/m) > 960MHz	Limits for H-Field Emissions dB(A/m) > 960MHz
M1	0	56 to 61	5.6 to 10.6


	-5	53.5 to 58.5	3.1 to 8.1
M2	0	51 to 56	0.6 to 5.6
	-5	48.5 to 53.5	-1.9 to 3.1
M3	0	46 to 51	-4.4 to 0.6
	-5	43.5 to 48.5	-6.9 to -1.9
M4	0	<46	<-4.4
	-5	<43.5	<-6.9
Category	AWF (dB)	Limits for E-Field Emissions dB(V/m) < 960MHz	Limits for H-Field Emissions dB(A/m) < 960 MHz
M1	0	46 to 51	-4.4 to 0.6
	-5	43.5 to 48.5	-6.9 to -1.9
M2	0	41 to 46	-9.4 to -4.4
	-5	38.5 to 43.5	-11.9 to -6.9
M3	0	36 to 41	-14.4 to -9.4
	-5	33.5 to 38.5	-16.9 to -11.9
M4	0	<36	<-14.4
	-5	<33.5	<-16.9

Cursor:

Total = -14.02 dB A/m

H Category: M4

Location: 0.5, 0.5, 363.7 mm

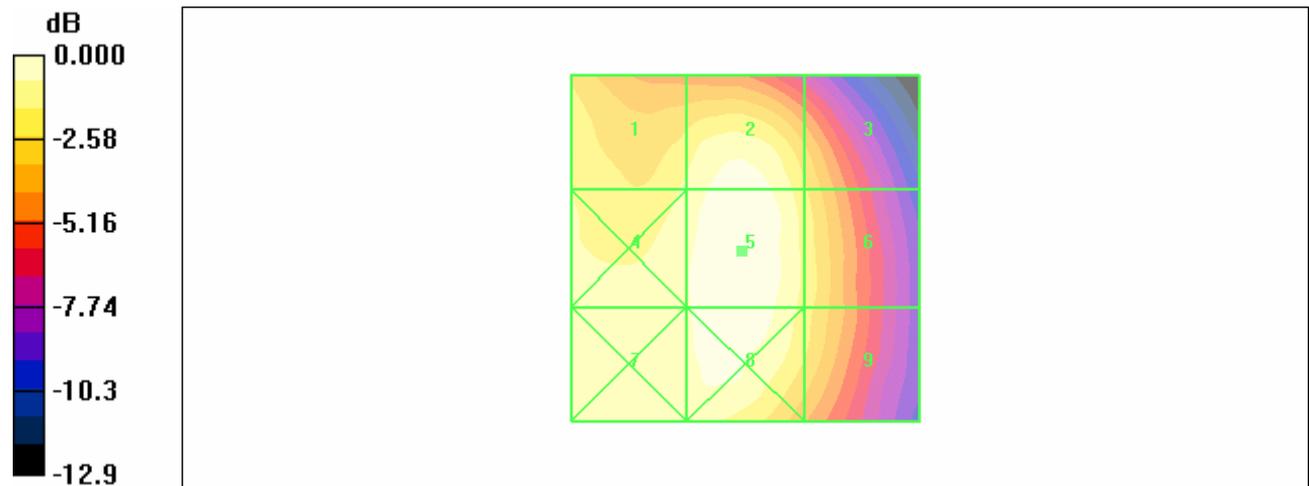

0 dB = 0.199A/m

HAC_H_C88_CDMA Cellular_CH777 (with Bluetooth active)

DUT: C88; Type: CDMA850;

Communication System: CDMA_850; Frequency: 848.31 MHz; Duty Cycle: 1:1

Medium: Air Medium parameters used: $\sigma = 0$ mho/m, $\epsilon_r = 1$; $\rho = 1$ kg/m³

Phantom section: H Device Section

DASY4 Configuration:

- Probe: H3DV6 - SN6142; ; Calibrated: 2007/4/20
- Sensor-Surface: (Fix Surface)
- Electronics: DAE4 Sn547; Calibrated: 2007/3/5
- Phantom: HAC Test Arch 4.6; Type: SD HAC P01 BA;
- Measurement SW: DASY4, V4.7 Build 53; Postprocessing SW: SEMCAD, V1.8 Build 172

H Scan - H3DV6 probe center 10mm above Device Reference/Hearing Aid Compatibility Test

(101x101x1): Measurement grid: dx=5mm, dy=5mm

Maximum value of peak Total field = 0.204 A/m

Probe Modulation Factor = 1.00

Reference Value = 0.192 A/m; Power Drift = 0.091 dB

Hearing Aid Near-Field Category: M4 (AWF 0 dB)

Peak H-field in A/m

Grid 1	Grid 2	Grid 3
0.178	0.203	0.184
Grid 4	Grid 5	Grid 6
0.182	0.204	0.190
Grid 7	Grid 8	Grid 9
0.186	0.199	0.183

Category	AWF (dB)	Limits for E-Field Emissions dB(V/m) > 960MHz	Limits for H-Field Emissions dB(A/m) > 960MHz
M1	0	56 to 61	5.6 to 10.6


	-5	53.5 to 58.5	3.1 to 8.1
M2	0	51 to 56	0.6 to 5.6
	-5	48.5 to 53.5	-1.9 to 3.1
M3	0	46 to 51	-4.4 to 0.6
	-5	43.5 to 48.5	-6.9 to -1.9
M4	0	<46	<-4.4
	-5	<43.5	<-6.9
Category	AWF (dB)	Limits for E-Field Emissions dB(V/m) < 960MHz	Limits for H-Field Emissions dB(A/m) < 960 MHz
M1	0	46 to 51	-4.4 to 0.6
	-5	43.5 to 48.5	-6.9 to -1.9
M2	0	41 to 46	-9.4 to -4.4
	-5	38.5 to 43.5	-11.9 to -6.9
M3	0	36 to 41	-14.4 to -9.4
	-5	33.5 to 38.5	-16.9 to -11.9
M4	0	<36	<-14.4
	-5	<33.5	<-16.9

Cursor:

Total = -13.81 dB A/m

H Category: M4

Location: -4, 0, 363.7 mm

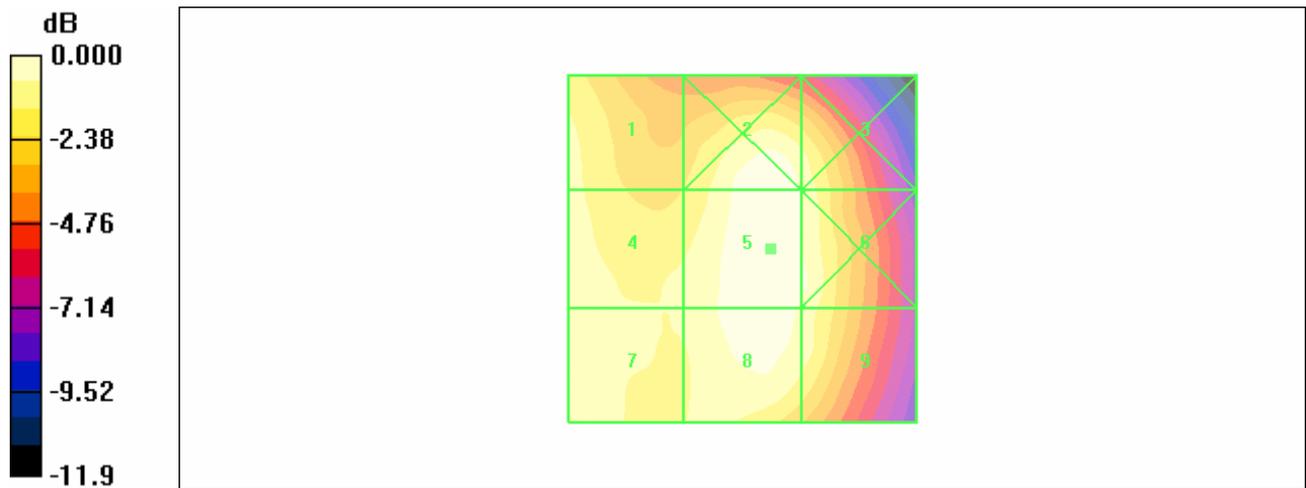

0 dB = 0.204A/m

HAC_H_C88_US PCS_CH25

DUT: C88; Type: CDMA;

Communication System: CDMA2000; Frequency: 1851.25 MHz; Duty Cycle: 1:1

Medium: Air Medium parameters used: $\sigma = 0$ mho/m, $\epsilon_r = 1$; $\rho = 1$ kg/m³

Phantom section: H Device Section

DASY4 Configuration:

- Probe: H3DV6 - SN6142; ; Calibrated: 2007/4/20
- Sensor-Surface: (Fix Surface)
- Electronics: DAE4 Sn547; Calibrated: 2007/3/5
- Phantom: HAC Test Arch 4.6; Type: SD HAC P01 BA;
- Measurement SW: DASY4, V4.7 Build 53; Postprocessing SW: SEMCAD, V1.8 Build 172

H Scan - H3DV6 probe center 10mm above Device Reference/Hearing Aid Compatibility Test

(101x101x1): Measurement grid: dx=5mm, dy=5mm

Maximum value of peak Total field = 0.108 A/m

Probe Modulation Factor = 1.00

Reference Value = 0.098 A/m; Power Drift = 0.029 dB

Hearing Aid Near-Field Category: M4 (AWF 0 dB)

Peak H-field in A/m

Grid 1	Grid 2	Grid 3
0.108	0.106	0.087
Grid 4	Grid 5	Grid 6
0.108	0.106	0.087
Grid 7	Grid 8	Grid 9
0.116	0.110	0.090

Category	AWF (dB)	Limits for E-Field Emissions dB(V/m) > 960MHz	Limits for H-Field Emissions dB(A/m) > 960MHz
M1	0	56 to 61	5.6 to 10.6


	-5	53.5 to 58.5	3.1 to 8.1
M2	0	51 to 56	0.6 to 5.6
	-5	48.5 to 53.5	-1.9 to 3.1
M3	0	46 to 51	-4.4 to 0.6
	-5	43.5 to 48.5	-6.9 to -1.9
M4	0	<46	<-4.4
	-5	<43.5	<-6.9
Category	AWF (dB)	Limits for E-Field Emissions dB(V/m) < 960MHz	Limits for H-Field Emissions dB(A/m) < 960 MHz
M1	0	46 to 51	-4.4 to 0.6
	-5	43.5 to 48.5	-6.9 to -1.9
M2	0	41 to 46	-9.4 to -4.4
	-5	38.5 to 43.5	-11.9 to -6.9
M3	0	36 to 41	-14.4 to -9.4
	-5	33.5 to 38.5	-16.9 to -11.9
M4	0	<36	<-14.4
	-5	<33.5	<-16.9

Cursor:

Total = -19.33 dB A/m

H Category: M4

Location: 23, 25, 363.7 mm

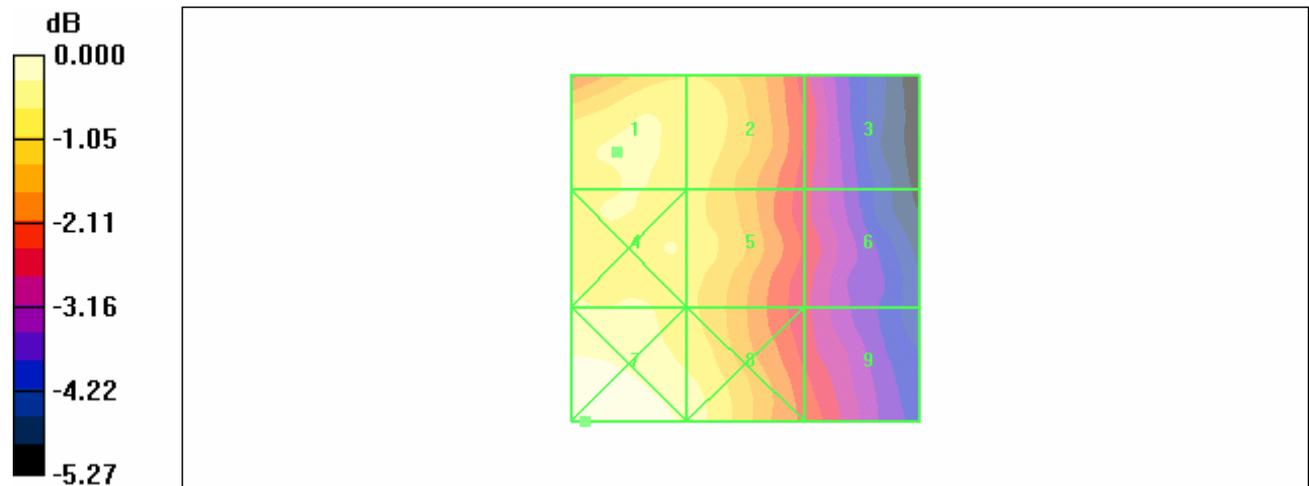

0 dB = 0.116A/m

HAC_H_C88_US PCS_CH600

DUT: C88; Type: CDMA;

Communication System: CDMA2000; Frequency: 1880 MHz; Duty Cycle: 1:1

Medium: Air Medium parameters used: $\sigma = 0$ mho/m, $\epsilon_r = 1$; $\rho = 1$ kg/m³

Phantom section: H Device Section

DASY4 Configuration:

- Probe: H3DV6 - SN6142; ; Calibrated: 2007/4/20
- Sensor-Surface: (Fix Surface)
- Electronics: DAE4 Sn547; Calibrated: 2007/3/5
- Phantom: HAC Test Arch 4.6; Type: SD HAC P01 BA;
- Measurement SW: DASY4, V4.7 Build 53; Postprocessing SW: SEMCAD, V1.8 Build 172

H Scan - H3DV6 probe center 10mm above Device Reference/Hearing Aid Compatibility Test

(101x101x1): Measurement grid: dx=5mm, dy=5mm

Maximum value of peak Total field = 0.139 A/m

Probe Modulation Factor = 1.00

Reference Value = 0.117 A/m; Power Drift = 0.201 dB

Hearing Aid Near-Field Category: M4 (AWF 0 dB)

Peak H-field in A/m

Grid 1	Grid 2	Grid 3
0.143	0.139	0.111
Grid 4	Grid 5	Grid 6
0.138	0.133	0.106
Grid 7	Grid 8	Grid 9
0.141	0.137	0.107

Category	AWF (dB)	Limits for E-Field Emissions dB(V/m) > 960MHz	Limits for H-Field Emissions dB(A/m) > 960MHz
M1	0	56 to 61	5.6 to 10.6


	-5	53.5 to 58.5	3.1 to 8.1
M2	0	51 to 56	0.6 to 5.6
	-5	48.5 to 53.5	-1.9 to 3.1
M3	0	46 to 51	-4.4 to 0.6
	-5	43.5 to 48.5	-6.9 to -1.9
M4	0	<46	<-4.4
	-5	<43.5	<-6.9
Category	AWF (dB)	Limits for E-Field Emissions dB(V/m) < 960MHz	Limits for H-Field Emissions dB(A/m) < 960 MHz
M1	0	46 to 51	-4.4 to 0.6
	-5	43.5 to 48.5	-6.9 to -1.9
M2	0	41 to 46	-9.4 to -4.4
	-5	38.5 to 43.5	-11.9 to -6.9
M3	0	36 to 41	-14.4 to -9.4
	-5	33.5 to 38.5	-16.9 to -11.9
M4	0	<36	<-14.4
	-5	<33.5	<-16.9

Cursor:

Total = -17.14 dB A/m

H Category: M4

Location: 19, -19, 363.7 mm

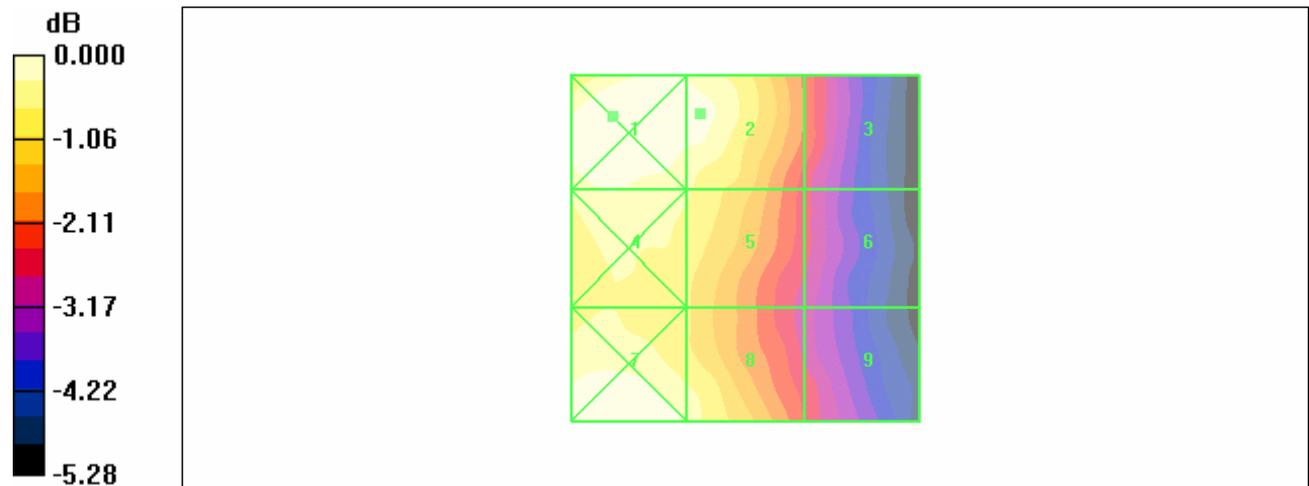

0 dB = 0.143A/m

HAC_H_C88_US_PCS_CH1175

DUT: C88; Type: CDMA;

Communication System: CDMA2000; Frequency: 1908.75 MHz; Duty Cycle: 1:1

Medium: Air Medium parameters used: $\sigma = 0$ mho/m, $\epsilon_r = 1$; $\rho = 1$ kg/m³

Phantom section: H Device Section

DASY4 Configuration:

- Probe: H3DV6 - SN6142; ; Calibrated: 2007/4/20
- Sensor-Surface: (Fix Surface)
- Electronics: DAE4 Sn547; Calibrated: 2007/3/5
- Phantom: HAC Test Arch 4.6; Type: SD HAC P01 BA;
- Measurement SW: DASY4, V4.7 Build 53; Postprocessing SW: SEMCAD, V1.8 Build 172

H Scan - H3DV6 probe center 10mm above Device Reference/Hearing Aid Compatibility Test

(101x101x1): Measurement grid: dx=5mm, dy=5mm

Maximum value of peak Total field = 0.136 A/m

Probe Modulation Factor = 1.00

Reference Value = 0.107 A/m; Power Drift = 0.189 dB

Hearing Aid Near-Field Category: M4 (AWF 0 dB)

Peak H-field in A/m

Grid 1	Grid 2	Grid 3
0.154	0.147	0.108
Grid 4	Grid 5	Grid 6
0.123	0.121	0.101
Grid 7	Grid 8	Grid 9
0.136	0.135	0.106

Category	AWF (dB)	Limits for E-Field Emissions dB(V/m) > 960MHz	Limits for H-Field Emissions dB(A/m) > 960MHz
M1	0	56 to 61	5.6 to 10.6


	-5	53.5 to 58.5	3.1 to 8.1
M2	0	51 to 56	0.6 to 5.6
	-5	48.5 to 53.5	-1.9 to 3.1
M3	0	46 to 51	-4.4 to 0.6
	-5	43.5 to 48.5	-6.9 to -1.9
M4	0	<46	<-4.4
	-5	<43.5	<-6.9
Category	AWF (dB)	Limits for E-Field Emissions dB(V/m) < 960MHz	Limits for H-Field Emissions dB(A/m) < 960 MHz
M1	0	46 to 51	-4.4 to 0.6
	-5	43.5 to 48.5	-6.9 to -1.9
M2	0	41 to 46	-9.4 to -4.4
	-5	38.5 to 43.5	-11.9 to -6.9
M3	0	36 to 41	-14.4 to -9.4
	-5	33.5 to 38.5	-16.9 to -11.9
M4	0	<36	<-14.4
	-5	<33.5	<-16.9

Cursor:

Total = -17.33 dB A/m

H Category: M4

Location: 17.5, -24.5, 363.7 mm

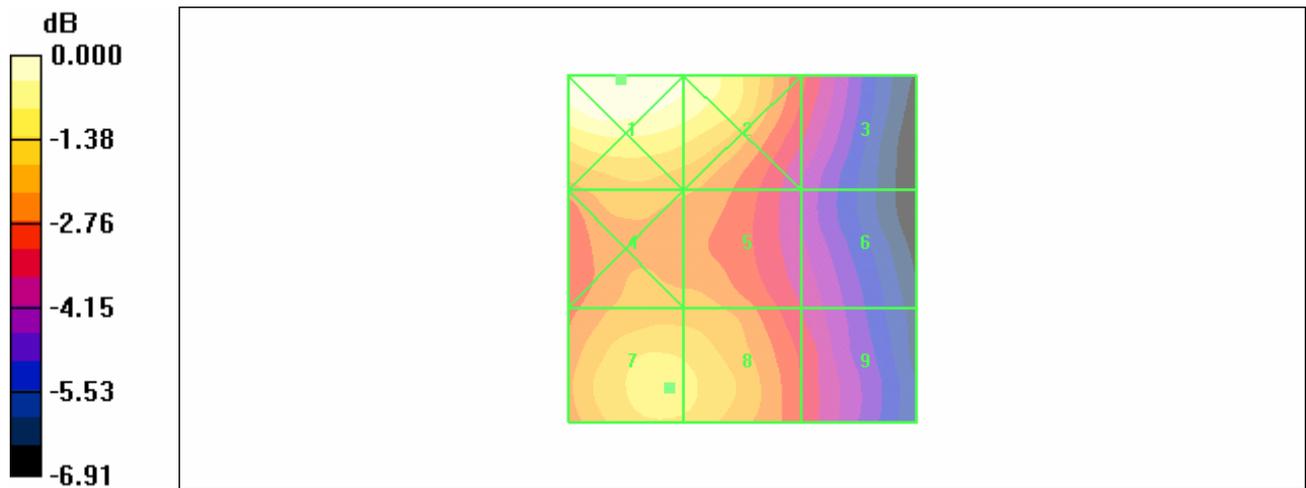

0 dB = 0.154A/m

HAC_H_C88_US PCS_CH600 (with Bluetooth active)

DUT: C88; Type: CDMA;

Communication System: CDMA2000; Frequency: 1880 MHz; Duty Cycle: 1:1

Medium: Air Medium parameters used: $\sigma = 0$ mho/m, $\epsilon_r = 1$; $\rho = 1$ kg/m³

Phantom section: H Device Section

DASY4 Configuration:

- Probe: H3DV6 - SN6142; ; Calibrated: 2007/4/20
- Sensor-Surface: (Fix Surface)
- Electronics: DAE4 Sn547; Calibrated: 2007/3/5
- Phantom: HAC Test Arch 4.6; Type: SD HAC P01 BA;
- Measurement SW: DASY4, V4.7 Build 53; Postprocessing SW: SEMCAD, V1.8 Build 172

H Scan - H3DV6 probe center 10mm above Device Reference/Hearing Aid Compatibility Test

(101x101x1): Measurement grid: dx=5mm, dy=5mm

Maximum value of peak Total field = 0.145 A/m

Probe Modulation Factor = 1.00

Reference Value = 0.130 A/m; Power Drift = -0.023 dB

Hearing Aid Near-Field Category: M4 (AWF 0 dB)

Peak H-field in A/m

Grid 1	Grid 2	Grid 3
0.147	0.145	0.122
Grid 4	Grid 5	Grid 6
0.142	0.140	0.116
Grid 7	Grid 8	Grid 9
0.145	0.143	0.118

Category	AWF (dB)	Limits for E-Field Emissions dB(V/m) > 960MHz	Limits for H-Field Emissions dB(A/m) > 960MHz
M1	0	56 to 61	5.6 to 10.6


	-5	53.5 to 58.5	3.1 to 8.1
M2	0	51 to 56	0.6 to 5.6
	-5	48.5 to 53.5	-1.9 to 3.1
M3	0	46 to 51	-4.4 to 0.6
	-5	43.5 to 48.5	-6.9 to -1.9
M4	0	<46	<-4.4
	-5	<43.5	<-6.9
Category	AWF (dB)	Limits for E-Field Emissions dB(V/m) < 960MHz	Limits for H-Field Emissions dB(A/m) < 960 MHz
M1	0	46 to 51	-4.4 to 0.6
	-5	43.5 to 48.5	-6.9 to -1.9
M2	0	41 to 46	-9.4 to -4.4
	-5	38.5 to 43.5	-11.9 to -6.9
M3	0	36 to 41	-14.4 to -9.4
	-5	33.5 to 38.5	-16.9 to -11.9
M4	0	<36	<-14.4
	-5	<33.5	<-16.9

Cursor:

Total = -16.639 dB A/m

H Category: M4

Location: 14.5, -18.5, 363.7 mm

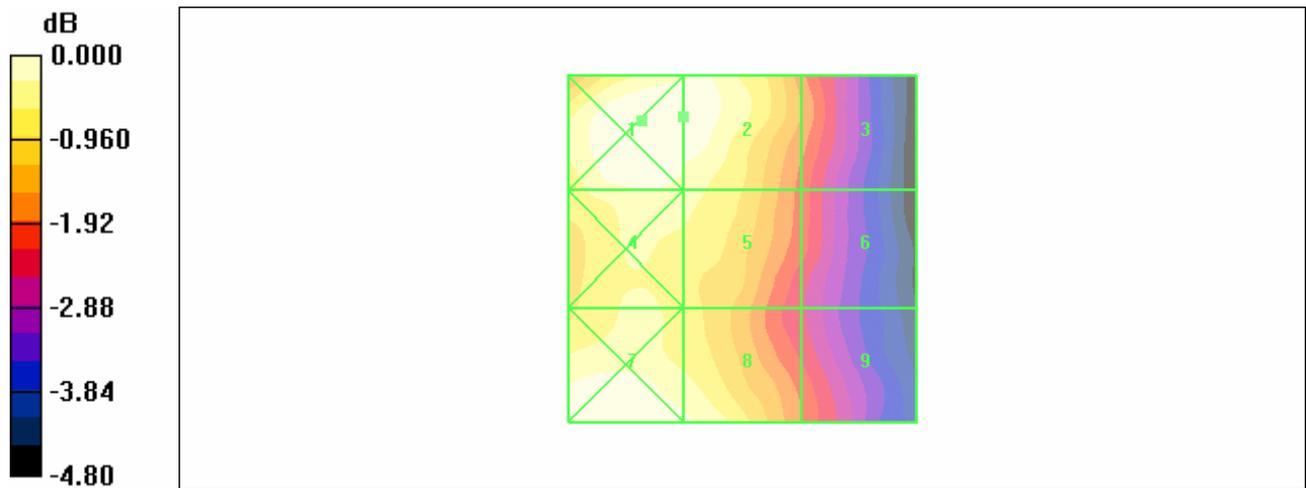

0 dB = 0.147A/m

HAC_E_Dipole_835MHz

DUT: HAC-Dipole 835 MHz; Type: CD835V3;

Communication System: CW; Frequency: 835 MHz; Duty Cycle: 1:1

Medium: Air Medium parameters used: $\sigma = 0$ mho/m, $\epsilon_r = 1$; $\rho = 1000$ kg/m³

Phantom section: E Dipole Section

DASY4 Configuration:

- Probe: ER3DV6 - SN2302; ConvF(1, 1, 1); Calibrated: 2007/3/21
- Sensor-Surface: (Fix Surface)
- Electronics: DAE4 Sn547; Calibrated: 2007/3/5
- Phantom: HAC Test Arch 4.6; Type: SD HAC P01 BA;
- Measurement SW: DASY4, V4.7 Build 53; Postprocessing SW: SEMCAD, V1.8 Build 172

E Scan - ER probe center 10mm above CD835 Dipole/Hearing Aid Compatibility Test

(41x361x1): Measurement grid: dx=5mm, dy=5mm

Maximum value of peak Total field = 165.9 V/m

Probe Modulation Factor = 1.00

Reference Value = 107.8 V/m; Power Drift = -0.010 dB

Hearing Aid Near-Field Category: M4 (AWF 0 dB)

Peak E-field in V/m

Grid 1	Grid 2	Grid 3
127.3	145.9	145.2
Grid 4	Grid 5	Grid 6
69.7	79.0	78.9
Grid 7	Grid 8	Grid 9
134.6	155.5	154.7

Category	AWF (dB)	Limits for E-Field Emissions dB(V/m) > 960MHz	Limits for H-Field Emissions dB(A/m) > 960MHz
M1	0	56 to 61	5.6 to 10.6


	-5	53.5 to 58.5	3.1 to 8.1
M2	0	51 to 56	0.6 to 5.6
	-5	48.5 to 53.5	-1.9 to 3.1
M3	0	46 to 51	-4.4 to 0.6
	-5	43.5 to 48.5	-6.9 to -1.9
M4	0	<46	<-4.4
	-5	<43.5	<-6.9
Category	AWF (dB)	Limits for E-Field Emissions dB(V/m) < 960MHz	Limits for H-Field Emissions dB(A/m) < 960 MHz
M1	0	46 to 51	-4.4 to 0.6
	-5	43.5 to 48.5	-6.9 to -1.9
M2	0	41 to 46	-9.4 to -4.4
	-5	38.5 to 43.5	-11.9 to -6.9
M3	0	36 to 41	-14.4 to -9.4
	-5	33.5 to 38.5	-16.9 to -11.9
M4	0	<36	<-14.4
	-5	<33.5	<-16.9

Cursor:

Total = 43.8319 dB V/m

E Category: M4

Location: -2, 75, 364.7 mm

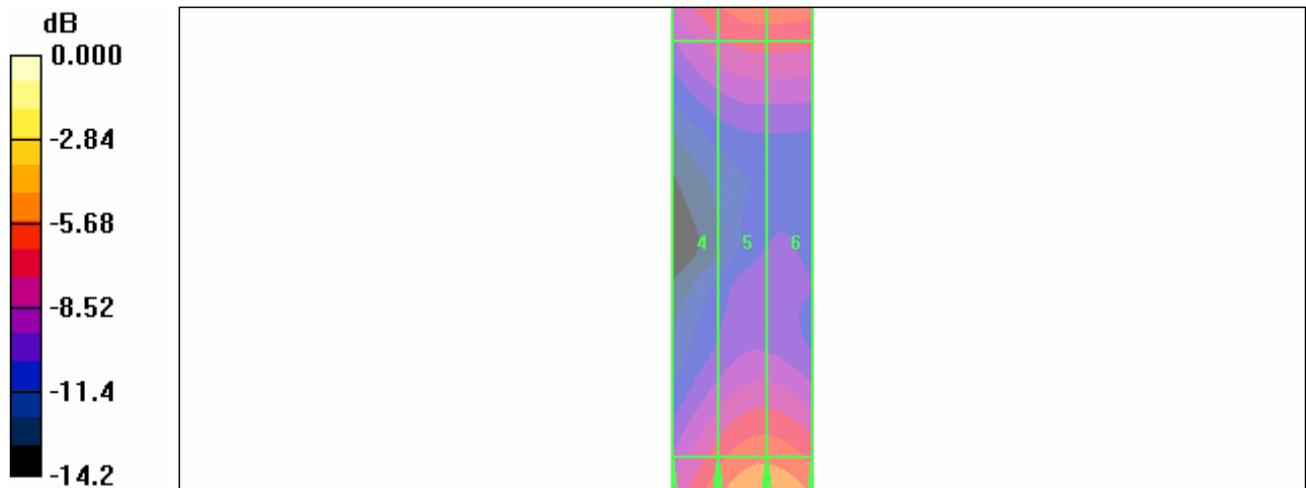

0 dB = 155.5V/m

HAC_E_Dipole_1880MHz

DUT: HAC-Dipole 1880MHz; Type: CD1880V3;

Communication System: CW; Frequency: 1880 MHz; Duty Cycle: 1:1

Medium: Air Medium parameters used: $\sigma = 0$ mho/m, $\epsilon_r = 1$; $\rho = 1000$ kg/m³

Phantom section: E Dipole Section

DASY4 Configuration:

- Probe: ER3DV6 - SN2302; ConvF(1, 1, 1); Calibrated: 2007/3/21
- Sensor-Surface: (Fix Surface)
- Electronics: DAE4 Sn547; Calibrated: 2007/3/5
- Phantom: HAC Test Arch 4.6; Type: SD HAC P01 BA;
- Measurement SW: DASY4, V4.7 Build 53; Postprocessing SW: SEMCAD, V1.8 Build 172

E Scan - ER probe center 10mm above CD1880 Dipole/Hearing Aid Compatibility Test

(41x181x1): Measurement grid: dx=5mm, dy=5mm

Maximum value of peak Total field = 138.5 V/m

Probe Modulation Factor = 1.00

Reference Value = 151.0 V/m; Power Drift = -0.001 dB

Hearing Aid Near-Field Category: M2 (AWF 0 dB)

Peak E-field in V/m

Grid 1	Grid 2	Grid 3
139.4	134.4	133.3
Grid 4	Grid 5	Grid 6
95.1	96.3	93.1
Grid 7	Grid 8	Grid 9
136.3	135.4	134.4

Category	AWF (dB)	Limits for E-Field Emissions dB(V/m) > 960MHz	Limits for H-Field Emissions dB(A/m) > 960MHz
M1	0	56 to 61	5.6 to 10.6


	-5	53.5 to 58.5	3.1 to 8.1
M2	0	51 to 56	0.6 to 5.6
	-5	48.5 to 53.5	-1.9 to 3.1
M3	0	46 to 51	-4.4 to 0.6
	-5	43.5 to 48.5	-6.9 to -1.9
M4	0	<46	<-4.4
	-5	<43.5	<-6.9
Category	AWF (dB)	Limits for E-Field Emissions dB(V/m) < 960MHz	Limits for H-Field Emissions dB(A/m) < 960 MHz
M1	0	46 to 51	-4.4 to 0.6
	-5	43.5 to 48.5	-6.9 to -1.9
M2	0	41 to 46	-9.4 to -4.4
	-5	38.5 to 43.5	-11.9 to -6.9
M3	0	36 to 41	-14.4 to -9.4
	-5	33.5 to 38.5	-16.9 to -11.9
M4	0	<36	<-14.4
	-5	<33.5	<-16.9

Cursor:

Total = 44.3194 dB V/m

E Category: M2

Location: -2, -37.5, 364.7 mm

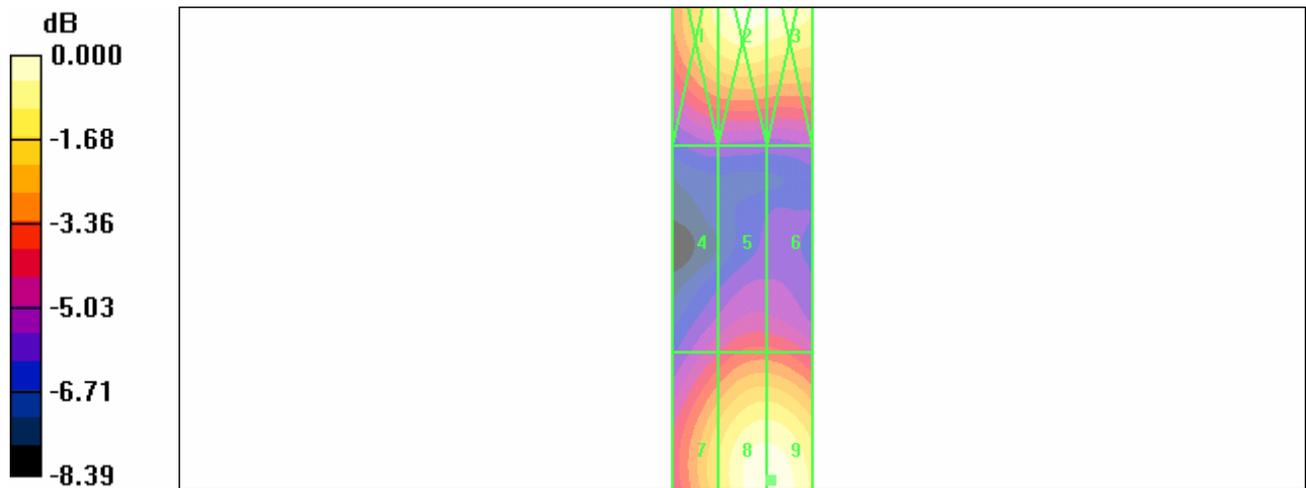

0 dB = 140.4V/m

HAC_H_Dipole_835MHz

DUT: HAC-Dipole 835 MHz; Type: CD835V3;

Communication System: CW; Frequency: 835 MHz; Duty Cycle: 1:1

Medium: Air Medium parameters used: $\sigma = 0$ mho/m, $\epsilon_r = 1$; $\rho = 1$ kg/m³

Phantom section: H Dipole Section

DASY4 Configuration:

- Probe: H3DV6 - SN6142; ; Calibrated: 2003/3/24
- Sensor-Surface: (Fix Surface)
- Electronics: DAE4 Sn547; Calibrated: 2007/3/5
- Phantom: HAC Test Arch 4.6; Type: SD HAC P01 BA;
- Measurement SW: DASY4, V4.7 Build 53; Postprocessing SW: SEMCAD, V1.8 Build 172

H Scan - H3DV6 probe center 10mm above CD835 Dipole/Hearing Aid Compatibility Test

(41x361x1): Measurement grid: dx=5mm, dy=5mm

Maximum value of peak Total field = 0.470 A/m

Probe Modulation Factor = 1.00

Reference Value = 0.472 A/m; Power Drift = -0.106 dB

Hearing Aid Near-Field Category: M4 (AWF 0 dB)

Peak H-field in A/m

Grid 1	Grid 2	Grid 3
0.333	0.403	0.403
Grid 4	Grid 5	Grid 6
0.389	0.470	0.470
Grid 7	Grid 8	Grid 9
0.354	0.432	0.432

Category	AWF (dB)	Limits for E-Field Emissions dB(V/m) > 960MHz	Limits for H-Field Emissions dB(A/m) > 960MHz
M1	0	56 to 61	5.6 to 10.6


	-5	53.5 to 58.5	3.1 to 8.1
M2	0	51 to 56	0.6 to 5.6
	-5	48.5 to 53.5	-1.9 to 3.1
M3	0	46 to 51	-4.4 to 0.6
	-5	43.5 to 48.5	-6.9 to -1.9
M4	0	<46	<-4.4
	-5	<43.5	<-6.9
Category	AWF (dB)	Limits for E-Field Emissions dB(V/m) < 960MHz	Limits for H-Field Emissions dB(A/m) < 960 MHz
M1	0	46 to 51	-4.4 to 0.6
	-5	43.5 to 48.5	-6.9 to -1.9
M2	0	41 to 46	-9.4 to -4.4
	-5	38.5 to 43.5	-11.9 to -6.9
M3	0	36 to 41	-14.4 to -9.4
	-5	33.5 to 38.5	-16.9 to -11.9
M4	0	<36	<-14.4
	-5	<33.5	<-16.9

Cursor:

Total = -6.55272 dB A/m

H Category: M4

Location: -4, 5, 364.7 mm

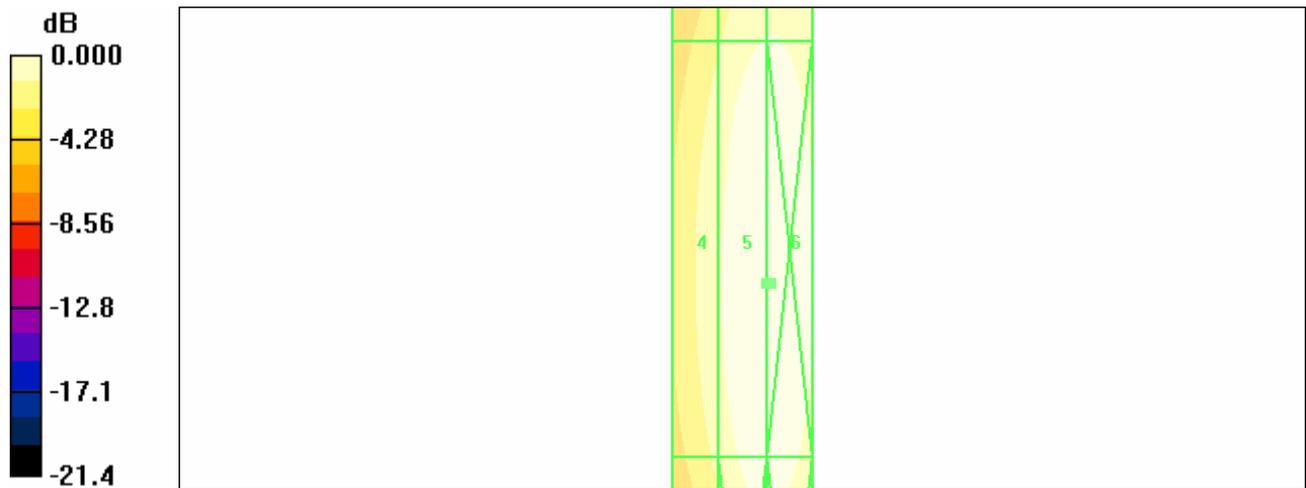

0 dB = 0.470A/m

HAC_H_Dipole_1880MHz

DUT: HAC-Dipole 1880MHz; Type: CD1880V3;

Communication System: CW; Frequency: 1880 MHz; Duty Cycle: 1:1

Medium: Air Medium parameters used: $\sigma = 0$ mho/m, $\epsilon_r = 1$; $\rho = 1$ kg/m³

Phantom section: H Dipole Section

DASY4 Configuration:

- Probe: H3DV6 - SN6142; ; Calibrated: 2003/3/24
- Sensor-Surface: (Fix Surface)
- Electronics: DAE4 Sn547; Calibrated: 2007/3/5
- Phantom: HAC Test Arch 4.6; Type: SD HAC P01 BA;
- Measurement SW: DASY4, V4.7 Build 53; Postprocessing SW: SEMCAD, V1.8 Build 172

H Scan - H3DV6 probe center 10mm above CD1880 Dipole/Hearing Aid Compatibility Test

(41x181x1): Measurement grid: dx=5mm, dy=5mm

Maximum value of peak Total field = 0.481 A/m

Probe Modulation Factor = 1.00

Reference Value = 0.478 A/m; Power Drift = -0.050 dB

Hearing Aid Near-Field Category: M2 (AWF 0 dB)

Peak H-field in A/m

Grid 1	Grid 2	Grid 3
0.353	0.438	0.438
Grid 4	Grid 5	Grid 6
0.388	0.481	0.481
Grid 7	Grid 8	Grid 9
0.344	0.430	0.430

Category	AWF (dB)	Limits for E-Field Emissions dB(V/m) > 960MHz	Limits for H-Field Emissions dB(A/m) > 960MHz
M1	0	56 to 61	5.6 to 10.6


	-5	53.5 to 58.5	3.1 to 8.1
M2	0	51 to 56	0.6 to 5.6
	-5	48.5 to 53.5	-1.9 to 3.1
M3	0	46 to 51	-4.4 to 0.6
	-5	43.5 to 48.5	-6.9 to -1.9
M4	0	<46	<-4.4
	-5	<43.5	<-6.9
Category	AWF (dB)	Limits for E-Field Emissions dB(V/m) < 960MHz	Limits for H-Field Emissions dB(A/m) < 960 MHz
M1	0	46 to 51	-4.4 to 0.6
	-5	43.5 to 48.5	-6.9 to -1.9
M2	0	41 to 46	-9.4 to -4.4
	-5	38.5 to 43.5	-11.9 to -6.9
M3	0	36 to 41	-14.4 to -9.4
	-5	33.5 to 38.5	-16.9 to -11.9
M4	0	<36	<-14.4
	-5	<33.5	<-16.9

Cursor:

Total = -6.35935 dB A/m

H Category: M2

Location: -4, -0.5, 364.7 mm

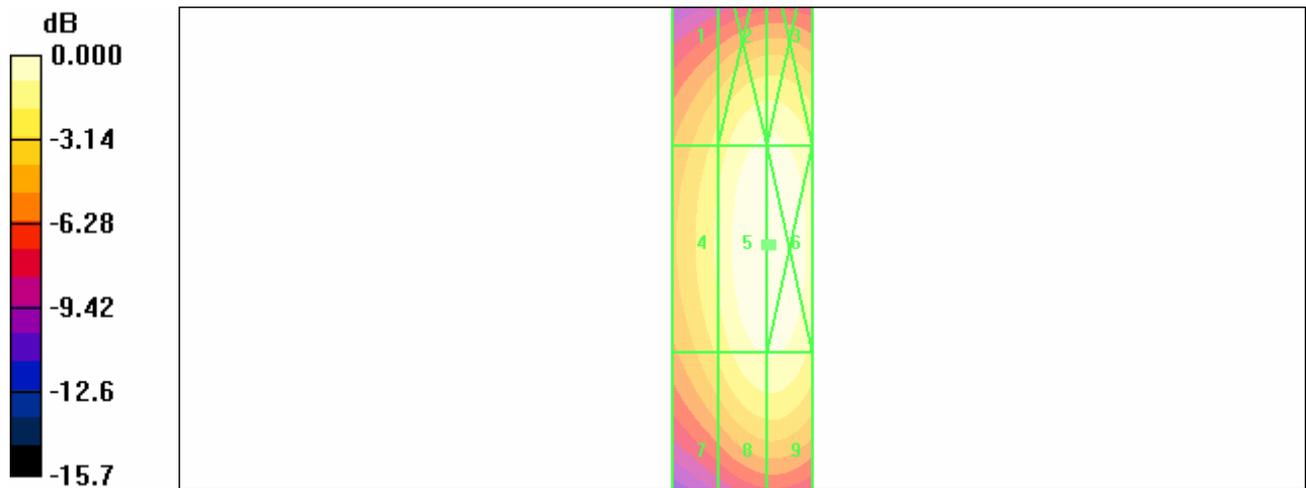

0 dB = 0.481A/m

14. DAE & Probe Calibration certificate

**Calibration Laboratory of
Schmid & Partner
Engineering AG**
Zeughausstrasse 43, 8004 Zurich, Switzerland



S Schweizerischer Kalibrierdienst
C Service suisse d'étalonnage
S Servizio svizzero di taratura
S Swiss Calibration Service

Accredited by the Swiss Federal Office of Metrology and Accreditation
The Swiss Accreditation Service is one of the signatories to the EA
Multilateral Agreement for the recognition of calibration certificates

Accreditation No.: **SCS 108**

Client **SGS (Auden)**

Certificate No: **DAE4-547_Mar07**

CALIBRATION CERTIFICATE

Object **DAE4 - SD 000 D04 BA - SN: 547**

Calibration procedure(s) **QA CAL-06.v12
Calibration procedure for the data acquisition electronics (DAE)**

Calibration date: **March 5, 2007**

Condition of the calibrated item **In Tolerance**

This calibration certificate documents the traceability to national standards, which realize the physical units of measurements (SI).
The measurements and the uncertainties with confidence probability are given on the following pages and are part of the certificate.

All calibrations have been conducted in the closed laboratory facility: environment temperature (22 ± 3)°C and humidity < 70%.

Calibration Equipment used (M&TE critical for calibration)

Primary Standards	ID #	Cal Date (Calibrated by, Certificate No.)	Scheduled Calibration
Fluke Process Calibrator Type 702	SN: 6295803	13-Oct-06 (Eical AG, No: 5492)	Oct-07
Keithley Multimeter Type 2001	SN: 0810278	03-Oct-06 (Eical AG, No: 5478)	Oct-07
Secondary Standards	ID #	Check Date (in house)	Scheduled Check
Calibrator Box V1.1	SE UMS 006 AB 1002	15-Jun-06 (SPEAG, in house check)	In house check Jun-07

Calibrated by:	Name Daniel Steinacher	Function Technician	Signature
Approved by:	Name Fin Bomholt	Function R&D Director	Signature

Issued: March 5, 2007

This calibration certificate shall not be reproduced except in full without written approval of the laboratory.

Calibration Laboratory of
 Schmid & Partner
 Engineering AG
 Zeughausstrasse 43, 8004 Zurich, Switzerland



S Schweizerischer Kalibrierdienst
C Service suisse d'étalonnage
S Servizio svizzero di taratura
S Swiss Calibration Service

Accredited by the Swiss Federal Office of Metrology and Accreditation
 The Swiss Accreditation Service is one of the signatories to the EA
 Multilateral Agreement for the recognition of calibration certificates

Accreditation No.: **SCS 108**

Client **SGS (Auden)**

Certificate No: **ER3-2306_Apr07**

CALIBRATION CERTIFICATE

Object **ER3DV6 - SN:2306**

Calibration procedure(s) **QA CAL-02.v5
 Calibration procedure for E-field probes optimized for close near field
 evaluations in air**

Calibration date: **April 20, 2007**

Condition of the calibrated item **In Tolerance**

This calibration certificate documents the traceability to national standards, which realize the physical units of measurements (SI).
 The measurements and the uncertainties with confidence probability are given on the following pages and are part of the certificate.

All calibrations have been conducted in the closed laboratory facility: environment temperature (22 ± 3)°C and humidity < 70%.

Calibration Equipment used (M&TE critical for calibration)

Primary Standards	ID #	Cal Date (Calibrated by, Certificate No.)	Scheduled Calibration
Power meter E4419B	GB41293874	29-Mar-07 (METAS, No. 217-00670)	Mar-08
Power sensor E4412A	MY41495277	29-Mar-07 (METAS, No. 217-00670)	Mar-08
Power sensor E4412A	MY41498087	29-Mar-07 (METAS, No. 217-00670)	Mar-08
Reference 3 dB Attenuator	SN: S5054 (3c)	10-Aug-06 (METAS, No. 217-00592)	Aug-07
Reference 20 dB Attenuator	SN: S5086 (20b)	29-Mar-07 (METAS, No. 217-00671)	Mar-08
Reference 30 dB Attenuator	SN: S5129 (30b)	10-Aug-06 (METAS, No. 217-00593)	Aug-07
Reference Probe ER3DV6	SN: 2328	2-Oct-06 (SPEAG, No. ER3-2328_Oct06)	Oct-07
DAE4	SN: 907	20-Jul-06 (SPEAG, No. DAE4-907_Jul06)	Jul-07

Secondary Standards	ID #	Check Date (in house)	Scheduled Check
RF generator HP 8648C	US3642U01700	4-Aug-99 (SPEAG, in house check Nov-05)	In house check: Nov-07
Network Analyzer HP 8753E	US37390585	18-Oct-01 (SPEAG, in house check Oct-06)	In house check: Oct-07

	Name	Function	Signature
Calibrated by:	Katja Pokovic	Technical Manager	<i>Katja Pokovic</i>
Approved by:	Niels Kuster	Quality Manager	<i>Niels Kuster</i>

Issued: April 21, 2007

This calibration certificate shall not be reproduced except in full without written approval of the laboratory.



Calibration Laboratory of
Schmid & Partner
Engineering AG
Zeughausstrasse 43, 8004 Zurich, Switzerland



S Schweizerischer Kalibrierdienst
C Service suisse d'étalonnage
S Servizio svizzero di taratura
S Swiss Calibration Service

Accredited by the Swiss Federal Office of Metrology and Accreditation
The Swiss Accreditation Service is one of the signatories to the EA
Multilateral Agreement for the recognition of calibration certificates

Accreditation No.: **SCS 108**

Glossary:

NORM_{x,y,z} sensitivity in free space
DCP diode compression point
Polarization φ φ rotation around probe axis
Polarization ϑ ϑ rotation around an axis that is in the plane normal to probe axis (at measurement center), i.e., $\vartheta = 0$ is normal to probe axis
Connector Angle information used in DASY system to align probe sensor X to the robot coordinate system

Calibration is Performed According to the Following Standards:

- a) IEEE Std 1309-2005, "IEEE Standard for calibration of electromagnetic field sensors and probes, excluding antennas, from 9 kHz to 40 GHz", December 2005.

Methods Applied and Interpretation of Parameters:

- **NORM_{x,y,z}**: Assessed for E-field polarization $\vartheta = 0$ for XY and $\vartheta = 90$ for Z sensor ($f \leq 900$ MHz in TEM-cell; $f > 1800$ MHz: R22 waveguide).
- **NORM(f)_{x,y,z}** = **NORM_{x,y,z}** * *frequency_response* (see Frequency Response Chart).
- **DCP_{x,y,z}**: DCP are numerical linearization parameters assessed based on the data of power sweep (no uncertainty required). DCP does not depend on frequency.
- **Spherical isotropy (3D deviation from isotropy)**: in a locally homogeneous field realized using an open waveguide setup.
- **Sensor Offset**: The sensor offset corresponds to the offset of virtual measurement center from the probe tip (on probe axis). No tolerance required.
- **Connector Angle**: The angle is assessed using the information gained by determining the **NORM_x** (no uncertainty required).

ER3DV6 SN:2306

April 20, 2007

Probe ER3DV6

SN:2306

Manufactured:	December 17, 2002
Last calibrated:	April 27, 2006
Recalibrated:	April 20, 2007

Calibrated for DASYS Systems

(Note: non-compatible with DASYS2 system!)

ER3DV6 SN:2306

April 20, 2007

DASY - Parameters of Probe: ER3DV6 SN:2306

Sensitivity in Free Space [$\mu\text{V}/(\text{V}/\text{m})^2$]		Diode Compression ^A	
NormX	1.09 ± 10.1 % (k=2)	DCP X	96 mV
NormY	1.12 ± 10.1 % (k=2)	DCP Y	96 mV
NormZ	1.26 ± 10.1 % (k=2)	DCP Z	100 mV

Frequency Correction

X	0.0
Y	0.0
Z	0.0

Sensor Offset (Probe Tip to Sensor Center)

X	2.5 mm
Y	2.5 mm
Z	2.5 mm

Connector Angle -223 °

The reported uncertainty of measurement is stated as the standard uncertainty of measurement multiplied by the coverage factor k=2, which for a normal distribution corresponds to a coverage probability of approximately 95%.


^A numerical linearization parameter: uncertainty not required

ER3DV6 SN:2306

April 20, 2007

Frequency Response of E-Field

(TEM-Cell:ifi110 EXX, Waveguide R22)

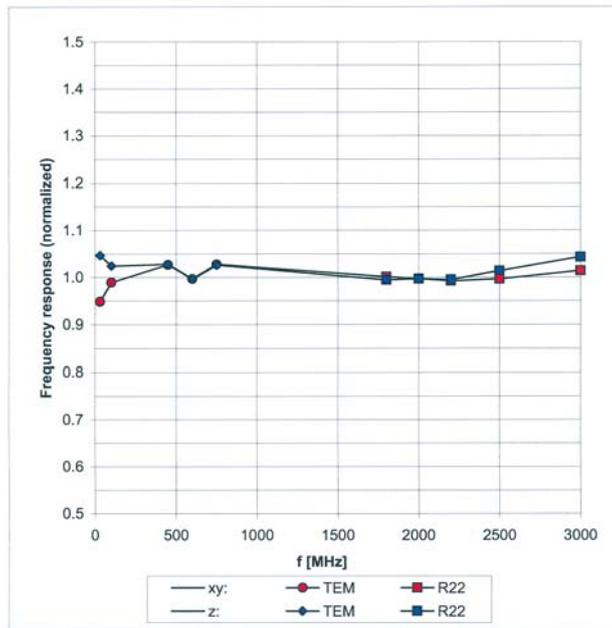


Uncertainty of Frequency Response of E-field: $\pm 6.3\%$ (k=2)


ER3DV6 SN:2306

April 20, 2007

Receiving Pattern (ϕ), $\vartheta = 0^\circ$

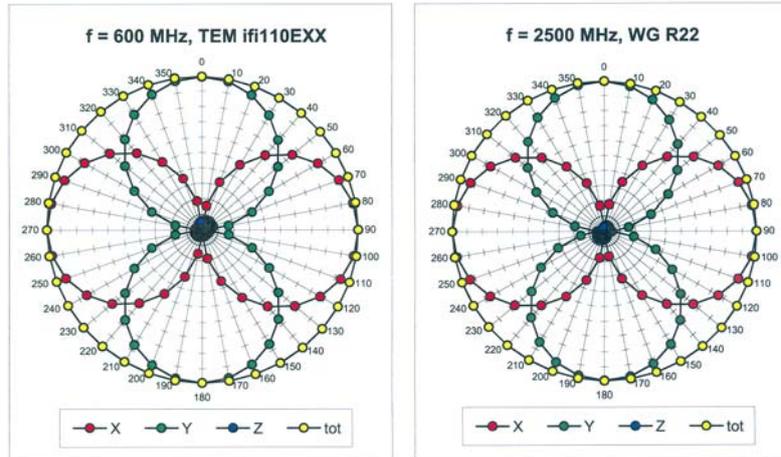


Receiving Pattern (ϕ), $\vartheta = 90^\circ$

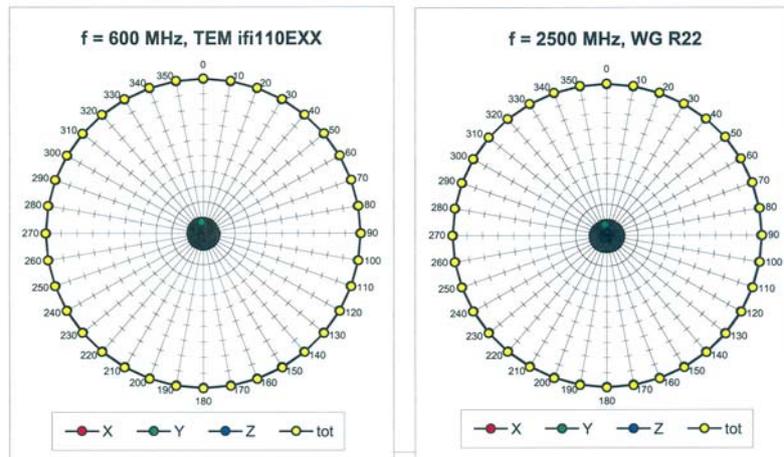

ER3DV6 SN:2306


April 20, 2007

Receiving Pattern (ϕ), $\vartheta = 0^\circ$

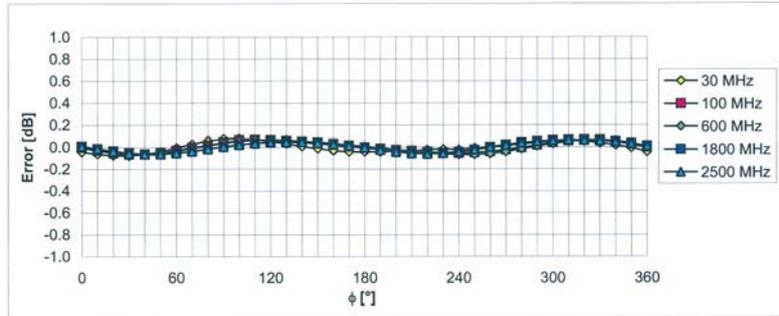

Uncertainty of Axial Isotropy Assessment: $\pm 0.5\%$ (k=2)

Receiving Pattern (ϕ), $\vartheta = 90^\circ$

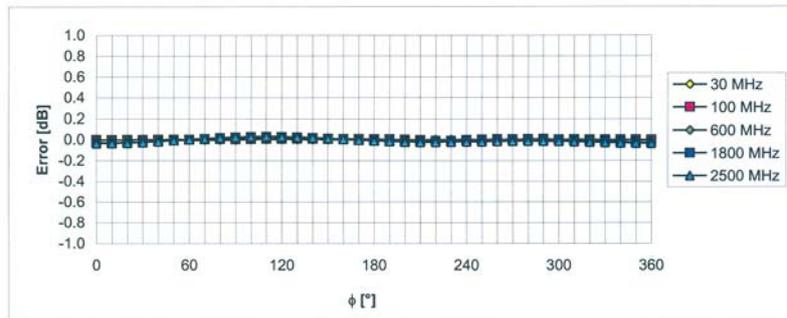



Uncertainty of Axial Isotropy Assessment: $\pm 0.5\%$ (k=2)

ER3DV6 SN:2306

April 20, 2007

Dynamic Range f(E-field)

(Waveguide R22, f = 1800 MHz)

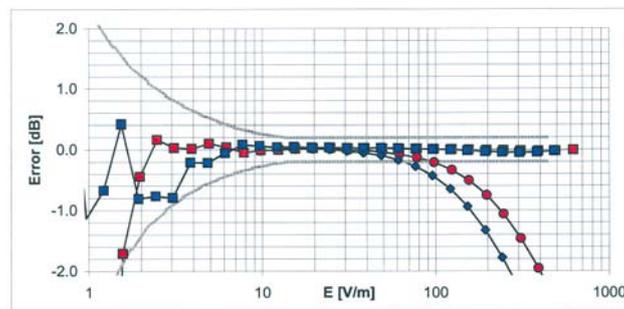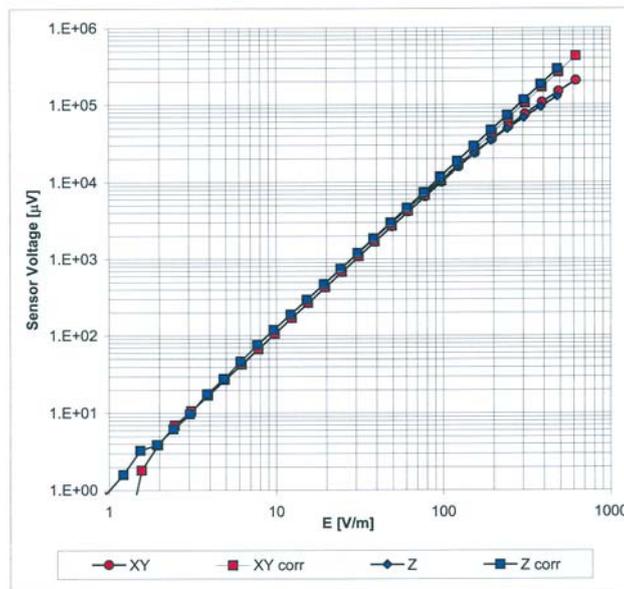


Uncertainty of Linearity Assessment: $\pm 0.6\%$ (k=2)

ER3DV6 SN:2306

April 20, 2007

Deviation from Isotropy in Air Error (ϕ, ϑ), $f = 900$ MHz

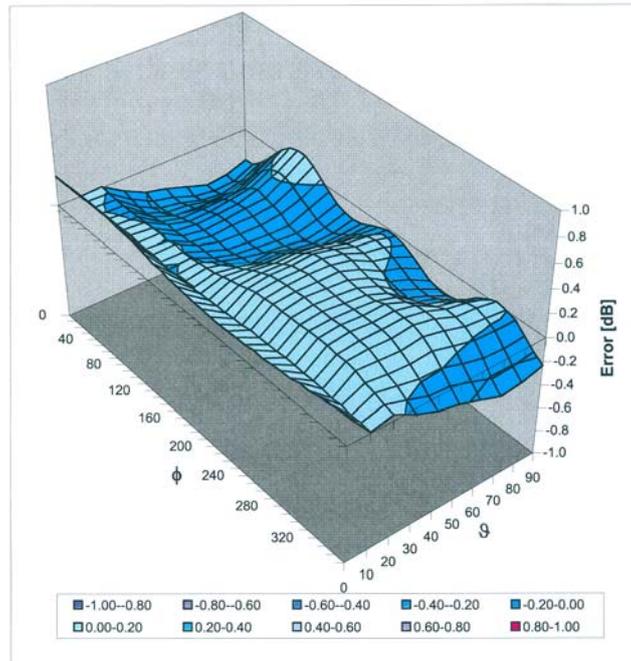

Uncertainty of Spherical Isotropy Assessment: $\pm 2.6\%$ ($k=2$)

**Calibration Laboratory of
Schmid & Partner
Engineering AG**
Zeughausstrasse 43, 8004 Zurich, Switzerland



S Schweizerischer Kalibrierdienst
C Service suisse d'étalonnage
S Servizio svizzero di taratura
S Swiss Calibration Service

Accredited by the Swiss Federal Office of Metrology and Accreditation
The Swiss Accreditation Service is one of the signatories to the EA
Multilateral Agreement for the recognition of calibration certificates

Accreditation No.: **SCS 108**

Client **SGS (Auden)**

Certificate No: **H3-6142_Apr07**

CALIBRATION CERTIFICATE

Object **H3DV6 - SN:6142**

Calibration procedure(s) **QA CAL-03.v5
Calibration procedure for H-field probes optimized for close near field
evaluations in air**

Calibration date: **April 20, 2007**

Condition of the calibrated item **In Tolerance**

This calibration certificate documents the traceability to national standards, which realize the physical units of measurements (SI).
The measurements and the uncertainties with confidence probability are given on the following pages and are part of the certificate.

All calibrations have been conducted in the closed laboratory facility: environment temperature (22 ± 3)°C and humidity < 70%.

Calibration Equipment used (M&TE critical for calibration)

Primary Standards	ID #	Cal Date (Calibrated by, Certificate No.)	Scheduled Calibration
Power meter E4419B	GB41293874	29-Mar-07 (METAS, No. 217-00670)	Mar-08
Power sensor E4412A	MY41495277	29-Mar-07 (METAS, No. 217-00670)	Mar-08
Power sensor E4412A	MY41498087	29-Mar-07 (METAS, No. 217-00670)	Mar-08
Reference 3 dB Attenuator	SN: S5054 (3c)	10-Aug-06 (METAS, No. 217-00592)	Aug-07
Reference 20 dB Attenuator	SN: S5086 (20b)	29-Mar-07 (METAS, No. 217-00671)	Mar-08
Reference 30 dB Attenuator	SN: S5129 (30b)	10-Aug-06 (METAS, No. 217-00593)	Aug-07
Reference Probe H3DV6	SN: 6182	2-Oct-06 (SPEAG, No. H3-6182_Oct06)	Oct-07
DAE4	SN: 907	20-Jul-06 (SPEAG, No. DAE4-907_Jul06)	Jul-07
Secondary Standards	ID #	Check Date (in house)	Scheduled Check
RF generator HP 8648C	US3642U01700	4-Aug-99 (SPEAG, in house check Nov-05)	In house check: Nov-07
Network Analyzer HP 8753E	US37390585	18-Oct-01 (SPEAG, in house check Oct-06)	In house check: Oct-07

	Name	Function	Signature
Calibrated by:	Katja Pokovic	Technical Manager	<i>[Signature]</i>
Approved by:	Niels Kuster	Quality Manager	<i>[Signature]</i>

Issued: April 21, 2007

This calibration certificate shall not be reproduced except in full without written approval of the laboratory.



Calibration Laboratory of
Schmid & Partner
Engineering AG
Zeughausstrasse 43, 8004 Zurich, Switzerland



S Schweizerischer Kalibrierdienst
C Service suisse d'étalonnage
S Servizio svizzero di taratura
S Swiss Calibration Service

Accredited by the Swiss Federal Office of Metrology and Accreditation
The Swiss Accreditation Service is one of the signatories to the EA
Multilateral Agreement for the recognition of calibration certificates

Accreditation No.: **SCS 108**

Glossary:

NORM_{x,y,z} sensitivity in free space
DCP diode compression point
Polarization φ φ rotation around probe axis
Polarization ϑ ϑ rotation around an axis that is in the plane normal to probe axis (at measurement center), i.e., $\vartheta = 0$ is normal to probe axis
Connector Angle information used in DASY system to align probe sensor X to the robot coordinate system

Calibration is Performed According to the Following Standards:

- a) IEEE Std 1309-2005, " IEEE Standard for calibration of electromagnetic field sensors and probes, excluding antennas, from 9 kHz to 40 GHz", December 2005.

Methods Applied and Interpretation of Parameters:

- X, Y, Z_{a0a1a2} : Assessed for E-field polarization $\vartheta = 90$ for XY sensors and $\vartheta = 0$ for Z sensor ($f \leq 900$ MHz in TEM-cell; $f > 1800$ MHz: R22 waveguide).
- $X, Y, Z(f)_{a0a1a2} = X, Y, Z_{a0a1a2} * frequency_response$ (see Frequency Response Chart).
- $DCP_{x,y,z}$: DCP are numerical linearization parameters assessed based on the data of power sweep (no uncertainty required). DCP does not depend on frequency.
- *Spherical isotropy (3D deviation from isotropy)*: in a locally homogeneous field realized using an open waveguide setup.
- *Sensor Offset*: The sensor offset corresponds to the offset of virtual measurement center from the probe tip (on probe axis). No tolerance required.
- *Connector Angle*: The angle is assessed using the information gained by determining the X_{a0a1a2} (no uncertainty required).

H3DV6 SN:6142

April 20, 2007

Probe H3DV6

SN:6142

Manufactured:	July 3, 2002
Last calibrated:	April 27, 2006
Recalibrated:	April 20, 2007

Calibrated for DASYS Systems

(Note: non-compatible with DASYS2 system!)

H3DV6 SN:6142

April 20, 2007

DASY - Parameters of Probe: H3DV6 SN:6142Sensitivity in Free Space [A/m / $\sqrt{(\mu V)}$]

	a0	a1	a2
X	2.674E-03	-9.212E-6	-3.625E-5 \pm 5.1 % (k=2)
Y	2.643E-03	-2.672E-5	-1.572E-5 \pm 5.1 % (k=2)
Z	3.005E-03	-2.017E-4	5.514E-6 \pm 5.1 % (k=2)

Diode Compression¹

DCP X	86 mV
DCP Y	86 mV
DCP Z	86 mV

Sensor Offset (Probe Tip to Sensor Center)

X	3.0 mm
Y	3.0 mm
Z	3.0 mm

Connector Angle -67 °

The reported uncertainty of measurement is stated as the standard uncertainty of measurement multiplied by the coverage factor k=2, which for a normal distribution corresponds to a coverage probability of approximately 95%.


¹ numerical linearization parameter: uncertainty not required

H3DV6 SN:6142

April 20, 2007

Frequency Response of H-Field

(TEM-Cell:ifi1110, Waveguide R22)

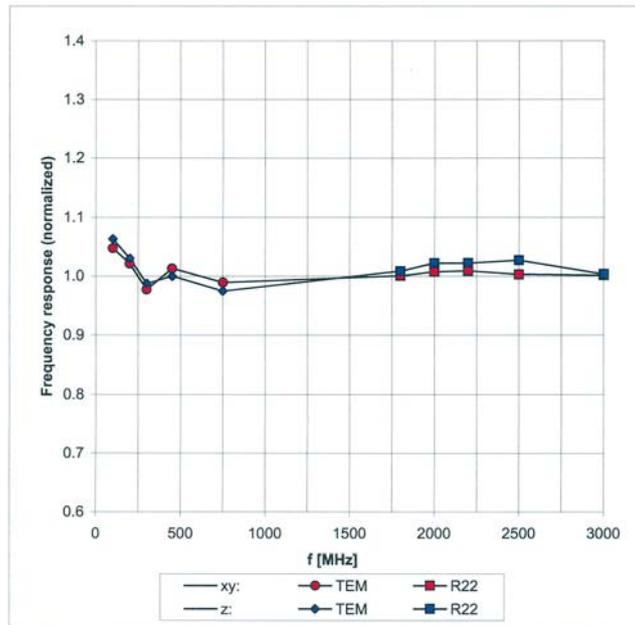


Uncertainty of Frequency Response of E-field: $\pm 6.3\%$ (k=2)


H3DV6 SN:6142

April 20, 2007

Receiving Pattern (ϕ), $\vartheta = 90^\circ$

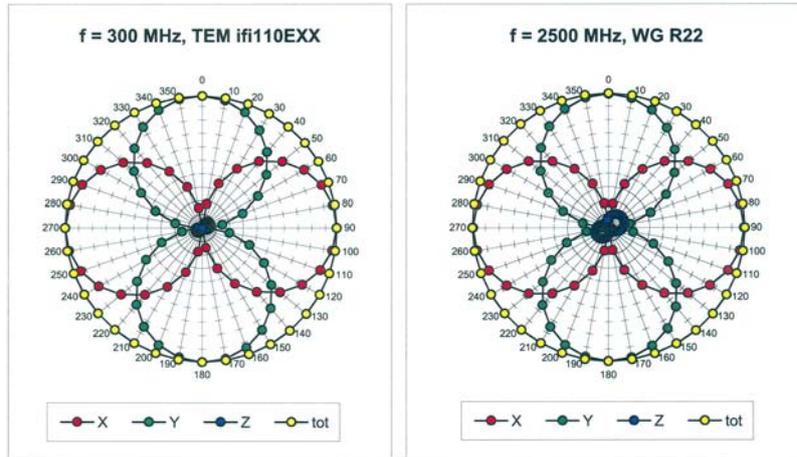


Receiving Pattern (ϕ), $\vartheta = 0^\circ$

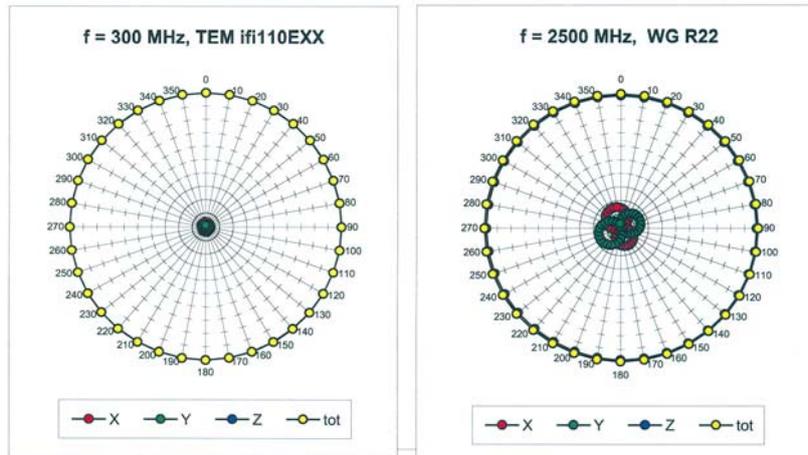

H3DV6 SN:6142


April 20, 2007

Receiving Pattern (ϕ), $\vartheta = 90^\circ$

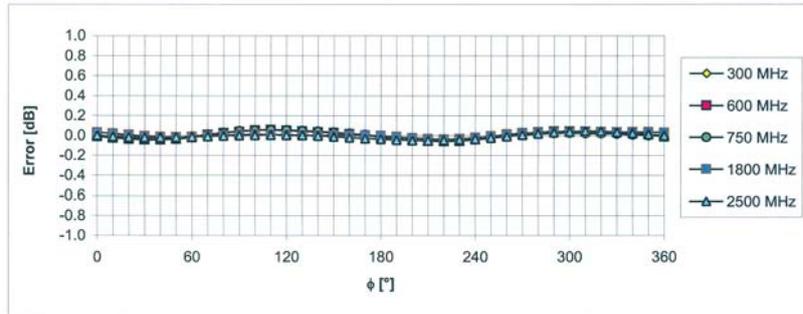

Uncertainty of Axial Isotropy Assessment: $\pm 0.5\%$ ($k=2$)

Receiving Pattern (ϕ), $\vartheta = 0^\circ$

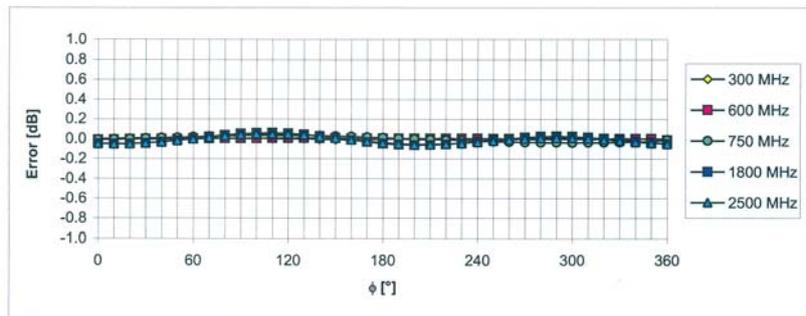



Uncertainty of Axial Isotropy Assessment: $\pm 0.5\%$ ($k=2$)

H3DV6 SN:6142

April 20, 2007

Dynamic Range f(H-field)

(Waveguide R22, f = 1800 MHz)

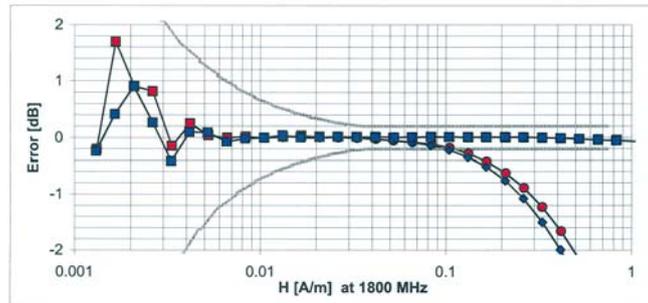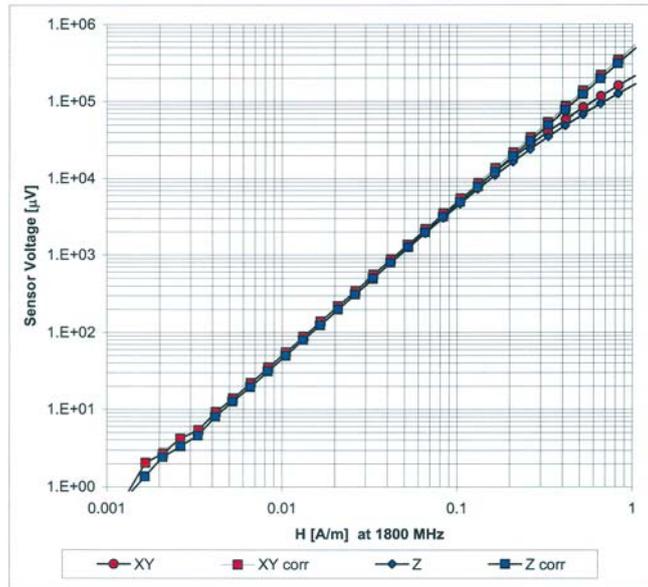

Uncertainty of Linearity Assessment: $\pm 0.6\%$ (k=2)

14. Uncertainty Analysis

HAC-Extension Setup Performance Test Using SPEAG Calibration Dipoles							
Error Description	Uncertainty value	Prob. Dist.	Div.	(c_1) E	(c_1) H	Std. Unc. E	Std. Unc. H
Measurement System							
Probe Calibration	±5.1%	N	1	1	1	±5.1%	±5.1%
Axial Isotropy	±4.7%	R	$\sqrt{3}$	1	1	±2.7%	±2.7%
Sensor Displacement	±16.5%	R	$\sqrt{3}$	1	0.145	±9.5%	±1.4%
Boundary Effects	±2.4%	R	$\sqrt{3}$	1	1	±1.4%	±1.4%
Linearity	±4.7%	R	$\sqrt{3}$	1	1	±2.7%	±2.7%
Scaling to Peak Envelope Power	±0%	R	$\sqrt{3}$	1	1	±0%	±0%
System Detection Limit	±1.0%	R	$\sqrt{3}$	1	1	±0.6%	±0.6%
Readout Electronics	±0.3%	N	1	1	1	±0.3%	±0.3%
Response Time	±0%	R	$\sqrt{3}$	1	1	±0%	±0%
Integration Time	±0%	R	$\sqrt{3}$	1	1	±0%	±0%
RF Ambient Conditions	±3.0%	R	$\sqrt{3}$	1	1	±1.7%	±1.7%
RF Reflections	±6.0%	R	$\sqrt{3}$	1	1	±3.5%	±3.5%
Probe Positioner	±1.2%	R	$\sqrt{3}$	1	0.67	±0.7%	±0.5%
Probe Positioning	±4.7%	R	$\sqrt{3}$	1	0.67	±2.7%	±1.8%
Extrap. and Interpolation	±1.0%	R	$\sqrt{3}$	1	1	±0.6%	±0.6%
Dipole Related							
Distance Dipole - Scanning Plane	±5.2%	R	$\sqrt{3}$	1	0.3	±3.0%	±0.9%
Input power	±4.7%	N	1	1	1	±4.7%	±4.7%
Combined Std. Uncertainty						±13.7%	±9.3%
Expanded Std. Uncertainty on Power						±27.4%	±18.6%
Expanded Std. Uncertainty on Field						±13.7%	±9.3%

Table 28.1: Uncertainty budget for HAC setup performance test. The budget is valid for the frequency range 800 MHz - 3 GHz and represents a worst-case analysis with respect to power uncertainty of the field. Some of the parameters are dependent on the user situations and need adjustment according to the actual laboratory conditions.

15. System Validation from Original equipment supplier

3.3.3 DASY4 E-Field Result

Date/Time: 1/16/2007 10:41:20 AM

Test Laboratory: SPEAG, Zurich, Switzerland

DUT: HAC-Dipole 835 MHz; Type: D835V3; Serial: 1052

Communication System: CW; Frequency: 835 MHz; Duty Cycle: 1:1

Medium: Air

Medium parameters used: $\sigma = 0$ mho/m, $\epsilon_r = 1$; $\rho = 1000$ kg/m³

Phantom section: E Dipole Section

DASY4 Configuration:

- Probe: ER3DV6 - SN2336; ConvF(1, 1, 1); Calibrated: 12/27/2006
- Sensor-Surface: (Fix Surface)
- Electronics: DAE4 Sn660; Calibrated: 3/1/2006
- Phantom: HAC Test Arch 4.6; Type: SD HAC P01 BA; Serial: 1002
- Measurement SW: DASY4, V4.7 Build 53; Postprocessing SW: SEMCAD, V1.8 Build 172

E Scan - Sensor Center 10mm above CD835 Dipole/Hearing Aid Compatibility Test (41x361x1):

Measurement grid: dx=5mm, dy=5mm

Maximum value of peak Total field = 166.6 V/m


Probe Modulation Factor = 1.00

Reference Value = 107.8 V/m; Power Drift = -0.062 dB

Hearing Aid Near-Field Category: M4 (AWF 0 dB)

Peak E-field in V/m

Grid 1	Grid 2	Grid 3
157.9	162.2	155.7
Grid 4	Grid 5	Grid 6
85.6	87.0	84.3
Grid 7	Grid 8	Grid 9
159.8	166.6	163.4

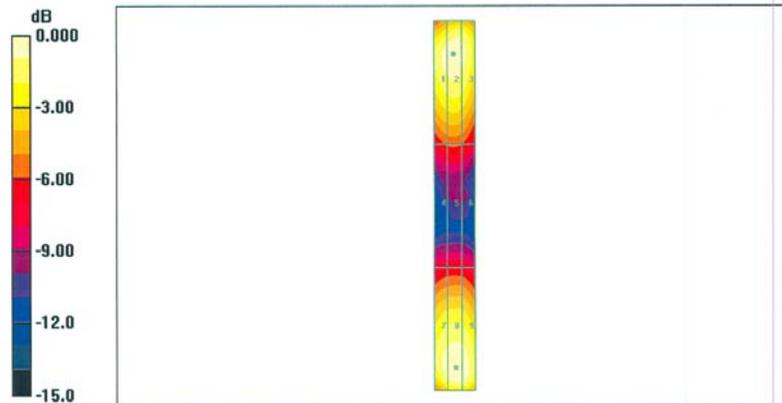

0 dB = 166.6V/m

3.3.2 DASY4 H-Field Result

Date/Time: 1/15/2007 12:33:14 PM

Test Laboratory: SPEAG, Zurich, Switzerland

DUT: HAC-Dipole 835 MHz; Type: CD835V3; Serial: 1052

Communication System: CW; Frequency: 835 MHz; Duty Cycle: 1:1

Medium: Air

Medium parameters used: $\sigma = 0$ mho/m, $\epsilon_r = 1$; $\rho = 1$ kg/m³

Phantom section: H Dipole Section

DASY4 Configuration:

- Probe: H3DV6 - SN6065; Calibrated: 12/27/2006
- Sensor-Surface: (Fix Surface)
- Electronics: DAE4 Sn660; Calibrated: 3/1/2006
- Phantom: HAC Test Arch 4.6; Type: SD HAC P01 BA; Serial: 1002
- Measurement SW: DASY4, V4.7 Build 53; Postprocessing SW: SEMCAD, V1.8 Build 172

H Scan - Sensor Center 10mm above CD835 Dipole/Hearing Aid Compatibility Test (41x361x1):

Measurement grid: dx=5mm, dy=5mm

Maximum value of peak Total field = 0.450 A/m



Probe Modulation Factor = 1.00

Reference Value = 0.476 A/m; Power Drift = 0.018 dB

Hearing Aid Near-Field Category: M4 (AWF 0 dB)

Peak H-field in A/m

Grid 1	Grid 2	Grid 3
0.371	0.401	0.385
Grid 4	Grid 5	Grid 6
0.415	0.450	0.437
Grid 7	Grid 8	Grid 9
0.361	0.394	0.387

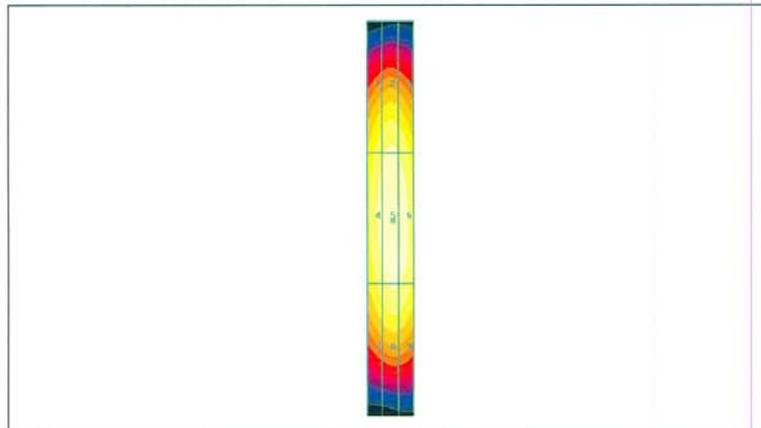

0 dB = 0.450A/m

3.3.3 DASY4 E-Field Result

Date/Time: 1/15/2007 5:52:23 PM

Test Laboratory: SPEAG, Zurich, Switzerland

DUT: HAC Dipole 1880 MHz; Type: CD1880V3; Serial: 1044

Communication System: CW; Frequency: 1880 MHz; Duty Cycle: 1:1

Medium: Air

Medium parameters used: $\sigma = 0$ mho/m, $\epsilon_r = 1$; $\rho = 1000$ kg/m³

Phantom section: E Dipole Section

DASY4 Configuration:

- Probe: ER3DV6 - SN2336; ConvF(1, 1, 1); Calibrated: 12/27/2006
- Sensor-Surface: (Fix Surface)
- Electronics: DAE4 Sn660; Calibrated: 3/1/2006
- Phantom: HAC Test Arch 4.6; Type: SD HAC P01 BA; Serial: 1002
- Measurement SW: DASY4, V4.7 Build 53; Postprocessing SW: SEMCAD, V1.8 Build 172

E Scan - Sensor Center 10mm above CD1880V3 Dipole/Hearing Aid Compatibility Test (41x181x1):

Measurement grid: dx=5mm, dy=5mm

Maximum value of peak Total field = 135.3 V/m


Probe Modulation Factor = 1.00

Reference Value = 152.1 V/m; Power Drift = -0.009 dB

Hearing Aid Near-Field Category: M2 (AWF 0 dB)

Peak E-field in V/m

Grid 1 130.6	Grid 2 135.3	Grid 3 132.3
Grid 4 89.5	Grid 5 90.7	Grid 6 87.5
Grid 7 129.8	Grid 8 135.0	Grid 9 131.1

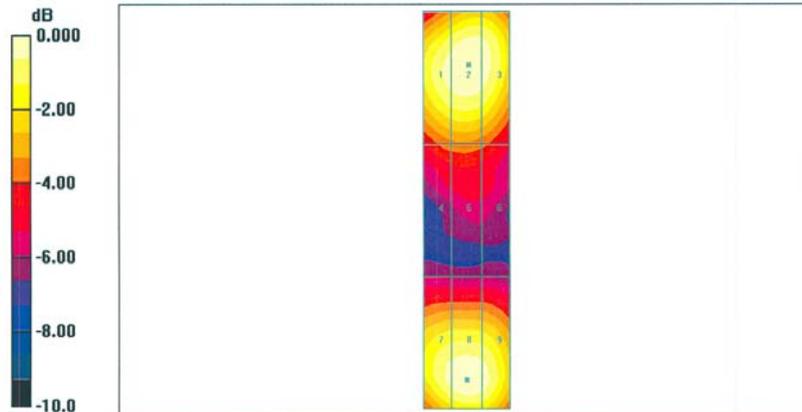

0 dB = 135.3V/m

3.3.2 DASY4 H-Field Result

Date/Time: 1/15/2007 3:53:10 PM

Test Laboratory: SPEAG, Zurich, Switzerland

DUT: HAC Dipole 1880 MHz; Type: CD1880V3; Serial: 1044

Communication System: CW; Frequency: 1880 MHz; Duty Cycle: 1:1

Medium: Air

Medium parameters used: $\sigma = 0$ mho/m, $\epsilon_r = 1$; $\rho = 1$ kg/m³

Phantom section: H Dipole Section

DASY4 Configuration:

- Probe: H3DV6 - SN6065; Calibrated: 12/27/2006
- Sensor-Surface: (Fix Surface)
- Electronics: DAE4 Sn660; Calibrated: 3/1/2006
- Phantom: HAC Test Arch 4.6; Type: SD HAC P01 BA; Serial: 1002
- Measurement SW: DASY4, V4.7 Build 53; Postprocessing SW: SEMCAD, V1.8 Build 172

H Scan - Sensor Center 10mm above CD1880V3 Dipole/Hearing Aid Compatibility Test (41x181x1):

Measurement grid: dx=5mm, dy=5mm

Maximum value of peak Total field = 0.457 A/m


Probe Modulation Factor = 1.00

Reference Value = 0.482 A/m; Power Drift = 0.021 dB

Hearing Aid Near-Field Category: M2 (AWF 0 dB)

Peak H-field in A/m

Grid 1	Grid 2	Grid 3
0.400	0.430	0.414
Grid 4	Grid 5	Grid 6
0.430	0.457	0.442
Grid 7	Grid 8	Grid 9
0.384	0.407	0.394

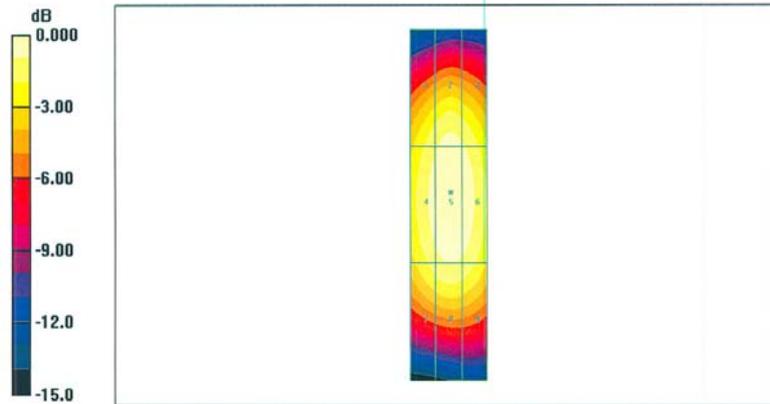

0 dB = 0.457A/m