



ONE WORLD ◊ OUR APPROVAL

## Internal photos

Date of issue: May 17, 2021

Applicant:  
Stryker Instruments

Product:  
SurgiCount®+

Model:  
SurgiCount®+ Cradle: 0694-002-002

FCC ID: Q9R-0042

[www.nemko.com](http://www.nemko.com)

Nemko Canada Inc., a testing laboratory, is accredited by the Standards Council of Canada. The tests included in this report are within the scope of this accreditation

*Internal photos.docx; Date: May 2013*




## Section 1. Internal photos

---

### 1.1 Top general view

---



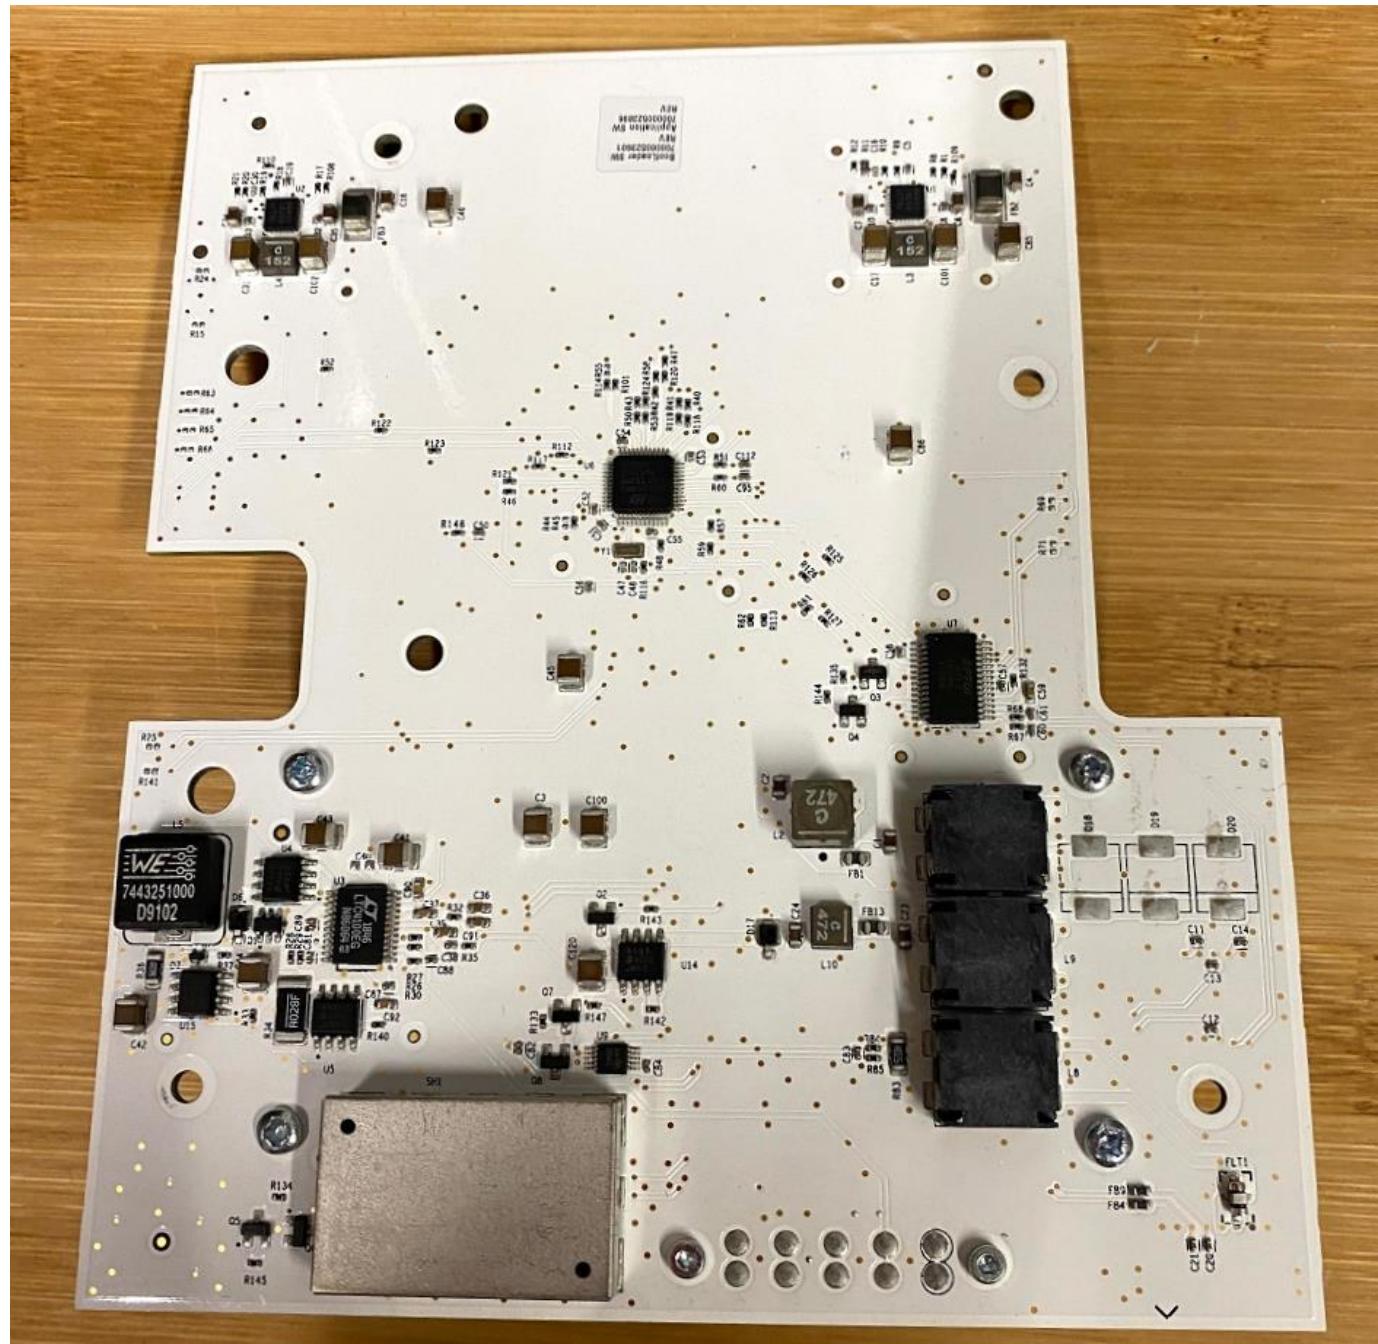


1.2 13.56 MHz module shielded view


---




### 1.3 RF modules view with removed shieldings

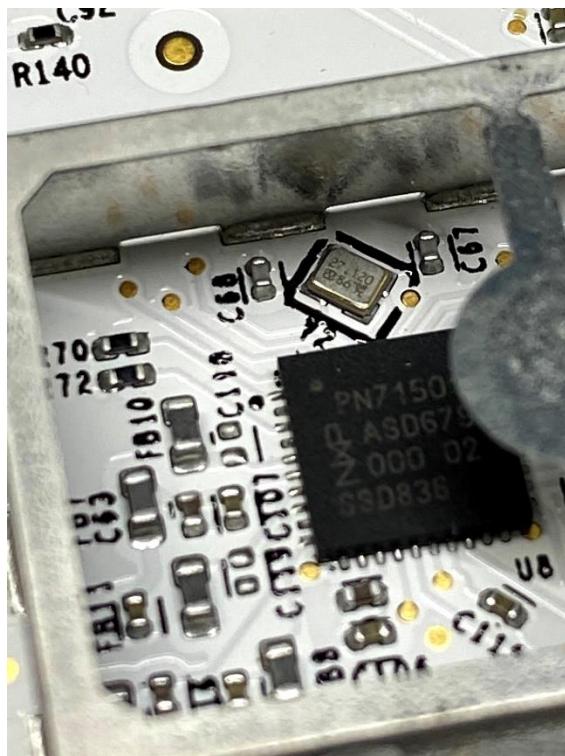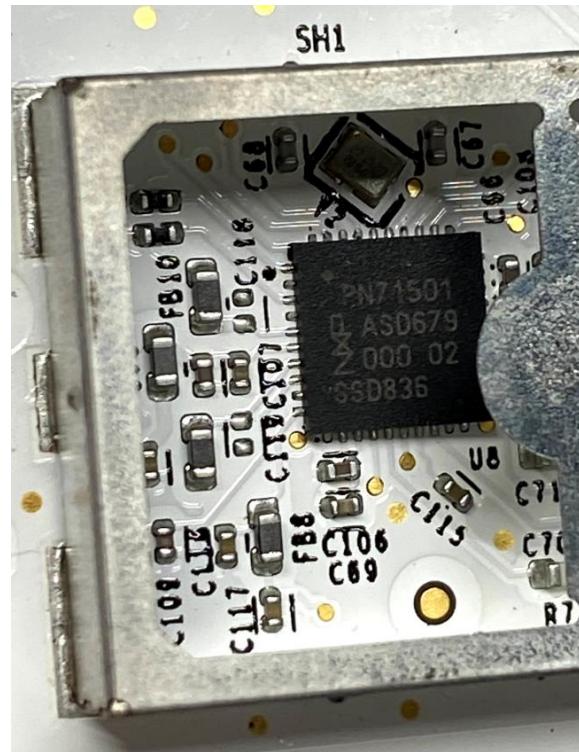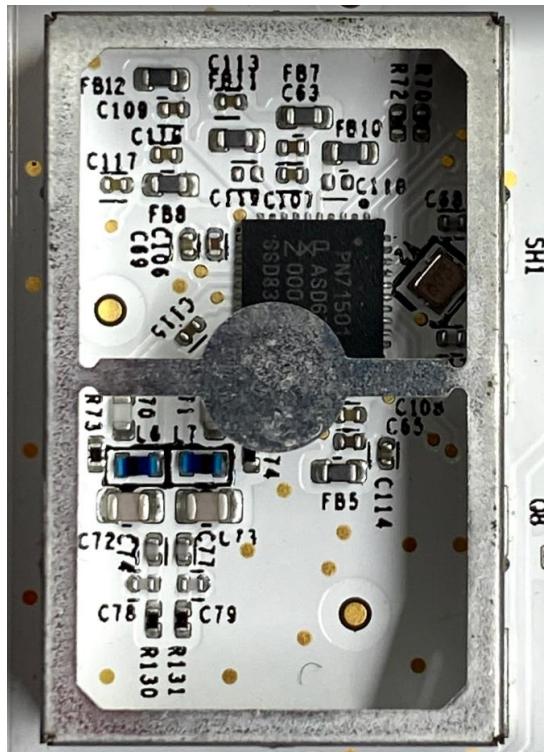


## 1.4 Antenna and Mounting view

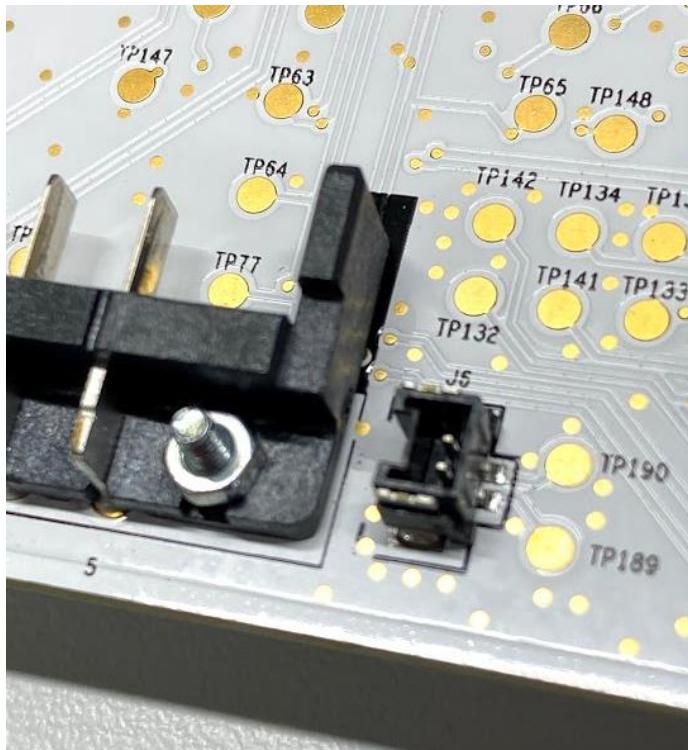


PCBA NFC Antenna Connector

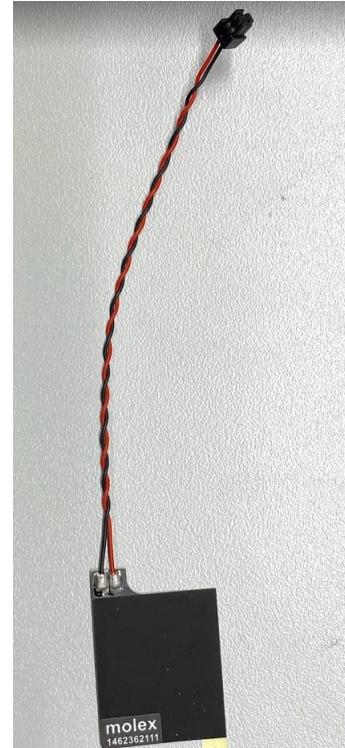

NFC Antenna

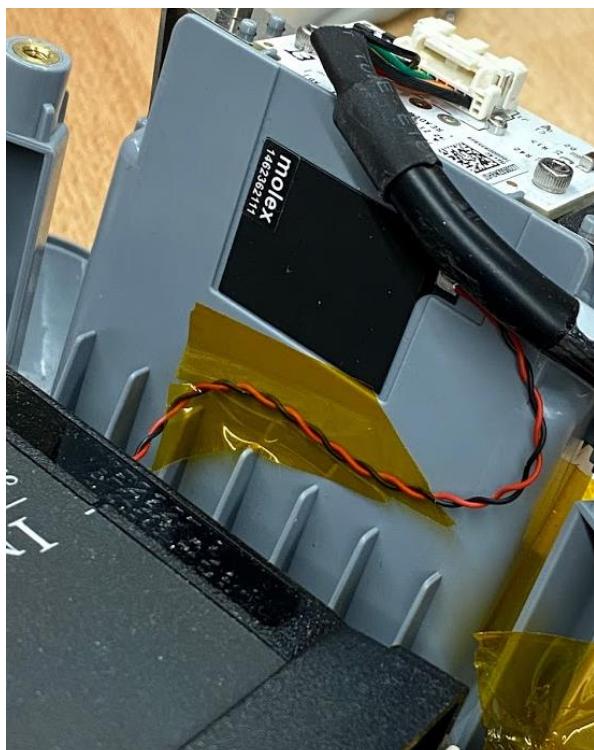

NFC Antenna Adhered to Enclosure

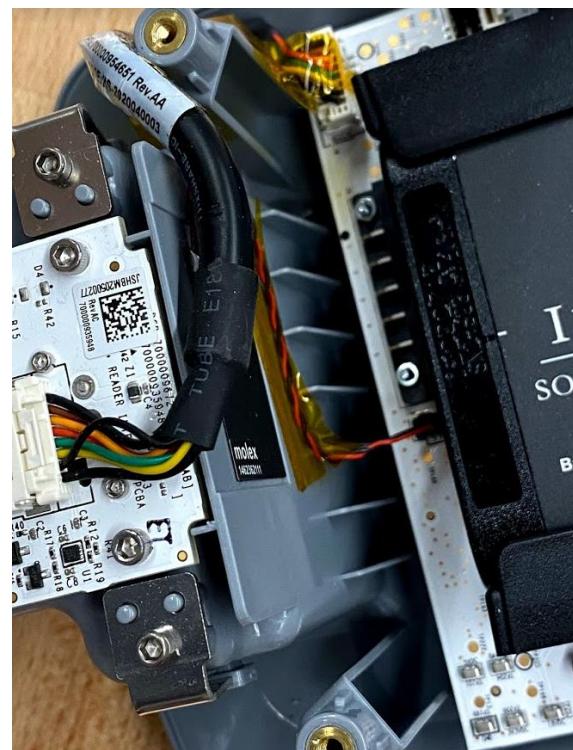

NFC Antenna Mounted and Connected to PCBA

## 1.5 PCB bottom view

