



RF EXPOSURE LAB, LLC

2867 Progress Place, Suite 4D • Escondido, CA 92029 • U.S.A.
TEL (760) 737-3131 • FAX (760) 737-9131
<http://www.rfexposurelab.com>

CERTIFICATE OF COMPLIANCE SAR EVALUATION

CardioNet Inc.
1010 Second Ave., #700
San Diego, CA 92101

Dates of Test: September 18-19, 2009
Test Report Number: SAR.20090901
Revision A

FCC ID:	QBI-1012
Model(s):	C5
Test Sample:	Engineering Unit Same as Production
Serial No.:	Eng 1 and Eng 2
Equipment Type:	Push to Talk Transmitter
Classification:	Portable Transmitter Held to Face and Next to Body
TX Frequency Range:	824.2 – 848.8 MHz, 1850.2 – 1909.8 MHz MHz
Frequency Tolerance:	± 2.5 ppm
Maximum RF Output:	850 MHz (CDMA) – 24.64 dBm, 850 MHz (GSM) – 33.16 dBm, 1900 MHz (CDMA) – 24.60 dBm, 1900 MHz (GSM) – 29.61 dBm Conducted
Signal Modulation:	GMSK, 8PSK, CDMA
Antenna Type (Length):	CardioNet P/N 010-0023-02
Battery:	Rosslare Enterprises Ltd.: P/N: ESB-RS670+001
Application Type:	Certification
FCC Rule Parts:	Part 2

This wireless mobile and/or portable device has been shown to be compliant for localized specific absorption rate (SAR) for uncontrolled environment/general exposure limits specified in ANSI/IEEE Std. C95.1-1999 and had been tested in accordance with the measurement procedures specified in IEEE 1528-2003, OET Bulletin 65 Supp. C, RSS-102 and Safety Code 6 (See test report).

I attest to the accuracy of the data. All measurements were performed by myself or were made under my supervision and are correct to the best of my knowledge and belief. I assume full responsibility for the completeness of these measurements and vouch for the qualifications of all persons taking them.

RF Exposure Lab, LLC certifies that no party to this application has been denied FCC benefits pursuant to Section 5301 of the Anti-Drug Abuse Act of 1988, 21 U.S.C. 853(a).

Jay M. Moulton
Vice President



Certificate # 2387.01

Table of Contents

1. Introduction.....	3
SAR Definition [5]	3
2. SAR Measurement Setup.....	4
Robotic System.....	4
System Hardware	4
System Description.....	4
E-Field Probe	5
3. Robot Specifications.....	7
4. Probe and Dipole Calibration	8
5. Phantom & Simulating Tissue Specifications.....	9
SAM Phantom.....	9
Brain & Muscle Simulating Mixture Characterization.....	9
Device Holder	9
6. Definition of Reference Points.....	10
Ear Reference Point	10
Device Reference Points	10
7. Test Configuration Positions	11
Positioning for Cheek/Touch [5].....	11
Positioning for Ear / 15° Tilt [5]	12
Body Worn Configurations.....	13
8. ANSI/IEEE C95.1 – 1999 RF Exposure Limits [2]	14
Uncontrolled Environment	14
Controlled Environment	14
9. Measurement Uncertainty	15
10. System Validation	16
Tissue Verification	16
Test System Verification	16
11. SAR Test Data Summary.....	17
Procedures Used To Establish Test Signal	17
Device Test Condition.....	17
12. FCC 3G Measurement Procedures – March 2008	18
12.1 Procedures Used to Establish RF Signal for SAR	18
12.2 SAR Measurement Conditions	18
12.3 SAR Measurement Conditions for GSM.....	18
SAR Data Summary – 835 MHz CDMA Face Position	20
SAR Data Summary – 835 MHz CDMA Body Position	21
SAR Data Summary – 835 MHz GSM Face Position.....	22
SAR Data Summary – 835 MHz GPRS Body Position	23
SAR Data Summary – 1900 MHz CDMA Face Position	24
SAR Data Summary – 1900 MHz CDMA Body Position	25
SAR Data Summary – 1900 MHz GSM Face Position.....	26
SAR Data Summary – 1900 MHz GPRS Body Position	27
Simultaneous Transmission.....	28
12.1 Test Equipment List	29
13.1 Conclusion	30
14.1 References.....	31
Appendix A – System Validation Plots and Data	32
Appendix B – SAR Test Data Plots.....	43
Appendix C – SAR Test Setup Photos	124
Appendix D – Probe Calibration Data Sheets.....	131
Appendix E – Dipole Calibration Data Sheets	172
Appendix F – Phantom Calibration Data Sheets	195

1. Introduction

This measurement report shows compliance of the CardioNet Inc. Model C5 FCC ID: QBI-1012 with FCC Part 2, 1093, ET Docket 93-62 Rules for mobile and portable devices. The FCC have adopted the guidelines for evaluating the environmental effects of radio frequency radiation in ET Docket 93-62 on August 6, 1996 to protect the public and workers from the potential hazards of RF emissions due to FCC regulated portable devices. [1], [6]

The test procedures, as described in ANSI C95.1 – 1999 Standard for Safety Levels with Respect to Human Exposure to Radio Frequency Electromagnetic Fields, 3 kHz to 300 GHz [2], ANSI C95.3 – 2002 Recommended Practice for the Measurement of Potentially Hazardous Electromagnetic Fields [3], FCC OET Bulletin 65 Supp. C – 2001 [4], IEEE Std.1528 – 2003 Recommended Practice [5], and Industry Canada Safety Code 6 Limits of Human Exposure to Radiofrequency Electromagnetic Fields in the Frequency Range from 3kHz to 300 GHz were employed.

SAR Definition [5]

Specific Absorption Rate is defined as the time derivative (rate) of the incremental energy (dW) absorbed by (dissipated in) an incremental mass (dm) contained in a volume element (dV) of a given density (ρ).

$$SAR = \frac{d}{dt} \left(\frac{dW}{dm} \right) = \frac{d}{dt} \left(\frac{dW}{\rho dV} \right)$$

SAR is expressed in units of watts per kilogram (W/kg). SAR can be related to the electric field at a point by

$$SAR = \frac{\sigma |E|^2}{\rho}$$

where:

σ = conductivity of the tissue (S/m)

ρ = mass density of the tissue (kg/m³)

E = rms electric field strength (V/m)

2. SAR Measurement Setup

Robotic System

The measurements are conducted utilizing the ALSAS-10-U automated dosimetric assessment system. The ALSAS-10-U is designed and manufactured by Aprel Laboratories in Nepean, Ontario, Canada. The system utilizes a Robcomm 3 robot manufactured by ThermoCRS located in Michigan USA.

System Hardware

The system consists of a six axis articulated arm, controller for precise probe positioning (0.05 mm repeatability), a power supply, a teach pendent for teaching area scans, near field probe, an IBM Pentium 4™ 2.66 GHz PC with Windows XP Pro™, and custom software developed to enable communications between the robot controller software and the host operating system.

An amplifier is located on the articulated arm, which is isolated from the custom designed end effector and robot arm. The end effector provides the mechanical touch detection functionality and probe connection interface. The amplifier is functionally validated within the manufacturer's site and calibrated at NCL Calibration Laboratories. A Data Acquisition Card (DAC) is used to collect the signal as detected by the isotropic e-field probe. The DAC manufacturer calibrates the DAC to NIST standards. A formal validation is executed using all mechanical and electronic components to prove conformity of the measurement platform as a whole.

System Description

The ALSAS-10-U has been designed to measure devices within the compliance environment to meet all recognized standards. The system also conforms to standards, which are currently being developed by the scientific and manufacturing community.

The course scan resolution is defined by the operator and reflects the requirements of the standard to which the device is being tested. Precise measurements are made within the predefined course scan area and the values are logged.

The user predefines the sample rate for which the measurements are made so as to ensure that the full duty-cycle of a pulse modulation device is covered during the sample. The following algorithm is an example of the function used by the system for linearization of the output for the probe.

$$V_i = U_i + U_i^2 \bullet \frac{cf}{dcpi}$$



The Aprel E-Field probe is evaluated to establish the diode compression point.

A complex algorithm is then used to calculate the values within the measured points down to a resolution of 1mm. The data from this process is then used to provide the co-ordinates from which the cube scan is created for the determination of the 1 g and 10 g averages.

Cube scan averaging consists of a number of complex algorithms, which are used to calculate the one, and ten gram averages. The basis for the cube scan process is centered on the location where the maximum measured SAR value was found. When a secondary peak value is found which is within 60% of the initial peak value, the system will report this back to the operator who can then assess the need for further analysis of both the peak values prior to the one and ten-gram cube scan averaging process. The algorithm consists of 3D cubic Spline, and Lagrange extrapolation to the surface, which form the matrix for calculating the measurement output for the one and ten gram average values. The resolution for the physical scan integral is user defined with a final calculated resolution down to 1mm.

In-depth analysis for the differential of the physical scanning resolution for the cube scan analysis has been carried out, to identify the optimum setting for the probe positioning steps, and this has been determined at 8mm increments on the X, & Y planes. The reduction of the physical step increment increased the time taken for analysis but did not provide a better uncertainty or return on measured values.

The final output from the system provides data for the area scan measurements, physical and splined (1mm resolution) cube scan with physical and calculated values (1mm resolution).

The overall uncertainty for the methodology and algorithms the ALSAS-10-U used during the SAR calculation was evaluated using the data from IEEE 1528 f3 algorithm:

$$f_3(x, y, z) = A \frac{a^2}{\frac{a^2}{4} + x'^2 + y'^2} \left(e^{-\frac{2z}{a}} + \frac{a^2}{2(a + 2z)^2} \right)$$

The probe used during the measurement process has been assessed to provide values for diode compression. These values are calculated during the probe calibration exercise and are used in the mathematical calculations for the assessment of SAR.

E-Field Probe

The E-field probe used by RF Exposure Lab, LLC, has been fully calibrated and assessed for isotropic, and boundary effect. The probe utilizes a triangular sensor arrangement as detailed in the diagram below right.



The SAR is assessed with the probe which moves at a default height of 5mm from the center of the diode, which is mounted to the sensor, to the phantom surface (Z height). The diagram above right shows how the center of the sensor is defined with the location of the diode placed at the center of the dipole. The 5mm default in the Z axis is the optimum height for assessing SAR where the boundary effect is at its least, with the probe located closest to the phantom surface (boundary).

The manufacturer specified precision of the robot is ± 0.05 mm and the precision of the APREL bottom detection device is ± 0.1 mm. These precisions are calibrated and tested in the manufacturing process of the bottom detection device. A constant distance is maintained because the surface of the phantom is dynamically detected for each point. The surface detection algorithm corrects the position of the robot so that the probe rests on the surface of the phantom. The probe is then moved to the measurement location 2.44 mm above the phantom surface resulting in the probe center location to be at 4.0 mm above the phantom surface. Therefore, the probe sensor will be at 4.0 mm above the phantom surface ± 0.1 mm for each SAR location for frequencies below 3 GHz. The probe is moved to the measurement location 1.44 mm above the phantom surface resulting in the probe center location to be at 2.0 mm above the phantom surface. Therefore, the probe sensor will be at 2.0 mm above the phantom surface ± 0.1 mm for each SAR location for frequencies above 3 GHz.

The probe boundary effect compensation cannot be disabled in the ALSAS-10U testing system. The probe tip will always be at least half a probe tip diameter from the phantom surface. For frequencies up to 3 GHz, the probe diameter is 5 mm. With the sensor offset set at 1.54 mm (default setting), the sensor to phantom gap will be 4.0 mm which is greater than half the probe tip diameter. For frequencies greater than 3 GHz, the probe diameter is 3 mm. With the sensor offset set at 0.56 mm (default setting), the sensor to phantom gap will be 3.0 mm which is greater than half the probe tip diameter.

The separation of the first 2 measurement points in the zoom scan is specified in the test setup software. For frequencies below 3 GHz, the user must specify a zoom scan resolution of less than 6 mm in the z-axis to have the first two measurements within 1 cm of the surface. The z-axis is set to 4 mm as shown on each of the data sheets in Appendix B. For frequencies above 3 GHz, the user must specify a zoom scan resolution of less than 3 mm in the z-axis to have the first two measurements within 5 mm of the surface. The z-axis is set to 2 mm as shown on each of the data sheets in Appendix B.

The zoom scan volume for devices ≤ 3 GHz with a cube scan of 5x5x8 yields a volume of $32 \times 32 \times 28$ mm³. For devices >3 GHz and <4.5 GHz, the cube scan of 9x9x9 yields a volume of $32 \times 32 \times 24$ mm³. For devices ≥ 4.5 GHz, the cube scan of 7x7x12 yields a volume of $24 \times 24 \times 22$ mm³.

3. Robot Specifications

Specifications

Positioner:	ThermoCRS, Robot Model: Robocomm 3
Repeatability:	0.05 mm
No. of axis:	6

Data Acquisition Card (DAC) System

Cell Controller

Processor:	Pentium 4™
Clock Speed:	2.66 GHz
Operating System:	Windows XP Pro™

Data Converter

Features:	Signal Amplifier, End Effector, DAC
Software:	ALSAS 10-U Software

E-Field Probe

Model:	Various See Probe Calibration Sheet
Serial Number:	Various See Probe Calibration Sheet
Construction:	Triangular Core Touch Detection System
Frequency:	10MHz to 6GHz

Phantom

Phantom:	Uniphantom, Right Phantom, Left Phantom
----------	---



4. Probe and Dipole Calibration

See Appendix D and E.

5. Phantom & Simulating Tissue Specifications

SAM Phantom



The Aprel system utilizes three separate phantoms. Each phantom for SAR assessment testing is a low loss dielectric shell, with shape and dimensions derived from the anthropomorphic data of the 90th percentile adult male head dimensions as tabulated by the US Army. The SAM phantom shell is bisected along the mid sagittal plane into right and left halves. The perimeter sidewalls of each phantom half is extended to allow filling with liquid to a depth of 15 cm that is sufficient to minimize reflections from the upper surface [5]. See photos in Appendix C.

Brain & Muscle Simulating Mixture Characterization

The brain and muscle mixtures consist of a glycol based chemical and saline solution. The mixture is calibrated to obtain proper dielectric constant (permittivity) and conductivity of the desired tissue. The head tissue dielectric parameters recommended by the IEEE SCC-34/SC-2 have been incorporated in the following tables. Other head and body tissue parameters that have not been specified in P1528 are derived from the issue dielectric parameters computed from the 4-Cole-Cole equations.

Table 5.1 Typical Composition of Ingredients for Tissue

Ingredients	Simulating Tissue	
	450 MHz Brain	450 MHz Muscle
Mixing Percentage		
Water	38.56	51.16
Sugar	56.32	46.78
Salt	3.95	1.49
HEC	0.98	0.52
Bactericide	0.19	0.05
DGBE	0.00	0.00
Dielectric Constant	Target	43.50
Conductivity (S/m)	Target	0.87
		56.70
		0.94

Device Holder



In combination with the SAM phantom, the mounting device enables the rotation of the mounted transmitter in spherical coordinates whereby the rotation point is the ear opening. The devices can easily, accurately, and repeatably be positioned according to the FCC specifications. The device holder can be locked at different phantom locations (left head, right head, and uni-phantom).

6. Definition of Reference Points

Ear Reference Point

Figure 6.2 shows the front, back and side views of the SAM Phantom. The point "M" is the reference point for the center of the mouth, "LE" is the left ear reference point (ERP), and "RE" is the right ERP. The ERPs are 15mm posterior to the entrance to the ear canal (EEC) along the B-M line (Back-Mouth), as shown in Figure 6.1. The plane passing through the two ear canals and M is defined as the Reference Plane. The line N-F (Neck-Front) is perpendicular to the reference plane and passing through the RE (or LE) is called the Reference Pivoting Line (see Figure 6.1). Line B-M is perpendicular to the N-F line. Both N-F and B-M lines are marked on the external phantom shell to facilitate handset positioning [5].

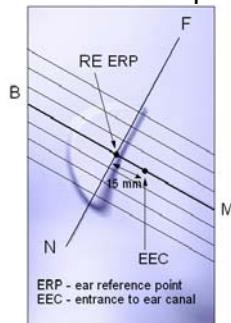


Figure 6.1 Close-up side view of ERP's

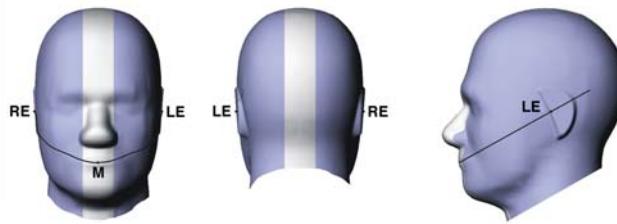


Figure 6.2 Front, back and side view of SAM

Device Reference Points

Two imaginary lines on the device need to be established: the vertical centerline and the horizontal line. The test device is placed in a normal operating position with the "test device reference point" located along the "vertical centerline" on the front of the device aligned to the "ear reference point" (See Fig. 6.3). The "test device reference point" is then located at the same level as the center of the ear reference point. The test device is positioned so that the "vertical centerline" is bisecting the front surface of the device at its top and bottom edges, positioning the "ear reference point" on the outer surface of both the left and right head phantoms on the ear reference point [5].

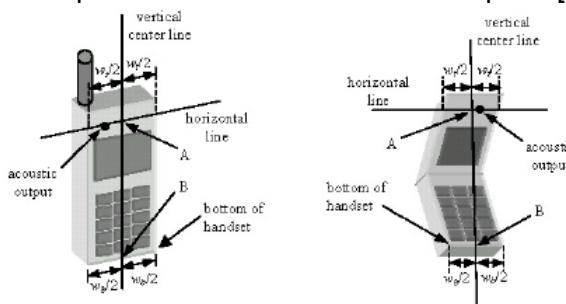


Figure 6.3 Handset Vertical Center & Horizontal Line Reference Points

7. Test Configuration Positions

Positioning for Cheek/Touch [5]

1. Position the device close to the surface of the phantom such that point A is on the (virtual) extension of the line passing through points RE and LE on the phantom (see Figure 7.1), such that the plane defined by the vertical center line and the horizontal line of the device is approximately parallel to the sagittal plane of the phantom.

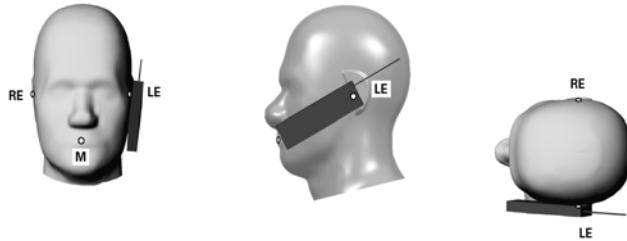


Figure 7.1 Front, Side and Top View of Cheek/Touch Position

2. Translate the device towards the phantom along the line passing through RE and LE until the device touches the ear.
3. While maintaining the device in this plane, rotate it around the LE-RE line until the vertical centerline is in the plane normal to MB-NF including the line MB (called the reference plane).
4. Rotate the device around the vertical centerline until the device (horizontal line) is symmetrical with respect to the line NF.
5. While maintaining the vertical centerline in the reference plane, keeping point A on the line passing through RE and LE and maintaining the device contact with the ear, rotate the device about the line NF until any point on the device is in contact with a phantom point below the ear (cheek). See Figure 7.2.




Figure 7.2 Side view w/ relevant markings

Positioning for Ear / 15° Tilt [5]

With the test device aligned in the Cheek/Touch Position":

1. While maintaining the orientation of the device, retracted the device parallel to the reference plane far enough to enable a rotation of the device by 15 degrees.
2. Rotate the device around the horizontal line by 15 degrees.
3. While maintaining the orientation of the device, move the device parallel to the reference plane until any part of the device touches the head. (In this position, point A is located on the line RE-LE). The tilted position is obtained when the contact is on the pinna. If the contact is at any location other than the pinna, the angle of the device shall be reduced. The tilted position is obtained when any part of the device is in contact with the ear as well as a second part of the device is in contact with the head (see Figure 7.3).

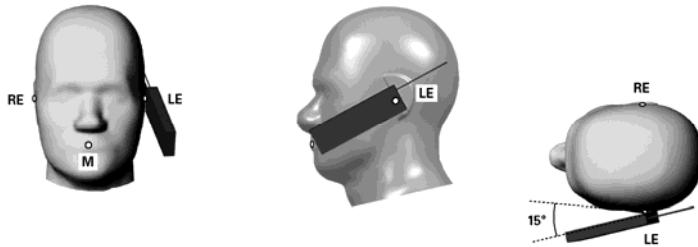


Figure 7.3 Front, Side and Top View of Ear/15° Tilt Position

Body Worn Configurations

Body-worn operating configurations are tested with the accessories attached to the device and positioned against a flat phantom in a normal use configuration. A device with a headset output is tested with a headset connected to the device. Body dielectric parameters are used.

Accessories for Body-worn operation configurations are divided into two categories: those that do not contain metallic components and those that do contain metallic components. When multiple accessories that do not contain metallic components are supplied with the device, the device is tested with only the accessory that dictates the closest spacing to the body. Then, when multiple accessories that contain metallic components are supplied with the device, the device is tested with each accessory that contains a unique metallic component. If multiple accessories share an identical metallic component (i.e. the same metallic belt-clip used with different holsters with no other metallic components) only the accessory that dictates the closest spacing to the body is tested.

Body-worn accessories may not always be supplied or available as options for some devices intended to be authorized for body-worn use. In this case, a test configuration where a separation distance between the back of the device and the flat phantom is used. All test position spacings are documented.

Transmitters that are designed to operate in front of a person's face, as in push-to-talk configurations, are tested for SAR compliance with the front of the device positioned to face the flat phantom. For devices that are carried next to the body such as a shoulder, waist or chest-worn transmitters, SAR compliance is tested with the accessory(ies), including headsets and microphones, attached to the device and positioned against a flat phantom in a normal use configuration.

In all cases SAR measurements are performed to investigate the worst-case positioning. Worst-case positioning is then documented and used to perform Body SAR testing.

In order for users to be aware of the body-worn operating requirements for meeting RF exposure compliance, operating instructions and cautions statements are included in the user's manual.

8. ANSI/IEEE C95.1 – 1999 RF Exposure Limits [2]

Uncontrolled Environment

Uncontrolled Environments are defined as locations where there is the exposure of individuals who have no knowledge or control of their exposure. The general population/uncontrolled exposure limits are applicable to situations in which the general public may be exposed or in which persons who are exposed as a consequence of their employment may not be made fully aware of the potential for exposure or cannot exercise control over their exposure. Members of the general public would come under this category when exposure is not employment-related; for example, in the case of a wireless transmitter that exposes persons in its vicinity.

Controlled Environment

Controlled Environments are defined as locations where there is exposure that may be incurred by persons who are aware of the potential for exposure, (i.e. as a result of employment or occupation). In general, occupational/controlled exposure limits are applicable to situations in which persons are exposed as a consequence of their employment, who have been made fully aware of the potential for exposure and can exercise control over their exposure. This exposure category is also applicable when the exposure is of a transient nature due to incidental passage through a location where the exposure levels may be higher than the general population/uncontrolled limits, but the exposed person is fully aware of the potential for exposure and can exercise control over his or her exposure by leaving the area or by some other appropriate means.

Table 8.1 Human Exposure Limits

	UNCONTROLLED ENVIRONMENT General Population (W/kg) or (mW/g)	CONTROLLED ENVIRONMENT Professional Population (W/kg) or (mW/g)
SPATIAL PEAK SAR ¹ Brain	1.60	8.00
SPATIAL AVERAGE SAR ² Whole Body	0.08	0.40
SPATIAL PEAK SAR ³ Hands, Feet, Ankles, Wrists	4.00	20.00

¹ The Spatial Peak value of the SAR averaged over any 1 gram of tissue (defined as a tissue volume in the shape of a cube) and over the appropriate averaging time.

² The Spatial Average value of the SAR averaged over the whole body.

³ The Spatial Peak value of the SAR averaged over any 10 grams of tissue (defined as a tissue volume in the shape of a cube) and over the appropriate averaging time.

9. Measurement Uncertainty

Exposure Assessment Measurement Uncertainty

Source of Uncertainty	Tolerance Value	Probability Distribution	Divisor	$c_i^1 (1-g)$	$c_i^1 (10-g)$	Standard Uncertainty (1-g) %	Standard Uncertainty (10-g) %
Measurement System							
Probe Calibration	3.5	normal	1	1	1	3.5	3.5
Axial Isotropy	3.7	rectangular	$\sqrt{3}$	$(1 - \frac{1}{cp})^{1/2}$	$(1 - \frac{1}{cp})^{1/2}$	1.5	1.5
Hemispherical Isotropy	10.9	rectangular	$\sqrt{3}$	\sqrt{cp}	\sqrt{cp}	4.4	4.4
Boundary Effect	1.0	rectangular	$\sqrt{3}$	1	1	0.6	0.6
Linearity	4.7	rectangular	$\sqrt{3}$	1	1	2.7	2.7
Detection Limit	1.0	rectangular	$\sqrt{3}$	1	1	0.6	0.6
Readout Electronics	1.0	normal	1	1	1	1.0	1.0
Response Time	0.8	rectangular	$\sqrt{3}$	1	1	0.5	0.5
Integration Time	1.7	rectangular	$\sqrt{3}$	1	1	1.0	1.0
RF Ambient Condition	3.0	rectangular	$\sqrt{3}$	1	1	1.7	1.7
Probe Positioner Mech.	0.4	rectangular	$\sqrt{3}$	1	1	0.2	0.2
Restriction							
Probe Positioning with respect to Phantom Shell	2.9	rectangular	$\sqrt{3}$	1	1	1.7	1.7
Extrapolation and Integration	3.7	rectangular	$\sqrt{3}$	1	1	2.1	2.1
Test Sample Positioning	4.0	normal	1	1	1	4.0	4.0
Device Holder Uncertainty	2.0	normal	1	1	1	2.0	2.0
Drift of Output Power	4.2	rectangular	$\sqrt{3}$	1	1	2.4	2.4
Phantom and Setup							
Phantom Uncertainty (shape & thickness tolerance)	3.4	rectangular	$\sqrt{3}$	1	1	2.0	2.0
Liquid Conductivity (target)	5.0	rectangular	$\sqrt{3}$	0.7	0.5	2.0	1.4
Liquid Conductivity (meas.)	0.5	normal	1	0.7	0.5	0.4	0.3
Liquid Permittivity (target)	5.0	rectangular	$\sqrt{3}$	0.6	0.5	1.7	1.4
Liquid Permittivity (meas.)	1.0	normal	1	0.6	0.5	0.6	0.5
Combined Uncertainty		RSS				9.6	9.4
Combined Uncertainty (coverage factor=2)		Normal (k=2)				19.1	18.8

10. System Validation

Tissue Verification

Table 10.1 Measured Tissue Parameters

		835 MHz Head		835 MHz Body	
Date(s)		Sept. 18, 2009		Sept. 19, 2009	
Liquid Temperature (°C)	20.0	Target	Measured	Target	Measured
Dielectric Constant: ϵ	41.50	41.46	55.20	53.81	
Conductivity: σ	0.90	0.91	0.97	0.98	

		1900 MHz Head		1900 MHz Body	
Date(s)		Sept. 18, 2009		Sept. 18, 2009	
Liquid Temperature (°C)	20.0	Target	Measured	Target	Measured
Dielectric Constant: ϵ	40.00	39.75	53.30	52.73	
Conductivity: σ	1.40	1.42	1.52	1.58	

See Appendix A for data printout.


Test System Verification

Prior to assessment, the system is verified to the $\pm 10\%$ of the specifications at the test frequency by using the system kit. Power is extrapolated to 1 watt. (Graphic Plots Attached)

Table 10.2 System Dipole Validation Target & Measured

	Test Frequency	Targeted SAR _{1g} (W/kg)	Measure SAR _{1g} (W/kg)	Deviation (%)
18-Sep-2009	835 MHz	9.50	9.07	- 4.53
19-Sep-2009	835 MHz	9.75	9.45	- 3.08
18-Sep-2009	1900 MHz	39.38	39.93	+ 1.40

See Appendix A for data plots.

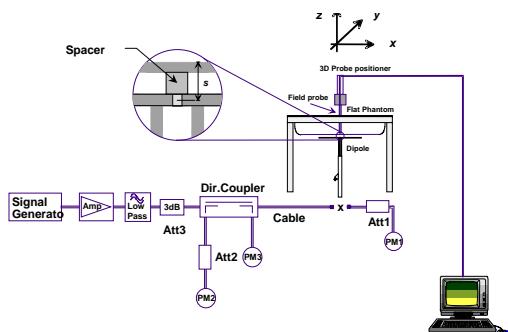
Figure 10.1 Dipole Validation Test Setup

11. SAR Test Data Summary

See Measurement Result Data Pages

See Appendix B for SAR Test Data Plots.

See Appendix C for SAR Test Setup Photos.

Procedures Used To Establish Test Signal

The device was placed into simulated transmit mode using the manufacturer's test codes. Such test signals offer a consistent means for testing SAR and are recommended for evaluating SAR. When test modes are not available or inappropriate for testing a device, the actual transmission is activated through a base station simulator or similar equipment. See data pages for actual procedure used in measurement.

Device Test Condition

In order to verify that the device was tested at full power, conducted output power measurements were performed before and after each SAR measurement to confirm the output power unless otherwise noted. If a conducted power deviation of more than 5% occurred, the test was repeated.

The testing was conducted with the device 2.5 cm face up from the phantom with head tissue in the phantom. The device was also tested with a gap of 10 mm on both the front and back side of the device. Therefore, a belt holster with no metal of at least 10 mm distance from the body.

This device is capable of operating in 850/1900 GSM/GPRS frequency bands. In GSM/GPRS mode, the device is in Class 4 for 850 MHz and Class 1 for 1900 MHz. The GSM/GPRS testing was conducted in the GSM mode for the held to face position and in GPRS mode for the body position. The GPRS mode has 2-slot and 4-slot configurations. The power measured is peak power. The average power in GSM is $\frac{1}{2}$ dB lower than the average power in GPRS 2-slot which is $\frac{1}{2}$ dB higher than 4-slot. Therefore, the device was only tested in the highest power configuration which was 2-slot GPRS for body measurements.

The 1xRTT testing was conducted in RC3 with the device configured using TDSO/SO32 with FCH transmitting at full rate. The power control was set to "All Bits Up." Multiple code channels were not tested due to the conducted power measured was less than $\frac{1}{4}$ dB higher than with FCH only.

12. FCC 3G Measurement Procedures – March 2008

Power measurements were performed using a base station simulator under average power.

12.1 Procedures Used to Establish RF Signal for SAR

The device was placed into a simulated call using a base station simulator in a screen room. Such test signals offer a consistent means for testing SAR and recommended for evaluating SAR. The SAR measurement software calculates a reference point at the start and end of the test to check for power drifts. If conducted power deviations of more than 5% occurred, the tests were repeated.

12.2 SAR Measurement Conditions

12.2.1 Face and Body SAR Measurements

SAR for body exposure configurations is measured in RC3 with the DUT configured using TDSO/SO32, to transmit at full rate on FCH with all other code channels disabled. SAR for multiple code channels (FCH+SCH_n) is not required when the maximum average output of each RF channel is less than 1/4 dB higher than that measured with FCH only. Otherwise, SAR is measured on the maximum output channel (FCH=SCH_n) with FCH at full rate and SCH₀ enabled at 9600 bps, using the exposure configuration that results in the highest SAR with FCH only for that channel. When multiple code channels are enabled, the DUT output may shift by more than 0.5 dB and lead to higher SAR drifts and SCH dropouts.

12.2.2 Output Power Verification 1x RTT

Maximum output power is verified on the High, Middle, and Low channels according to procedures in section 4.4.5.2 of 3 GPP2 C.S0011/TIA-98-E. Results for at least steps 3, 4 and 10 of the power measurement procedures should be tabulated in the SAR report. Steps 3 and 4 should be measured using SO55 with power control bits in “All Up” condition. TDSO / SO32 may be used instead of SO55 for step 4. Step 10 should be measured using TDSO / SO32 with power control bits in the “Bits Hold” condition (i.e. alternative Up/Down Bits). All power measurements defined in C.S0011/TIA-98-E that are inapplicable to the DUT or cannot be measured due to technical or equipment limitations should be clearly identified in the test report.

12.3 SAR Measurement Conditions for GSM

Configure the 8960 box to support GMSK and 8PSK call respectively, and set one timeslot and two timeslot transmission for GMSK GSM/GPRS and 8PSK EDGE. Measure and record power outputs for both modulations.

1xRTT Power Measurements

IS-2000	Channel	SO2 [dBm]	SO2 [dBm]	SO55 [dBm]	SO55 [dBm]	TDSO SO32 FCH Only [dBm]	TDSO SO32 FCH+SCH [dBm]
	F-RC	RC1	RC3	RC1	RC3	RC3	RC3
Band	Vocoder Rate	Full	Full	Full	Full	Full	Full
Cellular	1013	24.52	24.56	24.55	24.61	24.63	24.60
	384	24.59	24.58	24.59	24.60	24.60	24.53
	777	24.63	24.64	24.64	24.66	24.64	24.59
PCS	25	24.59	24.62	24.59	24.63	24.60	24.59
	600	24.46	24.50	24.51	24.45	24.53	24.50
	1175	24.48	24.53	24.56	24.56	24.59	24.54

GSM		
Band	Channel	Power
Cellular	128	32.53
	190	32.98
	251	33.16
PCS	512	29.61
	661	28.83
	810	29.28

GPRS/1 slot		
Band	Channel	Power
Cellular	128	32.46
	190	32.78
	251	32.98
PCS	512	29.43
	661	28.75
	810	29.19

GPRS/2 slot		
Band	Channel	Power
Cellular	128	29.92
	190	30.10
	251	30.56
PCS	512	26.98
	661	26.02
	810	26.85

SAR Data Summary – 835 MHz CDMA Face Position

MEASUREMENT RESULTS									
Gap	Side	Frequency		Modulation	End Power		Service Option	Code Channel	SAR (W/kg)
		MHz	Ch.		(dBm)				
25 mm	Front	824.07	1013	CDMA	24.63	TDSO/SO32	FCH Only	0.329	
		836.52	384	CDMA	24.60	TDSO/SO32	FCH Only	0.523	
		848.31	777	CDMA	24.64	TDSO/SO32	FCH Only	0.573	
					Muscle 1.6 W/kg (mW/g) averaged over 1 gram				

1. Battery is fully charged for all tests.
Power Measured Conducted ERP EIRP
2. SAR Measurement
Phantom Configuration Left Head Uniphantom Right Head
SAR Configuration Head Body
3. Test Signal Call Mode Test Code Base Station Simulator
4. Test Configuration With Belt Clip Without Belt Clip N/A



Jay M. Moulton
Vice President

SAR Data Summary – 835 MHz CDMA Body Position

MEASUREMENT RESULTS								
Gap	Side	Frequency		Modulation	End Power (dBm)	Service Option	Code Channel	SAR (W/kg)
		MHz	Ch.					
10 mm	Front	824.07	1013	CDMA	24.63	TDSO/SO32	FCH Only	0.657
		836.52	384	CDMA	24.60	TDSO/SO32	FCH Only	0.905
		848.31	777	CDMA	24.64	TDSO/SO32	FCH Only	1.017
	Back	824.07	1013	CDMA	24.63	TDSO/SO32	FCH Only	0.843
		836.52	384	CDMA	24.60	TDSO/SO32	FCH Only	1.066
		848.31	777	CDMA	24.64	TDSO/SO32	FCH Only	1.253

Muscle
1.6 W/kg (mW/g)
averaged over 1 gram

1. Battery is fully charged for all tests.
 Power Measured Conducted ERP EIRP
2. SAR Measurement
 Phantom Configuration Left Head Uniphantom Right Head
 SAR Configuration Head Body
3. Test Signal Call Mode Test Code Base Station Simulator
4. Test Configuration With Belt Clip Without Belt Clip N/A



Jay M. Moulton
Vice President

SAR Data Summary – 835 MHz GSM Face Position

MEASUREMENT RESULTS								
Gap	Side	Frequency		Modulation	End Power (dBm)	TX Level	Multislot Configuration	SAR (W/kg)
		MHz	Ch.					
25 mm	Front	824.2	128	GMSK	32.53	0	2 Slot	0.416
		836.6	190	GMSK	32.98	0	2 Slot	0.474
		848.8	251	GMSK	33.16	0	2 Slot	0.514

Muscle
1.6 W/kg (mW/g)
averaged over 1 gram

1. Battery is fully charged for all tests.

Power Measured Conducted ERP EIRP

2. SAR Measurement

Phantom Configuration Left Head Uniphantom Right Head
 SAR Configuration Head Body

3. Test Signal Call Mode

Test Code Base Station Simulator

4. Test Configuration

With Belt Clip Without Belt Clip N/A



Jay M. Moulton
Vice President

SAR Data Summary – 835 MHz GPRS Body Position

MEASUREMENT RESULTS							
Gap	Side	Frequency		Rev Level	End Power (dBm)	TX Level	Multislot Configuration
		MHz	Ch.				
10 mm	Front	824.2	128	GMSK	29.92	0	2 Slot
		836.6	190	GMSK	30.10	0	2 Slot
		848.8	251	GMSK	30.56	0	2 Slot
	Back	824.2	128	GMSK	29.92	0	2 Slot
		836.6	190	GMSK	30.10	0	2 Slot
		848.8	251	GMSK	30.56	0	2 Slot
				Muscle 1.6 W/kg (mW/g) <small>averaged over 1 gram</small>			

1. Battery is fully charged for all tests.
 Power Measured Conducted ERP EIRP
2. SAR Measurement
 Phantom Configuration Left Head Uniphantom Right Head
 SAR Configuration Head Body
3. Test Signal Call Mode Test Code Base Station Simulator
4. Test Configuration With Belt Clip Without Belt Clip N/A



Jay M. Moulton
Vice President

SAR Data Summary – 1900 MHz CDMA Face Position

MEASUREMENT RESULTS								
Gap	Side	Frequency		Modulation	End Power	Service Option	Code Channel	SAR (W/kg)
		MHz	Ch.		(dBm)			
25 mm	Front	1851.25	25	CDMA	24.60	TDSO/SO32	FCH Only	0.269
		1880.00	600	CDMA	24.53	TDSO/SO32	FCH Only	0.224
		1908.75	1175	CDMA	24.59	TDSO/SO32	FCH Only	0.260

Muscle
1.6 W/kg (mW/g)
averaged over 1 gram

1. Battery is fully charged for all tests.

Power Measured Conducted ERP EIRP

2. SAR Measurement

Phantom Configuration Left Head Uniphantom Right Head
 SAR Configuration Head Body

3. Test Signal Call Mode

Test Code Base Station Simulator

4. Test Configuration

With Belt Clip Without Belt Clip N/A



Jay M. Moulton
 Vice President

SAR Data Summary – 1900 MHz CDMA Body Position

MEASUREMENT RESULTS								
Gap	Side	Frequency		Modulation	End Power	Service Option	Code Channel	SAR (W/kg)
		MHz	Ch.		(dBm)			
10 mm	Front	1851.25	25	CDMA	24.60	TDSO/SO32	FCH Only	0.514
		1880.00	600	CDMA	24.53	TDSO/SO32	FCH Only	0.417
		1908.75	1175	CDMA	24.59	TDSO/SO32	FCH Only	0.568
	Back	1851.25	25	CDMA	24.60	TDSO/SO32	FCH Only	0.749
		1880.00	600	CDMA	24.53	TDSO/SO32	FCH Only	0.651
		1908.75	1175	CDMA	24.59	TDSO/SO32	FCH Only	0.897

Muscle
1.6 W/kg (mW/g)
averaged over 1 gram

1. Battery is fully charged for all tests.
 Power Measured Conducted ERP EIRP
2. SAR Measurement
 Phantom Configuration Left Head Uniphantom Right Head
 SAR Configuration Head Body
3. Test Signal Call Mode Test Code Base Station Simulator
4. Test Configuration With Belt Clip Without Belt Clip N/A



Jay M. Moulton
Vice President

SAR Data Summary – 1900 MHz GSM Face Position

MEASUREMENT RESULTS									
Gap	Side	Frequency		Modulation	End Power		TX Level	Multislot Configuration	SAR (W/kg)
		MHz	Ch.		(dBm)				
25 mm	Front	1850.2	512	GMSK	29.61	0	2 Slot	0.252	
		1880.0	661	GMSK	28.83	0	2 Slot	0.234	
		1909.8	810	GMSK	29.28	0	2 Slot	0.205	

Muscle
1.6 W/kg (mW/g)
averaged over 1 gram

1. Battery is fully charged for all tests.

Power Measured Conducted ERP EIRP

2. SAR Measurement

Phantom Configuration Left Head Uniphantom Right Head
 SAR Configuration Head Body

3. Test Signal Call Mode

Test Code Base Station Simulator

4. Test Configuration

With Belt Clip Without Belt Clip N/A



Jay M. Moulton
 Vice President

SAR Data Summary – 1900 MHz GPRS Body Position

MEASUREMENT RESULTS								
Gap	Side	Frequency		Rev Level	End Power (dBm)	TX Level	Multislot Configuration	SAR (W/kg)
		MHz	Ch.					
10 mm	Front	1850.2	512	GMSK	26.98	0	2 Slot	0.580
		1880.0	661	GMSK	26.02	0	2 Slot	0.527
		1909.8	810	GMSK	26.85	0	2 Slot	0.434
	Back	1850.2	512	GMSK	26.98	0	2 Slot	0.882
		1880.0	661	GMSK	26.02	0	2 Slot	0.794
		1909.8	810	GMSK	26.85	0	2 Slot	0.654

Muscle
1.6 W/kg (mW/g)
averaged over 1 gram

1. Battery is fully charged for all tests.

Power Measured Conducted ERP EIRP

2. SAR Measurement

Phantom Configuration Left Head Uniphantom Right Head
 SAR Configuration Head Body

3. Test Signal Call Mode

Test Code Base Station Simulator

4. Test Configuration

With Belt Clip Without Belt Clip N/A



Jay M. Moulton
Vice President

Simultaneous Transmission

The DTS band transmits at a maximum of +10 dB (10 mW). The Bluetooth transmitter transmits at a maximum of +6 dB(4 mW). The distance between the cellular antenna and the BT & DTS antennas is 10 cm. The distance between the DTS and BT antenna is 4.5 cm. Per KDB 648474 3), the DTS and BT transmitters as a stand-alone transmitter does not require any SAR testing for use in portable conditions as the source-based time-averaged output power is $\leq 60/f_{(\text{GHz})}$ (67 mW and 25 mW, respectively). Per KDB 648474 4), SAR is not required for simultaneous transmission for this device.

12.1 Test Equipment List

Table 12.1 Equipment Specifications

Type	Calibration Due Date	Serial Number
ThermoCRS Robot	N/A	RAF0338198
ThermoCRS Controller	N/A	RCF0338224
ThermoCRS Teach Pendant (Joystick)	N/A	STP0334405
IBM Computer, 2.66 MHz P4	N/A	8189D8U KCPR08N
Aprel E-Field Probe ALS-E020	11/03/2009	RFE-215
Aprel Dummy Probe	N/A	023
Aprel Left Phantom	N/A	RFE-267
Aprel Right Phantom	N/A	RFE-268
Aprel UniPhantom	N/A	RFE-273
Aprel Validation Dipole ALS-D-450-S-2	06/01/2011	RFE-362
Aprel Validation Dipole ALS-D-835-S-2	02/22/2010	RFE-274
Aprel Validation Dipole ALS-D-1900-S-2	02/21/2010	RFE-277
Aprel Validation Dipole ALS-D-2450-S-2	02/20/2010	RFE-278
Agilent (HP) 437B Power Meter	12/01/2009	3125U08837
Agilent (HP) 8481B Power Sensor	12/02/2009	3318A05384
Advantest R3261A Spectrum Analyzer	12/02/2009	31720068
Agilent (HP) 8350B Signal Generator	12/01/2009	2749A10226
Agilent (HP) 83525A RF Plug-In	12/01/2009	2647A01172
Agilent (HP) 8753C Vector Network Analyzer	12/01/2009	3135A01724
Agilent (HP) 85047A S-Parameter Test Set	12/01/2009	2904A00595
Agilent (HP) E55125C Base Station Sim.	10/30/2010	MY48360364
Aprel Dielectric Probe Assembly	N/A	0011
Brain Equivalent Matter (450 MHz)	N/A	N/A
Brain Equivalent Matter (835 MHz)	N/A	N/A
Brain Equivalent Matter (1900 MHz)	N/A	N/A
Brain Equivalent Matter (2450 MHz)	N/A	N/A
Muscle Equivalent Matter (450 MHz)	N/A	N/A
Muscle Equivalent Matter (835 MHz)	N/A	N/A
Muscle Equivalent Matter (1900 MHz)	N/A	N/A
Muscle Equivalent Matter (2450 MHz)	N/A	N/A
Muscle Equivalent Matter (5200 MHz)	N/A	N/A
Muscle Equivalent Matter (5800 MHz)	N/A	N/A

13.1 Conclusion

The SAR measurement indicates that the EUT complies with the RF radiation exposure limits of the FCC. These measurements are taken to simulate the RF effects exposure under worst-case conditions. Precise laboratory measures were taken to assure repeatability of the tests. The tested device complies with the requirements in respect to all parameters subject to the test. The test results and statements relate only to the item(s) tested.

Please note that the absorption and distribution of electromagnetic energy in the body is a very complex phenomena that depends on the mass, shape, and size of the body; the orientation of the body with respect to the field vectors; and, the electrical properties of both the body and the environment. Other variables that may play a substantial role in possible biological effects are those that characterize the environment (e.g. ambient temperature, air velocity, relative humidity, and body insulation) and those that characterize the individual (e.g. age, gender, activity level, debilitation, or disease). Because innumerable factors may interact to determine the specific biological outcome of an exposure to electromagnetic fields, any protection guide shall consider maximal amplification of biological effects as a result of field-body interactions, environmental conditions, and physiological variables. [3]

14.1 References

- [1] Federal Communications Commission, ET Docket 93-62, Guidelines for Evaluating the Environmental Effects of Radio Frequency Radiation, August 1996
- [2] ANSI/IEEE C95.1 – 1999, American National Standard Safety Levels with respect to Human Exposure to Radio Frequency Electromagnetic Fields, 300kHz to 100GHz, New York: IEEE, 1992.
- [3] ANSI/IEEE C95.3 – 2002, IEEE Recommended Practice for the Measurement of Potentially Hazardous Electromagnetic Fields – RF and Microwave, New York: IEEE, 1992.
- [4] Federal Communications Commission, OET Bulletin 65 (Edition 97-01), Supplement C (Edition 01-01), Evaluating Compliance with FCC Guidelines for Human Exposure to Radio Frequency Electromagnetic Fields, July 2001.
- [5] IEEE Standard 1528 – 2003, IEEE Recommended Practice for Determining the Peak-Spatial Average Specific Absorption Rate (SAR) in the Human Head from Wireless Communication Devices: Measurement Techniques, October 2003.
- [6] Industry Canada, RSS – 102e, Radio Frequency Exposure Compliance of Radiocommunication Apparatus (All Frequency Bands), November 2005.
- [7] Industry Canada, Safety Code 6, Limits of Human Exposure to Radiofrequency Electromagnetic Fields in the Frequency Range from 3kHz to 300 GHz, 1999.

Appendix A – System Validation Plots and Data

```
*****
Test Result for UIM Dielectric Parameter
Fri 18/Sep/2009 06:51:42
Freq  Frequency(GHz)
FCC_eH      FCC Bulletin 65 Supplement C ( June 2001) Limits for Head Epsilon
FCC_sH      FCC Bulletin 65 Supplement C (June 2001) Limits for Head Sigma
FCC_eB      FCC Limits for Body Epsilon
FCC_sB      FCC Limits for Body Sigma
Test_e      Epsilon of UIM
Test_s      Sigma of UIM
*****
Freq      FCC_eH      FCC_sH      Test_e      Test_s
0.8050    41.66      0.90       41.68      0.88
0.8150    41.60      0.90       41.60      0.89
0.8250    41.55      0.90       41.53      0.90
0.8350    41.50      0.90       41.46      0.91
0.8450    41.50      0.91       41.37      0.92
0.8550    41.50      0.92       41.31      0.93
0.8650    41.50      0.93       41.26      0.94
```

```
*****
Test Result for UIM Dielectric Parameter
Sat 19/Sep/2009 07:46:23
Freq  Frequency(GHz)
FCC_eH      FCC Bulletin 65 Supplement C ( June 2001) Limits for Head Epsilon
FCC_sH      FCC Bulletin 65 Supplement C (June 2001) Limits for Head Sigma
FCC_eB      FCC Limits for Body Epsilon
FCC_sB      FCC Limits for Body Sigma
Test_e      Epsilon of UIM
Test_s      Sigma of UIM
*****
Freq      FCC_eB      FCC_sB      Test_e      Test_s
0.8050    55.32      0.97       53.89      0.94
0.8150    55.28      0.97       53.85      0.94
0.8250    55.24      0.97       53.83      0.95
0.8350    55.20      0.97       53.81      0.98
0.8450    55.17      0.98       53.77      0.99
0.8550    55.14      0.99       53.75      1.01
0.8650    55.11      1.01       53.76      1.02
```

Test Result for UIM Dielectric Parameter
Fri 18/Sep/2009 07:44:23
Freq Frequency(GHz)
FCC_eH FCC Bulletin 65 Supplement C (June 2001) Limits for Head Epsilon
FCC_sH FCC Bulletin 65 Supplement C (June 2001) Limits for Head Sigma
Test_e Epsilon of UIM
Test_s Sigma of UIM

Freq	FCC_eH	FCC_sH	Test_e	Test_s
1.8700	40.00	1.40	39.86	1.39
1.8800	40.00	1.40	39.82	1.40
1.8900	40.00	1.40	39.78	1.41
1.9000	40.00	1.40	39.75	1.42
1.9100	40.00	1.40	39.69	1.43
1.9200	40.00	1.40	39.62	1.44
1.9300	40.00	1.40	39.57	1.45

Test Result for UIM Dielectric Parameter
Fri 18/Sep/2009 07:54:10
Freq Frequency(GHz)
FCC_eH FCC Bulletin 65 Supplement C (June 2001) Limits for Head Epsilon
FCC_sH FCC Bulletin 65 Supplement C (June 2001) Limits for Head Sigma
FCC_eB FCC Limits for Body Epsilon
FCC_sB FCC Limits for Body Sigma
Test_e Epsilon of UIM
Test_s Sigma of UIM

Freq	FCC_eB	FCC_sB	Test_e	Test_s
1.8700	53.30	1.52	52.92	1.51
1.8800	53.30	1.52	52.84	1.53
1.8900	53.30	1.52	52.82	1.55
1.9000	53.30	1.52	52.73	1.58
1.9100	53.30	1.52	52.72	1.59
1.9200	53.30	1.52	52.67	1.62
1.9300	53.30	1.52	52.66	1.64

SAR Test Report

By Operator : Jay
Measurement Date : 18-Sep-2009
Starting Time : 18-Sep-2009 06:55:41 AM
End Time : 18-Sep-2009 07:10:49 AM
Scanning Time : 908 secs

Product Data

Device Name : Validation
Serial No. : 835
Type : Dipole
Model : ALS-D-835-S-2
Frequency : 835.00 MHz
Max. Transmit Pwr : 0.1 W
Drift Time : 0 min(s)
Length : 161 mm
Width : 3.6 mm
Depth : 89.8 mm
Antenna Type : Internal
Orientation : Touch
Power Drift-Start : 0.999 W/kg
Power Drift-Finish: 0.972 W/kg
Power Drift (%) : -2.646

Phantom Data

Name : APREL-Uni
Type : Uni-Phantom
Size (mm) : 280 x 280 x 200
Serial No. : System Default
Location : Center
Description : Uni-Phantom

Tissue Data

Type : HEAD
Serial No. : 835
Frequency : 835.00 MHz
Last Calib. Date : 18-Sep-2009
Temperature : 20.00 °C
Ambient Temp. : 23.00 °C
Humidity : 49.00 RH%
Epsilon : 41.46 F/m
Sigma : 0.91 S/m
Density : 1000.00 kg/cu. m

Probe Data


Name : Probe 215 - RFEL
Model : E020
Type : E-Field Triangle
Serial No. : 215
Last Calib. Date : 03-Nov-2008
Frequency : 835.00 MHz
Duty Cycle Factor: 1
Conversion Factor: 6.2
Probe Sensitivity: 1.20 1.20 1.20 μ V/ (V/m)²
Compression Point: 95.00 mV
Offset : 1.56 mm

Measurement Data

Crest Factor : 1
Scan Type : Complete
Tissue Temp. : 20.00 °C
Ambient Temp. : 25.00 °C
Set-up Date : 18-Sep-2009
Set-up Time : 9:21:48 AM
Area Scan : 5x7x1 : Measurement x=10mm, y=10mm, z=4mm
Zoom Scan : 5x5x8 : Measurement x=8mm, y=8mm, z=4mm


Other Data

DUT Position : Touch
Separation : 15 mm
Channel : Mid

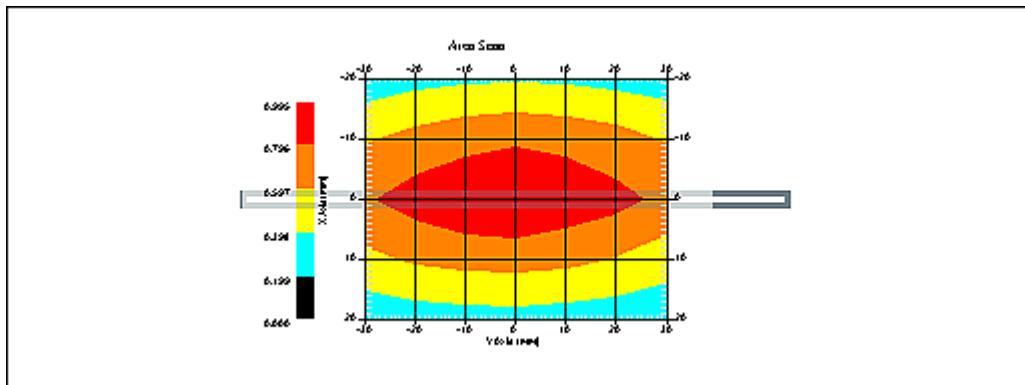

1 gram SAR value : 0.907 W/kg
10 gram SAR value : 0.570 W/kg
Area Scan Peak SAR : 0.994 W/kg
Zoom Scan Peak SAR : 1.341 W/kg

SAR-Z Axis
at Hotspot x:0.22 y:-0.17

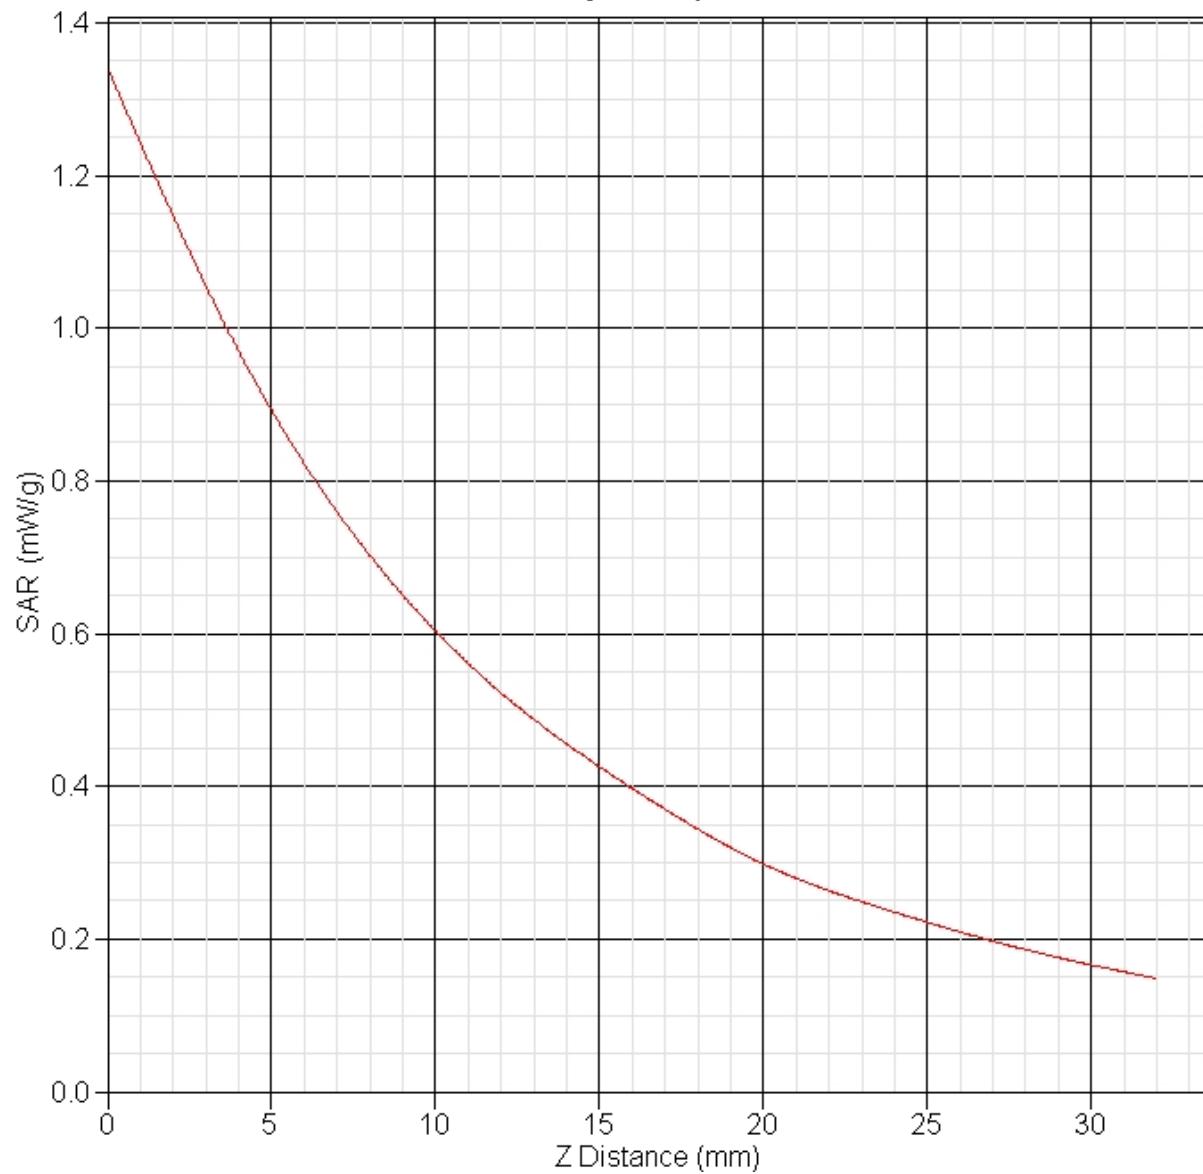

SAR Test Report

By Operator : Jay
Measurement Date : 19-Sep-2009
Starting Time : 19-Sep-2009 07:49:30 AM
End Time : 19-Sep-2009 08:04:35 AM
Scanning Time : 905 secs

Product Data

Device Name : Validation
Serial No. : 835
Type : Dipole
Model : ALS-D-835-S-2
Frequency : 835.00 MHz
Max. Transmit Pwr : 0.1 W
Drift Time : 0 min(s)
Length : 161 mm
Width : 3.6 mm
Depth : 89.8 mm
Antenna Type : Internal
Orientation : Touch
Power Drift-Start : 1.026 W/kg
Power Drift-Finish: 1.035 W/kg
Power Drift (%) : 0.881

Phantom Data

Name : APREL-Uni
Type : Uni-Phantom
Size (mm) : 280 x 280 x 200
Serial No. : System Default
Location : Center
Description : Uni-Phantom

Tissue Data

Type : BODY
Serial No. : 835
Frequency : 835.00 MHz
Last Calib. Date : 19-Sep-2009
Temperature : 20.00 °C
Ambient Temp. : 23.00 °C
Humidity : 49.00 RH%
Epsilon : 53.81 F/m
Sigma : 0.98 S/m
Density : 1000.00 kg/cu. m

Probe Data


Name : Probe 215 - RFEL
Model : E020
Type : E-Field Triangle
Serial No. : 215
Last Calib. Date : 03-Nov-2008
Frequency : 835.00 MHz
Duty Cycle Factor: 1
Conversion Factor: 6.3
Probe Sensitivity: 1.20 1.20 1.20 μ V/ (V/m)²
Compression Point: 95.00 mV
Offset : 1.56 mm

Measurement Data

Crest Factor : 1
Scan Type : Complete
Tissue Temp. : 20.00 °C
Ambient Temp. : 25.00 °C
Set-up Date : 19-Sep-2009
Set-up Time : 9:21:48 AM
Area Scan : 5x7x1 : Measurement x=10mm, y=10mm, z=4mm
Zoom Scan : 5x5x8 : Measurement x=8mm, y=8mm, z=4mm


Other Data

DUT Position : Touch
Separation : 15 mm
Channel : Mid

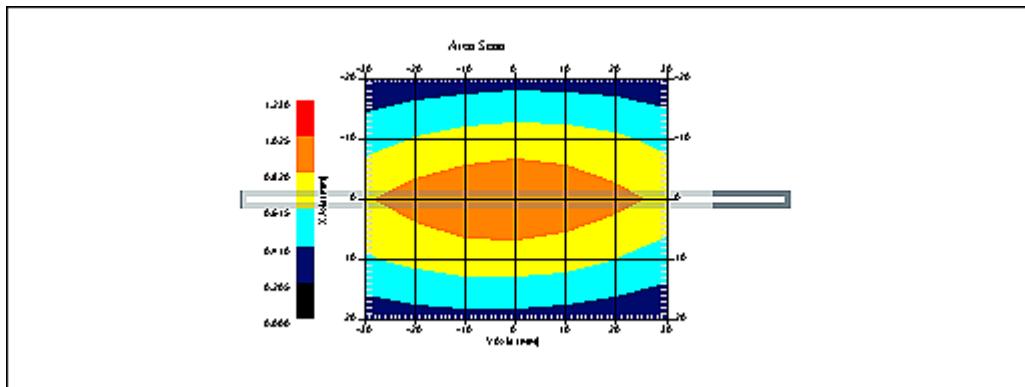

1 gram SAR value : 0.945 W/kg
10 gram SAR value : 0.598 W/kg
Area Scan Peak SAR : 1.026 W/kg
Zoom Scan Peak SAR : 1.451 W/kg

SAR-Z Axis
at Hotspot x:0.25 y:-0.13

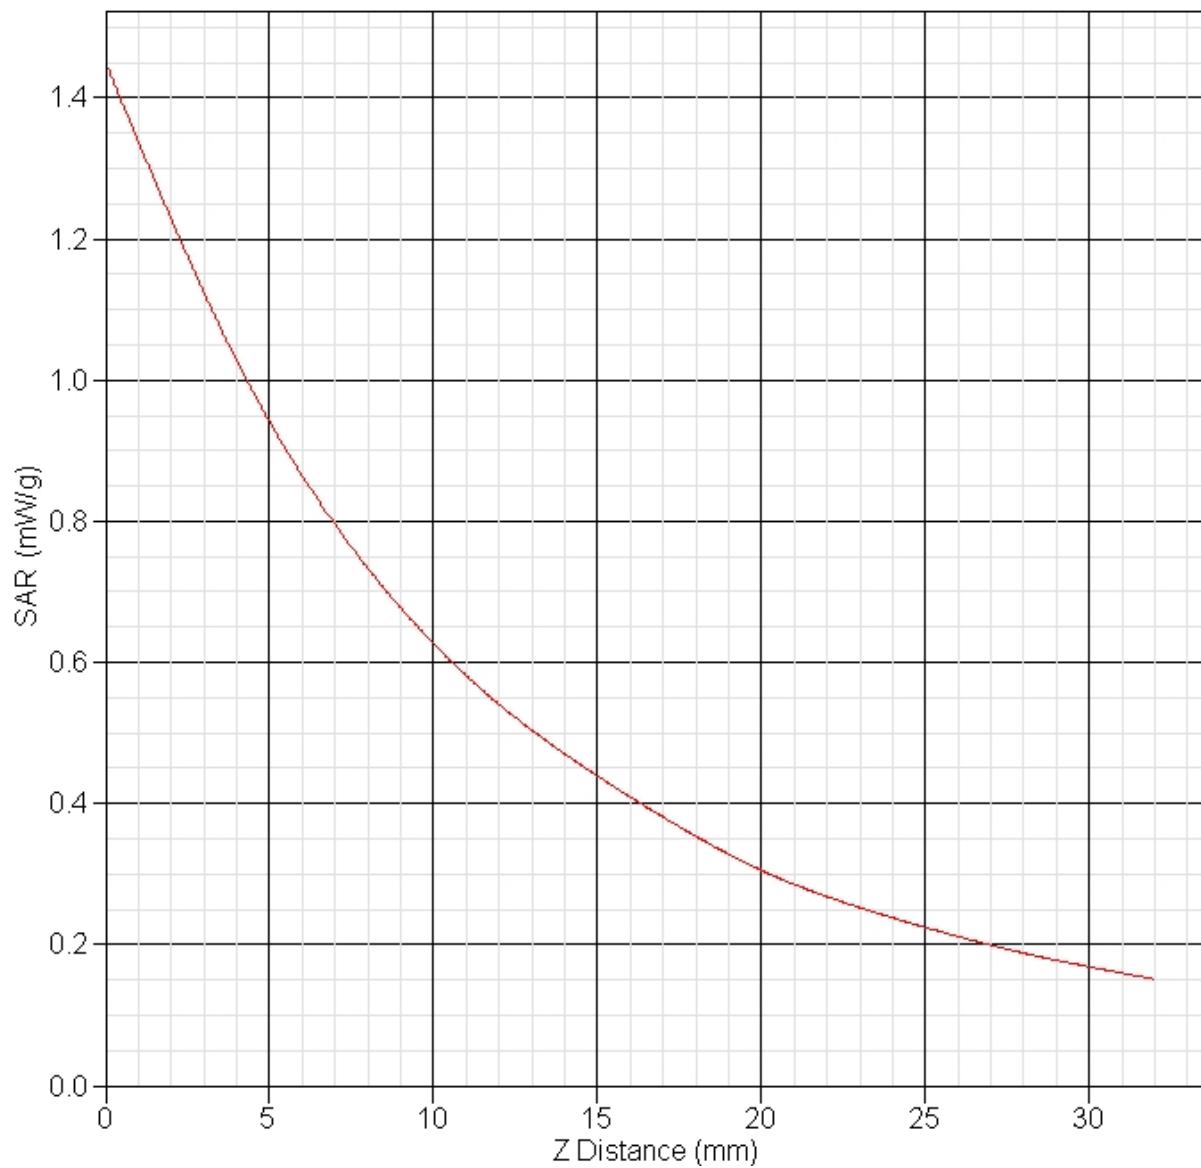

SAR Test Report

By Operator : Jay
Measurement Date : 18-Sep-2009
Starting Time : 18-Sep-2009 07:49:22 AM
End Time : 18-Sep-2009 08:02:21 AM
Scanning Time : 779 secs

Product Data

Device Name : Validation
Serial No. : 1900
Type : Dipole
Model : ALS-D-1900-S-2
Frequency : 1900.00 MHz
Max. Transmit Pwr : 0.1 W
Drift Time : 0 min(s)
Length : 68 mm
Width : 3.6 mm
Depth : 39.5 mm
Antenna Type : Internal
Orientation : Touch
Power Drift-Start : 4.552 W/kg
Power Drift-Finish: 4.532 W/kg
Power Drift (%) : -0.448

Phantom Data

Name : APREL-Uni
Type : Uni-Phantom
Size (mm) : 280 x 280 x 200
Serial No. : System Default
Location : Center
Description : Uni-Phantom

Tissue Data

Type : HEAD
Serial No. : 1900
Frequency : 1900.00 MHz
Last Calib. Date : 18-Sep-2009
Temperature : 20.00 °C
Ambient Temp. : 23.00 °C
Humidity : 49.00 RH%
Epsilon : 39.75 F/m
Sigma : 1.42 S/m
Density : 1000.00 kg/cu. m

Probe Data


Name : Probe 215 - RFEL
Model : E020
Type : E-Field Triangle
Serial No. : 215
Last Calib. Date : 03-Nov-2008
Frequency : 1900.00 MHz
Duty Cycle Factor: 1
Conversion Factor: 4.9
Probe Sensitivity: 1.20 1.20 1.20 μ V/ (V/m)²
Compression Point: 95.00 mV
Offset : 1.56 mm

Measurement Data

Crest Factor : 1
Scan Type : Complete
Tissue Temp. : 20.00 °C
Ambient Temp. : 23.00 °C
Set-up Date : 18-Sep-2009
Set-up Time : 8:39:41 AM
Area Scan : 5x5x1 : Measurement x=10mm, y=10mm, z=4mm
Zoom Scan : 5x5x8 : Measurement x=8mm, y=8mm, z=4mm


Other Data

DUT Position : Touch
Separation : 10 mm
Channel : Mid

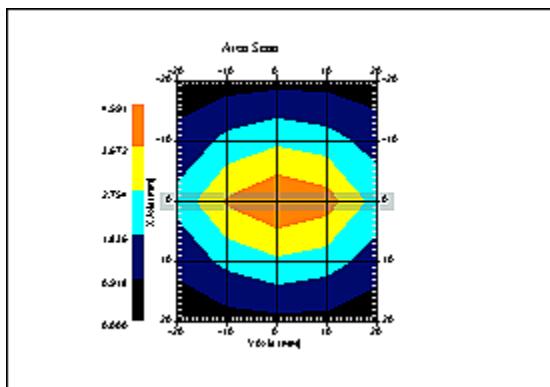

1 gram SAR value : 3.993 W/kg
10 gram SAR value : 2.076 W/kg
Area Scan Peak SAR : 4.591 W/kg
Zoom Scan Peak SAR : 7.066 W/kg

SAR-Z Axis
at Hotspot x:0.22 y:-0.14

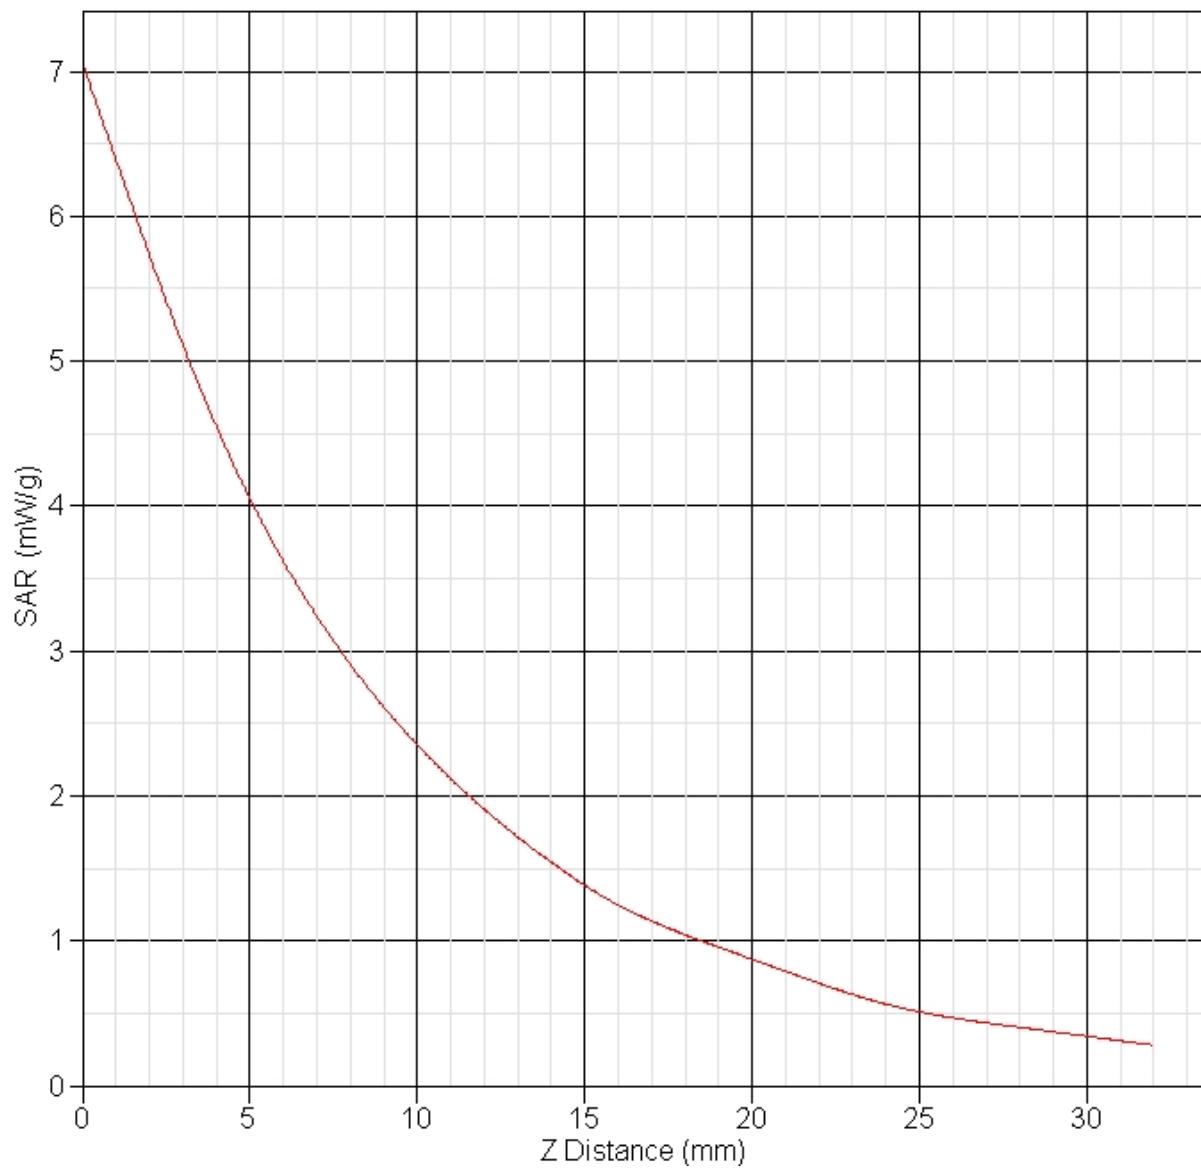

Appendix B – SAR Test Data Plots

SAR Test Report

By Operator : Jay
Measurement Date : 18-Sep-2009
Starting Time : 18-Sep-2009 06:09:13 PM
End Time : 18-Sep-2009 06:25:27 PM
Scanning Time : 974 secs

Product Data

Device Name : CardioNet
Serial No. : Eng 1
Mode : EvDo Rev. 0
Model : C5
Frequency : 850.00 MHz
Max. Transmit Pwr : 0.25 W
Drift Time : 0 min(s)
Length : 117 mm
Width : 64 mm
Depth : 23 mm
Antenna Type : Internal
Orientation : Held To Face
Power Drift-Start : 0.284 W/kg
Power Drift-Finish: 0.295 W/kg
Power Drift (%) : 3.735

Phantom Data

Name : APREL-Uni
Type : Uni-Phantom
Size (mm) : 280 x 280 x 200
Serial No. : System Default
Location : Center
Description : Uni-Phantom

Tissue Data

Type : HEAD
Serial No. : 835
Frequency : 835.00 MHz
Last Calib. Date : 18-Sep-2009
Temperature : 20.00 °C
Ambient Temp. : 23.00 °C
Humidity : 40.00 RH%
Epsilon : 41.46 F/m
Sigma : 0.91 S/m
Density : 1000.00 kg/cu. m

Probe Data


Name : Probe 215 - RFEL
Model : E020
Type : E-Field Triangle
Serial No. : 215
Last Calib. Date : 03-Nov-2008
Frequency : 835.00 MHz
Duty Cycle Factor: 1
Conversion Factor: 6.2
Probe Sensitivity: 1.20 1.20 1.20 μ V/ (V/m)²
Compression Point: 95.00 mV
Offset : 1.56 mm

Measurement Data

Crest Factor : 1
 Scan Type : Complete
 Tissue Temp. : 20.00 °C
 Ambient Temp. : 23.00 °C
 Set-up Date : 18-Sep-2009
 Set-up Time : 4:45:39 PM
 Area Scan : 6x7x1 : Measurement x=15mm, y=15mm, z=4mm
 Zoom Scan : 5x5x8 : Measurement x=8mm, y=8mm, z=4mm

Other Data

DUT Position : Held To Face
 Separation : 25 mm
 Channel : Low

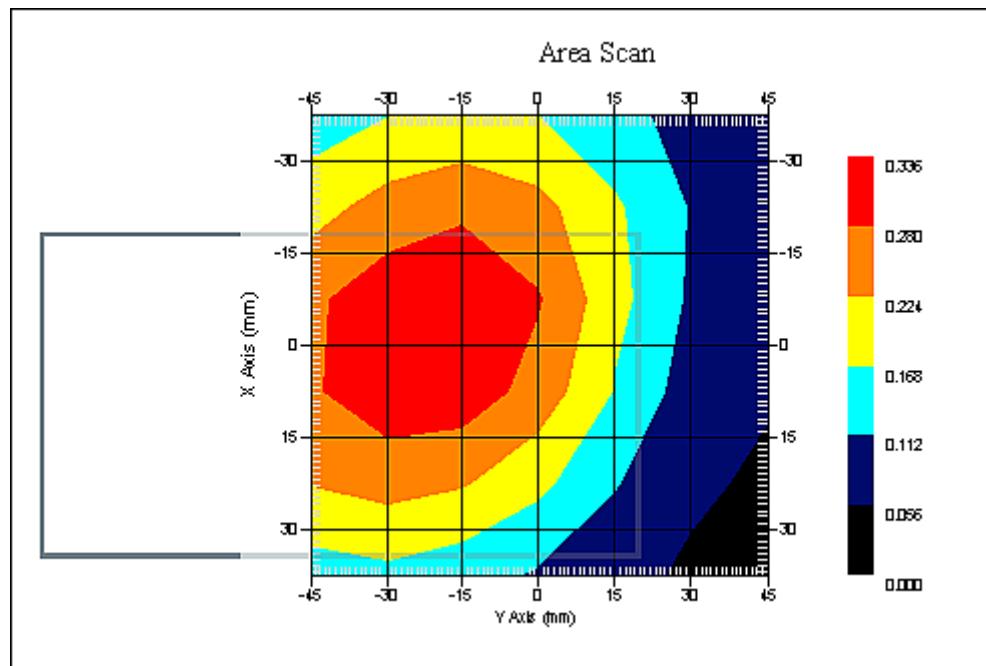

1 gram SAR value : 0.329 W/kg
 10 gram SAR value : 0.242 W/kg
 Area Scan Peak SAR : 0.336 W/kg
 Zoom Scan Peak SAR : 0.420 W/kg

SAR Test Report

By Operator : Jay
Measurement Date : 18-Sep-2009
Starting Time : 18-Sep-2009 05:51:53 PM
End Time : 18-Sep-2009 06:08:03 PM
Scanning Time : 970 secs

Product Data

Device Name : CardioNet
Serial No. : Eng 1
Mode : EvDo Rev. 0
Model : C5
Frequency : 850.00 MHz
Max. Transmit Pwr : 0.25 W
Drift Time : 0 min(s)
Length : 117 mm
Width : 64 mm
Depth : 23 mm
Antenna Type : Internal
Orientation : Held To Face
Power Drift-Start : 0.469 W/kg
Power Drift-Finish: 0.467 W/kg
Power Drift (%) : -0.428

Phantom Data

Name : APREL-Uni
Type : Uni-Phantom
Size (mm) : 280 x 280 x 200
Serial No. : System Default
Location : Center
Description : Uni-Phantom

Tissue Data

Type : HEAD
Serial No. : 835
Frequency : 835.00 MHz
Last Calib. Date : 18-Sep-2009
Temperature : 20.00 °C
Ambient Temp. : 23.00 °C
Humidity : 40.00 RH%
Epsilon : 41.46 F/m
Sigma : 0.91 S/m
Density : 1000.00 kg/cu. m

Probe Data


Name : Probe 215 - RFEL
Model : E020
Type : E-Field Triangle
Serial No. : 215
Last Calib. Date : 03-Nov-2008
Frequency : 835.00 MHz
Duty Cycle Factor: 1
Conversion Factor: 6.2
Probe Sensitivity: 1.20 1.20 1.20 μ V/ (V/m)²
Compression Point: 95.00 mV
Offset : 1.56 mm

Measurement Data

Crest Factor : 1
 Scan Type : Complete
 Tissue Temp. : 20.00 °C
 Ambient Temp. : 23.00 °C
 Set-up Date : 18-Sep-2009
 Set-up Time : 4:45:39 PM
 Area Scan : 6x7x1 : Measurement x=15mm, y=15mm, z=4mm
 Zoom Scan : 5x5x8 : Measurement x=8mm, y=8mm, z=4mm

Other Data

DUT Position : Held To Face
 Separation : 25 mm
 Channel : Mid

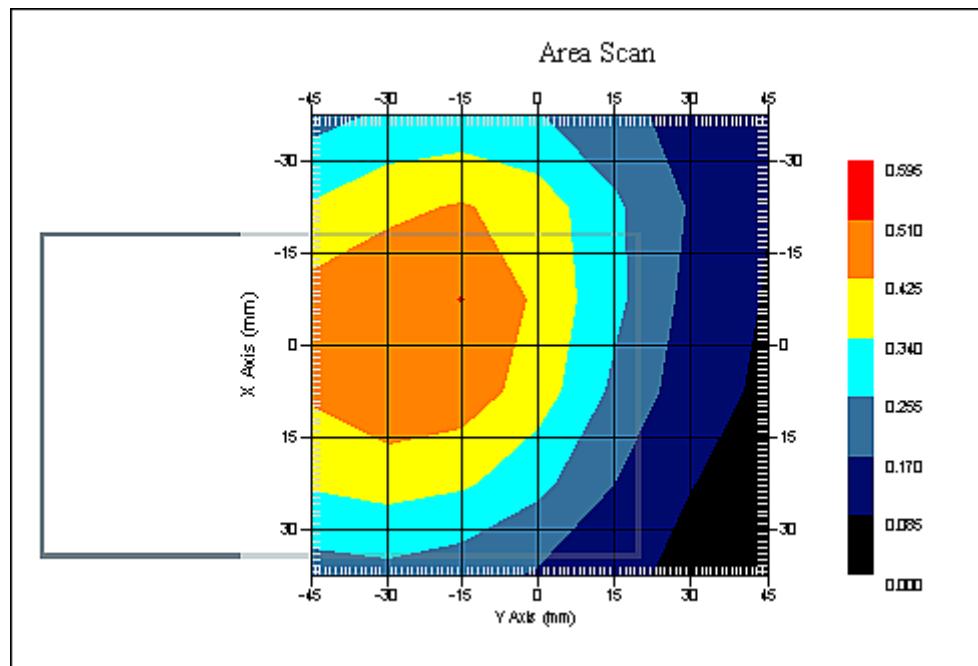

1 gram SAR value : 0.523 W/kg
 10 gram SAR value : 0.376 W/kg
 Area Scan Peak SAR : 0.512 W/kg
 Zoom Scan Peak SAR : 0.720 W/kg

SAR Test Report

By Operator : Jay
Measurement Date : 18-Sep-2009
Starting Time : 18-Sep-2009 06:43:00 PM
End Time : 18-Sep-2009 06:59:14 PM
Scanning Time : 974 secs

Product Data

Device Name : CardioNet
Serial No. : Eng 1
Mode : EvDo Rev. 0
Model : C5
Frequency : 850.00 MHz
Max. Transmit Pwr : 0.25 W
Drift Time : 0 min(s)
Length : 117 mm
Width : 64 mm
Depth : 23 mm
Antenna Type : Internal
Orientation : Held To Face
Power Drift-Start : 0.513 W/kg
Power Drift-Finish: 0.516 W/kg
Power Drift (%) : 0.588

Phantom Data

Name : APREL-Uni
Type : Uni-Phantom
Size (mm) : 280 x 280 x 200
Serial No. : System Default
Location : Center
Description : Uni-Phantom

Tissue Data

Type : HEAD
Serial No. : 835
Frequency : 835.00 MHz
Last Calib. Date : 18-Sep-2009
Temperature : 20.00 °C
Ambient Temp. : 23.00 °C
Humidity : 40.00 RH%
Epsilon : 41.46 F/m
Sigma : 0.91 S/m
Density : 1000.00 kg/cu. m

Probe Data


Name : Probe 215 - RFEL
Model : E020
Type : E-Field Triangle
Serial No. : 215
Last Calib. Date : 03-Nov-2008
Frequency : 835.00 MHz
Duty Cycle Factor: 1
Conversion Factor: 6.2
Probe Sensitivity: 1.20 1.20 1.20 μ V/ (V/m)²
Compression Point: 95.00 mV
Offset : 1.56 mm

Measurement Data

Crest Factor : 1
 Scan Type : Complete
 Tissue Temp. : 20.00 °C
 Ambient Temp. : 23.00 °C
 Set-up Date : 18-Sep-2009
 Set-up Time : 4:45:39 PM
 Area Scan : 6x7x1 : Measurement x=15mm, y=15mm, z=4mm
 Zoom Scan : 5x5x8 : Measurement x=8mm, y=8mm, z=4mm


Other Data

DUT Position : Held To Face
 Separation : 25 mm
 Channel : High

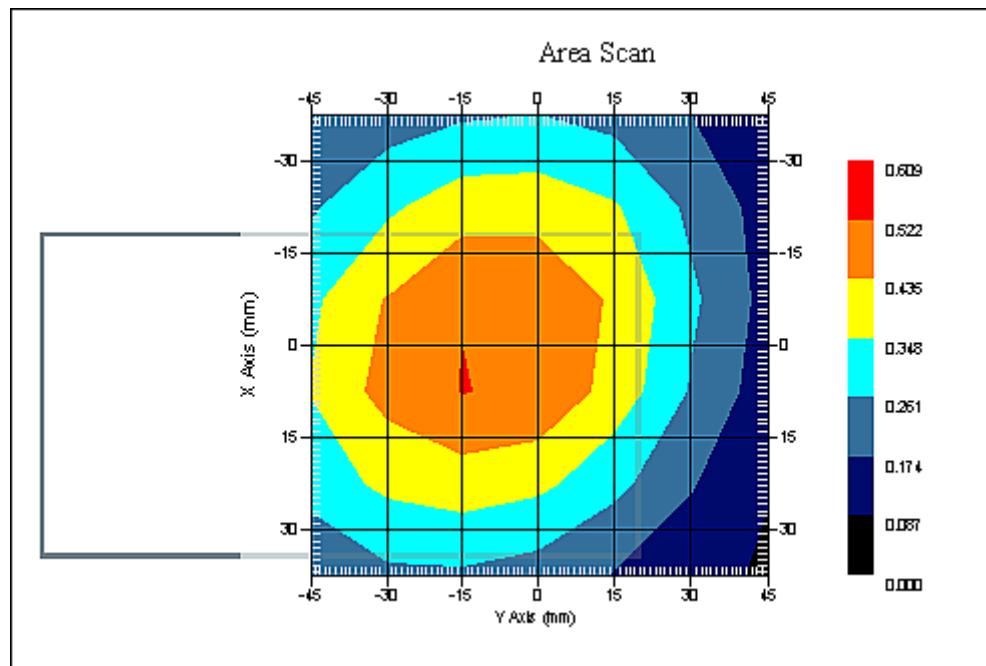

1 gram SAR value : 0.573 W/kg
 10 gram SAR value : 0.414 W/kg
 Area Scan Peak SAR : 0.524 W/kg
 Zoom Scan Peak SAR : 0.800 W/kg

SAR-Z Axis
at Hotspot x:7.05 y:-15.16

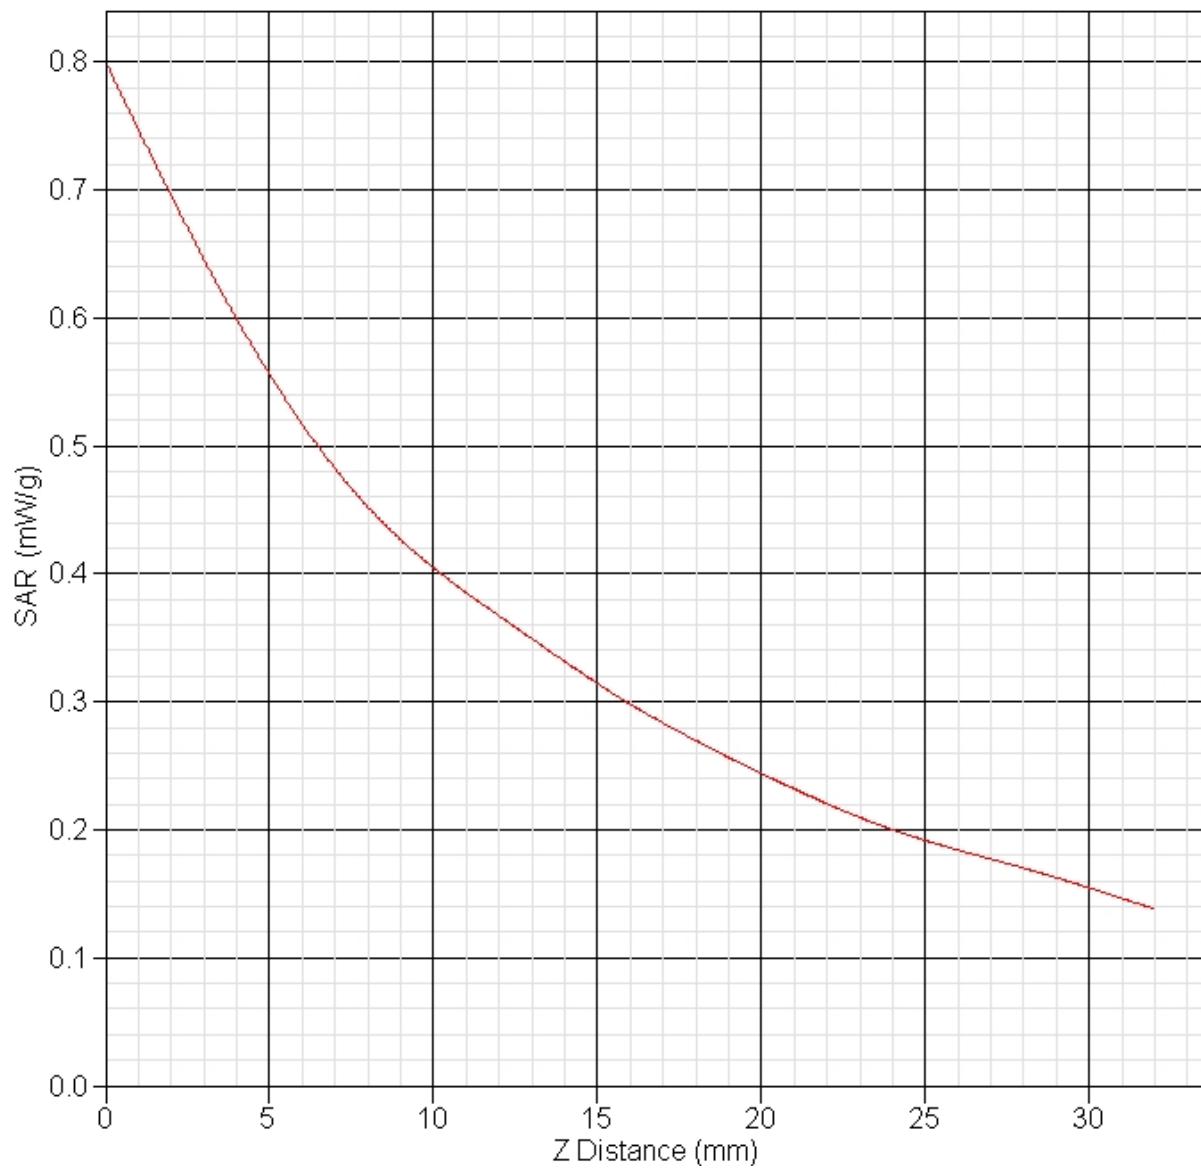

SAR Test Report

By Operator : Jay
Measurement Date : 19-Sep-2009
Starting Time : 19-Sep-2009 12:56:09 PM
End Time : 19-Sep-2009 01:12:29 PM
Scanning Time : 980 secs

Product Data

Device Name : CardioNet
Serial No. : Eng 1
Mode : EvDo Rev. 0
Model : C5
Frequency : 850.00 MHz
Max. Transmit Pwr : 0.25 W
Drift Time : 0 min(s)
Length : 117 mm
Width : 64 mm
Depth : 23 mm
Antenna Type : Internal
Orientation : Front
Power Drift-Start : 0.666 W/kg
Power Drift-Finish: 0.679 W/kg
Power Drift (%) : 2.055

Phantom Data

Name : APREL-Uni
Type : Uni-Phantom
Size (mm) : 280 x 280 x 200
Serial No. : System Default
Location : Center
Description : Uni-Phantom

Tissue Data

Type : BODY
Serial No. : 835
Frequency : 835.00 MHz
Last Calib. Date : 19-Sep-2009
Temperature : 20.00 °C
Ambient Temp. : 23.00 °C
Humidity : 40.00 RH%
Epsilon : 53.81 F/m
Sigma : 0.98 S/m
Density : 1000.00 kg/cu. m

Probe Data


Name : Probe 215 - RFEL
Model : E020
Type : E-Field Triangle
Serial No. : 215
Last Calib. Date : 03-Nov-2008
Frequency : 835.00 MHz
Duty Cycle Factor: 1
Conversion Factor: 6.3
Probe Sensitivity: 1.20 1.20 1.20 μ V/ (V/m)²
Compression Point: 95.00 mV
Offset : 1.56 mm

Measurement Data

Crest Factor : 1
Scan Type : Complete
Tissue Temp. : 20.00 °C
Ambient Temp. : 23.00 °C
Set-up Date : 19-Sep-2009
Set-up Time : 8:28:34 AM
Area Scan : 6x7x1 : Measurement x=15mm, y=15mm, z=4mm
Zoom Scan : 5x5x8 : Measurement x=8mm, y=8mm, z=4mm

Other Data

DUT Position : Front
Separation : 10 mm
Channel : Low

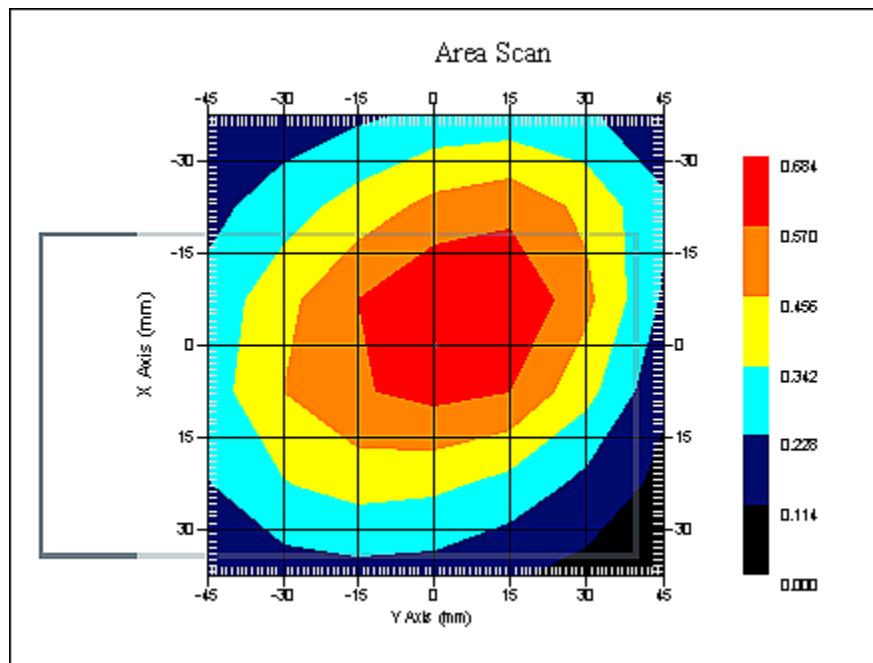

1 gram SAR value : 0.657 W/kg
10 gram SAR value : 0.494 W/kg
Area Scan Peak SAR : 0.682 W/kg
Zoom Scan Peak SAR : 0.840 W/kg

SAR Test Report

By Operator : Jay
Measurement Date : 19-Sep-2009
Starting Time : 19-Sep-2009 12:38:27 PM
End Time : 19-Sep-2009 12:54:54 PM
Scanning Time : 987 secs

Product Data

Device Name : CardioNet
Serial No. : Eng 1
Mode : EvDo Rev. 0
Model : C5
Frequency : 850.00 MHz
Max. Transmit Pwr : 0.25 W
Drift Time : 0 min(s)
Length : 117 mm
Width : 64 mm
Depth : 23 mm
Antenna Type : Internal
Orientation : Front
Power Drift-Start : 1.013 W/kg
Power Drift-Finish: 0.993 W/kg
Power Drift (%) : -1.973

Phantom Data

Name : APREL-Uni
Type : Uni-Phantom
Size (mm) : 280 x 280 x 200
Serial No. : System Default
Location : Center
Description : Uni-Phantom

Tissue Data

Type : BODY
Serial No. : 835
Frequency : 835.00 MHz
Last Calib. Date : 19-Sep-2009
Temperature : 20.00 °C
Ambient Temp. : 23.00 °C
Humidity : 40.00 RH%
Epsilon : 53.81 F/m
Sigma : 0.98 S/m
Density : 1000.00 kg/cu. m

Probe Data


Name : Probe 215 - RFEL
Model : E020
Type : E-Field Triangle
Serial No. : 215
Last Calib. Date : 03-Nov-2008
Frequency : 835.00 MHz
Duty Cycle Factor: 1
Conversion Factor: 6.3
Probe Sensitivity: 1.20 1.20 1.20 μ V/ (V/m)²
Compression Point: 95.00 mV
Offset : 1.56 mm

Measurement Data

Crest Factor : 1
Scan Type : Complete
Tissue Temp. : 20.00 °C
Ambient Temp. : 23.00 °C
Set-up Date : 19-Sep-2009
Set-up Time : 8:28:34 AM
Area Scan : 6x7x1 : Measurement x=15mm, y=15mm, z=4mm
Zoom Scan : 5x5x8 : Measurement x=8mm, y=8mm, z=4mm

Other Data

DUT Position : Front
Separation : 10 mm
Channel : Mid

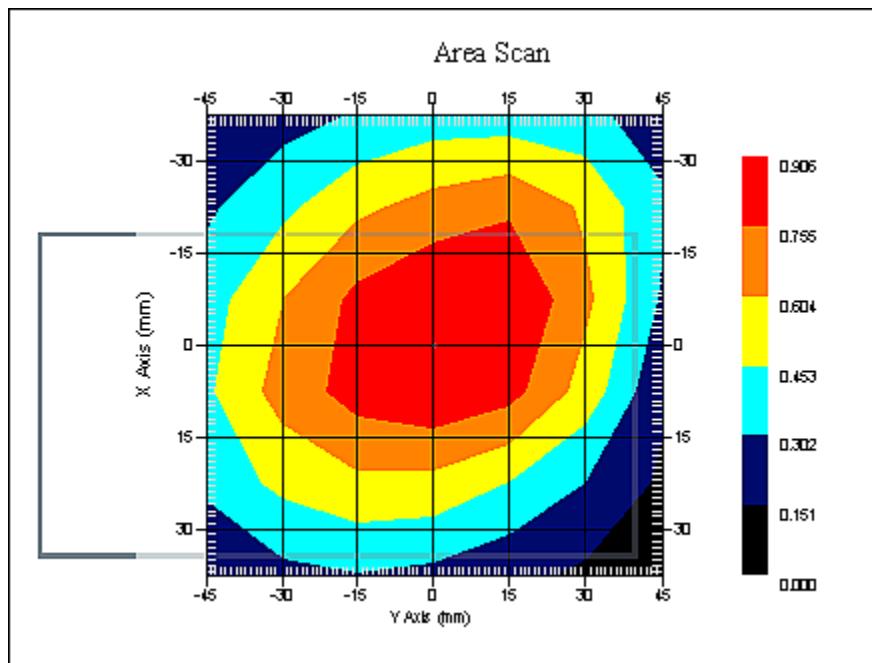

1 gram SAR value : 0.905 W/kg
10 gram SAR value : 0.665 W/kg
Area Scan Peak SAR : 0.906 W/kg
Zoom Scan Peak SAR : 1.181 W/kg

SAR Test Report

By Operator : Jay
Measurement Date : 19-Sep-2009
Starting Time : 19-Sep-2009 01:13:18 PM
End Time : 19-Sep-2009 01:29:34 PM
Scanning Time : 976 secs

Product Data

Device Name : CardioNet
Serial No. : Eng 1
Mode : EvDo Rev. 0
Model : C5
Frequency : 850.00 MHz
Max. Transmit Pwr : 0.25 W
Drift Time : 0 min(s)
Length : 117 mm
Width : 64 mm
Depth : 23 mm
Antenna Type : Internal
Orientation : Front
Power Drift-Start : 1.081 W/kg
Power Drift-Finish: 1.131 W/kg
Power Drift (%) : 4.649

Phantom Data

Name : APREL-Uni
Type : Uni-Phantom
Size (mm) : 280 x 280 x 200
Serial No. : System Default
Location : Center
Description : Uni-Phantom

Tissue Data

Type : BODY
Serial No. : 835
Frequency : 835.00 MHz
Last Calib. Date : 19-Sep-2009
Temperature : 20.00 °C
Ambient Temp. : 23.00 °C
Humidity : 40.00 RH%
Epsilon : 53.81 F/m
Sigma : 0.98 S/m
Density : 1000.00 kg/cu. m

Probe Data


Name : Probe 215 - RFEL
Model : E020
Type : E-Field Triangle
Serial No. : 215
Last Calib. Date : 03-Nov-2008
Frequency : 835.00 MHz
Duty Cycle Factor: 1
Conversion Factor: 6.3
Probe Sensitivity: 1.20 1.20 1.20 μ V/ (V/m)²
Compression Point: 95.00 mV
Offset : 1.56 mm

Measurement Data

Crest Factor : 1
 Scan Type : Complete
 Tissue Temp. : 20.00 °C
 Ambient Temp. : 23.00 °C
 Set-up Date : 19-Sep-2009
 Set-up Time : 8:28:34 AM
 Area Scan : 6x7x1 : Measurement x=15mm, y=15mm, z=4mm
 Zoom Scan : 5x5x8 : Measurement x=8mm, y=8mm, z=4mm

Other Data

DUT Position : Front
 Separation : 10 mm
 Channel : High

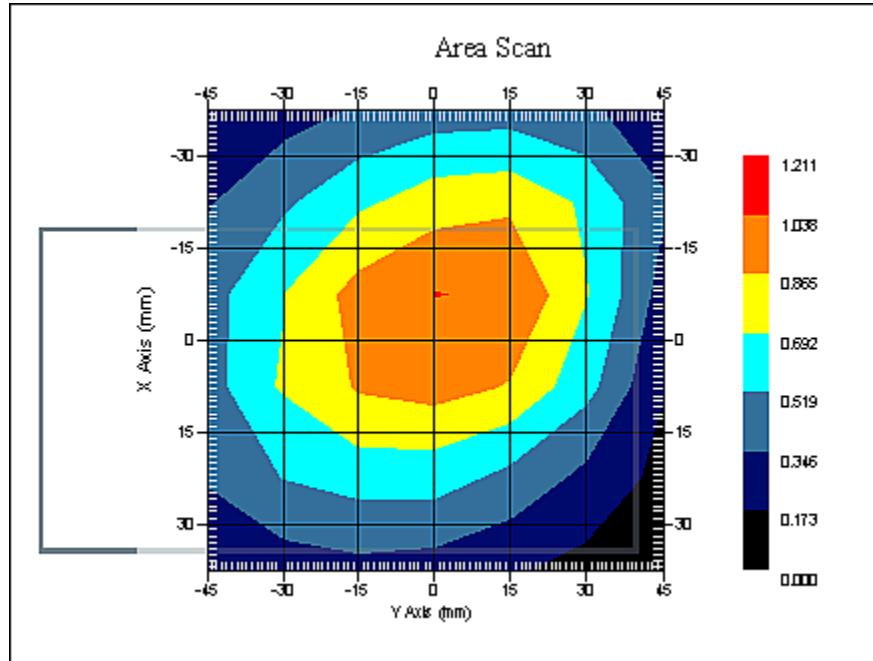

1 gram SAR value : 1.017 W/kg
 10 gram SAR value : 0.734 W/kg
 Area Scan Peak SAR : 1.040 W/kg
 Zoom Scan Peak SAR : 1.341 W/kg

SAR Test Report

By Operator : Jay
Measurement Date : 19-Sep-2009
Starting Time : 19-Sep-2009 02:45:30 PM
End Time : 19-Sep-2009 03:01:50 PM
Scanning Time : 980 secs

Product Data

Device Name : CardioNet
Serial No. : Eng 1
Mode : EvDo Rev. 0
Model : C5
Frequency : 850.00 MHz
Max. Transmit Pwr : 0.25 W
Drift Time : 0 min(s)
Length : 117 mm
Width : 64 mm
Depth : 23 mm
Antenna Type : Internal
Orientation : Back
Power Drift-Start : 0.739 W/kg
Power Drift-Finish: 0.747 W/kg
Power Drift (%) : 1.017

Phantom Data

Name : APREL-Uni
Type : Uni-Phantom
Size (mm) : 280 x 280 x 200
Serial No. : System Default
Location : Center
Description : Uni-Phantom

Tissue Data

Type : BODY
Serial No. : 835
Frequency : 835.00 MHz
Last Calib. Date : 19-Sep-2009
Temperature : 20.00 °C
Ambient Temp. : 23.00 °C
Humidity : 40.00 RH%
Epsilon : 53.81 F/m
Sigma : 0.98 S/m
Density : 1000.00 kg/cu. m

Probe Data


Name : Probe 215 - RFEL
Model : E020
Type : E-Field Triangle
Serial No. : 215
Last Calib. Date : 03-Nov-2008
Frequency : 835.00 MHz
Duty Cycle Factor: 1
Conversion Factor: 6.3
Probe Sensitivity: 1.20 1.20 1.20 μ V/ (V/m)²
Compression Point: 95.00 mV
Offset : 1.56 mm

Measurement Data

Crest Factor : 1
 Scan Type : Complete
 Tissue Temp. : 20.00 °C
 Ambient Temp. : 23.00 °C
 Set-up Date : 19-Sep-2009
 Set-up Time : 8:28:34 AM
 Area Scan : 6x7x1 : Measurement x=15mm, y=15mm, z=4mm
 Zoom Scan : 5x5x8 : Measurement x=8mm, y=8mm, z=4mm

Other Data

DUT Position : Back
 Separation : 10 mm
 Channel : Low

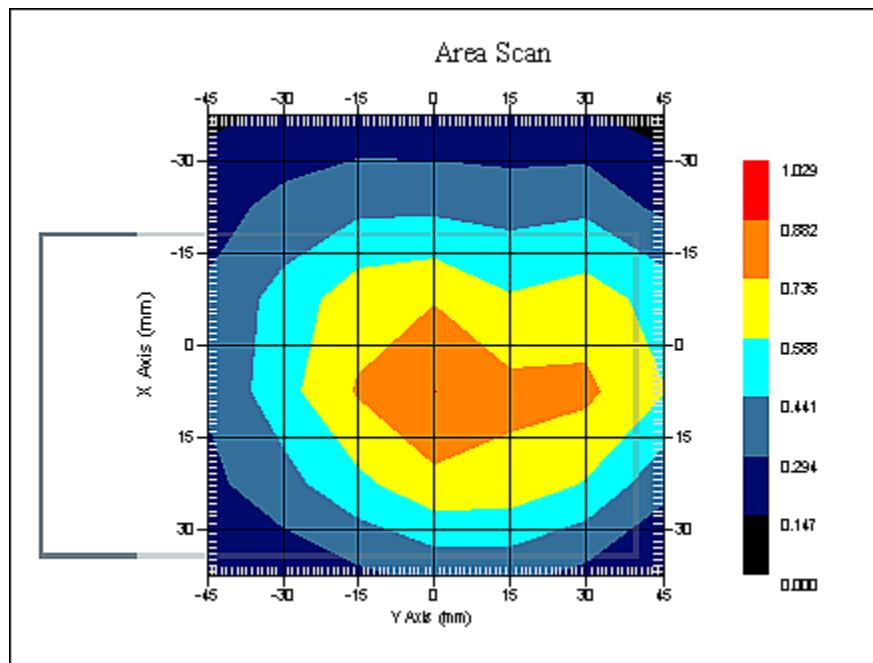

1 gram SAR value : 0.843 W/kg
 10 gram SAR value : 0.589 W/kg
 Area Scan Peak SAR : 0.885 W/kg
 Zoom Scan Peak SAR : 1.111 W/kg

SAR Test Report

By Operator : Jay
Measurement Date : 19-Sep-2009
Starting Time : 19-Sep-2009 02:28:28 PM
End Time : 19-Sep-2009 02:44:52 PM
Scanning Time : 984 secs

Product Data

Device Name : CardioNet
Serial No. : Eng 1
Mode : EvDo Rev. 0
Model : C5
Frequency : 850.00 MHz
Max. Transmit Pwr : 0.25 W
Drift Time : 0 min(s)
Length : 117 mm
Width : 64 mm
Depth : 23 mm
Antenna Type : Internal
Orientation : Back
Power Drift-Start : 1.021 W/kg
Power Drift-Finish: 1.000 W/kg
Power Drift (%) : -2.057

Phantom Data

Name : APREL-Uni
Type : Uni-Phantom
Size (mm) : 280 x 280 x 200
Serial No. : System Default
Location : Center
Description : Uni-Phantom

Tissue Data

Type : BODY
Serial No. : 835
Frequency : 835.00 MHz
Last Calib. Date : 19-Sep-2009
Temperature : 20.00 °C
Ambient Temp. : 23.00 °C
Humidity : 40.00 RH%
Epsilon : 53.81 F/m
Sigma : 0.98 S/m
Density : 1000.00 kg/cu. m

Probe Data


Name : Probe 215 - RFEL
Model : E020
Type : E-Field Triangle
Serial No. : 215
Last Calib. Date : 03-Nov-2008
Frequency : 835.00 MHz
Duty Cycle Factor: 1
Conversion Factor: 6.3
Probe Sensitivity: 1.20 1.20 1.20 μ V/ (V/m)²
Compression Point: 95.00 mV
Offset : 1.56 mm

Measurement Data

Crest Factor : 1
Scan Type : Complete
Tissue Temp. : 20.00 °C
Ambient Temp. : 23.00 °C
Set-up Date : 19-Sep-2009
Set-up Time : 8:28:34 AM
Area Scan : 6x7x1 : Measurement x=15mm, y=15mm, z=4mm
Zoom Scan : 5x5x8 : Measurement x=8mm, y=8mm, z=4mm

Other Data

DUT Position : Back
Separation : 10 mm
Channel : Mid

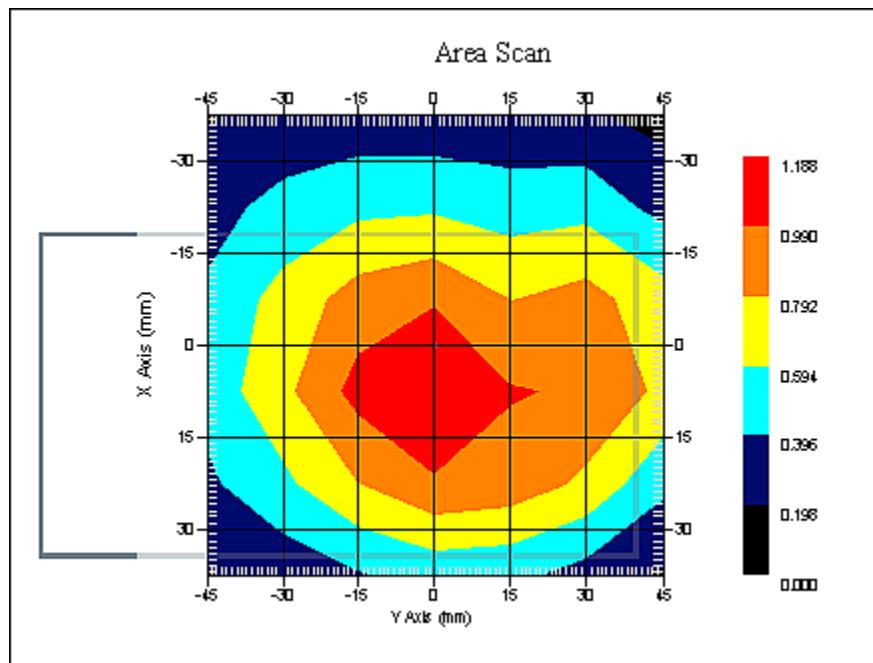

1 gram SAR value : 1.066 W/kg
10 gram SAR value : 0.741 W/kg
Area Scan Peak SAR : 1.187 W/kg
Zoom Scan Peak SAR : 1.401 W/kg

SAR Test Report

By Operator : Jay
Measurement Date : 19-Sep-2009
Starting Time : 19-Sep-2009 03:02:41 PM
End Time : 19-Sep-2009 03:18:56 PM
Scanning Time : 975 secs

Product Data

Device Name : CardioNet
Serial No. : Eng 1
Mode : EvDo Rev. 0
Model : C5
Frequency : 850.00 MHz
Max. Transmit Pwr : 0.25 W
Drift Time : 0 min(s)
Length : 117 mm
Width : 64 mm
Depth : 23 mm
Antenna Type : Internal
Orientation : Back
Power Drift-Start : 1.100 W/kg
Power Drift-Finish: 1.113 W/kg
Power Drift (%) : 1.160

Phantom Data

Name : APREL-Uni
Type : Uni-Phantom
Size (mm) : 280 x 280 x 200
Serial No. : System Default
Location : Center
Description : Uni-Phantom

Tissue Data

Type : BODY
Serial No. : 835
Frequency : 835.00 MHz
Last Calib. Date : 19-Sep-2009
Temperature : 20.00 °C
Ambient Temp. : 23.00 °C
Humidity : 40.00 RH%
Epsilon : 53.81 F/m
Sigma : 0.98 S/m
Density : 1000.00 kg/cu. m

Probe Data


Name : Probe 215 - RFEL
Model : E020
Type : E-Field Triangle
Serial No. : 215
Last Calib. Date : 03-Nov-2008
Frequency : 835.00 MHz
Duty Cycle Factor: 1
Conversion Factor: 6.3
Probe Sensitivity: 1.20 1.20 1.20 μ V/ (V/m)²
Compression Point: 95.00 mV
Offset : 1.56 mm

Measurement Data

Crest Factor : 1
 Scan Type : Complete
 Tissue Temp. : 20.00 °C
 Ambient Temp. : 23.00 °C
 Set-up Date : 19-Sep-2009
 Set-up Time : 8:28:34 AM
 Area Scan : 6x7x1 : Measurement x=15mm, y=15mm, z=4mm
 Zoom Scan : 5x5x8 : Measurement x=8mm, y=8mm, z=4mm


Other Data

DUT Position : Back
 Separation : 10 mm
 Channel : High

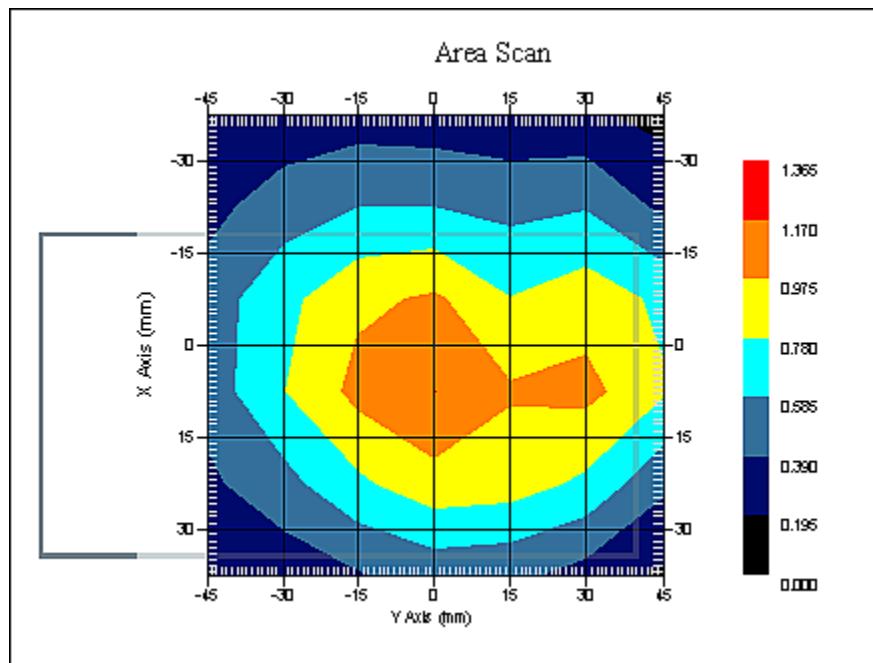

1 gram SAR value : 1.253 W/kg
 10 gram SAR value : 0.859 W/kg
 Area Scan Peak SAR : 1.172 W/kg
 Zoom Scan Peak SAR : 1.701 W/kg

SAR-Z Axis
at Hotspot x:15.04 y:-0.13

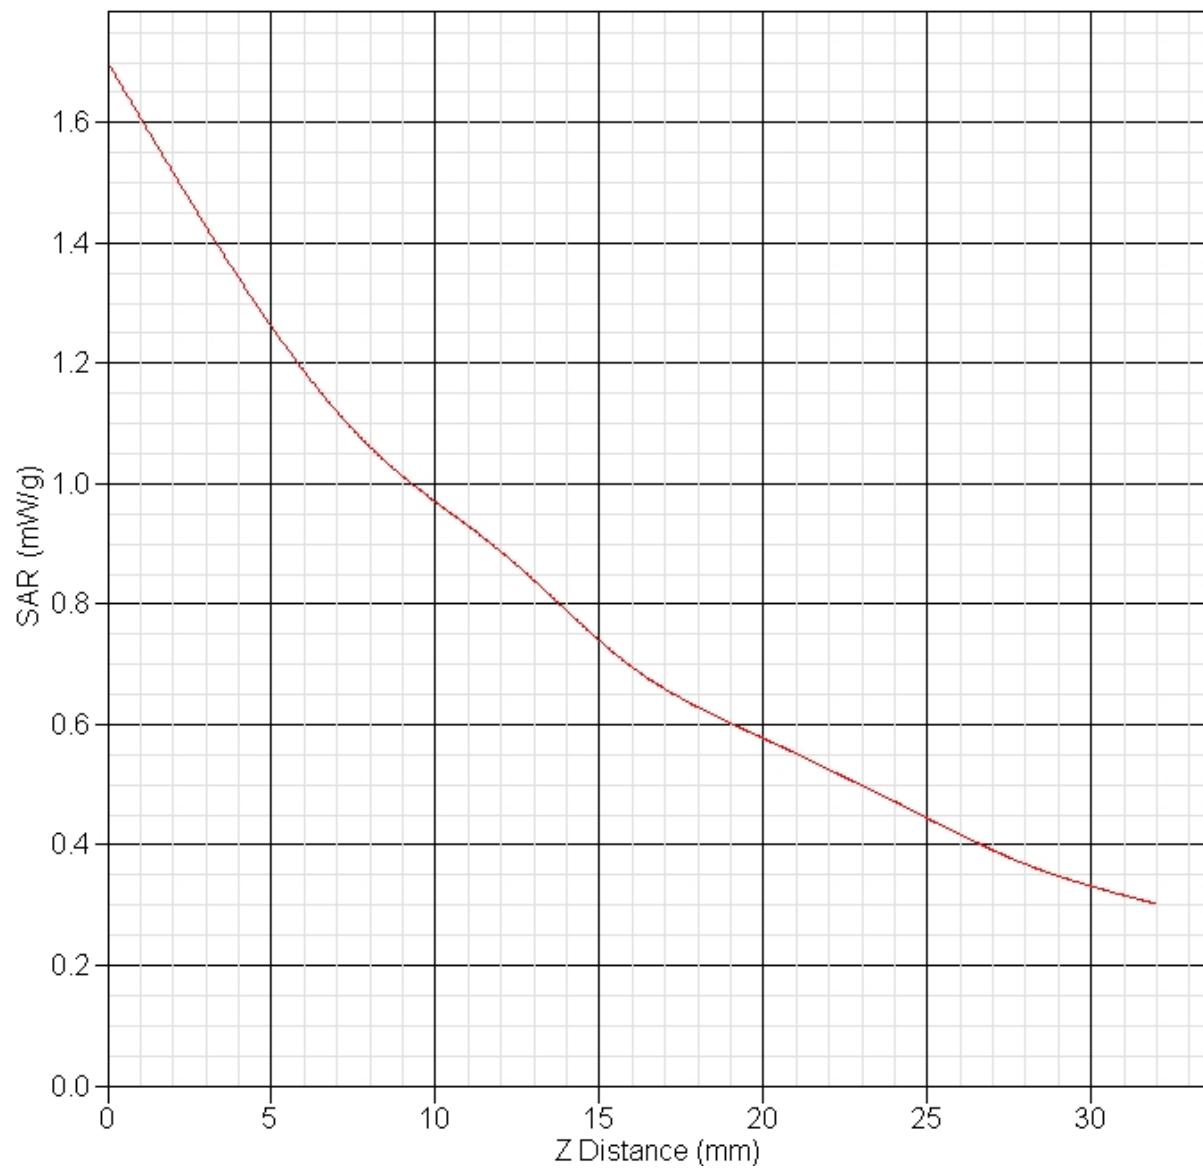

SAR Test Report

By Operator : Jay
Measurement Date : 18-Sep-2009
Starting Time : 18-Sep-2009 04:45:42 PM
End Time : 18-Sep-2009 05:02:08 PM
Scanning Time : 986 secs

Product Data

Device Name : CardioNet
Serial No. : Eng 2
Mode : GSM
Model : C5
Frequency : 850.00 MHz
Max. Transmit Pwr : 2 W
Drift Time : 0 min(s)
Length : 117 mm
Width : 64 mm
Depth : 23 mm
Antenna Type : Internal
Orientation : Held To Face
Power Drift-Start : 0.437 W/kg
Power Drift-Finish: 0.429 W/kg
Power Drift (%) : -1.774

Phantom Data

Name : APREL-Uni
Type : Uni-Phantom
Size (mm) : 280 x 280 x 200
Serial No. : System Default
Location : Center
Description : Uni-Phantom

Tissue Data

Type : HEAD
Serial No. : 835
Frequency : 835.00 MHz
Last Calib. Date : 18-Sep-2009
Temperature : 20.00 °C
Ambient Temp. : 23.00 °C
Humidity : 40.00 RH%
Epsilon : 41.46 F/m
Sigma : 0.91 S/m
Density : 1000.00 kg/cu. m

Probe Data


Name : Probe 215 - RFEL
Model : E020
Type : E-Field Triangle
Serial No. : 215
Last Calib. Date : 03-Nov-2008
Frequency : 835.00 MHz
Duty Cycle Factor: 8
Conversion Factor: 6.2
Probe Sensitivity: 1.20 1.20 1.20 μ V/ (V/m)²
Compression Point: 95.00 mV
Offset : 1.56 mm

Measurement Data

Crest Factor : 8
 Scan Type : Complete
 Tissue Temp. : 20.00 °C
 Ambient Temp. : 23.00 °C
 Set-up Date : 18-Sep-2009
 Set-up Time : 4:45:39 PM
 Area Scan : 6x7x1 : Measurement x=15mm, y=15mm, z=4mm
 Zoom Scan : 5x5x8 : Measurement x=8mm, y=8mm, z=4mm

Other Data

DUT Position : Held To Face
 Separation : 25 mm
 Channel : Low

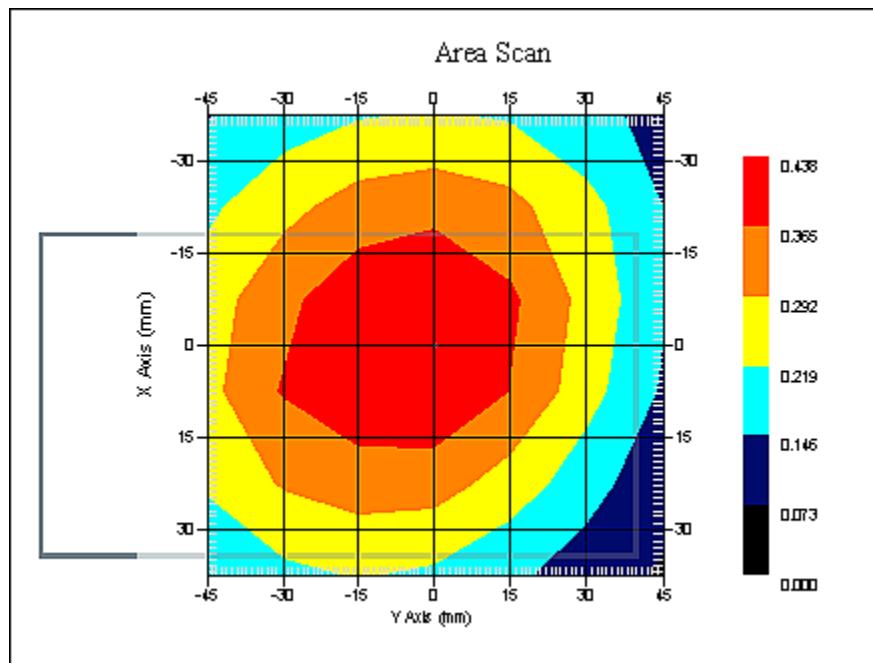

1 gram SAR value : 0.416 W/kg
 10 gram SAR value : 0.307 W/kg
 Area Scan Peak SAR : 0.436 W/kg
 Zoom Scan Peak SAR : 0.540 W/kg

SAR Test Report

By Operator : Jay
Measurement Date : 18-Sep-2009
Starting Time : 18-Sep-2009 04:11:26 PM
End Time : 18-Sep-2009 04:27:48 PM
Scanning Time : 982 secs

Product Data

Device Name : CardioNet
Serial No. : Eng 2
Mode : GSM
Model : C5
Frequency : 850.00 MHz
Max. Transmit Pwr : 2 W
Drift Time : 0 min(s)
Length : 117 mm
Width : 64 mm
Depth : 23 mm
Antenna Type : Internal
Orientation : Held To Face
Power Drift-Start : 0.448 W/kg
Power Drift-Finish: 0.457 W/kg
Power Drift (%) : 1.835

Phantom Data

Name : APREL-Uni
Type : Uni-Phantom
Size (mm) : 280 x 280 x 200
Serial No. : System Default
Location : Center
Description : Uni-Phantom

Tissue Data

Type : HEAD
Serial No. : 835
Frequency : 835.00 MHz
Last Calib. Date : 18-Sep-2009
Temperature : 20.00 °C
Ambient Temp. : 23.00 °C
Humidity : 40.00 RH%
Epsilon : 41.46 F/m
Sigma : 0.91 S/m
Density : 1000.00 kg/cu. m

Probe Data


Name : Probe 215 - RFEL
Model : E020
Type : E-Field Triangle
Serial No. : 215
Last Calib. Date : 03-Nov-2008
Frequency : 835.00 MHz
Duty Cycle Factor: 8
Conversion Factor: 6.2
Probe Sensitivity: 1.20 1.20 1.20 μ V/ (V/m)²
Compression Point: 95.00 mV
Offset : 1.56 mm

Measurement Data

Crest Factor : 8
 Scan Type : Complete
 Tissue Temp. : 20.00 °C
 Ambient Temp. : 23.00 °C
 Set-up Date : 18-Sep-2009
 Set-up Time : 4:00:43 PM
 Area Scan : 6x7x1 : Measurement x=15mm, y=15mm, z=4mm
 Zoom Scan : 5x5x8 : Measurement x=8mm, y=8mm, z=4mm

Other Data

DUT Position : Held To Face
 Separation : 25 mm
 Channel : Mid

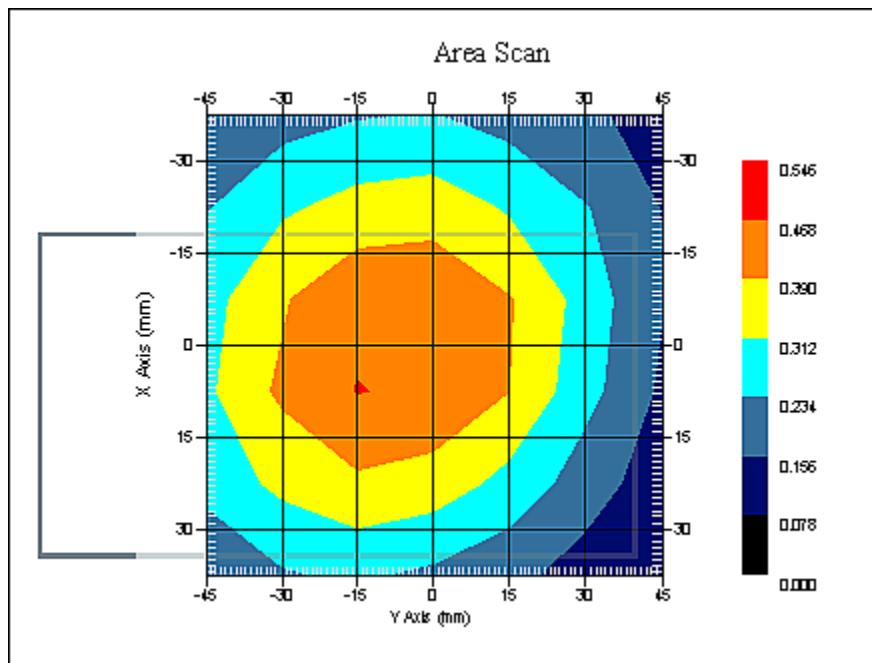

1 gram SAR value : 0.474 W/kg
 10 gram SAR value : 0.349 W/kg
 Area Scan Peak SAR : 0.470 W/kg
 Zoom Scan Peak SAR : 0.640 W/kg

SAR Test Report

By Operator : Jay
Measurement Date : 18-Sep-2009
Starting Time : 18-Sep-2009 05:03:12 PM
End Time : 18-Sep-2009 05:19:28 PM
Scanning Time : 976 secs

Product Data

Device Name : CardioNet
Serial No. : Eng 2
Mode : GSM
Model : C5
Frequency : 850.00 MHz
Max. Transmit Pwr : 2 W
Drift Time : 0 min(s)
Length : 117 mm
Width : 64 mm
Depth : 23 mm
Antenna Type : Internal
Orientation : Held To Face
Power Drift-Start : 0.500 W/kg
Power Drift-Finish: 0.502 W/kg
Power Drift (%) : 0.407

Phantom Data

Name : APREL-Uni
Type : Uni-Phantom
Size (mm) : 280 x 280 x 200
Serial No. : System Default
Location : Center
Description : Uni-Phantom

Tissue Data

Type : HEAD
Serial No. : 835
Frequency : 835.00 MHz
Last Calib. Date : 18-Sep-2009
Temperature : 20.00 °C
Ambient Temp. : 23.00 °C
Humidity : 40.00 RH%
Epsilon : 41.46 F/m
Sigma : 0.91 S/m
Density : 1000.00 kg/cu. m

Probe Data


Name : Probe 215 - RFEL
Model : E020
Type : E-Field Triangle
Serial No. : 215
Last Calib. Date : 03-Nov-2008
Frequency : 835.00 MHz
Duty Cycle Factor: 8
Conversion Factor: 6.2
Probe Sensitivity: 1.20 1.20 1.20 μ V/ (V/m)²
Compression Point: 95.00 mV
Offset : 1.56 mm

Measurement Data

Crest Factor : 8
 Scan Type : Complete
 Tissue Temp. : 20.00 °C
 Ambient Temp. : 23.00 °C
 Set-up Date : 18-Sep-2009
 Set-up Time : 4:45:39 PM
 Area Scan : 6x7x1 : Measurement x=15mm, y=15mm, z=4mm
 Zoom Scan : 5x5x8 : Measurement x=8mm, y=8mm, z=4mm


Other Data

DUT Position : Held To Face
 Separation : 25 mm
 Channel : High

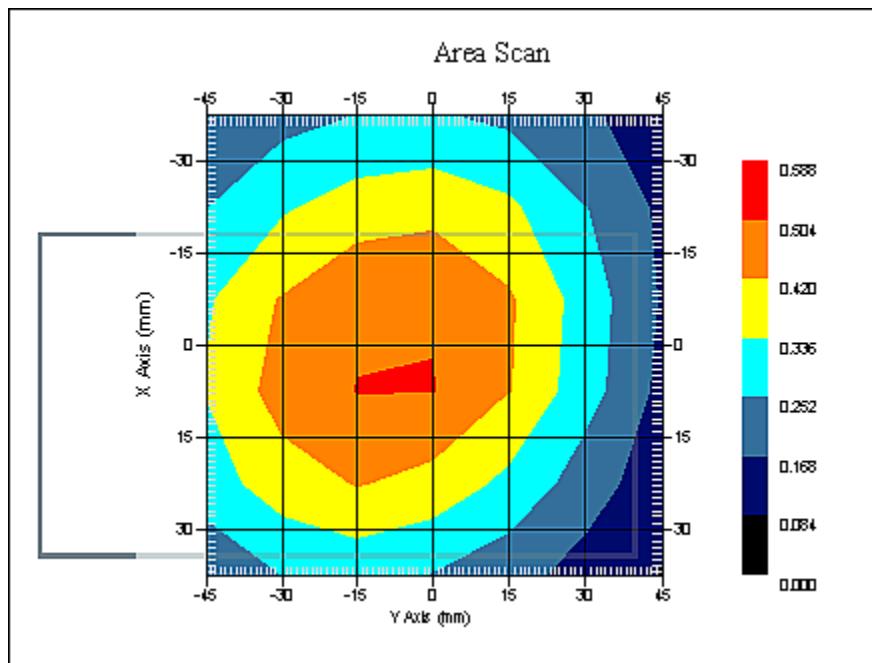

1 gram SAR value : 0.514 W/kg
 10 gram SAR value : 0.377 W/kg
 Area Scan Peak SAR : 0.506 W/kg
 Zoom Scan Peak SAR : 0.690 W/kg

SAR-Z Axis
at Hotspot x:7.08 y:-7.16

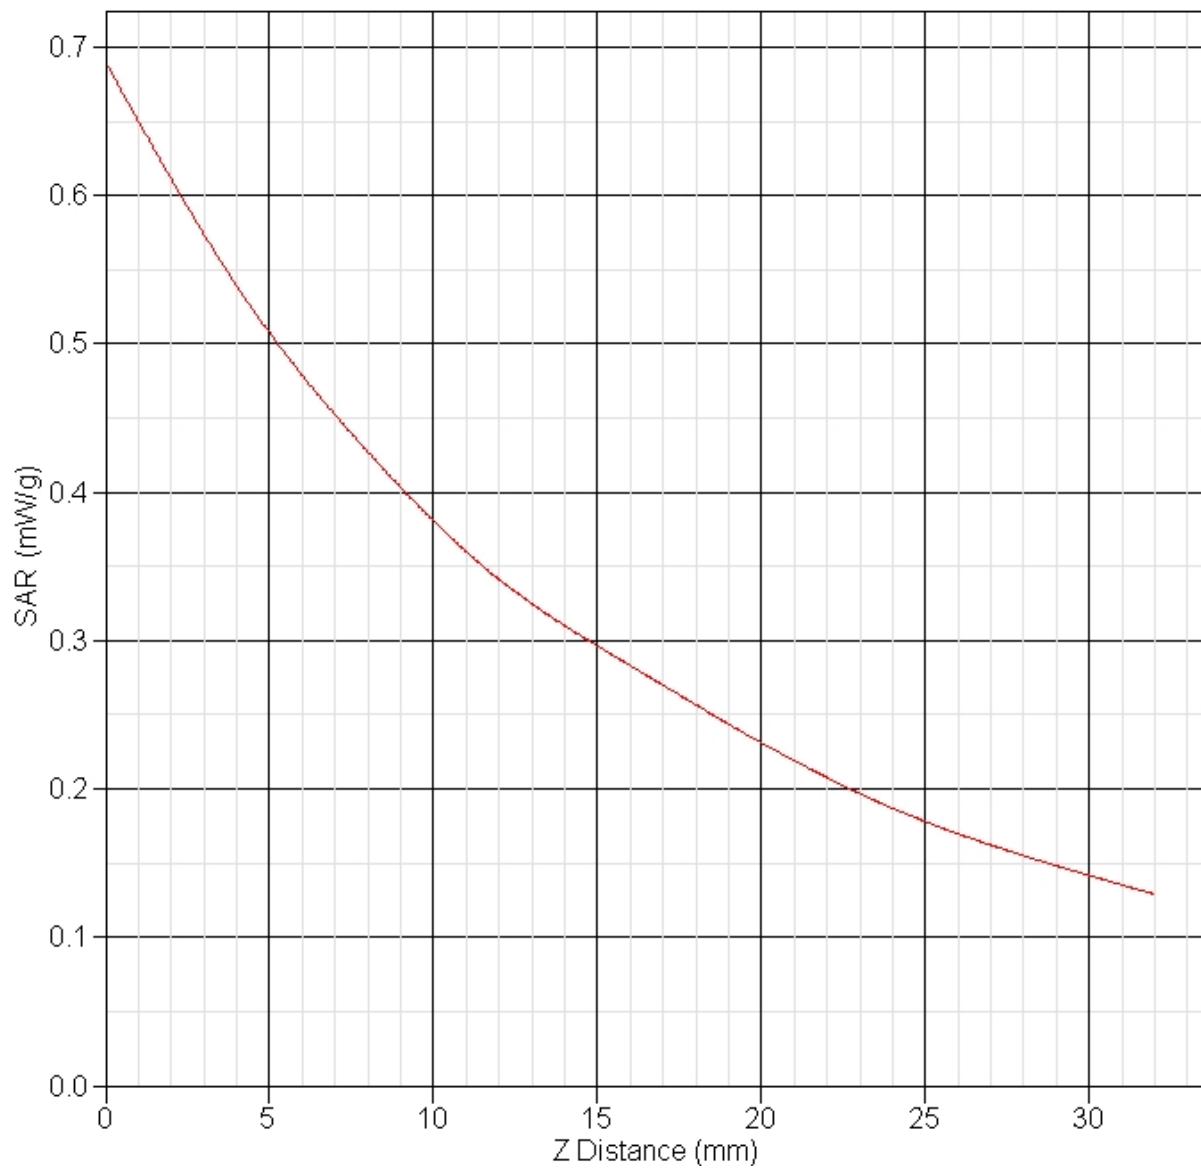

SAR Test Report

By Operator : Jay
Measurement Date : 19-Sep-2009
Starting Time : 19-Sep-2009 11:24:54 AM
End Time : 19-Sep-2009 11:41:14 AM
Scanning Time : 980 secs

Product Data

Device Name : CardioNet
Serial No. : Eng 2
Mode : GPRS
Model : C5
Frequency : 850.00 MHz
Max. Transmit Pwr : 2 W
Drift Time : 0 min(s)
Length : 117 mm
Width : 64 mm
Depth : 23 mm
Antenna Type : Internal
Orientation : Front
Power Drift-Start : 0.785 W/kg
Power Drift-Finish: 0.795 W/kg
Power Drift (%) : 1.241

Phantom Data

Name : APREL-Uni
Type : Uni-Phantom
Size (mm) : 280 x 280 x 200
Serial No. : System Default
Location : Center
Description : Uni-Phantom

Tissue Data

Type : BODY
Serial No. : 835
Frequency : 835.00 MHz
Last Calib. Date : 19-Sep-2009
Temperature : 20.00 °C
Ambient Temp. : 23.00 °C
Humidity : 40.00 RH%
Epsilon : 53.81 F/m
Sigma : 0.98 S/m
Density : 1000.00 kg/cu. m

Probe Data


Name : Probe 215 - RFEL
Model : E020
Type : E-Field Triangle
Serial No. : 215
Last Calib. Date : 03-Nov-2008
Frequency : 835.00 MHz
Duty Cycle Factor: 4
Conversion Factor: 6.3
Probe Sensitivity: 1.20 1.20 1.20 μ V/ (V/m)²
Compression Point: 95.00 mV
Offset : 1.56 mm

Measurement Data

Crest Factor : 4
Scan Type : Complete
Tissue Temp. : 20.00 °C
Ambient Temp. : 23.00 °C
Set-up Date : 19-Sep-2009
Set-up Time : 8:28:34 AM
Area Scan : 6x7x1 : Measurement x=15mm, y=15mm, z=4mm
Zoom Scan : 5x5x8 : Measurement x=8mm, y=8mm, z=4mm

Other Data

DUT Position : Front
Separation : 10 mm
Channel : Low

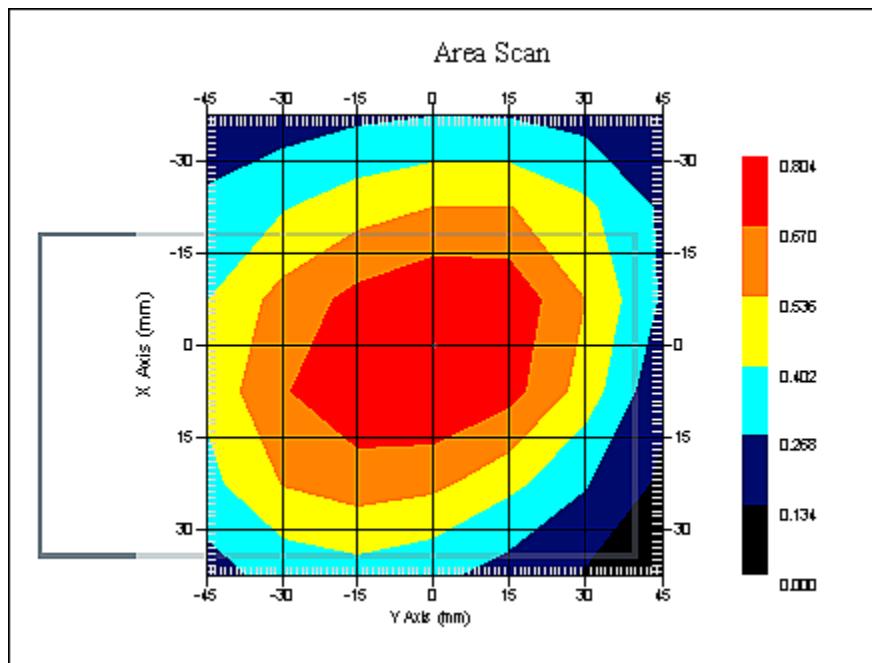

1 gram SAR value : 0.792 W/kg
10 gram SAR value : 0.585 W/kg
Area Scan Peak SAR : 0.802 W/kg
Zoom Scan Peak SAR : 1.010 W/kg

SAR Test Report

By Operator : Jay
Measurement Date : 19-Sep-2009
Starting Time : 19-Sep-2009 11:07:16 AM
End Time : 19-Sep-2009 11:23:41 AM
Scanning Time : 985 secs

Product Data

Device Name : CardioNet
Serial No. : Eng 2
Mode : GPRS
Model : C5
Frequency : 850.00 MHz
Max. Transmit Pwr : 2 W
Drift Time : 0 min(s)
Length : 117 mm
Width : 64 mm
Depth : 23 mm
Antenna Type : Internal
Orientation : Front
Power Drift-Start : 0.776 W/kg
Power Drift-Finish: 0.788 W/kg
Power Drift (%) : 1.454

Phantom Data

Name : APREL-Uni
Type : Uni-Phantom
Size (mm) : 280 x 280 x 200
Serial No. : System Default
Location : Center
Description : Uni-Phantom

Tissue Data

Type : BODY
Serial No. : 835
Frequency : 835.00 MHz
Last Calib. Date : 19-Sep-2009
Temperature : 20.00 °C
Ambient Temp. : 23.00 °C
Humidity : 40.00 RH%
Epsilon : 53.81 F/m
Sigma : 0.98 S/m
Density : 1000.00 kg/cu. m

Probe Data


Name : Probe 215 - RFEL
Model : E020
Type : E-Field Triangle
Serial No. : 215
Last Calib. Date : 03-Nov-2008
Frequency : 835.00 MHz
Duty Cycle Factor: 4
Conversion Factor: 6.3
Probe Sensitivity: 1.20 1.20 1.20 μ V/ (V/m)²
Compression Point: 95.00 mV
Offset : 1.56 mm

Measurement Data

Crest Factor : 4
 Scan Type : Complete
 Tissue Temp. : 20.00 °C
 Ambient Temp. : 23.00 °C
 Set-up Date : 19-Sep-2009
 Set-up Time : 8:28:34 AM
 Area Scan : 6x7x1 : Measurement x=15mm, y=15mm, z=4mm
 Zoom Scan : 5x5x8 : Measurement x=8mm, y=8mm, z=4mm

Other Data

DUT Position : Front
 Separation : 10 mm
 Channel : Mid

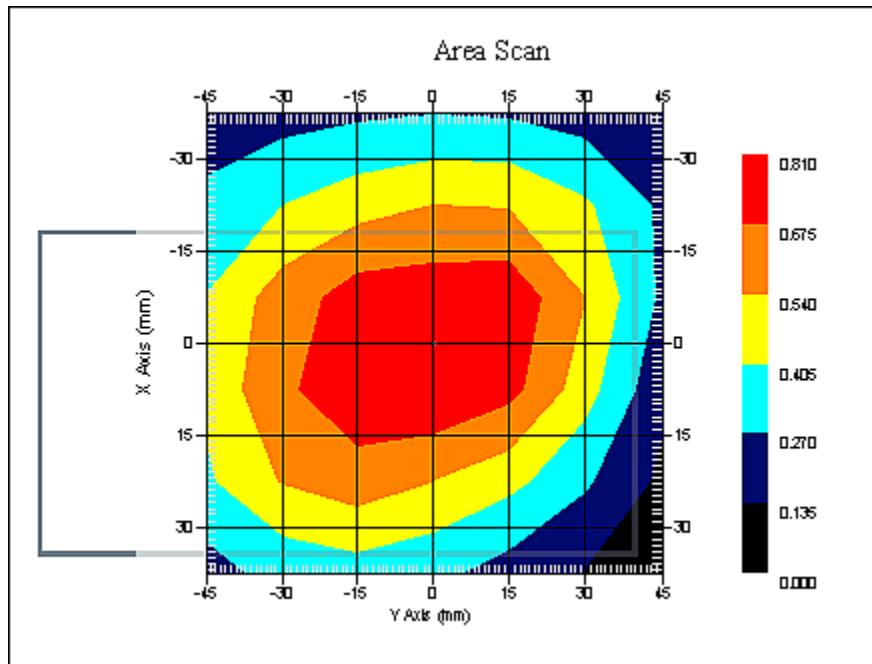

1 gram SAR value : 0.819 W/kg
 10 gram SAR value : 0.620 W/kg
 Area Scan Peak SAR : 0.810 W/kg
 Zoom Scan Peak SAR : 1.030 W/kg

SAR Test Report

By Operator : Jay
Measurement Date : 19-Sep-2009
Starting Time : 19-Sep-2009 11:43:50 AM
End Time : 19-Sep-2009 12:00:06 PM
Scanning Time : 976 secs

Product Data

Device Name : CardioNet
Serial No. : Eng 2
Mode : GPRS
Model : C5
Frequency : 850.00 MHz
Max. Transmit Pwr : 2 W
Drift Time : 0 min(s)
Length : 117 mm
Width : 64 mm
Depth : 23 mm
Antenna Type : Internal
Orientation : Front
Power Drift-Start : 0.883 W/kg
Power Drift-Finish: 0.847 W/kg
Power Drift (%) : -4.170

Phantom Data

Name : APREL-Uni
Type : Uni-Phantom
Size (mm) : 280 x 280 x 200
Serial No. : System Default
Location : Center
Description : Uni-Phantom

Tissue Data

Type : BODY
Serial No. : 835
Frequency : 835.00 MHz
Last Calib. Date : 19-Sep-2009
Temperature : 20.00 °C
Ambient Temp. : 23.00 °C
Humidity : 40.00 RH%
Epsilon : 53.81 F/m
Sigma : 0.98 S/m
Density : 1000.00 kg/cu. m

Probe Data


Name : Probe 215 - RFEL
Model : E020
Type : E-Field Triangle
Serial No. : 215
Last Calib. Date : 03-Nov-2008
Frequency : 835.00 MHz
Duty Cycle Factor: 4
Conversion Factor: 6.3
Probe Sensitivity: 1.20 1.20 1.20 μ V/ (V/m)²
Compression Point: 95.00 mV
Offset : 1.56 mm

Measurement Data

Crest Factor : 4
 Scan Type : Complete
 Tissue Temp. : 20.00 °C
 Ambient Temp. : 23.00 °C
 Set-up Date : 19-Sep-2009
 Set-up Time : 8:28:34 AM
 Area Scan : 6x7x1 : Measurement x=15mm, y=15mm, z=4mm
 Zoom Scan : 5x5x8 : Measurement x=8mm, y=8mm, z=4mm

Other Data

DUT Position : Front
 Separation : 10 mm
 Channel : High

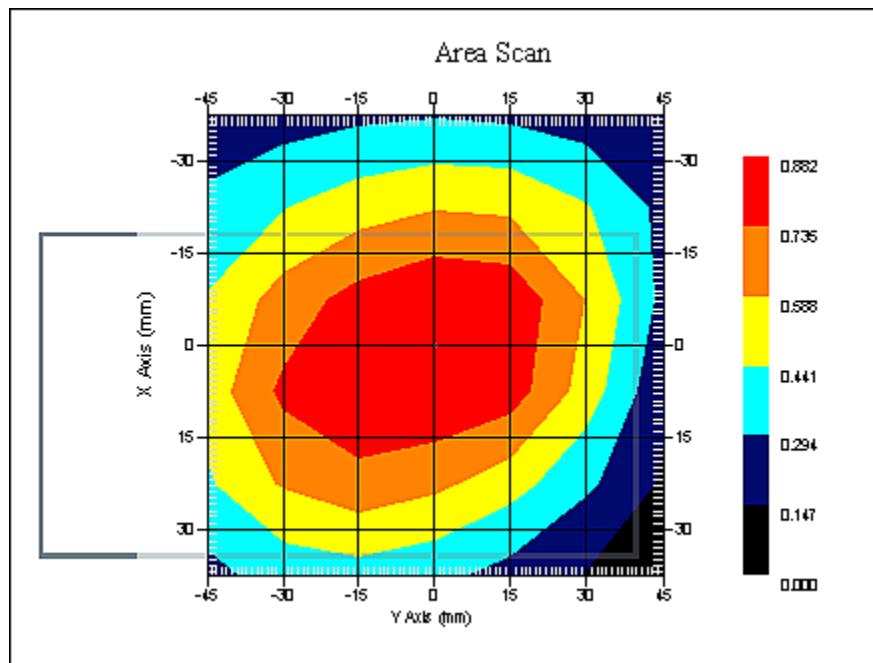

1 gram SAR value : 0.903 W/kg
 10 gram SAR value : 0.680 W/kg
 Area Scan Peak SAR : 0.880 W/kg
 Zoom Scan Peak SAR : 1.171 W/kg

SAR Test Report

By Operator : Jay
Measurement Date : 19-Sep-2009
Starting Time : 19-Sep-2009 03:40:19 PM
End Time : 19-Sep-2009 03:56:35 PM
Scanning Time : 976 secs

Product Data

Device Name : CardioNet
Serial No. : Eng 2
Mode : GPRS
Model : C5
Frequency : 850.00 MHz
Max. Transmit Pwr : 2 W
Drift Time : 0 min(s)
Length : 117 mm
Width : 64 mm
Depth : 23 mm
Antenna Type : Internal
Orientation : Back
Power Drift-Start : 0.813 W/kg
Power Drift-Finish: 0.817 W/kg
Power Drift (%) : 0.501

Phantom Data

Name : APREL-Uni
Type : Uni-Phantom
Size (mm) : 280 x 280 x 200
Serial No. : System Default
Location : Center
Description : Uni-Phantom

Tissue Data

Type : BODY
Serial No. : 835
Frequency : 835.00 MHz
Last Calib. Date : 19-Sep-2009
Temperature : 20.00 °C
Ambient Temp. : 23.00 °C
Humidity : 40.00 RH%
Epsilon : 53.81 F/m
Sigma : 0.98 S/m
Density : 1000.00 kg/cu. m

Probe Data


Name : Probe 215 - RFEL
Model : E020
Type : E-Field Triangle
Serial No. : 215
Last Calib. Date : 03-Nov-2008
Frequency : 835.00 MHz
Duty Cycle Factor: 4
Conversion Factor: 6.3
Probe Sensitivity: 1.20 1.20 1.20 μ V/ (V/m)²
Compression Point: 95.00 mV
Offset : 1.56 mm

Measurement Data

Crest Factor : 4
 Scan Type : Complete
 Tissue Temp. : 20.00 °C
 Ambient Temp. : 23.00 °C
 Set-up Date : 19-Sep-2009
 Set-up Time : 8:28:34 AM
 Area Scan : 6x7x1 : Measurement x=15mm, y=15mm, z=4mm
 Zoom Scan : 5x5x8 : Measurement x=8mm, y=8mm, z=4mm

Other Data

DUT Position : Back
 Separation : 10 mm
 Channel : Low

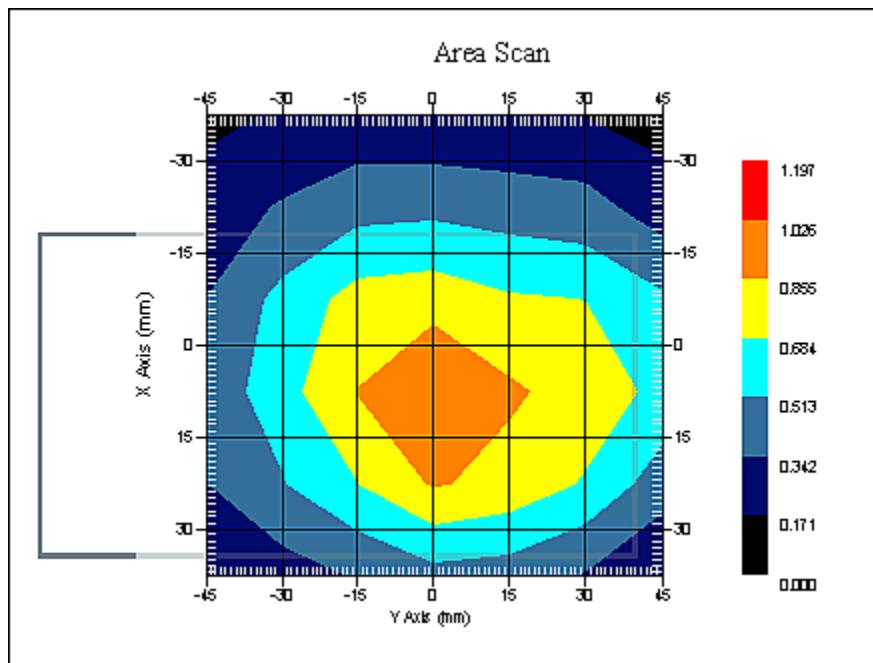

1 gram SAR value : 0.980 W/kg
 10 gram SAR value : 0.716 W/kg
 Area Scan Peak SAR : 1.027 W/kg
 Zoom Scan Peak SAR : 1.311 W/kg

SAR Test Report

By Operator : Jay
Measurement Date : 19-Sep-2009
Starting Time : 19-Sep-2009 03:23:19 PM
End Time : 19-Sep-2009 03:39:39 PM
Scanning Time : 980 secs

Product Data

Device Name : CardioNet
Serial No. : Eng 2
Mode : GPRS
Model : C5
Frequency : 850.00 MHz
Max. Transmit Pwr : 2 W
Drift Time : 0 min(s)
Length : 117 mm
Width : 64 mm
Depth : 23 mm
Antenna Type : Internal
Orientation : Back
Power Drift-Start : 0.869 W/kg
Power Drift-Finish: 0.873 W/kg
Power Drift (%) : 0.508

Phantom Data

Name : APREL-Uni
Type : Uni-Phantom
Size (mm) : 280 x 280 x 200
Serial No. : System Default
Location : Center
Description : Uni-Phantom

Tissue Data

Type : BODY
Serial No. : 835
Frequency : 835.00 MHz
Last Calib. Date : 19-Sep-2009
Temperature : 20.00 °C
Ambient Temp. : 23.00 °C
Humidity : 40.00 RH%
Epsilon : 53.81 F/m
Sigma : 0.98 S/m
Density : 1000.00 kg/cu. m

Probe Data


Name : Probe 215 - RFEL
Model : E020
Type : E-Field Triangle
Serial No. : 215
Last Calib. Date : 03-Nov-2008
Frequency : 835.00 MHz
Duty Cycle Factor: 4
Conversion Factor: 6.3
Probe Sensitivity: 1.20 1.20 1.20 μ V/ (V/m)²
Compression Point: 95.00 mV
Offset : 1.56 mm

Measurement Data

Crest Factor : 4
Scan Type : Complete
Tissue Temp. : 20.00 °C
Ambient Temp. : 23.00 °C
Set-up Date : 19-Sep-2009
Set-up Time : 8:28:34 AM
Area Scan : 6x7x1 : Measurement x=15mm, y=15mm, z=4mm
Zoom Scan : 5x5x8 : Measurement x=8mm, y=8mm, z=4mm

Other Data

DUT Position : Back
Separation : 10 mm
Channel : Mid

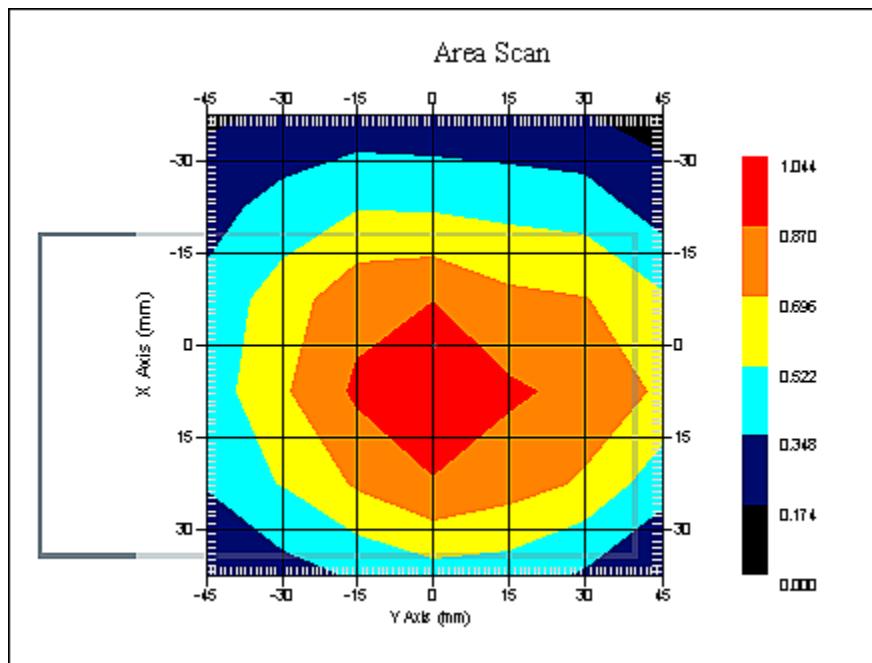

1 gram SAR value : 0.961 W/kg
10 gram SAR value : 0.681 W/kg
Area Scan Peak SAR : 1.041 W/kg
Zoom Scan Peak SAR : 1.311 W/kg

SAR Test Report

By Operator : Jay
Measurement Date : 19-Sep-2009
Starting Time : 19-Sep-2009 12:01:00 PM
End Time : 19-Sep-2009 12:17:13 PM
Scanning Time : 973 secs

Product Data

Device Name : CardioNet
Serial No. : Eng 2
Mode : GPRS
Model : C5
Frequency : 850.00 MHz
Max. Transmit Pwr : 2 W
Drift Time : 0 min(s)
Length : 117 mm
Width : 64 mm
Depth : 23 mm
Antenna Type : Internal
Orientation : Back
Power Drift-Start : 0.947 W/kg
Power Drift-Finish: 0.935 W/kg
Power Drift (%) : -1.212

Phantom Data

Name : APREL-Uni
Type : Uni-Phantom
Size (mm) : 280 x 280 x 200
Serial No. : System Default
Location : Center
Description : Uni-Phantom

Tissue Data

Type : BODY
Serial No. : 835
Frequency : 835.00 MHz
Last Calib. Date : 19-Sep-2009
Temperature : 20.00 °C
Ambient Temp. : 23.00 °C
Humidity : 40.00 RH%
Epsilon : 53.81 F/m
Sigma : 0.98 S/m
Density : 1000.00 kg/cu. m

Probe Data


Name : Probe 215 - RFEL
Model : E020
Type : E-Field Triangle
Serial No. : 215
Last Calib. Date : 03-Nov-2008
Frequency : 835.00 MHz
Duty Cycle Factor: 4
Conversion Factor: 6.3
Probe Sensitivity: 1.20 1.20 1.20 μ V/ (V/m)²
Compression Point: 95.00 mV
Offset : 1.56 mm

Measurement Data

Crest Factor : 4
 Scan Type : Complete
 Tissue Temp. : 20.00 °C
 Ambient Temp. : 23.00 °C
 Set-up Date : 19-Sep-2009
 Set-up Time : 8:28:34 AM
 Area Scan : 6x7x1 : Measurement x=15mm, y=15mm, z=4mm
 Zoom Scan : 5x5x8 : Measurement x=8mm, y=8mm, z=4mm


Other Data

DUT Position : Back
 Separation : 10 mm
 Channel : High

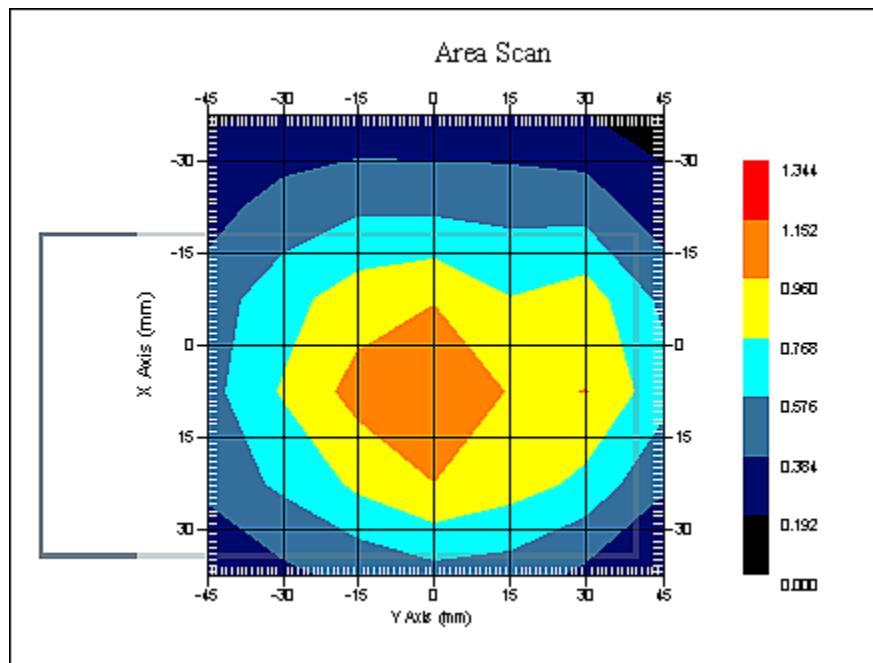

1 gram SAR value : 1.096 W/kg
 10 gram SAR value : 0.802 W/kg
 Area Scan Peak SAR : 1.154 W/kg
 Zoom Scan Peak SAR : 1.431 W/kg

SAR-Z Axis
at Hotspot x:15.10 y:-0.14

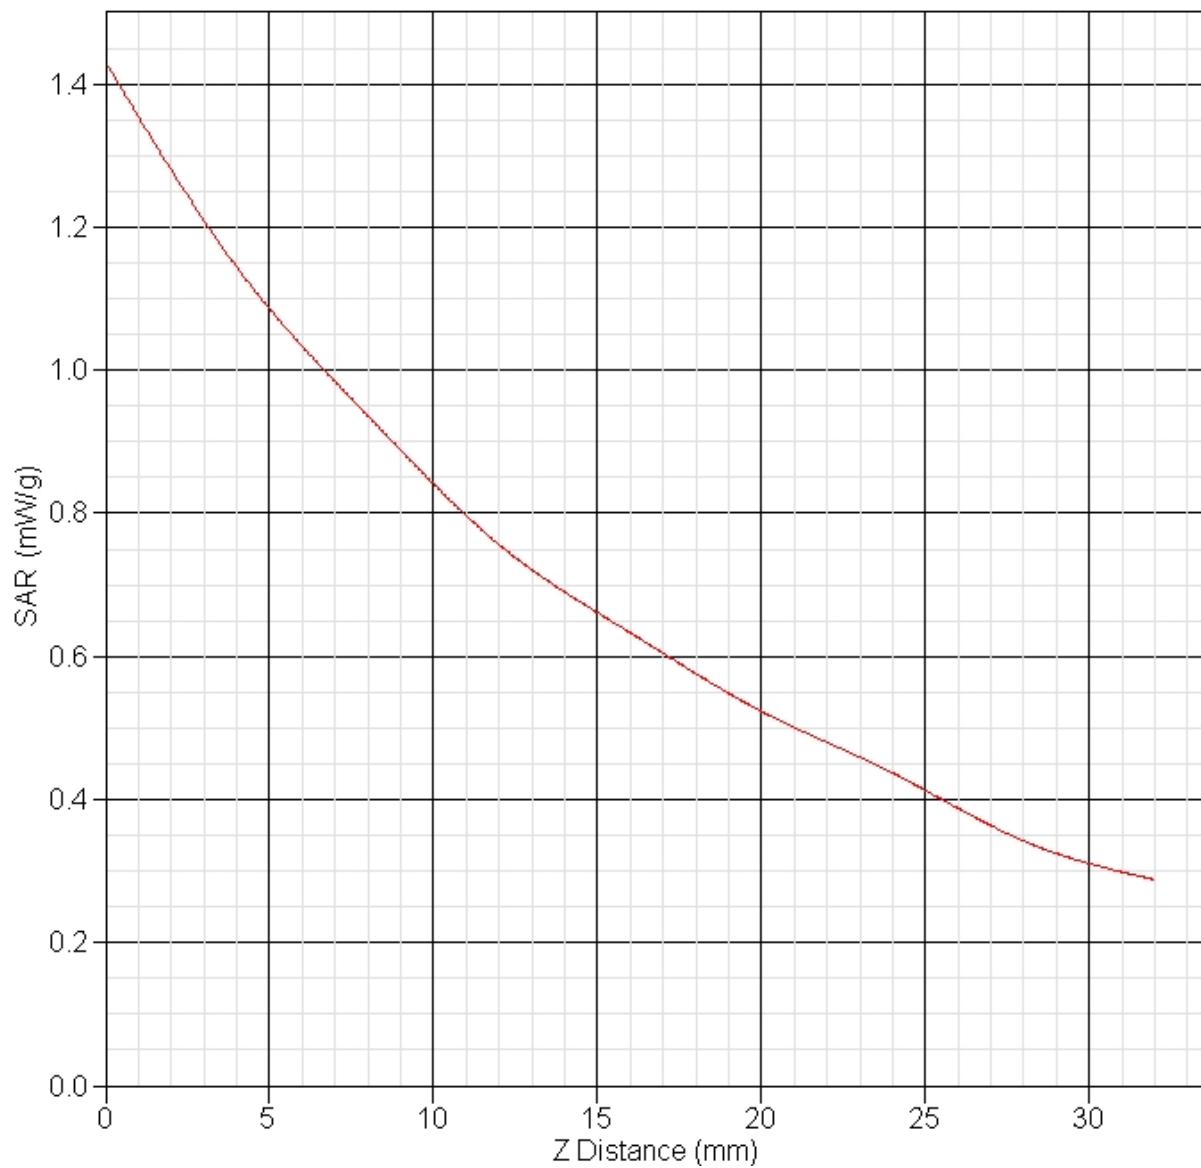

SAR Test Report

By Operator : Jay
Measurement Date : 18-Sep-2009
Starting Time : 18-Sep-2009 09:52:10 AM
End Time : 18-Sep-2009 10:08:34 AM
Scanning Time : 984 secs

Product Data

Device Name : CardioNet
Serial No. : Eng 1
Mode : EvDo Rev. 0
Model : C5
Frequency : 1900.00 MHz
Max. Transmit Pwr : 0.25 W
Drift Time : 0 min(s)
Length : 117 mm
Width : 64 mm
Depth : 23 mm
Antenna Type : Internal
Orientation : Held To Face
Power Drift-Start : 0.272 W/kg
Power Drift-Finish: 0.278 W/kg
Power Drift (%) : 2.209

Phantom Data

Name : APREL-Uni
Type : Uni-Phantom
Size (mm) : 280 x 280 x 200
Serial No. : System Default
Location : Center
Description : Uni-Phantom

Tissue Data

Type : HEAD
Serial No. : 1900
Frequency : 1900.00 MHz
Last Calib. Date : 18-Sep-2009
Temperature : 23.00 °C
Ambient Temp. : 24.00 °C
Humidity : 44.00 RH%
Epsilon : 39.75 F/m
Sigma : 1.42 S/m
Density : 1000.00 kg/cu. m

Probe Data


Name : Probe 215 - RFEL
Model : E020
Type : E-Field Triangle
Serial No. : 215
Last Calib. Date : 03-Nov-2008
Frequency : 1900.00 MHz
Duty Cycle Factor: 1
Conversion Factor: 4.9
Probe Sensitivity: 1.20 1.20 1.20 μ V/ (V/m)²
Compression Point: 95.00 mV
Offset : 1.56 mm

Measurement Data

Crest Factor : 1
 Scan Type : Complete
 Tissue Temp. : 23.00 °C
 Ambient Temp. : 24.00 °C
 Set-up Date : 18-Sep-2009
 Set-up Time : 9:03:43 AM
 Area Scan : 6x7x1 : Measurement x=15mm, y=15mm, z=4mm
 Zoom Scan : 5x5x8 : Measurement x=8mm, y=8mm, z=4mm


Other Data

DUT Position : Held To Face
 Separation : 25 mm
 Channel : Low

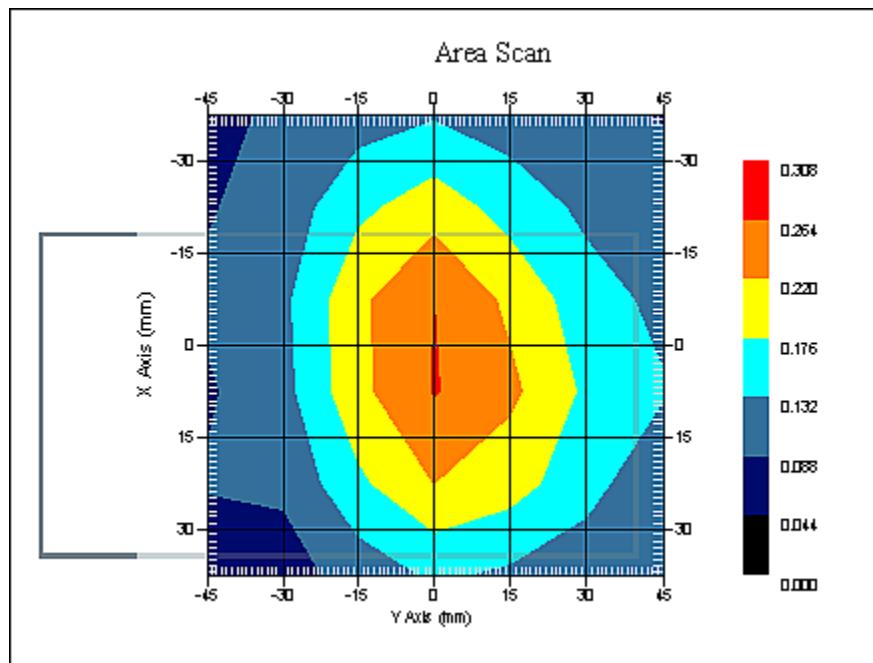

1 gram SAR value : 0.269 W/kg
 10 gram SAR value : 0.182 W/kg
 Area Scan Peak SAR : 0.267 W/kg
 Zoom Scan Peak SAR : 0.380 W/kg

SAR-Z Axis
at Hotspot x:15.08 y:-0.16

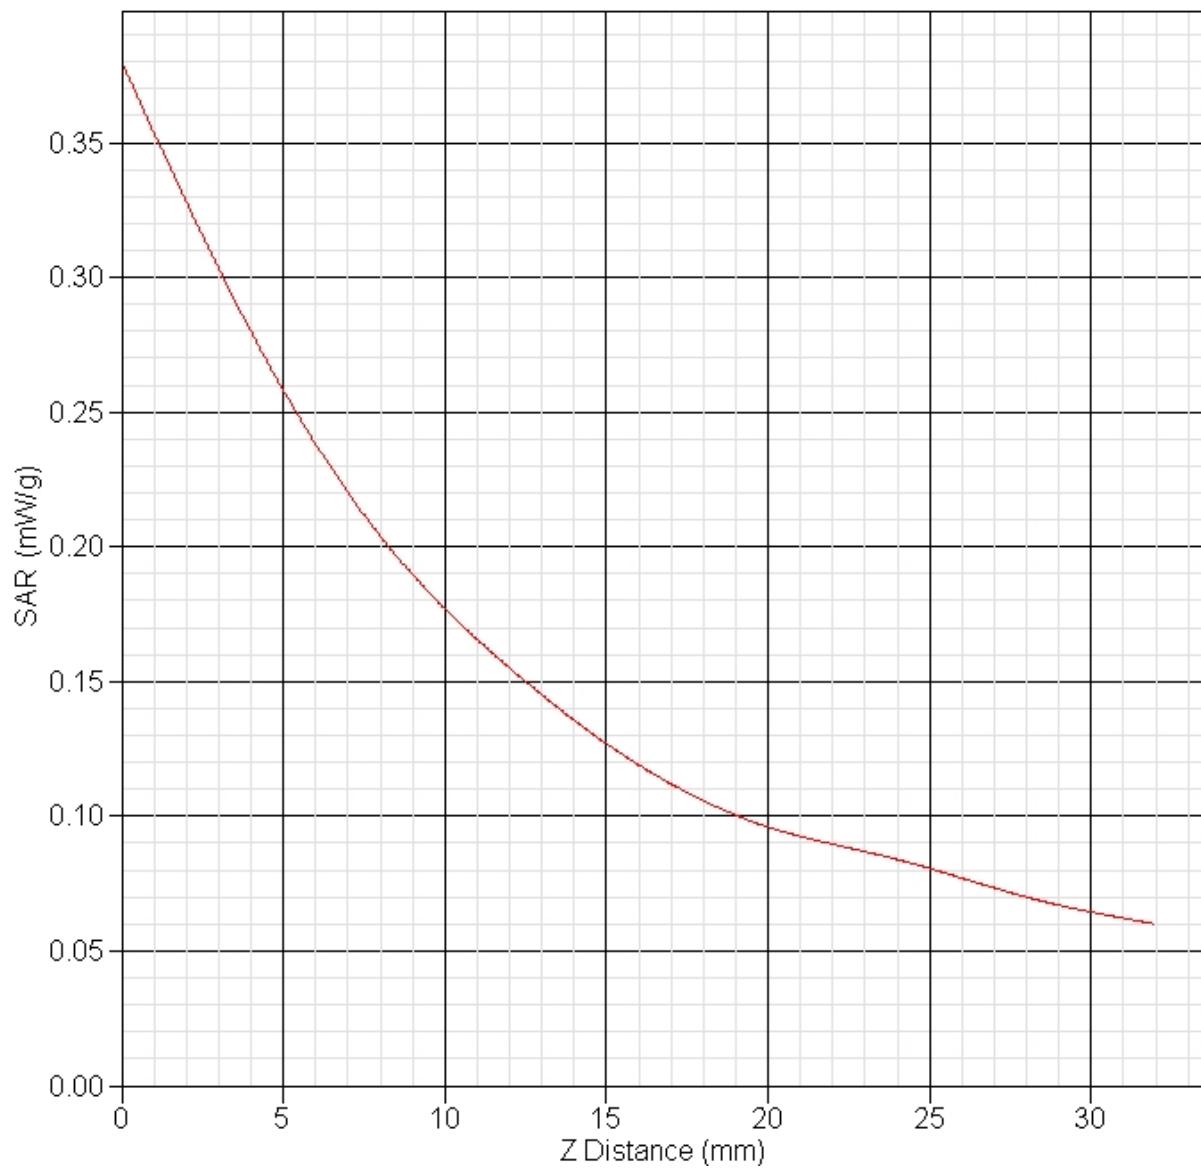

SAR Test Report

By Operator : Jay
Measurement Date : 18-Sep-2009
Starting Time : 18-Sep-2009 09:33:43 AM
End Time : 18-Sep-2009 09:50:09 AM
Scanning Time : 986 secs

Product Data

Device Name : CardioNet
Serial No. : Eng 1
Mode : EvDo Rev. 0
Model : C5
Frequency : 1900.00 MHz
Max. Transmit Pwr : 0.25 W
Drift Time : 0 min(s)
Length : 117 mm
Width : 64 mm
Depth : 23 mm
Antenna Type : Internal
Orientation : Held To Face
Power Drift-Start : 0.209 W/kg
Power Drift-Finish: 0.210 W/kg
Power Drift (%) : 0.576

Phantom Data

Name : APREL-Uni
Type : Uni-Phantom
Size (mm) : 280 x 280 x 200
Serial No. : System Default
Location : Center
Description : Uni-Phantom

Tissue Data

Type : HEAD
Serial No. : 1900
Frequency : 1900.00 MHz
Last Calib. Date : 18-Sep-2009
Temperature : 23.00 °C
Ambient Temp. : 24.00 °C
Humidity : 44.00 RH%
Epsilon : 39.75 F/m
Sigma : 1.42 S/m
Density : 1000.00 kg/cu. m

Probe Data


Name : Probe 215 - RFEL
Model : E020
Type : E-Field Triangle
Serial No. : 215
Last Calib. Date : 03-Nov-2008
Frequency : 1900.00 MHz
Duty Cycle Factor: 1
Conversion Factor: 4.9
Probe Sensitivity: 1.20 1.20 1.20 μ V/ (V/m)²
Compression Point: 95.00 mV
Offset : 1.56 mm

Measurement Data

Crest Factor : 1
 Scan Type : Complete
 Tissue Temp. : 23.00 °C
 Ambient Temp. : 24.00 °C
 Set-up Date : 18-Sep-2009
 Set-up Time : 9:03:43 AM
 Area Scan : 6x7x1 : Measurement x=15mm, y=15mm, z=4mm
 Zoom Scan : 5x5x8 : Measurement x=8mm, y=8mm, z=4mm

Other Data

DUT Position : Held To Face
 Separation : 25 mm
 Channel : Mid

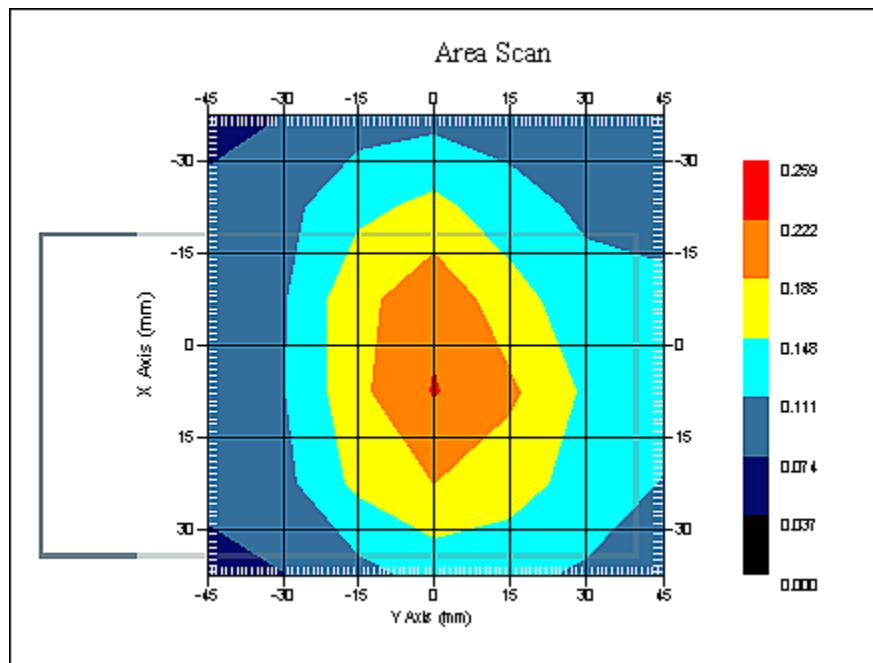

1 gram SAR value : 0.224 W/kg
 10 gram SAR value : 0.152 W/kg
 Area Scan Peak SAR : 0.225 W/kg
 Zoom Scan Peak SAR : 0.330 W/kg

SAR Test Report

By Operator : Jay
Measurement Date : 18-Sep-2009
Starting Time : 18-Sep-2009 10:09:31 AM
End Time : 18-Sep-2009 10:25:52 AM
Scanning Time : 981 secs

Product Data

Device Name : CardioNet
Serial No. : Eng 1
Mode : EvDo Rev. 0
Model : C5
Frequency : 1900.00 MHz
Max. Transmit Pwr : 0.25 W
Drift Time : 0 min(s)
Length : 117 mm
Width : 64 mm
Depth : 23 mm
Antenna Type : Internal
Orientation : Held To Face
Power Drift-Start : 0.238 W/kg
Power Drift-Finish: 0.244 W/kg
Power Drift (%) : 2.239

Phantom Data

Name : APREL-Uni
Type : Uni-Phantom
Size (mm) : 280 x 280 x 200
Serial No. : System Default
Location : Center
Description : Uni-Phantom

Tissue Data

Type : HEAD
Serial No. : 1900
Frequency : 1900.00 MHz
Last Calib. Date : 18-Sep-2009
Temperature : 23.00 °C
Ambient Temp. : 24.00 °C
Humidity : 44.00 RH%
Epsilon : 39.75 F/m
Sigma : 1.42 S/m
Density : 1000.00 kg/cu. m

Probe Data


Name : Probe 215 - RFEL
Model : E020
Type : E-Field Triangle
Serial No. : 215
Last Calib. Date : 03-Nov-2008
Frequency : 1900.00 MHz
Duty Cycle Factor: 1
Conversion Factor: 4.9
Probe Sensitivity: 1.20 1.20 1.20 μ V/ (V/m)²
Compression Point: 95.00 mV
Offset : 1.56 mm

Measurement Data

Crest Factor : 1
 Scan Type : Complete
 Tissue Temp. : 23.00 °C
 Ambient Temp. : 24.00 °C
 Set-up Date : 18-Sep-2009
 Set-up Time : 9:03:43 AM
 Area Scan : 6x7x1 : Measurement x=15mm, y=15mm, z=4mm
 Zoom Scan : 5x5x8 : Measurement x=8mm, y=8mm, z=4mm

Other Data

DUT Position : Held To Face
 Separation : 25 mm
 Channel : High

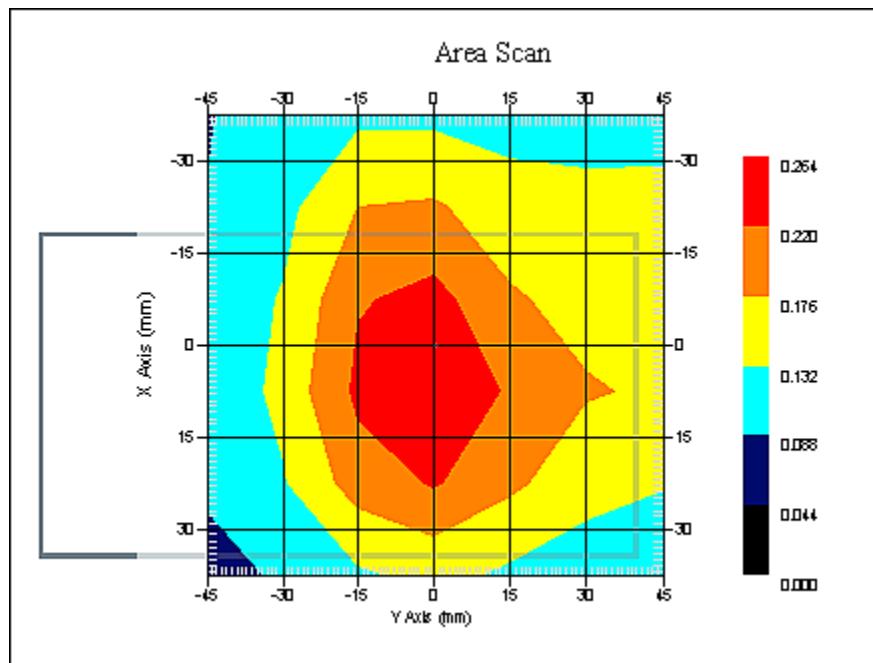

1 gram SAR value : 0.260 W/kg
 10 gram SAR value : 0.175 W/kg
 Area Scan Peak SAR : 0.264 W/kg
 Zoom Scan Peak SAR : 0.390 W/kg

SAR Test Report

By Operator : Jay
Measurement Date : 18-Sep-2009
Starting Time : 18-Sep-2009 01:56:41 PM
End Time : 18-Sep-2009 02:12:57 PM
Scanning Time : 976 secs

Product Data

Device Name : CardioNet
Serial No. : Eng 1
Mode : EvDo Rev. 0
Model : C5
Frequency : 1900.00 MHz
Max. Transmit Pwr : 0.25 W
Drift Time : 0 min(s)
Length : 117 mm
Width : 64 mm
Depth : 23 mm
Antenna Type : Internal
Orientation : Front
Power Drift-Start : 0.445 W/kg
Power Drift-Finish: 0.445 W/kg
Power Drift (%) : 0.185

Phantom Data

Name : APREL-Uni
Type : Uni-Phantom
Size (mm) : 280 x 280 x 200
Serial No. : System Default
Location : Center
Description : Uni-Phantom

Tissue Data

Type : BODY
Serial No. : 1900
Frequency : 1900.00 MHz
Last Calib. Date : 18-Sep-2009
Temperature : 23.00 °C
Ambient Temp. : 24.00 °C
Humidity : 44.00 RH%
Epsilon : 52.73 F/m
Sigma : 1.58 S/m
Density : 1000.00 kg/cu. m

Probe Data


Name : Probe 215 - RFEL
Model : E020
Type : E-Field Triangle
Serial No. : 215
Last Calib. Date : 03-Nov-2008
Frequency : 1900.00 MHz
Duty Cycle Factor: 1
Conversion Factor: 5
Probe Sensitivity: 1.20 1.20 1.20 μ V/ (V/m)²
Compression Point: 95.00 mV
Offset : 1.56 mm

Measurement Data

Crest Factor : 1
Scan Type : Complete
Tissue Temp. : 23.00 °C
Ambient Temp. : 24.00 °C
Set-up Date : 18-Sep-2009
Set-up Time : 11:46:48 AM
Area Scan : 6x7x1 : Measurement x=15mm, y=15mm, z=4mm
Zoom Scan : 5x5x8 : Measurement x=8mm, y=8mm, z=4mm

Other Data

DUT Position : Front
Separation : 10 mm
Channel : Low

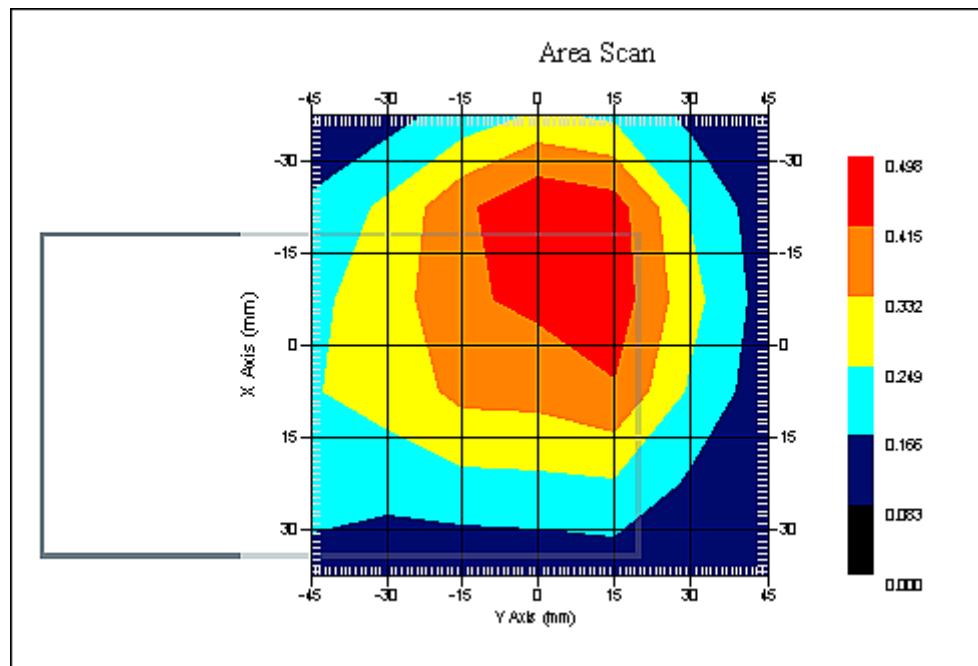

1 gram SAR value : 0.514 W/kg
10 gram SAR value : 0.331 W/kg
Area Scan Peak SAR : 0.495 W/kg
Zoom Scan Peak SAR : 0.780 W/kg

SAR Test Report

By Operator : Jay
Measurement Date : 18-Sep-2009
Starting Time : 18-Sep-2009 12:27:23 PM
End Time : 18-Sep-2009 12:43:46 PM
Scanning Time : 983 secs

Product Data

Device Name : CardioNet
Serial No. : Eng 1
Mode : EvDo Rev. 0
Model : C5
Frequency : 1900.00 MHz
Max. Transmit Pwr : 0.25 W
Drift Time : 0 min(s)
Length : 117 mm
Width : 64 mm
Depth : 23 mm
Antenna Type : Internal
Orientation : Front
Power Drift-Start : 0.417 W/kg
Power Drift-Finish: 0.402 W/kg
Power Drift (%) : -3.487

Phantom Data

Name : APREL-Uni
Type : Uni-Phantom
Size (mm) : 280 x 280 x 200
Serial No. : System Default
Location : Center
Description : Uni-Phantom

Tissue Data

Type : BODY
Serial No. : 1900
Frequency : 1900.00 MHz
Last Calib. Date : 18-Sep-2009
Temperature : 23.00 °C
Ambient Temp. : 24.00 °C
Humidity : 44.00 RH%
Epsilon : 52.73 F/m
Sigma : 1.58 S/m
Density : 1000.00 kg/cu. m

Probe Data


Name : Probe 215 - RFEL
Model : E020
Type : E-Field Triangle
Serial No. : 215
Last Calib. Date : 03-Nov-2008
Frequency : 1900.00 MHz
Duty Cycle Factor: 1
Conversion Factor: 5
Probe Sensitivity: 1.20 1.20 1.20 μ V/ (V/m)²
Compression Point: 95.00 mV
Offset : 1.56 mm

Measurement Data

Crest Factor : 1
Scan Type : Complete
Tissue Temp. : 23.00 °C
Ambient Temp. : 24.00 °C
Set-up Date : 18-Sep-2009
Set-up Time : 11:46:48 AM
Area Scan : 6x7x1 : Measurement x=15mm, y=15mm, z=4mm
Zoom Scan : 5x5x8 : Measurement x=8mm, y=8mm, z=4mm

Other Data

DUT Position : Front
Separation : 10 mm
Channel : Mid

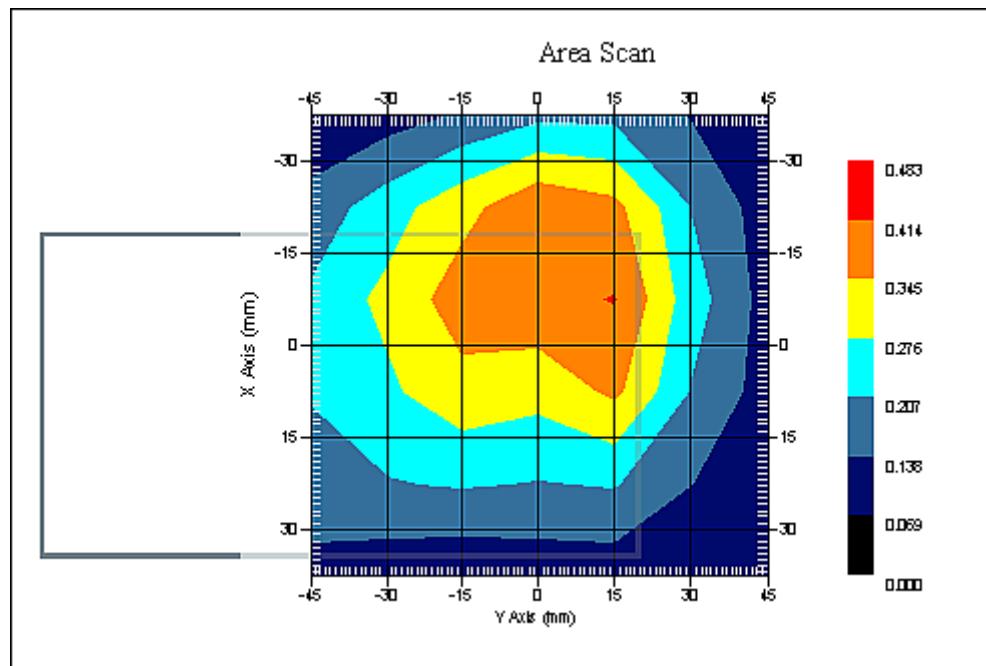

1 gram SAR value : 0.417 W/kg
10 gram SAR value : 0.275 W/kg
Area Scan Peak SAR : 0.417 W/kg
Zoom Scan Peak SAR : 0.620 W/kg

SAR Test Report

By Operator : Jay
Measurement Date : 18-Sep-2009
Starting Time : 18-Sep-2009 01:39:49 PM
End Time : 18-Sep-2009 01:55:54 PM
Scanning Time : 965 secs

Product Data

Device Name : CardioNet
Serial No. : Eng 1
Mode : EvDo Rev. 0
Model : C5
Frequency : 1900.00 MHz
Max. Transmit Pwr : 0.25 W
Drift Time : 0 min(s)
Length : 117 mm
Width : 64 mm
Depth : 23 mm
Antenna Type : Internal
Orientation : Front
Power Drift-Start : 0.551 W/kg
Power Drift-Finish: 0.557 W/kg
Power Drift (%) : 1.056

Phantom Data

Name : APREL-Uni
Type : Uni-Phantom
Size (mm) : 280 x 280 x 200
Serial No. : System Default
Location : Center
Description : Uni-Phantom

Tissue Data

Type : BODY
Serial No. : 1900
Frequency : 1900.00 MHz
Last Calib. Date : 18-Sep-2009
Temperature : 23.00 °C
Ambient Temp. : 24.00 °C
Humidity : 44.00 RH%
Epsilon : 52.73 F/m
Sigma : 1.58 S/m
Density : 1000.00 kg/cu. m

Probe Data


Name : Probe 215 - RFEL
Model : E020
Type : E-Field Triangle
Serial No. : 215
Last Calib. Date : 03-Nov-2008
Frequency : 1900.00 MHz
Duty Cycle Factor: 1
Conversion Factor: 5
Probe Sensitivity: 1.20 1.20 1.20 μ V/ (V/m)²
Compression Point: 95.00 mV
Offset : 1.56 mm

Measurement Data

Crest Factor : 1
Scan Type : Complete
Tissue Temp. : 23.00 °C
Ambient Temp. : 24.00 °C
Set-up Date : 18-Sep-2009
Set-up Time : 11:46:48 AM
Area Scan : 6x7x1 : Measurement x=15mm, y=15mm, z=4mm
Zoom Scan : 5x5x8 : Measurement x=8mm, y=8mm, z=4mm

Other Data

DUT Position : Front
Separation : 10 mm
Channel : High

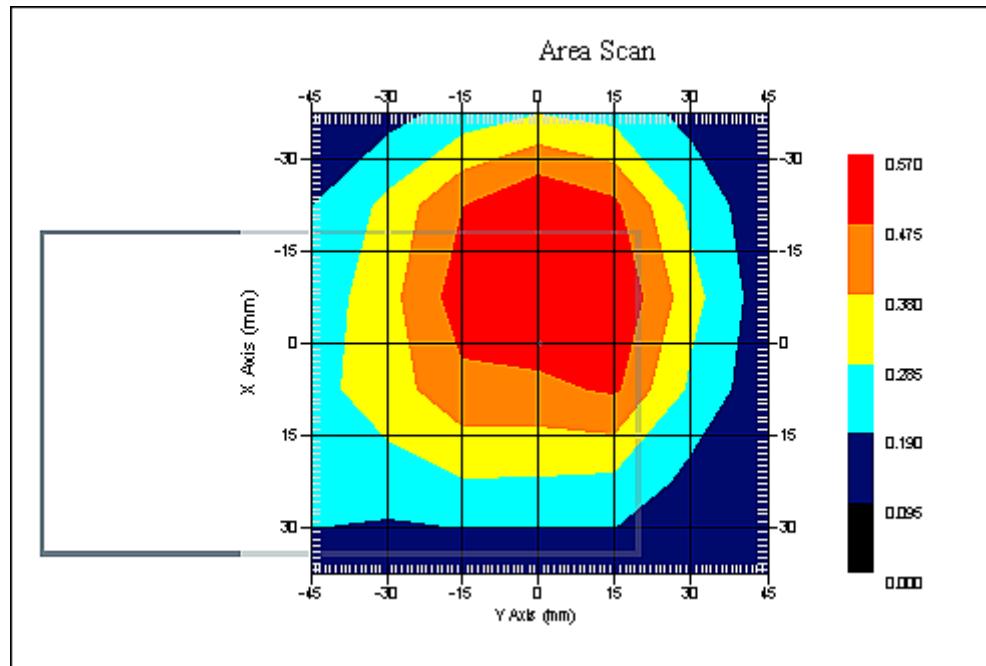

1 gram SAR value : 0.568 W/kg
10 gram SAR value : 0.366 W/kg
Area Scan Peak SAR : 0.570 W/kg
Zoom Scan Peak SAR : 0.850 W/kg

SAR Test Report

By Operator : Jay
Measurement Date : 18-Sep-2009
Starting Time : 18-Sep-2009 01:03:32 PM
End Time : 18-Sep-2009 01:19:45 PM
Scanning Time : 973 secs

Product Data

Device Name : CardioNet
Serial No. : Eng 1
Mode : EvDo Rev. 0
Model : C5
Frequency : 1900.00 MHz
Max. Transmit Pwr : 0.25 W
Drift Time : 0 min(s)
Length : 117 mm
Width : 64 mm
Depth : 23 mm
Antenna Type : Internal
Orientation : Back
Power Drift-Start : 0.512 W/kg
Power Drift-Finish: 0.517 W/kg
Power Drift (%) : 0.972

Phantom Data

Name : APREL-Uni
Type : Uni-Phantom
Size (mm) : 280 x 280 x 200
Serial No. : System Default
Location : Center
Description : Uni-Phantom

Tissue Data

Type : BODY
Serial No. : 1900
Frequency : 1900.00 MHz
Last Calib. Date : 18-Sep-2009
Temperature : 23.00 °C
Ambient Temp. : 24.00 °C
Humidity : 44.00 RH%
Epsilon : 52.73 F/m
Sigma : 1.58 S/m
Density : 1000.00 kg/cu. m

Probe Data


Name : Probe 215 - RFEL
Model : E020
Type : E-Field Triangle
Serial No. : 215
Last Calib. Date : 03-Nov-2008
Frequency : 1900.00 MHz
Duty Cycle Factor: 1
Conversion Factor: 5
Probe Sensitivity: 1.20 1.20 1.20 μ V/ (V/m)²
Compression Point: 95.00 mV
Offset : 1.56 mm

Measurement Data

Crest Factor : 1
Scan Type : Complete
Tissue Temp. : 23.00 °C
Ambient Temp. : 24.00 °C
Set-up Date : 18-Sep-2009
Set-up Time : 11:46:48 AM
Area Scan : 6x7x1 : Measurement x=15mm, y=15mm, z=4mm
Zoom Scan : 5x5x8 : Measurement x=8mm, y=8mm, z=4mm

Other Data

DUT Position : Back
Separation : 10 mm
Channel : Low

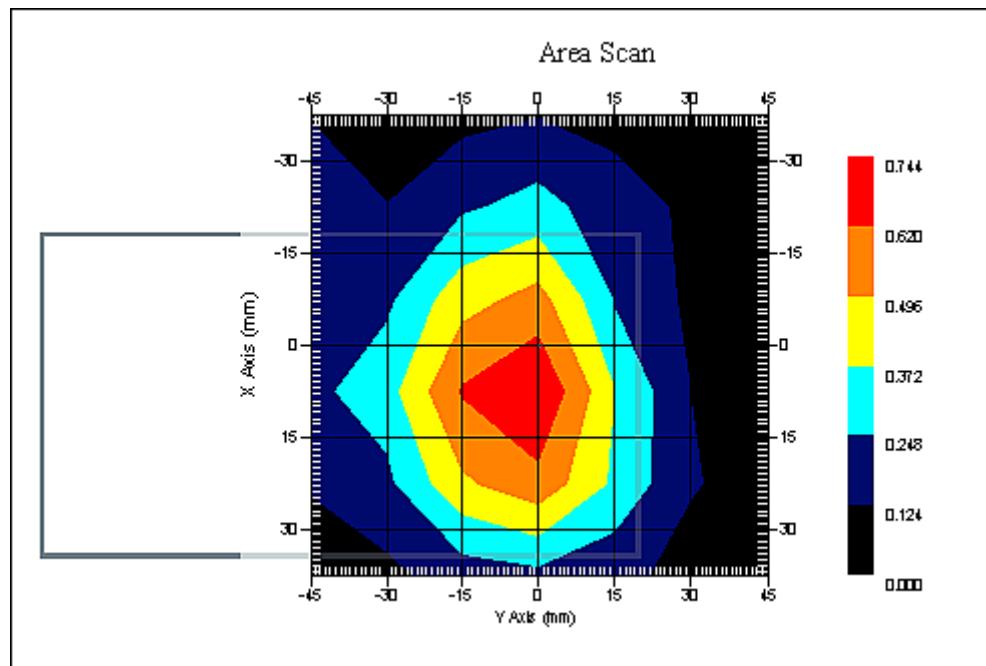

1 gram SAR value : 0.749 W/kg
10 gram SAR value : 0.456 W/kg
Area Scan Peak SAR : 0.742 W/kg
Zoom Scan Peak SAR : 1.191 W/kg

SAR Test Report

By Operator : Jay
Measurement Date : 18-Sep-2009
Starting Time : 18-Sep-2009 12:44:49 PM
End Time : 18-Sep-2009 01:01:08 PM
Scanning Time : 979 secs

Product Data

Device Name : CardioNet
Serial No. : Eng 1
Mode : EvDo Rev. 0
Model : C5
Frequency : 1900.00 MHz
Max. Transmit Pwr : 0.25 W
Drift Time : 0 min(s)
Length : 117 mm
Width : 64 mm
Depth : 23 mm
Antenna Type : Internal
Orientation : Back
Power Drift-Start : 0.493 W/kg
Power Drift-Finish: 0.502 W/kg
Power Drift (%) : 1.827

Phantom Data

Name : APREL-Uni
Type : Uni-Phantom
Size (mm) : 280 x 280 x 200
Serial No. : System Default
Location : Center
Description : Uni-Phantom

Tissue Data

Type : BODY
Serial No. : 1900
Frequency : 1900.00 MHz
Last Calib. Date : 18-Sep-2009
Temperature : 23.00 °C
Ambient Temp. : 24.00 °C
Humidity : 44.00 RH%
Epsilon : 52.73 F/m
Sigma : 1.58 S/m
Density : 1000.00 kg/cu. m

Probe Data


Name : Probe 215 - RFEL
Model : E020
Type : E-Field Triangle
Serial No. : 215
Last Calib. Date : 03-Nov-2008
Frequency : 1900.00 MHz
Duty Cycle Factor: 1
Conversion Factor: 5
Probe Sensitivity: 1.20 1.20 1.20 μ V/ (V/m)²
Compression Point: 95.00 mV
Offset : 1.56 mm

Measurement Data

Crest Factor : 1
Scan Type : Complete
Tissue Temp. : 23.00 °C
Ambient Temp. : 24.00 °C
Set-up Date : 18-Sep-2009
Set-up Time : 11:46:48 AM
Area Scan : 6x7x1 : Measurement x=15mm, y=15mm, z=4mm
Zoom Scan : 5x5x8 : Measurement x=8mm, y=8mm, z=4mm

Other Data

DUT Position : Back
Separation : 10 mm
Channel : Mid

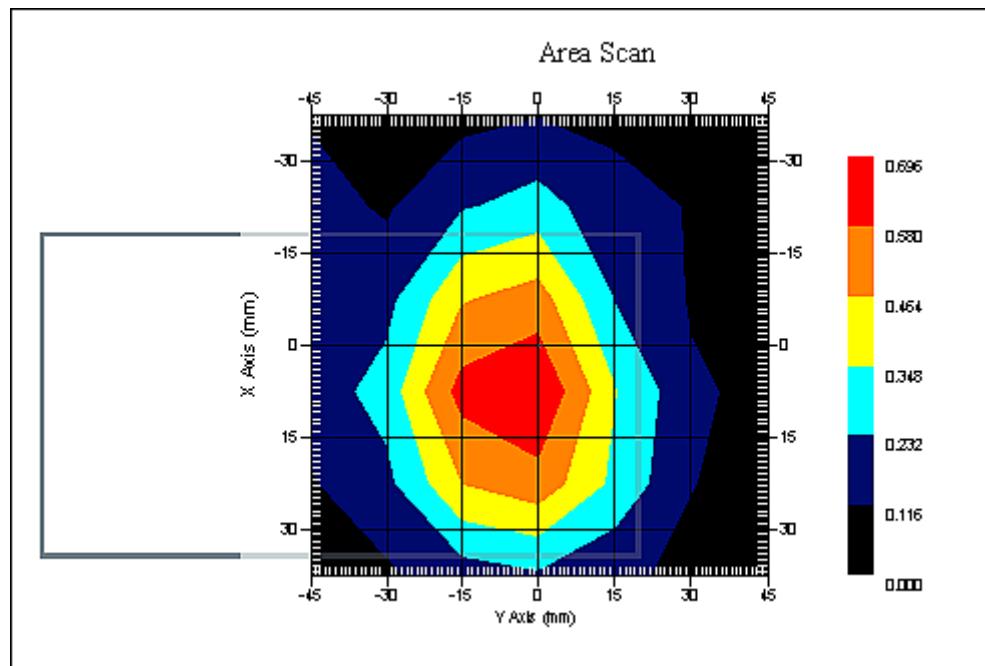

1 gram SAR value : 0.651 W/kg
10 gram SAR value : 0.397 W/kg
Area Scan Peak SAR : 0.695 W/kg
Zoom Scan Peak SAR : 1.020 W/kg

SAR Test Report

By Operator : Jay
Measurement Date : 18-Sep-2009
Starting Time : 18-Sep-2009 01:21:16 PM
End Time : 18-Sep-2009 01:37:45 PM
Scanning Time : 989 secs

Product Data

Device Name : CardioNet
Serial No. : Eng 1
Mode : EvDo Rev. 0
Model : C5
Frequency : 1900.00 MHz
Max. Transmit Pwr : 0.25 W
Drift Time : 0 min(s)
Length : 117 mm
Width : 64 mm
Depth : 23 mm
Antenna Type : Internal
Orientation : Back
Power Drift-Start : 0.729 W/kg
Power Drift-Finish: 0.750 W/kg
Power Drift (%) : 2.867

Phantom Data

Name : APREL-Uni
Type : Uni-Phantom
Size (mm) : 280 x 280 x 200
Serial No. : System Default
Location : Center
Description : Uni-Phantom

Tissue Data

Type : BODY
Serial No. : 1900
Frequency : 1900.00 MHz
Last Calib. Date : 18-Sep-2009
Temperature : 23.00 °C
Ambient Temp. : 24.00 °C
Humidity : 44.00 RH%
Epsilon : 52.73 F/m
Sigma : 1.58 S/m
Density : 1000.00 kg/cu. m

Probe Data


Name : Probe 215 - RFEL
Model : E020
Type : E-Field Triangle
Serial No. : 215
Last Calib. Date : 03-Nov-2008
Frequency : 1900.00 MHz
Duty Cycle Factor: 1
Conversion Factor: 5
Probe Sensitivity: 1.20 1.20 1.20 μ V/ (V/m)²
Compression Point: 95.00 mV
Offset : 1.56 mm

Measurement Data

Crest Factor : 1
Scan Type : Complete
Tissue Temp. : 23.00 °C
Ambient Temp. : 24.00 °C
Set-up Date : 18-Sep-2009
Set-up Time : 11:46:48 AM
Area Scan : 6x7x1 : Measurement x=15mm, y=15mm, z=4mm
Zoom Scan : 5x5x8 : Measurement x=8mm, y=8mm, z=4mm


Other Data

DUT Position : Back
Separation : 10 mm
Channel : High

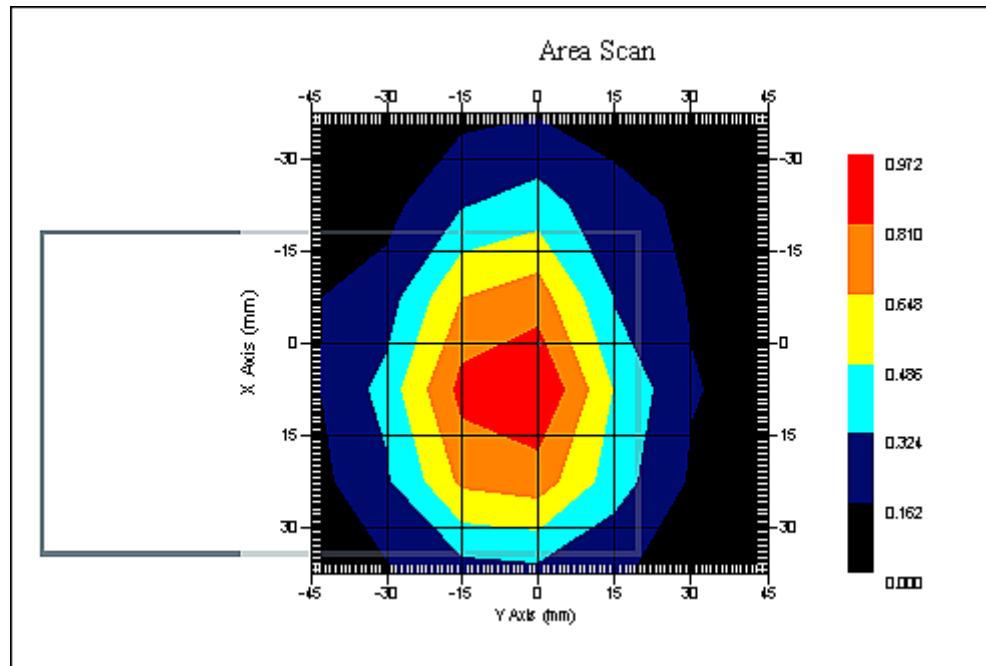

1 gram SAR value : 0.897 W/kg
10 gram SAR value : 0.542 W/kg
Area Scan Peak SAR : 0.972 W/kg
Zoom Scan Peak SAR : 1.331 W/kg

SAR-Z Axis
at Hotspot x:15.08 y:-8.14

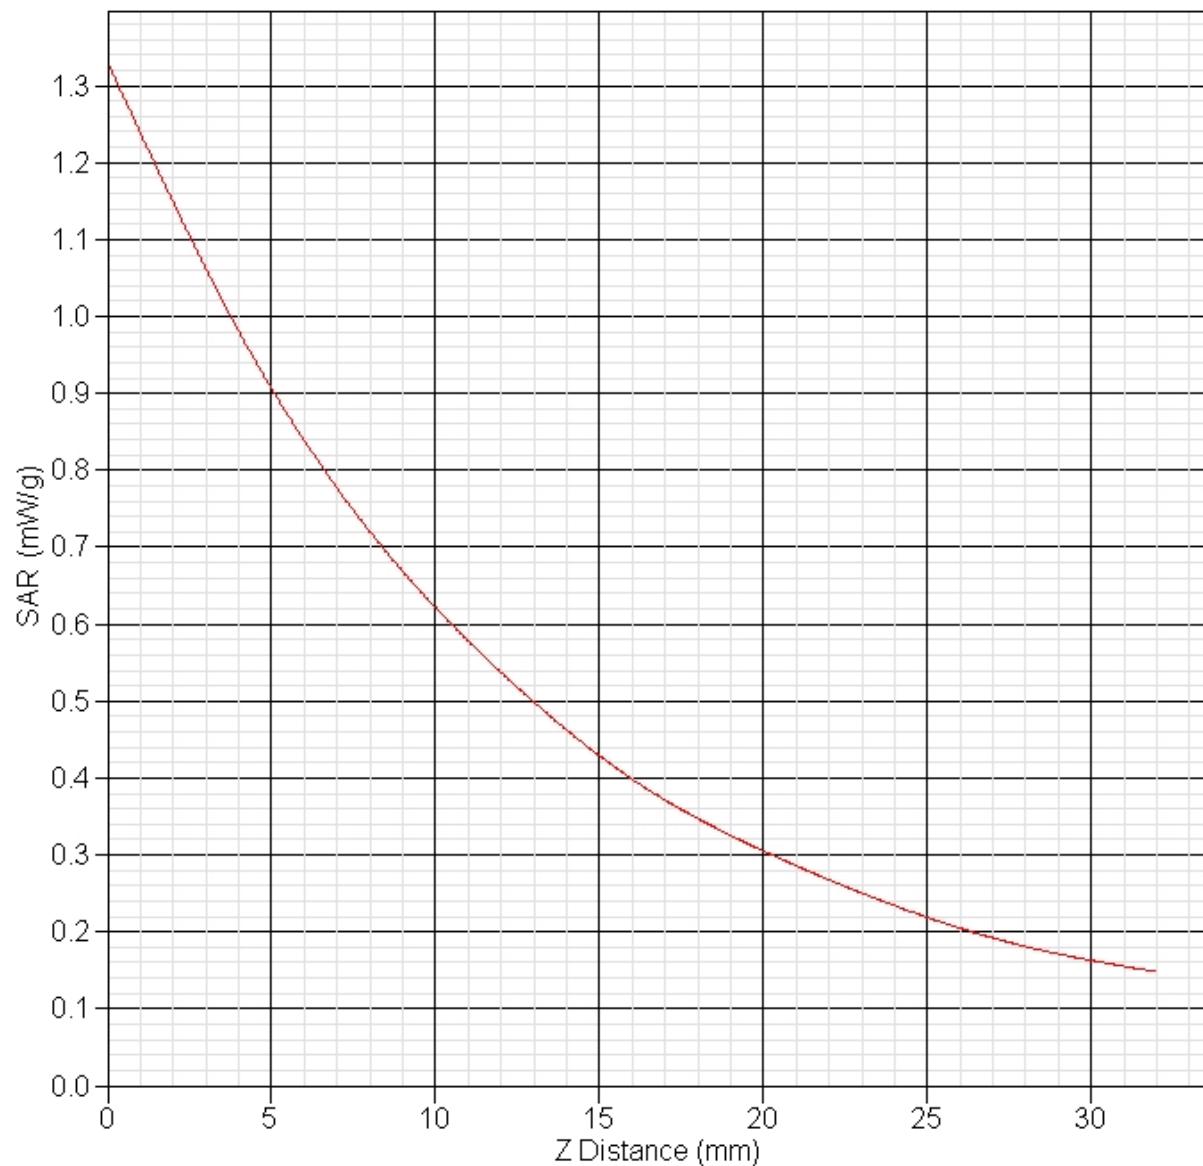

SAR Test Report

By Operator : Jay
Measurement Date : 18-Sep-2009
Starting Time : 18-Sep-2009 11:10:01 AM
End Time : 18-Sep-2009 11:26:12 AM
Scanning Time : 971 secs

Product Data

Device Name : CardioNet
Serial No. : Eng 2
Mode : GSM
Model : C5
Frequency : 1900.00 MHz
Max. Transmit Pwr : 1 W
Drift Time : 0 min(s)
Length : 117 mm
Width : 64 mm
Depth : 23 mm
Antenna Type : Internal
Orientation : Held To Face
Power Drift-Start : 0.235 W/kg
Power Drift-Finish: 0.245 W/kg
Power Drift (%) : 4.476

Phantom Data

Name : APREL-Uni
Type : Uni-Phantom
Size (mm) : 280 x 280 x 200
Serial No. : System Default
Location : Center
Description : Uni-Phantom

Tissue Data

Type : HEAD
Serial No. : 1900
Frequency : 1900.00 MHz
Last Calib. Date : 18-Sep-2009
Temperature : 23.00 °C
Ambient Temp. : 24.00 °C
Humidity : 44.00 RH%
Epsilon : 39.75 F/m
Sigma : 1.42 S/m
Density : 1000.00 kg/cu. m

Probe Data


Name : Probe 215 - RFEL
Model : E020
Type : E-Field Triangle
Serial No. : 215
Last Calib. Date : 03-Nov-2008
Frequency : 1900.00 MHz
Duty Cycle Factor: 8
Conversion Factor: 4.9
Probe Sensitivity: 1.20 1.20 1.20 μ V/ (V/m)²
Compression Point: 95.00 mV
Offset : 1.56 mm

Measurement Data

Crest Factor : 8
 Scan Type : Complete
 Tissue Temp. : 23.00 °C
 Ambient Temp. : 24.00 °C
 Set-up Date : 18-Sep-2009
 Set-up Time : 9:03:43 AM
 Area Scan : 6x7x1 : Measurement x=15mm, y=15mm, z=4mm
 Zoom Scan : 5x5x8 : Measurement x=8mm, y=8mm, z=4mm


Other Data

DUT Position : Held To Face
 Separation : 25 mm
 Channel : Low

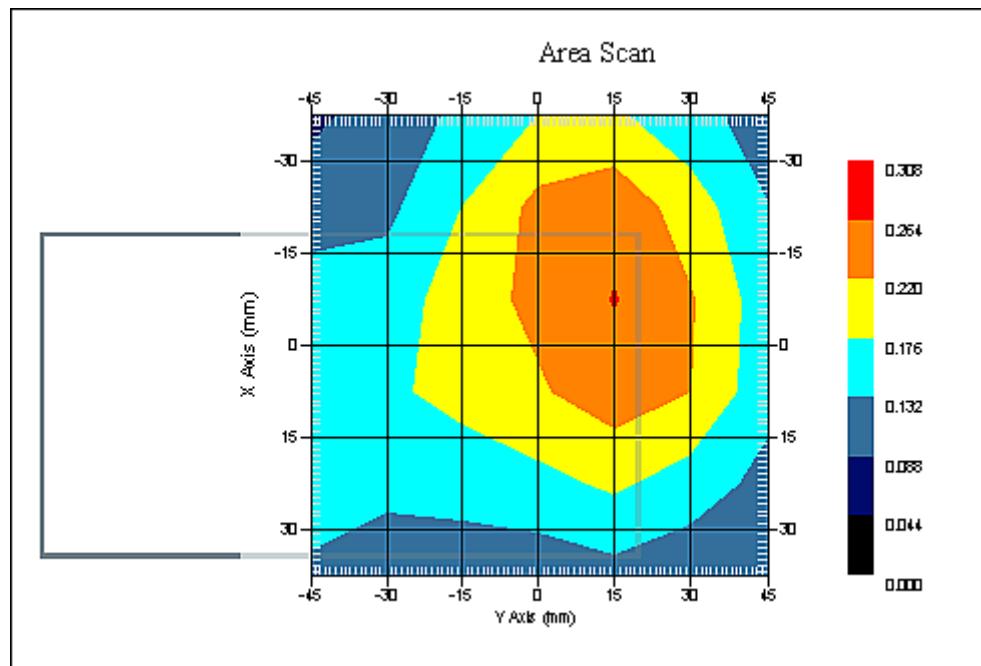

1 gram SAR value : 0.252 W/kg
 10 gram SAR value : 0.173 W/kg
 Area Scan Peak SAR : 0.266 W/kg
 Zoom Scan Peak SAR : 0.370 W/kg

SAR-Z Axis
at Hotspot x:0.04 y:14.87

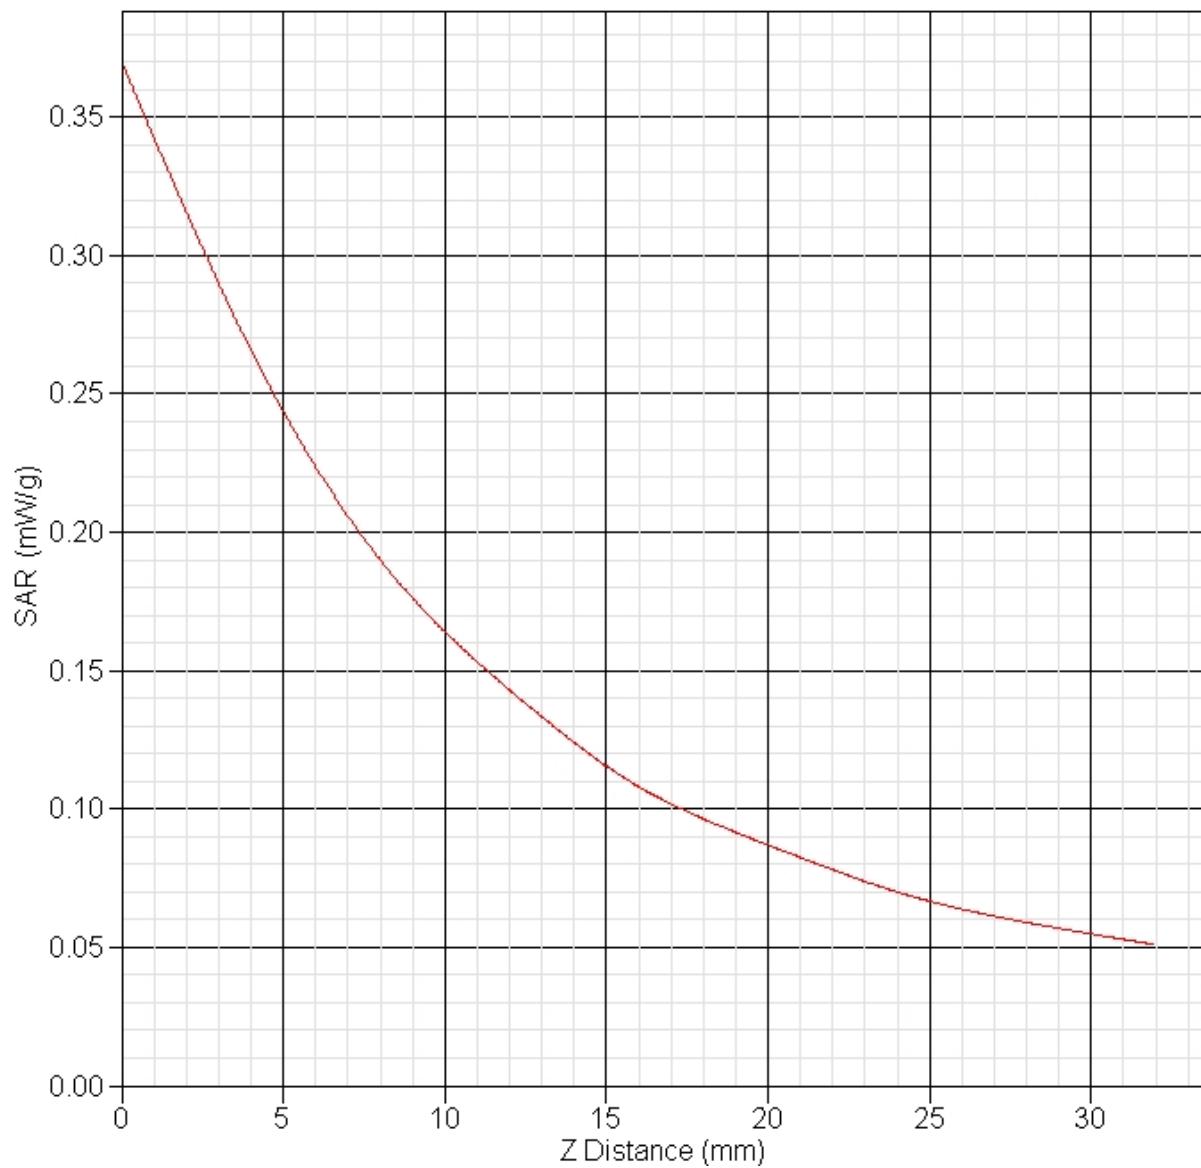

SAR Test Report

By Operator : Jay
Measurement Date : 18-Sep-2009
Starting Time : 18-Sep-2009 10:52:37 AM
End Time : 18-Sep-2009 11:08:58 AM
Scanning Time : 981 secs

Product Data

Device Name : CardioNet
Serial No. : Eng 2
Mode : GSM
Model : C5
Frequency : 1900.00 MHz
Max. Transmit Pwr : 1 W
Drift Time : 0 min(s)
Length : 117 mm
Width : 64 mm
Depth : 23 mm
Antenna Type : Internal
Orientation : Held To Face
Power Drift-Start : 0.211 W/kg
Power Drift-Finish: 0.210 W/kg
Power Drift (%) : -0.653

Phantom Data

Name : APREL-Uni
Type : Uni-Phantom
Size (mm) : 280 x 280 x 200
Serial No. : System Default
Location : Center
Description : Uni-Phantom

Tissue Data

Type : HEAD
Serial No. : 1900
Frequency : 1900.00 MHz
Last Calib. Date : 18-Sep-2009
Temperature : 23.00 °C
Ambient Temp. : 24.00 °C
Humidity : 44.00 RH%
Epsilon : 39.75 F/m
Sigma : 1.42 S/m
Density : 1000.00 kg/cu. m

Probe Data


Name : Probe 215 - RFEL
Model : E020
Type : E-Field Triangle
Serial No. : 215
Last Calib. Date : 03-Nov-2008
Frequency : 1900.00 MHz
Duty Cycle Factor: 8
Conversion Factor: 4.9
Probe Sensitivity: 1.20 1.20 1.20 μ V/ (V/m)²
Compression Point: 95.00 mV
Offset : 1.56 mm

Measurement Data

Crest Factor : 8
 Scan Type : Complete
 Tissue Temp. : 23.00 °C
 Ambient Temp. : 24.00 °C
 Set-up Date : 18-Sep-2009
 Set-up Time : 9:03:43 AM
 Area Scan : 6x7x1 : Measurement x=15mm, y=15mm, z=4mm
 Zoom Scan : 5x5x8 : Measurement x=8mm, y=8mm, z=4mm

Other Data

DUT Position : Held To Face
 Separation : 25 mm
 Channel : Mid

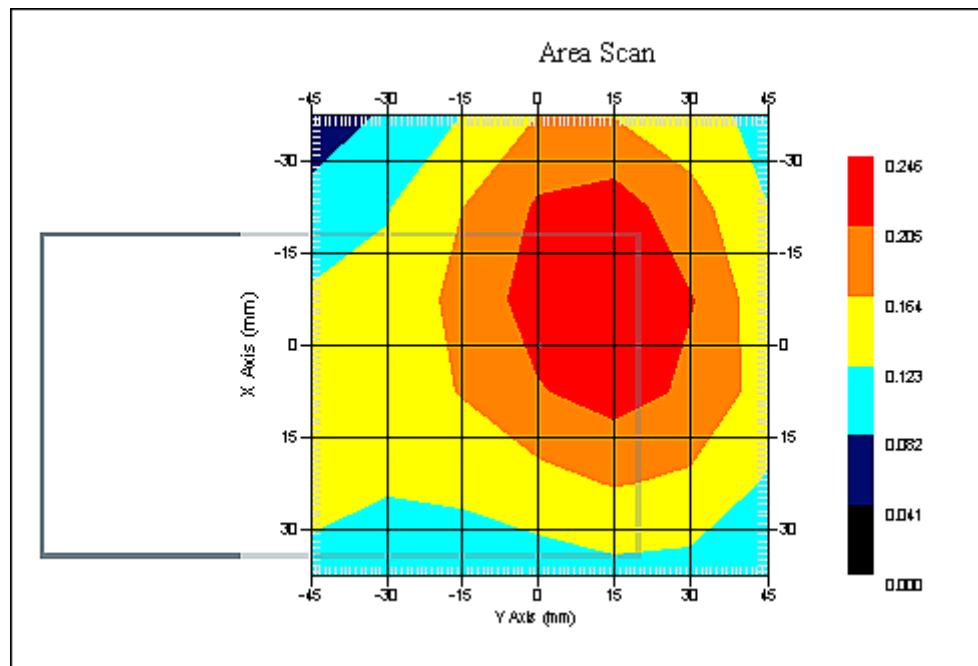

1 gram SAR value : 0.234 W/kg
 10 gram SAR value : 0.158 W/kg
 Area Scan Peak SAR : 0.243 W/kg
 Zoom Scan Peak SAR : 0.350 W/kg

SAR Test Report

By Operator : Jay
Measurement Date : 18-Sep-2009
Starting Time : 18-Sep-2009 11:46:58 AM
End Time : 18-Sep-2009 12:03:21 PM
Scanning Time : 983 secs

Product Data

Device Name : CardioNet
Serial No. : Eng 2
Mode : GSM
Model : C5
Frequency : 1900.00 MHz
Max. Transmit Pwr : 1 W
Drift Time : 0 min(s)
Length : 117 mm
Width : 64 mm
Depth : 23 mm
Antenna Type : Internal
Orientation : Held To Face
Power Drift-Start : 0.190 W/kg
Power Drift-Finish: 0.192 W/kg
Power Drift (%) : 1.152

Phantom Data

Name : APREL-Uni
Type : Uni-Phantom
Size (mm) : 280 x 280 x 200
Serial No. : System Default
Location : Center
Description : Uni-Phantom

Tissue Data

Type : HEAD
Serial No. : 1900
Frequency : 1900.00 MHz
Last Calib. Date : 18-Sep-2009
Temperature : 23.00 °C
Ambient Temp. : 24.00 °C
Humidity : 44.00 RH%
Epsilon : 39.75 F/m
Sigma : 1.42 S/m
Density : 1000.00 kg/cu. m

Probe Data


Name : Probe 215 - RFEL
Model : E020
Type : E-Field Triangle
Serial No. : 215
Last Calib. Date : 03-Nov-2008
Frequency : 1900.00 MHz
Duty Cycle Factor: 8
Conversion Factor: 4.9
Probe Sensitivity: 1.20 1.20 1.20 μ V/ (V/m)²
Compression Point: 95.00 mV
Offset : 1.56 mm

Measurement Data

Crest Factor : 8
 Scan Type : Complete
 Tissue Temp. : 23.00 °C
 Ambient Temp. : 24.00 °C
 Set-up Date : 18-Sep-2009
 Set-up Time : 11:46:48 AM
 Area Scan : 6x7x1 : Measurement x=15mm, y=15mm, z=4mm
 Zoom Scan : 5x5x8 : Measurement x=8mm, y=8mm, z=4mm

Other Data

DUT Position : Held To Face
 Separation : 25 mm
 Channel : High

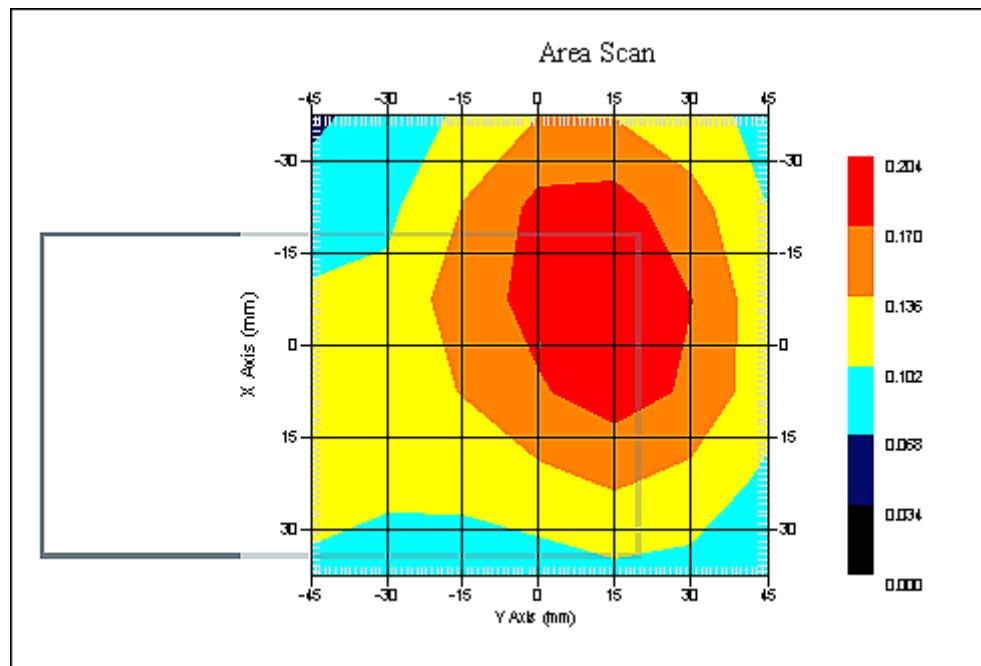

1 gram SAR value : 0.205 W/kg
 10 gram SAR value : 0.142 W/kg
 Area Scan Peak SAR : 0.201 W/kg
 Zoom Scan Peak SAR : 0.300 W/kg

SAR Test Report

By Operator : Jay
Measurement Date : 18-Sep-2009
Starting Time : 18-Sep-2009 02:32:41 PM
End Time : 18-Sep-2009 02:48:59 PM
Scanning Time : 978 secs

Product Data

Device Name : CardioNet
Serial No. : Eng 2
Mode : GPRS
Model : C5
Frequency : 1900.00 MHz
Max. Transmit Pwr : 1 W
Drift Time : 0 min(s)
Length : 117 mm
Width : 64 mm
Depth : 23 mm
Antenna Type : Internal
Orientation : Front
Power Drift-Start : 0.482 W/kg
Power Drift-Finish: 0.468 W/kg
Power Drift (%) : -2.928

Phantom Data

Name : APREL-Uni
Type : Uni-Phantom
Size (mm) : 280 x 280 x 200
Serial No. : System Default
Location : Center
Description : Uni-Phantom

Tissue Data

Type : BODY
Serial No. : 1900
Frequency : 1900.00 MHz
Last Calib. Date : 18-Sep-2009
Temperature : 23.00 °C
Ambient Temp. : 24.00 °C
Humidity : 44.00 RH%
Epsilon : 52.73 F/m
Sigma : 1.58 S/m
Density : 1000.00 kg/cu. m

Probe Data


Name : Probe 215 - RFEL
Model : E020
Type : E-Field Triangle
Serial No. : 215
Last Calib. Date : 03-Nov-2008
Frequency : 1900.00 MHz
Duty Cycle Factor: 4
Conversion Factor: 5
Probe Sensitivity: 1.20 1.20 1.20 μ V/ (V/m)²
Compression Point: 95.00 mV
Offset : 1.56 mm

Measurement Data

Crest Factor : 4
Scan Type : Complete
Tissue Temp. : 23.00 °C
Ambient Temp. : 24.00 °C
Set-up Date : 18-Sep-2009
Set-up Time : 11:46:48 AM
Area Scan : 6x7x1 : Measurement x=15mm, y=15mm, z=4mm
Zoom Scan : 5x5x8 : Measurement x=8mm, y=8mm, z=4mm

Other Data

DUT Position : Front
Separation : 10 mm
Channel : Low

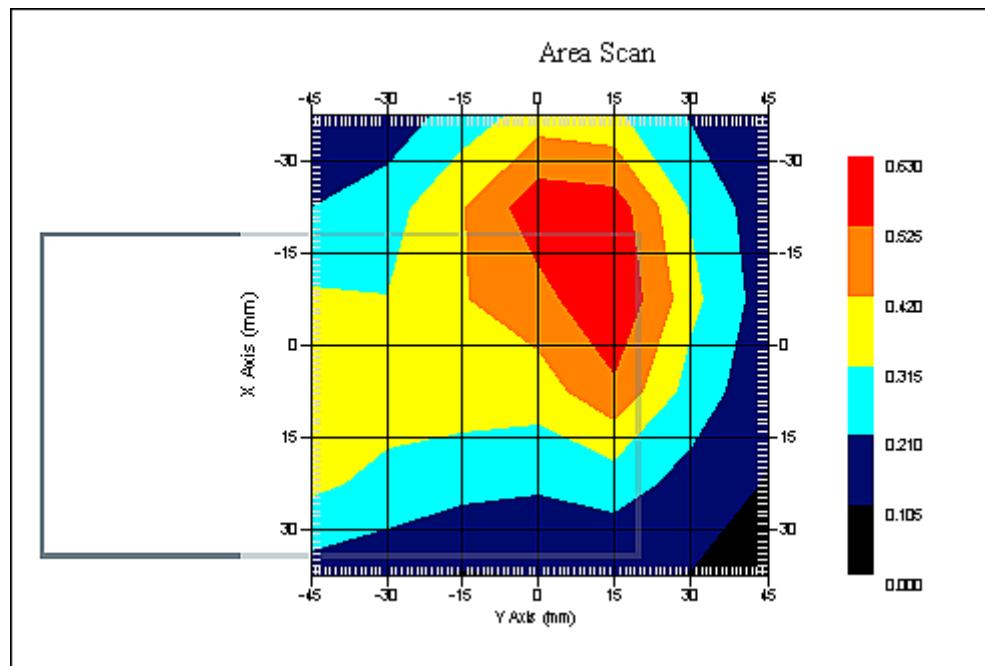

1 gram SAR value : 0.580 W/kg
10 gram SAR value : 0.379 W/kg
Area Scan Peak SAR : 0.630 W/kg
Zoom Scan Peak SAR : 0.880 W/kg

SAR Test Report

By Operator : Jay
Measurement Date : 18-Sep-2009
Starting Time : 18-Sep-2009 02:15:26 PM
End Time : 18-Sep-2009 02:31:40 PM
Scanning Time : 974 secs

Product Data

Device Name : CardioNet
Serial No. : Eng 2
Mode : GPRS
Model : C5
Frequency : 1900.00 MHz
Max. Transmit Pwr : 1 W
Drift Time : 0 min(s)
Length : 117 mm
Width : 64 mm
Depth : 23 mm
Antenna Type : Internal
Orientation : Front
Power Drift-Start : 0.435 W/kg
Power Drift-Finish: 0.435 W/kg
Power Drift (%) : -0.435

Phantom Data

Name : APREL-Uni
Type : Uni-Phantom
Size (mm) : 280 x 280 x 200
Serial No. : System Default
Location : Center
Description : Uni-Phantom

Tissue Data

Type : BODY
Serial No. : 1900
Frequency : 1900.00 MHz
Last Calib. Date : 18-Sep-2009
Temperature : 23.00 °C
Ambient Temp. : 24.00 °C
Humidity : 44.00 RH%
Epsilon : 52.73 F/m
Sigma : 1.58 S/m
Density : 1000.00 kg/cu. m

Probe Data


Name : Probe 215 - RFEL
Model : E020
Type : E-Field Triangle
Serial No. : 215
Last Calib. Date : 03-Nov-2008
Frequency : 1900.00 MHz
Duty Cycle Factor: 4
Conversion Factor: 5
Probe Sensitivity: 1.20 1.20 1.20 μ V/ (V/m)²
Compression Point: 95.00 mV
Offset : 1.56 mm

Measurement Data

Crest Factor : 4
Scan Type : Complete
Tissue Temp. : 23.00 °C
Ambient Temp. : 24.00 °C
Set-up Date : 18-Sep-2009
Set-up Time : 11:46:48 AM
Area Scan : 6x7x1 : Measurement x=15mm, y=15mm, z=4mm
Zoom Scan : 5x5x8 : Measurement x=8mm, y=8mm, z=4mm

Other Data

DUT Position : Front
Separation : 10 mm
Channel : Mid

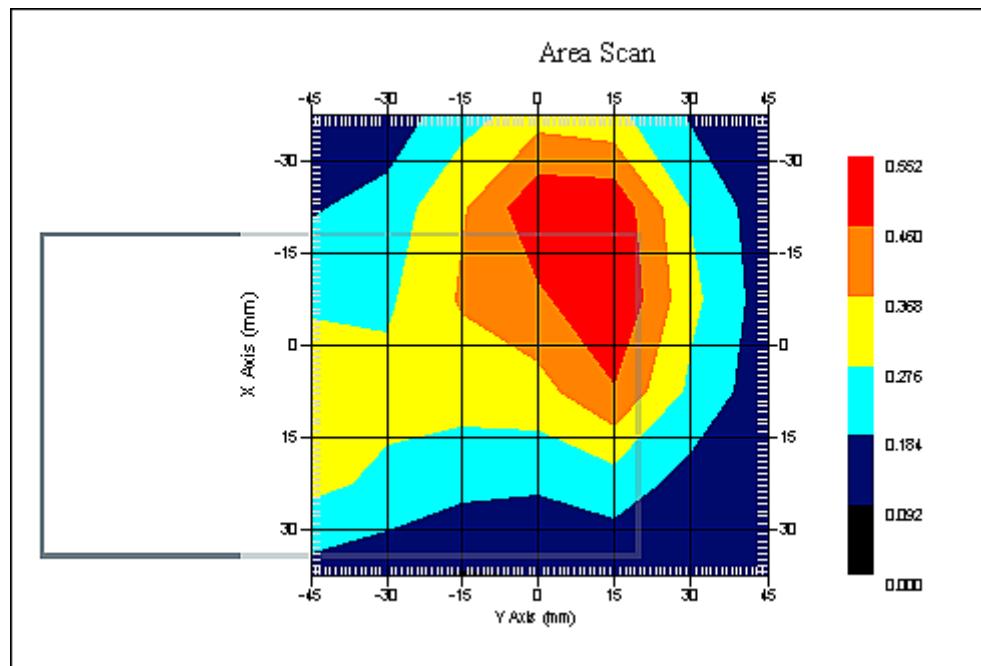

1 gram SAR value : 0.527 W/kg
10 gram SAR value : 0.336 W/kg
Area Scan Peak SAR : 0.549 W/kg
Zoom Scan Peak SAR : 0.800 W/kg

SAR Test Report

By Operator : Jay
Measurement Date : 18-Sep-2009
Starting Time : 18-Sep-2009 02:50:03 PM
End Time : 18-Sep-2009 03:06:09 PM
Scanning Time : 966 secs

Product Data

Device Name : CardioNet
Serial No. : Eng 2
Mode : GPRS
Model : C5
Frequency : 1900.00 MHz
Max. Transmit Pwr : 1 W
Drift Time : 0 min(s)
Length : 117 mm
Width : 64 mm
Depth : 23 mm
Antenna Type : Internal
Orientation : Front
Power Drift-Start : 0.386 W/kg
Power Drift-Finish: 0.391 W/kg
Power Drift (%) : 1.385

Phantom Data

Name : APREL-Uni
Type : Uni-Phantom
Size (mm) : 280 x 280 x 200
Serial No. : System Default
Location : Center
Description : Uni-Phantom

Tissue Data

Type : BODY
Serial No. : 1900
Frequency : 1900.00 MHz
Last Calib. Date : 18-Sep-2009
Temperature : 23.00 °C
Ambient Temp. : 24.00 °C
Humidity : 44.00 RH%
Epsilon : 52.73 F/m
Sigma : 1.58 S/m
Density : 1000.00 kg/cu. m

Probe Data


Name : Probe 215 - RFEL
Model : E020
Type : E-Field Triangle
Serial No. : 215
Last Calib. Date : 03-Nov-2008
Frequency : 1900.00 MHz
Duty Cycle Factor: 4
Conversion Factor: 5
Probe Sensitivity: 1.20 1.20 1.20 μ V/ (V/m)²
Compression Point: 95.00 mV
Offset : 1.56 mm

Measurement Data

Crest Factor : 4
 Scan Type : Complete
 Tissue Temp. : 23.00 °C
 Ambient Temp. : 24.00 °C
 Set-up Date : 18-Sep-2009
 Set-up Time : 11:46:48 AM
 Area Scan : 6x7x1 : Measurement x=15mm, y=15mm, z=4mm
 Zoom Scan : 5x5x8 : Measurement x=8mm, y=8mm, z=4mm

Other Data

DUT Position : Front
 Separation : 10 mm
 Channel : High

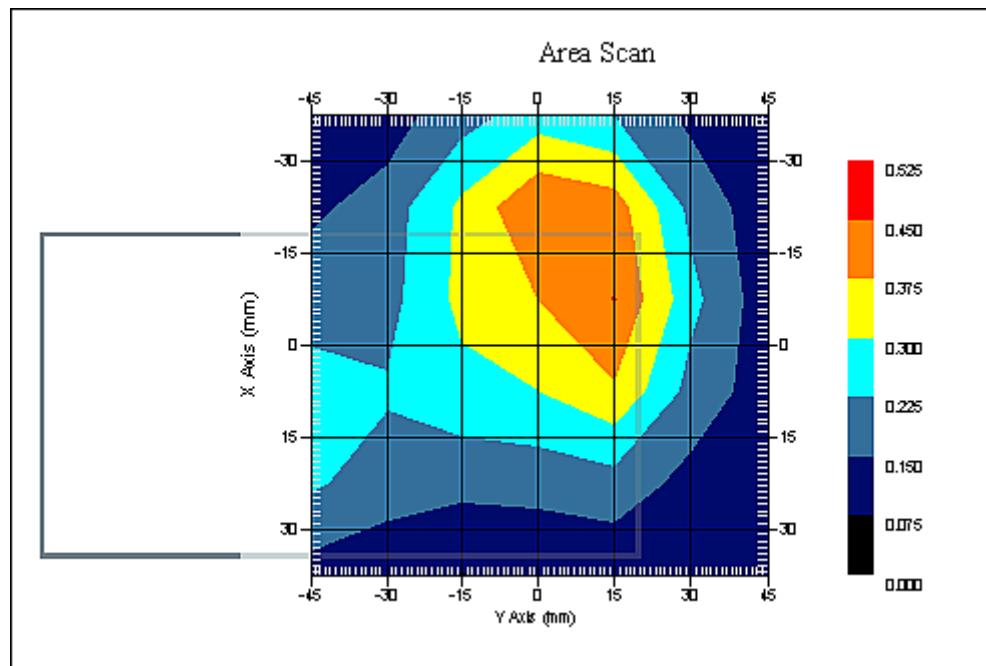

1 gram SAR value : 0.434 W/kg
 10 gram SAR value : 0.280 W/kg
 Area Scan Peak SAR : 0.452 W/kg
 Zoom Scan Peak SAR : 0.690 W/kg

SAR Test Report

By Operator : Jay
Measurement Date : 18-Sep-2009
Starting Time : 18-Sep-2009 03:41:36 PM
End Time : 18-Sep-2009 03:57:50 PM
Scanning Time : 974 secs

Product Data

Device Name : CardioNet
Serial No. : Eng 2
Mode : GPRS
Model : C5
Frequency : 1900.00 MHz
Max. Transmit Pwr : 1 W
Drift Time : 0 min(s)
Length : 117 mm
Width : 64 mm
Depth : 23 mm
Antenna Type : Internal
Orientation : Back
Power Drift-Start : 0.672 W/kg
Power Drift-Finish: 0.698 W/kg
Power Drift (%) : 3.942

Phantom Data

Name : APREL-Uni
Type : Uni-Phantom
Size (mm) : 280 x 280 x 200
Serial No. : System Default
Location : Center
Description : Uni-Phantom

Tissue Data

Type : BODY
Serial No. : 1900
Frequency : 1900.00 MHz
Last Calib. Date : 18-Sep-2009
Temperature : 23.00 °C
Ambient Temp. : 24.00 °C
Humidity : 44.00 RH%
Epsilon : 52.73 F/m
Sigma : 1.58 S/m
Density : 1000.00 kg/cu. m

Probe Data


Name : Probe 215 - RFEL
Model : E020
Type : E-Field Triangle
Serial No. : 215
Last Calib. Date : 03-Nov-2008
Frequency : 1900.00 MHz
Duty Cycle Factor: 4
Conversion Factor: 5
Probe Sensitivity: 1.20 1.20 1.20 μ V/ (V/m)²
Compression Point: 95.00 mV
Offset : 1.56 mm

Measurement Data

Crest Factor : 4
Scan Type : Complete
Tissue Temp. : 23.00 °C
Ambient Temp. : 24.00 °C
Set-up Date : 18-Sep-2009
Set-up Time : 11:46:48 AM
Area Scan : 6x7x1 : Measurement x=15mm, y=15mm, z=4mm
Zoom Scan : 5x5x8 : Measurement x=8mm, y=8mm, z=4mm


Other Data

DUT Position : Back
Separation : 10 mm
Channel : Low

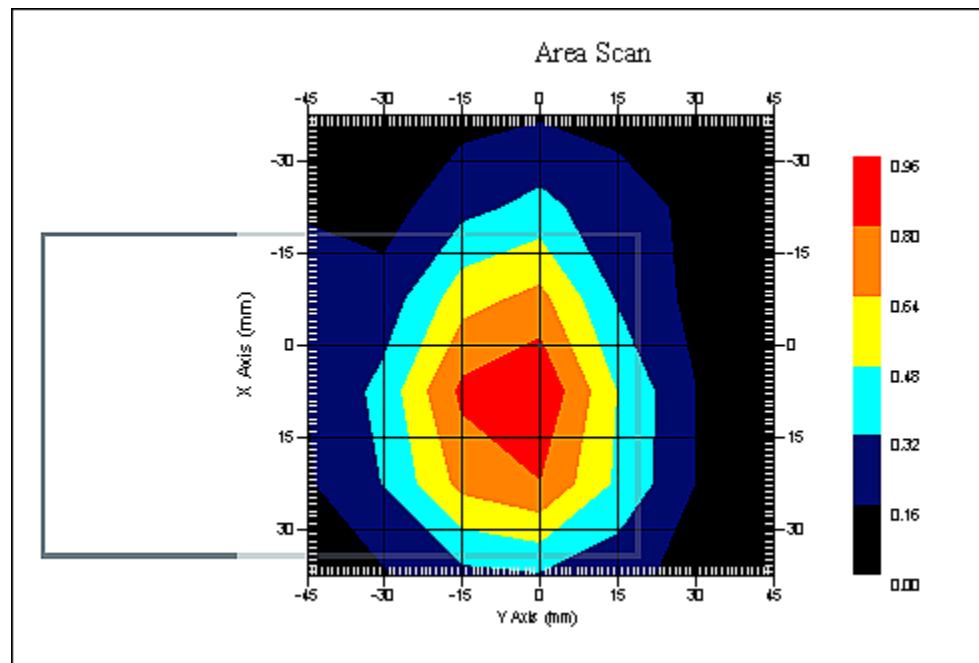

1 gram SAR value : 0.882 W/kg
10 gram SAR value : 0.544 W/kg
Area Scan Peak SAR : 0.957 W/kg
Zoom Scan Peak SAR : 1.281 W/kg

SAR-Z Axis
at Hotspot x:15.04 y:-8.13

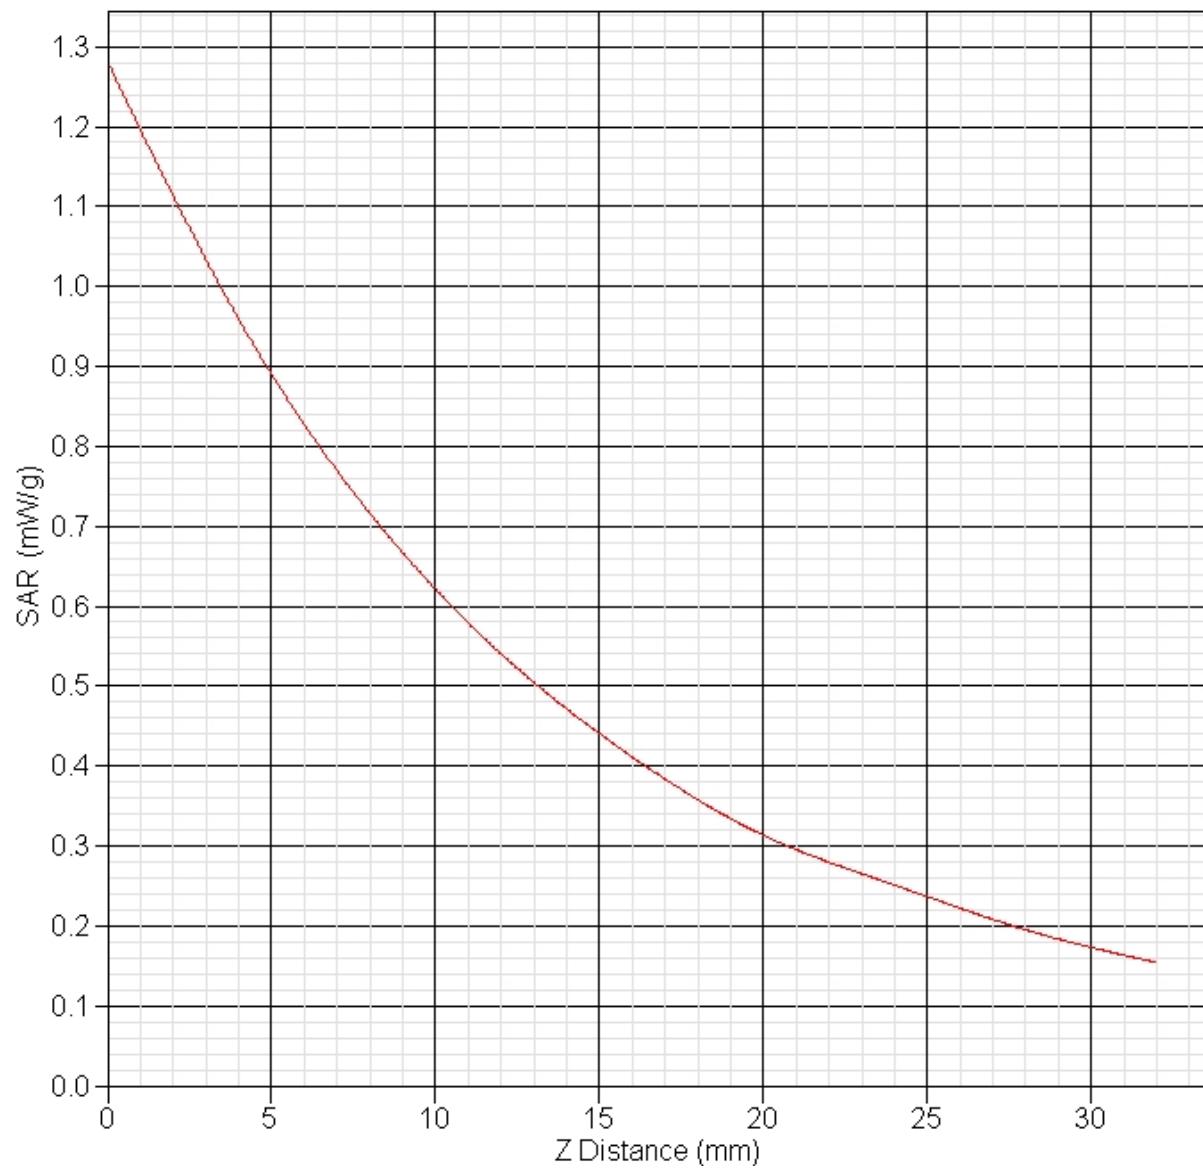

SAR Test Report

By Operator : Jay
Measurement Date : 18-Sep-2009
Starting Time : 18-Sep-2009 03:24:33 PM
End Time : 18-Sep-2009 03:40:48 PM
Scanning Time : 975 secs

Product Data

Device Name : CardioNet
Serial No. : Eng 2
Mode : GPRS
Model : C5
Frequency : 1900.00 MHz
Max. Transmit Pwr : 1 W
Drift Time : 0 min(s)
Length : 117 mm
Width : 64 mm
Depth : 23 mm
Antenna Type : Internal
Orientation : Back
Power Drift-Start : 0.614 W/kg
Power Drift-Finish: 0.609 W/kg
Power Drift (%) : -0.830

Phantom Data

Name : APREL-Uni
Type : Uni-Phantom
Size (mm) : 280 x 280 x 200
Serial No. : System Default
Location : Center
Description : Uni-Phantom

Tissue Data

Type : BODY
Serial No. : 1900
Frequency : 1900.00 MHz
Last Calib. Date : 18-Sep-2009
Temperature : 23.00 °C
Ambient Temp. : 24.00 °C
Humidity : 44.00 RH%
Epsilon : 52.73 F/m
Sigma : 1.58 S/m
Density : 1000.00 kg/cu. m

Probe Data


Name : Probe 215 - RFEL
Model : E020
Type : E-Field Triangle
Serial No. : 215
Last Calib. Date : 03-Nov-2008
Frequency : 1900.00 MHz
Duty Cycle Factor: 4
Conversion Factor: 5
Probe Sensitivity: 1.20 1.20 1.20 μ V/ (V/m)²
Compression Point: 95.00 mV
Offset : 1.56 mm

Measurement Data

Crest Factor : 4
 Scan Type : Complete
 Tissue Temp. : 23.00 °C
 Ambient Temp. : 24.00 °C
 Set-up Date : 18-Sep-2009
 Set-up Time : 11:46:48 AM
 Area Scan : 6x7x1 : Measurement x=15mm, y=15mm, z=4mm
 Zoom Scan : 5x5x8 : Measurement x=8mm, y=8mm, z=4mm

Other Data

DUT Position : Back
 Separation : 10 mm
 Channel : Mid

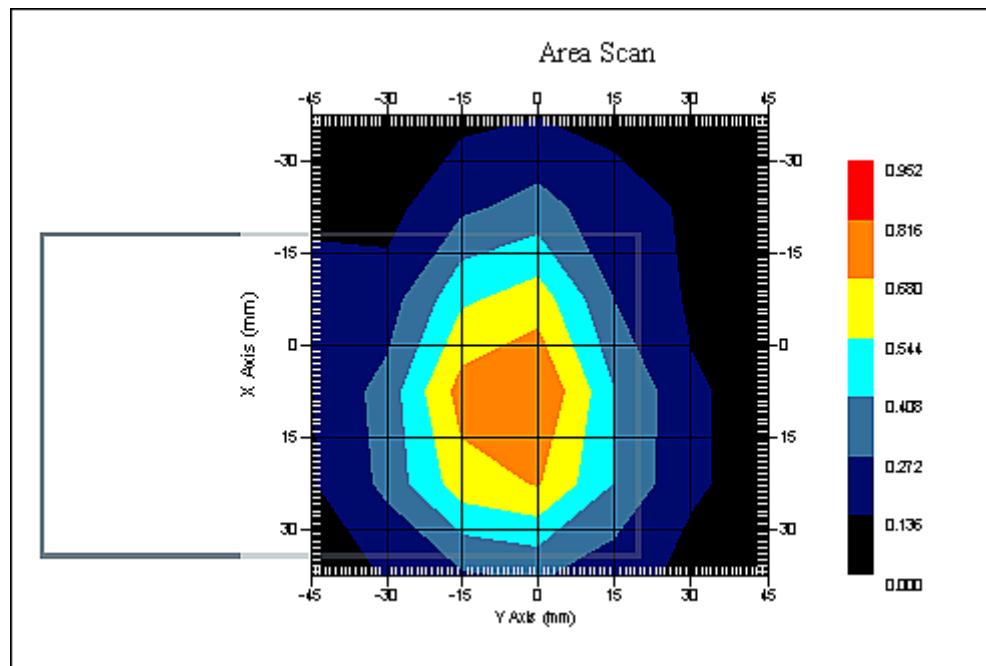

1 gram SAR value : 0.794 W/kg
 10 gram SAR value : 0.491 W/kg
 Area Scan Peak SAR : 0.817 W/kg
 Zoom Scan Peak SAR : 1.221 W/kg

SAR Test Report

By Operator : Jay
Measurement Date : 18-Sep-2009
Starting Time : 18-Sep-2009 03:07:20 PM
End Time : 18-Sep-2009 03:23:37 PM
Scanning Time : 977 secs

Product Data

Device Name : CardioNet
Serial No. : Eng 2
Mode : GPRS
Model : C5
Frequency : 1900.00 MHz
Max. Transmit Pwr : 1 W
Drift Time : 0 min(s)
Length : 117 mm
Width : 64 mm
Depth : 23 mm
Antenna Type : Internal
Orientation : Back
Power Drift-Start : 0.497 W/kg
Power Drift-Finish: 0.506 W/kg
Power Drift (%) : 1.920

Phantom Data

Name : APREL-Uni
Type : Uni-Phantom
Size (mm) : 280 x 280 x 200
Serial No. : System Default
Location : Center
Description : Uni-Phantom

Tissue Data

Type : BODY
Serial No. : 1900
Frequency : 1900.00 MHz
Last Calib. Date : 18-Sep-2009
Temperature : 23.00 °C
Ambient Temp. : 24.00 °C
Humidity : 44.00 RH%
Epsilon : 52.73 F/m
Sigma : 1.58 S/m
Density : 1000.00 kg/cu. m

Probe Data


Name : Probe 215 - RFEL
Model : E020
Type : E-Field Triangle
Serial No. : 215
Last Calib. Date : 03-Nov-2008
Frequency : 1900.00 MHz
Duty Cycle Factor: 4
Conversion Factor: 5
Probe Sensitivity: 1.20 1.20 1.20 μ V/ (V/m)²
Compression Point: 95.00 mV
Offset : 1.56 mm

Measurement Data

Crest Factor : 4
Scan Type : Complete
Tissue Temp. : 23.00 °C
Ambient Temp. : 24.00 °C
Set-up Date : 18-Sep-2009
Set-up Time : 11:46:48 AM
Area Scan : 6x7x1 : Measurement x=15mm, y=15mm, z=4mm
Zoom Scan : 5x5x8 : Measurement x=8mm, y=8mm, z=4mm

Other Data

DUT Position : Back
Separation : 10 mm
Channel : High

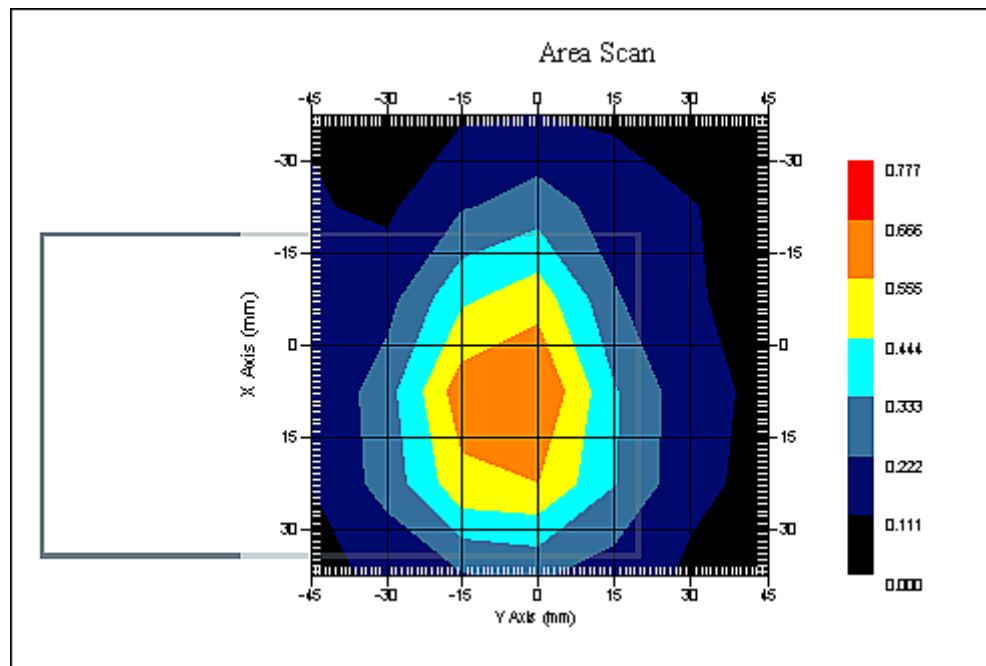


1 gram SAR value : 0.654 W/kg
10 gram SAR value : 0.408 W/kg
Area Scan Peak SAR : 0.667 W/kg
Zoom Scan Peak SAR : 0.960 W/kg

Appendix C – SAR Test Setup Photos



System Configuration

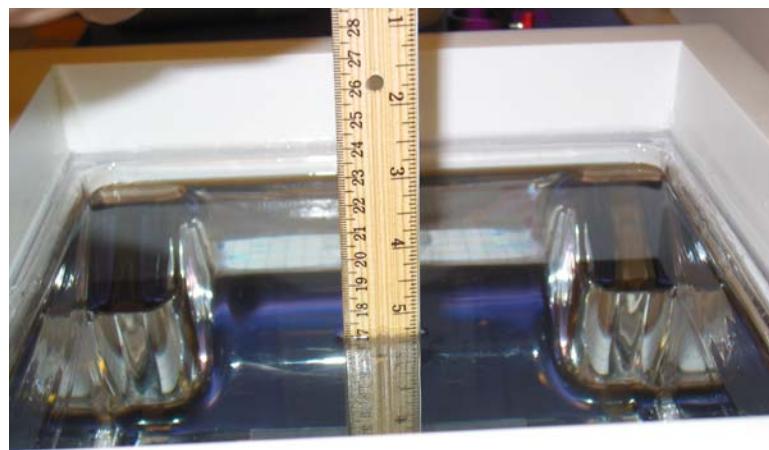

Body Tissue Depth



Held to Face Test Position 2.5 cm Gap



Body Test Position Front 1 cm Gap



Body Test Position Back 1 cm Gap



Front Of Device



Back Of Device



Back Cover Removed



Battery



Antenna



CDMA Module Installed



CDMA Module



GSM Module Installed



GSM Module

Appendix D – Probe Calibration Data Sheets

NCL CALIBRATION LABORATORIES

Calibration File No.: CP-928

Client.: RFEL

C E R T I F I C A T E O F C A L I B R A T I O N

It is certified that the equipment identified below has been calibrated in the
NCL CALIBRATION LABORATORIES by qualified personnel following recognized
procedures and using transfer standards traceable to NRC/NIST.

Equipment: Miniature Isotropic RF Probe 835 MHz

Manufacturer: APREL Laboratories

Model No.: E-020

Serial No.: 215

Head Calibration

Calibration Procedure: SSI/DRB-TP-D01-032-E020-V2


Project No: RFEL-00150-CAL-5367

Calibrated: 3rd November 2008
Released on: 3rd November 2008

This Calibration Certificate is Incomplete Unless Accompanied with the Calibration Results Summary
This calibration has been conducted in line with the SCC ISO-IEC 17025 Scope of Accreditation

Accredited Laboratory Number 48

Released By: _____



NCL CALIBRATION LABORATORIES

51 SPECTRUM WAY
NEPEAN, ONTARIO
CANADA K2R 1E6

Division of APREL Lab.
TEL: (613) 820-4988
FAX: (613) 820-4161

NCL Calibration Laboratories

Division of APREL Laboratories.

Introduction

This Calibration Report reproduces the results of the calibration performed in line with the SSI/DRB-TP-D01-032-E020-V2 E-Field Probe Calibration Procedure. The results contained within this report are for APREL E-Field Probe E-020 215.

References

SSI/DRB-TP-D01-032-E020-V2 E-Field Probe Calibration Procedure
IEEE 1528 "Recommended Practice for Determining the Peak Spatial-Average Specific Absorption Rate (SAR) in the Human Body Due to Wireless Communications Devices: Experimental Techniques"
IEEE 1309 "IEEE Standard for Calibration of Electromagnetic Field Sensors and Probes, Excluding Antennas, from 9 KHz to 40 GHz" 2005
SSI-TP-011 Tissue Calibration Procedure
IEC 62209 "Human exposure to radio frequency fields from handheld and body-mounted wireless communication devices –Human models, instrumentation and procedures Part 1 & 2: Procedure to determine the Specific Absorption Rate (SAR) for handheld devices used in close proximity of the ear (frequency range of 200MHz to 3GHz)"

Conditions


Probe 215 was a re-calibration.

Ambient Temperature of the Laboratory: 22 °C +/- 0.5°C
Temperature of the Tissue: 21 °C +/- 0.5°C

We the undersigned attest that to the best of our knowledge the calibration of this probe has been accurately conducted and that all information contained within this report has been reviewed for accuracy.



Stuart Nicol



Jesse Hones

Calibration Results Summary

Probe Type:	E-Field Probe E-020
Serial Number:	215
Frequency:	835 MHz
Sensor Offset:	1.56 mm
Sensor Length:	2.5 mm
Tip Enclosure:	Ertalyte*
Tip Diameter:	<5 mm
Tip Length:	60 mm
Total Length:	290 mm

*Resistive to recommended tissue recipes per IEEE-1528

Sensitivity in Air

Channel X:	$1.2 \mu\text{V}/(\text{V}/\text{m})^2$
Channel Y:	$1.2 \mu\text{V}/(\text{V}/\text{m})^2$
Channel Z:	$1.2 \mu\text{V}/(\text{V}/\text{m})^2$
Diode Compression Point:	95 mV

Sensitivity in Head Tissue Measured**Frequency:** 835 MHz**Epsilon:** 41.5 (+/-5%) **Sigma:** 0.90 S/m (+/-10%)**ConvF****Channel X:** 6.2**Channel Y:** 6.2**Channel Z:** 6.2

Tissue sensitivity values were calculated using the load impedance of the APREL Laboratories Daq-Paq.


Boundary Effect:



Uncertainty resulting from the boundary effect is less than 2% for the distance between the tip of the probe and the tissue boundary, when less than 2.44mm.

Spatial Resolution:

The measured probe tip diameter is 5 mm (+/- 0.01 mm) and therefore meets the requirements of SSI/DRB-TP-D01-032 for spatial resolution.


Receiving Pattern 835 MHz (Air)

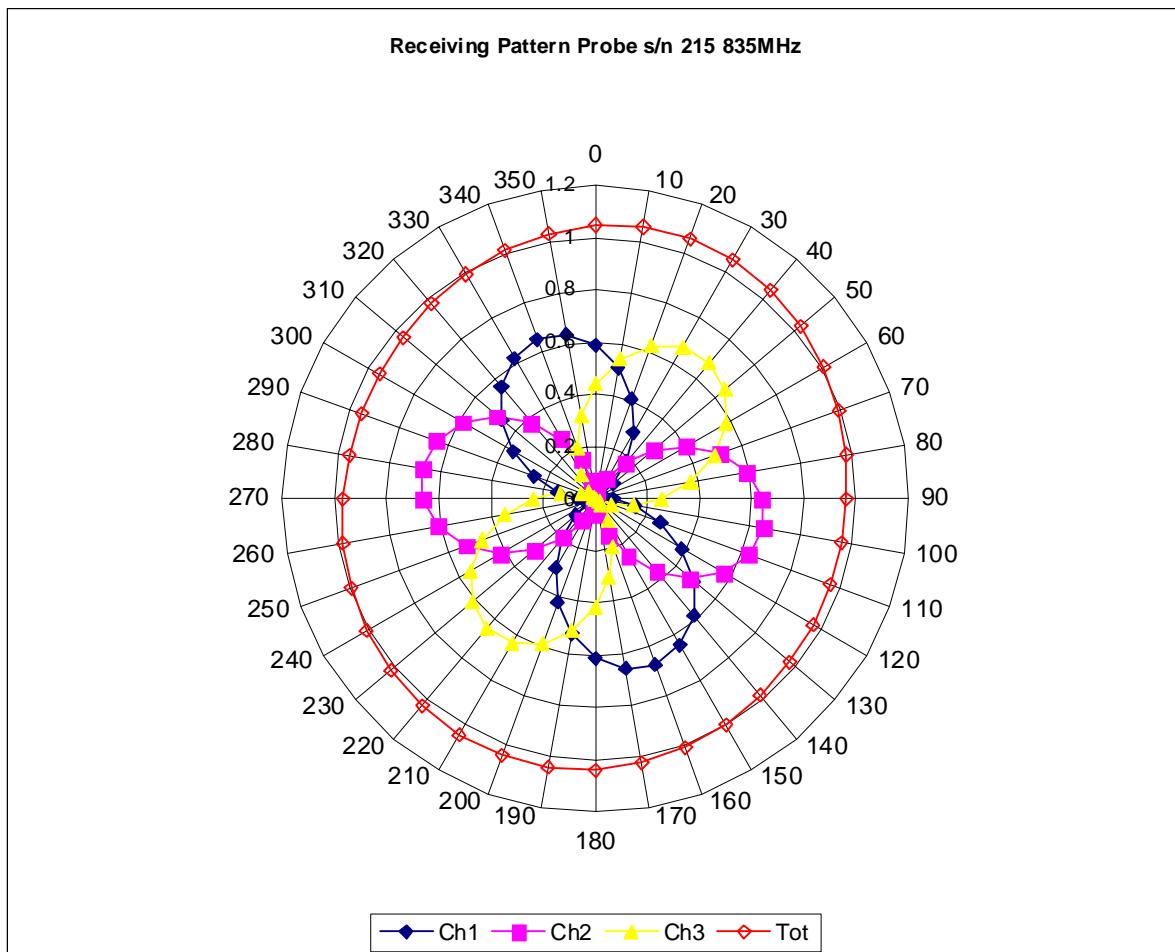

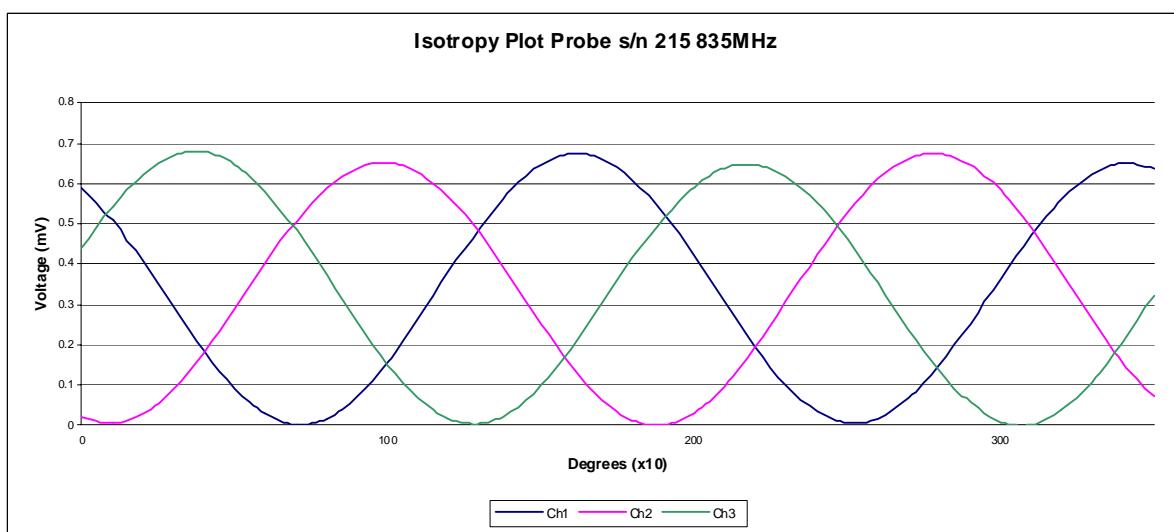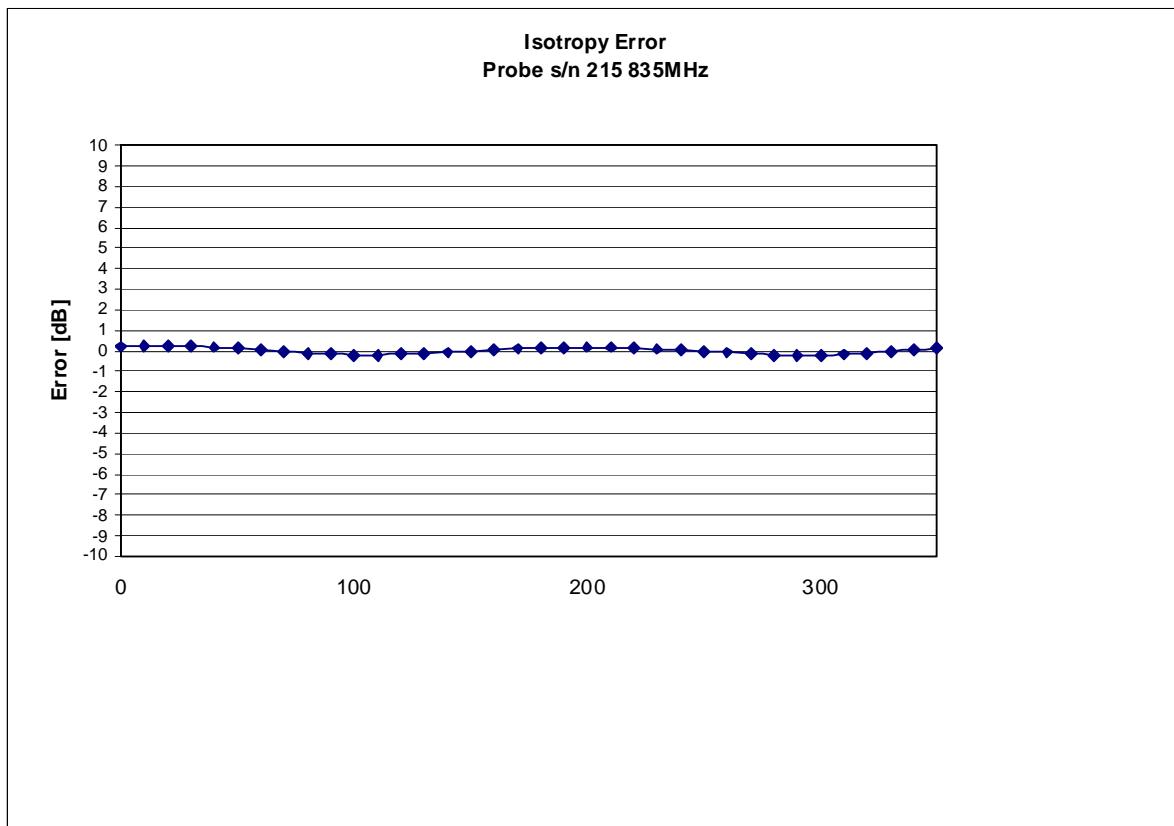Isotropy Error 835 MHz (Air)**Isotropicity Tissue:**


0.10 dB

Dynamic Range

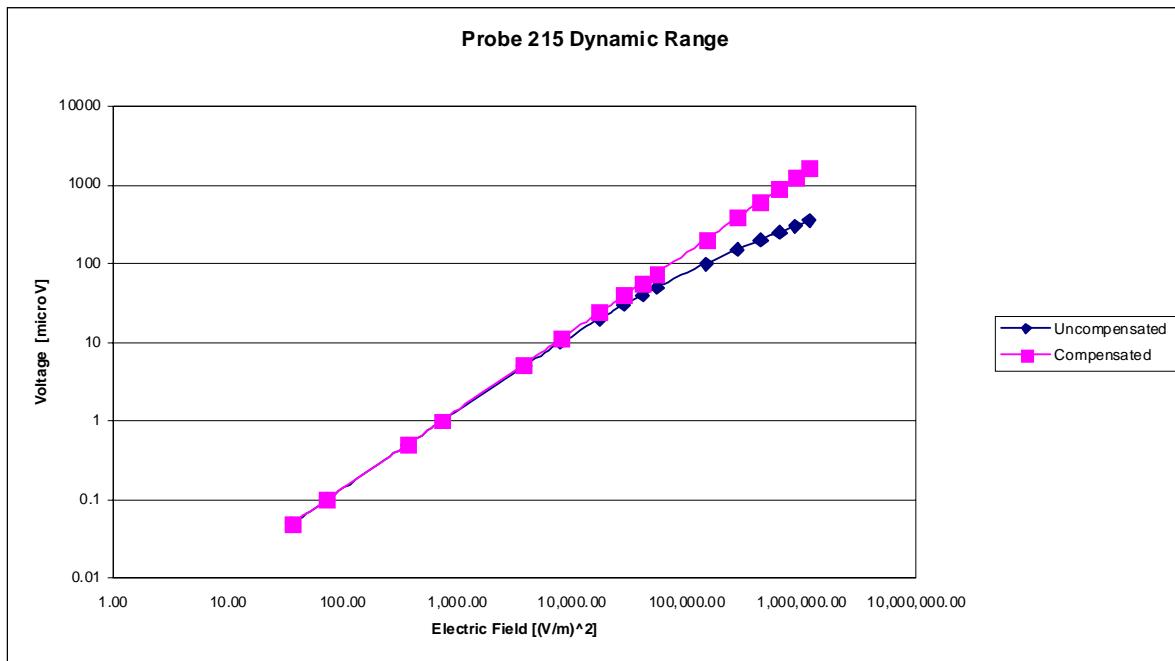

Video Bandwidth

Probe Frequency Characteristics

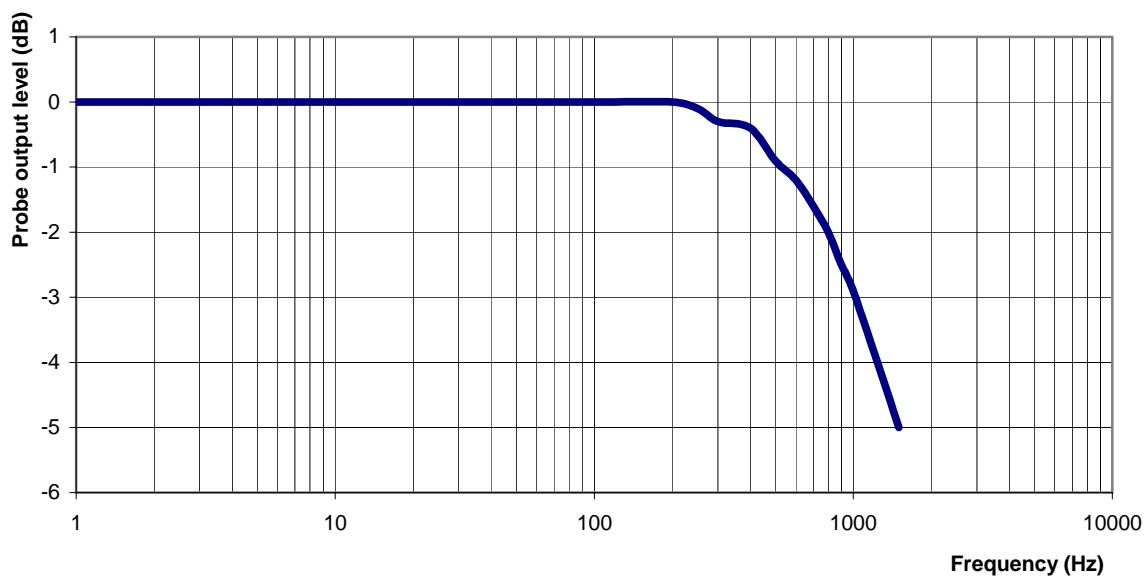

Video Bandwidth at 500 Hz 1 dB
Video Bandwidth at 1.02 KHz: 3 dB

Conversion Factor Uncertainty Assessment Measured

Frequency: 835MHz

Epsilon: 41.5 (+/-5%) **Sigma:** 0.90 S/m (+/-10%)

ConvF

Channel X: 6.2 7%(K=2)

Channel Y: 6.2 7%(K=2)

Channel Z: 6.2 7%(K=2)

To minimize the uncertainty calculation all tissue sensitivity values were calculated using a load impedance of 5 MΩ.

Boundary Effect:

For a distance of 2.5mm the evaluated uncertainty (increase in the probe sensitivity) is less than 2%.

Test Equipment

The test equipment used during Probe Calibration, manufacturer, model number and, current calibration status are listed and located on the main APREL server R:\NCL\Calibration Equipment\Instrument List May 2008.

NCL CALIBRATION LABORATORIES

Calibration File No.: CP-926

Client.: RFEL

C E R T I F I C A T E O F C A L I B R A T I O N

It is certified that the equipment identified below has been calibrated in the
NCL CALIBRATION LABORATORIES by qualified personnel following recognized
procedures and using transfer standards traceable to NRC/NIST.

Equipment: Miniature Isotropic RF Probe 835 MHz

BODY Calibration

Manufacturer: APREL Laboratories

Model No.: E-020

Serial No.: 215

Calibration Procedure: SSI/DRB-TP-D01-032-E020-V2

Project No: RFEL-00150-CAL-5367

Calibrated: 3rd November 2008
Released on: 3rd November 2008

This Calibration Certificate is Incomplete Unless Accompanied with the Calibration Results Summary
This calibration has been conducted in line with the SCC ISO-IEC 17025 Scope of Accreditation

Accredited Laboratory Number 48

Released By: _____

NCL CALIBRATION LABORATORIES

51 SPECTRUM WAY
NEPEAN, ONTARIO
CANADA K2R 1E6

Division of APREL Lab.
TEL: (613) 820-4988
FAX: (613) 820-4161

NCL Calibration Laboratories

Division of APREL Laboratories.

Introduction

This Calibration Report reproduces the results of the calibration performed in line with the SSI/DRB-TP-D01-032-E020-V2 E-Field Probe Calibration Procedure. The results contained within this report are for APREL E-Field Probe E-020 215.

References

SSI/DRB-TP-D01-032-E020-V2 E-Field Probe Calibration Procedure
IEEE 1528 "Recommended Practice for Determining the Peak Spatial-Average Specific Absorption Rate (SAR) in the Human Body Due to Wireless Communications Devices: Experimental Techniques"
IEEE 1309 "IEEE Standard for Calibration of Electromagnetic Field Sensors and Probes, Excluding Antennas, from 9 KHz to 40 GHz" 2005
SSI-TP-011 Tissue Calibration Procedure
IEC 62209 "Human exposure to radio frequency fields from handheld and body-mounted wireless communication devices –Human models, instrumentation and procedures Part 1 & 2: Procedure to determine the Specific Absorption Rate (SAR) for handheld devices used in close proximity of the ear (frequency range of 200MHz to 3GHz)"

Conditions


Probe 215 was a re-calibration.

Ambient Temperature of the Laboratory: 22 °C +/- 0.5°C
Temperature of the Tissue: 21 °C +/- 0.5°C

We the undersigned attest that to the best of our knowledge the calibration of this probe has been accurately conducted and that all information contained within this report has been reviewed for accuracy.



Stuart Nicol



Jesse Hones

Calibration Results Summary

Probe Type:	E-Field Probe E-020
Serial Number:	215
Frequency:	835 MHz
Sensor Offset:	1.56 mm
Sensor Length:	2.5 mm
Tip Enclosure:	Ertalyte*
Tip Diameter:	<5 mm
Tip Length:	60 mm
Total Length:	290 mm

*Resistive to recommended tissue recipes per IEEE-1528

Sensitivity in Air

Channel X:	$1.2 \mu\text{V}/(\text{V}/\text{m})^2$
Channel Y:	$1.2 \mu\text{V}/(\text{V}/\text{m})^2$
Channel Z:	$1.2 \mu\text{V}/(\text{V}/\text{m})^2$
Diode Compression Point:	95 mV

Sensitivity in Body Tissue Measured**Frequency:** 835 MHz**Epsilon:** 55.2 (+/-5%) **Sigma:** 0.96 S/m (+/-5%)**ConvF****Channel X:** 6.3**Channel Y:** 6.3**Channel Z:** 6.3

Tissue sensitivity values were calculated using the load impedance of the APREL Laboratories Daq-Paq.


Boundary Effect:



Uncertainty resulting from the boundary effect is less than 2% for the distance between the tip of the probe and the tissue boundary, when less than 2.44mm.

Spatial Resolution:

The measured probe tip diameter is 5 mm (+/- 0.01 mm) and therefore meets the requirements of SSI/DRB-TP-D01-032 for spatial resolution.


Receiving Pattern 835 MHz (Air)

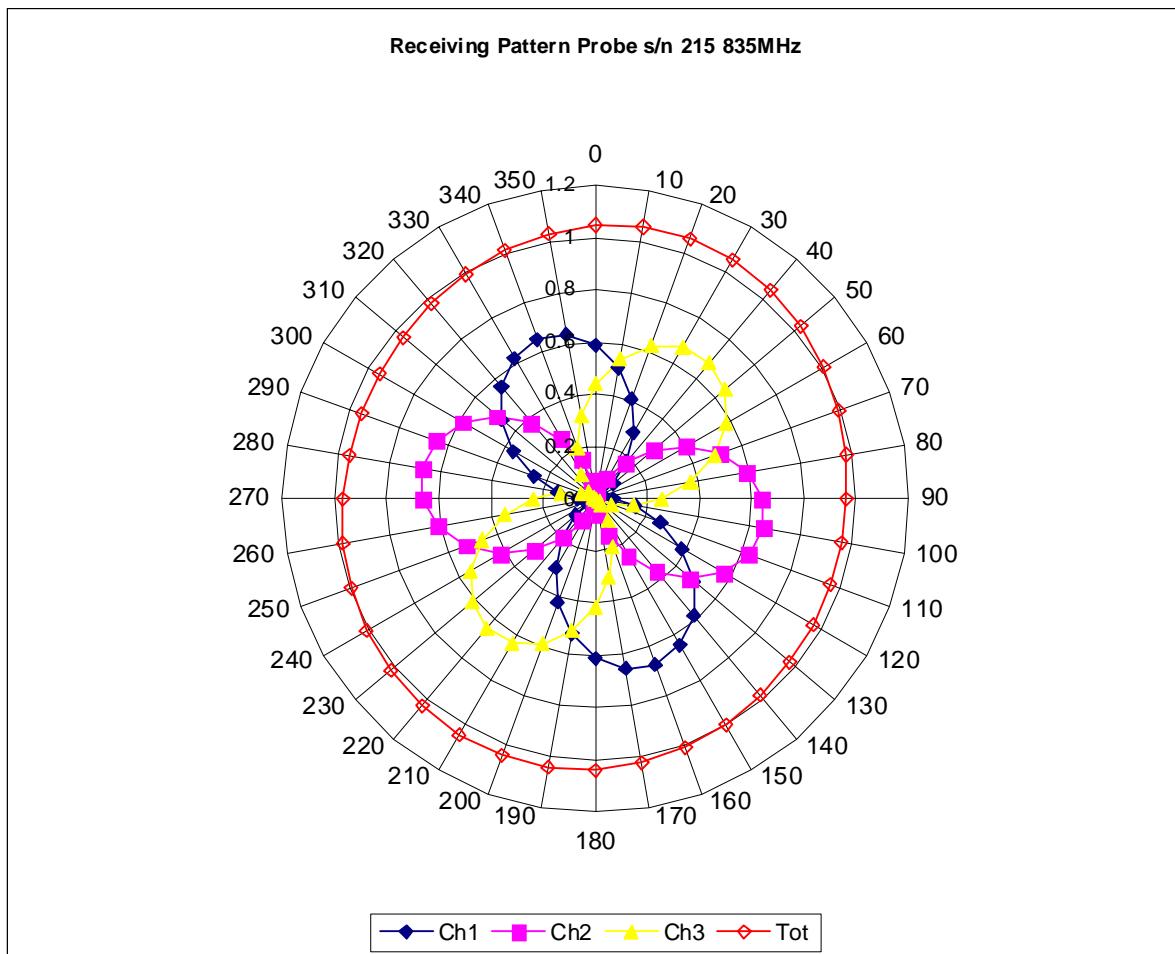

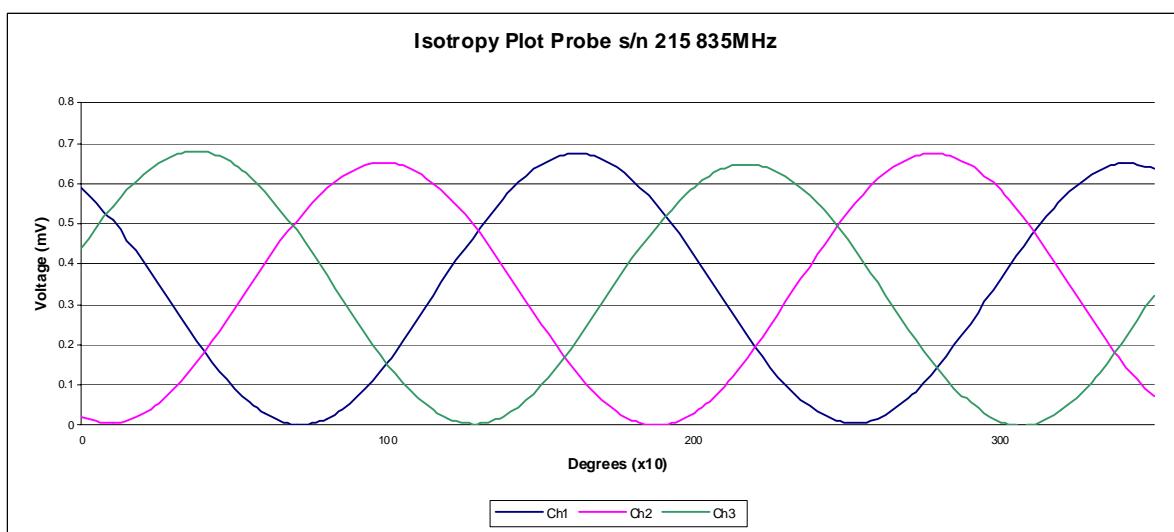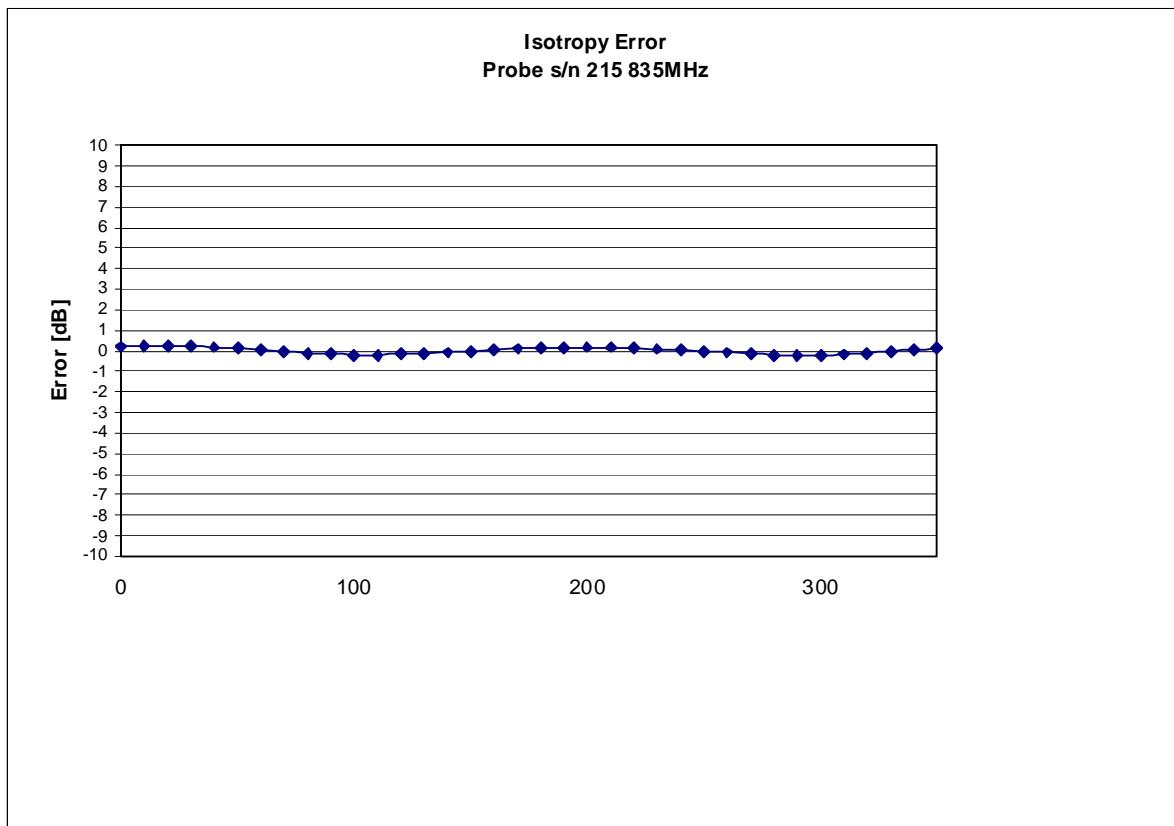Isotropy Error 835 MHz (Air)**Isotropicity Tissue:**


0.10 dB

Dynamic Range

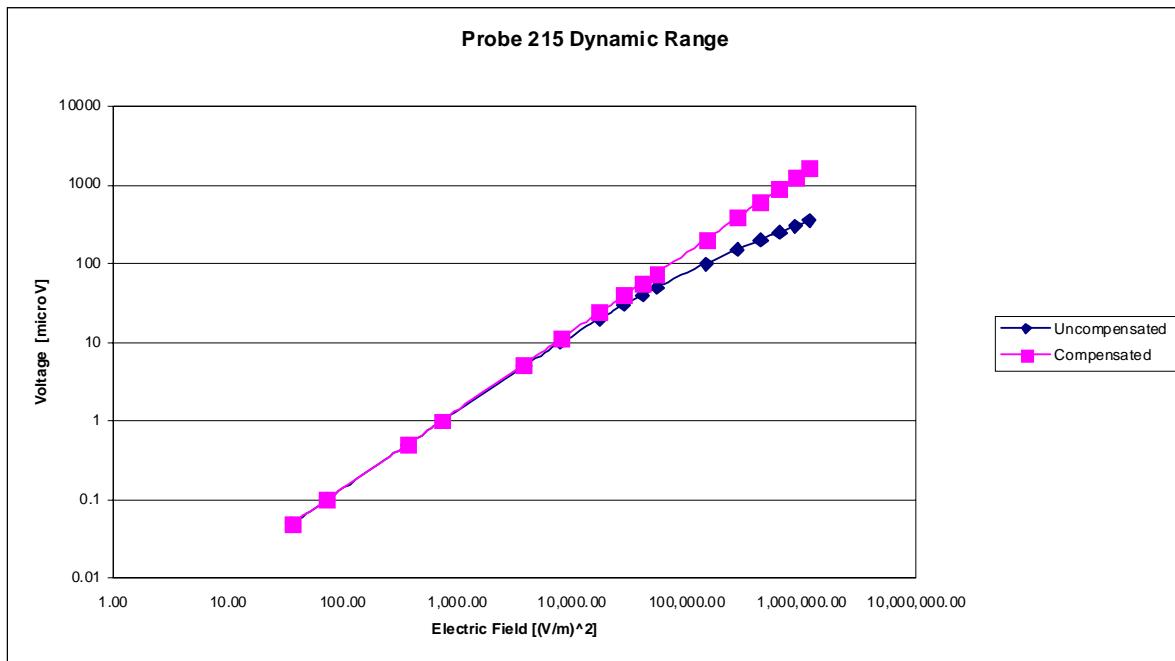

Video Bandwidth

Probe Frequency Characteristics

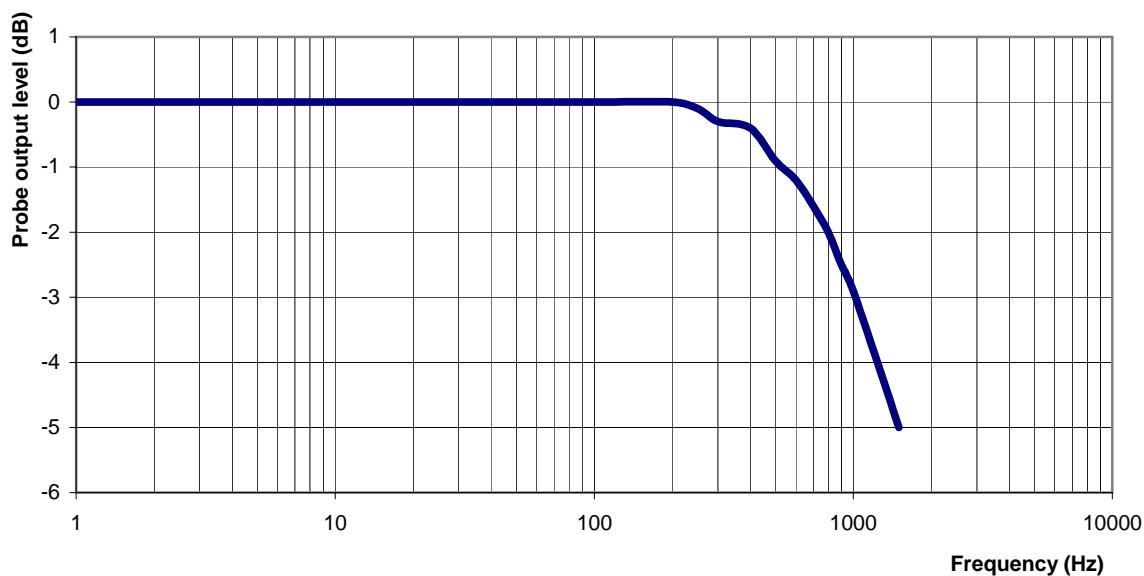

Video Bandwidth at 500 Hz 1 dB
Video Bandwidth at 1.02 KHz: 3 dB

Conversion Factor Uncertainty Assessment Measured

Sensitivity in Body Tissue

Frequency: 835 MHz

Epsilon: 55.2 (+/-5%) **Sigma:** 0.96 S/m (+/-5%)

ConvF

Channel X: 6.3 7%(K=2)

Channel Y: 6.3 7%(K=2)

Channel Z: 6.3 7%(K=2)

To minimize the uncertainty calculation all tissue sensitivity values were calculated using a load impedance of 5 MΩ.

Boundary Effect:

For a distance of 2.5mm the evaluated uncertainty (increase in the probe sensitivity) is less than 2%.

Test Equipment

The test equipment used during Probe Calibration, manufacturer, model number and, current calibration status are listed and located on the main APREL server R:\NCL\Calibration Equipment\Instrument List May 2008.

NCL CALIBRATION LABORATORIES

Calibration File No.: CP-932

Client.: RFEL

C E R T I F I C A T E O F C A L I B R A T I O N

It is certified that the equipment identified below has been calibrated in the
NCL CALIBRATION LABORATORIES by qualified personnel following recognized
procedures and using transfer standards traceable to NRC/NIST.

Equipment: Miniature Isotropic RF Probe 1900 MHz

Manufacturer: APREL Laboratories

Model No.: E-020

Serial No.: 215

Head Tissue

Calibration Procedure: SSI/DRB-TP-D01-032-E020-V2

Project No: RFEB-ALS-E-020-5318

Calibrated: 3rd November 2008
Released on: 3rd November 2008

This Calibration Certificate is Incomplete Unless Accompanied with the Calibration Results Summary
This calibration has been conducted in line with the SCC ISO-IEC 17025 Scope of Accreditation

Accredited Laboratory Number 48

Released By: _____

NCL CALIBRATION LABORATORIES

51 SPECTRUM WAY
NEPEAN, ONTARIO
CANADA K2R 1E6

Division of APREL Lab.
TEL: (613) 820-4988
FAX: (613) 820-4161

NCL Calibration Laboratories

Division of APREL Laboratories.

Introduction

This Calibration Report reproduces the results of the calibration performed in line with the SSI/DRB-TP-D01-032-E020-V2 E-Field Probe Calibration Procedure. The results contained within this report are for APREL E-Field Probe E-020 215.

References


SSI/DRB-TP-D01-032-E020-V2 E-Field Probe Calibration Procedure
IEEE 1528 "Recommended Practice for Determining the Peak Spatial-Average Specific Absorption Rate (SAR) in the Human Body Due to Wireless Communications Devices: Experimental Techniques"
IEEE 1309 "IEEE Standard for Calibration of Electromagnetic Field Sensors and Probes, Excluding Antennas, from 9 KHz to 40 GHz" 2005
SSI-TP-011 Tissue Calibration Procedure
IEC 62209 "Human exposure to radio frequency fields from handheld and body-mounted wireless communication devices –Human models, instrumentation and procedures Part 1 & 2: Procedure to determine the Specific Absorption Rate (SAR) for handheld devices used in close proximity of the ear (frequency range of 200MHz to 3GHz)"

Conditions


Probe 215 was a re-calibration.

Ambient Temperature of the Laboratory: 22 °C +/- 0.5°C
Temperature of the Tissue: 21 °C +/- 0.5°C

We the undersigned attest that to the best of our knowledge the calibration of this probe has been accurately conducted and that all information contained within this report has been reviewed for accuracy.



Stuart Nicol



Jesse Hones

Calibration Results Summary

Probe Type:	E-Field Probe E-020
Serial Number:	215
Frequency:	1900 MHz
Sensor Offset:	1.56 mm
Sensor Length:	2.5 mm
Tip Enclosure:	Ertalyte*
Tip Diameter:	<5 mm
Tip Length:	60 mm
Total Length:	290 mm

*Resistive to recommended tissue recipes per IEEE-1528

Sensitivity in Air

Channel X:	$1.2 \mu\text{V}/(\text{V}/\text{m})^2$
Channel Y:	$1.2 \mu\text{V}/(\text{V}/\text{m})^2$
Channel Z:	$1.2 \mu\text{V}/(\text{V}/\text{m})^2$
Diode Compression Point:	95 mV

Sensitivity in Head Tissue Measured**Frequency:** 1900 MHz**Epsilon:** 39.0 (+/-5%) **Sigma:** 1.43 S/m (+/-5%)**ConvF****Channel X:** 4.9**Channel Y:** 4.9**Channel Z:** 4.9

Tissue sensitivity values were calculated using the load impedance of the APREL Laboratories Daq-Paq.


Boundary Effect:



Uncertainty resulting from the boundary effect is less than 2% for the distance between the tip of the probe and the tissue boundary, when less than 2.44mm.

Spatial Resolution:

The measured probe tip diameter is 5 mm (+/- 0.01 mm) and therefore meets the requirements of SSI/DRB-TP-D01-032 for spatial resolution.


Receiving Pattern 1900 MHz (Air)

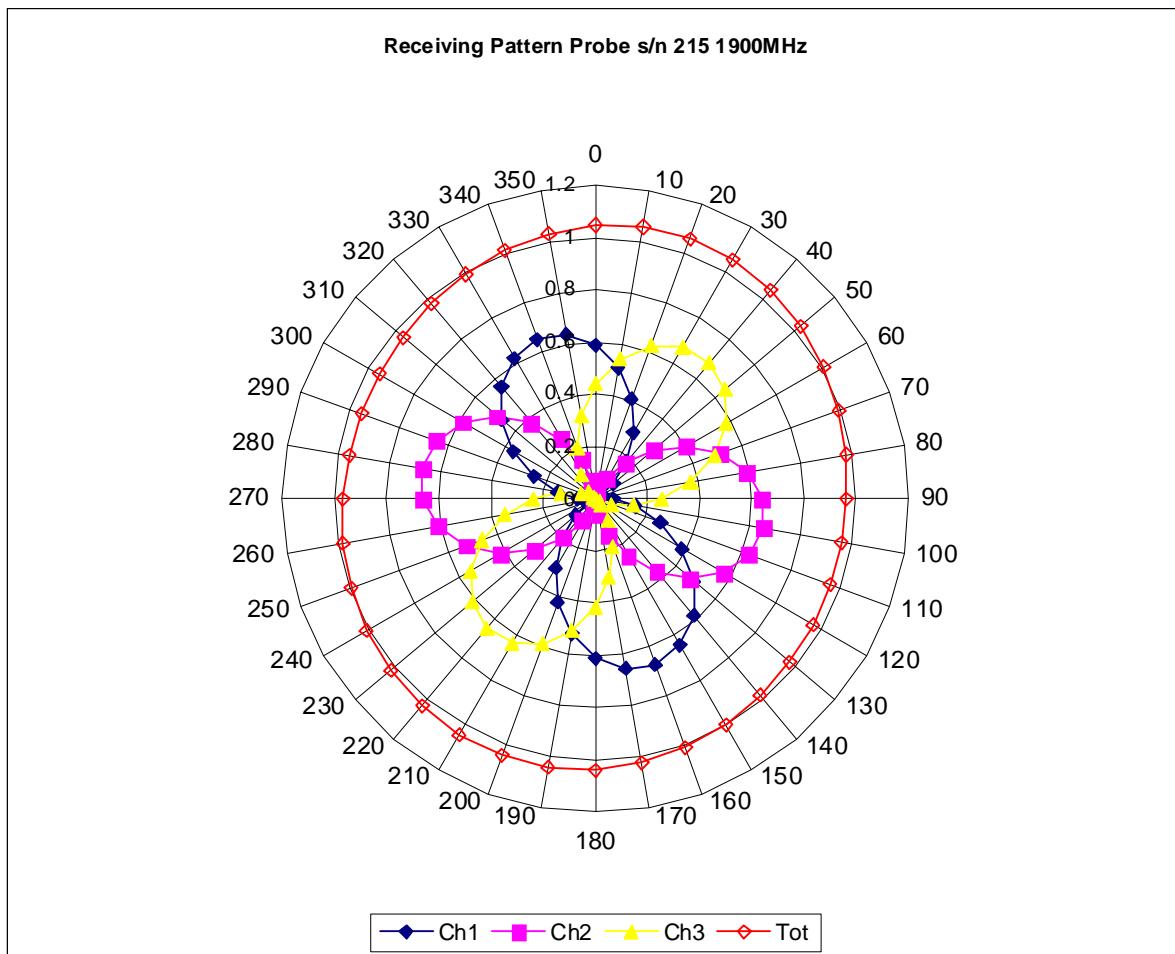

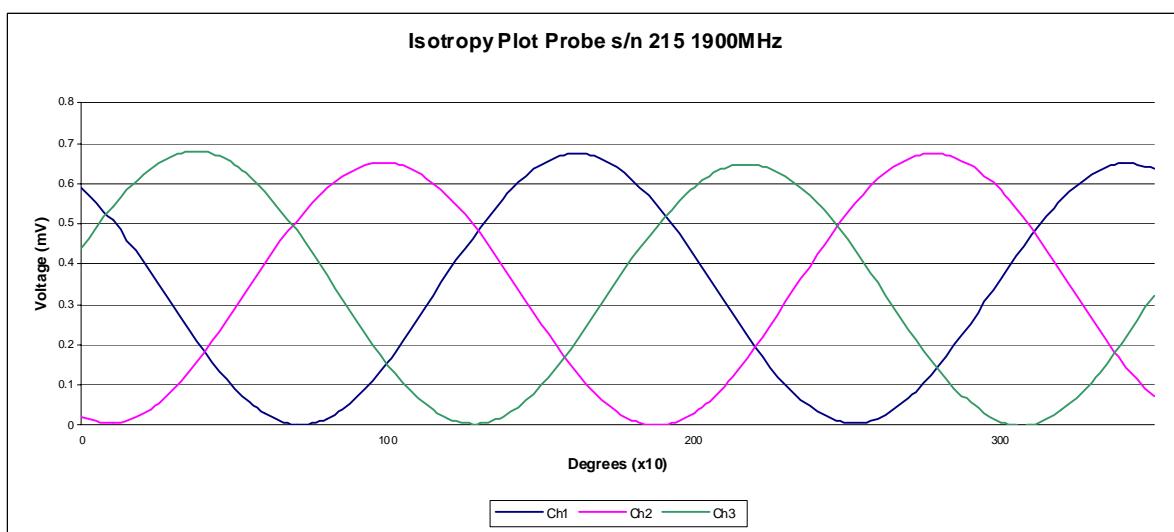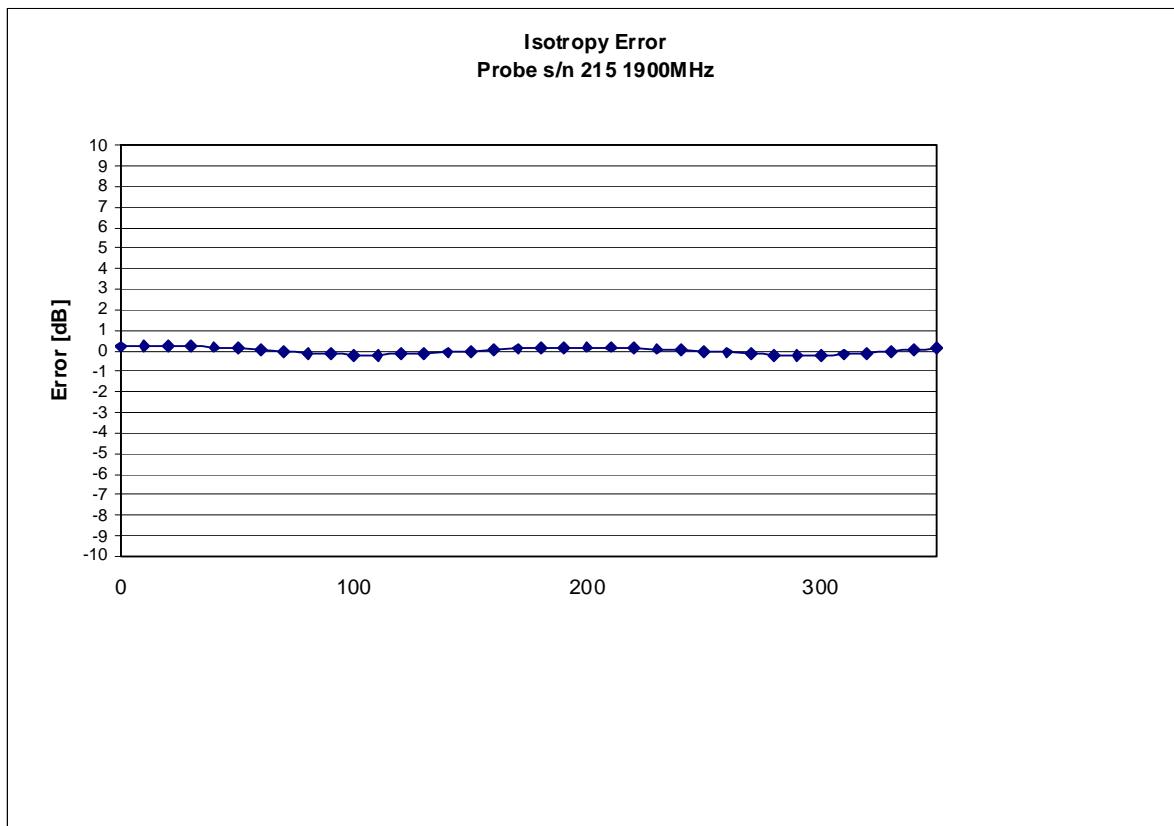Isotropy Error 1900 MHz (Air)**Isotropicity Tissue:**


0.10 dB

Dynamic Range

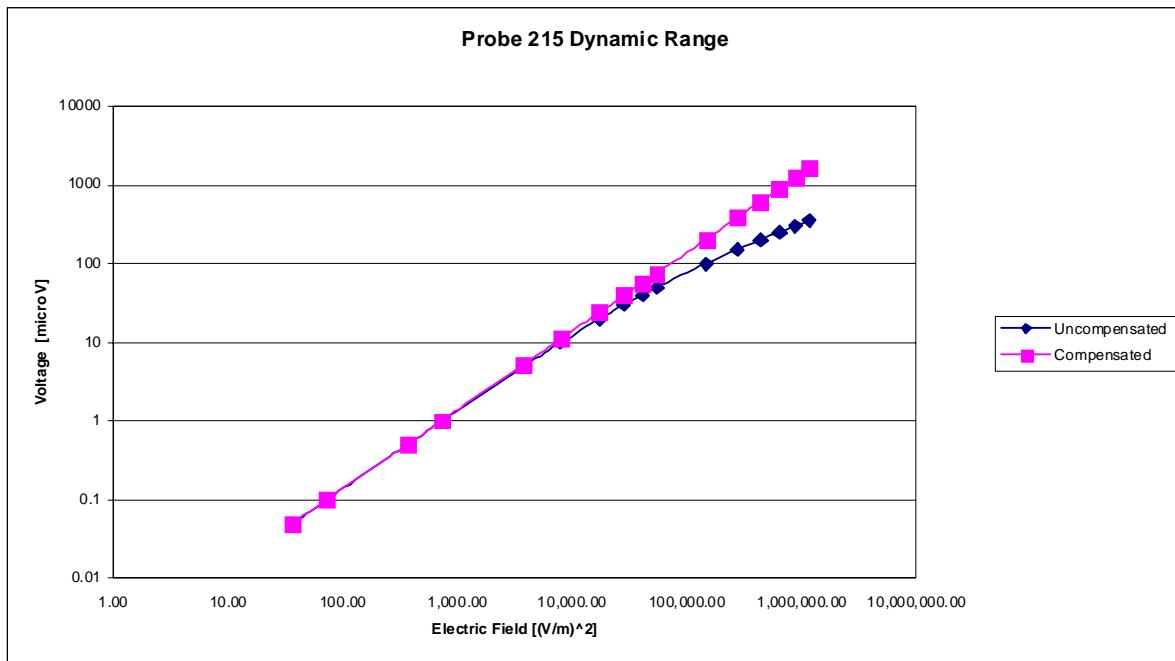

Video Bandwidth

Probe Frequency Characteristics

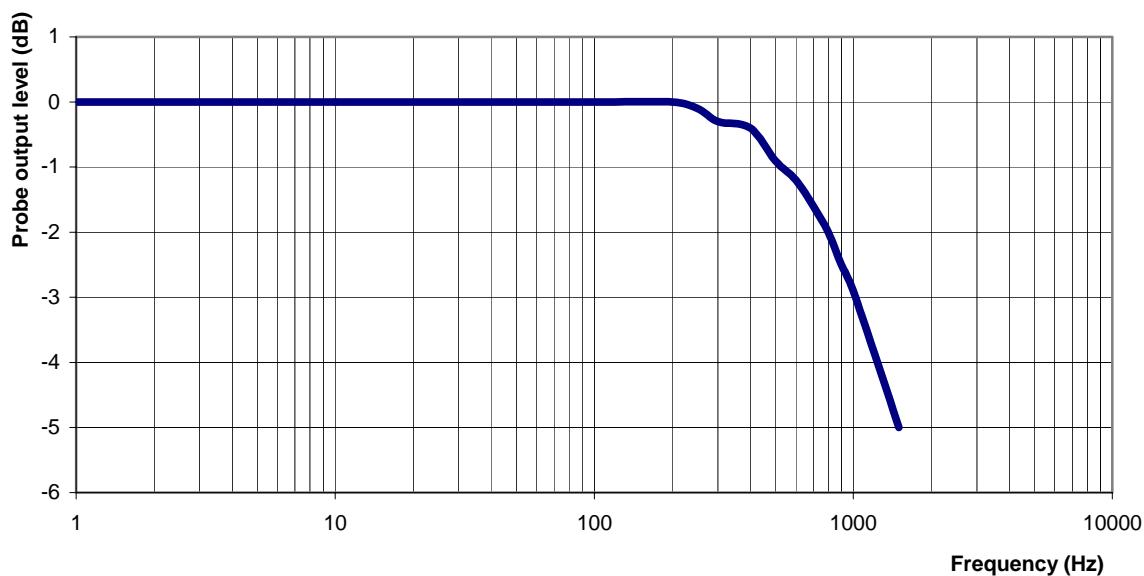

Video Bandwidth at 500 Hz 1 dB
Video Bandwidth at 1.02 KHz: 3 dB

Conversion Factor Uncertainty Assessment Measured

Sensitivity in Head Tissue

Frequency: 1900 MHz

Epsilon: 39.0 (+/-5%) **Sigma:** 1.43 S/m (+/-5%)

ConvF

Channel X: 4.9 7%(K=2)

Channel Y: 4.9 7%(K=2)

Channel Z: 4.9 7%(K=2)

To minimize the uncertainty calculation all tissue sensitivity values were calculated using a load impedance of 5 MΩ.

Boundary Effect:

For a distance of 2.5mm the evaluated uncertainty (increase in the probe sensitivity) is less than 2%.

Test Equipment

The test equipment used during Probe Calibration, manufacturer, model number and, current calibration status are listed and located on the main APREL server R:\NCL\Calibration Equipment\Instrument List May 2008.

NCL CALIBRATION LABORATORIES

Calibration File No.: CP-933

Client.: RFEL

C E R T I F I C A T E O F C A L I B R A T I O N

It is certified that the equipment identified below has been calibrated in the
NCL CALIBRATION LABORATORIES by qualified personnel following recognized
procedures and using transfer standards traceable to NRC/NIST.

Equipment: Miniature Isotropic RF Probe 1900 MHz

BODY Calibration

Manufacturer: APREL Laboratories

Model No.: E-020

Serial No.: 215

Calibration Procedure: SSI/DRB-TP-D01-032-E020-V2

Project No: RFEL-00150-CAL-5367

Calibrated: 3rd November 2008
Released on: 3rd November 2008

This Calibration Certificate is Incomplete Unless Accompanied with the Calibration Results Summary
This calibration has been conducted in line with the SCC ISO-IEC 17025 Scope of Accreditation

Accredited Laboratory Number 48

Released By: _____

NCL CALIBRATION LABORATORIES

51 SPECTRUM WAY
NEPEAN, ONTARIO
CANADA K2R 1E6

Division of APREL Lab.
TEL: (613) 820-4988
FAX: (613) 820-4161

NCL Calibration Laboratories

Division of APREL Laboratories.

Introduction

This Calibration Report reproduces the results of the calibration performed in line with the SSI/DRB-TP-D01-032-E020-V2 E-Field Probe Calibration Procedure. The results contained within this report are for APREL E-Field Probe E-020 215.

References


SSI/DRB-TP-D01-032-E020-V2 E-Field Probe Calibration Procedure
IEEE 1528 "Recommended Practice for Determining the Peak Spatial-Average Specific Absorption Rate (SAR) in the Human Body Due to Wireless Communications Devices: Experimental Techniques"
IEEE 1309 "IEEE Standard for Calibration of Electromagnetic Field Sensors and Probes, Excluding Antennas, from 9 KHz to 40 GHz" 2005
SSI-TP-011 Tissue Calibration Procedure
IEC 62209 "Human exposure to radio frequency fields from handheld and body-mounted wireless communication devices –Human models, instrumentation and procedures Part 1 & 2: Procedure to determine the Specific Absorption Rate (SAR) for handheld devices used in close proximity of the ear (frequency range of 200MHz to 3GHz)"

Conditions


Probe 215 was a re-calibration.

Ambient Temperature of the Laboratory: 22 °C +/- 0.5°C
Temperature of the Tissue: 21 °C +/- 0.5°C

We the undersigned attest that to the best of our knowledge the calibration of this probe has been accurately conducted and that all information contained within this report has been reviewed for accuracy.



Stuart Nicol



Jesse Hones

Calibration Results Summary

Probe Type:	E-Field Probe E-020
Serial Number:	215
Frequency:	1900 MHz
Sensor Offset:	1.56 mm
Sensor Length:	2.5 mm
Tip Enclosure:	Ertalyte*
Tip Diameter:	<5 mm
Tip Length:	60 mm
Total Length:	290 mm

*Resistive to recommended tissue recipes per IEEE-1528

Sensitivity in Air

Channel X:	$1.2 \mu\text{V}/(\text{V}/\text{m})^2$
Channel Y:	$1.2 \mu\text{V}/(\text{V}/\text{m})^2$
Channel Z:	$1.2 \mu\text{V}/(\text{V}/\text{m})^2$
Diode Compression Point:	95 mV

Sensitivity in Body Tissue Measured

Frequency: 1900 MHz

Epsilon: 54.2 (+/-5%) **Sigma:** 1.57 S/m (+/-5%)

ConvF

Channel X: 5.0

Channel Y: 5.0

Channel Z: 5.0

Tissue sensitivity values were calculated using the load impedance of the APREL Laboratories Daq-Paq.


Boundary Effect:



Uncertainty resulting from the boundary effect is less than 2% for the distance between the tip of the probe and the tissue boundary, when less than 2.44mm.

Spatial Resolution:

The measured probe tip diameter is 5 mm (+/- 0.01 mm) and therefore meets the requirements of SSI/DRB-TP-D01-032 for spatial resolution.


Receiving Pattern 1900 MHz (Air)

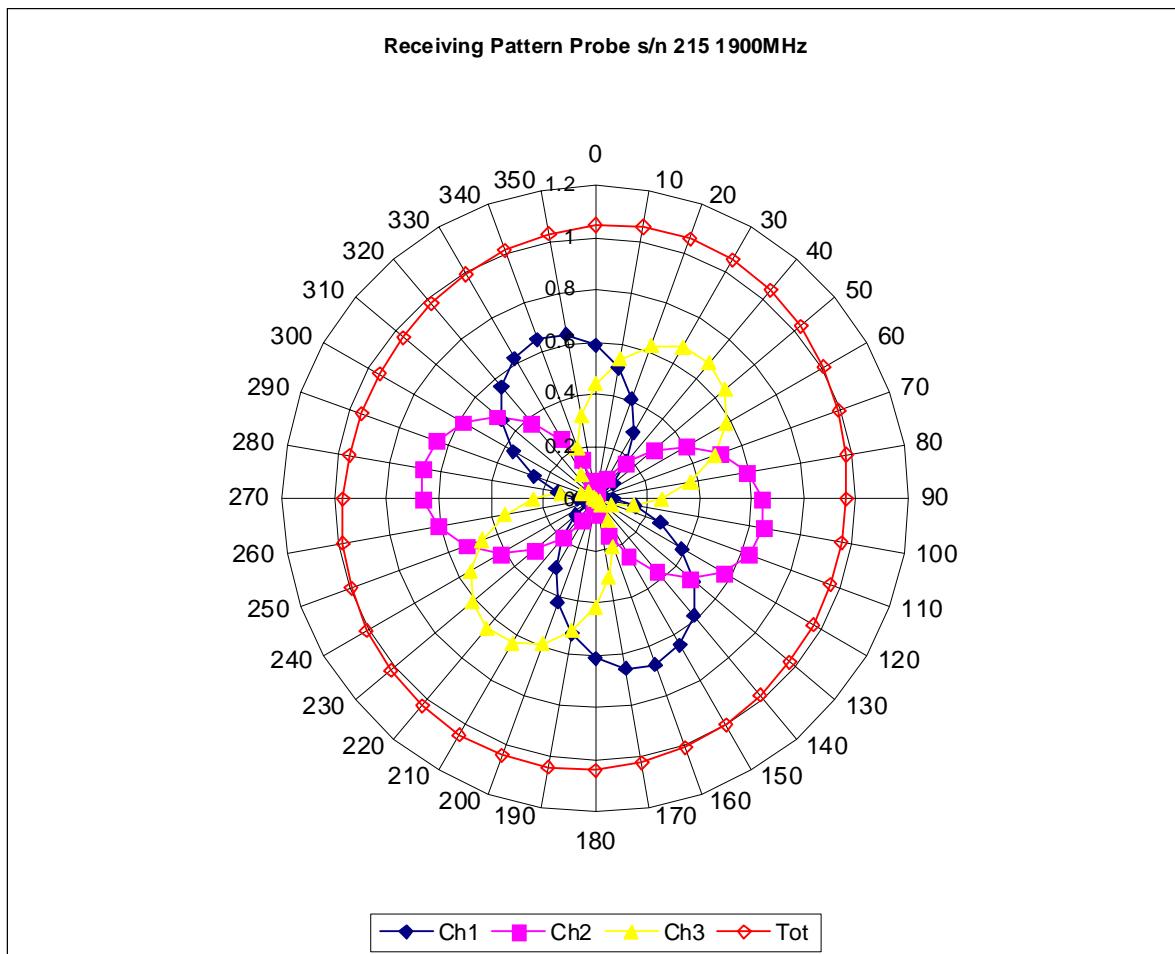

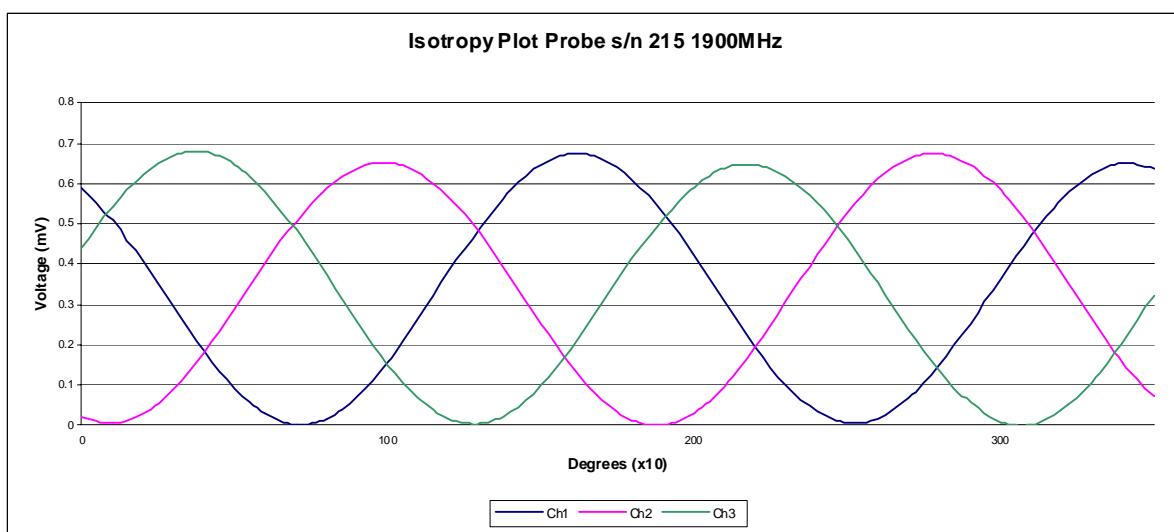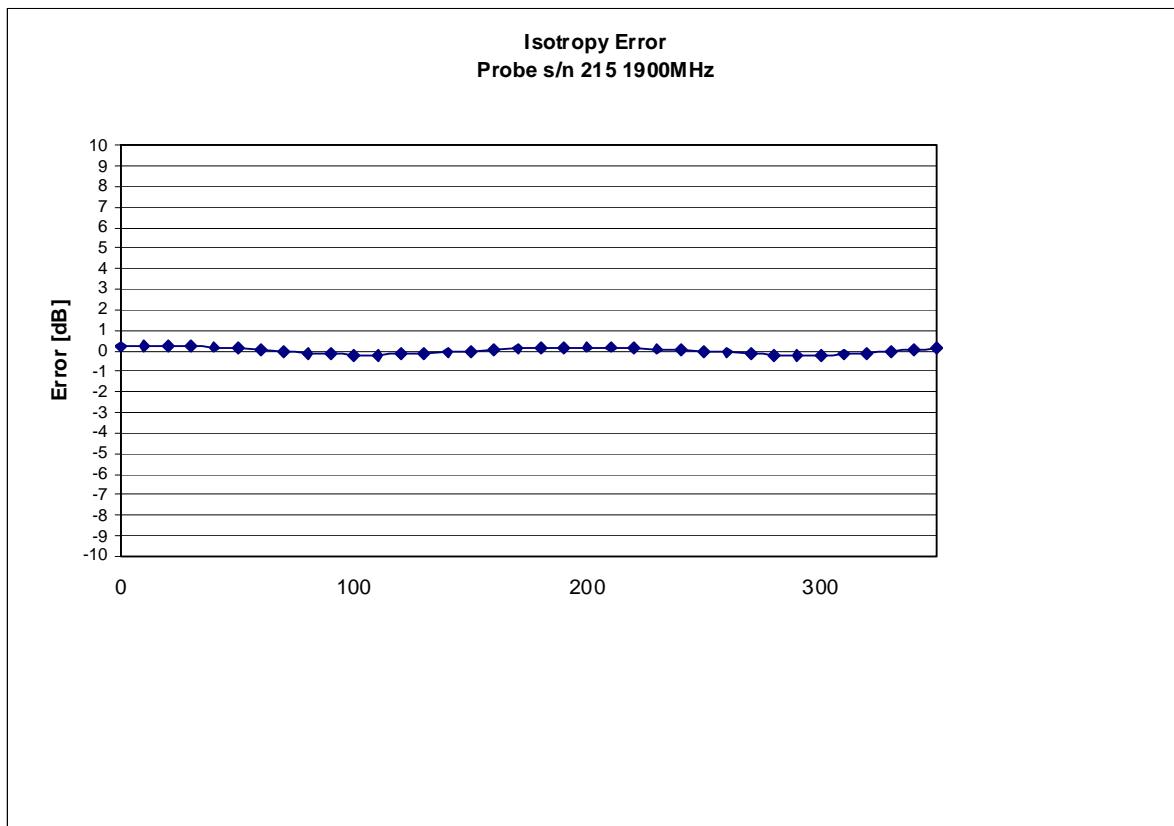Isotropy Error 1900 MHz (Air)**Isotropicity Tissue:**


0.10 dB

Dynamic Range

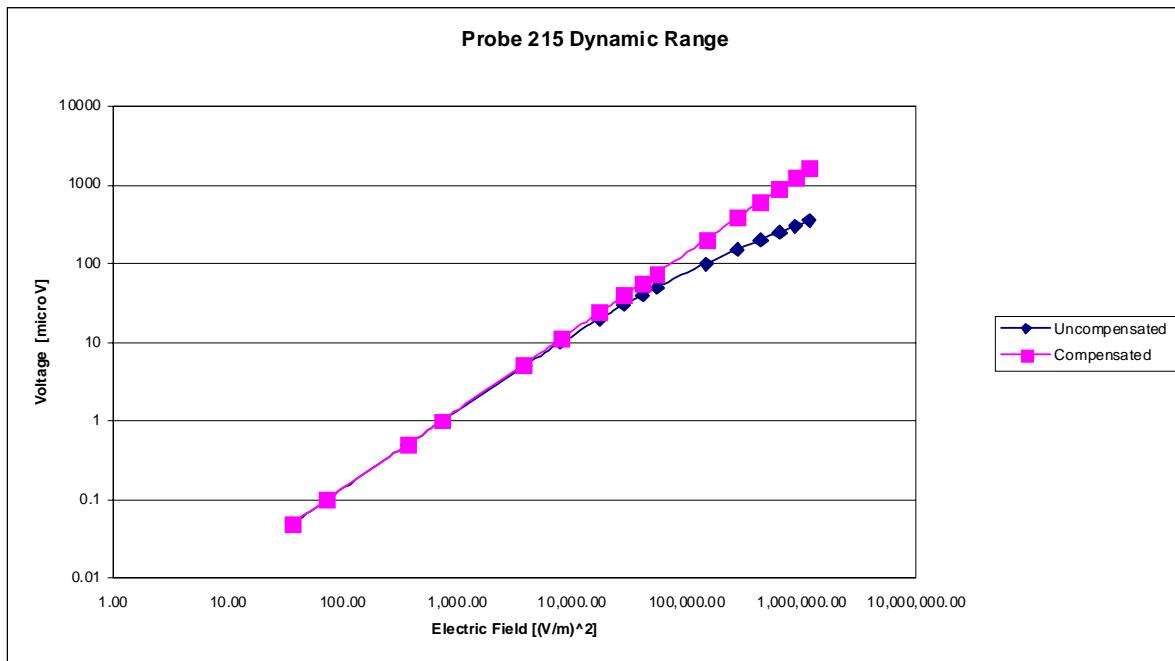

Video Bandwidth

Probe Frequency Characteristics

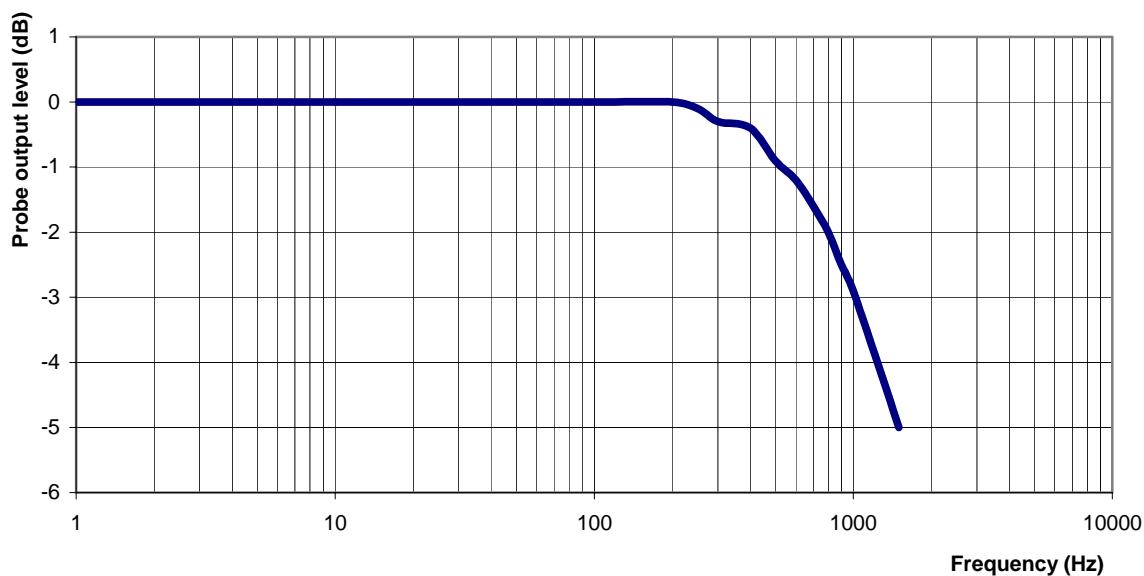

Video Bandwidth at 500 Hz 1 dB
Video Bandwidth at 1.02 KHz: 3 dB

Conversion Factor Uncertainty Assessment Measured

Sensitivity in Body Tissue

Frequency: 1900 MHz

Epsilon: 54.2 (+/-5%) **Sigma:** 1.57 S/m (+/-5%)

ConvF

Channel X: 5.0 7%(K=2)

Channel Y: 5.0 7%(K=2)

Channel Z: 5.0 7%(K=2)

To minimize the uncertainty calculation all tissue sensitivity values were calculated using a load impedance of 5 MΩ.

Boundary Effect:

For a distance of 2.5mm the evaluated uncertainty (increase in the probe sensitivity) is less than 2%.

Test Equipment

The test equipment used during Probe Calibration, manufacturer, model number and, current calibration status are listed and located on the main APREL server R:\NCL\Calibration Equipment\Instrument List May 2008.

Appendix E – Dipole Calibration Data Sheets

RF Exposure Lab, LLC

Calibration File No: CAL.20080203

C E R T I F I C A T E O F C A L I B R A T I O N

It is certified that the equipment identified below has been calibrated at RF Exposure Lab, LLC by qualified personnel following recognized procedures and using transfer standards traceable to NRC/NIST.

Validation Dipole

Manufacturer: APREL Laboratories

Part Number: ALS-D-835-S-2

Frequency: 835 MHz

Serial No: RFE-274

Manufactured: 20 February 2004

Calibrated: 22 February 2008

Calibrated By: Signature on File
Jay Moulton – Technical Manager

Approved By: Signature on File
Tamara Moulton – Quality Manager

Measurement Uncertainty:

Repeatability:	2.3%
Tissue Uncertainty:	3.2%
Network Analyzer:	2.5%



RF EXPOSURE LAB, LLC

2867 Progress Place, Suite 4D
Escondido, CA 92029

Tel: (760) 737-3131
FAX: (760) 737-9131

Calibration Results Summary

The following results relate to the Calibrated Dipole and should be used as a quick reference for the user.

Mechanical Dimensions

Length: 161.8 mm
Height: 91.1 mm

Electrical Specifications

Head

SWR: 1.1182 U
Return Loss: -27.508 dB
Impedance: 49.648 Ω

System Validation Results

Frequency	1 Gram	10 Gram
835 MHz	9.500	6.000

Body

SWR: 1.1533 U
Return Loss: -23.596 dB
Impedance: 51.395 Ω

System Validation Results

Frequency	1 Gram	10 Gram
835 MHz	9.750	6.240

Head Measurement Conditions

The measurements were performed in the Uni-Phantom filled with head simulating liquid of the following electrical parameters at 835 MHz:

Relative Dielectricity	41.48	± 5%
Conductivity	0.92 mho/m	± 5%

The APREL Laboratories ALSAS system with a dosimetric E-field probe E-020 (SN:217, Conversion factor 6.0 at 835 MHz) was used for the measurements.

The dipole was mounted so that the dipole feed point was positioned below the center marking of the flat phantom and the dipole was oriented parallel to the body axis (the long side of the phantom). The standard measuring distance was 15mm from the dipole center to the solution surface.

The coarse grid with a grid spacing of 10mm was aligned with the dipole. The 5x5x8 fine cube was chosen for cube integration. The dipole input power (forward power) was 100mW ± 3%. The results are normalized to 1W input power.

The laboratories environmental conditions were as follows during the calibration sequence.


Ambient Temperature of the Laboratory:	24 °C ± 1.0 °C
Temperature of the Tissue:	20 °C ± 1.0 °C
Relative Humidity:	40%

SAR Measurement

Standard SAR measurements were performed according to the measurement conditions described above. The results have been normalized to a dipole input power of 1W (forward power). The resulting averaged SAR values measured with the dosimetric probe E-020 SN:217 and applying the advanced extrapolation are:

Averaged over 1 cm³ (1 g) of tissue: 9.500 mW/g ± 19.0% (k=2)¹

Averaged over 10 cm³ (10 g) of tissue: 6.000 mW/g ± 18.5% (k=2)¹

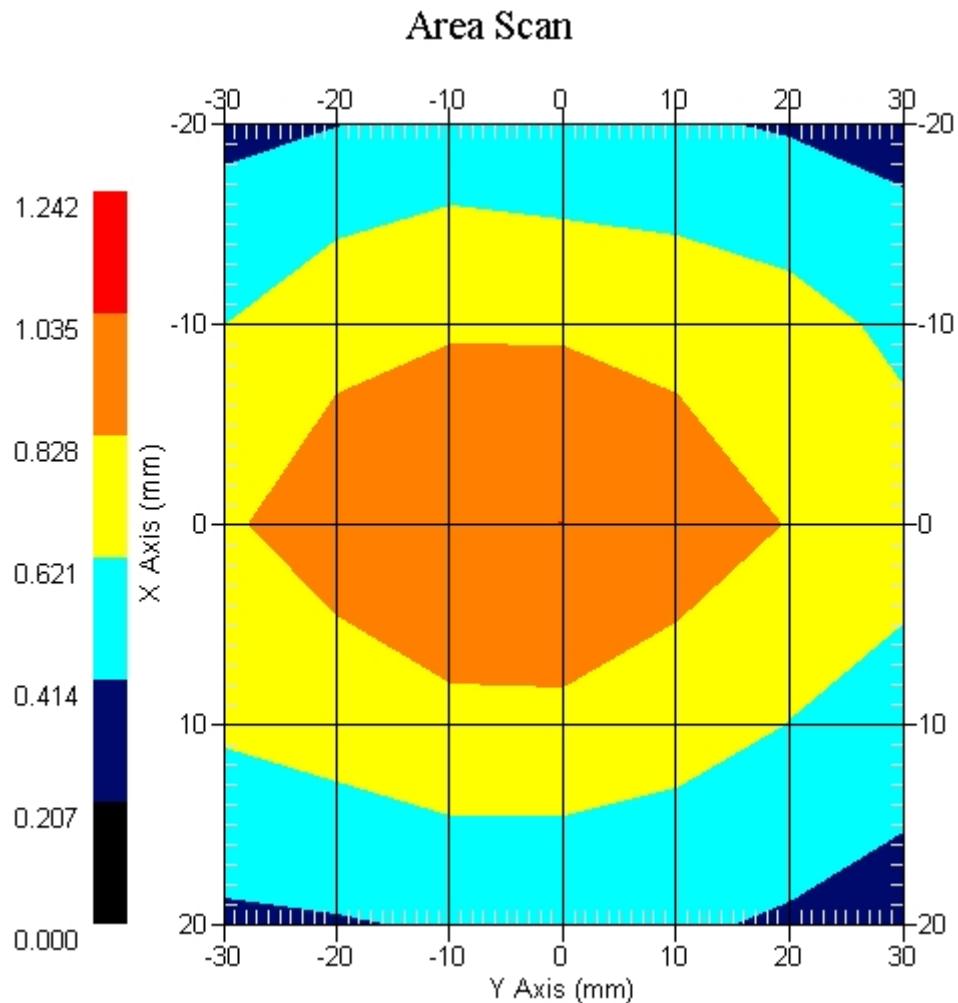

1 gram SAR value : 0.950 W/kg

10 gram SAR value : 0.600 W/kg

Area Scan Peak SAR : 1.037 W/kg

Zoom Scan Peak SAR : 1.541 W/kg

¹ validation uncertainty


Dipole Impedance and Return Loss



The impedance was measured at the SMA connector with a network analyzer. The dipole was positioned at the flat phantom sections according to measurement conditions stated above during impedance measurements.

Test	Result
S11 R/L	-27.508 dB
SWR	1.1182 U
Impedance	49.648 Ω

The following graphs are the results as displayed on the Vector Network Analyzer.

S11 Parameter Return Loss

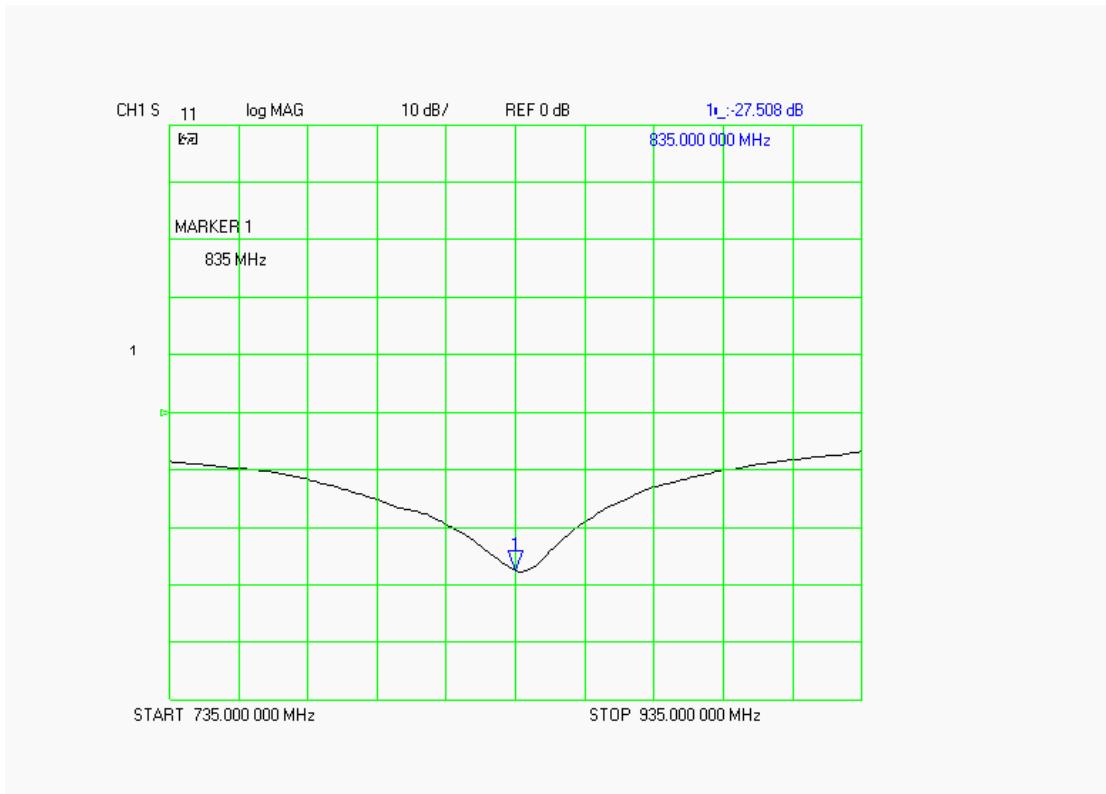

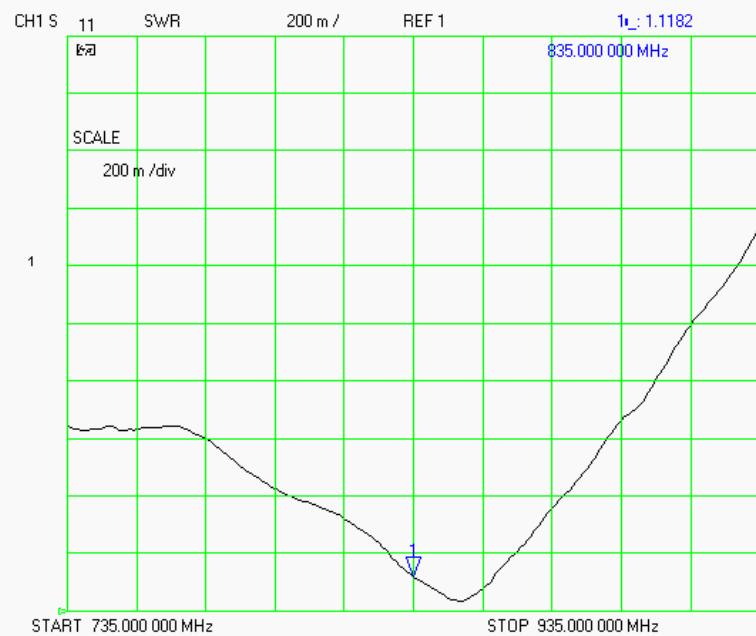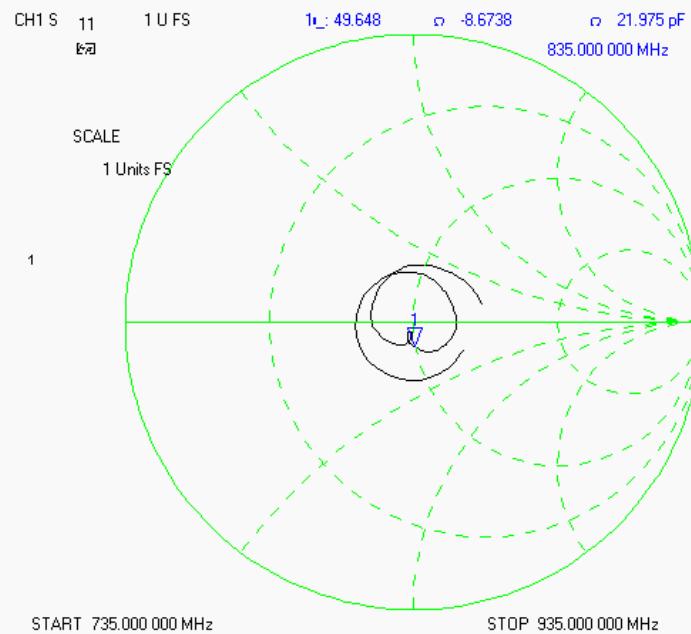SWR

Smith Chart Dipole Impedance


Body Measurement Conditions

The measurements were performed in the Uni-Phantom filled with body simulating liquid of the following electrical parameters at 835 MHz:

Relative Dielectricity	55.20	± 5%
Conductivity	0.96 mho/m	± 5%

The APREL Laboratories ALSAS system with a dosimetric E-field probe E-020 (SN:217, Conversion factor 6.1 at 835 MHz) was used for the measurements.

The dipole was mounted so that the dipole feed point was positioned below the center marking of the flat phantom and the dipole was oriented parallel to the body axis (the long side of the phantom). The standard measuring distance was 15mm from the dipole center to the solution surface.

The coarse grid with a grid spacing of 10mm was aligned with the dipole. The 5x5x8 fine cube was chosen for cube integration. The dipole input power (forward power) was 100mW ± 3%. The results are normalized to 1W input power.

The laboratories environmental conditions were as follows during the calibration sequence.

Ambient Temperature of the Laboratory:	24 °C ± 1.0 °C
Temperature of the Tissue:	20 °C ± 1.0 °C
Relative Humidity:	40%


SAR Measurement

Standard SAR measurements were performed according to the measurement conditions described above. The results have been normalized to a dipole input power of 1W (forward power). The resulting averaged SAR values measured with the dosimetric probe E-020 SN:217 and applying the advanced extrapolation are:

Averaged over 1 cm³ (1 g) of tissue: 9.750 mW/g ± 19.1% (k=2)¹

Averaged over 10 cm³ (10 g) of tissue: 6.240 mW/g ± 18.6% (k=2)¹

Area Scan

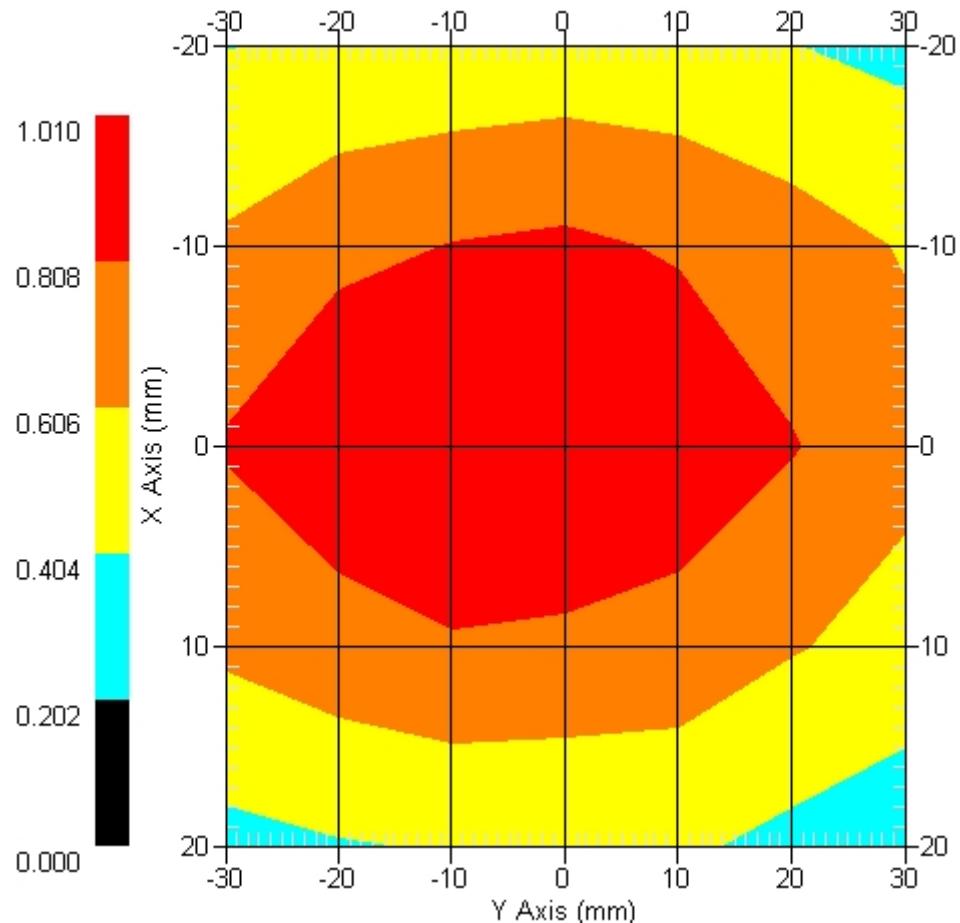

1 gram SAR value : 0.975 W/kg

10 gram SAR value : 0.624 W/kg

Area Scan Peak SAR : 1.009 W/kg

Zoom Scan Peak SAR : 1.571 W/kg

¹ validation uncertainty


Dipole Impedance and Return Loss



The impedance was measured at the SMA connector with a network analyzer. The dipole was positioned at the flat phantom sections according to measurement conditions stated above during impedance measurements.

Test	Result
S11 R/L	-23.596 dB
SWR	1.1533 U
Impedance	51.395 Ω

The following graphs are the results as displayed on the Vector Network Analyzer.

S11 Parameter Return Loss

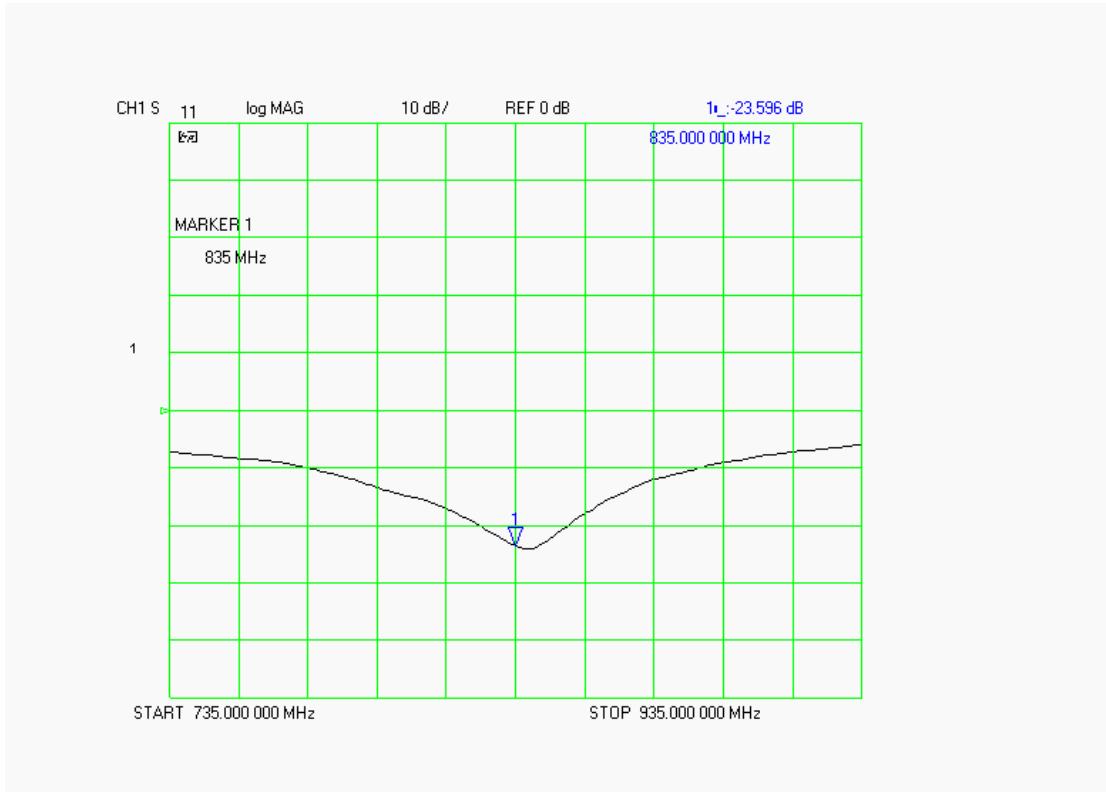

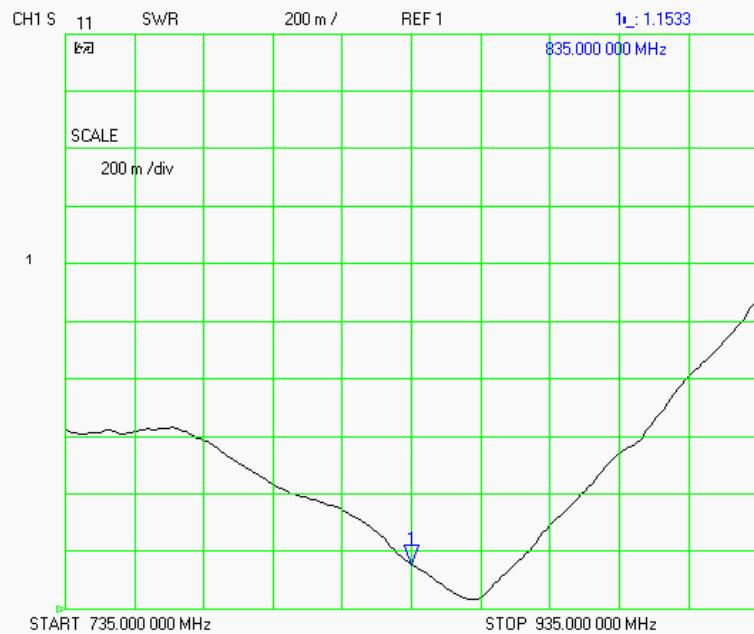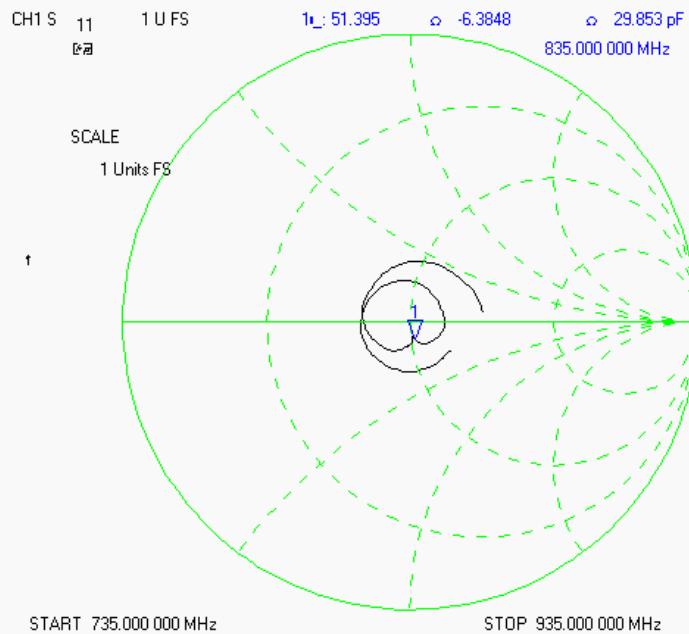SWR

Smith Chart Dipole Impedance


Test Equipment List

The test equipment used during Dipole Calibration, manufacturer, model number and, current calibration status are listed and located on the RF Exposure Lab, LLC system computer C:\Test Equipment\Calibration Equipment\Instrument List February 2008.

RF Exposure Lab, LLC

Calibration File No: CAL.20080202

C E R T I F I C A T E O F C A L I B R A T I O N

It is certified that the equipment identified below has been calibrated at RF Exposure Lab, LLC by qualified personnel following recognized procedures and using transfer standards traceable to NRC/NIST.

Validation Dipole

Manufacturer: APREL Laboratories

Part Number: ALS-D-1900-S-2

Frequency: 1.9 GHz

Serial No: RFE-277

Manufactured: 20 February 2004

Calibrated: 21 February 2008

Calibrated By: Signature on File
Jay Moulton – Technical Manager

Approved By: Signature on File
Tamara Moulton – Quality Manager

Measurement Uncertainty:

Repeatability:	2.3%
Tissue Uncertainty:	3.2%
Network Analyzer:	2.5%



RF EXPOSURE LAB, LLC

2867 Progress Place, Suite 4D
Escondido, CA 92029

Tel: (760) 737-3131
FAX: (760) 737-9131

Calibration Results Summary

The following results relate to the Calibrated Dipole and should be used as a quick reference for the user.

Mechanical Dimensions

Length: 68.0 mm
Height: 37.5 mm

Electrical Specifications

Head

SWR: 1.0793 U
Return Loss: -38.514 dB
Impedance: 49.063 Ω

System Validation Results

Frequency	1 Gram	10 Gram
1.9 GHz	39.380	20.270

Body

SWR: 1.1006 U
Return Loss: -41.682 dB
Impedance: 53.580 Ω

System Validation Results

Frequency	1 Gram	10 Gram
1.9 GHz	40.990	21.090

Head Measurement Conditions

The measurements were performed in the Uni-Phantom filled with head simulating liquid of the following electrical parameters at 1900 MHz:

Relative Dielectricity	39.97	± 5%
Conductivity	1.41 mho/m	± 5%

The APREL Laboratories ALSAS system with a dosimetric E-field probe E-020 (SN:217, Conversion factor 4.65 at 1900 MHz) was used for the measurements.

The dipole was mounted so that the dipole feed point was positioned below the center marking of the flat phantom and the dipole was oriented parallel to the body axis (the long side of the phantom). The standard measuring distance was 10mm from the dipole center to the solution surface.

The coarse grid with a grid spacing of 10mm was aligned with the dipole. The 5x5x8 fine cube was chosen for cube integration. The dipole input power (forward power) was 100mW ± 3%. The results are normalized to 1W input power.

The laboratories environmental conditions were as follows during the calibration sequence.

Ambient Temperature of the Laboratory:	23 °C ± 1.0 °C
Temperature of the Tissue:	20 °C ± 1.0 °C
Relative Humidity:	40%


SAR Measurement

Standard SAR measurements were performed according to the measurement conditions described above. The results have been normalized to a dipole input power of 1W (forward power). The resulting averaged SAR values measured with the dosimetric probe E-020 SN:217 and applying the advanced extrapolation are:

Averaged over 1 cm³ (1 g) of tissue: 39.380 mW/g ± 19.2% (k=2)¹

Averaged over 10 cm³ (10 g) of tissue: 20.270 mW/g ± 18.8% (k=2)¹

Area Scan

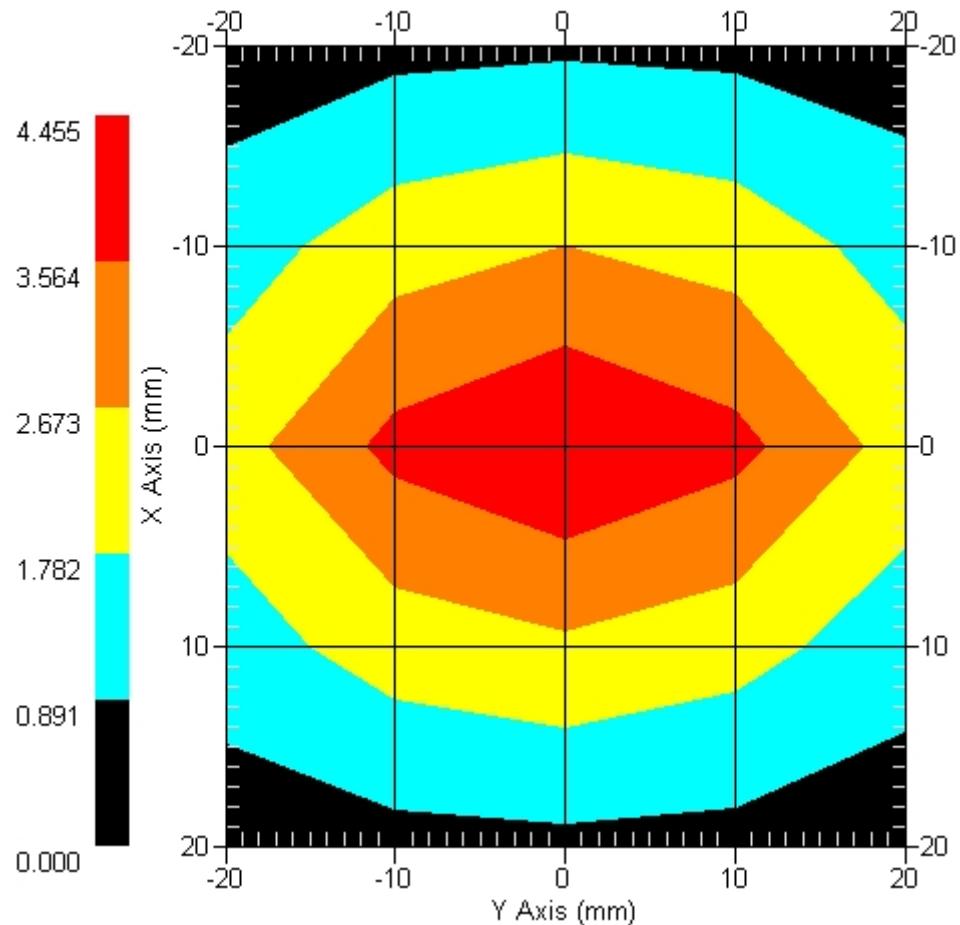

1 gram SAR value : 3.938 W/kg

10 gram SAR value : 2.027 W/kg

Area Scan Peak SAR : 4.455 W/kg

Zoom Scan Peak SAR : 7.246 W/kg

¹ validation uncertainty


Dipole Impedance and Return Loss

The impedance was measured at the SMA connector with a network analyzer. The dipole was positioned at the flat phantom sections according to measurement conditions stated above during impedance measurements.


Test	Result
S11 R/L	-38.514 dB
SWR	1.0793 U
Impedance	49.063 Ω

The following graphs are the results as displayed on the Vector Network Analyzer.


S11 Parameter Return Loss

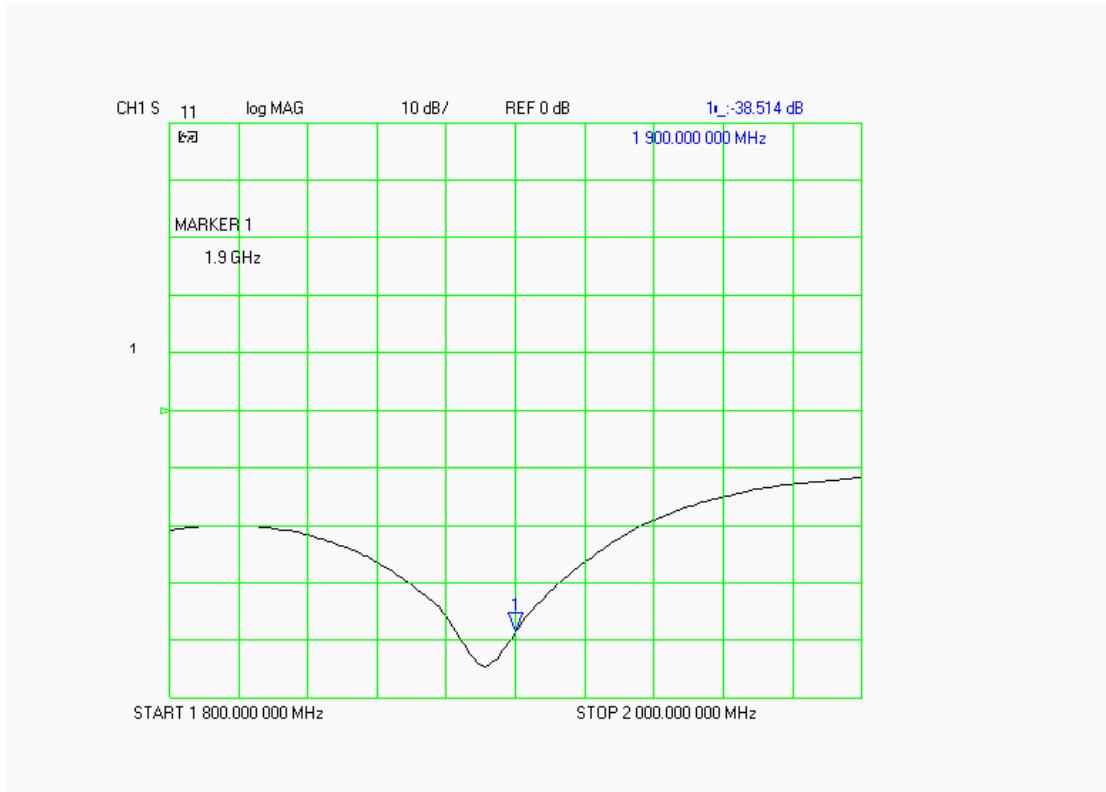

SWR

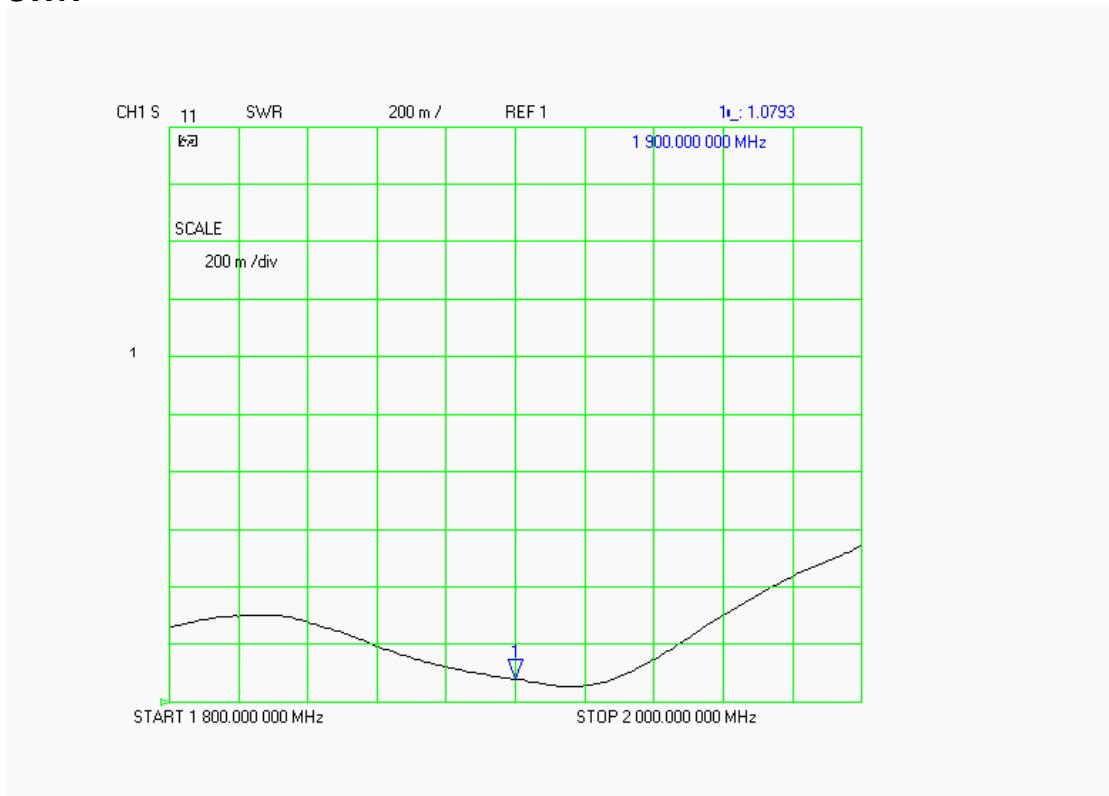

Smith Chart Dipole Impedance

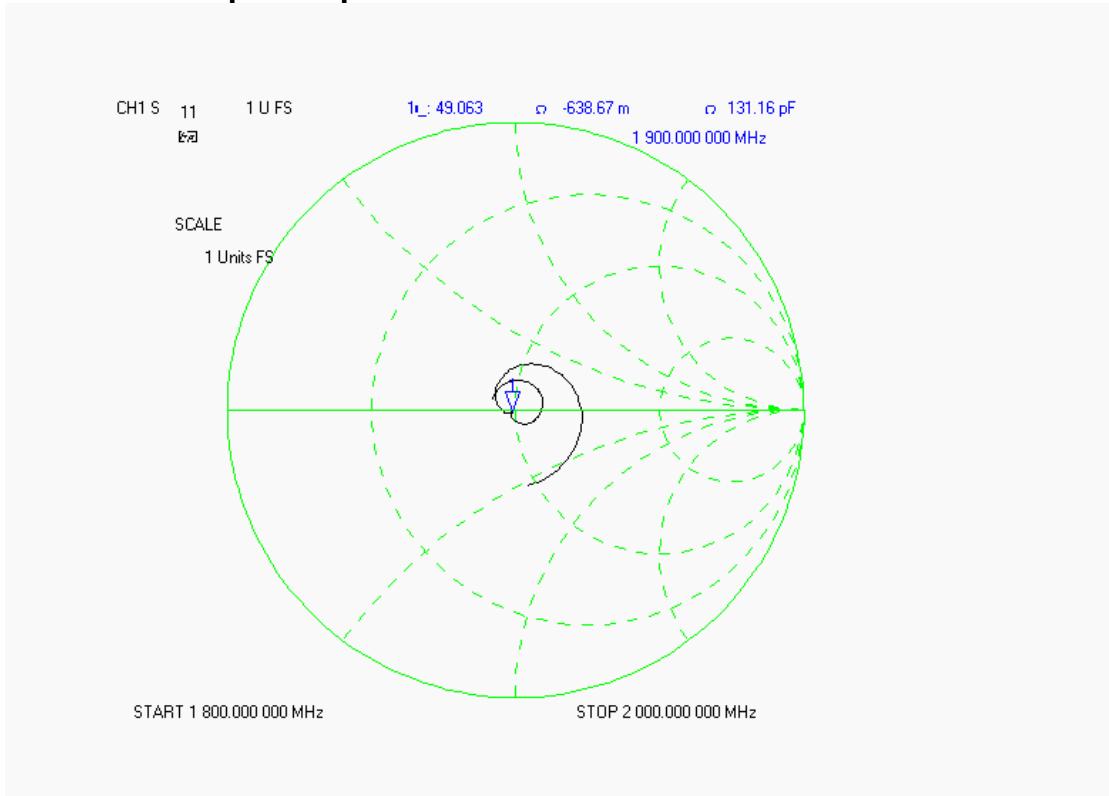

Body Measurement Conditions

The measurements were performed in the Uni-Phantom filled with body simulating liquid of the following electrical parameters at 1900 MHz:

Relative Dielectricity	53.27	± 5%
Conductivity	1.50 mho/m	± 5%

The APREL Laboratories ALSAS system with a dosimetric E-field probe E-020 (SN:217, Conversion factor 4.85 at 1900 MHz) was used for the measurements.

The dipole was mounted so that the dipole feed point was positioned below the center marking of the flat phantom and the dipole was oriented parallel to the body axis (the long side of the phantom). The standard measuring distance was 10mm from the dipole center to the solution surface.

The coarse grid with a grid spacing of 10mm was aligned with the dipole. The 5x5x8 fine cube was chosen for cube integration. The dipole input power (forward power) was 100mW ± 3%. The results are normalized to 1W input power.

The laboratories environmental conditions were as follows during the calibration sequence.

Ambient Temperature of the Laboratory:	23 °C ± 1.0 °C
Temperature of the Tissue:	20 °C ± 1.0 °C
Relative Humidity:	40%


SAR Measurement

Standard SAR measurements were performed according to the measurement conditions described above. The results have been normalized to a dipole input power of 1W (forward power). The resulting averaged SAR values measured with the dosimetric probe E-020 SN:217 and applying the advanced extrapolation are:

Averaged over 1 cm³ (1 g) of tissue: 40.990 mW/g ± 18.9% (k=2)¹

Averaged over 10 cm³ (10 g) of tissue: 21.090 mW/g ± 18.5% (k=2)¹

Area Scan

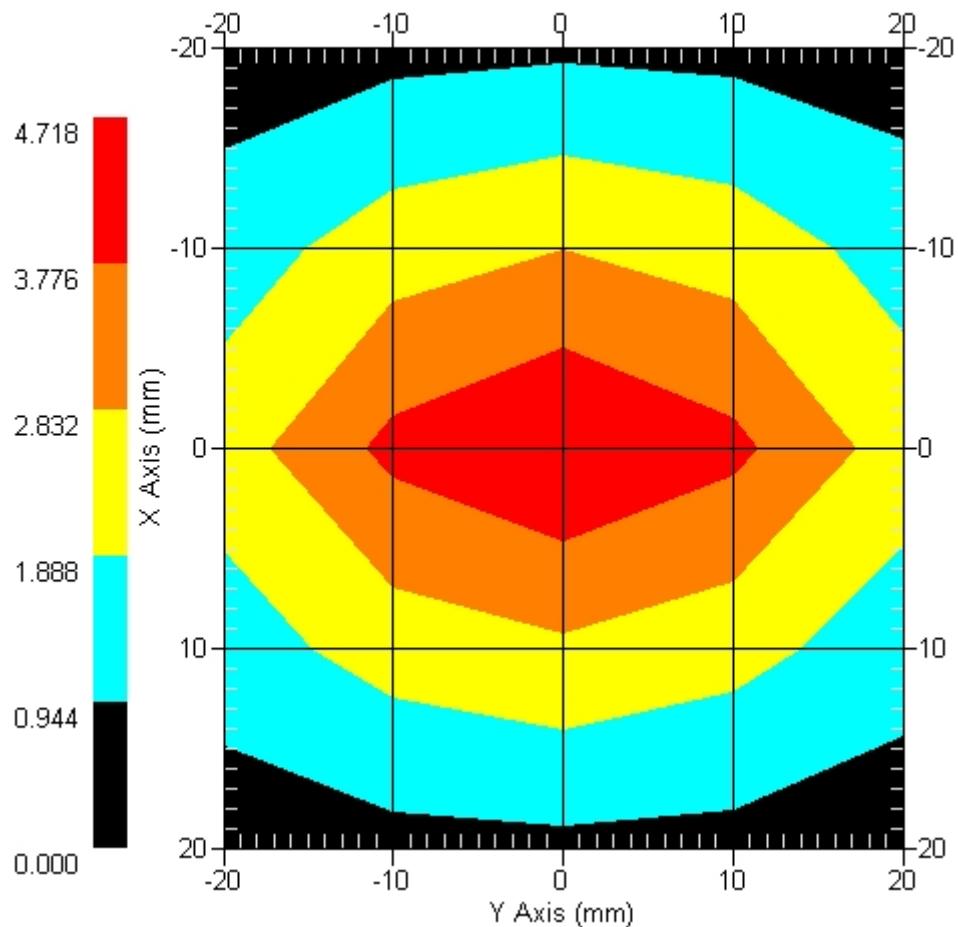

1 gram SAR value : 4.099 W/kg

10 gram SAR value : 2.109 W/kg

Area Scan Peak SAR : 4.718 W/kg

Zoom Scan Peak SAR : 7.606 W/kg

¹ validation uncertainty


Dipole Impedance and Return Loss

The impedance was measured at the SMA connector with a network analyzer. The dipole was positioned at the flat phantom sections according to measurement conditions stated above during impedance measurements.


Test	Result
S11 R/L	-41.682 dB
SWR	1.1006 U
Impedance	53.580 Ω

The following graphs are the results as displayed on the Vector Network Analyzer.


S11 Parameter Return Loss

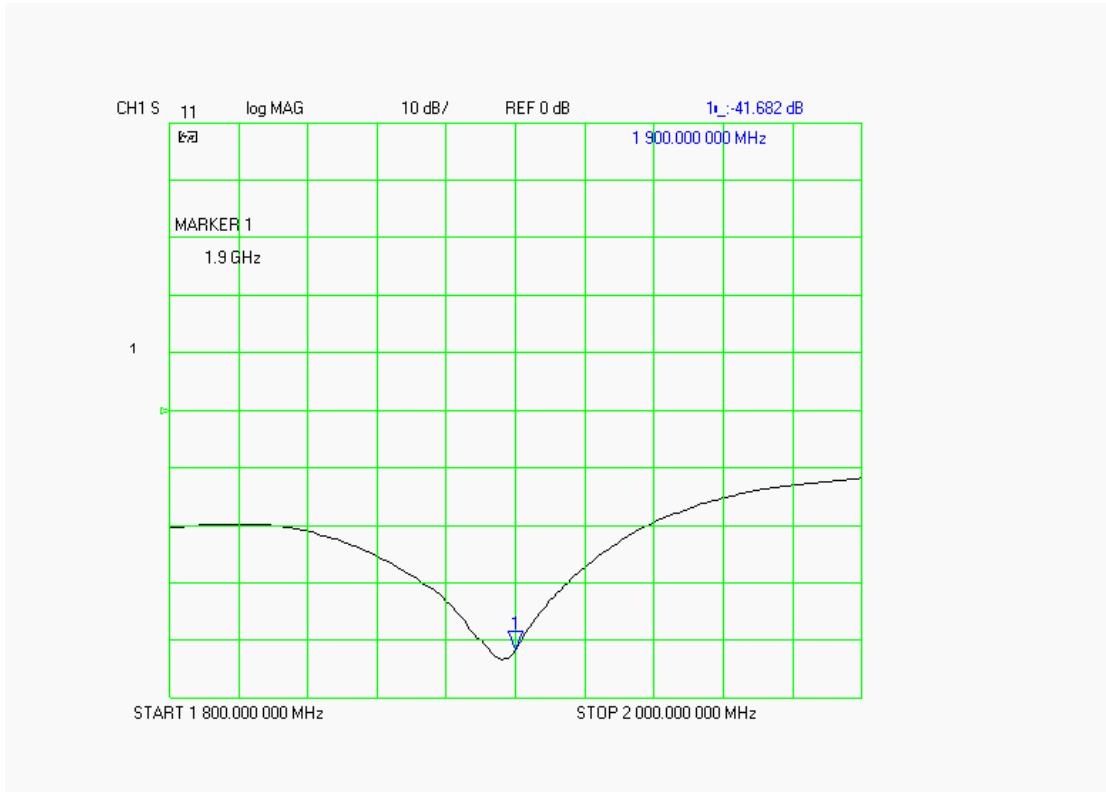

SWR

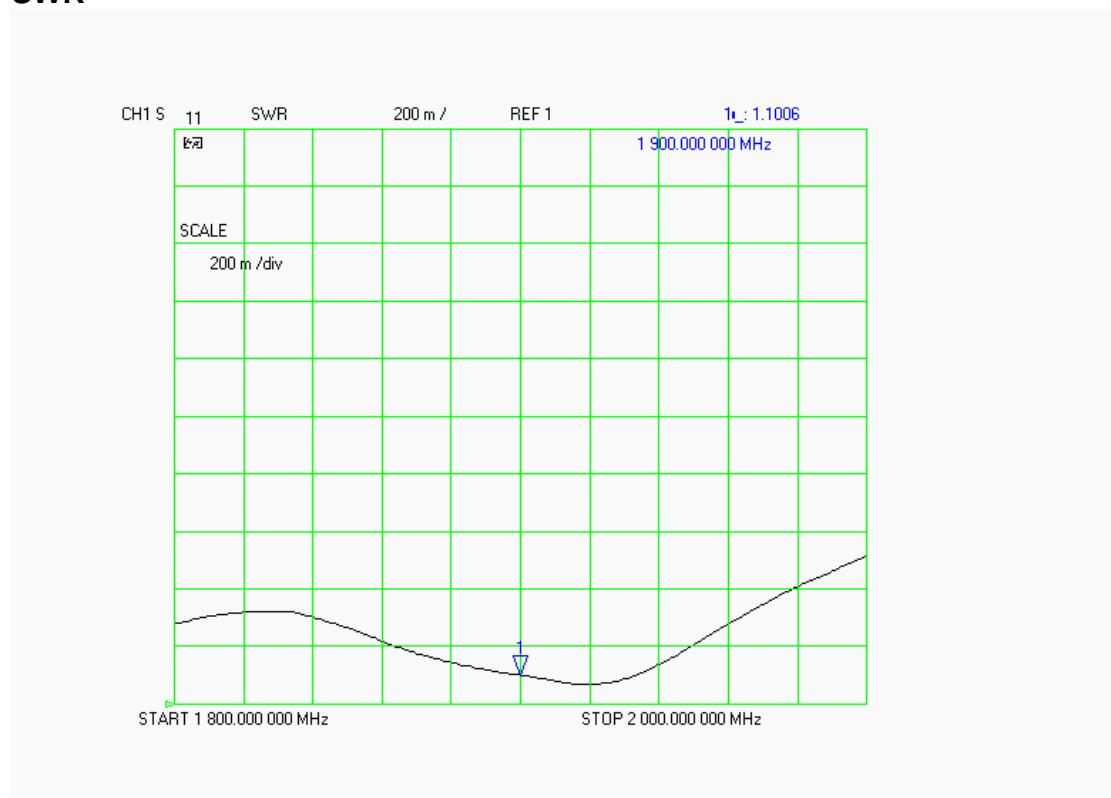

Smith Chart Dipole Impedance

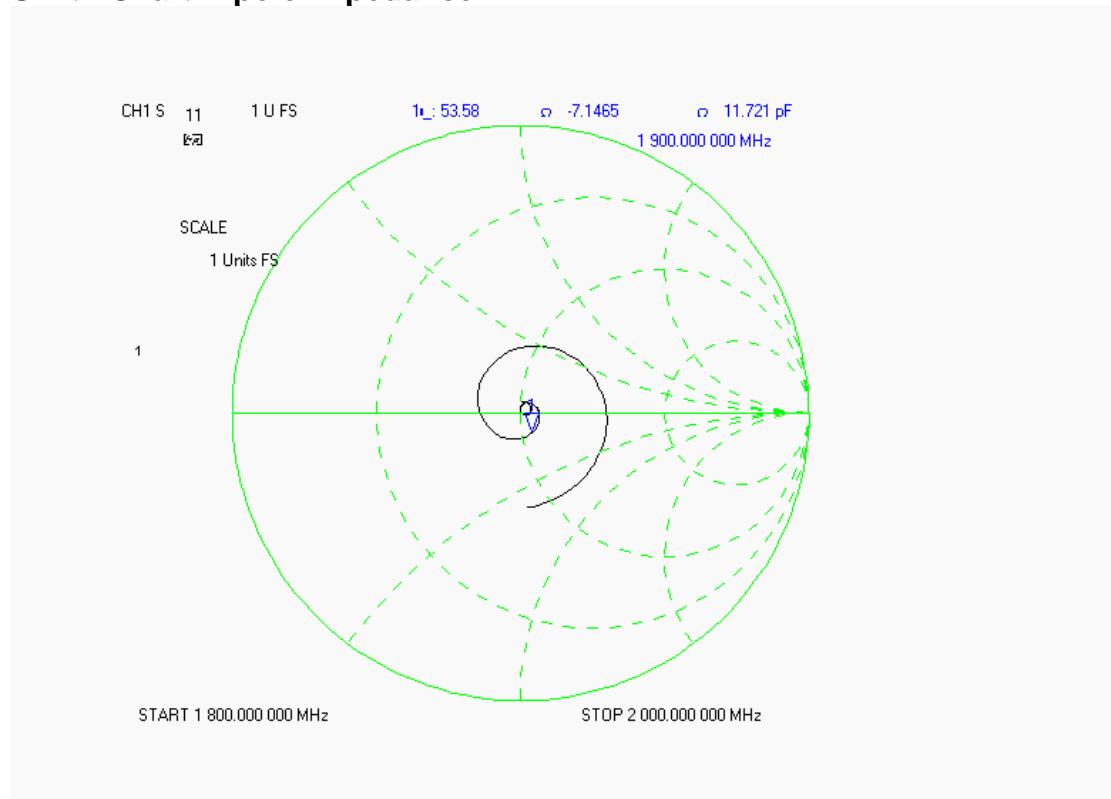

Test Equipment List

The test equipment used during Dipole Calibration, manufacturer, model number and, current calibration status are listed and located on the RF Exposure Lab, LLC system computer C:\Test Equipment\Calibration Equipment\Instrument List February 2008.

Appendix F – Phantom Calibration Data Sheets

NCL CALIBRATION LABORATORIES

Calibration File No.: RFE-273

CERTIFICATE OF CALIBRATION

It is certified that the equipment identified below has been calibrated in the
NCL CALIBRATION LABORATORIES by qualified personnel following recognized
procedures and using transfer standards traceable to National Standards.

Thickness of the UniPhantom is 2 mm \pm 10%
Pinna thickness is 6 mm \pm 10%

Resolution: 0.01 mm Calibrated to: 0.0 mm
Stability: OK Accuracy: < 0.1 mm

Calibrated By:

Karen K. Feb 17/04

NCL CALIBRATION LABORATORIES

51 SPECTRUM WAY
NEPEAN, ONTARIO
CANADA K2R 1E6

Division of APREL Lab.
TEL: (613) 820-4988
FAX: (613) 820-4161