

**20160406\_System check\_Diple5GHzv2 SN1004**

Frequency: 5200 MHz; Duty Cycle: 1:1; Room Ambient Temperature: 25.0°C; Liquid Temperature: 24.0°C

Medium parameters used (interpolated):  $f = 5200$  MHz;  $\sigma = 5.41$  mho/m;  $\epsilon_r = 49.4$ ;  $\rho = 1000$  kg/m<sup>3</sup>;

DASY4 Configuration:

- Area Scan setting - Find Secondary Maximum Within: 2.0 dB and with a peak SAR value greater than 0.0012W/kg
- Electronics: DAE4 Sn558; Calibrated: 7/16/2015
- Probe: EX3DV4 - SN3554; ConvF(3.85, 3.85, 3.85); Calibrated: 10/1/2015
- Sensor-Surface: 2.5mm (Mechanical Surface Detection)
- Phantom: Flat Phantom ELI4.0; Type: QDOVA001BA; Serial: SN: 1052

**Body/5200MHz,Pin=100mW,d= 2/Area Scan (7x7x1):** Measurement grid: dx=10mm, dy=10mm

[Info: Interpolated medium parameters used for SAR evaluation.](#)

Maximum value of SAR (measured) = 13.8 mW/g

**Body/5200MHz,Pin=100mW,d= 2/Zoom Scan (8x8x9)/Cube 0:** Measurement grid: dx=4mm, dy=4mm, dz=2.5mm


Reference Value = 54.1 V/m; Power Drift = -0.084 dB

Peak SAR (extrapolated) = 27.4 W/kg

**SAR(1 g) = 7.55 mW/g; SAR(10 g) = 2.12 mW/g**

[Info: Interpolated medium parameters used for SAR evaluation.](#)

Maximum value of SAR (measured) = 12.9 mW/g

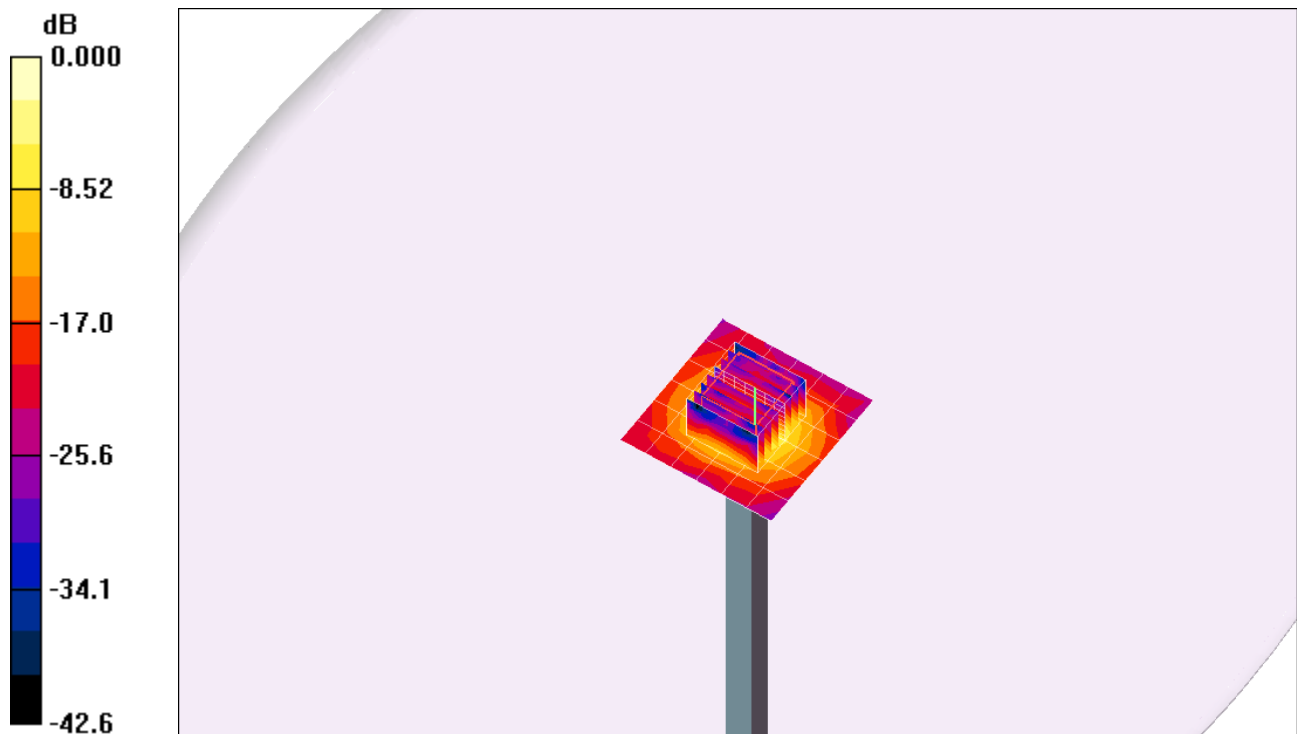


0 dB = 12.9mW/g

**20160406\_System check\_Diple5GHzv2 SN1004**

Frequency: 5200 MHz; Duty Cycle: 1:1

**Body/5200MHz,Pin=100mW,d= 2/Z Scan (1x1x21):** Measurement grid: dx=20mm, dy=20mm, dz=5mm[Info: Interpolated medium parameters used for SAR evaluation.](#)

Maximum value of SAR (measured) = 12.9 mW/g

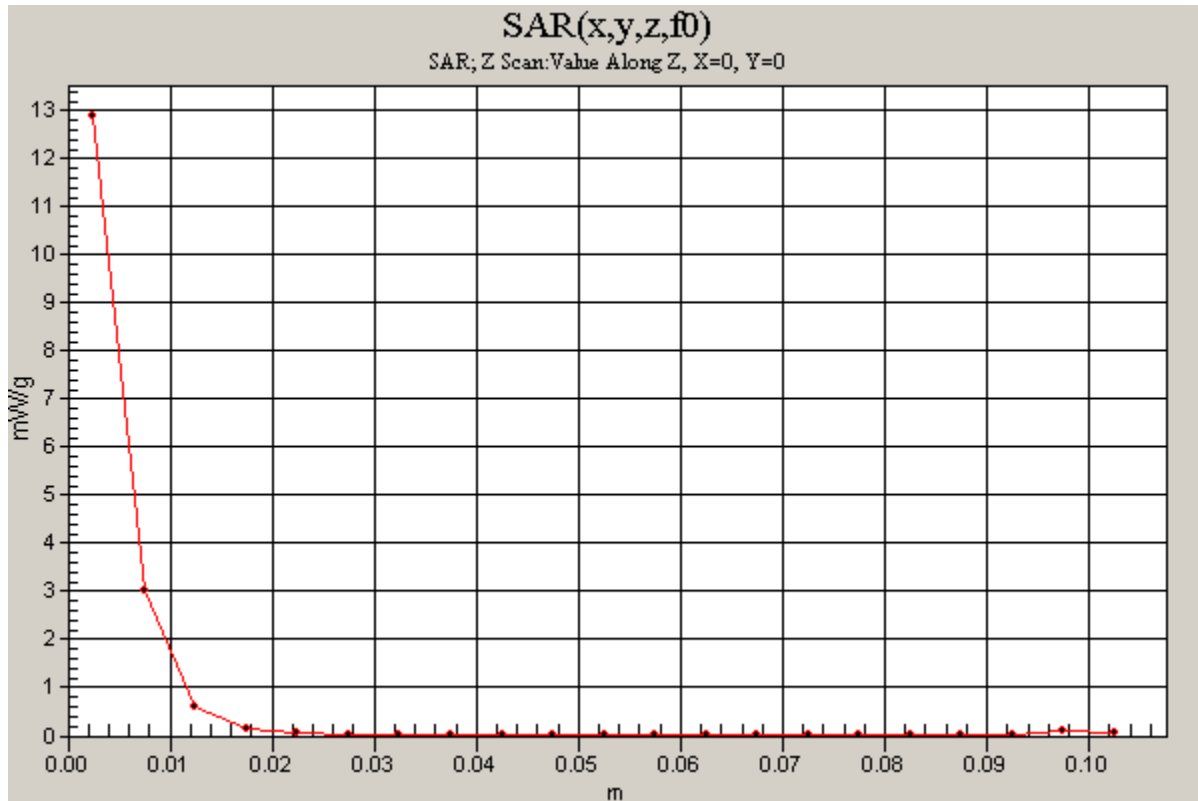

**20160406\_System check\_Diple5GHzv2 SN1004**

Frequency: 5300 MHz; Duty Cycle: 1:1; Room Ambient Temperature: 25.0°C; Liquid Temperature: 24.0°C

Medium parameters used:  $f = 5300.2$  MHz;  $\sigma = 5.55$  mho/m;  $\epsilon_r = 49.2$ ;  $\rho = 1000$  kg/m<sup>3</sup>;

DASY4 Configuration:

- Area Scan setting - Find Secondary Maximum Within: 2.0 dB and with a peak SAR value greater than 0.0012W/kg
- Electronics: DAE4 Sn558; Calibrated: 7/16/2015
- Probe: EX3DV4 - SN3554; ConvF(3.66, 3.66, 3.66); Calibrated: 10/1/2015
- Sensor-Surface: 2.5mm (Mechanical Surface Detection (Locations From Previous Scan Used))Sensor-Surface: 2.5mm (Mechanical Surface Detection)
- Phantom: Flat Phantom ELI4.0; Type: QDOVA001BA; Serial: SN: 1052

**Body/5300MHz,Pin=100mW,d= 2/Area Scan (7x7x1):** Measurement grid: dx=10mm, dy=10mm

Maximum value of SAR (measured) = 13.3 mW/g


**Body/5300MHz,Pin=100mW,d= 2/Zoom Scan (8x8x9)/Cube 0:** Measurement grid: dx=4mm, dy=4mm, dz=2.5mm

Reference Value = 52.2 V/m; Power Drift = 0.010 dB

Peak SAR (extrapolated) = 29.5 W/kg

**SAR(1 g) = 7.88 mW/g; SAR(10 g) = 2.21 mW/g**

Maximum value of SAR (measured) = 13.7 mW/g

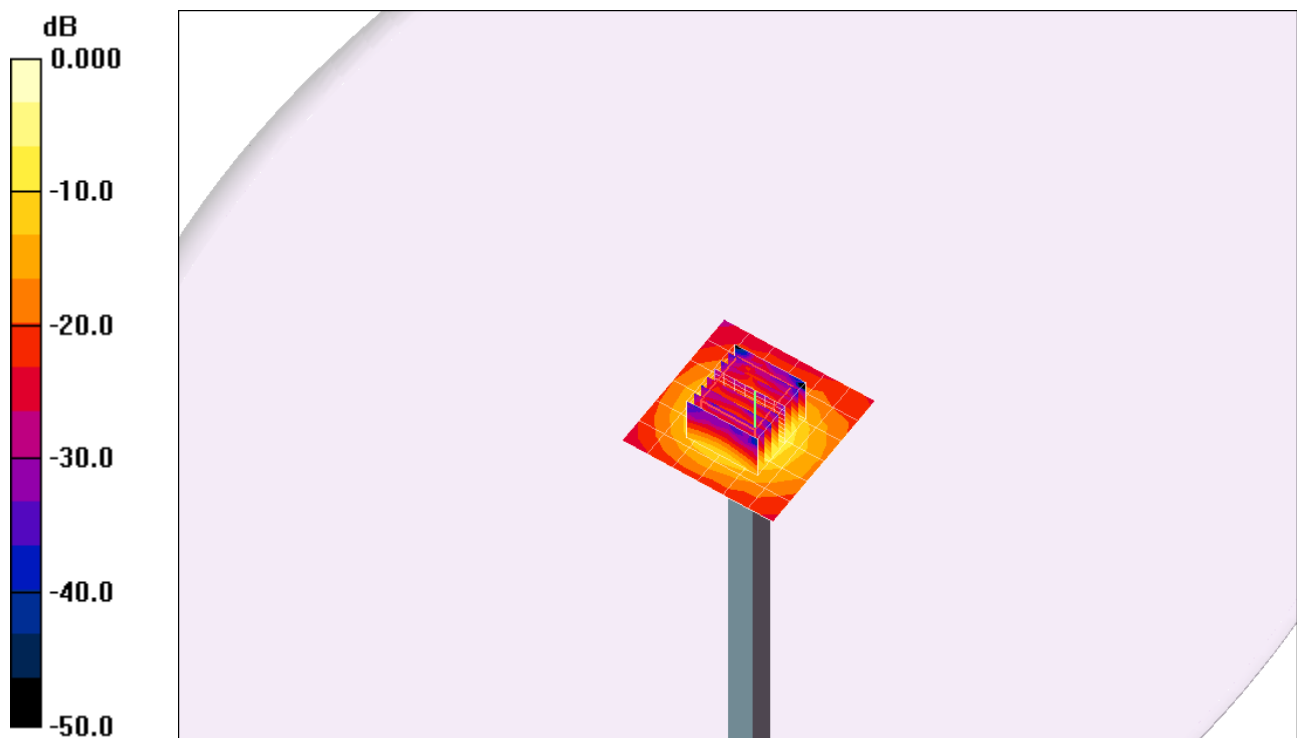


0 dB = 13.7mW/g

**20160406\_System check\_Diple5GHzv2 SN1004**

Frequency: 5300 MHz; Duty Cycle: 1:1

**Body/5300MHz,Pin=100mW,d= 2/Z Scan (1x1x21):** Measurement grid: dx=20mm, dy=20mm, dz=5mm  
Maximum value of SAR (measured) = 13.7 mW/g

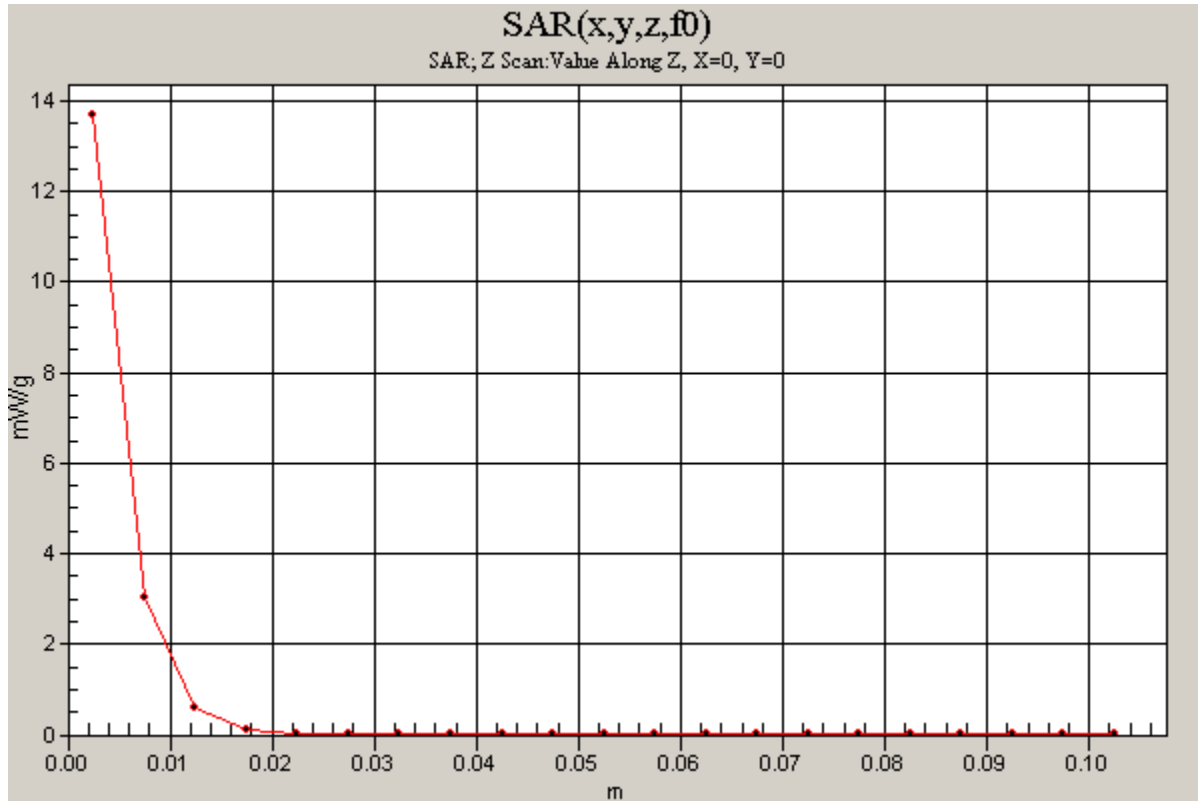

**20160406\_System check\_Diple5GHzv2 SN1004**

Frequency: 5600 MHz; Duty Cycle: 1:1; Room Ambient Temperature: 25.0°C; Liquid Temperature: 24.0°C

Medium parameters used:  $f = 5600.5$  MHz;  $\sigma = 5.97$  mho/m;  $\epsilon_r = 48.5$ ;  $\rho = 1000$  kg/m<sup>3</sup>;

DASY4 Configuration:

- Area Scan setting - Find Secondary Maximum Within: 2.0 dB and with a peak SAR value greater than 0.0012W/kg
- Electronics: DAE4 Sn558; Calibrated: 7/16/2015
- Probe: EX3DV4 - SN3554; ConvF(3.17, 3.17, 3.17); Calibrated: 10/1/2015
- Sensor-Surface: 2.5mm (Mechanical Surface Detection (Locations From Previous Scan Used))Sensor-Surface: 2.5mm (Mechanical Surface Detection)
- Phantom: Flat Phantom ELI4.0; Type: QDOVA001BA; Serial: SN: 1052

**Body/5600MHz,Pin=100mW,d= 2/Area Scan (7x7x1):** Measurement grid: dx=10mm, dy=10mm

Maximum value of SAR (measured) = 13.6 mW/g


**Body/5600MHz,Pin=100mW,d= 2/Zoom Scan (8x8x9)/Cube 0:** Measurement grid: dx=4mm, dy=4mm, dz=2.5mm

Reference Value = 51.2 V/m; Power Drift = 0.000 dB

Peak SAR (extrapolated) = 31.8 W/kg

**SAR(1 g) = 8.23 mW/g; SAR(10 g) = 2.28 mW/g**


Maximum value of SAR (measured) = 14.2 mW/g

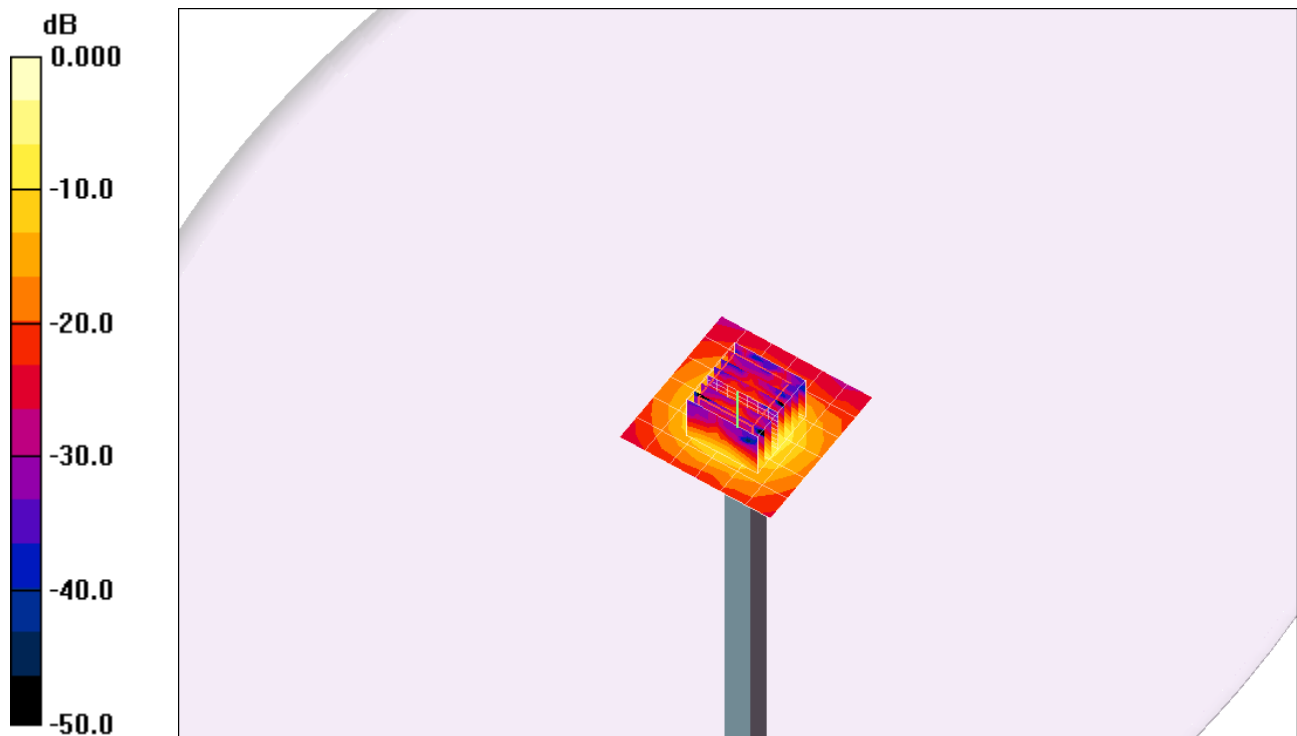

**20160406\_System check\_Diple5GHzv2 SN1004**

Frequency: 5600 MHz; Duty Cycle: 1:1

**Body/5600MHz,Pin=100mW,d= 2/Z Scan (1x1x21):** Measurement grid: dx=20mm, dy=20mm, dz=5mm  
Maximum value of SAR (measured) = 14.3 mW/g

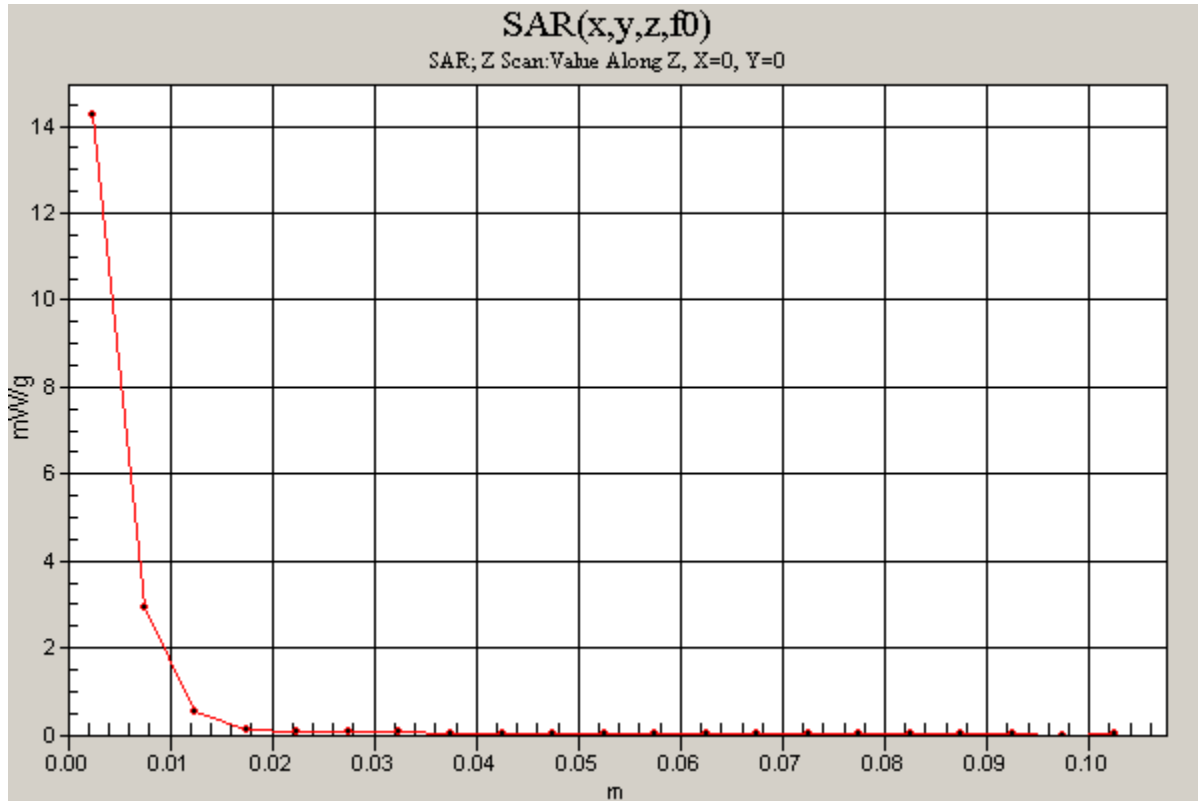

**20160406\_System check\_Diple5GHzv2 SN1004**

Frequency: 5800 MHz; Duty Cycle: 1:1; Room Ambient Temperature: 25.0°C; Liquid Temperature: 24.0°C

Medium parameters used (interpolated):  $f = 5800$  MHz;  $\sigma = 6.24$  mho/m;  $\epsilon_r = 48.2$ ;  $\rho = 1000$  kg/m<sup>3</sup>;

DASY4 Configuration:

- Area Scan setting - Find Secondary Maximum Within: 2.0 dB and with a peak SAR value greater than 0.0012W/kg
- Electronics: DAE4 Sn558; Calibrated: 7/16/2015
- Probe: EX3DV4 - SN3554; ConvF(3.37, 3.37, 3.37); Calibrated: 10/1/2015
- Sensor-Surface: 2.5mm (Mechanical Surface Detection (Locations From Previous Scan Used))Sensor-Surface: 2.5mm (Mechanical Surface Detection)
- Phantom: Flat Phantom ELI4.0; Type: QDOVA001BA; Serial: SN: 1052

**Body/5800MHz,Pin=100mW,d= 2/Area Scan (7x7x1):** Measurement grid: dx=10mm, dy=10mm

[Info: Interpolated medium parameters used for SAR evaluation.](#)

Maximum value of SAR (measured) = 13.3 mW/g

**Body/5800MHz,Pin=100mW,d= 2/Zoom Scan (8x8x9)/Cube 0:** Measurement grid: dx=4mm, dy=4mm, dz=2.5mm


Reference Value = 49.7 V/m; Power Drift = -0.008 dB

Peak SAR (extrapolated) = 31.1 W/kg

**SAR(1 g) = 7.76 mW/g; SAR(10 g) = 2.17 mW/g**

[Info: Interpolated medium parameters used for SAR evaluation.](#)

Maximum value of SAR (measured) = 13.5 mW/g

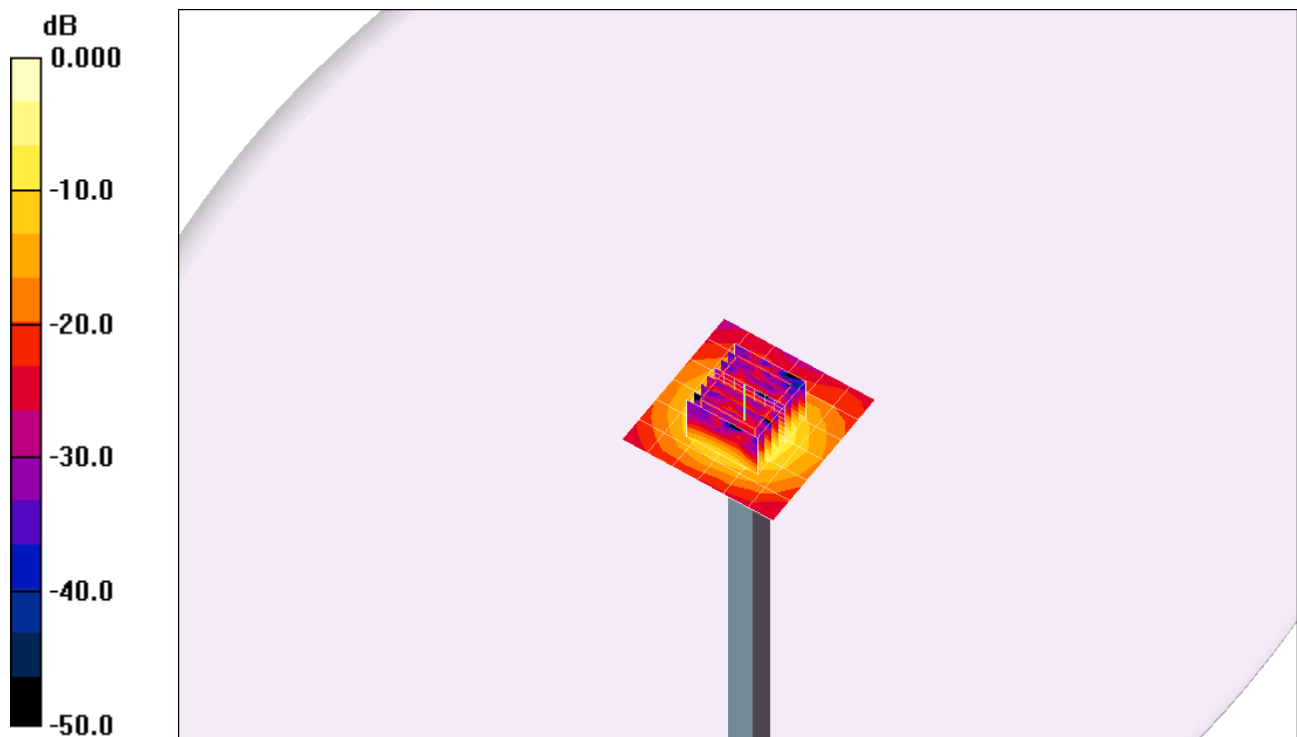


0 dB = 13.5mW/g

**20160406\_System check\_Diple5GHzv2 SN1004**

Frequency: 5800 MHz; Duty Cycle: 1:1

**Body/5800MHz,Pin=100mW,d= 2/Z Scan (1x1x21):** Measurement grid: dx=20mm, dy=20mm, dz=5mm[Info: Interpolated medium parameters used for SAR evaluation.](#)

Maximum value of SAR (measured) = 13.3 mW/g

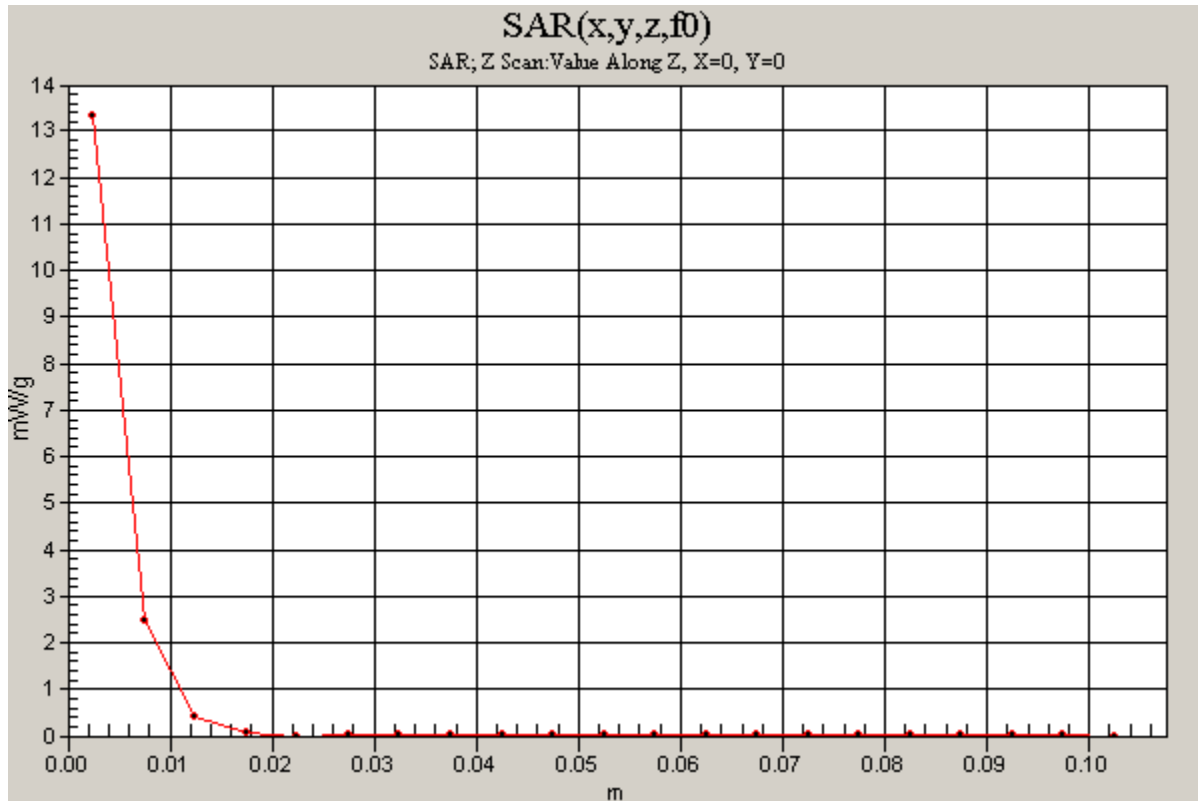

**20160407\_System Check\_Dipole2450 sn728**

Frequency: 2450 MHz; Duty Cycle: 1:1; Room Ambient Temperature: 24.0°C; Liquid Temperature: 23.0°C

Medium parameters used (interpolated):  $f = 2450$  MHz;  $\sigma = 1.92$  mho/m;  $\epsilon_r = 51.1$ ;  $\rho = 1000$  kg/m<sup>3</sup>;

DASY4 Configuration:

- Area Scan setting - Find Secondary Maximum Within: 2.0 dB and with a peak SAR value greater than 0.0012W/kg
- Electronics: DAE4 Sn558; Calibrated: 7/16/2015
- Probe: EX3DV4 - SN3554; ConvF(6.1, 6.1, 6.1); Calibrated: 10/1/2015
- Sensor-Surface: 2mm (Mechanical Surface Detection)
- Phantom: Flat Phantom ELI4.0; Type: QDOVA001BA; Serial: SN: 1052

**Body/Pin=100mW, d=10mm/Area Scan (8x9x1):** Measurement grid: dx=15mm, dy=15mm

[Info: Interpolated medium parameters used for SAR evaluation.](#)

Maximum value of SAR (measured) = 5.11 mW/g

**Body/Pin=100mW, d=10mm/Zoom Scan (7x7x7)/Cube 0:** Measurement grid: dx=5mm, dy=5mm, dz=5mm


Reference Value = 65.9 V/m; Power Drift = -0.090 dB

Peak SAR (extrapolated) = 10.4 W/kg

**SAR(1 g) = 5.24 mW/g; SAR(10 g) = 2.48 mW/g**

[Info: Interpolated medium parameters used for SAR evaluation.](#)

Maximum value of SAR (measured) = 7.74 mW/g

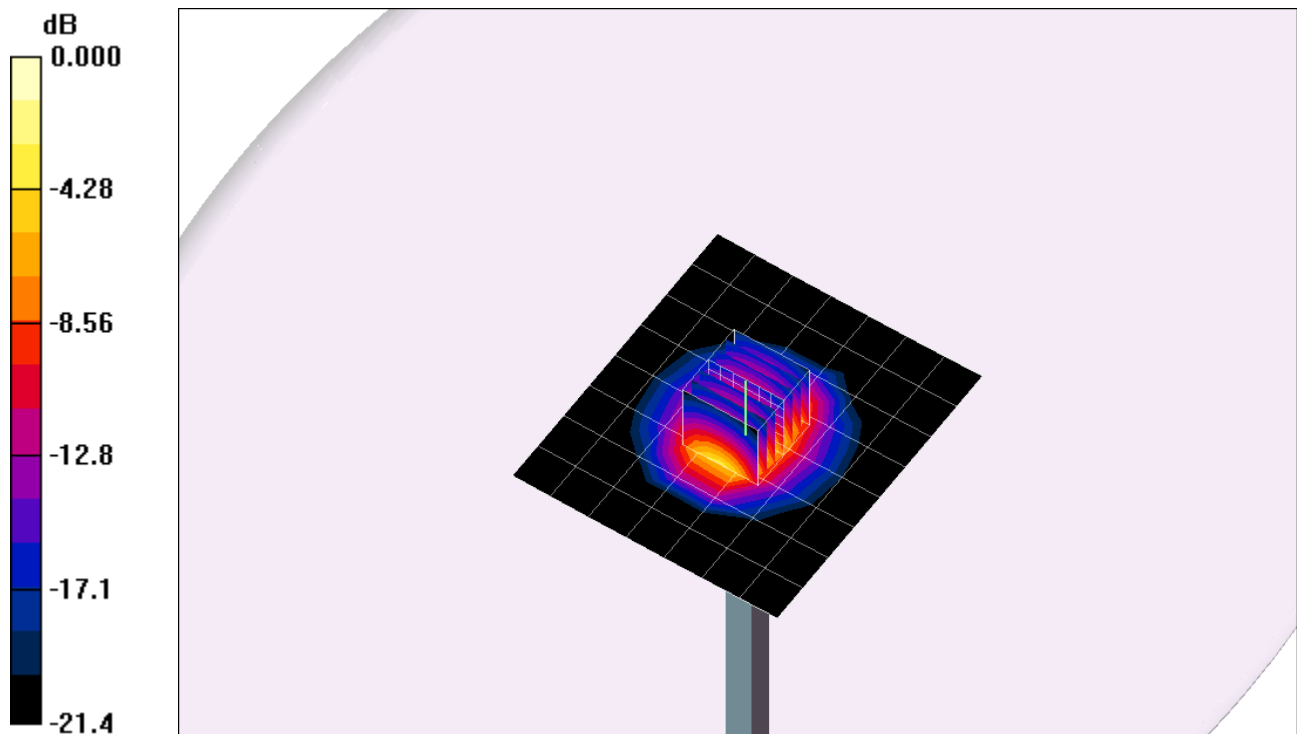

0 dB = 7.74mW/g

**20160407\_System Check\_Dipole2450 sn728**

Frequency: 2450 MHz; Duty Cycle: 1:1

**Body/Pin=100mW, d=10mm/Z Scan (1x1x21):** Measurement grid: dx=20mm, dy=20mm, dz=5mm[Info: Interpolated medium parameters used for SAR evaluation.](#)

Maximum value of SAR (measured) = 7.79 mW/g

