



Canada

EMC & RF Test Report

As per

RSS-247 Issue 2:2017 & FCC Part 15 Subpart 15.247:2015

Unlicensed Intentional Radiators

on the

StimRay
Model: CSST1

Issued by:

TÜV SÜD Canada Inc.
11 Gordon Collins Dr,
Gormley, ON, L0H 1G0
Canada
Ph: (905) 883-7255

Sanjiv Vyas,
Project Engineer

Testing produced for

 **Rehabtronics**
technology for recovery
See Appendix A for full client & EUT details.

 **Industry**
Canada
Registration #
6844A-3




Testing Laboratory
Certificate #2955.02


R-4023, G-506
C-4498, T-1246


FEDERAL COMMUNICATIONS
COMMISSION
USA
Registration #
CA6844

Client	Rehabtronics Inc.	 Canada
Product	StimRay	
Standard(s)	RSS-247 Issue 2:2017 FCC Part 15 Subpart 15.247:2015	

Table of Contents

Table of Contents	2
Report Scope	3
Summary	4
Test Results Summary	5
Notes, Justifications, or Deviations	6
Sample Calculation(s)	7
Applicable Standards, Specifications and Methods	8
Document Revision Status	9
Definitions and Acronyms	10
Testing Facility	11
Calibrations and Accreditations	11
Testing Environmental Conditions and Dates	12
Detailed Test Results Section	13
6dB Bandwidth of Digitally Modulated Systems	14
Maximum Peak Envelope Conducted Power	22
Antenna Spurious Conducted Emissions (-20 dBc Requirement)	27
Transmitter Spurious Radiated Emissions	31
Power Spectral Density	58
Power Line Conducted Emissions	63
Appendix A – EUT Summary	70
Appendix B – EUT and Test Setup Photos	72

Client	Rehabtronics Inc.	 Canada
Product	StimRay	
Standard(s)	RSS-247 Issue 2:2017 FCC Part 15 Subpart 15.247:2015	

Report Scope

This report addresses the EMC verification testing and test results of the **StimRay**, Model: **CSST1**, and is herein referred to as EUT (Equipment Under Test). The EUT was tested for compliance against the following standards:

RSS-247 Issue 2:2017

FCC Part 15 Subpart C 15.247:2015

Test procedures, results, justifications, and engineering considerations, if any, follow later in this report.

This report does not imply product endorsement by any government, accreditation agency, or TÜV SÜD Canada Inc.

Opinions or interpretations expressed in this report, if any, are outside the scope of TÜV SÜD Canada Inc accreditations. Any opinions expressed do not necessarily reflect the opinions of TÜV SÜD Canada Inc, unless otherwise stated.

Client	Rehabtronics Inc.	 Canada
Product	StimRay	
Standard(s)	RSS-247 Issue 2:2017 FCC Part 15 Subpart 15.247:2015	

Summary

The results contained in this report relate only to the item(s) tested.

EUT:	StimRay
FCC Certification #, FCC ID:	QIQCST1
Industry Canada Certification #, IC:	10685A-CSST1
EUT passed all tests performed	Yes
Tests conducted by	Sanjiv Vyas

For testing dates, see "Testing Environmental Conditions and Dates".

Client	Rehabtronics Inc.	 Canada
Product	StimRay	
Standard(s)	RSS-247 Issue 2:2017 FCC Part 15 Subpart 15.247:2015	

Test Results Summary

Standard/Method	Description	Class/Limit	Result
FCC 15.203	Antenna Requirement	Unique	Pass See Justification
FCC 15.205 RSS-GEN (Table 6)	Restricted Bands for Intentional Operation	QuasiPeak Average	Pass
FCC 15.207 RSS-GEN (Table 3)	Power Line Conducted Emissions	QuasiPeak Average	Pass
FCC 15.209 RSS-GEN (Table 4)	Spurious Radiated Emissions	QuasiPeak Average	Pass
FCC 15.247(a)2 RSS-247 5.2(a)	6 dB Bandwidth	> 500 kHz	Pass
FCC 15.247(b)2 RSS-247 5.4(d)	Max Output Power	< 1 Watt	Pass
FCC 15.247(b)4 RSS-247 5.4(d)	Antenna Gain	< 6 dBi	Pass See Justifications
FCC 15.247(d) RSS-247 5.5	Antenna Conducted Spurious	< 20 dBc	Pass
FCC 15.247(e) RSS-247 5.2(b)	Spectral Density	< 8 dBm (3 kHz BW)	Pass
Overall Result			Pass

If the product as tested or otherwise complies with the specification, the EUT is deemed to comply with the requirement and is deemed a 'PASS' grade. If not 'FAIL' grade will be issued. Note that 'PASS' / 'FAIL' grade is independent of any measurement uncertainties. A 'PASS' / 'FAIL' grade within measurement uncertainty is marked with a '*'.

Client	Rehabtronics Inc.	 Canada
Product	StimRay	
Standard(s)	RSS-247 Issue 2:2017 FCC Part 15 Subpart 15.247:2015	

Notes, Justifications, or Deviations

The following notes, justifications for tests not performed or deviations from the above listed specifications apply:

For the antenna requirement specified in FCC 15.203 (RSS-247 section 5.4(d)), the antenna has a peak gain of 5.3dBi as specified by the manufacturer, which is less than the 6 dBi gain limit and EUT uses Inverted-F (as PCB trace) antenna inside the enclosure, and has no provision for end-user replacement.

For the Restricted Bands of operation requirement specified in FCC15.205, the EUT is designed to only operate between 2.4 to 2.4835 GHz band and does not intentionally transmit in any of the restricted bands.

The EUT is not a hybrid system and FCC 15.247 (f) does not apply to it. However the 15.247 (d) requirement of power density were met and are detailed later in this test report.

For FCC 15.207 requirements, when connected to the AC/DC power supply adaptor (Model: EP-TA10JWE, Make: SAMSUNG), this product charges and does not transmit therefore conducted emission test was performed in this mode of operation.

The EUT was mounted in three orthogonal axis. Worst case results were obtained with the EUT in the X-axis. Worst case results are presented. See Appendix B for axis details.

Client	Rehabtronics Inc.	 Canada
Product	StimRay	
Standard(s)	RSS-247 Issue 2:2017 FCC Part 15 Subpart 15.247:2015	

Sample Calculation(s)

Radiated Emission Test

Margin = Limit – (Received Signal + Antenna Factor + Cable Loss – Pre-Amp Gain)

Margin = $50.5 \text{ dB}\mu\text{V/m} - (50 \text{ dB}\mu\text{V} + 10 \text{ dB} + 2.5 \text{ dB} - 20 \text{ dB})$

Margin = 8.0 dB (pass)

Power Line Conducted Emission Test

Margin = Limit – (Received Signal + Attenuation Factor + Cable Loss + LISN Factor)

Margin = $73.0 \text{ dB}\mu\text{V} - (50 \text{ dB}\mu\text{V} + 10 \text{ dB} + 2.5 \text{ dB} + 0.5 \text{ dB})$

Margin = 10.0 dB (pass)

Client	Rehabtronics Inc.	 Canada
Product	StimRay	
Standard(s)	RSS-247 Issue 2:2017 FCC Part 15 Subpart 15.247:2015	

Applicable Standards, Specifications and Methods

ANSI C63.4:2014 Methods of Measurement of Radio-Noise Emissions from Low-Voltage Electrical and Electronic Equipment in the Range of 9 kHz to 40 GHz

ANSI C63.10:2013 American National Standard For Testing Unlicensed Wireless Devices

CFR 47 FCC 15 Subpart C:2015 Code of Federal Regulations – Radio Frequency Devices, Intentional Radiators

FCC KDB 558074 v04: 2017 FCC KDB 558074 Digital Transmission Systems, measurements and procedures

ICES-003 Issue 6 2016 Digital Apparatus - Spectrum Management and Telecommunications Policy Interference-Causing Equipment Standard

RSS-GEN Issue 4 2014 General Requirements and Information for the Certification of Radio Apparatus

RSS-247 Issue 2:2017 Issue 2: Digital Transmission Systems (DTSs), Frequency Hopping Systems (FHSs) and Licence-Exempt Local Area Network (LE-LAN) Devices

ISO 17025:2005 General Requirements for the Competence of Testing and Calibration Laboratories

Client	Rehabtronics Inc.
Product	StimRay
Standard(s)	RSS-247 Issue 2:2017 FCC Part 15 Subpart 15.247:2015



Document Revision Status

Revision 1 - September 22, 2017
Initial Release

Client	Rehabtronics Inc.	 Canada
Product	StimRay	
Standard(s)	RSS-247 Issue 2:2017 FCC Part 15 Subpart 15.247:2015	

Definitions and Acronyms

The following definitions and acronyms are applicable in this report.
See also ANSI C63.14.

AE – Auxiliary Equipment. A digital accessory that feeds data into or receives data from another device (host) that in turn, controls its operation.

BW – Bandwidth. Unless otherwise stated, this is refers to the 6 dB bandwidth.

EMC – Electro-Magnetic Compatibility. The ability of an equipment or system to function satisfactorily in its electromagnetic environment without introducing intolerable electromagnetic disturbances to anything in that environment.

EMI – Electro-Magnetic Immunity. The ability to maintain a specified performance when the equipment is subjected to disturbance (unwanted) signals of specified levels.

EUT – Equipment Under Test. A device or system being evaluated for compliance that is representative of a product to be marketed.

ITE – Information Technology Equipment with a primary function(s) of entry, storage, display, retrieval, transmission, processing, switching, or control, of data.

LISN – Line Impedance Stabilization Network

NCR – No Calibration Required

RF – Radio Frequency

Client	Rehabtronics Inc.	 Canada
Product	StimRay	
Standard(s)	RSS-247 Issue 2:2017 FCC Part 15 Subpart 15.247:2015	

Testing Facility

Testing for EMC on the EUT was carried out at TÜV SÜD Canada labs near Toronto, Ontario. The testing lab consists of a 3m semi-anechoic chamber calibrated to be able to allow measurements on a EUT that has a maximum width or length of up to 2m and a height of up to 3m. The chamber is equipped with a turntable that is capable of testing devices up to 3300lb in weight. This facility is capable of testing products that are rated for 120Vac and 240Vac single phase, or devices that are rated for a 208Vac 3 phase input. DC capability is also available for testing. The chamber is equipped with a mast that controls the polarization and height of the antenna. Control of the mast occurs in the control room adjoining the shielded chamber. Radiated emission measurements are performed using a BiLog antenna and a Horn antenna where applicable. Conducted emissions, unless otherwise stated, are performed using a LISN and using the Vertical Ground plane if applicable.

Calibrations and Accreditations

The 3m semi-anechoic chamber is registered with Federal Communications Commission (FCC, CA6844), Industry Canada (IC, 6844A-3) and Voluntary Control Council for Interference (VCCI, R-4023, G-506, C-4498, and T-1246). This chamber was calibrated for Normalized Site Attenuation (NSA) using test procedures outlined in ANSI C63.4 "Methods of Measurement of Radio-Noise Emissions from Low-Voltage Electrical and Electronic Equipment in the Range of 9 kHz to 40 GHz". The chamber is lined with ferrite tiles and absorption cones to minimize any undesired reflections. The NSA data is kept on file at TÜV SÜD Canada. For radiated susceptibility testing, a 16 point field calibration has been performed on the chamber. The field uniformity data is kept on file at TÜV SÜD Canada. TÜV SÜD Canada Inc. is accredited to ISO 17025 by A2LA with Testing Certificate #2555.01. The laboratory's current scope of accreditation listing can be found as listed on the A2LA website. All measuring equipment is calibrated on an annual or bi-annual basis as listed for each respective test.

Client	Rehabtronics Inc.	 Canada
Product	StimRay	
Standard(s)	RSS-247 Issue 2:2017 FCC Part 15 Subpart 15.247:2015	

Testing Environmental Conditions and Dates

Following environmental conditions were recorded in the facility during time of testing

Date	Test	Initials	Temperature (°C)	Humidity (%)	Pressure (kPa)
September 13 & 18, 2017	Antenna Conducted Emissions	SV	24.2	50.7	100.8
September 18, 2017	Radiated Emissions	SV	25.4	56.9	101.1
September 7 & 8, 2017	Power Line Conducted Emissions	SV	22.4	48.0	100.7

Client	Rehabtronics Inc.
Product	StimRay
Standard(s)	RSS-247 Issue 2:2017 FCC Part 15 Subpart 15.247:2015


Canada

Detailed Test Results Section

Client	Rehabtronics Inc.	 Canada
Product	StimRay	
Standard(s)	RSS-247 Issue 2:2017 FCC Part 15 Subpart 15.247:2015	

6dB Bandwidth of Digitally Modulated Systems

Purpose

The purpose of this test is to ensure that the bandwidth occupied exceeds a stated minimum. This helps ensure the utilization of the frequency allocation is sufficiently wide. This also helps prevent corruption of data by ensuring adequate data separation to distinguish the reception of the intended information.

Limits and Method

The limit is as specified in FCC Part 15.247(a)2 and RSS-247.

Systems using digital modulation techniques may operate in the 902 - 928 MHz, 2400 - 2483.5 MHz, and 5725 - 5850 MHz bands. The minimum 6 dB bandwidth shall be at least 500 kHz. This should be measured with a 100 kHz RBW and a 300 kHz VBW.

The method is given in Section 8.1 of FCC KDB 558074 and ANSI C63.10.

Results


The EUT passed. The minimum 6 dB BW measured was 0.8093 MHz and the maximum 99% BW at full power setting was 1.8269 MHz.

Channel	Frequency (MHz)	6dB Bandwidth (MHz)	99% Bandwidth (MHz)
Low	2402	0.8415	1.7900
Mid	2440	0.8814	1.8070
High	2480	0.8093	1.8269

Client	Rehabtronics Inc.	 Canada
Product	StimRay	
Standard(s)	RSS-247 Issue 2:2017 FCC Part 15 Subpart 15.247:2015	

Graphs


The graphs showed below show the OBW during the operation of the device. This is measured by a max hold on the spectrum analyzer and the highest resolution bandwidth that is sufficiently low to exhibit the 6 dB bandwidth of a channel during operation of the EUT. Max hold is performed for a duration of not less than 1 minute.

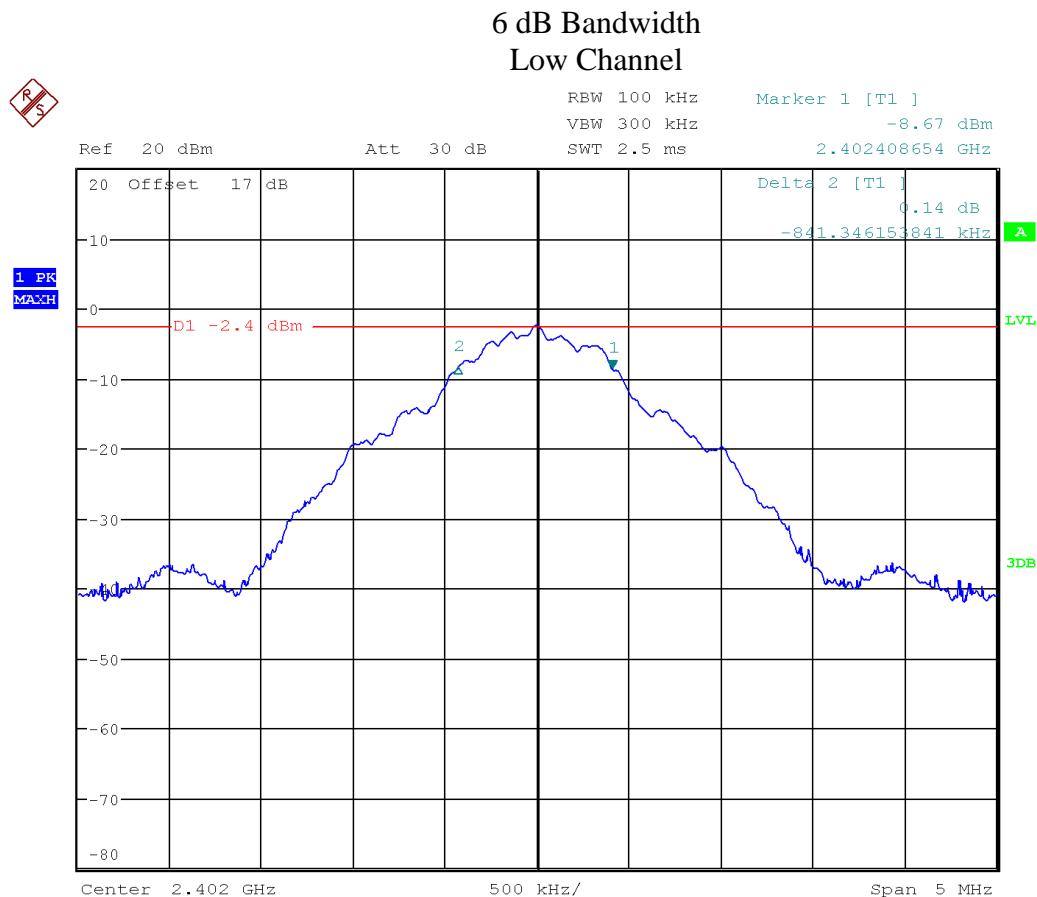

Date: 13.SEP.2017 16:24:25

Client	Rehabtronics Inc.	 Canada
Product	StimRay	
Standard(s)	RSS-247 Issue 2:2017 FCC Part 15 Subpart 15.247:2015	


6 dB Bandwidth Mid Channel

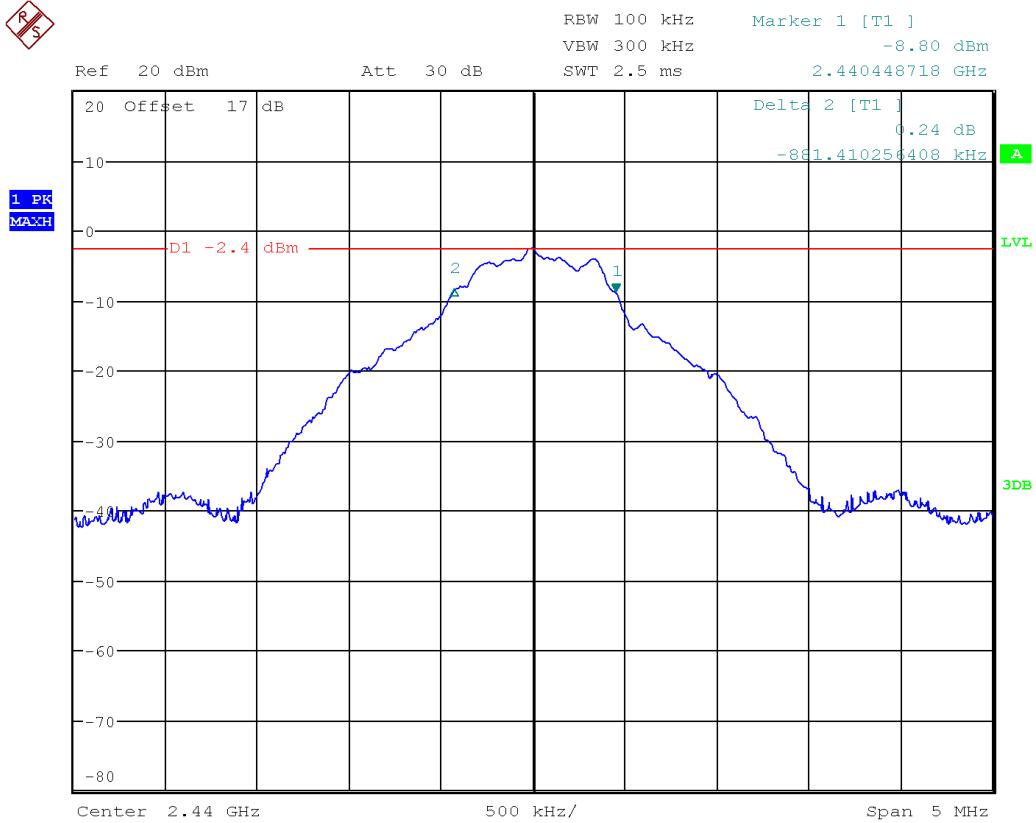

Date: 13.SEP.2017 16:32:07

Client	Rehabtronics Inc.	 Canada
Product	StimRay	
Standard(s)	RSS-247 Issue 2:2017 FCC Part 15 Subpart 15.247:2015	


6 dB Bandwidth Hi Channel

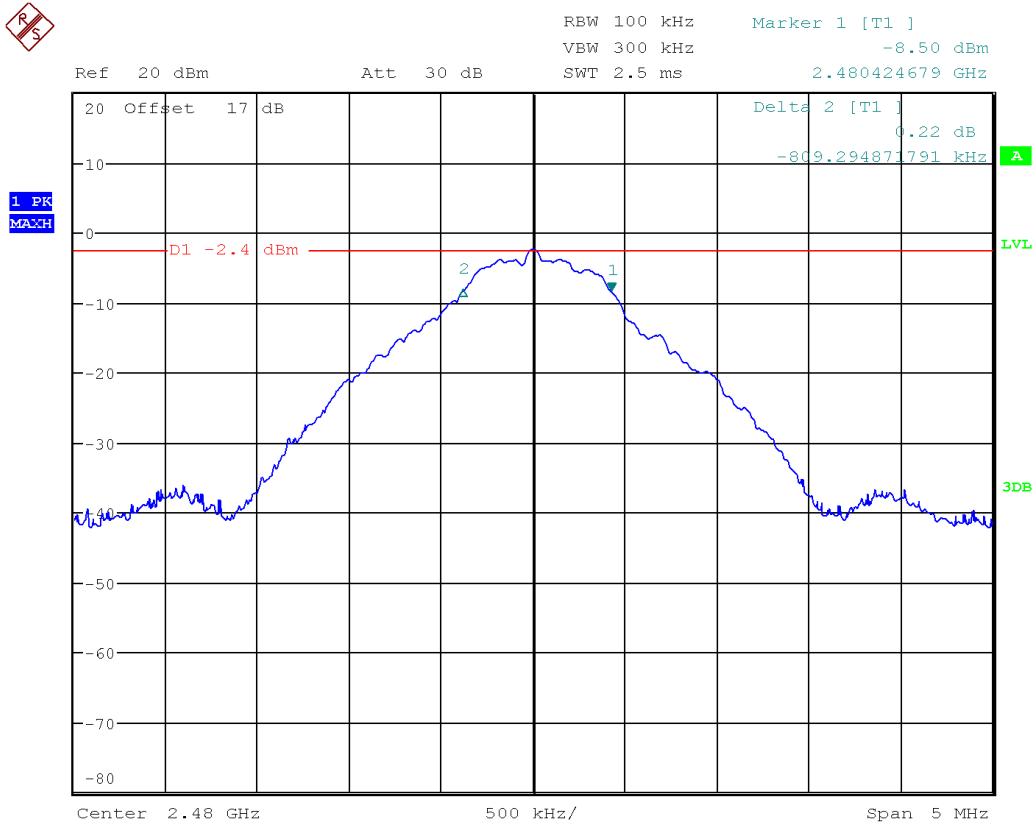

Date: 13.SEP.2017 16:35:09

Client	Rehabtronics Inc.	 Canada
Product	StimRay	
Standard(s)	RSS-247 Issue 2:2017 FCC Part 15 Subpart 15.247:2015	


99% Bandwidth Low Channel

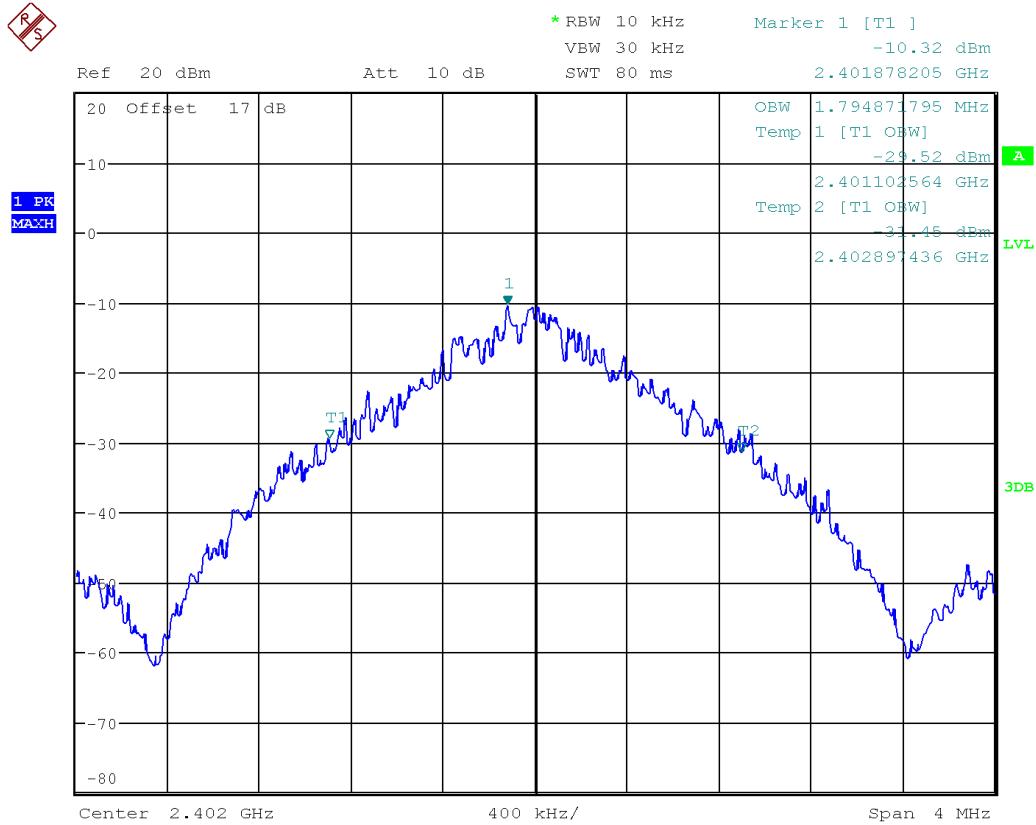

Date: 18.SEP.2017 13:35:04

Client	Rehabtronics Inc.	 Canada
Product	StimRay	
Standard(s)	RSS-247 Issue 2:2017 FCC Part 15 Subpart 15.247:2015	


99% Bandwidth
Mid Channel

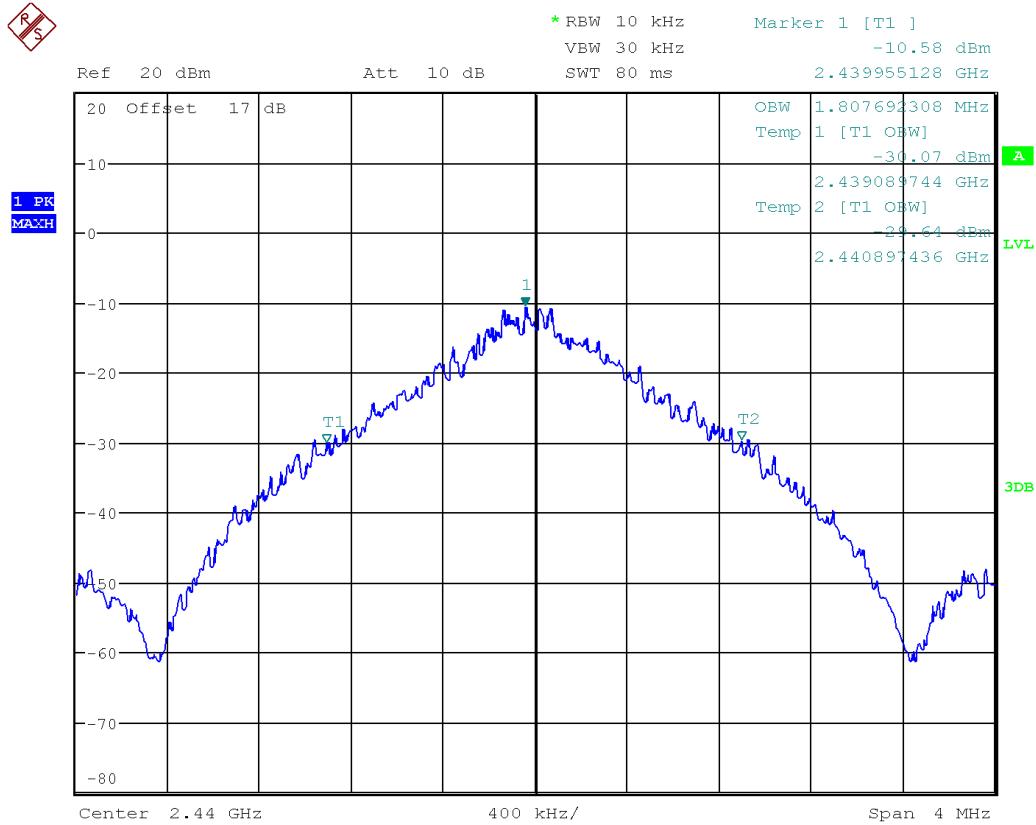

Date: 18.SEP.2017 13:45:40

Client	Rehabtronics Inc.	 Canada
Product	StimRay	
Standard(s)	RSS-247 Issue 2:2017 FCC Part 15 Subpart 15.247:2015	

99% Bandwidth
High Channel

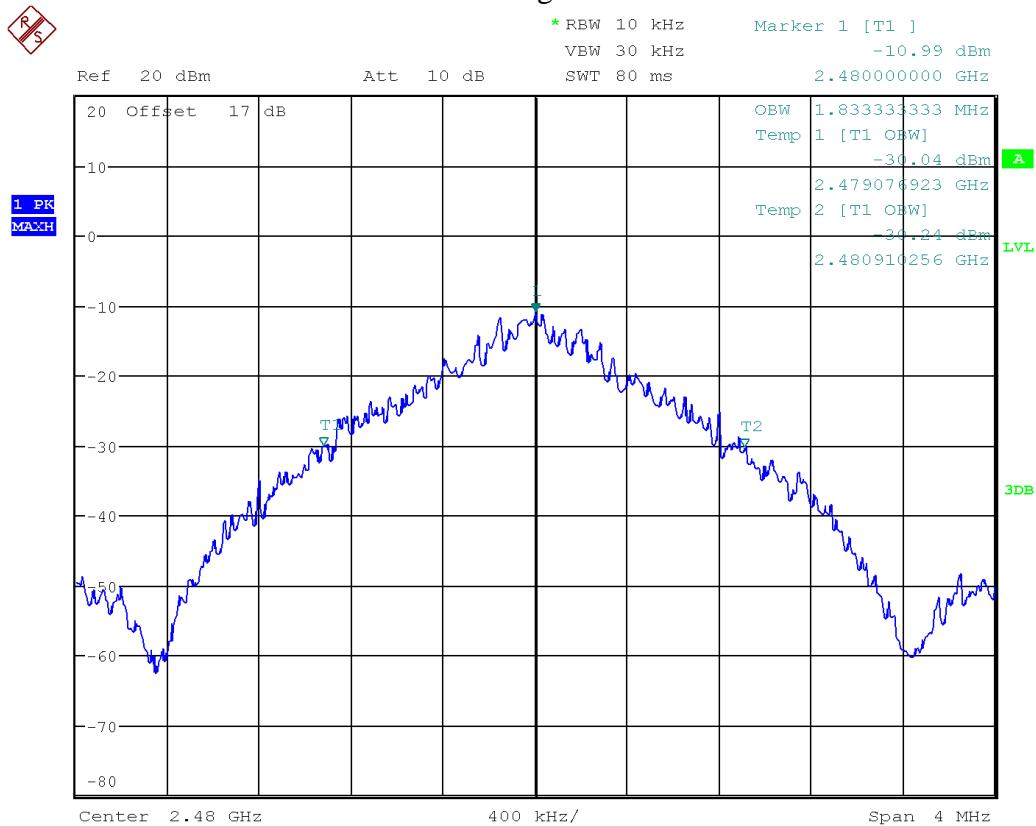

Date: 18.SEP.2017 13:54:33

Note: See 'Appendix B – EUT & Test Setup Photos' for photos showing the test set-up.

Client	Rehabtronics Inc.	 Canada
Product	StimRay	
Standard(s)	RSS-247 Issue 2:2017 FCC Part 15 Subpart 15.247:2015	

Test Equipment List

Equipment	Model No.	Manufacturer	Last Calibration / Verification Date	Next Calibration / Verification Date	Asset #
Spectrum Analyzer	FSU 26	Rohde & Schwarz	Feb. 15, 2017	Feb. 15, 2019	GEMC 232
Attenuator 10 dB	8493B	Agilent	Feb. 20, 2017	Feb. 20, 2018	GEMC 133
Attenuator 6 dB	3M-6	Weinschel	Feb. 20, 2017	Feb. 20, 2018	GEMC 278

Client	Rehabtronics Inc.	 Canada
Product	StimRay	
Standard(s)	RSS-247 Issue 2:2017 FCC Part 15 Subpart 15.247:2015	

Maximum Peak Envelope Conducted Power

Purpose

The purpose of this test is to ensure that the maximum power conducted to the radiating element does not exceed the limits specified. This ensures that if the end-user replaces the antenna, the maximum power does not exceed an amount which may create an excessive power level.

Limits and Method

The limits are defined in FCC Part 15.247(b) and RSS-247.

For systems using digital modulation in the 902-928 MHz, 2400-2483.5 MHz, and 5725-5850 MHz bands, the peak limit is 1 watt (30 dBm).

The method is given in Section 9.1 of FCC KDB 558074 and ANSI C63.10.

Results

The EUT passed. The EUT was set to transmit at maximum power (100%). Three channels were measured. The following table show the peak power:

Channel	Frequency (MHz)	Peak Power (dBm)	Peak Power (mW)
Low	2402	-1.99	0.63
Mid	2440	-2.02	0.63
High	2480	-2.05	0.62


Note: The external attenuator and cable loss are accounted for as reference offset in the spectrum analyzer

Graphs

The plots shown below show the peak power output of the device. This is measured by a max hold on the spectrum analyzer using a RBW of 1MHz. This measurement is a peak measurement. Max hold is performed for a duration of not less than 1 minute.

Client	Rehabtronics Inc.	 Canada
Product	StimRay	
Standard(s)	RSS-247 Issue 2:2017 FCC Part 15 Subpart 15.247:2015	


Peak Power, Low Channel

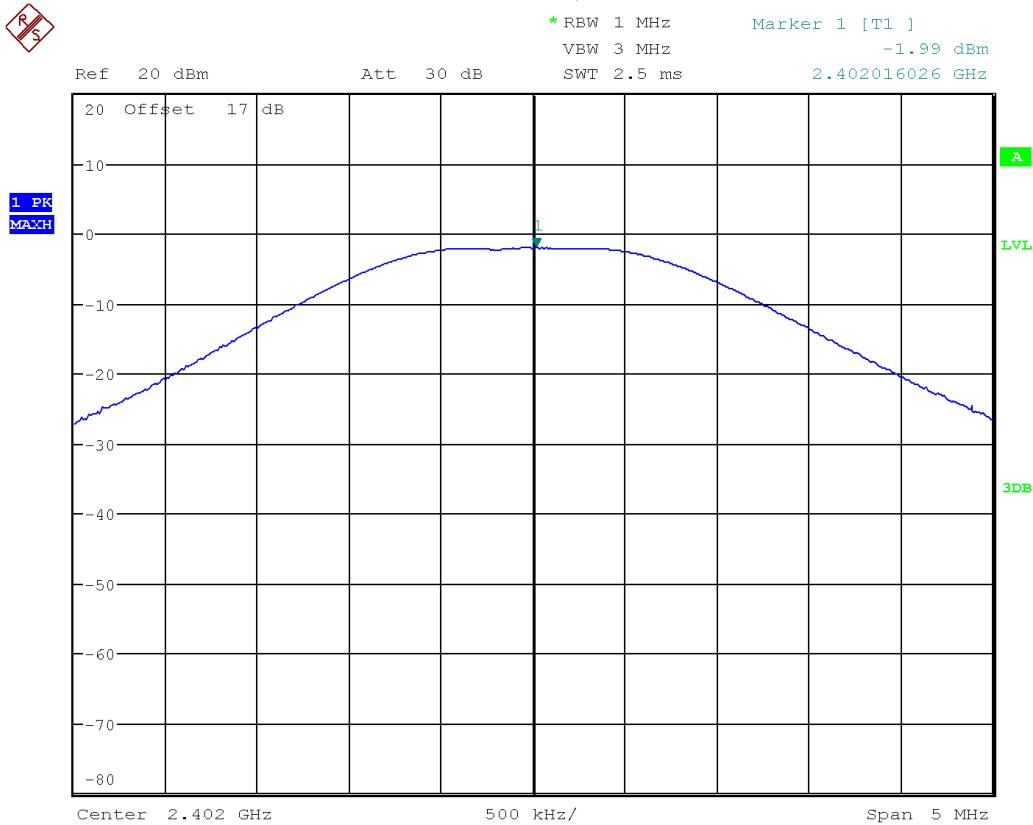

Date: 18.SEP.2017 11:15:24

Client	Rehabtronics Inc.	 Canada
Product	StimRay	
Standard(s)	RSS-247 Issue 2:2017 FCC Part 15 Subpart 15.247:2015	


Peak Power, Mid Channel

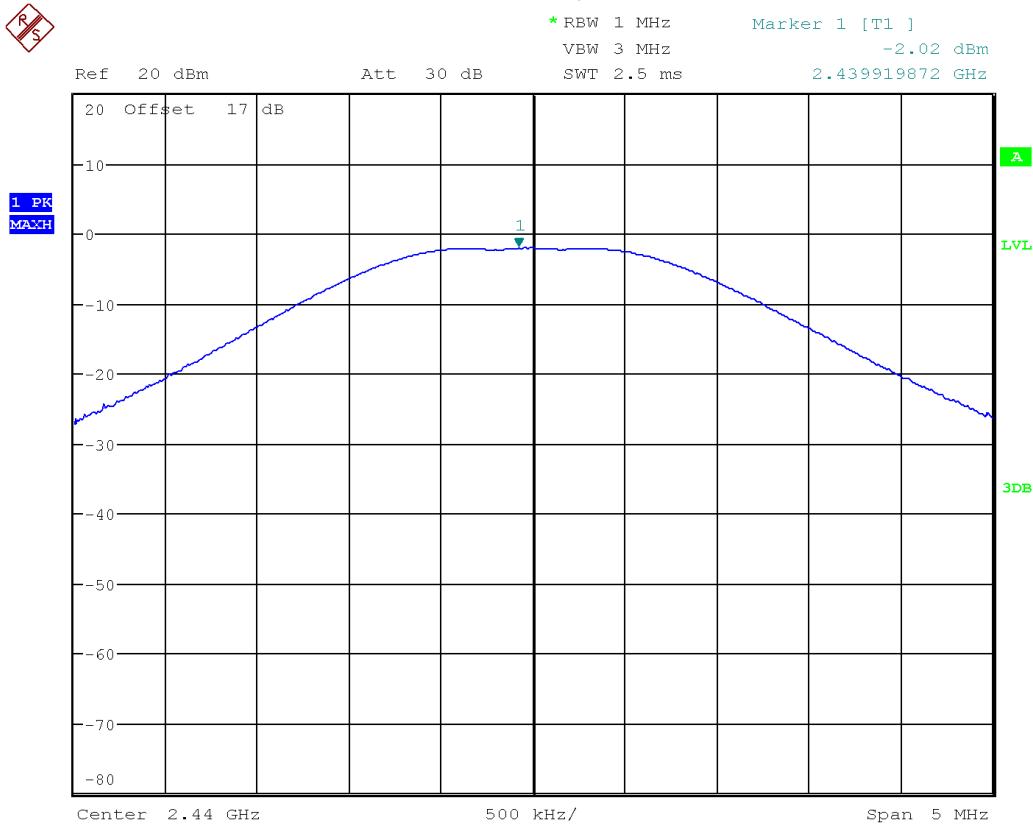

Date: 18.SEP.2017 11:17:28

Client	Rehabtronics Inc.	 Canada
Product	StimRay	
Standard(s)	RSS-247 Issue 2:2017 FCC Part 15 Subpart 15.247:2015	

Peak Power, Hi Channel

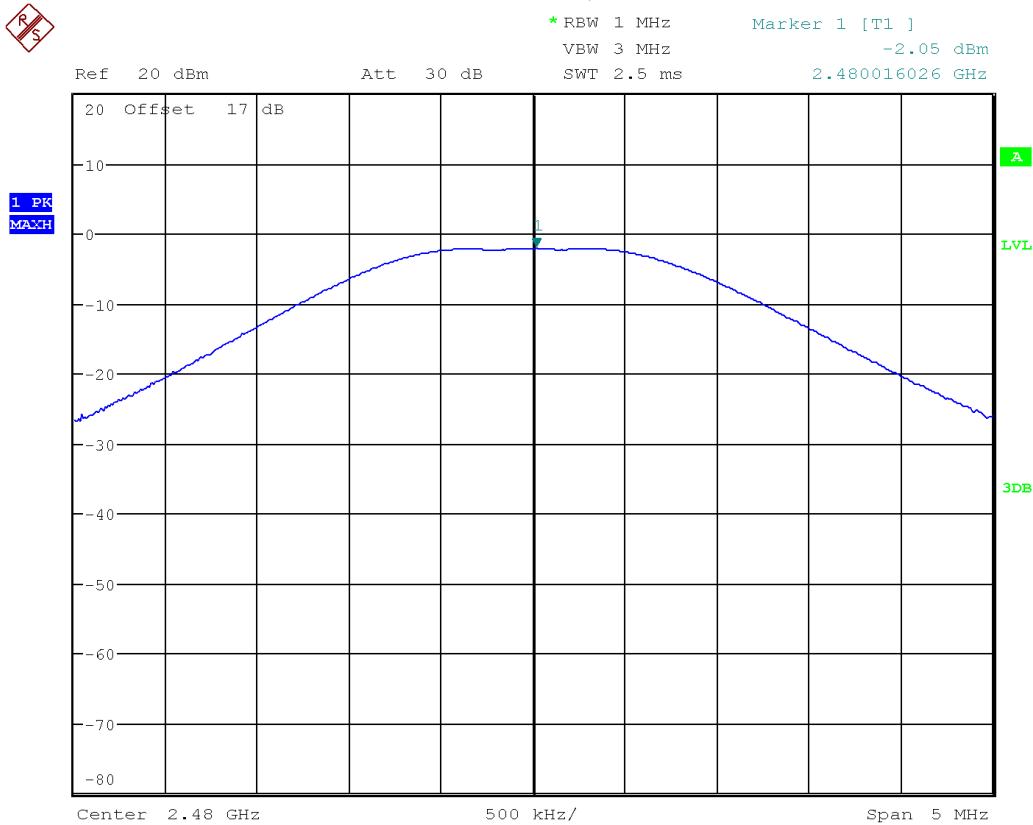

Date: 18.SEP.2017 11:18:59

See 'Appendix B – EUT and Test Setup Photos' for photos showing the test set-up.

Client	Rehabtronics Inc.	 Canada
Product	StimRay	
Standard(s)	RSS-247 Issue 2:2017 FCC Part 15 Subpart 15.247:2015	

Test Equipment List

Equipment	Model No.	Manufacturer	Last Calibration / Verification Date	Next Calibration / Verification Date	Asset #
Spectrum Analyzer	FSU 26	Rohde & Schwarz	Feb. 15, 2017	Feb. 15, 2019	GEMC 232
Attenuator 10 dB	8493B	Agilent	Feb. 20, 2017	Feb. 20, 2018	GEMC 133
Attenuator 6 dB	3M-6	Weinschel	Feb. 20, 2017	Feb. 20, 2018	GEMC 278

Client	Rehabtronics Inc.	 Canada
Product	StimRay	
Standard(s)	RSS-247 Issue 2:2017 FCC Part 15 Subpart 15.247:2015	

Antenna Spurious Conducted Emissions (-20 dBc Requirement)

Purpose

The purpose of this test is to ensure that the maximum power conducted to the radiating element at frequencies outside of the authorized spectrum does not exceed the limits specified. This ensures that the only the intended signal is delivered to the radiating element.

Limits and Method

The limits are defined in 15.247(d). In any 100 kHz band, the peak spurious harmonics emissions must be at least 20 dB below the fundamental. Spurious Conducted emissions are to be evaluated up to the 10th harmonic. This -20 dBc requirement also applies at the 'band edge' or 2.4 GHz and 2.4835 GHz.

The method is given in Section 11 of FCC KDB 558074 and ANSI C63.10


Results

The EUT passed. Low, middle and high bands were measured. The worst case is presented as a graph for the spectrum. The -20 dBc requirement is shown for the lower band edge at 2.4 GHz in the low band and also for the higher band edge at 2.4835 GHz in the high band.


Client	Rehabtronics Inc.	 Canada
Product	StimRay	
Standard(s)	RSS-247 Issue 2:2017 FCC Part 15 Subpart 15.247:2015	

Graphs

The graphs shown below show the peak power output of the device during the antenna conducted measurement during transmit operation of the EUT.

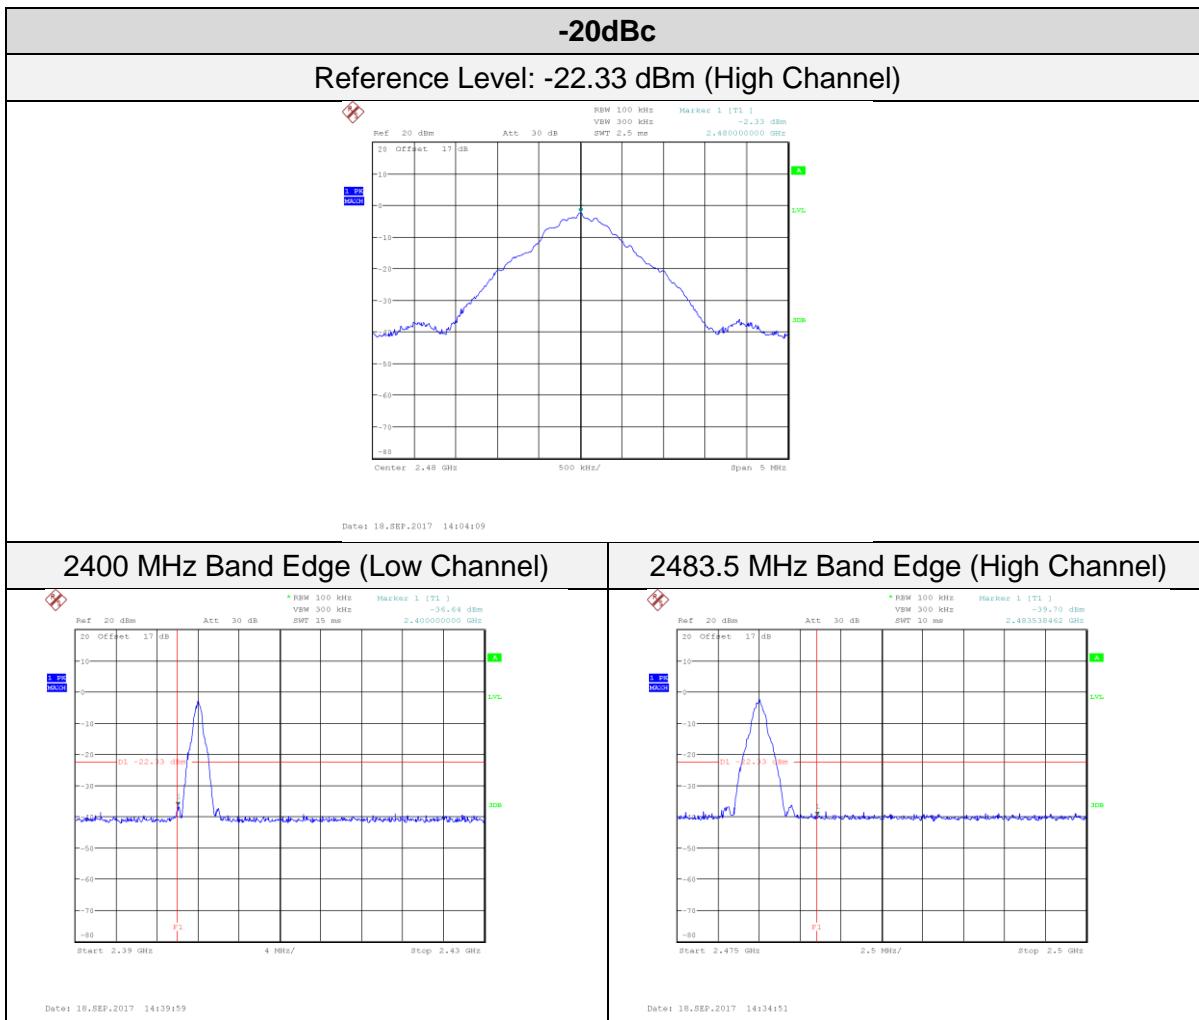

Client	Rehabtronics Inc.	 Canada
Product	StimRay	
Standard(s)	RSS-247 Issue 2:2017 FCC Part 15 Subpart 15.247:2015	

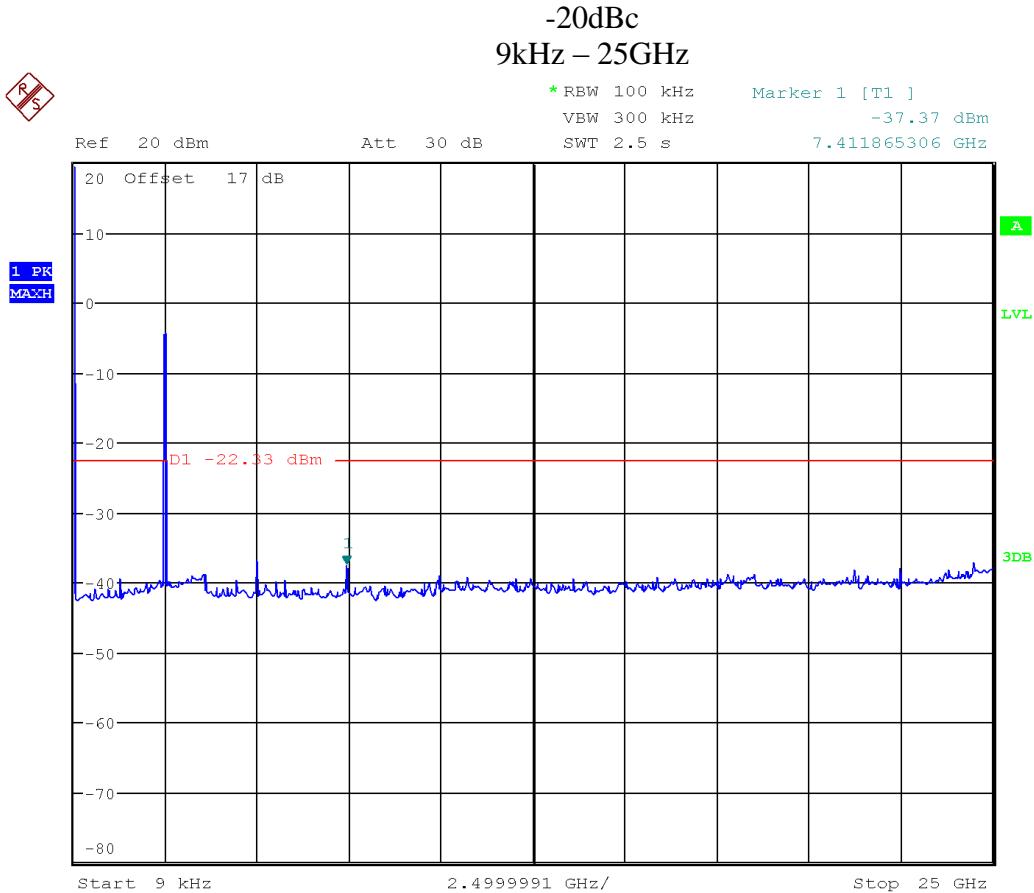

Date: 18.SEP.2017 14:22:37

See 'Appendix B – EUT and Test Setup Photos' for photos showing the test set-up.

Client	Rehabtronics Inc.	 Canada
Product	StimRay	
Standard(s)	RSS-247 Issue 2:2017 FCC Part 15 Subpart 15.247:2015	

Test Equipment List

Equipment	Model No.	Manufacturer	Last Calibration / Verification Date	Next Calibration / Verification Date	Asset #
Spectrum Analyzer	FSU 26	Rohde & Schwarz	Feb. 15, 2017	Feb. 15, 2019	GEMC 232
Attenuator 10 dB	8493B	Agilent	Feb. 20, 2017	Feb. 20, 2018	GEMC 133
Attenuator 6 dB	3M-6	Weinschel	Feb. 20, 2017	Feb. 20, 2018	GEMC 278

Client	Rehabtronics Inc.	 Canada
Product	StimRay	
Standard(s)	RSS-247 Issue 2:2017 FCC Part 15 Subpart 15.247:2015	

Transmitter Spurious Radiated Emissions

Purpose

The purpose of this test is to ensure that the RF energy unintentionally emitted from the EUT does not exceed the limits listed below as defined in the applicable test standard, as measured from a receiving antenna. This helps protect broadcast radio services such as television, FM radio, pagers, cellular telephones, emergency services, and so on, from unwanted interference.

Limits and Method

The method is as defined in Section 12.2.7 of FCC KDB 558074 and ANSI C63.10.

The limits, as defined in 15.247(d) for unintentional radiated emissions, apply for those emissions that fall in the restricted bands, as defined in Section 15.205(a). These emissions must comply with the radiated emission limits specified in Section 15.209(a).

All unintentional emissions must also meet the ‘Spurious Conducted Emissions’ requirements of -20 dBc or greater. See also ‘Antenna Spurious Conducted Emissions (-20dBc)’ for further details.

Frequency	Limit
0.009 MHz – 0.490 MHz	2400/F(kHz) uV/m at 300m ¹
0.490 MHz – 1.705 MHz	24000/F(kHz) uV/m at 30m ¹
1.705 MHz – 30 MHz	30 uV/m at 30m ¹
30 MHz – 88 MHz	100 uV/m (40.0 dBuV/m ¹) at 3m
88 MHz – 216 MHz	150 uV/m (43.5 dBuV/m ¹) at 3m
216 MHz – 960 MHz	200 uV/m (46.0 dBuV/m ¹) at 3m
Above 960 MHz	500 uV/m (54.0 dBuV/m ¹) at 3m
Above 1000 MHz	500 uV/m (54 dBuV/m ²) at 3m
Above 1000 MHz	500 uV/m (74 dBuV/m ³) at 3m

¹Limit is with Quasi Peak detector with bandwidths as defined in CISPR-16-1-1


²Limit is with 1 MHz measurement bandwidth and using an Average detector

³Limit is with 1 MHz measurement bandwidth and using a Peak detector

Based on ANSI C63.4 Section 4.2, if the Peak detector measurements do not exceed the Quasi-Peak limits, where defined, then the EUT is deemed to have passed the requirements.

Client	Rehabtronics Inc.	 Canada
Product	StimRay	
Standard(s)	RSS-247 Issue 2:2017 FCC Part 15 Subpart 15.247:2015	

Typical Radiated Emissions Setup

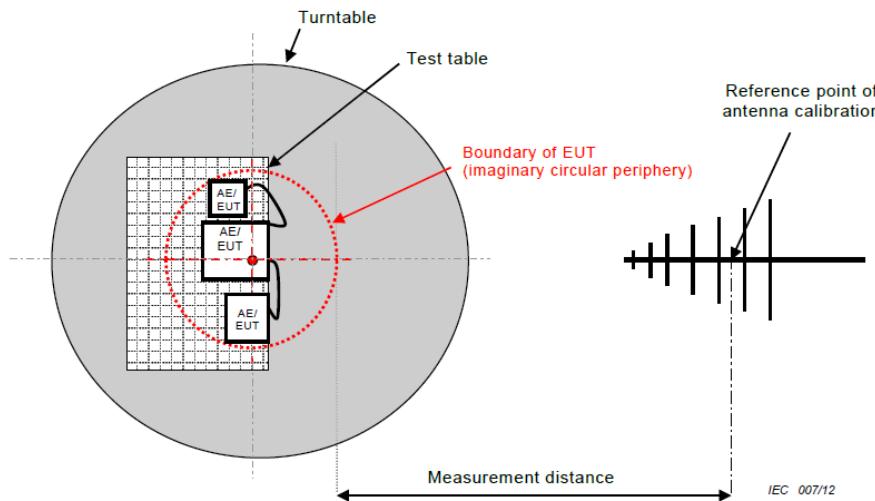

Measurement Uncertainty

The expanded measurement uncertainty is calculated in accordance with CISPR 16-4-2 and is $\pm 4.25\text{dB}$ for 30MHz – 1GHz and $\pm 4.93\text{dB}$ for 1GHz – 18GHz with a 'k=2' coverage factor and a 95% confidence level.

Preliminary Graphs

The graphs shown below are maximized peak measurement graphs measured with a resolution bandwidth greater than or equal to the final required detector over a full 0-360°. This peaking process is done as a worst case measurement and enables the detection of frequencies of concern for final measurement. For final measurements with the appropriate detector, where applicable, please refer to the tables under Final Measurements.


In accordance with FCC Part 15, Subpart A, Section 15.33, the device was scanned to the 10th harmonic (a minimum of 24.835 GHz).

Devices scanned may be scanned at alternate test distances and in accordance with FCC Part 15, Subpart A, Section 15.31, an extrapolation factor of 20 dB/decade was used above 30 MHz and 40 dB/decade below 30 MHz. For example for 1 meter measurements, an extrapolation factor 9.5 dB from 20 Log (1m / 3m) is applied.

Low, middle and high channels, each in three orthogonal axis were checked. However, the worst case graphs are presented.

Client	Rehabtronics Inc.	 Canada
Product	StimRay	
Standard(s)	RSS-247 Issue 2:2017 FCC Part 15 Subpart 15.247:2015	


Band-edge measurement graphs are shown for illustration purposes. See final measurement section for all measurements.

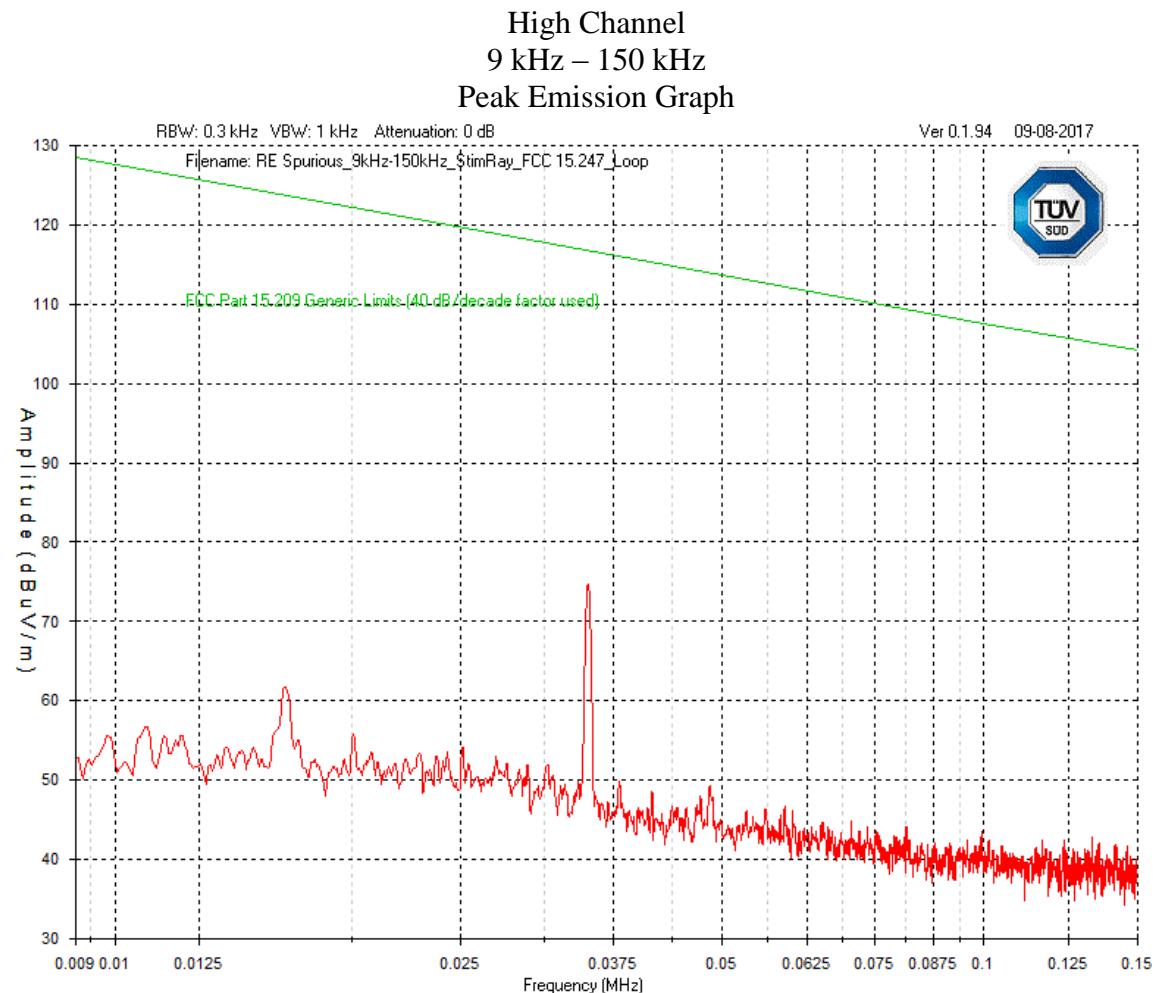

Client	Rehabtronics Inc.
Product	StimRay
Standard(s)	RSS-247 Issue 2:2017 FCC Part 15 Subpart 15.247:2015




High Channel
150 kHz – 30 MHz
Peak Emission Graph

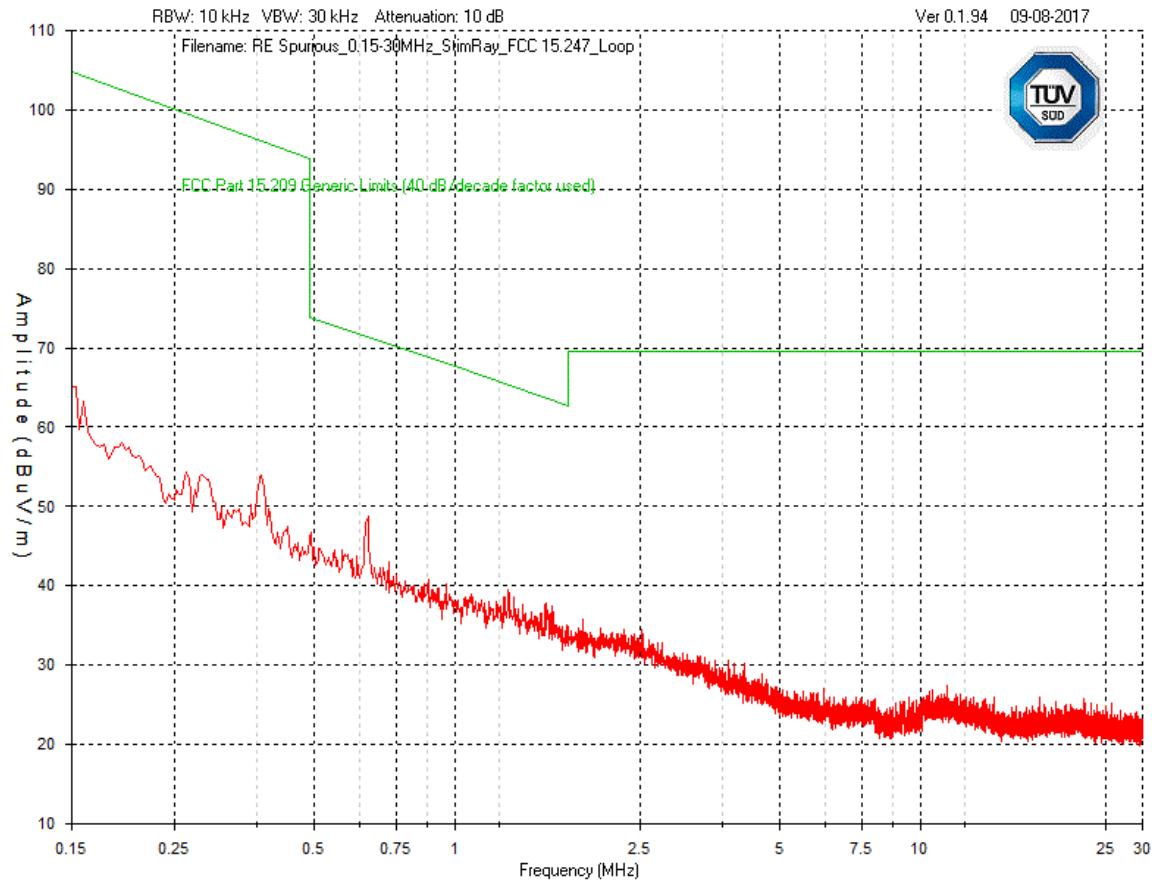

Client	Rehabtronics Inc.
Product	StimRay
Standard(s)	RSS-247 Issue 2:2017 FCC Part 15 Subpart 15.247:2015




High Channel – 30 MHz – 1 GHz Horizontal - Peak Emission Graph

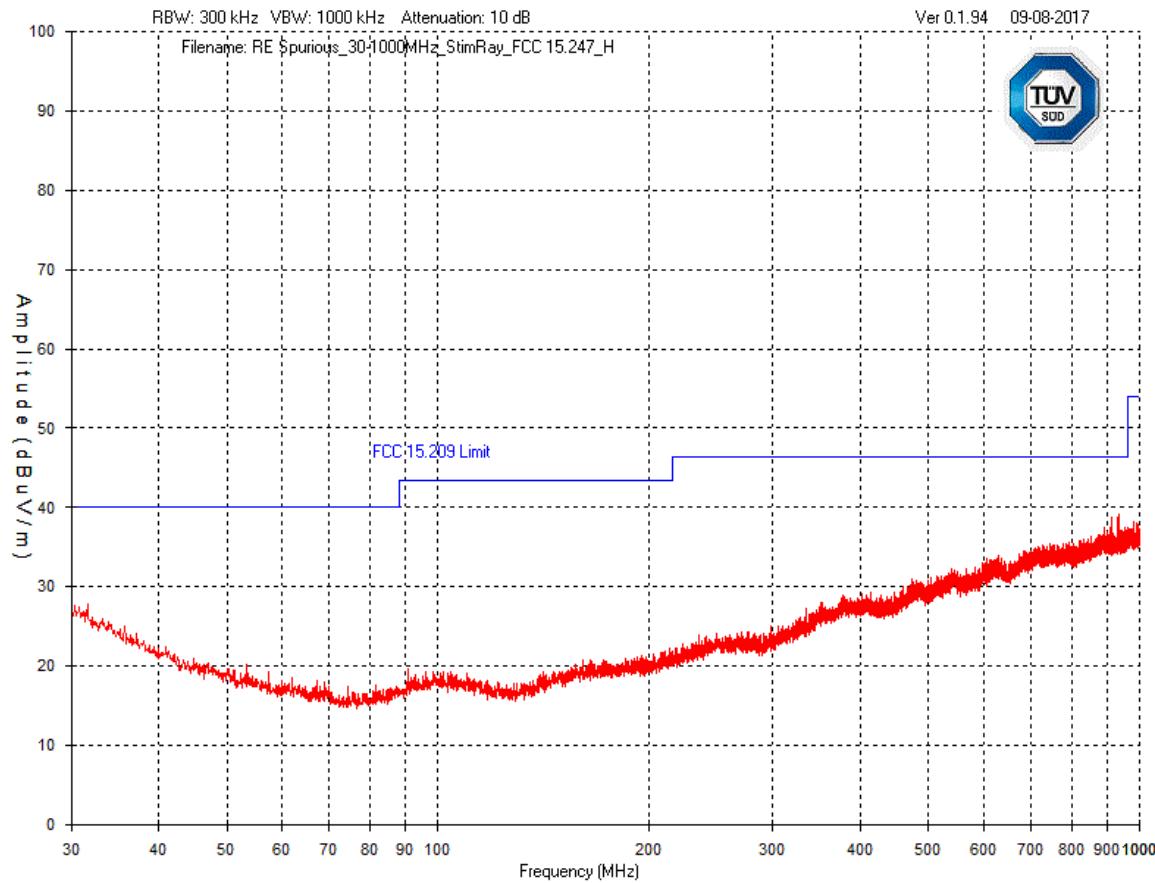


Client	Rehabtronics Inc.	 Canada
Product	StimRay	
Standard(s)	RSS-247 Issue 2:2017 FCC Part 15 Subpart 15.247:2015	

High Channel – 1 GHz – 2 GHz Horizontal - Peak Emission Graph

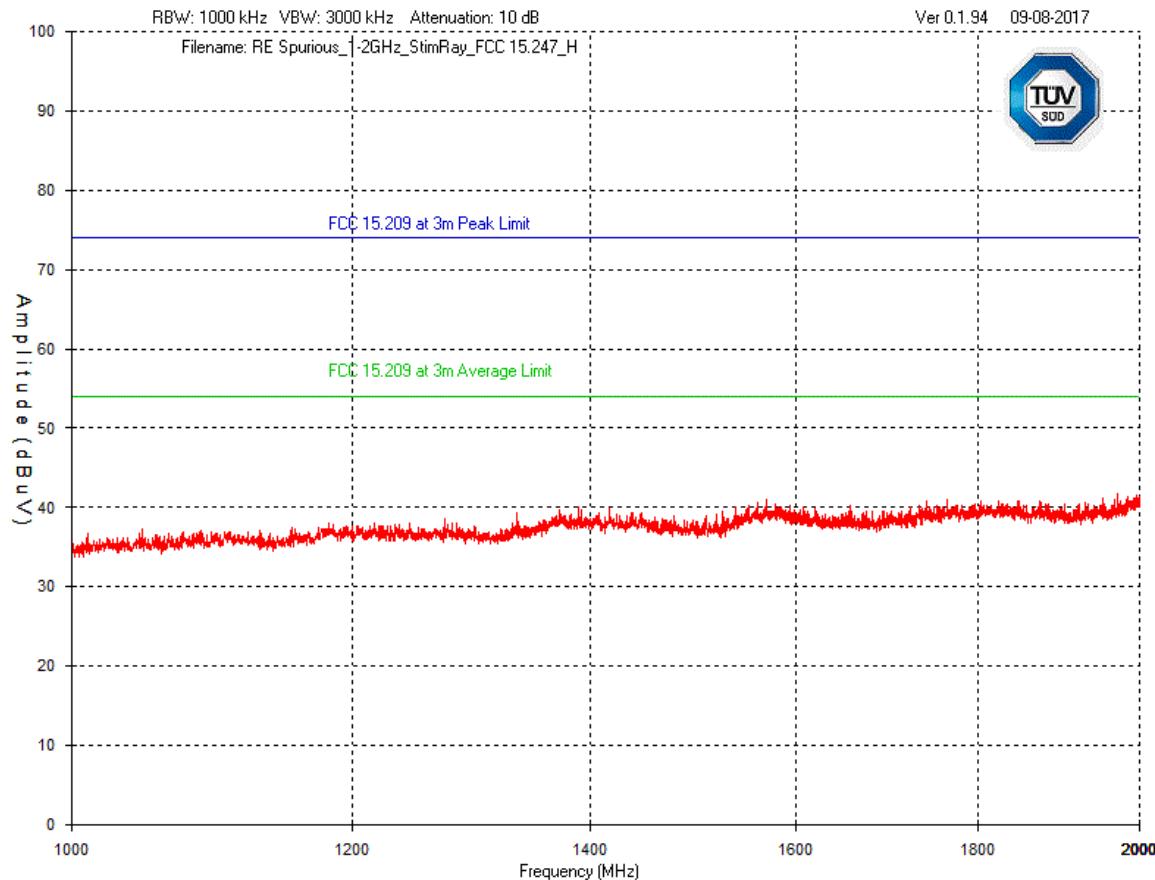


Client	Rehabtronics Inc.	 Canada
Product	StimRay	
Standard(s)	RSS-247 Issue 2:2017 FCC Part 15 Subpart 15.247:2015	

High Channel – 2 GHz – 4 GHz Horizontal - Peak Emission Graph

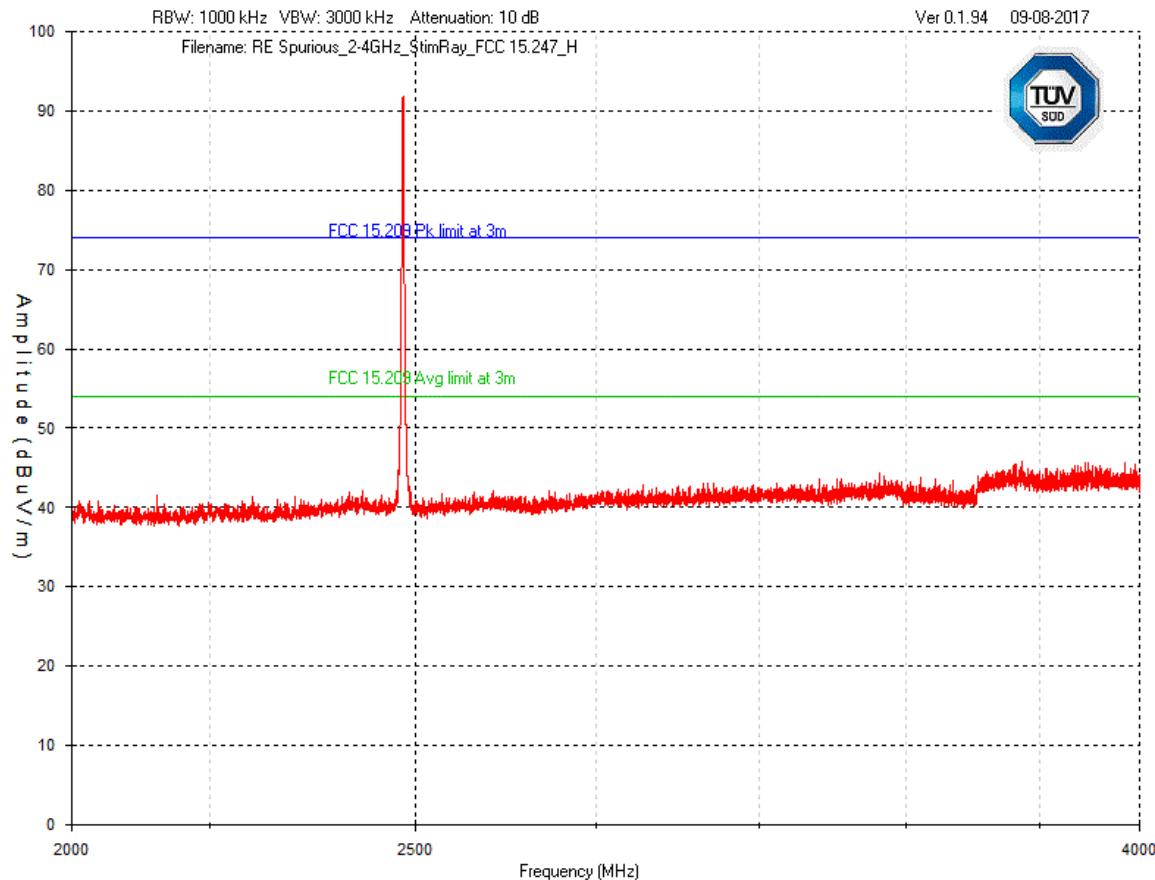


Client	Rehabtronics Inc.	 Canada
Product	StimRay	
Standard(s)	RSS-247 Issue 2:2017 FCC Part 15 Subpart 15.247:2015	

High Channel – 4 GHz – 10 GHz Horizontal - Peak Emission Graph

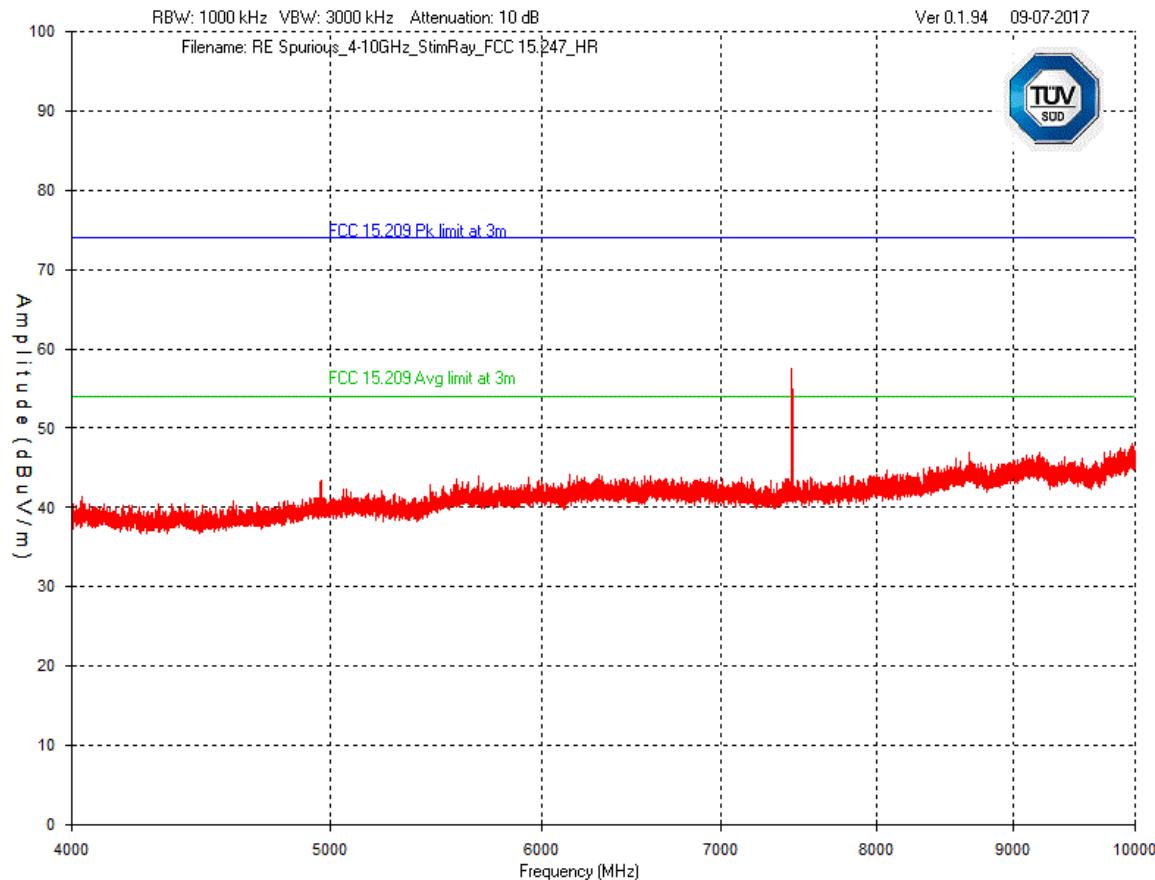

Client	Rehabtronics Inc.	 Canada
Product	StimRay	
Standard(s)	RSS-247 Issue 2:2017 FCC Part 15 Subpart 15.247:2015	


High Channel – 10 GHz – 18 GHz Horizontal - Peak Emission Graph

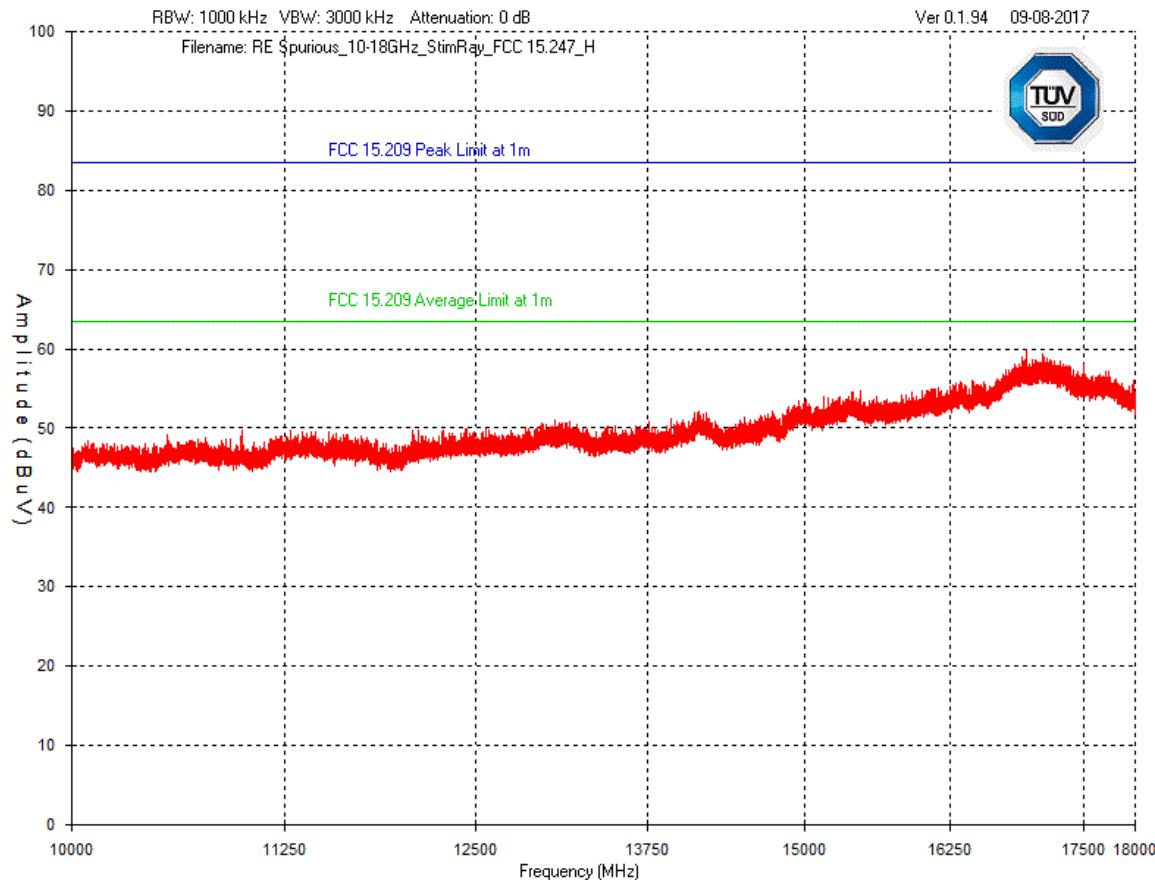

Plot was taken at a 1 meter distance. All emissions were noise floor of measurement instrument. No emissions were found in this frequency range.

Client	Rehabtronics Inc.	 Canada
Product	StimRay	
Standard(s)	RSS-247 Issue 2:2017 FCC Part 15 Subpart 15.247:2015	


High Channel – 18 GHz – 26.5 GHz Horizontal - Peak Emission Graph

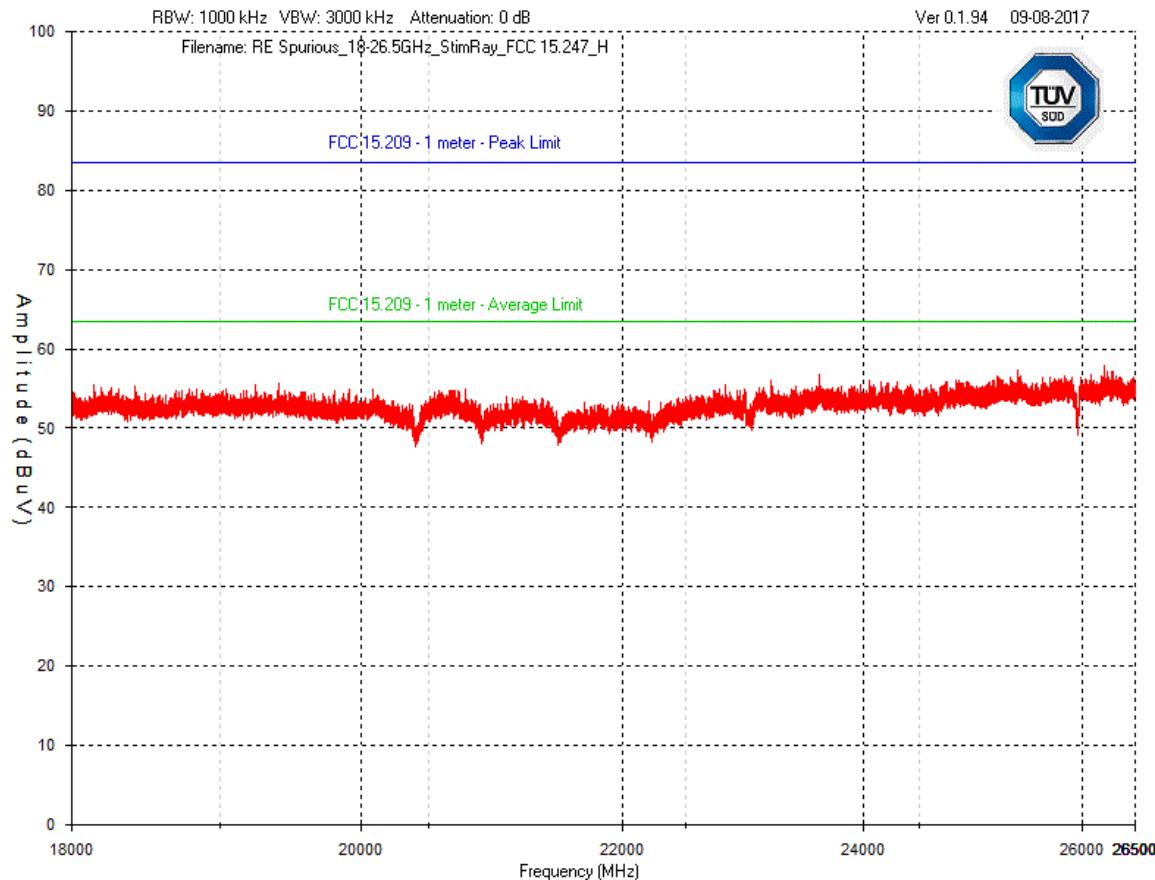

Plot was taken at a 1 meter distance. All emissions were noise floor of measurement instrument. No emissions were found in this frequency range.


Client	Rehabtronics Inc.	 Canada
Product	StimRay	
Standard(s)	RSS-247 Issue 2:2017 FCC Part 15 Subpart 15.247:2015	

High Channel – 30 MHz – 1 GHz Vertical - Peak Emission Graph

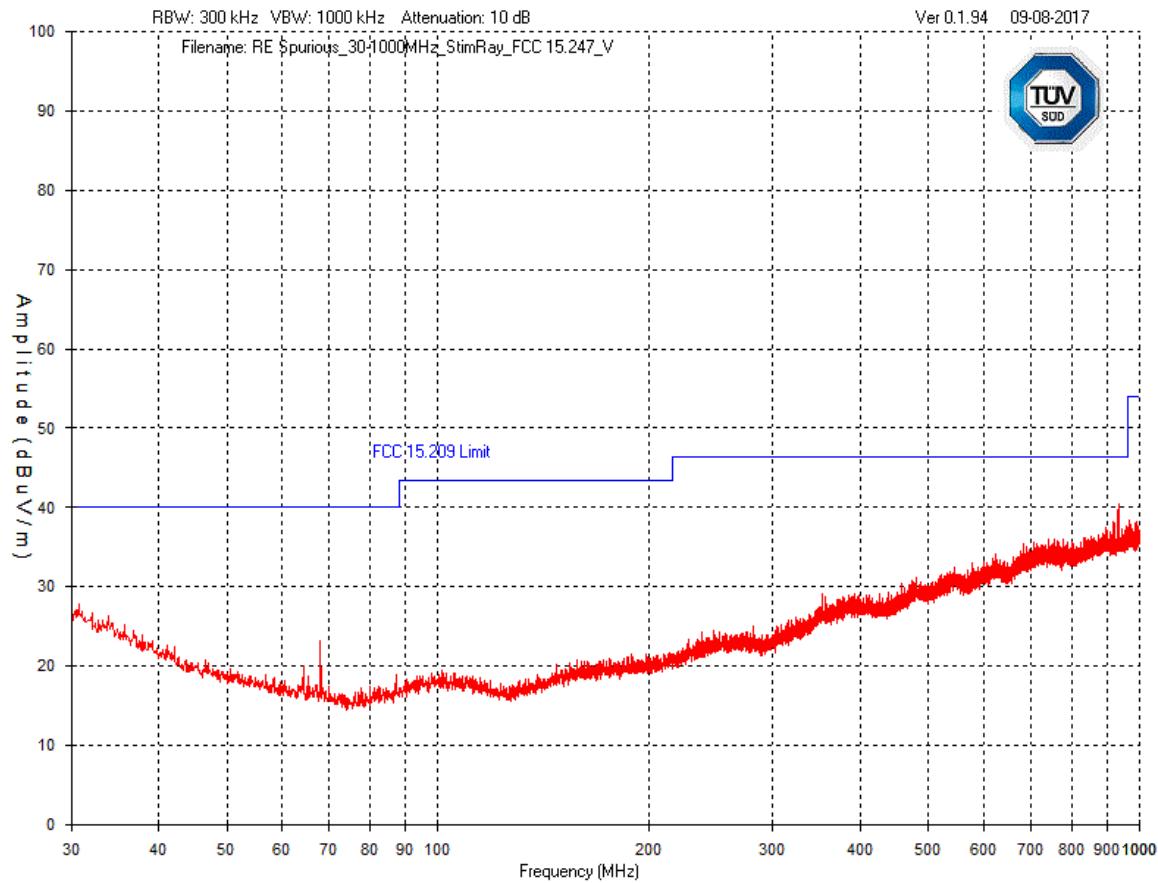


Client	Rehabtronics Inc.	 Canada
Product	StimRay	
Standard(s)	RSS-247 Issue 2:2017 FCC Part 15 Subpart 15.247:2015	

High Channel – 1 GHz – 2 GHz Vertical - Peak Emission Graph

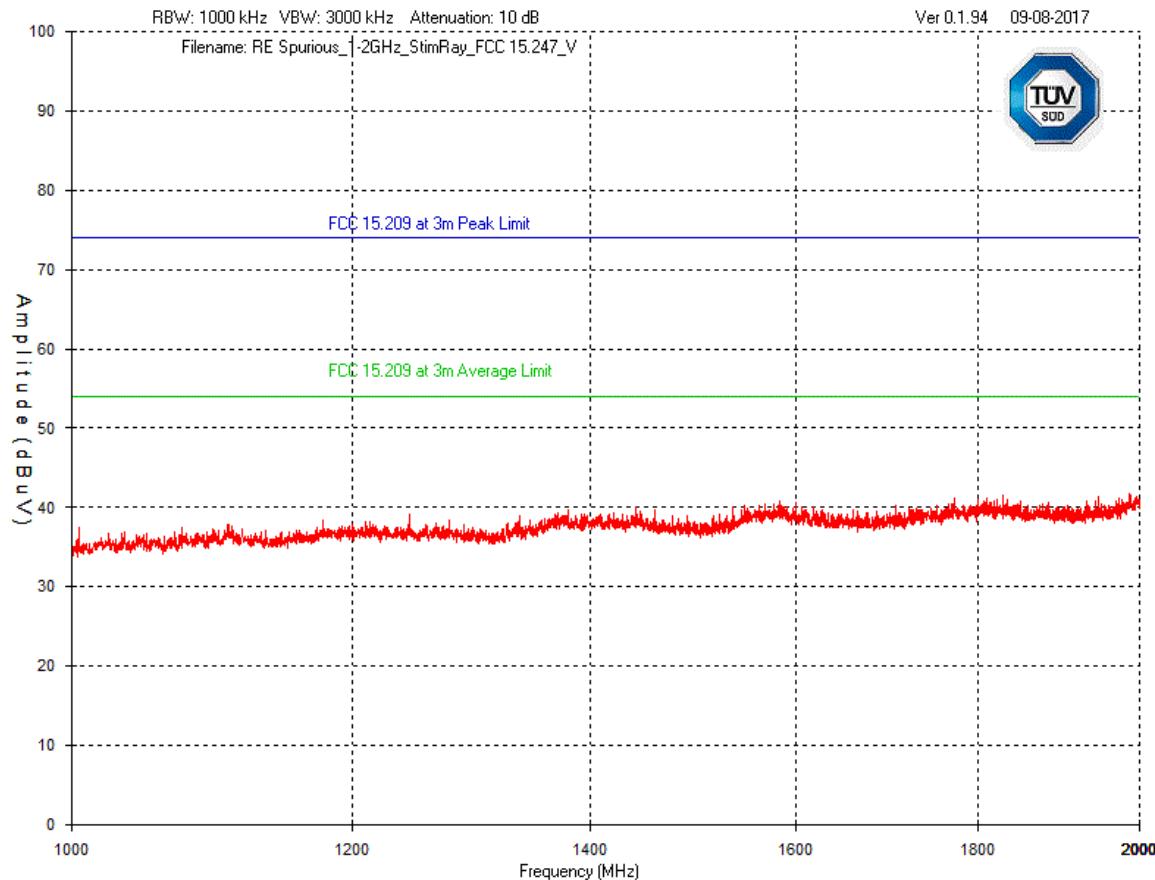


Client	Rehabtronics Inc.	 Canada
Product	StimRay	
Standard(s)	RSS-247 Issue 2:2017 FCC Part 15 Subpart 15.247:2015	

High Channel – 2 GHz – 4 GHz Vertical - Peak Emission Graph

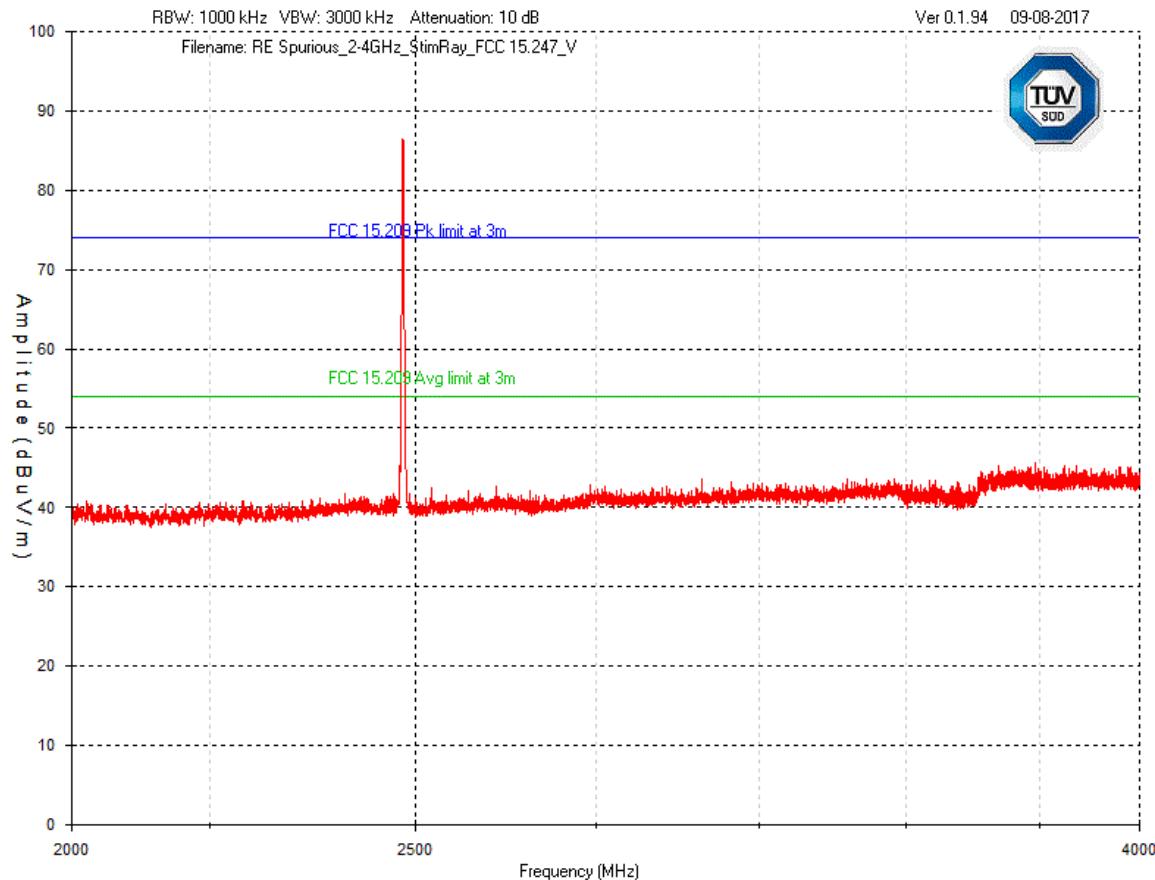


Client	Rehabtronics Inc.	 Canada
Product	StimRay	
Standard(s)	RSS-247 Issue 2:2017 FCC Part 15 Subpart 15.247:2015	

High Channel – 4 GHz – 10 GHz Vertical - Peak Emission Graph

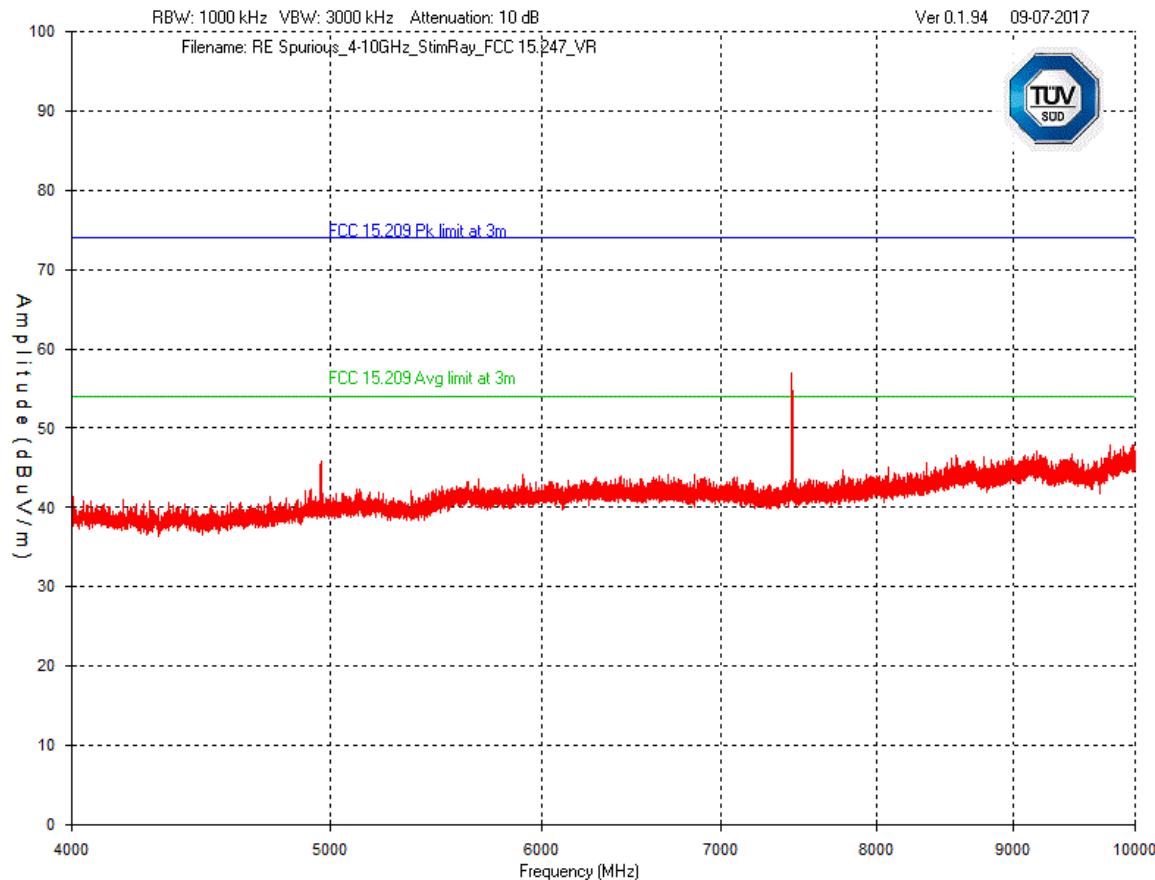

Client	Rehabtronics Inc.	 Canada
Product	StimRay	
Standard(s)	RSS-247 Issue 2:2017 FCC Part 15 Subpart 15.247:2015	


High Channel – 10 GHz – 18 GHz Vertical - Peak Emission Graph

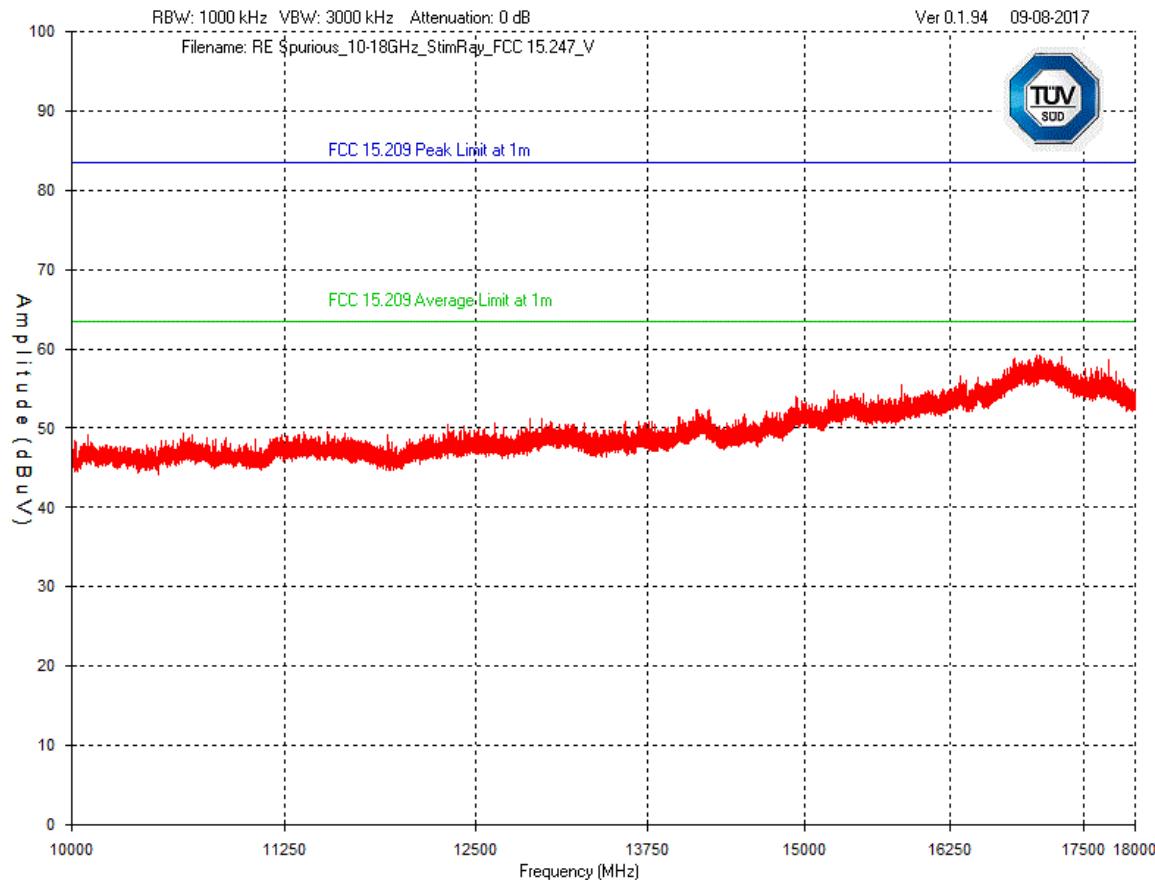

Plot was taken at a 1 meter distance. All emissions were noise floor of measurement instrument. No emissions were found in this frequency range.

Client	Rehabtronics Inc.	 Canada
Product	StimRay	
Standard(s)	RSS-247 Issue 2:2017 FCC Part 15 Subpart 15.247:2015	


High Channel – 18 GHz – 26.5 GHz
Vertical - Peak Emission Graph

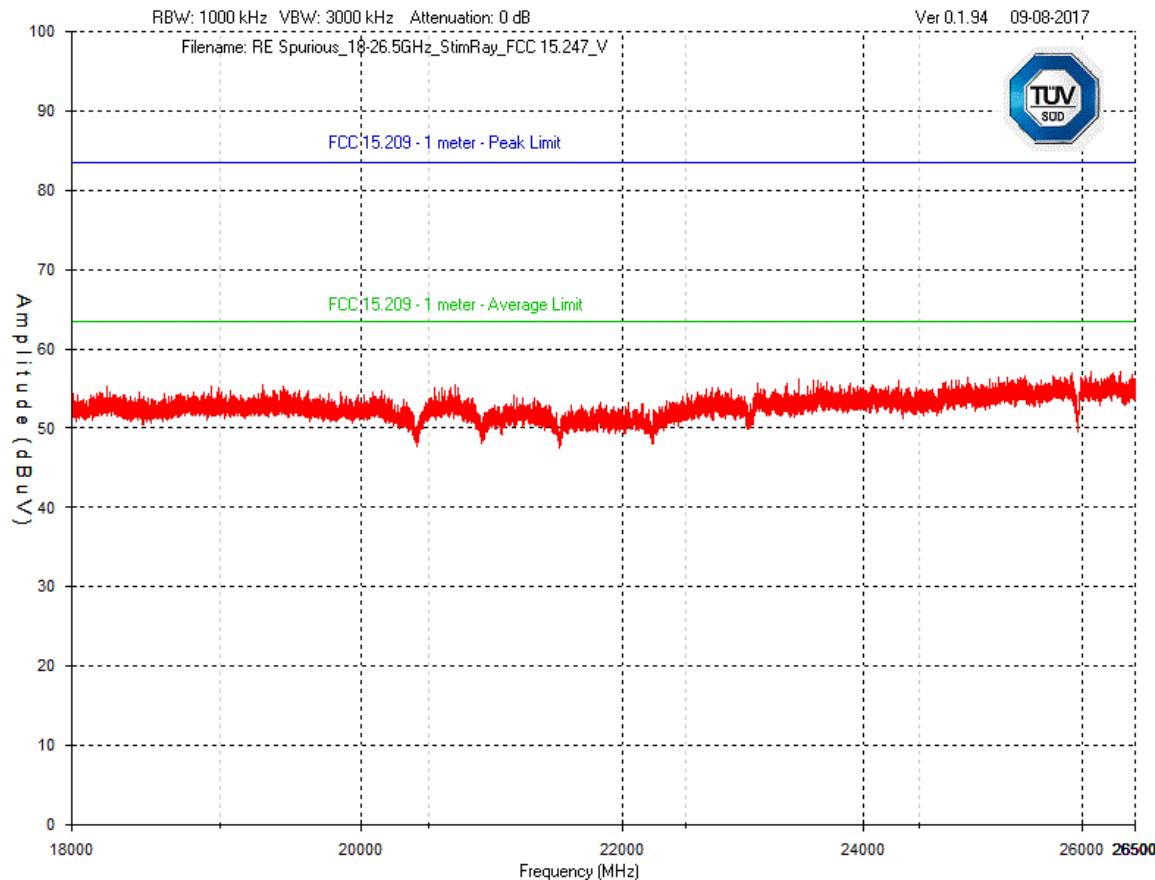

Plot was taken at a 1 meter distance. All emissions were noise floor of measurement instrument. No emissions were found in this frequency range.

Client	Rehabtronics Inc.	 Canada
Product	StimRay	
Standard(s)	RSS-247 Issue 2:2017 FCC Part 15 Subpart 15.247:2015	

Low Channel
Band Edge – 2310MHz – 2390MHz
Horizontal - Peak Emission

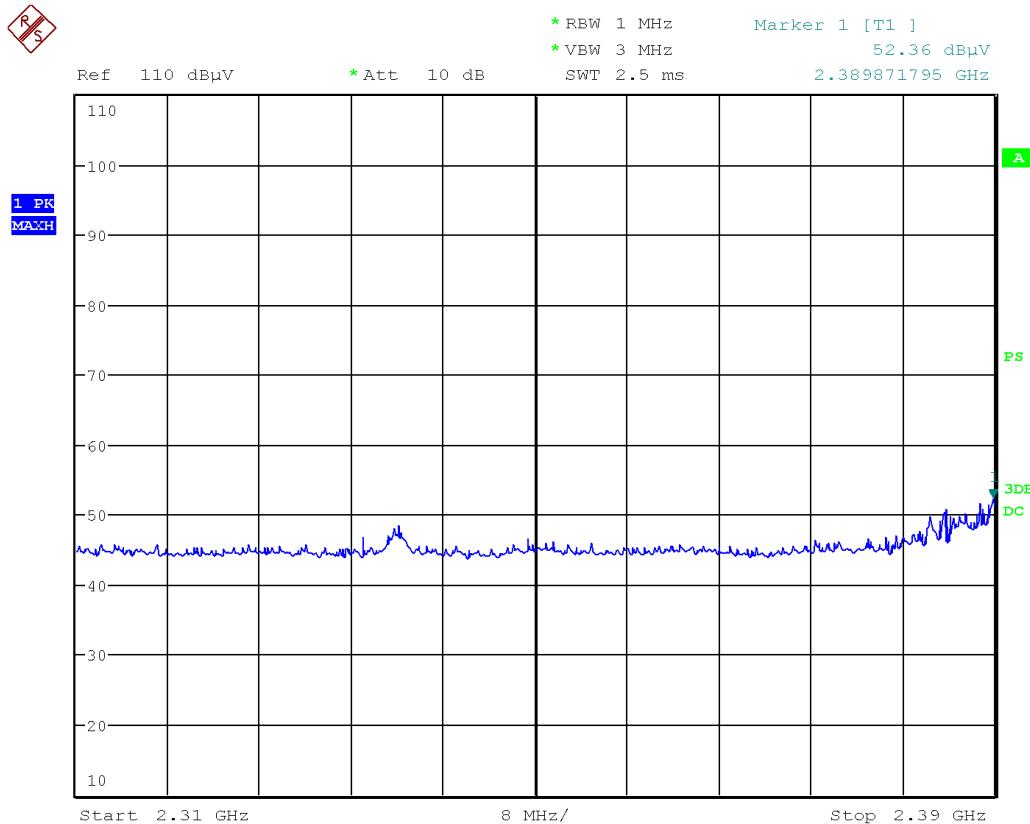


Date: 7.SEP.2017 14:20:01

Note: Restricted band Band Edge plot was taken at a 3m measurement distance. The marker shows the raw value. See the Final Measurements and Results section below for correct values.

Client	Rehabtronics Inc.	 Canada
Product	StimRay	
Standard(s)	RSS-247 Issue 2:2017 FCC Part 15 Subpart 15.247:2015	

Low Channel
Band Edge – 2483.5MHz – 2500MHz
Horizontal - Peak Emission

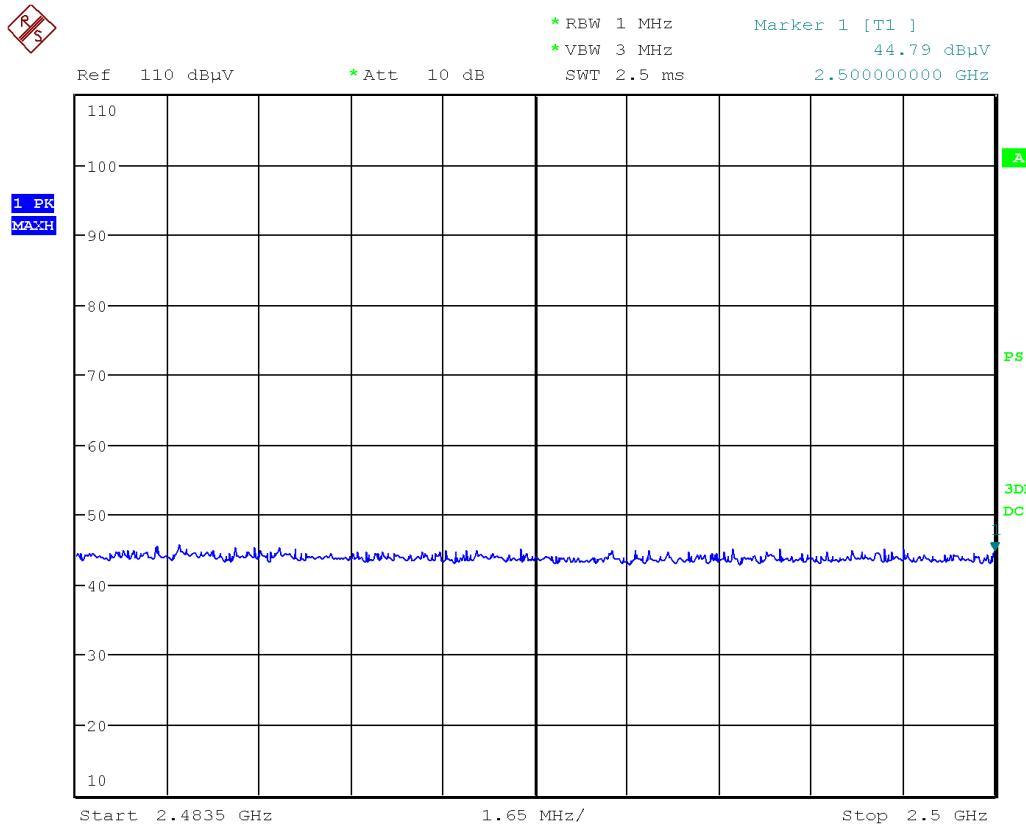


Date: 7.SEP.2017 14:36:51

Note: Restricted band Band Edge plot was taken at a 3m measurement distance. The marker shows the raw value. See the Final Measurements and Results section below for correct values.

Client	Rehabtronics Inc.	 Canada
Product	StimRay	
Standard(s)	RSS-247 Issue 2:2017 FCC Part 15 Subpart 15.247:2015	

Low Channel
Band Edge – 2310MHz – 2390MHz
Vertical - Peak Emission

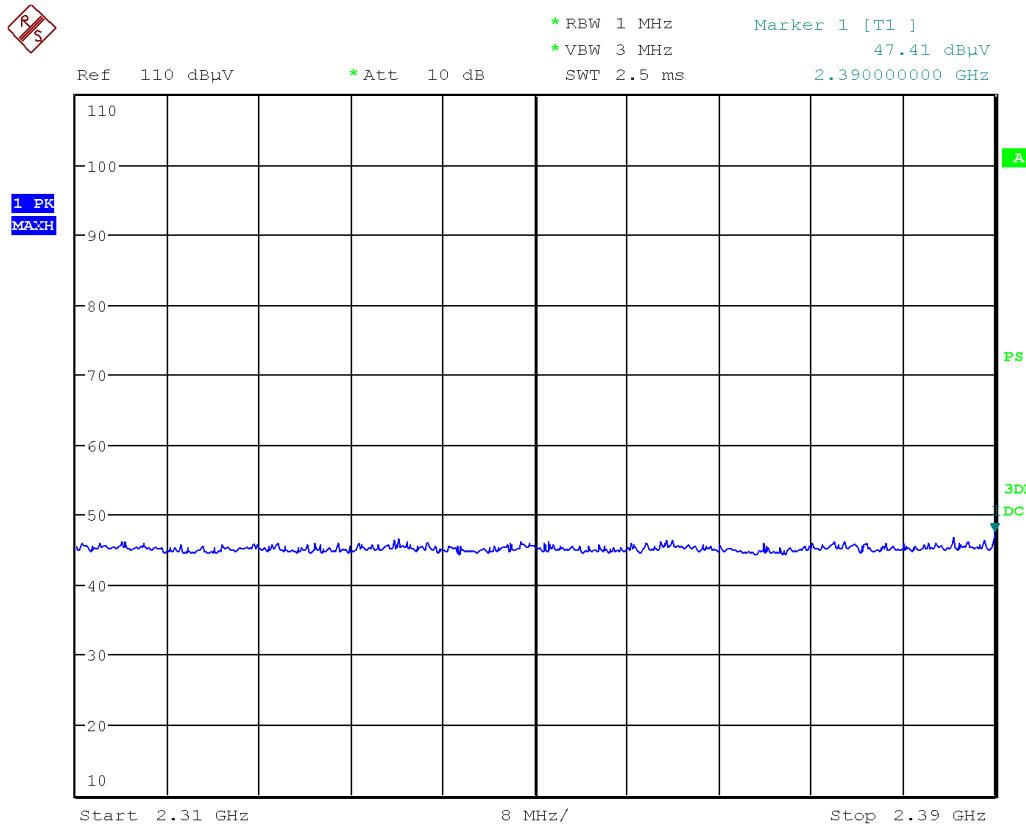


Date: 7.SEP.2017 14:16:25

Note: Restricted band Band Edge plot was taken at a 3m measurement distance. The marker shows the raw value. See the Final Measurements and Results section below for correct values.

Client	Rehabtronics Inc.	 Canada
Product	StimRay	
Standard(s)	RSS-247 Issue 2:2017 FCC Part 15 Subpart 15.247:2015	

Low Channel
Band Edge – 2483.5MHz – 2500MHz
Vertical - Peak Emission

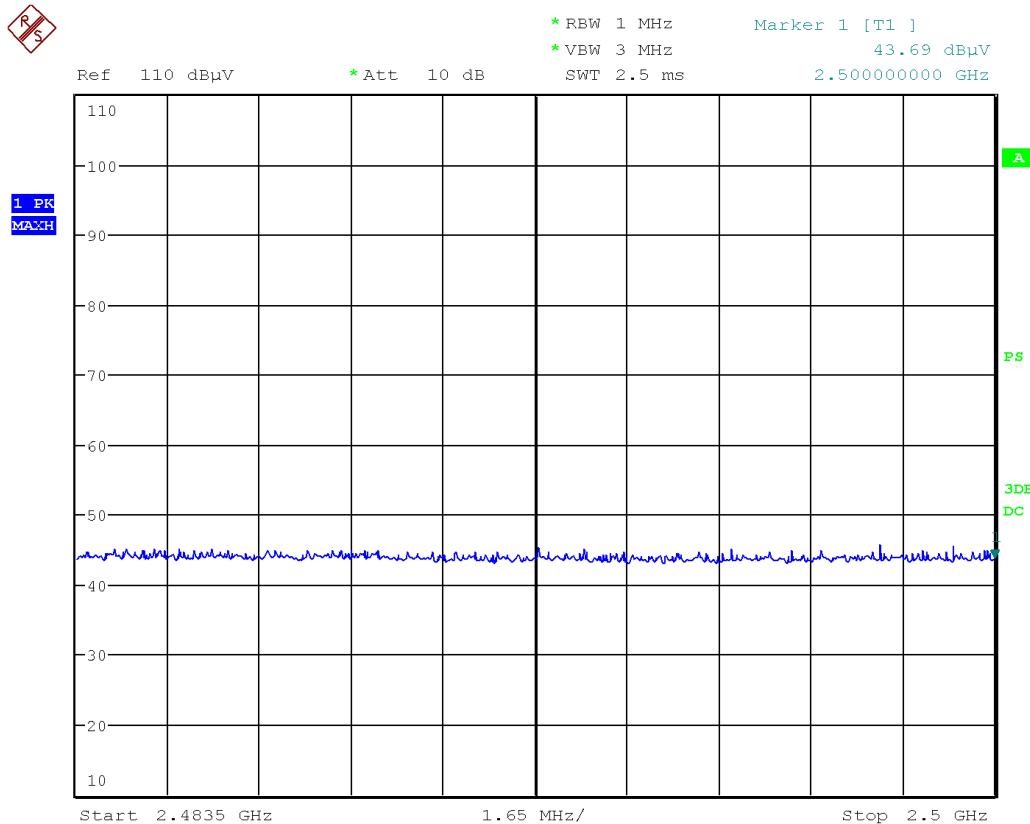


Date: 7.SEP.2017 14:34:43

Note: Restricted band Band Edge plot was taken at a 3m measurement distance. The marker shows the raw value. See the Final Measurements and Results section below for correct values.

Client	Rehabtronics Inc.	 Canada
Product	StimRay	
Standard(s)	RSS-247 Issue 2:2017 FCC Part 15 Subpart 15.247:2015	

Hi Channel
 Band Edge – 2310MHz – 2390MHz
 Horizontal - Peak Emission

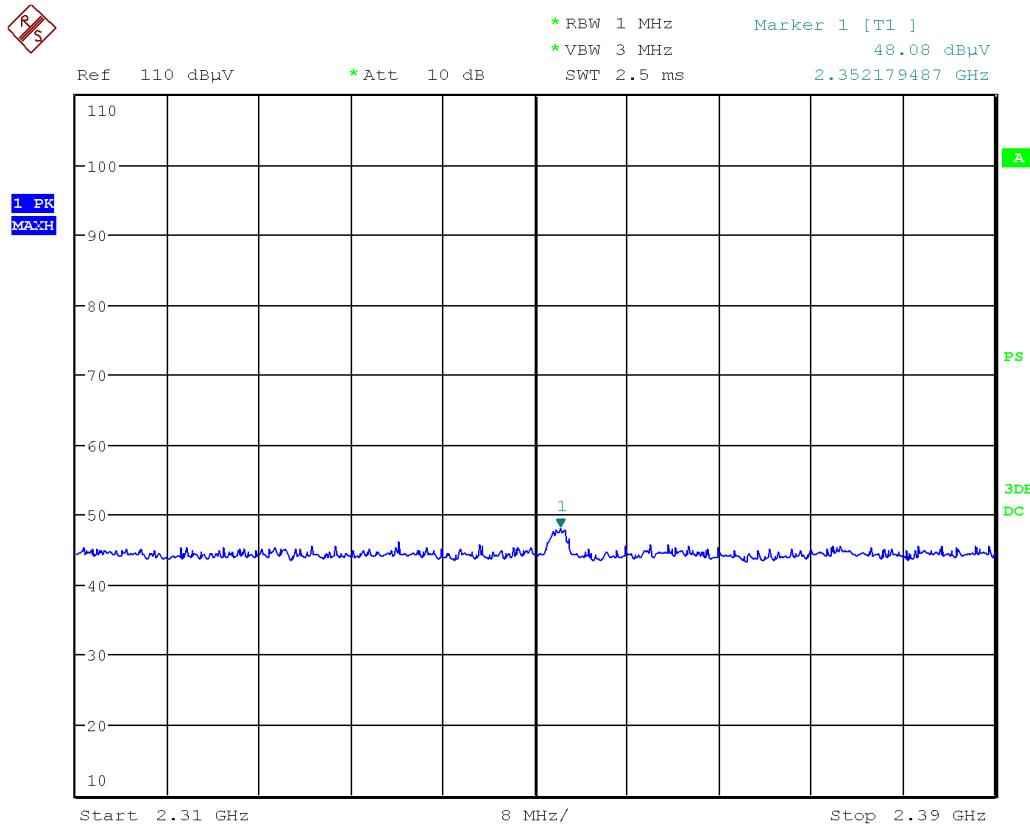


Date: 7.SEP.2017 14:53:25

Note: Restricted band Band Edge plot was taken at a 3m measurement distance. The marker shows the raw value. See the Final Measurements and Results section below for correct values.

Client	Rehabtronics Inc.	 Canada
Product	StimRay	
Standard(s)	RSS-247 Issue 2:2017 FCC Part 15 Subpart 15.247:2015	

Hi Channel
Band Edge – 2483.5MHz – 2500MHz
Horizontal - Peak Emission

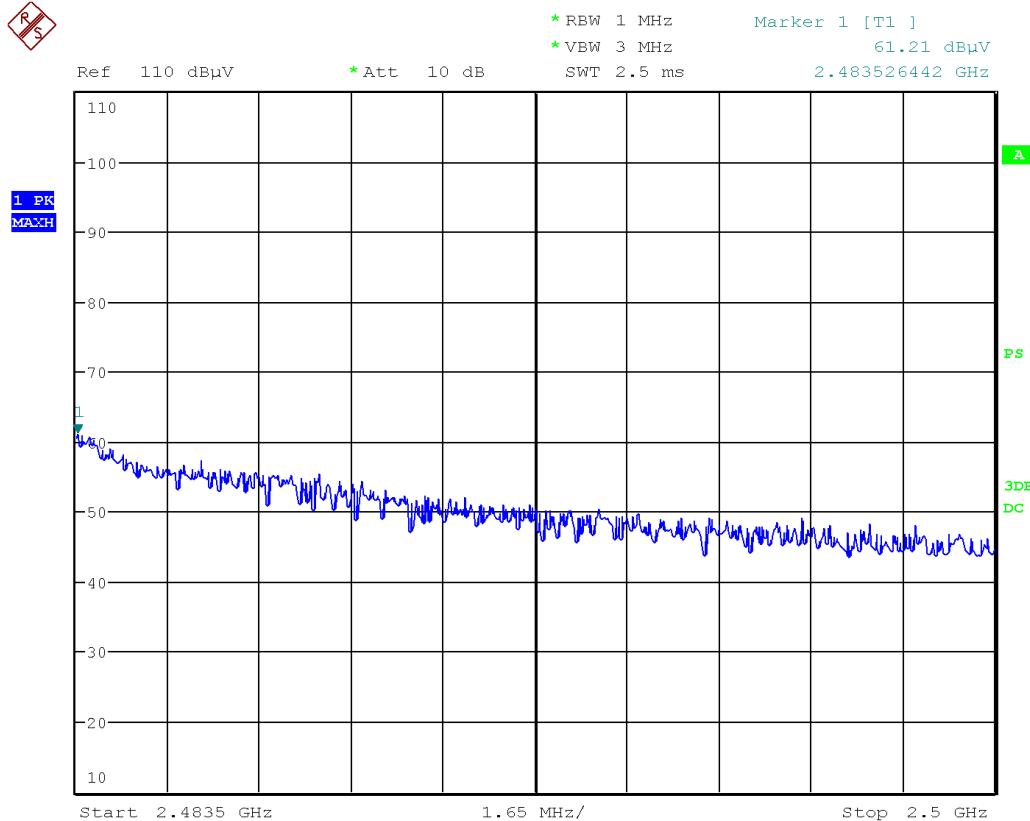


Date: 7.SEP.2017 14:59:34

Note: Restricted band Band Edge plot was taken at a 3m measurement distance. The marker shows the raw value. See the Final Measurements and Results section below for correct values.

Client	Rehabtronics Inc.	 Canada
Product	StimRay	
Standard(s)	RSS-247 Issue 2:2017 FCC Part 15 Subpart 15.247:2015	

Hi Channel (11)
 Band Edge – 2310MHz – 2390MHz
 Vertical - Peak Emission

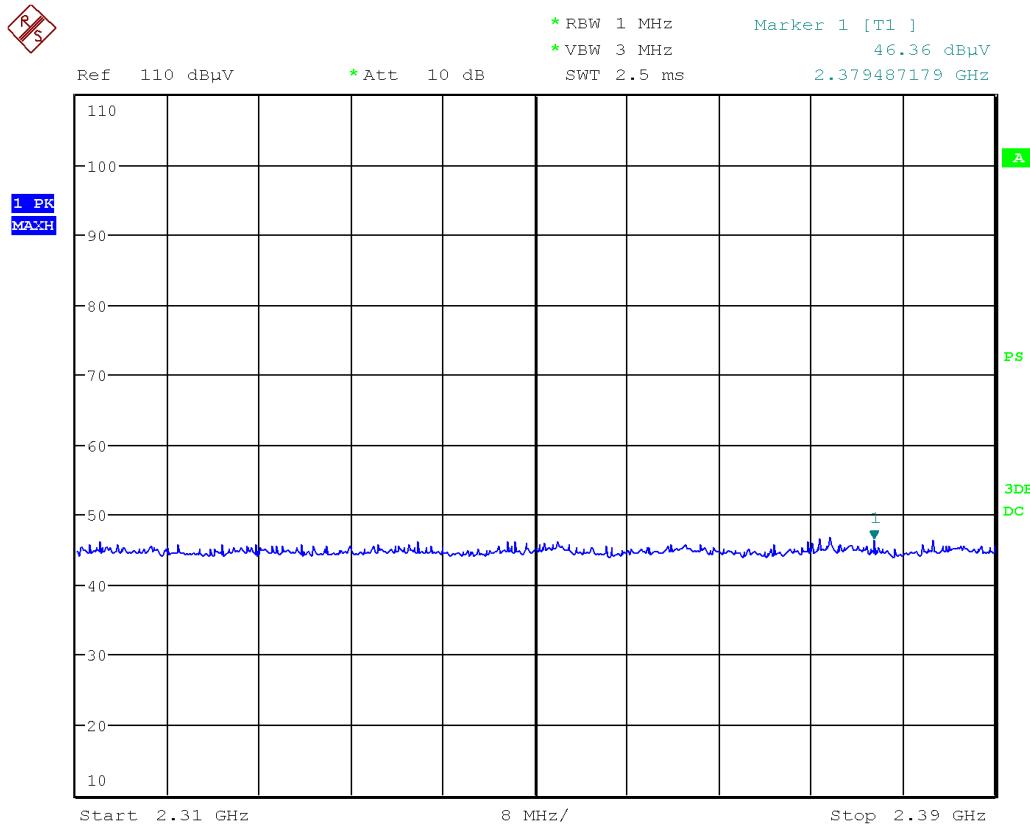


Date: 7.SEP.2017 14:52:29

Note: Restricted band Band Edge plot was taken at a 3m measurement distance. The marker shows the raw value. See the Final Measurements and Results section below for correct values.

Client	Rehabtronics Inc.	 Canada
Product	StimRay	
Standard(s)	RSS-247 Issue 2:2017 FCC Part 15 Subpart 15.247:2015	

Hi Channel (11)
Band Edge – 2483.5MHz – 2500MHz
Vertical - Peak Emission

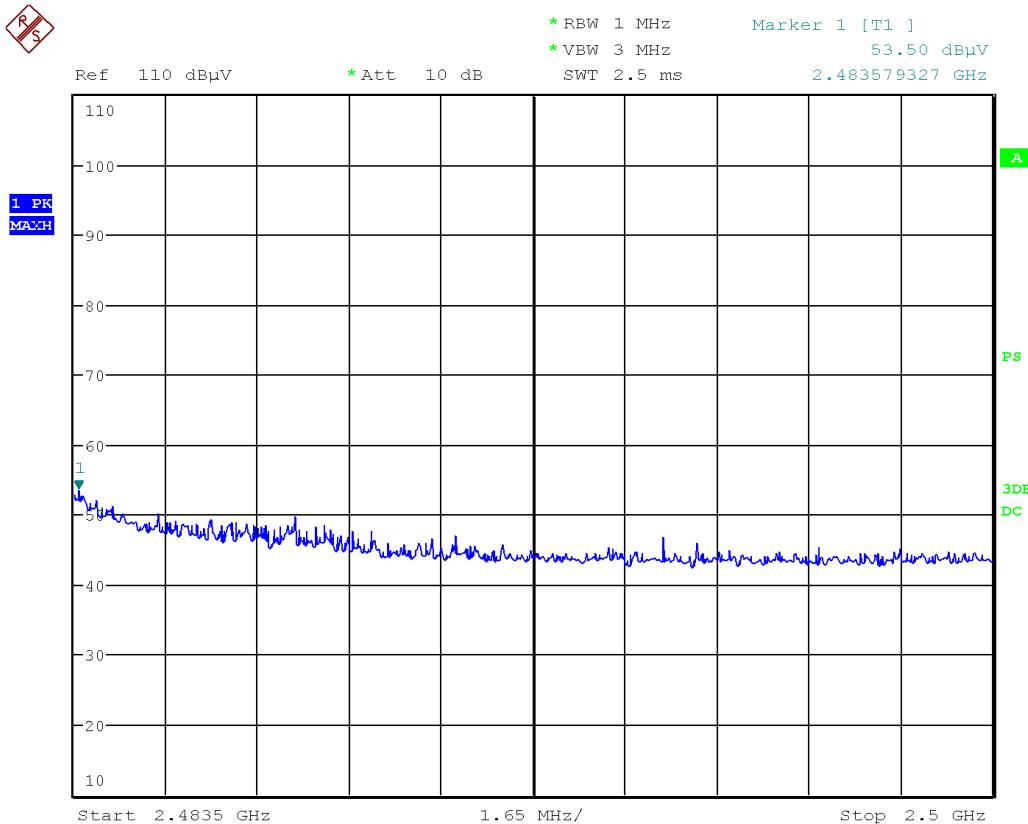

Date: 7.SEP.2017 15:00:46

Note: Restricted band Band Edge plot was taken at a 3m measurement distance. The marker shows the raw value. See the Final Measurements and Results section below for correct values.

Client	Rehabtronics Inc.	RSS-247 Issue 2:2017 FCC Part 15 Subpart 15.247:2015
Product	StimRay	
Standard(s)		



Final Measurements and Results

The EUT passed. Low, middle, and high bands were measured.

In accordance with 15.247(d), only frequencies exceeding the 15.209 limit that occur within the bands listed in 15.205 need to be verified with a final detector. Emissions outside the restricted bands were measured for informational purposes.

The measurements were maximized by rotating the turn table over a full 0-360 rotation and the antenna height was varied from 1 m to 4 m.

Spurious Emission Measurements

Supply			120Vac 60Hz								
Frequency (MHz)	Detector Peak/QP/AVG	Received Signal (dB μ V)	Antenna Factor (dB/m)	Atten Factor (dB)	Cable Factor (dB)	Pre-Amp (dB)	Level (dB μ V/m)	QP Limit (dB μ V/m)	QP Margin (dB)	Pass/Fail	
Horizontal Antenna Polarization											
931.644	Peak	35.3	23.4	6.0	2.6	-28.1	39.2	46.4	7.2	Pass	
911.156	Peak	35.1	23.4	6.0	2.5	-28.1	38.9	46.4	7.5	Pass	
31.651	Peak	34.0	15.8	6.0	0.4	-28.5	27.7	40.0	12.3	Pass	
718.807	Peak	31.3	22.4	6.0	2.3	-28.6	33.4	46.4	13.0	Pass	
30.000	Peak	31.9	16.4	6.0	0.4	-28.5	26.2	40.0	13.8	Pass	
7441.44	AVG	47.2	29.2	0.0	7.6	-35.7	48.3	54.0	5.7	Pass	
Vertical Antenna Polarization											
931.644	Peak	36.7	23.4	6.0	2.6	-28.1	40.6	46.4	5.8	Pass	
916.205	Peak	34.5	23.4	6.0	2.5	-28.1	38.3	46.4	8.1	Pass	
742.013	Peak	34.0	22.3	6.0	2.3	-28.6	36.0	46.4	10.4	Pass	
30.777	Peak	33.4	16.6	6.0	0.4	-28.5	27.9	40.0	12.1	Pass	
30.000	Peak	32.1	16.4	6.0	0.4	-28.5	26.4	40.0	13.6	Pass	
7439.54	AVG	46.8	29.2	0.0	7.6	-35.7	47.9	54.0	6.1	Pass	

Client	Rehabtronics Inc.	 Canada
Product	StimRay	
Standard(s)	RSS-247 Issue 2:2017 FCC Part 15 Subpart 15.247:2015	

Peak Power and Band Edge Measurements

Test Frequency (MHz)	Detection Mode	Antenna Polarity (Horz/Vert)	Received Signal (dB μ V)	Antenna Factor (dB/m)	Cable Factor (dB)	Attenuator (dB)	Pre-Amp Gain (dB)	Level (dB μ V/m)	Emission Limit (dB μ V/m)	Margin (dB)	Result
Low Channel - X axis											
2402	Peak	Horz	99.2	26.4	3.6	0.0	-35.8	93.4			PASS
2402	Avg	Horz	92.3	26.4	3.6	0.0	-35.8	86.5			PASS
2402	Peak	Vert	100.6	26.4	3.6	0.0	-35.8	94.8			PASS
2402	Avg	Vert	91.9	26.4	3.6	0.0	-35.8	86.1			PASS
2390	Peak	Horz	52.4	26.4	3.6	0.0	-35.8	46.5	74.0	27.5	PASS
2390	Avg	Horz	32.9	26.4	3.6	0.0	-35.8	27.0	54.0	27.0	PASS
2390	Peak	Vert	47.4	26.4	3.6	0.0	-35.8	41.5	74.0	32.5	PASS
2390	Avg	Vert	32.2	26.4	3.6	0.0	-35.8	26.3	54.0	27.7	PASS
2338	Avg	Horz	38.6	26.2	3.5	0.0	-35.9	32.4	54.0	21.6	PASS
2338	Avg	Vert	33.6	26.2	3.5	0.0	-35.9	27.4	54.0	26.6	PASS
2485	Peak	Horz	45.6	26.2	3.6	0.0	-35.8	39.6	74.0	34.4	PASS
2485	Avg	Vert	31.3	26.2	3.6	0.0	-35.8	25.3	54.0	28.7	PASS
2492	Peak	Vert	45.2	26.2	3.6	0.0	-35.8	39.2	74.0	34.8	PASS
2498	Avg	Horz	31.8	26.2	3.6	0.0	-35.8	25.8	54.0	28.2	PASS
2500	Peak	Horz	44.8	26.2	3.6	0.0	-35.8	38.7	74.0	35.3	PASS
2500	Avg	Horz	31.1	26.2	3.6	0.0	-35.8	25.0	54.0	29.0	PASS
2500	Peak	Vert	30.9	26.2	3.6	0.0	-35.8	24.8	74.0	49.2	PASS
2500	Avg	Vert	32.2	26.2	3.6	0.0	-35.8	26.1	54.0	27.9	PASS
Mid Channel - X axis											
2440	Peak	Horz	100.7	26.3	3.6	0.0	-35.8	94.8			PASS
2440	Avg	Horz	92.4	26.3	3.6	0.0	-35.8	86.5			PASS
2440	Peak	Vert	95.5	26.3	3.6	0.0	-35.8	89.6			PASS
2440	Avg	Vert	87.4	26.3	3.6	0.0	-35.8	81.5			PASS
High Channel - X axis											
2480	Peak	Horz	99.5	26.2	3.6	0.0	-35.8	93.5			PASS
2480	Avg	Horz	92.3	26.2	3.6	0.0	-35.8	86.3			PASS
2480	Peak	Vert	101.3	26.2	3.6	0.0	-35.8	95.3			PASS
2480	Avg	Vert	89.1	26.2	3.6	0.0	-35.8	83.1			PASS
2352	Peak	Horz	48.1	26.2	3.5	0.0	-35.8	42.0	74.0	32.0	PASS
2352	Avg	Horz	36.3	26.2	3.5	0.0	-35.8	30.2	54.0	23.8	PASS
2379	Peak	Vert	46.4	26.2	3.5	0.0	-35.8	40.3	74.0	33.7	PASS
2352	Avg	Vert	33.9	26.2	3.5	0.0	-35.8	27.8	54.0	26.2	PASS
2483.5	Peak	Horz	61.2	26.2	3.6	0.0	-35.8	55.2	74.0	18.8	PASS
2483.5	Avg	Horz	49.7	26.2	3.6	0.0	-35.8	43.7	54.0	10.3	PASS
2483.5	Peak	Vert	53.5	26.2	3.6	0.0	-35.8	47.5	74.0	26.5	PASS
2483.5	Avg	Vert	41.5	26.2	3.6	0.0	-35.8	35.5	54.0	18.5	PASS

RENote: Maximum of -20dB duty cycle correction factor is applicable to the peak pulse amplitude for calculating the average emissions of this unit, however the EUT pass the test without applying any duty cycle correction factor.

Client	Rehabtronics Inc.	 Canada
Product	StimRay	
Standard(s)	RSS-247 Issue 2:2017 FCC Part 15 Subpart 15.247:2015	

Test Equipment List

Equipment	Model No.	Manufacturer	Last Calibration / Verification Date	Next Calibration / Verification Date	Asset #
Spectrum Analyzer	ESU 40	Rohde & Schwarz	Jan. 06, 2016	Jan. 06, 2018	GEMC 233
Horn Antenna 2 – 18 GHz	WBH218HN	Q-par	Feb. 12, 2016	Feb. 12, 2018	GEMC 6375
Pre-Amp 1 – 26.5 GHz	HP 8449B	HP	Oct. 12, 2016	Oct. 12, 2018	GEMC 6351
Horn Antenna 18 – 26.5 GHz	SAS-572	A.H. Systems	Oct. 11, 2016	Oct. 11, 2018	GEMC 6371
Pre-Amp 9 kHz – 1 GHz	CPA9231A	Chase	Oct. 12, 2016	Oct. 12, 2018	GEMC 6403
Loop Antenna	EM 6871	Electro-Metrics	Feb. 13, 2017	Feb. 13, 2019	GEMC 70
Loop Antenna	EM 6872	Electro-Metrics	Feb. 13, 2017	Feb. 13, 2019	GEMC 71
BiLog Antenna	3142-C	ETS	Feb. 22, 2017	Feb. 22, 2019	GEMC 137
RF Cable 10m	LMR-400-10M-50Ω-MN-MN	LexTec	Feb. 20, 2017	Feb. 20, 2018	GEMC 274
RF Cable 2m	Sucoflex 104A	Huber+Suhner	Feb. 20, 2017	Feb. 20, 2018	GEMC 272
Emissions Software	0.1.94	TUV SUD Canada	NCR	NCR	GEMC 58

FCC - 15.209 -Radiated Emissions_Rev1

Client	Rehabtronics Inc.	 Canada
Product	StimRay	
Standard(s)	RSS-247 Issue 2:2017 FCC Part 15 Subpart 15.247:2015	

Power Spectral Density

Purpose

The purpose of this test is to ensure that the maximum power spectral density to the radiating element does not exceed the limits specified. This ensures that the modulation is significantly wide enough, or low enough in power that it will allow for co-operation of other wireless devices operating within this frequency allocation.

Limits and Method

The limits are defined in 15.247(e).

For digitally modulated systems, the power spectral density conducted from the intentional radiator to the antenna shall not be greater than 8 dBm in any 3 kHz band during any time interval of continuous transmission.

The method is given in Section 10.2 of FCC KDB 558074.

Results


The EUT passed. Low, medium, and high bands were tested. The worst case value is -2.55 dBm for Mid channel as measured with a 3 kHz resolution bandwidth (peak power).

Graphs

The graphs shown below show the power spectral density of the device during the conducted measurement operation of the EUT. Low, middle, and high channel was investigated in each mode, with the worst case being presented. The external attenuator and cable loss are accounted for as reference offset in the spectrum analyzer.

Client	Rehabtronics Inc.	 Canada
Product	StimRay	
Standard(s)	RSS-247 Issue 2:2017 FCC Part 15 Subpart 15.247:2015	


PSD - Low Channel

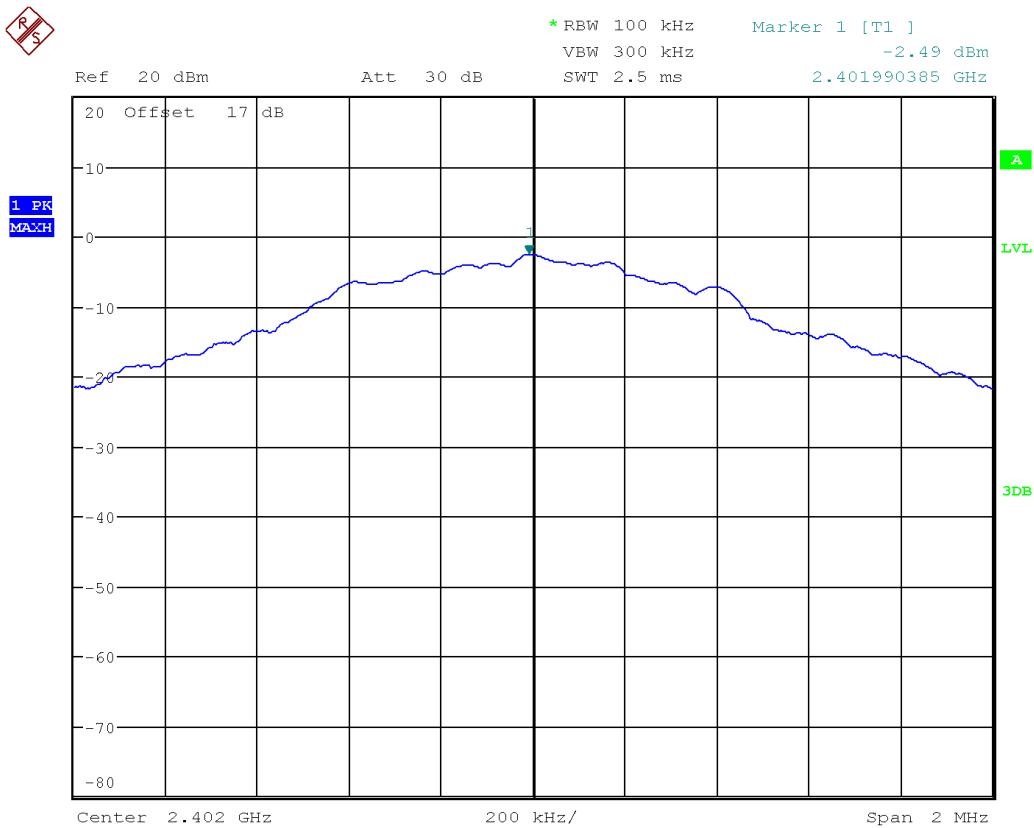

Date: 18.SEP.2017 11:48:51

Client	Rehabtronics Inc.	 Canada
Product	StimRay	
Standard(s)	RSS-247 Issue 2:2017 FCC Part 15 Subpart 15.247:2015	


PSD - Mid Channel

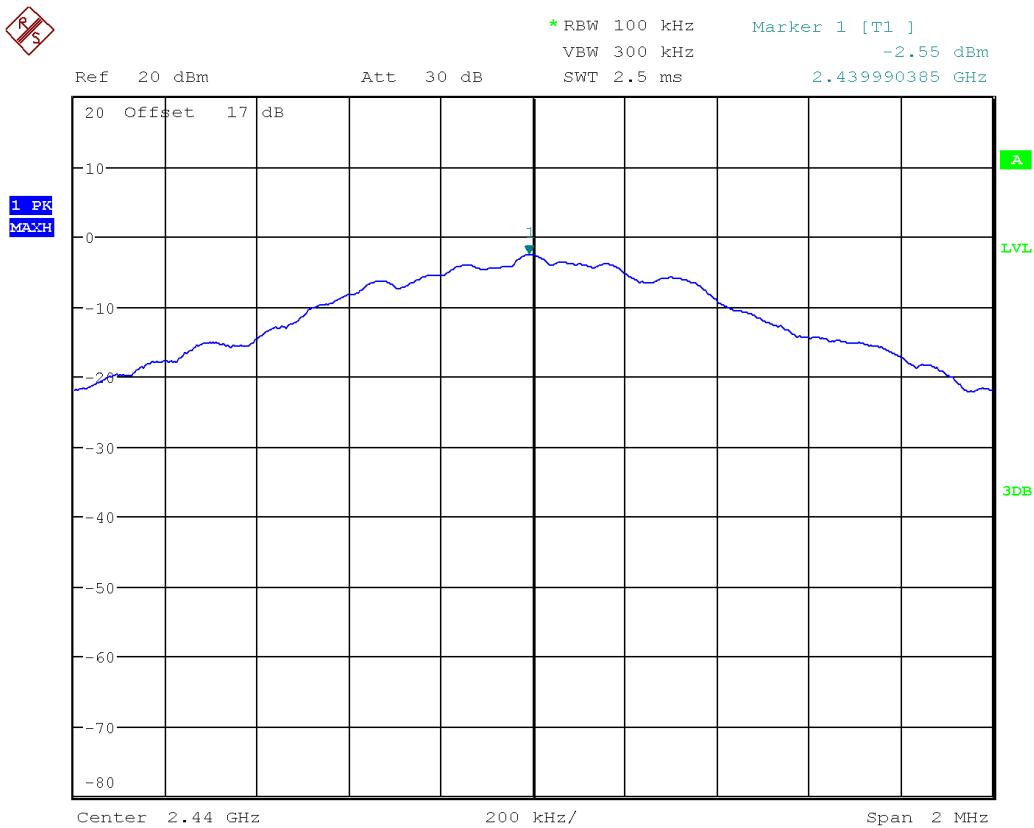

Date: 18.SEP.2017 11:46:31

Client	Rehabtronics Inc.	 Canada
Product	StimRay	
Standard(s)	RSS-247 Issue 2:2017 FCC Part 15 Subpart 15.247:2015	

PSD - Hi Channel

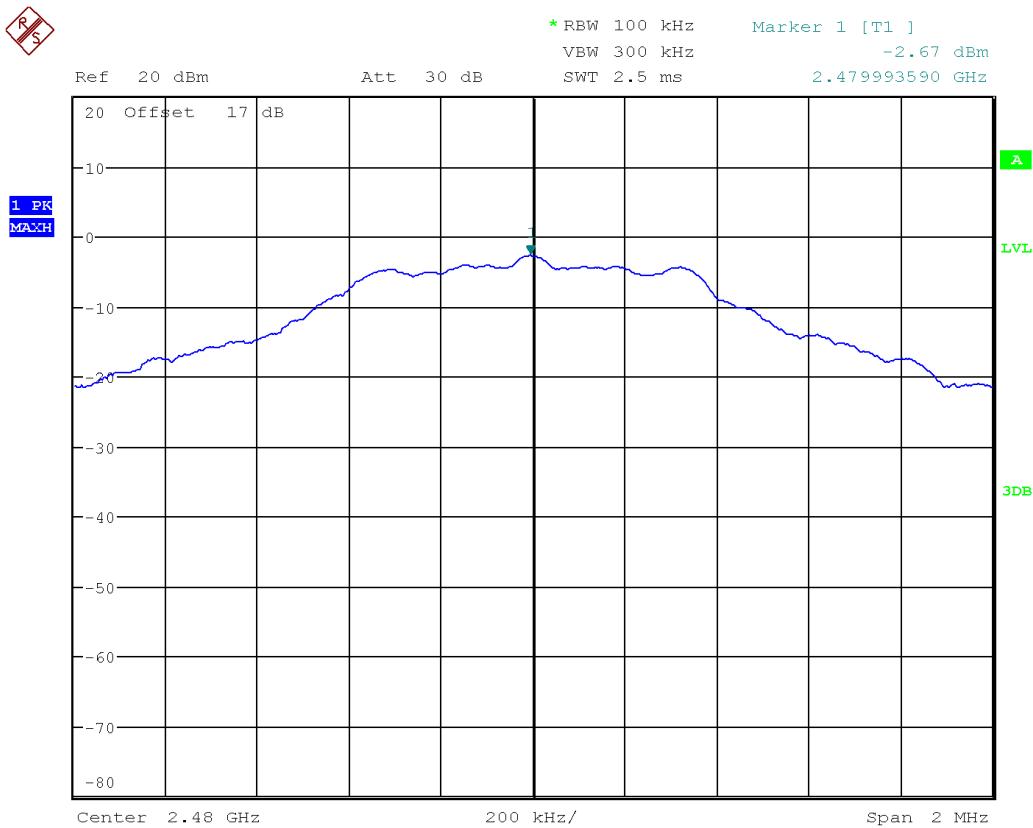

Date: 18.SEP.2017 11:51:05

See 'Appendix B – EUT and Test Setup Photos' for photos showing the test set-up.

Client	Rehabtronics Inc.	 Canada
Product	StimRay	
Standard(s)	RSS-247 Issue 2:2017 FCC Part 15 Subpart 15.247:2015	

Test Equipment List

Equipment	Model No.	Manufacturer	Last Calibration / Verification Date	Next Calibration / Verification Date	Asset #
Spectrum Analyzer	FSU 26	Rohde & Schwarz	Feb. 15, 2017	Feb. 15, 2019	GEMC 232
Attenuator 10 dB	8493B	Agilent	Feb. 20, 2017	Feb. 20, 2018	GEMC 133
Attenuator 6 dB	3M-6	Weinschel	Feb. 20, 2017	Feb. 20, 2018	GEMC 278

Client	Rehabtronics Inc.	 Canada
Product	StimRay	
Standard(s)	RSS-247 Issue 2:2017 FCC Part 15 Subpart 15.247:2015	

Power Line Conducted Emissions

Purpose

The purpose of this test is to ensure that the RF energy unintentionally emitted from the EUT's power line does not exceed the limits listed below as defined in the applicable test standard, as measured from a LISN. This helps protect lower frequency radio services such as AM radio, shortwave radio, amateur radio operators, maritime radio, CB radio, and so on, from unwanted interference.

Limits and Method

The limits are as defined in 47 CFR FCC Part 15 Section 15.207

Method is as defined in ANSI C63.4

Average Limits		Quasi-Peak Limits	
150 kHz – 500 kHz	56 to 46* dB μ V	150 kHz – 500 kHz	66 to 56* dB μ V
500 kHz – 5 MHz	46 dB μ V	500 kHz – 5 MHz	56 dB μ V
5 MHz – 30 MHz	50 dB μ V	5 MHz – 30 MHz	60 dB μ V


* Decreases linearly with the logarithm of the frequency

Both Quasi-Peak and Average limits are applicable and each is specified as being measured with a resolution bandwidth of 9 kHz. For Quasi-Peak, a video bandwidth at least three times greater than the resolution bandwidth is used.

Based on ANSI C63.4 Section 4.2, if the Peak or Quasi-Peak detector measurements do not exceed the Average limits, then the EUT is deemed to have passed the requirements.

Client	Rehabtronics Inc.	 Canada
Product	StimRay	
Standard(s)	RSS-247 Issue 2:2017 FCC Part 15 Subpart 15.247:2015	

Typical Setup Diagram

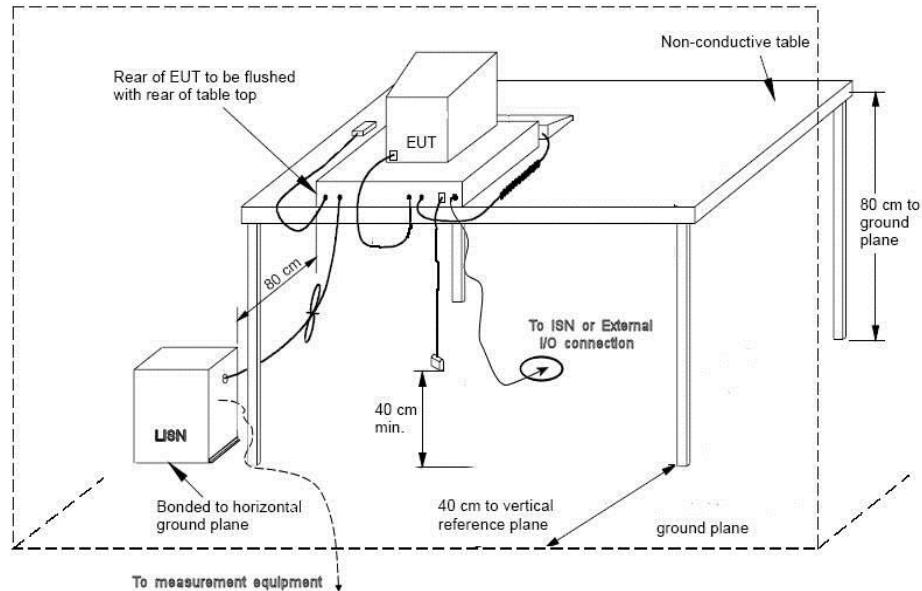

Measurement Uncertainty


The expanded measurement uncertainty is calculated in accordance with CISPR 16-4-2 and is $\pm 2.91\text{dB}$ with a 'k=2' coverage factor and a 95% confidence level.

Preliminary Graphs

The graphs shown below are maximized peak measurement graphs measured with a resolution bandwidth greater than or equal to the final required detector. This peaking process is done as a worst case measurement and enables the detection of frequencies of concern for final measurement. For final measurements with the appropriate detector, where applicable, please refer to the tables under Final Measurements.

Client	Rehabtronics Inc.	 Canada
Product	StimRay	
Standard(s)	RSS-247 Issue 2:2017 FCC Part 15 Subpart 15.247:2015	


Line 1 (L1) – 120Vac 60Hz
Peak

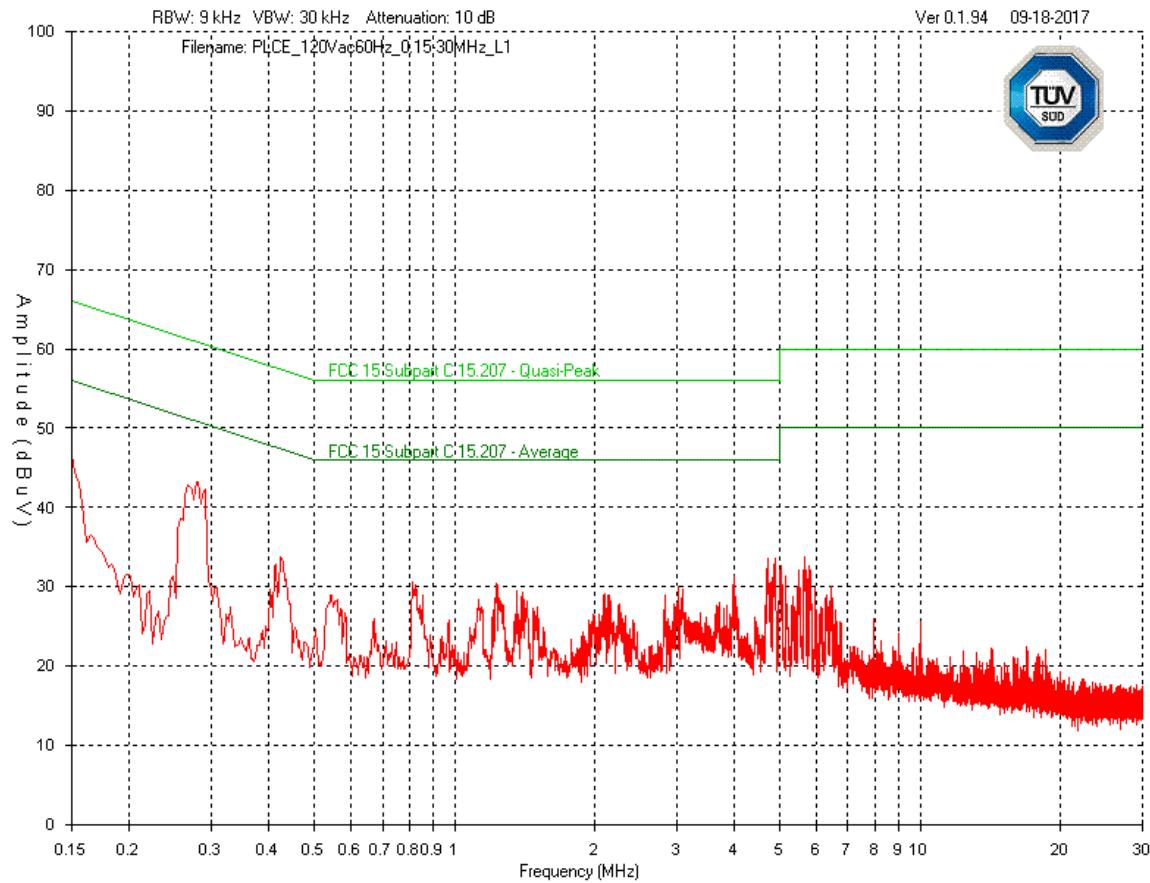

Client	Rehabtronics Inc.
Product	StimRay
Standard(s)	RSS-247 Issue 2:2017 FCC Part 15 Subpart 15.247:2015



Line 2 (L2) – 120Vac 60Hz
Peak

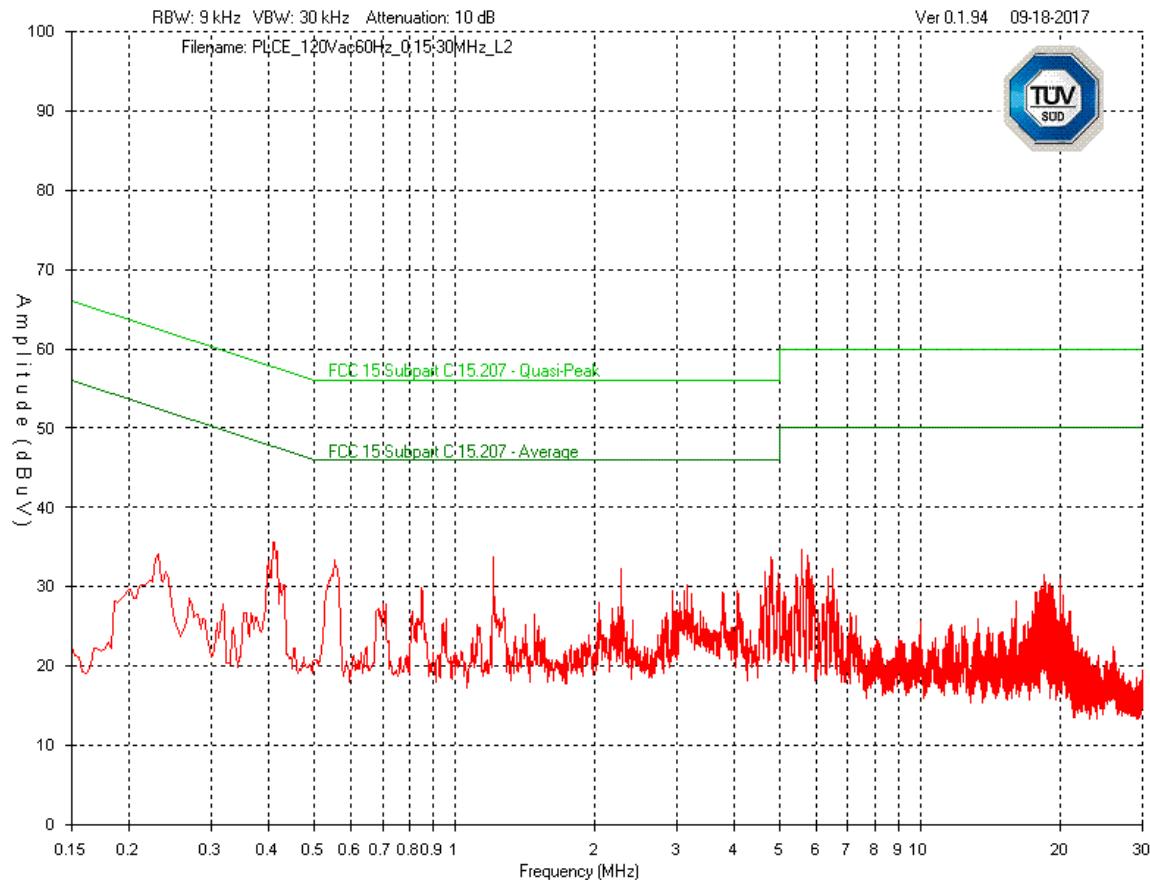

Client	Rehabtronics Inc.	 Canada
Product	StimRay	
Standard(s)	RSS-247 Issue 2:2017 FCC Part 15 Subpart 15.247:2015	

Final Measurements

Quasi-Peak Emissions Table

Supply			120Vac 60Hz						
Frequency (MHz)	Detector Peak/QP/ AVG	Received Signal (dB μ V)	Atten Factor (dB)	Cable Factor (dB)	LISN Factor (dB)	Level (dB μ V)	QP Limit (dB μ V)	QP Margin (dB)	Pass/ Fail
Line 1									
0.2786	Peak	33.1	10.0	0.1	0.1	43.3	60.9	17.6	Pass
0.1530	Peak	34.3	10.0	0.0	0.2	44.5	65.8	21.3	Pass
4.8787	Peak	23.4	10.0	0.1	0.1	33.6	56.0	22.4	Pass
4.7023	Peak	23.3	10.0	0.1	0.1	33.5	56.0	22.5	Pass
0.4222	Peak	23.6	10.0	0.1	0.1	33.8	57.4	23.6	Pass
3.9755	Peak	21.1	10.0	0.1	0.1	31.3	56.0	24.7	Pass
Line 2									
0.4072	Peak	25.4	10.0	0.1	0.1	35.6	57.7	22.1	Pass
4.7830	Peak	23.6	10.0	0.1	0.1	33.8	56.0	22.2	Pass
1.2118	Peak	23.6	10.0	0.1	0.1	33.8	56.0	22.2	Pass
0.5508	Peak	23.1	10.0	0.1	0.1	33.3	56.0	22.7	Pass
2.2826	Peak	22.2	10.0	0.1	0.1	32.4	56.0	23.6	Pass
4.6335	Peak	21.7	10.0	0.1	0.1	31.9	56.0	24.1	Pass

Client	Rehabtronics Inc.	 Canada
Product	StimRay	
Standard(s)	RSS-247 Issue 2:2017 FCC Part 15 Subpart 15.247:2015	

Average Emissions Table

Supply			120Vac 60Hz						
Frequency (MHz)	Detector Peak/Avg	Received Signal (dB μ V)	Atten Factor (dB)	Cable Factor (dB)	LISN Factor (dB)	Level (dB μ V)	AVG Limit (dB μ V)	AVG Margin (dB)	Pass/Fail
Line 1									
0.2786	Peak	33.1	10.0	0.1	0.1	43.3	50.9	7.6	Pass
0.1530	Peak	34.3	10.0	0.0	0.2	44.5	55.8	11.3	Pass
4.8787	Peak	23.4	10.0	0.1	0.1	33.6	46.0	12.4	Pass
4.7023	Peak	23.3	10.0	0.1	0.1	33.5	46.0	12.5	Pass
0.4222	Peak	23.6	10.0	0.1	0.1	33.8	47.4	13.6	Pass
3.9755	Peak	21.1	10.0	0.1	0.1	31.3	46.0	14.7	Pass
Line 2									
0.4072	Peak	25.4	10.0	0.1	0.1	35.6	47.7	12.1	Pass
4.7830	Peak	23.6	10.0	0.1	0.1	33.8	46.0	12.2	Pass
1.2118	Peak	23.6	10.0	0.1	0.1	33.8	46.0	12.2	Pass
0.5508	Peak	23.1	10.0	0.1	0.1	33.3	46.0	12.7	Pass
2.2826	Peak	22.2	10.0	0.1	0.1	32.4	46.0	13.6	Pass
4.6335	Peak	21.7	10.0	0.1	0.1	31.9	46.0	14.1	Pass

Note:

Peak = Peak measurement

AVG = Average measurement

QP = Quasi-Peak measurement

See 'Appendix B – EUT, Peripherals and Test Setup Photos' for photos showing the test set-up for the highest line conducted emission

Client	Rehabtronics Inc.	 Canada
Product	StimRay	
Standard(s)	RSS-247 Issue 2:2017 FCC Part 15 Subpart 15.247:2015	

Test Equipment List

Equipment	Model No.	Manufacturer	Last Calibration / Verification Date	Next Calibration / Verification Date	Asset #
Spectrum Analyzer	ESL 6	Rohde & Schwarz	Nov. 25, 2015	Nov. 25, 2017	GEMC 160
LISN	FCC-LISN-50/250-16-2-01	FCC	Feb. 1, 2017	Feb. 1, 2019	GEMC 65
RF Cable 3m	LMR-400-3M-50Ω-MN-MN	LexTec	Feb 20, 2017	Feb 20, 2018	GEMC 276
Attenuator 10 dB	612-10-1	Meca Electronics, Inc	Feb 20, 2017	Feb 20, 2018	GEMC 223
Emissions Software	0.1.94	TUV SUD Canada	NCR	NCR	GEMC 58

FCC_ICES003_CE_Rev1

Client	Rehabtronics Inc.	
Product	StimRay	
Standard(s)	RSS-247 Issue 2:2017 FCC Part 15 Subpart 15.247:2015	 Canada

Appendix A – EUT Summary

Client	Rehabtronics Inc.	 Canada
Product	StimRay	
Standard(s)	RSS-247 Issue 2:2017 FCC Part 15 Subpart 15.247:2015	

General EUT Description

Client	
Organization / Address	Rehabtronics Inc., #4352, 10230 Jasper Avenue, Edmonton Alberta T5J 4P6
Phone	780 638 2520
EUT Details	
EUT Name	StimRay
EUT Model	CSST1 with charger and electrodes, system model RHTCS1
Equipment Category	Medical device, BLE
Basic EUT Functionality	The StimRay is a Muscle stimulator used for exercising different muscles groups on a body.
EUT is powered using	Lithium/Ion battery 3.7 V in normal use and 5V DC using USB charger while charging
Input Voltage and Frequency	5V DC using USB charger
Rated Input Current	2A while charging
Connectors available on EUT	One connector to fit both charger and the electrodes
Peripherals Required for Test	N/A
Intentional Radiator Frequency range	Operating between 2402 – 2480 MHz
EUT Configuration	Wireless configured to transmit at maximum possible duty cycle.

Note: The EUT is considered to have been received the date of the commencement of the first test, unless otherwise stated. For a close-up picture of the EUT, see 'Appendix B – EUT and Test Setup Photos'.

Client	Rehabtronics Inc.	
Product	StimRay	
Standard(s)	RSS-247 Issue 2:2017 FCC Part 15 Subpart 15.247:2015	 Canada

Appendix B – EUT and Test Setup Photos

Refer to the files separate from this test report.