



Appendix D

Photographs

1. SAR measurement System
2. Photographs of Tissue Simulate Liquid
3. Photographs of EUT test position
4. EUT Constructional Details

1. SAR measurement System



2. Photographs of Tissue Simulate Liquid

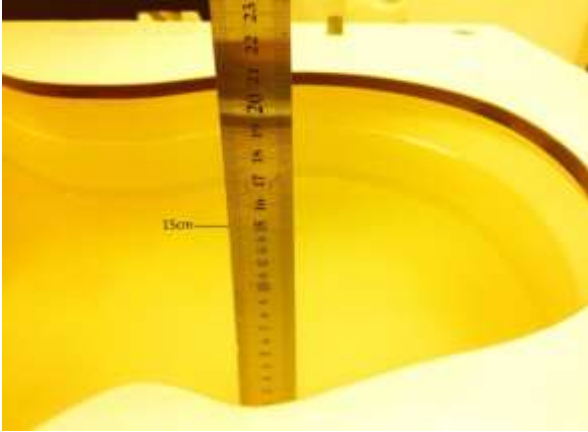
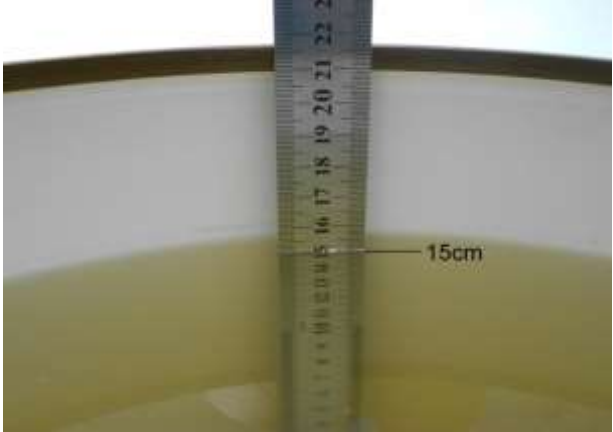
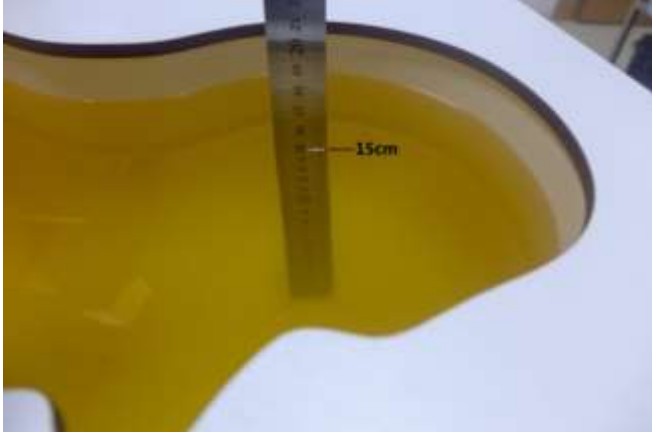
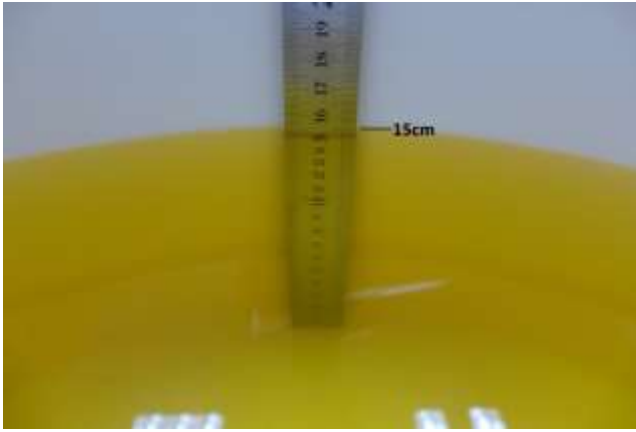
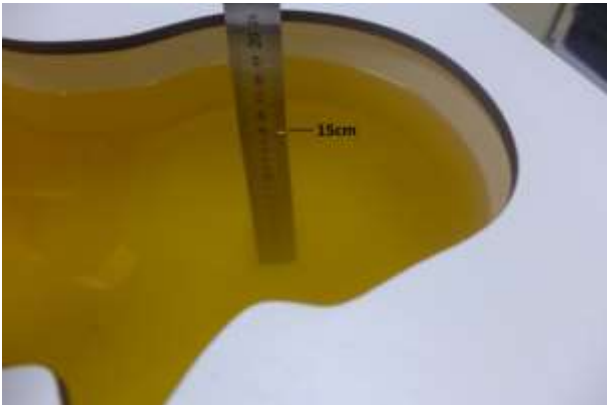
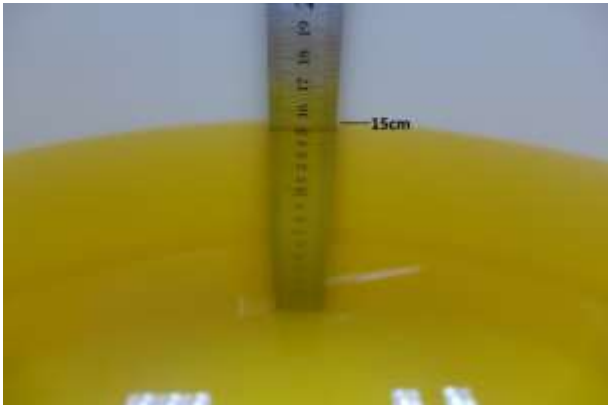
<p>Photo 1: Tissue Simulant Liquid for Head 835</p>	<p>Photo 2: Tissue Simulant Liquid for Head 835</p>
	
<p>Photo 3: Tissue Simulant Liquid for Head 1750</p>	<p>Photo 4: Tissue Simulant Liquid for Body 1750</p>
	
<p>Photo 5: Tissue Simulant Liquid for Head 1900</p>	<p>Photo 6: Tissue Simulant Liquid for Body 1900</p>
	

Photo 7: Tissue Simulant Liquid for Head 2450

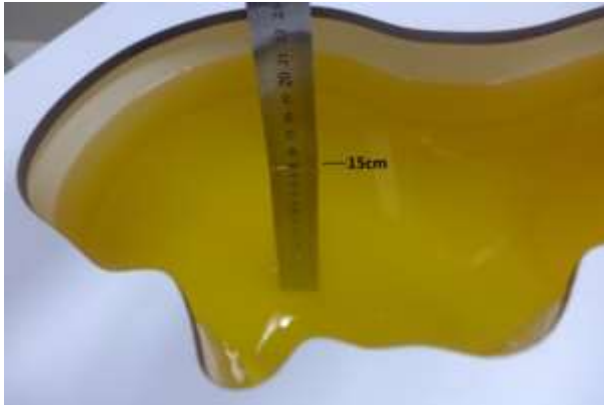


Photo 8: Tissue Simulant Liquid for Body 2450

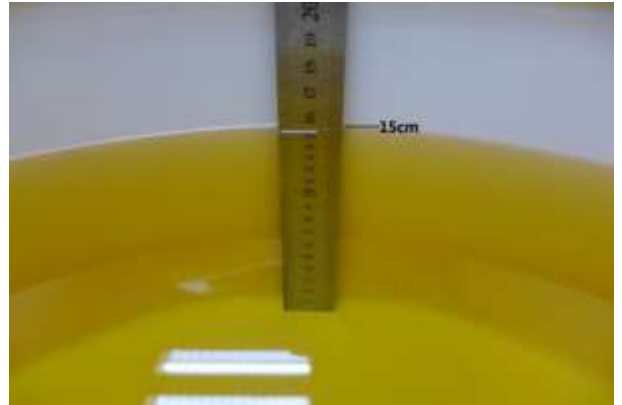


Photo 9: Tissue Simulant Liquid for Head 2600

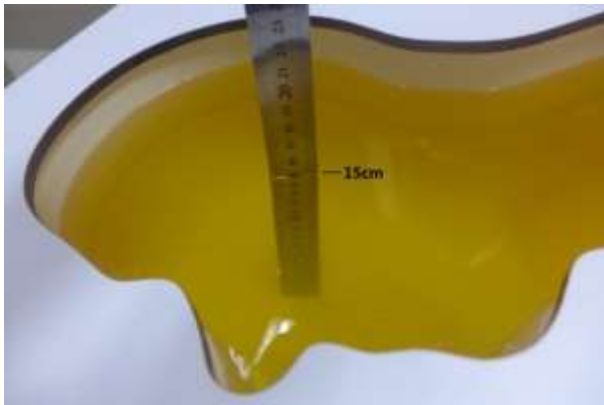
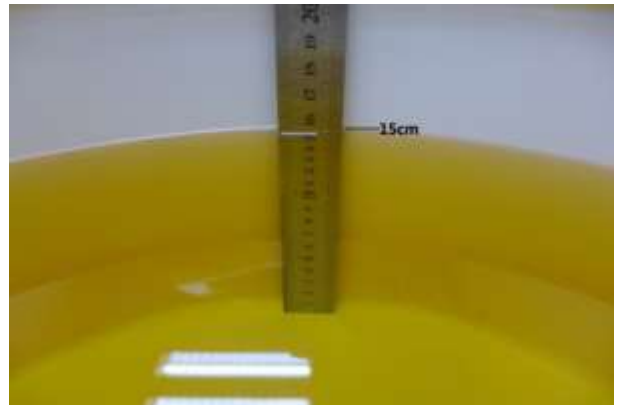
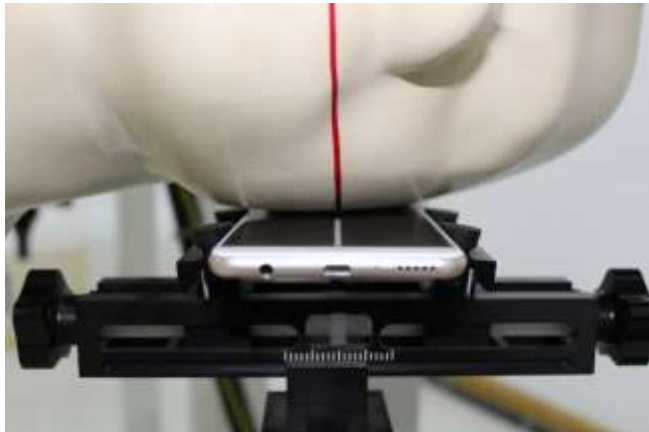


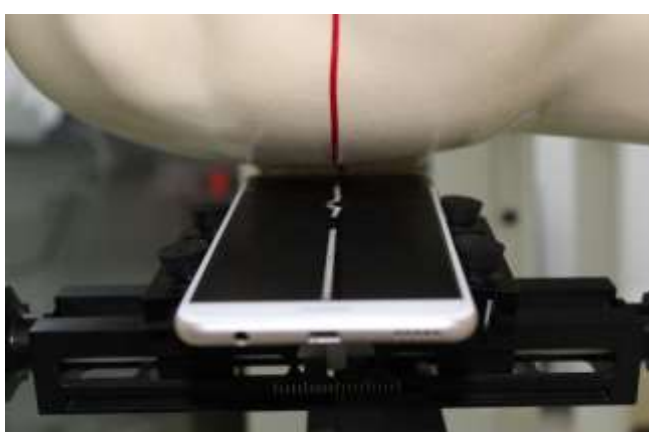















Photo 10: Tissue Simulant Liquid for Body 2600



3. Photographs of EUT test position

<p>Photo 11: Left touch cheek</p>	<p>Photo 12: Left tilted 15 degree</p>
	
<p>Photo 13: Right touch cheek</p>	<p>Photo 14: Right tilted 15 degree</p>
	
<p>Photo 15: Front side 10mm</p>	<p>Photo 16: Back side 10mm</p>
	

<p>Photo 17: Left side 10mm</p>	<p>Photo 18: Right side 10mm</p>
	
<p>Photo 19: Top side 10mm</p>	<p>Photo 20: Bottom side 10mm</p>
	
<p>Photo 21: Front Side 0mm</p>	<p>Photo 22: Back Side 0mm</p>
	

<p>Photo 23: Bottom Side 0mm</p>	<p>Photo 24: Back Side 15mm</p>
	
<p>Photo 25: Front Side 15mm</p>	<p>Photo 26: Back Side 16mm</p>
	
<p>Photo 27: Front Side 12mm</p>	<p>NA</p>
	<p>NA</p>

4. EUT Constructional Details

