



# element

**BIOTRONIK, Inc.**

**Neuro SCS IPG**

**FCC 15.209:2021**

**Inductive**

**Report: BIOT0080.1 Rev. 1, Issue Date: October 14, 2021**



NVLAP LAB CODE: 200630-0



*This report must not be used to claim product certification, approval, or endorsement by NVLAP, NIST, or any agency of the U.S. Government. This Report shall not be reproduced, except in full without written approval of the laboratory.*

*EAR-Controlled Data - This document contains technical data whose export and reexport/retransfer is subject to control by the U.S. Department of Commerce under the Export Administration Act and the Export Administration Regulations. The Department of Commerce's prior written approval may be required for the export or re-export/retransfer of such technical data to any foreign person, foreign entity or foreign organization whether in the United States or abroad.*

# CERTIFICATE OF TEST

Last Date of Test: January 20, 2021

BIOTRONIK, Inc.

EUT: Neuro SCS IPG

## Radio Equipment Testing

### Standards

| Specification   | Method           |
|-----------------|------------------|
| FCC 15.209:2021 | ANSI C63.10:2013 |

### Results

| Method Clause | Test Description              | Applied | Results | Comments                                |
|---------------|-------------------------------|---------|---------|-----------------------------------------|
| 6.2           | Powerline Conducted Emissions | No      | N/A     | Not required for a battery powered EUT. |
| 6.4           | Field Strength of Fundamental | Yes     | Pass    |                                         |
| 6.4, 6.5      | Spurious Radiated Emissions   | Yes     | Pass    |                                         |

### Deviations From Test Standards

None

### Approved By:



Kyle Holgate, Operations Manager

*Product compliance is the responsibility of the client; therefore, the tests and equipment modes of operation represented in this report were agreed upon by the client, prior to testing. The results of this test pertain only to the sample(s) tested. The specific description is noted in each of the individual sections of the test report supporting this certificate of test. This report reflects only those tests from the referenced standards shown in the certificate of test. It does not include inspection or verification of labels, identification, marking or user information. As indicated in the Statement of Work sent with the quotation, Element's standard process is to always use the latest published version of the test methods even when earlier versions are cited in the test specification. Issuance of a purchase order was de facto acceptance of this approach. Otherwise, the client would have advised Element in writing of the specific version of the test methods they wanted applied to the subject testing.*

# REVISION HISTORY



| Revision Number | Description                                          | Date<br>(yyyy-mm-dd) | Page Number |
|-----------------|------------------------------------------------------|----------------------|-------------|
| 01              | Updated power settings to inductive radio.           | 2021-10-14           | 8           |
|                 | Removed 10m data from Field Strength of Fundamental. | 2021-10-14           | 14          |

# ACCREDITATIONS AND AUTHORIZATIONS



---

## United States

**FCC** - Designated by the FCC as a Telecommunications Certification Body (TCB). Certification chambers, Open Area Test Sites, and conducted measurement facilities are listed with the FCC.

**A2LA** - Accredited by A2LA to ISO / IEC 17065 as a product certifier. This allows Element to certify transmitters to FCC and IC specifications.

**NVLAP** - Each laboratory is accredited by NVLAP to ISO 17025

---

## Canada

**ISED** - Recognized by Innovation, Science and Economic Development Canada as a Certification Body (CB) and as a CAB for the acceptance of test data.

---

## European Union

**European Commission** – Within Element, we have a EU Notified Body validated for the EMCD and RED Directives.

---

## Australia/New Zealand

**ACMA** - Recognized by ACMA as a CAB for the acceptance of test data.

---

## Korea

**MSIT / RRA** - Recognized by KCC's RRA as a CAB for the acceptance of test data.

---

## Japan

**VCCI** - Associate Member of the VCCI. Conducted and radiated measurement facilities are registered.

---

## Taiwan

**BSMI** – Recognized by BSMI as a CAB for the acceptance of test data.

**NCC** - Recognized by NCC as a CAB for the acceptance of test data.

---

## Singapore

**IDA** – Recognized by IDA as a CAB for the acceptance of test data.

---

## Israel

**MOC** – Recognized by MOC as a CAB for the acceptance of test data.

---

## Hong Kong

**OFCA** – Recognized by OFCA as a CAB for the acceptance of test data.

---

## Vietnam

**MIC** – Recognized by MIC as a CAB for the acceptance of test data.

---

## SCOPE

For details on the Scopes of our Accreditations, please visit:

<https://www.nwemc.com/emc-testing-accreditations>

# FACILITIES



|                                                                                       |                                                                                                       |                                                                                                       |                                                                                        |                                                                                                           |
|---------------------------------------------------------------------------------------|-------------------------------------------------------------------------------------------------------|-------------------------------------------------------------------------------------------------------|----------------------------------------------------------------------------------------|-----------------------------------------------------------------------------------------------------------|
| <b>California</b><br>Labs OC01-17<br>41 Tesla<br>Irvine, CA 92618<br>(949) 861-8918   | <b>Minnesota</b><br>Labs MN01-11<br>9349 W Broadway Ave.<br>Brooklyn Park, MN 55445<br>(612)-638-5136 | <b>Oregon</b><br>Labs EV01-12<br>6775 NE Evergreen Pkwy #400<br>Hillsboro, OR 97124<br>(503) 844-4066 | <b>Texas</b><br>Labs TX01-09<br>3801 E Plano Pkwy<br>Plano, TX 75074<br>(469) 304-5255 | <b>Washington</b><br>Labs NC01-05<br>19201 120 <sup>th</sup> Ave NE<br>Bothell, WA 98011<br>(425)984-6600 |
| <b>NVLAP</b>                                                                          |                                                                                                       |                                                                                                       |                                                                                        |                                                                                                           |
| NVLAP Lab Code: 200676-0                                                              | NVLAP Lab Code: 200881-0                                                                              | NVLAP Lab Code: 200630-0                                                                              | NVLAP Lab Code:201049-0                                                                | NVLAP Lab Code: 200629-0                                                                                  |
| <b>Innovation, Science and Economic Development Canada</b>                            |                                                                                                       |                                                                                                       |                                                                                        |                                                                                                           |
| 2834B-1, 2834B-3                                                                      | 2834E-1, 2834E-3                                                                                      | 2834D-1                                                                                               | 2834G-1                                                                                | 2834F-1                                                                                                   |
| <b>BSMI</b>                                                                           |                                                                                                       |                                                                                                       |                                                                                        |                                                                                                           |
| SL2-IN-E-1154R                                                                        | SL2-IN-E-1152R                                                                                        | SL2-IN-E-1017                                                                                         | SL2-IN-E-1158R                                                                         | SL2-IN-E-1153R                                                                                            |
| <b>VCCI</b>                                                                           |                                                                                                       |                                                                                                       |                                                                                        |                                                                                                           |
| A-0029                                                                                | A-0109                                                                                                | A-0108                                                                                                | A-0201                                                                                 | A-0110                                                                                                    |
| <b>Recognized Phase I CAB for ISED, ACMA, BSMI, IDA, KCC/RRA, MIC, MOC, NCC, OFCA</b> |                                                                                                       |                                                                                                       |                                                                                        |                                                                                                           |
| US0158                                                                                | US0175                                                                                                | US0017                                                                                                | US0191                                                                                 | US0157                                                                                                    |



# MEASUREMENT UNCERTAINTY

## Measurement Uncertainty

When a measurement is made, the result will be different from the true or theoretically correct value. The difference is the result of tolerances in the measurement system that cannot be completely eliminated. To the extent that technology allows us, it has been our aim to minimize this error. Measurement uncertainty is a statistical expression of measurement error qualified by a probability distribution.


A measurement uncertainty estimation has been performed for each test per our internal quality document QM205.4.6. The estimation is used to compare the measured result with its "true" or theoretically correct value. The expanded measurement uncertainty (K=2) can be found included as part of the applicable test description page. Our measurement data meets or exceeds the measurement uncertainty requirements of the applicable specification; therefore, the test data can be compared directly to the specification limit to determine compliance. The calculations for estimating measurement uncertainty are based upon ETSI TR 100 028 (or CISPR 16-4-2 as applicable), and are available upon request.

The following table represents the Measurement Uncertainty (MU) budgets for each of the tests that may be contained in this report.


| Test                                  | + MU    | - MU     |
|---------------------------------------|---------|----------|
| Frequency Accuracy                    | 0.0007% | -0.0007% |
| Amplitude Accuracy (dB)               | 1.2 dB  | -1.2 dB  |
| Conducted Power (dB)                  | 1.2 dB  | -1.2 dB  |
| Radiated Power via Substitution (dB)  | 0.7 dB  | -0.7 dB  |
| Temperature (degrees C)               | 0.7°C   | -0.7°C   |
| Humidity (% RH)                       | 2.5% RH | -2.5% RH |
| Voltage (AC)                          | 1.0%    | -1.0%    |
| Voltage (DC)                          | 0.7%    | -0.7%    |
| Field Strength (dB)                   | 5.2 dB  | -5.2 dB  |
| AC Powerline Conducted Emissions (dB) | 2.6 dB  | -2.6 dB  |

# Test Setup Block Diagrams


## Antenna Port Conducted Measurements

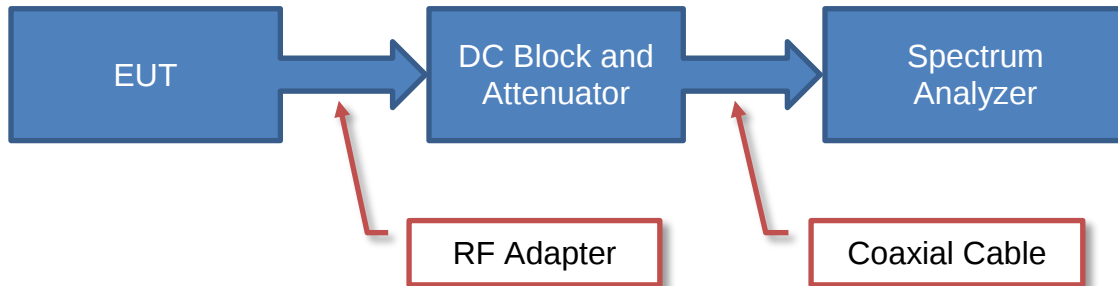

## Near Field Test Fixture Measurements

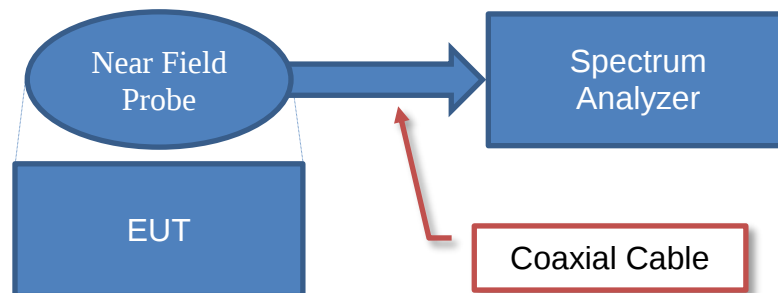

## Spurious Radiated Emissions

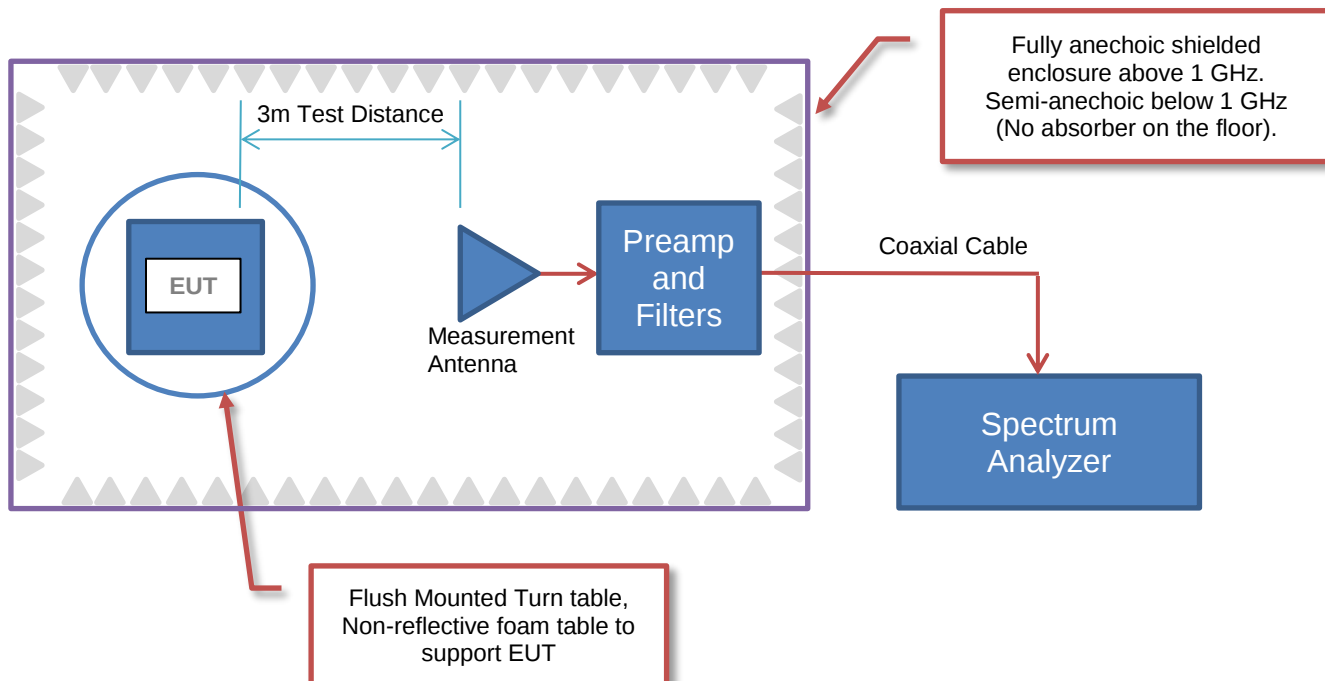

# POWER SETTINGS AND ANTENNAS



The power settings, antenna gain value(s) and cable loss (if applicable) used for the testing contained in this report were provided by the customer and will affect the validity of the results. Element assumes no responsibility for the accuracy of this information.

## ANTENNA GAIN (dBi)

| Type                          | Provided by: | Frequency Range (MHz) | Gain (dBi) |
|-------------------------------|--------------|-----------------------|------------|
| 3mm Diameter coil, 1600 turns | Manufacturer | Inductive Radio       | N/A        |

No adjustable power settings were provided. The EUT was tested using power settings pre-defined by the manufacturer.

# PRODUCT DESCRIPTION



## Client and Equipment Under Test (EUT) Information

|                          |                        |
|--------------------------|------------------------|
| Company Name:            | BIOTRONIK, Inc.        |
| Address:                 | 6024 Jean Road, BLDG B |
| City, State, Zip:        | Lake Oswego, OR 97035  |
| Test Requested By:       | Roy Wang               |
| EUT:                     | Neuro SCS IPG          |
| First Date of Test:      | January 19, 2021       |
| Last Date of Test:       | January 20, 2021       |
| Receipt Date of Samples: | January 18, 2021       |
| Equipment Design Stage:  | Production             |
| Equipment Condition:     | No Damage              |
| Purchase Authorization:  | Verified               |

## Information Provided by the Party Requesting the Test

|                                                                                                     |
|-----------------------------------------------------------------------------------------------------|
| <b>Functional Description of the EUT:</b>                                                           |
| Implantable Neurostimulator                                                                         |
| <b>Testing Objective:</b>                                                                           |
| To demonstrate compliance of the inductive portion of the device to FCC Part 15.209 specifications. |

# CONFIGURATIONS



## Configuration BIOT0080- 1

| Software/Firmware Running during test |         |
|---------------------------------------|---------|
| Description                           | Version |
| SCS ROM                               | 2.1     |

| EUT                         |                 |                   |               |
|-----------------------------|-----------------|-------------------|---------------|
| Description                 | Manufacturer    | Model/Part Number | Serial Number |
| Implantable Neurostimulator | BIOTRONIK, Inc. | Prospera          | 88200467      |

# MODIFICATIONS



## Equipment Modifications

| Item | Date       | Test                          | Modification                         | Note                                                                | Disposition of EUT                          |
|------|------------|-------------------------------|--------------------------------------|---------------------------------------------------------------------|---------------------------------------------|
| 1    | 2021-01-19 | Field Strength of Fundamental | Tested as delivered to Test Station. | No EMI suppression devices were added or modified during this test. | EUT remained at Element following the test. |
| 2    | 2021-01-20 | Spurious Radiated Emissions   | Tested as delivered to Test Station. | No EMI suppression devices were added or modified during this test. | Scheduled testing was completed.            |

# FIELD STRENGTH OF FUNDAMENTAL



PSA-ESCI 2020.12.30.0

Testing was performed using the mode(s) of operation and configuration(s) noted within the report. The individuals and/or the organization requesting the test provided the modes, configurations and settings used to complete the evaluation. The actual test parameters are specified in the test data, this includes items such as investigated frequency range (scanned) and test levels. The testing methods and performance specifications, as well as the test site used for the evaluation are indicated in the test data. The test data represents the configuration / operating mode/ model that produced the highest emission levels as compared to the specification limit.

## MODES OF OPERATION

Continuous transmit inductive, 32kHz

## POWER SETTINGS INVESTIGATED

Battery

## CONFIGURATIONS INVESTIGATED

BIOT0080 - 1

## FREQUENCY RANGE INVESTIGATED

|                 |       |                |        |
|-----------------|-------|----------------|--------|
| Start Frequency | 9 kHz | Stop Frequency | 30 MHz |
|-----------------|-------|----------------|--------|

## SAMPLE CALCULATIONS

Radiated Emissions: Field Strength = Measured Level + Antenna Factor + Cable Factor - Amplifier Gain + Distance Adjustment Factor + External Attenuation

## TEST EQUIPMENT

| Description                  | Manufacturer | Model                  | ID  | Last Cal.  | Cal. Due  |
|------------------------------|--------------|------------------------|-----|------------|-----------|
| Cable                        | None         | 3m Test Distance Cable | EVM | 2020-02-28 | 2/28/2021 |
| Antenna - Loop               | EMCO         | 6502                   | AOA | 2020-07-06 | 7/6/2022  |
| Analyzer - Spectrum Analyzer | Agilent      | E4443A                 | AFB | 2020-06-26 | 6/26/2021 |

## MEASUREMENT BANDWIDTHS

| Frequency Range (MHz) | Peak Data (kHz) | Quasi-Peak Data (kHz) | Average Data (kHz) |
|-----------------------|-----------------|-----------------------|--------------------|
| 0.01 - 0.15           | 1.0             | 0.2                   | 0.2                |
| 0.15 - 30.0           | 10.0            | 9.0                   | 9.0                |
| 30.0 - 1000           | 100.0           | 120.0                 | 120.0              |
| Above 1000            | 1000.0          | N/A                   | 1000.0             |

## TEST DESCRIPTION

The antennas to be used with the EUT were tested. The EUT was continuously transmitting while set to the channel specified.

The fundamental carrier of the EUT was maximized by rotating the EUT on a turntable, adjusting the position of the EUT and EUT antenna in three orthogonal axis, and adjusting the measurement antenna polarization (per ANSI C63.10). A calibrated active loop antenna was used for this test in order to provide sufficient measurement sensitivity. The reference point of the loop antenna was maintained at 1m above the ground plane during the testing.

Measurements were made with the required detectors and annotated on the data for each individual point using the following annotation:

QP = Quasi-Peak Detector  
PK = Peak Detector  
AV = RMS Detector

As outlined in 15.209(e), 15.31(f)(2), and RSS-GEN, 6.5, measurements may be performed at a distance closer than what is specified with the limit. The limit at the specified distance is shown on the data sheet. Measurements are made at a closer distance and the data is adjusted using a distance correction factor of 40dB/decade for comparison to the limit.

# FIELD STRENGTH OF FUNDAMENTAL




EmiRS 2020.12.09.0 PSA-ESCI 2020.12.30.0

|                                                                                          |          |                   |            |                          |
|------------------------------------------------------------------------------------------|----------|-------------------|------------|--------------------------|
| Work Order:                                                                              | BIOT0080 | Date:             | 2021-01-19 |                          |
| Project:                                                                                 | None     | Temperature:      | 23.9 °C    |                          |
| Job Site:                                                                                | EV11     | Humidity:         | 30% RH     |                          |
| Serial Number:                                                                           | 88200467 | Barometric Pres.: | 1031 mbar  |                          |
| EUT: Neuro SCS IPG                                                                       |          |                   |            | Tested by: Cole Ghizzone |
| Configuration: 1                                                                         |          |                   |            |                          |
| Customer: BIOTRONIK, Inc.                                                                |          |                   |            |                          |
| Attendees: Roy Wang                                                                      |          |                   |            |                          |
| EUT Power: Battery                                                                       |          |                   |            |                          |
| Operating Mode: Continuous transmit inductive, 32kHz                                     |          |                   |            |                          |
| Deviations: None                                                                         |          |                   |            |                          |
| Comments: See data comments for EUT orientation. EUT leads terminated in distilled water |          |                   |            |                          |

|                     |                  |
|---------------------|------------------|
| Test Specifications | Test Method      |
| FCC 15.209:2021     | ANSI C63.10:2013 |

|       |   |                   |   |                   |       |         |      |
|-------|---|-------------------|---|-------------------|-------|---------|------|
| Run # | 2 | Test Distance (m) | 1 | Antenna Height(s) | 1 (m) | Results | Pass |
|-------|---|-------------------|---|-------------------|-------|---------|------|

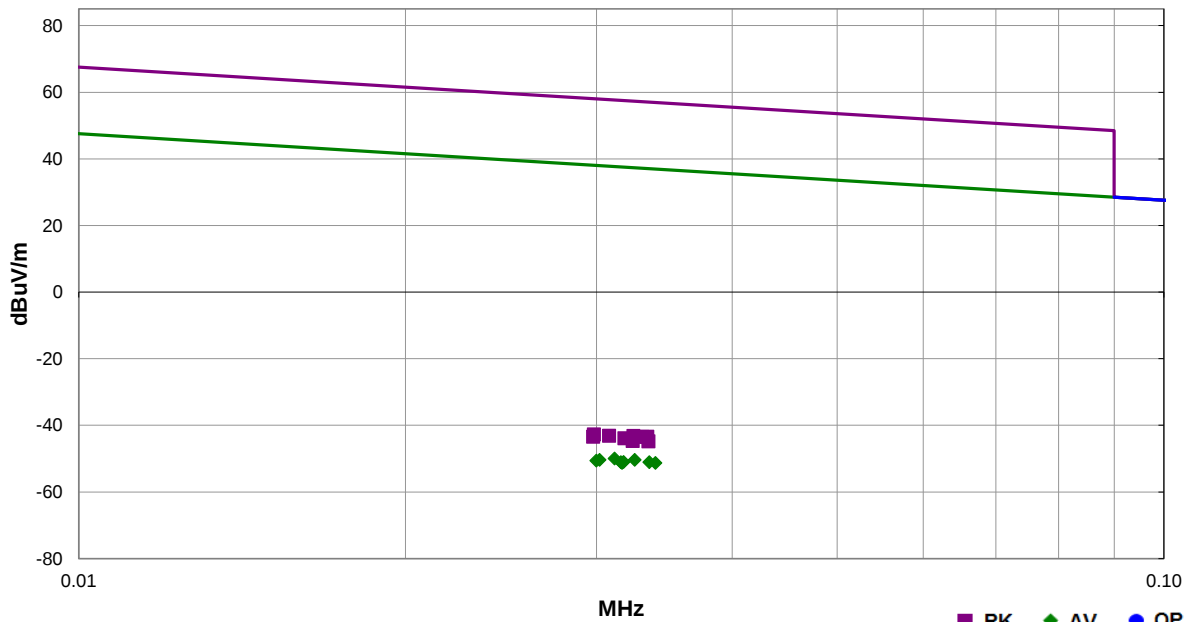

| Freq (MHz) | Amplitude (dBuV) | Factor (dB) | Antenna Height (meters) | Azimuth (degrees) | Test Distance (meters) | External Attenuation (dB) | Polarity/ Transducer Type | Detector | Distance Adjustment (dB) | Adjusted (dBuV/m) | Spec. Limit (dBuV/m) | Compared to Spec. (dB) | Comments       |
|------------|------------------|-------------|-------------------------|-------------------|------------------------|---------------------------|---------------------------|----------|--------------------------|-------------------|----------------------|------------------------|----------------|
| 0.033      | 34.9             | 13.8        | 1.0                     | 358.0             | 1.0                    | 0.0                       | Perp EUT                  | AV       | -99.1                    | -50.4             | 37.3                 | -87.7                  | EUT Horizontal |
| 0.031      | 35.1             | 14.0        | 1.0                     | 222.0             | 1.0                    | 0.0                       | Para EUT                  | AV       | -99.1                    | -50.0             | 37.7                 | -87.7                  | EUT Vertical   |
| 0.034      | 34.3             | 13.7        | 1.0                     | 27.0              | 1.0                    | 0.0                       | Para Floor                | AV       | -99.1                    | -51.1             | 37.1                 | -88.2                  | EUT Horizontal |
| 0.034      | 34.2             | 13.6        | 1.0                     | 197.0             | 1.0                    | 0.0                       | Perp EUT                  | AV       | -99.1                    | -51.3             | 37.0                 | -88.3                  | EUT On Side    |
| 0.030      | 34.6             | 14.1        | 1.0                     | 350.0             | 1.0                    | 0.0                       | Para Floor                | AV       | -99.1                    | -50.4             | 38.0                 | -88.4                  | EUT On Side    |
| 0.032      | 34.2             | 13.9        | 1.0                     | 31.0              | 1.0                    | 0.0                       | Para EUT                  | AV       | -99.1                    | -51.0             | 37.5                 | -88.5                  | EUT On Side    |
| 0.030      | 34.4             | 14.1        | 1.0                     | 310.0             | 1.0                    | 0.0                       | Para Floor                | AV       | -99.1                    | -50.6             | 38.0                 | -88.6                  | EUT Vertical   |
| 0.032      | 34.1             | 13.9        | 1.0                     | 349.0             | 1.0                    | 0.0                       | Para EUT                  | AV       | -99.1                    | -51.1             | 37.6                 | -88.7                  | EUT Horizontal |
| 0.032      | 33.9             | 13.9        | 1.0                     | 47.0              | 1.0                    | 0.0                       | Perp EUT                  | AV       | -99.1                    | -51.3             | 37.6                 | -88.9                  | EUT Vertical   |
| 0.033      | 42.0             | 13.7        | 1.0                     | 47.0              | 1.0                    | 0.0                       | Perp EUT                  | PK       | -99.1                    | -43.4             | 57.1                 | -100.5                 | EUT Vertical   |
| 0.032      | 42.1             | 13.8        | 1.0                     | 222.0             | 1.0                    | 0.0                       | Para EUT                  | PK       | -99.1                    | -43.2             | 57.4                 | -100.6                 | EUT Vertical   |
| 0.033      | 41.9             | 13.7        | 1.0                     | 358.0             | 1.0                    | 0.0                       | Perp EUT                  | PK       | -99.1                    | -43.5             | 57.2                 | -100.7                 | EUT Horizontal |
| 0.030      | 42.3             | 14.1        | 1.0                     | 27.0              | 1.0                    | 0.0                       | Para Floor                | PK       | -99.1                    | -42.7             | 58.1                 | -100.8                 | EUT Horizontal |
| 0.031      | 42.0             | 14.0        | 1.0                     | 349.0             | 1.0                    | 0.0                       | Para EUT                  | PK       | -99.1                    | -43.1             | 57.8                 | -100.9                 | EUT Horizontal |
| 0.032      | 41.3             | 13.9        | 1.0                     | 197.0             | 1.0                    | 0.0                       | Perp EUT                  | PK       | -99.1                    | -43.9             | 57.5                 | -101.4                 | EUT On Side    |
| 0.030      | 41.6             | 14.1        | 1.0                     | 350.0             | 1.0                    | 0.0                       | Para Floor                | PK       | -99.1                    | -43.4             | 58.1                 | -101.5                 | EUT On Side    |
| 0.034      | 40.6             | 13.7        | 1.0                     | 310.0             | 1.0                    | 0.0                       | Para Floor                | PK       | -99.1                    | -44.8             | 57.1                 | -101.9                 | EUT Vertical   |
| 0.032      | 40.6             | 13.8        | 1.0                     | 31.0              | 1.0                    | 0.0                       | Para EUT                  | PK       | -99.1                    | -44.7             | 57.4                 | -102.1                 | EUT On Side    |

# SPURIOUS RADIATED EMISSIONS



PSA-ESCI 2020.12.30.0

Testing was performed using the mode(s) of operation and configuration(s) noted within the report. The individuals and/or the organization requesting the test provided the modes, configurations and settings used to complete the evaluation. The actual test parameters are specified in the test data, this includes items such as investigated frequency range (scanned) and test levels. The testing methods and performance specifications, as well as the test site used for the evaluation are indicated in the test data. The test data represents the configuration / operating mode/ model that produced the highest emission levels as compared to the specification limit.

## MODES OF OPERATION

Continuous transmit inductive, 32kHz

## POWER SETTINGS INVESTIGATED

Battery

## CONFIGURATIONS INVESTIGATED

BIOT0080 - 1

## FREQUENCY RANGE INVESTIGATED

Start Frequency | 9 kHz | Stop Frequency | 30 MHz

## SAMPLE CALCULATIONS

Radiated Emissions: Field Strength = Measured Level + Antenna Factor + Cable Factor - Amplifier Gain + Distance Adjustment Factor + External Attenuation

## TEST EQUIPMENT

| Description                  | Manufacturer | Model                  | ID  | Last Cal.  | Cal. Due  |
|------------------------------|--------------|------------------------|-----|------------|-----------|
| Cable                        | None         | 3m Test Distance Cable | EVM | 2020-02-28 | 2/28/2021 |
| Antenna - Loop               | EMCO         | 6502                   | AOA | 2020-07-06 | 7/6/2022  |
| Analyzer - Spectrum Analyzer | Agilent      | E4443A                 | AFB | 2020-06-26 | 6/26/2021 |

## MEASUREMENT BANDWIDTHS

| Frequency Range (MHz) | Peak Data (kHz) | Quasi-Peak Data (kHz) | Average Data (kHz) |
|-----------------------|-----------------|-----------------------|--------------------|
| 0.01 - 0.15           | 1.0             | 0.2                   | 0.2                |
| 0.15 - 30.0           | 10.0            | 9.0                   | 9.0                |
| 30.0 - 1000           | 100.0           | 120.0                 | 120.0              |
| Above 1000            | 1000.0          | N/A                   | 1000.0             |

## TEST DESCRIPTION

The antennas to be used with the EUT were tested. The EUT was continuously transmitting while set to the channel specified.

For each configuration, the spectrum was scanned throughout the specified range as part of the exploratory investigation of the emissions. These "pre-scans" are not included in the report. Final measurements on individual emissions were then made and included in this test report.

The individual emissions from the EUT were maximized by rotating the EUT on a turntable, adjusting the position of the EUT and EUT antenna in three orthogonal axis, and adjusting the measurement antenna height (where applicable) and polarization (per ANSIC63.10). A calibrated active loop antenna was used for this test in order to provide sufficient measurement sensitivity. The reference point of the loop antenna was maintained at 1m above the ground plane during the testing.

Measurements were made with the required detectors and annotated on the data for each individual point using the following annotation:

QP = Quasi-Peak Detector  
PK = Peak Detector  
AV = CISPR Detector

If there are no detectable emissions above the noise floor, the data included may show noise floor measurements for reference only.

As outlined in 15.209(e), 15.31(f)(2), and RSS-GEN, 6.5, measurements may be performed at a distance closer than what is specified with the limit. The limit at the specified distance is shown on the data sheet. Measurements are made at a closer distance and the data is adjusted using a distance correction factor of 40dB/decade for comparison to the limit.


# SPURIOUS RADIATED EMISSIONS



|                 |                                         |                   |            |                                                                |
|-----------------|-----------------------------------------|-------------------|------------|----------------------------------------------------------------|
| Work Order:     | BIOT0080                                | Date:             | 2021-01-20 | <div>EmiRS 2020.12.09.0</div> <div>PSA-ESCI 2020.12.30.0</div> |
| Project:        | None                                    | Temperature:      | 21.8 °C    |                                                                |
| Job Site:       | EV11                                    | Humidity:         | 29% RH     |                                                                |
| Serial Number:  | 88200467                                | Barometric Pres.: | 1025 mbar  |                                                                |
| EUT:            | Neuro SCS IPG                           |                   |            | Tested by: Cole Ghizzone                                       |
| Configuration:  | 1                                       |                   |            |                                                                |
| Customer:       | BIOTRONIK, Inc.                         |                   |            |                                                                |
| Attendees:      | Roy Wang                                |                   |            |                                                                |
| EUT Power:      | Battery                                 |                   |            |                                                                |
| Operating Mode: | Continuous transmit inductive, 32kHz    |                   |            |                                                                |
| Deviations:     | None                                    |                   |            |                                                                |
| Comments:       | EUT leads terminated in distilled water |                   |            |                                                                |

|                     |                  |
|---------------------|------------------|
| Test Specifications | Test Method      |
| FCC 15.209:2021     | ANSI C63.10:2013 |

|       |   |                   |   |                   |           |         |      |
|-------|---|-------------------|---|-------------------|-----------|---------|------|
| Run # | 7 | Test Distance (m) | 1 | Antenna Height(s) | 1 to 4(m) | Results | Pass |
|-------|---|-------------------|---|-------------------|-----------|---------|------|

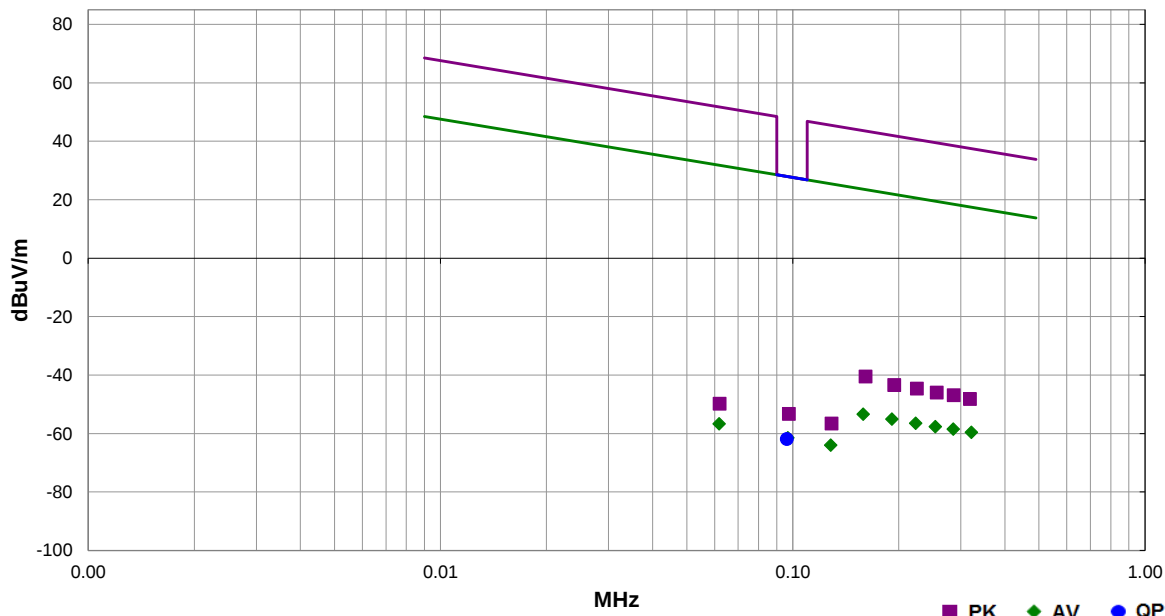

18

| Freq (MHz) | Amplitude (dBuV) | Factor (dB) | Antenna Height (meters) | Azimuth (degrees) | Test Distance (meters) | External Attenuation (dB) | Polarity/ Transducer Type | Detector | Distance Adjustment (dB) | Adjusted (dBuV/m) | Spec. Limit (dBuV/m) | Compared to Spec. (dB) | Comments       |
|------------|------------------|-------------|-------------------------|-------------------|------------------------|---------------------------|---------------------------|----------|--------------------------|-------------------|----------------------|------------------------|----------------|
| 0.158      | 34.7             | 11.0        | 1.0                     | 130.0             | 1.0                    | 0.0                       | Perp EUT                  | AV       | -99.1                    | -53.4             | 23.6                 | -77.0                  | EUT Horizontal |
| 0.286      | 29.9             | 10.7        | 1.0                     | 100.0             | 1.0                    | 0.0                       | Perp EUT                  | AV       | -99.1                    | -58.5             | 18.5                 | -77.0                  | EUT Horizontal |
| 0.191      | 33.2             | 10.8        | 1.0                     | 177.0             | 1.0                    | 0.0                       | Perp EUT                  | AV       | -99.1                    | -55.1             | 22.0                 | -77.1                  | EUT Horizontal |
| 0.223      | 31.8             | 10.8        | 1.0                     | 366.0             | 1.0                    | 0.0                       | Perp EUT                  | AV       | -99.1                    | -56.5             | 20.6                 | -77.1                  | EUT Horizontal |
| 0.321      | 28.7             | 10.8        | 1.0                     | 366.0             | 1.0                    | 0.0                       | Perp EUT                  | AV       | -99.1                    | -59.6             | 17.5                 | -77.1                  | EUT Horizontal |
| 0.254      | 30.7             | 10.7        | 1.0                     | 306.0             | 1.0                    | 0.0                       | Perp EUT                  | AV       | -99.1                    | -57.7             | 19.5                 | -77.2                  | EUT Horizontal |
| 0.097      | 34.6             | 11.2        | 1.0                     | 58.0              | 1.0                    | 0.0                       | Perp EUT                  | PK       | -99.1                    | -53.3             | 27.8                 | -81.1                  | EUT Horizontal |
| 0.161      | 47.6             | 11.0        | 1.0                     | 130.0             | 1.0                    | 0.0                       | Perp EUT                  | PK       | -99.1                    | -40.5             | 43.5                 | -84.0                  | EUT Horizontal |
| 0.225      | 43.7             | 10.8        | 1.0                     | 366.0             | 1.0                    | 0.0                       | Perp EUT                  | PK       | -99.1                    | -44.6             | 40.6                 | -85.2                  | EUT Horizontal |
| 0.194      | 44.9             | 10.8        | 1.0                     | 177.0             | 1.0                    | 0.0                       | Perp EUT                  | PK       | -99.1                    | -43.4             | 41.9                 | -85.3                  | EUT Horizontal |
| 0.256      | 42.4             | 10.7        | 1.0                     | 306.0             | 1.0                    | 0.0                       | Perp EUT                  | PK       | -99.1                    | -46.0             | 39.4                 | -85.4                  | EUT Horizontal |
| 0.287      | 41.5             | 10.7        | 1.0                     | 100.0             | 1.0                    | 0.0                       | Perp EUT                  | PK       | -99.1                    | -46.9             | 38.5                 | -85.4                  | EUT Horizontal |
| 0.318      | 40.1             | 10.8        | 1.0                     | 366.0             | 1.0                    | 0.0                       | Perp EUT                  | PK       | -99.1                    | -48.2             | 37.5                 | -85.7                  | EUT Horizontal |
| 0.062      | 30.6             | 11.8        | 1.0                     | 303.0             | 1.0                    | 0.0                       | Perp EUT                  | AV       | -99.1                    | -56.7             | 31.8                 | -88.5                  | EUT Horizontal |
| 0.097      | 26.4             | 11.2        | 1.0                     | 58.0              | 1.0                    | 0.0                       | Perp EUT                  | AV       | -99.1                    | -61.5             | 27.9                 | -89.4                  | EUT Horizontal |
| 0.128      | 24.2             | 10.9        | 1.0                     | 193.0             | 1.0                    | 0.0                       | Perp EUT                  | AV       | -99.1                    | -64.0             | 25.5                 | -89.5                  | EUT Horizontal |
| 0.096      | 26.0             | 11.2        | 1.0                     | 58.0              | 1.0                    | 0.0                       | Perp EUT                  | QP       | -99.1                    | -61.9             | 27.9                 | -89.8                  | EUT Horizontal |
| 0.062      | 37.5             | 11.8        | 1.0                     | 303.0             | 1.0                    | 0.0                       | Perp EUT                  | PK       | -99.1                    | -49.8             | 51.7                 | -101.5                 | EUT Horizontal |
| 0.129      | 31.6             | 10.9        | 1.0                     | 193.0             | 1.0                    | 0.0                       | Perp EUT                  | PK       | -99.1                    | -56.6             | 45.4                 | -102.0                 | EUT Horizontal |