

Appendix B


RF power output conducted

Appendix C

RF power output radiated


**Equivalent Isotropically Radiated Power
FCC RULES PART 24 SUBPART E**

Approval Holder: BIOTRONIK GmbH & CO. KG
EUT : TELEX III
Model / Channel : CARDIOMESSENGER II / 512
Temperature/ Voltage: Temp.: 23°C / Unom.: 4.20 V DC
Test Site / Operator: ETS / Mr. Handrik
Test Specification: according to §24.232
Comment 1: Dist.: 3m, Ant.: HL025, PCL 0
Comment 2: Freq: 1.850GHz, Pmax: 27.63dBm, RBW: 3MHz

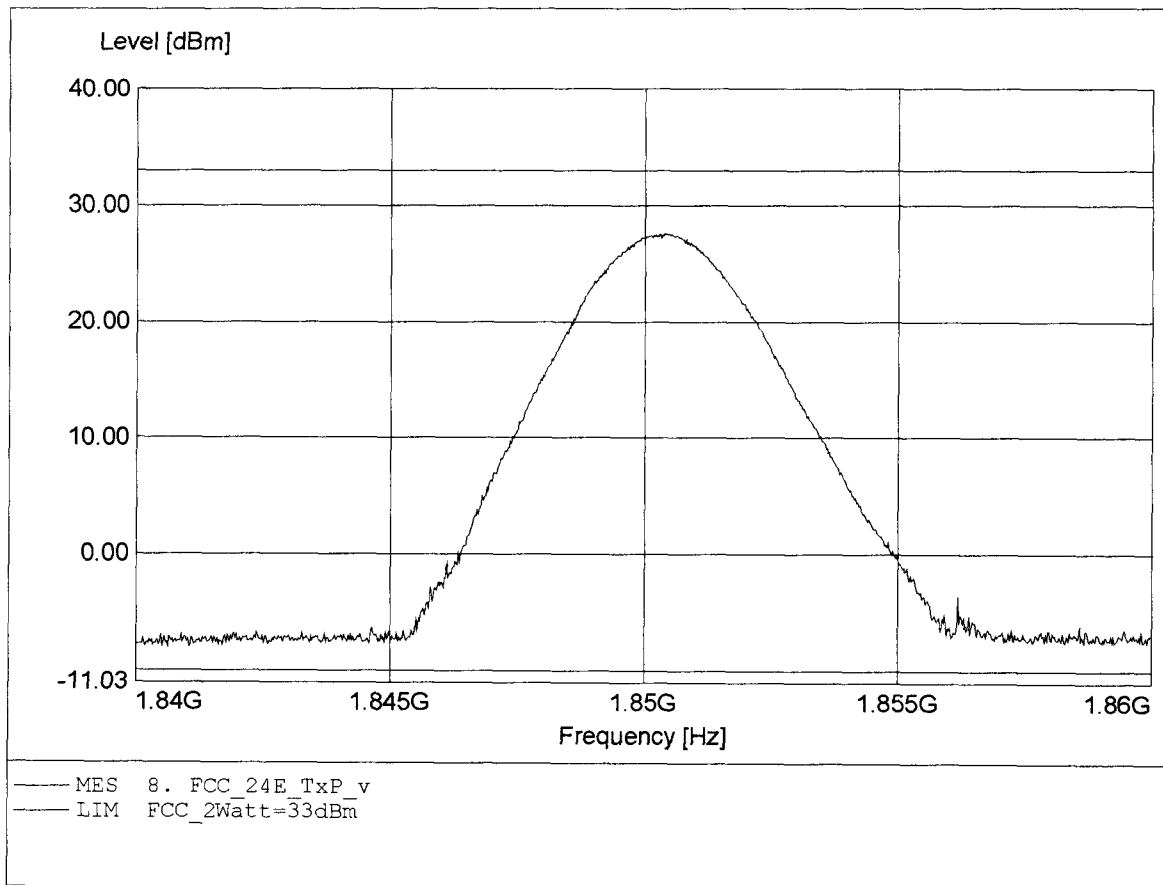


**Equivalent Isotropically Radiated Power
FCC RULES PART 24 SUBPART E**

Approval Holder: BIOTRONIK GmbH & CO. KG
EUT : TELEX III
Model / Channel : CARDIOMESSENGER II / 512
Temperature/ Voltage: Temp.: 23°C / Unom.: 4.20 V DC
Test Site / Operator: ETS / Mr. Handrik
Test Specification: according to S24.232
Comment 1: Dist.: 3m, Ant.: HL025,PCL 0
Comment 2: Freq: 1.850GHz, Pmax: 23.18dBm, RBW: 3MHz

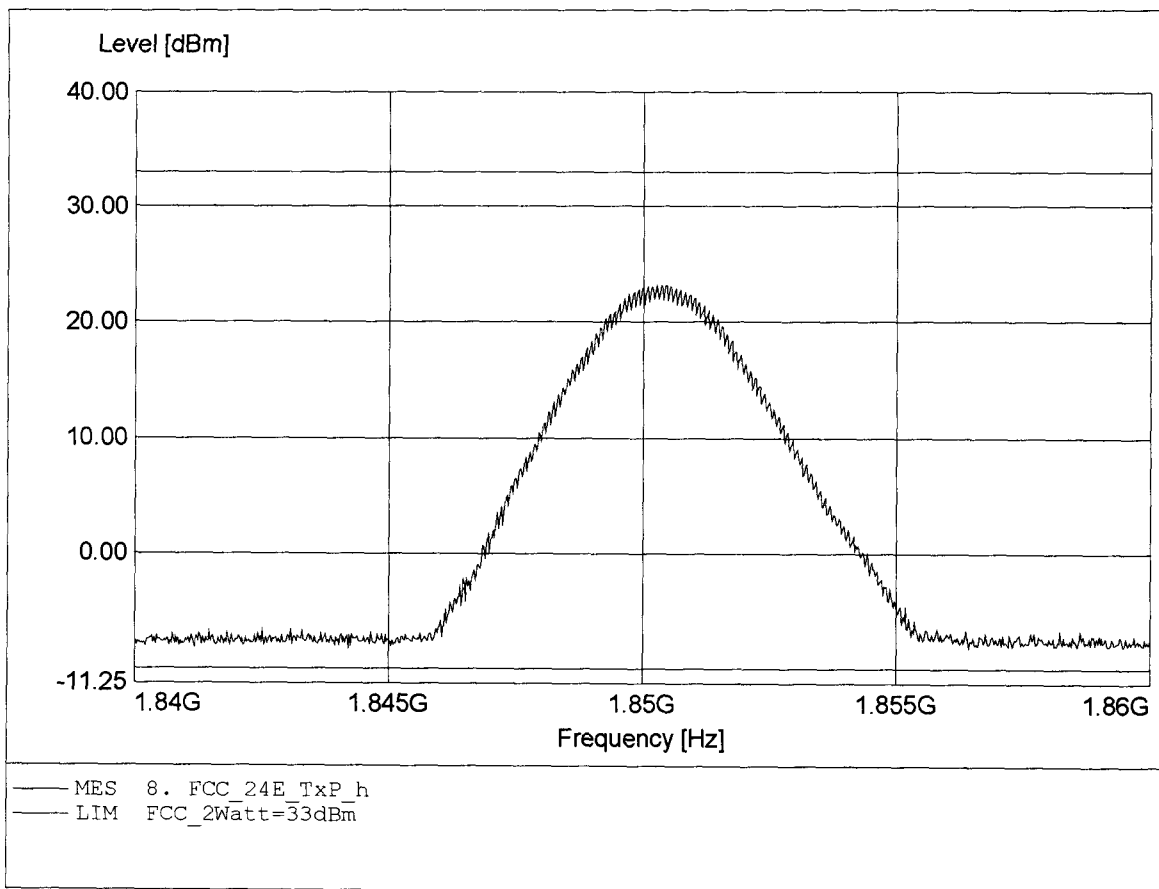


**Equivalent Isotropically Radiated Power
FCC RULES PART 24 SUBPART E**

Approval Holder: BIOTRONIK GmbH & CO. KG
EUT : TELEX III
Model / Channel : CARDIOMESSENGER II / 661
Temperature/ Voltage: Temp.: 23°C / Unom.: 4.20 V DC
Test Site / Operator: ETS / Mr. Handrik
Test Specification: according to S24.232
Comment 1: Dist.: 3m, Ant.: HL025,PCL 0
Comment 2: Freq: 1.880GHz, Pmax: 26.83dBm, RBW: 3MHz

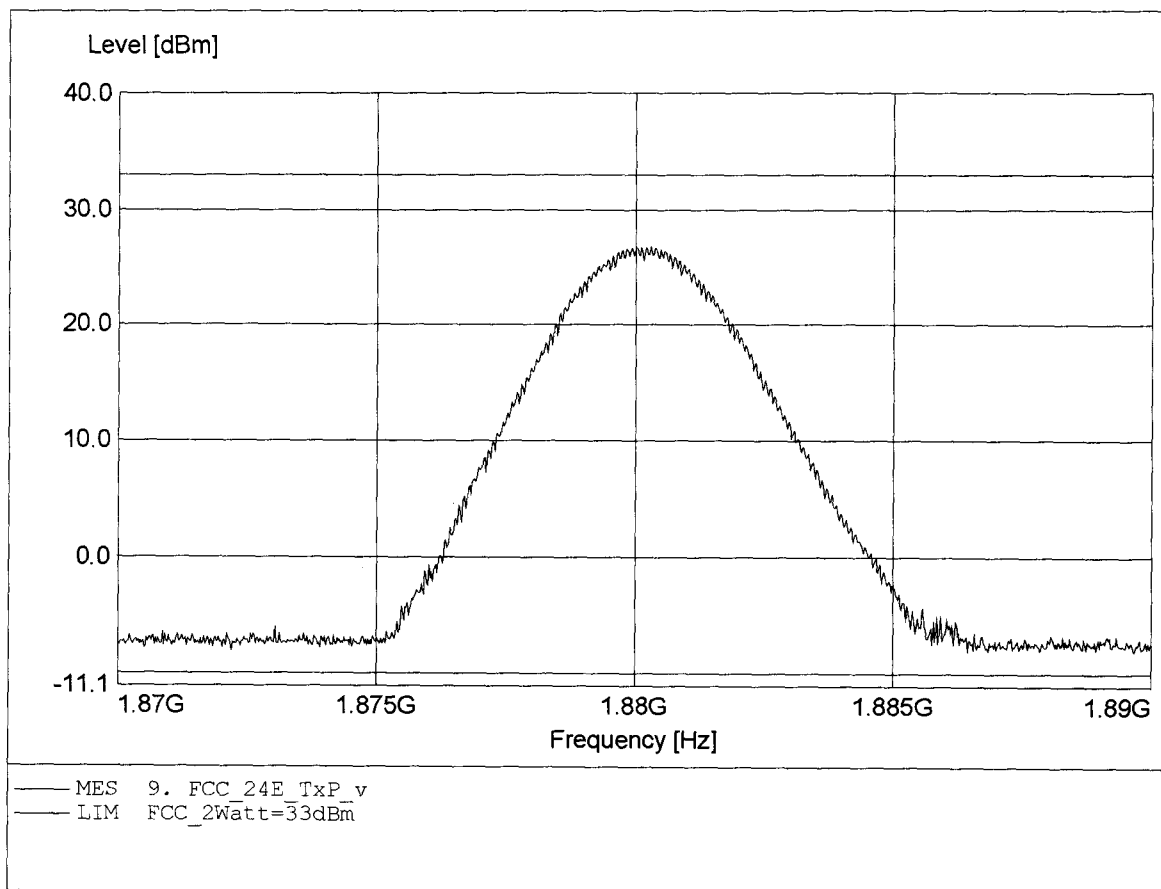


**Equivalent Isotropically Radiated Power
FCC RULES PART 24 SUBPART E**

Approval Holder: BIOTRONIK GmbH & CO. KG
EUT : TELEX III
Model / Channel : CARDIOMESSENGER II / 661
Temperature/ Voltage: Temp.: 23°C / Unom.: 4.20 V DC
Test Site / Operator: ETS / Mr. Handrik
Test Specification: according to S24.232
Comment 1: Dist.: 3m, Ant.: HL025, PCL 0
Comment 2: Freq: 1.880GHz, Pmax: 22.83dBm, RBW: 3MHz

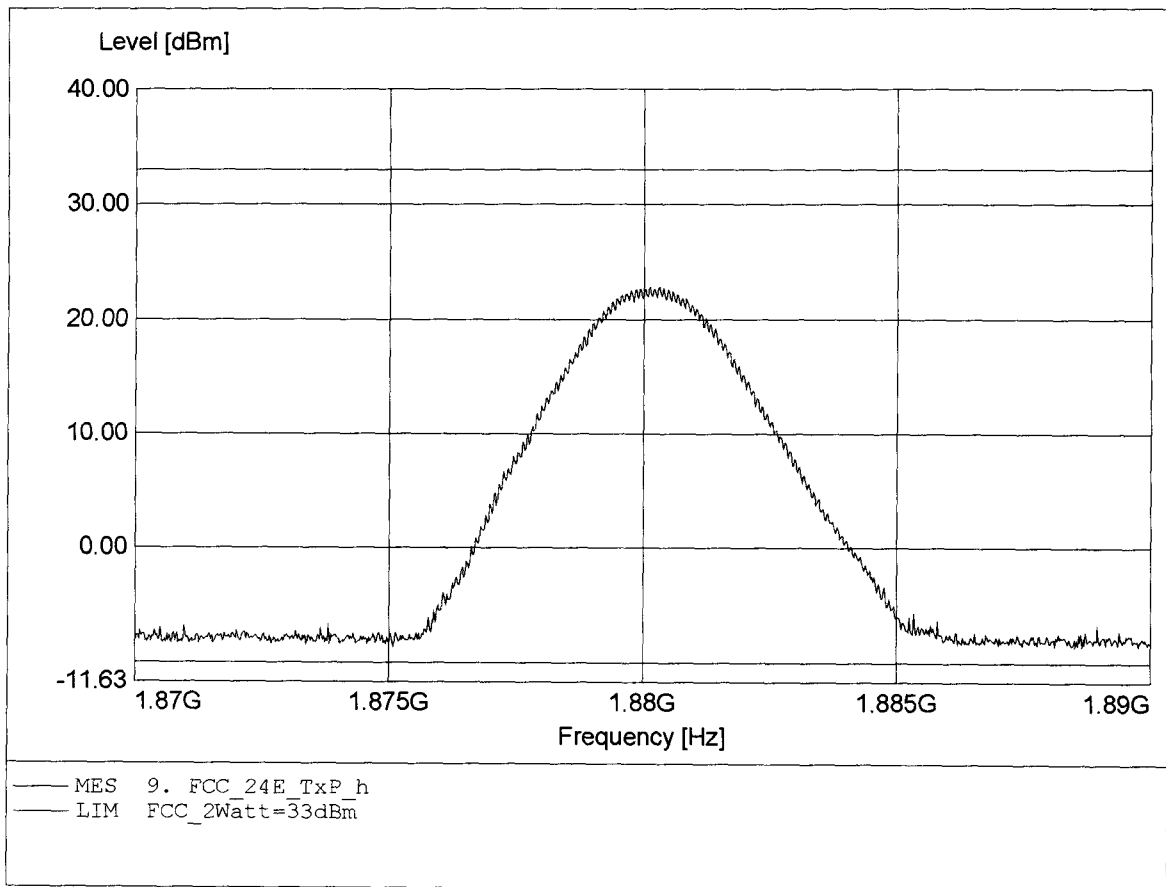


**Equivalent Isotropically Radiated Power
FCC RULES PART 24 SUBPART E**

Approval Holder: BIOTRONIK GmbH & CO. KG
EUT : TELEX III
Model / Channel : CARDIOMESSENGER II / 810
Temperature/ Voltage: Temp.: 23°C / Unom.: 4.20 V DC
Test Site / Operator: ETS / Mr. Handrik
Test Specification: according to §24.232
Comment 1: Dist.: 3m, Ant.: HL025,PCL 0
Comment 2: Freq: 1.910GHz, Pmax: 26.57dBm, RBW: 3MHz

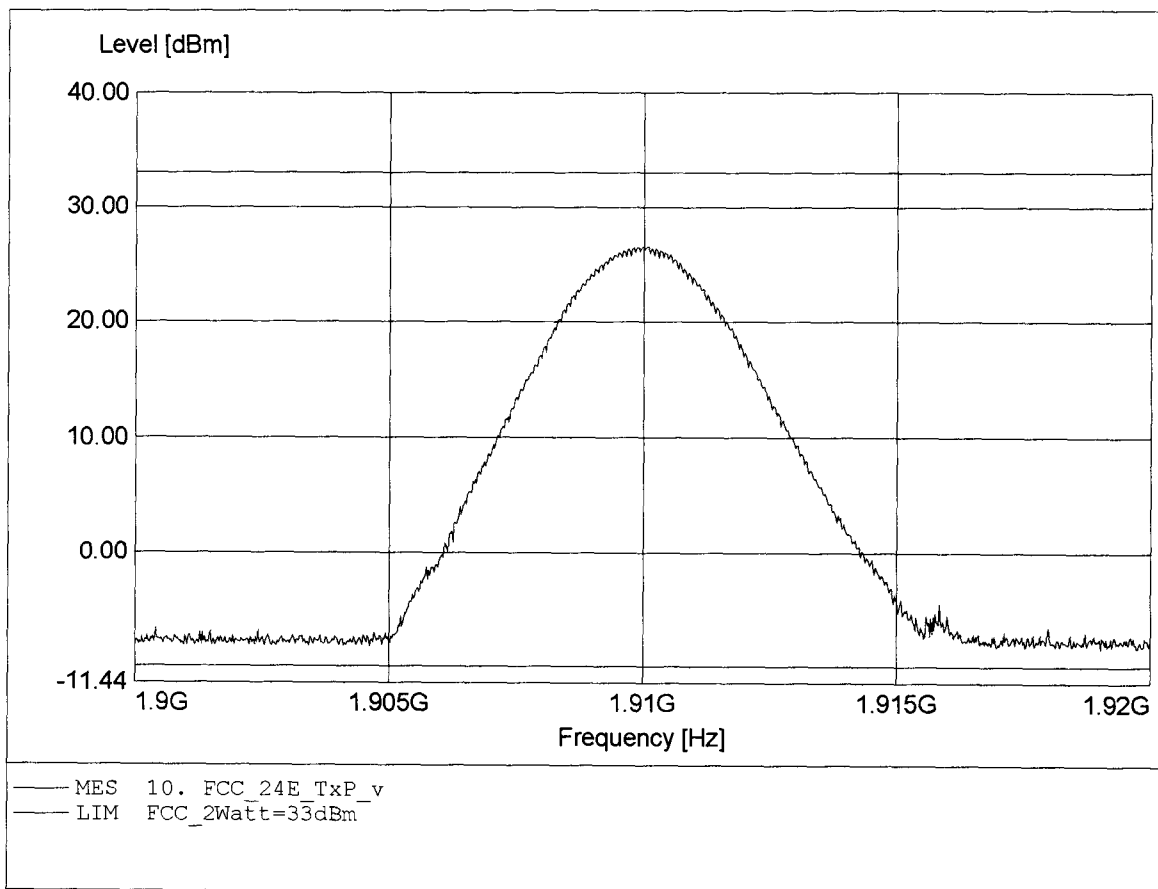


**Equivalent Isotropically Radiated Power
FCC RULES PART 24 SUBPART E**

Approval Holder: BIOTRONIK GmbH & CO. KG
EUT : TELEX III
Model / Channel : CARDIOMESSENGER II / 810
Temperature/ Voltage: Temp.: 23°C / Unom.: 4.20 V DC
Test Site / Operator: ETS / Mr. Handrik
Test Specification: according to §24.232
Comment 1: Dist.: 3m, Ant.: HL025,PCL 0
Comment 2: Freq: 1.910GHz, Pmax: 24.00dBm, RBW: 3MHz

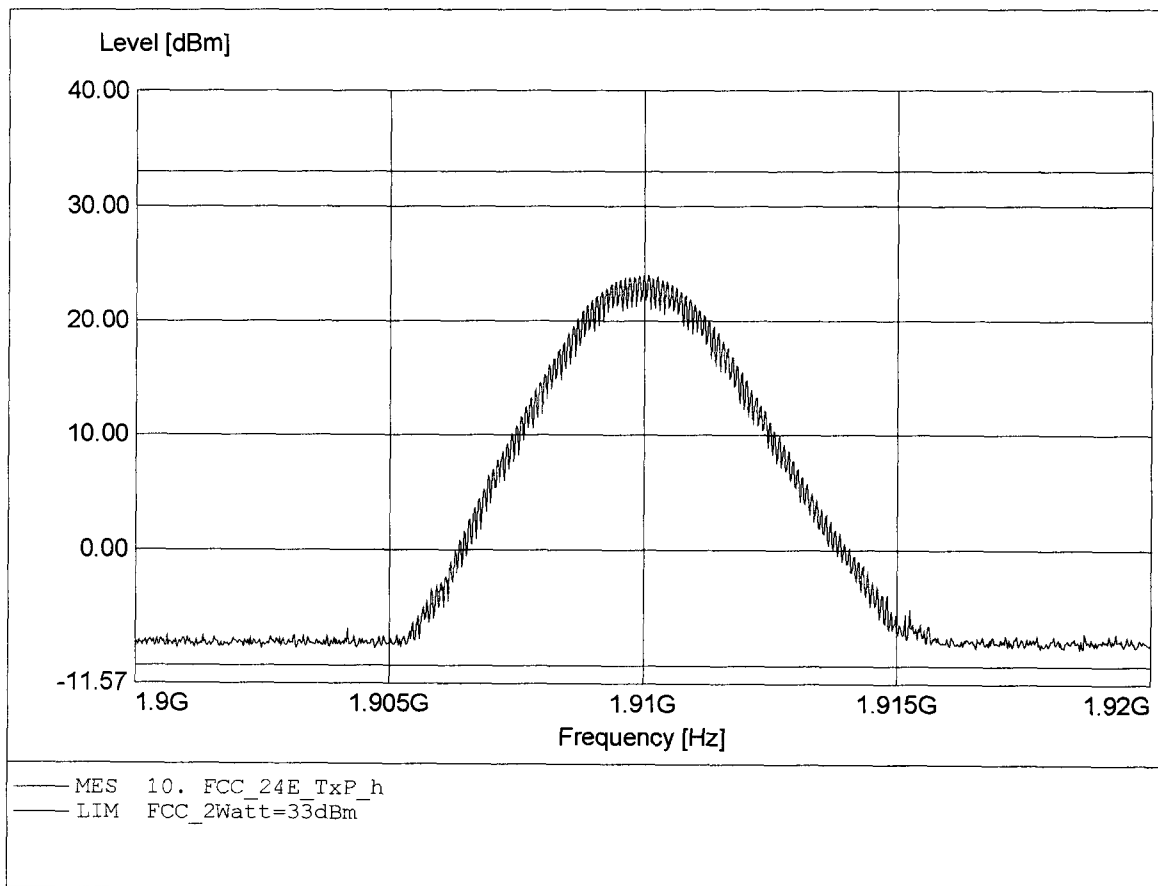


Effective Radiated Power
FCC RULES PART 22 SUBPART H

Approval Holder: BIOTRONIK GmbH & CO. KG
EUT : TELEX III
Model / Channel : CARDIOMESSENGER II / 128
Temperature/ Voltage: Temp.: 23°C / Unom.: 4.20 V DC
Test Site / Operator: ETS / Mr. Handrik
Test Specification: according to §22.913
Comment 1: Dist.: 3m, Ant.: HL223
Comment 2: Freq: 824.278MHz, Pmax: 29.72dBm, RBW: 3MHz

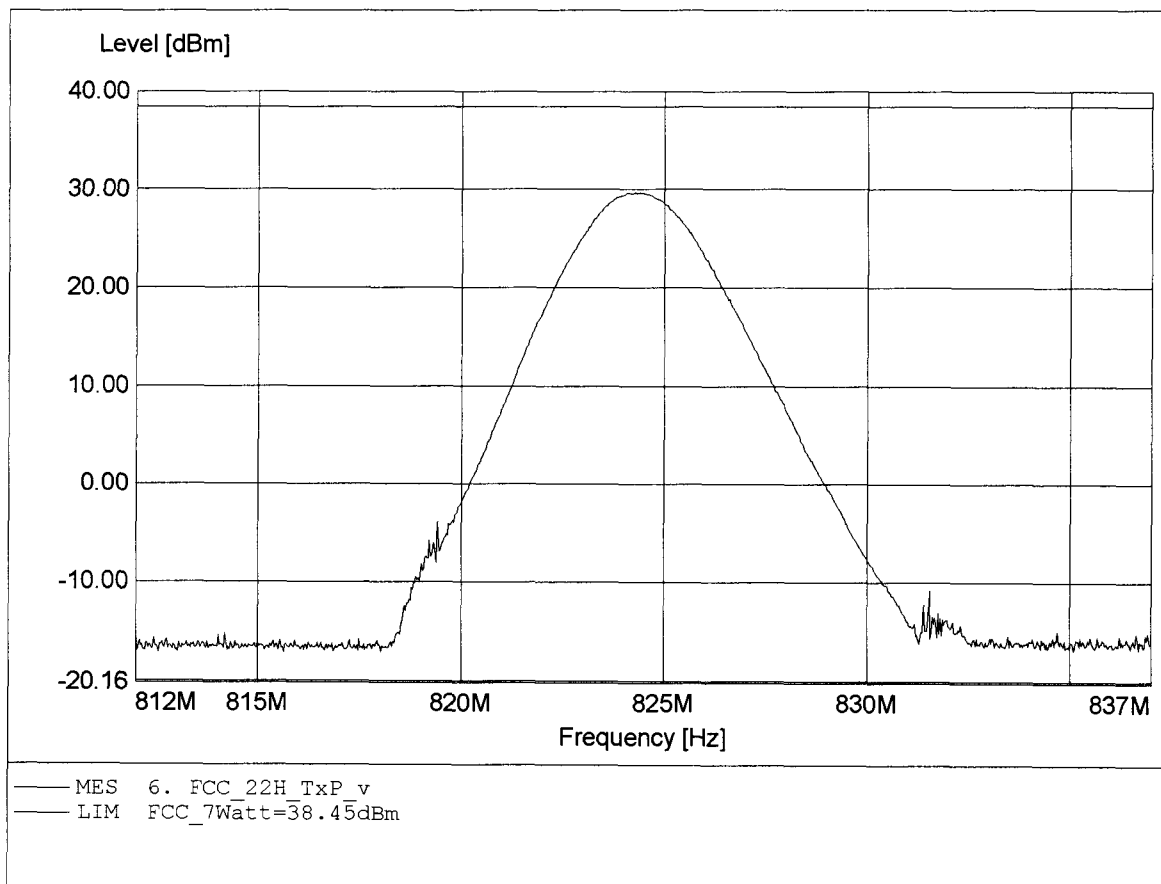


Effective Radiated Power
FCC RULES PART 22 SUBPART H

Approval Holder: BIOTRONIK GmbH & CO. KG
EUT : TELEX III
Model / Channel : CARDIOMESSENGER II / 128
Temperature/ Voltage: Temp.: 23°C / Unom.: 4.20 V DC
Test Site / Operator: ETS / Mr. Handrik
Test Specification: according to §22.913
Comment 1: Dist.: 3m, Ant.: HL223
Comment 2: Freq: 824.333MHz, Pmax: 23.59dBm, RBW: 3MHz

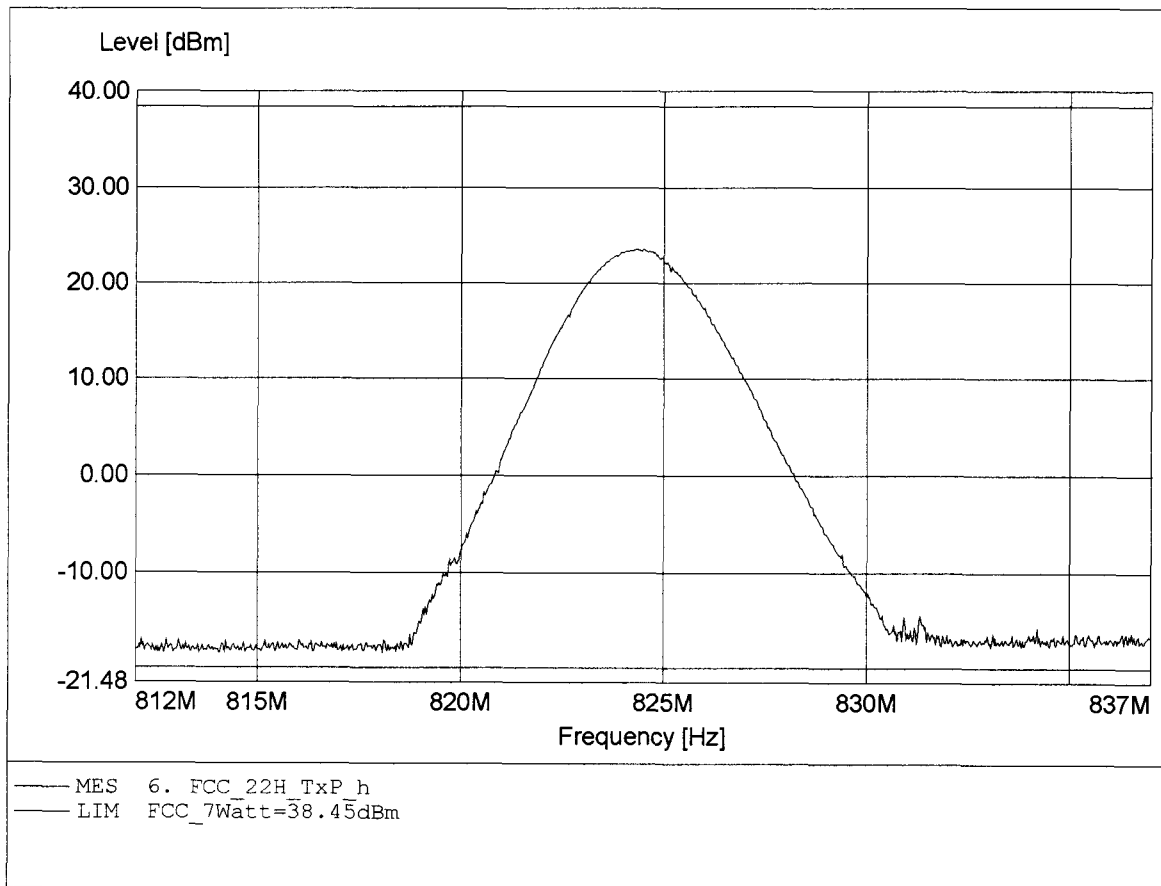


Effective Radiated Power
FCC RULES PART 22 SUBPART H

Approval Holder: BIOTRONIK GmbH & CO. KG
EUT : TELEX III
Model / Channel : CARDIOMESSENGER II / 188
Temperature/ Voltage: Temp.: 23°C / Unom.: 4.20 V DC
Test Site / Operator: ETS / Mr. Handrik
Test Specification: according to §22.913
Comment 1: Dist.: 3m, Ant.: HL223
Comment 2: Freq: 836.347MHz, Pmax: 29.90dBm, RBW: 3MHz

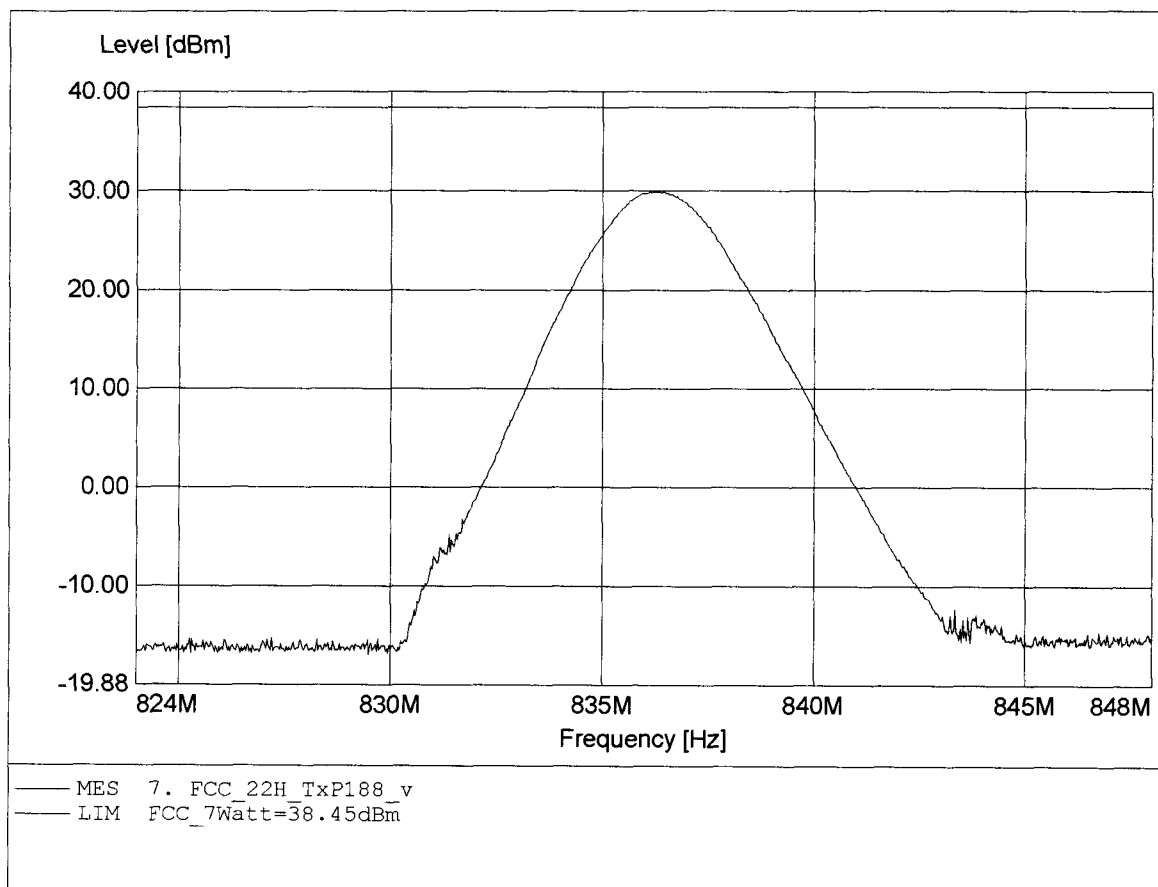


Effective Radiated Power
FCC RULES PART 22 SUBPART H

Approval Holder: BIOTRONIK GmbH & CO. KG
EUT : TELEX III
Model / Channel : CARDIOMESSENGER II / 188
Temperature/ Voltage: Temp.: 23°C / Unom.: 4.20 V DC
Test Site / Operator: ETS / Mr. Handrik
Test Specification: according to §22.913
Comment 1: Dist.: 3m, Ant.: HL223
Comment 2: Freq: 836.187MHz, Pmax: 23.10dBm, RBW: 3MHz

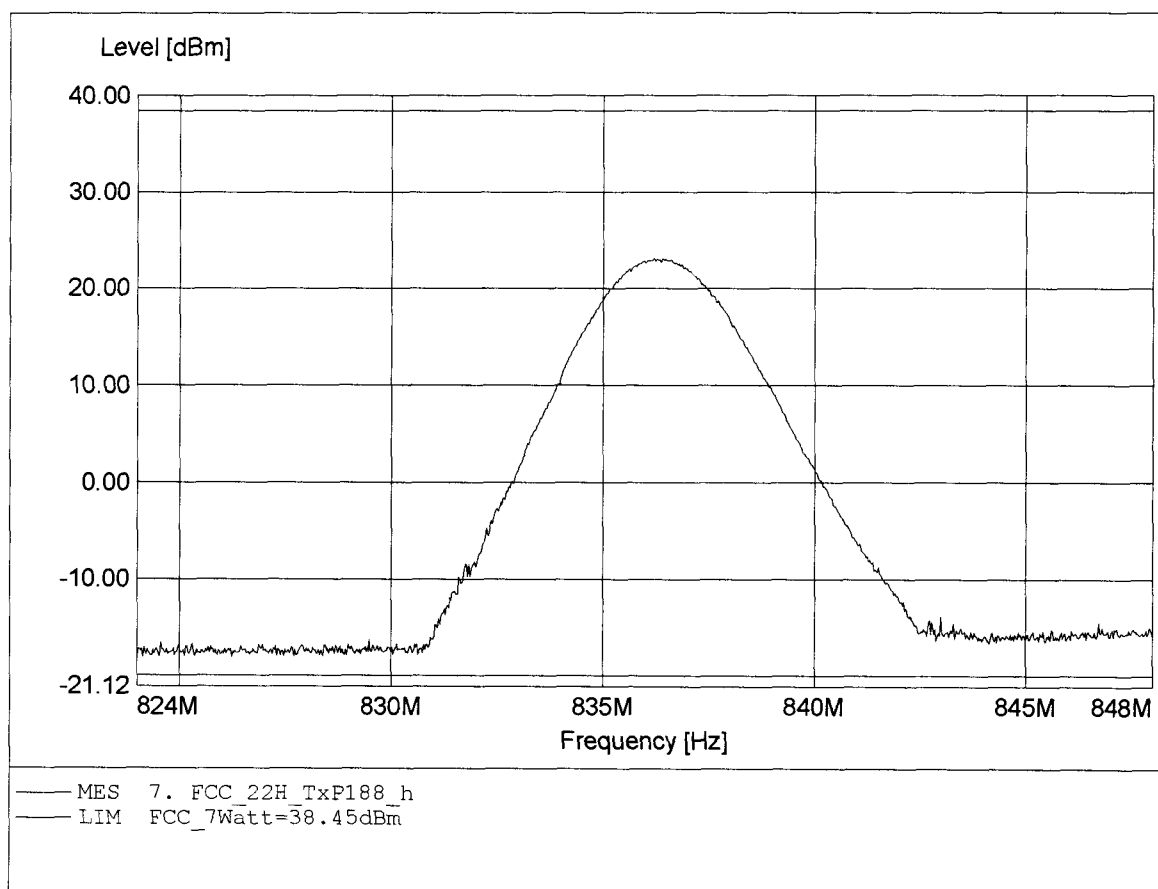


Effective Radiated Power
FCC RULES PART 22 SUBPART H

Approval Holder: BIOTRONIK GmbH & CO. KG
EUT : TELEX III
Model / Channel : CARDIOMESSENGER II / 251
Temperature/ Voltage: Temp.: 23°C / Unom.: 4.20 V DC
Test Site / Operator: ETS / Mr. Handrik
Test Specification: according to §22.913
Comment 1: Dist.: 3m, Ant.: HL223
Comment 2: Freq: 848.920MHz, Pmax: 30.12dBm, RBW: 3MHz

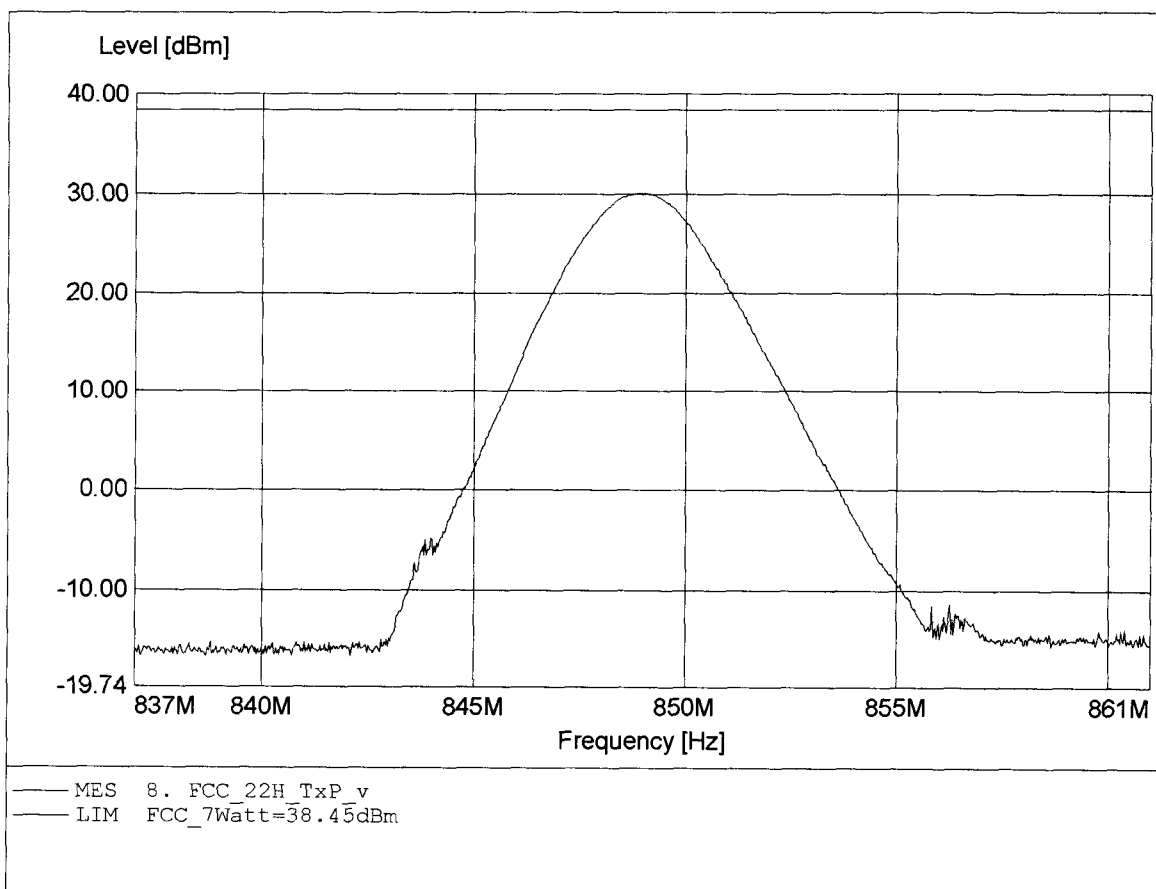

Effective Radiated Power
FCC RULES PART 22 SUBPART H

Approval Holder: BIOTRONIK GmbH & CO. KG
EUT : TELEX III
Model / Channel : CARDIOMESSENGER II / 251
Temperature/ Voltage: Temp.: 23°C / Unom.: 4.20 V DC
Test Site / Operator: ETS / Mr. Handrik
Test Specification: according to §22.913
Comment 1: Dist.: 3m, Ant.: HL223
Comment 2: Freq: 848.947MHz, Pmax: 22.54dBm, RBW: 3MHz

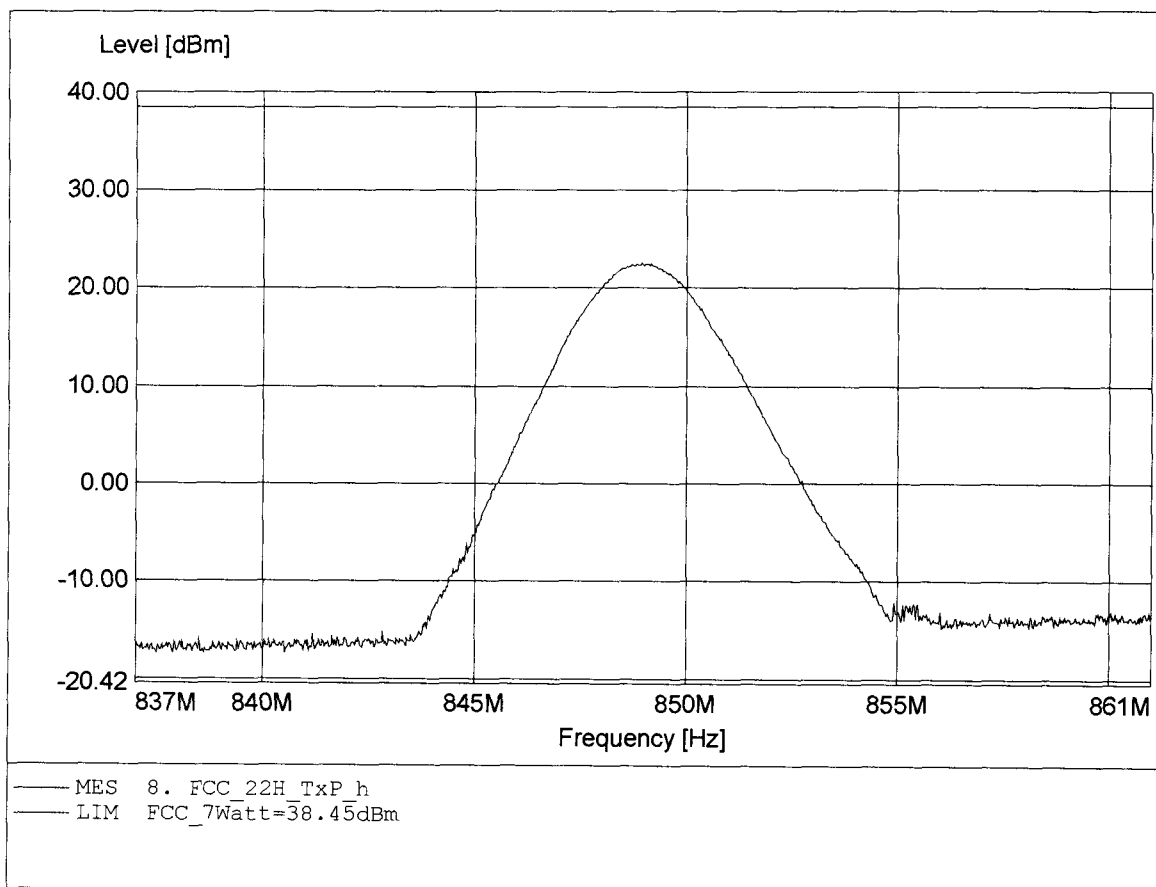

Appendix D

Occupied bandwidth, emission bandwidth

Appendix E

Frequency stability

Appendix F


Spurious emission conducted (antenna terminal)

Appendix G

Spurious emission radiated


Radiated Emissions Tx
FCC RULES PART 24 SUBPART E

Approval Holder: BIOTRONIK GmbH & CO. KG
EUT : TELEX III
Model / Channel : CARDIOMESSENGER II / 512
Temperature/ Voltage: Temp.: 23°C / Unom.: 4.20 V DC
Test Site / Operator: ETS / Mr. Handrik
Test Specification: according to §24.238
Comment 1: Dist.: 3m, Ant.: HK 116
Comment 2: Freq: 62.489MHz, Pmax: -51.78dBm, RBW: 1MHz

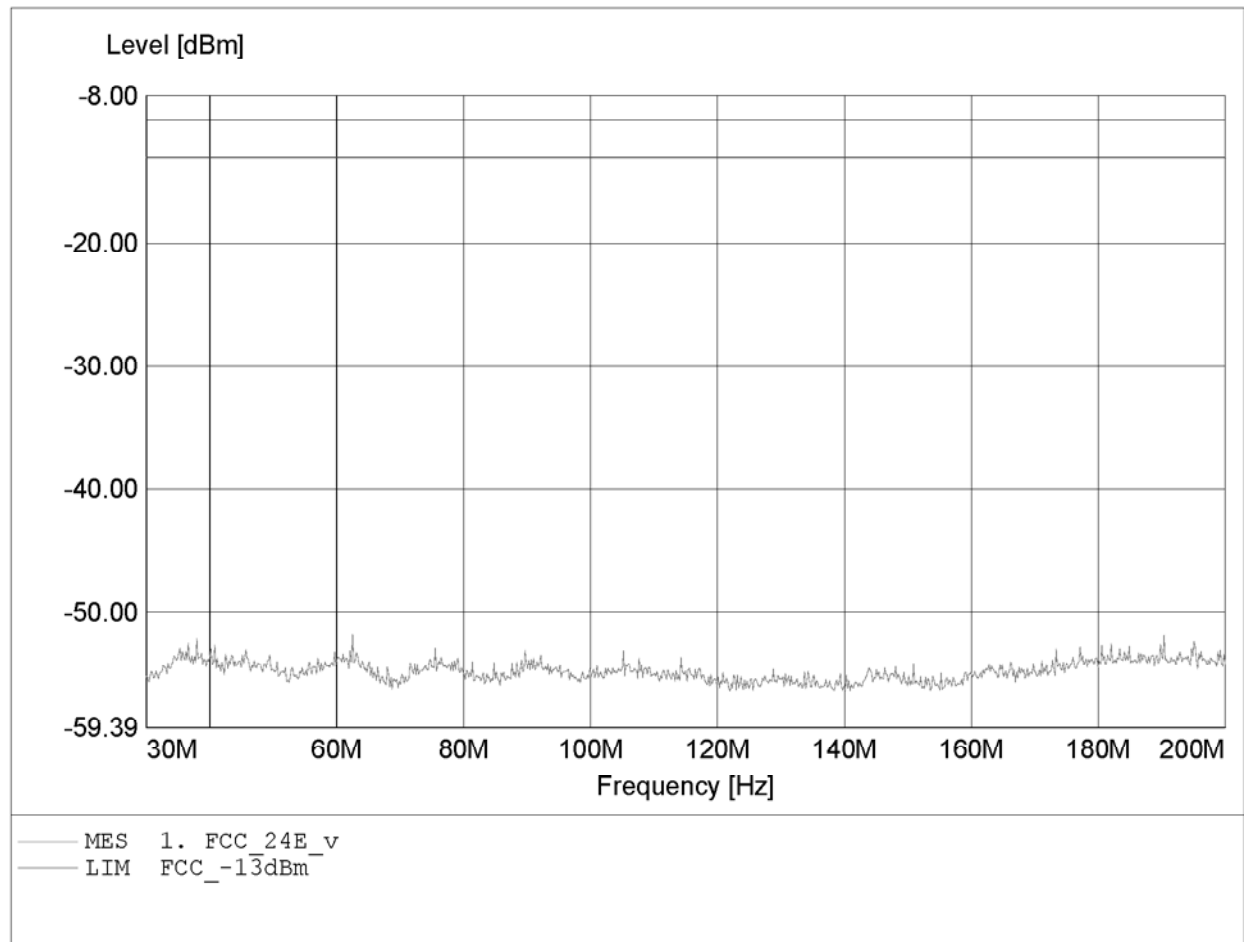


Radiated Emissions Tx
FCC RULES PART 24 SUBPART E

Approval Holder: BIOTRONIK GmbH & CO. KG
EUT : TELEX III
Model / Channel : CARDIOMESSENGER II / 512
Temperature/ Voltage: Temp.: 23°C / Unom.: 4.20 V DC
Test Site / Operator: ETS / Mr. Handrik
Test Specification: according to §24.238
Comment 1: Dist.: 3m, Ant.: HK 116
Comment 2: Freq: 61.733MHz, Pmax: -51.94dBm, RBW: 1MHz

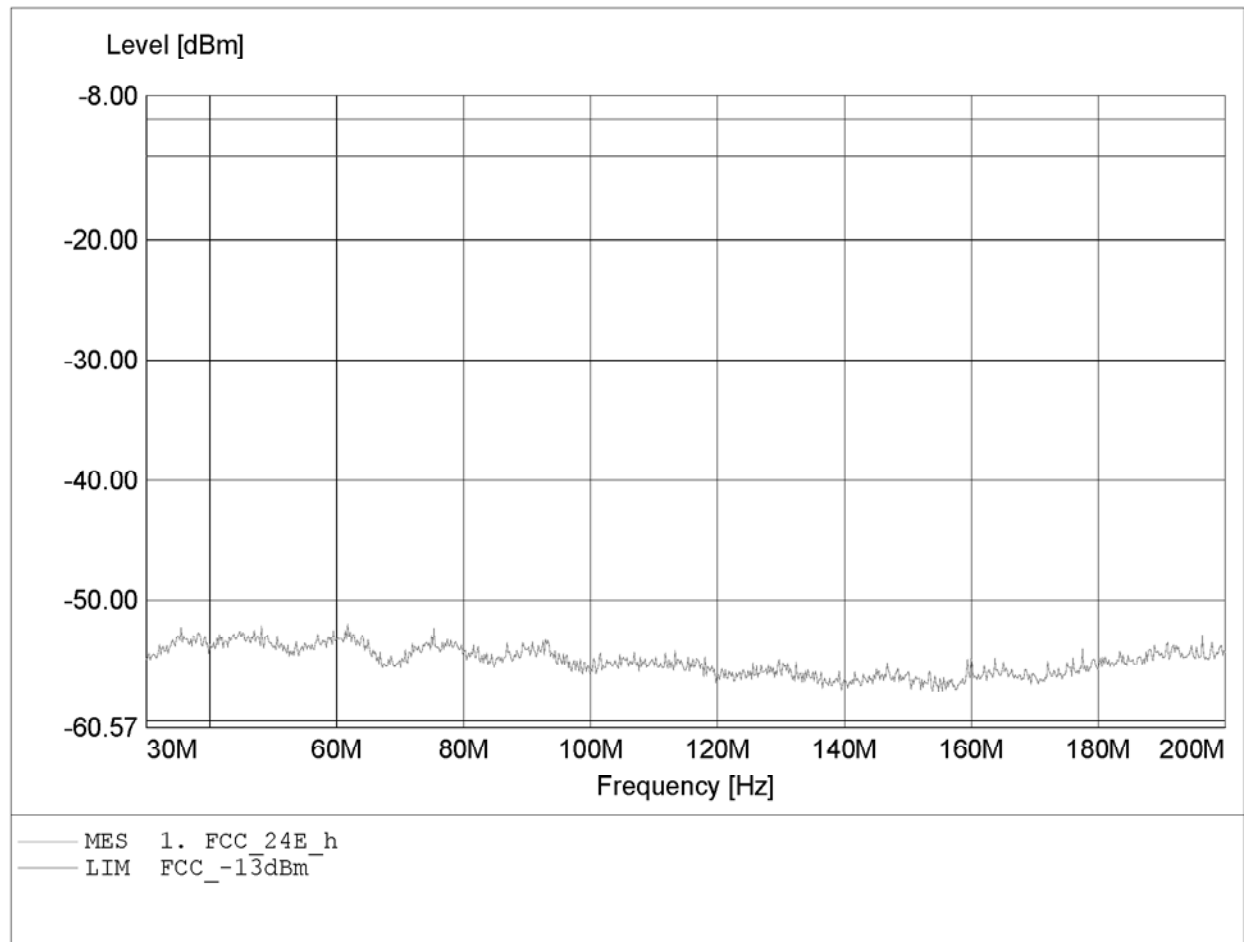


Radiated Emissions Tx
FCC RULES PART 24 SUBPART E

Approval Holder: BIOTRONIK GmbH & CO. KG
EUT : TELEX III
Model / Channel : CARDIOMESSENGER II / 512
Temperature/ Voltage: Temp.: 23°C / Unom.: 4.20 V DC
Test Site / Operator: ETS / Mr. Handrik
Test Specification: according to §24.238
Comment 1: Dist.: 3m, Ant.: HL 223
Comment 2: Freq: 976.889MHz, Pmax: -39.54dBm, RBW: 1MHz

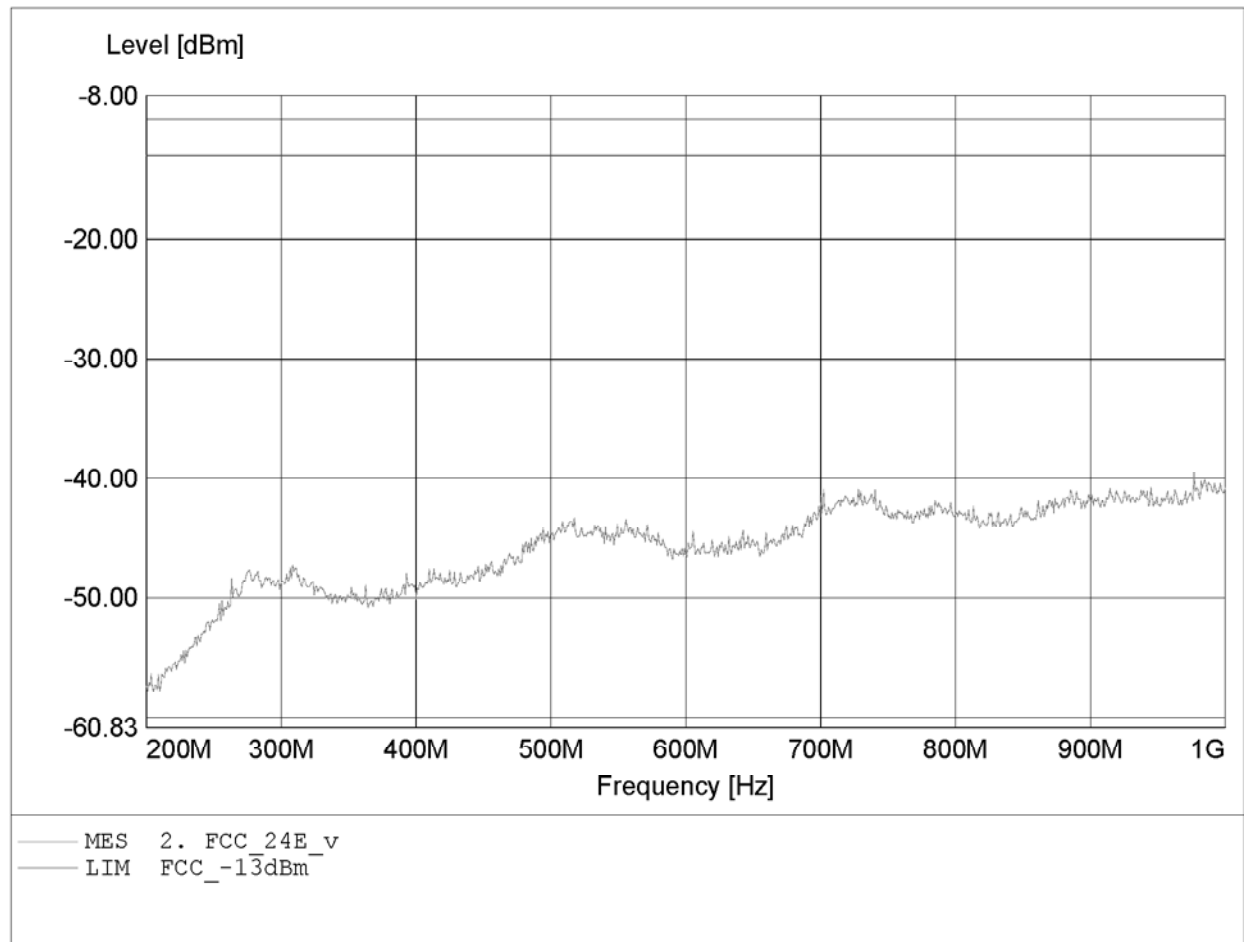


Radiated Emissions Tx
FCC RULES PART 24 SUBPART E

Approval Holder: BIOTRONIK GmbH & CO. KG
EUT : TELEX III
Model / Channel : CARDIOMESSENGER II / 512
Temperature/ Voltage: Temp.: 23°C / Unom.: 4.20 V DC
Test Site / Operator: ETS / Mr. Handrik
Test Specification: according to §24.238
Comment 1: Dist.: 3m, Ant.: HL 223
Comment 2: Freq: 852.444MHz, Pmax: -38.68dBm, RBW: 1MHz

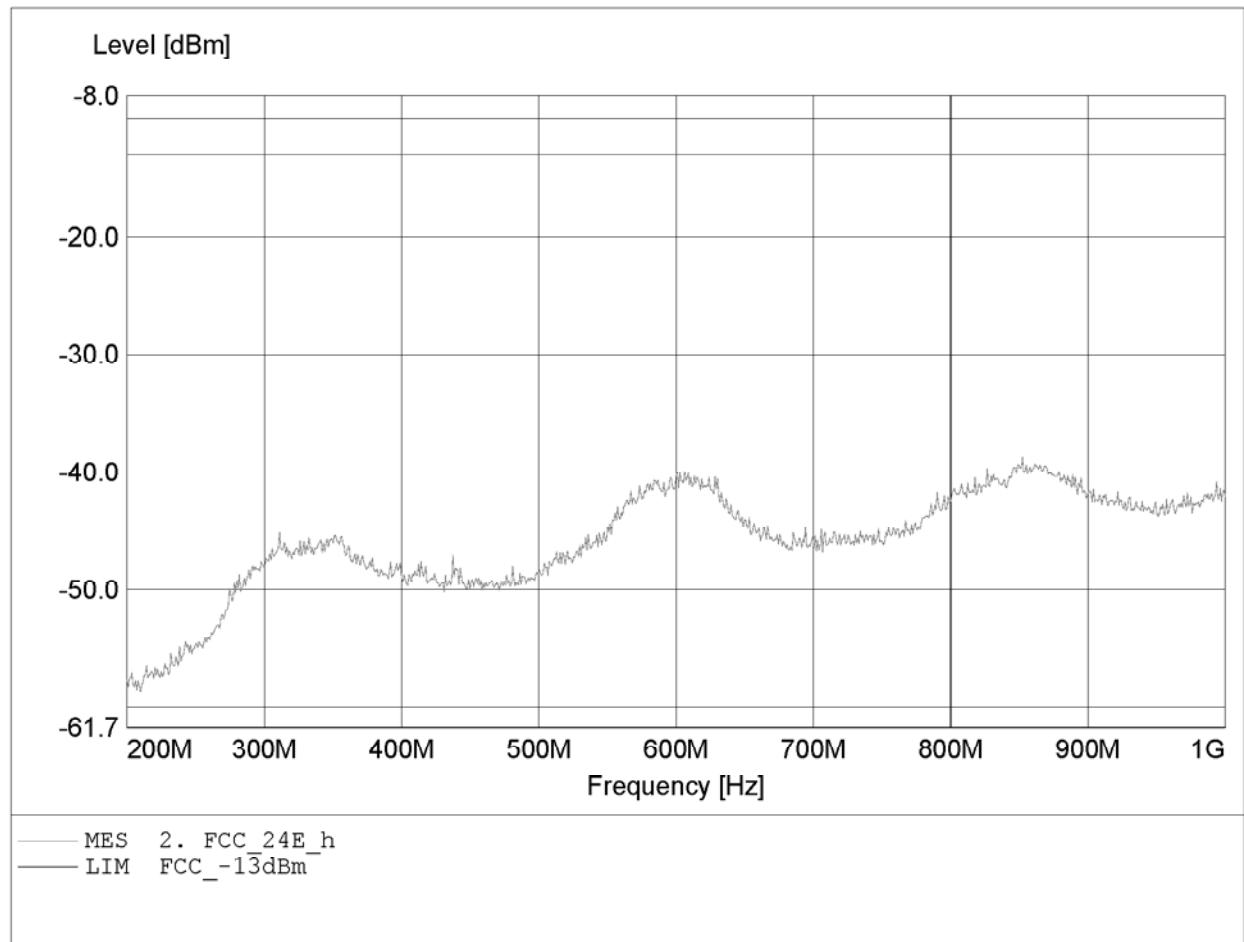


Radiated Emissions Tx
FCC RULES PART 24 SUBPART E

Approval Holder: BIOTRONIK GmbH & CO. KG
EUT : TELEX III
Model / Channel : CARDIOMESSENGER II / 512
Temperature/ Voltage: Temp.: 23°C / Unom.: 4.20 V DC
Test Site / Operator: ETS / Mr. Handrik
Test Specification: according to §24.238
Comment 1: Dist.: 3m, Ant.: HL025
Comment 2: Freq: 3.643GHz, Pmax: -22.18dBm, RBW: 1MHz/3kHz

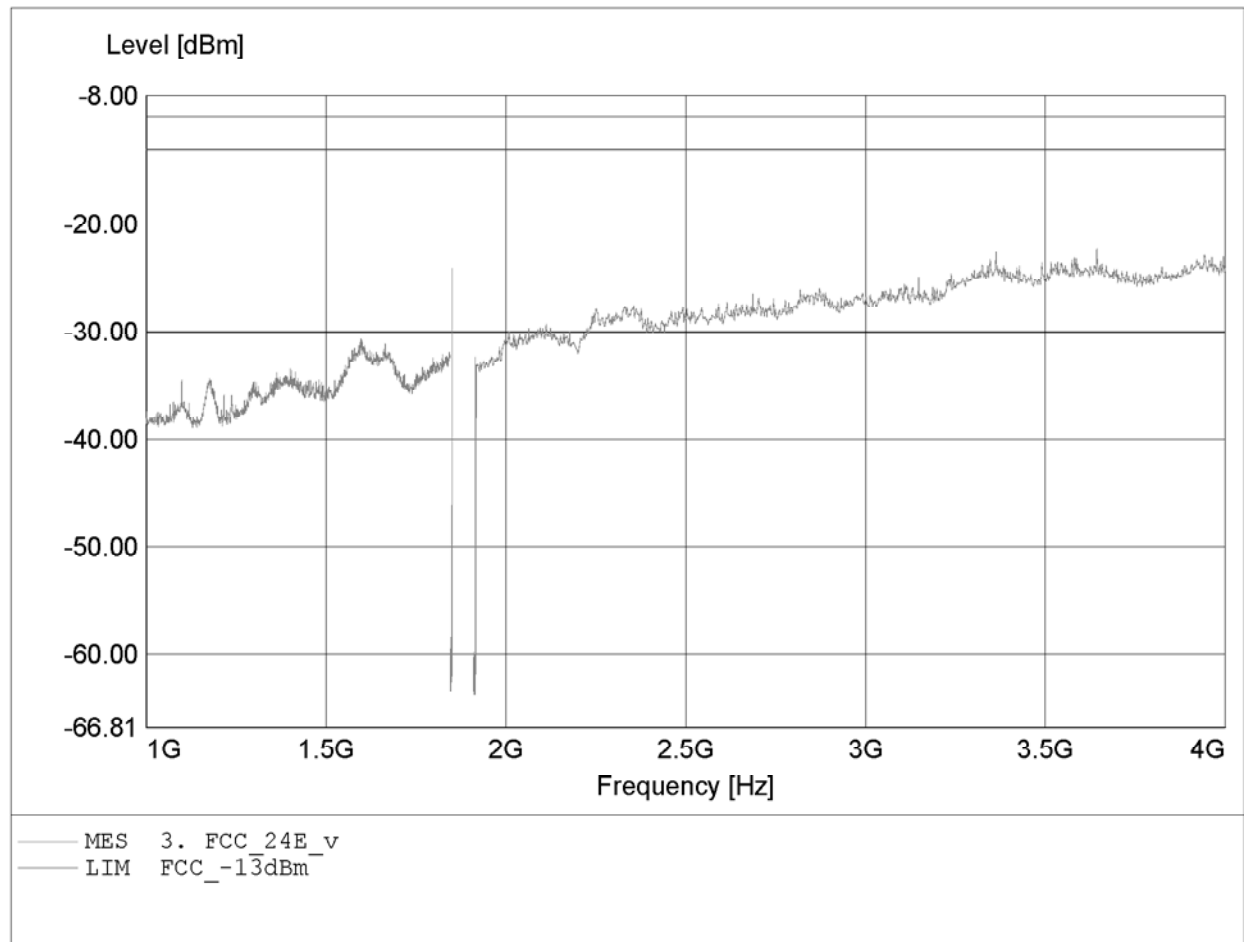


Radiated Emissions Tx
FCC RULES PART 24 SUBPART E

Approval Holder: BIOTRONIK GmbH & CO. KG
EUT : TELEX III
Model / Channel : CARDIOMESSENGER II / 512
Temperature/ Voltage: Temp.: 23°C / Unom.: 4.20 V DC
Test Site / Operator: ETS / Mr. Handrik
Test Specification: according to §24.238
Comment 1: Dist.: 3m, Ant.: HL025
Comment 2: Freq: 3.972GHz, Pmax: -22.15dBm, RBW: 1MHz/3kHz

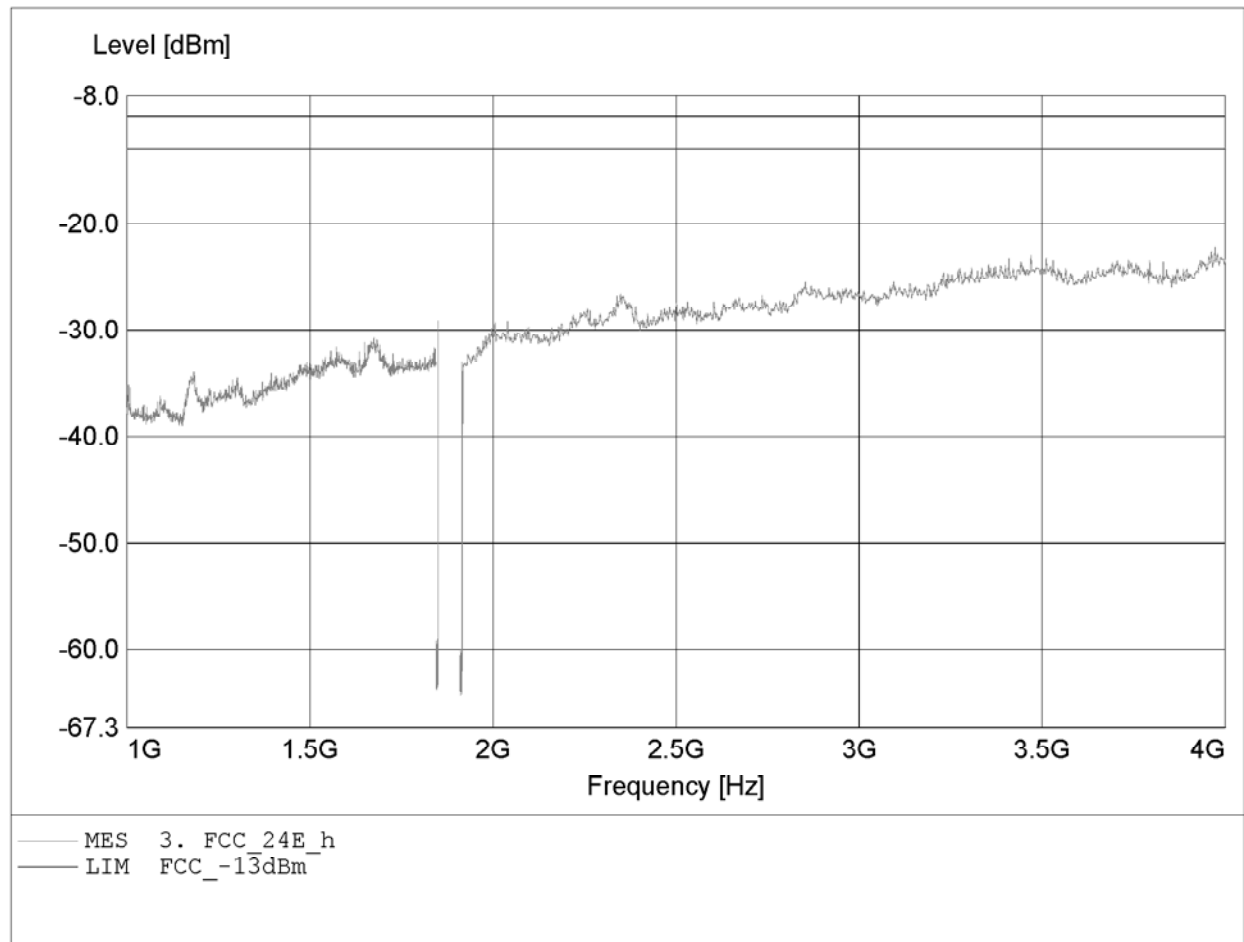


Radiated Emissions Tx
FCC RULES PART 24 SUBPART E

Approval Holder: BIOTRONIK GmbH & CO. KG
EUT : TELEX III
Model / Channel : CARDIOMESSENGER II / 512
Temperature/ Voltage: Temp.: 23°C / Unom.: 4.20 V DC
Test Site / Operator: ETS / Mr. Handrik
Test Specification: according to §24.238
Comment 1: Dist.: 3m, Ant.: HL025, ampl.+HP.
Comment 2: Freq: 7.560GHz, Pmax: -44.85dBm, RBW: 1MHz

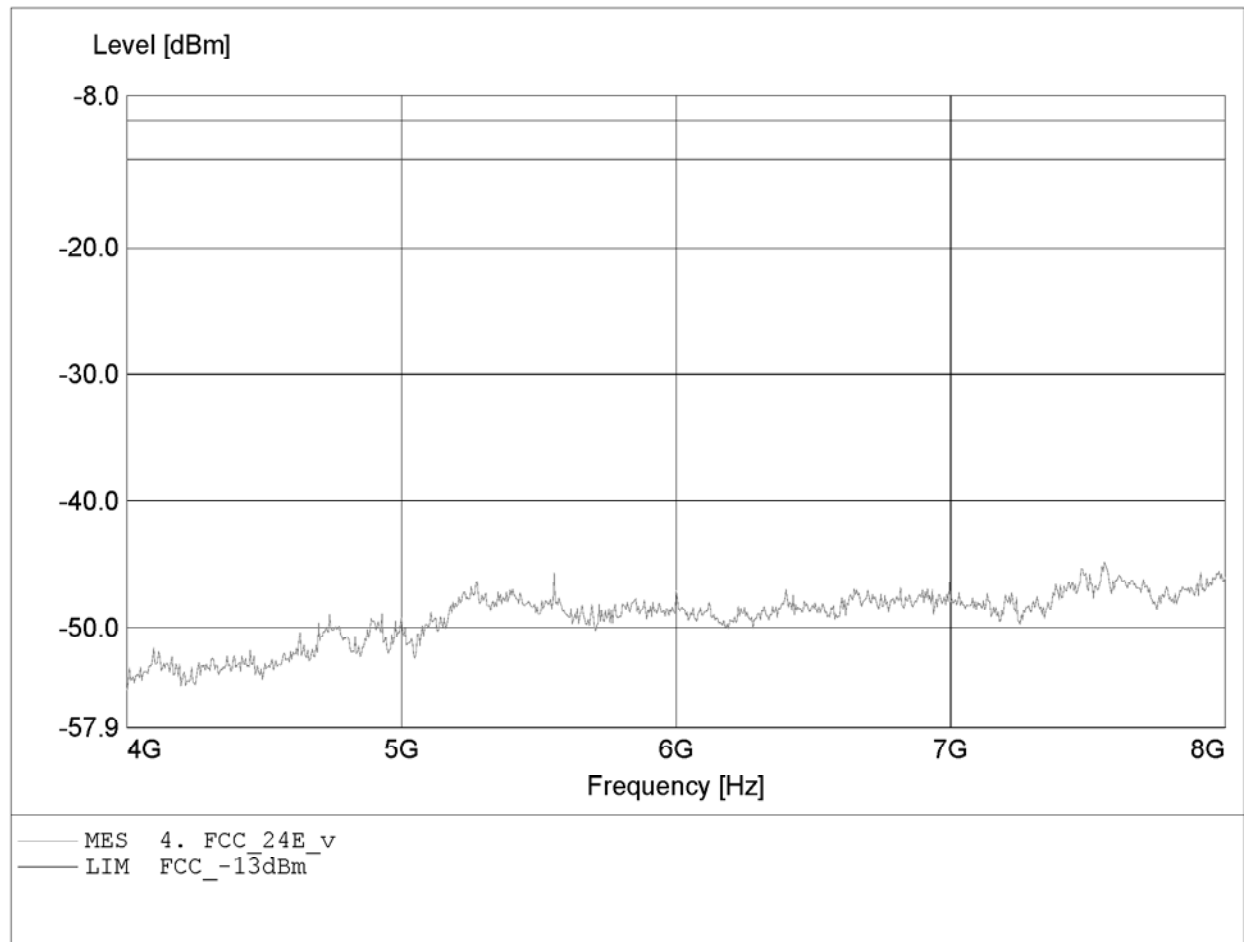


Radiated Emissions Tx
FCC RULES PART 24 SUBPART E

Approval Holder: BIOTRONIK GmbH & CO. KG
EUT : TELEX III
Model / Channel : CARDIOMESSENGER II / 512
Temperature/ Voltage: Temp.: 23°C / Unom.: 4.20 V DC
Test Site / Operator: ETS / Mr. Handrik
Test Specification: according to §24.238
Comment 1: Dist.: 3m, Ant.: HL025, ampl.+HP.
Comment 2: Freq: 7.560GHz, Pmax: -44.55dBm, RBW: 1MHz

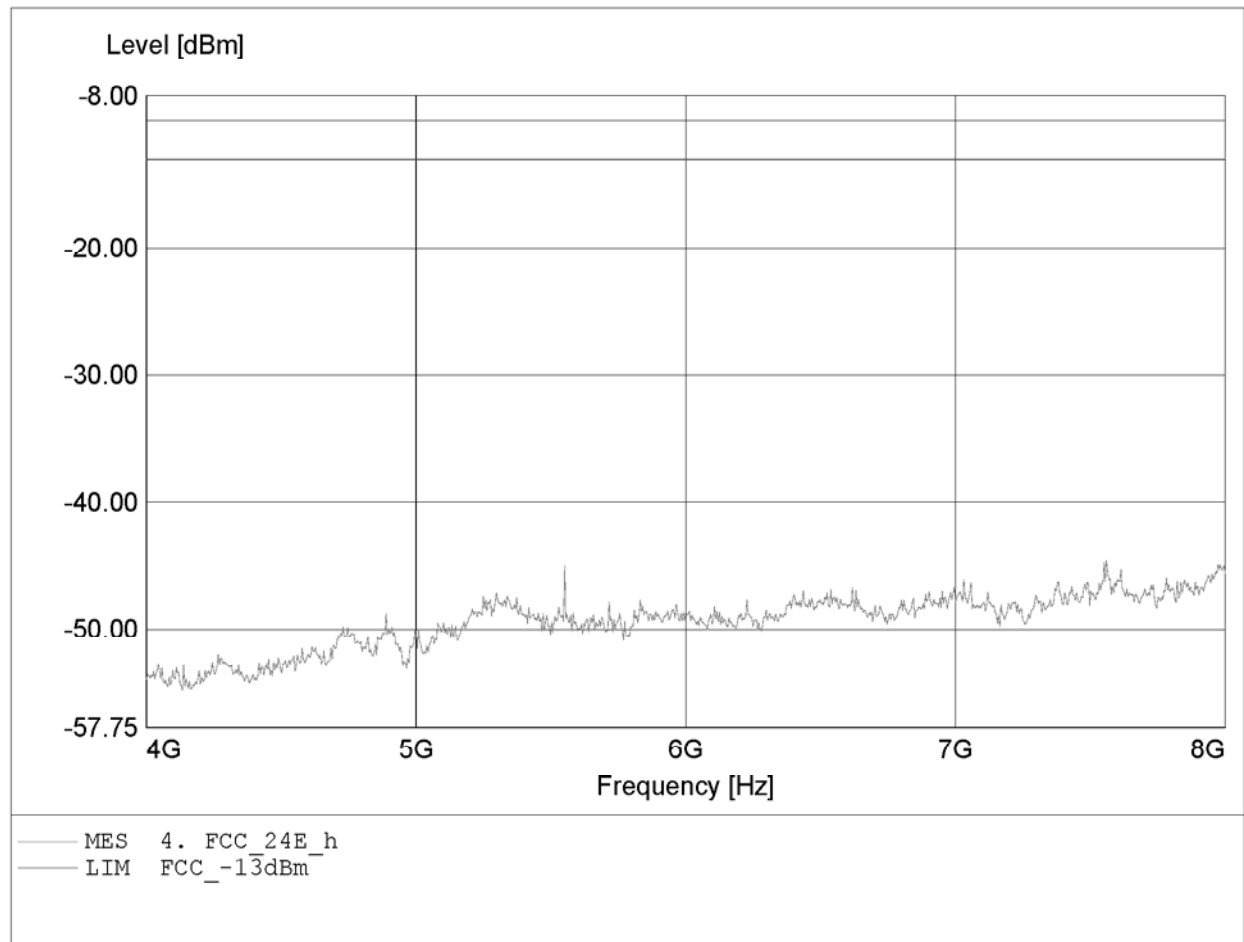


Radiated Emissions Tx
FCC RULES PART 24 SUBPART E

Approval Holder: BIOTRONIK GmbH & CO. KG
EUT : TELEX III
Model / Channel : CARDIOMESSENGER II / 512
Temperature/ Voltage: Temp.: 23°C / Unom.: 4.20 V DC
Test Site / Operator: ETS / Mr. Handrik
Test Specification: according to §24.238
Comment 1: Dist.: 3m, Ant.: HL025, ampl.+HP.
Comment 2: Freq: 9.253GHz, Pmax: -33.06dBm, RBW: 1MHz

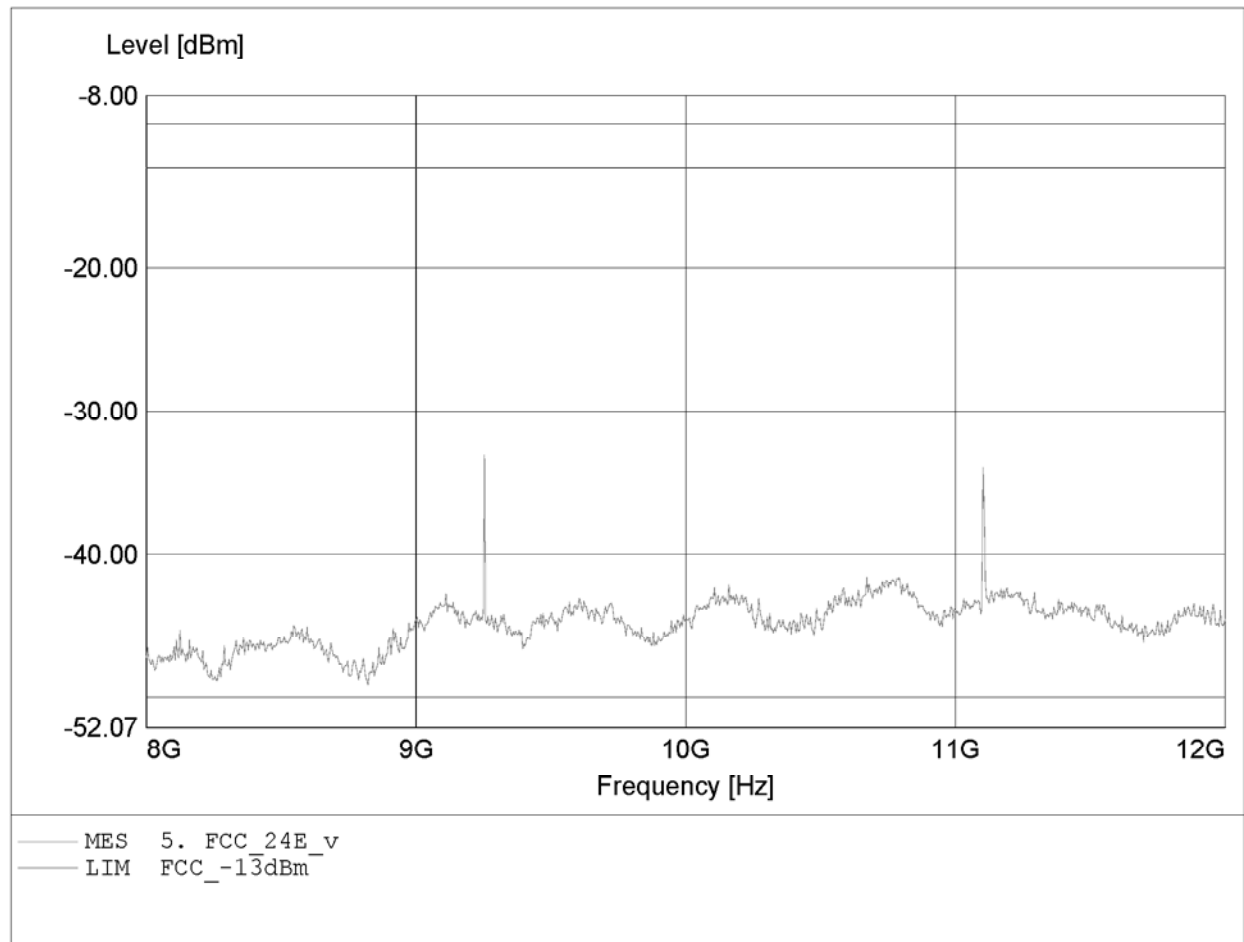


Radiated Emissions Tx
FCC RULES PART 24 SUBPART E

Approval Holder: BIOTRONIK GmbH & CO. KG
EUT : TELEX III
Model / Channel : CARDIOMESSENGER II / 512
Temperature/ Voltage: Temp.: 23°C / Unom.: 4.20 V DC
Test Site / Operator: ETS / Mr. Handrik
Test Specification: according to §24.238
Comment 1: Dist.: 3m, Ant.: HL025, ampl.+HP.
Comment 2: Freq: 11.102GHz, Pmax: -39.70dBm, RBW: 1MHz

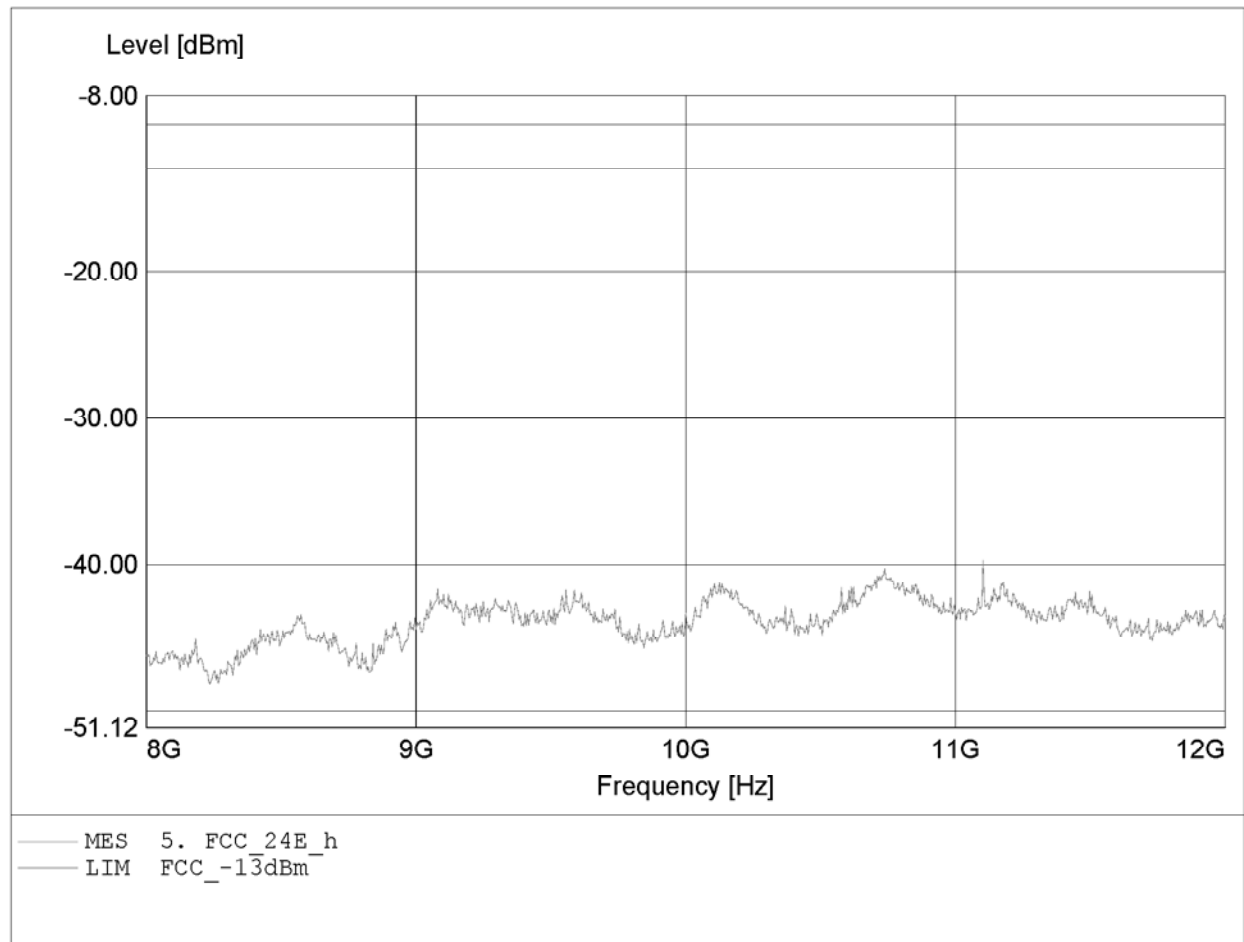


Radiated Emissions Tx
FCC RULES PART 24 SUBPART E

Approval Holder: BIOTRONIK GmbH & CO. KG
EUT : TELEX III
Model / Channel : CARDIOMESSENGER II / 512
Temperature/ Voltage: Temp.: 23°C / Unom.: 4.20 V DC
Test Site / Operator: ETS / Mr. Handrik
Test Specification: according to §24.238
Comment 1: Dist.: 3m, Ant.: HL025, ampl.+HP.
Comment 2: Freq: 14.807GHz, Pmax: -30.92dBm, RBW: 1MHz

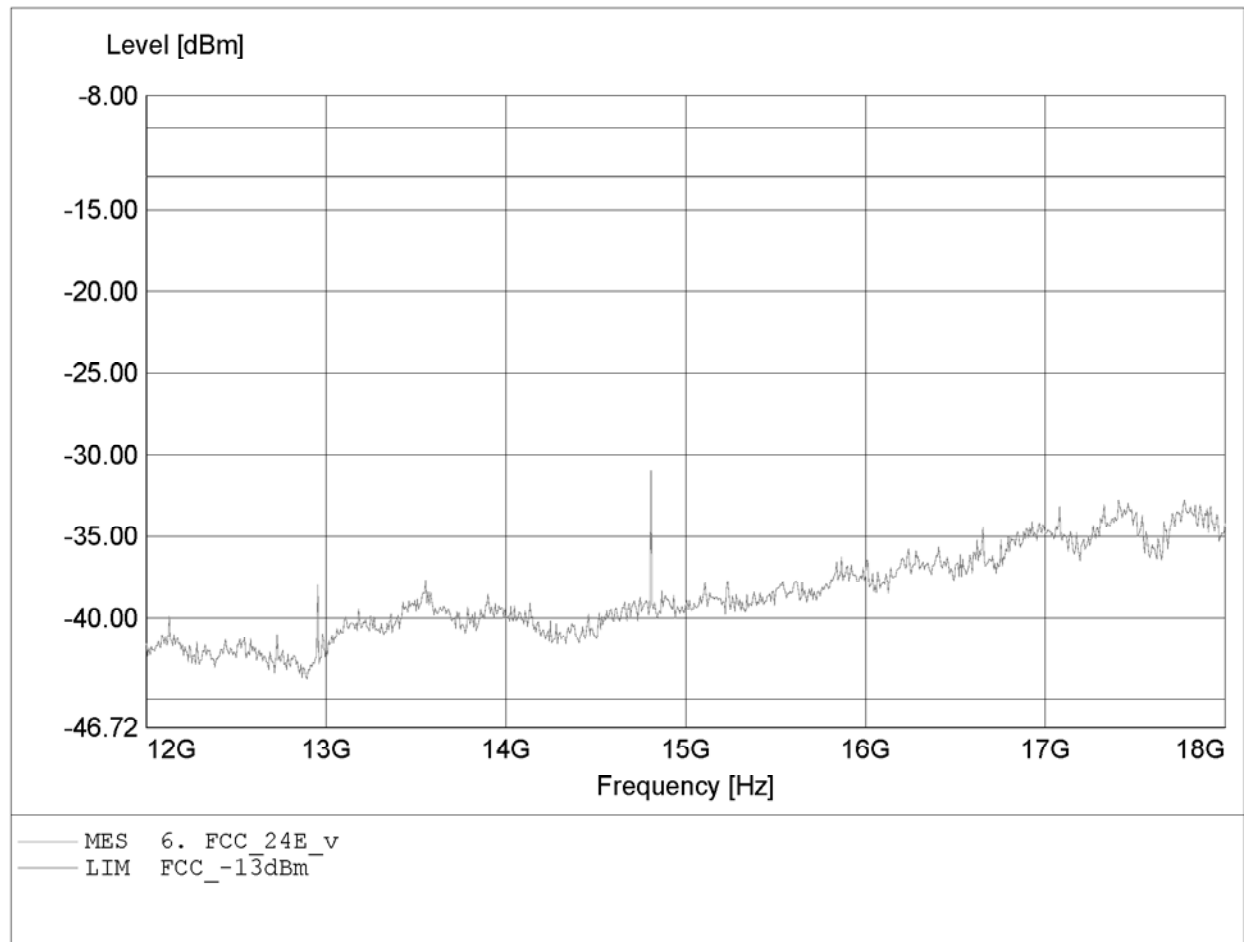


Radiated Emissions Tx
FCC RULES PART 24 SUBPART E

Approval Holder: BIOTRONIK GmbH & CO. KG
EUT : TELEX III
Model / Channel : CARDIOMESSENGER II / 512
Temperature/ Voltage: Temp.: 23°C / Unom.: 4.20 V DC
Test Site / Operator: ETS / Mr. Handrik
Test Specification: according to §24.238
Comment 1: Dist.: 3m, Ant.: HL025, ampl.+HP.
Comment 2: Freq: 14.807GHz, Pmax: -30.95dBm, RBW: 1MHz

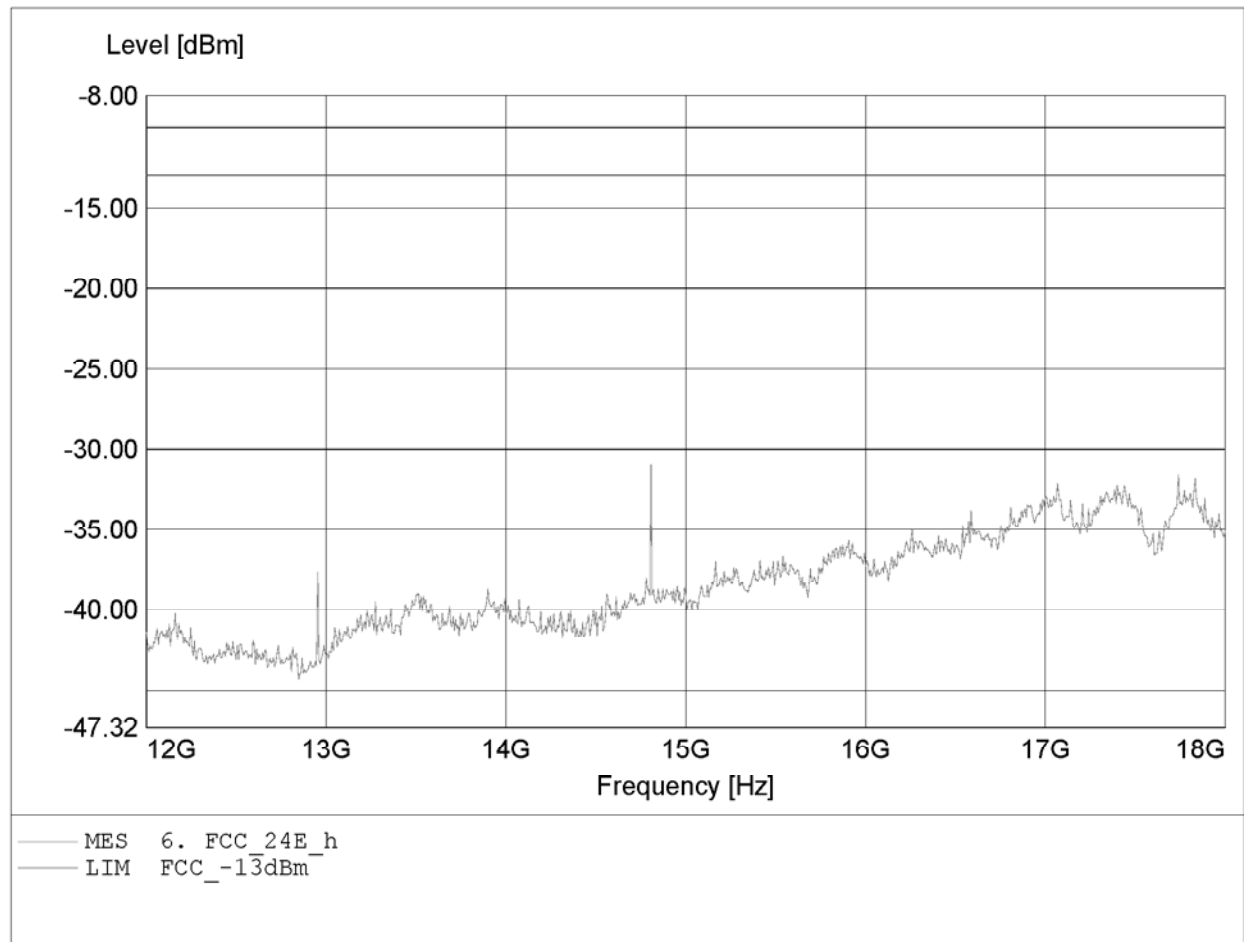


Radiated Emissions Tx
FCC RULES PART 24 SUBPART E

Approval Holder: BIOTRONIK GmbH & CO. KG
EUT : TELEX III
Model / Channel : CARDIOMESSENGER II / 512
Temperature/ Voltage: Temp.: 23°C / Unom.: 4.20 V DC
Test Site / Operator: ETS / Mr. Handrik
Test Specification: according to §24.238
Comment 1: Dist.: 3m, Ant.: HL025, amplif.
Comment 2: Freq: 18.425GHz, Pmax: -22.39dBm, RBW: 1MHz

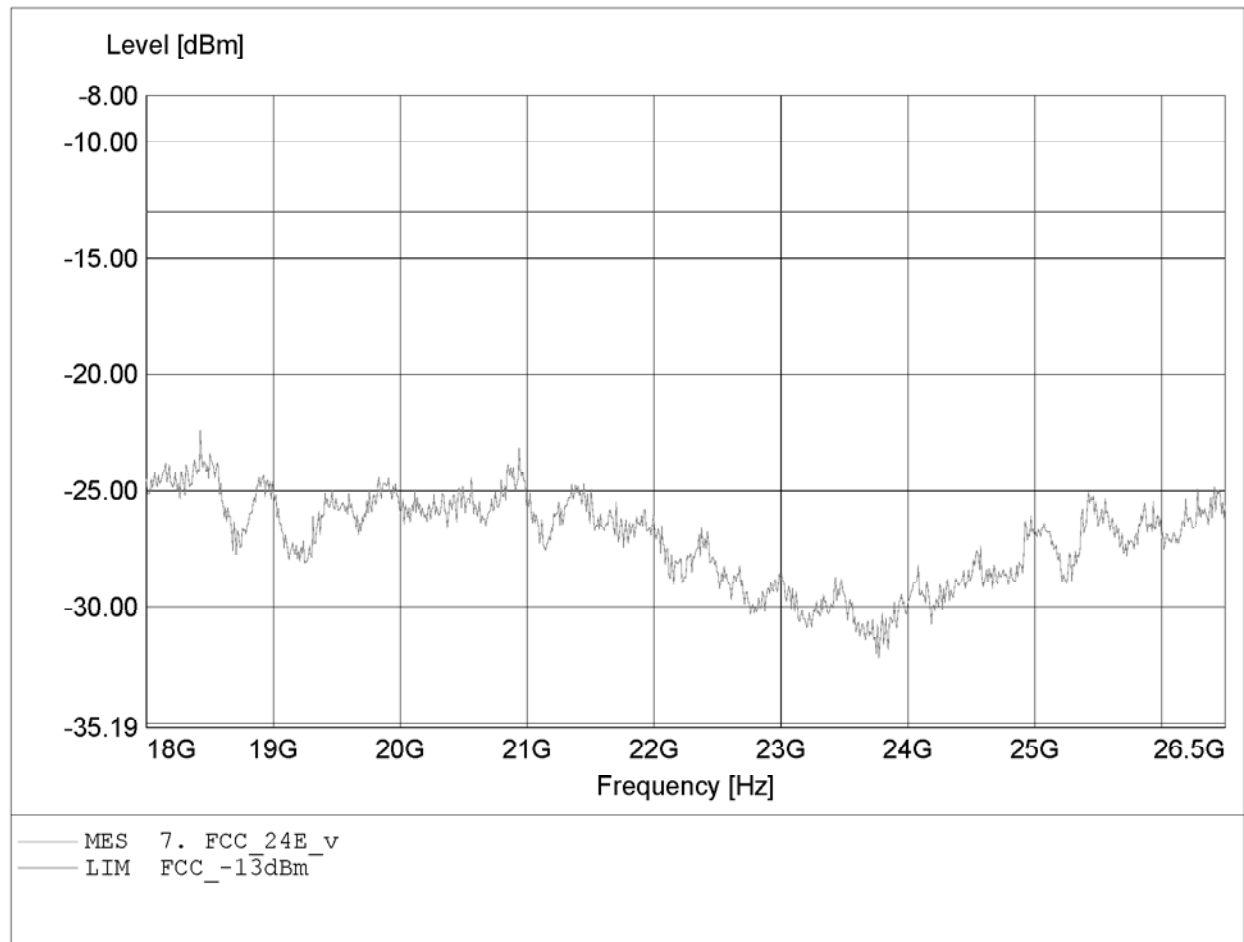


Radiated Emissions Tx
FCC RULES PART 24 SUBPART E

Approval Holder: BIOTRONIK GmbH & CO. KG
EUT : TELEX III
Model / Channel : CARDIOMESSENGER II / 512
Temperature/ Voltage: Temp.: 23°C / Unom.: 4.20 V DC
Test Site / Operator: ETS / Mr. Handrik
Test Specification: according to §24.238
Comment 1: Dist.: 3m, Ant.: HL025, amplif.
Comment 2: Freq: 19.946GHz, Pmax: -23.45dBm, RBW: 1MHz

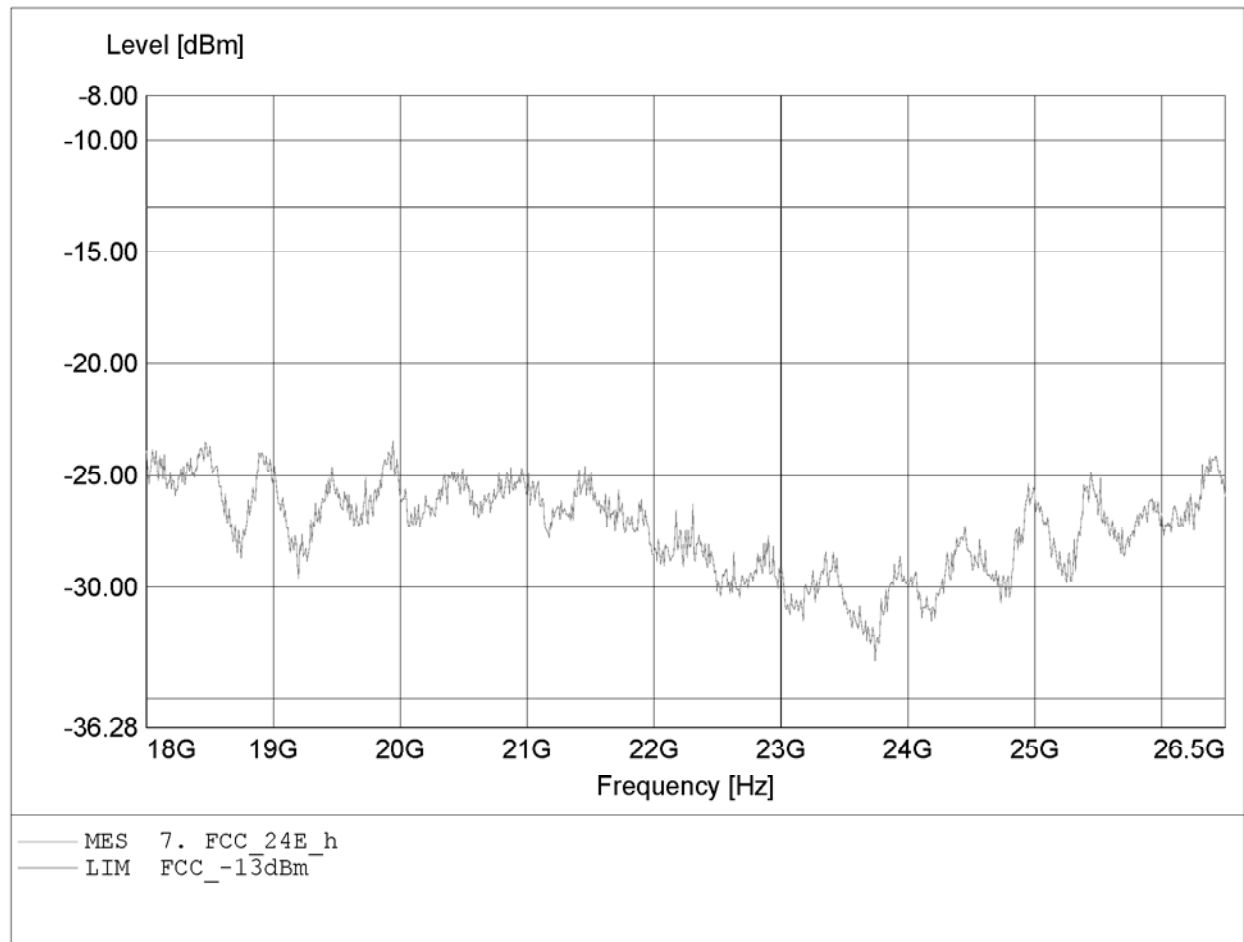


Radiated Emissions Tx
FCC RULES PART 24 SUBPART E

Approval Holder: BIOTRONIK GmbH & CO. KG
EUT : TELEX III
Model / Channel : CARDIOMESSENGER II / 661
Temperature/ Voltage: Temp.: 23°C / Unom.: 4.20 V DC
Test Site / Operator: ETS / Mr. Handrik
Test Specification: according to §24.238
Comment 1: Dist.: 3m, Ant.: HK 116
Comment 2: Freq: 59.656MHz, Pmax: -52.28dBm, RBW: 1MHz

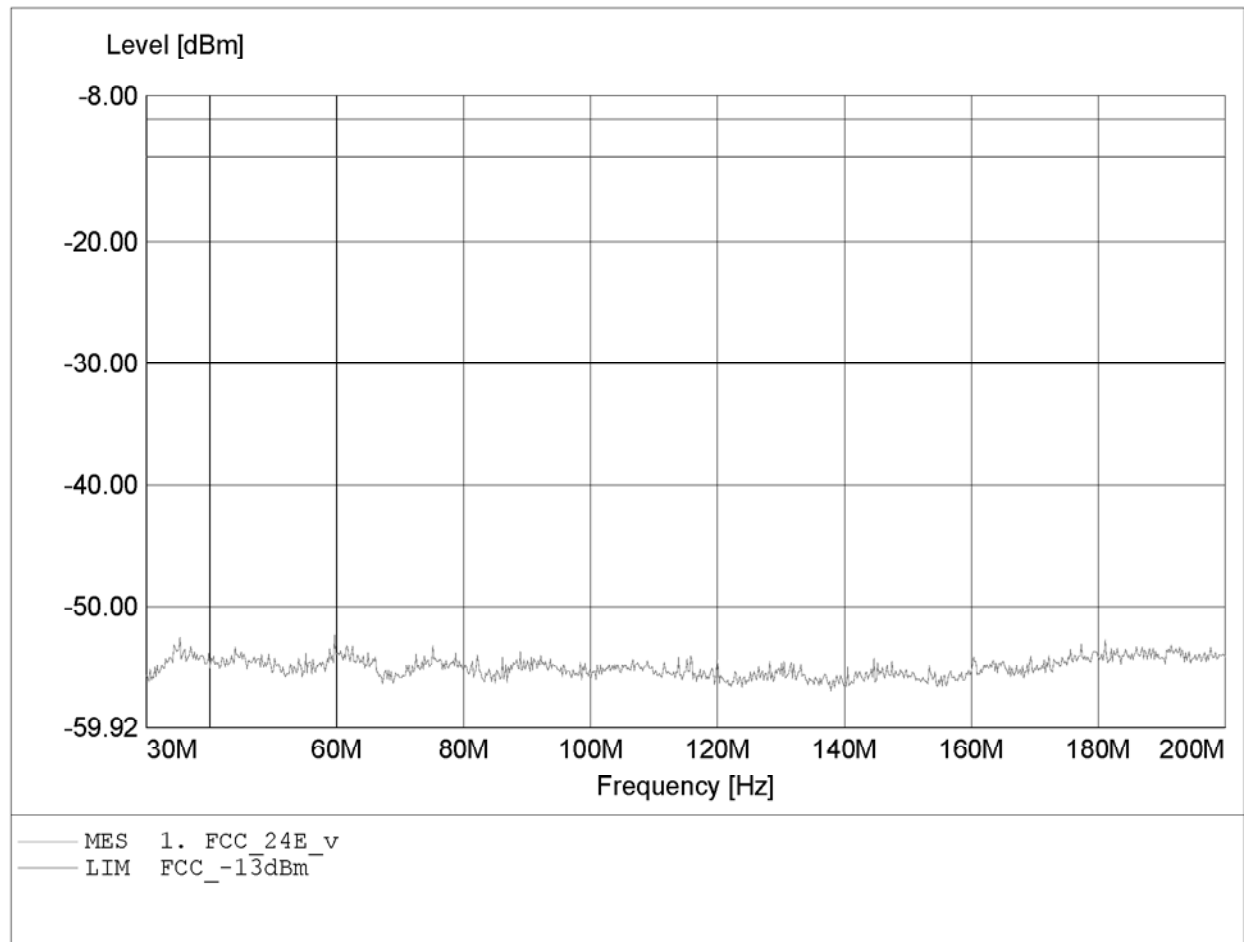


Radiated Emissions Tx
FCC RULES PART 24 SUBPART E

Approval Holder: BIOTRONIK GmbH & CO. KG
EUT : TELEX III
Model / Channel : CARDIOMESSENGER II / 661
Temperature/ Voltage: Temp.: 23°C / Unom.: 4.20 V DC
Test Site / Operator: ETS / Mr. Handrik
Test Specification: according to §24.238
Comment 1: Dist.: 3m, Ant.: HK 116
Comment 2: Freq: 75.144MHz, Pmax: -41.45dBm, RBW: 1MHz

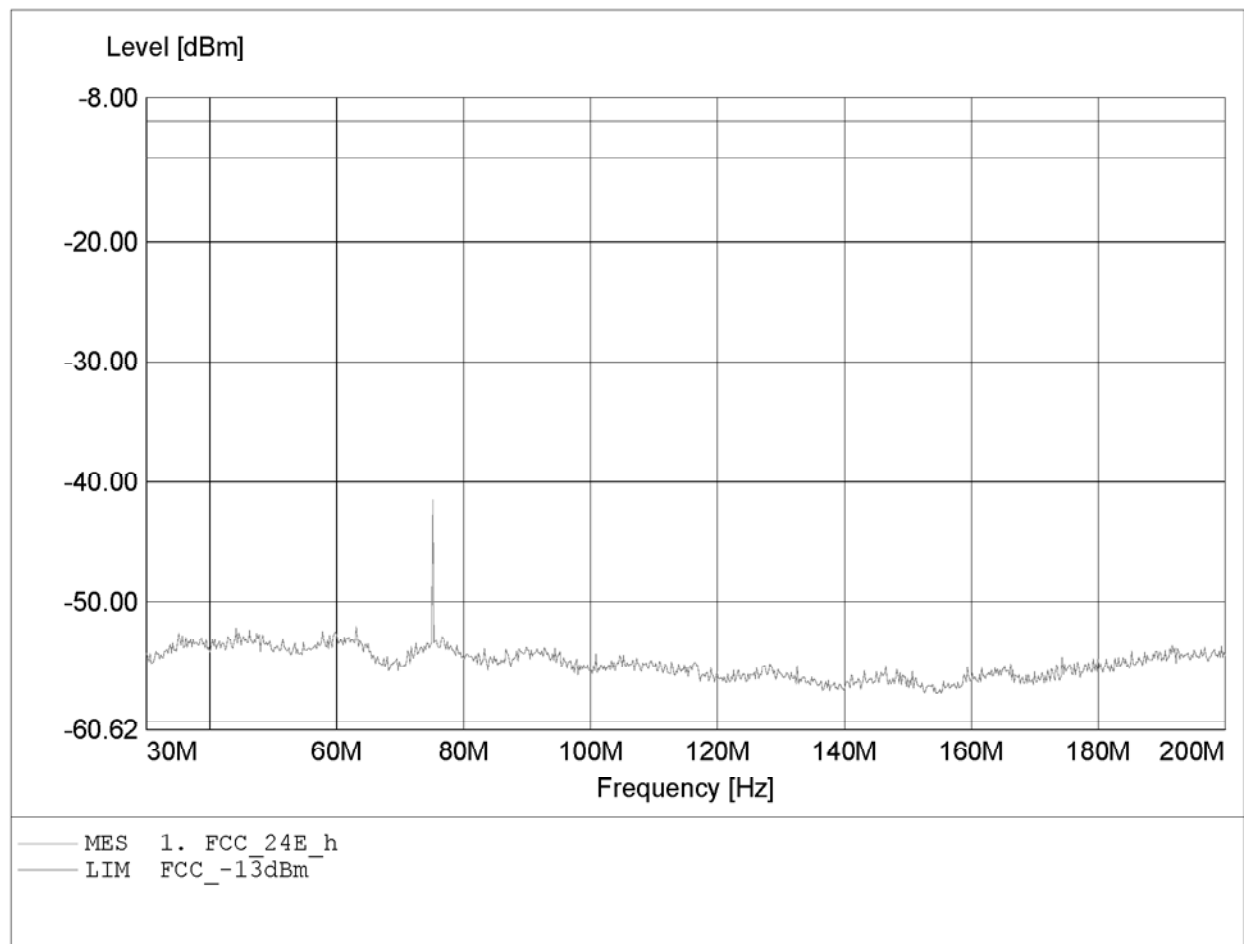


Radiated Emissions Tx
FCC RULES PART 24 SUBPART E

Approval Holder: BIOTRONIK GmbH & CO. KG
EUT : TELEX III
Model / Channel : CARDIOMESSENGER II / 661
Temperature/ Voltage: Temp.: 23°C / Unom.: 4.20 V DC
Test Site / Operator: ETS / Mr. Handrik
Test Specification: according to §24.238
Comment 1: Dist.: 3m, Ant.: HL 223
Comment 2: Freq: 989.333MHz, Pmax: -39.43dBm, RBW: 1MHz

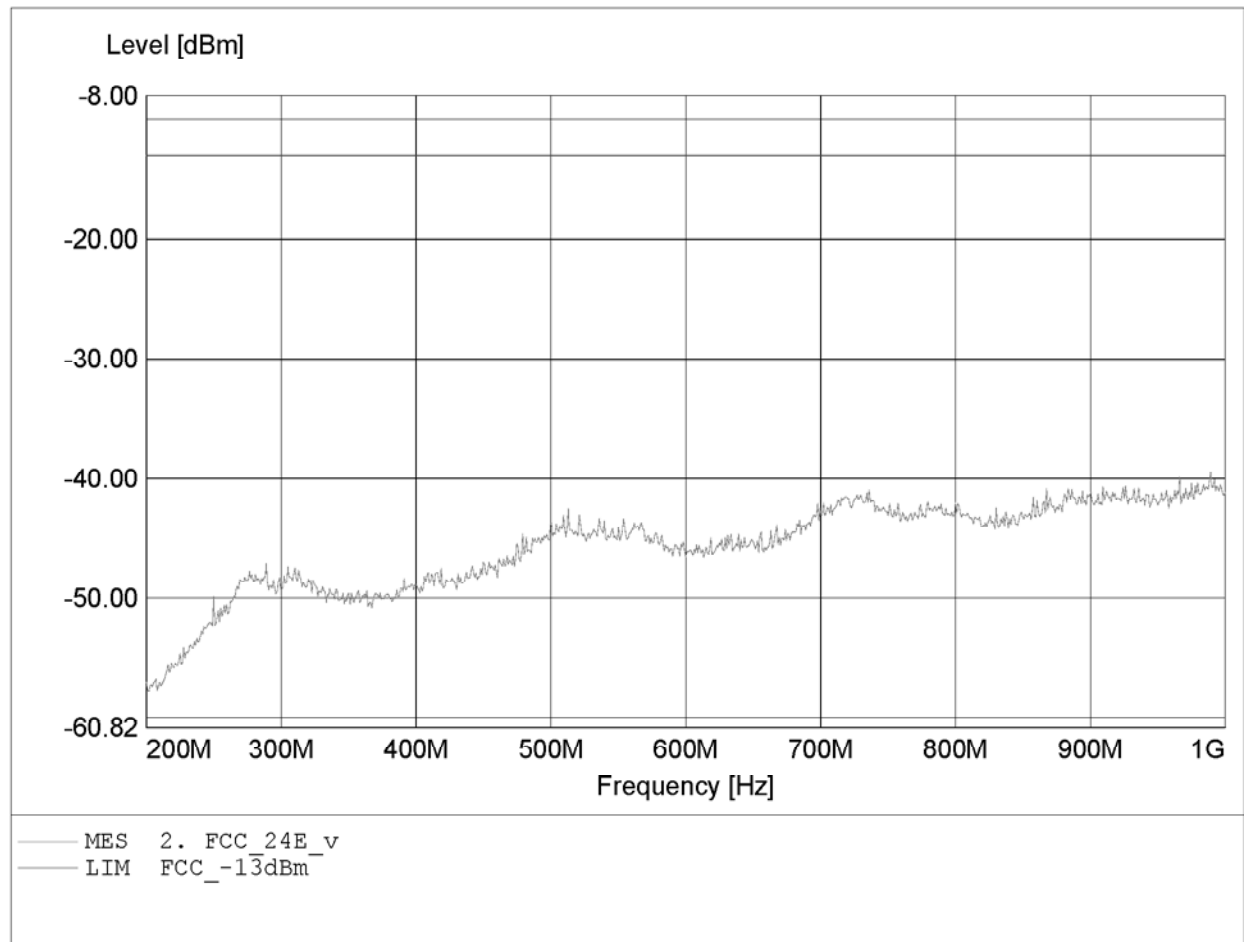


Radiated Emissions Tx
FCC RULES PART 24 SUBPART E

Approval Holder: BIOTRONIK GmbH & CO. KG
EUT : TELEX III
Model / Channel : CARDIOMESSENGER II / 661
Temperature/ Voltage: Temp.: 23°C / Unom.: 4.20 V DC
Test Site / Operator: ETS / Mr. Handrik
Test Specification: according to §24.238
Comment 1: Dist.: 3m, Ant.: HL 223
Comment 2: Freq: 843.556MHz, Pmax: -37.19dBm, RBW: 1MHz

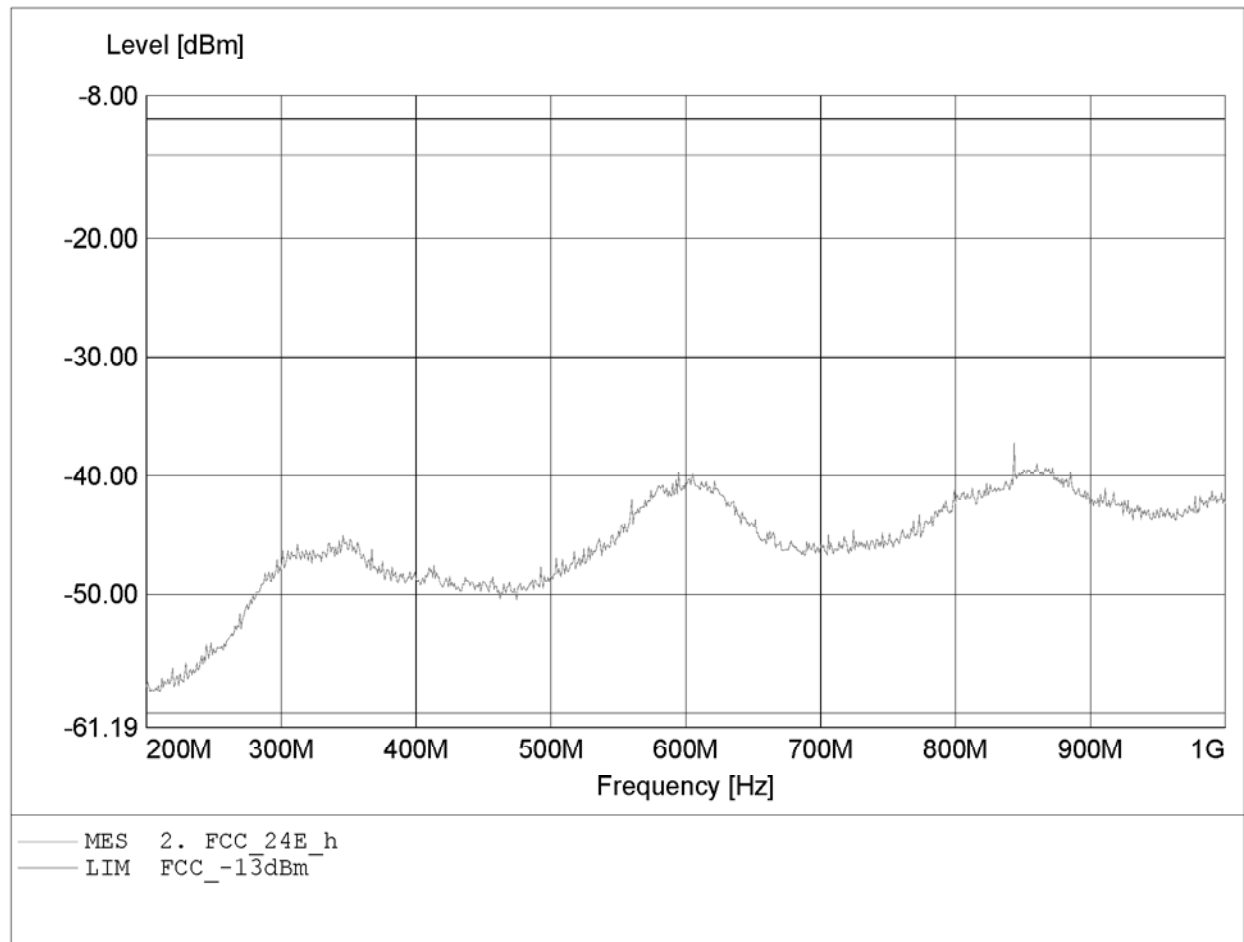


Radiated Emissions Tx
FCC RULES PART 24 SUBPART E

Approval Holder: BIOTRONIK GmbH & CO. KG
EUT : TELEX III
Model / Channel : CARDIOMESSENGER II / 661
Temperature/ Voltage: Temp.: 23°C / Unom.: 4.20 V DC
Test Site / Operator: ETS / Mr. Handrik
Test Specification: according to §24.238
Comment 1: Dist.: 3m, Ant.: HL025
Comment 2: Freq: 3.641GHz, Pmax: -20.99dBm, RBW: 1MHz/3kHz

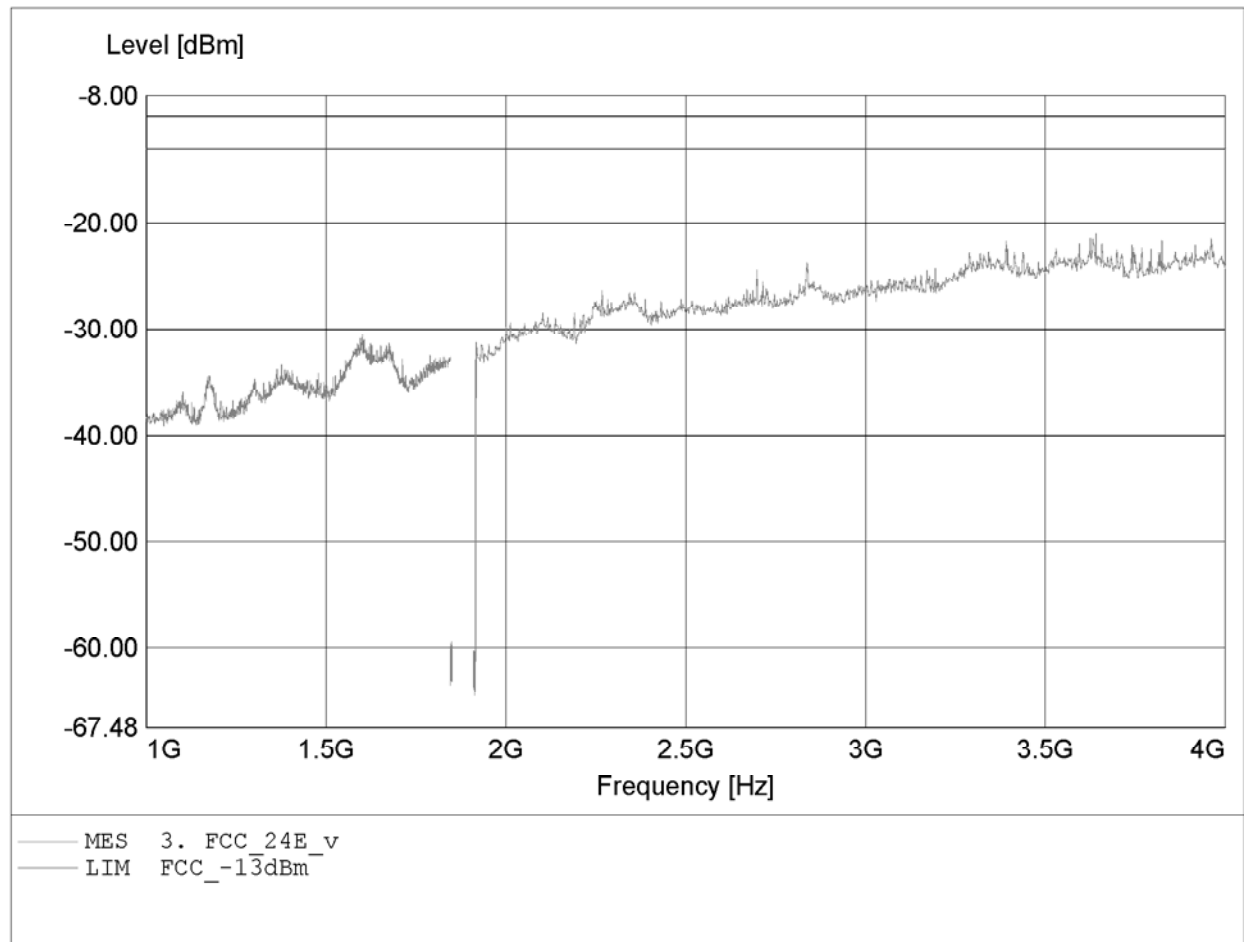


Radiated Emissions Tx
FCC RULES PART 24 SUBPART E

Approval Holder: BIOTRONIK GmbH & CO. KG
EUT : TELEX III
Model / Channel : CARDIOMESSENGER II / 661
Temperature/ Voltage: Temp.: 23°C / Unom.: 4.20 V DC
Test Site / Operator: ETS / Mr. Handrik
Test Specification: according to §24.238
Comment 1: Dist.: 3m, Ant.: HL025
Comment 2: Freq: 3.386GHz, Pmax: -22.76dBm, RBW: 1MHz/3kHz

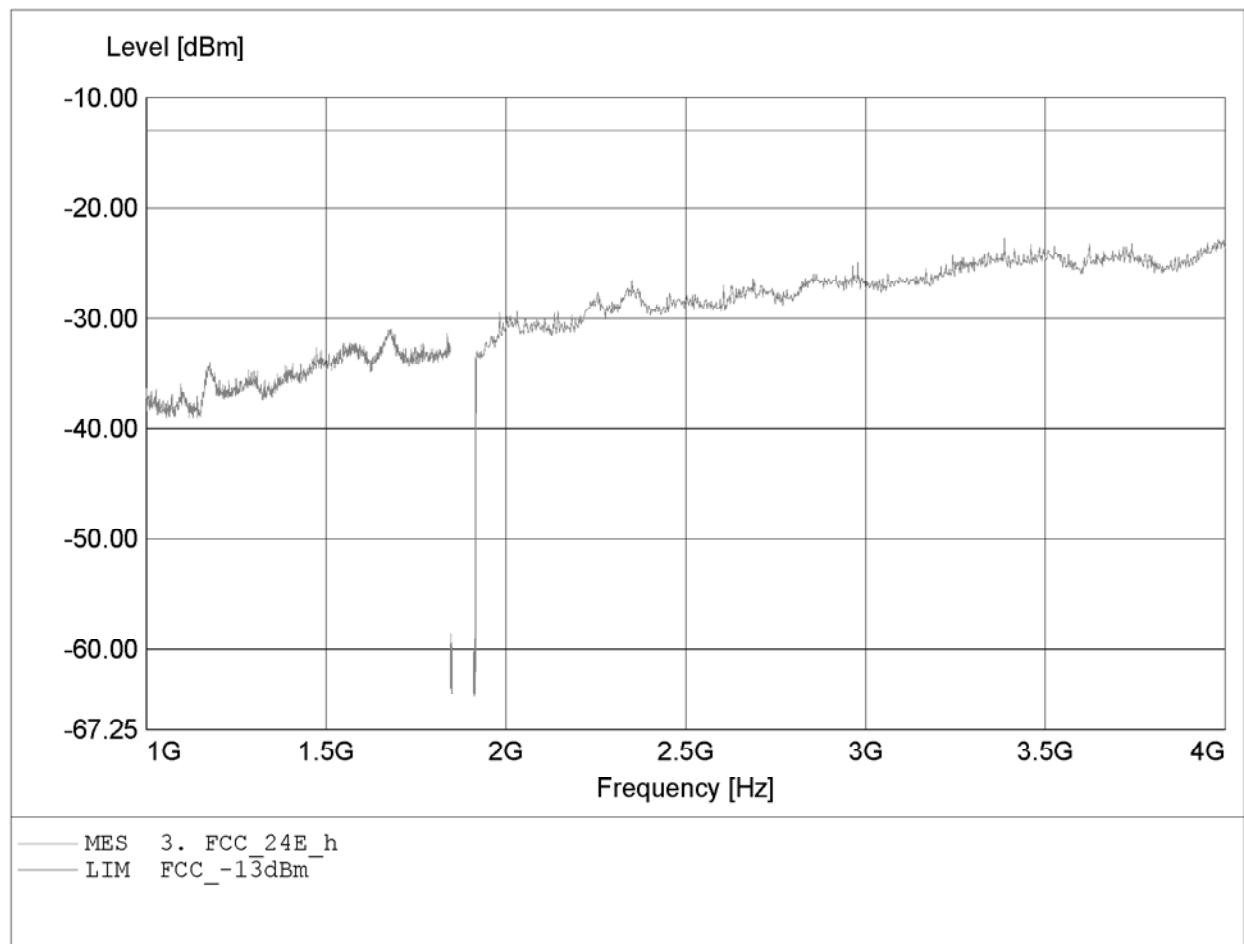


Radiated Emissions Tx
FCC RULES PART 24 SUBPART E

Approval Holder: BIOTRONIK GmbH & CO. KG
EUT : TELEX III
Model / Channel : CARDIOMESSENGER II / 661
Temperature/ Voltage: Temp.: 23°C / Unom.: 4.20 V DC
Test Site / Operator: ETS / Mr. Handrik
Test Specification: according to §24.238
Comment 1: Dist.: 3m, Ant.: HL025, ampl.+HP.
Comment 2: Freq: 7.987GHz, Pmax: -45.17dBm, RBW: 1MHz

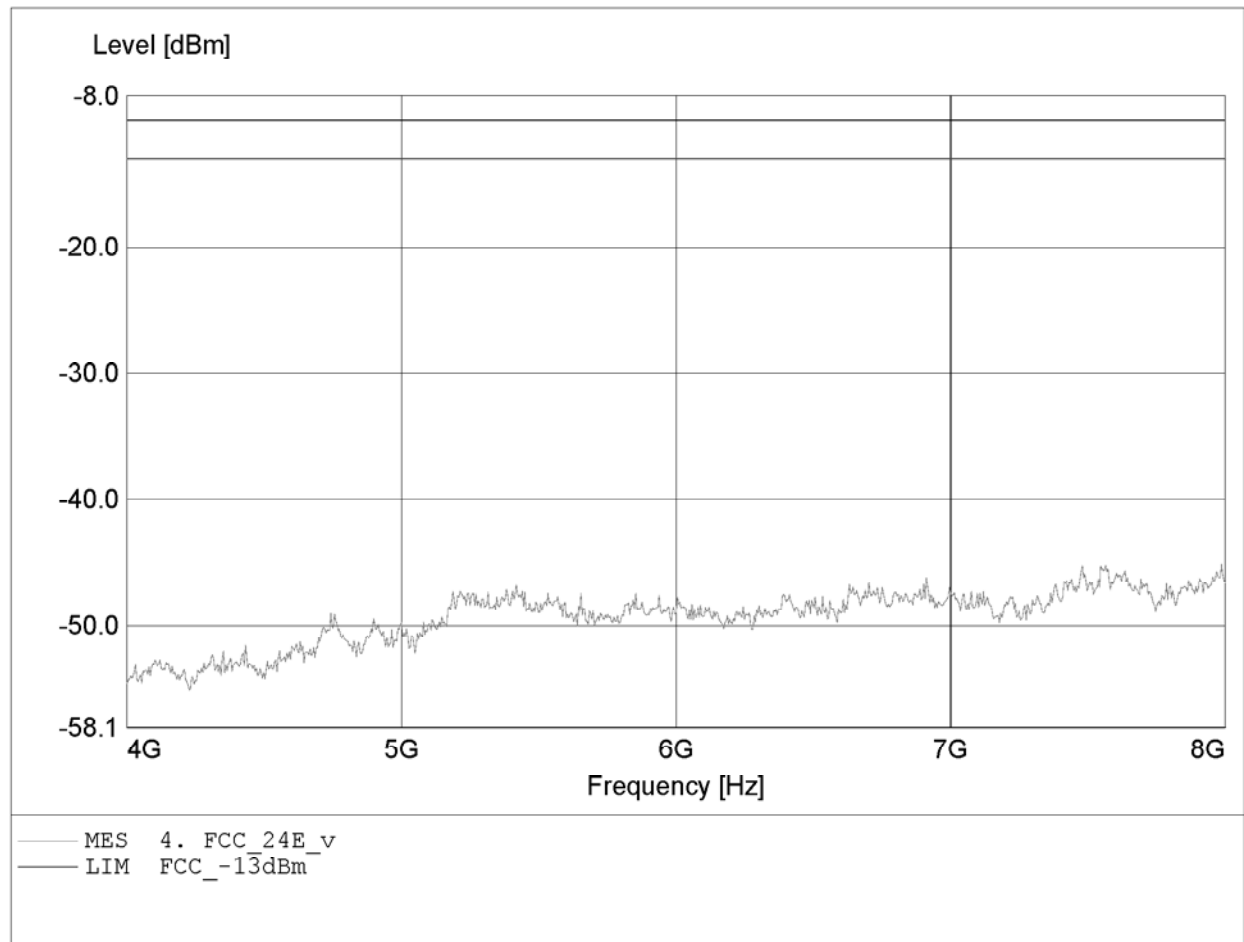


Radiated Emissions Tx
FCC RULES PART 24 SUBPART E

Approval Holder: BIOTRONIK GmbH & CO. KG
EUT : TELEX III
Model / Channel : CARDIOMESSENGER II / 661
Temperature/ Voltage: Temp.: 23°C / Unom.: 4.20 V DC
Test Site / Operator: ETS / Mr. Handrik
Test Specification: according to §24.238
Comment 1: Dist.: 3m, Ant.: HL025, ampl.+HP.
Comment 2: Freq: 7.960GHz, Pmax: -44.91dBm, RBW: 1MHz

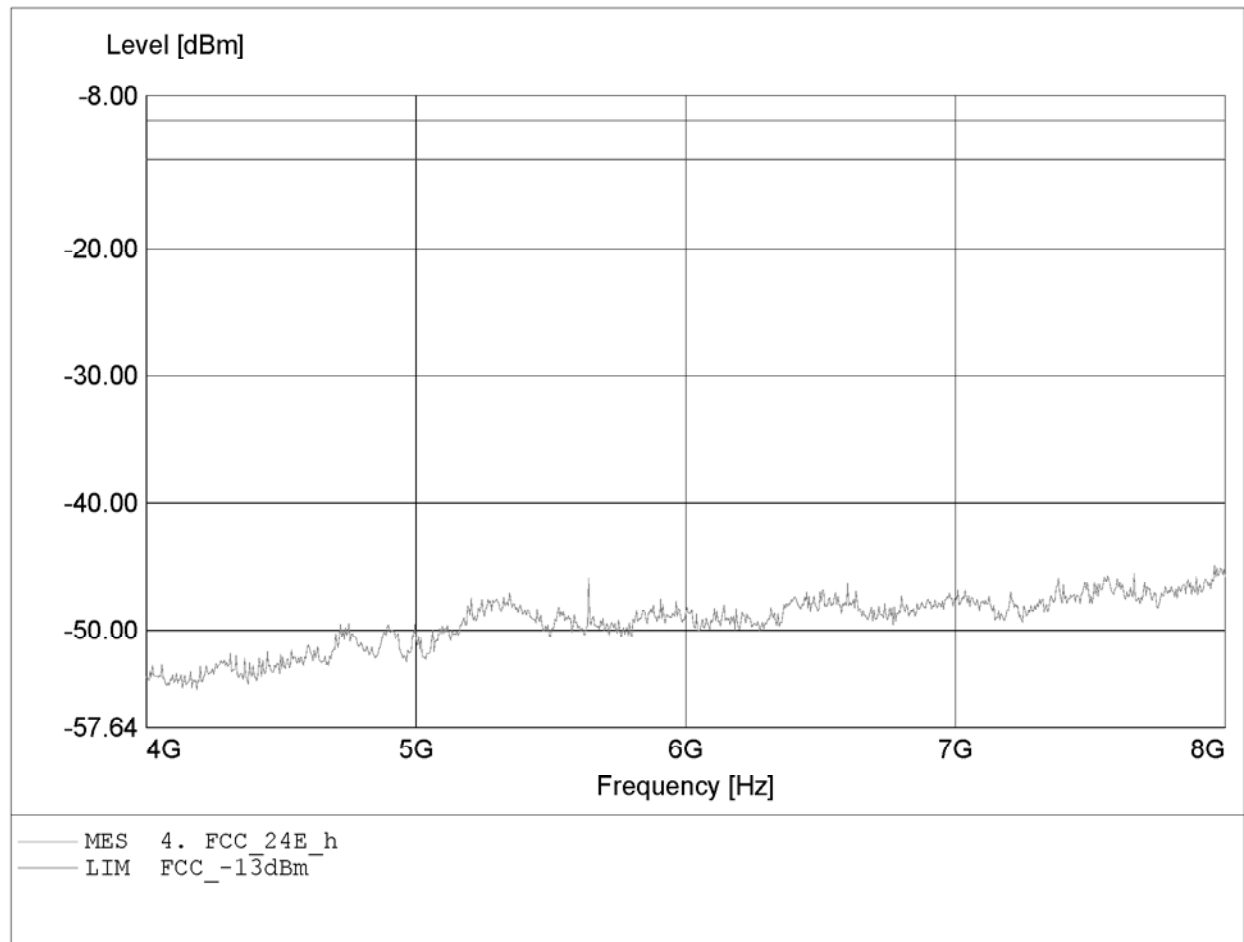


Radiated Emissions Tx
FCC RULES PART 24 SUBPART E

Approval Holder: BIOTRONIK GmbH & CO. KG
EUT : TELEX III
Model / Channel : CARDIOMESSENGER II / 661
Temperature/ Voltage: Temp.: 23°C / Unom.: 4.20 V DC
Test Site / Operator: ETS / Mr. Handrik
Test Specification: according to §24.238
Comment 1: Dist.: 3m, Ant.: HL025, ampl.+HP.
Comment 2: Freq: 9.404GHz, Pmax: -36.69dBm, RBW: 1MHz

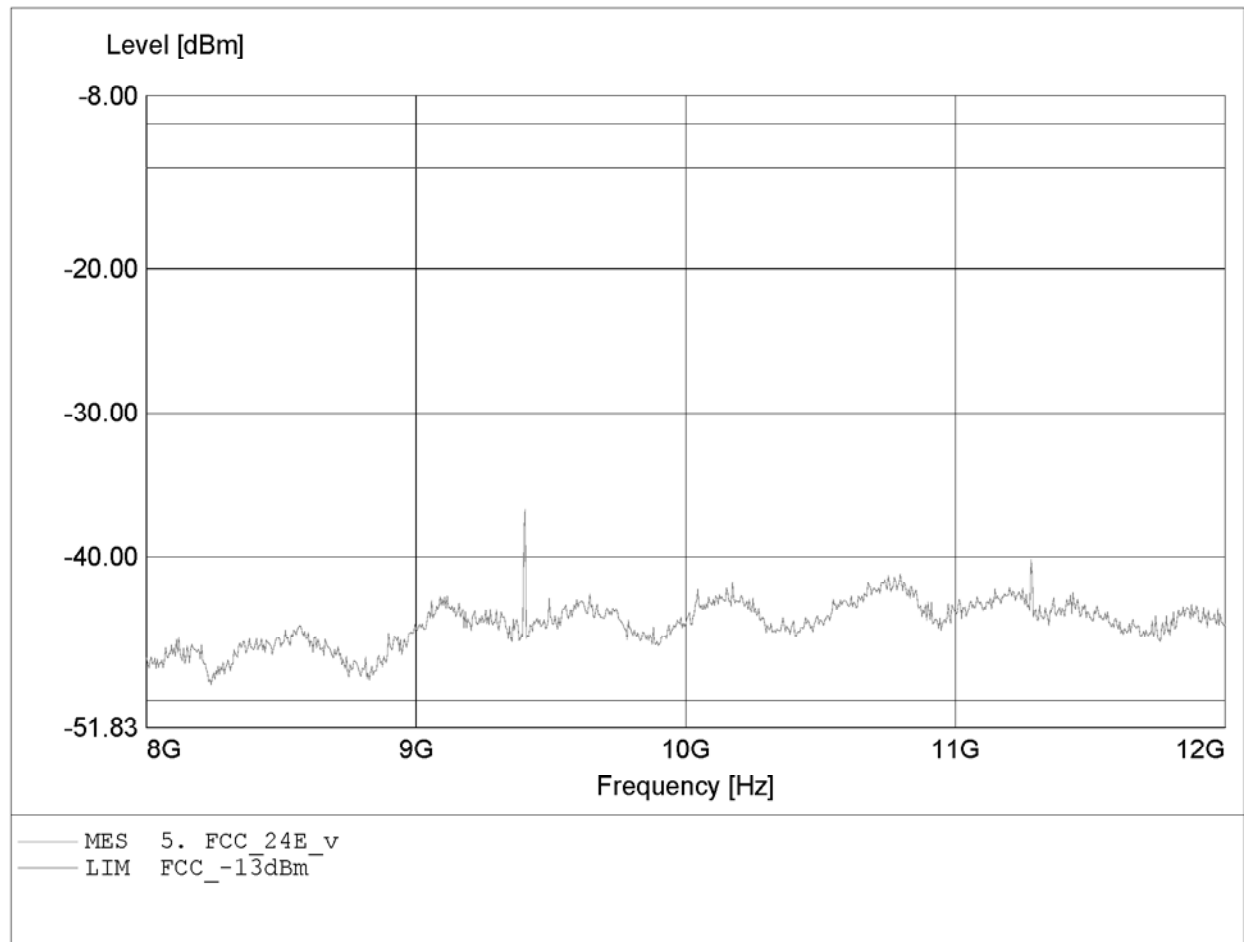


Radiated Emissions Tx
FCC RULES PART 24 SUBPART E

Approval Holder: BIOTRONIK GmbH & CO. KG
EUT : TELEX III
Model / Channel : CARDIOMESSENGER II / 661
Temperature/ Voltage: Temp.: 23°C / Unom.: 4.20 V DC
Test Site / Operator: ETS / Mr. Handrik
Test Specification: according to §24.238
Comment 1: Dist.: 3m, Ant.: HL025, ampl.+HP.
Comment 2: Freq: 9.404GHz, Pmax: -36.80dBm, RBW: 1MHz

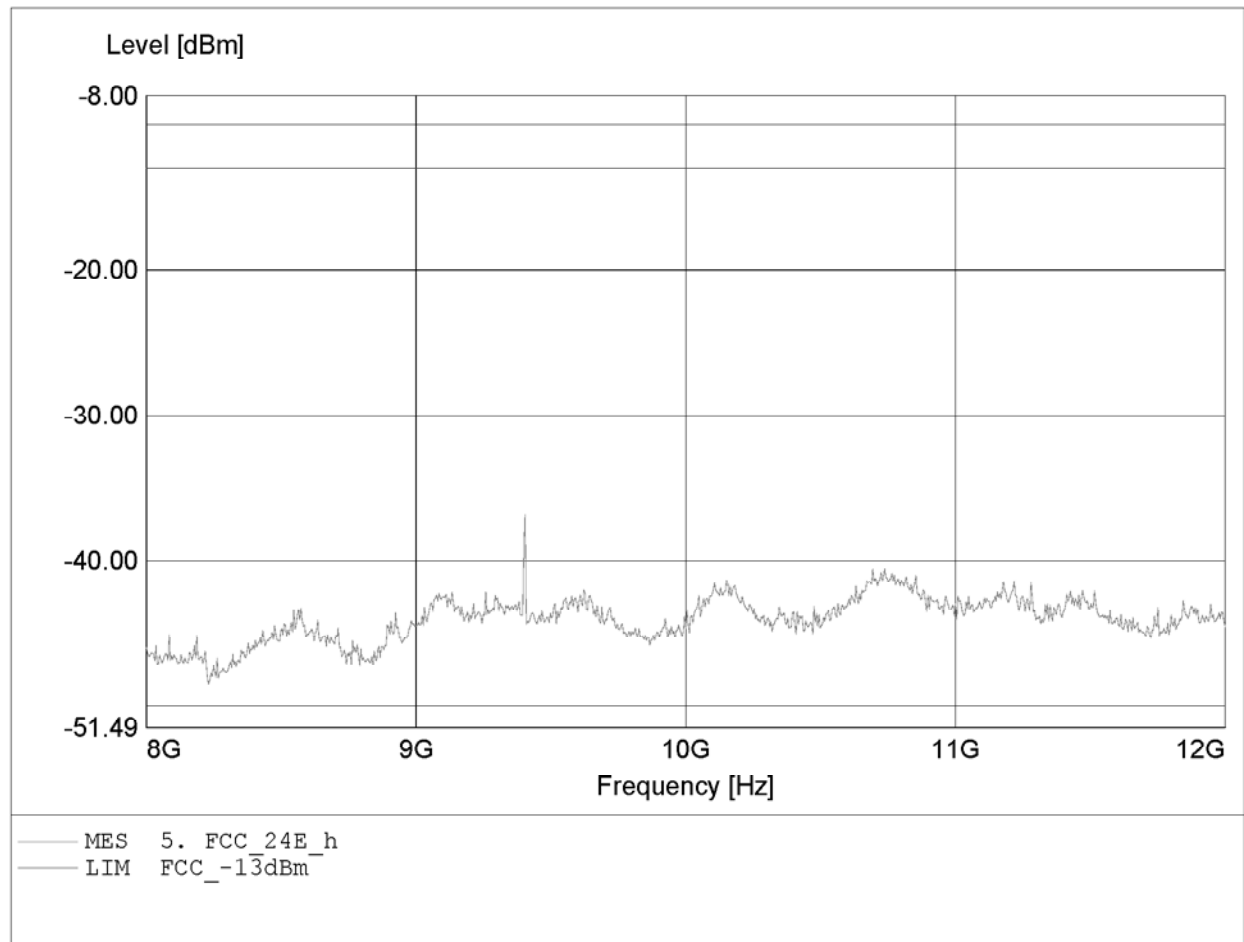


Radiated Emissions Tx
FCC RULES PART 24 SUBPART E

Approval Holder: BIOTRONIK GmbH & CO. KG
EUT : TELEX III
Model / Channel : CARDIOMESSENGER II / 661
Temperature/ Voltage: Temp.: 23°C / Unom.: 4.20 V DC
Test Site / Operator: ETS / Mr. Handrik
Test Specification: according to §24.238
Comment 1: Dist.: 3m, Ant.: HL025, ampl.+HP.
Comment 2: Freq: 15.047GHz, Pmax: -29.06dBm, RBW: 1MHz

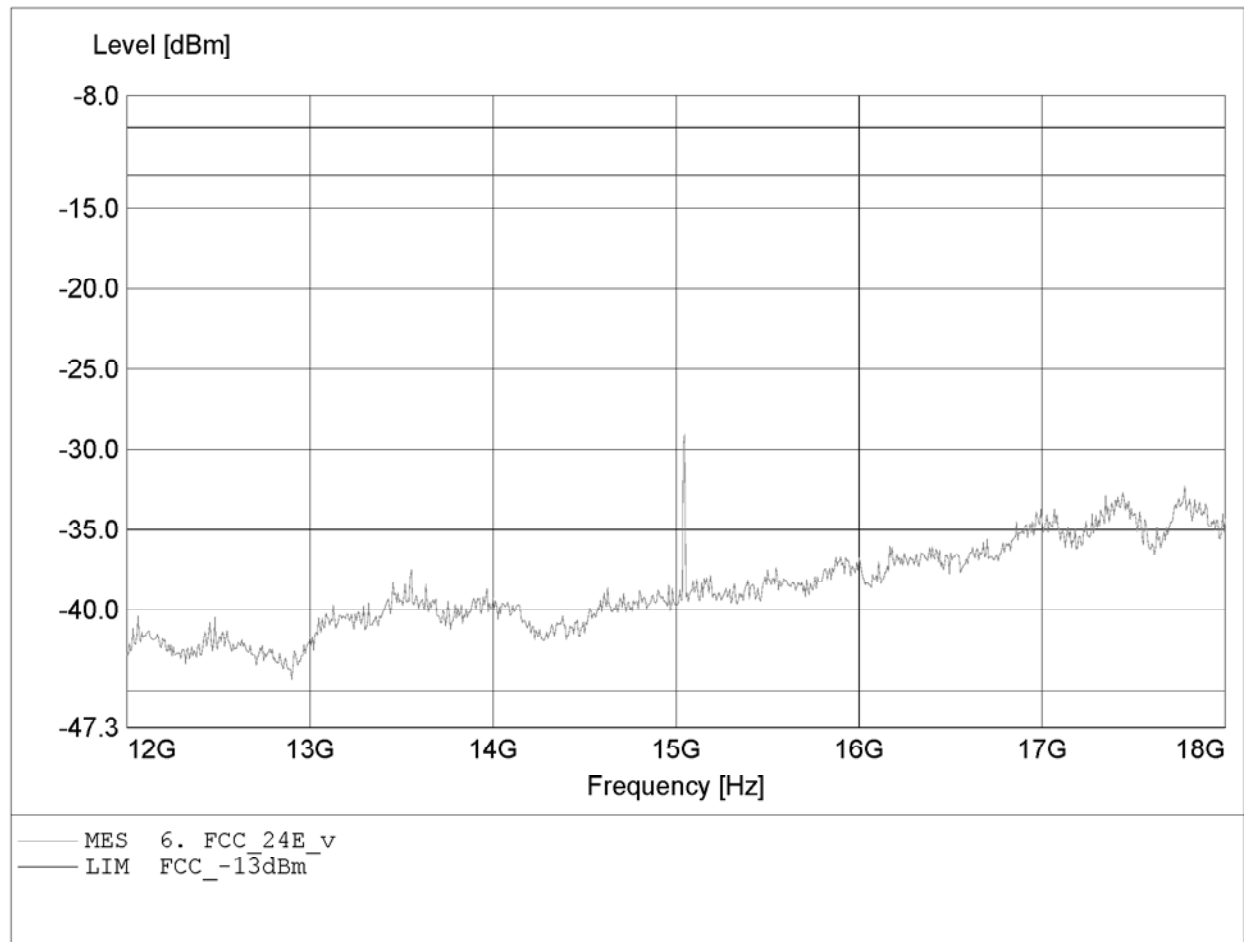


Radiated Emissions Tx
FCC RULES PART 24 SUBPART E

Approval Holder: BIOTRONIK GmbH & CO. KG
EUT : TELEX III
Model / Channel : CARDIOMESSENGER II / 661
Temperature/ Voltage: Temp.: 23°C / Unom.: 4.20 V DC
Test Site / Operator: ETS / Mr. Handrik
Test Specification: according to §24.238
Comment 1: Dist.: 3m, Ant.: HL025, ampl.+HP.
Comment 2: Freq: 14.807GHz, Pmax: -27.39dBm, RBW: 1MHz

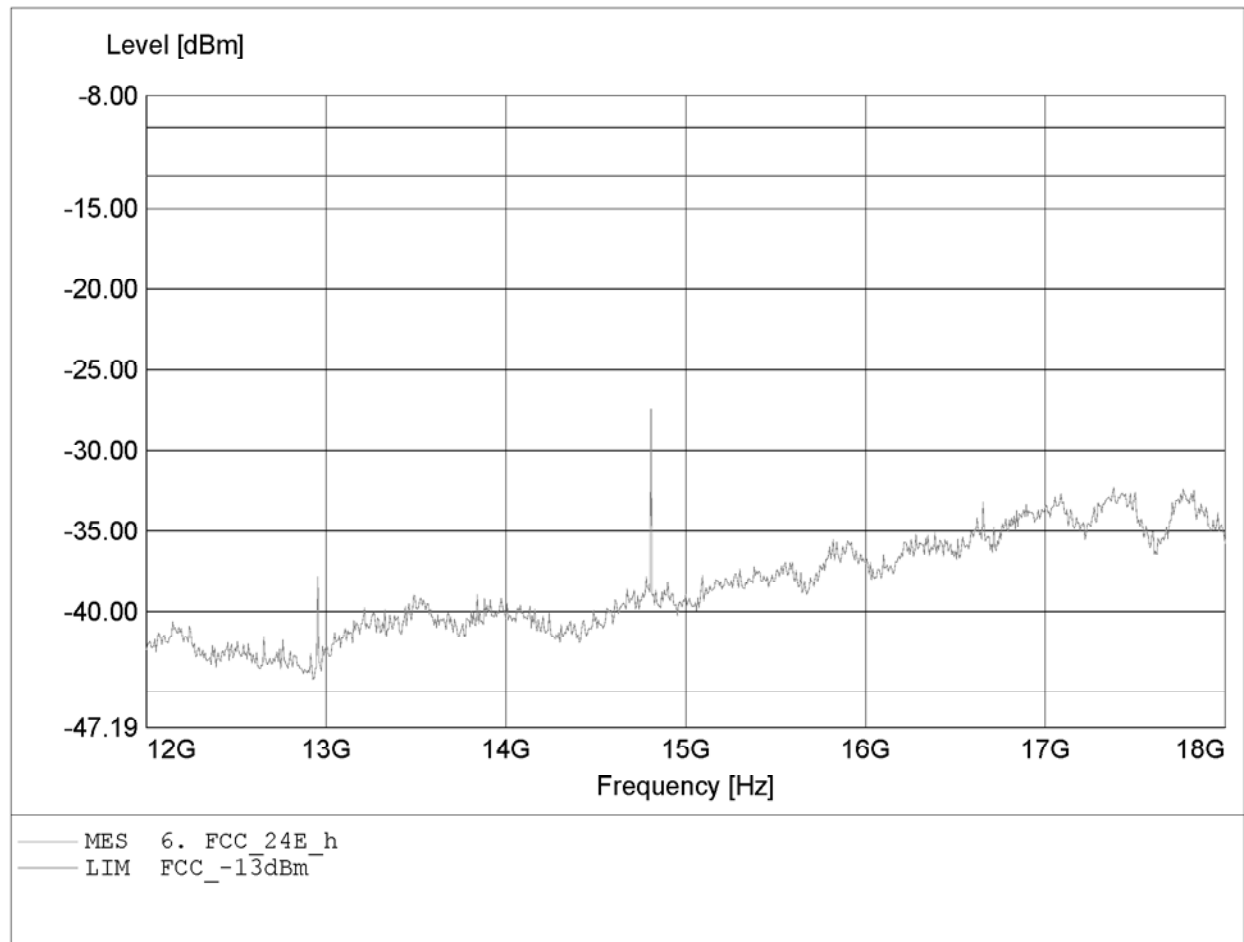


Radiated Emissions Tx
FCC RULES PART 24 SUBPART E

Approval Holder: BIOTRONIK GmbH & CO. KG
EUT : TELEX III
Model / Channel : CARDIOMESSENGER II / 661
Temperature/ Voltage: Temp.: 23°C / Unom.: 4.20 V DC
Test Site / Operator: ETS / Mr. Handrik
Test Specification: according to §24.238
Comment 1: Dist.: 3m, Ant.: HL025, amplif.
Comment 2: Freq: 18.416GHz, Pmax: -23.41dBm, RBW: 1MHz

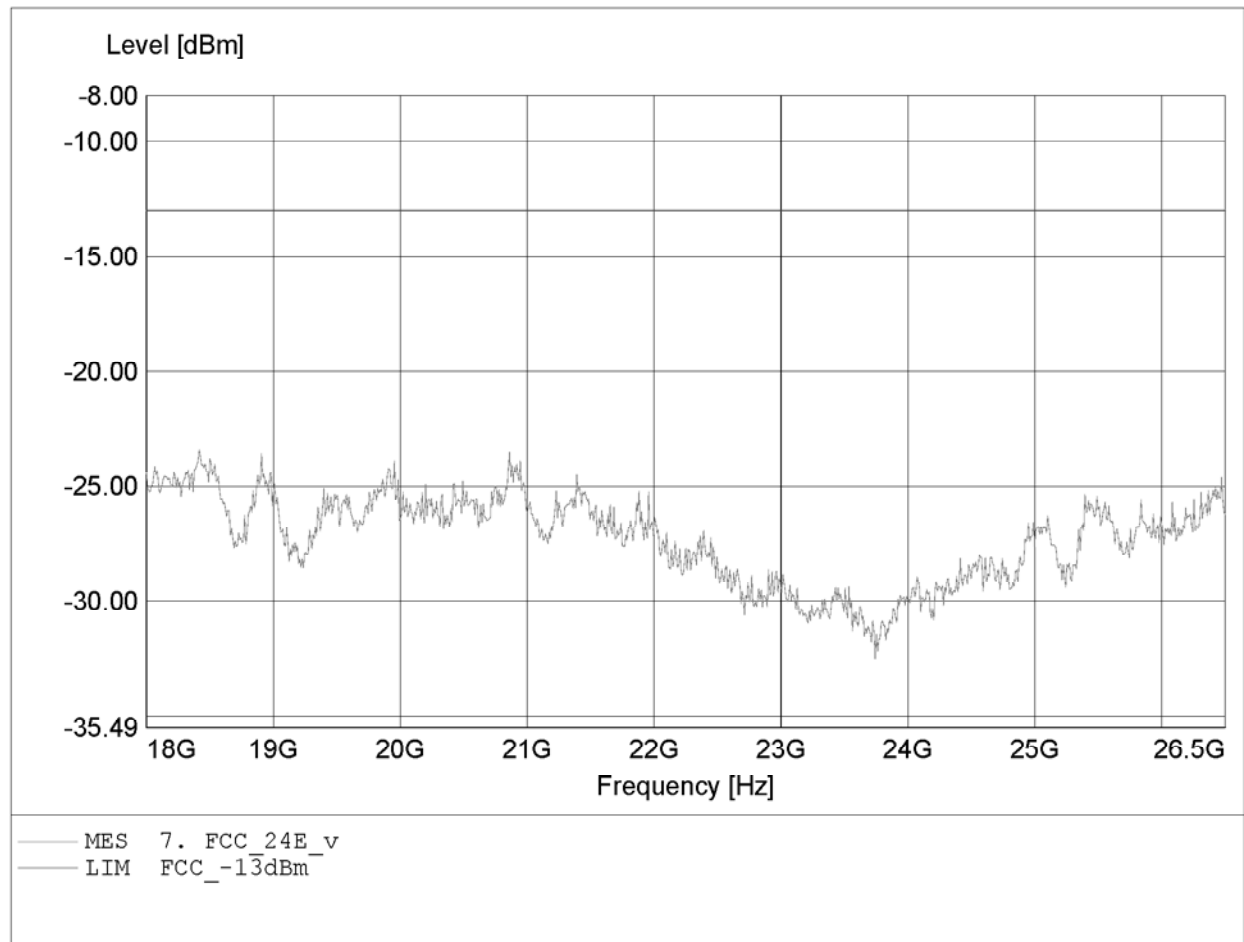


Radiated Emissions Tx
FCC RULES PART 24 SUBPART E

Approval Holder: BIOTRONIK GmbH & CO. KG
EUT : TELEX III
Model / Channel : CARDIOMESSENGER II / 661
Temperature/ Voltage: Temp.: 23°C / Unom.: 4.20 V DC
Test Site / Operator: ETS / Mr. Handrik
Test Specification: according to §24.238
Comment 1: Dist.: 3m, Ant.: HL025, amplif.
Comment 2: Freq: 18.453GHz, Pmax: -23.23dBm, RBW: 1MHz

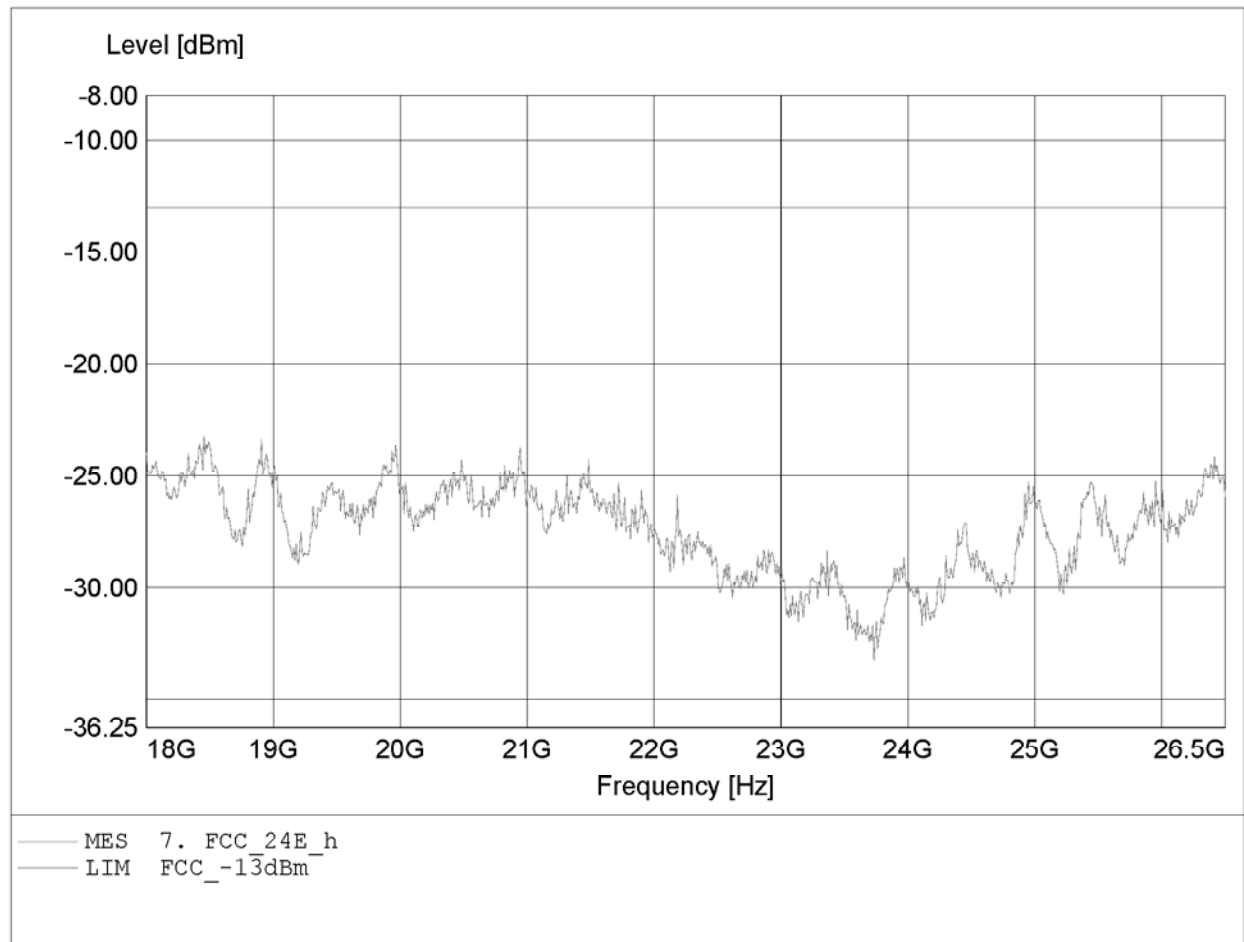


Radiated Emissions Tx
FCC RULES PART 24 SUBPART E

Approval Holder: BIOTRONIK GmbH & CO. KG
EUT : TELEX III
Model / Channel : CARDIOMESSENGER II / 810
Temperature/ Voltage: Temp.: 23°C / Unom.: 4.20 V DC
Test Site / Operator: ETS / Mr. Handrik
Test Specification: according to §24.238
Comment 1: Dist.: 3m, Ant.: HK 116
Comment 2: Freq: 179.600MHz, Pmax: -52.81dBm, RBW: 1MHz

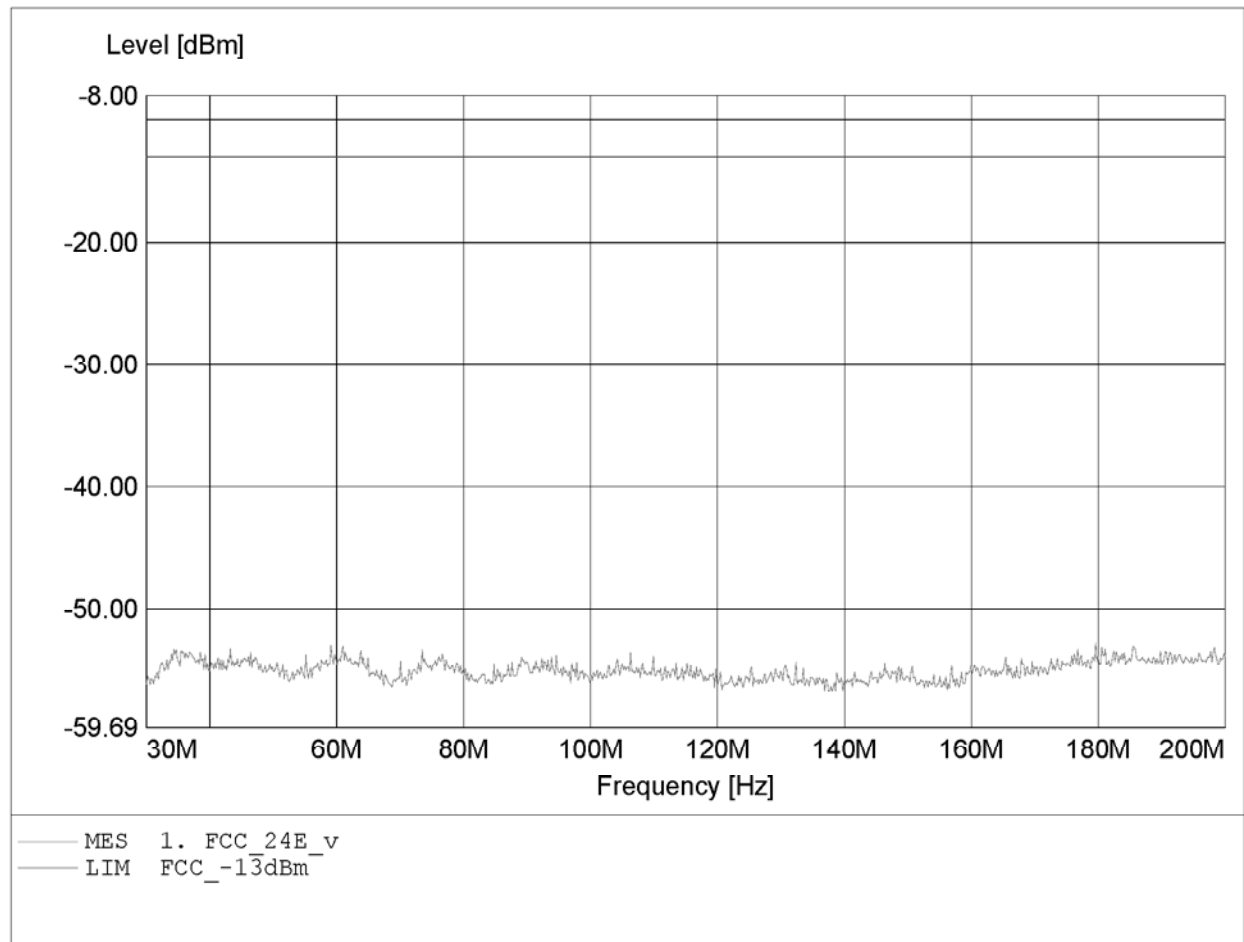


Radiated Emissions Tx
FCC RULES PART 24 SUBPART E

Approval Holder: BIOTRONIK GmbH & CO. KG
EUT : TELEX III
Model / Channel : CARDIOMESSENGER II / 810
Temperature/ Voltage: Temp.: 23°C / Unom.: 4.20 V DC
Test Site / Operator: ETS / Mr. Handrik
Test Specification: according to §24.238
Comment 1: Dist.: 3m, Ant.: HK 116
Comment 2: Freq: 46.244MHz, Pmax: -51.64dBm, RBW: 1MHz

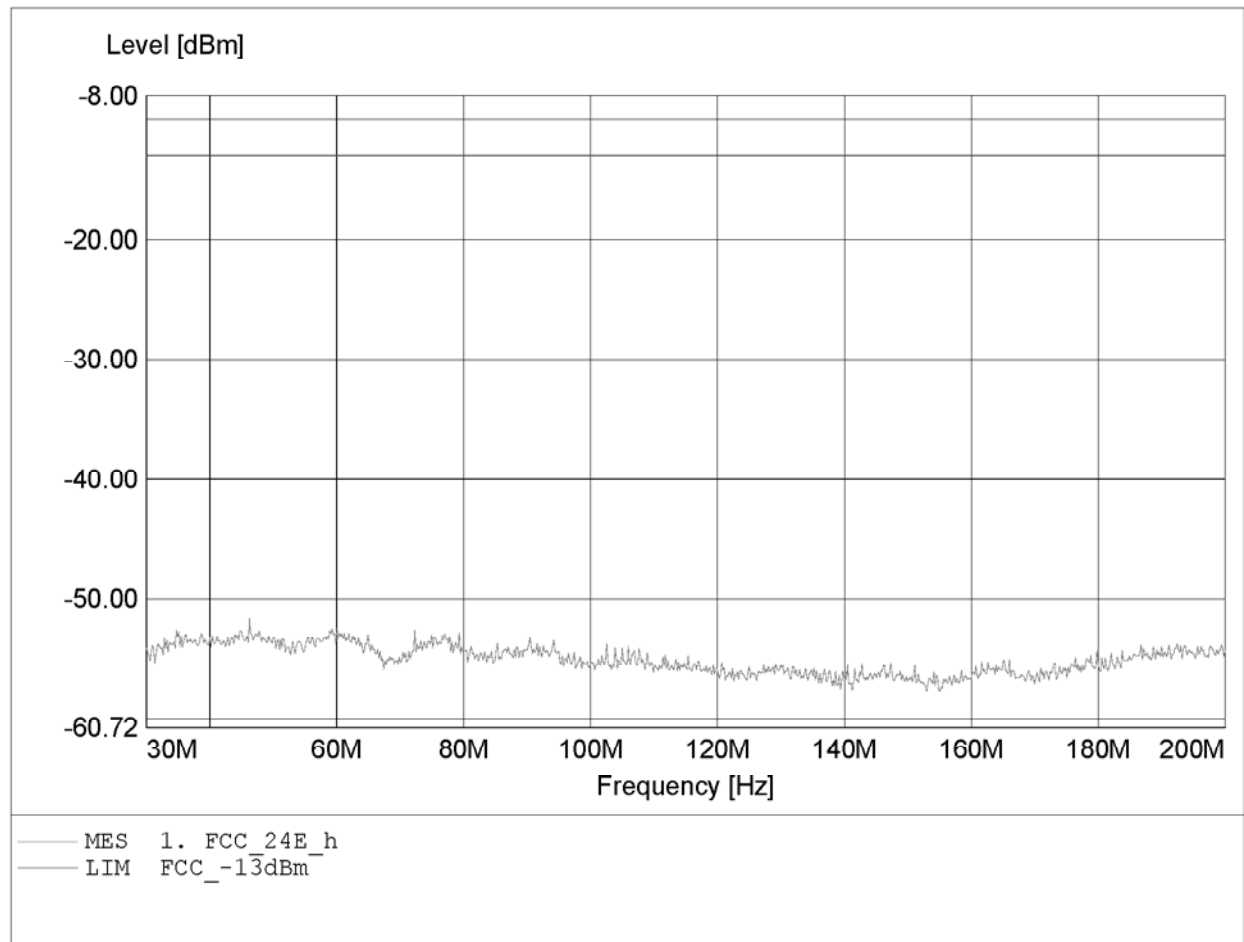


Radiated Emissions Tx
FCC RULES PART 24 SUBPART E

Approval Holder: BIOTRONIK GmbH & CO. KG
EUT : TELEX III
Model / Channel : CARDIOMESSENGER II / 810
Temperature/ Voltage: Temp.: 23°C / Unom.: 4.20 V DC
Test Site / Operator: ETS / Mr. Handrik
Test Specification: according to §24.238
Comment 1: Dist.: 3m, Ant.: HL 223
Comment 2: Freq: 985.778MHz, Pmax: -40.09dBm, RBW: 1MHz

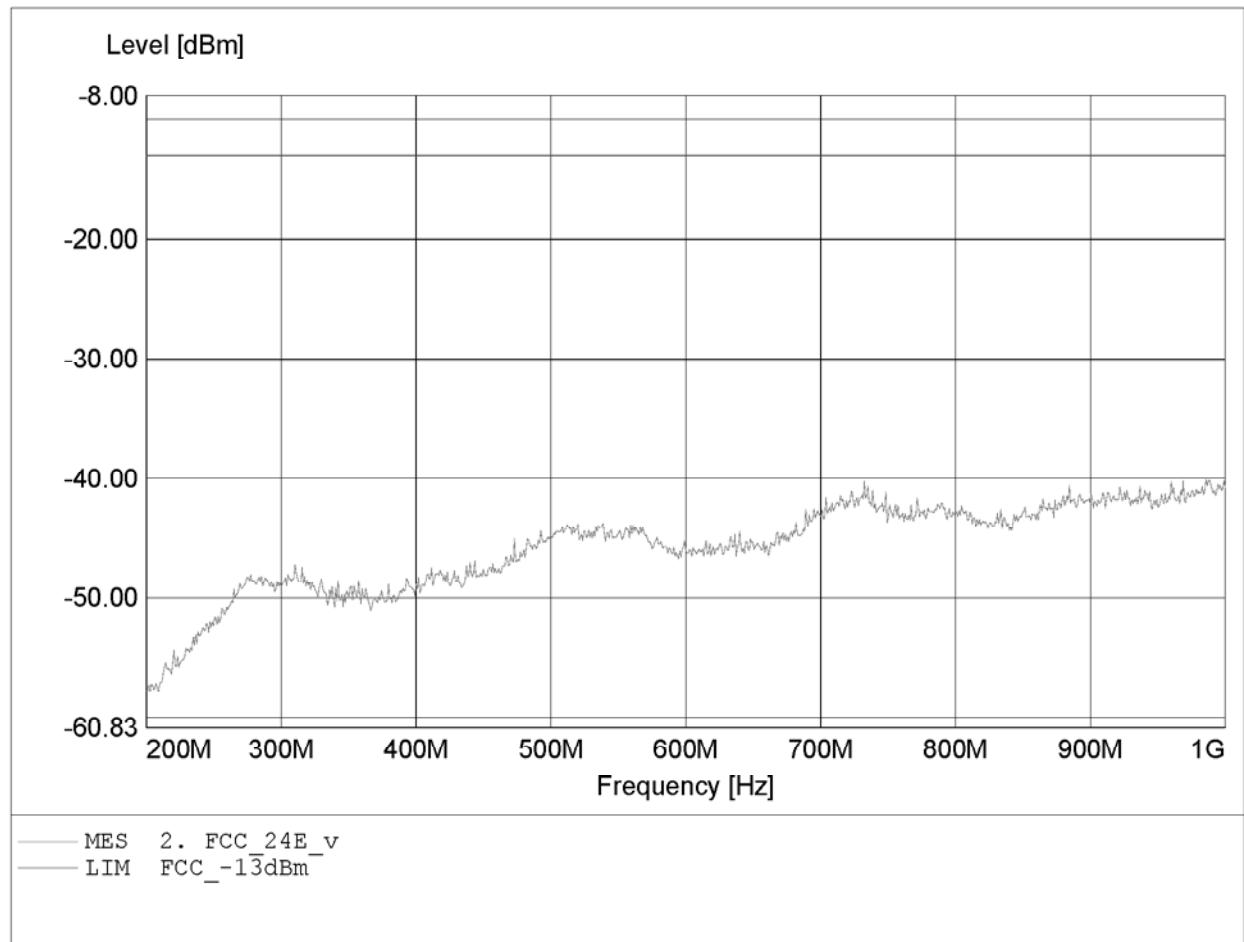


Radiated Emissions Tx
FCC RULES PART 24 SUBPART E

Approval Holder: BIOTRONIK GmbH & CO. KG
EUT : TELEX III
Model / Channel : CARDIOMESSENGER II / 810
Temperature/ Voltage: Temp.: 23°C / Unom.: 4.20 V DC
Test Site / Operator: ETS / Mr. Handrik
Test Specification: according to §24.238
Comment 1: Dist.: 3m, Ant.: HL 223
Comment 2: Freq: 863.111MHz, Pmax: -38.41dBm, RBW: 1MHz

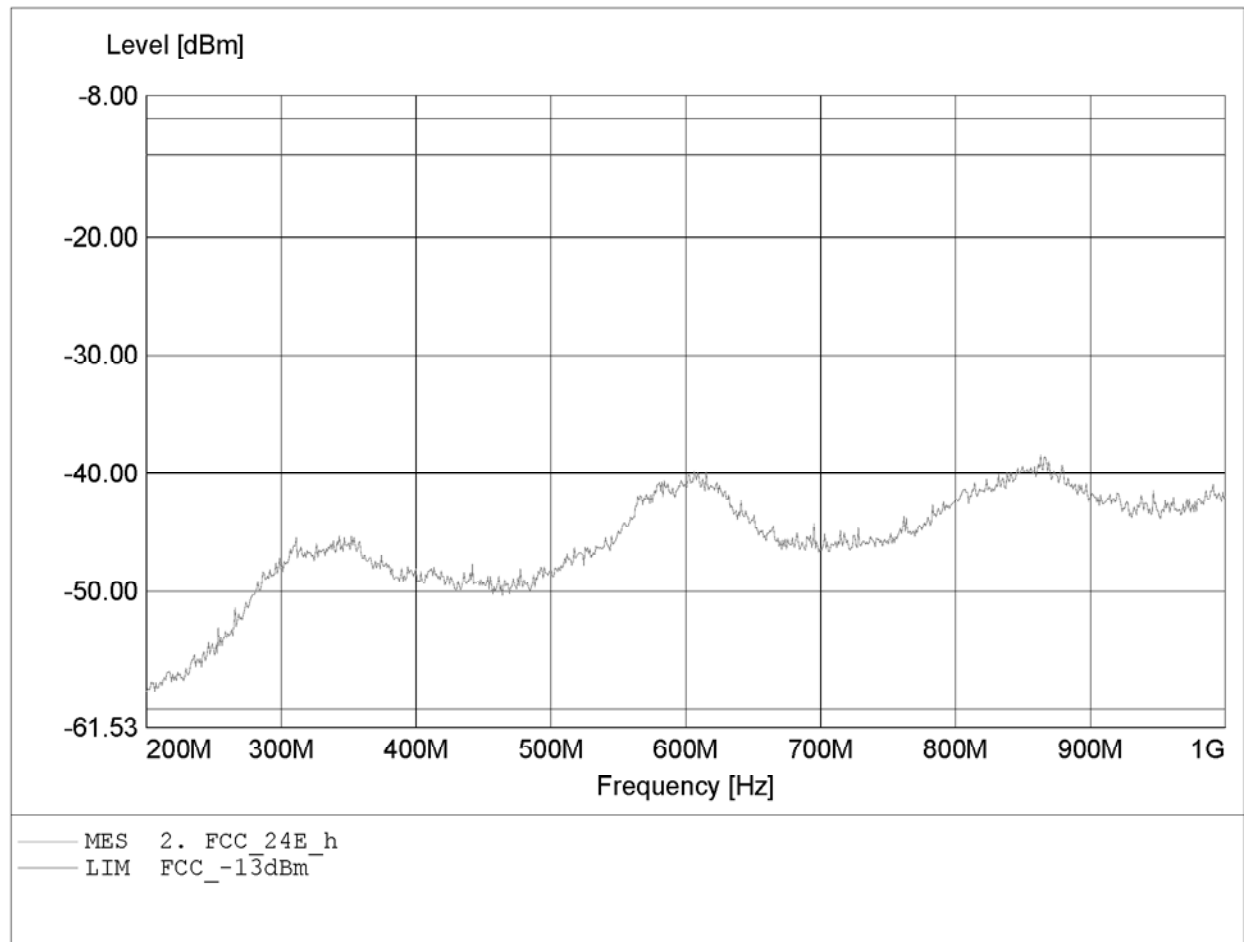


Radiated Emissions Tx
FCC RULES PART 24 SUBPART E

Approval Holder: BIOTRONIK GmbH & CO. KG
EUT : TELEX III
Model / Channel : CARDIOMESSENGER II / 810
Temperature/ Voltage: Temp.: 23°C / Unom.: 4.20 V DC
Test Site / Operator: ETS / Mr. Handrik
Test Specification: according to §24.238
Comment 1: Dist.: 3m, Ant.: HL025
Comment 2: Freq: 3.903GHz, Pmax: -22.25dBm, RBW: 1MHz/3kHz

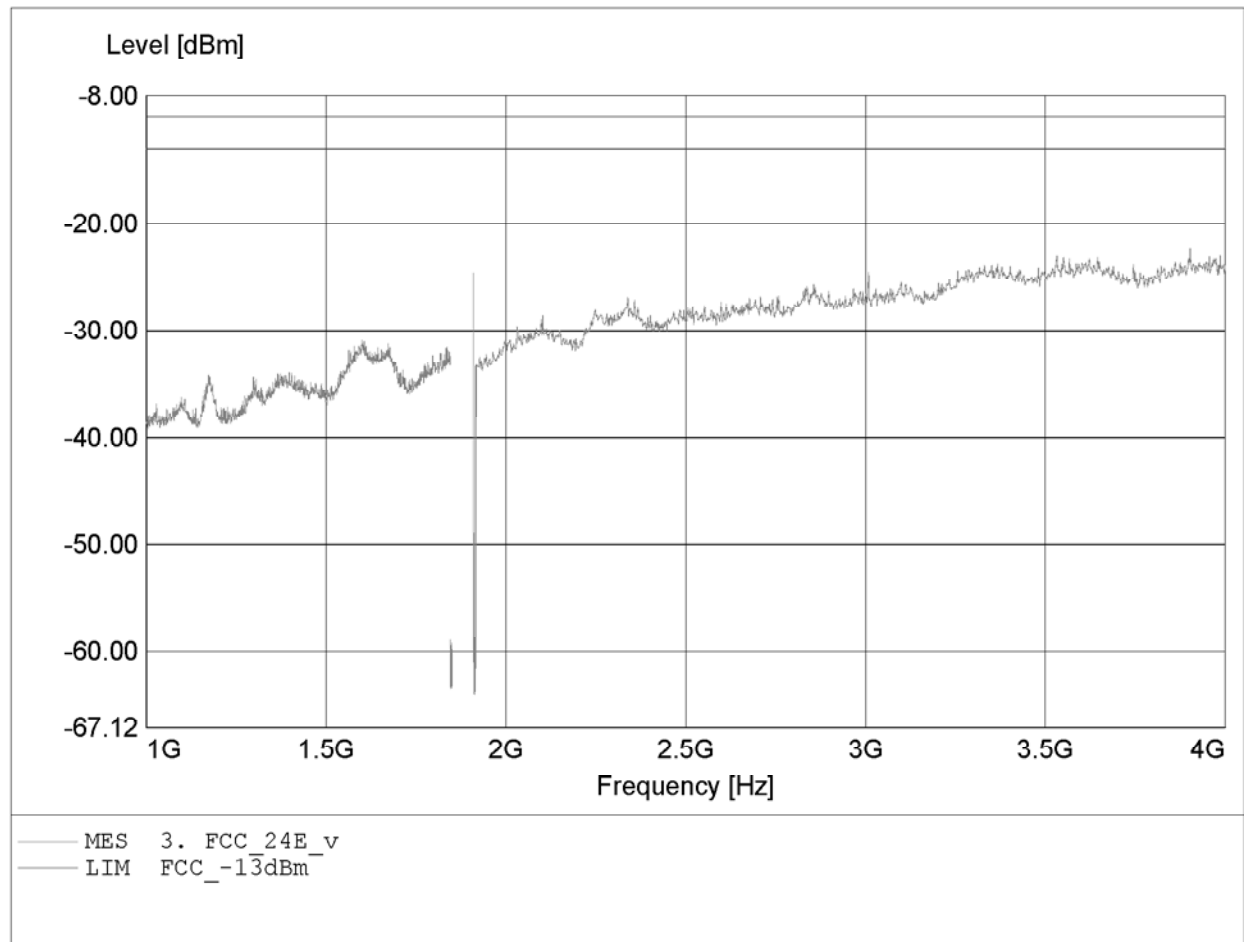


Radiated Emissions Tx
FCC RULES PART 24 SUBPART E

Approval Holder: BIOTRONIK GmbH & CO. KG
EUT : TELEX III
Model / Channel : CARDIOMESSENGER II / 810
Temperature/ Voltage: Temp.: 23°C / Unom.: 4.20 V DC
Test Site / Operator: ETS / Mr. Handrik
Test Specification: according to §24.238
Comment 1: Dist.: 3m, Ant.: HL025
Comment 2: Freq: 3.972GHz, Pmax: -22.50dBm, RBW: 1MHz/3kHz

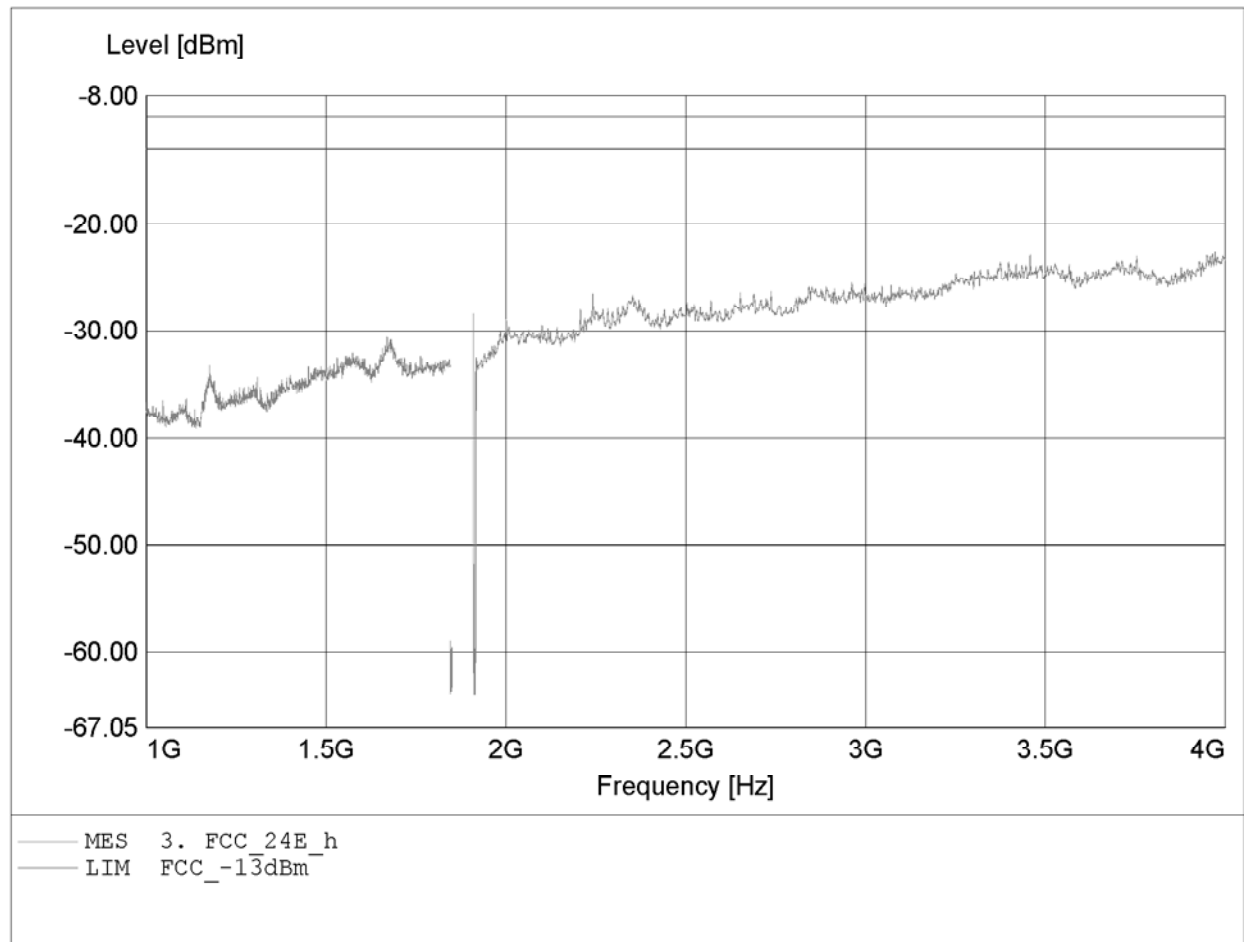


Radiated Emissions Tx
FCC RULES PART 24 SUBPART E

Approval Holder: BIOTRONIK GmbH & CO. KG
EUT : TELEX III
Model / Channel : CARDIOMESSENGER II / 810
Temperature/ Voltage: Temp.: 23°C / Unom.: 4.20 V DC
Test Site / Operator: ETS / Mr. Handrik
Test Specification: according to §24.238
Comment 1: Dist.: 3m, Ant.: HL025, ampl.+HP.
Comment 2: Freq: 7.564GHz, Pmax: -44.52dBm, RBW: 1MHz

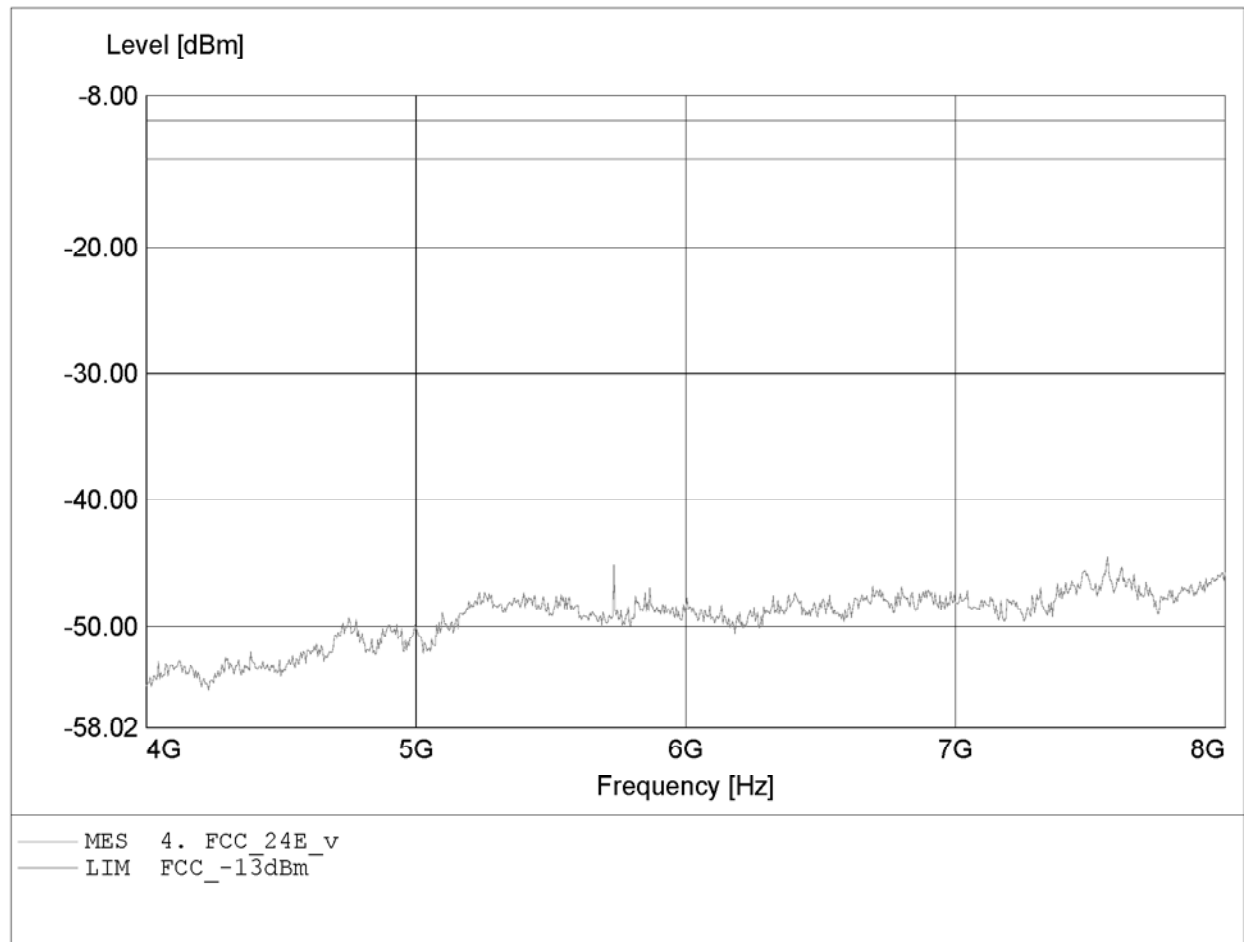


Radiated Emissions Tx
FCC RULES PART 24 SUBPART E

Approval Holder: BIOTRONIK GmbH & CO. KG
EUT : TELEX III
Model / Channel : CARDIOMESSENGER II / 810
Temperature/ Voltage: Temp.: 23°C / Unom.: 4.20 V DC
Test Site / Operator: ETS / Mr. Handrik
Test Specification: according to §24.238
Comment 1: Dist.: 3m, Ant.: HL025, ampl.+HP.
Comment 2: Freq: 5.733GHz, Pmax: -42.10dBm, RBW: 1MHz

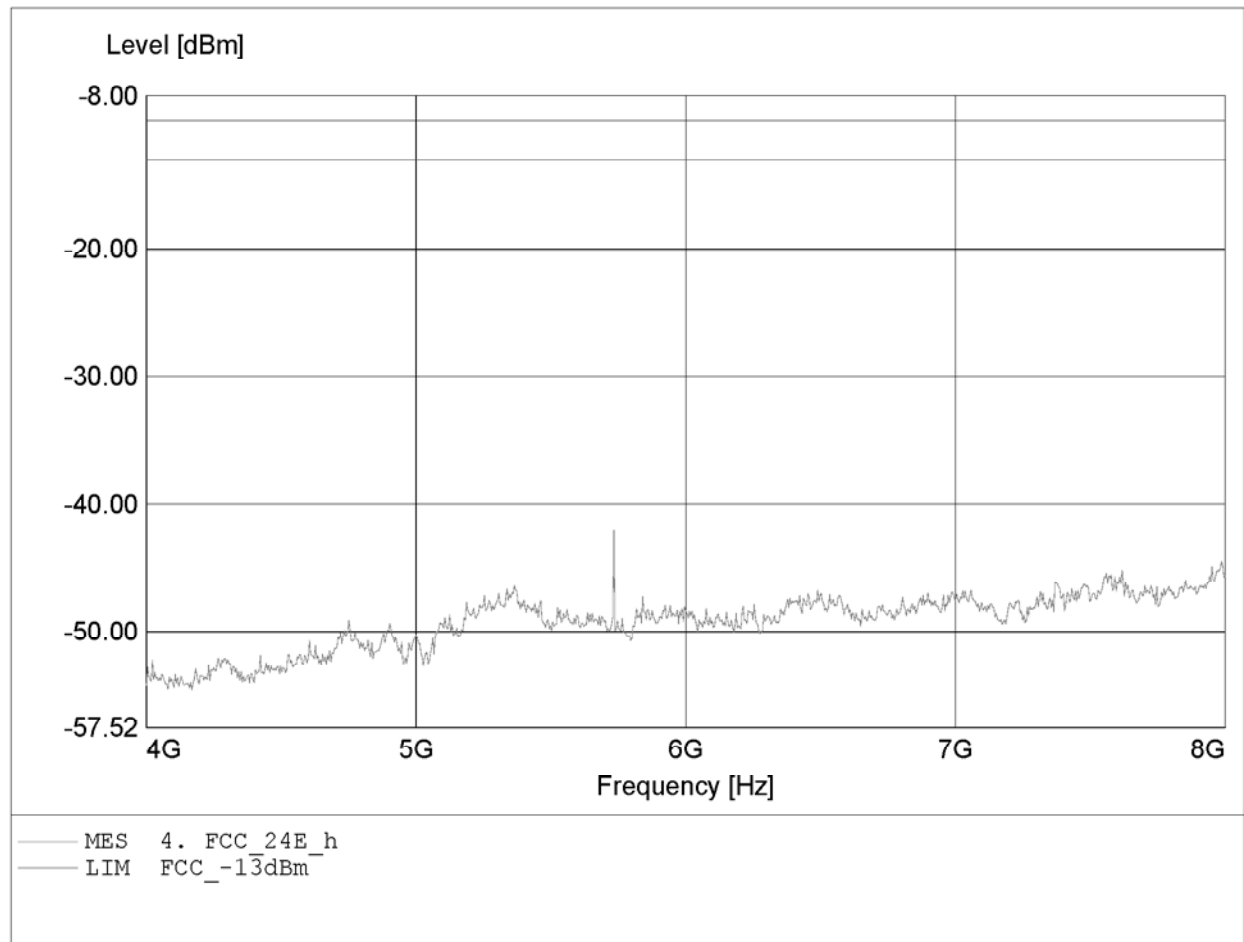


Radiated Emissions Tx
FCC RULES PART 24 SUBPART E

Approval Holder: BIOTRONIK GmbH & CO. KG
EUT : TELEX III
Model / Channel : CARDIOMESSENGER II / 810
Temperature/ Voltage: Temp.: 23°C / Unom.: 4.20 V DC
Test Site / Operator: ETS / Mr. Handrik
Test Specification: according to §24.238
Comment 1: Dist.: 3m, Ant.: HL025, ampl.+HP.
Comment 2: Freq: 9.551GHz, Pmax: -28.48dBm, RBW: 1MHz

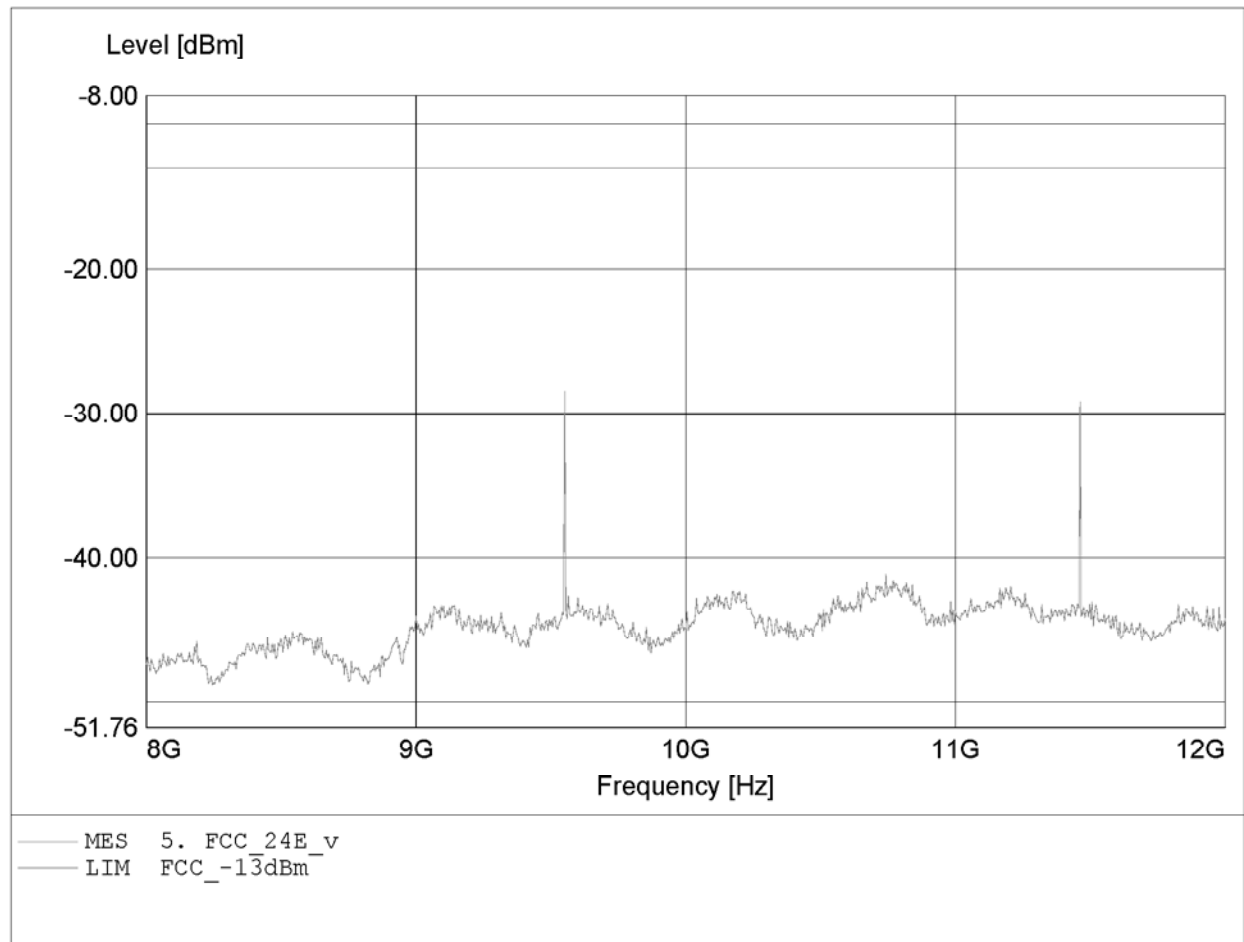


Radiated Emissions Tx
FCC RULES PART 24 SUBPART E

Approval Holder: BIOTRONIK GmbH & CO. KG
EUT : TELEX III
Model / Channel : CARDIOMESSENGER II / 810
Temperature/ Voltage: Temp.: 23°C / Unom.: 4.20 V DC
Test Site / Operator: ETS / Mr. Handrik
Test Specification: according to §24.238
Comment 1: Dist.: 3m, Ant.: HL025, ampl.+HP.
Comment 2: Freq: 10.711GHz, Pmax: -40.62dBm, RBW: 1MHz

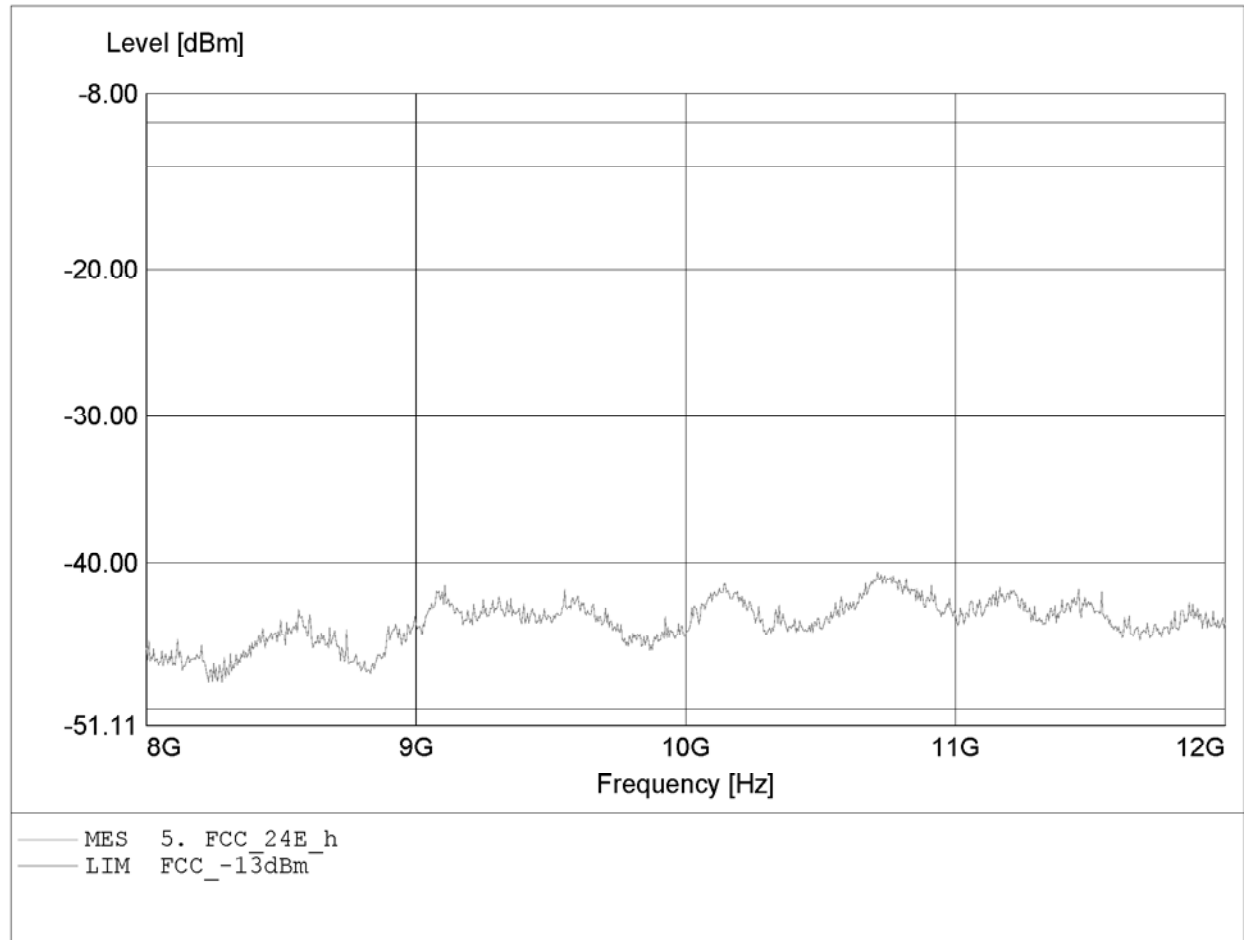


Radiated Emissions Tx
FCC RULES PART 24 SUBPART E

Approval Holder: BIOTRONIK GmbH & CO. KG
EUT : TELEX III
Model / Channel : CARDIOMESSENGER II / 810
Temperature/ Voltage: Temp.: 23°C / Unom.: 4.20 V DC
Test Site / Operator: ETS / Mr. Handrik
Test Specification: according to §24.238
Comment 1: Dist.: 3m, Ant.: HL025, ampl.+HP.
Comment 2: Freq: 15.280GHz, Pmax: -27.50dBm, RBW: 1MHz

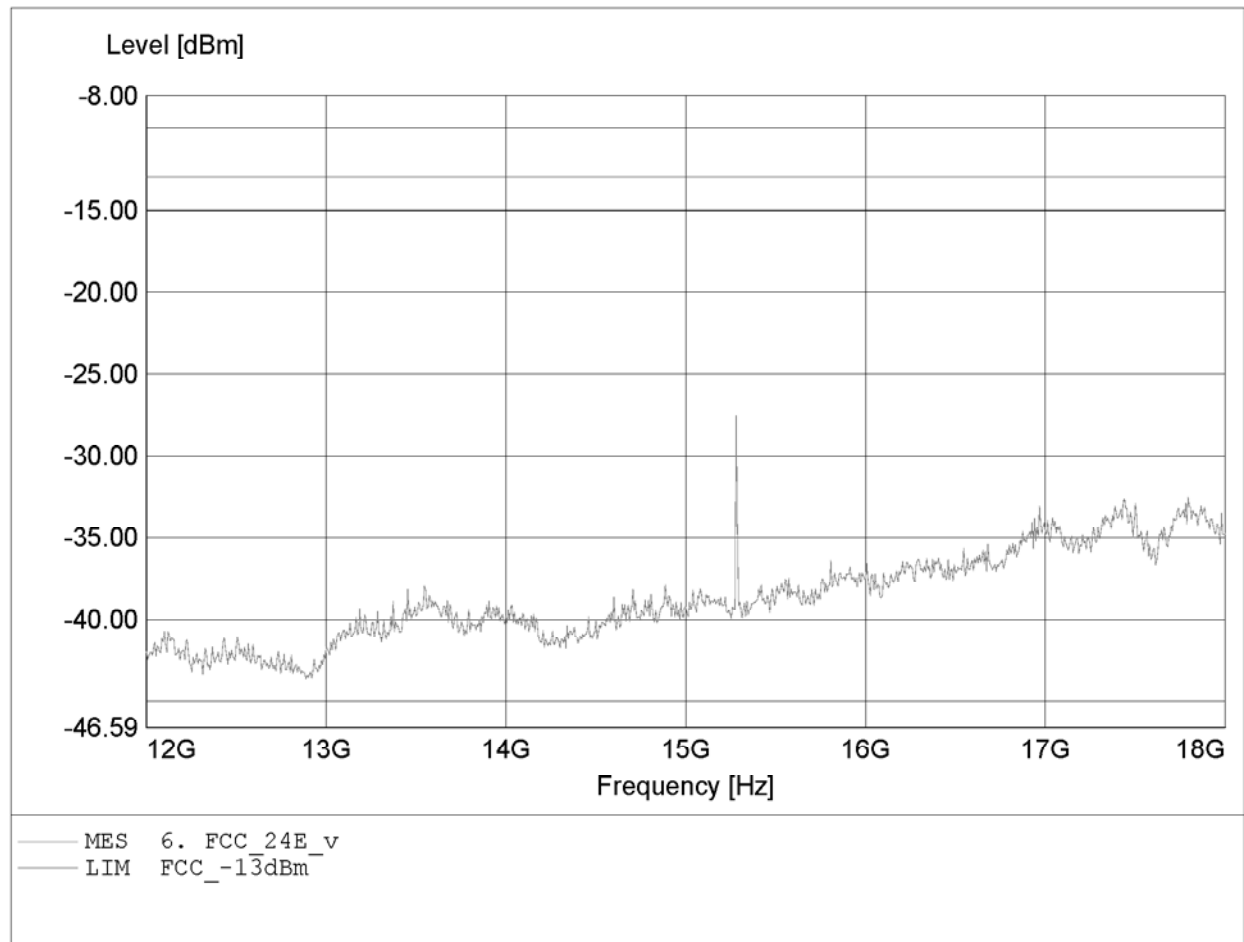


Radiated Emissions Tx
FCC RULES PART 24 SUBPART E

Approval Holder: BIOTRONIK GmbH & CO. KG
EUT : TELEX III
Model / Channel : CARDIOMESSENGER II / 810
Temperature/ Voltage: Temp.: 23°C / Unom.: 4.20 V DC
Test Site / Operator: ETS / Mr. Handrik
Test Specification: according to §24.238
Comment 1: Dist.: 3m, Ant.: HL025, ampl.+HP.
Comment 2: Freq: 15.280GHz, Pmax: -26.96dBm, RBW: 1MHz

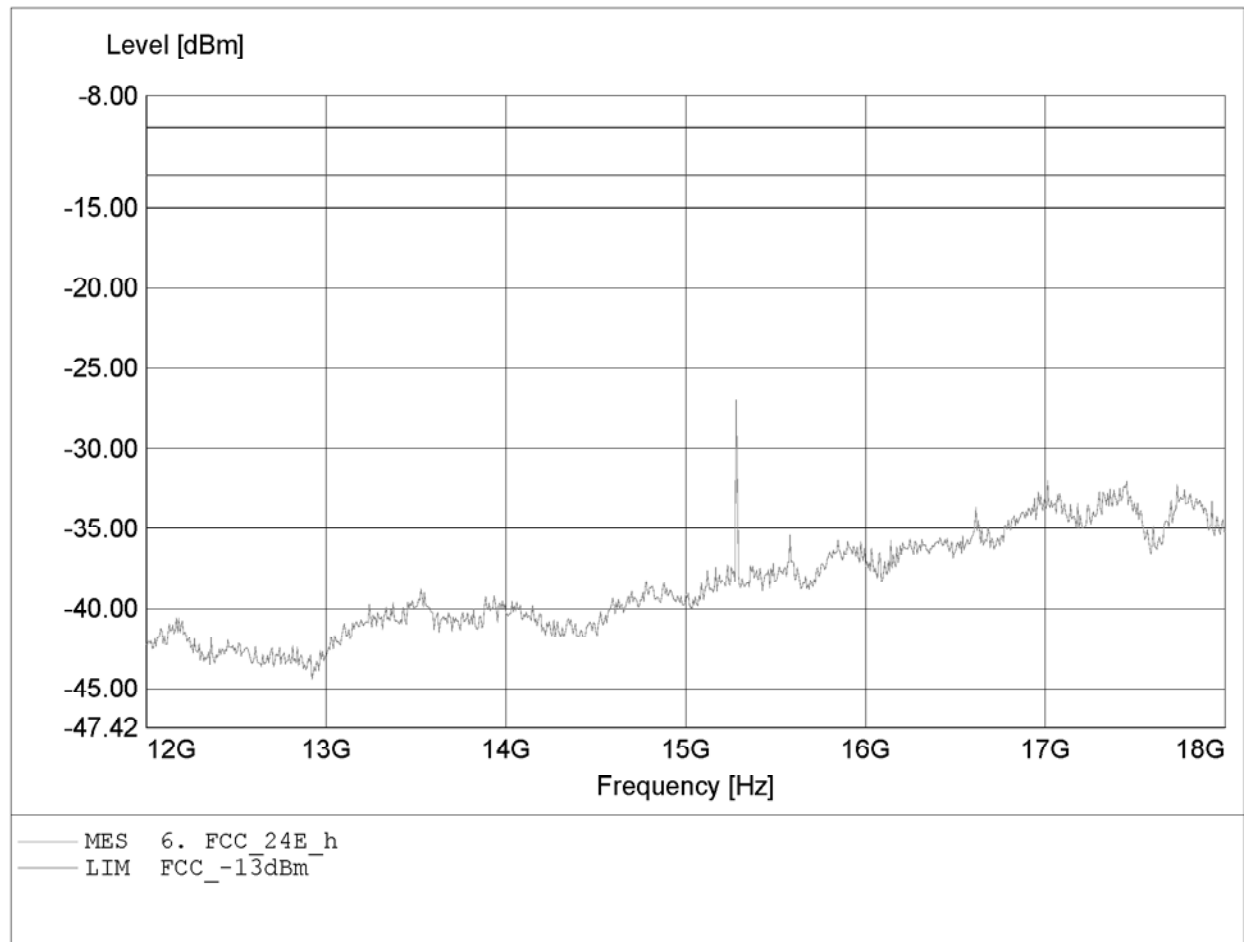


Radiated Emissions Tx
FCC RULES PART 24 SUBPART E

Approval Holder: BIOTRONIK GmbH & CO. KG
EUT : TELEX III
Model / Channel : CARDIOMESSENGER II / 810
Temperature/ Voltage: Temp.: 23°C / Unom.: 4.20 V DC
Test Site / Operator: ETS / Mr. Handrik
Test Specification: according to §24.238
Comment 1: Dist.: 3m, Ant.: HL025, amplif.
Comment 2: Freq: 18.425GHz, Pmax: -23.05dBm, RBW: 1MHz

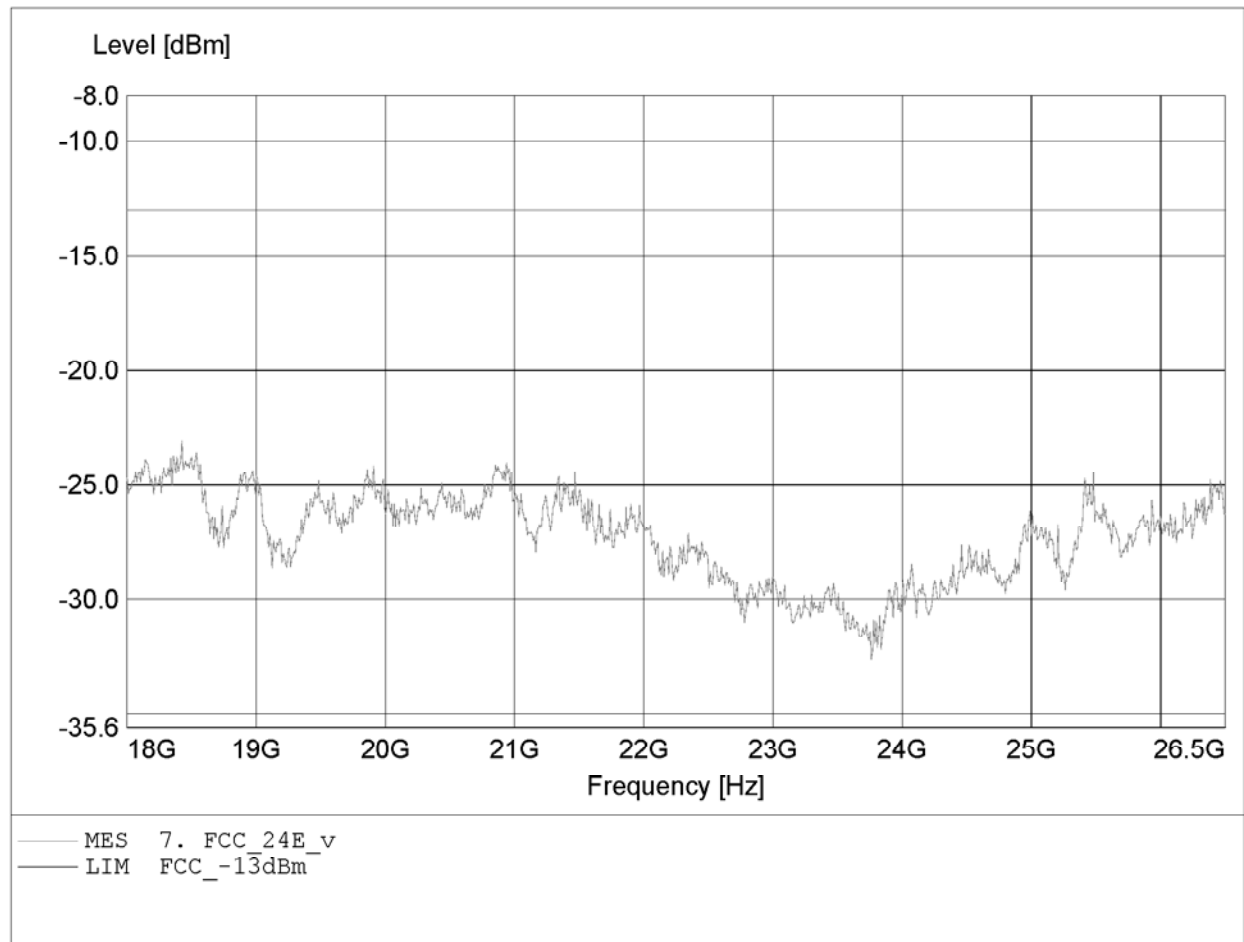


Radiated Emissions Tx
FCC RULES PART 24 SUBPART E

Approval Holder: BIOTRONIK GmbH & CO. KG
EUT : TELEX III
Model / Channel : CARDIOMESSENGER II / 810
Temperature/ Voltage: Temp.: 23°C / Unom.: 4.20 V DC
Test Site / Operator: ETS / Mr. Handrik
Test Specification: according to §24.238
Comment 1: Dist.: 3m, Ant.: HL025, amplif.
Comment 2: Freq: 18.491GHz, Pmax: -23.38dBm, RBW: 1MHz

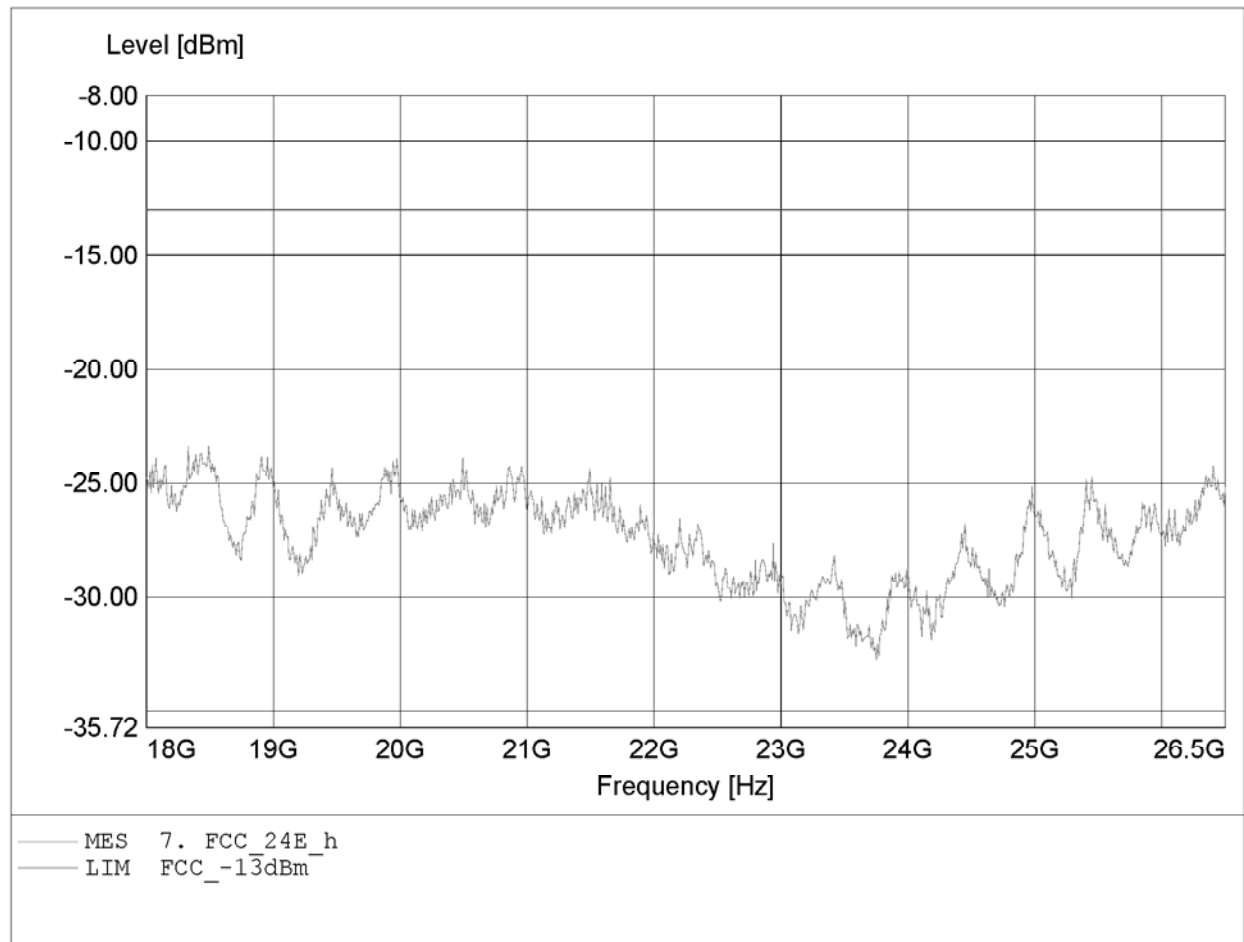


Radiated Emissions Tx
FCC RULES PART 22 SUBPART H

Approval Holder: BIOTRONIK GmbH & CO. KG
EUT : TELEX III
Model / Channel : CARDIOMESSENGER II / 128
Temperature/ Voltage: Temp.: 23°C / Unom.: 4.20 V DC
Test Site / Operator: ETS / Mr. Handrik
Test Specification: according to §22.917
Comment 1: Dist.: 3m, Ant.: HK 116
Comment 2: Freq: 194.522MHz, Pmax: -52.77dBm, RBW: 1MHz

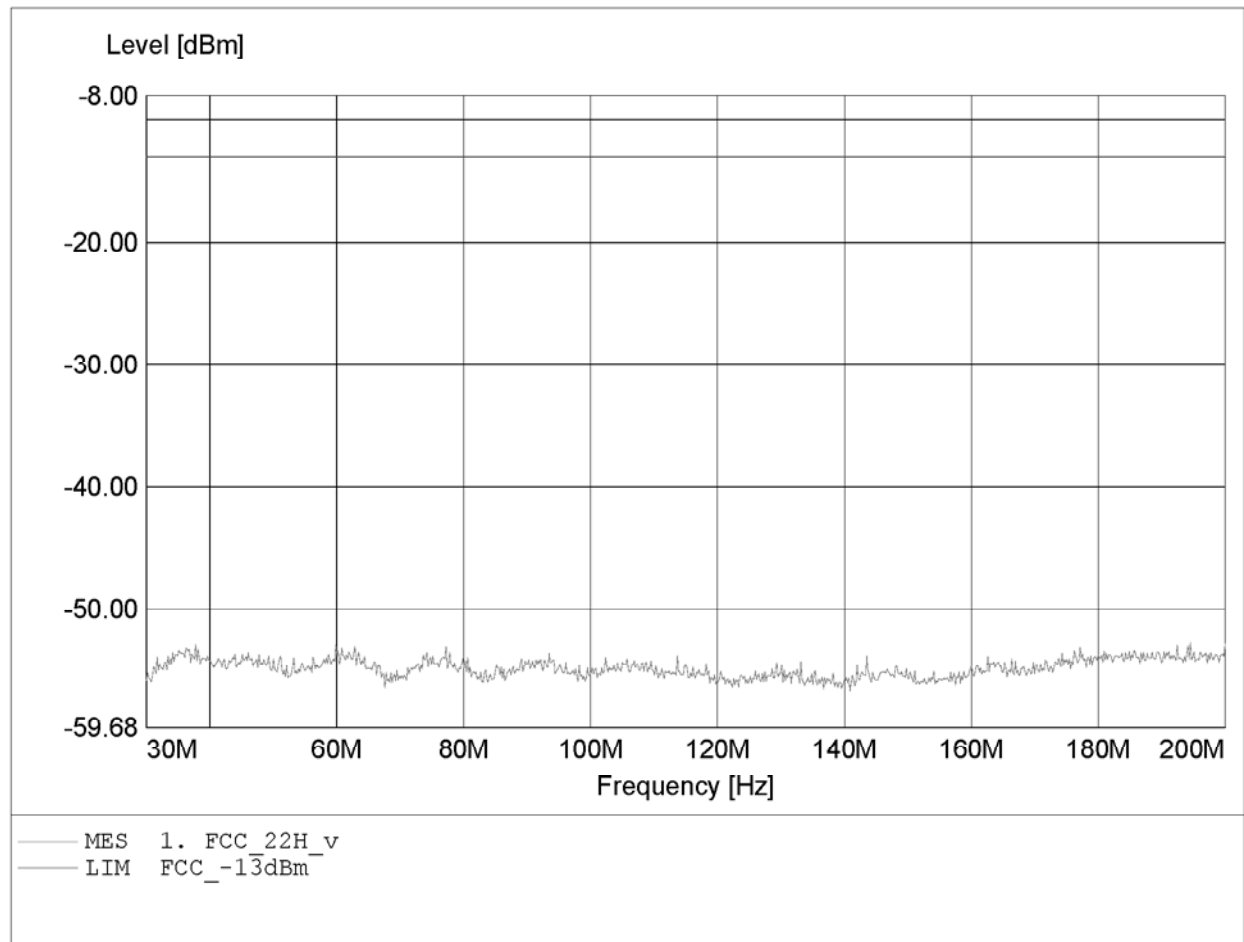


Radiated Emissions Tx
FCC RULES PART 22 SUBPART H

Approval Holder: BIOTRONIK GmbH & CO. KG
EUT : TELEX III
Model / Channel : CARDIOMESSENGER II / 128
Temperature/ Voltage: Temp.: 23°C / Unom.: 4.20 V DC
Test Site / Operator: ETS / Mr. Handrik
Test Specification: according to §22.917
Comment 1: Dist.: 3m, Ant.: HK 116
Comment 2: Freq: 47.378MHz, Pmax: -52.05dBm, RBW: 1MHz

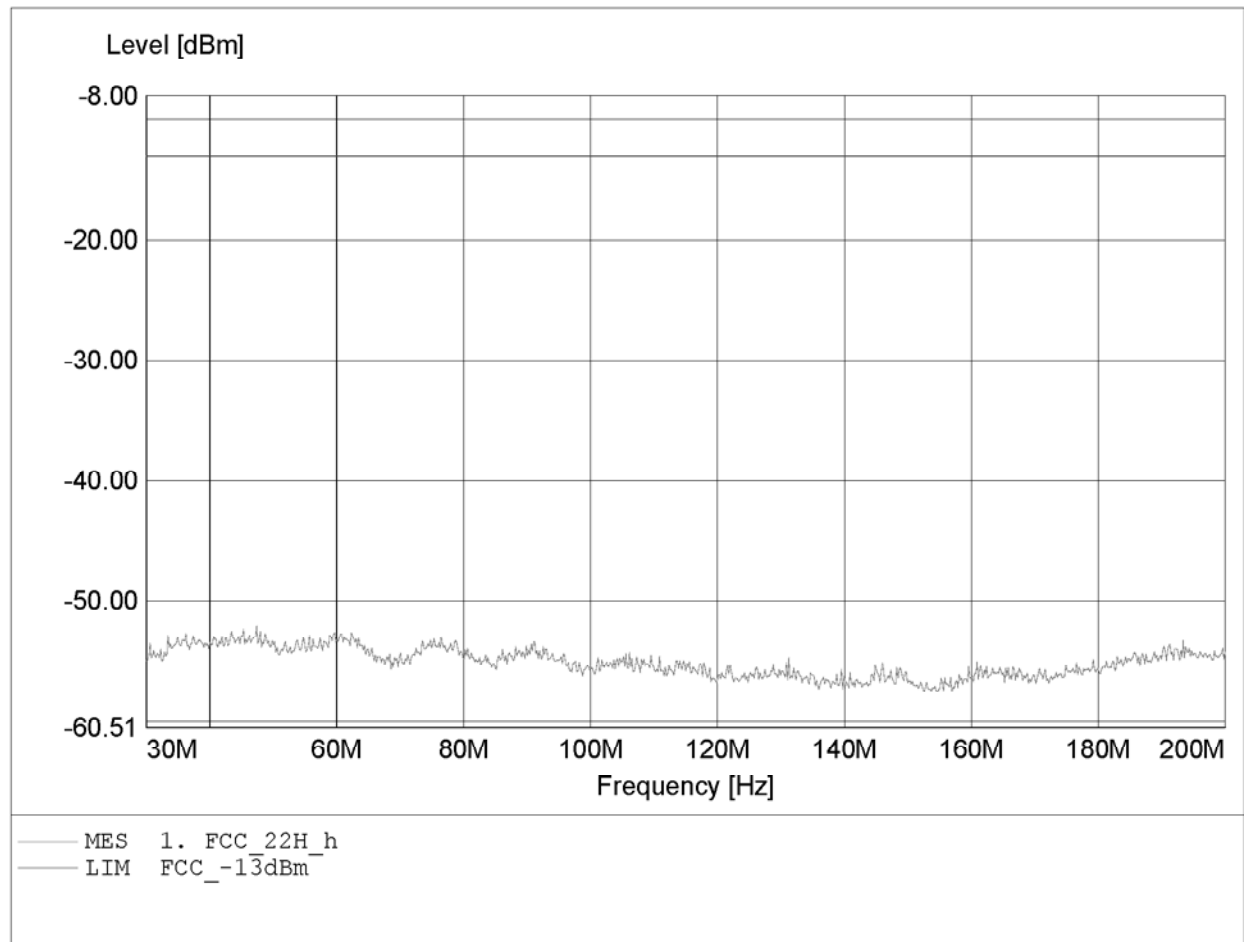


Radiated Emissions Tx
FCC RULES PART 22 SUBPART H

Approval Holder: BIOTRONIK GmbH & CO. KG
EUT : TELEX III
Model / Channel : CARDIOMESSENGER II / 128
Temperature/ Voltage: Temp.: 23°C / Unom.: 4.20 V DC
Test Site / Operator: ETS / Mr. Handrik
Test Specification: according to §22.917
Comment 1: Dist.: 3m, Ant.: HL 223+notch
Comment 2: Freq: 823.994MHz, Pmax: -25.04dBm, RBW: 1MHz

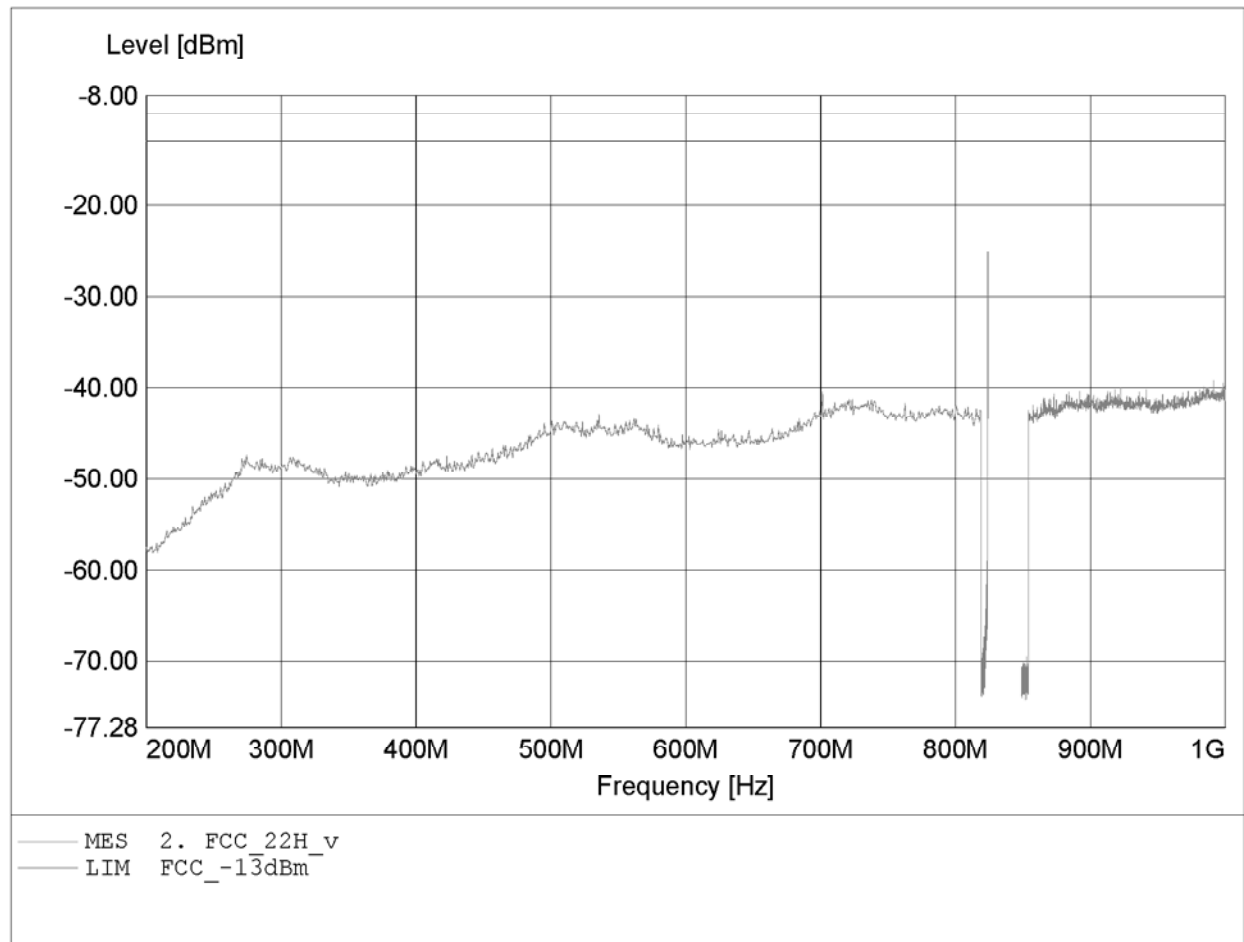


Radiated Emissions Tx
FCC RULES PART 22 SUBPART H

Approval Holder: BIOTRONIK GmbH & CO. KG
EUT : TELEX III
Model / Channel : CARDIOMESSENGER II / 128
Temperature/ Voltage: Temp.: 23°C / Unom.: 4.20 V DC
Test Site / Operator: ETS / Mr. Handrik
Test Specification: according to §22.917
Comment 1: Dist.: 3m, Ant.: HL 223+notch
Comment 2: Freq: 823.994MHz, Pmax: -25.22dBm, RBW: 1MHz

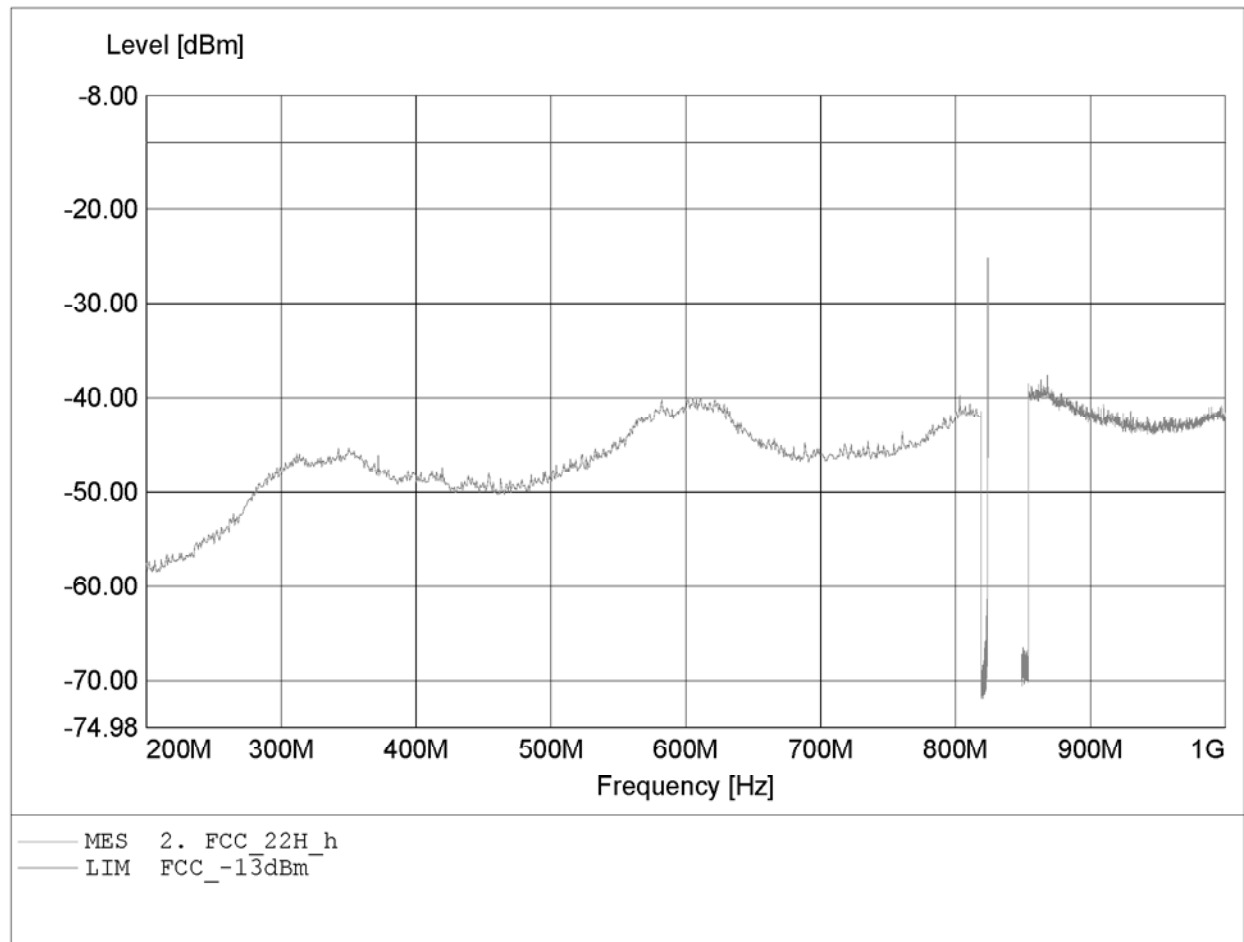


Radiated Emissions Tx
FCC RULES PART 22 SUBPART H

Approval Holder: BIOTRONIK GmbH & CO. KG
EUT : TELEX III
Model / Channel : CARDIOMESSENGER II / 128
Temperature/ Voltage: Temp.: 23°C / Unom.: 4.20 V DC
Test Site / Operator: ETS / Mr. Handrik
Test Specification: according to §22.917
Comment 1: Dist.: 3m, Ant.: HL025
Comment 2: Freq: 3.653GHz, Pmax: -23.10dBm, RBW: 1MHz

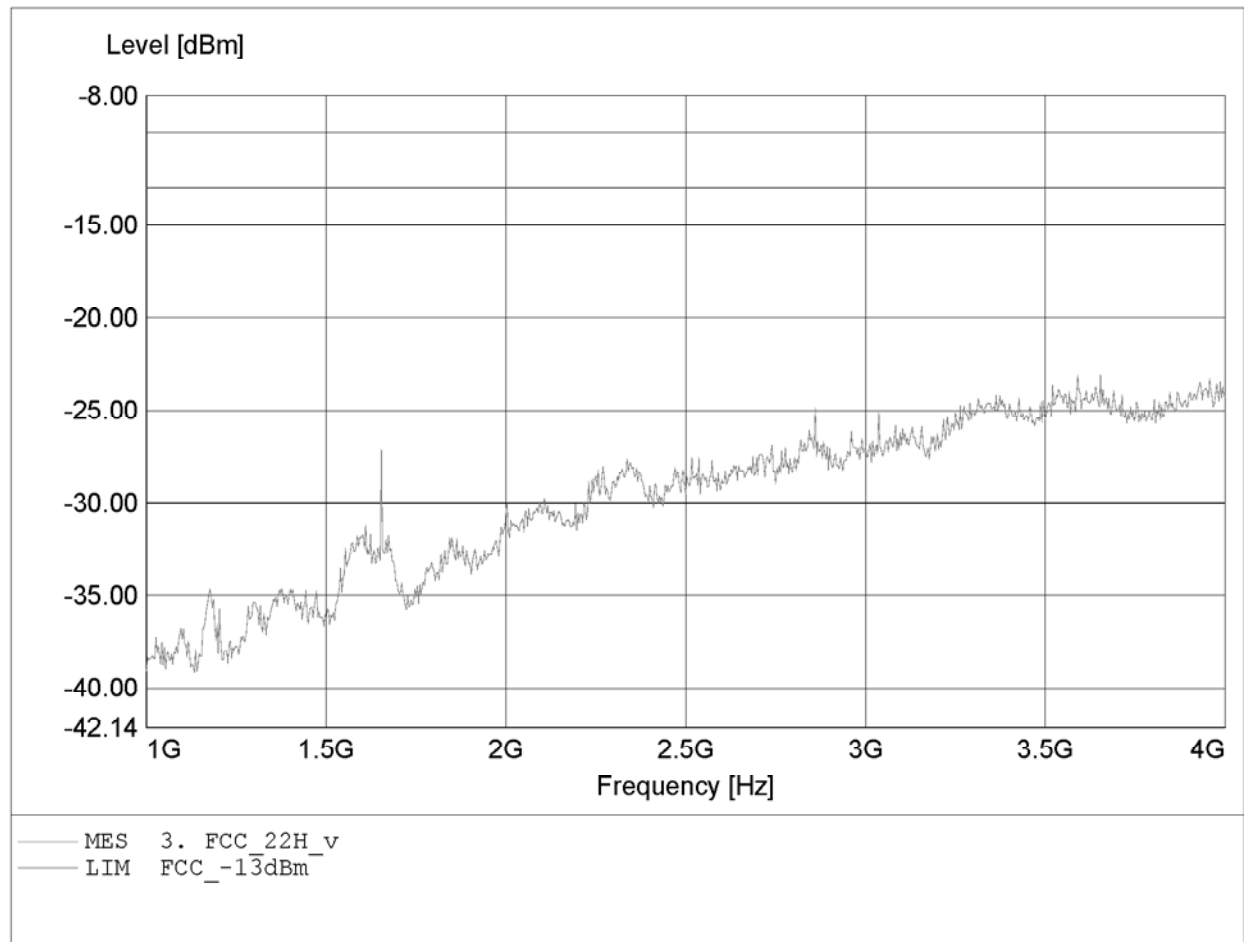


Radiated Emissions Tx
FCC RULES PART 22 SUBPART H

Approval Holder: BIOTRONIK GmbH & CO. KG
EUT : TELEX III
Model / Channel : CARDIOMESSENGER II / 128
Temperature/ Voltage: Temp.: 23°C / Unom.: 4.20 V DC
Test Site / Operator: ETS / Mr. Handrik
Test Specification: according to §22.917
Comment 1: Dist.: 3m, Ant.: HL025
Comment 2: Freq: 3.940GHz, Pmax: -22.55dBm, RBW: 1MHz

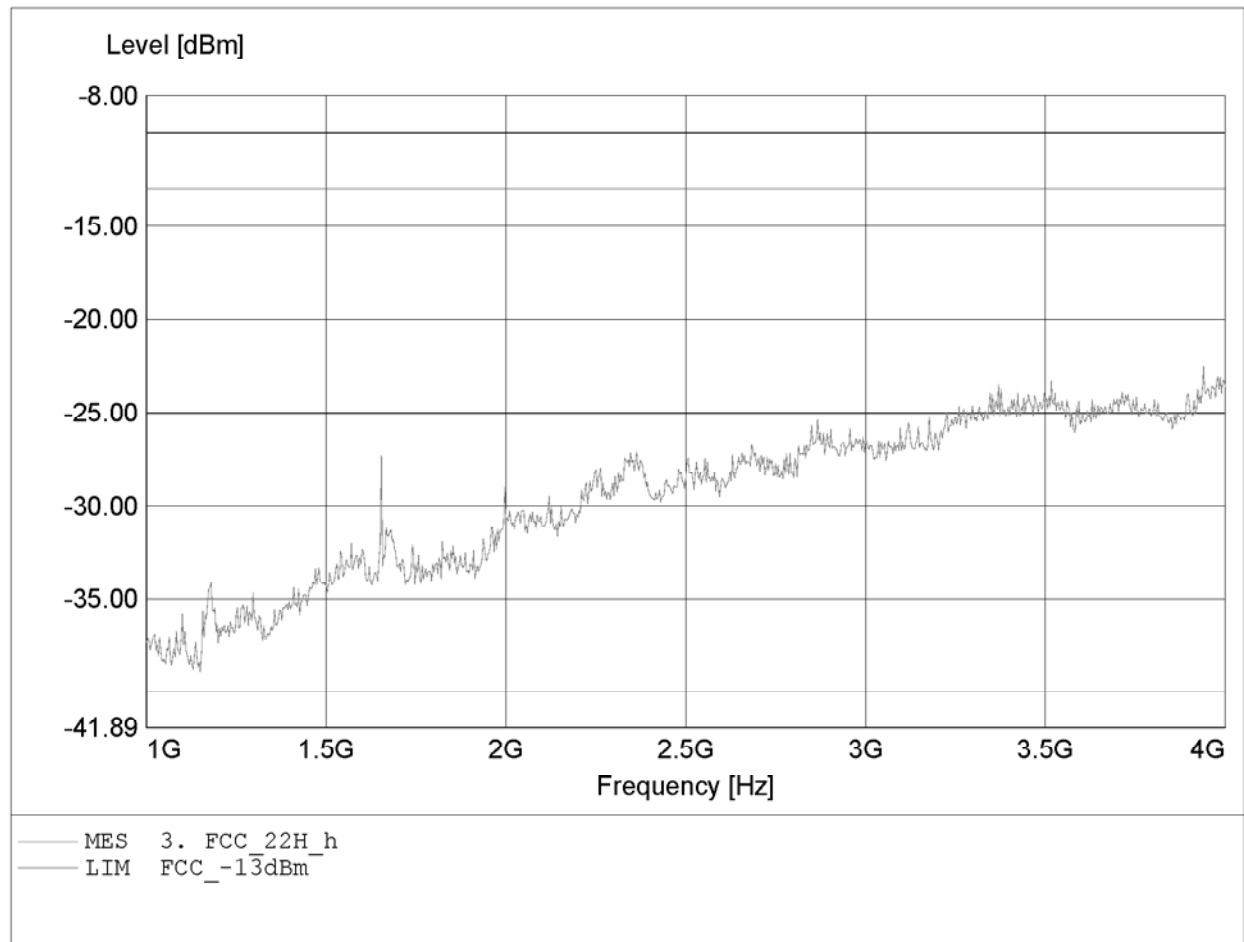


Radiated Emissions Tx
FCC RULES PART 22 SUBPART H

Approval Holder: BIOTRONIK GmbH & CO. KG
EUT : TELEX III
Model / Channel : CARDIOMESSENGER II / 128
Temperature/ Voltage: Temp.: 23°C / Unom.: 4.20 V DC
Test Site / Operator: ETS / Mr. Handrik
Test Specification: according to §22.917
Comment 1: Dist.: 3m, Ant.: HL025, ampl.+HP.
Comment 2: Freq: 7.978GHz, Pmax: -45.20dBm, RBW: 1MHz

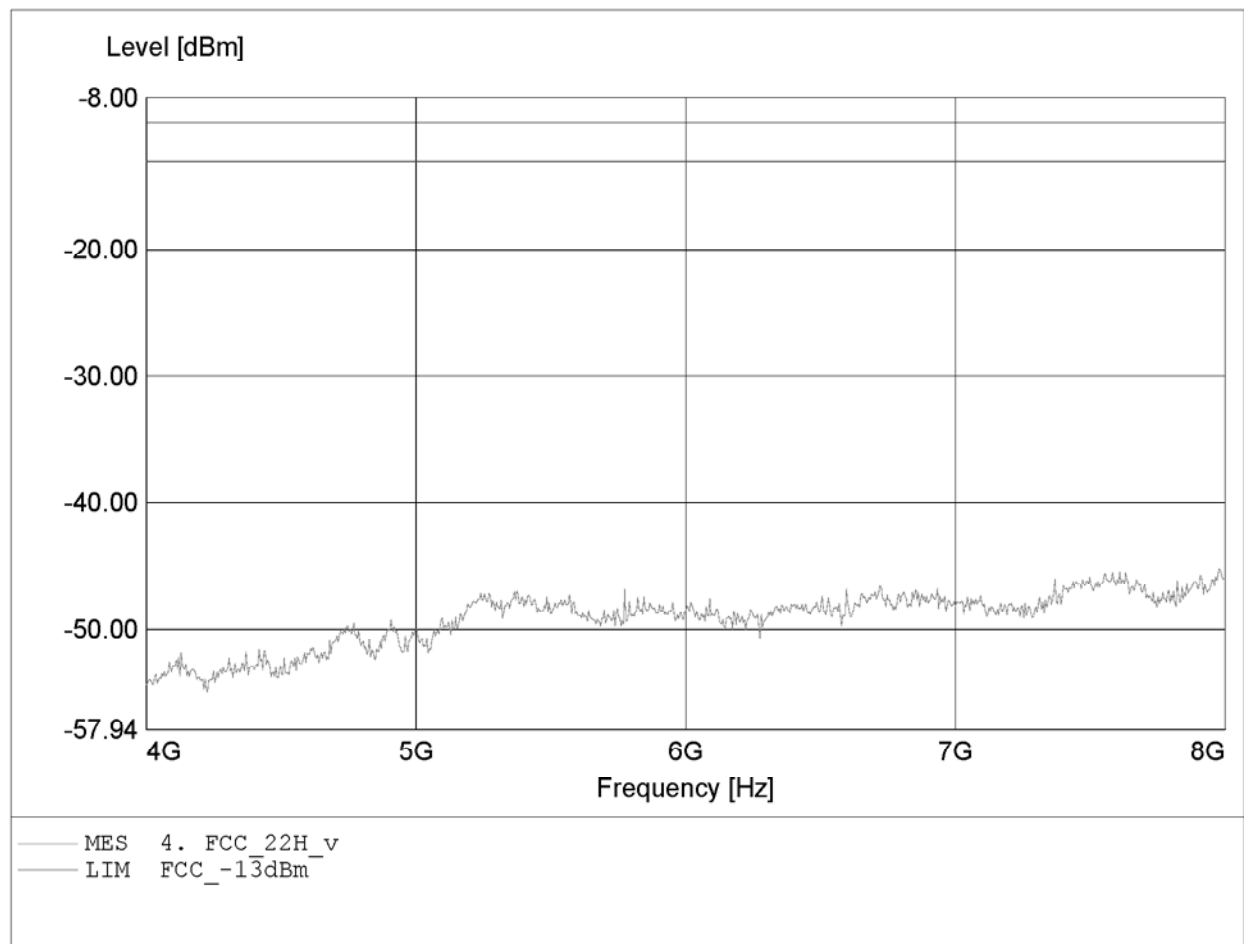


Radiated Emissions Tx
FCC RULES PART 22 SUBPART H

Approval Holder: BIOTRONIK GmbH & CO. KG
EUT : TELEX III
Model / Channel : CARDIOMESSENGER II / 128
Temperature/ Voltage: Temp.: 23°C / Unom.: 4.20 V DC
Test Site / Operator: ETS / Mr. Handrik
Test Specification: according to §22.917
Comment 1: Dist.: 3m, Ant.: HL025, ampl.+HP.
Comment 2: Freq: 7.991GHz, Pmax: -43.85dBm, RBW: 1MHz

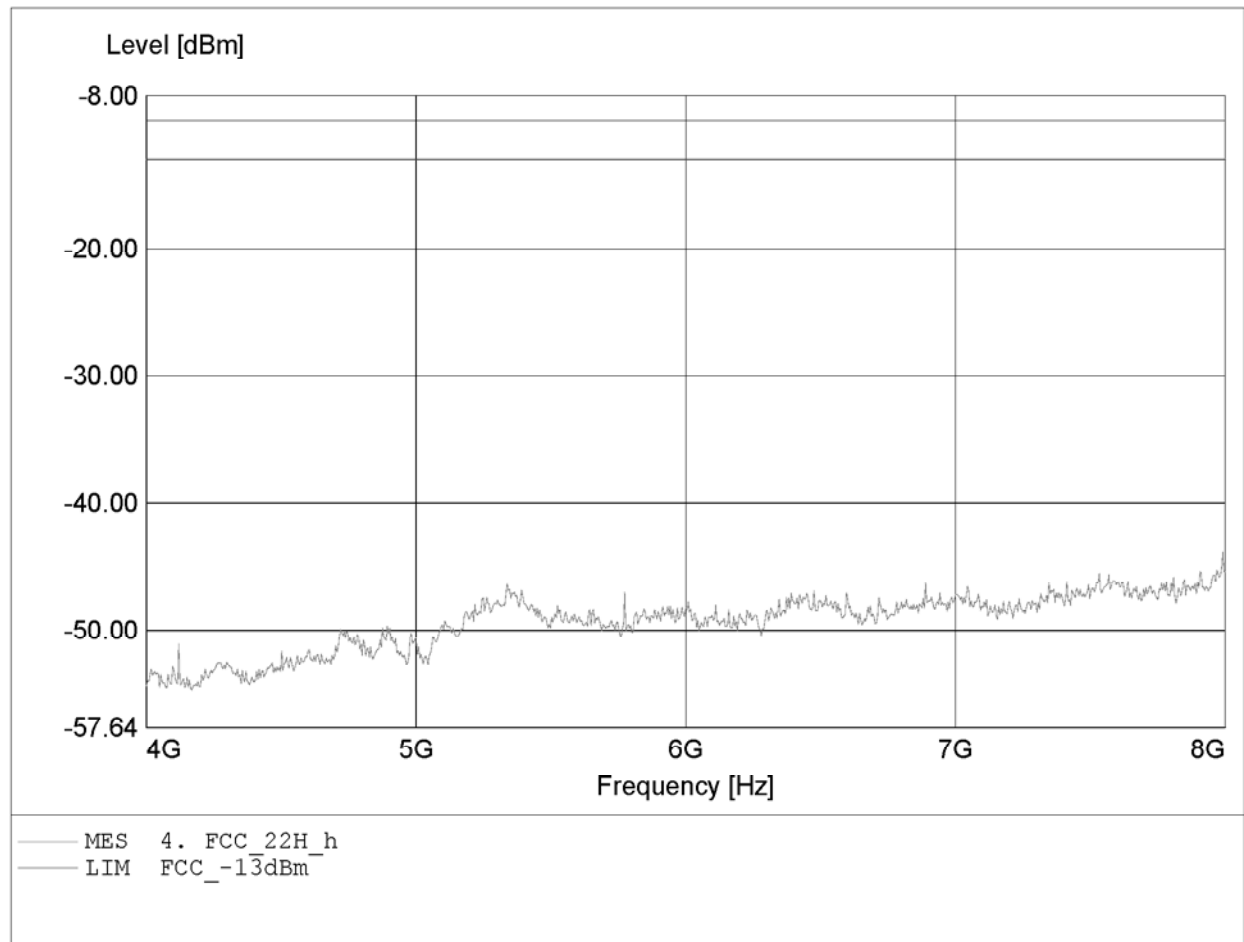


Radiated Emissions Tx
FCC RULES PART 22 SUBPART H

Approval Holder: BIOTRONIK GmbH & CO. KG
EUT : TELEX III
Model / Channel : CARDIOMESSENGER II / 128
Temperature/ Voltage: Temp.: 23°C / Unom.: 4.20 V DC
Test Site / Operator: ETS / Mr. Handrik
Test Specification: according to §22.917
Comment 1: Dist.: 3m, Ant.: HL025, ampl.+HP.
Comment 2: Freq: 10.778GHz, Pmax: -41.19dBm, RBW: 1MHz

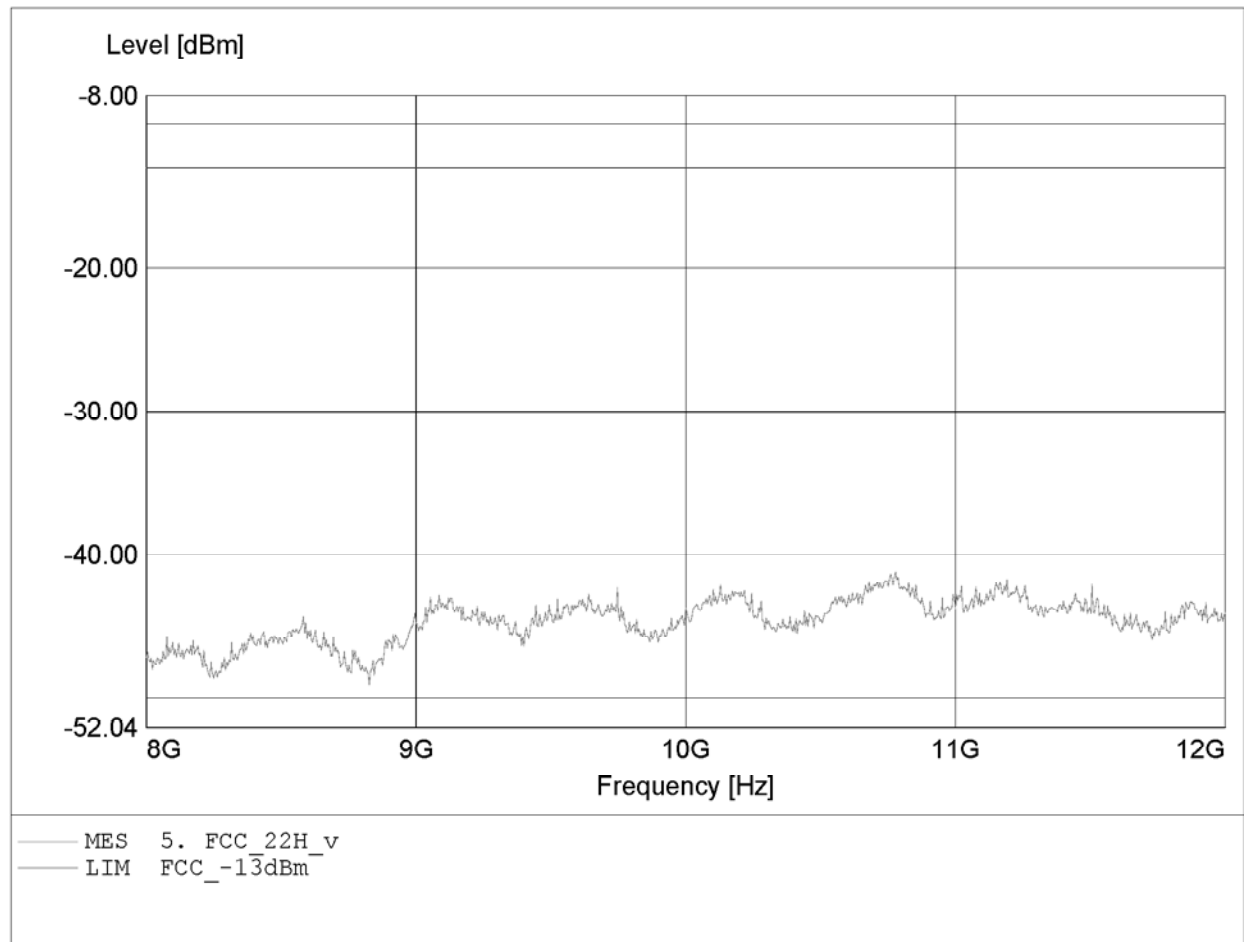


Radiated Emissions Tx
FCC RULES PART 22 SUBPART H

Approval Holder: BIOTRONIK GmbH & CO. KG
EUT : TELEX III
Model / Channel : CARDIOMESSENGER II / 128
Temperature/ Voltage: Temp.: 23°C / Unom.: 4.20 V DC
Test Site / Operator: ETS / Mr. Handrik
Test Specification: according to §22.917
Comment 1: Dist.: 3m, Ant.: HL025, ampl.+HP.
Comment 2: Freq: 10.769GHz, Pmax: -40.04dBm, RBW: 1MHz

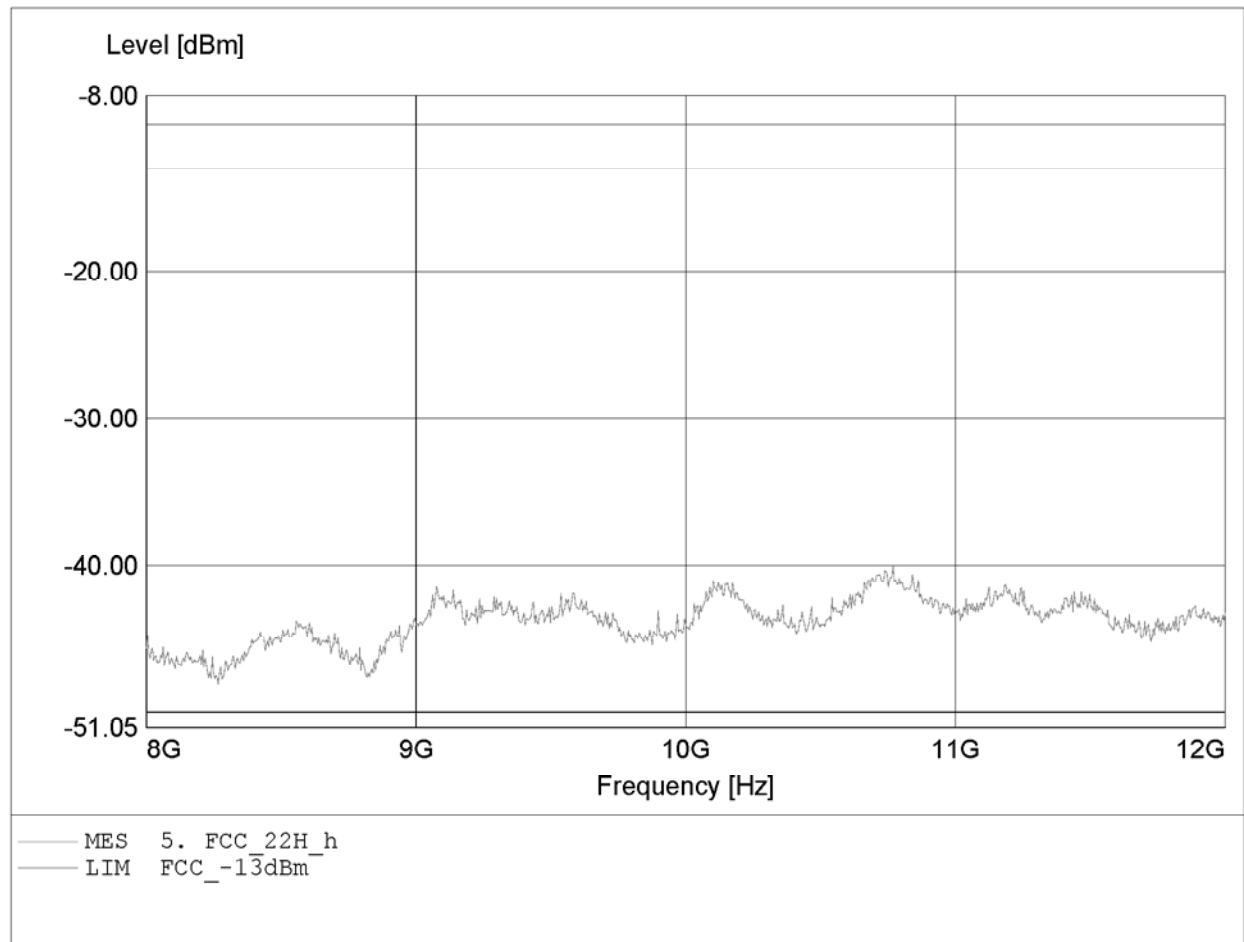


Radiated Emissions Tx
FCC RULES PART 22 SUBPART H

Approval Holder: BIOTRONIK GmbH & CO. KG
EUT : TELEX III
Model / Channel : CARDIOMESSENGER II / 188
Temperature/ Voltage: Temp.: 23°C / Unom.: 4.20 V DC
Test Site / Operator: ETS / Mr. Handrik
Test Specification: according to §22.917
Comment 1: Dist.: 3m, Ant.: HK 116
Comment 2: Freq: 33.589MHz, Pmax: -52.40dBm, RBW: 1MHz

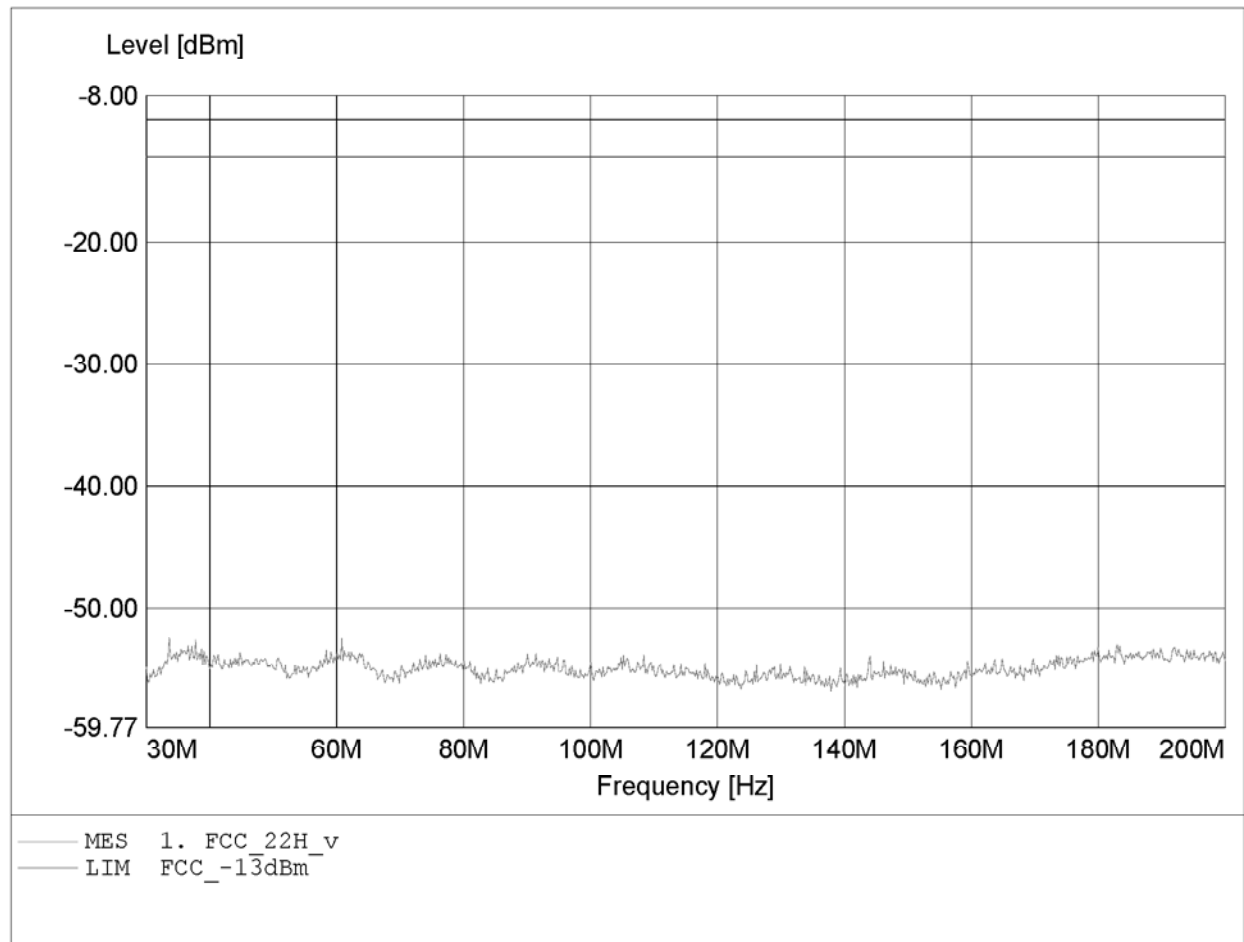


Radiated Emissions Tx
FCC RULES PART 22 SUBPART H

Approval Holder: BIOTRONIK GmbH & CO. KG
EUT : TELEX III
Model / Channel : CARDIOMESSENGER II / 188
Temperature/ Voltage: Temp.: 23°C / Unom.: 4.20 V DC
Test Site / Operator: ETS / Mr. Handrik
Test Specification: according to §22.917
Comment 1: Dist.: 3m, Ant.: HK 116
Comment 2: Freq: 34.533MHz, Pmax: -51.99dBm, RBW: 1MHz

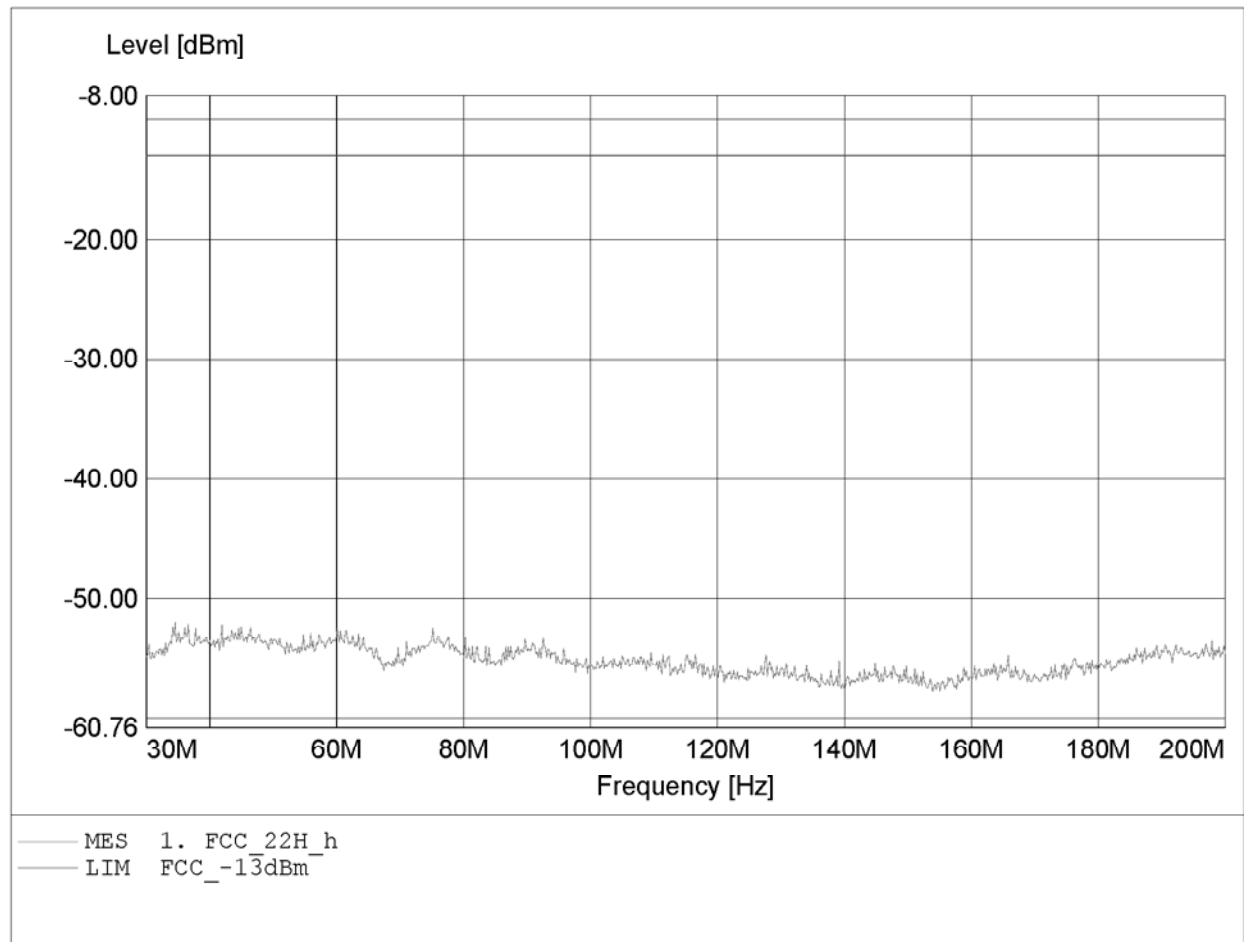


Radiated Emissions Tx
FCC RULES PART 22 SUBPART H

Approval Holder: BIOTRONIK GmbH & CO. KG
EUT : TELEX III
Model / Channel : CARDIOMESSENGER II / 188
Temperature/ Voltage: Temp.: 23°C / Unom.: 4.20 V DC
Test Site / Operator: ETS / Mr. Handrik
Test Specification: according to §22.917
Comment 1: Dist.: 3m, Ant.: HL 223+notch
Comment 2: Freq: 987.347MHz, Pmax: -39.48dBm, RBW: 1MHz

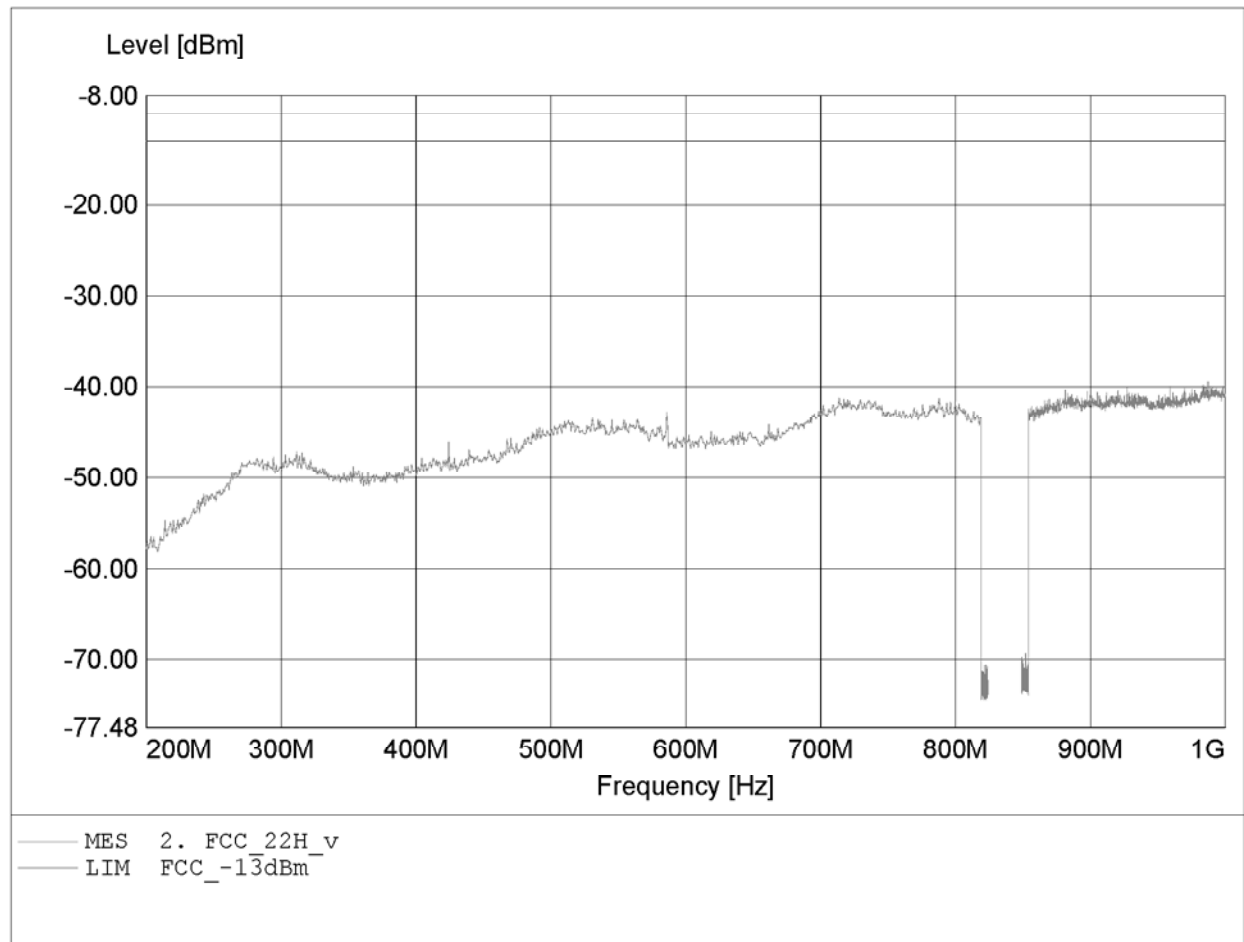


Radiated Emissions Tx
FCC RULES PART 22 SUBPART H

Approval Holder: BIOTRONIK GmbH & CO. KG
EUT : TELEX III
Model / Channel : CARDIOMESSENGER II / 188
Temperature/ Voltage: Temp.: 23°C / Unom.: 4.20 V DC
Test Site / Operator: ETS / Mr. Handrik
Test Specification: according to §22.917
Comment 1: Dist.: 3m, Ant.: HL 223+notch
Comment 2: Freq: 896.827MHz, Pmax: -37.79dBm, RBW: 1MHz

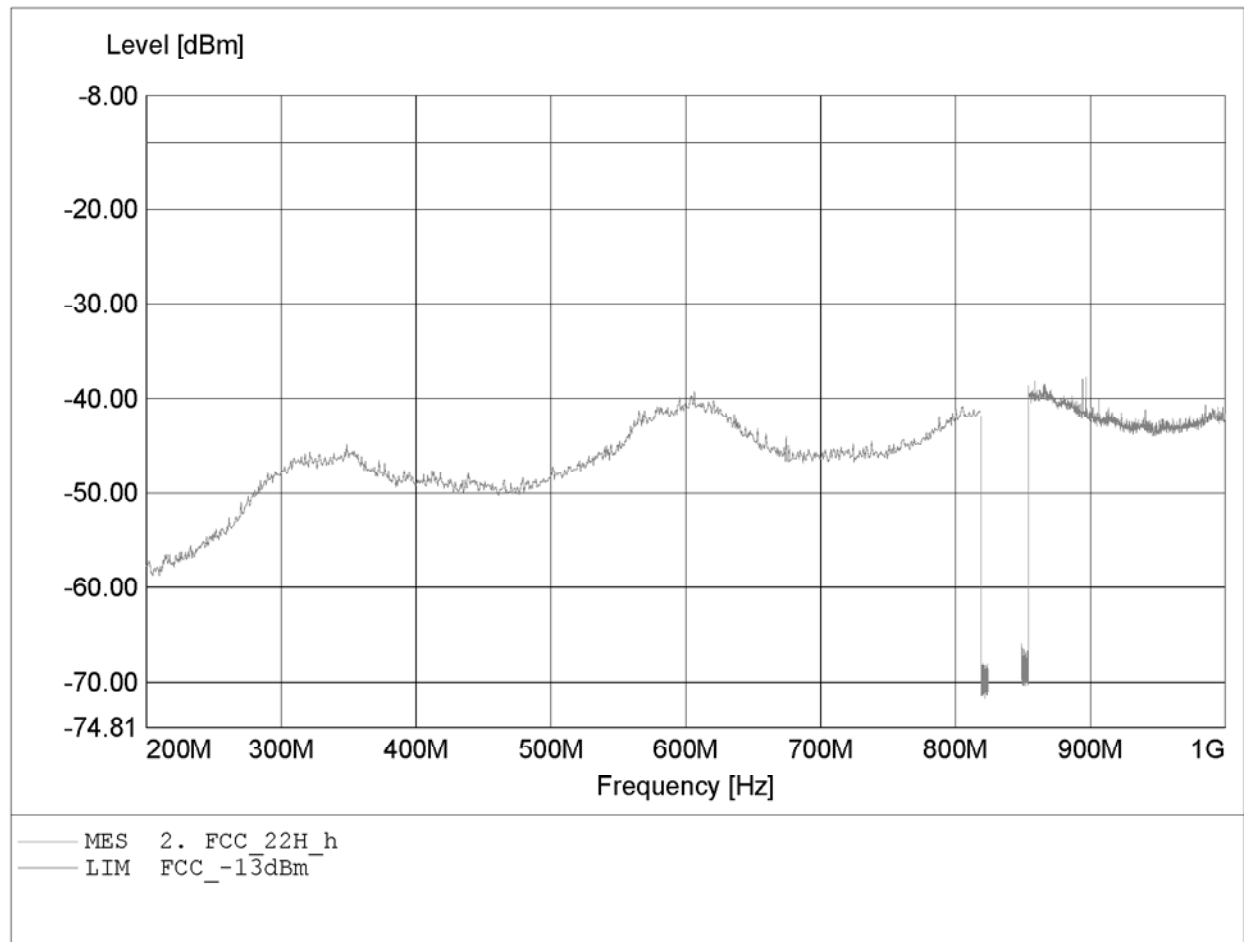


Radiated Emissions Tx
FCC RULES PART 22 SUBPART H

Approval Holder: BIOTRONIK GmbH & CO. KG
EUT : TELEX III
Model / Channel : CARDIOMESSENGER II / 188
Temperature/ Voltage: Temp.: 23°C / Unom.: 4.20 V DC
Test Site / Operator: ETS / Mr. Handrik
Test Specification: according to §22.917
Comment 1: Dist.: 3m, Ant.: HL025
Comment 2: Freq: 1.677GHz, Pmax: -18.94dBm, RBW: 1MHz

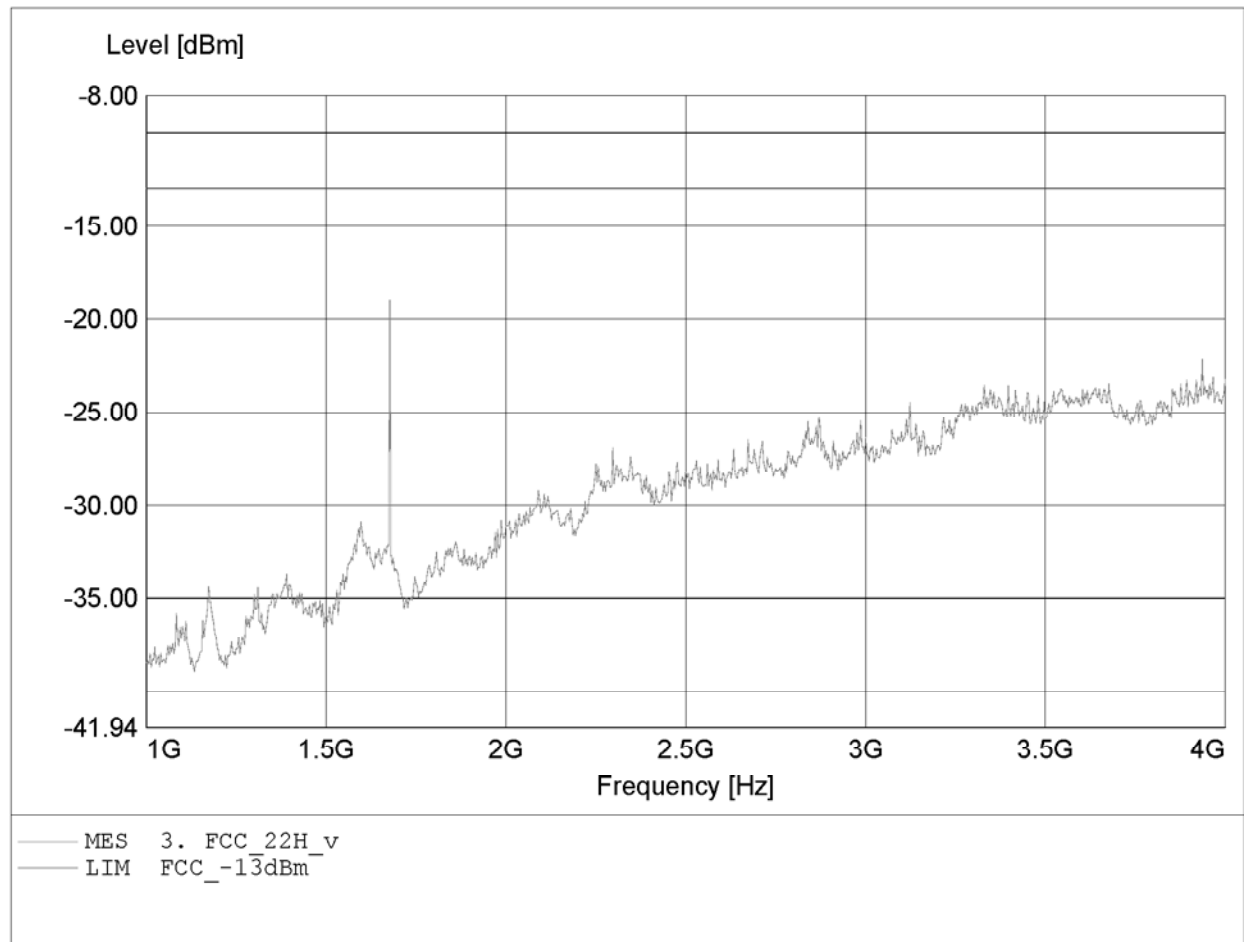


Radiated Emissions Tx
FCC RULES PART 22 SUBPART H

Approval Holder: BIOTRONIK GmbH & CO. KG
EUT : TELEX III
Model / Channel : CARDIOMESSENGER II / 188
Temperature/ Voltage: Temp.: 23°C / Unom.: 4.20 V DC
Test Site / Operator: ETS / Mr. Handrik
Test Specification: according to §22.917
Comment 1: Dist.: 3m, Ant.: HL025
Comment 2: Freq: 1.677GHz, Pmax: -19.74dBm, RBW: 1MHz

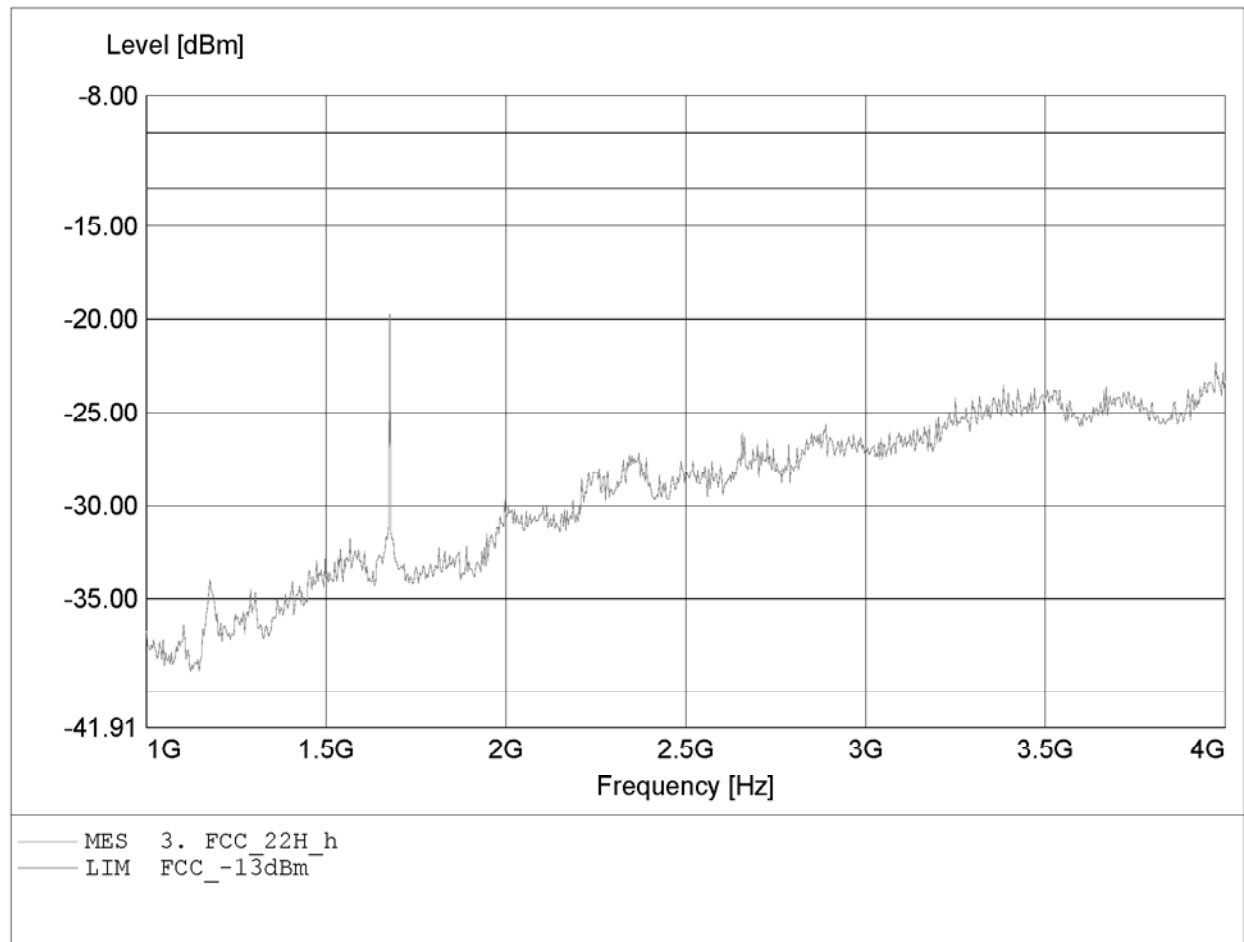


Radiated Emissions Tx
FCC RULES PART 22 SUBPART H

Approval Holder: BIOTRONIK GmbH & CO. KG
EUT : TELEX III
Model / Channel : CARDIOMESSENGER II / 188
Temperature/ Voltage: Temp.: 23°C / Unom.: 4.20 V DC
Test Site / Operator: ETS / Mr. Handrik
Test Specification: according to §22.917
Comment 1: Dist.: 3m, Ant.: HL025, ampl.+HP.
Comment 2: Freq: 8.000GHz, Pmax: -45.40dBm, RBW: 1MHz

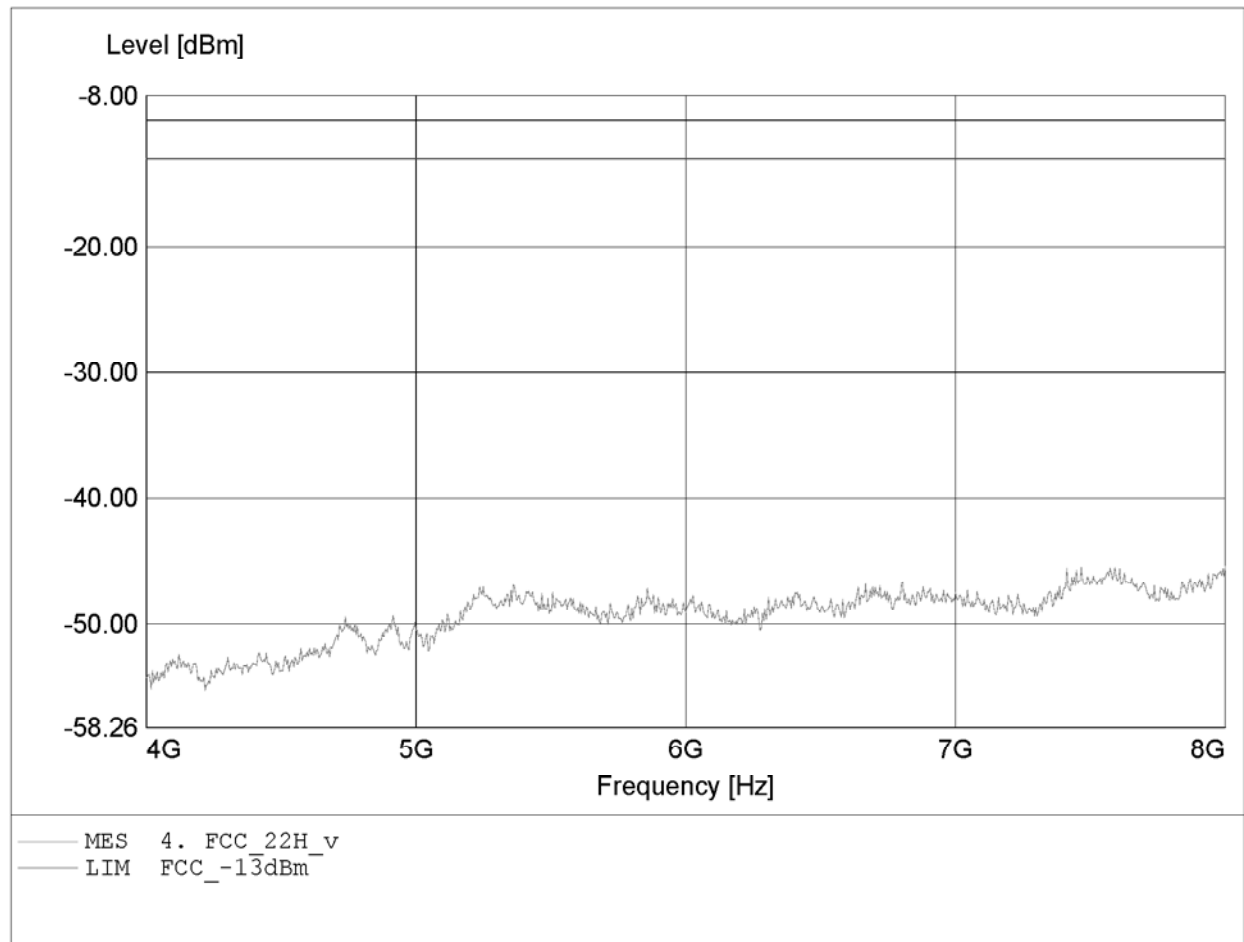


Radiated Emissions Tx
FCC RULES PART 22 SUBPART H

Approval Holder: BIOTRONIK GmbH & CO. KG
EUT : TELEX III
Model / Channel : CARDIOMESSENGER II / 188
Temperature/ Voltage: Temp.: 23°C / Unom.: 4.20 V DC
Test Site / Operator: ETS / Mr. Handrik
Test Specification: according to §22.917
Comment 1: Dist.: 3m, Ant.: HL025, ampl.+HP.
Comment 2: Freq: 7.987GHz, Pmax: -44.77dBm, RBW: 1MHz

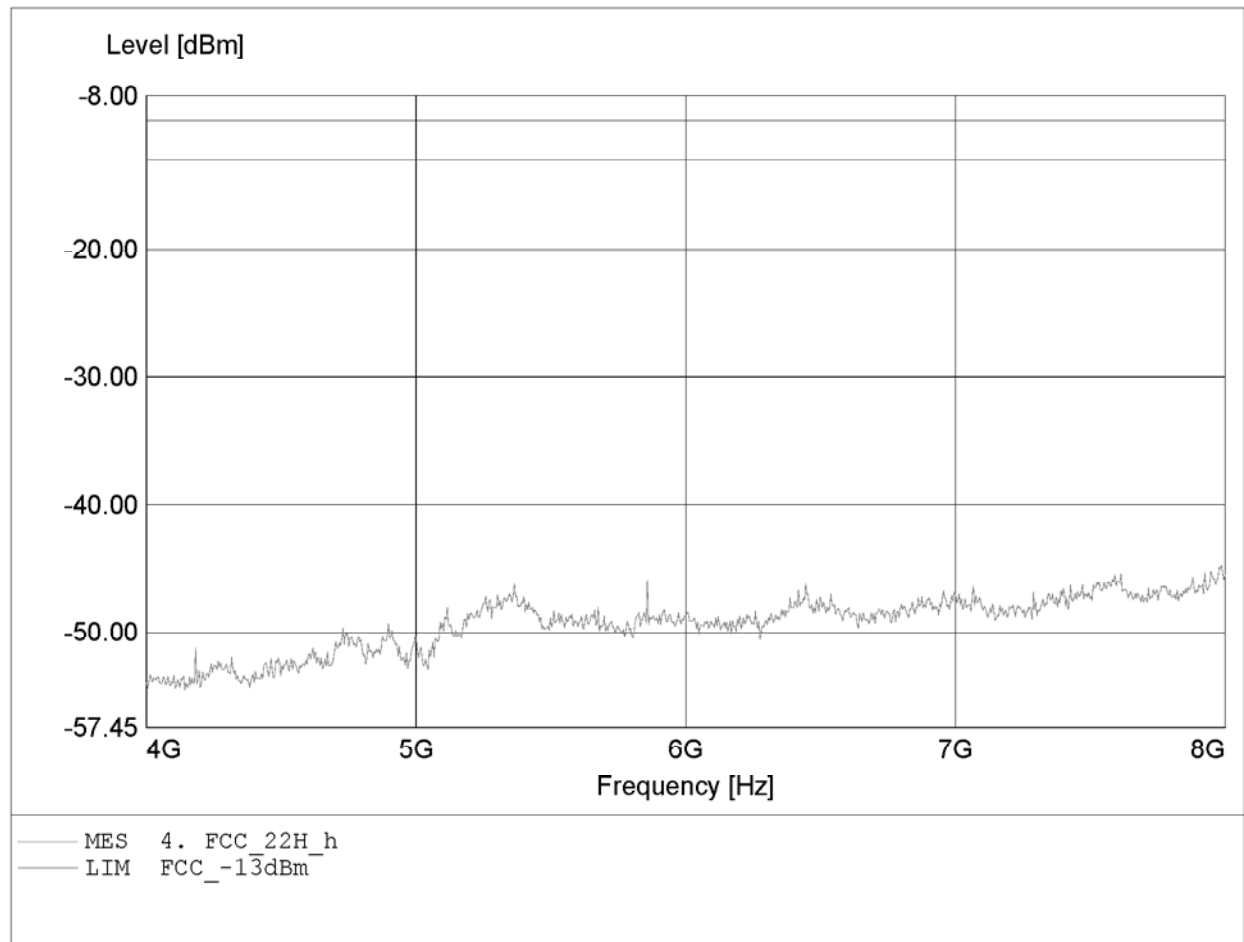


Radiated Emissions Tx
FCC RULES PART 22 SUBPART H

Approval Holder: BIOTRONIK GmbH & CO. KG
EUT : TELEX III
Model / Channel : CARDIOMESSENGER II / 188
Temperature/ Voltage: Temp.: 23°C / Unom.: 4.20 V DC
Test Site / Operator: ETS / Mr. Handrik
Test Specification: according to §22.917
Comment 1: Dist.: 3m, Ant.: HL025, ampl.+HP.
Comment 2: Freq: 10.676GHz, Pmax: -40.92dBm, RBW: 1MHz

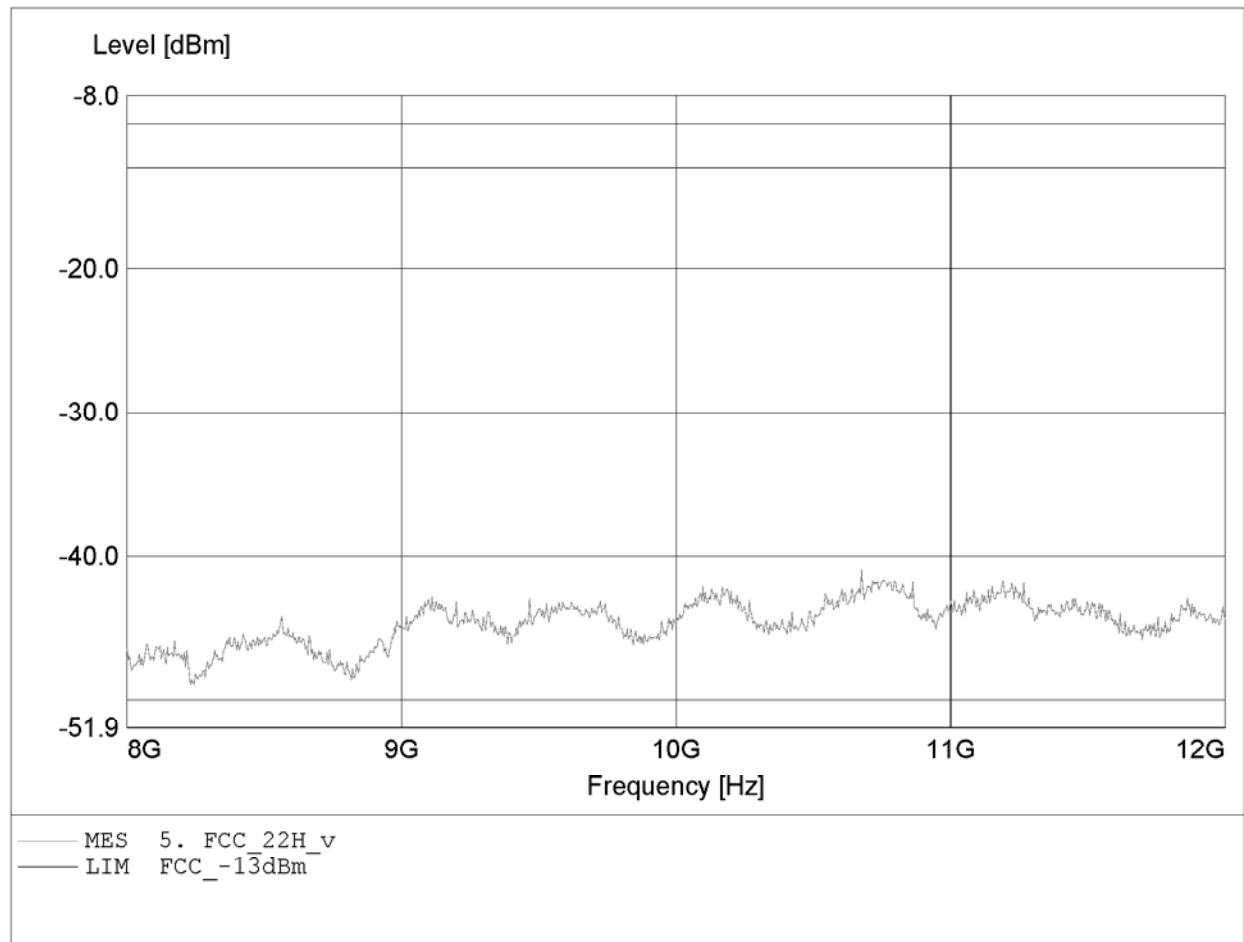


Radiated Emissions Tx
FCC RULES PART 22 SUBPART H

Approval Holder: BIOTRONIK GmbH & CO. KG
EUT : TELEX III
Model / Channel : CARDIOMESSENGER II / 188
Temperature/ Voltage: Temp.: 23°C / Unom.: 4.20 V DC
Test Site / Operator: ETS / Mr. Handrik
Test Specification: according to §22.917
Comment 1: Dist.: 3m, Ant.: HL025, ampl.+HP.
Comment 2: Freq: 10.742GHz, Pmax: -40.14dBm, RBW: 1MHz

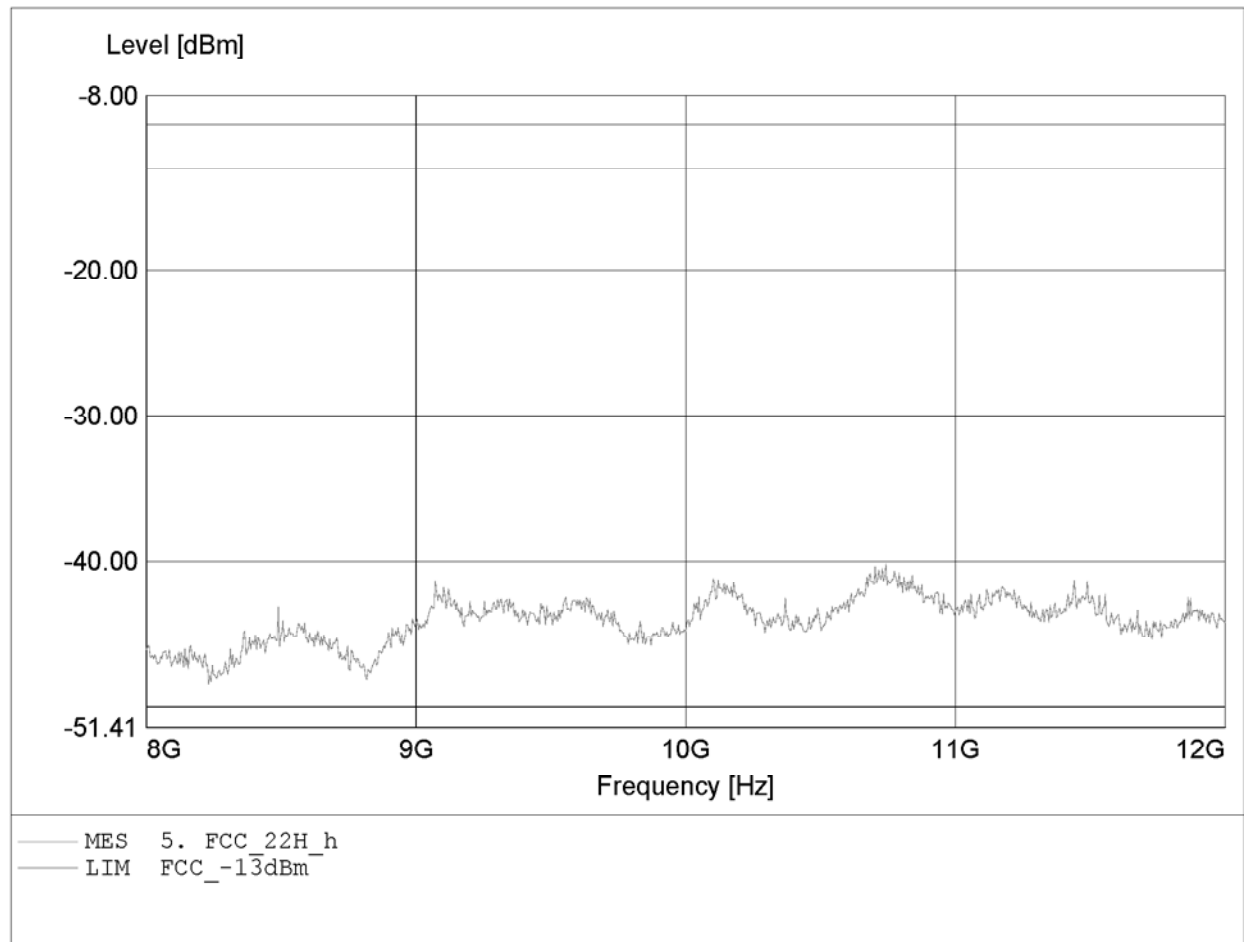


Radiated Emissions Tx
FCC RULES PART 22 SUBPART H

Approval Holder: BIOTRONIK GmbH & CO. KG
EUT : TELEX III
Model / Channel : CARDIOMESSENGER II / 251
Temperature/ Voltage: Temp.: 23°C / Unom.: 4.20 V DC
Test Site / Operator: ETS / Mr. Handrik
Test Specification: according to §22.917
Comment 1: Dist.: 3m, Ant.: HK 116
Comment 2: Freq: 61.356MHz, Pmax: -52.13dBm, RBW: 1MHz

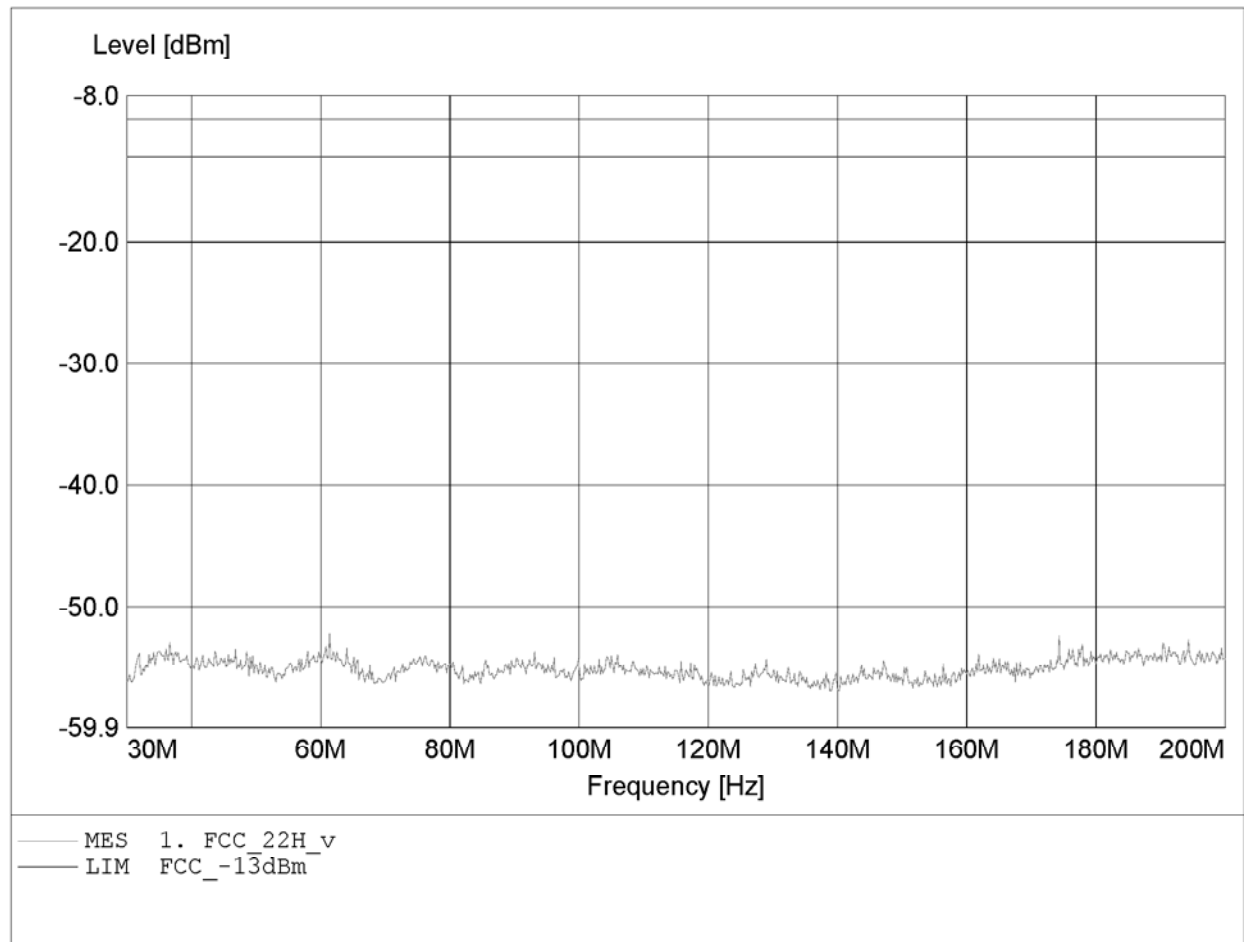


Radiated Emissions Tx
FCC RULES PART 22 SUBPART H

Approval Holder: BIOTRONIK GmbH & CO. KG
EUT : TELEX III
Model / Channel : CARDIOMESSENGER II / 251
Temperature/ Voltage: Temp.: 23°C / Unom.: 4.20 V DC
Test Site / Operator: ETS / Mr. Handrik
Test Specification: according to §22.917
Comment 1: Dist.: 3m, Ant.: HK 116
Comment 2: Freq: 34.722MHz, Pmax: -51.38dBm, RBW: 1MHz

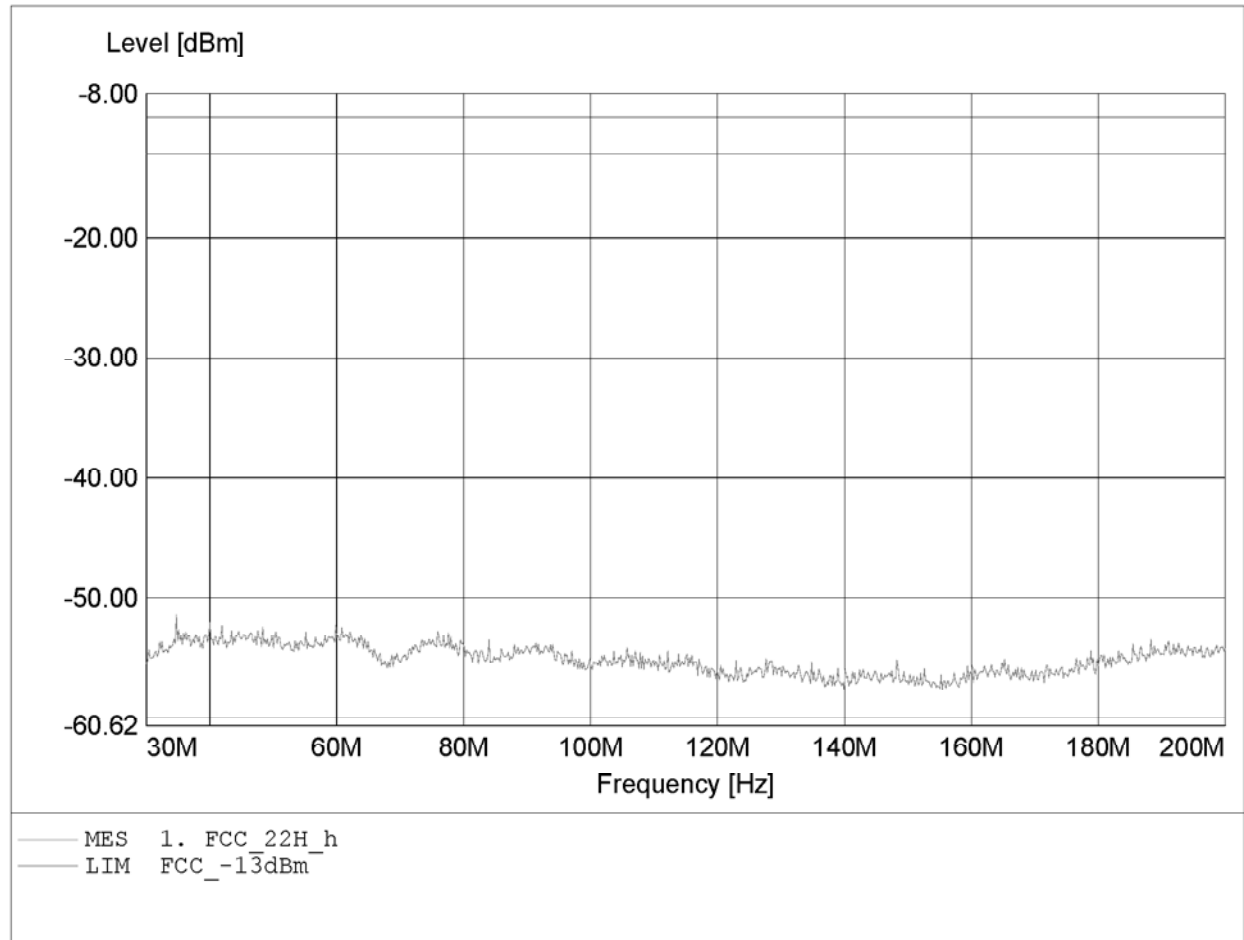


Radiated Emissions Tx
FCC RULES PART 22 SUBPART H

Approval Holder: BIOTRONIK GmbH & CO. KG
EUT : TELEX III
Model / Channel : CARDIOMESSENGER II / 251
Temperature/ Voltage: Temp.: 23°C / Unom.: 4.20 V DC
Test Site / Operator: ETS / Mr. Handrik
Test Specification: according to §22.917
Comment 1: Dist.: 3m, Ant.: HL 223+notch
Comment 2: Freq: 849.017MHz, Pmax: -22.89dBm, RBW: 1MHz

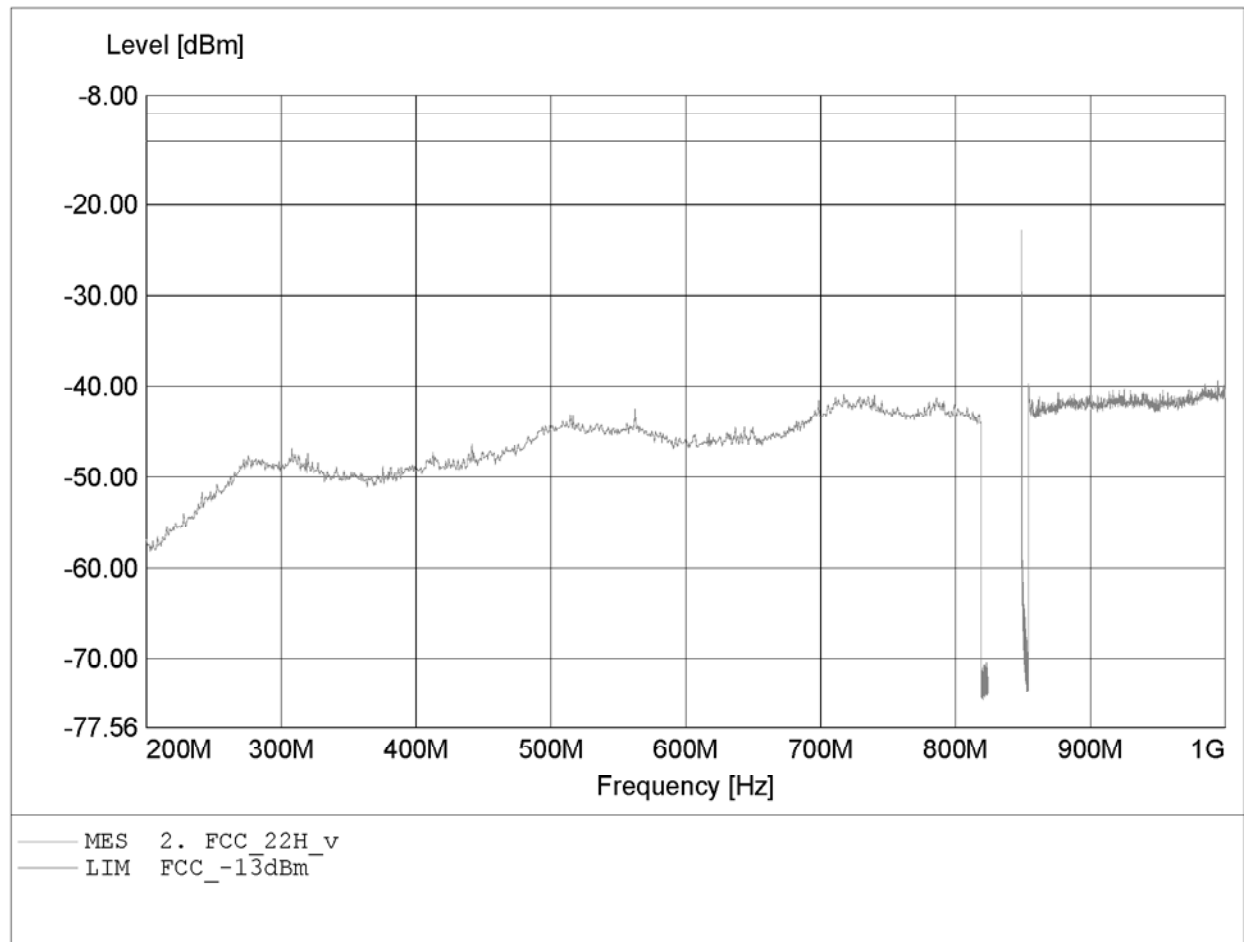


Radiated Emissions Tx
FCC RULES PART 22 SUBPART H

Approval Holder: BIOTRONIK GmbH & CO. KG
EUT : TELEX III
Model / Channel : CARDIOMESSENGER II / 251
Temperature/ Voltage: Temp.: 23°C / Unom.: 4.20 V DC
Test Site / Operator: ETS / Mr. Handrik
Test Specification: according to §22.917
Comment 1: Dist.: 3m, Ant.: HL 223+notch
Comment 2: Freq: 849.017MHz, Pmax: -28.06dBm, RBW: 1MHz

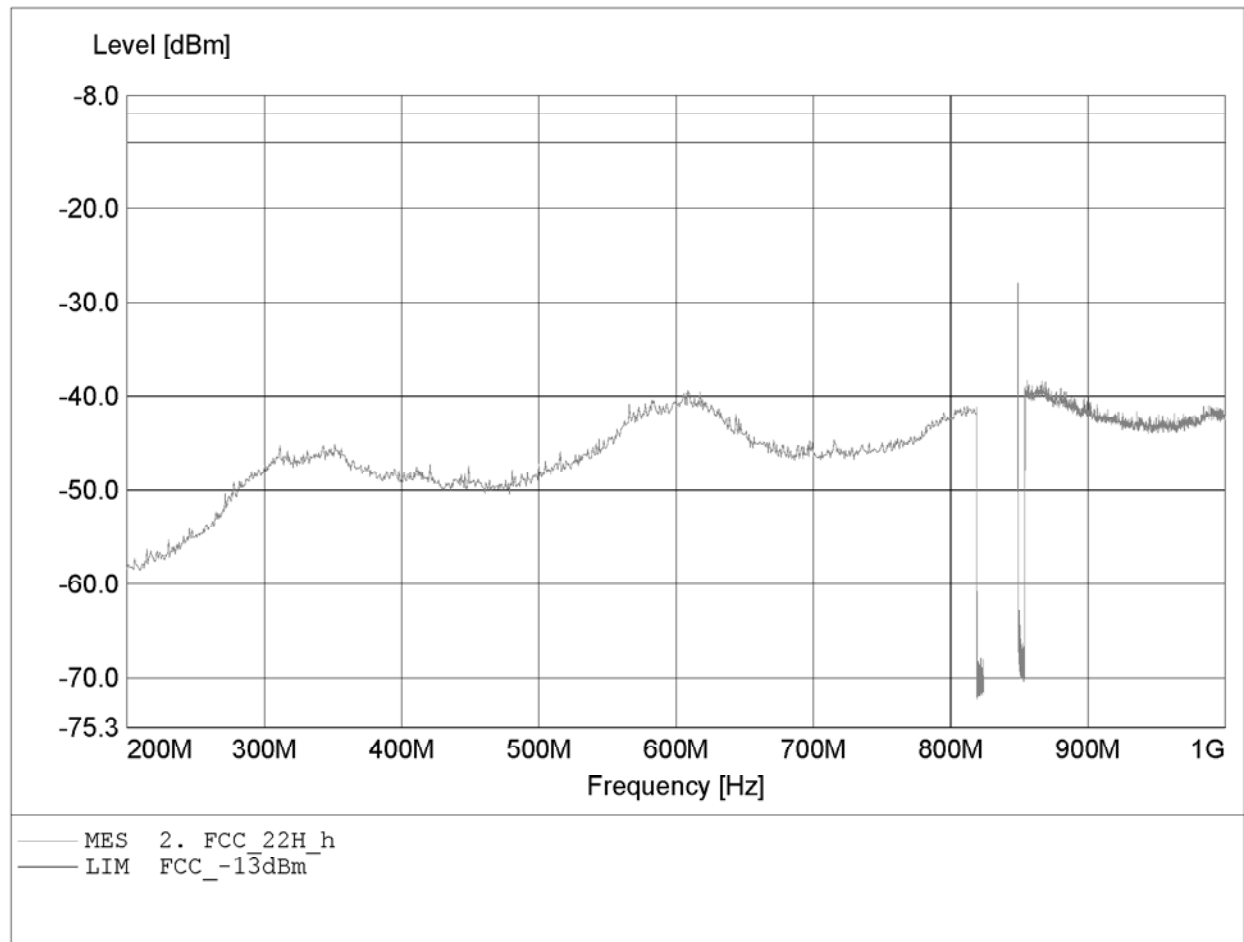


Radiated Emissions Tx
FCC RULES PART 22 SUBPART H

Approval Holder: BIOTRONIK GmbH & CO. KG
EUT : TELEX III
Model / Channel : CARDIOMESSENGER II / 251
Temperature/ Voltage: Temp.: 23°C / Unom.: 4.20 V DC
Test Site / Operator: ETS / Mr. Handrik
Test Specification: according to §22.917
Comment 1: Dist.: 3m, Ant.: HL025
Comment 2: Freq: 1.700GHz, Pmax: -18.67dBm, RBW: 1MHz

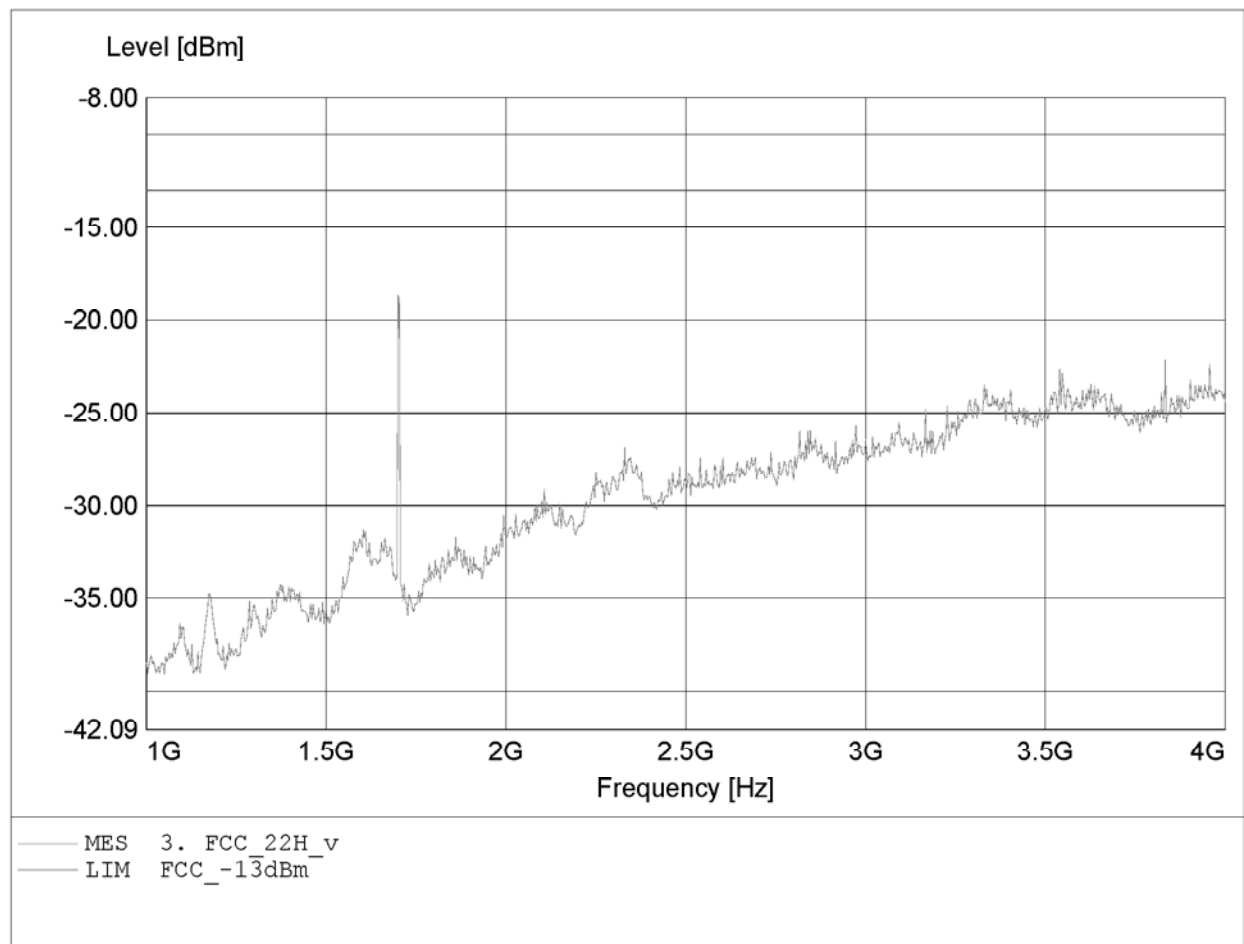


Radiated Emissions Tx
FCC RULES PART 22 SUBPART H

Approval Holder: BIOTRONIK GmbH & CO. KG
EUT : TELEX III
Model / Channel : CARDIOMESSENGER II / 251
Temperature/ Voltage: Temp.: 23°C / Unom.: 4.20 V DC
Test Site / Operator: ETS / Mr. Handrik
Test Specification: according to §22.917
Comment 1: Dist.: 3m, Ant.: HL025
Comment 2: Freq: 1.703GHz, Pmax: -17.70dBm, RBW: 1MHz

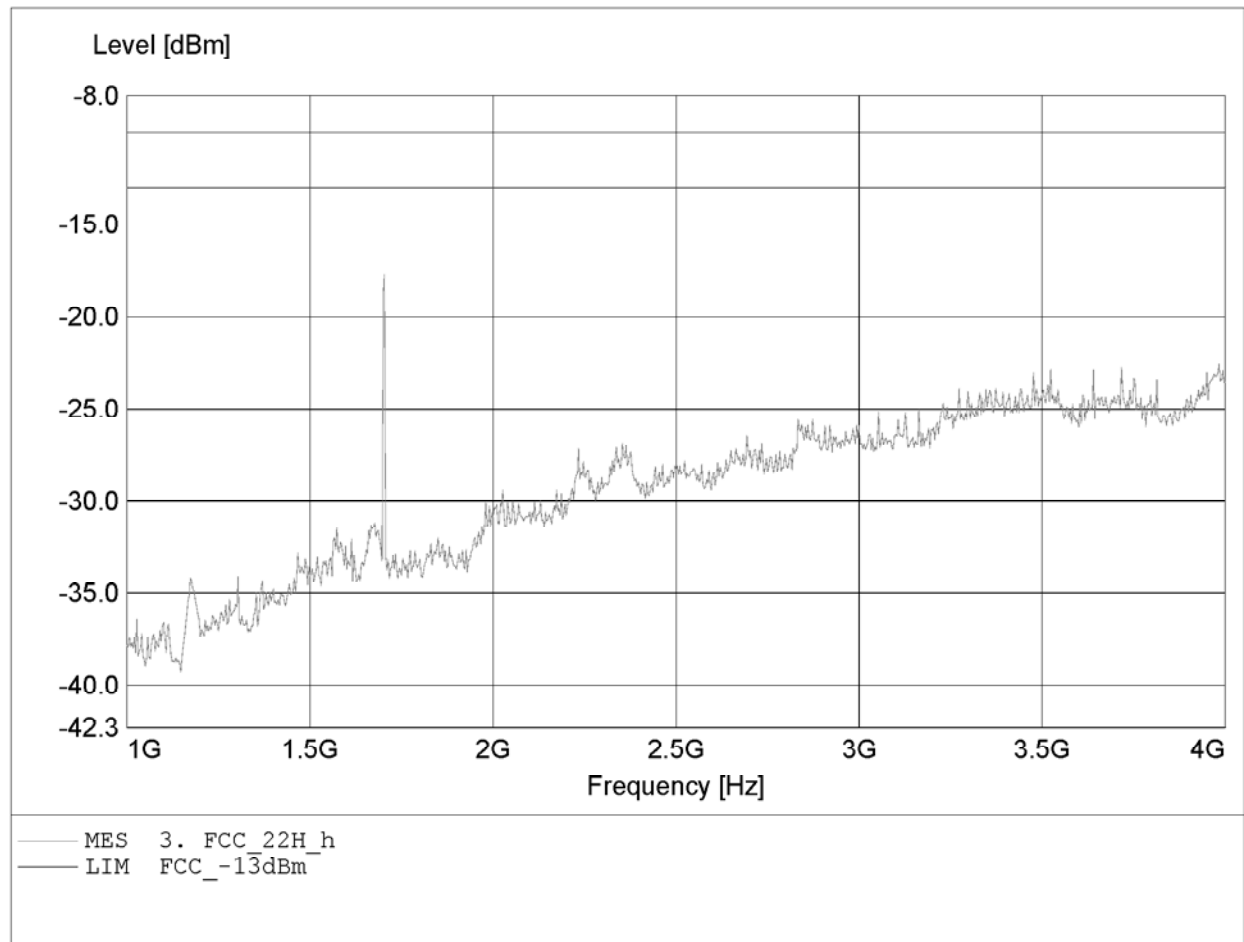


Radiated Emissions Tx
FCC RULES PART 22 SUBPART H

Approval Holder: BIOTRONIK GmbH & CO. KG
EUT : TELEX III
Model / Channel : CARDIOMESSENGER II / 251
Temperature/ Voltage: Temp.: 23°C / Unom.: 4.20 V DC
Test Site / Operator: ETS / Mr. Handrik
Test Specification: according to §22.917
Comment 1: Dist.: 3m, Ant.: HL025, ampl.+HP.
Comment 2: Freq: 7.493GHz, Pmax: -44.89dBm, RBW: 1MHz

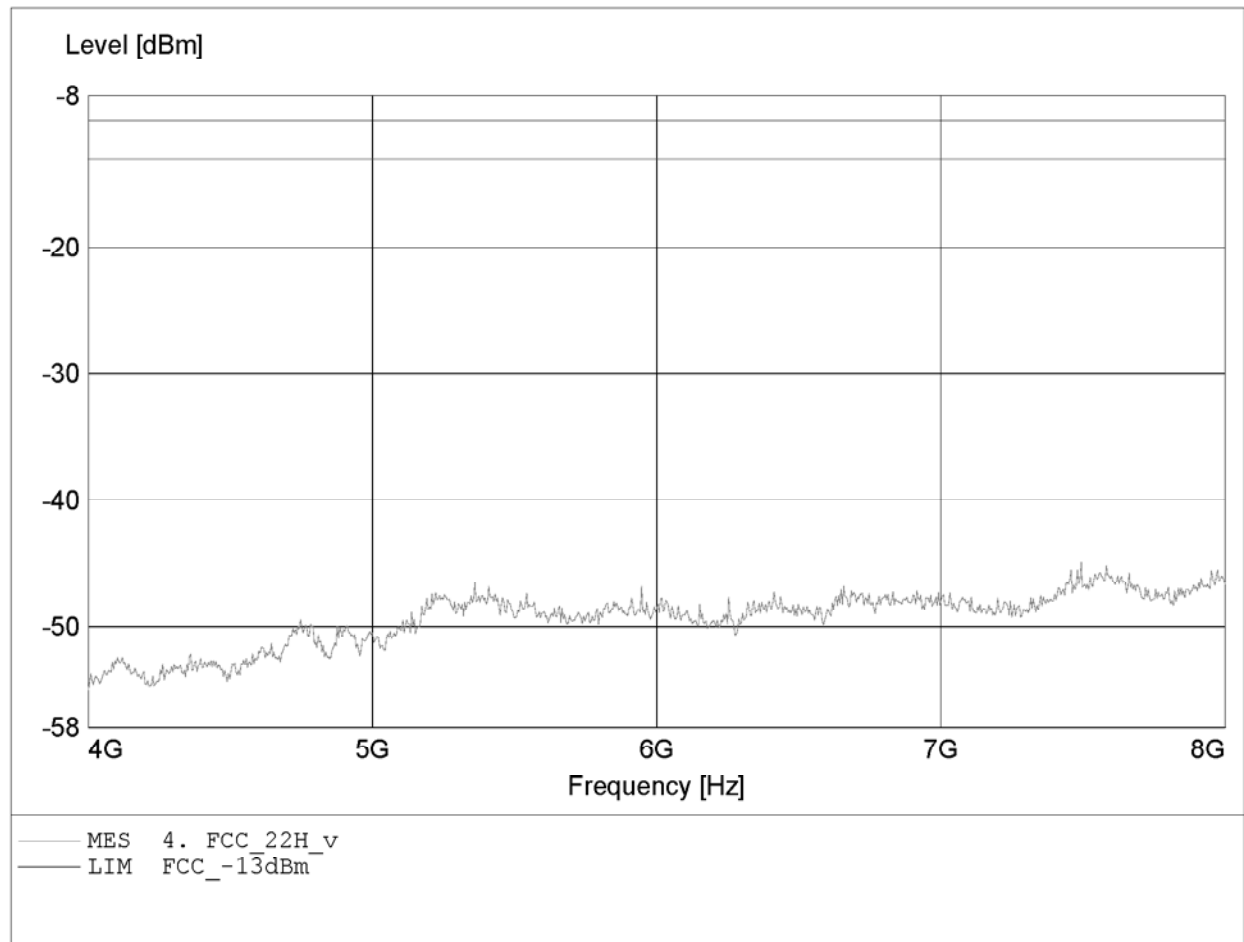


Radiated Emissions Tx
FCC RULES PART 22 SUBPART H

Approval Holder: BIOTRONIK GmbH & CO. KG
EUT : TELEX III
Model / Channel : CARDIOMESSENGER II / 251
Temperature/ Voltage: Temp.: 23°C / Unom.: 4.20 V DC
Test Site / Operator: ETS / Mr. Handrik
Test Specification: according to §22.917
Comment 1: Dist.: 3m, Ant.: HL025, ampl.+HP.
Comment 2: Freq: 7.973GHz, Pmax: -43.94dBm, RBW: 1MHz

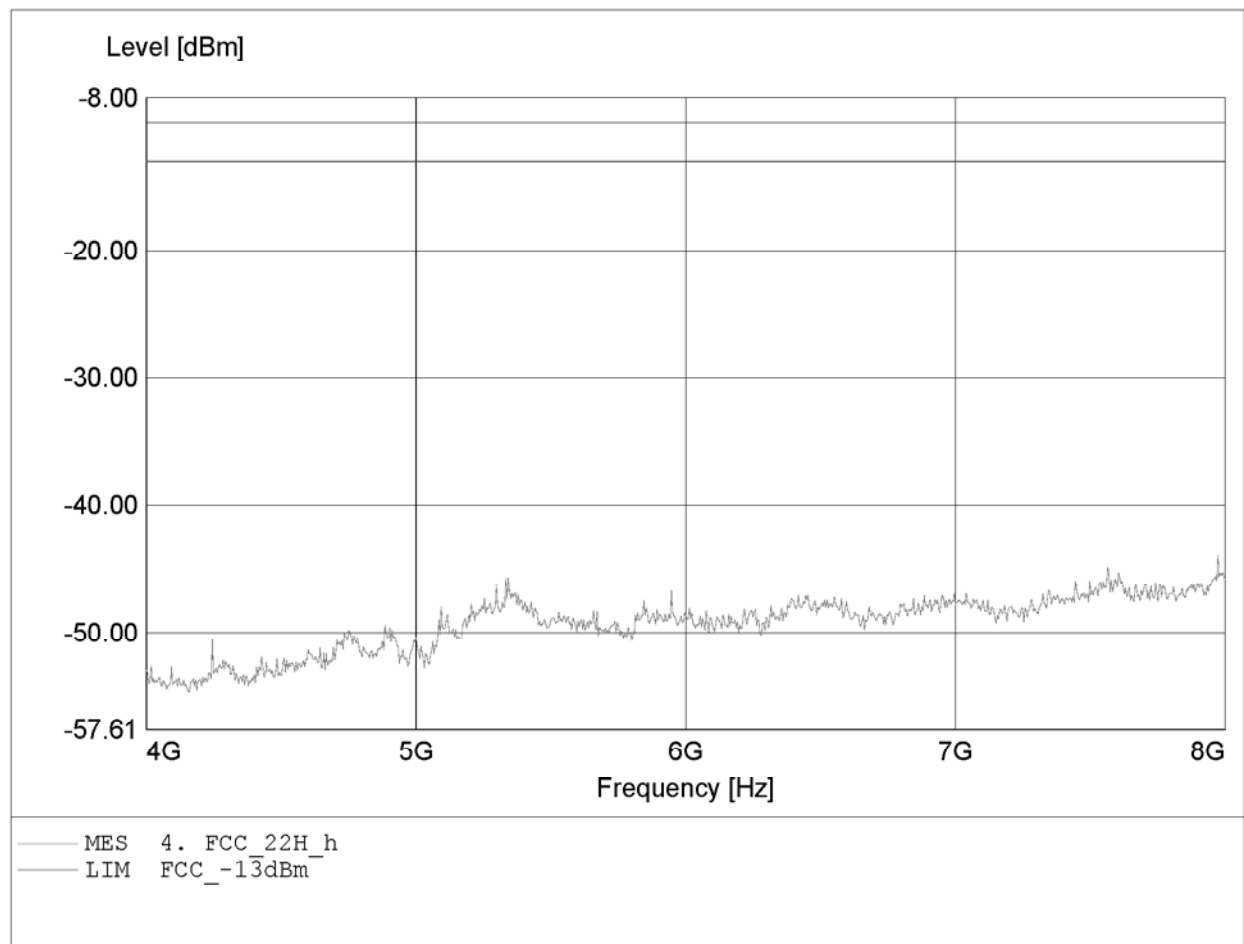


Radiated Emissions Tx
FCC RULES PART 22 SUBPART H

Approval Holder: BIOTRONIK GmbH & CO. KG
EUT : TELEX III
Model / Channel : CARDIOMESSENGER II / 251
Temperature/ Voltage: Temp.: 23°C / Unom.: 4.20 V DC
Test Site / Operator: ETS / Mr. Handrik
Test Specification: according to §22.917
Comment 1: Dist.: 3m, Ant.: HL025, ampl.+HP.
Comment 2: Freq: 10.769GHz, Pmax: -41.11dBm, RBW: 1MHz

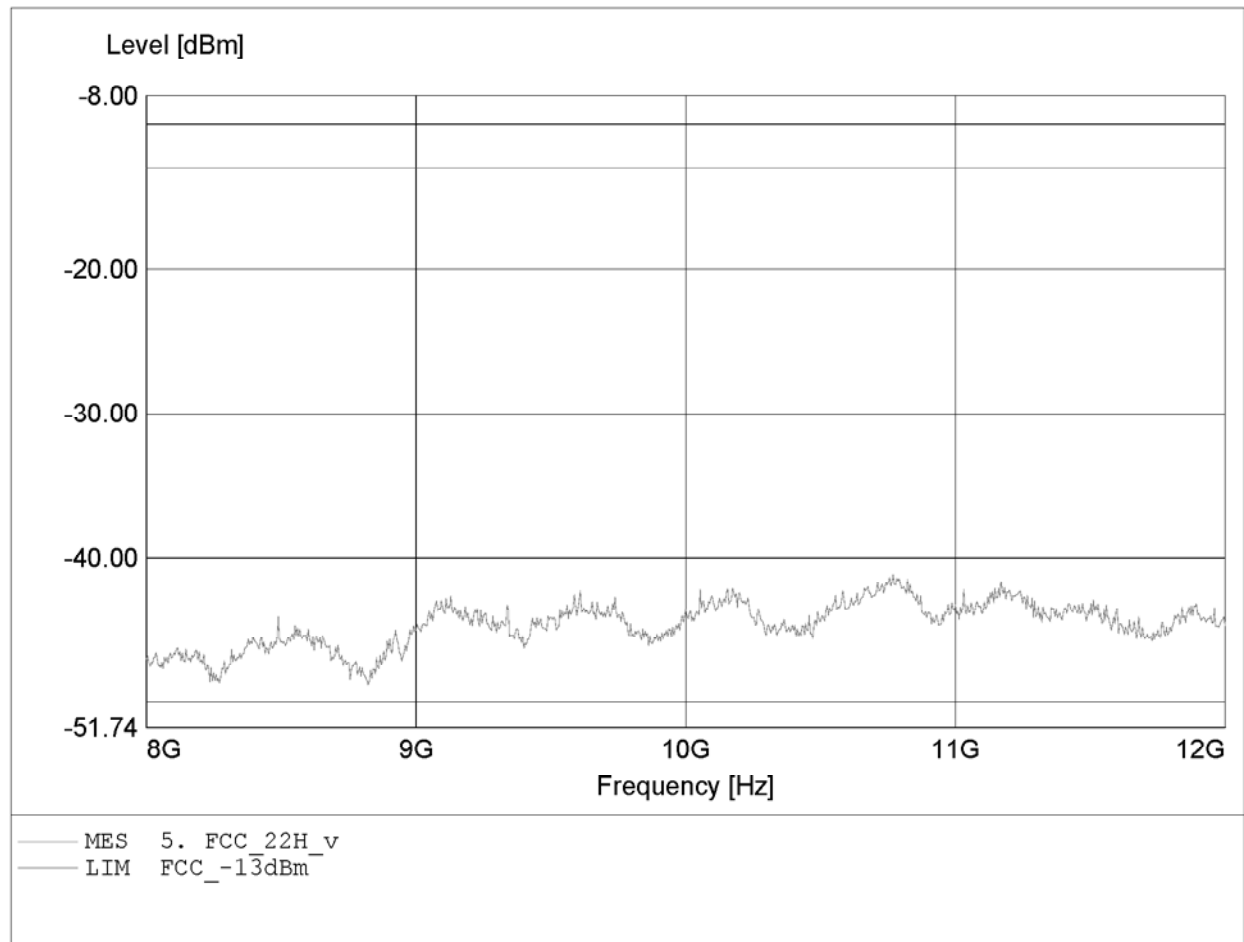

Radiated Emissions Tx
FCC RULES PART 22 SUBPART H

Approval Holder: BIOTRONIK GmbH & CO. KG
EUT : TELEX III
Model / Channel : CARDIOMESSENGER II / 251
Temperature/ Voltage: Temp.: 23°C / Unom.: 4.20 V DC
Test Site / Operator: ETS / Mr. Handrik
Test Specification: according to §22.917
Comment 1: Dist.: 3m, Ant.: HL025, ampl.+HP.
Comment 2: Freq: 10.738GHz, Pmax: -40.58dBm, RBW: 1MHz

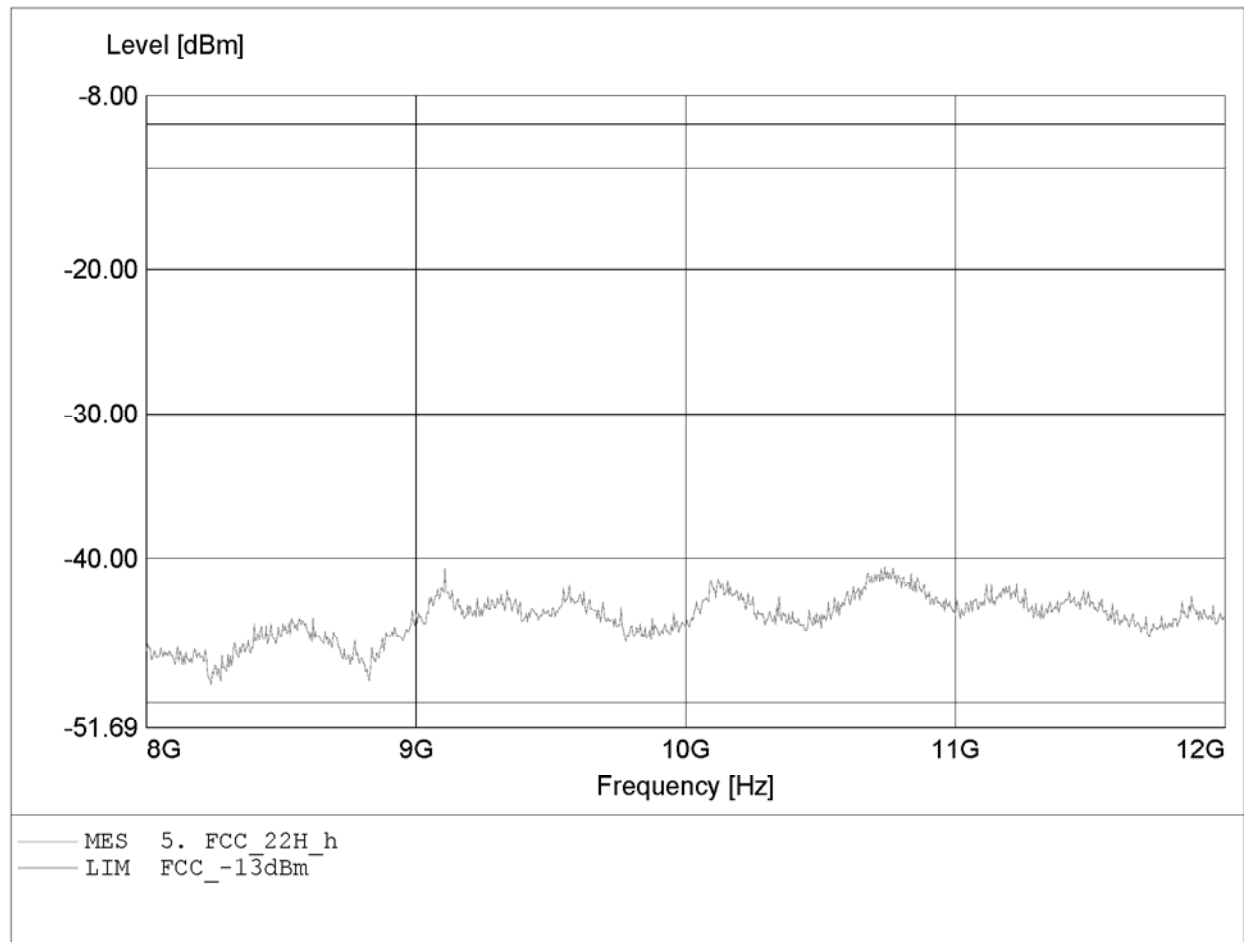

Appendix H


Block edge compliance

Appendix I

AC power line conducted emissions


EMI voltage test in the ac-mains according to FCC part 15

EUT: CARDIOMESSENGER II
Manufacturer: BIOTRONIK GmbH
Operating Condition: Unom: 120 V AC (AC/DC-ADAPTOR) , Tnom: 23°C
Test Site: ETS
Operator: Mr. Pflug
Test Specification: V-Network: ESH2-Z5 (L1)
Comment: model: TELEX mode: GSM, PSTN, CHARGING

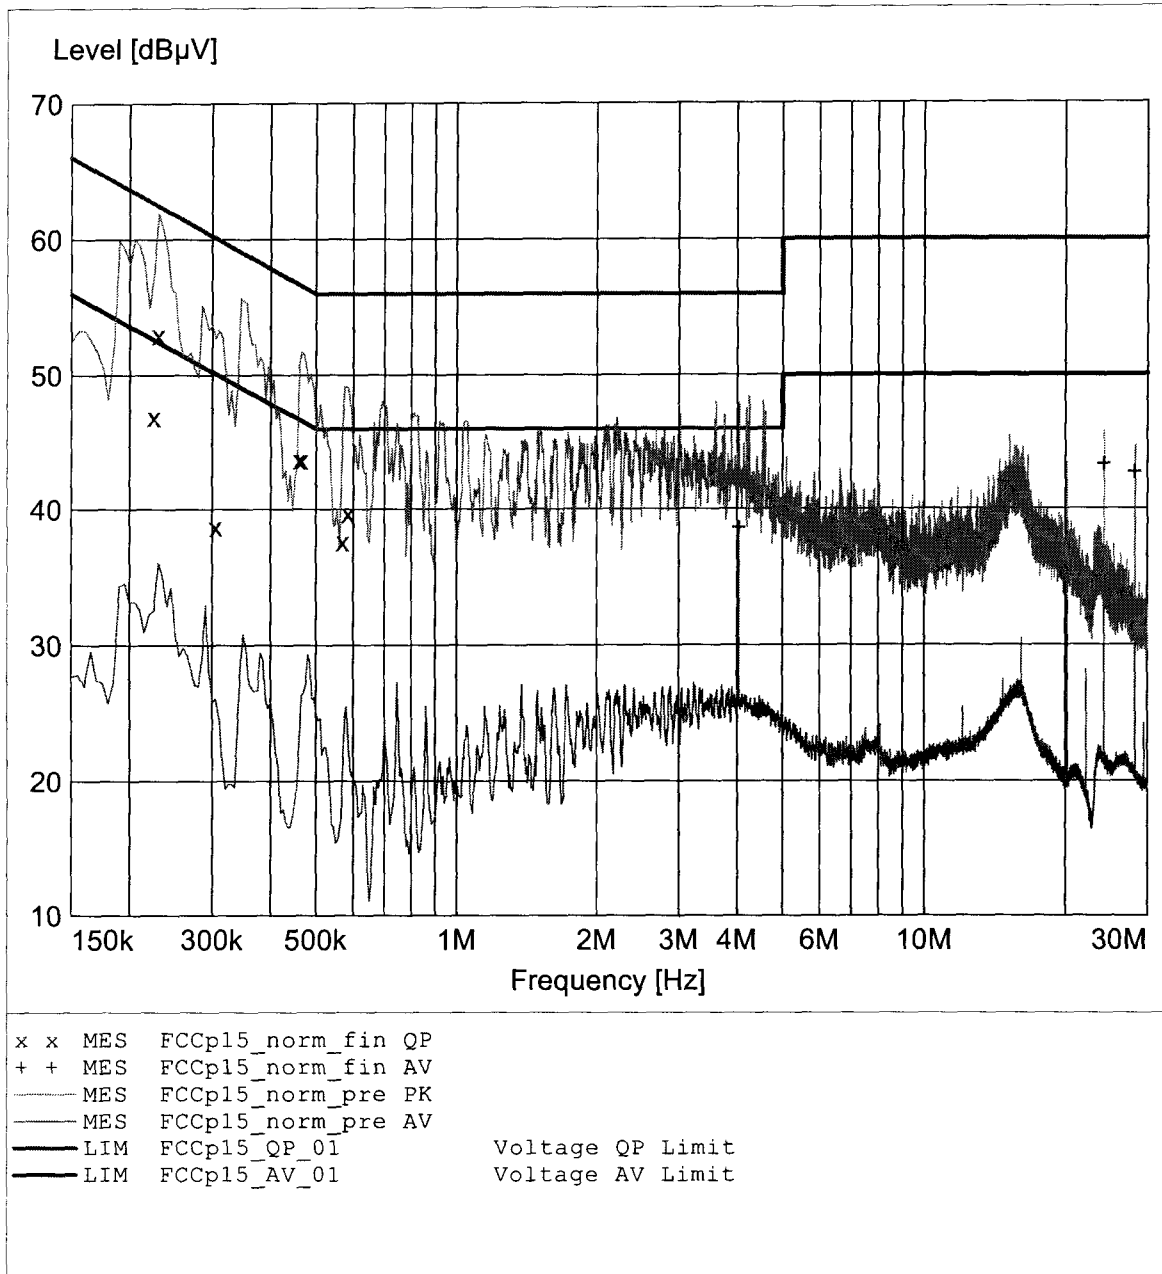

EMI voltage test in the ac-mains according to FCC part 15

EUT: CARDIOMESSENGER II
Manufacturer: BIOTRONIK GmbH
Operating Condition: Unom: 120 V AC (AC/DC-ADAPTOR) , Tnom: 23°C
Test Site: ETS
Operator: Mr. Pflug
Test Specification: V-Network: ESH2-Z5 (N)
Comment: model: TELEX mode: GSM, PSTN, CHARGING

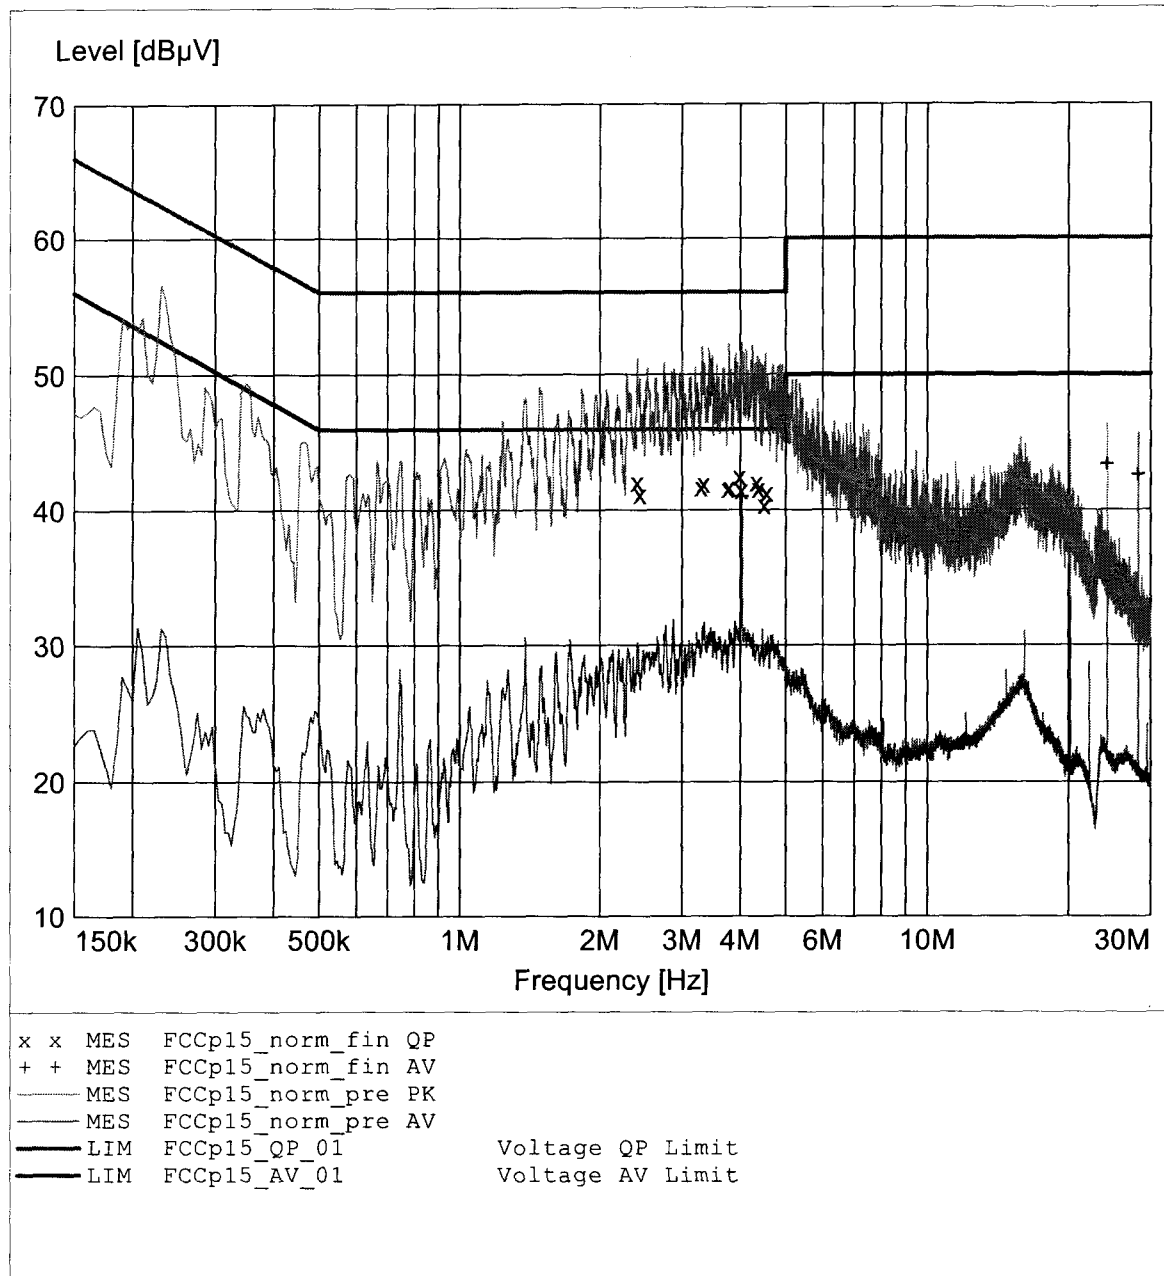


Appendix J

Receiver radiated emission

Receiver spurious emissions

in accordance to the EN 301 839


Approval Holder: Biotronik GmbH
EUT: Cardio messenger II
Model: Telex III / antenna (both, worst case), Ch.: 0
Test Site / Operator: ETS / Mr. Treffke
Temperature/ Voltage: 25°C / Unom: 3.7 V DC (lithium accu)
Test Specification: Fully anechoic chamber / mode: RX
Comment 1: Dist.: 3m, Ant.: HK 116, ampl.: None
Comment 2: Freq:156.393MHz Pmax:-67.90dBm RBW: 10/100 kHz

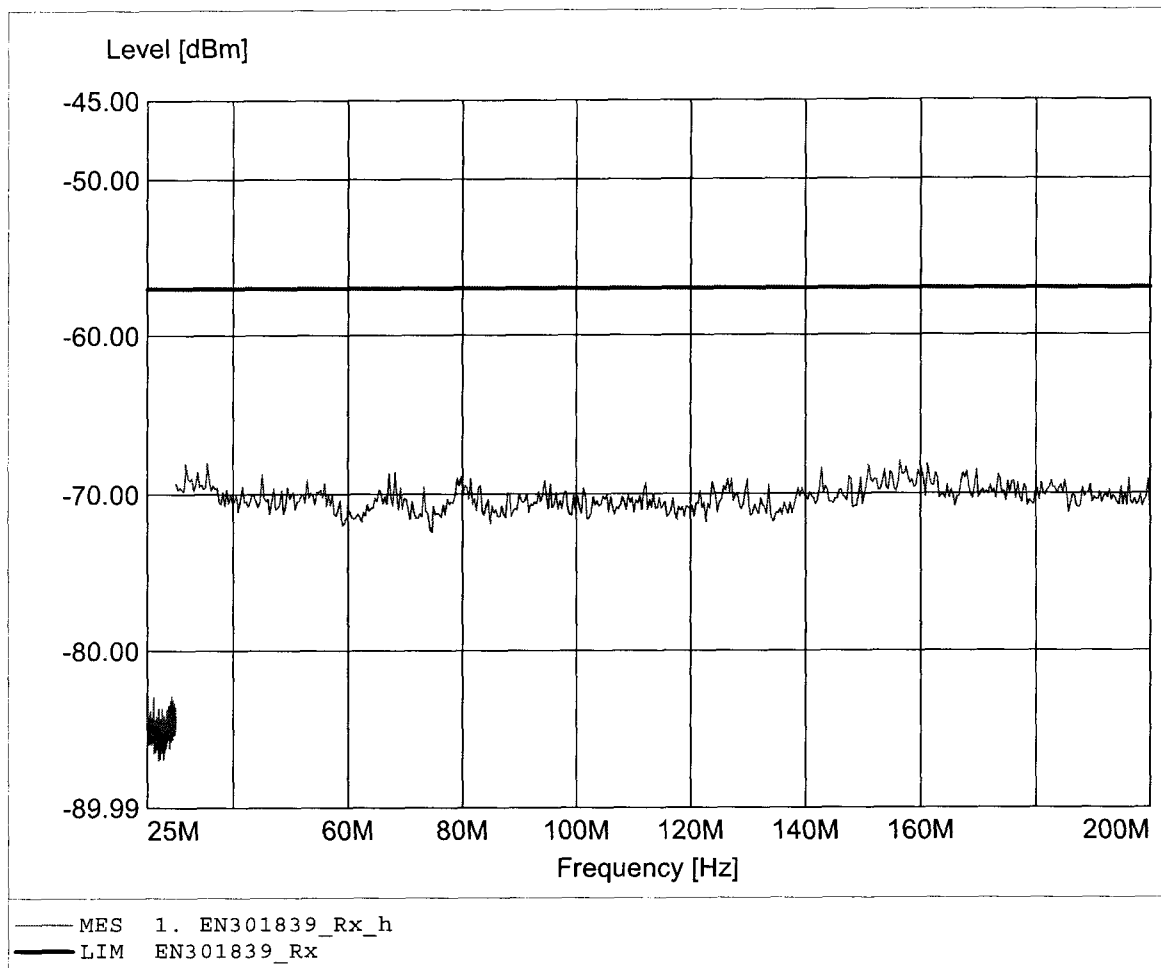

Receiver spurious emissions

in accordance to the EN 301 839


Approval Holder: Biotronik GmbH
EUT: Cardio messenger II
Model: Telex III / antenna (both, worst case), Ch.: 0
Test Site / Operator: ETS / Mr. Treffke
Temperature/ Voltage: 25°C / Unom: 3.7 V DC (lithium accu)
Test Specification: Fully anechoic chamber / mode: RX
Comment 1: Dist.: 3m, Ant.: HK 116, ampl.: None
Comment 2: Freq:159.118MHz Pmax:-65.26dBm RBW: 10/100 kHz

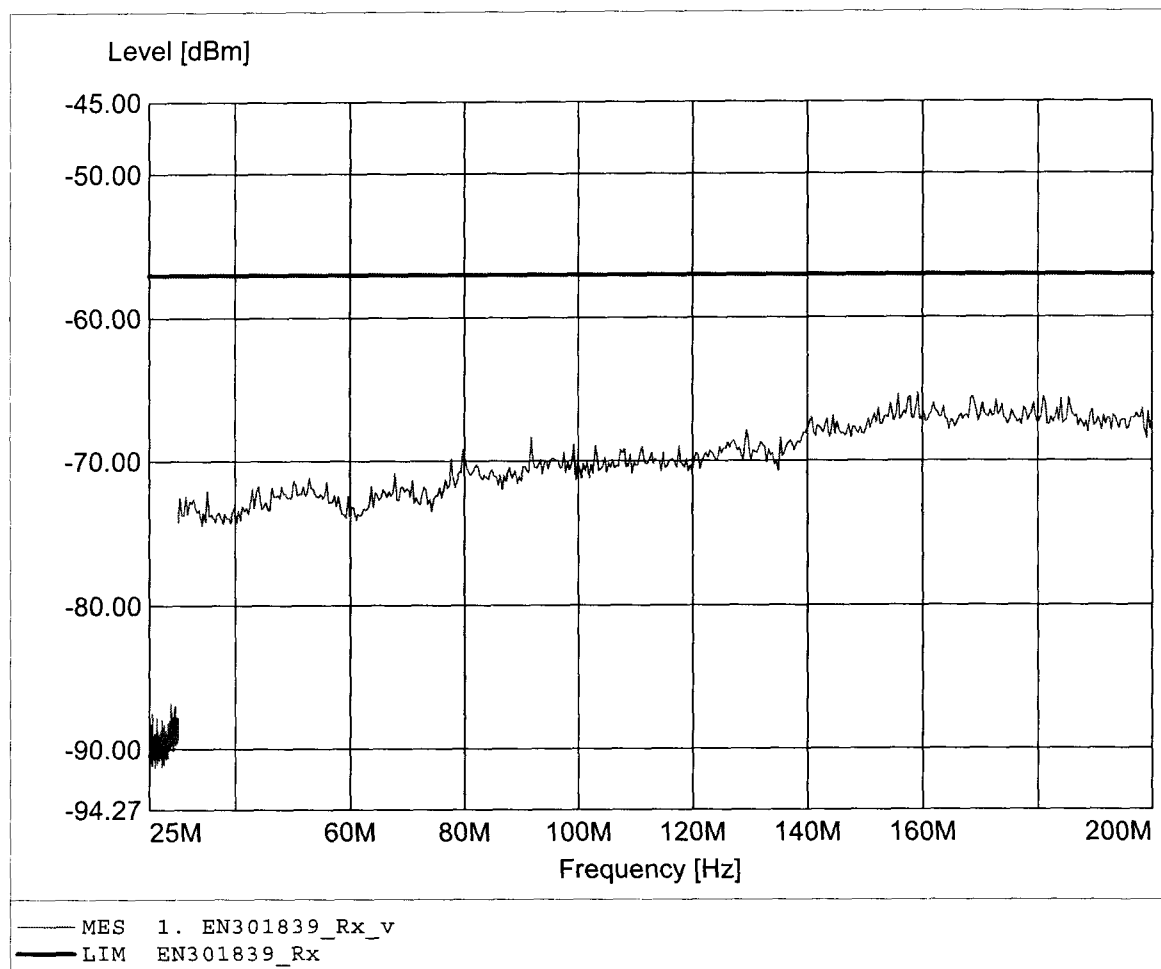

Receiver spurious emissions

in accordance to the EN 301 839


Approval Holder: Biotronik GmbH
EUT: Cardio messenger II
Model: Telex III / antenna (both, worst case), Ch.: 0
Test Site / Operator: ETS / Mr. Treffke
Temperature/ Voltage: 25°C / Unom: 3.7 V DC (lithium accu)
Test Specification: Fully anechoic chamber / mode: RX
Comment 1: Dist.: 3m, Ant.: HL 223, ampl.: 0.1-1GHz
Comment 2: Freq: 818.838MHz Pmax: -76.86dBm RBW: 100 kHz

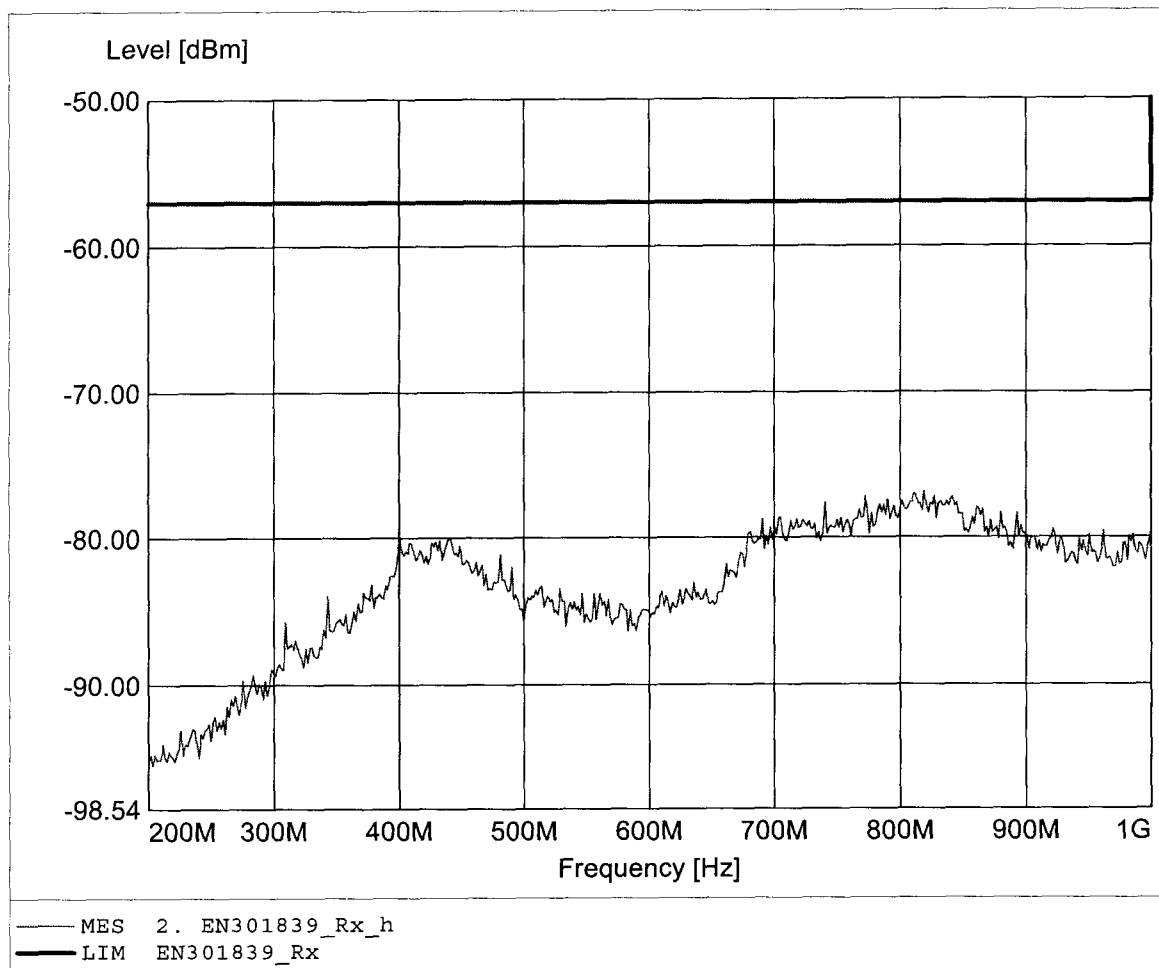

Receiver spurious emissions

in accordance to the EN 301 839


Approval Holder: Biotronik GmbH
EUT: Cardio messenger II
Model: Telex III / antenna (both, worst case), Ch.: 0
Test Site / Operator: ETS / Mr. Treffke
Temperature/ Voltage: 25°C / Unom: 3.7 V DC (lithium accu)
Test Specification: Fully anechoic chamber / mode: RX
Comment 1: Dist.: 3m, Ant.: HL 223, ampl.: 0.1-1GHz
Comment 2: Freq:897.395MHz Pmax:-76.62dBm RBW: 100 kHz

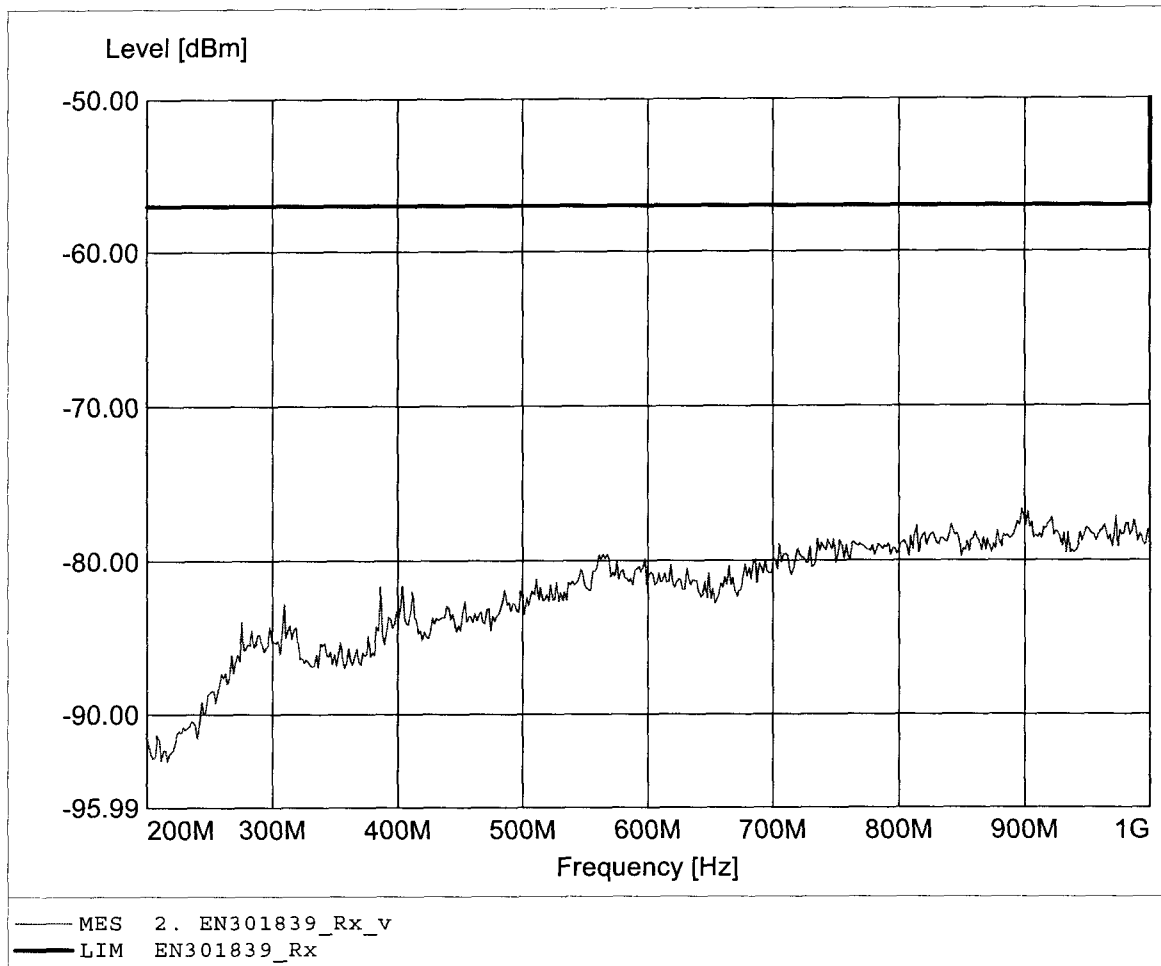

Receiver spurious emissions

in accordance to the EN 301 839

Approval Holder: Biotronik GmbH
EUT: Cardio messenger II
Model: Telex III / antenna (both, worst case), Ch.: 0
Test Site / Operator: ETS / Mr. Treffke
Temperature/ Voltage: 25°C / Unom: 3.7 V DC (lithium accu)
Test Specification: Fully anechoic chamber / mode: RX
Comment 1: Dist.: 1m, Ant.: HL 025, ampl.: 1-4GHz
Comment 2: Freq: 3.621GHz Pmax: -60.07dBm RBW: 1 MHz

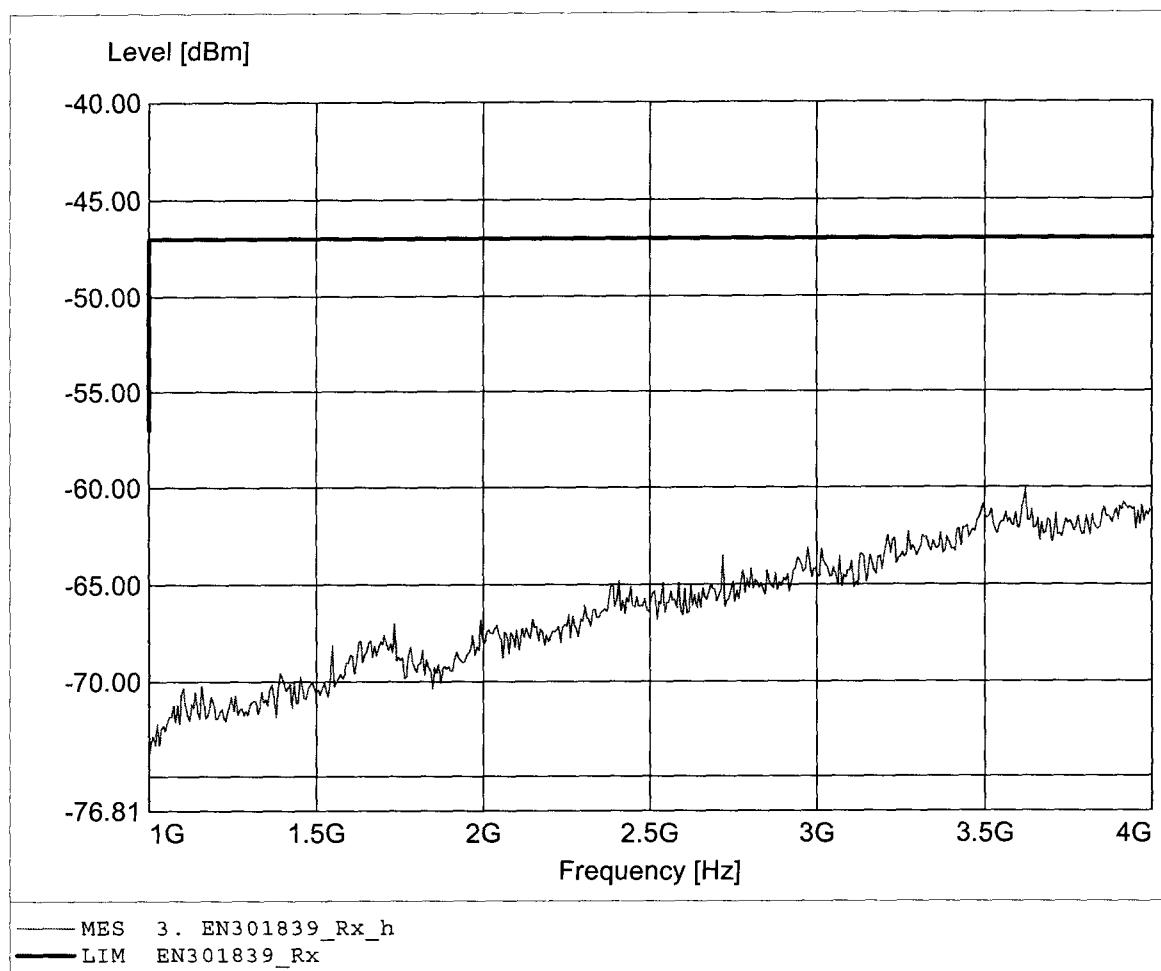

Receiver spurious emissions

in accordance to the EN 301 839

Approval Holder: Biotronik GmbH
EUT: Cardio messenger II
Model: Telex III / antenna (both, worst case), Ch.: 0
Test Site / Operator: ETS / Mr. Treffke
Temperature/ Voltage: 25°C / Unom: 3.7 V DC (lithium accu)
Test Specification: Fully anechoic chamber / mode: RX
Comment 1: Dist.: 1m, Ant.: HL 025, ampl.: 1-4GHz
Comment 2: Freq: 3.621GHz Pmax: -59.14dBm RBW: 1 MHz

