BIOTRONIK GmbH & Co. KG • Postfach 47 02 55 • 12311 Berlin

Federal Communications Commission
Equipment Authorization Branch
7435 Oakland Mills Road
Columbia, MD 21046
USA

Berlin, September 20, 2006

Re: Label Sample FCC ID: QRILUMAXT

BIOTRONIK GmbH & Co. KG
Woermannkehre 1
D-12359 Berlin
Steuer-Nr.: 30/062/05167
USt.-Ident Nr.: 136651322

Telefon (+49 30) 689 05-0
Telefax (+49 30) 689 05-1921
E-mail: info@biotronik.de
www.biotronik.de

Geschäftsführer:
Dr. Max Schaldach
Christoph Böhmer
Dr. Werner Braun
Dr. Lothar Krings

Kommanditgesellschaft:
HRA 6501, AG Berlin-Charlottenburg
Komplementärin: BIOTRONIK Meß- und Therapiegeräte GmbH
HRB 2918, AG Berlin-Charlottenburg

Lumax 300 VR-T

BIOTRONIK

IS-1
DF-1
DF-1

REF 355270 Cat. No.

SN 12345678 Serial No.

2007-09 Use Before

41-113 °F Stor. Temp.

(01)04035479094454(17)070920(21)12345678

Implantable Cardioverter Defibrillator

Lumax 300 VR-T

PID 89 Prod. ID

Caution: Federal law (U.S.A.) restricts this device to sale by, or on the order of, a physican (or properly licenced practitioner)



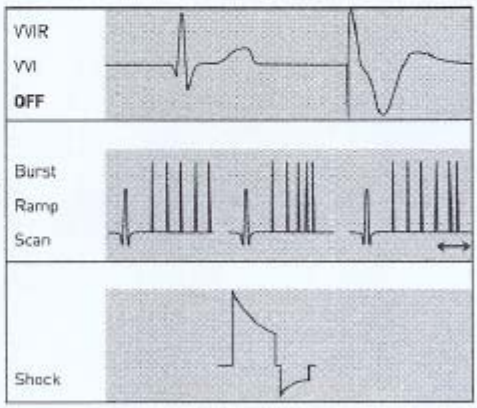

FCC ID: QRILUMAXT

BIOTRONIK GmbH & Co. KG
Woermannkehre 1
12359 Berlin · Germany
Tel. +49 (0) 30 68905-0
Fax +49 (0) 30 6852804
sales@biotronik.com

For single use only, do not resterilize. Do not use if packaging is damaged.
Refer to technical manual for instructions. ICD is shipped with all therapy disabled.

BIOTRONIK

C1609 30009

Lumax 300 DR-T

BIOTRONIK

REF 355266 Cat. No.

SN 12345678 Serial No.

2007-09 Use Before

41-113 °F Stor. Temp.

(01)04035479094416(17)070920(21)12345678

Implantable Cardioverter Defibrillator

Lumax 300 DR-T

PID 89 Prod. ID

Caution: Federal law (U.S.A.) restricts this device to sale by, or on the order of, a physican (or properly licenced practitioner)

403,6 MHz



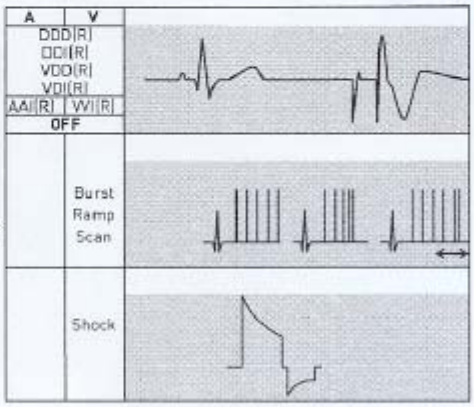

FCC ID:QRILUMAXT

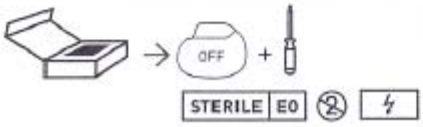

BIOTRONIK GmbH & Co. KG
Woermannkehre 1
12359 Berlin · Germany
Tel +49 (0) 30 68905-0
Fax +49 (0) 30 6852804
sales@biotronik.com

For single use only, do not resterilize. Do not use if packaging is damaged.
Refer to technical manual for instructions. ICD is shipped with all therapy disabled.

BIOTRONIK

Lumax 300 HF-T

BIOTRONIK

IS-1
IS-1
IS-1
DF-1
DF-1

REF 355262 Cat. No.

SN 12345678 Serial No.

2007-09 Use Before

41-113 °F Stor. Temp.

(01)04035479094379(17)070920(21)12345678

Cardiac Resynchronization Therapy Defibrillator

Lumax 300 HF-T

PID 89
Prod. ID

Caution: Federal law (U.S.A.) restricts this device to sale by, or on the order of, a physican (or properly licenced practitioner)

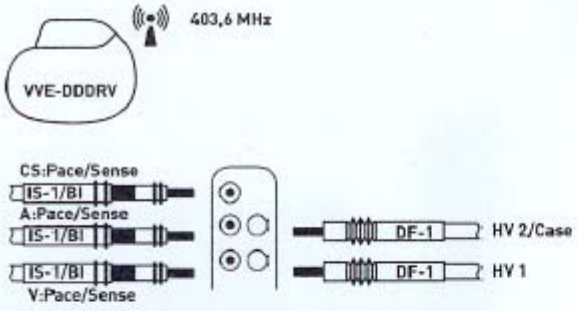

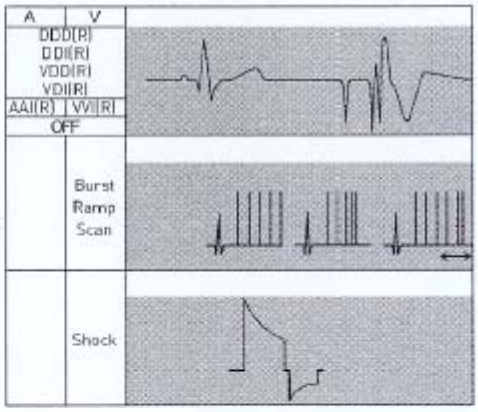

FCC ID: QRILUMAXT

BIOTRONIK GmbH & Co. KG
Woermannkehre 1
12359 Berlin · Germany
Tel. +49 (0) 30 68905-0
Fax +49 (0) 30 6852804
sales@biotronik.com

BIOTRONIK

For single use only, do not resterilize. Do not use if packaging is damaged.
Refer to technical manual for instructions. ICD is shipped with all therapy disabled.

E/A09 2007

Lumax 340 VR-T

BIOTRONIK

IS-1
DF-1
DF-1

REF 355271 Cat. No.

SN 12345678 Serial No.

2007-09 Use Before

41-113 °F Stor. Temp.

(01)04035479094461(17)070920(21)12345678

Implantable Cardioverter Defibrillator

Lumax 340 VR-T

PID 89 Prod. ID

Caution: Federal law (U.S.A.) restricts this device to sale by, or on the order of, a physican (or properly licenced practitioner)



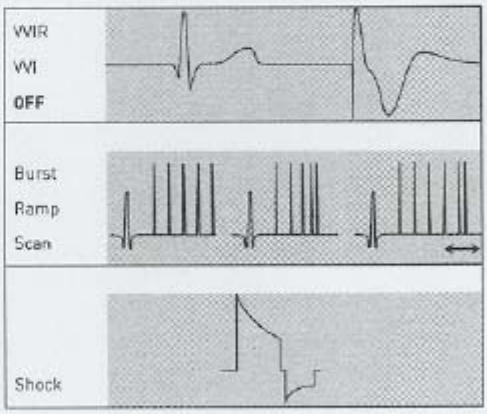

FCC ID: QRILUMAXT

BIOTRONIK GmbH & Co. KG
Woermannkehre 1
12359 Berlin - Germany
Tel +49 (0) 30 68905-0
Fax +49 (0) 30 6852804
sales@biotronik.com

For single use only, do not resterilize. Do not use if packaging is damaged.
Refer to technical manual for instructions. ICD is shipped with all therapy disabled.

BIOTRONIK

60000 - 60V/D

Lumax 340 DR-T

BIOTRONIK

REF 355267 Cat. No.

SN 12345678 Serial No.

2007-09 Use Before

41-113 °F Stor. Temp.

(01)04035479094423(17)070920(21)12345678

Implantable Cardioverter Defibrillator

Lumax 340 DR-T

PID 89 Prod. ID

Caution: Federal law (U.S.A.) restricts this device to sale by, or on the order of, a physican (or properly licenced practitioner)



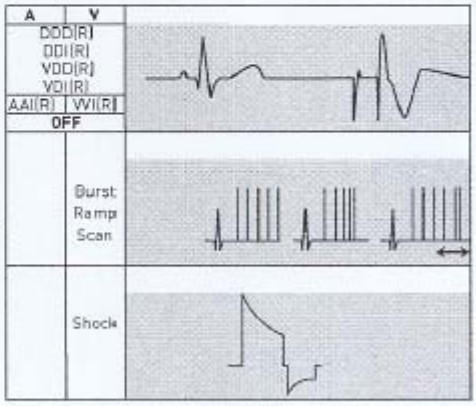

FCC ID: QRILUMAXT

C409 3009

BIOTRONIK GmbH & Co. KG
Woermannkehre 1
12359 Berlin · Germany
Tel +49 (0) 30 68905-0
Fax +49 (0) 30 6852804
sales@biotronik.com

For single use only, do not resterilize. Do not use if packaging is damaged.
Refer to technical manual for instructions. ICD is shipped with all therapy disabled.

BIOTRONIK

Lumax 340 HF-T

BIOTRONIK

IS-1
IS-1
IS-1
DF-1
DF-1

REF 355263 Cat. No.

SN 12345678 Serial No.

2007-09 Use Before

41-113 °F Stor. Temp.

(01)04035479094386(17)070920(21)12345678

Cardiac Resynchronization Therapy Defibrillator

Lumax 340 HF-T

PID 89 Prod. ID

Caution: Federal law (U.S.A.) restricts this device to sale by, or on the order of, a physican (or properly licenced practitioner)

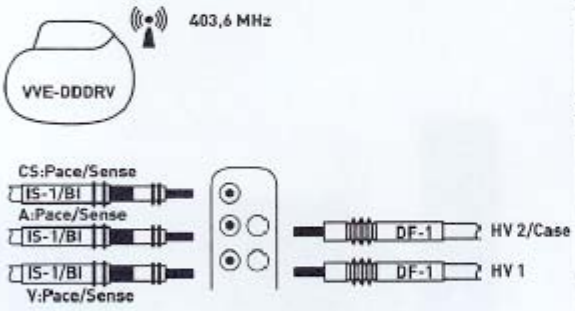

FCC ID: QRILUMAXT

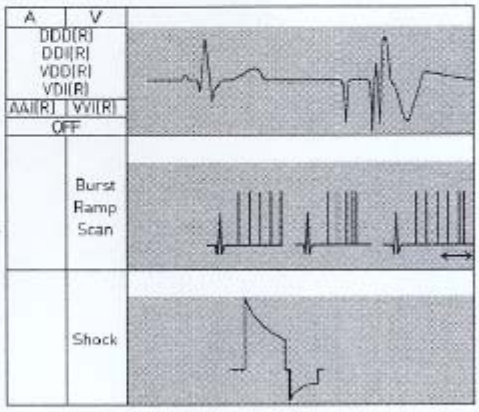

BIOTRONIK GmbH & Co. KG
Woermannkehre 1
12359 Berlin - Germany
Tel +49 (0) 30 68905-0
Fax +49 (0) 30 6852804
sales@biotronik.com

BIOTRONIK

For single use only, do not resterilize. Do not use if packaging is damaged.
Refer to technical manual for instructions. ICD is shipped with all therapy disabled.