


Appendix B

RF power output conducted

FCC part 15.247
Peak output power conducted

| | |
|-----------------------|------------------------------------|
| EUT | RTX3370 Monitor |
| Model | RTX3370 |
| Approval Holder | RTX Healthcare A/S |
| Temperature / Voltage | 25°C / Vnom |
| Test Site / Operator | ETS Product Service AG / Mr. Hoppe |
| Test Specification | FCC part 15 section 247(b) |
| Comment 1 | Peak output power |
| Comment 2 | Channel: 0 / 2402 MHz |
| Comment 3 | |

| | | | | | |
|--|---------------|----------------|-------|--------|----------|
| | Marker 1 [T1] | RBW | 1 MHz | RF Att | 50 dB |
| | Ref Lvl | 12.72 dBm | VBW | 1 MHz | |
| | 30 dBm | 2.40183868 GHz | SWT | 5 ms | Unit dBm |

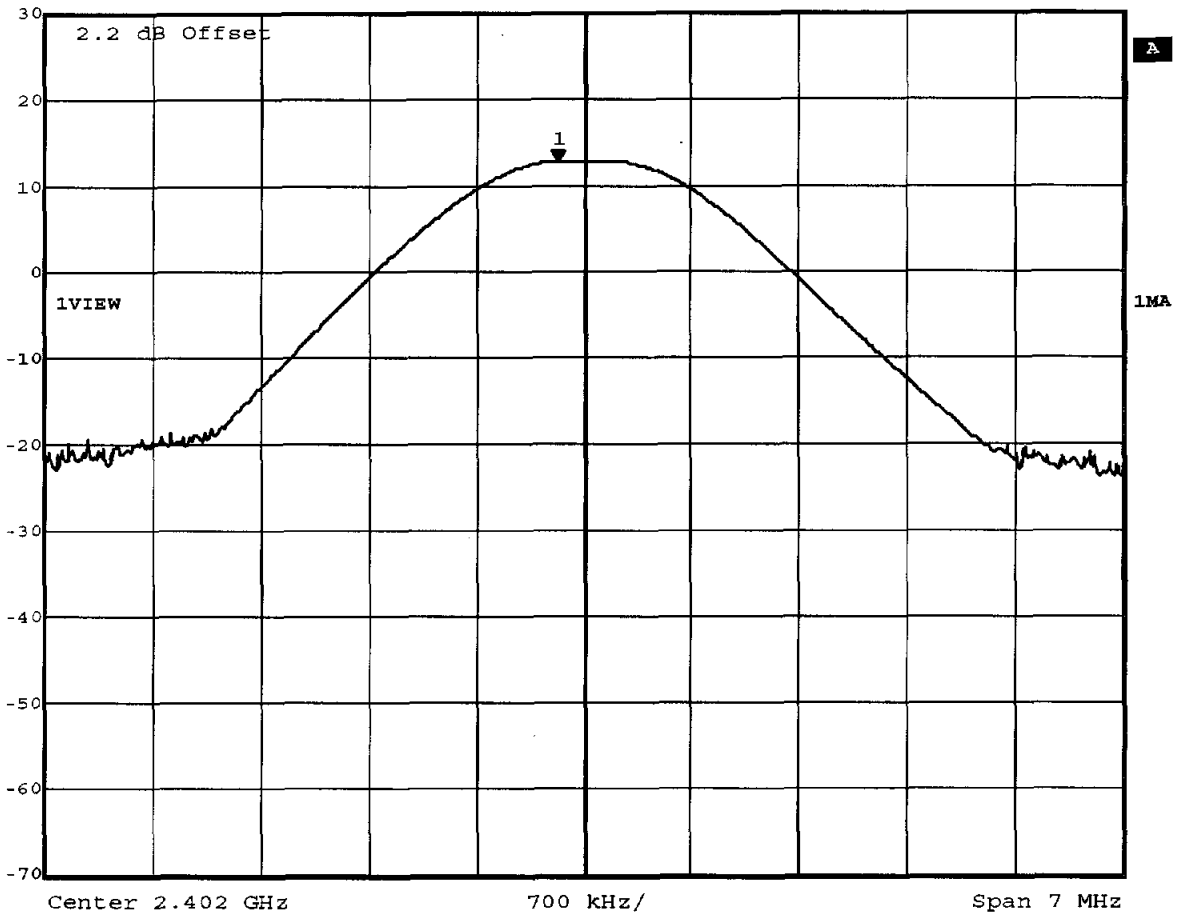

Comment A: Output power=12.72 dBm; verdict: PASS
Date: 20.APR.2007 11:54:51


Measurement diagram

FCC part 15.247
Peak output power conducted

| | |
|-----------------------|------------------------------------|
| EUT | RTX3370 Monitor |
| Model | RTX3370 |
| Approval Holder | RTX Healthcare A/S |
| Temperature / Voltage | 25°C / Vnom |
| Test Site / Operator | ETS Product Service AG / Mr. Hoppe |
| Test Specification | FCC part 15 section 247(b) |
| Comment 1 | Peak output power |
| Comment 2 | Channel.: 39 / 2441 MHz |
| Comment 3 | |



| | | | | |
|---------------|----------------|-------|--------|----------|
| Marker 1 [T1] | RBW | 1 MHz | RF Att | 50 dB |
| Ref Lvl | 12.15 dBm | VBW | 1 MHz | |
| 30 dBm | 2.44085271 GHz | SWT | 5 ms | Unit dBm |

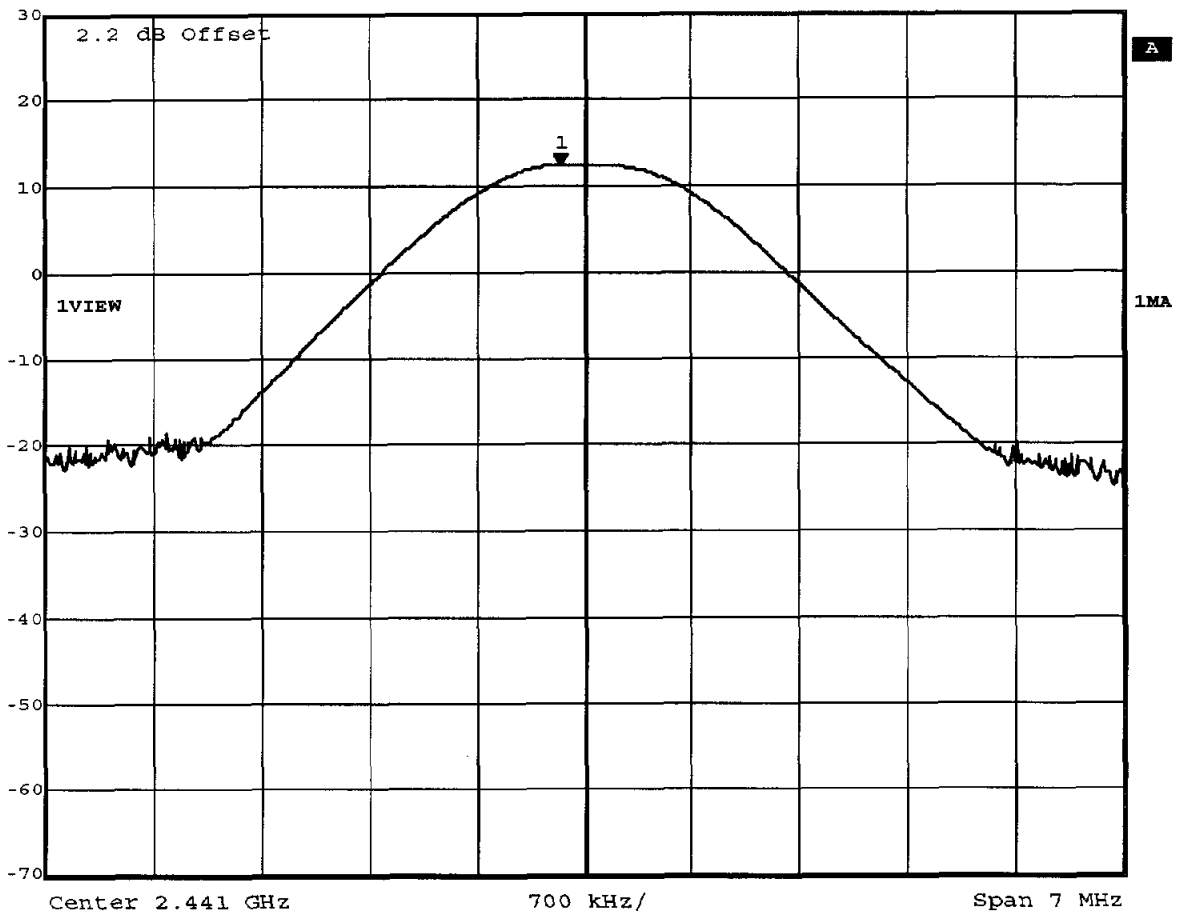

Comment A: Output power=12.15 dBm; verdict: PASS
Date: 20.APR.2007 12:04:11


Measurement diagram

FCC part 15.247
Peak output power conducted

| | |
|-----------------------|------------------------------------|
| EUT | RTX3370 Monitor |
| Model | RTX3370 |
| Approval Holder | RTX Healthcare A/S |
| Temperature / Voltage | 25°C / Vnom |
| Test Site / Operator | ETS Product Service AG / Mr. Hoppe |
| Test Specification | FCC part 15 section 247(b) |
| Comment 1 | Peak output power |
| Comment 2 | Channel.: 78 / 2480 MHz |
| Comment 3 | |



| | | | | |
|---------------|----------------|-------|--------|----------|
| Marker 1 [T1] | RBW | 1 MHz | RF Att | 50 dB |
| Ref Lvl | 12.75 dBm | VBW | 1 MHz | |
| 30 dBm | 2.47988076 GHz | SWT | 5 ms | Unit dBm |

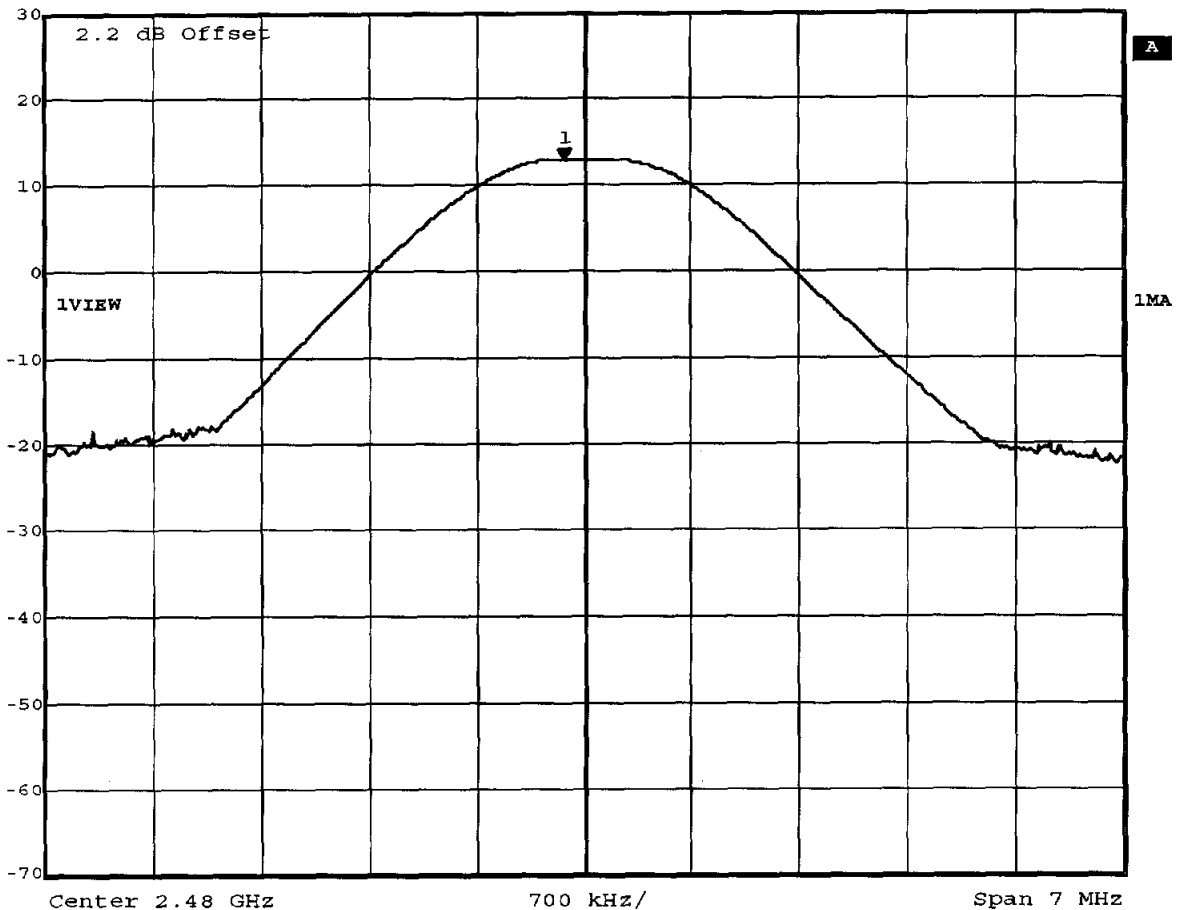


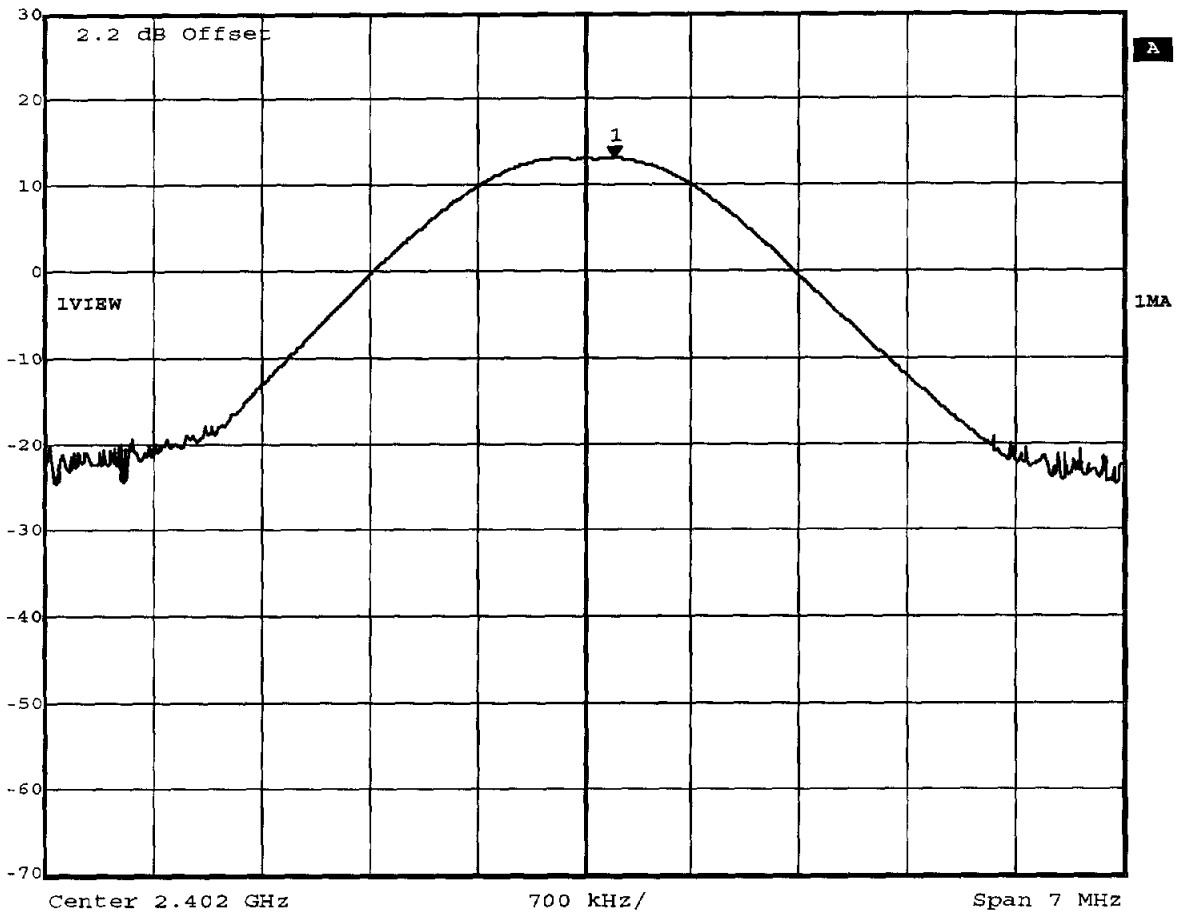
Comment A: Output power=12.75 dBm; verdict: PASS
Date: 20.APR.2007 12:44:21

Measurement diagram

FCC part 15.247
Peak output power conducted

| | |
|-----------------------|------------------------------------|
| EUT | RTX3370 Monitor |
| Model | RTX3370 |
| Approval Holder | RTX Healthcare A/S |
| Temperature / Voltage | 25°C / Vmin |
| Test Site / Operator | ETS Product Service AG / Mr. Hoppe |
| Test Specification | FCC part 15 section 247(b) |
| Comment 1 | Peak output power |
| Comment 2 | Channel.: 0 / 2402 MHz |
| Comment 3 | |

| | | | | | |
|---|---------------|----------------|-------|--------|----------|
|  | Marker 1 [T1] | RBW | 1 MHz | RF Att | 50 dB |
| | Ref Lvl | 12.84 dBm | VBW | 1 MHz | |
| | 30 dBm | 2.40220341 GHz | SWT | 5 ms | Unit dBm |



Comment A: Output power=12.84 dBm; verdict: PASS
Date: 20.APR.2007 12:57:49


Measurement diagram

FCC part 15.247
Peak output power conducted

| | |
|-----------------------|------------------------------------|
| EUT | RTX3370 Monitor |
| Model | RTX3370 |
| Approval Holder | RTX Healthcare A/S |
| Temperature / Voltage | 25°C / Vmin |
| Test Site / Operator | ETS Product Service AG / Mr. Hoppe |
| Test Specification | FCC part 15 section 247(b) |
| Comment 1 | Peak output power |
| Comment 2 | Channel.: 39 / 2441 MHz |
| Comment 3 | |



| | | | | |
|---------------|----------------|-------|--------|----------|
| Marker 1 [T1] | RBW | 1 MHz | RF Att | 50 dB |
| Ref Lvl | 12.24 dBm | VBW | 1 MHz | |
| 30 dBm | 2.44088076 GHz | SWT | 5 ms | Unit dBm |

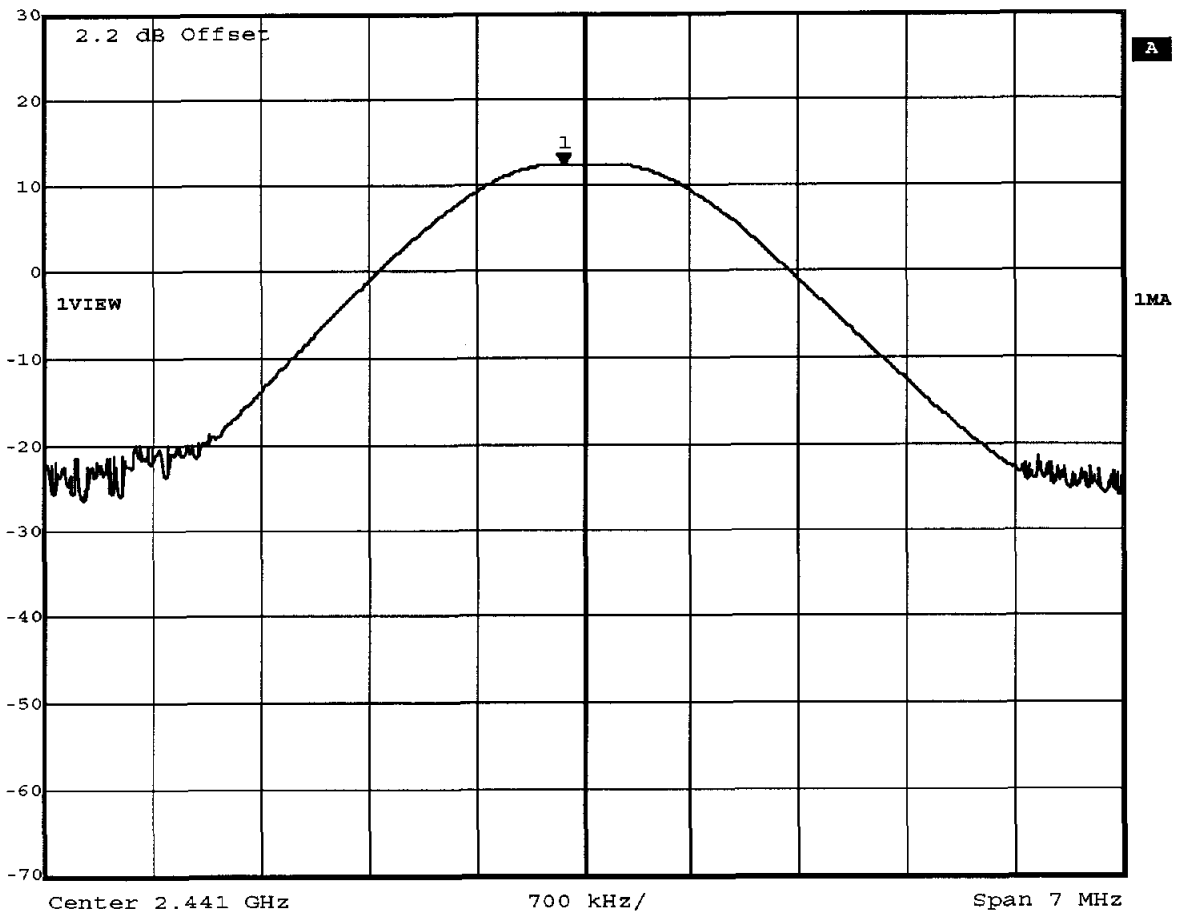


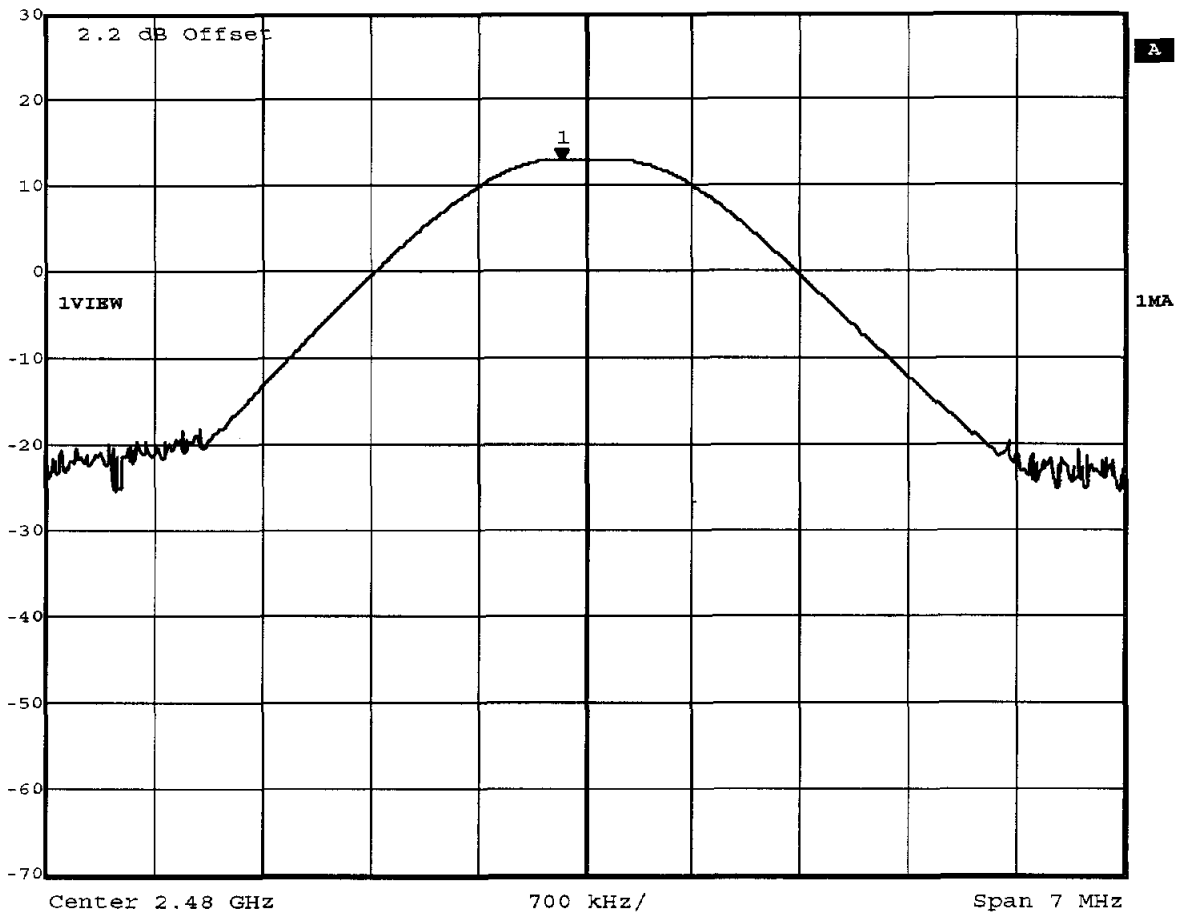
Comment A: Output power=12.24 dBm; verdict: PASS
Date: 20.APR.2007 12:51:47

Measurement diagram

FCC part 15.247
Peak output power conducted

| | |
|-----------------------|------------------------------------|
| EUT | RTX3370 Monitor |
| Model | RTX3370 |
| Approval Holder | RTX Healthcare A/S |
| Temperature / Voltage | 25°C / Vmin |
| Test Site / Operator | ETS Product Service AG / Mr. Hoppe |
| Test Specification | FCC part 15 section 247(b) |
| Comment 1 | Peak output power |
| Comment 2 | Channel.: 78 / 2480 MHz |
| Comment 3 | |

| | | | | | |
|---|---------------|----------------|-------|--------|----------|
|  | Marker 1 [T1] | RBW | 1 MHz | RF Att | 50 dB |
| | Ref Lvl | 12.74 dBm | VBW | 1 MHz | |
| | 30 dBm | 2.47985271 GHz | SWT | 5 ms | Unit dBm |



Comment A: Output power=12.74 dBm; verdict: PASS
Date: 20.APR.2007 12:54:54

Measurement diagram


FCC part 15.247

Peak output power conducted

| | |
|-----------------------|------------------------------------|
| EUT | RTX3370 Monitor |
| Model | RTX3370 |
| Approval Holder | RTX Healthcare A/S |
| Temperature / Voltage | 25°C / Vmax |
| Test Site / Operator | ETS Product Service AG / Mr. Hoppe |
| Test Specification | FCC part 15 section 247(b) |
| Comment 1 | Peak output power |
| Comment 2 | Channel.: 0 / 2402 MHz |
| Comment 3 | |



| | | | | |
|---------------|----------------|-------|--------|----------|
| Marker 1 [T1] | RBW | 1 MHz | RF Att | 50 dB |
| Ref Lvl | 12.85 dBm | VBW | 1 MHz | |
| 30 dBm | 2.40186673 GHz | SWT | 5 ms | Unit dBm |

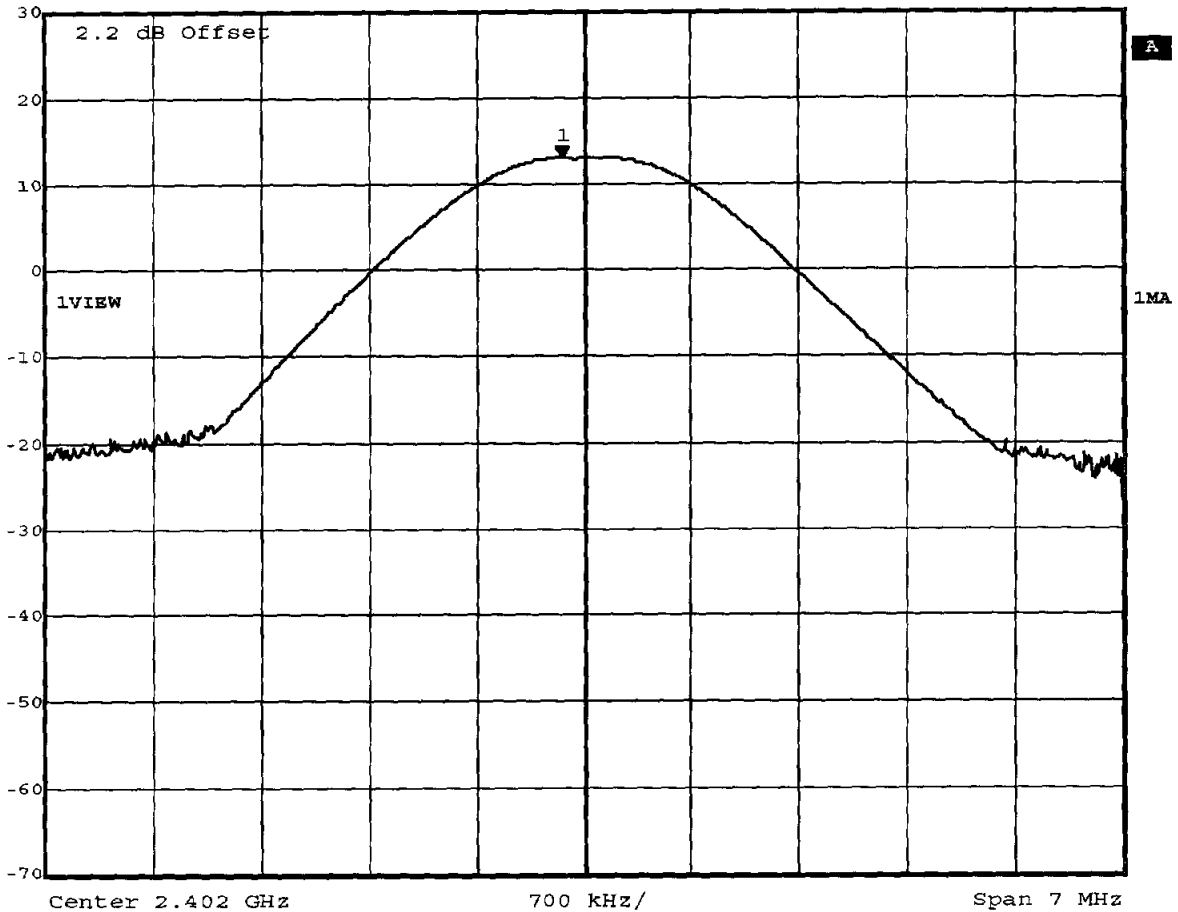


Comment A: Output power=12.85 dBm; verdict: PASS
 Date: 20.APR.2007 13:04:38

Measurement diagram

FCC part 15.247
Peak output power conducted

| | |
|-----------------------|------------------------------------|
| EUT | RTX3370 Monitor |
| Model | RTX3370 |
| Approval Holder | RTX Healthcare A/S |
| Temperature / Voltage | 25°C / Vmax |
| Test Site / Operator | ETS Product Service AG / Mr. Hoppe |
| Test Specification | FCC part 15 section 247(b) |
| Comment 1 | Peak output power |
| Comment 2 | Channel.: 39 / 2441 MHz |
| Comment 3 | |

| | | | | | |
|--|---------------|----------------|-------|--------|----------|
| | Marker 1 [T1] | RBW | 1 MHz | RF Att | 50 dB |
| | Ref Lvl | 12.26 dBm | VBW | 1 MHz | |
| | 30 dBm | 2.44085271 GHz | SWT | 5 ms | Unit dBm |

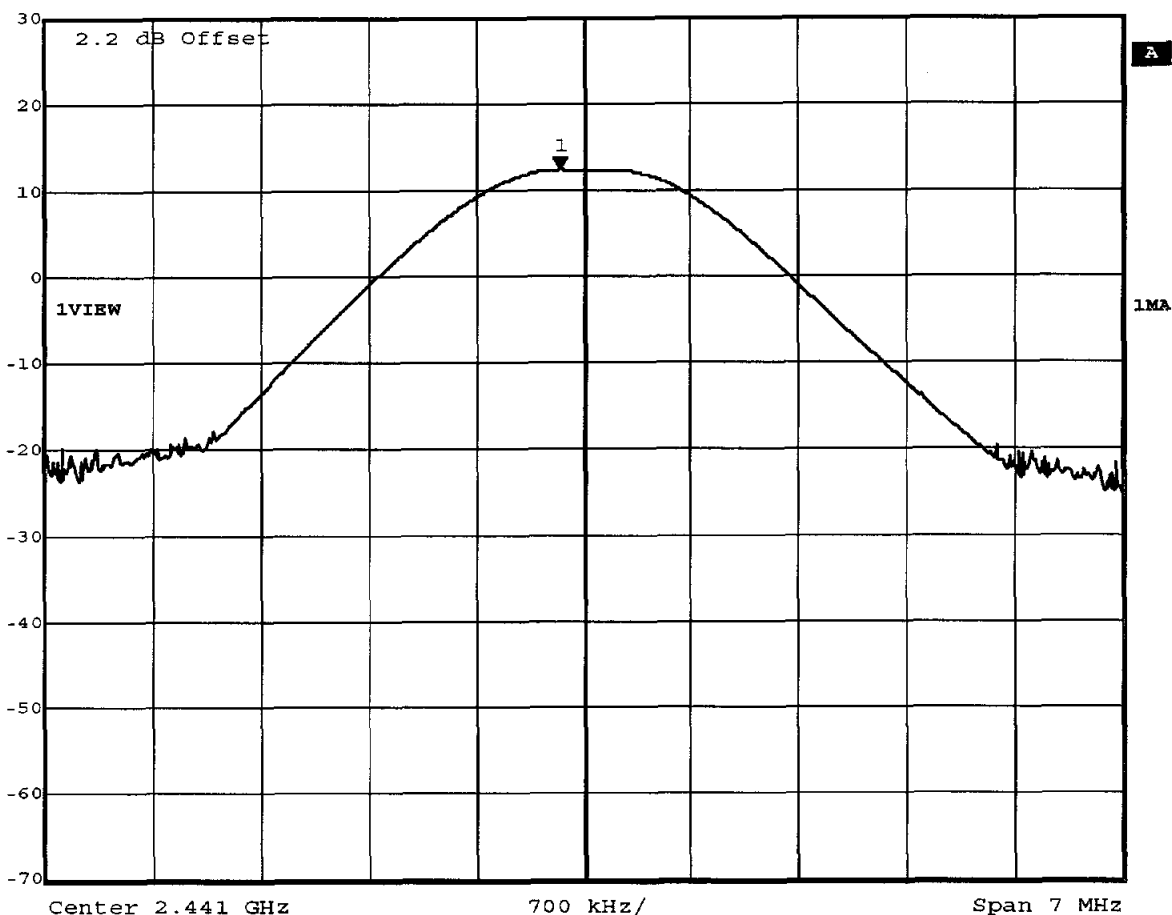

Comment A: Output power=12.26 dBm; verdict: PASS
Date: 20.APR.2007 13:09:51

Measurement diagram

Appendix C

RF power output radiated (EIRP)


Appendix D

20 dB bandwidth

FCC part 15.247
20 dB bandwidth

| | |
|-----------------------|------------------------------------|
| EUT | RTX3370 Monitor |
| Model | RTX3370 |
| Approval Holder | RTX Healthcare A/S |
| Temperature / Voltage | 25°C / Vnom |
| Test Site / Operator | ETS Product Service AG / Mr. Hoppe |
| Test Specification | FCC part 15 section 247(a) |
| Comment 1 | 20 dB bandwidth |
| Comment 2 | Channel.: 0 / 2402 MHz |
| Comment 3 | |

| | | | | | |
|--|--------------|------------------|--------|--------|----------|
| | Delta 1 [T1] | RBW | 10 kHz | RF Att | 40 dB |
| | Ref Lvl | -0.01 dB | VBW | 10 kHz | |
| | 20 dBm | 872.89298597 kHz | SWT | 56 ms | Unit dBm |

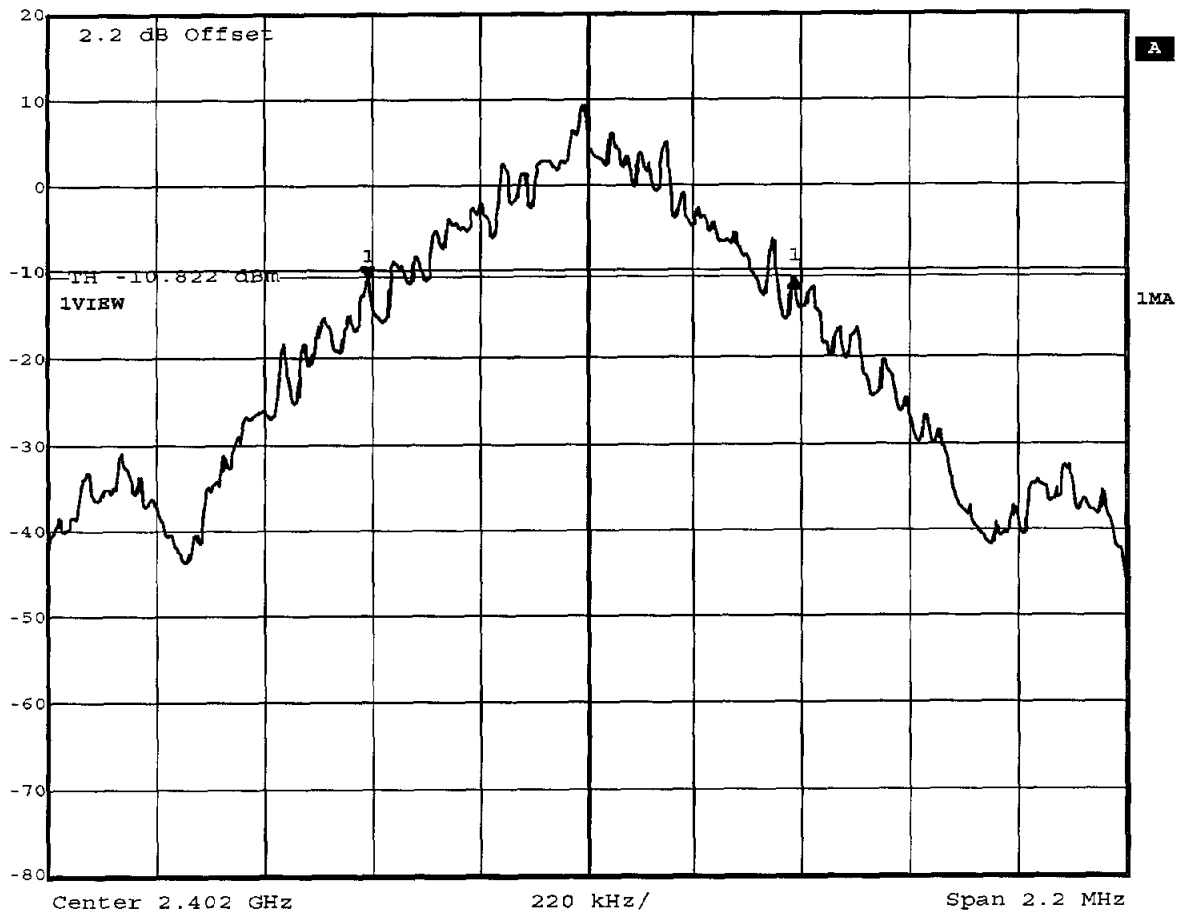


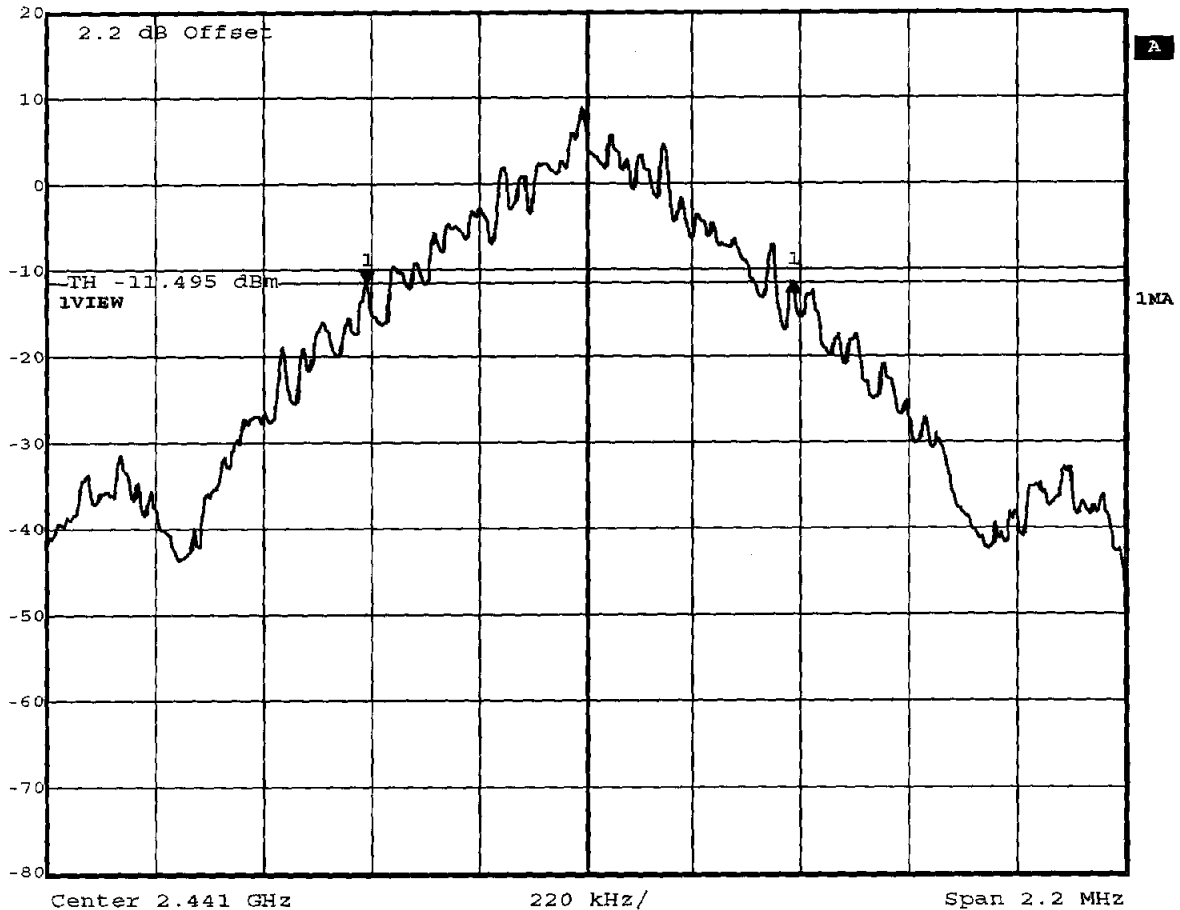
Comment A: 20 dB bandwidth: 872.9 KHz < 1MHz; verdict: PASS
Date: 20.APR.2007 13:30:30

Measurement diagram

FCC part 15.247
20 dB bandwidth

| | |
|-----------------------|------------------------------------|
| EUT | RTX3370 Monitor |
| Model | RTX3370 |
| Approval Holder | RTX Healthcare A/S |
| Temperature / Voltage | 25°C / Vnom |
| Test Site / Operator | ETS Product Service AG / Mr. Hoppe |
| Test Specification | FCC part 15 section 247(a) |
| Comment 1 | 20 dB bandwidth |
| Comment 2 | Channel.: 39 / 2441 MHz |
| Comment 3 | |

| | | | | | |
|---|--------------|------------------|--------|--------|-------|
|  | Delta 1 [T1] | RBW | 10 kHz | RF Att | 40 dB |
| | Ref Lvl | 0.03 dB | VBW | 10 kHz | |
| | 20 dBm | 872.89298597 kHz | SWT | 56 ms | Unit |




Comment A: 20 dB bandwidth: 872.9 KHz < 1MHz; verdict: PASS
Date: 20.APR.2007 13:27:14

Measurement diagram

FCC part 15.247
20 dB bandwidth

EUT RTX3370 Monitor
 Model RTX3370
 Approval Holder RTX Healthcare A/S
 Temperature / Voltage 25°C / Vnom
 Test Site / Operator ETS Product Service AG / Mr. Hoppe
 Test Specification FCC part 15 section 247(a)
 Comment 1 20 dB bandwidth
 Comment 2 Channel.: 78 / 2480 MHz
 Comment 3

| | | | | | |
|--|--------------|------------------|--------|--------|---------------------|
| | Delta 1 [T1] | RBW | 10 kHz | RF Att | 40 dB |
| | Ref Lvl | 0.21 dB | VBW | 10 kHz | |
| | 20 dBm | 872.89298597 kHz | SWT | 56 ms | Unit dBm |

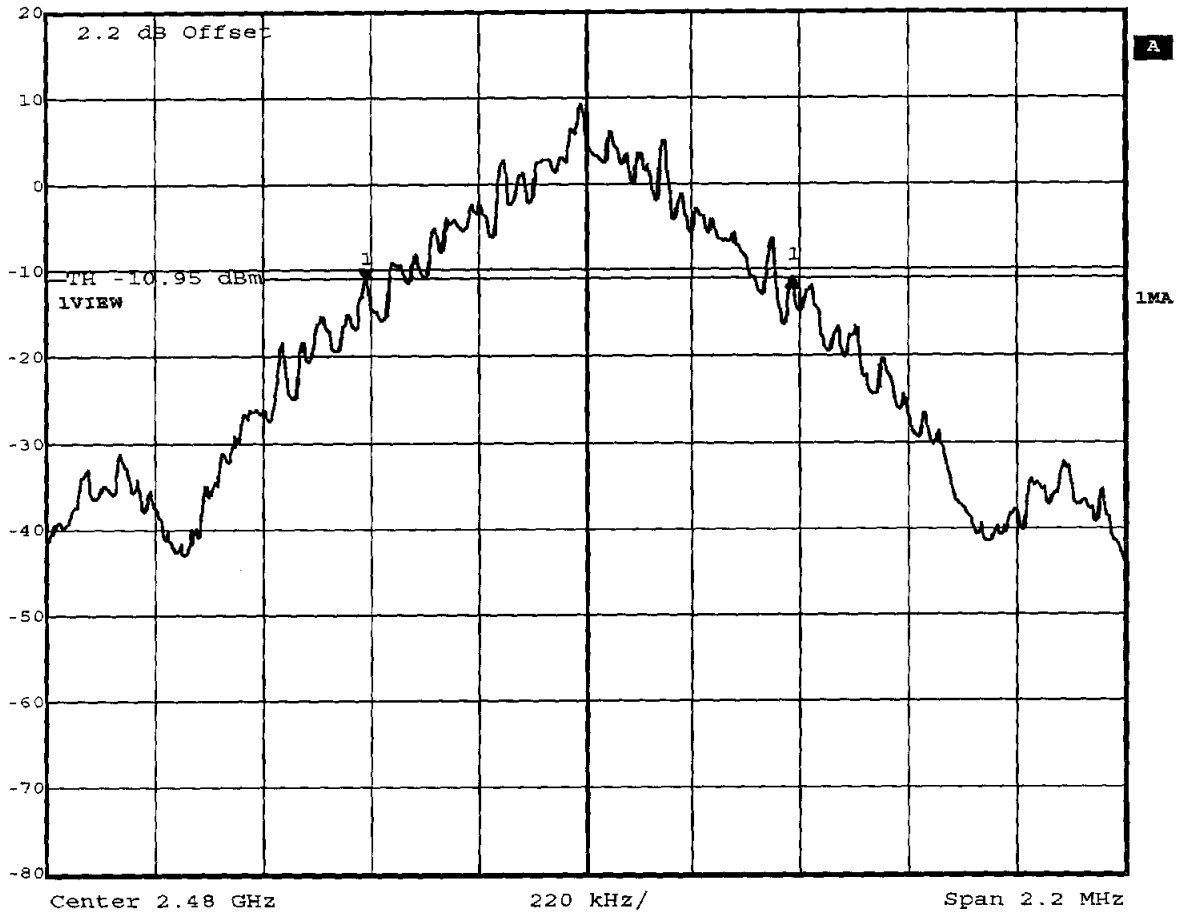

Comment A: 20 dB bandwidth: 872.9 KHz < 1MHz; verdict: PASS
 Date: 20.APR.2007 13:22:53


Measurement diagram

ETS Product Service AG

Storkower Str. 38C, D-15526 REICHENWALDE B. BERLIN

RSS Gen
Occupied Bandwidth

EUT RTX3370 Monitor
 Model RTX3370
 Approval Holder RTX Healthcare A/S
 Temperature / Voltage 25°C / Vnom
 Test Site / Operator ETS Product Service AG / Mr. Hoppe
 Test Specification 4.4.1 Occupied Bandwidth
 Comment 1 Channel.: 39 / 2441 MHz
 Comment 2 A spectrum analyzer with an integrated 99% power bandwidth function is used
 Comment 3

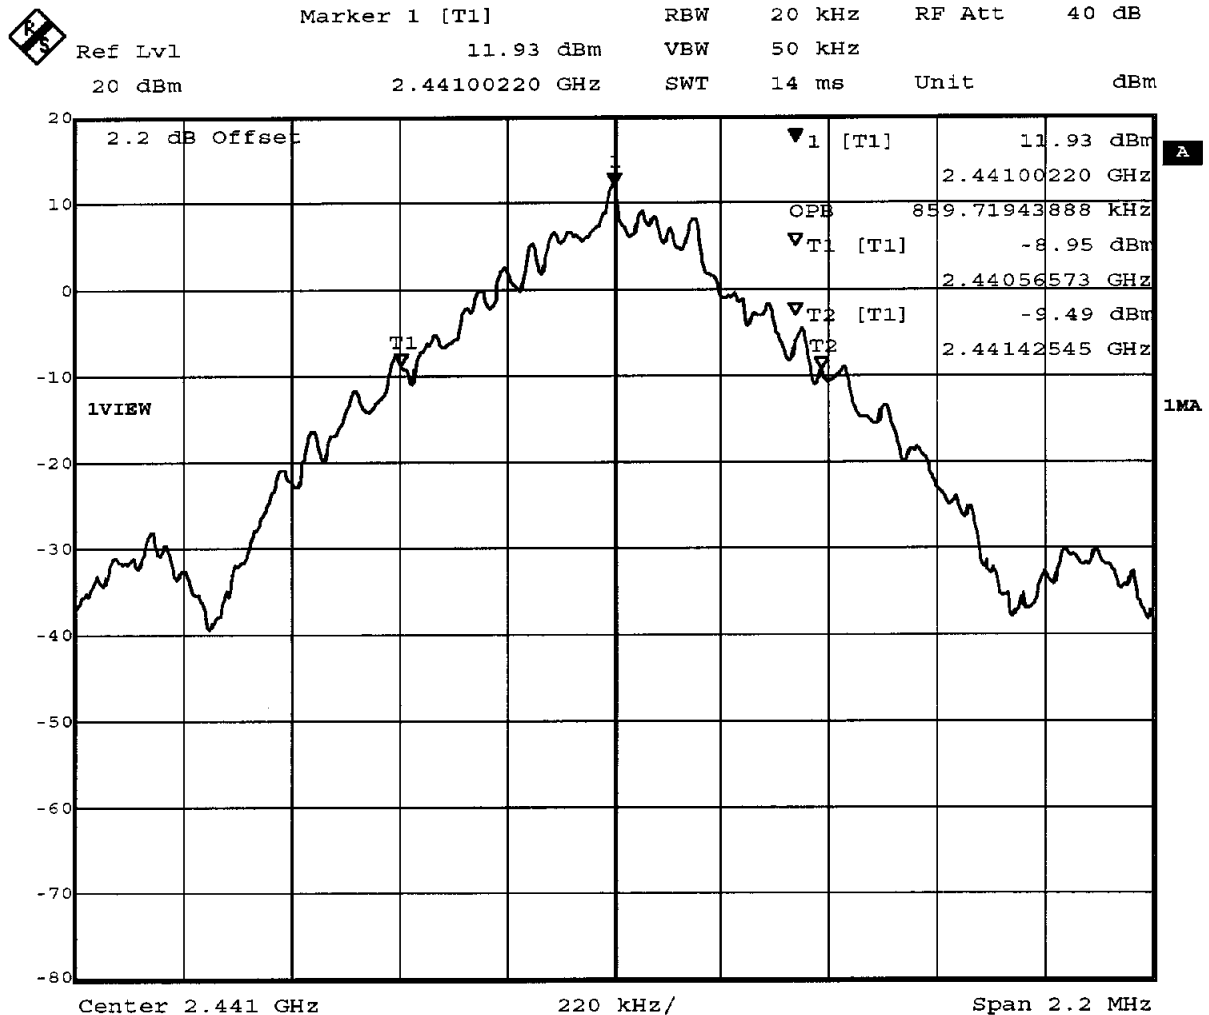


Comment A: Occupied bandwidth: 859.7 KHz
 Date: 20.APR.2007 14:00:07

Measurement diagram

RSS Gen
Occupied Bandwidth

EUT RTX3370 Monitor
 Model RTX3370
 Approval Holder RTX Healthcare A/S
 Temperature / Voltage 25°C / Vnom
 Test Site / Operator ETS Product Service AG / Mr. Hoppe
 Test Specification 4.4.1 Occupied Bandwidth
 Comment 1 Channel.: 78 / 2480 MHz
 Comment 2 A spectrum analyzer with an integrated 99% power bandwidth function is used
 Comment 3

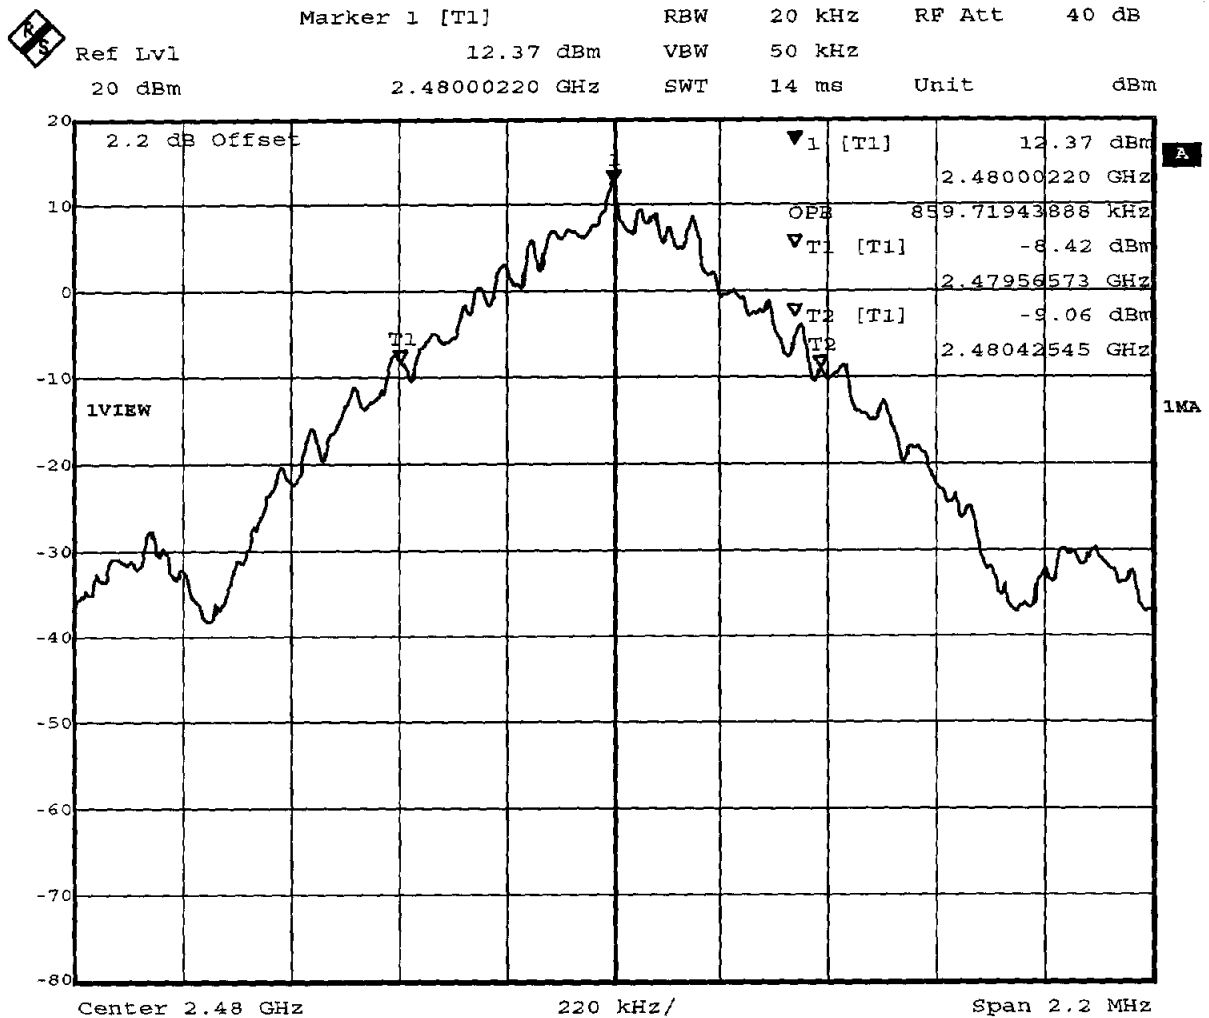

Comment A: Occupied bandwidth: 859.7 KHz
 Date: 20.APR.2007 14:02:12

Measurement diagram

Appendix E


Time of occupancy (dwell time)

FCC part 15.247

Time of occupancy (dwell time)

| | |
|-----------------------|---|
| EUT | RTX3370 Monitor |
| Model | RTX3370 |
| Approval Holder | RTX Healthcare A/S |
| Temperature / Voltage | 25°C / Vnom |
| Test Site / Operator | ETS Product Service AG / Mr. Hoppe |
| Test Specification | FCC part 15 section 247(a) |
| Comment 1 | Time of occupancy |
| Comment 2 | Channel.: 39 / 2441 MHz (Hopping mode) |
| Comment 3 | 63 events * 2.932 ms result: 184.716 ms |

| | | | | | |
|--|--------------|-------------|-------|--------|----------|
| | Delta 1 [T1] | RBW | 1 MHz | RF Att | 40 dB |
| | Ref Lvl | -0.05 dB | VBW | 1 MHz | |
| | 30 dBm | 2.931549 ms | SWT | 4 ms | Unit dBm |

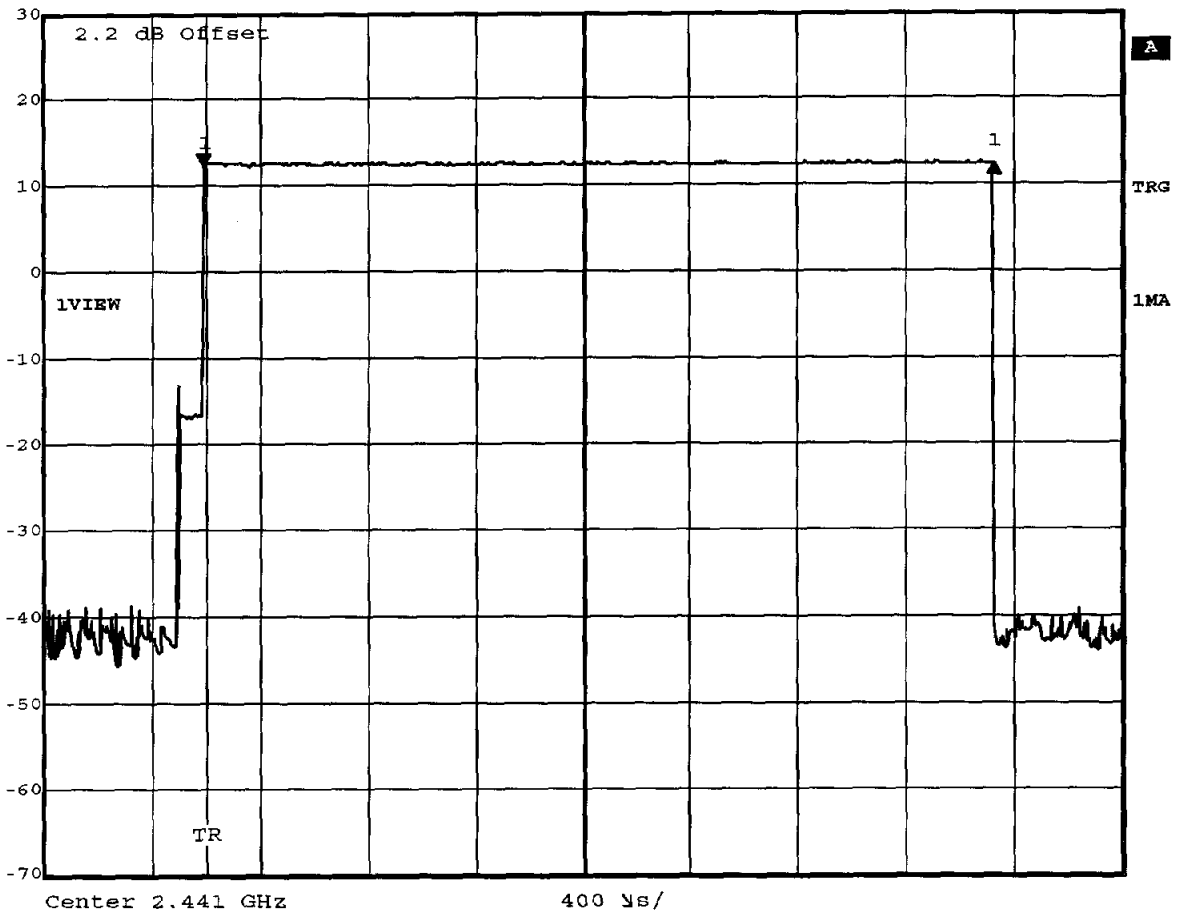

Comment A: Burst length=2.93155 ms
 Date: 20.APR.2007 14:36:53

Measurement diagram

Appendix F


Number of hopping frequencies

FCC part 15.247
Number of hopping frequencies

| | |
|-----------------------|------------------------------------|
| EUT | RTX3370 Monitor |
| Model | RTX3370 |
| Approval Holder | RTX Healthcare A/S |
| Temperature / Voltage | 25°C / Vnom |
| Test Site / Operator | ETS Product Service AG / Mr. Hoppe |
| Test Specification | FCC part 15 section 247(a) |
| Comment 1 | Number of hopping frequencies |
| Comment 2 | Channel.: 0-13 |
| Comment 3 | |



| | | | | | |
|---------|--------|-----|---------|--------|-------|
| Ref Lvl | 30 dBm | RBW | 300 kHz | RF Att | 50 dB |
| | | VBW | 300 kHz | Unit | dBm |
| | | SWT | 5 ms | | |

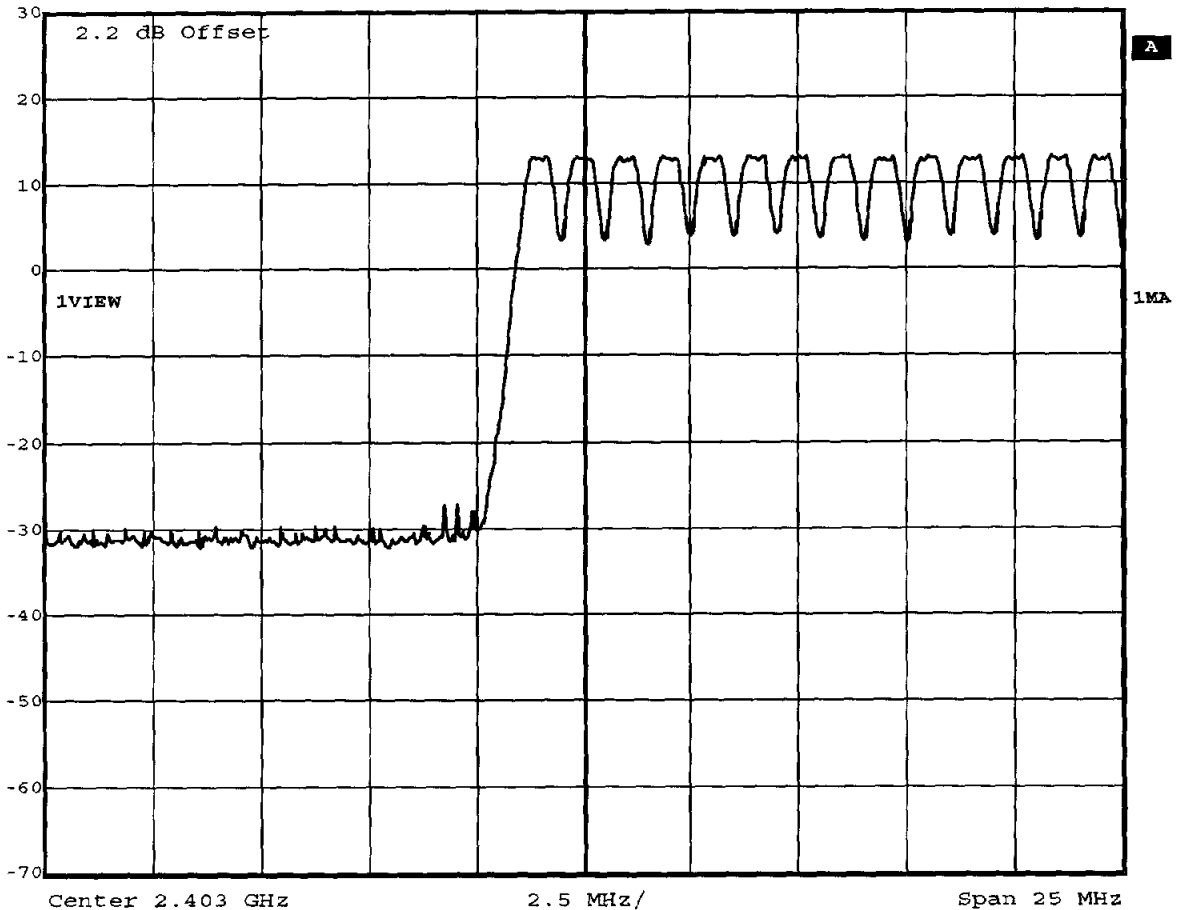


Comment A: Number of hopping frequencies
Date: 20.APR.2007 14:23:04

Measurement diagram

FCC part 15.247
Number of hopping frequencies

| | |
|-----------------------|------------------------------------|
| EUT | RTX3370 Monitor |
| Model | RTX3370 |
| Approval Holder | RTX Healthcare A/S |
| Temperature / Voltage | 25°C / Vnom |
| Test Site / Operator | ETS Product Service AG / Mr. Hoppe |
| Test Specification | FCC part 15 section 247(a) |
| Comment 1 | Number of hopping frequencies |
| Comment 2 | Channel.: 14-38 |
| Comment 3 | |

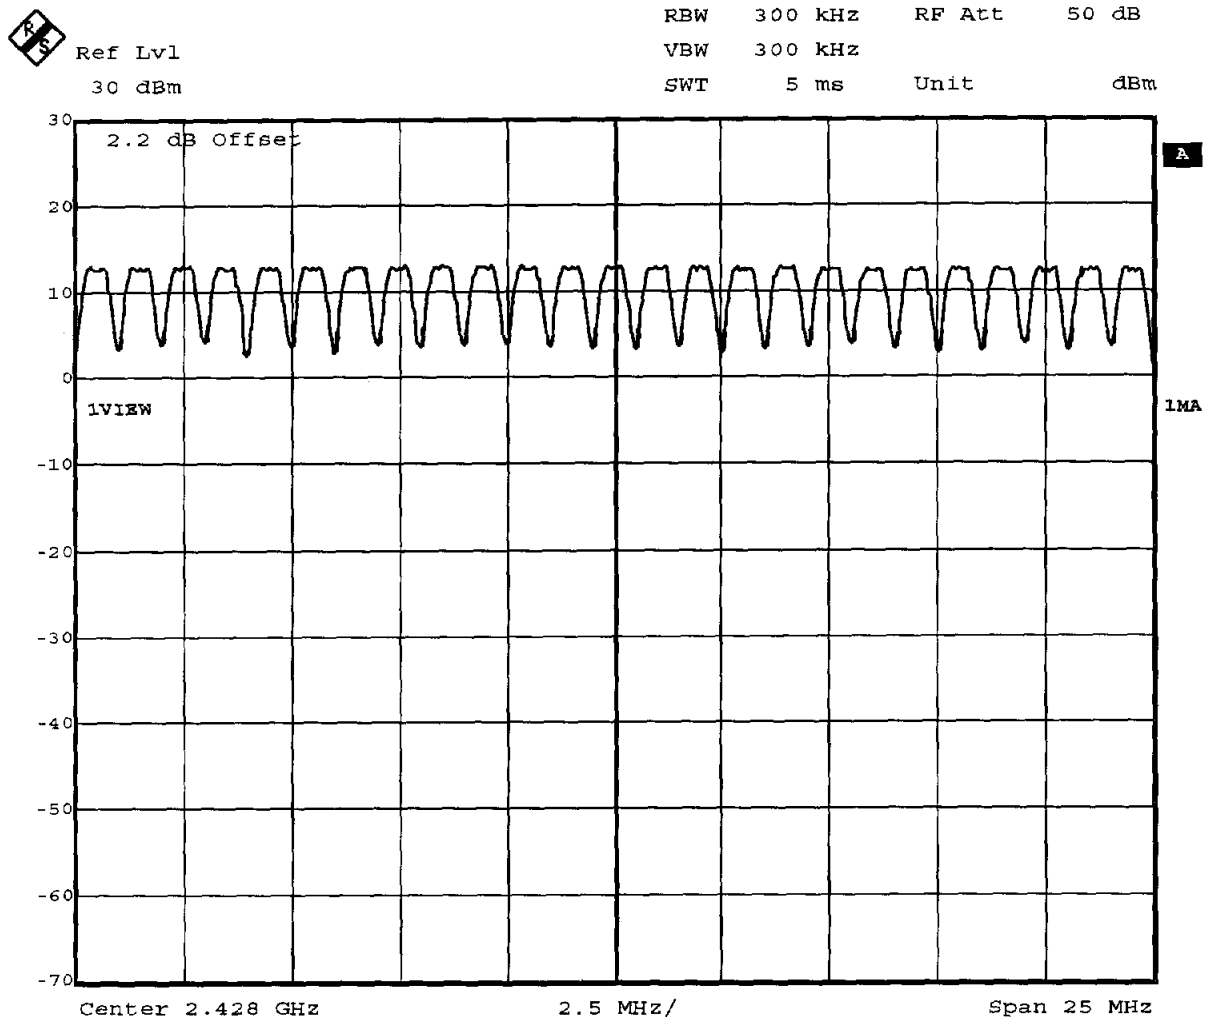


Comment A: Number of hopping frequencies
Date: 20.APR.2007 14:26:04

Measurement diagram

FCC part 15.247
Number of hopping frequencies

| | |
|-----------------------|------------------------------------|
| EUT | RTX3370 Monitor |
| Model | RTX3370 |
| Approval Holder | RTX Healthcare A/S |
| Temperature / Voltage | 25°C / Vnom |
| Test Site / Operator | ETS Product Service AG / Mr. Hoppe |
| Test Specification | FCC part 15 section 247(a) |
| Comment 1 | Number of hopping frequencies |
| Comment 2 | Channel.:39-63 |
| Comment 3 | |

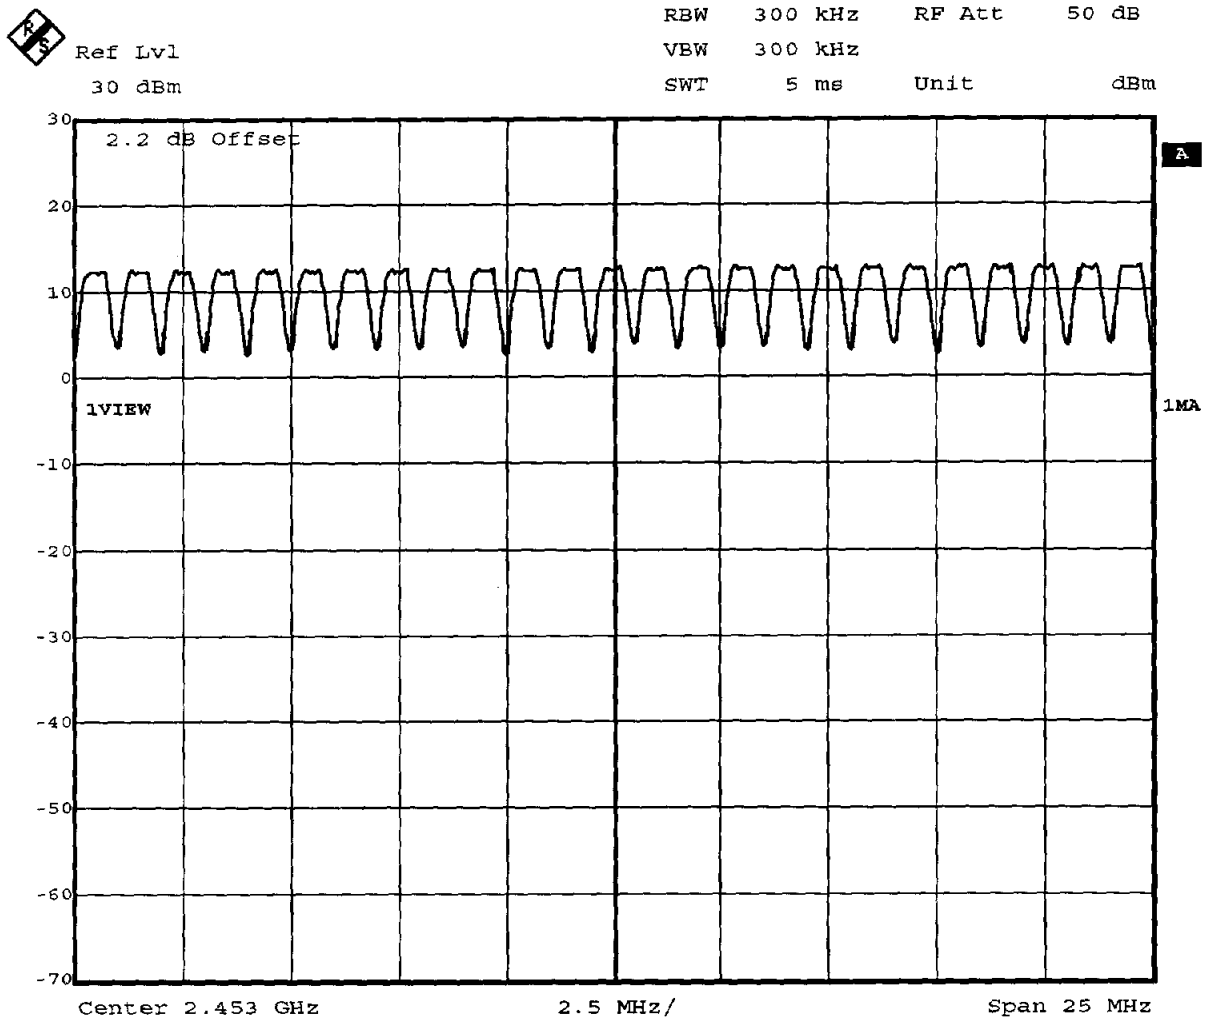


Comment A: Number of hopping frequencies
 Date: 20.APR.2007 14:28:37

Measurement diagram

FCC part 15.247
Number of hopping frequencies

| | |
|-----------------------|------------------------------------|
| EUT | RTX3370 Monitor |
| Model | RTX3370 |
| Approval Holder | RTX Healthcare A/S |
| Temperature / Voltage | 25°C / Vnom |
| Test Site / Operator | ETS Product Service AG / Mr. Hoppe |
| Test Specification | FCC part 15 section 247(a) |
| Comment 1 | Number of hopping frequencies |
| Comment 2 | Channel.: 64-78 |
| Comment 3 | |

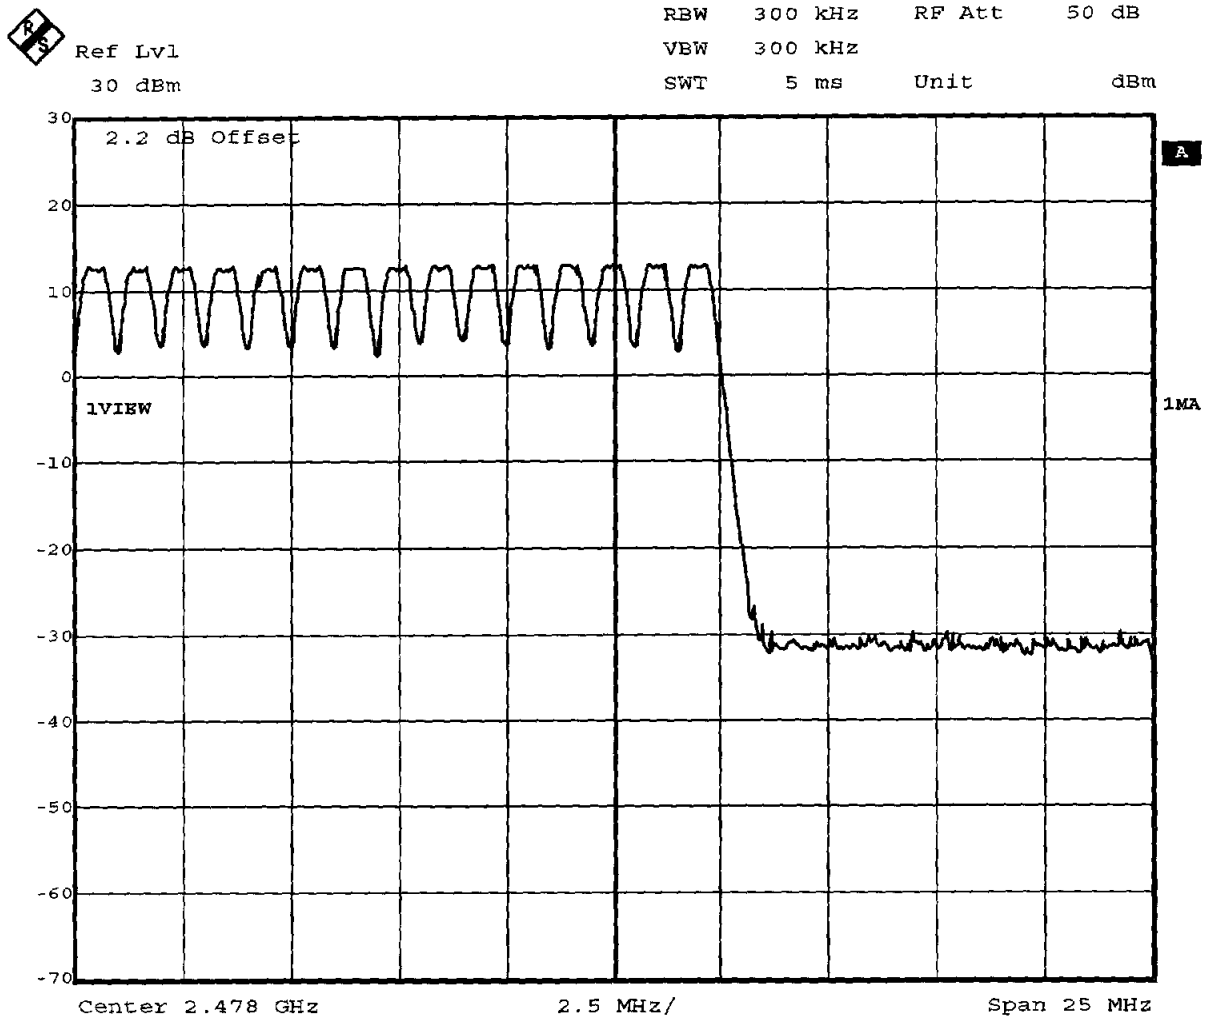

Comment A: Number of hopping frequencies
 Date: 20.APR.2007 14:30:58

Measurement diagram


Appendix G

Carrier frequency separation

FCC part 15.247
Carrier frequency separation

EUT RTX3370 Monitor
 Model RTX3370
 Approval Holder RTX Healthcare A/S
 Temperature / Voltage 25°C / Vnom
 Test Site / Operator ETS Product Service AG / Mr. Hoppe
 Test Specification FCC part 15 section 247(b)
 Comment 1 Carrier frequency separation
 Comment 2 Channel: 39/40 / 2441/2442 MHz
 Comment 3 Hopping mode

| | | | | | |
|--|--------------|----------------|---------|---------|---------------------|
| | Delta 1 [T1] | RBW | 100 kHz | RF Att | 40 dB |
| | Ref Lvl | -0.14 dB | VBW | 100 kHz | |
| | 20 dBm | 1.01843687 MHz | SWT | 5 ms | Unit dBm |

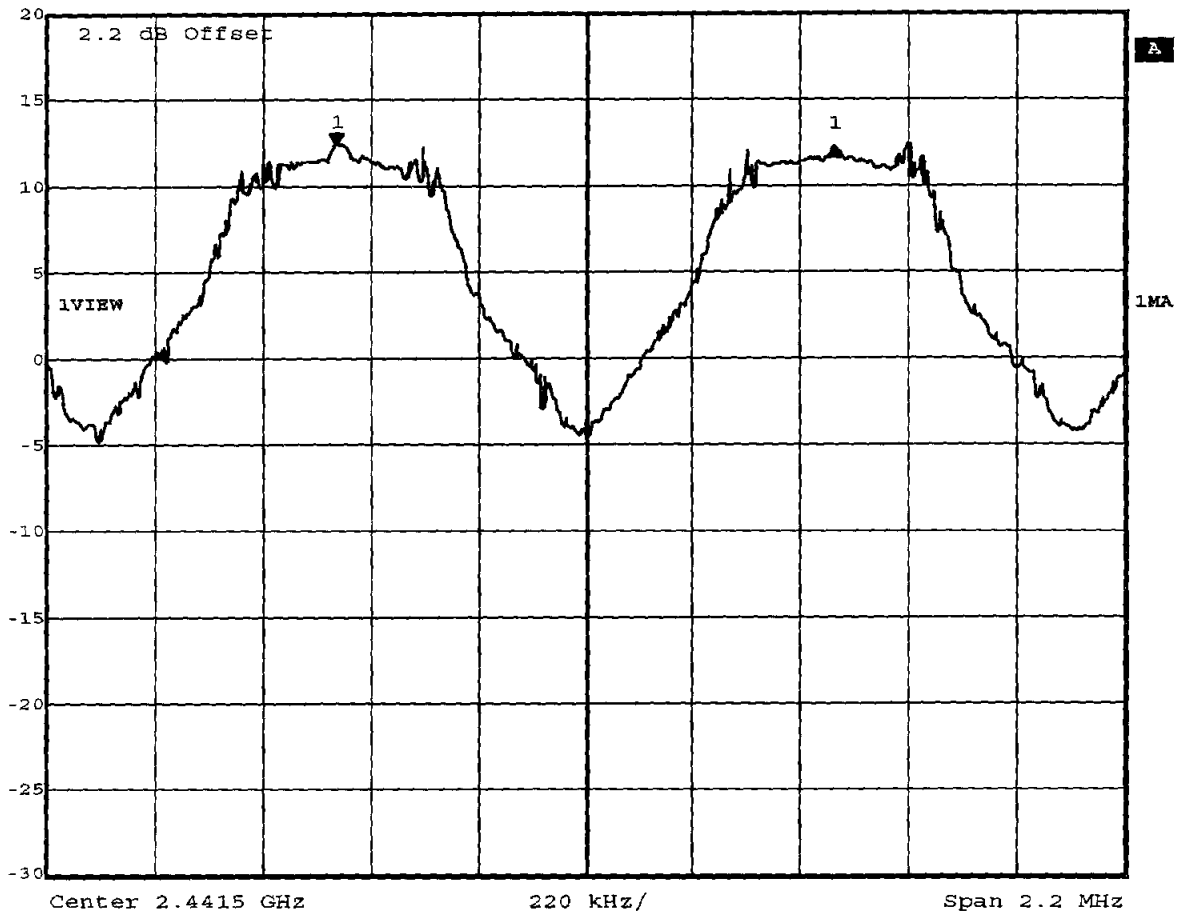

Comment A: Limit: > two-thirds of the 20 dB bandwidth ; Result: Pass
 Date: 20.APR.2007 14:18:28

Measurement diagram

Appendix H

Spurious emission conducted


Appendix I

Spurious emission radiated

Carrier power (Field Strength)

FCC RULES PART 15, SUBPART C


Approval Holder: RTX Healthcare A/S
EUT: RTX3370 Monitor
Model: RTX3370 / 2480 MHz
Test Site / Operator: ETS / Mr. Meng
Test Condition: 25°C / Unom: 6.0 V DC
Test Specification: according to S15.247
Comment 1: Dist.: 3m, Ant.: BBHA9120D
Comment 2: Freq: 2.480GHz, Emax: 111.36dBµV/m, RBW: 100kHz

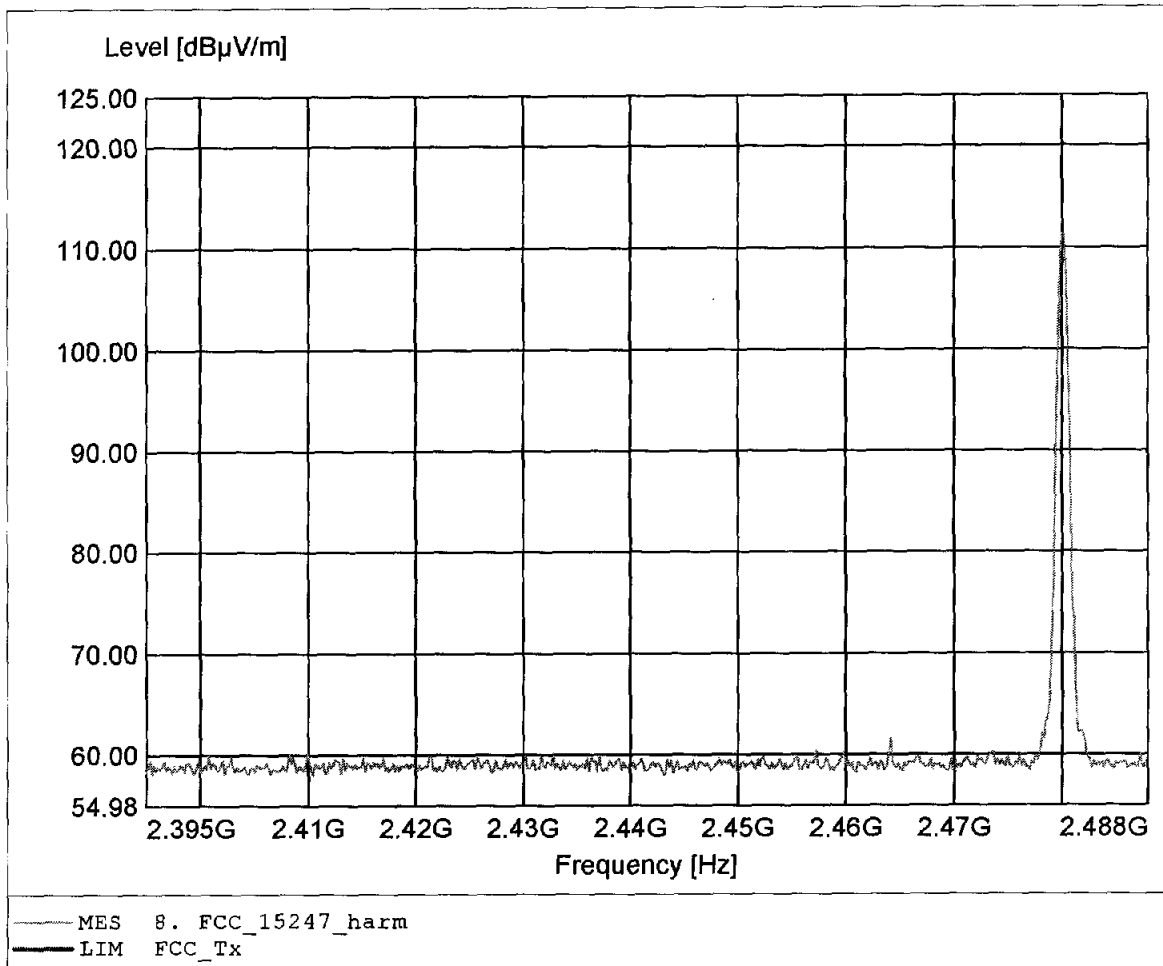

Spurious emissions Field Strength

FCC RULES PART 15, SUBPART C


Approval Holder: RTX Healthcare A/S
EUT: RTX3370 Monitor
Model: RTX3370 / 2402 MHz
Test Site / Operator: ETS / Mr. Meng
Test Condition: 25°C / Unom: 6.0 V DC
Test Specification: according to S15.247
Comment 1: Dist.: 3m, Ant.: HK 116
Comment 2: Freq: 199.319MHz, Emax: 37.62dB μ V/m, RBW: 100kHz

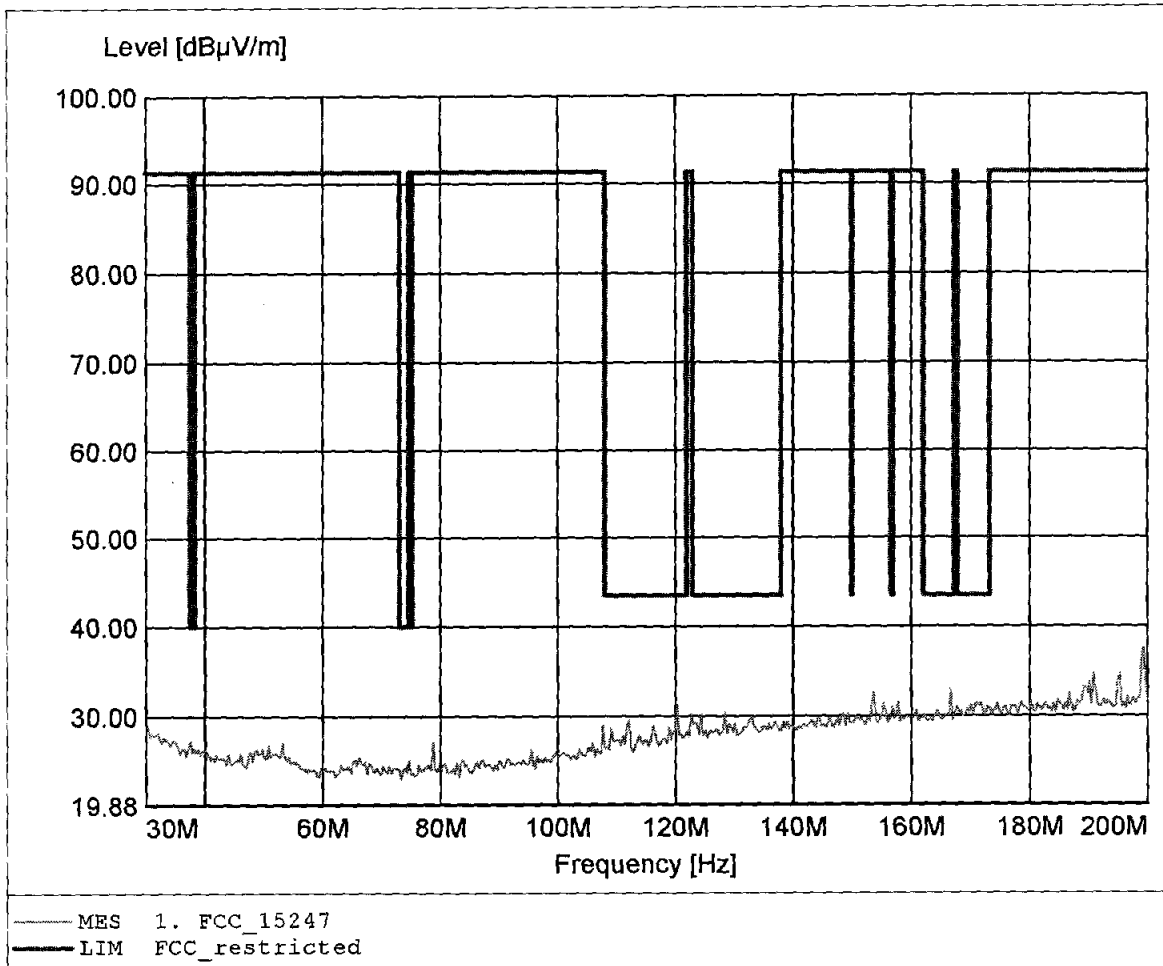

Spurious emissions Field Strength

FCC RULES PART 15, SUBPART C


Approval Holder: RTX Healthcare A/S
EUT: RTX3370 Monitor
Model: RTX3370 / 2402 MHz
Test Site / Operator: ETS / Mr. Meng
Test Condition: 25°C / Unom: 6.0 V DC
Test Specification: according to §15.247
Comment 1: Dist.: 3m, Ant.: HK 116
Comment 2: Freq: 198.978MHz, Emax: 37.09dBµV/m, RBW: 100kHz

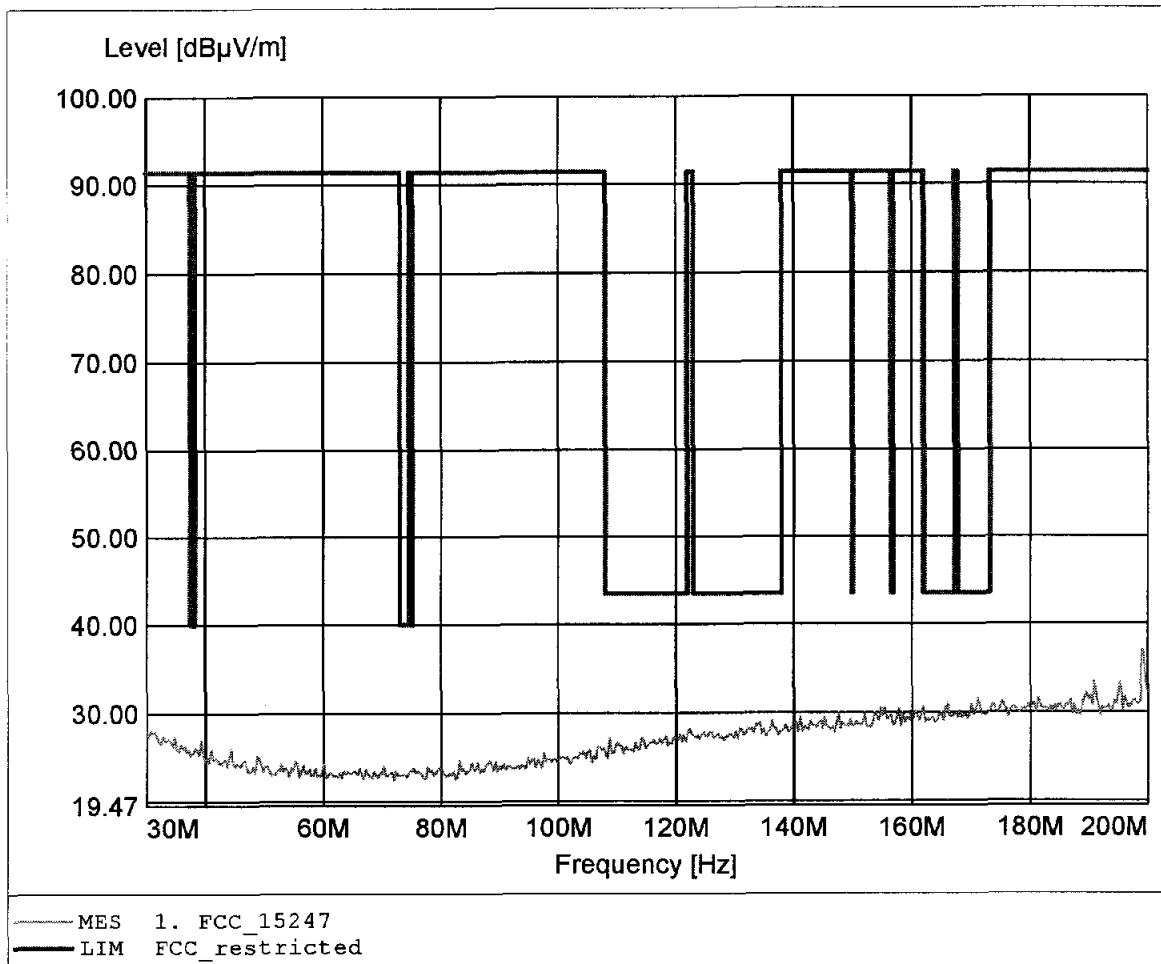

Spurious emissions Field Strength

FCC RULES PART 15, SUBPART C


Approval Holder: RTX Healthcare A/S
EUT: RTX3370 Monitor
Model: RTX3370 / 2402 MHz
Test Site / Operator: ETS / Mr. Meng
Test Condition: 25°C / Unom: 6.0 V DC
Test Specification: according to §15.247
Comment 1: Dist.: 3m, Ant.: HL 223, amplif.
Comment 2: Freq: 464.529MHz, Emax: 35.02dBµV/m, RBW: 100kHz

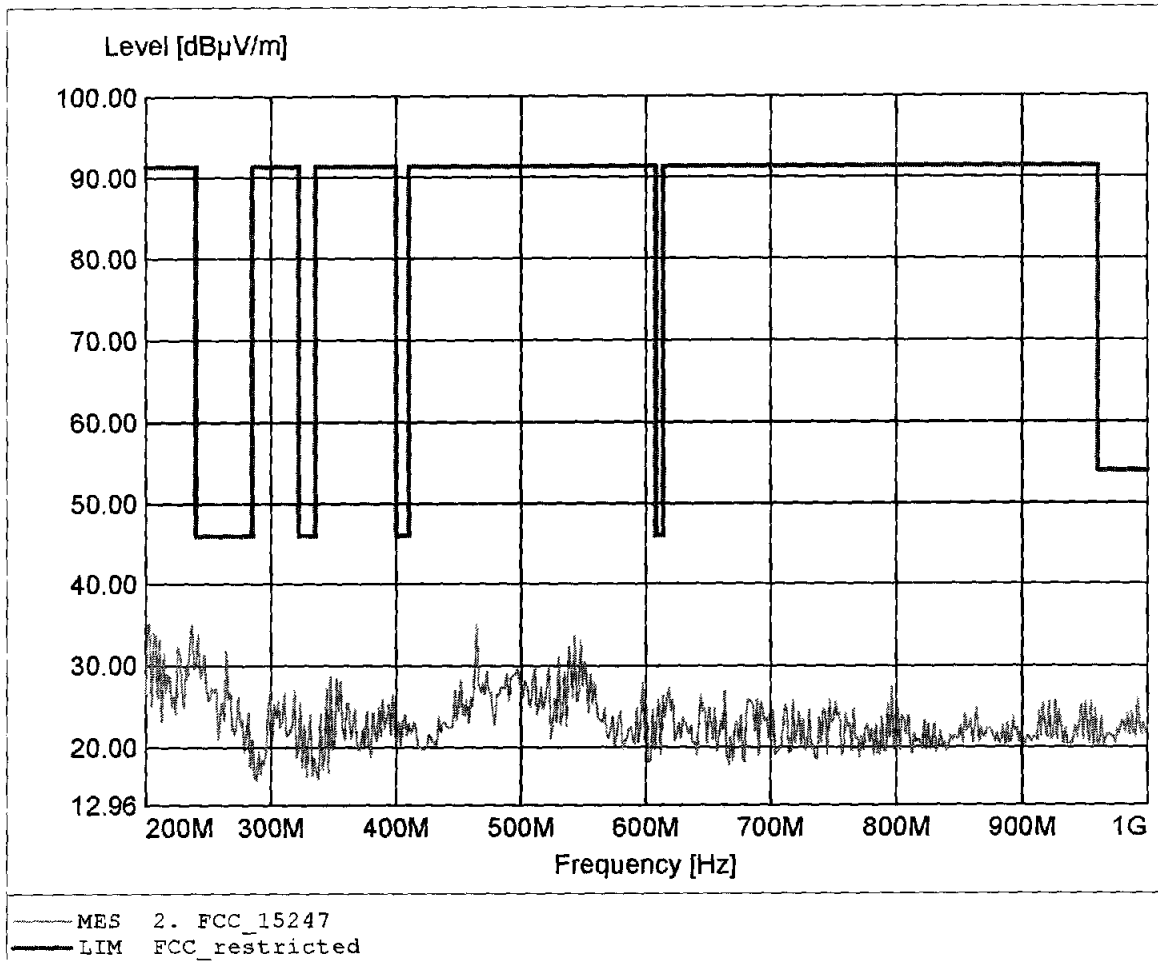

Spurious emissions Field Strength

FCC RULES PART 15, SUBPART C


Approval Holder: RTX Healthcare A/S
EUT: RTX3370 Monitor
Model: RTX3370 / 2402 MHz
Test Site / Operator: ETS / Mr. Meng
Test Condition: 25°C / Unom: 6.0 V DC
Test Specification: according to S15.247
Comment 1: Dist.: 3m, Ant.: HL 223, amplif.
Comment 2: Freq: 597.595MHz, Emax: 34.98dBµV/m, RBW: 100kHz

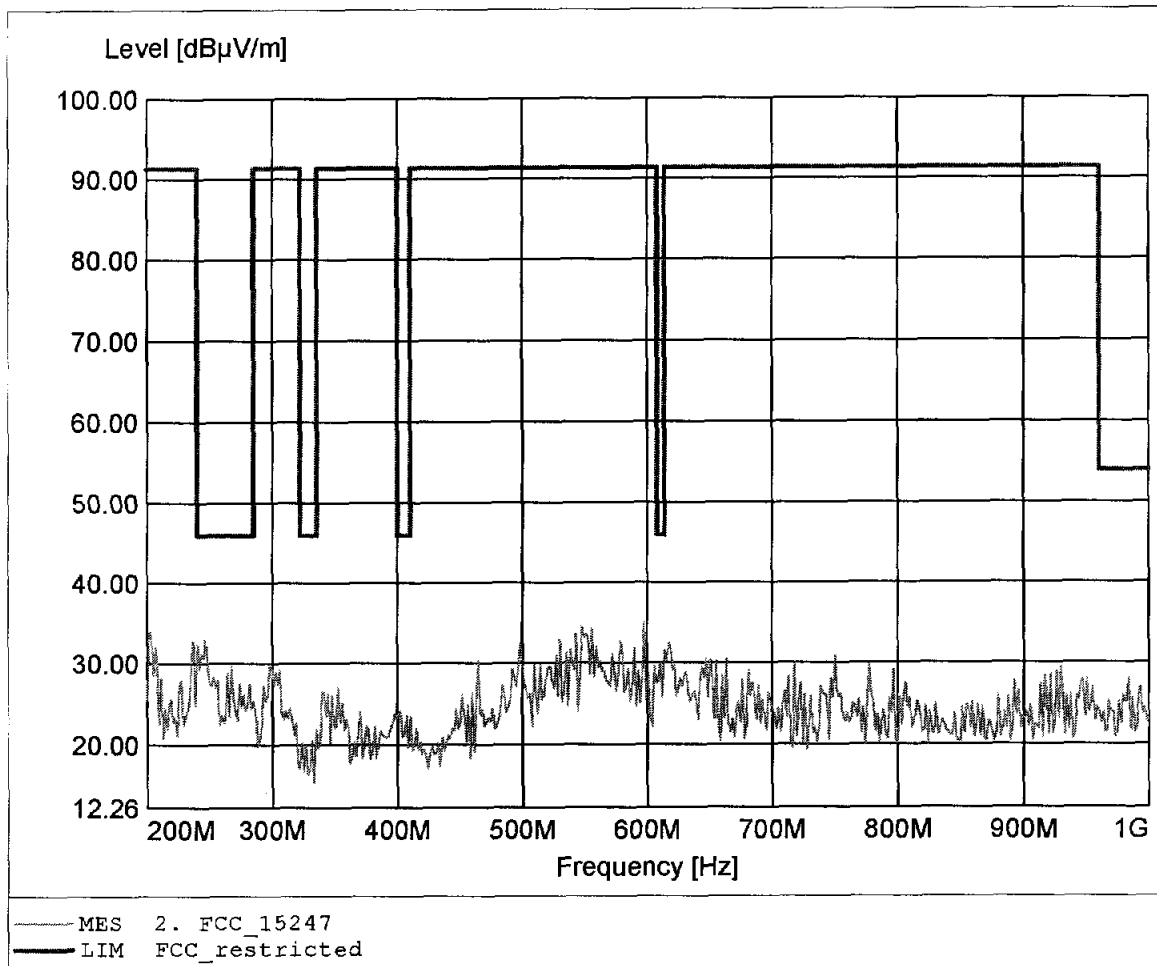

Spurious emissions Field Strength

FCC RULES PART 15, SUBPART C


Approval Holder: RTX Healthcare A/S
EUT: RTX3370 Monitor
Model: RTX3370 / 2402 MHz
Test Site / Operator: ETS / Mr. Meng
Test Condition: 25°C / Unom: 6.0 V DC
Test Specification: according to §15.247, peak detector
Comment 1: Dist.: 3m, Ant.: BBHA9120D, amplif.
Comment 2: Freq: 2.397GHz, Emax: 66.48dBµV/m, RBW: 1MHz

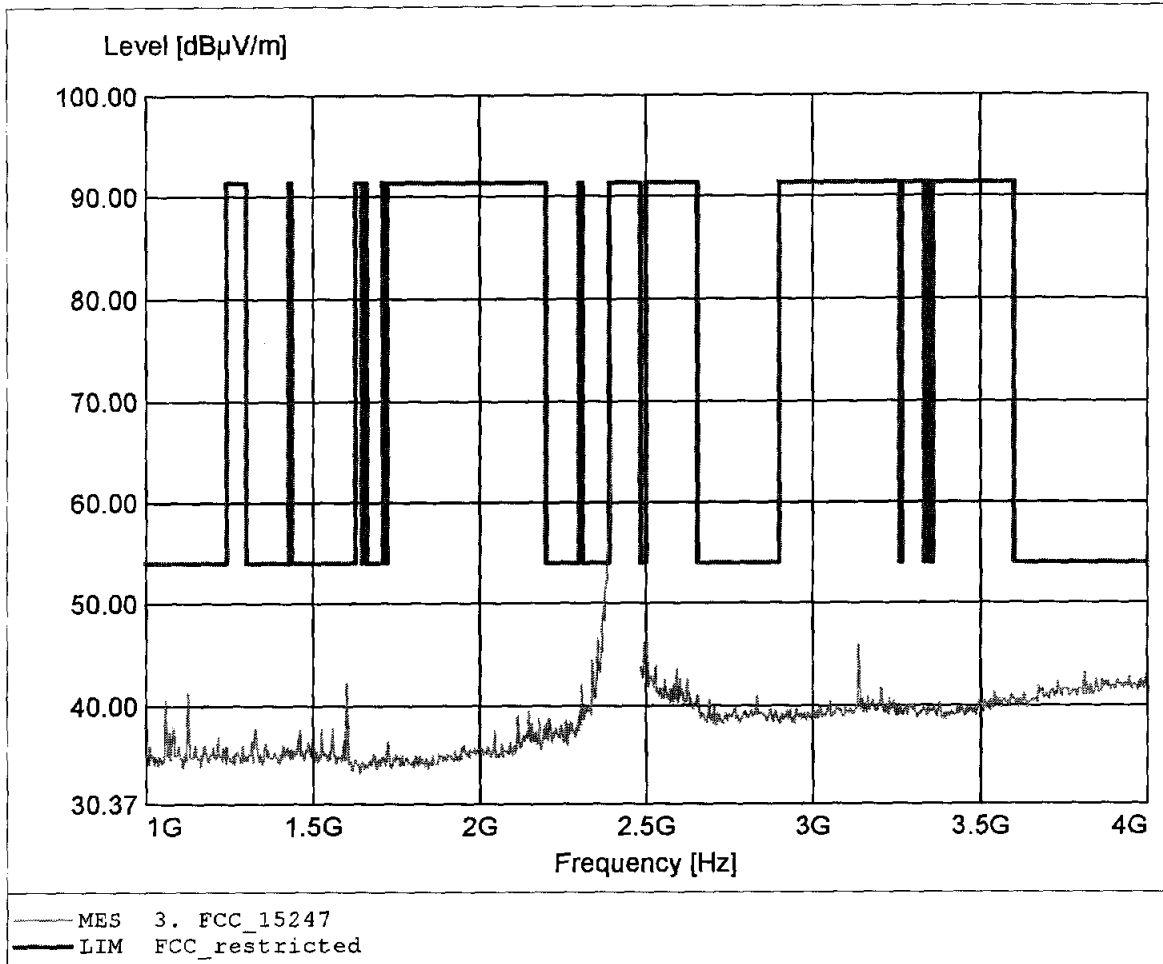

Spurious emissions Field Strength

FCC RULES PART 15, SUBPART C


Approval Holder: RTX Healthcare A/S
EUT: RTX3370 Monitor
Model: RTX3370 / 2402 MHz
Test Site / Operator: ETS / Mr. Meng
Test Condition: 25°C / Unom: 6.0 V DC
Test Specification: according to S15.247, average detector
Comment 1: Dist.: 3m, Ant.: BBHA9120D, amplif.
Comment 2: Freq: 2.397GHz, Emax: 48.68dBµV/m, RBW: 1MHz

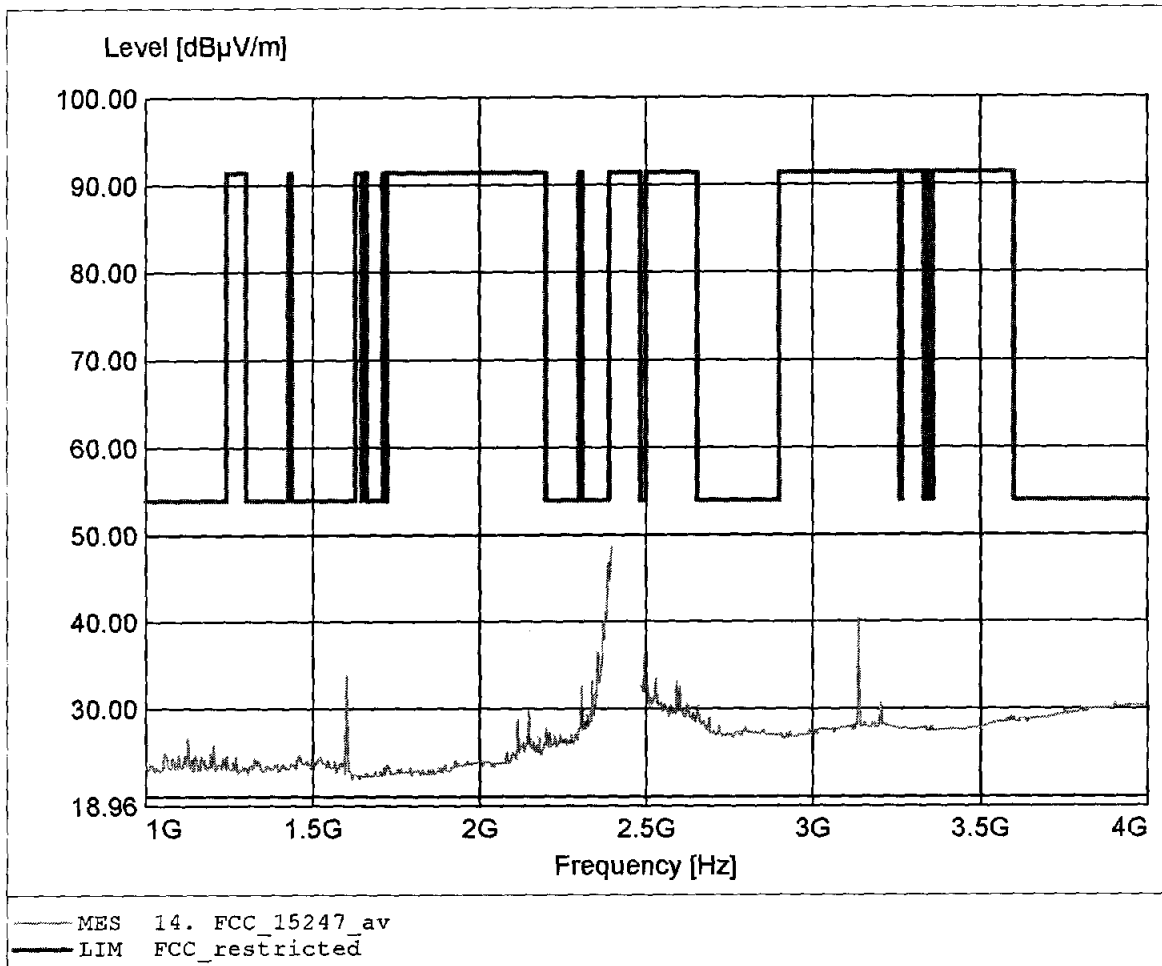

Spurious emissions Field Strength

FCC RULES PART 15, SUBPART C


Approval Holder: RTX Healthcare A/S
EUT: RTX3370 Monitor
Model: RTX3370 / 2402 MHz
Test Site / Operator: ETS / Mr. Meng
Test Condition: 25°C / Unom: 6.0 V DC
Test Specification: according to S15.247, peak detector
Comment 1: Dist.: 3m, Ant.: BBHA9120D, amplif.
Comment 2: Freq: 2.397GHz, Emax: 64.76dBμV/m, RBW: 1MHz

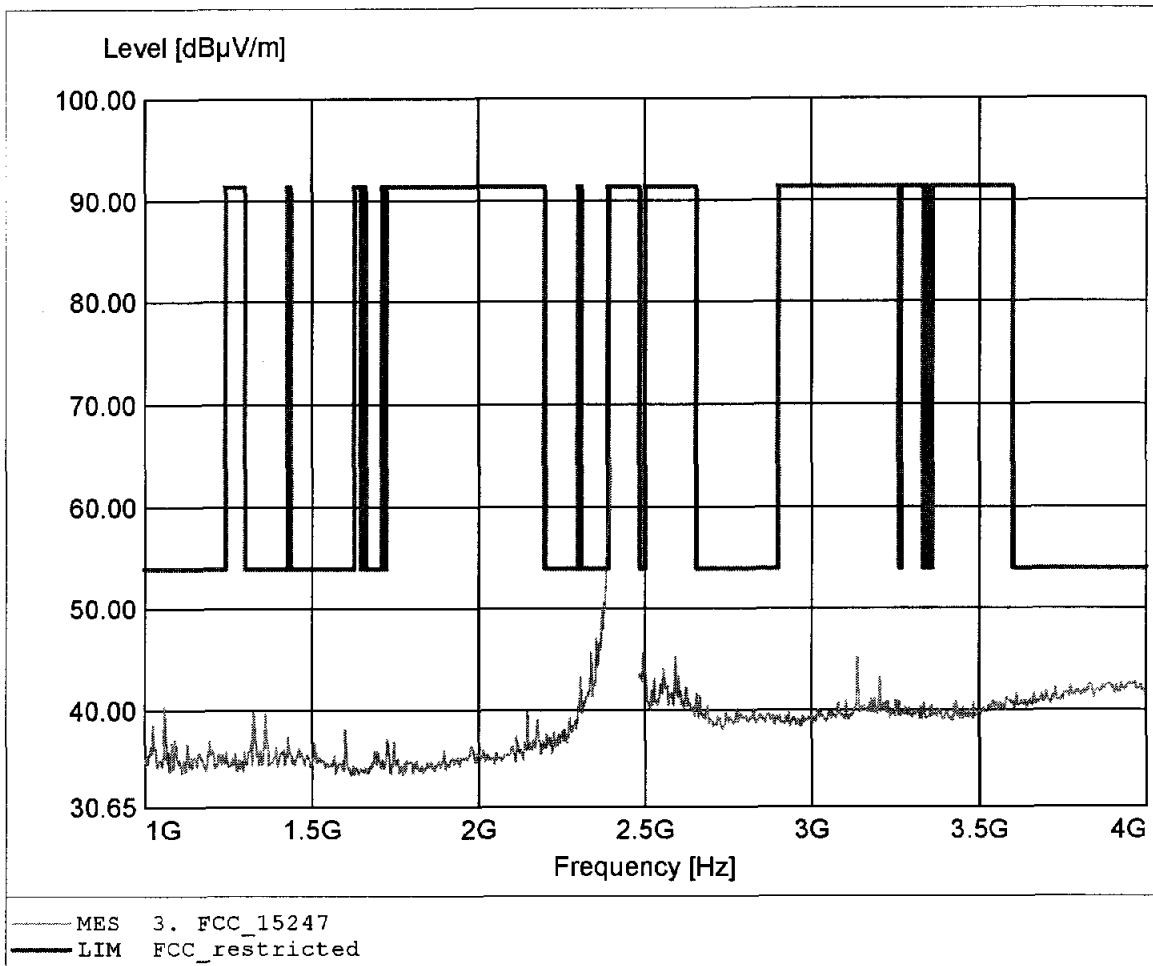

Spurious emissions Field Strength

FCC RULES PART 15, SUBPART C


Approval Holder: RTX Healthcare A/S
EUT: RTX3370 Monitor
Model: RTX3370 / 2402 MHz
Test Site / Operator: ETS / Mr. Meng
Test Condition: 25°C / Unom: 6.0 V DC
Test Specification: according to S15.247, average detector
Comment 1: Dist.: 3m, Ant.: BBHA9120D, amplif.
Comment 2: Freq: 2.397GHz, Emax: 47.82dBμV/m, RBW: 1MHz

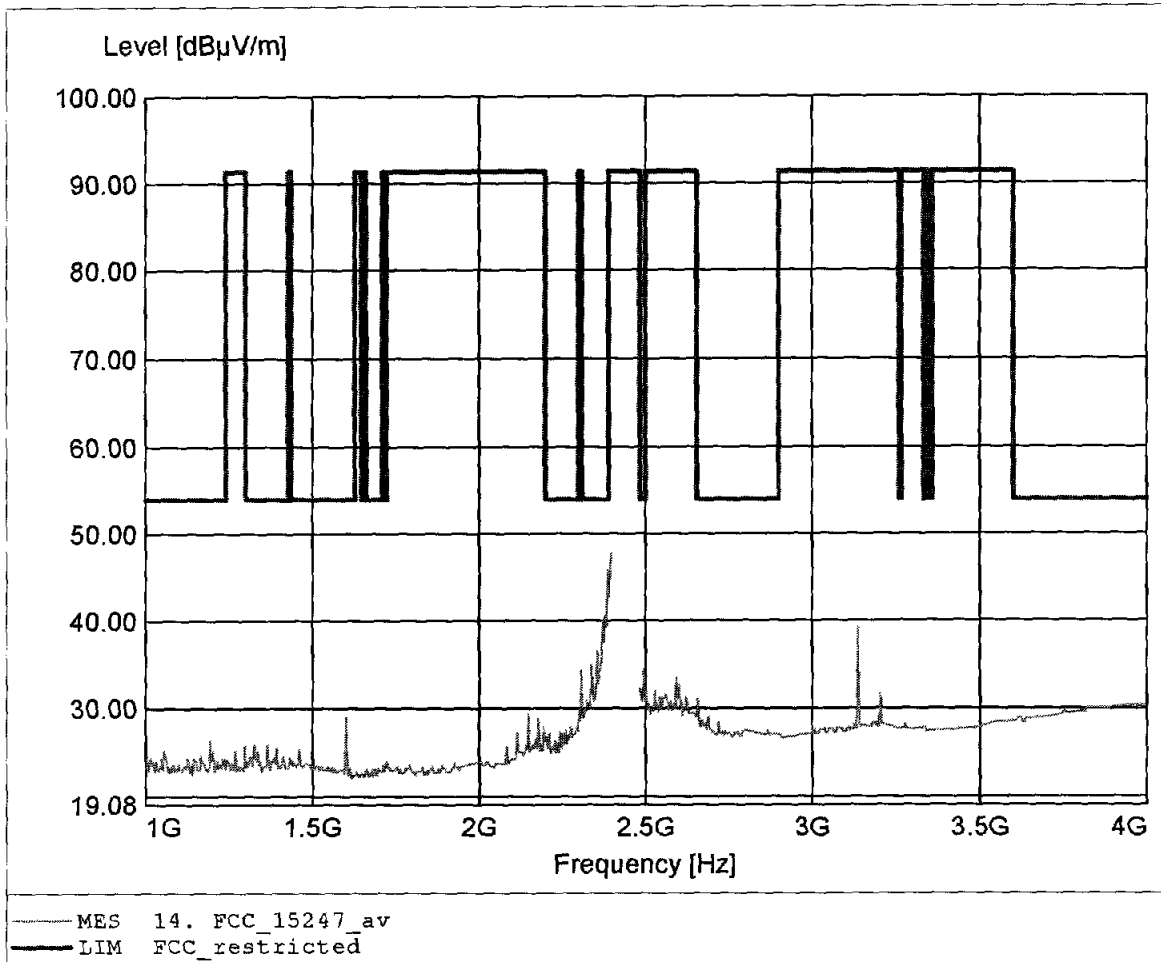

Spurious emissions Field Strength

FCC RULES PART 15, SUBPART C


Approval Holder: RTX Healthcare A/S
EUT: RTX3370 Monitor
Model: RTX3370 / 2402 MHz
Test Site / Operator: ETS / Mr. Meng
Test Condition: 25°C / Unom: 6.0 V DC
Test Specification: according to S15.247, peak detector
Comment 1: Dist.: 3m, Ant.: BBHA9120D, ampl.+HP.
Comment 2: Freq: 6.870GHz, Emax: 45.32dBμV/m, RBW: 1MHz

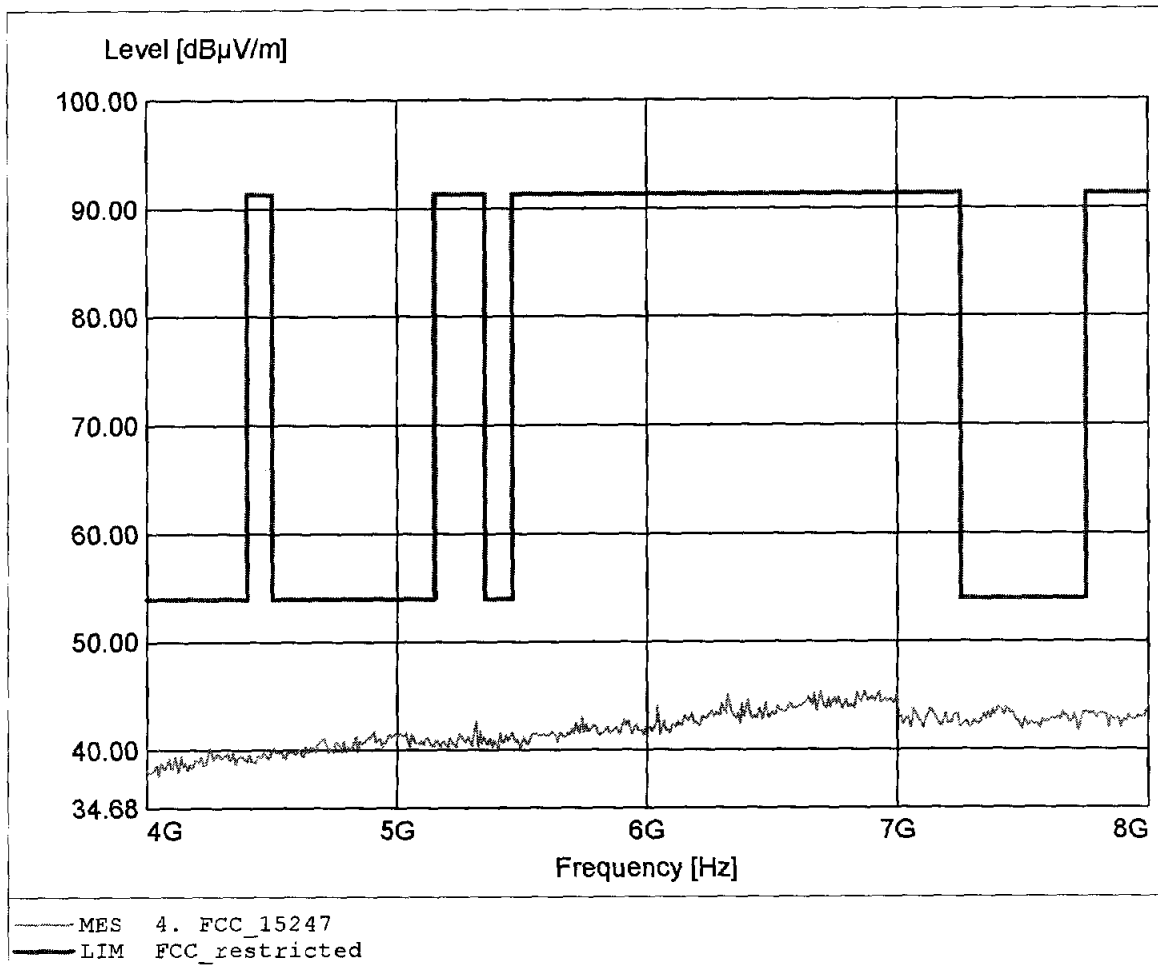

Spurious emissions Field Strength

FCC RULES PART 15, SUBPART C


Approval Holder: RTX Healthcare A/S
EUT: RTX3370 Monitor
Model: RTX3370 / 2402 MHz
Test Site / Operator: ETS / Mr. Meng
Test Condition: 25°C / Unom: 6.0 V DC
Test Specification: according to §15.247, peak detector
Comment 1: Dist.: 3m, Ant.: BBHA9120D, ampl.+HP.
Comment 2: Freq: 6.934GHz, Emax: 45.76dBµV/m, RBW: 1MHz

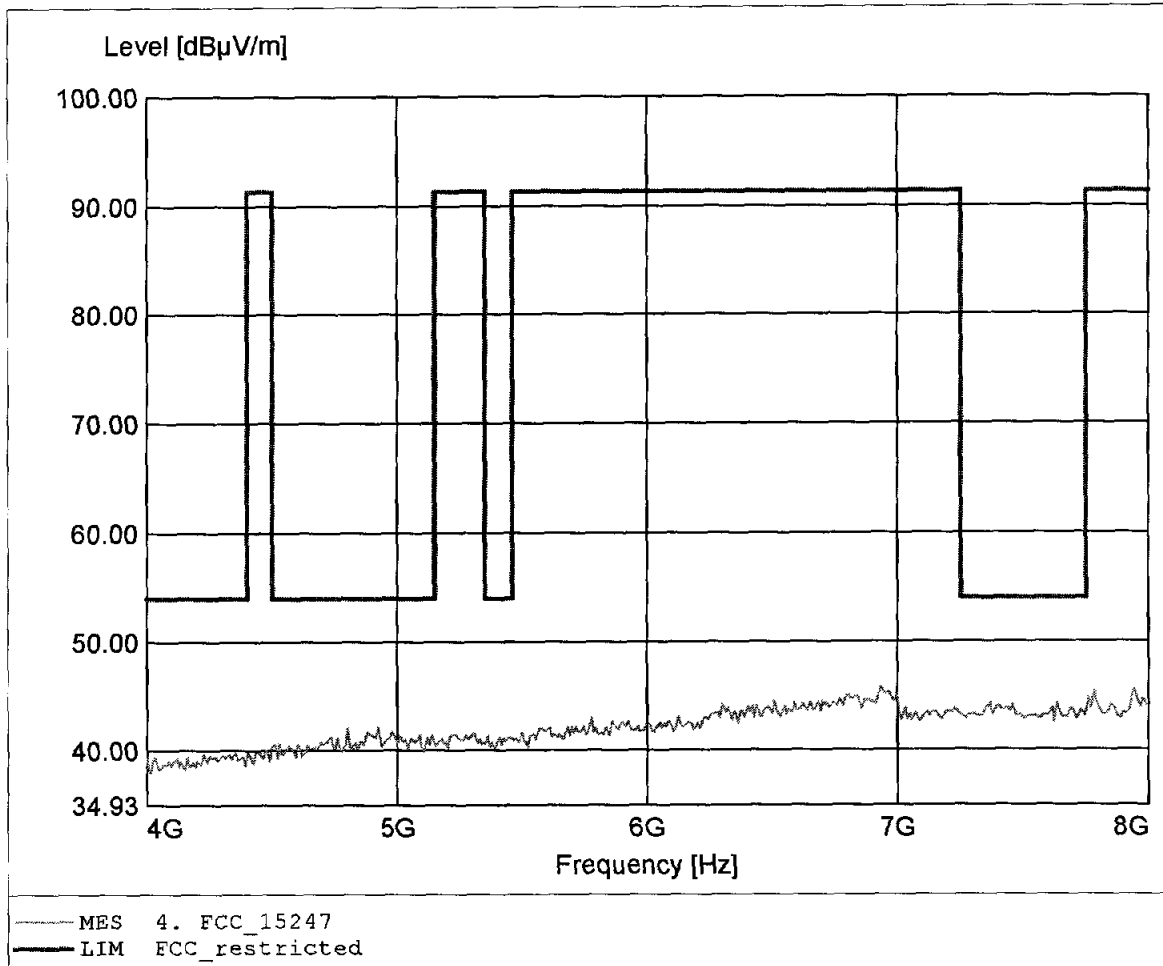

Spurious emissions Field Strength

FCC RULES PART 15, SUBPART C


Approval Holder: RTX Healthcare A/S
EUT: RTX3370 Monitor
Model: RTX3370 / 2402 MHz
Test Site / Operator: ETS / Mr. Meng
Test Condition: 25°C / Unom: 6.0 V DC
Test Specification: according to §15.247, peak detector
Comment 1: Dist.: 3m, Ant.: BBHA9120D, ampl.+HP.
Comment 2: Freq: 11.070GHz, Emax: 39.11dBµV/m, RBW: 1MHz

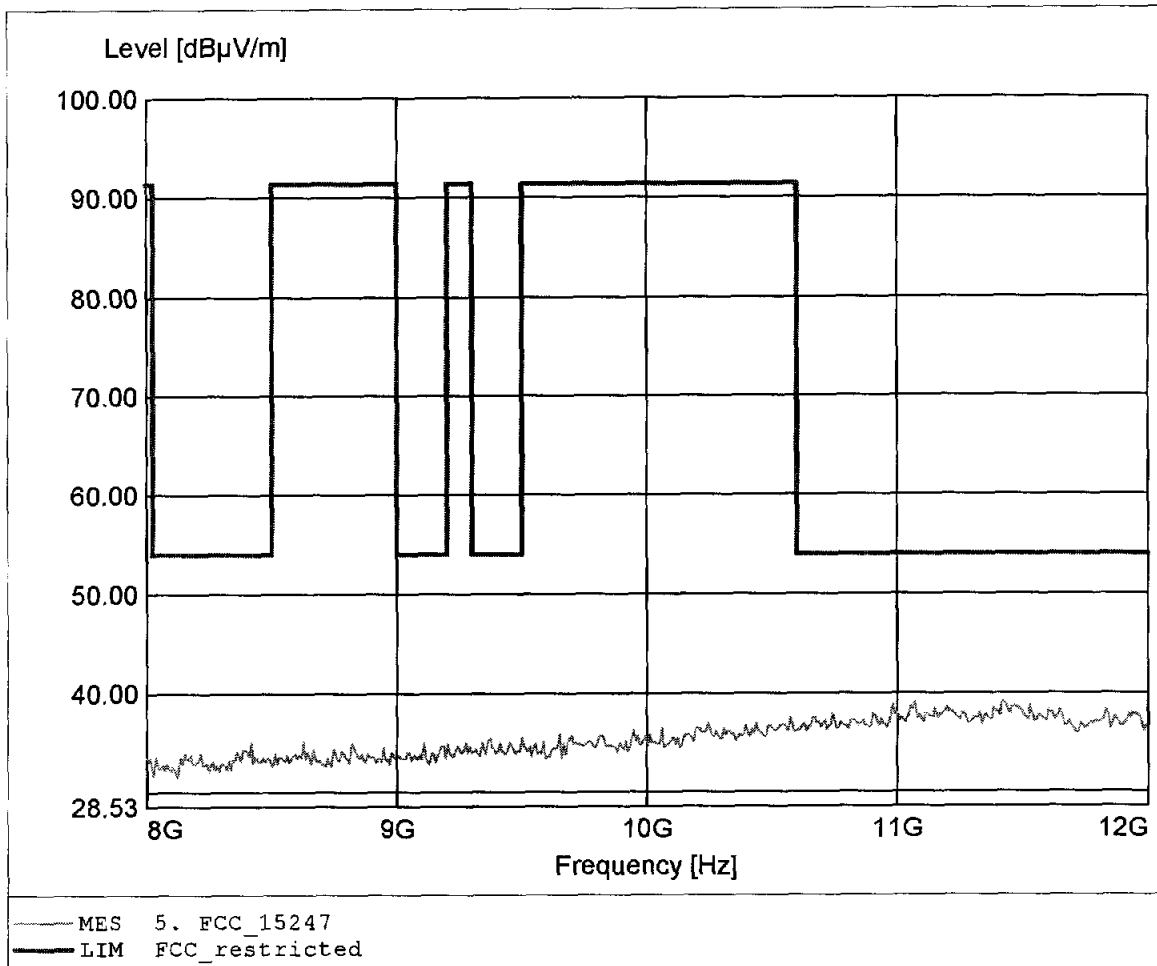

Spurious emissions Field Strength

FCC RULES PART 15, SUBPART C


Approval Holder: RTX Healthcare A/S
EUT: RTX3370 Monitor
Model: RTX3370 / 2402 MHz
Test Site / Operator: ETS / Mr. Meng
Test Condition: 25°C / Unom: 6.0 V DC
Test Specification: according to S15.247, peak detector
Comment 1: Dist.: 3m, Ant.: BBHA9120D, ampl.+HP.
Comment 2: Freq: 11.182GHz, Emax: 39.21dBμV/m, RBW: 1MHz

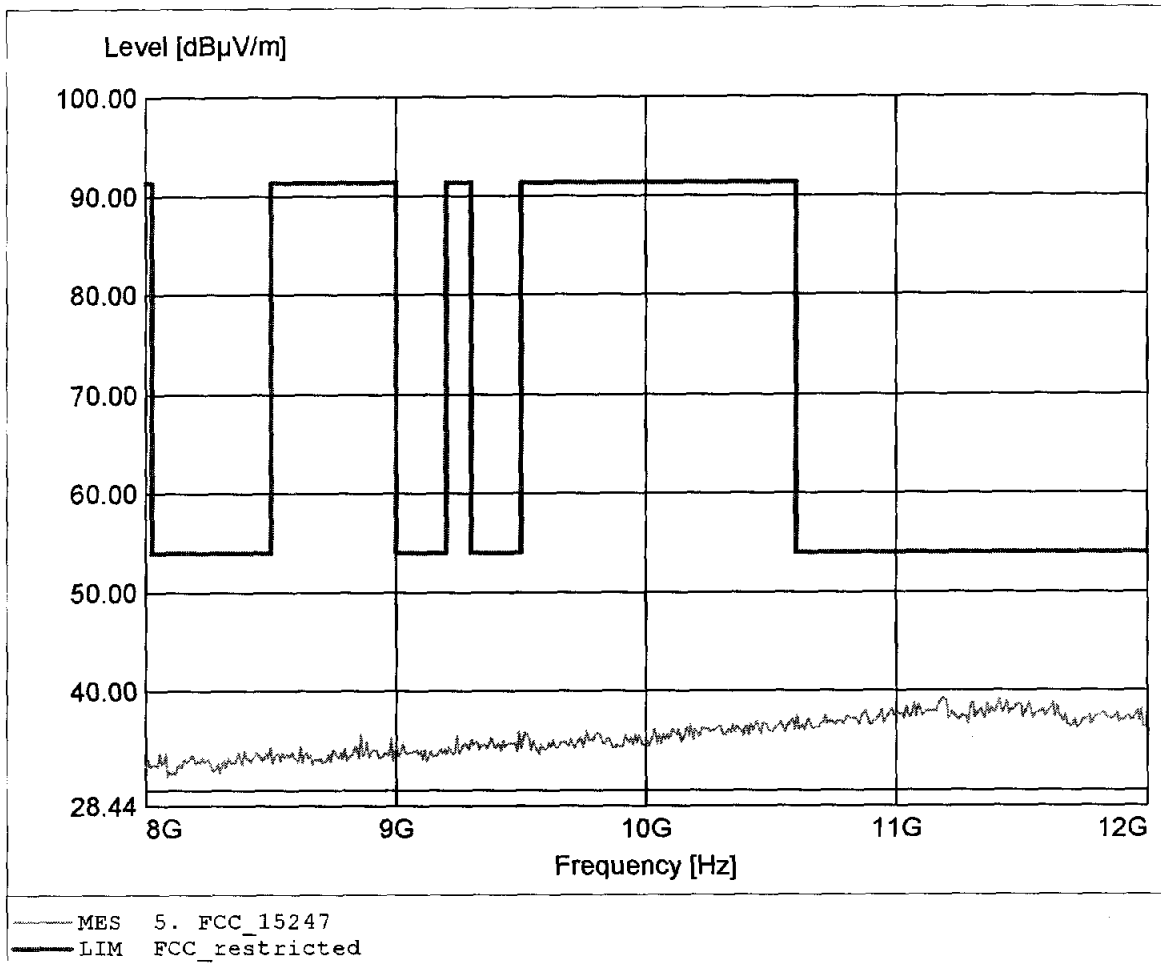

Spurious emissions Field Strength

FCC RULES PART 15, SUBPART C


Approval Holder: RTX Healthcare A/S
EUT: RTX3370 Monitor
Model: RTX3370 / 2402 MHz
Test Site / Operator: ETS / Mr. Meng
Test Condition: 25°C / Unom: 6.0 V DC
Test Specification: according to §15.247, peak detector
Comment 1: Dist.: 3m, Ant.: BBHA9120D, ampl.+HP.
Comment 2: Freq: 12.010GHz, Emax: 41.23dBµV/m, RBW: 1MHz

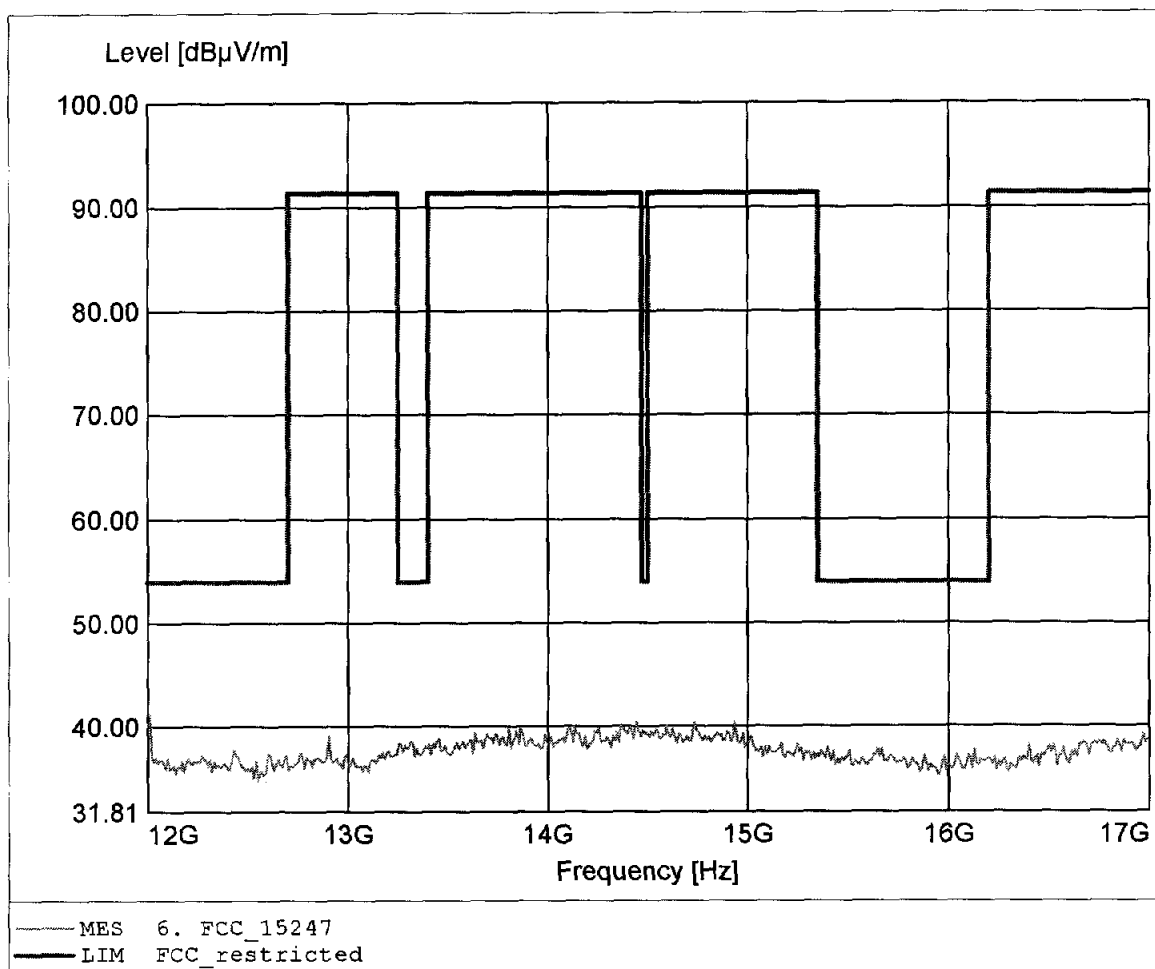

Spurious emissions Field Strength

FCC RULES PART 15, SUBPART C


Approval Holder: RTX Healthcare A/S
EUT: RTX3370 Monitor
Model: RTX3370 / 2402 MHz
Test Site / Operator: ETS / Mr. Meng
Test Condition: 25°C / Unom: 6.0 V DC
Test Specification: according to S15.247, peak detector
Comment 1: Dist.: 3m, Ant.: BBHA9120D, ampl.+HP.
Comment 2: Freq: 12.000GHz, Emax: 45.60dBμV/m, RBW: 1MHz

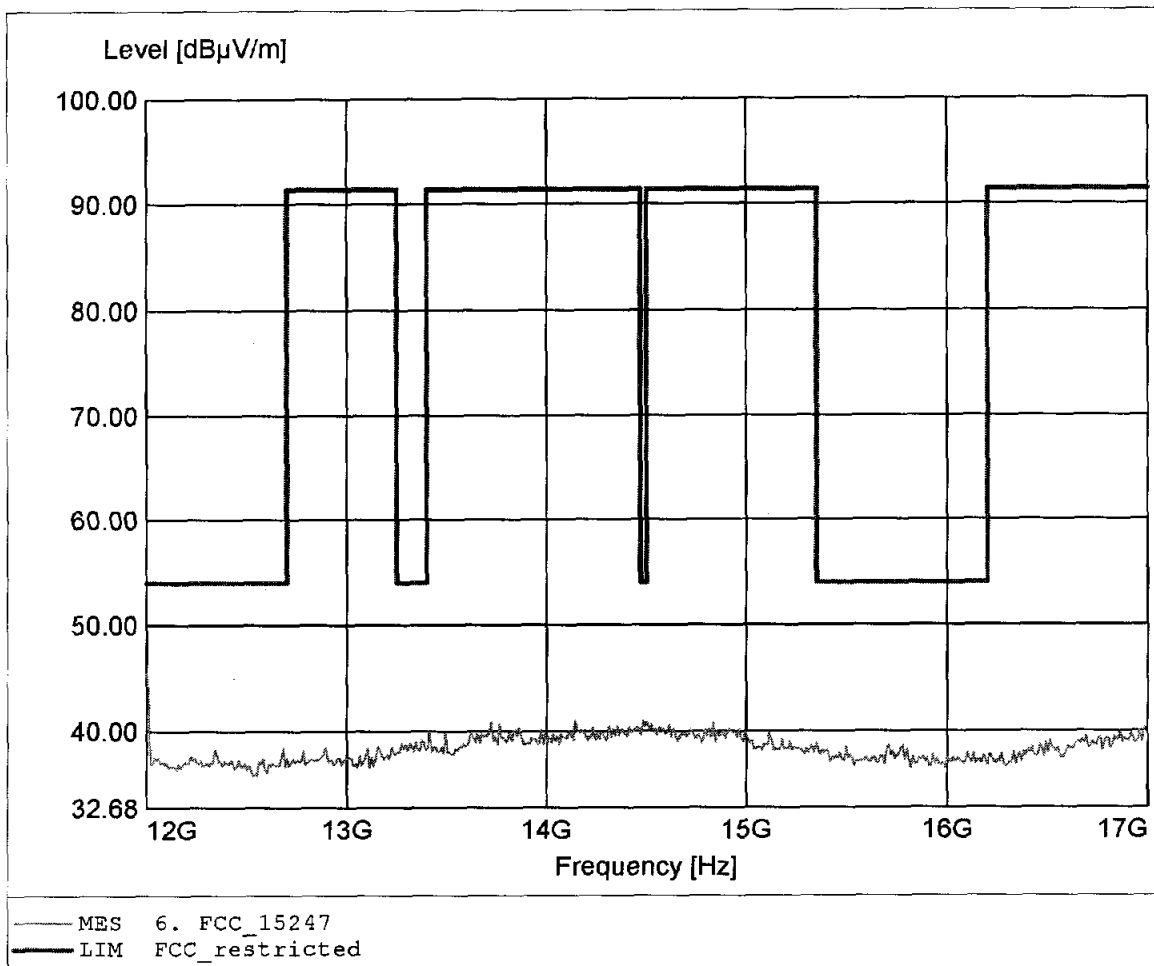

Spurious emissions Field Strength

FCC RULES PART 15, SUBPART C


Approval Holder: RTX Healthcare A/S
EUT: RTX3370 Monitor
Model: RTX3370 / 2402 MHz
Test Site / Operator: ETS / Mr. Meng
Test Condition: 25°C / Unom: 6.0 V DC
Test Specification: according to S15.247, peak detector
Comment 1: Dist.: 3m, Ant.: HL025, amplif.
Comment 2: Freq: 24.558GHz, Emax: 48.86dBμV/m, RBW: 1MHz

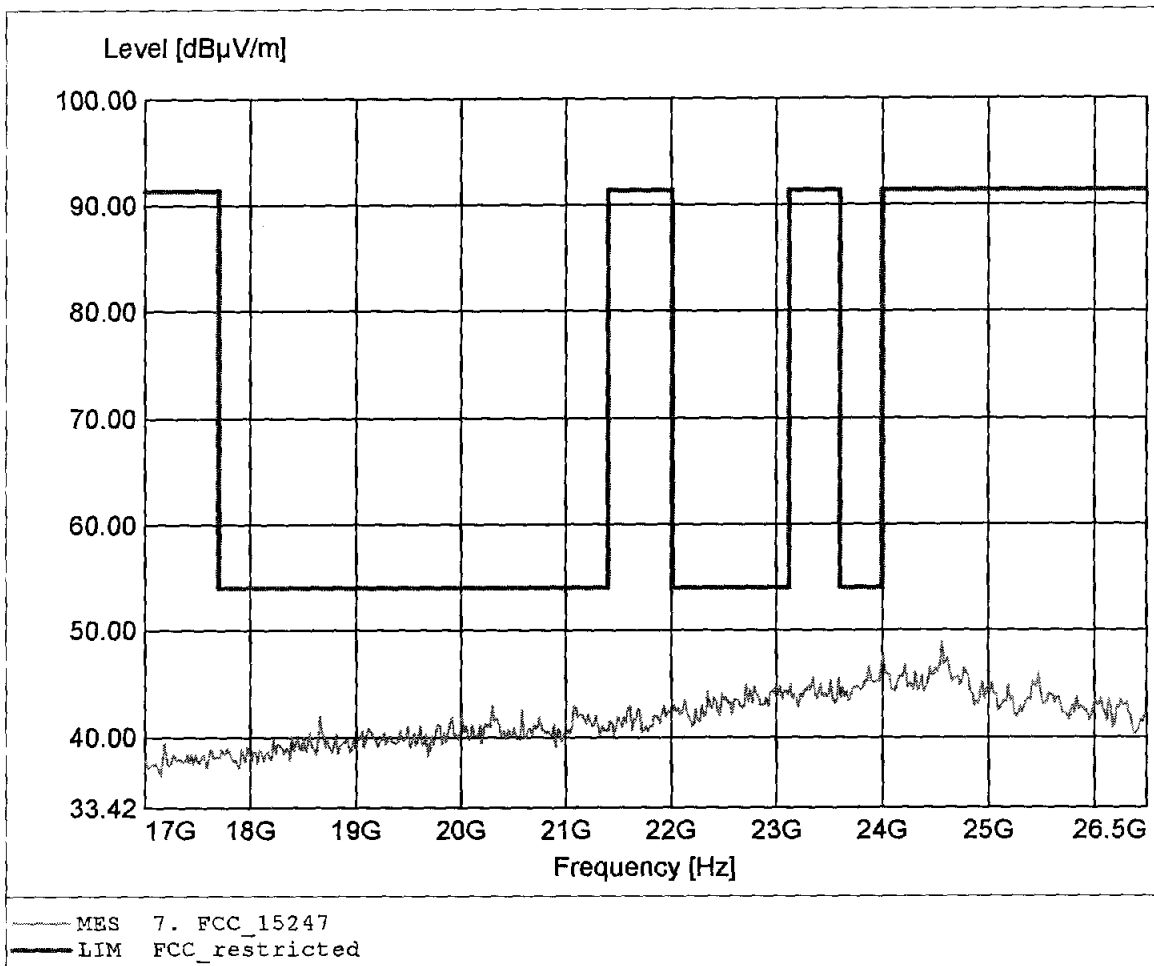

Spurious emissions Field Strength

FCC RULES PART 15, SUBPART C


Approval Holder: RTX Healthcare A/S
EUT: RTX3370 Monitor
Model: RTX3370 / 2402 MHz
Test Site / Operator: ETS / Mr. Meng
Test Condition: 25°C / Unom: 6.0 V DC
Test Specification: according to §15.247, peak detector
Comment 1: Dist.: 3m, Ant.: HL025, amplif.
Comment 2: Freq: 24.482GHz, Emax: 48.75dBµV/m, RBW: 1MHz

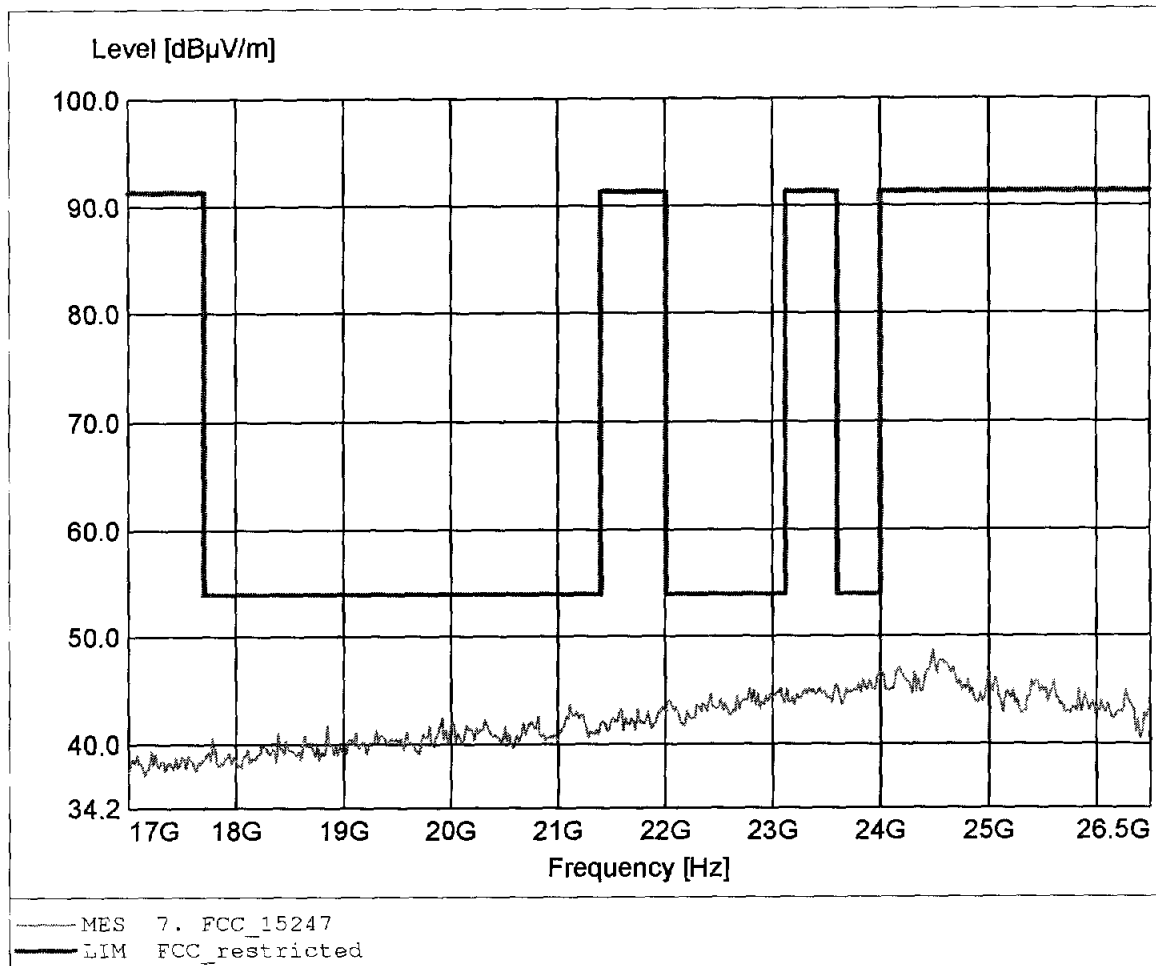

Spurious emissions Field Strength

FCC RULES PART 15, SUBPART C


Approval Holder: RTX Healthcare A/S
EUT: RTX3370 Monitor
Model: RTX3370 / 2441 MHz
Test Site / Operator: ETS / Mr. Meng
Test Condition: 25°C / Unom: 6.0 V DC
Test Specification: according to S15.247
Comment 1: Dist.: 3m, Ant.: HK 116
Comment 2: Freq: 199.319MHz, Emax: 43.55dBµV/m, RBW: 100kHz

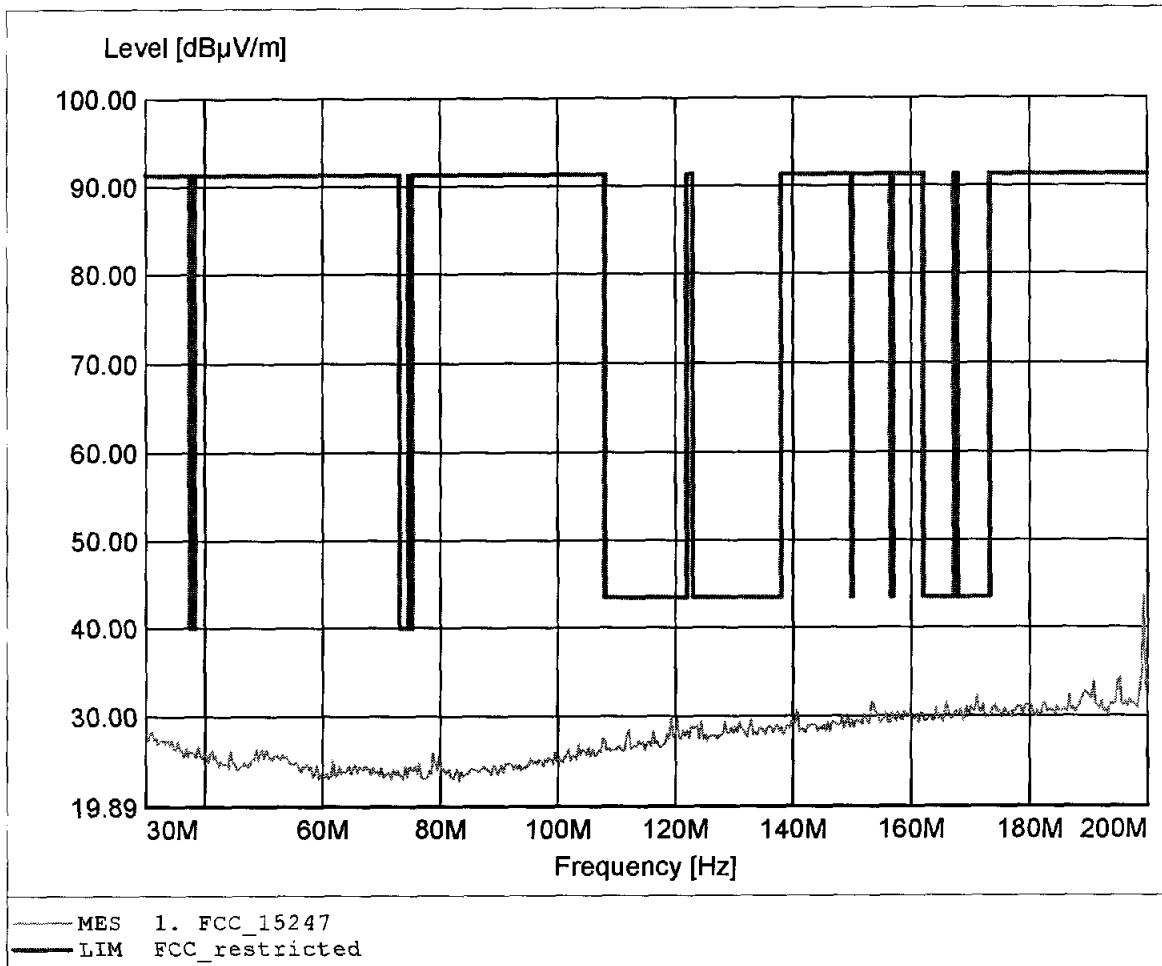

Spurious emissions Field Strength

FCC RULES PART 15, SUBPART C


Approval Holder: RTX Healthcare A/S
EUT: RTX3370 Monitor
Model: RTX3370 / 2441 MHz
Test Site / Operator: ETS / Mr. Meng
Test Condition: 25°C / Unom: 6.0 V DC
Test Specification: according to §15.247
Comment 1: Dist.: 3m, Ant.: HK 116
Comment 2: Freq: 199.319MHz, Emax: 36.28dBµV/m, RBW: 100kHz

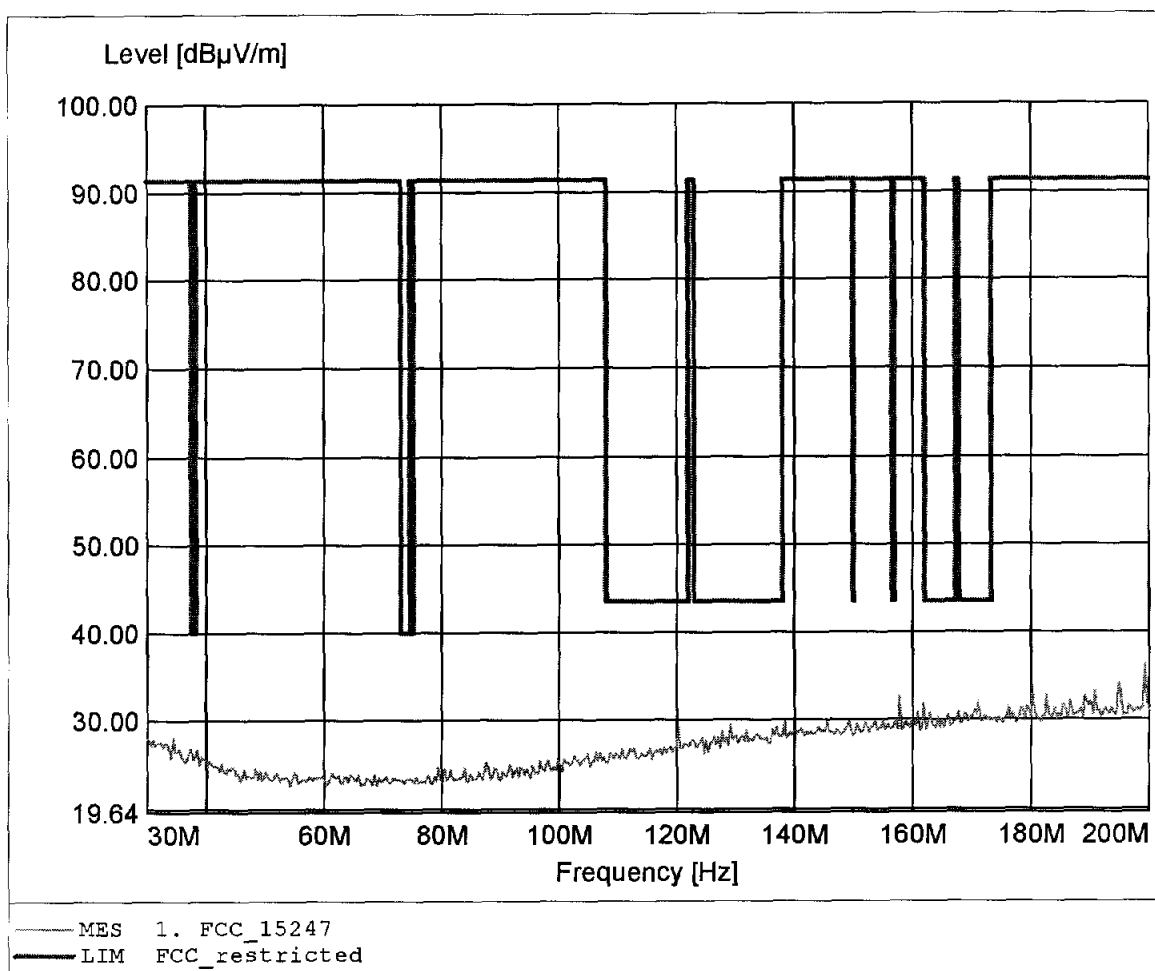

Spurious emissions Field Strength

FCC RULES PART 15, SUBPART C


Approval Holder: RTX Healthcare A/S
EUT: RTX3370 Monitor
Model: RTX3370 / 2441 MHz
Test Site / Operator: ETS / Mr. Meng
Test Condition: 25°C / Unom: 6.0 V DC
Test Specification: according to §15.247
Comment 1: Dist.: 3m, Ant.: HL 223, amplif.
Comment 2: Freq: 236.874MHz, Emax: 35.96dBµV/m, RBW: 100kHz

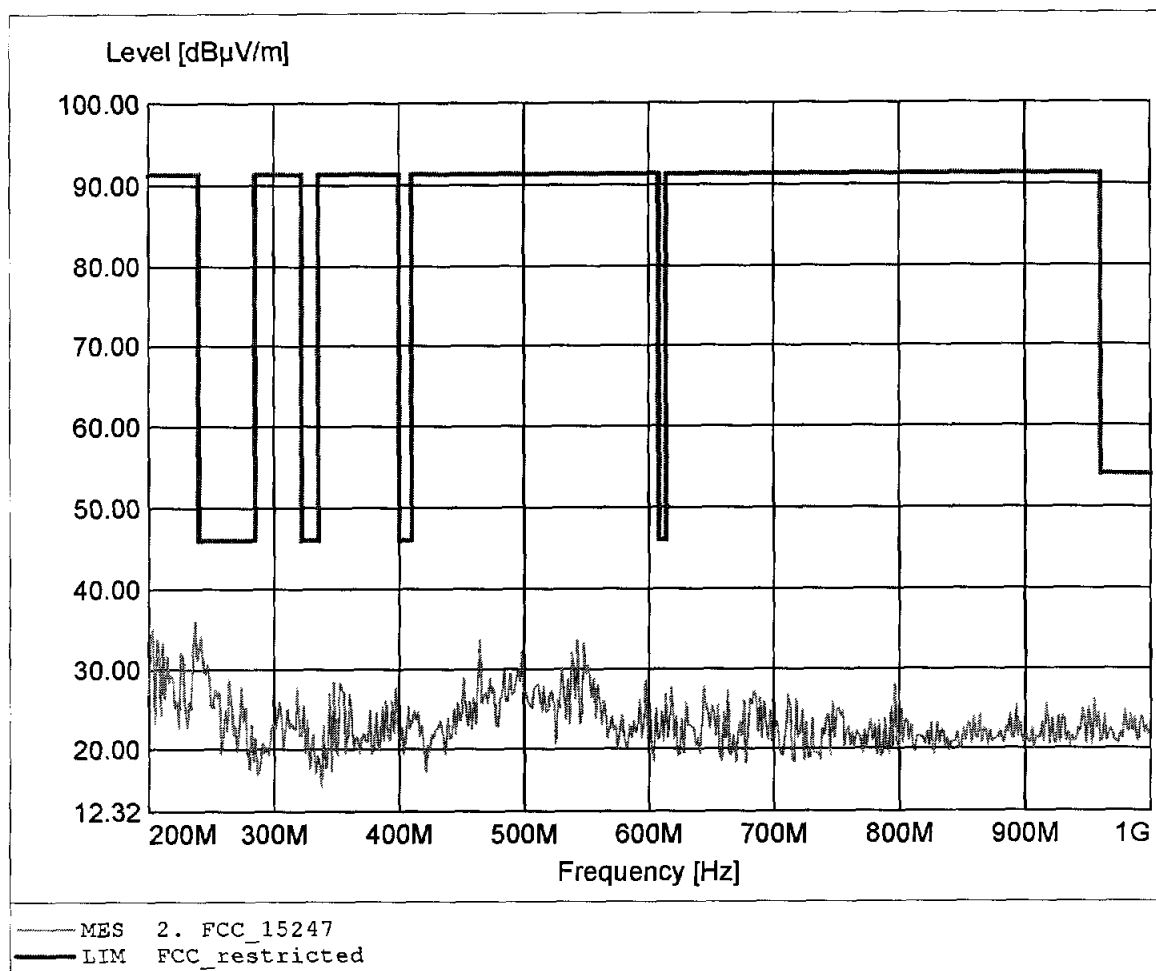

Spurious emissions Field Strength

FCC RULES PART 15, SUBPART C


Approval Holder: RTX Healthcare A/S
EUT: RTX3370 Monitor
Model: RTX3370 / 2441 MHz
Test Site / Operator: ETS / Mr. Meng
Test Condition: 25°C / Unom: 6.0 V DC
Test Specification: according to §15.247
Comment 1: Dist.: 3m, Ant.: HL 223, amplif.
Comment 2: Freq: 530.261MHz, Emax: 35.87dBµV/m, RBW: 100kHz

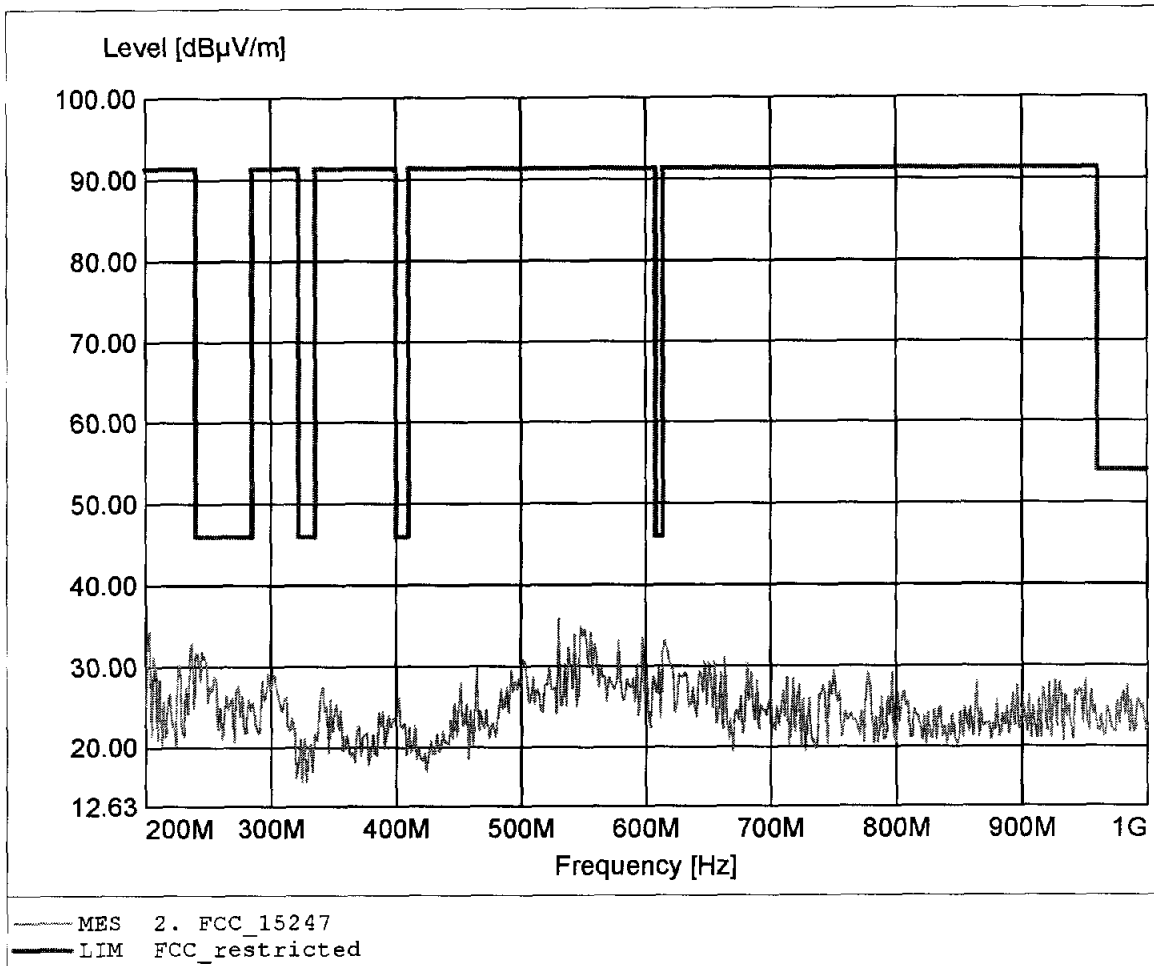

Spurious emissions Field Strength

FCC RULES PART 15, SUBPART C


Approval Holder: RTX Healthcare A/S
EUT: RTX3370 Monitor
Model: RTX3370 / 2441 MHz
Test Site / Operator: ETS / Mr. Meng
Test Condition: 25°C / Unom: 6.0 V DC
Test Specification: according to §15.247, peak detector
Comment 1: Dist.: 3m, Ant.: BBHA9120D, amplif.
Comment 2: Freq: 2.394GHz, Emax: 50.68dBµV/m, RBW: 1MHz

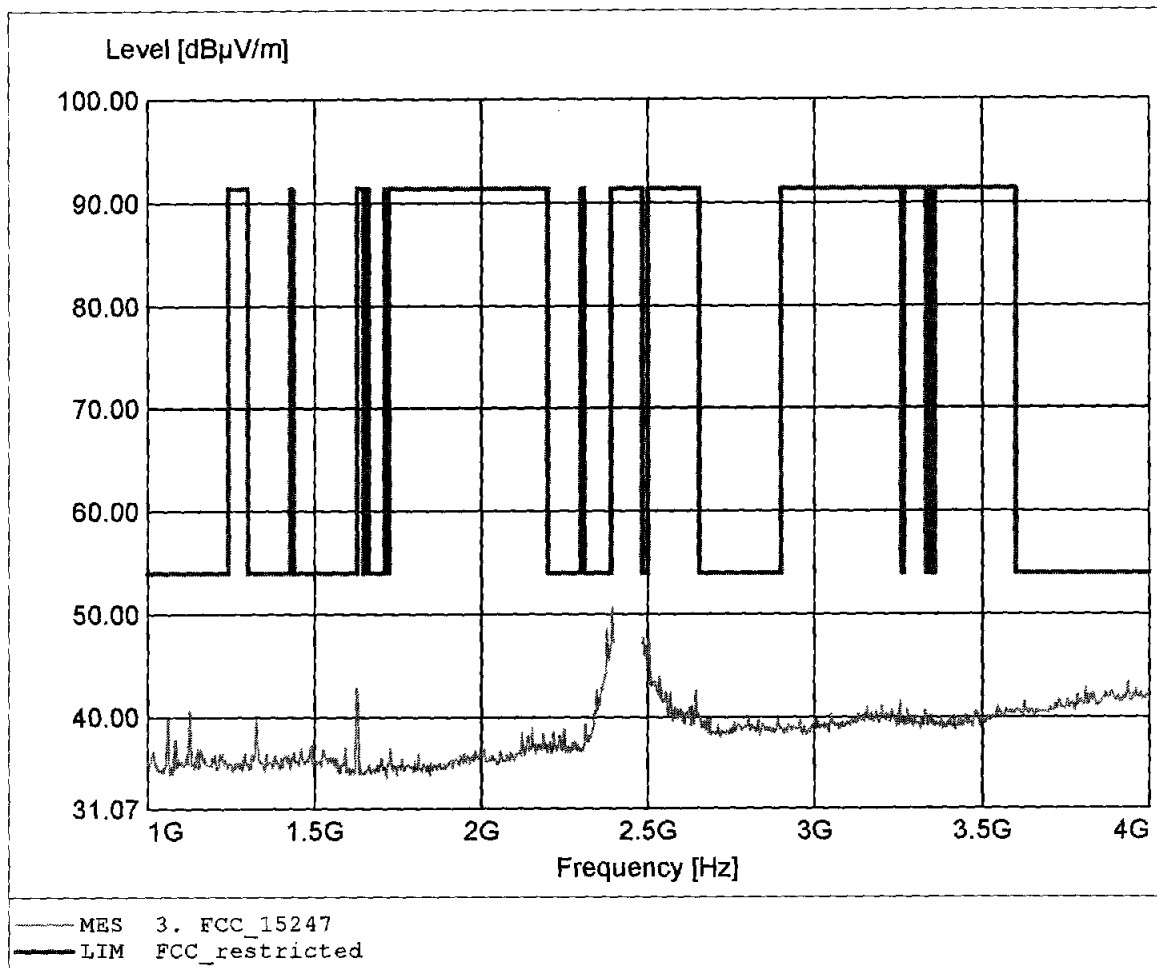

Spurious emissions Field Strength

FCC RULES PART 15, SUBPART C


Approval Holder: RTX Healthcare A/S
EUT: RTX3370 Monitor
Model: RTX3370 / 2441 MHz
Test Site / Operator: ETS / Mr. Meng
Test Condition: 25°C / Unom: 6.0 V DC
Test Specification: according to §15.247, peak detector
Comment 1: Dist.: 3m, Ant.: BBHA9120D, amplif.
Comment 2: Freq: 2.394GHz, Emax: 49.79dBµV/m, RBW: 1MHz

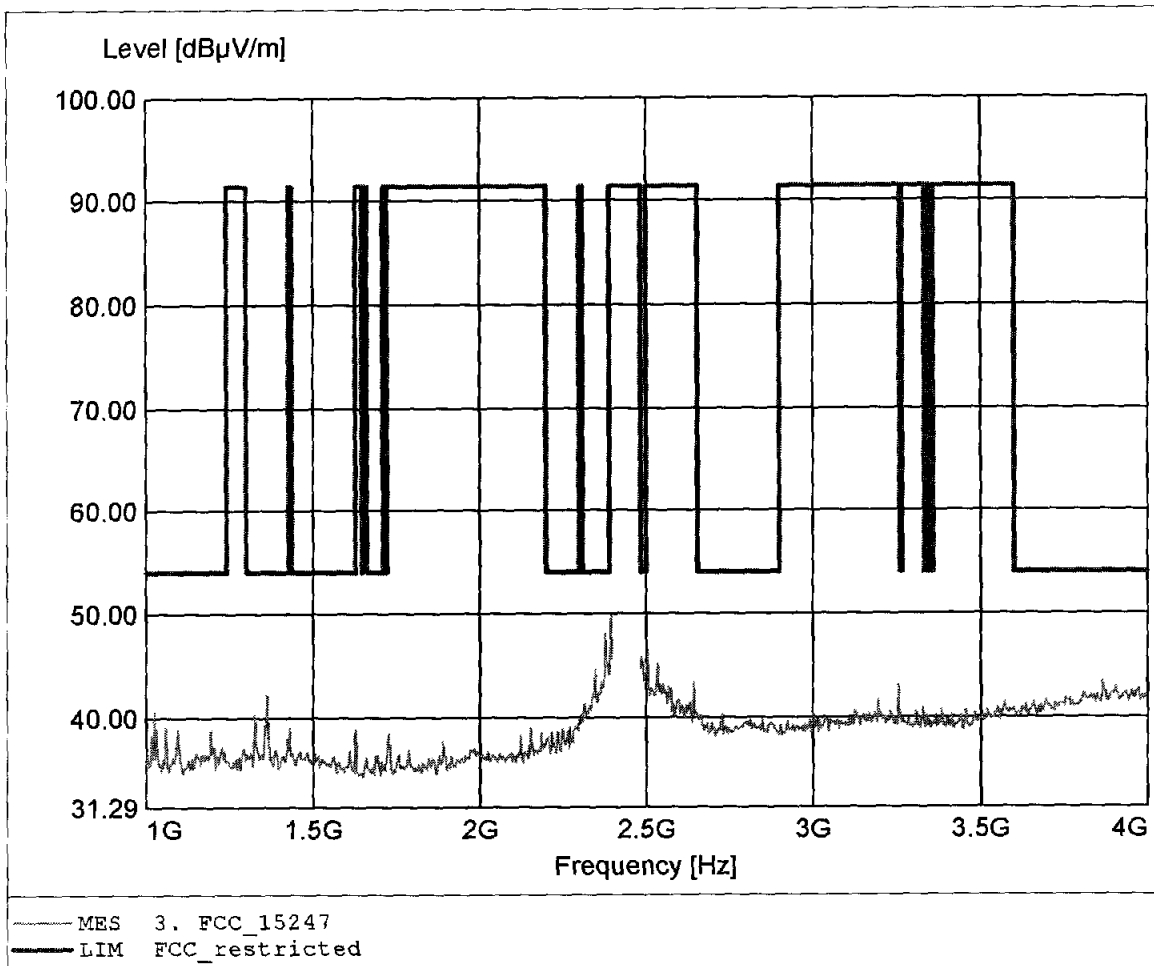

Spurious emissions Field Strength

FCC RULES PART 15, SUBPART C


Approval Holder: RTX Healthcare A/S
EUT: RTX3370 Monitor
Model: RTX3370 / 2441 MHz
Test Site / Operator: ETS / Mr. Meng
Test Condition: 25°C / Unom: 6.0 V DC
Test Specification: according to §15.247, peak detector
Comment 1: Dist.: 3m, Ant.: BBHA9120D, ampl.+HP.
Comment 2: Freq: 6.974GHz, Emax: 46.03dBµV/m, RBW: 1MHz

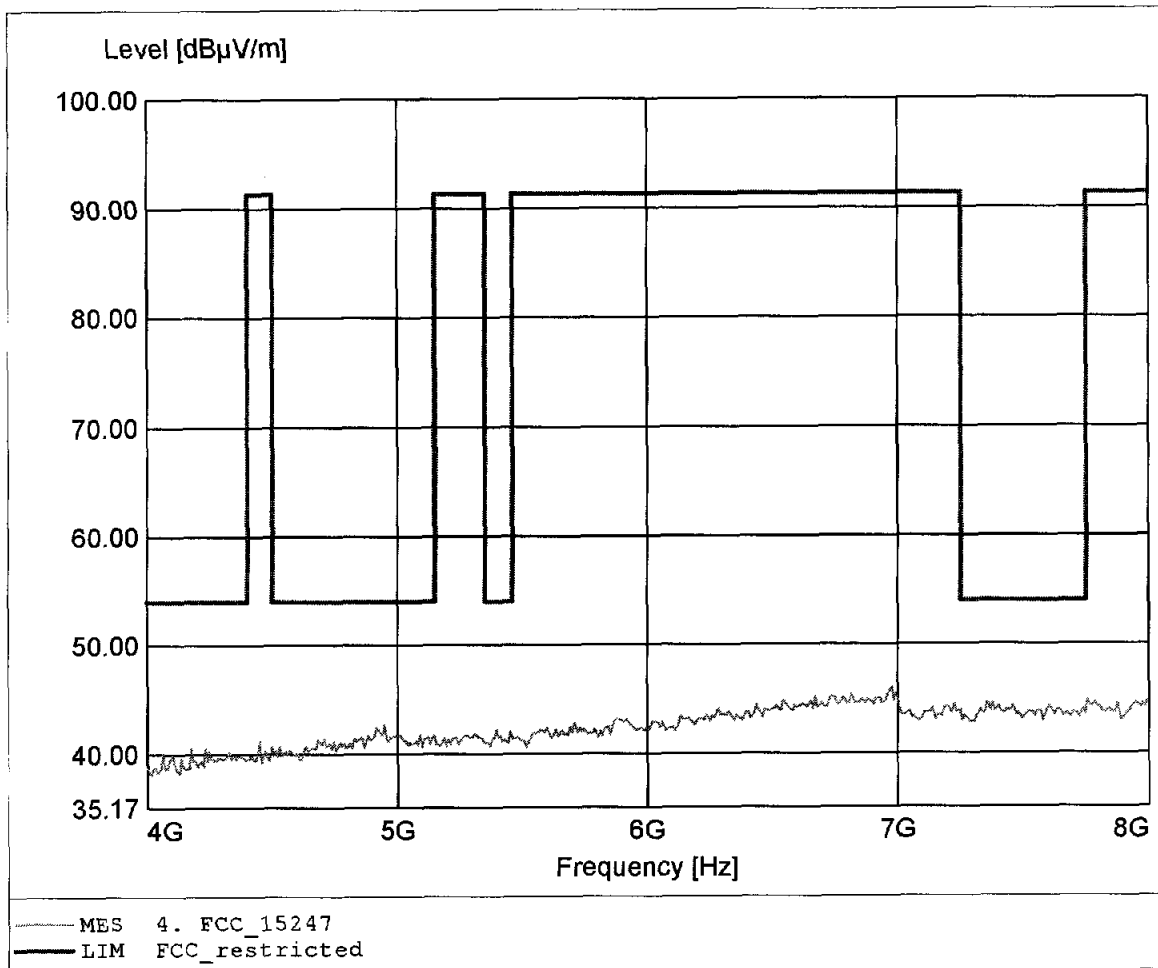

Spurious emissions Field Strength

FCC RULES PART 15, SUBPART C


Approval Holder: RTX Healthcare A/S
EUT: RTX3370 Monitor
Model: RTX3370 / 2441 MHz
Test Site / Operator: ETS / Mr. Meng
Test Condition: 25°C / Unom: 6.0 V DC
Test Specification: according to S15.247, peak detector
Comment 1: Dist.: 3m, Ant.: BBHA9120D, ampl.+HP.
Comment 2: Freq: 6.854GHz, Emax: 45.81dBµV/m, RBW: 1MHz

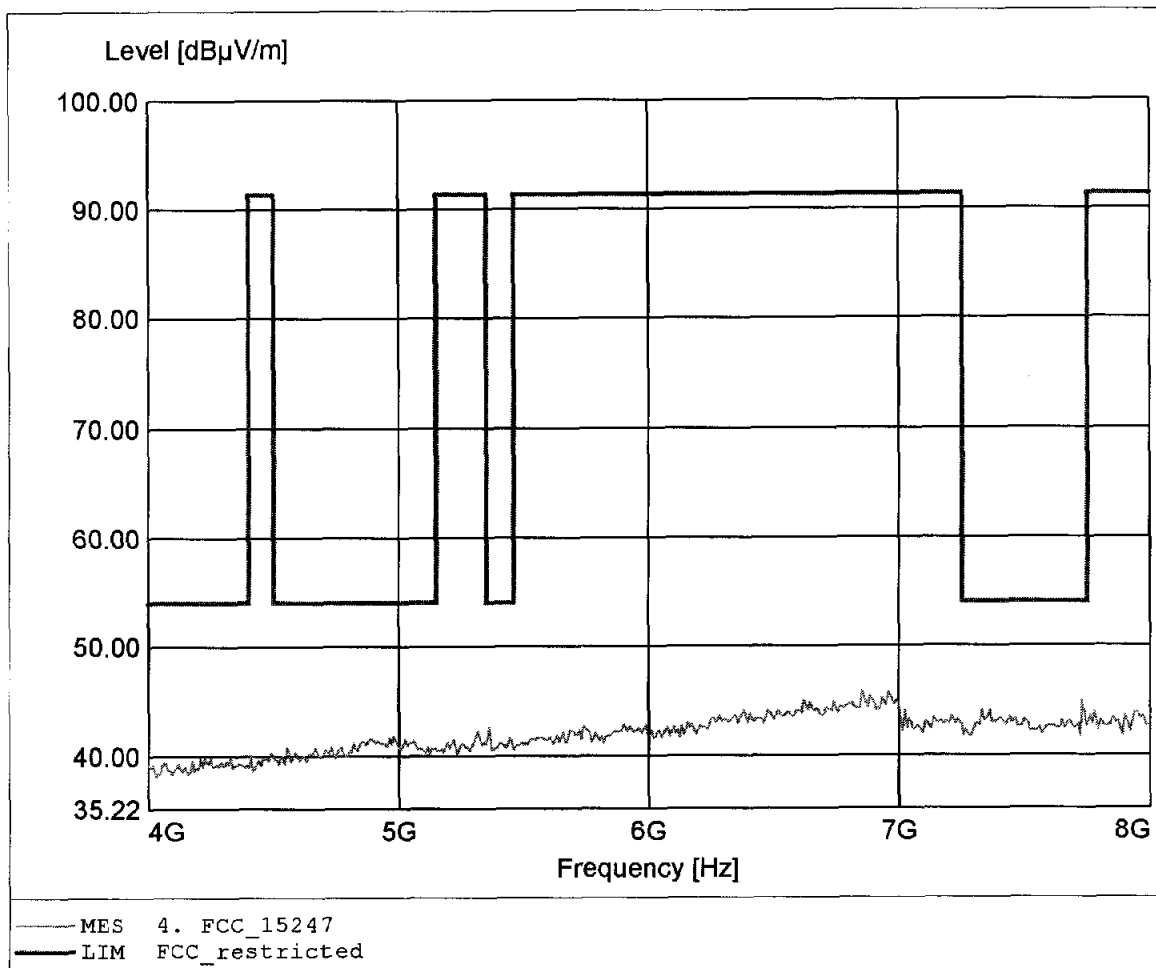

Spurious emissions Field Strength

FCC RULES PART 15, SUBPART C


Approval Holder: RTX Healthcare A/S
EUT: RTX3370 Monitor
Model: RTX3370 / 2441 MHz
Test Site / Operator: ETS / Mr. Meng
Test Condition: 25°C / Unom: 6.0 V DC
Test Specification: according to §15.247, peak detector
Comment 1: Dist.: 3m, Ant.: BBHA9120D, ampl.+HP.
Comment 2: Freq: 11.094GHz, Emax: 39.81dBµV/m, RBW: 1MHz

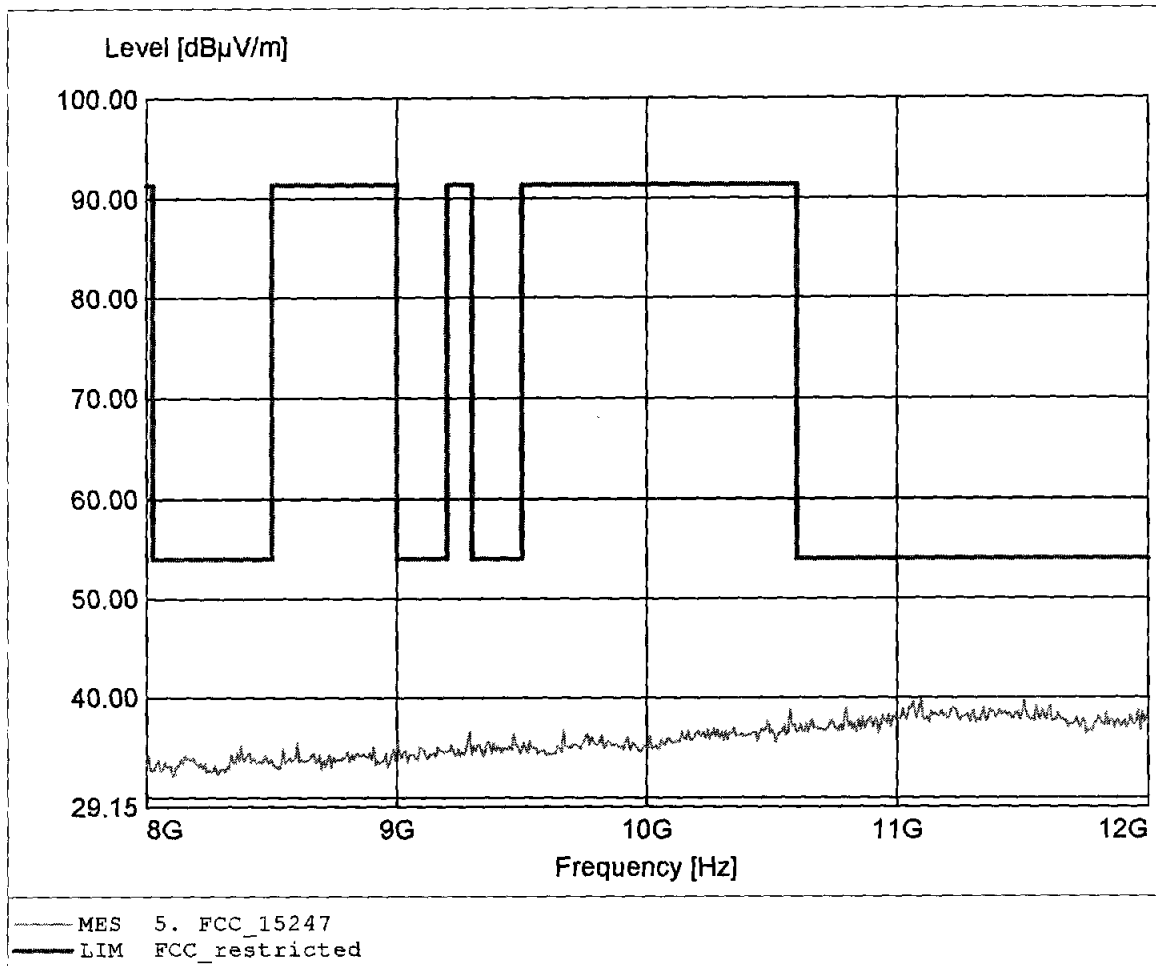

Spurious emissions Field Strength

FCC RULES PART 15, SUBPART C


Approval Holder: RTX Healthcare A/S
EUT: RTX3370 Monitor
Model: RTX3370 / 2441 MHz
Test Site / Operator: ETS / Mr. Meng
Test Condition: 25°C / Unom: 6.0 V DC
Test Specification: according to §15.247, peak detector
Comment 1: Dist.: 3m, Ant.: BBHA9120D, ampl.+HP.
Comment 2: Freq: 11.423GHz, Emax: 39.61dBµV/m, RBW: 1MHz

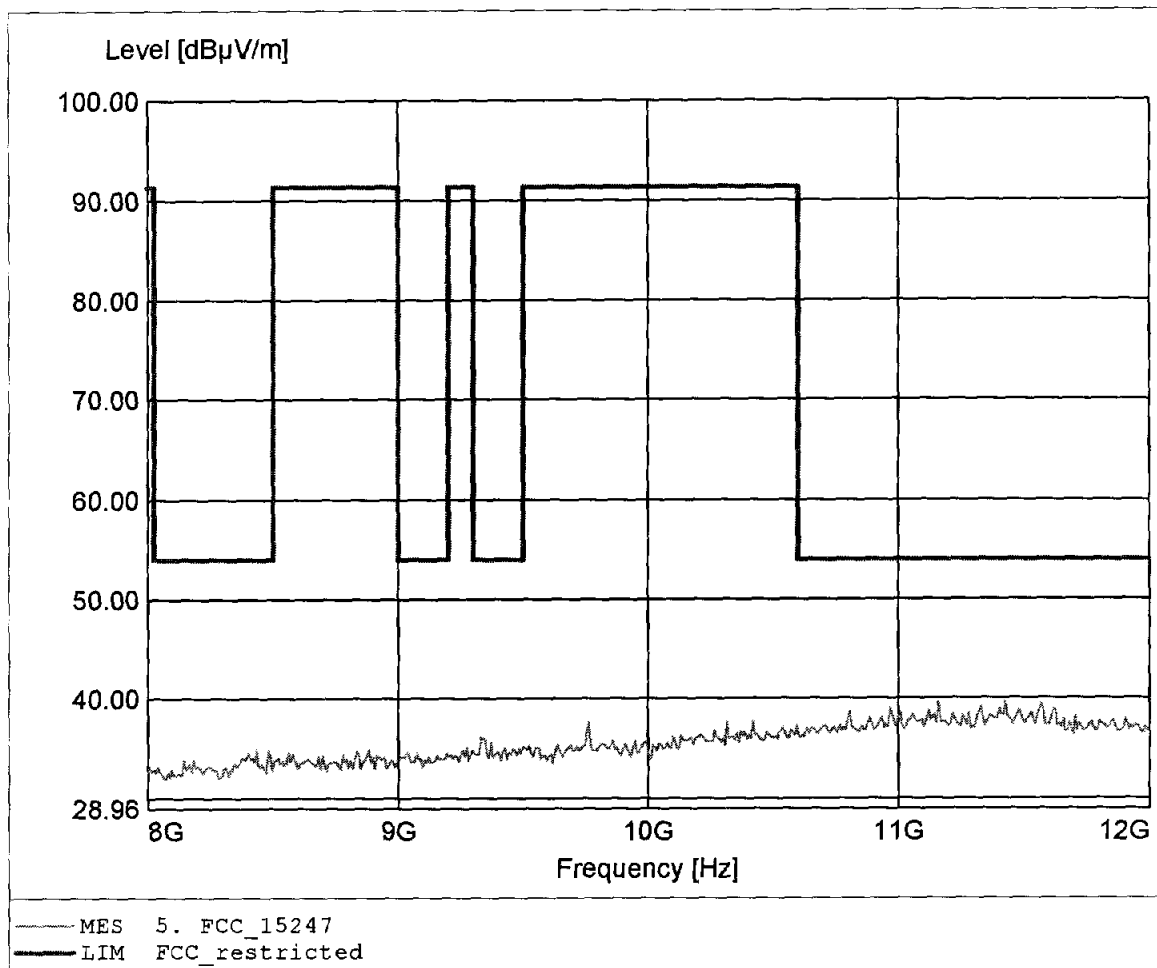

Spurious emissions Field Strength

FCC RULES PART 15, SUBPART C


Approval Holder: RTX Healthcare A/S
EUT: RTX3370 Monitor
Model: RTX3370 / 2441 MHz
Test Site / Operator: ETS / Mr. Meng
Test Condition: 25°C / Unom: 6.0 V DC
Test Specification: according to S15.247, peak detector
Comment 1: Dist.: 3m, Ant.: BBHA9120D, ampl.+HP.
Comment 2: Freq: 14.535GHz, Emax: 41.75dBuV/m, RBW: 1MHz

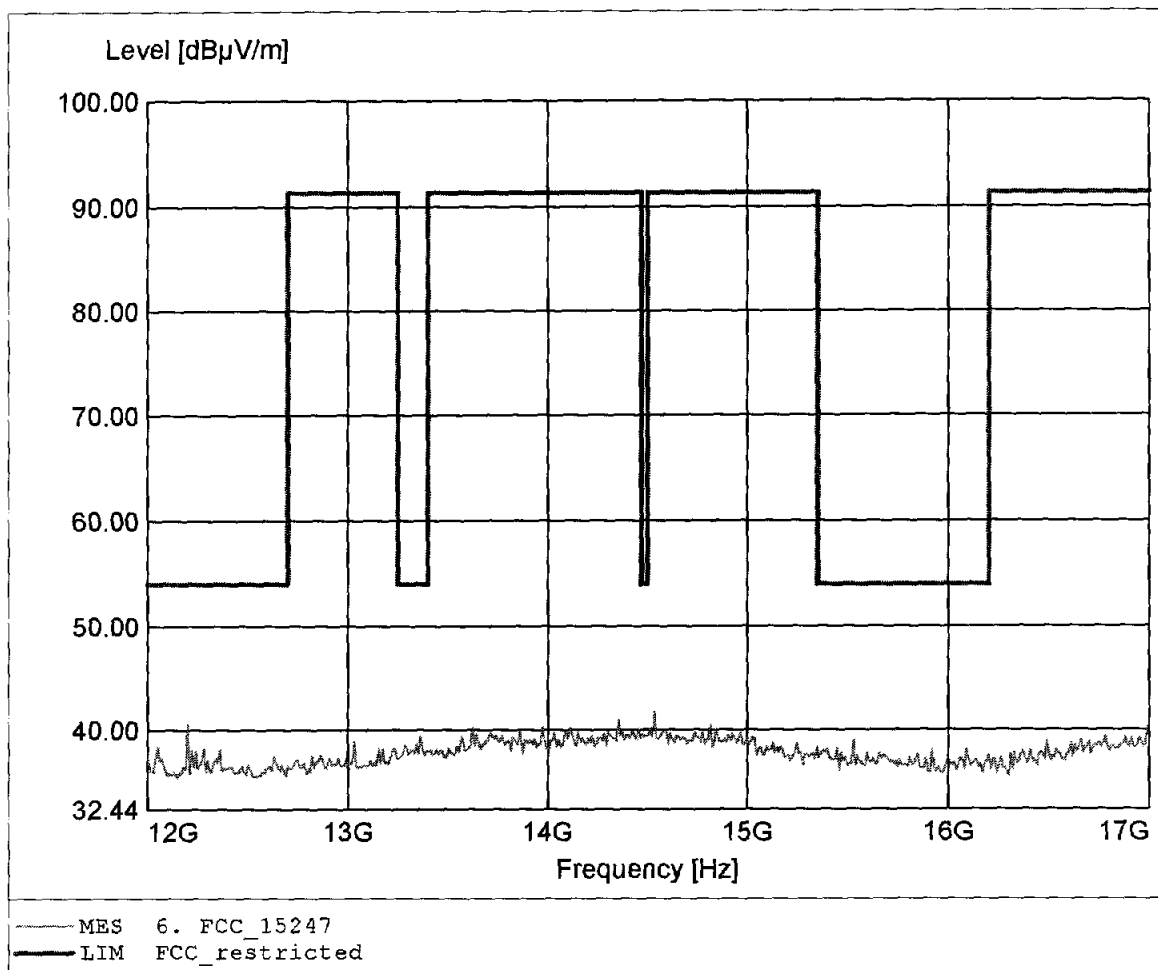

Spurious emissions Field Strength

FCC RULES PART 15, SUBPART C


Approval Holder: RTX Healthcare A/S
EUT: RTX3370 Monitor
Model: RTX3370 / 2441 MHz
Test Site / Operator: ETS / Mr. Meng
Test Condition: 25°C / Unom: 6.0 V DC
Test Specification: according to §15.247, peak detector
Comment 1: Dist.: 3m, Ant.: BBHA9120D, ampl.+HP.
Comment 2: Freq: 12.200GHz, Emax: 41.37dBμV/m, REW: 1MHz

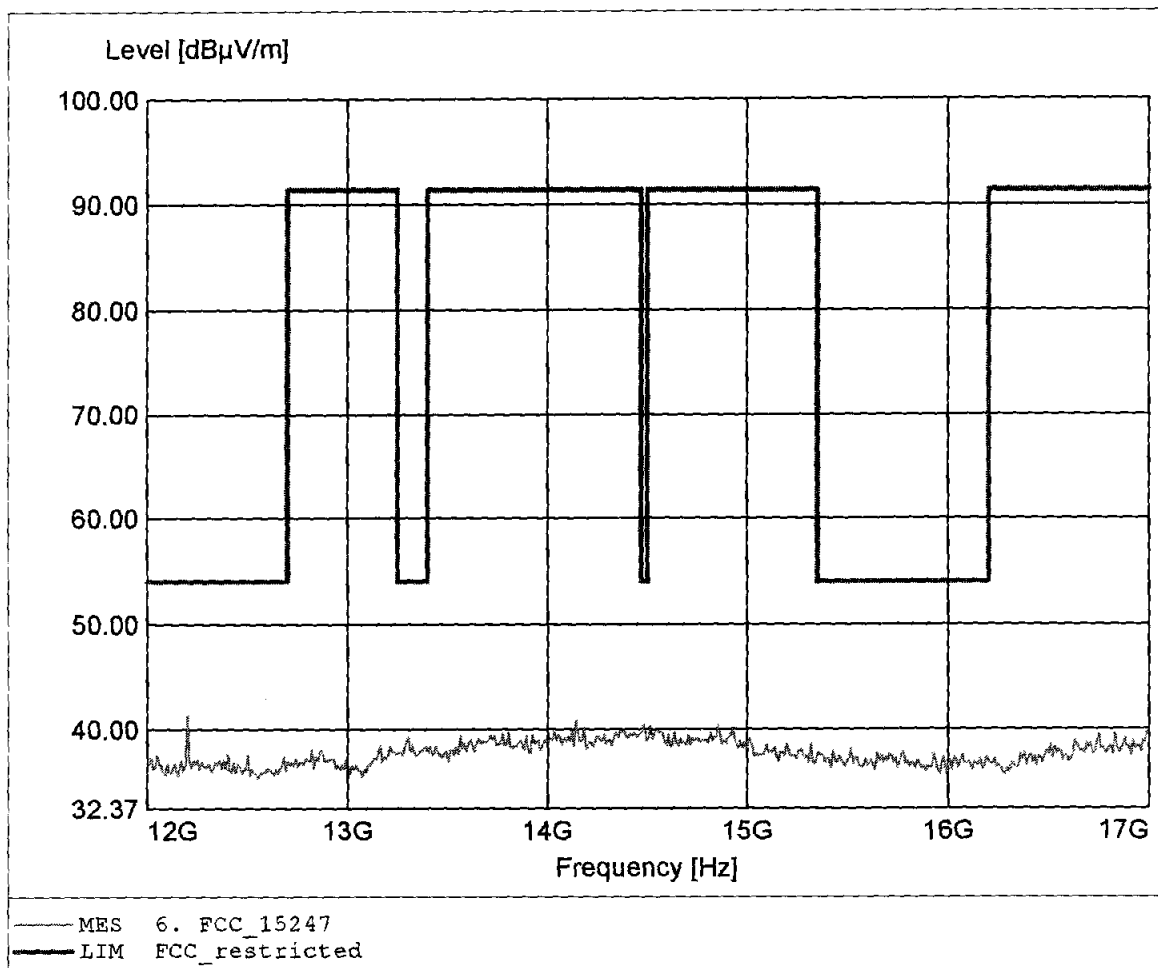

Spurious emissions Field Strength

FCC RULES PART 15, SUBPART C


Approval Holder: RTX Healthcare A/S
EUT: RTX3370 Monitor
Model: RTX3370 / 2441 MHz
Test Site / Operator: ETS / Mr. Meng
Test Condition: 25°C / Unom: 6.0 V DC
Test Specification: according to §15.247, peak detector
Comment 1: Dist.: 3m, Ant.: HL025, amplif.
Comment 2: Freq: 24.596GHz, Emax: 48.21dBµV/m, RBW: 1MHz

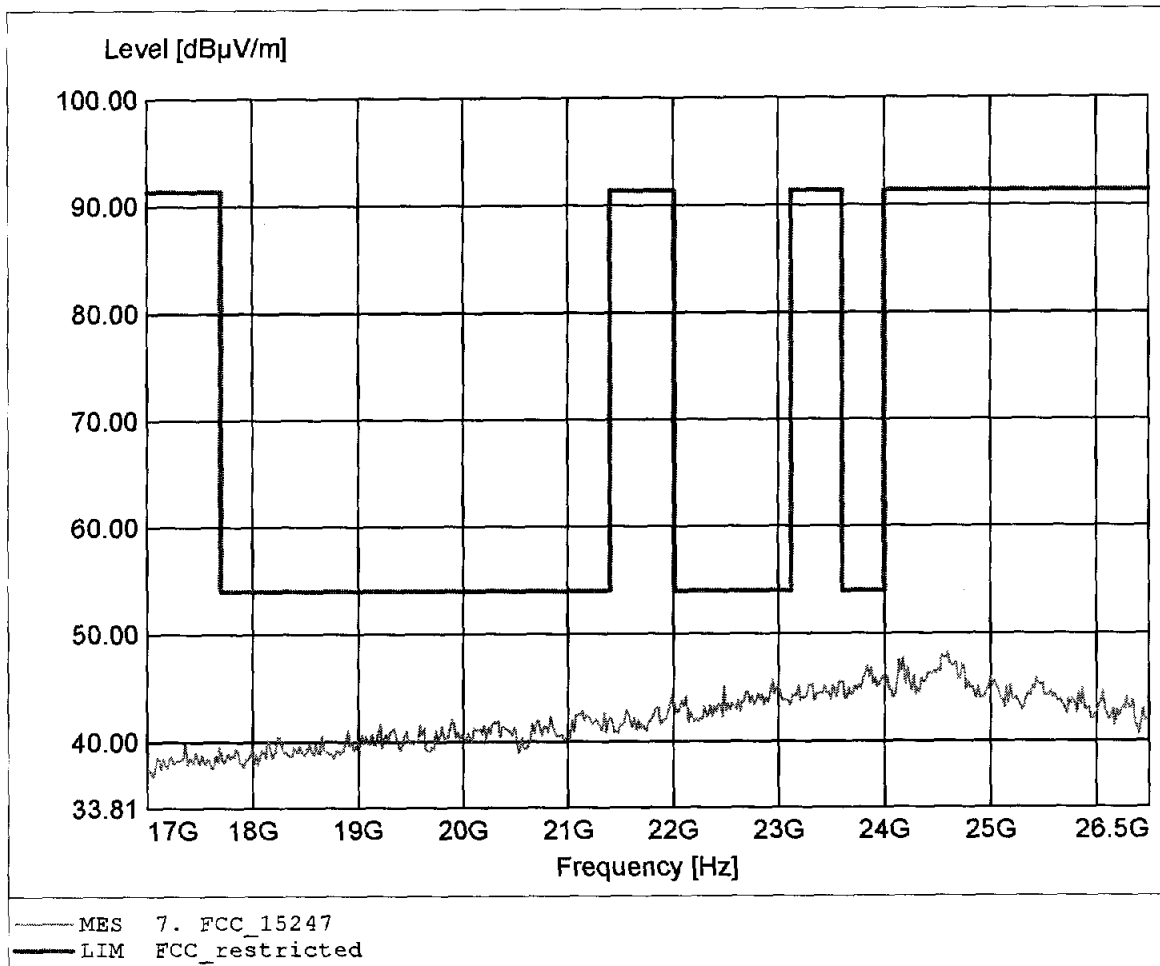

Spurious emissions Field Strength

FCC RULES PART 15, SUBPART C


Approval Holder: RTX Healthcare A/S
EUT: RTX3370 Monitor
Model: RTX3370 / 2441 MHz
Test Site / Operator: ETS / Mr. Meng
Test Condition: 25°C / Unom: 6.0 V DC
Test Specification: according to §15.247, peak detector
Comment 1: Dist.: 3m, Ant.: HL025, amplif.
Comment 2: Freq: 24.482GHz, Emax: 47.69dBµV/m, RBW: 1MHz

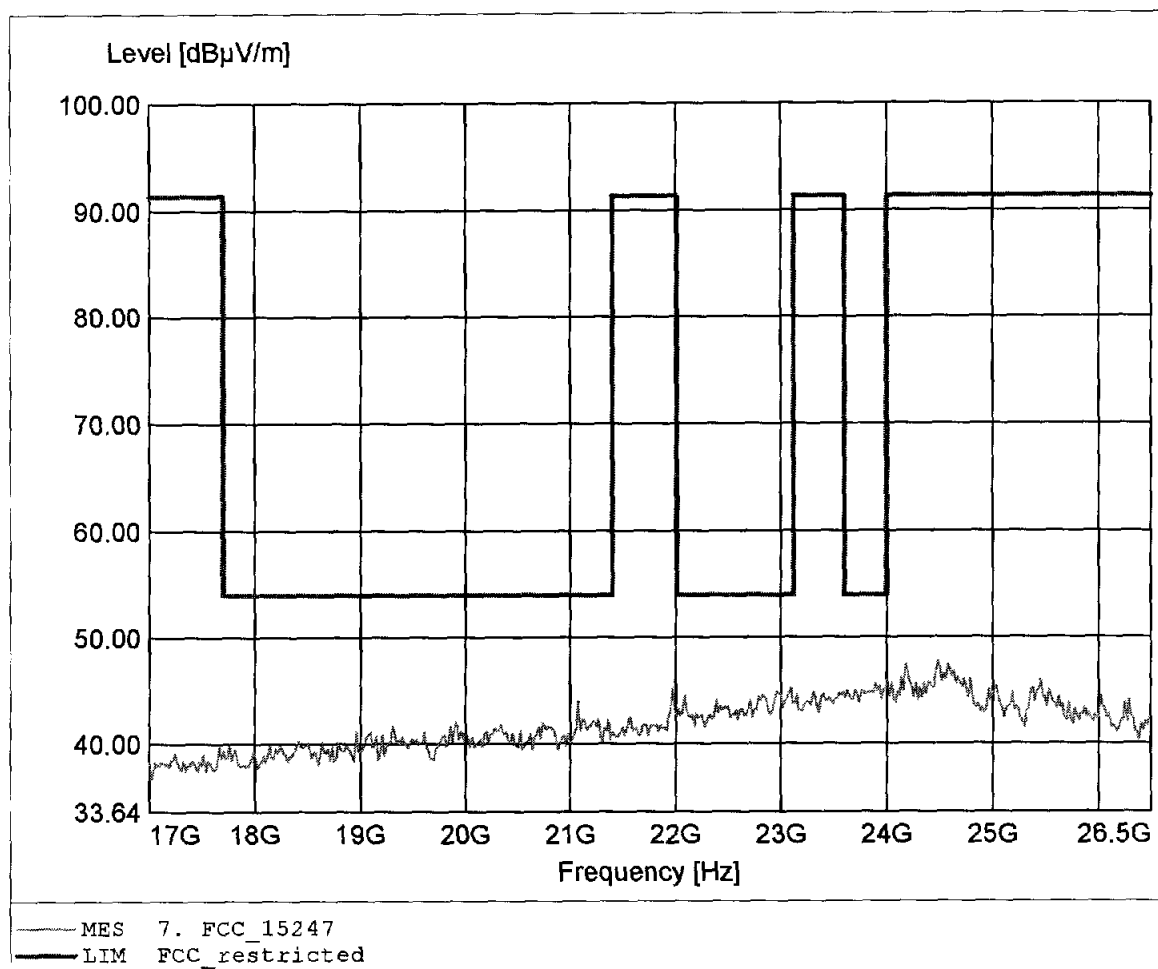

Spurious emissions Field Strength

FCC RULES PART 15, SUBPART C


Approval Holder: RTX Healthcare A/S
EUT: RTX3370 Monitor
Model: RTX3370 / 2480 MHz
Test Site / Operator: ETS / Mr. Meng
Test Condition: 25°C / Unom: 6.0 V DC
Test Specification: according to §15.247
Comment 1: Dist.: 3m, Ant.: HK 116
Comment 2: Freq: 199.319MHz, Emax: 39.27dBµV/m, REW: 100kHz

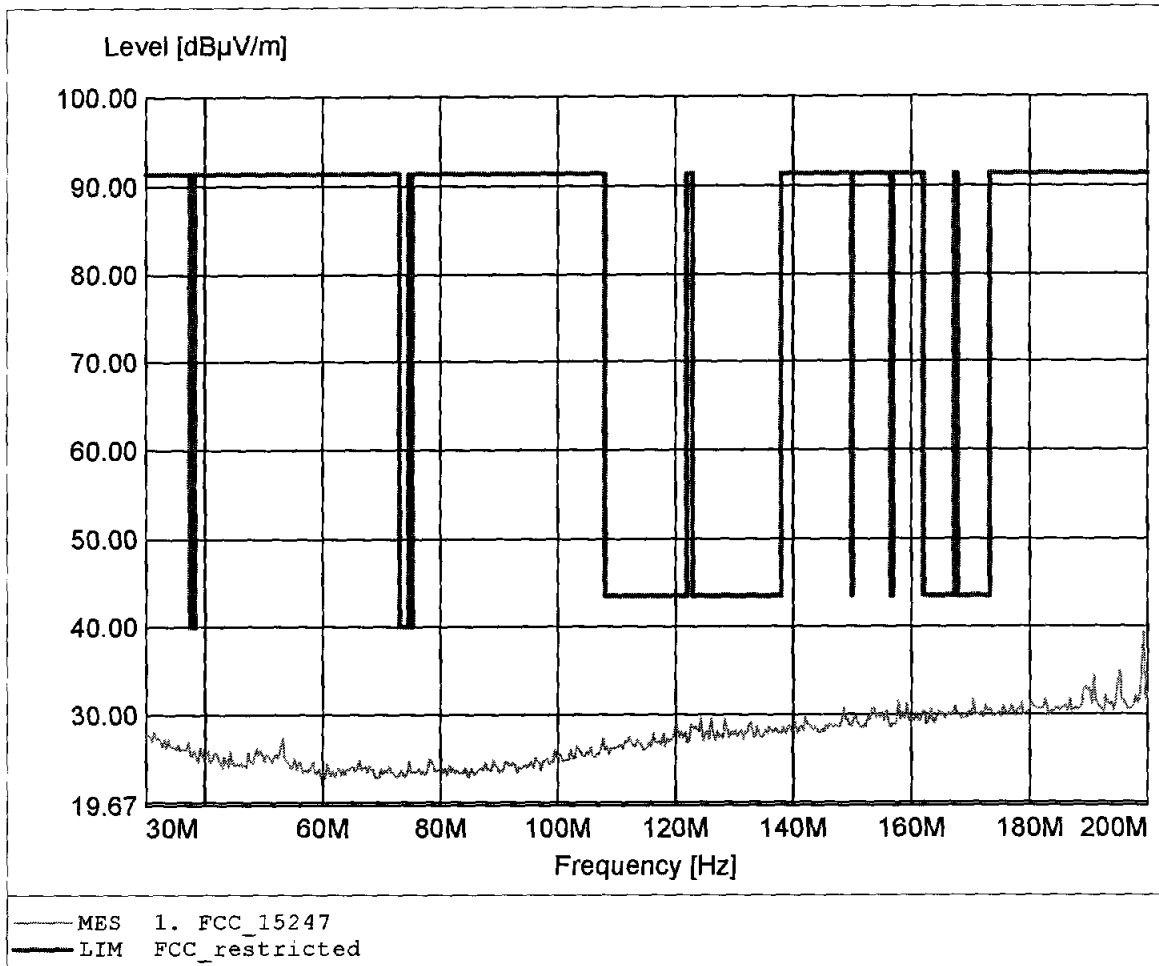

Spurious emissions Field Strength

FCC RULES PART 15, SUBPART C


Approval Holder: RTX Healthcare A/S
EUT: RTX3370 Monitor
Model: RTX3370 / 2480 MHz
Test Site / Operator: ETS / Mr. Meng
Test Condition: 25°C / Unom: 6.0 V DC
Test Specification: according to §15.247
Comment 1: Dist.: 3m, Ant.: HK 116
Comment 2: Freq: 199.319MHz, Emax: 38.26dBµV/m, RBW: 100kHz

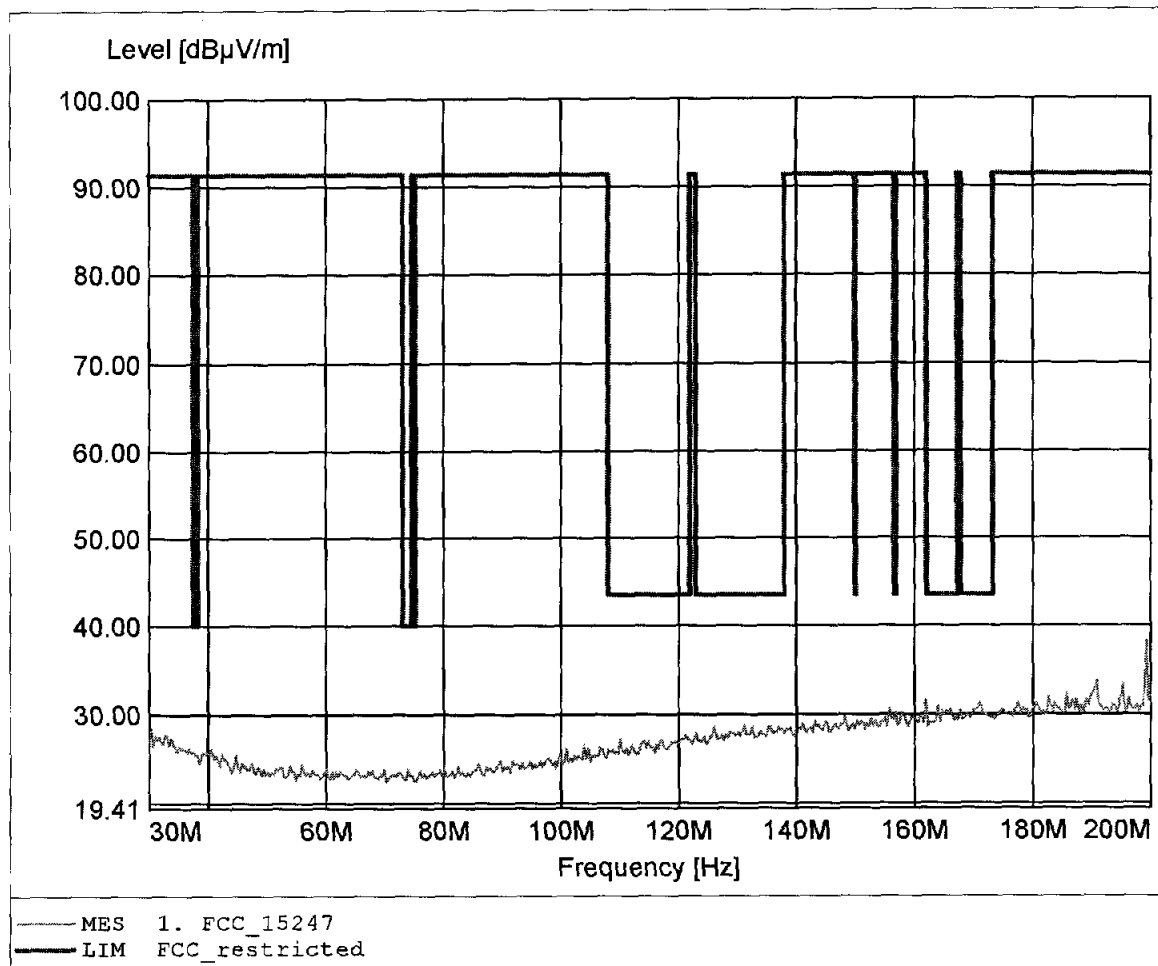

Spurious emissions Field Strength

FCC RULES PART 15, SUBPART C


Approval Holder: RTX Healthcare A/S
EUT: RTX3370 Monitor
Model: RTX3370 / 2480 MHz
Test Site / Operator: ETS / Mr. Meng
Test Condition: 25°C / Unom: 6.0 V DC
Test Specification: according to §15.247
Comment 1: Dist.: 3m, Ant.: HL 223, amplif.
Comment 2: Freq: 203.206MHz, Emax: 35.80dBµV/m, RBW: 100kHz

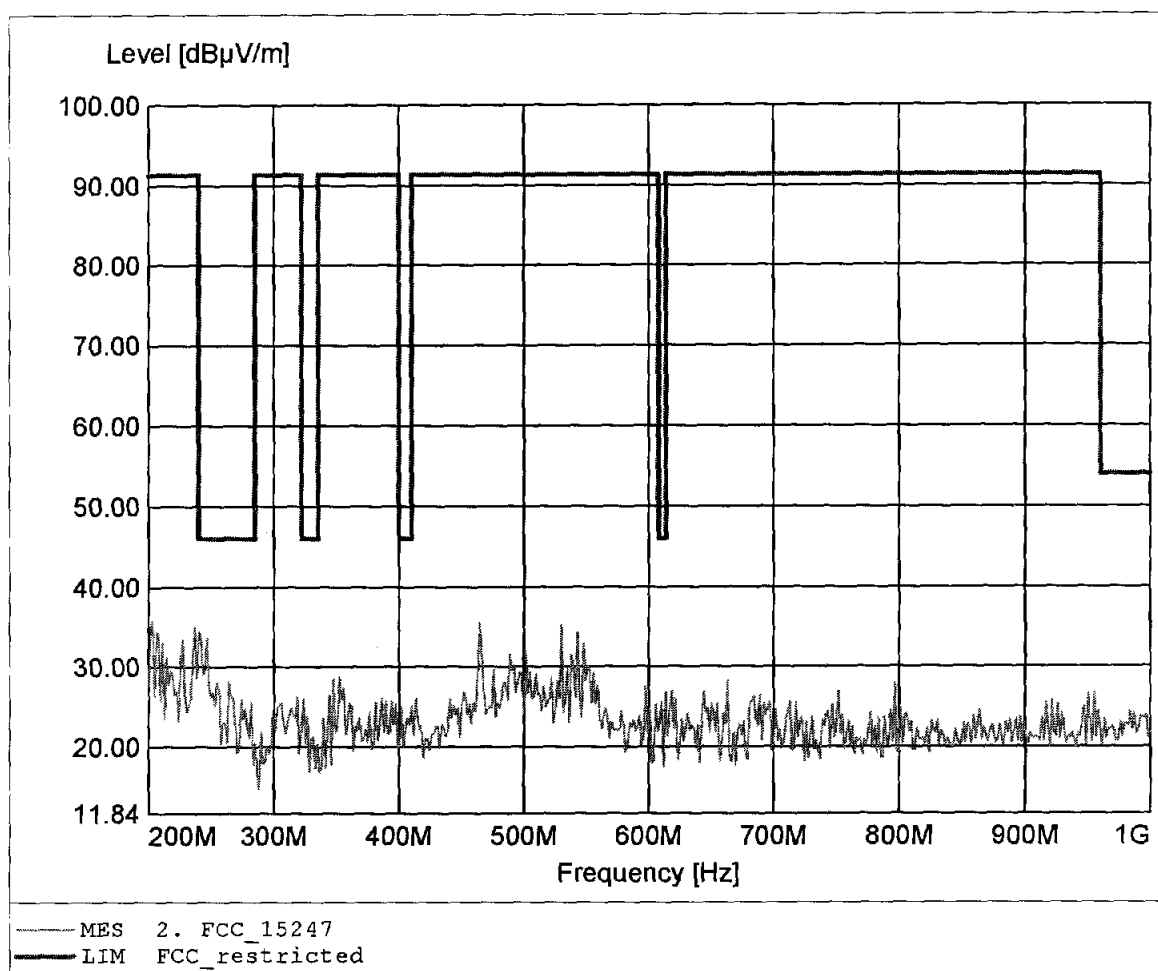

Spurious emissions Field Strength

FCC RULES PART 15, SUBPART C


Approval Holder: RTX Healthcare A/S
EUT: RTX3370 Monitor
Model: RTX3370 / 2480 MHz
Test Site / Operator: ETS / Mr. Meng
Test Condition: 25°C / Unom: 6.0 V DC
Test Specification: according to §15.247
Comment 1: Dist.: 3m, Ant.: HL 223, amplif.
Comment 2: Freq: 929.459MHz, Emax: 40.14dBµV/m, REW: 100kHz

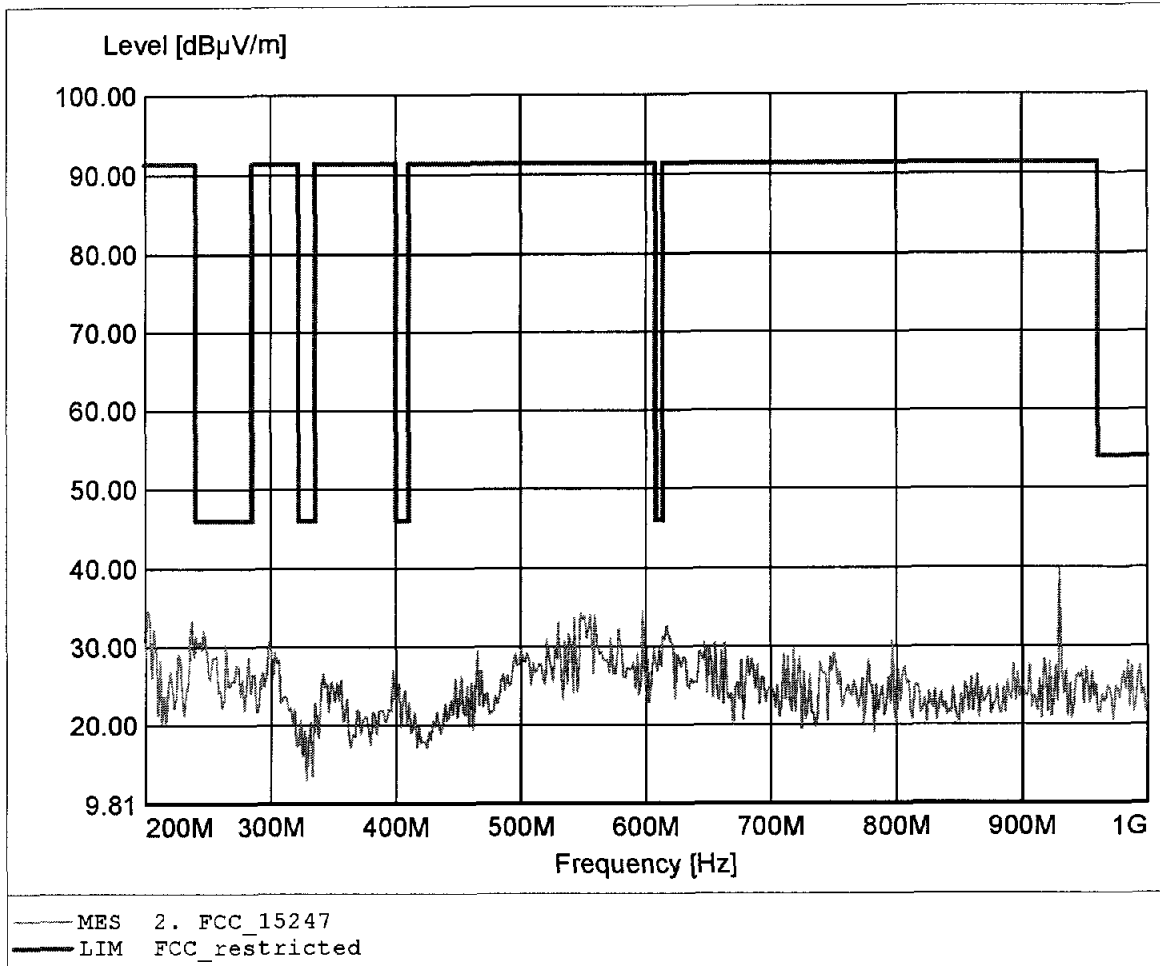

Spurious emissions Field Strength

FCC RULES PART 15, SUBPART C


Approval Holder: RTX Healthcare A/S
EUT: RTX3370 Monitor
Model: RTX3370 / 2480 MHz
Test Site / Operator: ETS / Mr. Meng
Test Condition: 25°C / Unom: 6.0 V DC
Test Specification: according to §15.247, peak detector
Comment 1: Dist.: 3m, Ant.: BBHA9120D, amplif.
Comment 2: Freq: 2.484GHz, Emax: 66.95dBµV/m, RBW: 1MHz

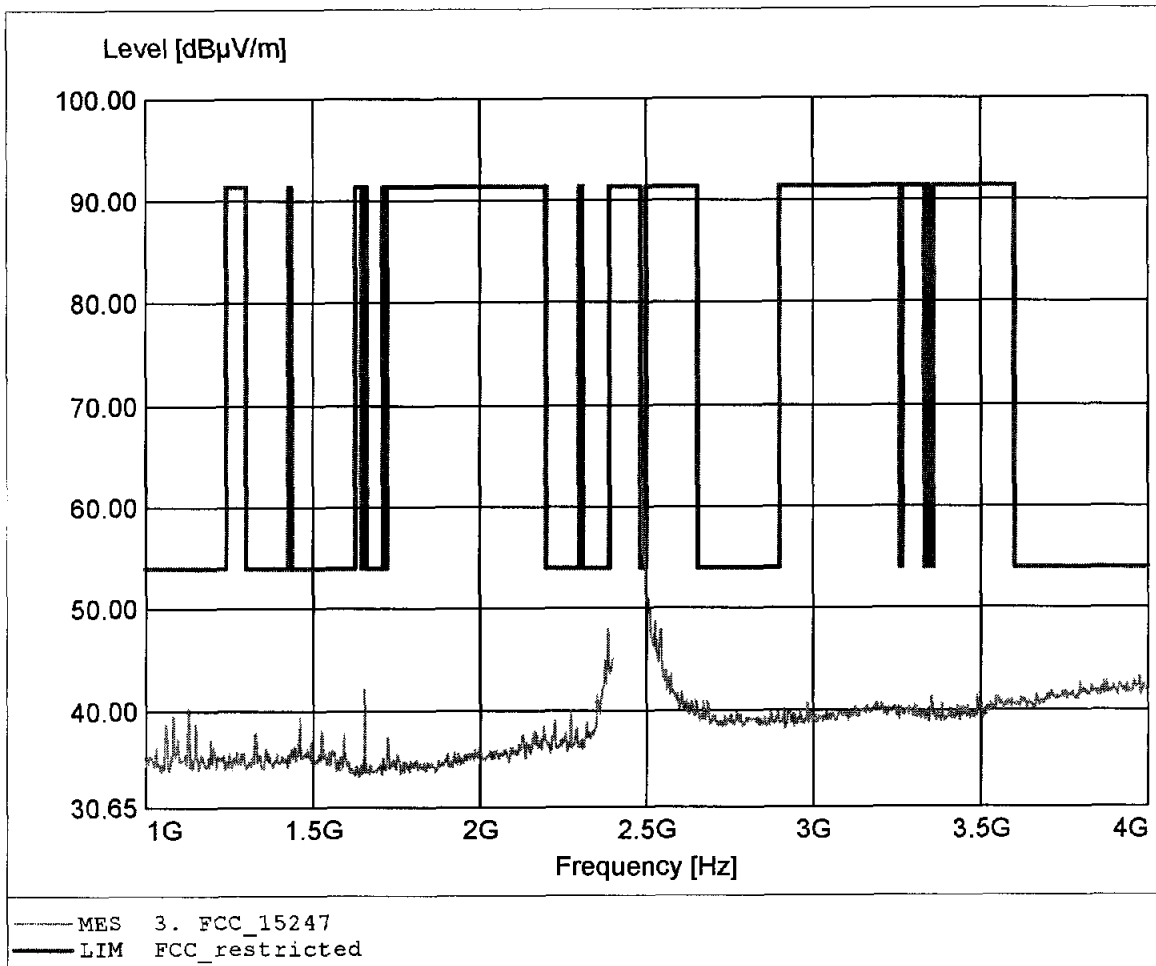

Spurious emissions Field Strength

FCC RULES PART 15, SUBPART C


Approval Holder: RTX Healthcare A/S
EUT: RTX3370 Monitor
Model: RTX3370 / 2480 MHz
Test Site / Operator: ETS / Mr. Meng
Test Condition: 25°C / Unom: 6.0 V DC
Test Specification: according to §15.247, average detector
Comment 1: Dist.: 3m, Ant.: BBHA9120D, amplif.
Comment 2: Freq: 2.484GHz, Emax: 50.46dBμV/m, RBW: 1MHz

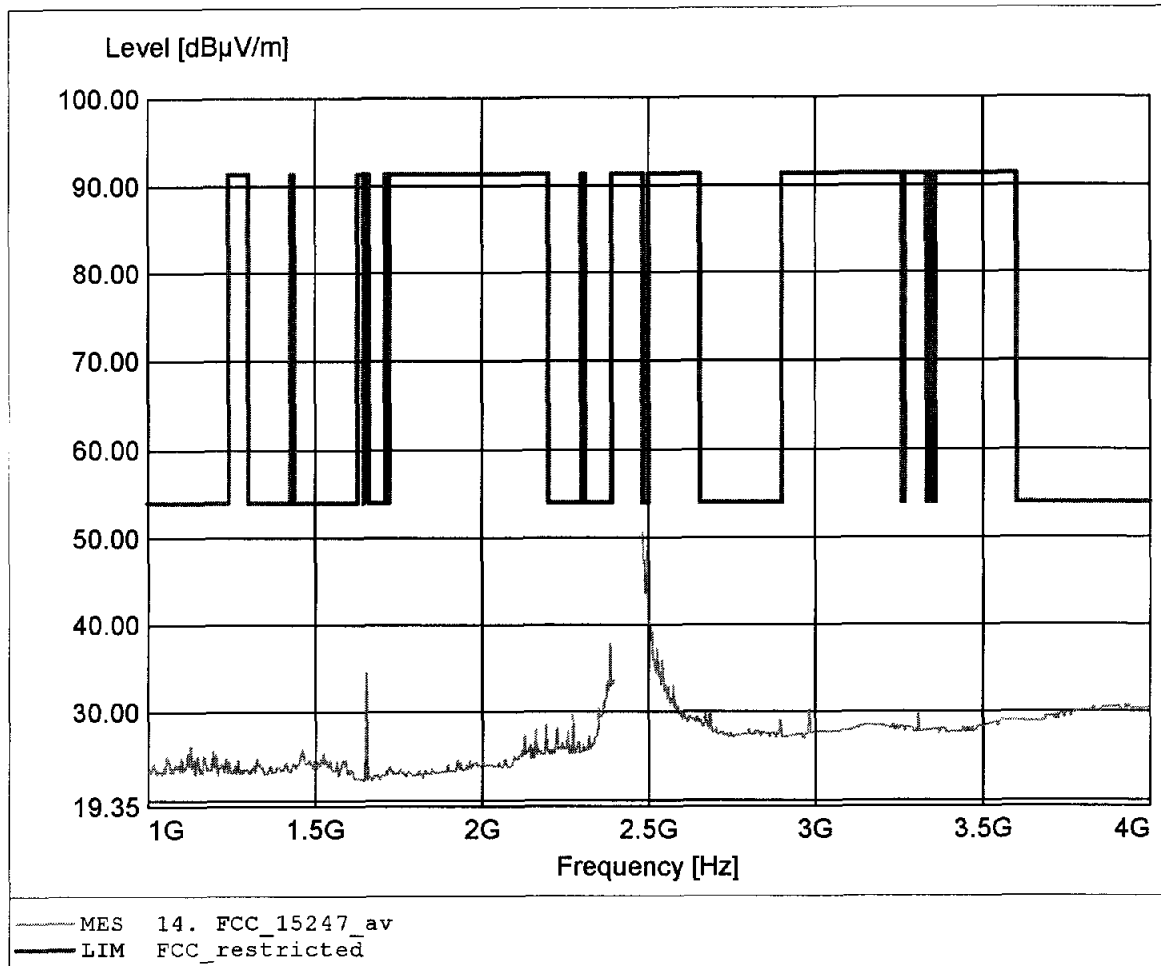

Spurious emissions Field Strength

FCC RULES PART 15, SUBPART C


Approval Holder: RTX Healthcare A/S
EUT: RTX3370 Monitor
Model: RTX3370 / 2480 MHz
Test Site / Operator: ETS / Mr. Meng
Test Condition: 25°C / Unom: 6.0 V DC
Test Specification: according to §15.247, peak detector
Comment 1: Dist.: 3m, Ant.: BBHA9120D, amplif.
Comment 2: Freq: 2.484GHz, Emax: 63.67dB μ V/m, RBW: 1MHz

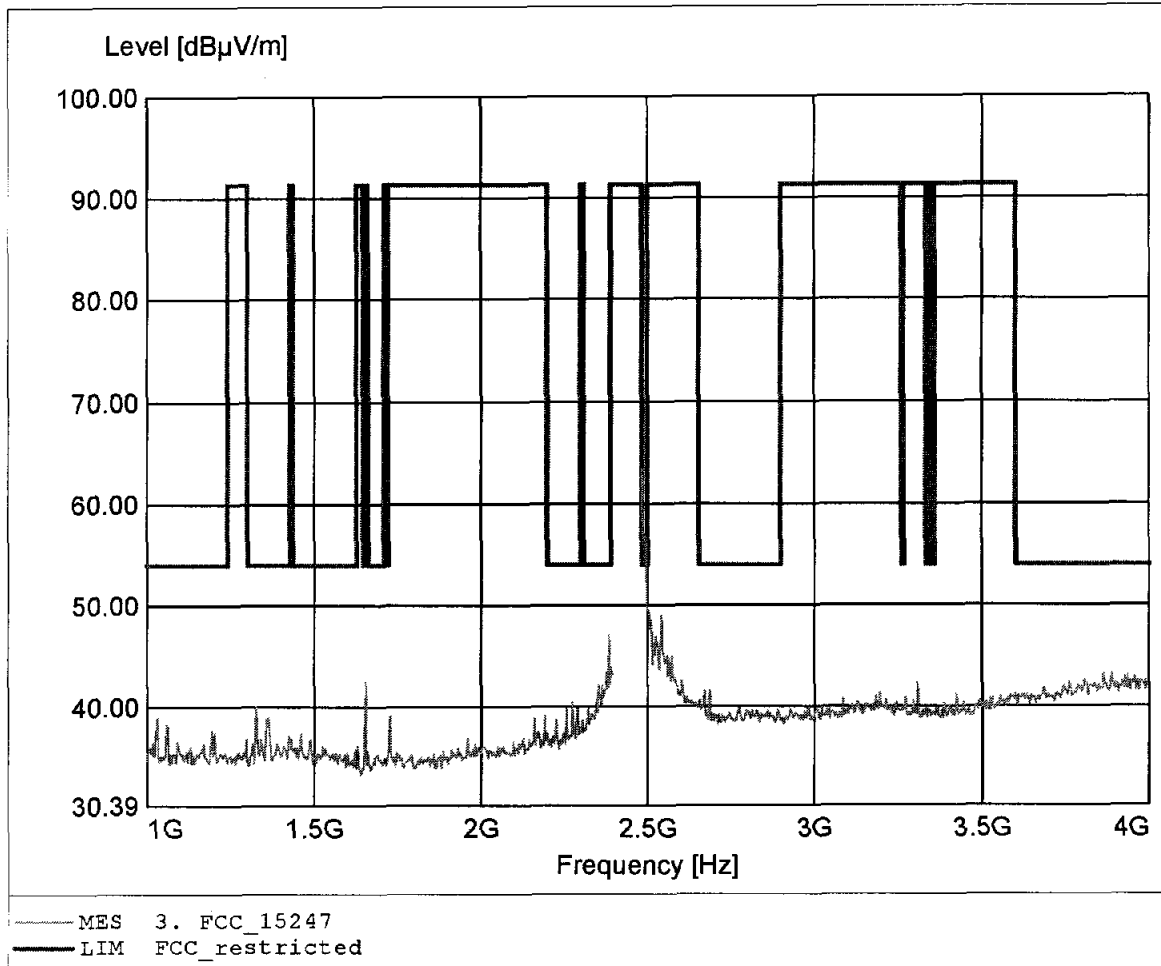

Spurious emissions Field Strength

FCC RULES PART 15, SUBPART C


Approval Holder: RTX Healthcare A/S
EUT: RTX3370 Monitor
Model: RTX3370 / 2480 MHz
Test Site / Operator: ETS / Mr. Meng
Test Condition: 25°C / Unom: 6.0 V DC
Test Specification: according to S15.247, average detector
Comment 1: Dist.: 3m, Ant.: BBHA9120D, amplif.
Comment 2: Freq: 2.484GHz, Emax: 48.56dBμV/m, RBW: 1MHz

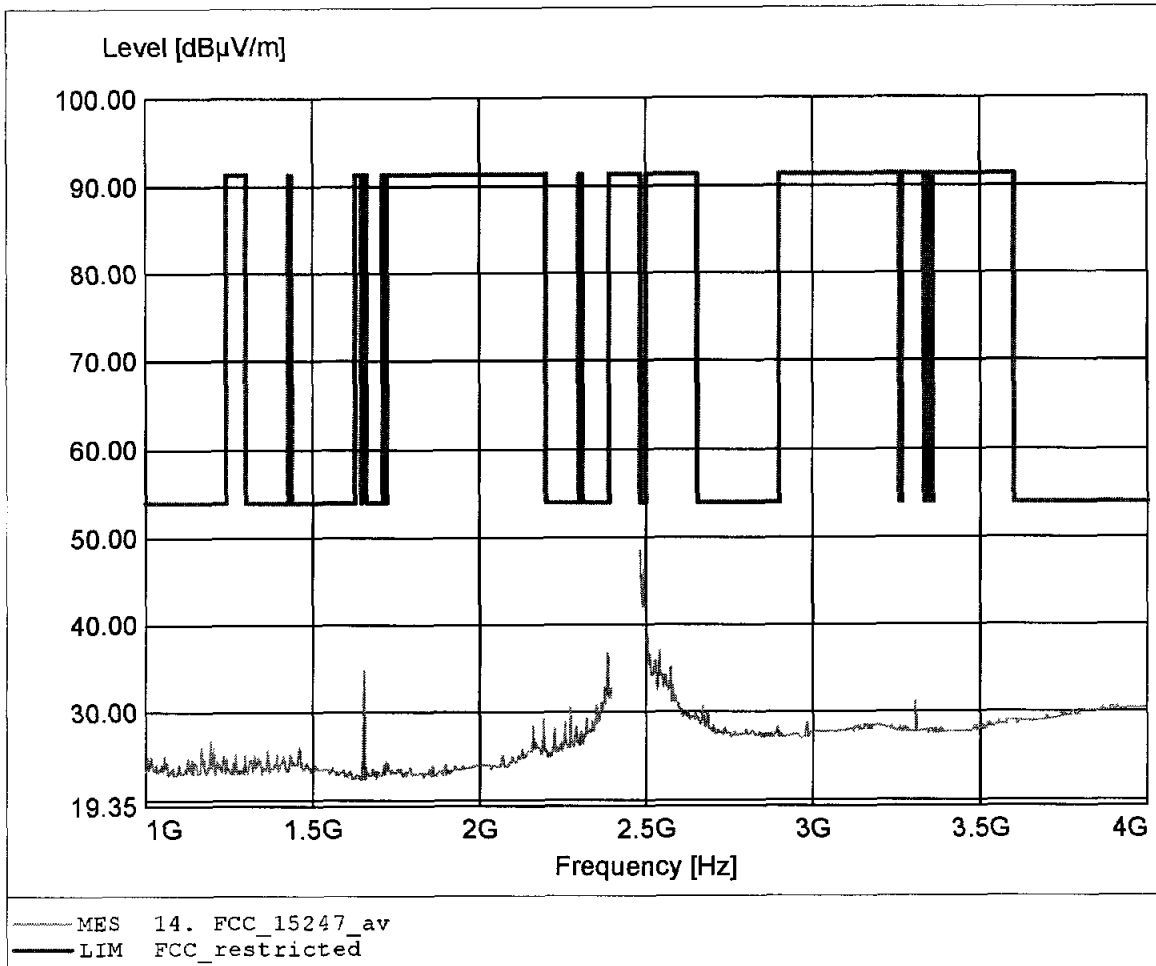

Spurious emissions Field Strength

FCC RULES PART 15, SUBPART C


Approval Holder: RTX Healthcare A/S
EUT: RTX3370 Monitor
Model: RTX3370 / 2480 MHz
Test Site / Operator: ETS / Mr. Meng
Test Condition: 25°C / Unom: 6.0 V DC
Test Specification: according to §15.247, peak detector
Comment 1: Dist.: 3m, Ant.: BBHA9120D, ampl.+HP.
Comment 2: Freq: 6.950GHz, Emax: 45.67dBμV/m, RBW: 1MHz

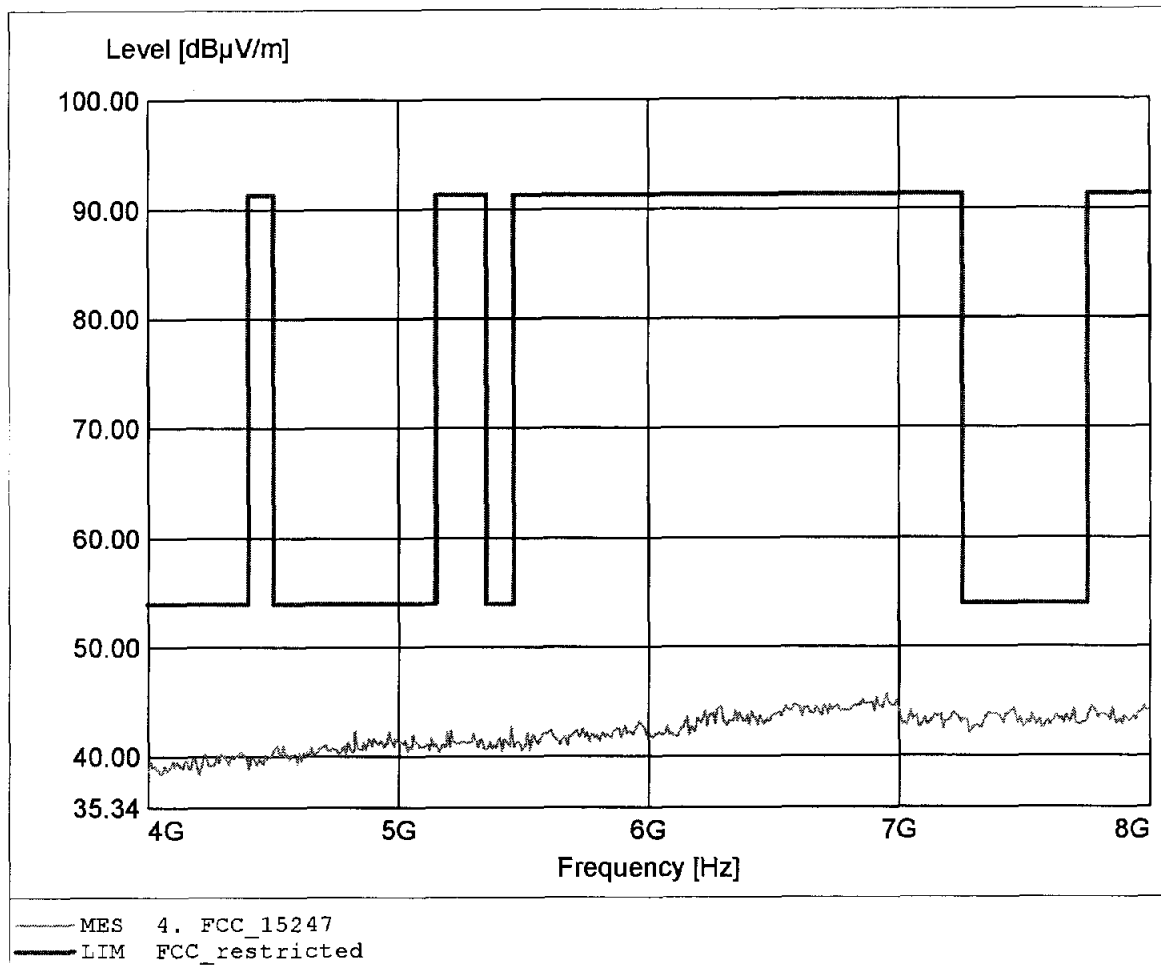

Spurious emissions Field Strength

FCC RULES PART 15, SUBPART C


Approval Holder: RTX Healthcare A/S
EUT: RTX3370 Monitor
Model: RTX3370 / 2480 MHz
Test Site / Operator: ETS / Mr. Meng
Test Condition: 25°C / Unom: 6.0 V DC
Test Specification: according to §15.247, peak detector
Comment 1: Dist.: 3m, Ant.: BBHA9120D, ampl.+HP.
Comment 2: Freq: 6.990GHz, Emax: 46.51dBµV/m, RBW: 1MHz

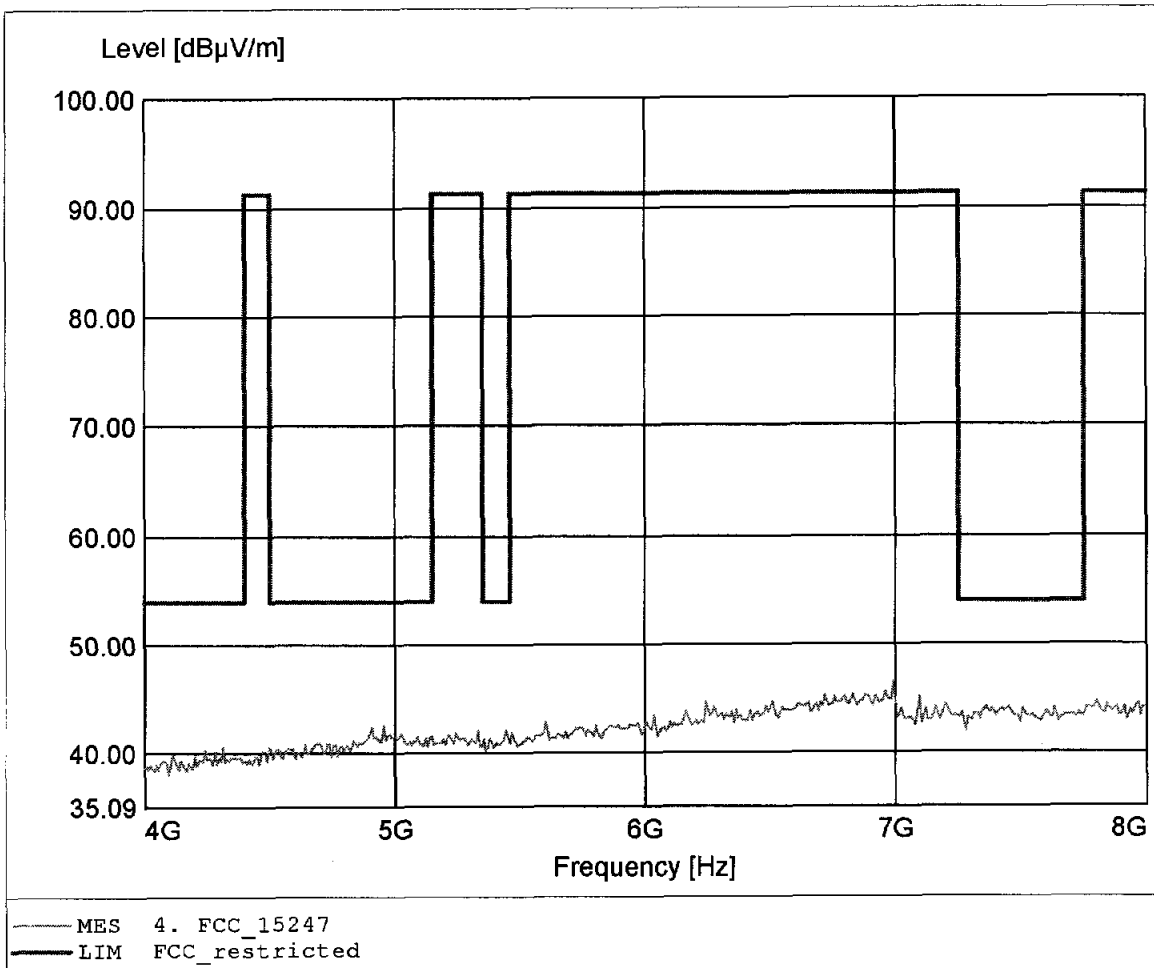

Spurious emissions Field Strength

FCC RULES PART 15, SUBPART C


Approval Holder: RTX Healthcare A/S
EUT: RTX3370 Monitor
Model: RTX3370 / 2480 MHz
Test Site / Operator: ETS / Mr. Meng
Test Condition: 25°C / Unom: 6.0 V DC
Test Specification: according to §15.247, peak detector
Comment 1: Dist.: 3m, Ant.: BBHA9120D, ampl.+HP.
Comment 2: Freq: 11.150GHz, Emax: 39.77dBµV/m, RBW: 1MHz

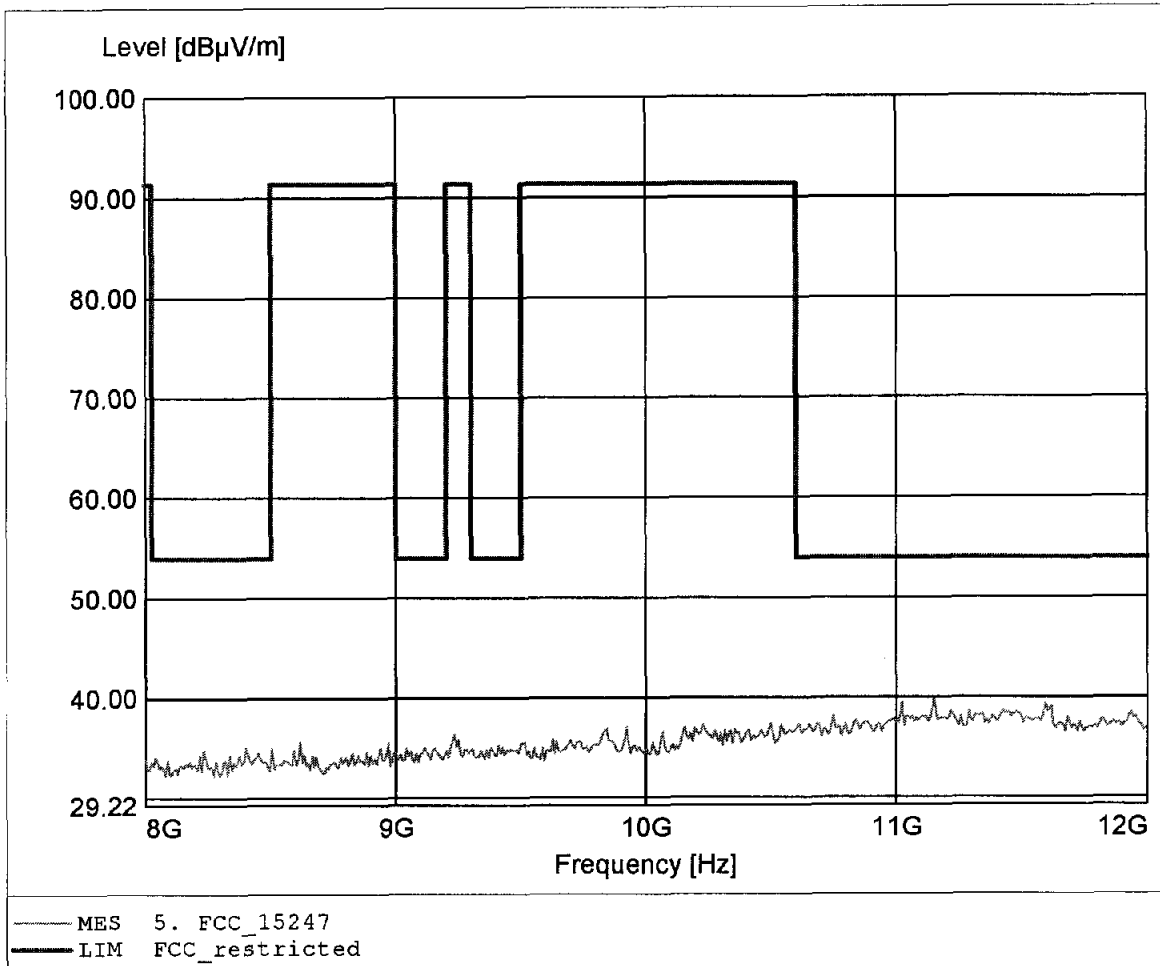

Spurious emissions Field Strength

FCC RULES PART 15, SUBPART C


Approval Holder: RTX Healthcare A/S
EUT: RTX3370 Monitor
Model: RTX3370 / 2480 MHz
Test Site / Operator: ETS / Mr. Meng
Test Condition: 25°C / Unom: 6.0 V DC
Test Specification: according to §15.247, peak detector
Comment 1: Dist.: 3m, Ant.: BBHA9120D, ampl.+HP.
Comment 2: Freq: 9.924GHz, Emax: 44.10dBµV/m, RBW: 1MHz

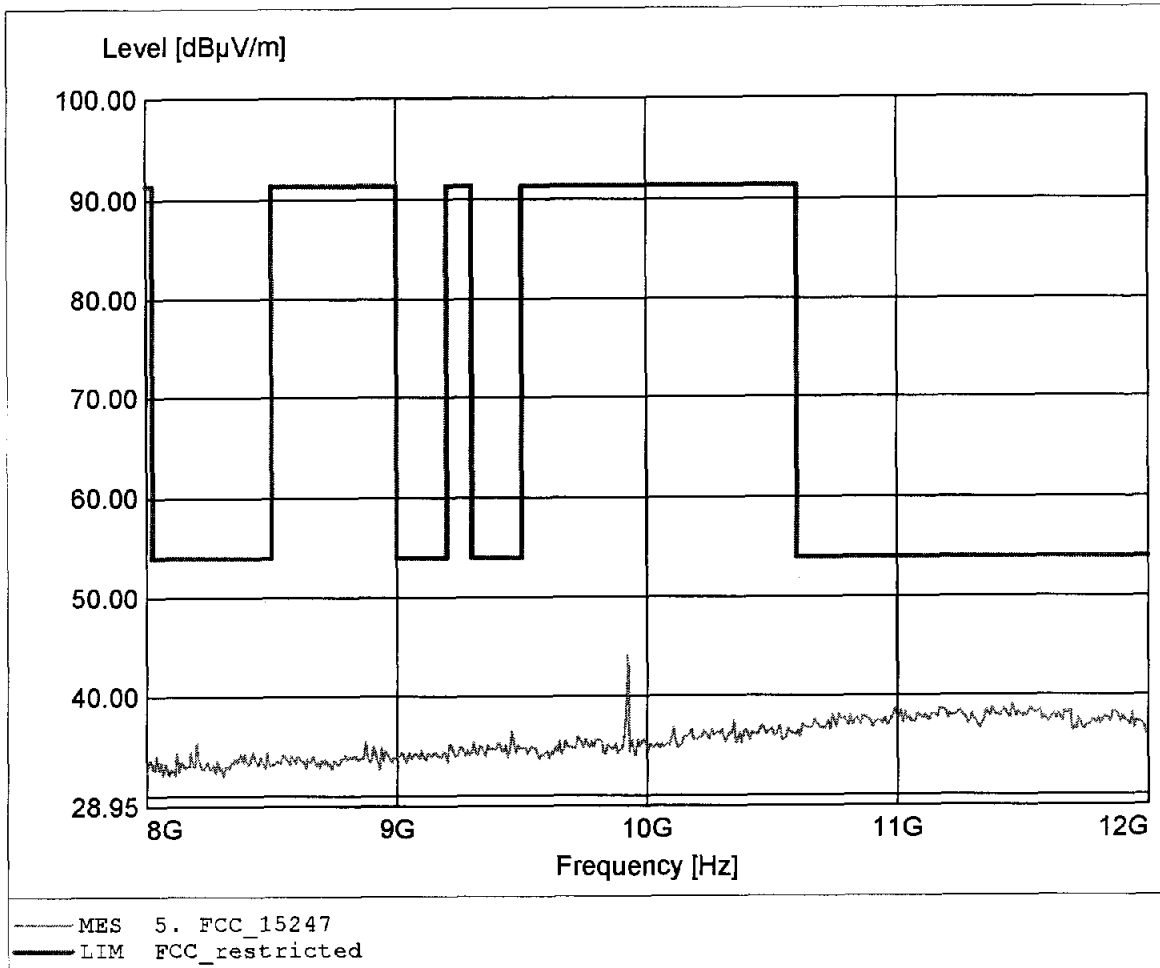

Spurious emissions Field Strength

FCC RULES PART 15, SUBPART C


Approval Holder: RTX Healthcare A/S
EUT: RTX3370 Monitor
Model: RTX3370 / 2480 MHz
Test Site / Operator: ETS / Mr. Meng
Test Condition: 25°C / Unom: 6.0 V DC
Test Specification: according to §15.247, peak detector
Comment 1: Dist.: 3m, Ant.: BBHA9120D, ampl.+HP.
Comment 2: Freq: 12.401GHz, Emax: 44.79dBµV/m, RBW: 1MHz

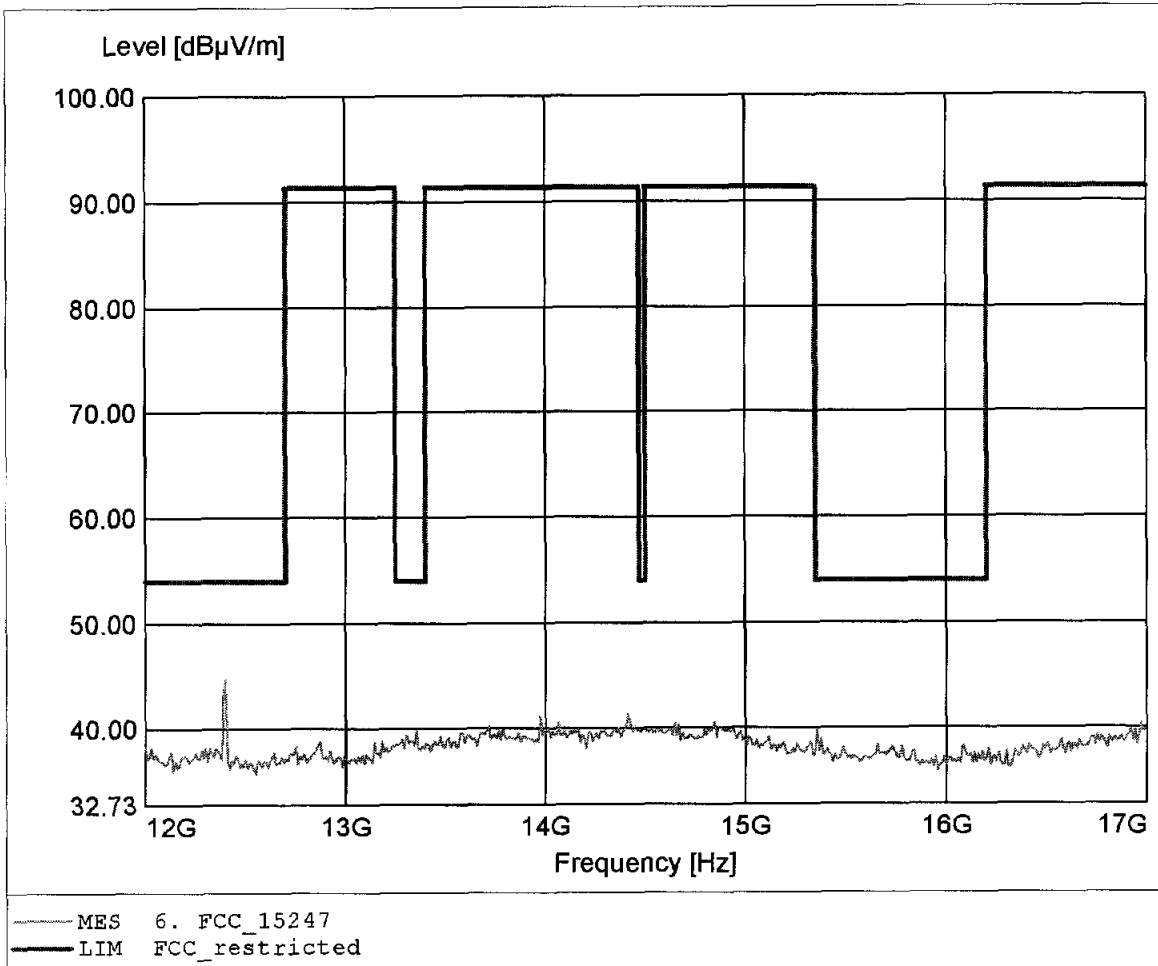

Spurious emissions Field Strength

FCC RULES PART 15, SUBPART C


Approval Holder: RTX Healthcare A/S
EUT: RTX3370 Monitor
Model: RTX3370 / 2480 MHz
Test Site / Operator: ETS / Mr. Meng
Test Condition: 25°C / Unom: 6.0 V DC
Test Specification: according to §15.247, peak detector
Comment 1: Dist.: 3m, Ant.: BBHA9120D, ampl.+HP.
Comment 2: Freq: 12.391GHz, Emax: 47.60dBµV/m, RBW: 1MHz

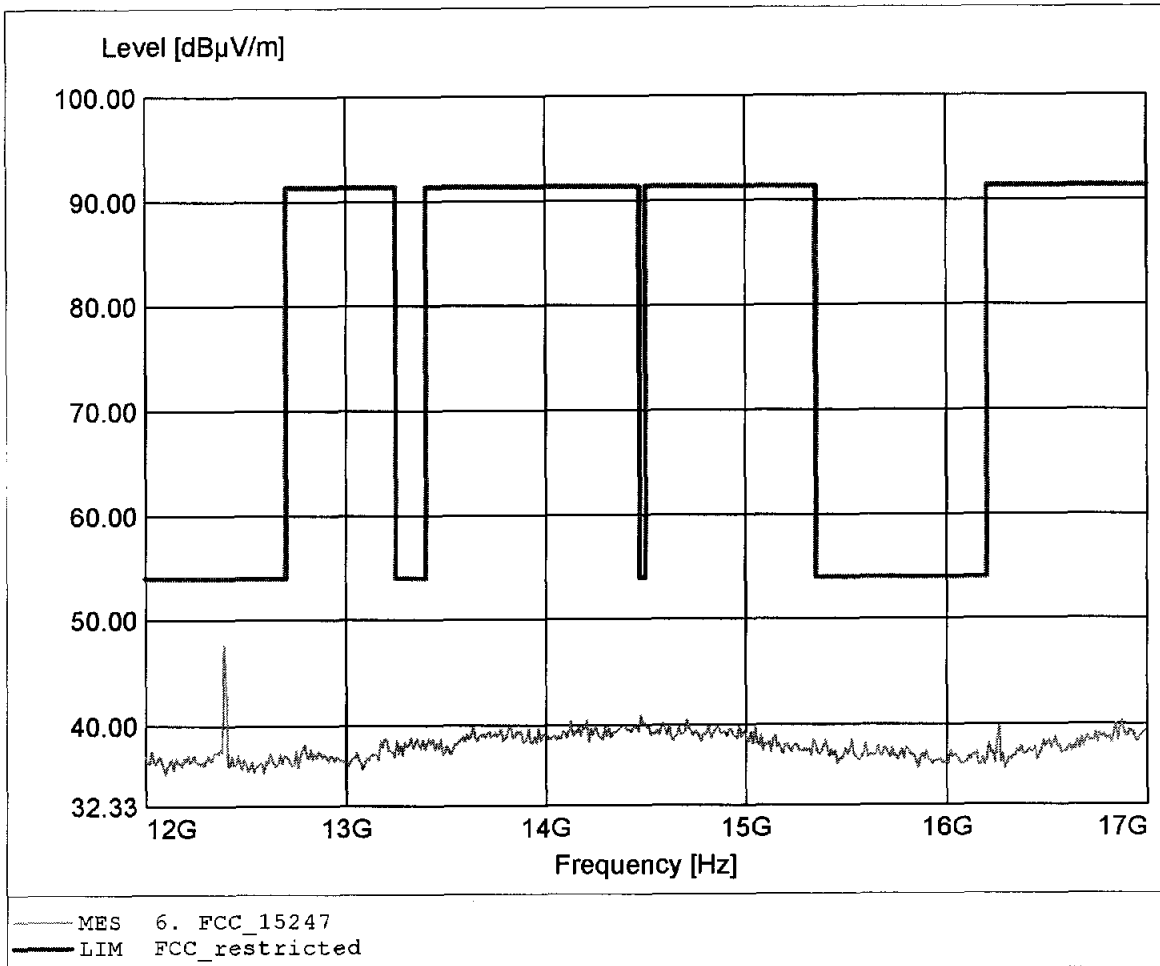

Spurious emissions Field Strength

FCC RULES PART 15, SUBPART C


Approval Holder: RTX Healthcare A/S
EUT: RTX3370 Monitor
Model: RTX3370 / 2480 MHz
Test Site / Operator: ETS / Mr. Meng
Test Condition: 25°C / Unom: 6.0 V DC
Test Specification: according to §15.247, peak detector
Comment 1: Dist.: 3m, Ant.: HL025, amplif.
Comment 2: Freq: 24.577GHz, Emax: 48.10dBµV/m, REW: 1MHz

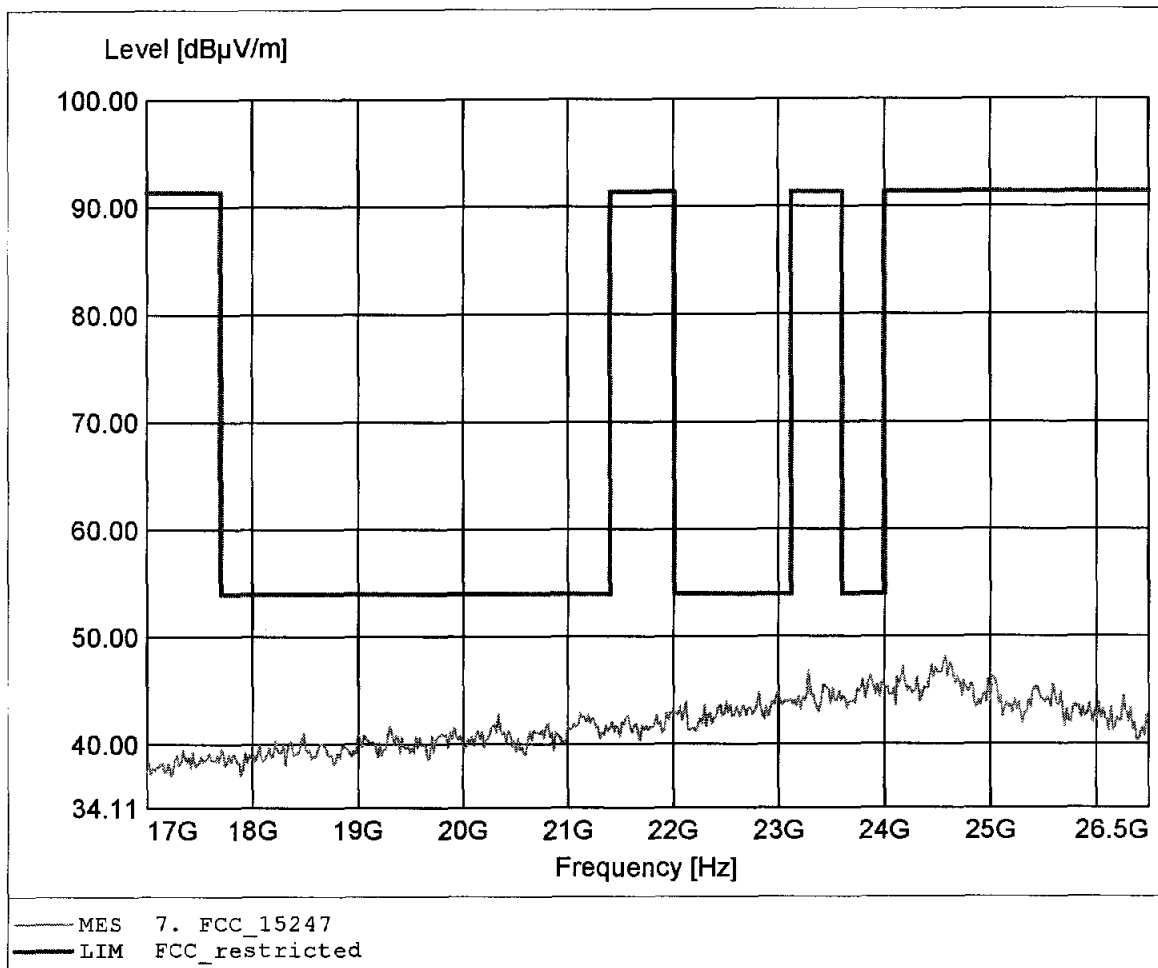

Spurious emissions Field Strength

FCC RULES PART 15, SUBPART C

Approval Holder: RTX Healthcare A/S
EUT: RTX3370 Monitor
Model: RTX3370 / 2480 MHz
Test Site / Operator: ETS / Mr. Meng
Test Condition: 25°C / Unom: 6.0 V DC
Test Specification: according to §15.247, peak detector
Comment 1: Dist.: 3m, Ant.: HL025, amplif.
Comment 2: Freq: 24.577GHz, Emax: 47.80dBµV/m, REW: 1MHz

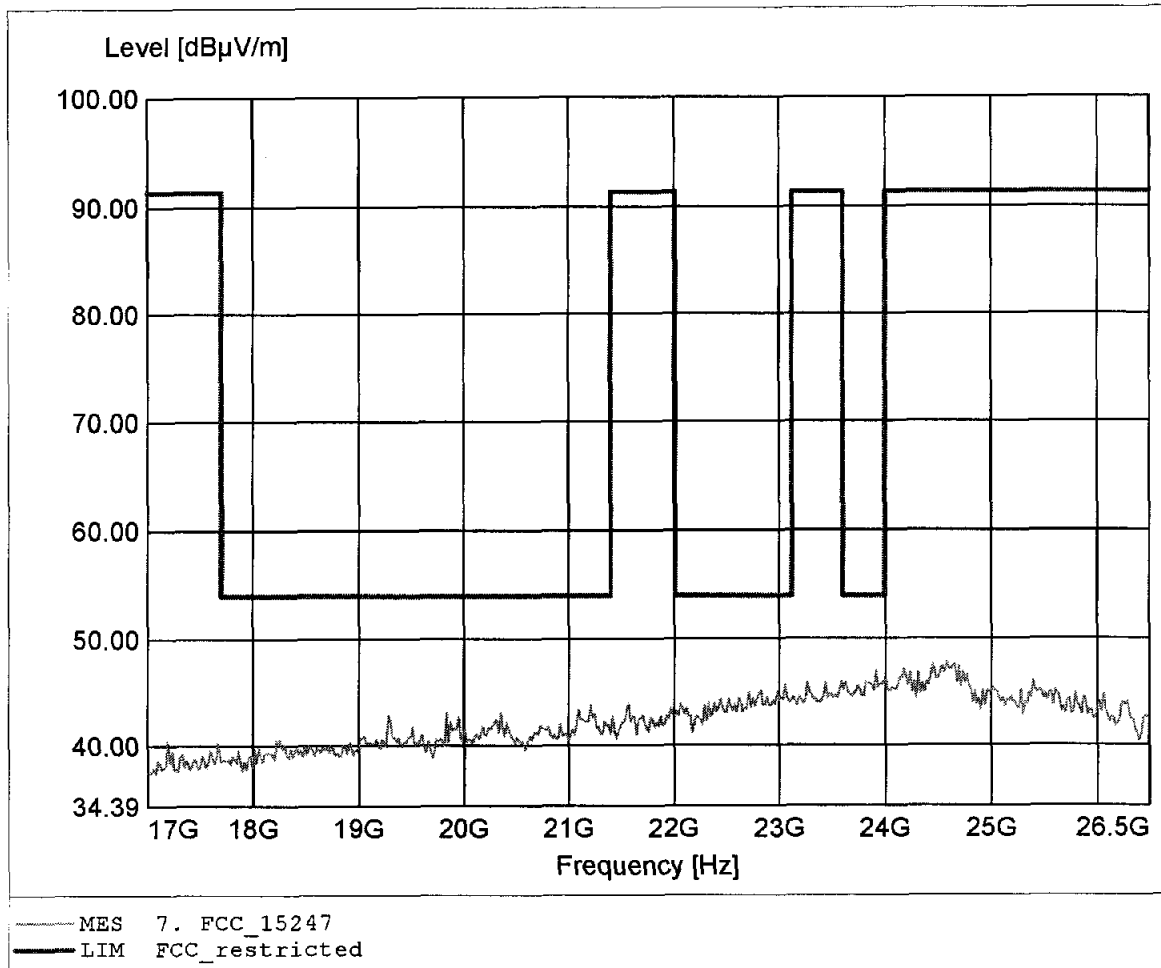


Appendix J

Band-edge compliance

FCC part 15.247
Band-edge compliance of RF conducted emissions

EUT RTX3370 Monitor
 Model RTX3370
 Approval Holder RTX Healthcare A/S
 Temperature / Voltage 25°C / Vnom
 Test Site / Operator ETS Product Service AG / Mr. Hoppe
 Test Specification FCC part 15 section 247(c)
 Comment 1 Band-edge compliance
 Comment 2 Channel.: 0 / 2402 MHz
 Comment 3 Single frequency mode

| | | | | | |
|--|--------------|-----------------|--------|--------|---------------------|
| | Delta 1 [T1] | RBW | 50 kHz | RF Att | 40 dB |
| | Ref Lvl | -52.54 dB | VBW | 50 kHz | |
| | 20 dBm | -2.18436874 MHz | SWT | 5 ms | Unit dBm |

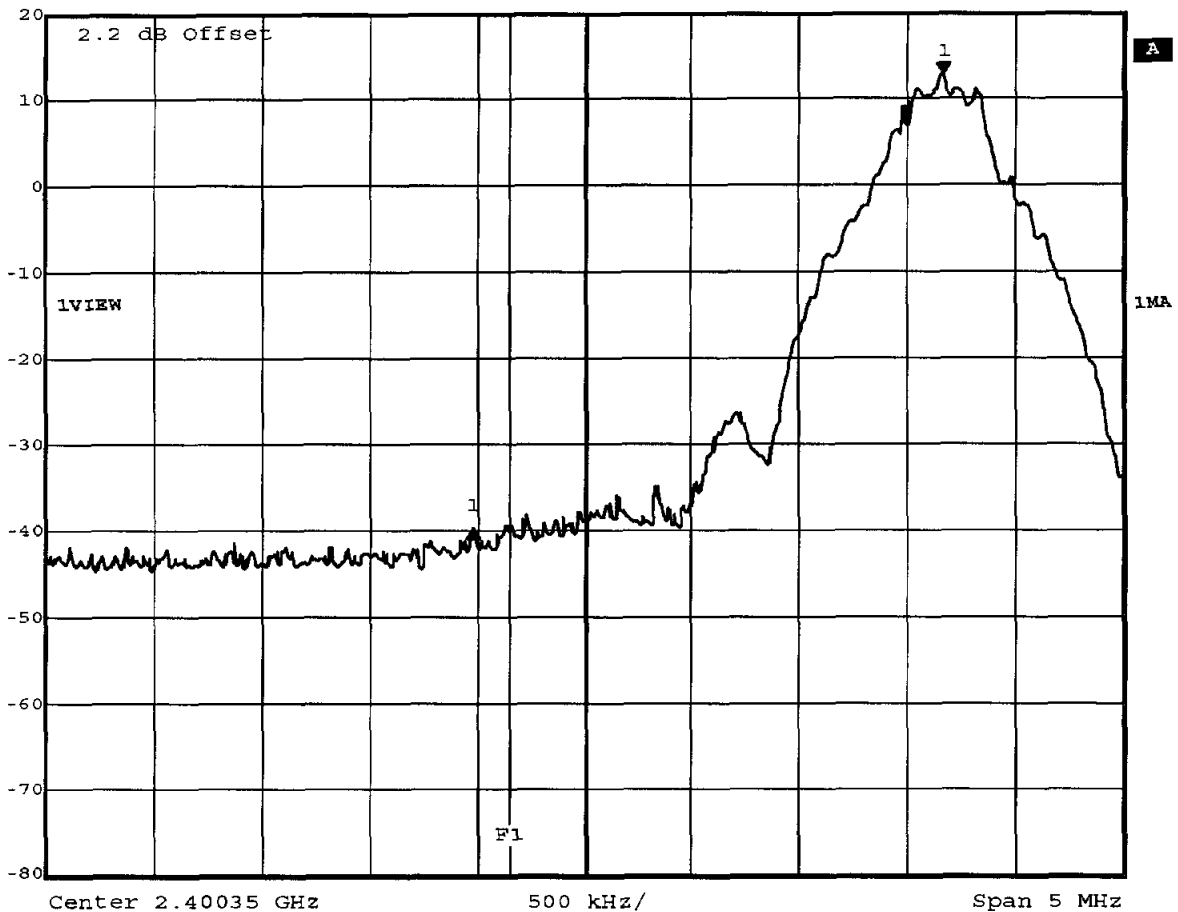


Comment A: Limit: Marker Delta value >20 dB; Result: PASS
 Date: 20.APR.2007 13:35:45

Measurement diagram

FCC part 15.247
 Band-edge compliance of RF conducted emissions

| | |
|-----------------------|------------------------------------|
| EUT | RTX3370 Monitor |
| Model | RTX3370 |
| Approval Holder | RTX Healthcare A/S |
| Temperature / Voltage | 25°C / Vnom |
| Test Site / Operator | ETS Product Service AG / Mr. Hoppe |
| Test Specification | FCC part 15 section 247(c) |
| Comment 1 | Band-edge compliance |
| Comment 2 | Channel: 78 / 2480 MHz |
| Comment 3 | Single frequency mode |

| | | | | | |
|--|--------------|----------------|--------|--------|-------|
| | Delta 1 [T1] | RBW | 50 kHz | RF Att | 40 dB |
| | Ref Lvl | -54.33 dB | VBW | 50 kHz | |
| | 20 dBm | 3.90781563 MHz | SWT | 5 ms | Unit |

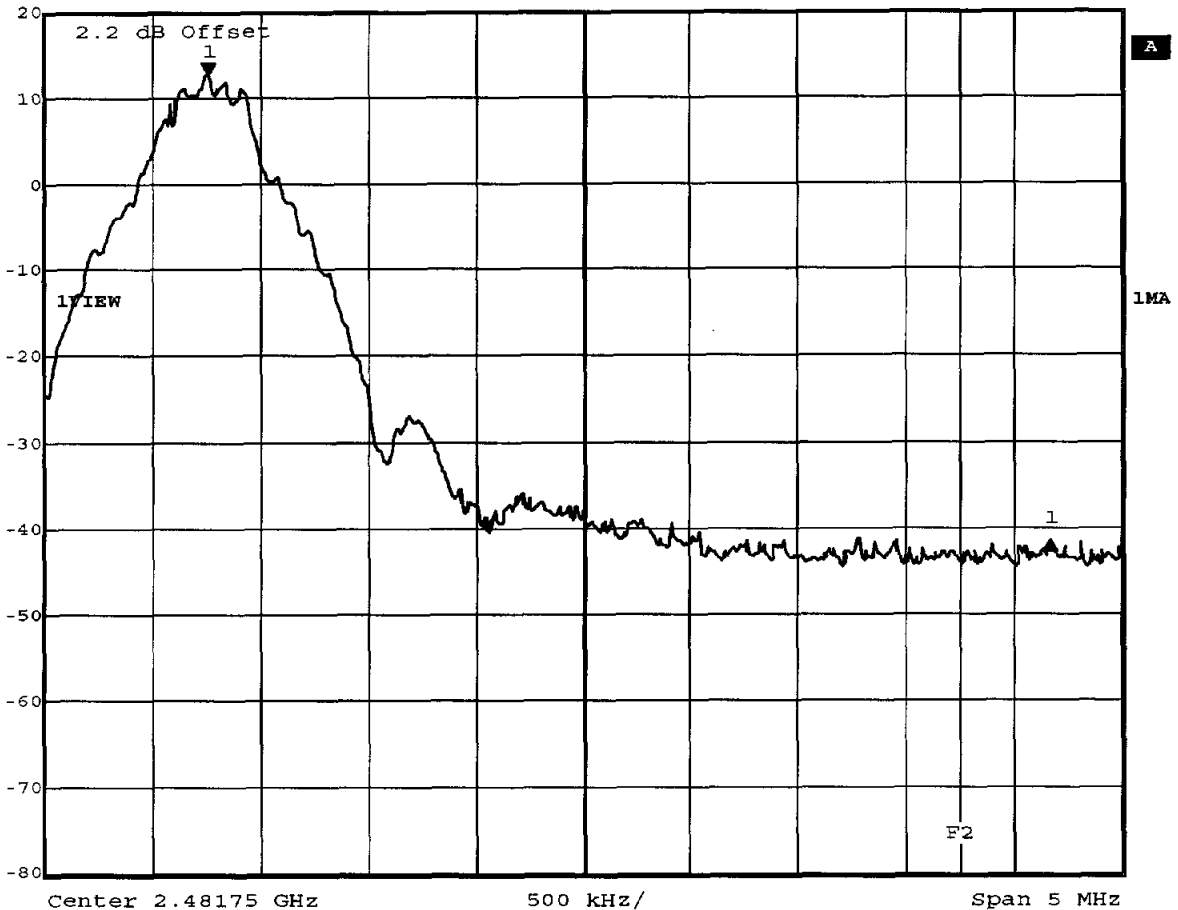


Comment A: Limit: Marker Delta value >20 dB; Result: PASS
 Date: 20.APR.2007 13:44:57

Measurement diagram

**FCC part 15.247
Band-edge compliance of RF conducted emissions**

| | |
|-----------------------|------------------------------------|
| EUT | RTX3370 Monitor |
| Model | RTX3370 |
| Approval Holder | RTX Healthcare A/S |
| Temperature / Voltage | 25°C / Vnom |
| Test Site / Operator | ETS Product Service AG / Mr. Hoppe |
| Test Specification | FCC part 15 section 247(c) |
| Comment 1 | Band-edge compliance |
| Comment 2 | Channel.: 0 / 2402 MHz |
| Comment 3 | Hopping mode |

| | | | | | |
|--|--------------|-----------------|--------|--------|-------|
| | Delta 1 [T1] | RBW | 50 kHz | RF Att | 40 dB |
| | Ref Lvl | -52.66 dB | VBW | 50 kHz | |
| | 20 dBm | -4.09819639 MHz | SWT | 5 ms | Unit |

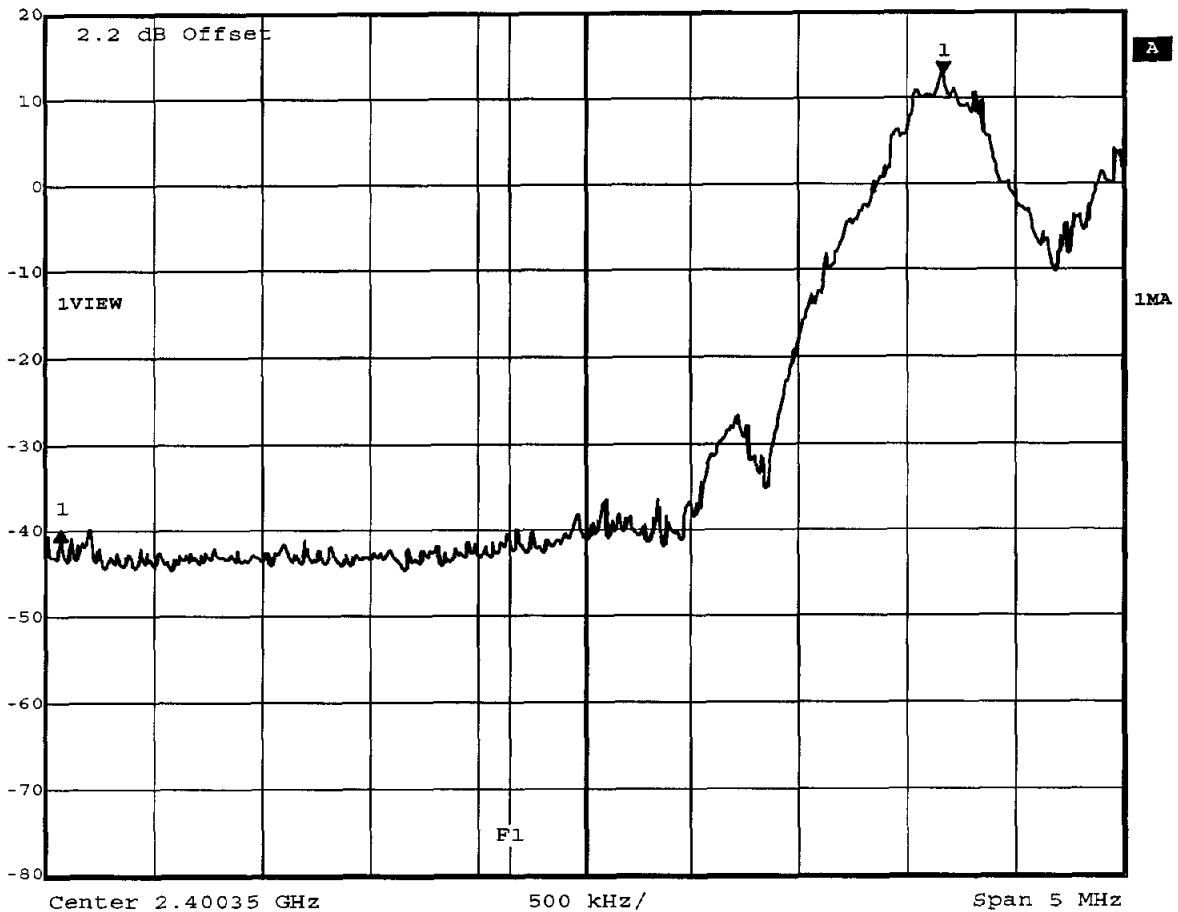


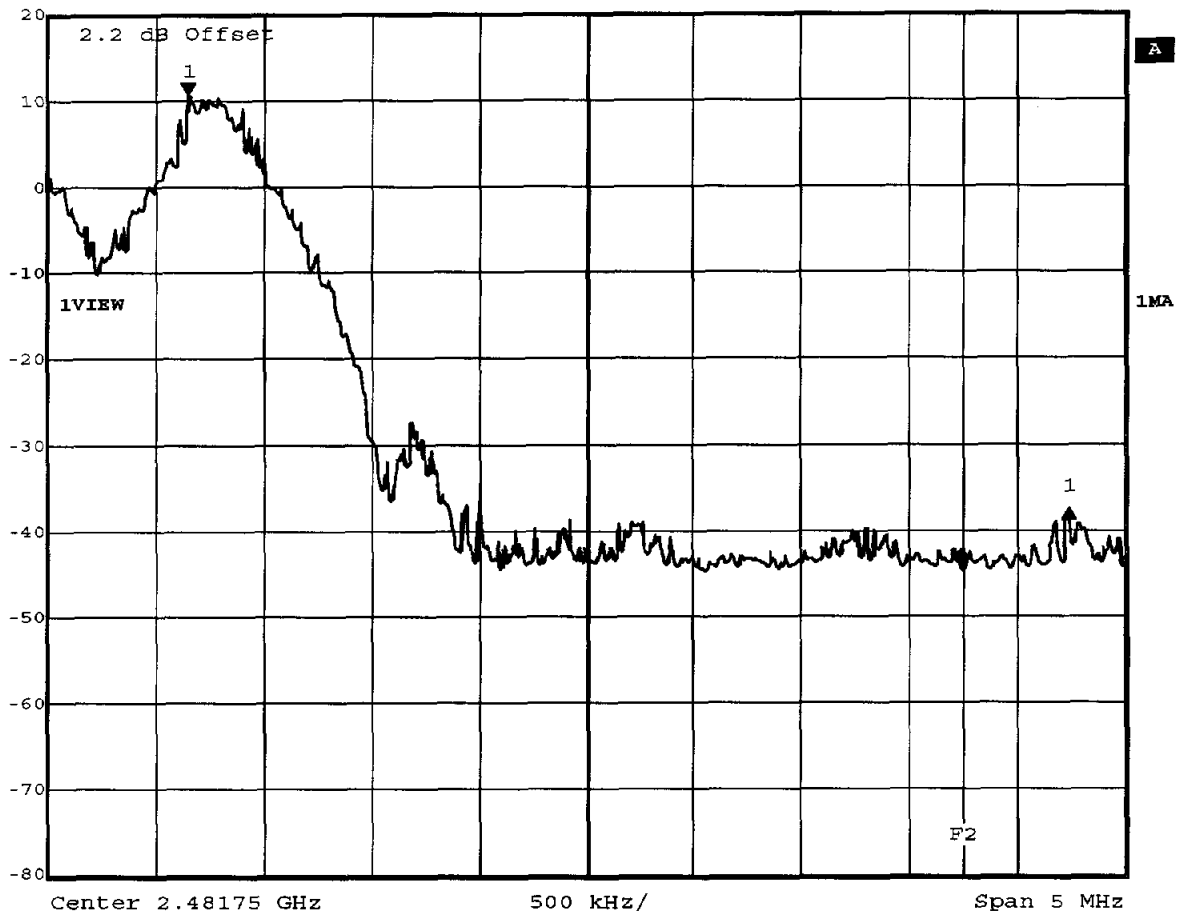
Comment A: Limit: Marker Delta value >20 dB; Result: PASS
Date: 20.APR.2007 13:38:14

Measurement diagram

**FCC part 15.247
Band-edge compliance of RF conducted emissions**

| | |
|-----------------------|------------------------------------|
| EUT | RTX3370 Monitor |
| Model | RTX3370 |
| Approval Holder | RTX Healthcare A/S |
| Temperature / Voltage | 25°C / Vnom |
| Test Site / Operator | ETS Product Service AG / Mr. Hoppe |
| Test Specification | FCC part 15 section 247(c) |
| Comment 1 | Band-edge compliance |
| Comment 2 | Channel.: 78 / 2480 MHz |
| Comment 3 | Hopping mode |

| | | | | | |
|---|--------------|----------------|--------|--------|-------|
|  | Delta 1 [T1] | RBW | 50 kHz | RF Att | 40 dB |
| | Ref Lvl | -48.13 dB | VBW | 50 kHz | |
| | 20 dBm | 4.08817635 MHz | SWT | 5 ms | Unit |



Comment A: Limit: Marker Delta value >20 dB; Result: PASS
Date: 20.APR.2007 13:41:35


Measurement diagram

Appendix K

AC power line conducted emissions


EMI voltage test in the ac-mains according to FCC part 15

EUT: RTX3370 Monitor
 Manufacturer: RTX Healthcare A/S
 Operating Condition: Unom: 120 VAC (AC/DC adaptor), Tnom: 23°C
 Test Site: ETS
 Operator: Mr. Marquardt
 Test Specification: V-Network: ESH2-Z5 (L1)
 Comment: model: RTX3370
 adaptor: FW7333M/06

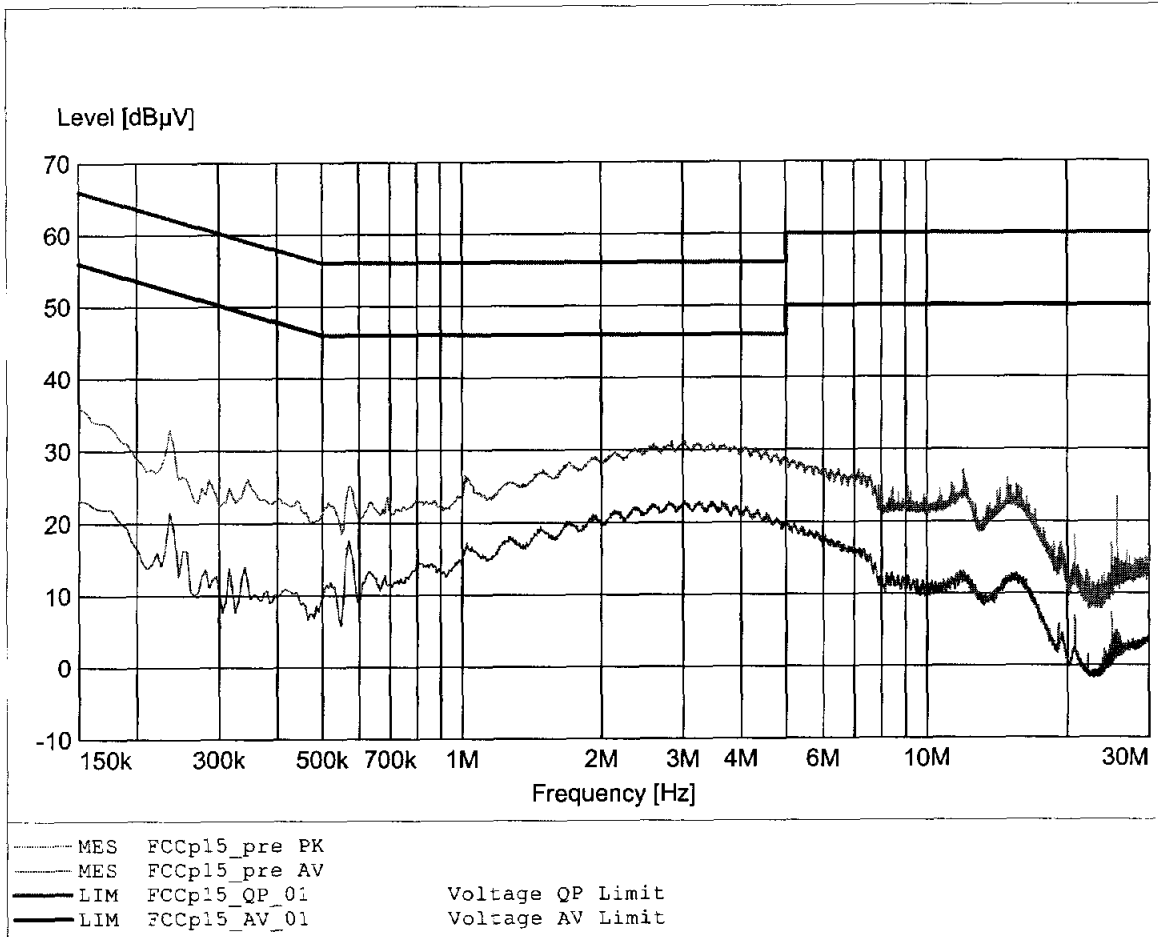

EMI voltage test in the ac-mains according to FCC part 15

EUT: RTX3370 Monitor
 Manufacturer: RTX Healthcare A/S
 Operating Condition: Unom: 120 VAC (AC/DC adaptor), Tnom: 23°C
 Test Site: ETS
 Operator: Mr. Marquardt
 Test Specification: V-Network: ESH2-Z5 (N)
 Comment: model: RTX3370
 adaptor: FW7333M/06

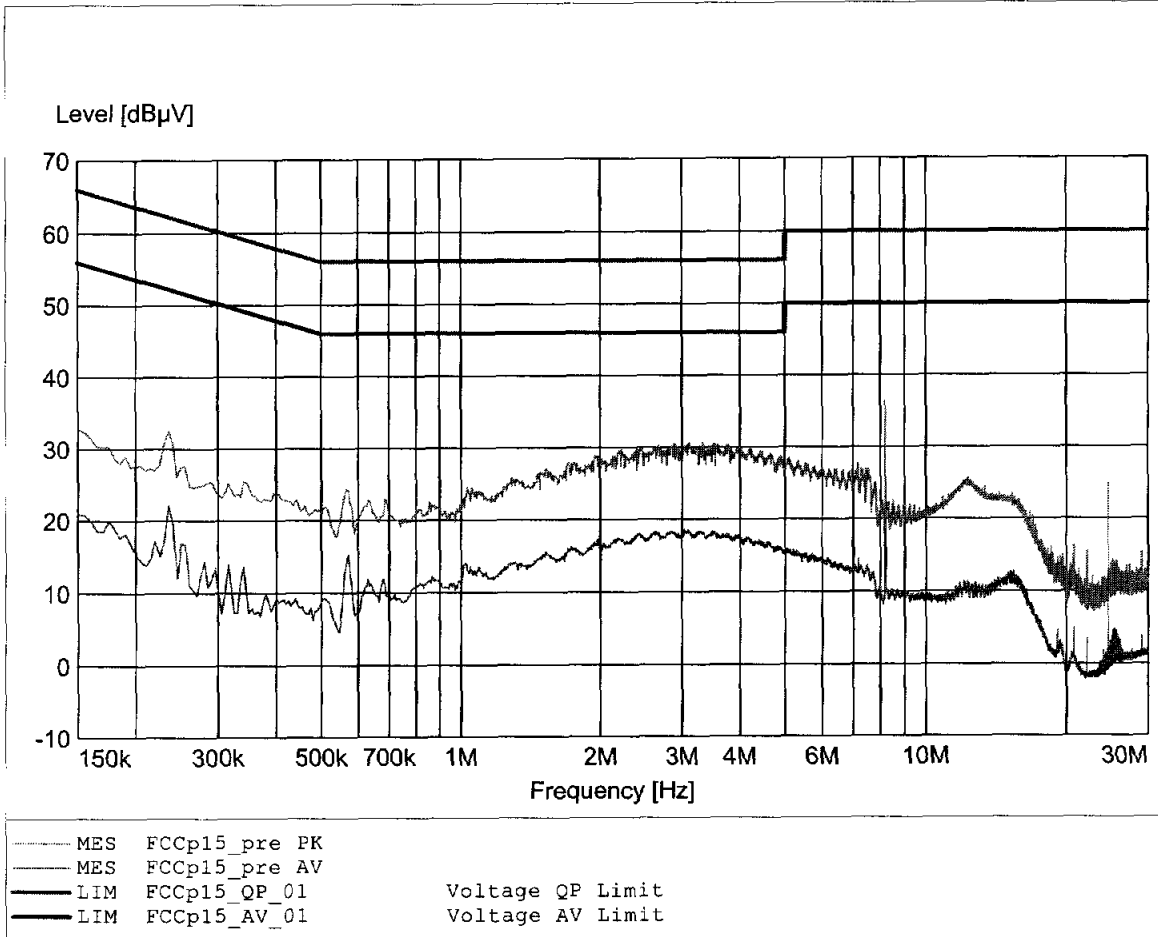


Appendix L

Receiver radiated emissions

Field Strength under normal conditions

Standards Industry Canada, RSS-GEN


Approval Holder: RTX Healthcare A/S
EUT: RTX3370 Monitor
Model: RTX3370 / 2441 MHz
Test Site / Operator: ETS / Mr. Meng
Test Condition: 25°C / Unom: 6.0 V DC
Test Specification: according to RSS-Gen Issue 1
Comment 1: Dist.: 3m, Ant.: HK 116
Comment 2: Freq:199.319MHz Emax:36.96dBµV/m RBW: 100 kHz

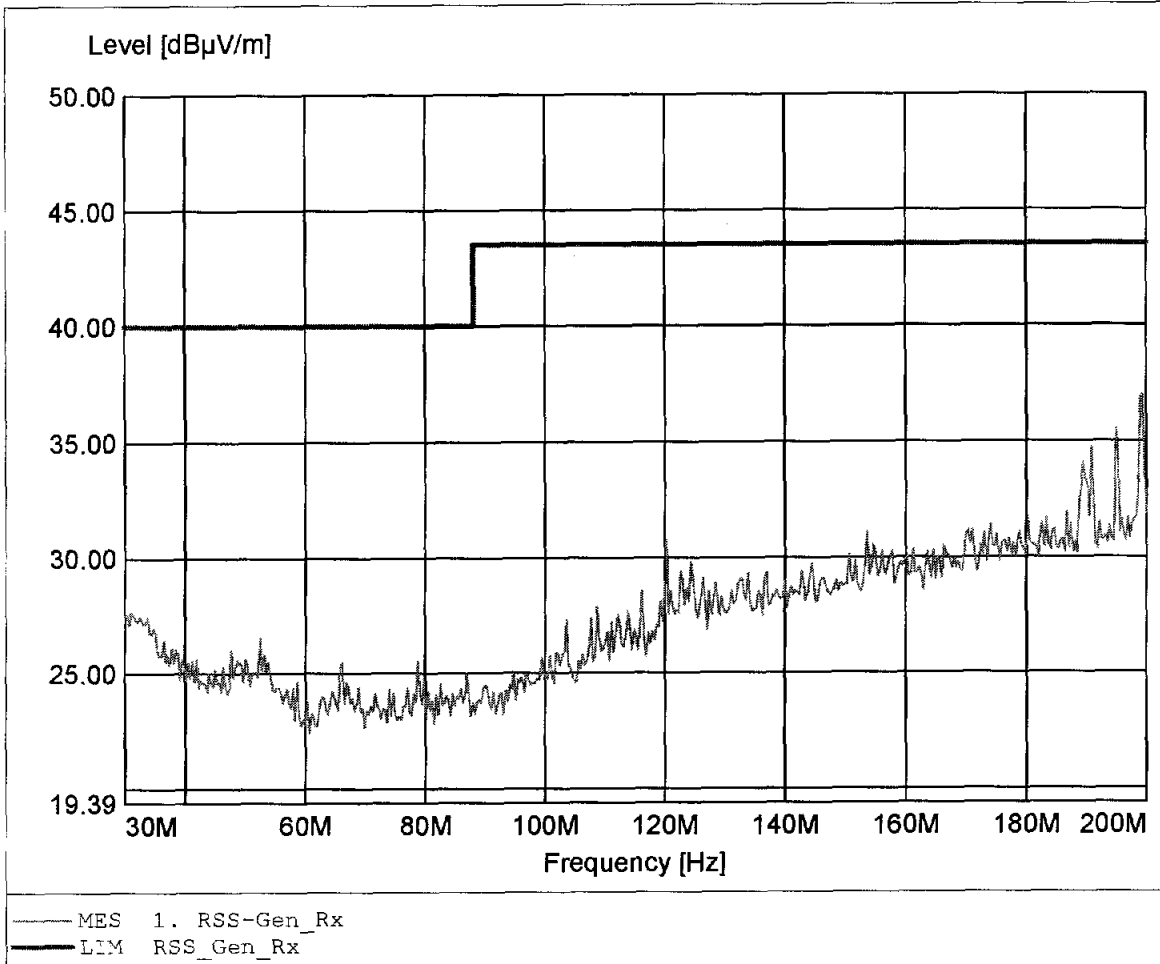

Field Strength under normal conditions

Standards Industry Canada, RSS-GEN


Approval Holder: RTX Healthcare A/S
EUT: RTX3370 Monitor
Model: RTX3370 / 2441 MHz
Test Site / Operator: ETS / Mr. Meng
Test Condition: 25°C / Unom: 6.0 V DC
Test Specification: according to RSS-Gen Issue 1
Comment 1: Dist.: 3m, Ant.: HK 116
Comment 2: Freq:199.319MHz Emax:35.72dBµV/m RBW: 100 kHz

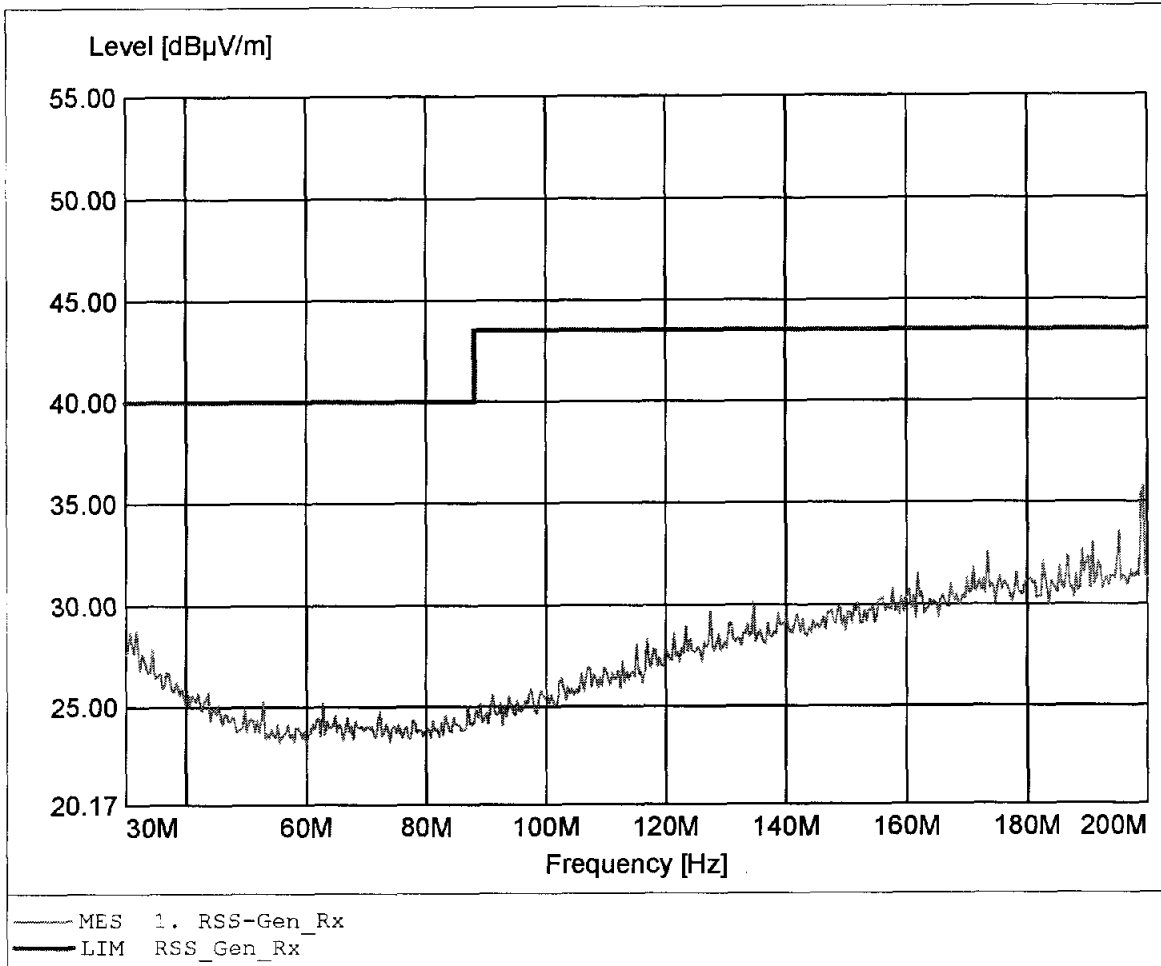

Field Strength under normal conditions

Standards Industry Canada, RSS-GEN


Approval Holder: RTX Healthcare A/S
EUT: RTX3370 Monitor
Model: RTX3370 / 2441 MHz
Test Site / Operator: ETS / Mr. Meng
Test Condition: 25°C / Unom: 6.0 V DC
Test Specification: according to RSS-Gen Issue 1
Comment 1: Dist.: 3m, Ant.: HL 223, ampl.
Comment 2: Freq:236.874MHz Emax:36.19dBµV/m RBW: 100 kHz

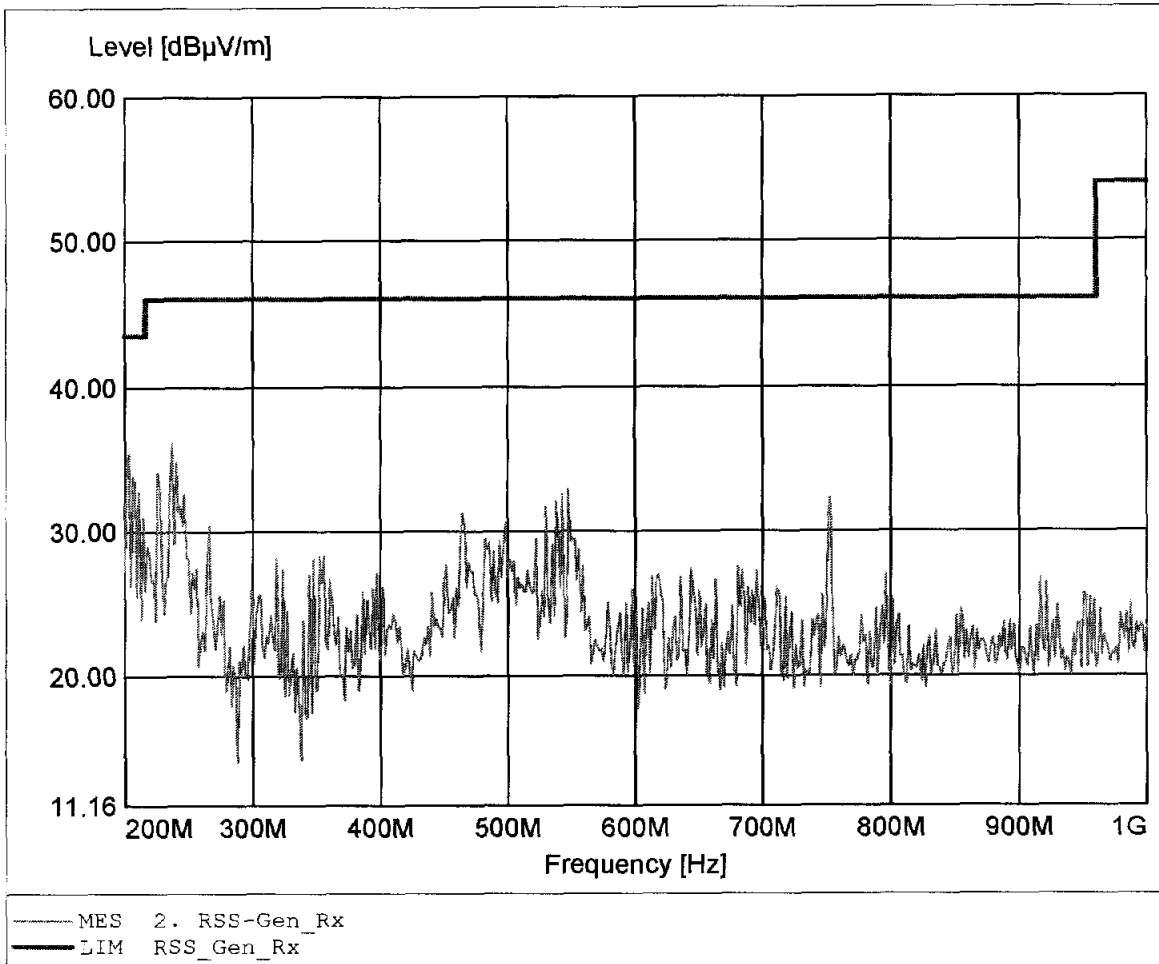

Field Strength under normal conditions

Standards Industry Canada, RSS-GEN


Approval Holder: RTX Healthcare A/S
EUT: RTX3370 Monitor
Model: RTX3370 / 2441 MHz
Test Site / Operator: ETS / Mr. Meng
Test Condition: 25°C / Unom: 6.0 V DC
Test Specification: according to RSS-Gen Issue 1
Comment 1: Dist.: 3m, Ant.: HL 223, ampl.
Comment 2: Freq:597.595MHz Emax:36.26dBµV/m RBW: 100 kHz

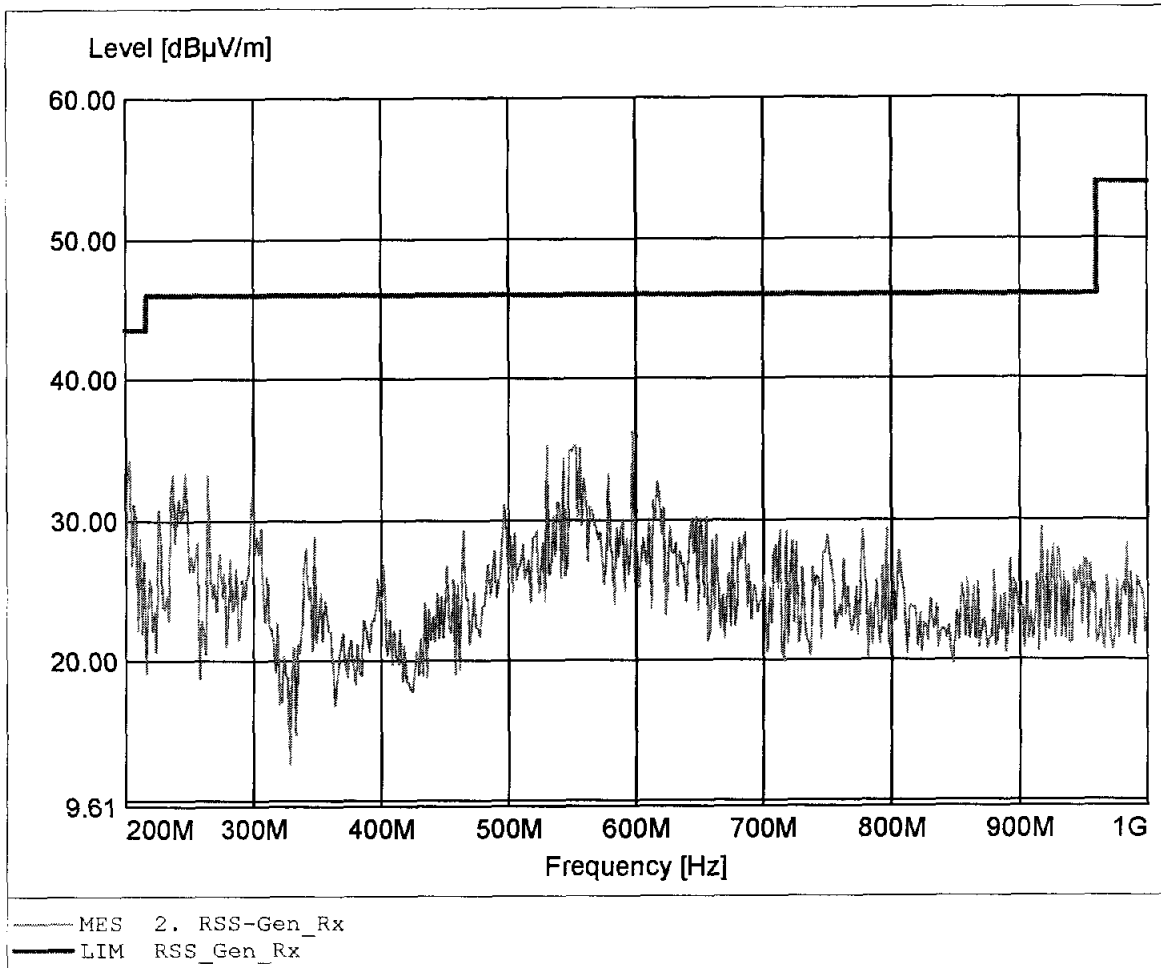

Field Strength under normal conditions

Standards Industry Canada, RSS-GEN


Approval Holder: RTX Healthcare A/S
EUT: RTX3370 Monitor
Model: RTX3370 / 2441 MHz
Test Site / Operator: ETS / Mr. Meng
Test Condition: 25°C / Unom: 6.0 V DC
Test Specification: according to RSS-Gen Issue 1
Comment 1: Dist.: 3m, Ant.: BBHA9120D, ampl.
Comment 2: Freq:3.850GHz Emax:42.59dBµV/m RBW: 1 MHz

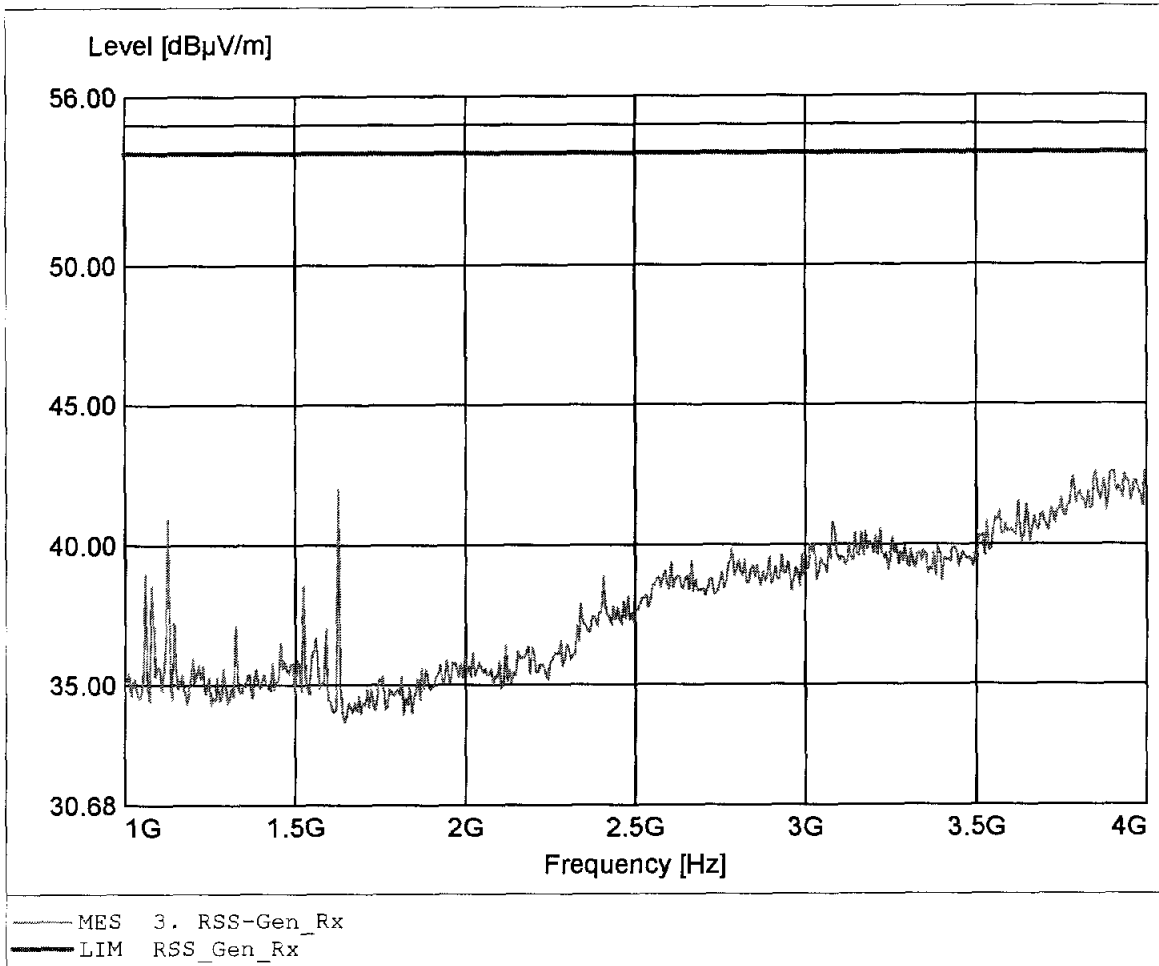

Field Strength under normal conditions

Standards Industry Canada, RSS-GEN


Approval Holder: RTX Healthcare A/S
EUT: RTX3370 Monitor
Model: RTX3370 / 2441 MHz
Test Site / Operator: ETS / Mr. Meng
Test Condition: 25°C / Unom: 6.0 V DC
Test Specification: according to RSS-Gen Issue 1
Comment 1: Dist.: 3m, Ant.: BBHA9120D, ampl.
Comment 2: Freq:3.910GHz Emax:43.86dBµV/m RBW: 1 MHz

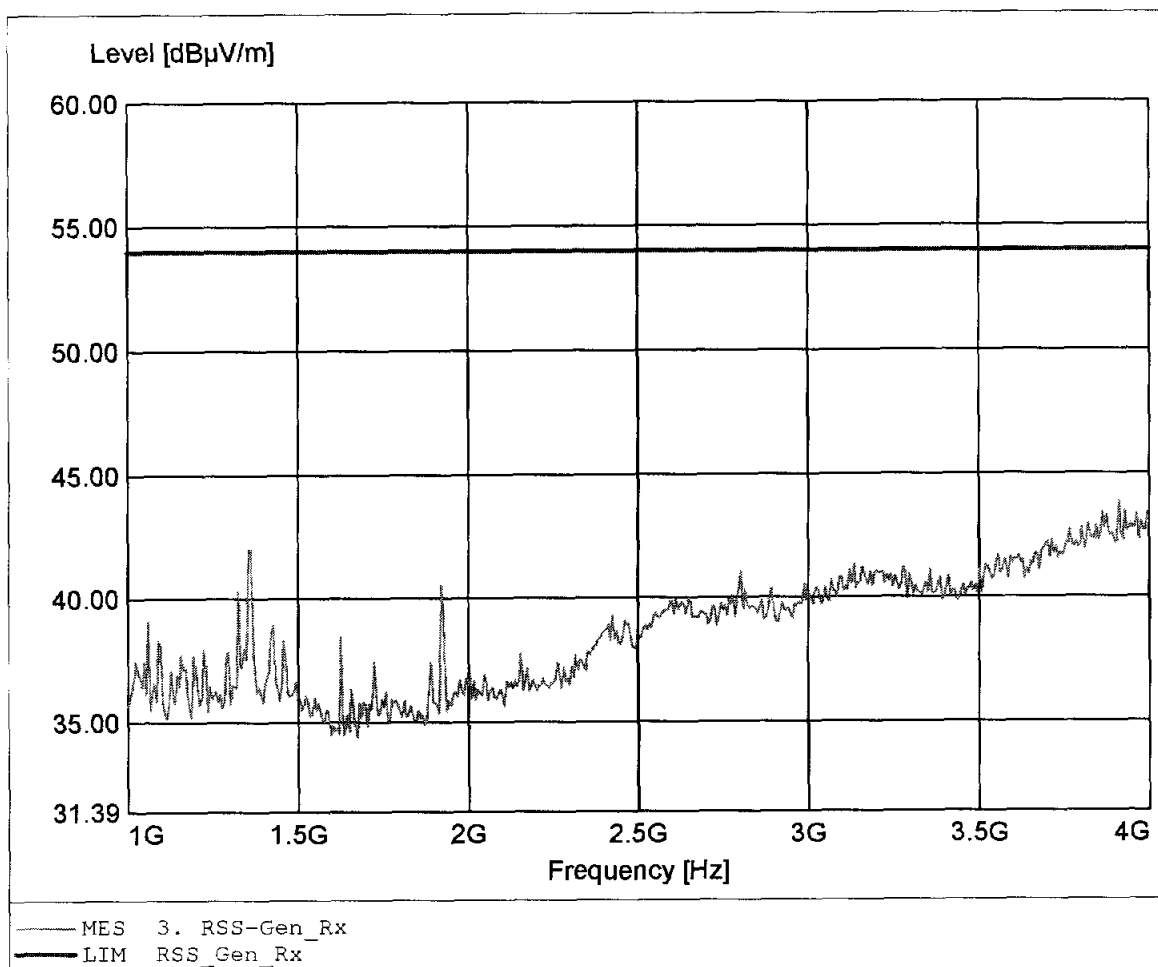

Field Strength under normal conditions

Standards Industry Canada, RSS-GEN


Approval Holder: RTX Healthcare A/S
EUT: RTX3370 Monitor
Model: RTX3370 / 2441 MHz
Test Site / Operator: ETS / Mr. Meng
Test Condition: 25°C / Unom: 6.0 V DC
Test Specification: according to RSS-Gen Issue 1
Comment 1: Dist.: 3m, Ant.: BBHA9120D, ampl.
Comment 2: Freq:6.854GHz Emax:45.70dBμV/m RBW: 1 MHz

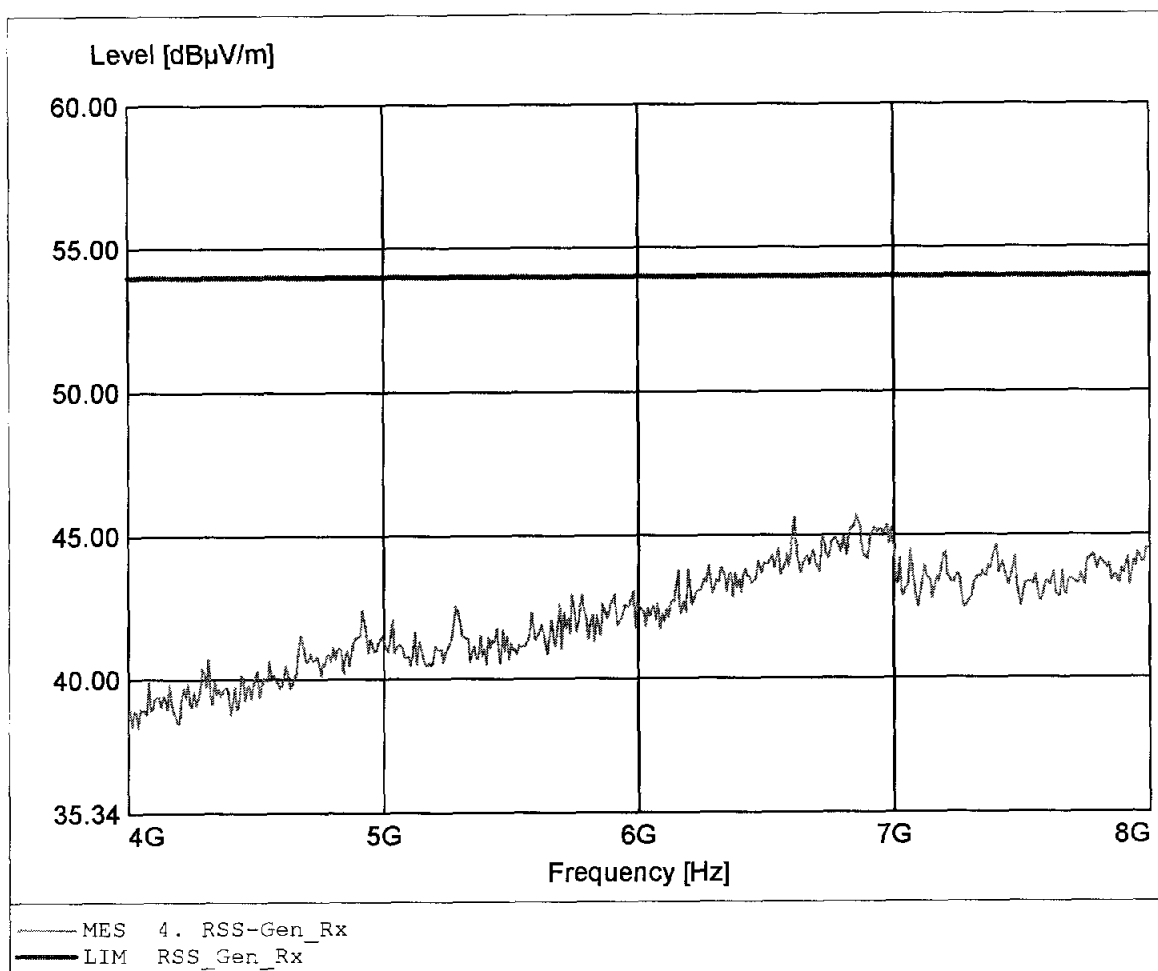

Field Strength under normal conditions

Standards Industry Canada, RSS-GEN


Approval Holder: RTX Healthcare A/S
EUT: RTX3370 Monitor
Model: RTX3370 / 2441 MHz
Test Site / Operator: ETS / Mr. Meng
Test Condition: 25°C / Unom: 6.0 V DC
Test Specification: according to RSS-Gen Issue 1
Comment 1: Dist.: 3m, Ant.: BBHA9120D, ampl.
Comment 2: Freq: 6.854GHz Emax:45.25dBµV/m RBW: 1 MHz

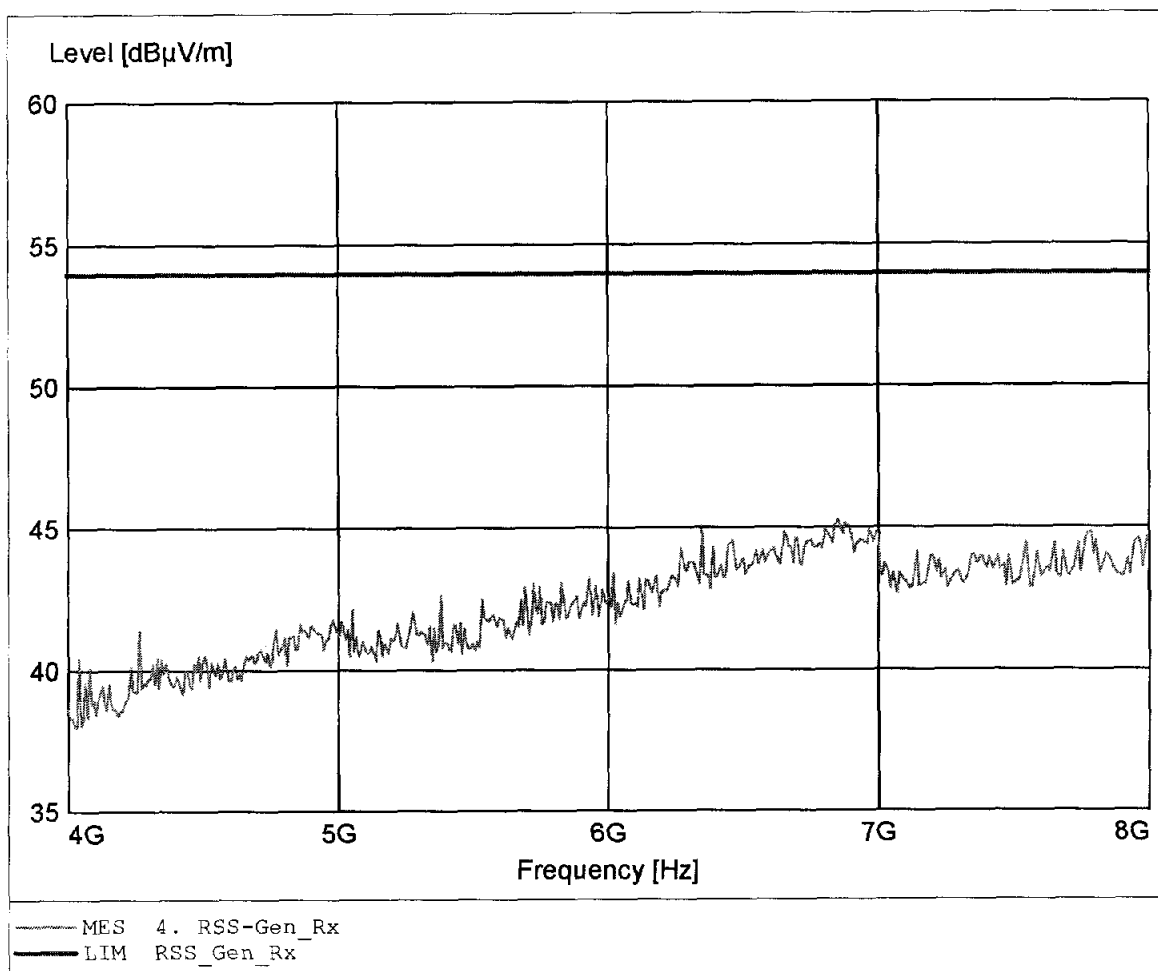

Field Strength under normal conditions

Standards Industry Canada, RSS-GEN

Approval Holder: RTX Healthcare A/S
EUT: RTX3370 Monitor
Model: RTX3370 / 2441 MHz
Test Site / Operator: ETS / Mr. Meng
Test Condition: 25°C / Unom: 6.0 V DC
Test Specification: according to RSS-Gen Issue 1
Comment 1: Dist.: 3m, Ant.: BBHA9120D, ampl.
Comment 2: Freq:11.174GHz Emax:39.90dBuV/m RBW: 1 MHz

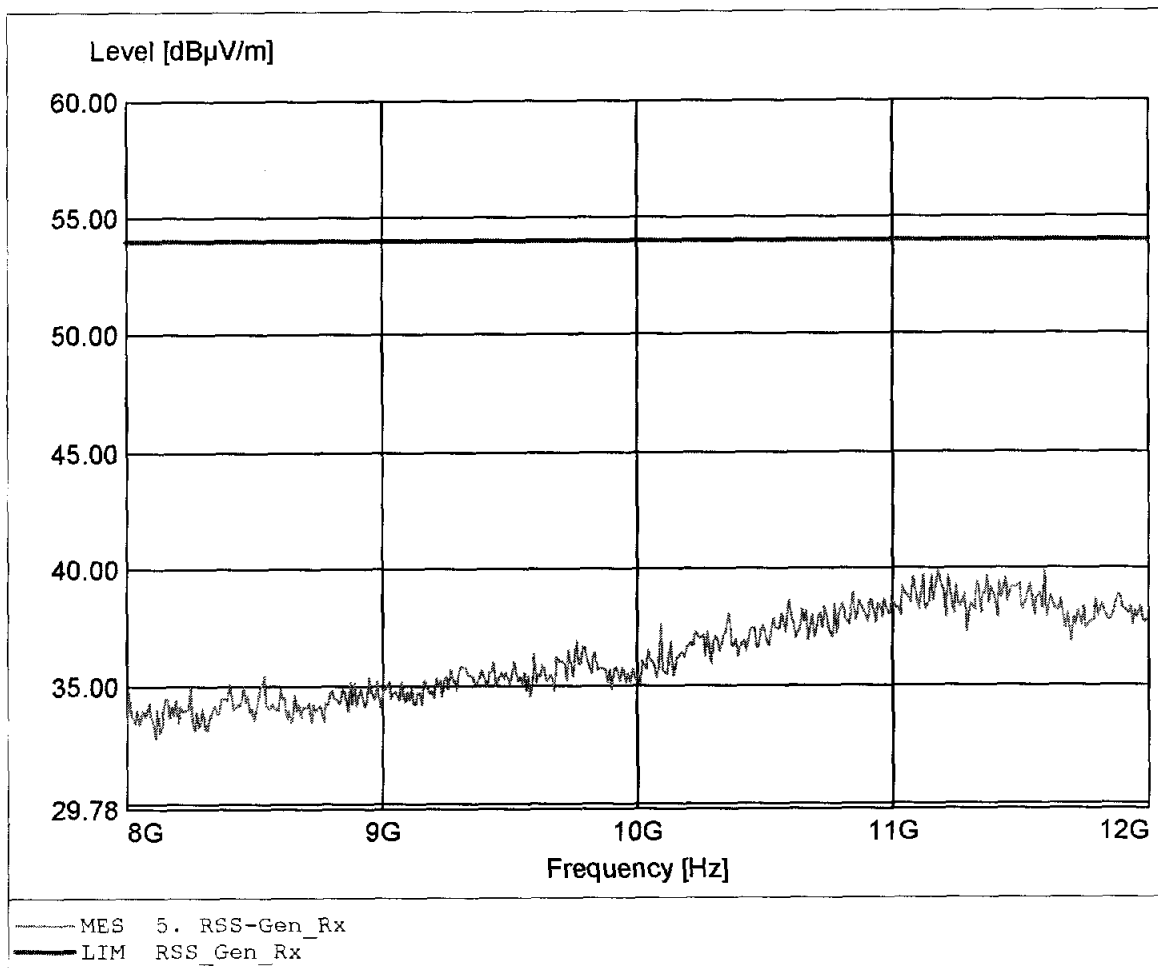

Field Strength under normal conditions

Standards Industry Canada, RSS-GEN

Approval Holder: RTX Healthcare A/S
EUT: RTX3370 Monitor
Model: RTX3370 / 2441 MHz
Test Site / Operator: ETS / Mr. Meng
Test Condition: 25°C / Unom: 6.0 V DC
Test Specification: according to RSS-Gen Issue 1
Comment 1: Dist.: 3m, Ant.: BBHA9120D, ampl.
Comment 2: Freq:11.182GHz Emax:39.64dBuV/m RBW: 1 MHz

