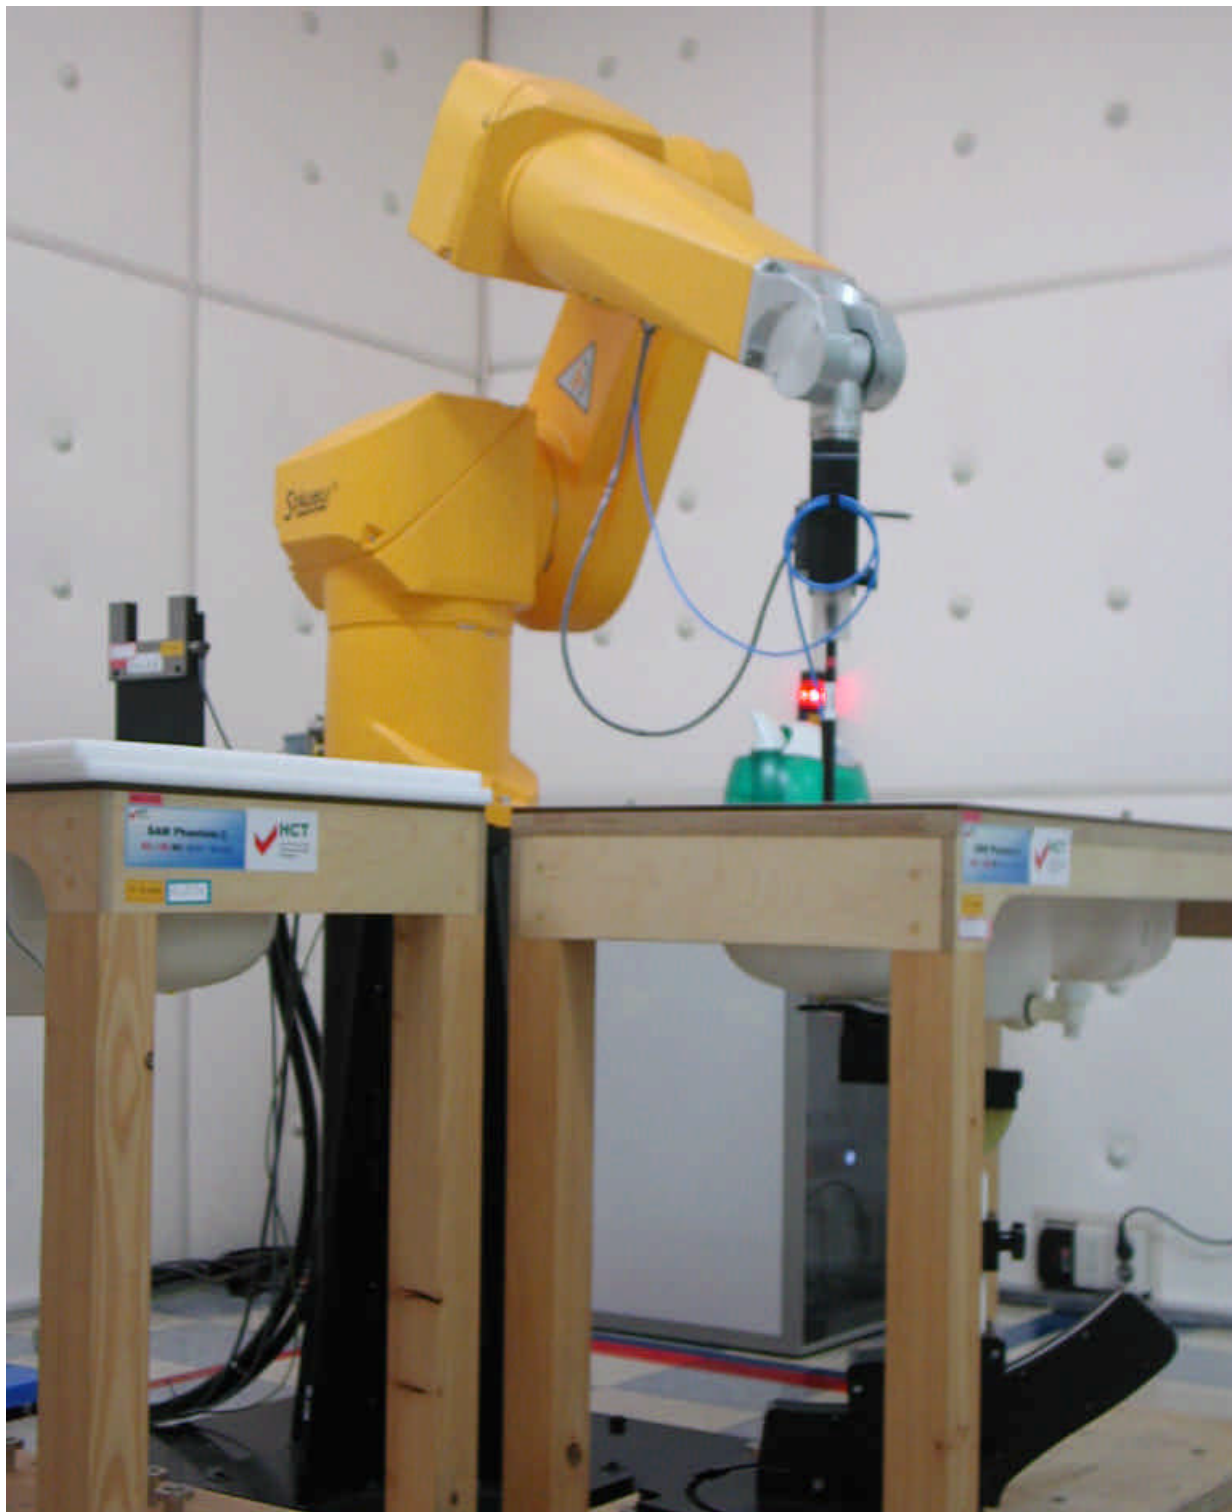
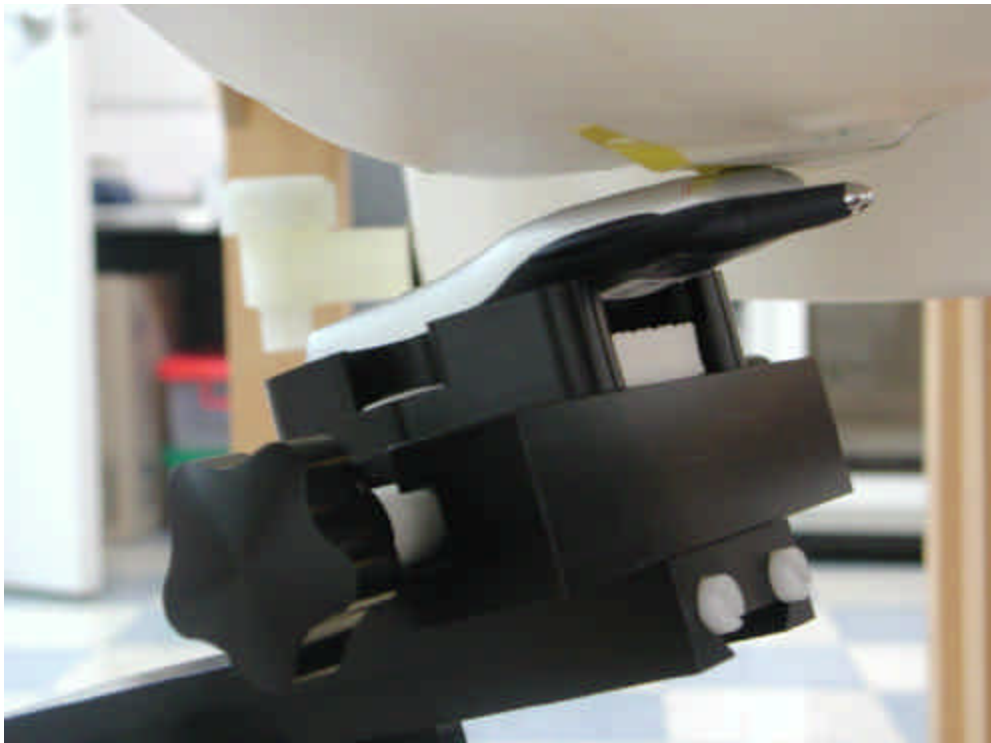
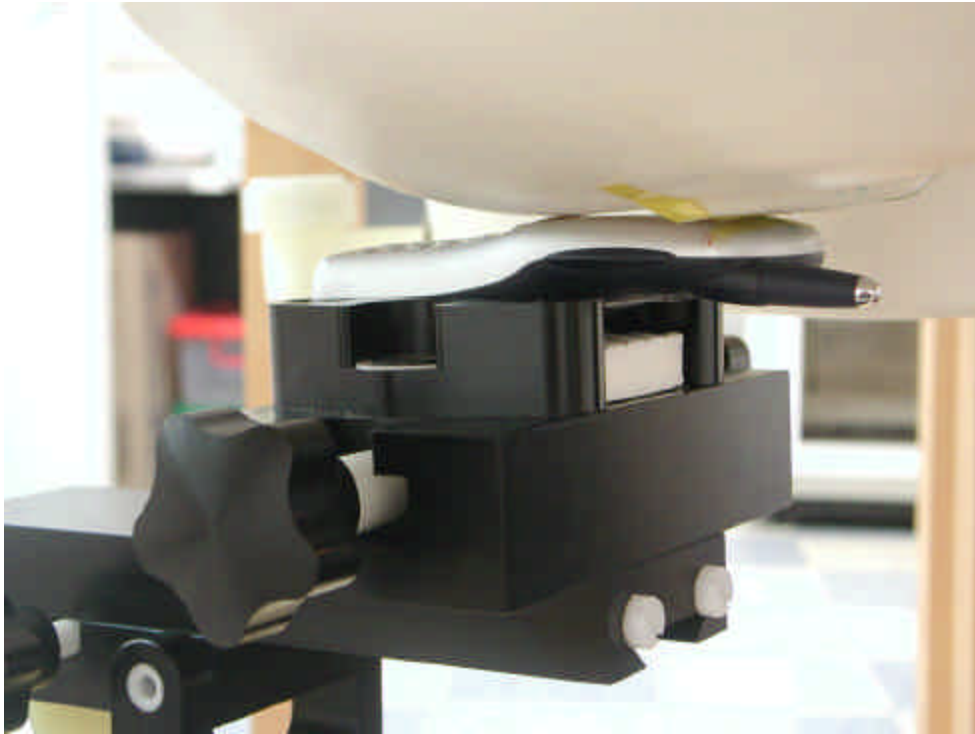
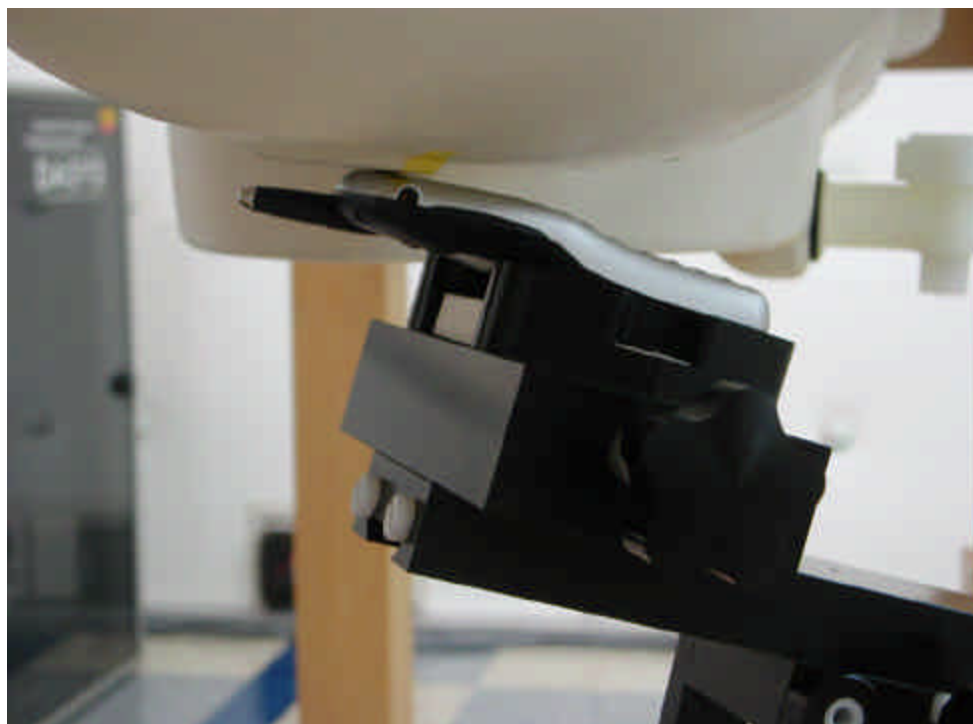
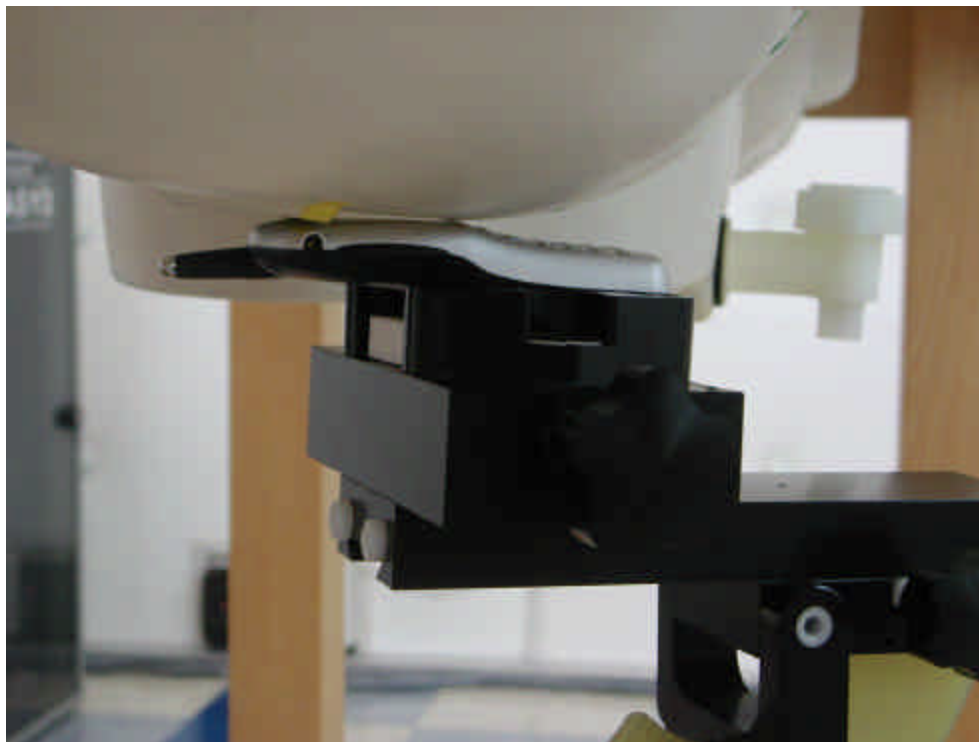



1. Test Setup Photo

1. Test Setup Photo


1. Test Setup Photo

1. Test Setup Photo

1. Test Setup Photo

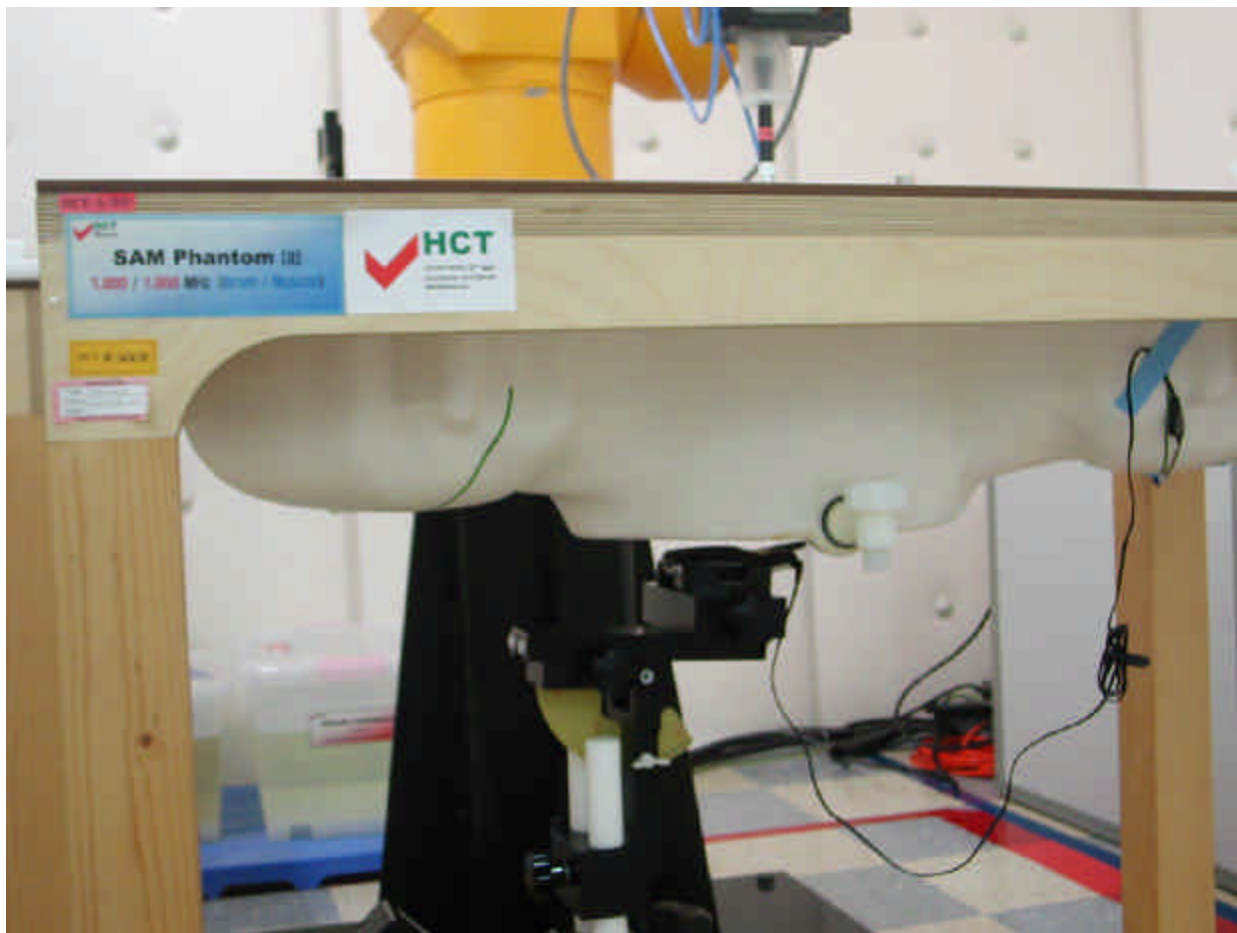


1. Test Setup Photo

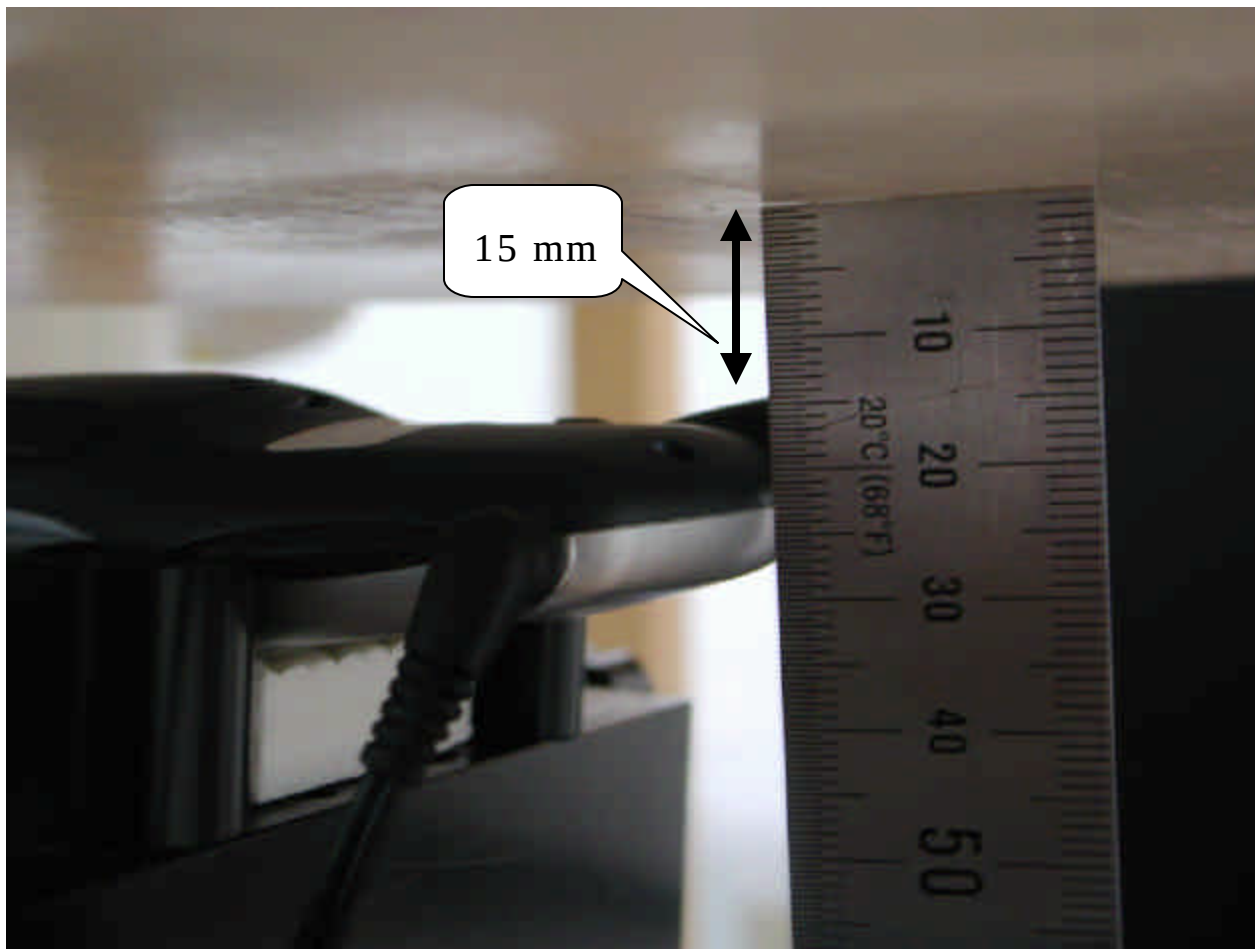


Test Setup Photo

[1900MHz Head Tissue Liquid Depth : 15cm]

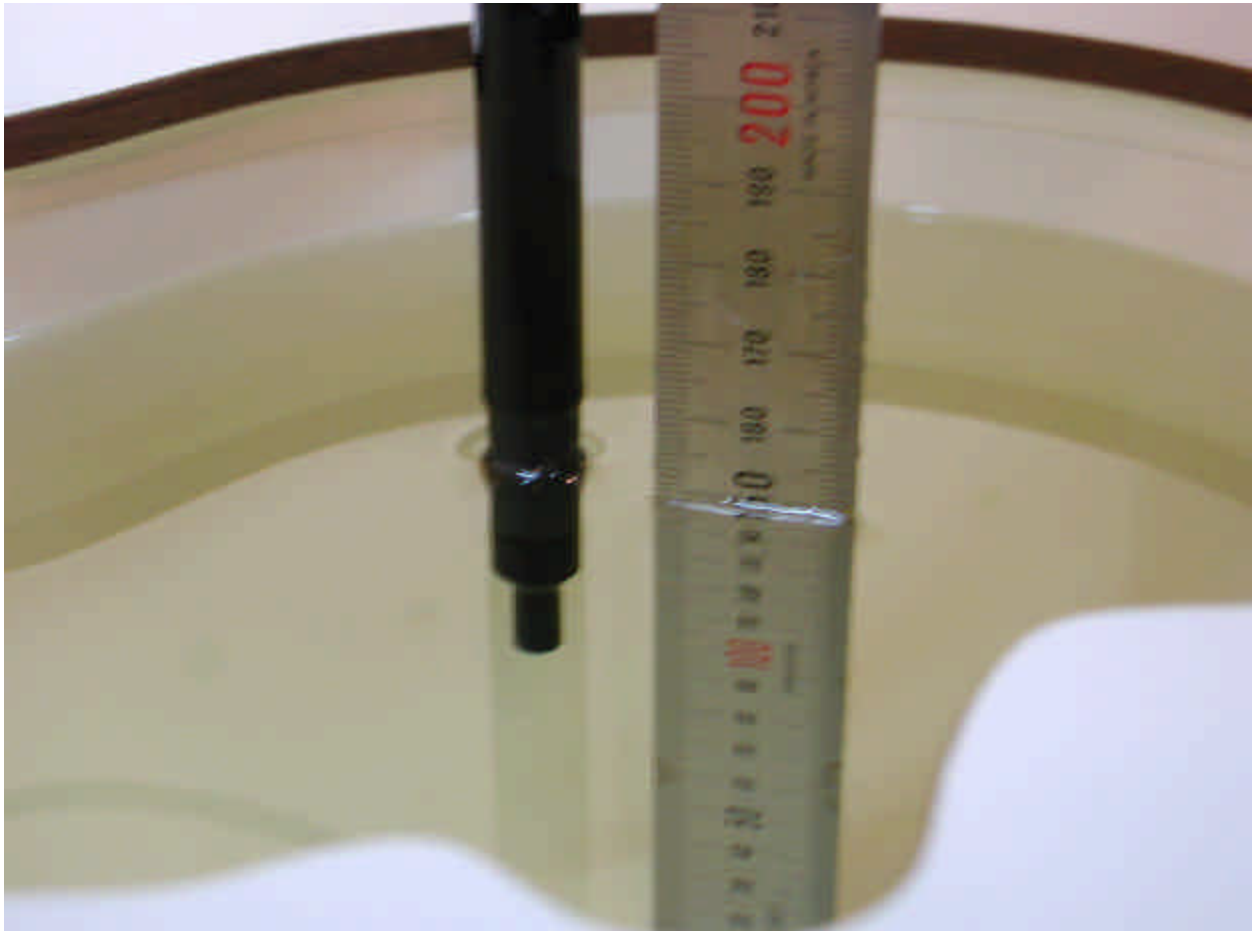

Test Setup Photo

[1900MHz Body Tissue Liquid Depth : 15cm]

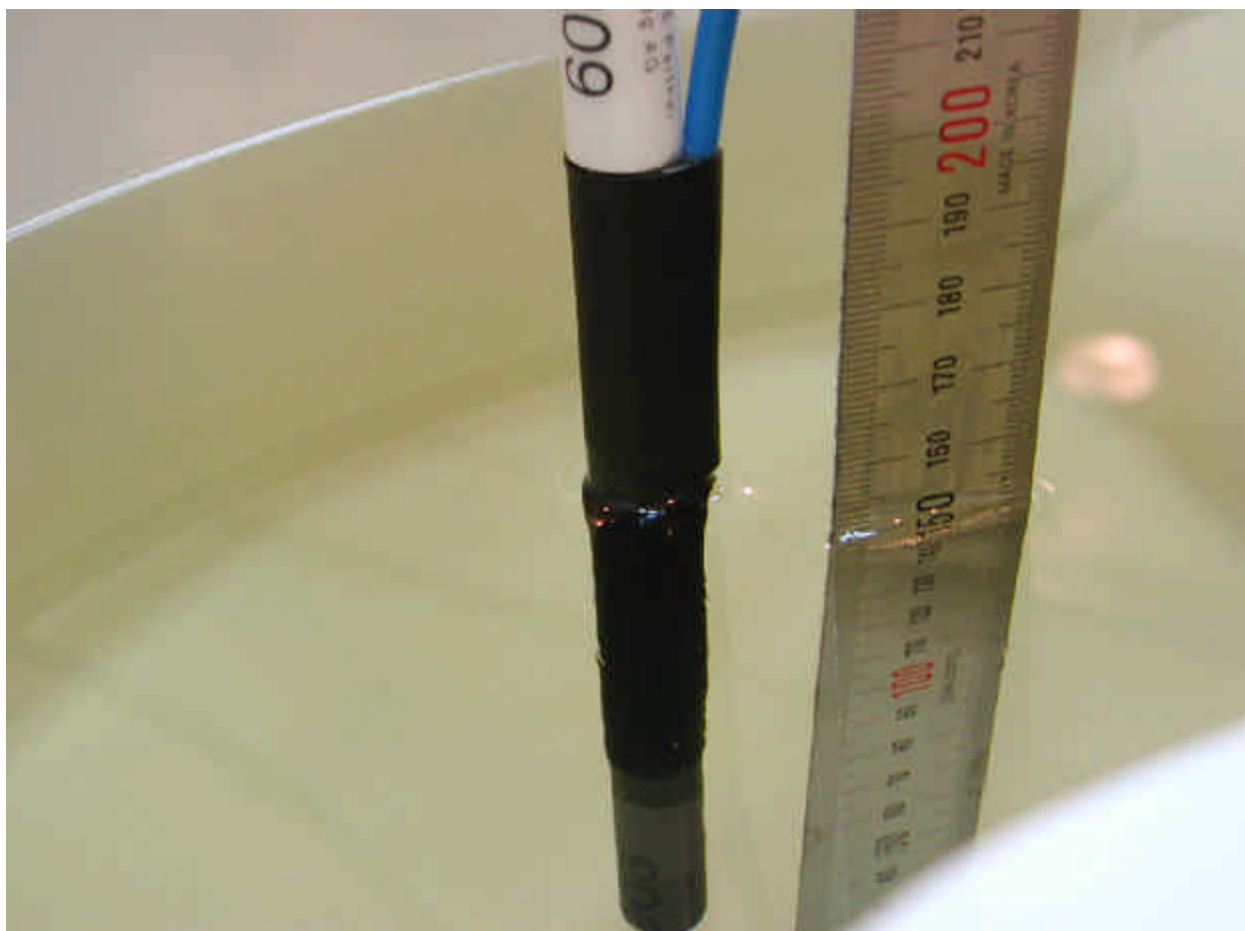

1. Test Setup Photo