

## DASY5 Validation Report for Head TSL

Date: 21.05.2024

Test Laboratory: SPEAG, Zurich, Switzerland

**DUT: CLA13; Type: CLA13; Serial: CLA13 - SN: 1009**

Communication System: UID 0 - CW; Frequency: 13 MHz

Medium parameters used:  $f = 13$  MHz;  $\sigma = 0.72$  S/m;  $\epsilon_r = 52.4$ ;  $\rho = 1000$  kg/m<sup>3</sup>

Phantom section: Flat Section

Measurement Standard: DASY5 (IEEE/IEC/ANSI C63.19-2011)

DASY52 Configuration:

- Probe: EX3DV4 - SN3877; ConvF(15.33, 15.33, 15.33) @ 13 MHz; Calibrated: 10.01.2024
- Sensor-Surface: 1.4mm (Mechanical Surface Detection)
- Electronics: DAE4 Sn654; Calibrated: 15.01.2024
- Phantom: ELI v6.0; Type: QDOVA003AA; Serial: TP:2034
- DASY52 52.10.4(1527); SEMCAD X 14.6.14(7483)

**CLA Calibration for HSL-LF Tissue/CLA-13, touch configuration, Pin=1W/Zoom Scan, dist=1.4mm (8x10x8)/Cube 0:** Measurement grid: dx=4mm, dy=4mm, dz=1.4mm

Reference Value = 31.57 V/m; Power Drift = -0.00 dB


Peak SAR (extrapolated) = 1.17 W/kg

**SAR(1 g) = 0.553 W/kg; SAR(10 g) = 0.340 W/kg**


Smallest distance from peaks to all points 3 dB below = 16 mm

Ratio of SAR at M2 to SAR at M1 = 77.1%

Maximum value of SAR (measured) = 0.832 W/kg

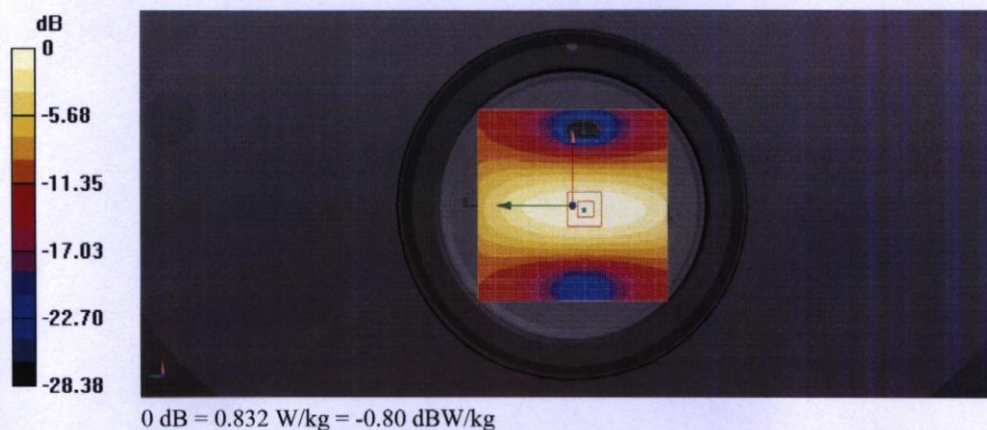

## Impedance Measurement Plot for Head TSL

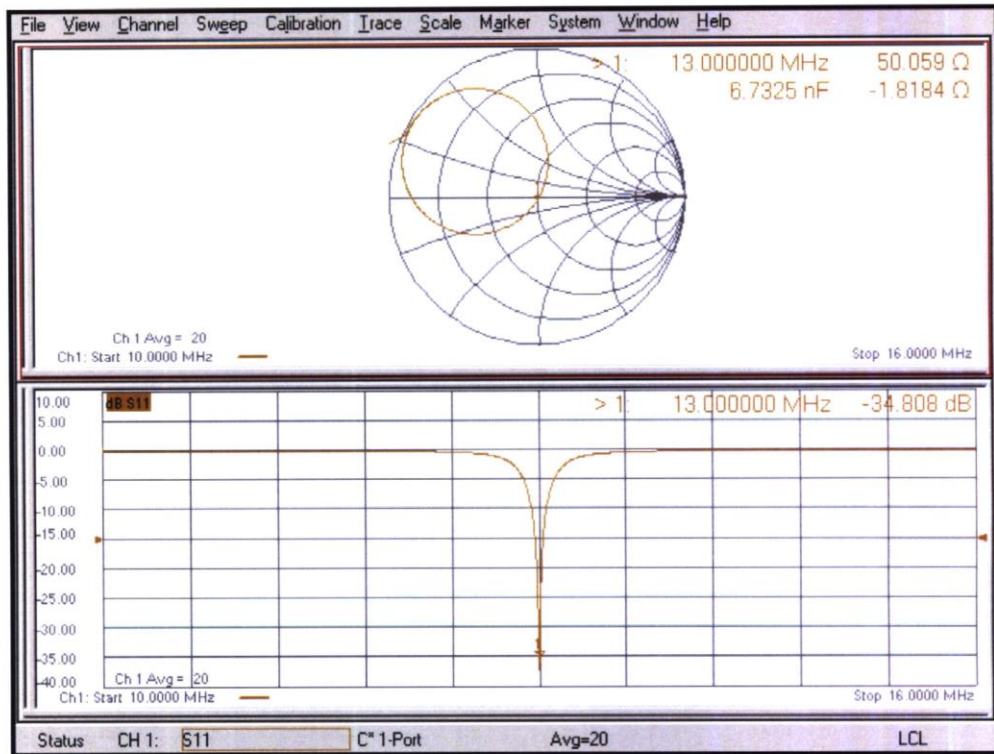

# 10 GHz Dipole Calibration Certificate

**Calibration Laboratory of**  
**Schmid & Partner**  
**Engineering AG**  
Zeughausstrasse 43, 8004 Zurich, Switzerland



**S** Schweizerischer Kalibrierdienst  
**C** Service suisse d'étalonnage  
**S** Servizio svizzero di taratura  
**S** Swiss Calibration Service

Accredited by the Swiss Accreditation Service (SAS)  
The Swiss Accreditation Service is one of the signatories to the EA  
Multilateral Agreement for the recognition of calibration certificates

Accreditation No.: **SCS 0108**

Client **CTTL**  
**Beijing**

Certificate No. **5G-Veri10-1005\_Jan24**

| CALIBRATION CERTIFICATE                                                                                                                                                                                                                                                       |                                                                      |                                   |                          |
|-------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------|----------------------------------------------------------------------|-----------------------------------|--------------------------|
| Object                                                                                                                                                                                                                                                                        | 5G Verification Source 10 GHz - SN: 1005                             |                                   |                          |
| Calibration procedure(s)                                                                                                                                                                                                                                                      | QA CAL-45.v4<br>Calibration procedure for sources in air above 6 GHz |                                   |                          |
| Calibration date:                                                                                                                                                                                                                                                             | January 18, 2024                                                     |                                   |                          |
| This calibration certificate documents the traceability to national standards, which realize the physical units of measurements (SI).<br>The measurements and the uncertainties with confidence probability are given on the following pages and are part of the certificate. |                                                                      |                                   |                          |
| All calibrations have been conducted in the closed laboratory facility: environment temperature (22 ± 3)°C and humidity < 70%.                                                                                                                                                |                                                                      |                                   |                          |
| Calibration Equipment used (M&TE critical for calibration)                                                                                                                                                                                                                    |                                                                      |                                   |                          |
| Primary Standards                                                                                                                                                                                                                                                             | ID #                                                                 | Cal Date (Certificate No.)        | Scheduled Calibration    |
| Reference Probe EUMMWV3                                                                                                                                                                                                                                                       | SN: 9374                                                             | 04-Dec-23 (No. EUMm-9374_Dec23)   | Dec-24                   |
| DAE4                                                                                                                                                                                                                                                                          | SN: 1215                                                             | 29-Jun-23 (No. DAE4-1215_Jun23)   | Jun-24                   |
| Secondary Standards                                                                                                                                                                                                                                                           | ID #                                                                 | Check Date (in house)             | Scheduled Check          |
| RF generator R&S SMF100A                                                                                                                                                                                                                                                      | SN: 100184                                                           | 29-Nov-23 (in house check Nov-23) | In house check: Nov-24   |
| Power sensor R&S NRP18S-10                                                                                                                                                                                                                                                    | SN: 101258                                                           | 29-Nov-23 (in house check Nov-23) | In house check: Nov-24   |
| Network Analyzer Keysight E5063A                                                                                                                                                                                                                                              | SN: MY54504221                                                       | 31-Oct-19 (in house check Oct-22) | In house check: Oct-25   |
| Calibrated by:                                                                                                                                                                                                                                                                | Name<br>Joanna Lleshaj                                               | Function<br>Laboratory Technician | Signature<br>            |
| Approved by:                                                                                                                                                                                                                                                                  | Sven Kühn                                                            | Technical Manager                 |                          |
|                                                                                                                                                                                                                                                                               |                                                                      |                                   | Issued: January 19, 2024 |
| This calibration certificate shall not be reproduced except in full without written approval of the laboratory.                                                                                                                                                               |                                                                      |                                   |                          |



## Glossary

Accredited by the Swiss Accreditation Service (SAS)

Accreditation No.: **SCS 0108**

The Swiss Accreditation Service is one of the signatories to the EA  
Multilateral Agreement for the recognition of calibration certificates

**CW** Continuous wave

## Calibration is Performed According to the Following Standards

- Internal procedure QA CAL-45, Calibration procedure for sources in air above 6 GHz.
- IEC/IEEE 63195-1, "Assessment of power density of human exposure to radio frequency fields from wireless devices in close proximity to the head and body (frequency range of 6 GHz to 300 GHz)", May 2022

## Methods Applied and Interpretation of Parameters

- *Coordinate System:* z-axis in the waveguide horn boresight, x-axis is in the direction of the E-field, y-axis normal to the others in the field scanning plane parallel to the horn flare and horn flange.
- *Measurement Conditions:* (1) 10 GHz: The radiated power is the forward power to the horn antenna minus ohmic and mismatch loss. The forward power is measured prior and after the measurement with a power sensor. During the measurements, the horn is directly connected to the cable and the antenna ohmic and mismatch losses are determined by far-field measurements. (2) 30, 45, 60 and 90 GHz: The verification sources are switched on for at least 30 minutes. Absorbers are used around the probe cub and at the ceiling to minimize reflections.
- *Horn Positioning:* The waveguide horn is mounted vertically on the flange of the waveguide source to allow vertical positioning of the EUmmW probe during the scan. The plane is parallel to the phantom surface. Probe distance is verified using mechanical gauges positioned on the flare of the horn.
- *E-field distribution:* E field is measured in two x-y-plane (10mm, 10mm +  $\lambda/4$ ) with a vectorial E-field probe. The E-field value stated as calibration value represents the E-field-maxima and the averaged (1cm<sup>2</sup> and 4cm<sup>2</sup>) power density values at 10mm in front of the horn.
- *Field polarization:* Above the open horn, linear polarization of the field is expected. This is verified graphically in the field representation.

## Calibrated Quantity

- Local peak E-field (V/m) and average of peak spatial components of the poynting vector (W/m<sup>2</sup>) averaged over the surface area of 1 cm<sup>2</sup> and 4cm<sup>2</sup> at the nominal operational frequency of the verification source. Both square and circular averaging results are listed.

The reported uncertainty of measurement is stated as the standard uncertainty of measurement multiplied by the coverage factor k=2, which for a normal distribution corresponds to a coverage probability of approximately 95%.

## Measurement Conditions

DASY system configuration, as far as not given on page 1.

|                                       |                               |      |
|---------------------------------------|-------------------------------|------|
| <b>DASY Version</b>                   | DASY8 Module mmWave           | V3.2 |
| <b>Phantom</b>                        | 5G Phantom                    |      |
| <b>Distance Horn Aperture - plane</b> | 10 mm                         |      |
| <b>Number of measured planes</b>      | 2 (10mm, 10mm + $\lambda/4$ ) |      |
| <b>Frequency</b>                      | 10 GHz $\pm$ 10 MHz           |      |

## Calibration Parameters, 10 GHz

### Circular Averaging

| Distance Horn Aperture to Measured Plane | <i>Prad</i> <sup>1</sup> (mW) | Max E-field (V/m) | Uncertainty (k = 2) | Avg Power Density<br>Avg (psPDn+, psPDtot+, psPDmod+)<br>(W/m <sup>2</sup> ) |                   | Uncertainty (k = 2) |
|------------------------------------------|-------------------------------|-------------------|---------------------|------------------------------------------------------------------------------|-------------------|---------------------|
|                                          |                               |                   |                     | 1 cm <sup>2</sup>                                                            | 4 cm <sup>2</sup> |                     |
| 10 mm                                    | 93.3                          | 151               | 1.27 dB             | 59.4                                                                         | 55.5              | 1.28 dB             |

| Distance Horn Aperture to Measured Plane | <i>Prad</i> <sup>1</sup> (mW) | Max E-field (V/m) | Uncertainty (k = 2) | Power Density<br>psPDn+, psPDtot+, psPDmod+<br>(W/m <sup>2</sup> ) |                   | Uncertainty (k = 2) |
|------------------------------------------|-------------------------------|-------------------|---------------------|--------------------------------------------------------------------|-------------------|---------------------|
|                                          |                               |                   |                     | 1 cm <sup>2</sup>                                                  | 4 cm <sup>2</sup> |                     |
| 10 mm                                    | 93.3                          | 151               | 1.27 dB             | 59.2, 59.4, 59.6                                                   | 55.2, 55.5, 55.7  | 1.28 dB             |

### Square Averaging

| Distance Horn Aperture to Measured Plane | <i>Prad</i> <sup>1</sup> (mW) | Max E-field (V/m) | Uncertainty (k = 2) | Avg Power Density<br>Avg (psPDn+, psPDtot+, psPDmod+)<br>(W/m <sup>2</sup> ) |                   | Uncertainty (k = 2) |
|------------------------------------------|-------------------------------|-------------------|---------------------|------------------------------------------------------------------------------|-------------------|---------------------|
|                                          |                               |                   |                     | 1 cm <sup>2</sup>                                                            | 4 cm <sup>2</sup> |                     |
| 10 mm                                    | 93.3                          | 151               | 1.27 dB             | 59.4                                                                         | 55.4              | 1.28 dB             |

| Distance Horn Aperture to Measured Plane | <i>Prad</i> <sup>1</sup> (mW) | Max E-field (V/m) | Uncertainty (k = 2) | Power Density<br>psPDn+, psPDtot+, psPDmod+<br>(W/m <sup>2</sup> ) |                   | Uncertainty (k = 2) |
|------------------------------------------|-------------------------------|-------------------|---------------------|--------------------------------------------------------------------|-------------------|---------------------|
|                                          |                               |                   |                     | 1 cm <sup>2</sup>                                                  | 4 cm <sup>2</sup> |                     |
| 10 mm                                    | 93.3                          | 151               | 1.27 dB             | 59.1, 59.4, 59.6                                                   | 55.1, 55.4, 55.7  | 1.28 dB             |

### Max Power Density

| Distance Horn Aperture to Measured Plane | <i>Prad</i> <sup>1</sup> (mW) | Max E-field (V/m) | Uncertainty (k = 2) | Max Power Density<br>Sn, Stot,  Stot <br>(W/m <sup>2</sup> ) | Uncertainty (k = 2) |
|------------------------------------------|-------------------------------|-------------------|---------------------|--------------------------------------------------------------|---------------------|
| 10 mm                                    | 93.3                          | 151               | 1.27 dB             | 60.5, 60.7, 60.9                                             | 1.28 dB             |


<sup>1</sup> Assessed ohmic and mismatch loss plus numerical offset: 0.30 dB

## Appendix (Additional assessments outside the scope of SCS 0108)

### Antenna Parameters

|                                      |                                |
|--------------------------------------|--------------------------------|
| Impedance, transformed to feed point | 53.5 $\Omega$ - 0.1 j $\Omega$ |
| Return Loss                          | - 29.5 dB                      |

### Impedance Measurement Plot

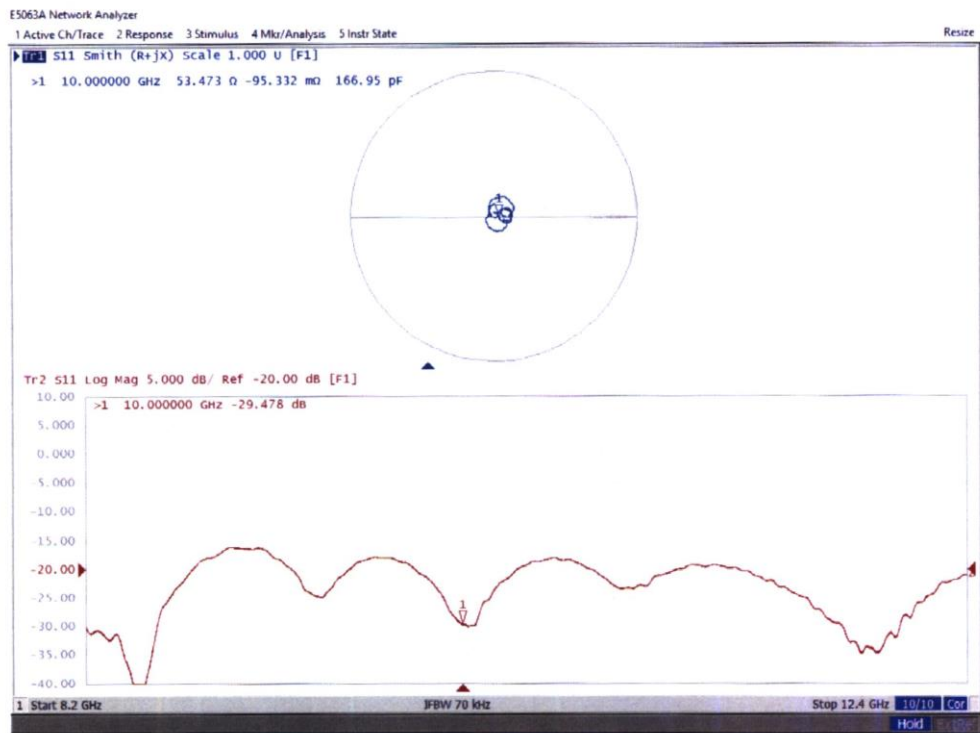

DASY Report

Measurement Report for 5G Verification Source 10 GHz, UID 0 -, Channel 10000 (10000.0MHz)

Device under Test Properties

| Name, Manufacturer            | Dimensions [mm]       | IMEI     | DUT Type |
|-------------------------------|-----------------------|----------|----------|
| 5G Verification Source 10 GHz | 100.0 x 100.0 x 172.0 | SN: 1005 | -        |

Exposure Conditions

| Phantom Section | Position, Test Distance [mm] | Band            | Group, | Frequency [MHz], Channel Number | Conversion Factor |
|-----------------|------------------------------|-----------------|--------|---------------------------------|-------------------|
| 5G -            | 10.0 mm                      | Validation band | CW     | 10000.0, 10000                  | 1.0               |

Hardware Setup


| Phantom               | Medium | Probe, Calibration Date               | DAE, Calibration Date   |
|-----------------------|--------|---------------------------------------|-------------------------|
| mmWave Phantom - 1002 | Air    | EUmmWV3 - SN9374_F1-55GHz, 2023-12-04 | DAE4 Sn1215, 2023-06-29 |

Scan Setup

| Sensor Surface [mm] | 5G Scan               |
|---------------------|-----------------------|
| MAIA                | 10.0<br>MAIA not used |

Measurement Results

|                                 | 5G Scan            |
|---------------------------------|--------------------|
| Date                            | 2024-01-18, 15:51  |
| Avg. Area [cm <sup>2</sup> ]    | 1.00               |
| Avg. Type                       | Circular Averaging |
| psPDn+ [W/m <sup>2</sup> ]      | 59.2               |
| psPDtot+ [W/m <sup>2</sup> ]    | 59.4               |
| psPDmod+ [W/m <sup>2</sup> ]    | 59.6               |
| Max(Sn) [W/m <sup>2</sup> ]     | 60.5               |
| Max(Stot) [W/m <sup>2</sup> ]   | 60.7               |
| Max( Stot ) [W/m <sup>2</sup> ] | 60.9               |
| E <sub>max</sub> [V/m]          | 151                |
| Power Drift [dB]                | -0.01              |

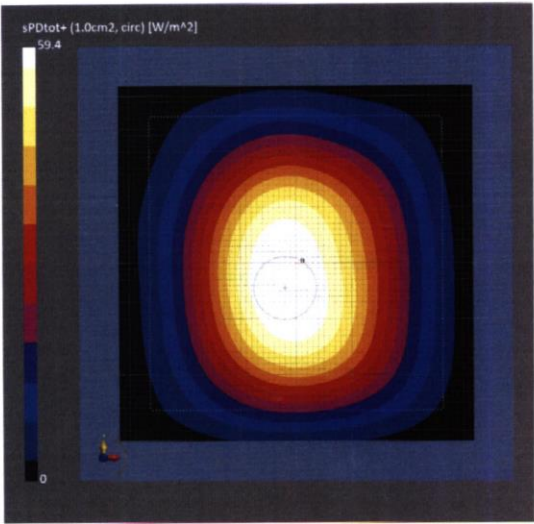

DASY Report

Measurement Report for 5G Verification Source 10 GHz, UID 0 -, Channel 10000 (10000.0MHz)

Device under Test Properties

| Name, Manufacturer            | Dimensions [mm]       | IMEI     | DUT Type |
|-------------------------------|-----------------------|----------|----------|
| 5G Verification Source 10 GHz | 100.0 x 100.0 x 172.0 | SN: 1005 | -        |

Exposure Conditions

| Phantom Section | Position, Test Distance [mm] | Band            | Group, | Frequency [MHz], Channel Number | Conversion Factor |
|-----------------|------------------------------|-----------------|--------|---------------------------------|-------------------|
| 5G -            | 10.0 mm                      | Validation band | CW     | 10000.0, 10000                  | 1.0               |

Hardware Setup


| Phantom               | Medium | Probe, Calibration Date               | DAE, Calibration Date   |
|-----------------------|--------|---------------------------------------|-------------------------|
| mmWave Phantom - 1002 | Air    | EUmmWV3 - SN9374_F1-55GHz, 2023-12-04 | DAE4 Sn1215, 2023-06-29 |

Scan Setup

| Sensor Surface [mm] | 5G Scan               |
|---------------------|-----------------------|
| MAIA                | 10.0<br>MAIA not used |

Measurement Results

|                                 | 5G Scan            |
|---------------------------------|--------------------|
| Date                            | 2024-01-18, 15:51  |
| Avg. Area [cm <sup>2</sup> ]    | 4.00               |
| Avg. Type                       | Circular Averaging |
| psPDn+ [W/m <sup>2</sup> ]      | 55.2               |
| psPDtot+ [W/m <sup>2</sup> ]    | 55.5               |
| psPDmod+ [W/m <sup>2</sup> ]    | 55.7               |
| Max(Sn) [W/m <sup>2</sup> ]     | 60.5               |
| Max(Stot) [W/m <sup>2</sup> ]   | 60.7               |
| Max( Stot ) [W/m <sup>2</sup> ] | 60.9               |
| E <sub>max</sub> [V/m]          | 151                |
| Power Drift [dB]                | -0.01              |

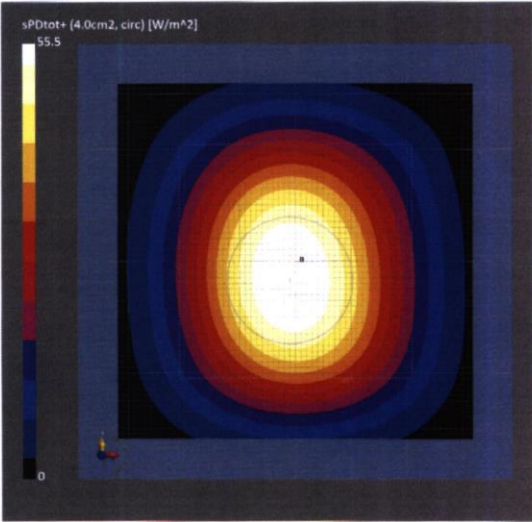

DASY Report

Measurement Report for 5G Verification Source 10 GHz, UID 0 -, Channel 10000 (10000.0MHz)

Device under Test Properties

| Name, Manufacturer            | Dimensions [mm]       | IMEI     | DUT Type |
|-------------------------------|-----------------------|----------|----------|
| 5G Verification Source 10 GHz | 100.0 x 100.0 x 172.0 | SN: 1005 | -        |

Exposure Conditions

| Phantom Section | Position, Test Distance [mm] | Band            | Group, | Frequency [MHz], Channel Number | Conversion Factor |
|-----------------|------------------------------|-----------------|--------|---------------------------------|-------------------|
| 5G -            | 10.0 mm                      | Validation band | CW     | 10000.0, 10000                  | 1.0               |

Hardware Setup


| Phantom               | Medium | Probe, Calibration Date               | DAE, Calibration Date   |
|-----------------------|--------|---------------------------------------|-------------------------|
| mmWave Phantom - 1002 | Air    | EUmmWV3 - SN9374_F1-55GHz, 2023-12-04 | DAE4 Sn1215, 2023-06-29 |

Scan Setup

| Sensor Surface [mm] | 5G Scan               |
|---------------------|-----------------------|
| MAIA                | 10.0<br>MAIA not used |

Measurement Results

| Date                            | 5G Scan          |
|---------------------------------|------------------|
| 2024-01-18, 15:51               | 1.00             |
| Avg. Area [cm <sup>2</sup> ]    | Square Averaging |
| Avg. Type                       | 59.1             |
| psPDn+ [W/m <sup>2</sup> ]      | 59.4             |
| psPDtot+ [W/m <sup>2</sup> ]    | 59.6             |
| psPDmod+ [W/m <sup>2</sup> ]    | 60.5             |
| Max(Sn) [W/m <sup>2</sup> ]     | 60.7             |
| Max(Stot) [W/m <sup>2</sup> ]   | 60.9             |
| Max( Stot ) [W/m <sup>2</sup> ] | 151              |
| E <sub>max</sub> [V/m]          | -0.01            |
| Power Drift [dB]                |                  |

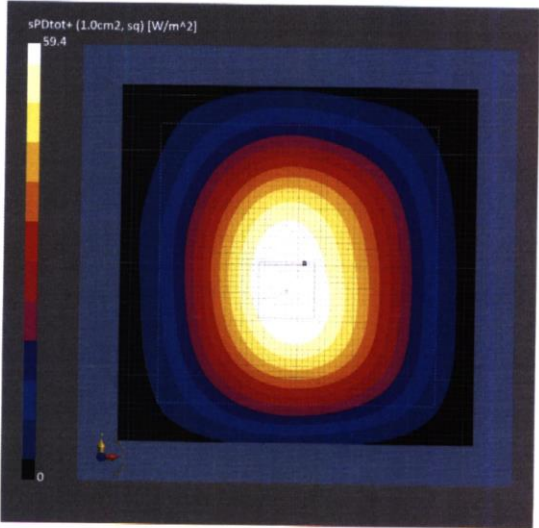

DASY Report

Measurement Report for 5G Verification Source 10 GHz, UID 0 -, Channel 10000 (10000.0MHz)

Device under Test Properties

| Name, Manufacturer            | Dimensions [mm]       | IMEI     | DUT Type |
|-------------------------------|-----------------------|----------|----------|
| 5G Verification Source 10 GHz | 100.0 x 100.0 x 172.0 | SN: 1005 | -        |

Exposure Conditions

| Phantom Section | Position, Test Distance [mm] | Band            | Group, | Frequency [MHz], Channel Number | Conversion Factor |
|-----------------|------------------------------|-----------------|--------|---------------------------------|-------------------|
| 5G -            | 10.0 mm                      | Validation band | CW     | 10000.0, 10000                  | 1.0               |

Hardware Setup


| Phantom               | Medium | Probe, Calibration Date               | DAE, Calibration Date   |
|-----------------------|--------|---------------------------------------|-------------------------|
| mmWave Phantom - 1002 | Air    | EUmmWV3 - SN9374_F1-55GHz, 2023-12-04 | DAE4 Sn1215, 2023-06-29 |

Scan Setup

| Sensor Surface [mm] | 5G Scan               |
|---------------------|-----------------------|
| MAIA                | 10.0<br>MAIA not used |

Measurement Results

|                                 | 5G Scan           |
|---------------------------------|-------------------|
| Date                            | 2024-01-18, 15:51 |
| Avg. Area [cm <sup>2</sup> ]    | 4.00              |
| Avg. Type                       | Square Averaging  |
| psPDn+ [W/m <sup>2</sup> ]      | 55.1              |
| psPDtot+ [W/m <sup>2</sup> ]    | 55.4              |
| psPDmod+ [W/m <sup>2</sup> ]    | 55.7              |
| Max(Sn) [W/m <sup>2</sup> ]     | 60.5              |
| Max(Stot) [W/m <sup>2</sup> ]   | 60.7              |
| Max( Stot ) [W/m <sup>2</sup> ] | 60.9              |
| E <sub>max</sub> [V/m]          | 151               |
| Power Drift [dB]                | -0.01             |

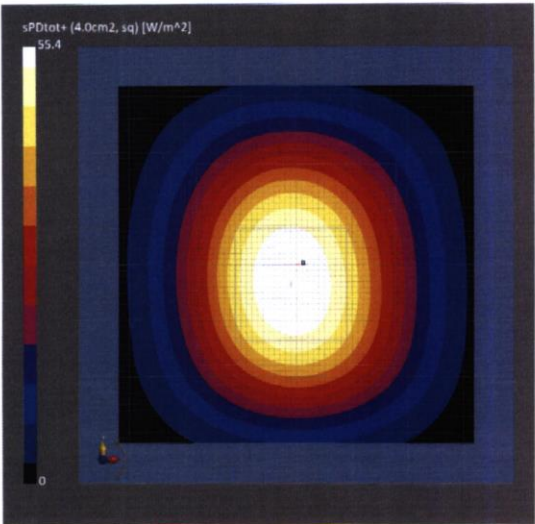

ANNEX I    Accreditation Certificate



Accredited Laboratory

A2LA has accredited

TELECOMMUNICATION TECHNOLOGY LABS, CAICT

Beijing, People's Republic of China

for technical competence in the field of

Electrical Testing

This laboratory is accredited in accordance with the recognized International Standard ISO/IEC 17025:2017 *General requirements for the competence of testing and calibration laboratories*. This accreditation demonstrates technical competence for a defined scope and the operation of a laboratory quality management system (refer to joint ISO-ILAC-IAF Communiqué dated April 2017).



Presented this 23<sup>rd</sup> day of July 2024.

A blue ink signature of Mr. Trace McInturf.

Mr. Trace McInturf, Vice President, Accreditation Services  
For the Accreditation Council  
Certificate Number 7049.01  
Valid to July 31, 2026

*For the tests to which this accreditation applies, please refer to the laboratory's Electrical Scope of Accreditation.*