

Date: 2025-01-24

System Check_Head_2450MHz**DUT: D2450V2 - SN806**

Communication System: CW; Frequency: 2450.000 MHz

Medium: HSL_2450_250124 Medium parameters used: $f = 2450.000$ MHz; $\sigma = 1.81$ S/m; $\epsilon_r = 39.0$

Ambient Temperature: 23.6°C; Liquid Temperature: 22.6°C

DASY6 Configuration:

- Probe: EX3DV4 - SN7814; ConvF(7.01, 6.71, 6.88); Calibrated: 2024-06-20
- Sensor-Surface: 1.4 mm
- Electronics: DAE4 Sn1424; Calibrated: 2024-12-19
- Phantom: ELI V5.0 (20deg probe tilt); Serial: 1227; Section: Flat
- Measurement Software: 16.2.4.2524
- UID: CW, 0--

Pin=17.0dBm/Area Scan (40.0 mm x 80.0 mm): Measurement Grid: 10.0 mm x 10.0 mm

SAR (1g) = 2.65 W/kg; SAR (10g) = 1.22 W/kg;


Pin=17.0dBm/Zoom Scan (30.0 mm x 30.0 mm x 30.0 mm): Measurement Grid: 5.0 mm x 5.0 mm x 1.5 mm

Power Drift = -0.06 dB

SAR (1g) = 2.59 W/kg; SAR (8g) = 1.36 W/kg; SAR (10g) = 1.23 W/kg

Smallest distance from peaks to all points 3 dB below = 9.0 mm

Ratio of SAR at M2 to SAR at M1 = 81.8 %

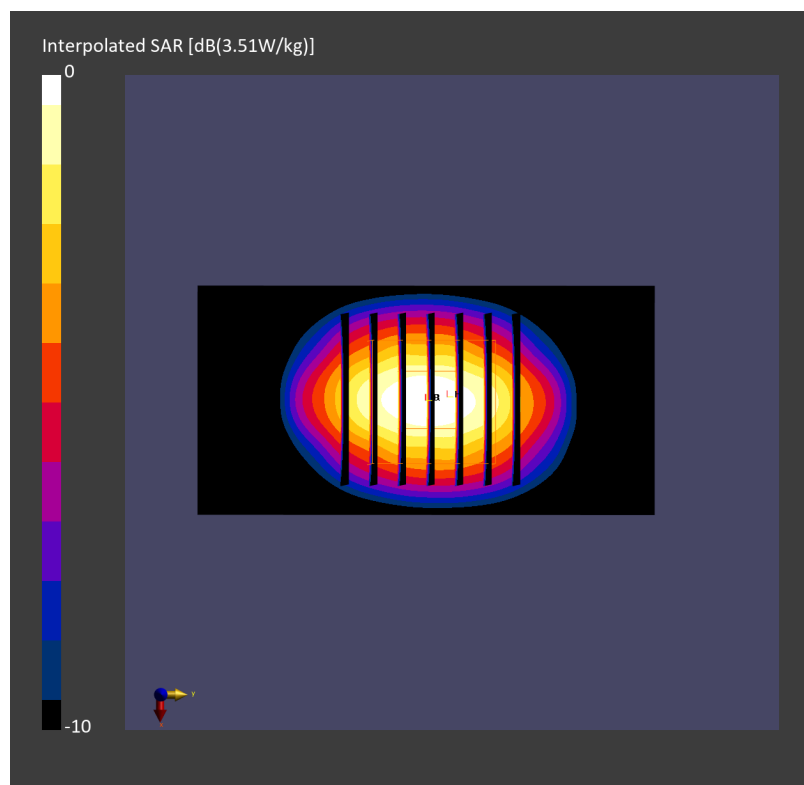

Date: 2025-01-30

System Check_Head_2450MHz**DUT: D2450V2 - SN929**

Communication System: CW; Frequency: 2450.000 MHz

Medium: HSL_2450_250130 Medium parameters used: $f = 2450.000$ MHz; $\sigma = 1.81$ S/m; $\epsilon_r = 39.9$

Ambient Temperature: 23.2°C; Liquid Temperature: 22.2°C

DASY6 Configuration:

- Probe: EX3DV4 - SN3931; ConvF(7.2, 6.94, 6.84); Calibrated: 2024-11-19
- Sensor-Surface: 1.4 mm
- Electronics: DAE4 Sn703; Calibrated: 2024-04-22
- Phantom: ELI V8.0 (20deg probe tilt); Serial: 2055; Section: Flat
- Measurement Software: 16.2.4.2524
- UID: CW, 0--

Pin=24.0dBm/Area Scan (40.0 mm x 80.0 mm): Measurement Grid: 10.0 mm x 10.0 mm

SAR (1g) = 13.6 W/kg; SAR (10g) = 6.29 W/kg;


Pin=24.0dBm/Zoom Scan (30.0 mm x 30.0 mm x 30.0 mm): Measurement Grid: 5.0 mm x 5.0 mm x 1.5 mm

Power Drift = 0.00 dB

SAR (1g) = 13.4 W/kg; SAR (8g) = 6.94 W/kg; SAR (10g) = 6.29 W/kg

Smallest distance from peaks to all points 3 dB below = 9.0 mm

Ratio of SAR at M2 to SAR at M1 = 82.1 %

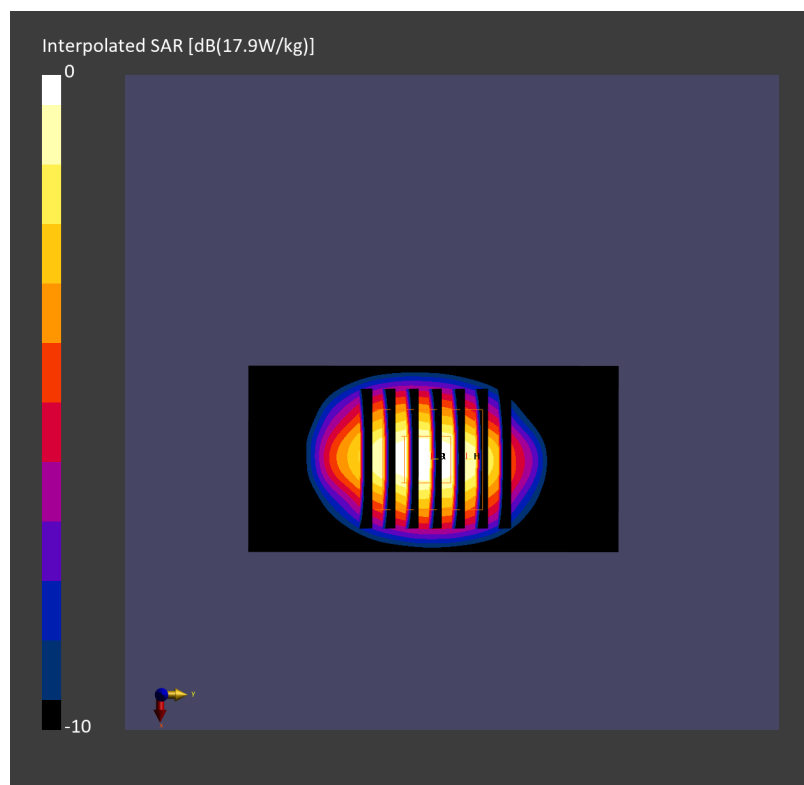

Date: 2025-01-23

System Check_Head_5250MHz**DUT: D5GHzV2 - SN1006**

Communication System: CW; Frequency: 5250.000 MHz

Medium: HSL_5250_250123 Medium parameters used: $f = 5250.000$ MHz; $\sigma = 4.70$ S/m; $\epsilon_r = 35.8$

Ambient Temperature: 23.3°C; Liquid Temperature: 22.3°C

DASY6 Configuration:

- Probe: EX3DV4 - SN3931; ConvF(5.49, 5.29, 5.21); Calibrated: 2024-11-19
- Sensor-Surface: 1.4 mm
- Electronics: DAE4 Sn703; Calibrated: 2024-04-22
- Phantom: ELI V8.0 (20deg probe tilt); Serial: 2055; Section: Flat
- Measurement Software: 16.2.4.2524
- UID: CW, 0--

Pin=17.0dBm/Area Scan (40.0 mm x 80.0 mm): Measurement Grid: 10.0 mm x 10.0 mm

SAR (1g) = 3.47 W/kg; SAR (10g) = 0.980 W/kg;


Pin=17.0dBm/Zoom Scan (22.0 mm x 22.0 mm x 22.0 mm): Measurement Grid: 4.0 mm x 4.0 mm x 1.4 mm

Power Drift = -0.02 dB

SAR (1g) = 3.71 W/kg; SAR (8g) = 1.22 W/kg; SAR (10g) = 1.04 W/kg

Smallest distance from peaks to all points 3 dB below = 7.3 mm

Ratio of SAR at M2 to SAR at M1 = 61.4 %

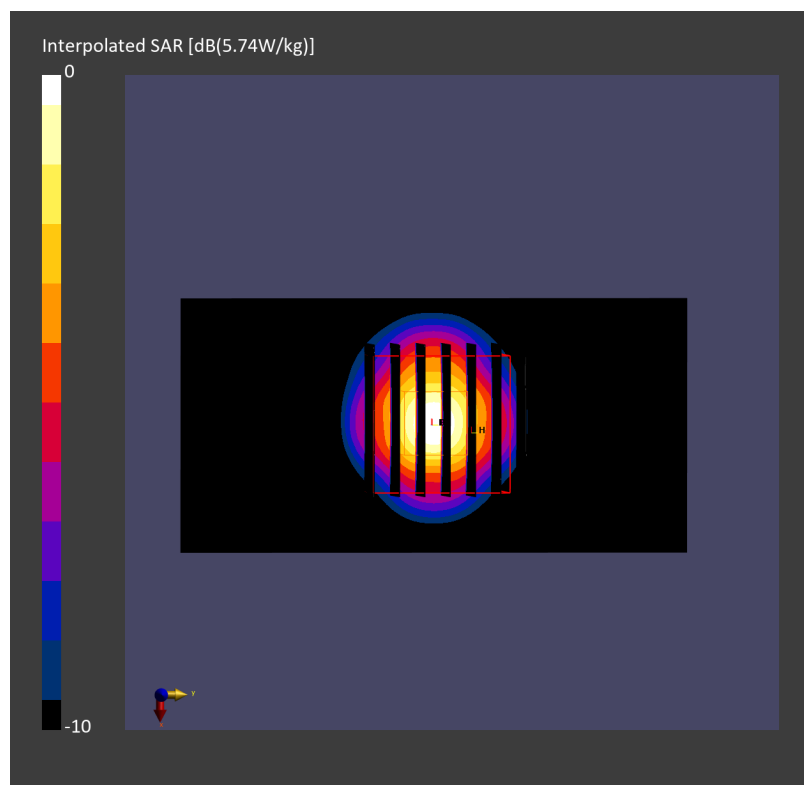

Date: 2025-01-23

System Check_Head_5600MHz**DUT: D5GHzV2 - SN1006**

Communication System: CW; Frequency: 5600.000 MHz

Medium: HSL_5600_250123 Medium parameters used: $f = 5600.000$ MHz; $\sigma = 5.10$ S/m; $\epsilon_r = 35.2$

Ambient Temperature: 23.3°C; Liquid Temperature: 22.3°C

DASY6 Configuration:

- Probe: EX3DV4 - SN3931; ConvF(5.11, 4.92, 4.85); Calibrated: 2024-11-19
- Sensor-Surface: 1.4 mm
- Electronics: DAE4 Sn703; Calibrated: 2024-04-22
- Phantom: ELI V8.0 (20deg probe tilt); Serial: 2055; Section: Flat
- Measurement Software: 16.2.4.2524
- UID: CW, 0--

Pin=17.0dBm/Area Scan (40.0 mm x 80.0 mm): Measurement Grid: 10.0 mm x 10.0 mm

SAR (1g) = 3.63 W/kg; SAR (10g) = 1.02 W/kg;


Pin=17.0dBm/Zoom Scan (22.0 mm x 22.0 mm x 22.0 mm): Measurement Grid: 4.0 mm x 4.0 mm x 1.4 mm

Power Drift = -0.01 dB

SAR (1g) = 3.94 W/kg; SAR (8g) = 1.29 W/kg; SAR (10g) = 1.10 W/kg

Smallest distance from peaks to all points 3 dB below = 7.4 mm

Ratio of SAR at M2 to SAR at M1 = 57.6 %

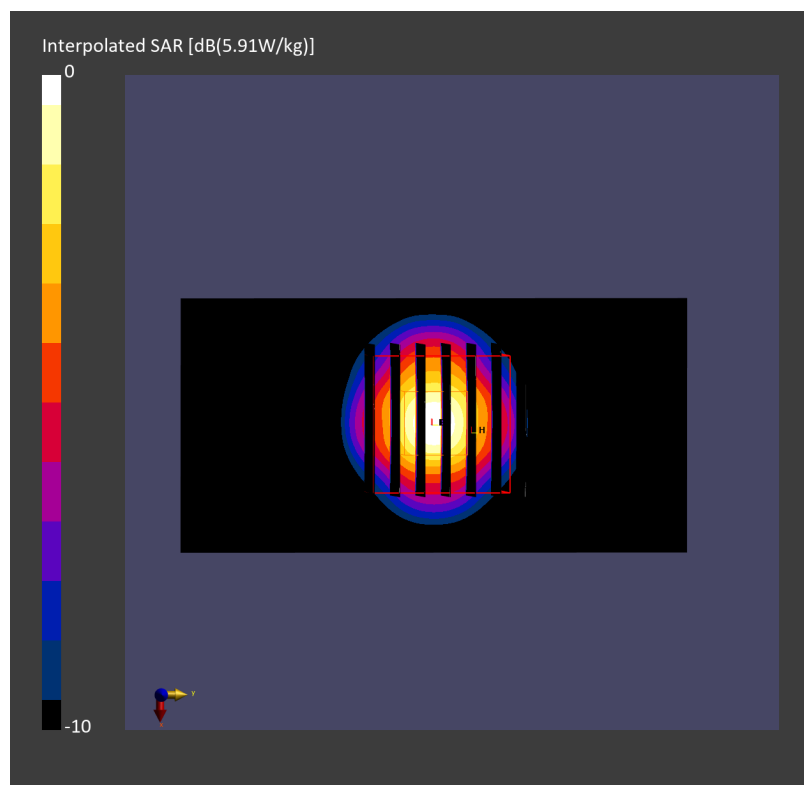

Date: 2025-01-23

System Check_Head_5800MHz**DUT: D5GHzV2 - SN1006**

Communication System: CW; Frequency: 5800.000 MHz

Medium: HSL_5800_250123 Medium parameters used: $f = 5800.000$ MHz; $\sigma = 5.35$ S/m; $\epsilon_r = 34.8$

Ambient Temperature: 23.3°C; Liquid Temperature: 22.3°C

DASY6 Configuration:

- Probe: EX3DV4 - SN3931; ConvF(5.01, 4.83, 4.76); Calibrated: 2024-11-19
- Sensor-Surface: 1.4 mm
- Electronics: DAE4 Sn703; Calibrated: 2024-04-22
- Phantom: ELI V8.0 (20deg probe tilt); Serial: 2055; Section: Flat
- Measurement Software: 16.2.4.2524
- UID: CW, 0--

Pin=17.0dBm/Area Scan (40.0 mm x 80.0 mm): Measurement Grid: 10.0 mm x 10.0 mm

SAR (1g) = 3.58 W/kg; SAR (10g) = 1.01 W/kg;


Pin=17.0dBm/Zoom Scan (22.0 mm x 22.0 mm x 22.0 mm): Measurement Grid: 4.0 mm x 4.0 mm x 1.4 mm

Power Drift = -0.02 dB

SAR (1g) = 3.93 W/kg; SAR (8g) = 1.28 W/kg; SAR (10g) = 1.10 W/kg

Smallest distance from peaks to all points 3 dB below = 7.6 mm

Ratio of SAR at M2 to SAR at M1 = 54.9 %

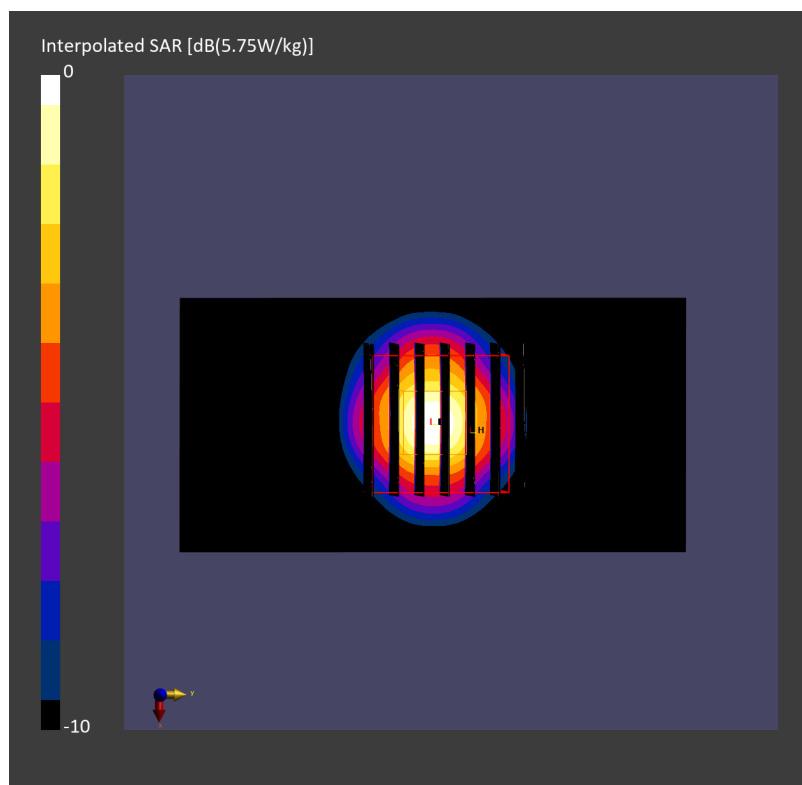

Date: 2025-01-28

System Check_Head_6500MHz**DUT: D6.5GHzV2 - SN1003**

Communication System: CW; Frequency: 6500.000 MHz

Medium: HSL_6500_250128 Medium parameters used: $f = 6500.000$ MHz; $\sigma = 6.04$ S/m; $\epsilon_r = 35.1$

Ambient Temperature: 23.4°C; Liquid Temperature: 22.4°C

DASY6 Configuration:

- Probe: EX3DV4 - SN3931; ConvF(5.52, 5.32, 5.24); Calibrated: 2024-11-19
- Sensor-Surface: 1.4 mm
- Electronics: DAE4 Sn703; Calibrated: 2024-04-22
- Phantom: ELI V8.0 (20deg probe tilt); Serial: 2055; Section: Flat
- Measurement Software: 16.2.4.2524
- UID: CW, 0--

Pin=20.0dBm/Area Scan (51.0 mm x 85.0 mm): Measurement Grid: 8.5 mm x 8.5 mm

SAR (1g) = 23.4 W/kg; SAR (10g) = 4.66 W/kg;

Pin=20.0dBm/Zoom Scan (22.0 mm x 22.0 mm x 22.0 mm): Measurement Grid: 3.4 mm x 3.4 mm x 1.4 mm

Power Drift = -0.02 dB

SAR (1g) = 28.4 W/kg; SAR (8g) = 6.29 W/kg; SAR (10g) = 5.14 W/kg

Smallest distance from peaks to all points 3 dB below = 4.6 mm

Ratio of SAR at M2 to SAR at M1 = 48.7 %

psAPD (1.0cm², sq) = 284 [W/m²]; psAPD (4.0cm², sq) = 126 [W/m²]