

Date: 2025-01-02

System Check_Head_2450MHz**DUT: D2450V2 - SN806**

Communication System: CW; Frequency: 2450.000 MHz

Medium: HSL_2450_250102 Medium parameters used: $f = 2450.000$ MHz; $\sigma = 1.83$ S/m; $\epsilon_r = 38.8$

Ambient Temperature: 23.3°C; Liquid Temperature: 22.3°C

DASY6 Configuration:

- Probe: EX3DV4 - SN7694; ConvF(7.27, 7.09, 7.93); Calibrated: 2024-11-18
- Sensor-Surface: 1.4 mm
- Electronics: DAE4 Sn1697; Calibrated: 2024-11-14
- Phantom: ELI V8.0 (20deg probe tilt); Serial: 2055_for Gap; Section: Flat
- Measurement Software: 16.2.4.2524
- UID: CW, 0--

Pin=17.0dBm/Area Scan (40.0 mm x 80.0 mm): Measurement Grid: 10.0 mm x 10.0 mm

SAR (1g) = 2.30 W/kg; SAR (10g) = 1.07 W/kg;


Pin=17.0dBm/Zoom Scan (30.0 mm x 30.0 mm x 30.0 mm): Measurement Grid: 5.0 mm x 5.0 mm x 1.5 mm

Power Drift = -0.09 dB

SAR (1g) = 2.42 W/kg; SAR (8g) = 1.21 W/kg; SAR (10g) = 1.12 W/kg

Smallest distance from peaks to all points 3 dB below = 9.0 mm

Ratio of SAR at M2 to SAR at M1 = 81.0 %

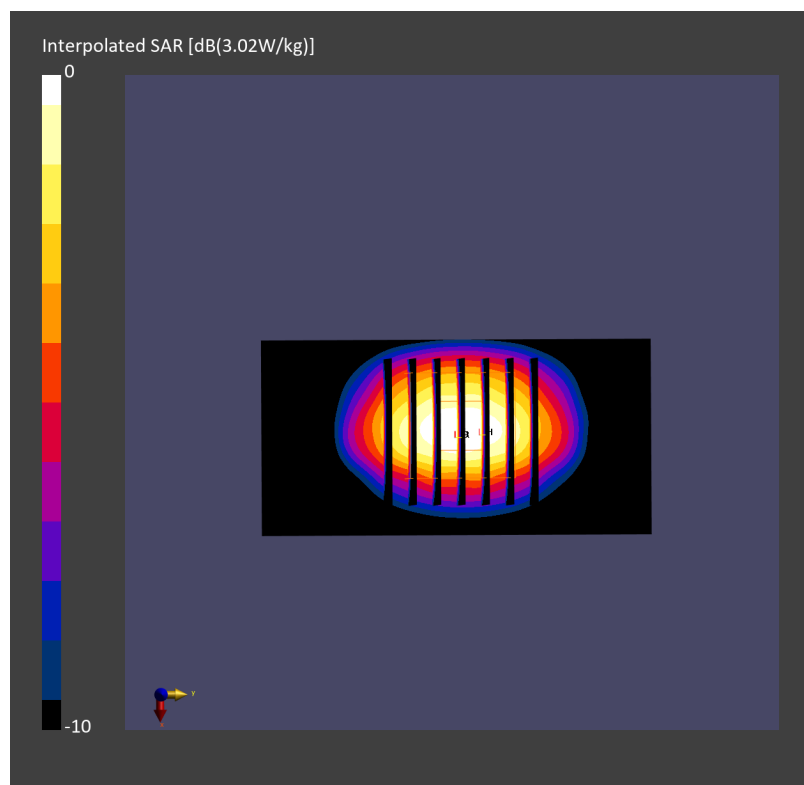

Date: 2025-01-07

System Check_Head_2450MHz**DUT: D2450V2 - SN806**

Communication System: CW; Frequency: 2450.000 MHz

Medium: HSL_2450_250107 Medium parameters used: $f = 2450.000$ MHz; $\sigma = 1.80$ S/m; $\epsilon_r = 38.7$

Ambient Temperature: 23.3°C; Liquid Temperature: 22.3°C

DASY6 Configuration:

- Probe: EX3DV4 - SN7814; ConvF(7.01, 6.71, 6.88); Calibrated: 2024-06-20
- Sensor-Surface: 1.4 mm
- Electronics: DAE4 Sn1424; Calibrated: 2024-12-19
- Phantom: ELI V5.0 (20deg probe tilt); Serial: 1227; Section: Flat
- Measurement Software: 16.2.4.2524
- UID: CW, 0--

Pin=17.0dBm/Area Scan (40.0 mm x 80.0 mm): Measurement Grid: 10.0 mm x 10.0 mm

SAR (1g) = 2.60 W/kg; SAR (10g) = 1.21 W/kg;


Pin=17.0dBm/Zoom Scan (30.0 mm x 30.0 mm x 30.0 mm): Measurement Grid: 5.0 mm x 5.0 mm x 1.5 mm

Power Drift = 0.01 dB

SAR (1g) = 2.57 W/kg; SAR (8g) = 1.35 W/kg; SAR (10g) = 1.22 W/kg

Smallest distance from peaks to all points 3 dB below = 9.0 mm

Ratio of SAR at M2 to SAR at M1 = 82.2 %

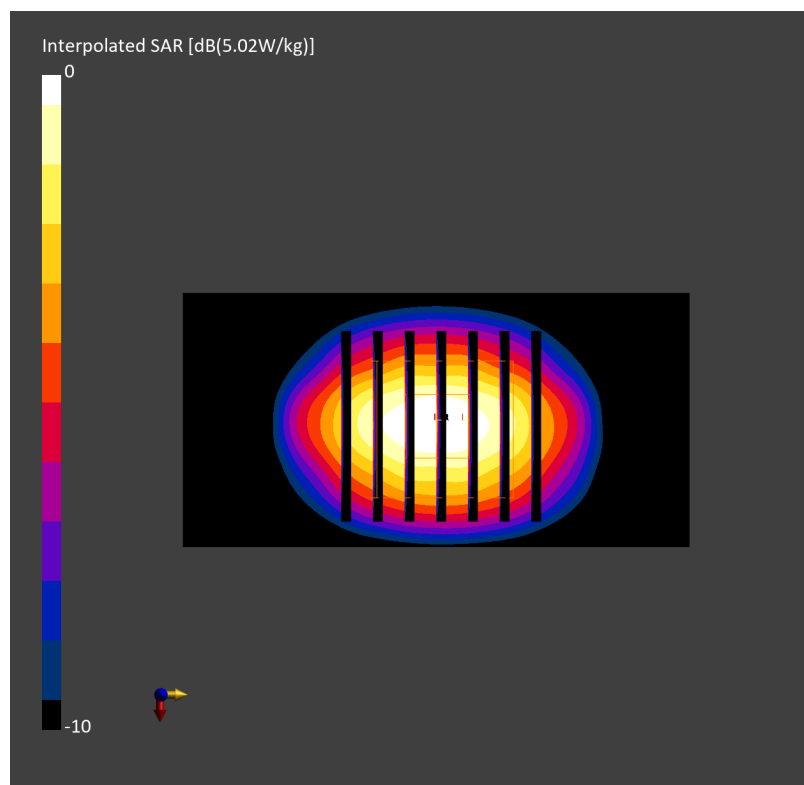

Date: 2024-12-30

System Check_Head_5250MHz**DUT: D5GHzV2 - SN1006**

Communication System: CW; Frequency: 5250.000 MHz

Medium: HSL_5G_241230 Medium parameters used: $f=5250.000$ MHz; $\sigma=4.71$ S/m; $\epsilon_r=36.4$

Ambient Temperature: 23.5°C; Liquid Temperature: 22.5°C

DASY8 Configuration:

- Probe: EX3DV4 - SN7814; ConvF(5.59, 5.35, 5.48); Calibrated: 2024-06-20
- Sensor-Surface: 1.4 mm
- Electronics: DAE4ip Sn1800; Calibrated: 2024-06-18
- Phantom: ELI V8.0 (20deg probe tilt); Serial: 2204; Section: Flat
- Measurement Software: 16.2.4.2524
- UID: CW, 0

Pin=20.0dBm/Area Scan (40.0 mm x 80.0 mm): Measurement Grid: 10.0 mm x 10.0 mm

SAR (1g) = 7.50 W/kg; SAR (10g) = 2.36 W/kg;


Pin=20.0dBm/Zoom Scan (22.0 mm x 22.0 mm x 22.0 mm): Measurement Grid: 4.0 mm x 4.0 mm x 1.4 mm

Power Drift = -0.02 dB

SAR (1g) = 8.77 W/kg; SAR (8g) = 2.88 W/kg; SAR (10g) = 2.46 W/kg

Smallest distance from peaks to all points 3 dB below = 7.2 mm

Ratio of SAR at M2 to SAR at M1 = 62.1 %

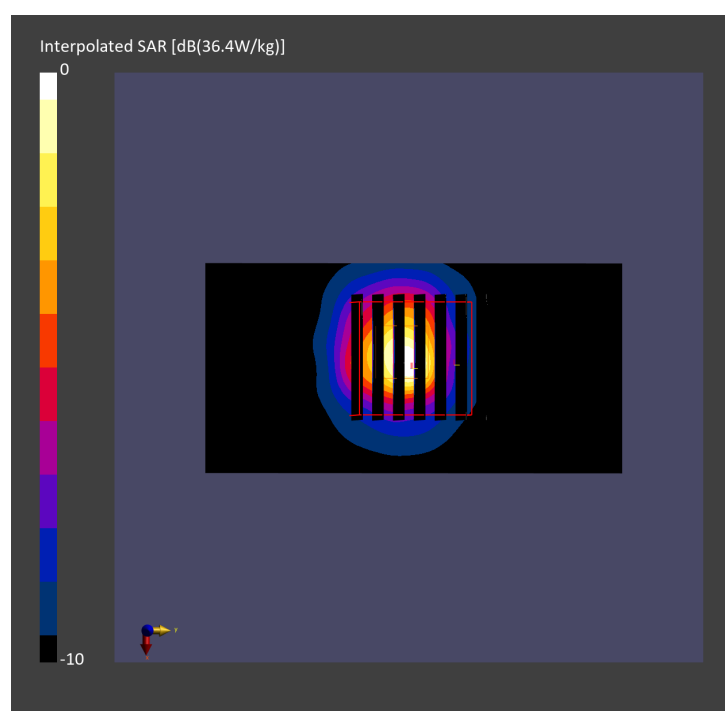

Date: 2025-01-02

System Check_Head_5250MHz**DUT: D5GHzV2 - SN1006**

Communication System: CW; Frequency: 5250.000 MHz

Medium: HSL_5G_250102 Medium parameters used: $f = 5250.000$ MHz; $\sigma = 4.86$ S/m; $\epsilon_r = 36.8$

Ambient Temperature: 23.3°C; Liquid Temperature: 22.3°C

DASY6 Configuration:

- Probe: EX3DV4 - SN7694; ConvF(5.25, 5.13, 5.73); Calibrated: 2024-11-18
- Sensor-Surface: 1.4 mm
- Electronics: DAE4 Sn1697; Calibrated: 2024-11-14
- Phantom: ELI V8.0 (20deg probe tilt); Serial: 2055_for Gap; Section: Flat
- Measurement Software: 16.2.4.2524
- UID: CW, 0--

Pin=17.0dBm/Area Scan (40.0 mm x 80.0 mm): Measurement Grid: 10.0 mm x 10.0 mm

SAR (1g) = 3.06 W/kg; SAR (10g) = 1.05 W/kg;


Pin=17.0dBm/Zoom Scan (22.0 mm x 22.0 mm x 22.0 mm): Measurement Grid: 4.0 mm x 4.0 mm x 1.4 mm

Power Drift = -0.08 dB

SAR (1g) = 3.77 W/kg; SAR (8g) = 1.33 W/kg; SAR (10g) = 1.08 W/kg

Smallest distance from peaks to all points 3 dB below = 7.2 mm

Ratio of SAR at M2 to SAR at M1 = 61.0 %

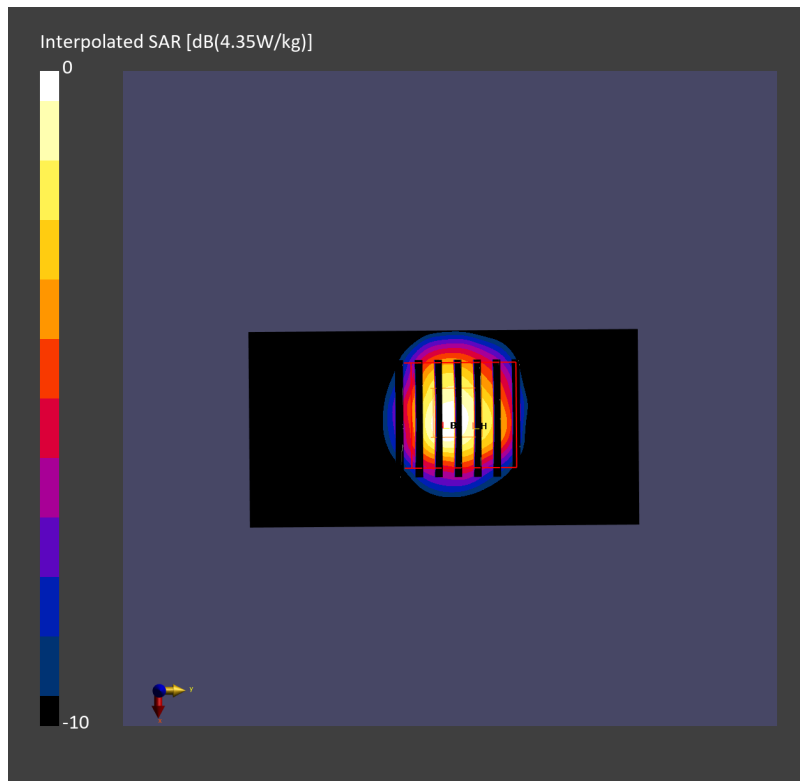

Date: 2025-01-08

System Check_Head_5250MHz**DUT: D5GHzV2 - SN1006**

Communication System: CW; Frequency: 5250.000 MHz

Medium: HSL_5G_250108 Medium parameters used: $f = 5250.000$ MHz; $\sigma = 4.68$ S/m; $\epsilon_r = 37.0$

Ambient Temperature: 23.5°C; Liquid Temperature: 22.5°C

DASY8 Configuration:

- Probe: EX3DV4 - SN7590; ConvF(5.82, 5.53, 5.73); Calibrated: 2024-03-19
- Sensor-Surface: 1.4 mm
- Electronics: DAE4 Sn1776; Calibrated: 2024-02-13
- Phantom: ELI V8.0 (20deg probe tilt); Serial: 2157; Section: Flat
- Measurement Software: 16.2.4.2524
- UID: CW, 0--

Pin=20.0dBm/Area Scan (40.0 mm x 80.0 mm): Measurement Grid: 10.0 mm x 10.0 mm

SAR (1g) = 7.76 W/kg; SAR (10g) = 2.23 W/kg;


Pin=20.0dBm/Zoom Scan (22.0 mm x 22.0 mm x 22.0 mm): Measurement Grid: 4.0 mm x 4.0 mm x 1.4 mm

Power Drift = 0.00 dB

SAR (1g) = 8.16 W/kg; SAR (8g) = 2.76 W/kg; SAR (10g) = 2.36 W/kg

Smallest distance from peaks to all points 3 dB below = 7.4 mm

Ratio of SAR at M2 to SAR at M1 = 63.5 %

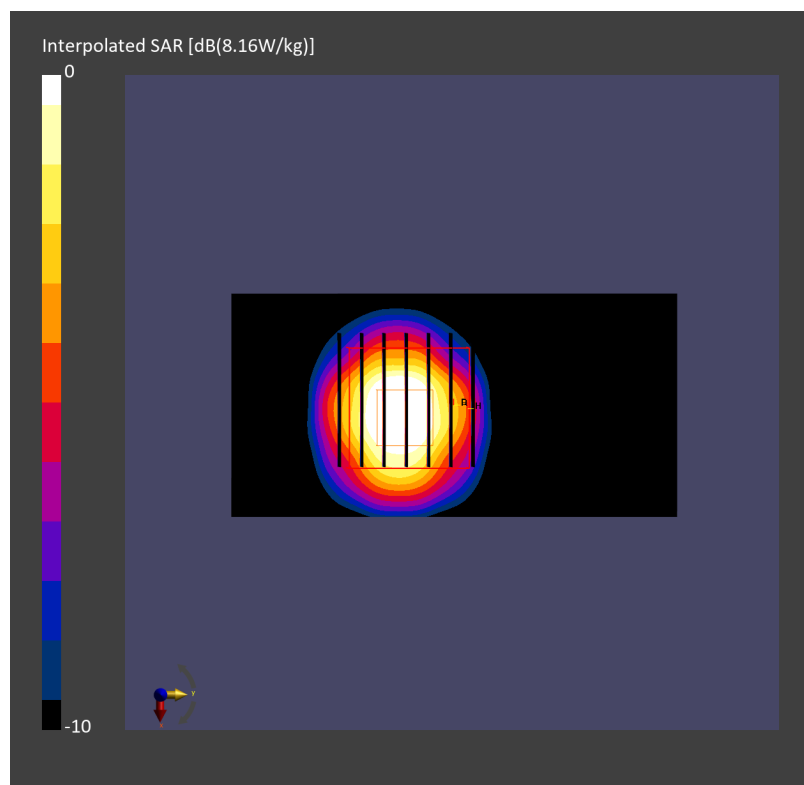

Date: 2025-01-02

System Check_Head_5600MHz**DUT: D5GHzV2 - SN1006**

Communication System: CW; Frequency: 5600.000 MHz

Medium: HSL_5G_250102 Medium parameters used: $f = 5600.000$ MHz; $\sigma = 5.25$ S/m; $\epsilon_r = 36.2$

Ambient Temperature: 23.3°C; Liquid Temperature: 22.3°C

DASY6 Configuration:

- Probe: EX3DV4 - SN7694; ConvF(4.9, 4.79, 5.35); Calibrated: 2024-11-18
- Sensor-Surface: 1.4 mm
- Electronics: DAE4 Sn1697; Calibrated: 2024-11-14
- Phantom: ELI V8.0 (20deg probe tilt); Serial: 2055_for Gap; Section: Flat
- Measurement Software: 16.2.4.2524
- UID: CW, 0--

Pin=17.0dBm/Area Scan (40.0 mm x 80.0 mm) : Measurement Grid: 10.0 mm x 10.0 mm

SAR (1g) = 4.02 W/kg; SAR (10g) = 1.15 W/kg;


Pin=17.0dBm/Zoom Scan (22.0 mm x 22.0 mm x 22.0 mm) : Measurement Grid: 4.0 mm x 4.0 mm x 1.4 mm

Power Drift = -0.05 dB

SAR (1g) = 4.31 W/kg; SAR (8g) = 1.42 W/kg; SAR (10g) = 1.22 W/kg

Smallest distance from peaks to all points 3 dB below = 7.2 mm

Ratio of SAR at M2 to SAR at M1 = 58.5 %

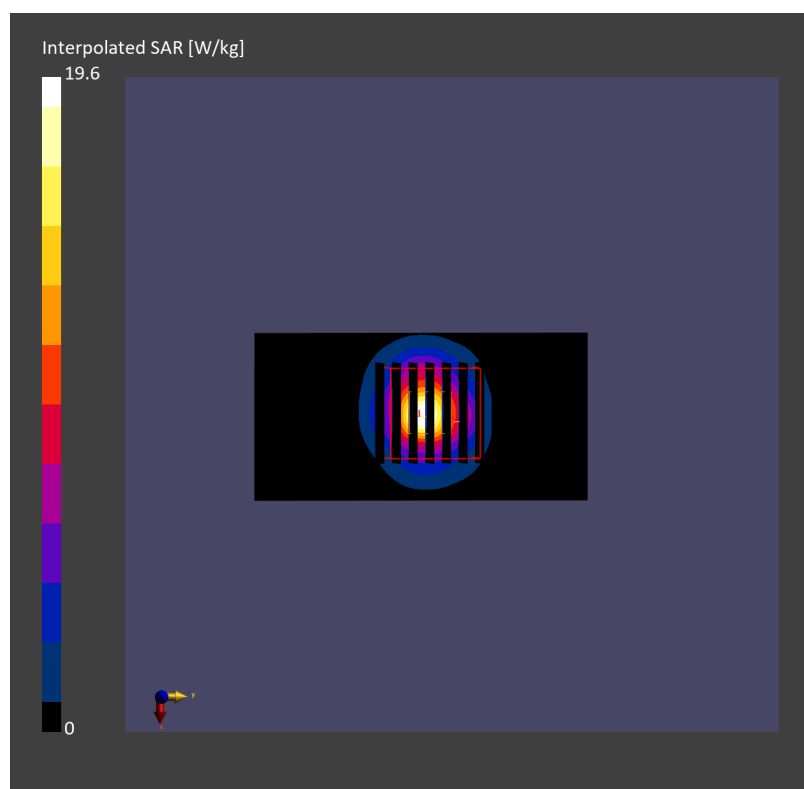

Date: 2025-01-08

System Check_Head_5600MHz**DUT: D5GHzV2 - SN1006**

Communication System: CW; Frequency: 5600.000 MHz

Medium: HSL_5G_250108 Medium parameters used: $f = 5600.000$ MHz; $\sigma = 5.10$ S/m; $\epsilon_r = 36.3$

Ambient Temperature: 23.5°C; Liquid Temperature: 22.5°C

DASY8 Configuration:

- Probe: EX3DV4 - SN7590; ConvF(4.86, 4.69, 4.82); Calibrated: 2024-03-19
- Sensor-Surface: 1.4 mm
- Electronics: DAE4 Sn1776; Calibrated: 2024-02-13
- Phantom: ELI V8.0 (20deg probe tilt); Serial: 2157; Section: Flat
- Measurement Software: 16.2.4.2524
- UID: CW, 0--

Pin=20.0dBm/Area Scan (40.0 mm x 80.0 mm): Measurement Grid: 10.0 mm x 10.0 mm

SAR (1g) = 7.97 W/kg; SAR (10g) = 2.29 W/kg;


Pin=20.0dBm/Zoom Scan (22.0 mm x 22.0 mm x 22.0 mm): Measurement Grid: 4.0 mm x 4.0 mm x 1.4 mm

Power Drift = -0.03 dB

SAR (1g) = 8.28 W/kg; SAR (8g) = 2.82 W/kg; SAR (10g) = 2.42 W/kg

Smallest distance from peaks to all points 3 dB below = 7.6 mm

Ratio of SAR at M2 to SAR at M1 = 62.3 %

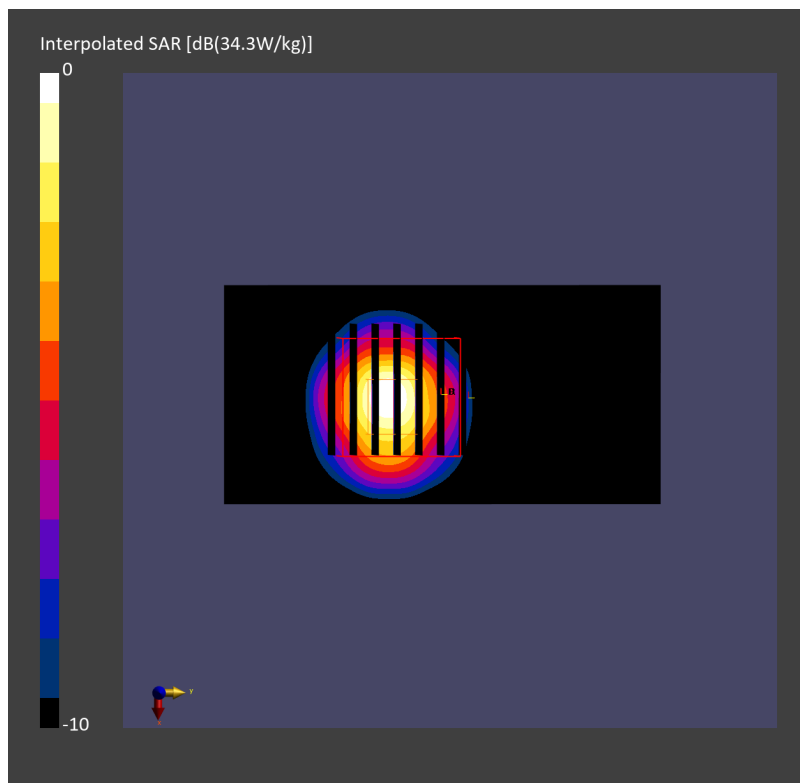

Date: 2024-12-30

System Check_Head_5800MHz**DUT: D5GHzV2 - SN1006**

Communication System: CW; Frequency: 5800.000 MHz

Medium: HSL_5G_241230 Medium parameters used: $f = 5800.000$ MHz; $\sigma = 5.30$ S/m; $\epsilon_r = 35.6$

Ambient Temperature: 23.5°C; Liquid Temperature: 22.5°C

DASY8 Configuration:

- Probe: EX3DV4 - SN7814; ConvF(5.02, 4.8, 4.92); Calibrated: 2024-06-20
- Sensor-Surface: 1.4 mm
- Electronics: DAE4ip Sn1800; Calibrated: 2024-06-18
- Phantom: ELI V8.0 (20deg probe tilt); Serial: 2204; Section: Flat
- Measurement Software: 16.2.4.2524
- UID: CW, 0

Pin=20.0dBm/Area Scan (40.0 mm x 80.0 mm): Measurement Grid: 10.0 mm x 10.0 mm

SAR (1g) = 7.29 W/kg; SAR (10g) = 2.25 W/kg;


Pin=20.0dBm/Zoom Scan (22.0 mm x 22.0 mm x 22.0 mm): Measurement Grid: 4.0 mm x 4.0 mm x 1.4 mm

Power Drift = -0.03 dB

SAR (1g) = 8.52 W/kg; SAR (8g) = 2.77 W/kg; SAR (10g) = 2.36 W/kg

Smallest distance from peaks to all points 3 dB below = 7.2 mm

Ratio of SAR at M2 to SAR at M1 = 58.8 %

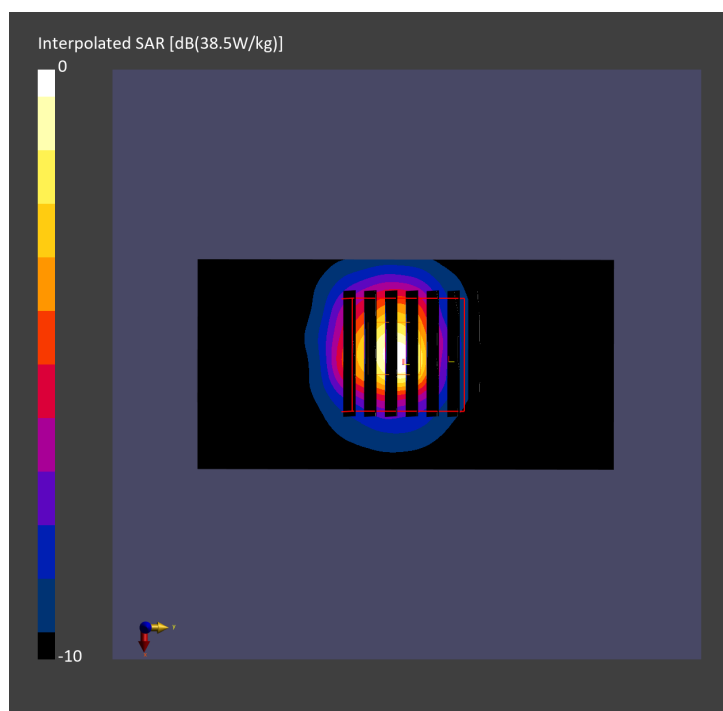

Date: 2025-01-02

System Check_Head_5800MHz**DUT: D5GHzV2 - SN1006**

Communication System: CW; Frequency: 5800.000 MHz

Medium: HSL_5G_250102 Medium parameters used: $f = 5800.000$ MHz; $\sigma = 5.47$ S/m; $\epsilon_r = 36.0$

Ambient Temperature: 23.3°C; Liquid Temperature: 22.3°C

DASY6 Configuration:

- Probe: EX3DV4 - SN7694; ConvF(4.82, 4.7, 5.25); Calibrated: 2024-11-18
- Sensor-Surface: 1.4 mm
- Electronics: DAE4 Sn1697; Calibrated: 2024-11-14
- Phantom: ELI V8.0 (20deg probe tilt); Serial: 2055_for Gap; Section: Flat
- Measurement Software: 16.2.4.2524
- UID: CW, 0--

Pin=17.0dBm/Area Scan (40.0 mm x 80.0 mm): Measurement Grid: 10.0 mm x 10.0 mm

SAR (1g) = 3.75 W/kg; SAR (10g) = 1.07 W/kg;


Pin=17.0dBm/Zoom Scan (22.0 mm x 22.0 mm x 22.0 mm): Measurement Grid: 4.0 mm x 4.0 mm x 1.4 mm

Power Drift = -0.00 dB

SAR (1g) = 4.03 W/kg; SAR (8g) = 1.32 W/kg; SAR (10g) = 1.13 W/kg

Smallest distance from peaks to all points 3 dB below = 7.2 mm

Ratio of SAR at M2 to SAR at M1 = 56.5 %

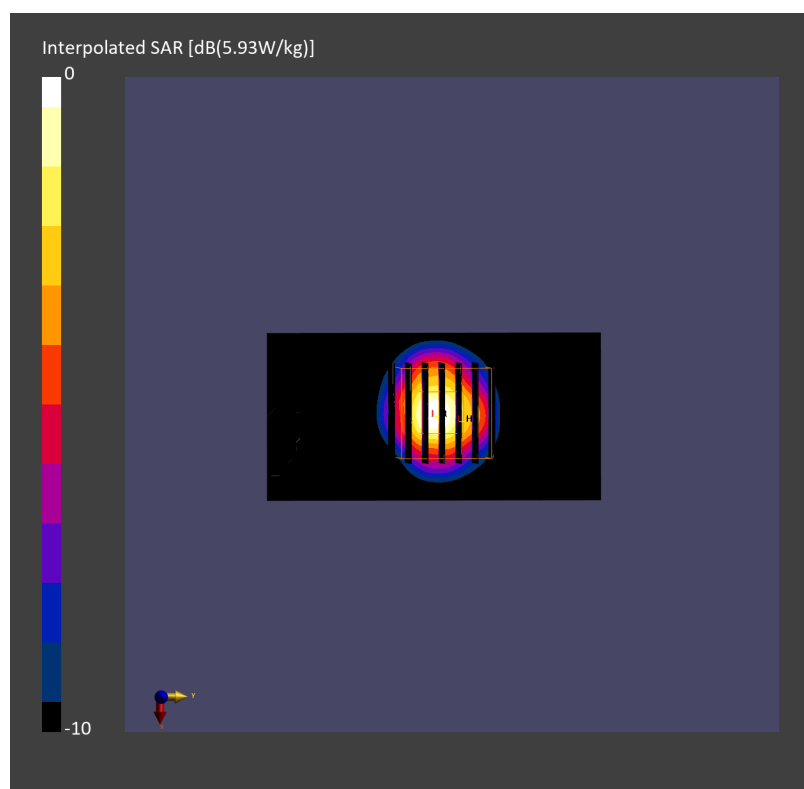

Date: 2025-01-08

System Check_Head_5800MHz**DUT: D5GHzV2 - SN1006**

Communication System: CW; Frequency: 5800.000 MHz

Medium: HSL_5G_250108 Medium parameters used: $f = 5800.000$ MHz; $\sigma = 5.20$ S/m; $\epsilon_r = 36.1$

Ambient Temperature: 23.5°C; Liquid Temperature: 22.5°C

DASY8 Configuration:

- Probe: EX3DV4 - SN7590; ConvF(5.05, 4.92, 5.06); Calibrated: 2024-03-19
- Sensor-Surface: 1.4 mm
- Electronics: DAE4 Sn1776; Calibrated: 2024-02-13
- Phantom: ELI V8.0 (20deg probe tilt); Serial: 2157; Section: Flat
- Measurement Software: 16.2.4.2524
- UID: CW, 0--

Pin=20.0dBm/Area Scan (40.0 mm x 80.0 mm): Measurement Grid: 10.0 mm x 10.0 mm

SAR (1g) = 7.86 W/kg; SAR (10g) = 2.23 W/kg;


Pin=20.0dBm/Zoom Scan (22.0 mm x 22.0 mm x 22.0 mm): Measurement Grid: 4.0 mm x 4.0 mm x 1.4 mm

Power Drift = 0.01 dB

SAR (1g) = 8.15 W/kg; SAR (8g) = 2.75 W/kg; SAR (10g) = 2.35 W/kg

Smallest distance from peaks to all points 3 dB below = 7.6 mm

Ratio of SAR at M2 to SAR at M1 = 60.8 %

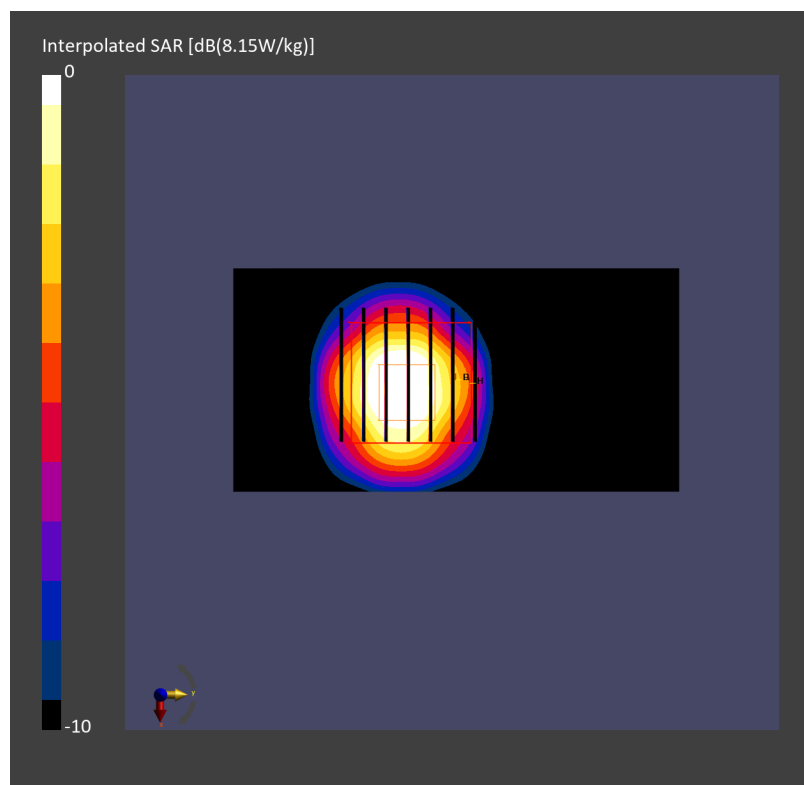

Date: 2025-01-02

System Check_Head_6500MHz**DUT: D6.5GHzV2 - SN1003**

Communication System: CW; Frequency: 6500.000 MHz

Medium: HSL_6G_250102 Medium parameters used: $f = 6500.000$ MHz; $\sigma = 5.93$ S/m; $\epsilon_r = 34.2$

Ambient Temperature: 23.5°C; Liquid Temperature: 22.5°C

DASY6 Configuration:

- Probe: EX3DV4 - SN7694; ConvF(5.62, 4.77, 5.35); Calibrated: 2024-11-18
- Sensor-Surface: 1.4 mm
- Electronics: DAE4 Sn1697; Calibrated: 2024-11-14
- Phantom: ELI V8.0 (20deg probe tilt); Serial: 2055_for Gap; Section: Flat
- Measurement Software: 16.2.4.2524
- UID: CW, 0--

Pin=20.0dBm/Area Scan (51.0 mm x 85.0 mm): Measurement Grid: 8.5 mm x 8.5 mm

SAR (1g) = 22.6 W/kg; SAR (10g) = 4.58 W/kg;


Pin=20.0dBm/Zoom Scan (22.0 mm x 22.0 mm x 22.0 mm): Measurement Grid: 3.4 mm x 3.4 mm x 1.4 mm

Power Drift = -0.10 dB

SAR (1g) = 26.9 W/kg; SAR (8g) = 5.93 W/kg; SAR (10g) = 4.86 W/kg

Smallest distance from peaks to all points 3 dB below = 4.4 mm

Ratio of SAR at M2 to SAR at M1 = 49.1 %

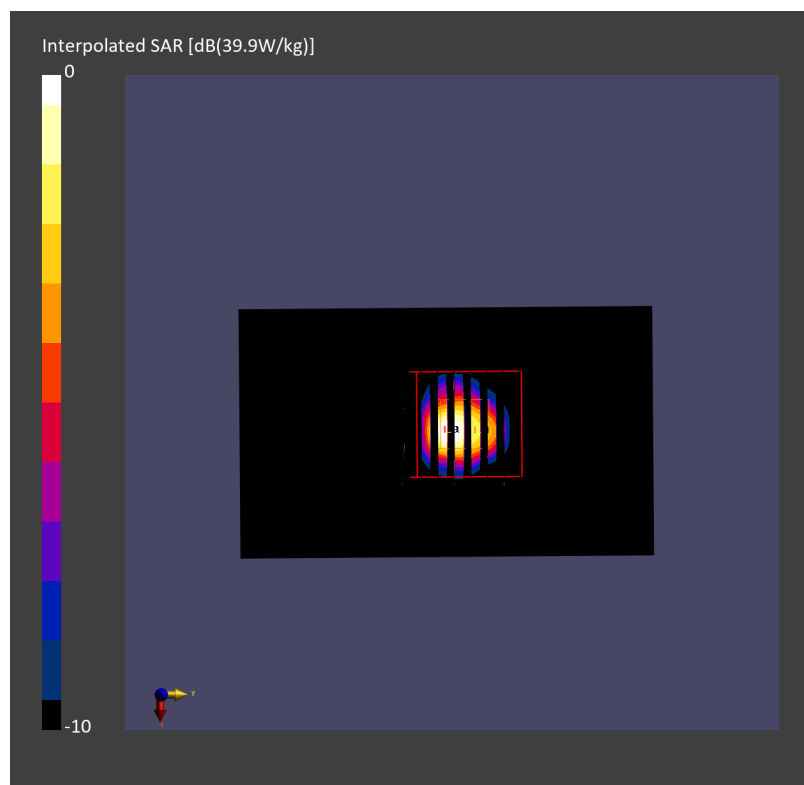psAPD (1.0cm², sq) = 269 [W/m²]; psAPD (4.0cm², sq) = 119 [W/m²]

Date: 2025-01-07

System Check_Head_6500MHz**DUT: D6.5GHzV2 - SN1003**

Communication System: CW; Frequency: 6500.000 MHz

Medium: HSL_6G_250107 Medium parameters used: $f = 6500.000$ MHz; $\sigma = 6.15$ S/m; $\epsilon_r = 34.84$

Ambient Temperature: 23.3°C; Liquid Temperature: 22.3°C

DASY6 Configuration:

- Probe: EX3DV4 - SN7814; ConvF(5.41, 5.18, 5.31); Calibrated: 2024-06-20
- Sensor-Surface: 1.4 mm
- Electronics: DAE4 Sn1424; Calibrated: 2024-12-19
- Phantom: ELI V5.0 (20deg probe tilt); Serial: 1227; Section: Flat
- Measurement Software: 16.2.4.2524
- UID: CW, 0--

Pin=20.0dBm/Area Scan (51.0 mm x 85.0 mm): Measurement Grid: 8.5 mm x 8.5 mm

SAR (1g) = 26.1 W/kg; SAR (10g) = 5.04 W/kg;

Pin=20.0dBm/Zoom Scan (22.0 mm x 22.0 mm x 22.0 mm): Measurement Grid: 3.4 mm x 3.4 mm x 1.4 mm

Power Drift = -0.01 dB

SAR (1g) = 28.8 W/kg; SAR (8g) = 6.41 W/kg; SAR (10g) = 5.26 W/kg

Smallest distance from peaks to all points 3 dB below = 4.8 mm

Ratio of SAR at M2 to SAR at M1 = 49.9 %

psAPD (1.0cm², sq) = 288 [W/m²]; psAPD (4.0cm², sq) = 128 [W/m²]