

Date: 2024-12-28

System Check_Head_2450MHz**DUT: D2450V2 - SN929**

Communication System: CW; Frequency: 2450.000 MHz

Medium: HSL_2450_241228 Medium parameters used: $f = 2450.000$ MHz; $\sigma = 1.82$ S/m; $\epsilon_r = 38.9$

Ambient Temperature: 23.8°C; Liquid Temperature: 22.8°C

DASY8 Configuration:

- Probe: EX3DV4 - SN3931; ConvF(7.2, 6.94, 6.84); Calibrated: 2024-11-19
- Sensor-Surface: 1.4 mm
- Electronics: DAE4 Sn703; Calibrated: 2024-04-22
- Phantom: ELI V8.0 (20deg probe tilt); Serial: 2205; Section: Flat
- Measurement Software: 16.2.4.2524
- UID: CW, 0

Pin=17.0dBm/Area Scan (40.0 mm x 80.0 mm): Measurement Grid: 10.0 mm x 10.0 mm

SAR (1g) = 2.44 W/kg; SAR (10g) = 1.15 W/kg;


Pin=17.0dBm/Zoom Scan (30.0 mm x 30.0 mm x 30.0 mm): Measurement Grid: 5.0 mm x 5.0 mm x 1.5 mm

Power Drift = -0.01 dB

SAR (1g) = 2.46 W/kg; SAR (8g) = 1.29 W/kg; SAR (10g) = 1.17 W/kg

Smallest distance from peaks to all points 3 dB below = 9.1 mm

Ratio of SAR at M2 to SAR at M1 = 82.0 %

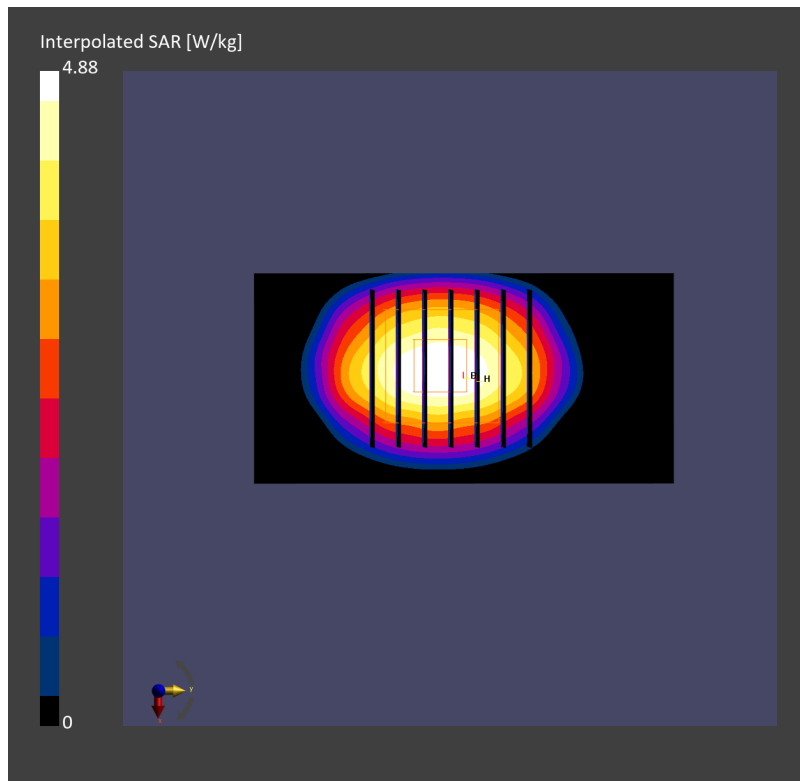

Date: 2024-12-25

System Check_Head_5250MHz**DUT: D5GHzV2 - SN1006**

Communication System: CW; Frequency: 5250.000 MHz

Medium: HSL_5G_241225 Medium parameters used: $f = 5250.000$ MHz; $\sigma = 4.67$ S/m; $\epsilon_r = 36.4$

Ambient Temperature: 23.5°C; Liquid Temperature: 22.5°C

DASY8 Configuration:

- Probe: EX3DV4 - SN7793; ConvF(4.89, 5.03, 5.05); Calibrated: 2024-03-01
- Sensor-Surface: 1.4 mm
- Electronics: DAE4 Sn1794; Calibrated: 2024-02-15
- Phantom: ELI V8.0 (20deg probe tilt); Serial: 2155; Section: Flat
- Measurement Software: 16.2.4.2524
- UID: CW, 0

Pin=20.0dBm/Area Scan (40.0 mm x 80.0 mm): Measurement Grid: 10.0 mm x 10.0 mm

SAR (1g) = 7.23 W/kg; SAR (10g) = 2.24 W/kg;


Pin=20.0dBm/Zoom Scan (22.0 mm x 22.0 mm x 22.0 mm): Measurement Grid: 4.0 mm x 4.0 mm x 1.4 mm

Power Drift = -0.01 dB

SAR (1g) = 8.35 W/kg; SAR (8g) = 2.80 W/kg; SAR (10g) = 2.40 W/kg

Smallest distance from peaks to all points 3 dB below = 7.2 mm

Ratio of SAR at M2 to SAR at M1 = 63.8 %

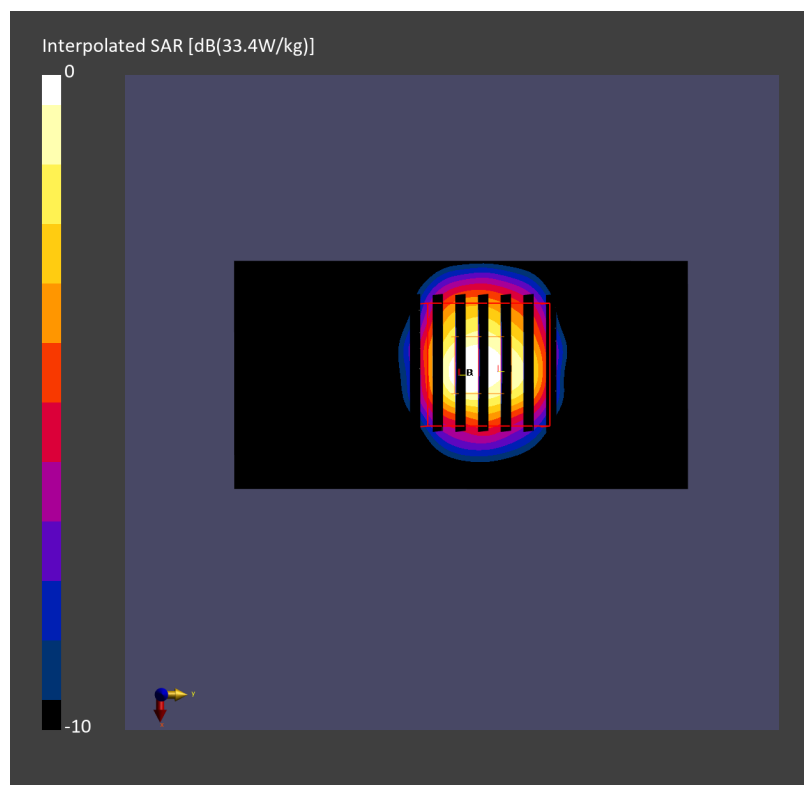

Date: 2024-12-26

System Check_Head_5250MHz**DUT: D5GHzV2 - SN1006**

Communication System: CW; Frequency: 5250.000 MHz

Medium: HSL_5G_241226 Medium parameters used: $f = 5250.000$ MHz; $\sigma = 4.58$ S/m; $\epsilon_r = 35.4$

Ambient Temperature: 23.6°C; Liquid Temperature: 22.6°C

DASY8 Configuration:

- Probe: EX3DV4 - SN3931; ConvF(5.49, 5.29, 5.21); Calibrated: 2024-11-19
- Sensor-Surface: 1.4 mm
- Electronics: DAE4 Sn703; Calibrated: 2024-04-22
- Phantom: ELI V8.0 (20deg probe tilt); Serial: 2205; Section: Flat
- Measurement Software: 16.2.4.2524
- UID: CW, 0

Pin=20.0dBm/Area Scan (40.0 mm x 80.0 mm): Measurement Grid: 10.0 mm x 10.0 mm

SAR (1g) = 7.43 W/kg; SAR (10g) = 2.18 W/kg;


Pin=20.0dBm/Zoom Scan (22.0 mm x 22.0 mm x 22.0 mm): Measurement Grid: 4.0 mm x 4.0 mm x 1.4 mm

Power Drift = -0.12 dB

SAR (1g) = 8.08 W/kg; SAR (8g) = 2.71 W/kg; SAR (10g) = 2.31 W/kg

Smallest distance from peaks to all points 3 dB below = 7.4 mm

Ratio of SAR at M2 to SAR at M1 = 62.2 %

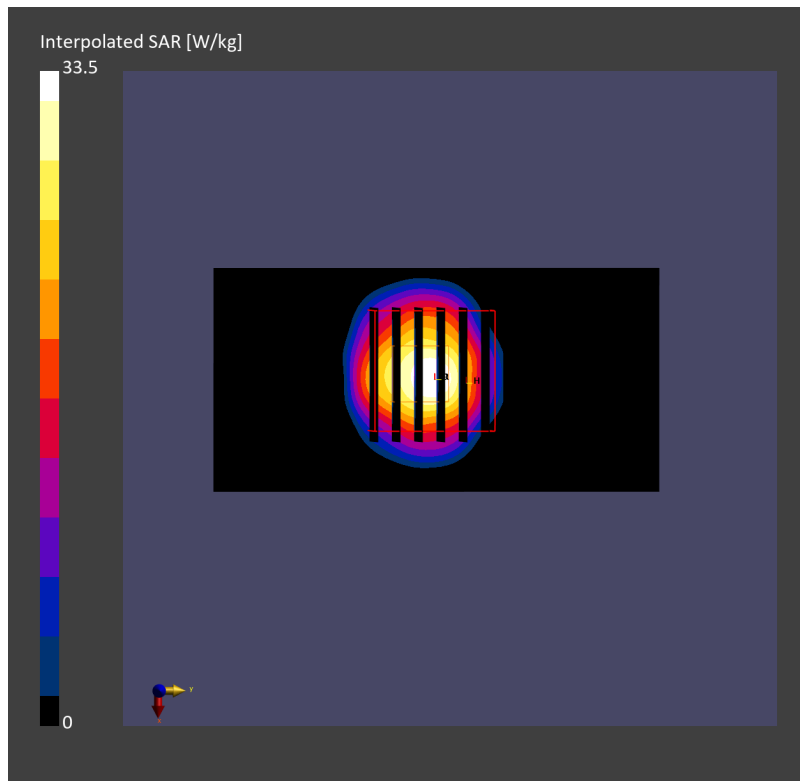

Date: 2024-12-25

System Check_Head_5600MHz**DUT: D5GHzV2 - SN1006**

Communication System: CW; Frequency: 5600.000 MHz

Medium: HSL_5G_241225 Medium parameters used: $f = 5600.000$ MHz; $\sigma = 5.04$ S/m; $\epsilon_r = 35.9$

Ambient Temperature: 23.5°C; Liquid Temperature: 22.5°C

DASY8 Configuration:

- Probe: EX3DV4 - SN7793; ConvF(4.12, 4.35, 4.32); Calibrated: 2024-03-01
- Sensor-Surface: 1.4 mm
- Electronics: DAE4 Sn1794; Calibrated: 2024-02-15
- Phantom: ELI V8.0 (20deg probe tilt); Serial: 2155; Section: Flat
- Measurement Software: 16.2.4.2524
- UID: CW, 0

Pin=20.0dBm/Area Scan (40.0 mm x 80.0 mm): Measurement Grid: 10.0 mm x 10.0 mm

SAR (1g) = 8.00 W/kg; SAR (10g) = 2.34 W/kg;


Pin=20.0dBm/Zoom Scan (22.0 mm x 22.0 mm x 22.0 mm): Measurement Grid: 4.0 mm x 4.0 mm x 1.4 mm

Power Drift = -0.01 dB

SAR (1g) = 8.75 W/kg; SAR (8g) = 2.91 W/kg; SAR (10g) = 2.50 W/kg

Smallest distance from peaks to all points 3 dB below = 7.6 mm

Ratio of SAR at M2 to SAR at M1 = 61.7 %

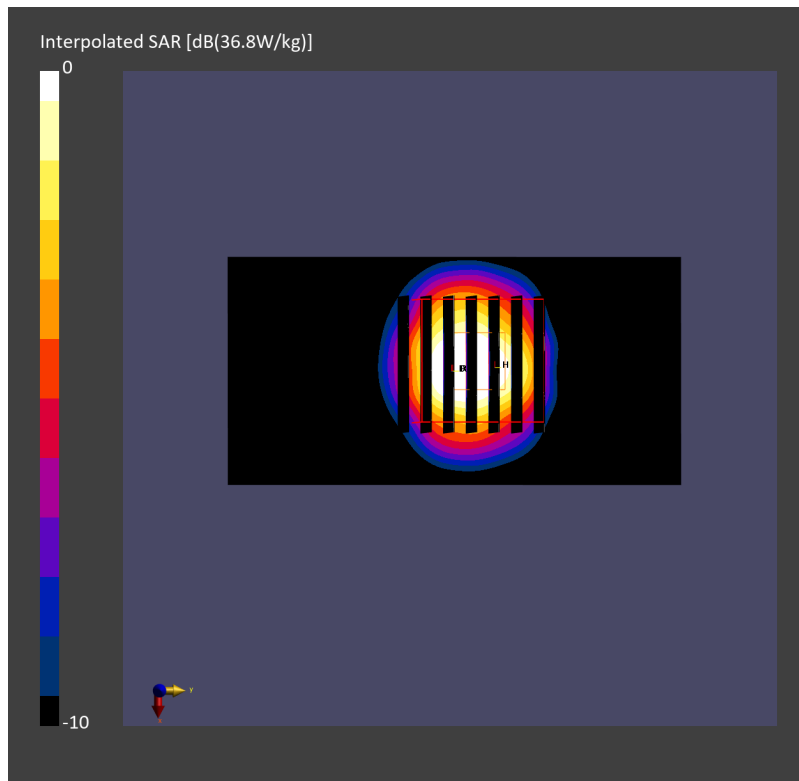

Date: 2024-12-26

System Check_Head_5600MHz**DUT: D5GHzV2 - SN1006**

Communication System: CW; Frequency: 5600.000 MHz

Medium: HSL_5G_241226 Medium parameters used: $f = 5600.000$ MHz; $\sigma = 4.97$ S/m; $\epsilon_r = 34.8$

Ambient Temperature: 23.6°C; Liquid Temperature: 22.6°C

DASY8 Configuration:

- Probe: EX3DV4 - SN3931; ConvF(5.11, 4.92, 4.85); Calibrated: 2024-11-19
- Sensor-Surface: 1.4 mm
- Electronics: DAE4 Sn703; Calibrated: 2024-04-22
- Phantom: ELI V8.0 (20deg probe tilt); Serial: 2205; Section: Flat
- Measurement Software: 16.2.4.2524
- UID: CW, 0

Pin=20.0dBm/Area Scan (40.0 mm x 80.0 mm): Measurement Grid: 10.0 mm x 10.0 mm

SAR (1g) = 7.47 W/kg; SAR (10g) = 2.18 W/kg;


Pin=20.0dBm/Zoom Scan (22.0 mm x 22.0 mm x 22.0 mm): Measurement Grid: 4.0 mm x 4.0 mm x 1.4 mm

Power Drift = -0.01 dB

SAR (1g) = 8.23 W/kg; SAR (8g) = 2.75 W/kg; SAR (10g) = 2.34 W/kg

Smallest distance from peaks to all points 3 dB below = 7.6 mm

Ratio of SAR at M2 to SAR at M1 = 59.7 %

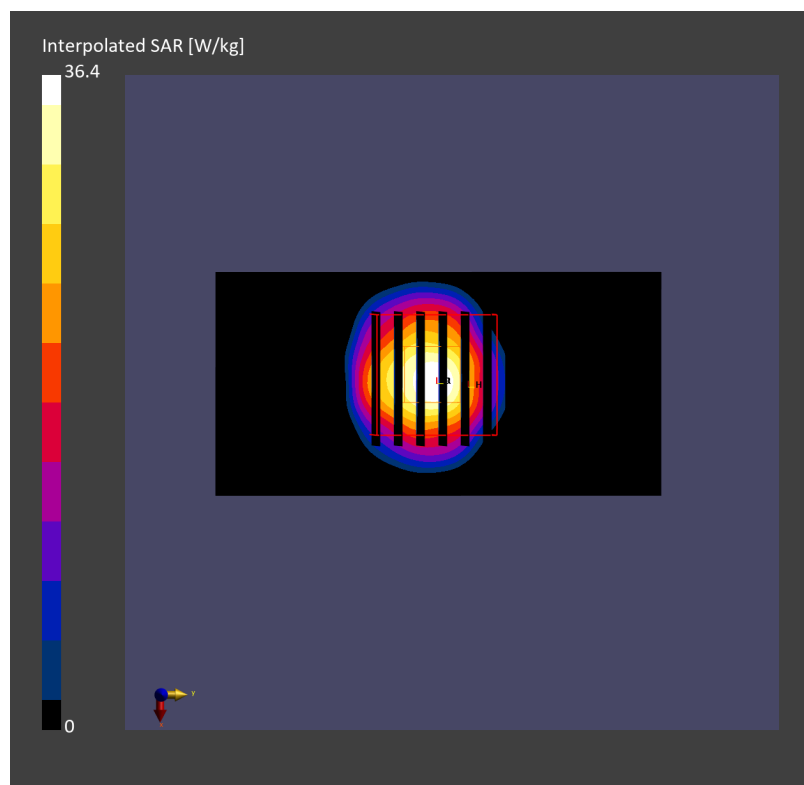

Date: 2024-12-25

System Check_Head_5800MHz**DUT: D5GHzV2 - SN1006**

Communication System: CW; Frequency: 5800.000 MHz

Medium: HSL_5G_241225 Medium parameters used: $f = 5800.000$ MHz; $\sigma = 5.25$ S/m; $\epsilon_r = 35.6$

Ambient Temperature: 23.5°C; Liquid Temperature: 22.5°C

DASY8 Configuration:

- Probe: EX3DV4 - SN7793; ConvF(4.37, 4.42, 4.46); Calibrated: 2024-03-01
- Sensor-Surface: 1.4 mm
- Electronics: DAE4 Sn1794; Calibrated: 2024-02-15
- Phantom: ELI V8.0 (20deg probe tilt); Serial: 2155; Section: Flat
- Measurement Software: 16.2.4.2524
- UID: CW, 0

Pin=20.0dBm/Area Scan (40.0 mm x 80.0 mm): Measurement Grid: 10.0 mm x 10.0 mm

SAR (1g) = 7.89 W/kg; SAR (10g) = 2.30 W/kg;


Pin=20.0dBm/Zoom Scan (22.0 mm x 22.0 mm x 22.0 mm): Measurement Grid: 4.0 mm x 4.0 mm x 1.4 mm

Power Drift = 0.01 dB

SAR (1g) = 8.70 W/kg; SAR (8g) = 2.88 W/kg; SAR (10g) = 2.47 W/kg

Smallest distance from peaks to all points 3 dB below = 7.6 mm

Ratio of SAR at M2 to SAR at M1 = 59.4 %

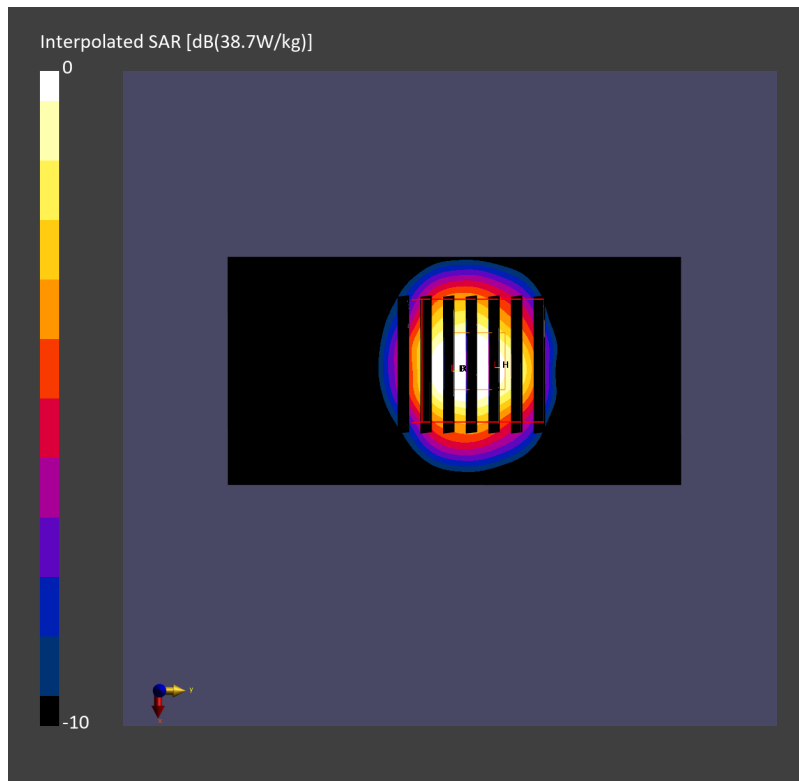

Date: 2024-12-26

System Check_Head_5800MHz**DUT: D5GHzV2 - SN1006**

Communication System: CW; Frequency: 5800.000 MHz

Medium: HSL_5G_241226 Medium parameters used: $f = 5800.000$ MHz; $\sigma = 5.21$ S/m; $\epsilon_r = 34.5$

Ambient Temperature: 23.6°C; Liquid Temperature: 22.6°C

DASY8 Configuration:

- Probe: EX3DV4 - SN3931; ConvF(5.01, 4.83, 4.76); Calibrated: 2024-11-19
- Sensor-Surface: 1.4 mm
- Electronics: DAE4 Sn703; Calibrated: 2024-04-22
- Phantom: ELI V8.0 (20deg probe tilt); Serial: 2205; Section: Flat
- Measurement Software: 16.2.4.2524
- UID: CW, 0

Pin=20.0dBm/Area Scan (40.0 mm x 80.0 mm): Measurement Grid: 10.0 mm x 10.0 mm

SAR (1g) = 7.34 W/kg; SAR (10g) = 2.14 W/kg;


Pin=20.0dBm/Zoom Scan (22.0 mm x 22.0 mm x 22.0 mm): Measurement Grid: 4.0 mm x 4.0 mm x 1.4 mm

Power Drift = -0.02 dB

SAR (1g) = 8.13 W/kg; SAR (8g) = 2.71 W/kg; SAR (10g) = 2.31 W/kg

Smallest distance from peaks to all points 3 dB below = 7.6 mm

Ratio of SAR at M2 to SAR at M1 = 57.9 %

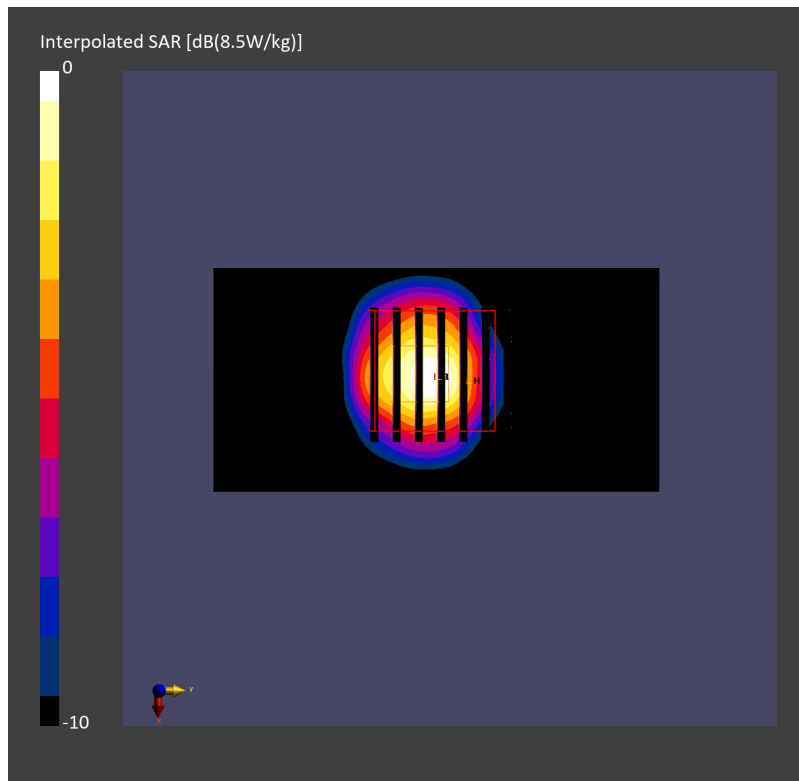

Date: 2024-12-24

System Check_Head_6500MHz**DUT: D6.5GHzV2 - SN1003**

Communication System: CW; Frequency: 6500.000 MHz

Medium: HSL_6G_241224 Medium parameters used: $f = 6500.000$ MHz; $\sigma = 6.01$ S/m; $\epsilon_r = 35.1$

Ambient Temperature: 23.4°C; Liquid Temperature: 22.4°C

DASY8 Configuration:

- Probe: EX3DV4 - SN7814; ConvF(5.41, 5.18, 5.31); Calibrated: 2024-06-20
- Sensor-Surface: 1.4 mm
- Electronics: DAE4ip Sn1800; Calibrated: 2024-06-18
- Phantom: ELI V8.0 (20deg probe tilt); Serial: 2204; Section: Flat
- Measurement Software: 16.2.4.2524
- UID: CW, 0

Pin=20.0dBm/Area Scan (51.0 mm x 85.0 mm): Measurement Grid: 8.5 mm x 8.5 mm

SAR (1g) = 24.6 W/kg; SAR (10g) = 5.50 W/kg;


Pin=20.0dBm/Zoom Scan (22.0 mm x 22.0 mm x 22.0 mm): Measurement Grid: 3.4 mm x 3.4 mm x 1.4 mm

Power Drift = -0.09 dB

SAR (1g) = 29.6 W/kg; SAR (8g) = 6.83 W/kg; SAR (10g) = 5.59 W/kg

Smallest distance from peaks to all points 3 dB below = 4.8 mm

Ratio of SAR at M2 to SAR at M1 = 50.2 %

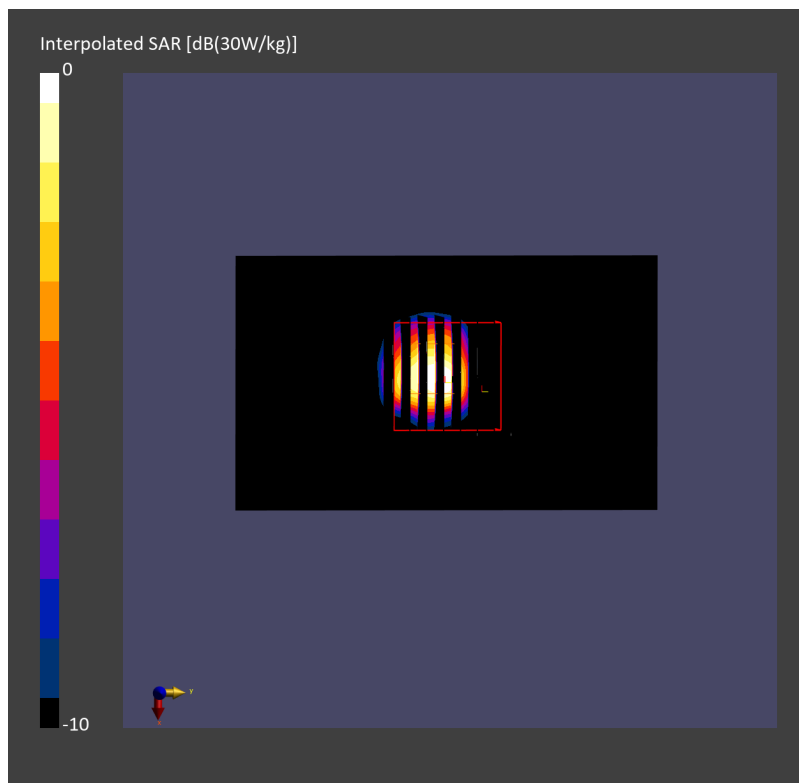psAPD (1.0cm², sq) = 296 [W/m²]; psAPD (4.0cm², sq) = 137 [W/m²]

Date: 2024-12-25

System Check_Head_6500MHz**DUT: D6.5GHzV2 - SN1003**

Communication System: CW; Frequency: 6500.000 MHz

Medium: HSL_6G_241225 Medium parameters used: $f = 6500.000$ MHz; $\sigma = 6.09$ S/m; $\epsilon_r = 34.6$

Ambient Temperature: 23.5°C; Liquid Temperature: 22.5°C

DASY8 Configuration:

- Probe: EX3DV4 - SN7793; ConvF(4.75, 4.82, 4.91); Calibrated: 2024-03-01
- Sensor-Surface: 1.4 mm
- Electronics: DAE4 Sn1794; Calibrated: 2024-02-15
- Phantom: ELI V8.0 (20deg probe tilt); Serial: 2155; Section: Flat
- Measurement Software: 16.2.4.2524
- UID: CW, 0

Pin=20.0dBm/Area Scan (51.0 mm x 85.0 mm): Measurement Grid: 8.5 mm x 8.5 mm

SAR (1g) = 24.1 W/kg; SAR (10g) = 5.20 W/kg;


Pin=20.0dBm/Zoom Scan (22.0 mm x 22.0 mm x 22.0 mm): Measurement Grid: 3.4 mm x 3.4 mm x 1.4 mm

Power Drift = 0.03 dB

SAR (1g) = 29.4 W/kg; SAR (8g) = 6.76 W/kg; SAR (10g) = 5.55 W/kg

Smallest distance from peaks to all points 3 dB below = 4.8 mm

Ratio of SAR at M2 to SAR at M1 = 52.9 %

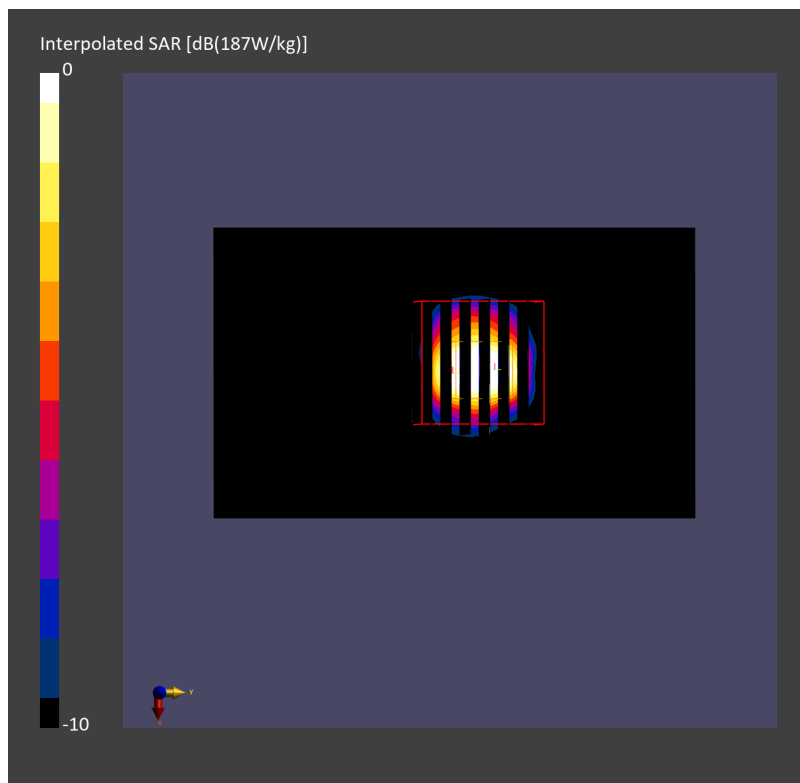psAPD (1.0cm², sq) = 294 [W/m²]; psAPD (4.0cm², sq) = 135 [W/m²]

Date: 2024-12-27

System Check_Head_6500MHz**DUT: D6.5GHzV2 - SN1003**

Communication System: CW; Frequency: 6500.000 MHz

Medium: HSL_6G_241227 Medium parameters used: $f = 6500.000$ MHz; $\sigma = 6.07$ S/m; $\epsilon_r = 34.6$

Ambient Temperature: 23.7°C; Liquid Temperature: 22.7°C

DASY8 Configuration:

- Probe: EX3DV4 - SN3931; ConvF(5.52, 5.32, 5.24); Calibrated: 2024-11-19
- Sensor-Surface: 1.4 mm
- Electronics: DAE4 Sn703; Calibrated: 2024-04-22
- Phantom: ELI V8.0 (20deg probe tilt); Serial: 2205; Section: Flat
- Measurement Software: 16.2.4.2524
- UID: CW, 0

Pin=20.0dBm/Area Scan (51.0 mm x 85.0 mm): Measurement Grid: 8.5 mm x 8.5 mm

SAR (1g) = 22.3 W/kg; SAR (10g) = 4.74 W/kg;

Pin=20.0dBm/Zoom Scan (22.0 mm x 22.0 mm x 22.0 mm): Measurement Grid: 3.4 mm x 3.4 mm x 1.4 mm

Power Drift = -0.00 dB

SAR (1g) = 27.0 W/kg; SAR (8g) = 6.21 W/kg; SAR (10g) = 5.09 W/kg

Smallest distance from peaks to all points 3 dB below = 5.0 mm

Ratio of SAR at M2 to SAR at M1 = 51.1 %

psAPD (1.0cm², sq) = 270 [W/m²]; psAPD (4.0cm², sq) = 124 [W/m²]