
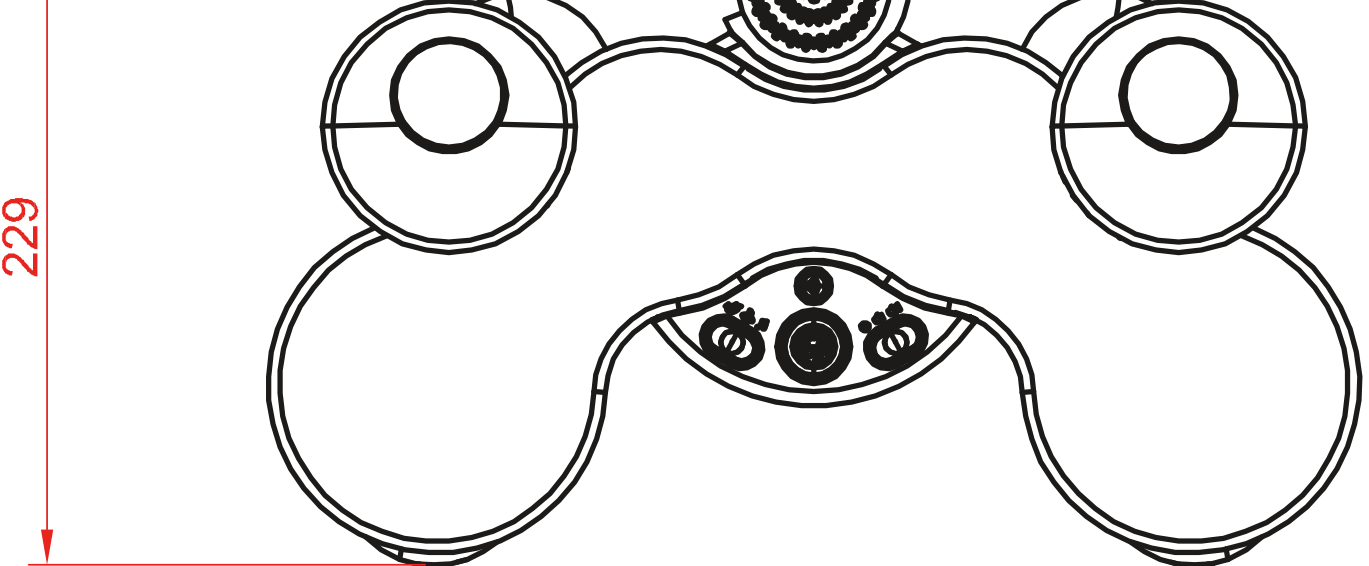
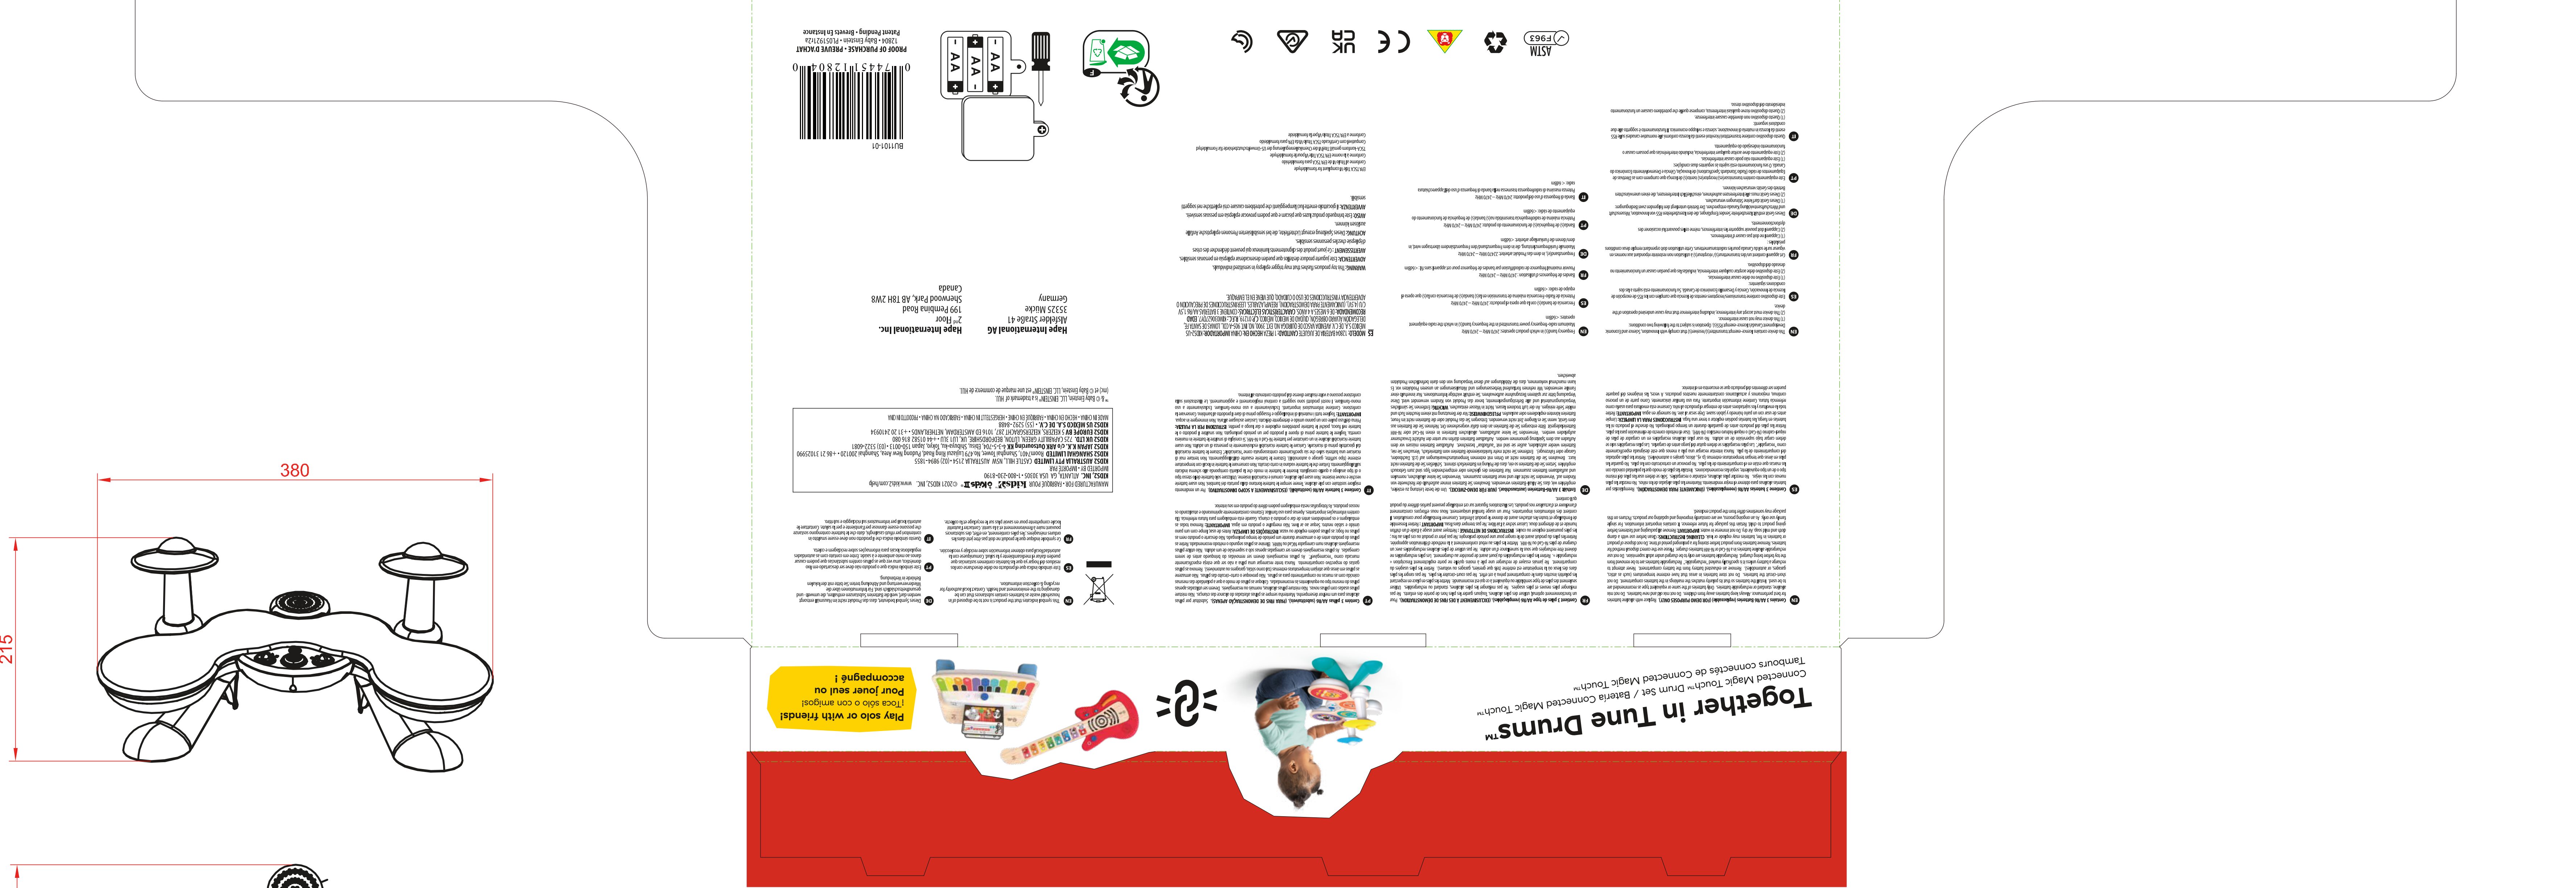


There are two color bars on this proof and in the art file. One to be used with X-rite D50 Pro Spectrophotometer. The other can be used with most other spectrophotometers. Printers must repeat one of the two color bars all the way across the width (grasper edge) of the press sheets on sample runs and production runs. Failure to comply will result in the remaking of the run and/or plates at your cost. 此印刷品及设计文件包含两个色标。其中一个色标用于X-rite D50 Pro分光光度计。另一个色标用于其他分光光度计。印刷厂必须重复其中一个色标在所有样张和生产单张的宽度(抓手边缘)上。不遵守此规定将导致重新制作印单和/或印版，费用由客户承担。没有按照上述要求将色标重复输出到样张、出版或生产单张的印刷厂将自行承担。

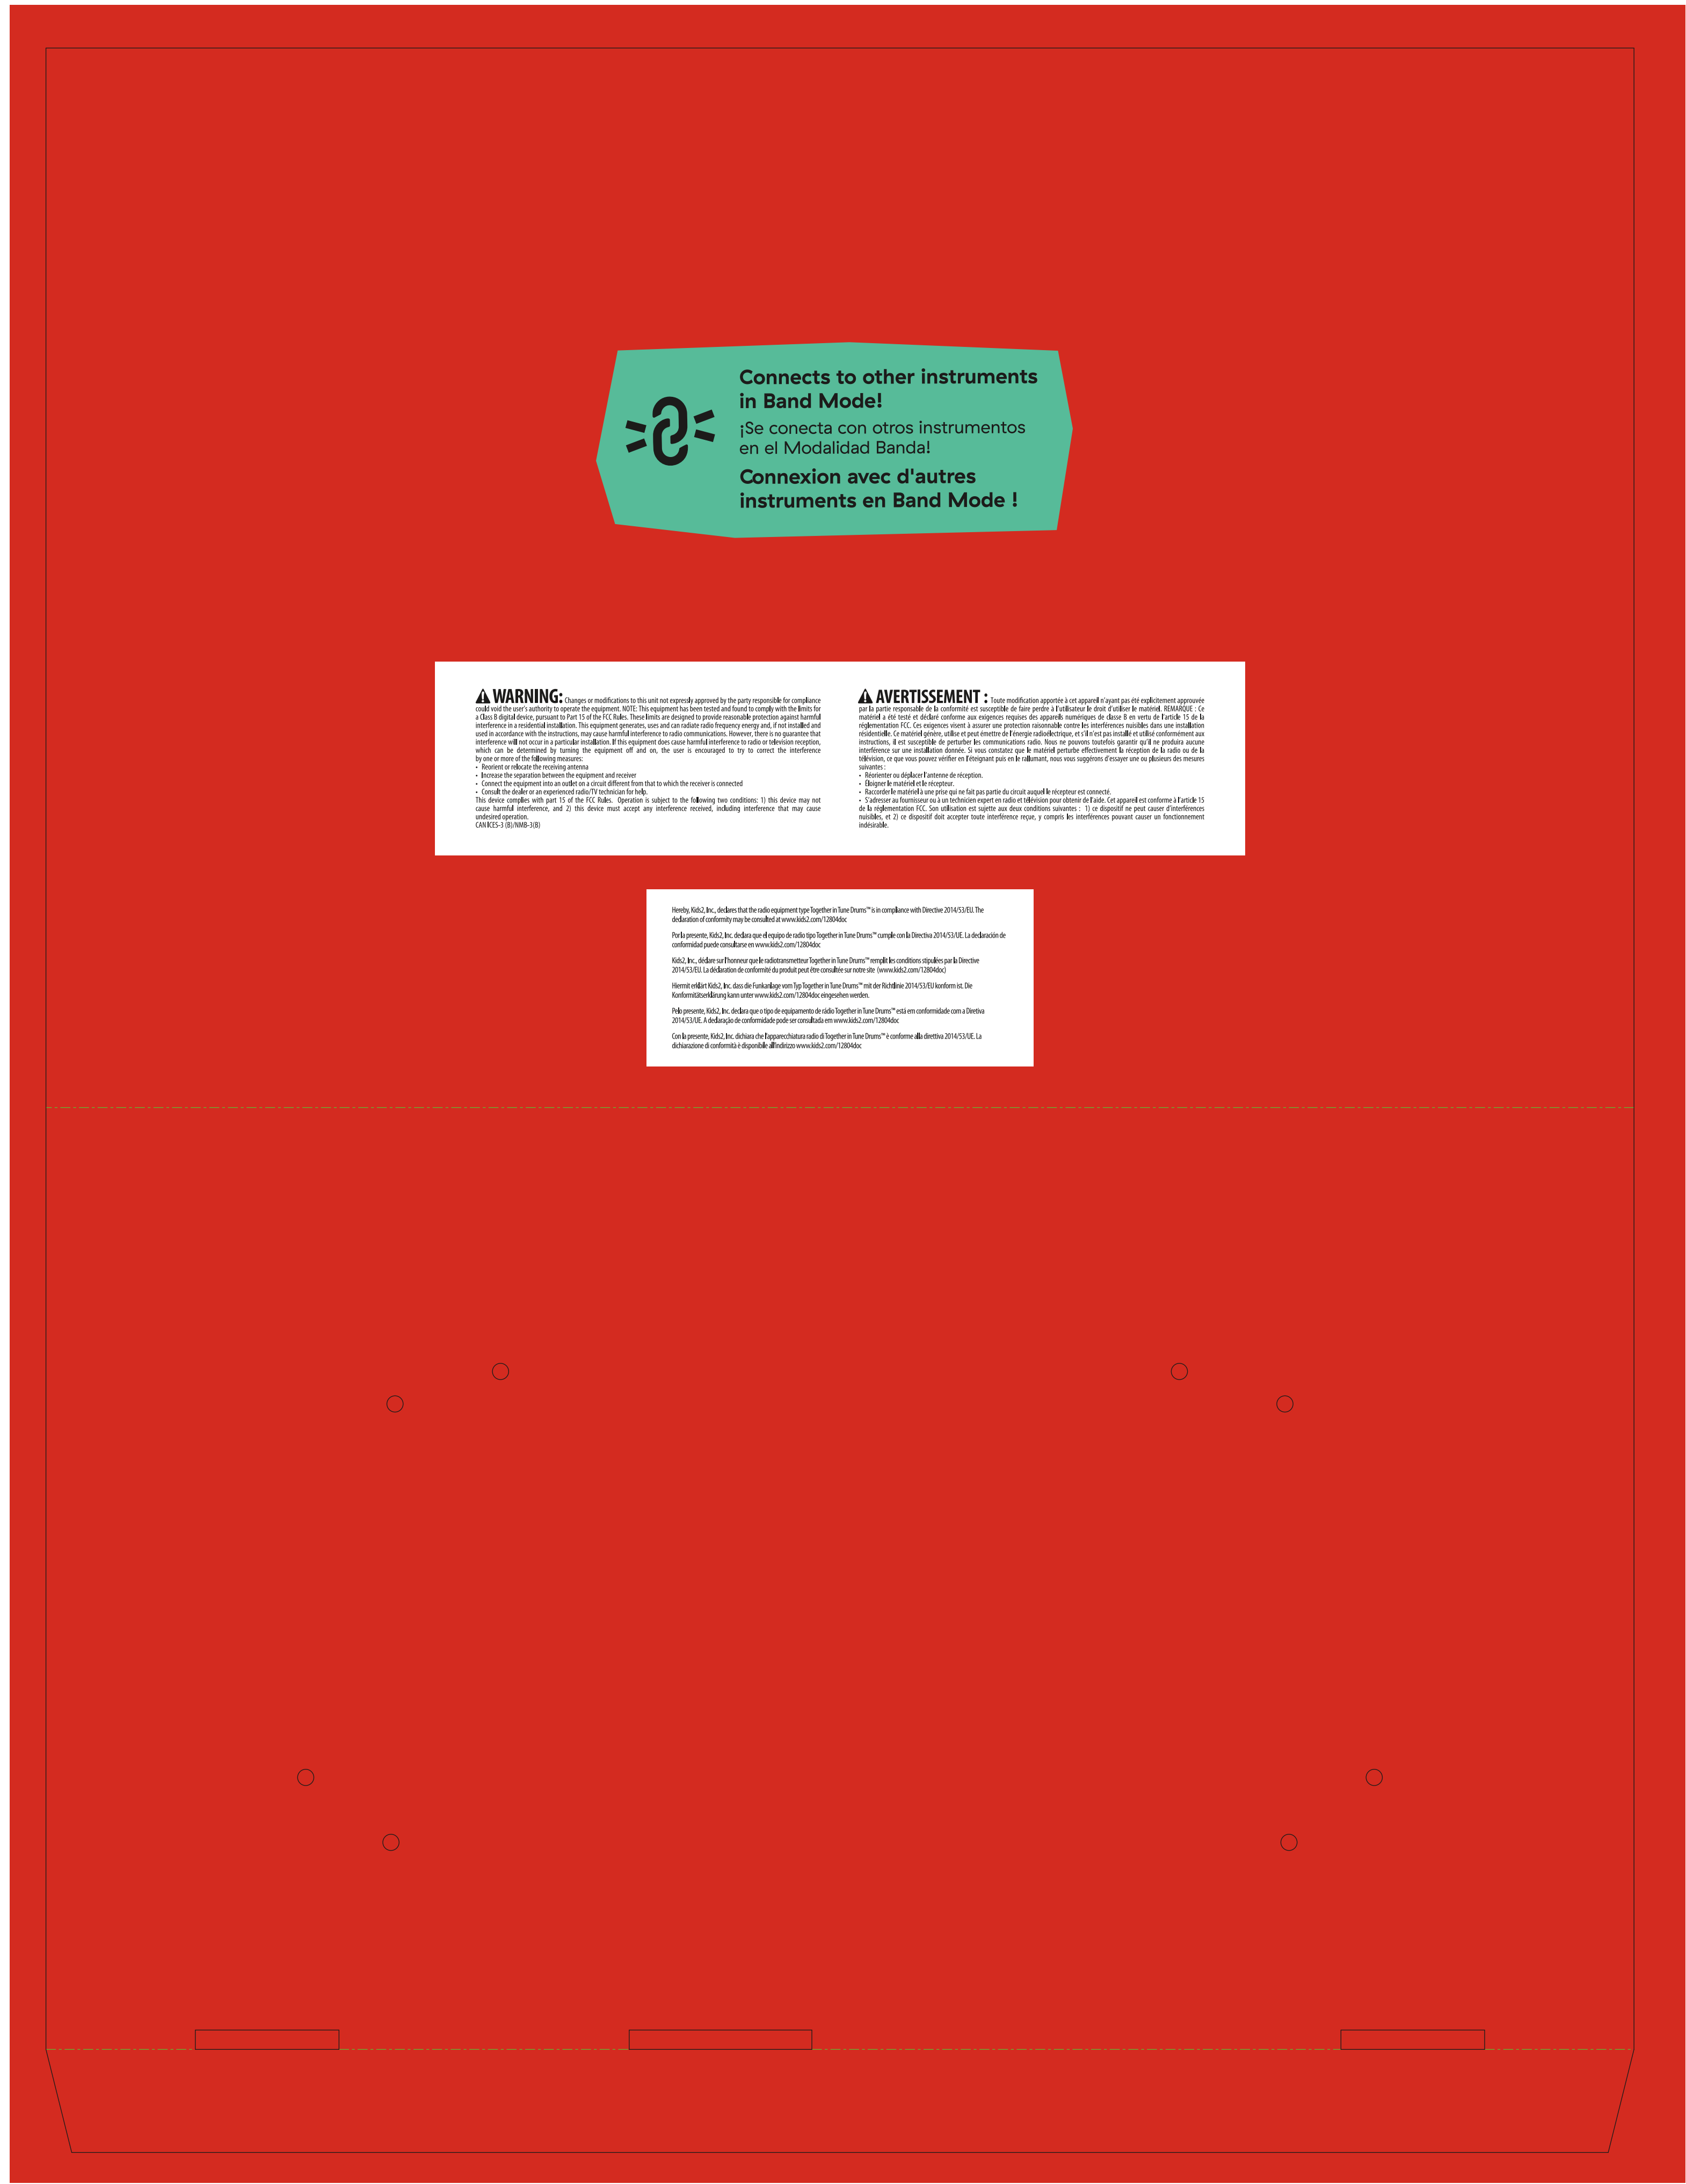

please secure the toy using cable ties

hole locations will be created by manufacturer