Specific Absorption Rate (SAR) Test Reportfor

Amigo Technology Co., Ltd.

on the

802.11b+g wireless USB Dongle

Report No. : O432406-F Brand Name : Amigo/ PTI

Model Name : AWU-901W/ Wireless Pocket USB

PTI-610G/ WLU2454

Date of Testing : Apr. 22, 2004
Date of Report : Apr. 27, 2004
Date of Review : Apr. 27, 2004

- The test results refer exclusively to the presented test model / sample only.
- Without written approval of SPORTON International Inc., the test report shall not be reproduced except in full.

SPORTON International Inc.

6F, No.106, Sec. 1, Hsin Tai Wu Rd., Hsi Chih, Taipei Hsien, Taiwan, R.O.C.

Test Report No: 0432406-F

Table of Contents

1. Statement of Compliance	
2. Administration Data	
2.1. Testing Laboratory	
2.2. Detail of Applicant	2
2.3. Detail of Manfacturer	2
2.4. Application Detail	2
3. Scope	, 3
3.1. Description of Device Under Test (DUT)	
3.2. Applied Standards:	
3.3. Device Category and SAR Limits	
3.4. Test Conditons	
3.4.1. Ambient Condition:	<i>(</i>
3.4.2. Test Configuration:	
4. Specific Absorption Rate (SAR)	,
4.1. Introduction	
4.2. SAR Definition	
5. SAR Measurement Setup	
5.1. DASY4 E-Field Probe System	
5.1.1. ET3DV6 E-Field Probe Specification	
5.1.2. ET3DV6 E-Field Probe Calibration	
5.2. DATA Acquisition Electronics (DAE)	
5.3. Robot	
5.4. Measurement Server	
5.5. SAM Twin Phantom	
5.6. Data Storage and Evaluation	
5.6.1. Data Storage	
5.6.2. Data Evaluation	
5.7. Test Equipment List	
6. Tissue Simulating Liquids	
7. Uncertainty Assessment	
8. SAR Measurement Evaluation	
8.1. Purpose of System Performance check	
8.2. System Setup	
8.3. Validation Results	
9. Description for DUT Testing Position	
10. Measurement Procedures	
10.1. Spatial Peak SAR Evaluation	
10.2. Scan Procedures	
10.3. SAR Averaged Methods	
11. SAR Test Results	
11.1. DUT BTM Touch	
11.2. DUT BTM with 1.5 cm Gap	
12. References	29
Appendix A – System Performance Check Data	
Appendix B – SAR Measurement Data	
Appendix C – Calibration Data	

1. Statement of Compliance

The Specific Absorption Rate (SAR) maximum result found during testing for the **Amigo Technology Co., Ltd. 802.11 b+g wireless USB Dongle is 0.706 W/Kg on body SAR** with expanded uncertainty 19.6%. It is in compliance with Specific Absorption Rate (SAR) for general population/uncontrolled exposure limits specified in FCC 47 CFR part 2 (2.1093) and ANSI/IEEE C95.1-1999 and had been tested in accordance with the measurement methods and procedures specified in OET Bulletin 65 Supplement C (Edition 01-01).

Tested by Phillip Lin

Phillip Lin

Phillip Lin Project Leader Reviewed by Daniel Lee

Dr. C.H. Daniel Lee SAR Lab. Manager

Daniel Lee 4/8/2004

Test Report No : 0432406-F



2. Administration Data

2.1. Testing Laboratory

Company Name: Sporton International Inc.

Department: Antenna Design/SAR

Address: No.52, Hwa-Ya 1st RD., Hwa Ya Technology Park, Kwei-Shan Hsiang,

TaoYuan Hsien, Taiwan, R.O.C.

Telephone Number: 886-3-327-3456 **Fax Number:** 886-3-327-0973

2.2. Detail of Applicant

Company Name: Amigo Technology Co., Ltd

Address: No. 6, Lane 35, Jihu Rd., Neihu, Taipei Taiwan 114, R.O.C.

 Telephone Number:
 886-2-2659-6888

 Fax Number:
 886-2-2659-6889

 Contact Person:
 sam@amigo.com.tw

2.3. Detail of Manfacturer

Company Name: FAIR WAY ELECTRONICS FACTORY

Address: Huang Chong No.3 Ind Area, Zhong Tang Town, Dong Guan City,

Guang Dong, P.R. China

2.4. Application Detail

Date of reception of application:Apr. 22, 2004Start of test:Apr. 26, 2004End of test:Apr. 26, 2004



3. Scope

3.1. Description of Device Under Test (DUT)

DUT Type:	802.11b+g wireless USB Dongle
Trade Name:	Amigo/ PTI
Model Name:	AWU-901W/ Wireless Pocket USB/ PTI-610G/ WLU2454
Modulation Type/Data Rate:	(CCK11/5M)/(DQPSK2M)/(DBPSK1M)(OFDM54/48/36/24/18/9M)
Frequency Range:	2400~2462 MHz
Channel Bandwidth	54 MHz
Expected Max. Conducted RF Power:	18dBm
Antenna Type :	Chip Antenna
Antenna Gain :	1.8 dBi
Operation Temperature :	0°C∼ +65°C
DUT Stage :	Production Unit
Application Type:	Certification

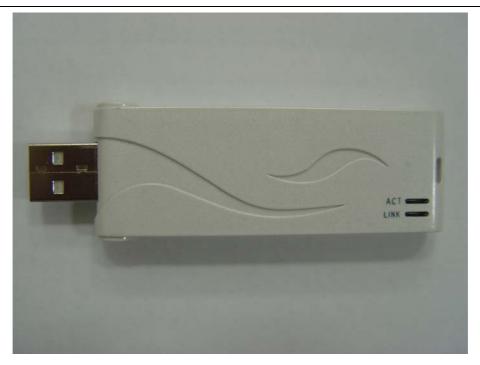


Fig. 3.1 Top View



Fig. 3.2 Bottom view



3.2. Applied Standards:

The Specific Absorption Rate (SAR) testing specification, method and procedure for this 802.11b+g wireless USB Dongle is in accordance with the following standards:

47 CFR Part 2 (2.1093), IEEE C95.1-1999, IEEE C95.3-1991, IEEE P1528 -200X, and OET Bulletin 65 Supplement C (Edition 01-01)

3.3. Device Category and SAR Limits

This device belongs to portable device category because its radiating structure is allowed to be used within 20 centimeters of the body of the user.

Limit for General Population/Uncontrolled exposure should be applied for this device, it is 1.6 W/kg as averaged over any 1 gram of tissue.

3.4. Test Conditions

3.4.1. Ambient Condition:

Ambient Temperature (°C)	21 ~ 23°C
Tissue simulating liquid temperature (°C)	21.5℃
Humidity (%)	$40 \sim 60\%$

3.4.2. <u>Test Configuration:</u>

Engineering testing software installed on the notebook can provide continuous transmitting RF signal. This RF signal utilized in SAR measurement is continuous wave (CW) and its crest factor is 1. The measurements were performed on the lowest, middle, and highest channel, i.e. channel 1, channel 6, and channel 11 for each testing position. However, if the SAR value is 3 dB lower than SAR limit, only one channel is tested for this testing position.

4. Specific Absorption Rate (SAR)

4.1.Introduction

SAR is related to the rate at which energy is absorbed per unit mass in an object exposed to a radio field. The SAR distribution in a biological body is complicated and is usually carried out by experimental techniques or numerical modeling. The FCC recommends limits for two tiers of groups, occupational/controlled and general population/uncontrolled, based on a person's awareness and ability to exercise control over his or her exposure. In general, occupational/controlled exposure limits are higher than the limits for general population/uncontrolled.

4.2.SAR Definition

The SAR definition is the time derivative (rate) of the incremental energy (dW) absorbed by (dissipated in) an incremental mass (dm) contained in a volume element (dv) of a given density.

 ρ). The equation description is as below:

$$\mathbf{SAR} = \frac{d}{dt} \left(\frac{dW}{dm} \right) = \frac{d}{dt} \left(\frac{dW}{\rho dv} \right)$$

SAR is expressed in units of Watts per kilogram (W/kg)

SAR measurement can be either related to the temperature elevation in tissue by

$$\mathbf{SAR} = C \frac{\delta T}{\delta t}$$

, where C is the specific head capacity, δT is the temperature rise and δt the exposure duration,

or related to the electrical field in the tissue by

$$\mathbf{SAR} = \frac{\sigma |E|^2}{\rho}$$

, where σ is the conductivity of the tissue, ρ is the mass density of the tissue and E is the rms electrical field strength.

However for evaluating SAR of low power transmitter, electrical field measurement is typically applied.

5. SAR Measurement Setup

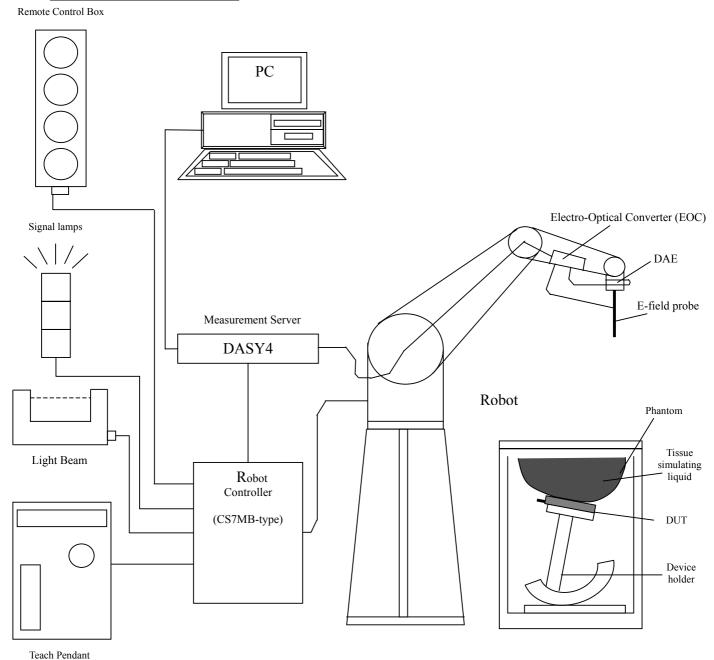


Fig. 5.1 DASY4 system

The DASY4 system for performance compliance tests is illustrated above graphically. This system consists of the following items:

- A standard high precision 6-axis robot with controller, a teach pendant and software
- A data acquisition electronic (DAE) attached to the robot arm extension
- A dosimetric probe equipped with an optical surface detector system
- > The electro-optical converter (ECO) performs the conversion between optical and electrical signals
- A measurement server performs the time critical tasks such as signal filtering, control of the robot operation and fast movement interrupts.
- A probe alignment unit which improves the accuracy of the probe positioning
- A computer operating Windows XP
- ➤ DASY4 software
- Remove control with teach pendant and additional circuitry for robot safety such as warming lamps, etc.
- The SAM twin phantom
- ➤ A device holder
- Tissue simulating liquid
- Dipole for evaluating the proper functioning of the system

Some of the components are described in details in the following sub-sections.

5.1.DASY4 E-Field Probe System

The SAR measurement is conducted with the dosimetric probe ET3DV6 (manufactured by SPEAG). The probe is specially designed and calibrated for use in liquid with high permittivity. The dosimetric probe has special calibration in liquid at different frequency. This probe has a built in optical surface detection system to prevent from collision with phantom.

Calibration: Required once a year.

Test Report No : O432406-F



5.1.1. ET3DV6 E-Field Probe Specification

Construction Symmetrical design with triangular core

Built-in optical fiber for surface detection

system

Built-in shielding against static charges PEEK enclosure material (resistant to

organic solvents)

Calibration Simulating tissue at frequencies of

900MHz, 1.8GHz and 2.45GHz for brain

and muscle (accuracy ±8%)

Frequency 10 MHz to > 3 GHz

Directivity ± 0.2 dB in brain tissue (rotation around

probe axis)

 \pm 0.4 dB in brain tissue (rotation perpendicular to probe axis)

Dynamic Range $5 \mu \text{ W/g to} > 100 \text{mW/g}$; Linearity: $\pm 0.2 \text{dB}$ **Surface Detection** $\pm 0.2 \text{ mm}$ repeatability in air and clear

liquids on reflecting surface

Dimensions Overall length: 330mm

Tip length: 16mm Body diameter: 12mm

Tip diameter: 6.8mm

Distance from probe tip to dipole centers:

2.7mm

Application General dosimetry up to 3GHz

Compliance tests for mobile phones and

Wireless LAN

Fast automatic scanning in arbitrary

phantoms



Fig. 5.2 Probe setup on robot

5.1.2. ET3DV6 E-Field Probe Calibration

Each probe needs to be calibrated according to a dosimetric assessment procedure with accuracy better than \pm 10%. The spherical isotropy shall be evaluated and within \pm 0.25dB. The sensitivity parameters (NormX, NormY, and NormZ), the diode compression parameter (DCP) and the conversion factor (ConvF) of the probe are tested. The calibration data are as below:

Sensitivity	X axis : 1.68 μV	Y axis : 1.62 μV	Z axis :1.71 μV
Diode compression point	X axis : 95 mV	Y axis : 95 mV	Z axis : 95 mV
Conversion factor	X axis	Y axis	Z axis
2400~2500 MHz (Body)	4.5	4.5	4.5
Boundary effect	Alpha	Depth	
2400~2500 MHz (Body)	1.01	1.74	

NOTE:

- 1. The probe parameters have been calibrated by the SPEAG.
- 2. For the detailed calibration data is shown in Appendix C.

5.2.DATA Acquisition Electronics (DAE)

The data acquisition electronics (DAE4) consists of a highly sensitive electrometer-grade preamplifier with auto-zeroing, a channel and gain-switching multiplexer, a fast 16 bit AD-converter and a command decoder and control logic unit. Transmission to the measurement server is accomplished through an optical downlink for data and status information as well as an optical uplink for commands and the clock.

The mechanical probe mounting device includes two different sensor systems for frontal and sideways probe contacts. They are used for mechanical surface detection and probe collision detection.

The input impedance of the DAE4 is 200M Ohm; the inputs are symmetrical and floating. Common mode rejection is above 80dB.

Calibration: Required once a year. Calibration data is attached in Appendix C.

5.3.<u>Robot</u>

The DASY4 system uses the high precision robots RX90BL type out of the newer series from Stäubli SA (France). For the 6-axis controller DASYS system, the CS7MB robot controller version from Stäubli is used. The RX robot series have many features that are important for our application:

- ➤ High precision (repeatability 0.02 mm)
- High reliability (industrial design)
- > Jerk-free straight movements
- Low ELF interference (the closed metallic construction shields against motor control fields)
- ► 6-axis controller

5.4. Measurement Server

The DASY4 measurement server is based on a PC/104 CPU board with 166 MHz CPU 32 MB chipset and 64 MB RAM

Communication with the DAE4 electronic box

the 16-bit AD-converter system for optical detection and digital I/O interface.

The measurement server performs all the real-time data evaluation for field measurements and surface detection, controls robot movements and handles safety operations.

Calibration: No calibration required.

5.5.SAM Twin Phantom

The SAM twin phantom is a fiberglass shell phantom with 2mm shell thickness (except the ear region where shell thickness increases to 6mm). It has three measurement areas:

- Left head
- Right head
- Flat phantom

The bottom plate contains three pair of bolts for locking the device holder. The device holder positions are adjusted to the standard measurement positions in the three sections.

A white cover is provided to tap the phantom during off-periods to prevent water evaporation and changes in the liquid parameters.

On the phantom top, three reference markers are provided to identify the phantom position with respect to the robot.

The phantom can be used with the following tissue simulating liquids:

- *Water-sugar based liquid
- *Glycol based liquids



Fig. 5.3 Top view of twin phantom



Fig. 5.4 Bottom view of twin phantom

5.6. Data Storage and Evaluation

5.6.1. Data Storage

The DASY4 software stores the assessed data from the data acquisition electronics as raw data (in microvolt readings from the probe sensors), together with all the necessary software parameters for the data evaluation (probe calibration data, liquid parameters and device frequency and modulation data) in measurement files with the extension .DA4. The postprocessing software evaluates the desired unit and format for output each time the data is visualized or exported. This allows verification of the complete software setup even after the measurement and allows correction of erroneous parameter settings. For example, if a measurement has been performed with an incorrect crest factor parameter in the device setup, the parameter can be corrected afterwards and the data can be reevaluated.

The measured data can be visualized or exported in different units or formats, depending on the selected probe type (e.g., [V/m], [A/m], [mW/g]). Some of these units are not available in certain situations or give meaningless results, e.g., a SAR-output in a loseless media, will always be zero. Raw data can also be exported to perform the evaluation with other software packages.

5.6.2. Data Evaluation

Device parameters:

The DASY4 postprocessing software (SEMCAD) automatically executes the following procedures to calculate the field units from the microvolt readings at the probe connector. The parameters used in the evaluation are stored in the configuration modules of the software:

Probe parameters:	- Sensitivity	$Norm_i, a_{i0}, a_{i1}, a_{i2}$
--------------------------	---------------	----------------------------------

- Conversion factor ConvF_i - Diode compression point dcp_i - Frequency f

- Crest factor cf **Media parameters**: - Conductivity σ

- Density o

These parameters must be set correctly in the software. They can be found in the component documents or they can be imported into the software from the configuration files issued for the DASY components. In the direct measuring mode of the multimeter option, the parameters of the actual system setup are used. In the scan visualization and export modes, the parameters stored in the corresponding document files are used. The first step of the evaluation is a linearization of the filtered input signal to account for the compression characteristics of the detector diode. The compensation depends on the input signal, the diode type and the DC-transmission factor from the diode to the evaluation electronics. If the exciting field is pulsed, the crest factor of the signal must be known to correctly compensate for peak power. The formula for each channel



FCC SAR Test Report Test Report No : 0432406-F

can be given as:

$$Vi = U_i + U_i^2 \cdot \frac{cf}{dcp_i}$$

with

 V_i = compensated signal of channel i (i = x, y, z)

 U_i = input signal of channel i (i = x, y, z)

cf = crest factor of exciting field (DASY parameter)

 $dcp_i = diode\ compression\ point\ (DASY\ parameter)$

From the compensated input signals, the primary field data for each channel can be evaluated:

E-field probes : $E_i = \sqrt{\frac{V_i}{Norm_i ConvF}}$

H-field probes: $H_i = \sqrt{V_i} \frac{a_{i0+} a_{i1} f + a_{i2} f^2}{f}$

with

 V_i = compensated signal of channel i (i = x, y, z)

 $Norm_i$ = sensor sensitivity of channel i (i = x, y, z)

 $\mu V/(V/m)$ 2 for E-field Probes

ConvF = sensitivity enhancement in solution

 a_{ii} = sensor sensitivity factors for H-field probes

f = carrier frequency [GHz]

 E_i = electric field strength of channel i in V/m

 H_i = magnetic field strength of channel i in A/m

The RSS value of the field components gives the total field strength (Hermitian magnitude):

$$E_{tot} = \sqrt{E_X^2 + E_Y^2 + E_Z^2}$$

The primary field data are used to calculate the derived field units.

$$SAR = E_{tot}^2 \cdot \frac{\sigma}{\rho \cdot 1000}$$

with

SAR = local specific absorption rate in mW/g

Etot = total field strength in V/m

 $\sigma = \text{conductivity in [mho/m] or [Siemens/m]}$

 ρ = equivalent tissue density in g/cm³



with

Test Report No : O432406-F

* Note that the density is set to 1, to account for actual head tissue density rather than the density of the tissue simulating liquid.

The power flow density is calculated assuming the excitation field to be a free space field.

$$P_{pwe} = \frac{E_{tot}^2}{3770}$$
 or $P_{pwe} = H_{tot}^2 \cdot 37.7$

 P_{pwe} = equivalent power density of a plane wave in mW/cm²

 E_{tot} = total electric field strength in V/m

 H_{tot} = total magnetic field strength in A/m

5.7. Test Equipment List

Manufacture	Name of Equipment	Type/Model	Serial Number	C	alibration
Manufacture	Name of Equipment	Type/Model	Seriai Number	Last Cal.	Due Date
SPEAG	Dosimetric E-Filed Probe	ET3DV6	1788	Aug. 29, 2003	Aug. 29, 2004
SPEAG	900MHz System Validation Kit	D900V2	190	Jul. 17, 2003	Jul. 17, 2005
SPEAG	1800MHz System Validation Kit	D1800V2	2d076	Jul. 16, 2003	Jul. 16, 2005
SPEAG	2450MHz System Validation Kit	D2450V2	736	Aug. 26, 2003	Aug. 26, 2004
SPEAG	Data Acquisition Electronics	DAE3	577	Nov. 21, 2003	Nov. 21, 2004
SPEAG	Device Holder	N/A	N/A	NCR	NCR
SPEAG	Phantom	QD 000 P40 C	TP-1150	NCR	NCR
SPEAG	Robot	Staubli RX90BL	F03/5W15A1/A/01	NCR	NCR
SPEAG	Software	DASY4 V4.1 Build 47	N/A	NCR	NCR
SPEAG	Software	SEMCAD V1.6 Build 116	N/A	NCR	NCR
SPEAG	Measurement Server	SE UMS 001 BA	1021	NCR	NCR
Agilent	S-Parameter Network Analyzer (PNA)	E8358A	US40260131	Oct 17, 2003	Oct. 17, 2004
Agilent	Dielectric Probe Kit	85070D	US01440205	NCR	NCR
R&S	Power Meter	NRVS	100444	May 28, 2003	May 28, 2004
R&S	Power Sensor	NRV-Z32	100057	May 28, 2003	May 28, 2004
R&S	Signal Generator	SMR40	100116	Nov.06, 2003	Nov.06, 2004
Agilent	Dual Directional Coupler	778D	50422	NCR	NCR
Agilent	Power Amplifier	8449B	3008A01917	Sep. 16, 2003	Sep. 16, 2004

Table 5.1 Test Equipment List

6. Tissue Simulating Liquids

For the measurement of the field distribution inside the SAM phantom with DASY4, the phantom must be filled with around 25 liters of homogeneous body tissue simulating liquid. The liquid height from the bottom of the phantom body is 15.2 centimeters, which is shown in Fig. 6.1.

The following ingredients for tissue simulating liquid are used:

- **Water**: deionized water (pure H_20), resistivity ≥ 16M Ω as basis for the liquid
- Sugar: refined sugar in crystals, as available in food shops to reduce relative permittyvity
- Salt: pure NaCl to increase conductivity
- ➤ Cellulose: Hydroxyethyl-cellulose, medium viscosity (75-125 mPa.s, 2% in water, 20°C), CAS#54290-to increase viscosity and to keep sugar in solution.
- ➤ **Preservative**: Preventol D-7 Bayer AG, D-51368 Leverkusen, CAS#55965-84-9- to prevent the spread of bacteria and molds.
- ➤ **DGMBE**: Deithlenglycol-monobuthyl ether (DGMBE), Fluka Chemie GmbH, CAS#112-34-5 to reduce relative permittivity.

Table 6.1 gives the recipes for one liter of tissue simulating liquid for frequency band 2450 MHz.

Ingredient	MSL-2450
Water	698.3 ml
DGMBE	301.7 ml
Total amount	1 liter (1.0 kg)
Dielectric Parameters at 22°	f = 2450MHz
	ε_1 = 52.5±5%, σ = 2.00±5% S/m

Table 6.1

The dielectric parameters of the liquids were verified prior to the SAR evaluation using an Agilent 85070D Dielectric Probe Kit and an Agilent E8358A Network Analyzer.

Table 6.2 shows the measuring results for muscle simulating liquid in this 2450 MHz frequency band at the temperature = 21.5°C

Test Report No	: (O432406-F	
----------------	-----	-----------	--

Bands	Frequency(MHz)	Permittivity ($\varepsilon_{ m r}$)	Conductivity (\sigma)
	2412	52.89	1.921
ISM band	2437	52.67	1.950
(2450 MHz)	2462	52.55	1.987
	2472	52.55	2.004

^{*}The testing date is Apr. 26, 2004.

Table 6.2

The measuring data are consistent with $\varepsilon_{\Gamma} = 52.5 \pm 5\%$ and $\sigma = 2.00 \pm 5\%$.



Fig. 6.1

7. Uncertainty Assessment

The component of uncertainly may generally be categorized according to the methods used to evaluate them. The evaluation of uncertainly by the statistical analysis of a series of observations is termed a Type A evaluation of uncertainty. The evaluation of uncertainty by means other than the statistical analysis of a series of observation is termed a Type B evaluation of uncertainty. Each component of uncertainty, however evaluated, is represented by an estimated standard deviation, termed standard uncertainty, which is determined by the positive square root of the estimated variance.

A Type A evaluation of standard uncertainty may be based on any valid statistical method for treating data. This includes calculating the standard deviation of the mean of a series of independent observations; using the method of least squares to fit a curve to the data in order to estimate the parameter of the curve and their standard deviations; or carrying out an analysis of variance in order to identify and quantify random effects in certain kinds of measurement.

A type B evaluation of standard uncertainty is typically based on scientific judgment using all of the relevant information available. These may include previous measurement data, experience and knowledge of the behavior and properties of relevant materials and instruments, manufacture's specification, data provided in calibration reports and uncertainties assigned to reference data taken from handbooks. Broadly speaking, the uncertainty is either obtained from an outdoor source or obtained from an assumed distribution, such as the normal distribution, rectangular or triangular distributions indicated in Table 7.1

Uncertainty Distributions	Normal	Rectangular	Triangular	U-shape
Multiplying factor ^(a)	$1/k^{(b)}$	1/√3	1/√6	1/√2

⁽a) standard uncertainty is determined as the product of the multiplying factor and the estimated range of variations in the measured quantity

Table 7.1

The combined standard uncertainty of the measurement result represents the estimated standard deviation of the result. It is obtained by combining the individual standard uncertainties of both Type A and Type B evaluation using the usual "root-sum-squares" (RSS) methods of combining standard deviations by taking the positive square root of the estimated variances.

Expanded uncertainty is a measure of uncertainty that defines an interval about the measurement result within which the measured value is confidently believed to lie. It is obtained by multiplying the combined standard uncertainty by a coverage factor. Typically, the coverage factor ranges from 2 to 3. Using a coverage factor allows the true value of a measured quantity to be specified with a defined probability within the specified uncertainty range. For purpose of this document, a coverage factor two is used, which corresponds to confidence interval of about 95 %. The DASY4 uncertainty Budget is showed

⁽b) κ is the coverage factor



in Table 7.2.

Error Description	Uncertainty Value ± %	Probability Distribution	Divisor	Ci Ig	Standard Unc. (1-g)	vi or V <i>eff</i>
Measurement System				1		1
Probe Calibration	± 4.8	Normal	1	1	±4.8	∞
Axial Isotropy	± 4.7	Rectangular	√3	$(1-Cp)^{1/2}$	±1.9	∞
Hemispherical Isotropy	± 9.6	Rectangular	√3	$(Cp)^{1/2}$	±3.9	∞
Boundary Effect	± 1.0	Rectangular	$\sqrt{3}$	1	±0.6	∞
Linearity	± 4.7	Rectangular	$\sqrt{3}$	1	±2.7	∞
System Detection Limit	± 1.0	Rectangular	$\sqrt{3}$	1	±0.6	∞
Readout Electronics	± 1.0	Rectangular	1	1	±1.0	∞
Response Time	± 0	Normal	$\sqrt{3}$	1	± 0	∞
Integration time	± 0	Rectangular	$\sqrt{3}$	1	± 0	∞
RF Ambient Conditions	± 3.0	Rectangular	√3	1	±1.7	∞
Probe Positioner Mech. Tolerance	± 0.4	Rectangular	√3	1	±0.2	∞
Probe Positioning with respect to Phantom Shell	± 2.9	Rectangular	√3	1	±1.7	∞
Extrapolation and Interpolation Algorithms for Max. SAR Evaluation	± 1.0	Rectangular	$\sqrt{3}$	1	±0.6	∞
Test sample Related						
Test sample Positioning	±2.9	Normal	1	1	±2.9	145
Device Holder Uncertainty	±3.6	Normal	1	1	±3.6	5
Output Power Variation-SAR drift measurement	±2.5	Rectangular	√3	1	±1.4	∞
Phantom and Tissue						
parameters						
Phantom uncertainty(Including shar and thickness tolerances)	±4.0	Rectangular	√3	1	±2.3	∞
Liquid Conductivity Target tolerance	±5.0	Rectangular	√3	0.64	±1.8	∞
Liquid Conductivity measurement uncertainty	±2.5	Normal	1	0.64	±1.6	∞
Liquid Permittivity Target tolerance	±5.0	Rectangular	$\sqrt{3}$	0.6	±1.7	∞
Liquid Permittivity measurement uncertainty	±2.0	Normal	1	0.6	±1.2	∞
Combined standard uncertainty					±9.79	330
Coverage Factor for 95 %		<u>K=2</u>				
Expanded uncertainty (Coverage factor = 2)			Normal (k=2) 27		±19.6	

Test Report No : O432406-F

Table 7.2. Uncertainty Budget of DASY

8. SAR Measurement Evaluation


Each DASY system is equipped with one or more system validation kits. These units, together with the predefined measurement procedures within the DASY software, enable the user to conduct the system performance check and system validation. System validation kit includes a dipole, tripod holder to fix it underneath the flat phantom and a corresponding distance holder.

8.1. Purpose of System Performance check

The system performance check verifies that the system operates within its specifications. System and operator errors can be detected and corrected. It is recommended that the system performance check be performed prior to any usage of the system in order to guarantee reproducible results. The system performance check uses normal SAR measurements in a simplified setup with a well characterized source. This setup was selected to give a high sensitivity to all parameters that might fail or vary over time. The system check does not intend to replace the calibration of the components, but indicates situations where the system uncertainty is exceeded due to drift or failure.

8.2.System Setup

In the simplified setup for system evaluation, the DUT is replaced by a calibrated dipole and the power source is replaced by a continuous wave which comes from a signal generator at frequency 2450 MHz. The calibrated dipole must be placed beneath the flat phantom section of the SAM twin phantom with the correct distance holder. The distance holder should touch the phantom surface with a light pressure at the reference marking and be oriented parallel to the long side of the phantom. The equipment setup is shown below:

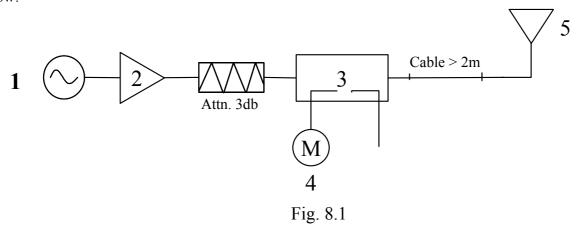

- 1. Signal Generator
- 2. Amplifier
- 3. Directional Coupler
- 4. Power Meter
- 5. 2450 MHz Dipole

The output power on dipole port must be calibrated to 100 mW (20 dBm) before dipole is connected.

8.3. Validation Results

Comparing to the original SAR value provided by Speag, the validation data should within its specification of 10 %. Table 8.1 shows the target SAR and measured SAR after normalized to 1W input power.

		Target (W/kg)	Measurement data (W/kg)	Variation
ISM band	SAR (1g)	56	53.1	5.18 %
(2450 MHz)	SAR (10g)	25.8	24.2	6.20 %

Table 8.1

The table above indicates the system performance check can meet the variation criterion.

9. Description for DUT Testing Position

This DUT was tested in 2 different positions. The first one is "NB Bottom Touch" shown in Fig. 9.1. In this position, the bottom of the laptop is touched with the flat phantom.



Fig. 9.1

The second position are "NB Bottom with 1.5cm Gap" in Fig. 9.2 In this position, the bottom face of the DUT has 1.5cm gap with the flat phantom.



Fig. 9.2

10. Measurement Procedures

The measurement procedures are as follows:

- Plugging DUT into the notebook
- Using engineering software to transmit RF power continuously (continuous Tx) in the low channel
- ▶ Placing the DUT in the positions described in the last section
- Setting scan area, grid size and other setting on the DASY4 software
- Taking data for the low channel
- Repeat the previous steps for the middle and high channels.

According to the IEEE P1528 draft standard, the recommended procedure for assessing the peak spatial-average SAR value consists of the following steps:

- Power reference measurement
- > Area scan
- > Zoom scan
- > Power reference measurement

10.1. Spatial Peak SAR Evaluation

The procedure for spatial peak SAR evaluation has been implemented according to the IEEE1528-200X standard. It can be conducted for 1g and 10g, as well as for user-specific masses. The DASY4 software includes all numerical procedures necessary to evaluate the spatial peak SAR value.

Base on the Draft: SCC-34, SC-2, WG-2-Computational Dosimetry, IEEE P1529/D0.0 (Draft Recommended Practice for Determining the Spatial-Peal Specific Absorption Rate (SAR) Associated with the Use of Wireless Handset-Computational techniques), a new algorithm has been implemented. The spatial-peak SAR can be computed over any required mass.

The base for the evaluation is a "cube" measurement. The measured volume must include the 1g and 10g cubes with the highest averaged SAR values. For that purpose, the center of the measured volume is aligned to the interpolated peak SAR value of a previously performed area scan.

The entire evaluation of the spatial peak values is performed within the postprocessing engine (SEMCAD). The system always gives the maximum values for the 1g and 10g cubes. The algorithm to find the cube with highest averaged SAR is divided into the following stages:

- extraction of the measured data (grid and values) from the Zoom Scan
- calculation of the SAR value at every measurement point based on all stored data (A/D values and measurement parameters)
- generation of a high-resolution mesh within the measured volume
- interpolation of all measured values form the measurement grid to the high-resolution grid
- extrapolation of the entire 3-D field distribution to the phantom surface over the distance from sensor to surface
- calculation of the averaged SAR within masses of 1g and 10g

10.2. Scan Procedures

First **Area Scan** is used to locate the approximate location(s) of the local peak SAR value(s). The measurement grid within an **Area Scan** is defined by the grid extent, grid step size and grid offset. Next, in order to determine the EM field distribution in a three-dimensional spatial extension, **Zoom Scan** is required. The **Zoom Scan** measures 7x7x7 points with step size 5, 5 and 5 mm. The **Zoom Scan** is performed around the highest E-field value to determine the averaged SAR-distribution over 1 g.

10.3. SAR Averaged Methods

In DASY4, the interpolation and extrapolation are both based on the modified Quadratic Shepard's method. The interpolation scheme combines a least-square fitted function method and a weighted average method which are the two basic types of computational interpolation and approximation. Extrapolation routines are used to obtain SAR values between the lowest measurement points and the inner phantom surface. The extrapolation distance is determined by the surface detection distance and the probe sensor offset. The uncertainty increases with the extrapolation distance. To keep the uncertainty within 1% for the 1 g and 10 g cubes, the extrapolation distance should not be larger then 5 mm.

Test Report No : O432406-F

11.SAR Test Results 11.1. DUT BTM Touch

Mode	Chan.	Freq (MHz)	Modulation type	Conducted Power (dBm)	Power Drift (dB)	Measured 1g SAR (W/kg)	Limits (W/Kg)	Results
802.11b	1	2412(Low)	CCK	17.5	-0.2	0.594	1.6	Pass
	6	2437(Mid)	CCK	17.4	-0.1	0.706	1.6	Pass
	11	2462(High)	CCK	17.6	-0.2	0.675	1.6	Pass
802.11.g	1	2412(Low)	OFDM	18.0	0.2	0.213	1.6	Pass
	6	2437(Mid)	OFDM	18.1	-0.1	0.294	1.6	Pass
	11	2462(High)	OFDM	17.8	-0.2	0.286	1.6	Pass

11.2. DUT BTM with 1.5 cm Gap

Mode	Chan.	Freq (MHz)	Modulation type	Conducted Power (dBm)	Power Drift (dB)	Measured 1g SAR (W/kg)		Results
802.11b	1	2412(Low)	CCK	17.5	-	-	-	-
	6	2437(Mid)	CCK	17.4	0.2	0.1170	1.6	Pass
	11	2462(High)	CCK	17.6	-	-	-	-
802.11g	1	2412(Low)	OFDM	18.0	-	_	-	-
	6	2437(Mid)	OFDM	18.1	-0.03	0.0479	1.6	Pass
	11	2462(High)	OFDM	17.8	-	_	-	-

12.References

- [1] FCC 47 CFR Part 2 "Frequency Allocations and Radio Treaty Matters; General Rules and Regulations"
- [2] IEEE Std. 1528-200X, Draft CD 1.1 "Recommended Practice for Determining the Spatial-Peak Specific Absorption Rate (SAR) in the Human Body Due to Wireless Communications Devices: Experimental Techniques", December 2002
- [3] Supplement C (Edition 01-10) to OET Bulletin 65 (Edition 97-01), "Additional Information for Evaluating Compliance of Mobile and Portable Devices with FCC Limits for Human Exposure to RF Emissions", June 2001
- [4] IEEE Std. C95.3, "IEEE Recommended Practice for the Meaurement of Potentially Hazardous Electromagnetic Fields-RF and Microwave", 1991
- [5] IEEE Std. C95.1, "IEEE Standard for Safety Levels with Respect to Human Exposure to Radio Frequency Electromagnetic Fields, 3 kHz to 300 GHz", 1999
- [6] Robert J. Renka, "Multivariate Interpolation Of Large Sets Of Scattered Data", University of Noth Texas ACM Transactions on Mathematical Software, vol. 14, no. 2, June 1988, pp. 139-148
- [7] DAYS4 System Handbook

Test Report No : O432406-F

Appendix A - System Performance Check Data

Date/Time: 04/26/04 15:07:10

Test Report No : 0432406-F

Test Laboratory: SPORTON

2.4GHz Diploe System Calbration

DUT: Dipole 2450 MHz; Type: D2450V2; Serial: D2450V2 - SN:736 Program Name: System Performance Check

Communication System: CW; Frequency: 2450 MHz; Duty Cycle: 1:1 Medium: M2450 (σ = 1.96866 mho/m, ε_r = 52.584, ρ = 1000 kg/m³)

Phantom section: Flat Section; Ambient Temp=21~23C; Liquid Temp=21.5C; Liquid height=15.2cm

DASY4 Configuration:

- Probe: ET3DV6 SN1788; ConvF(4.5, 4.5, 4.5); Calibrated: 8/29/2003
- Sensor-Surface: 4mm (Mechanical Surface Detection)
- Electronics: DAE3 Sn577; Calibrated: 11/21/2003
- Phantom: SAM 12; Type: QD 000 P40 C; Serial: TP-1150
- Measurement SW: DASY4, V4.1 Build 47; Postprocessing SW: SEMCAD, V1.6 Build 116

Pin = 100mW; d = 10mm/Area Scan (51x51x1): Measurement grid: dx=15mm, dy=15mm

Reference Value = 56.9 V/m

Power Drift = -0.04 dB

Maximum value of SAR = 6.15 mW/g

Pin = 100mW; d = 10mm/Zoom Scan (7x7x7)/Cube 0: Measurement grid: dx=5mm, dy=5mm, dz=5mm


Peak SAR (extrapolated) = 11.4 W/kg

SAR(1 g) = 5.31 mW/g; SAR(10 g) = 2.42 mW/g

Reference Value = 56.9 V/m

Power Drift = -0.04 dB

Maximum value of SAR = 5.92 mW/g

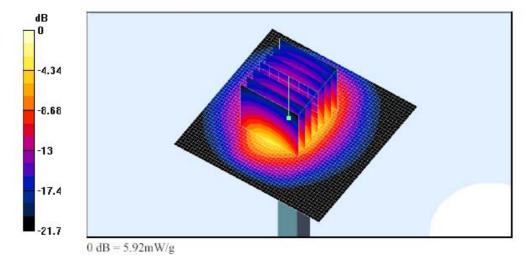

Appendix B - SAR Measurement Data

Date/Time: 04/26/04 16:14:42

Test Laboratory: SPORTON

NB BTM Touch CH 01

DUT: AMIGO; Type: USB Dongle Program Name: NB BTM Touch

Communication System: 802.11b ; Frequency: 2412 MHz; Duty Cycle: 1:1 Medium: MSL2450 (σ = 1.9206 mho/m, ϵ_r = 52.8945, ρ = 1000 kg/m³)

Phantom section: Flat Section; Ambient Temp=21~23C; Liquid Temp=21.5C; Liquid height=15.2cm

DASY4 Configuration:

- Probe: ET3DV6 SN1788; ConvF(4.5, 4.5, 4.5); Calibrated: 8/29/2003
- Sensor-Surface: 4mm (Mechanical Surface Detection)
- Electronics: DAE3 Sn577; Calibrated: 11/21/2003
- Phantom: SAM 12; Type: QD 000 P40 C; Serial: TP-1150
- Measurement SW: DASY4, V4.1 Build 47; Postprocessing SW: SEMCAD, V1.6 Build 116

Channel 1 2412MHz/Area Scan (81x71x1): Measurement grid: dx=10mm, dy=10mm

Reference Value = 14.4 V/m

Power Drift = -0.2 dB

Maximum value of SAR = 0.695 mW/g

Channel 1 2412MHz/Zoom Scan (7x7x7)/Cube 0: Measurement grid: dx=5mm, dy=5mm, dz=5mm


Peak SAR (extrapolated) = 1.27 W/kg

SAR(1 g) = 0.594 mW/g; SAR(10 g) = 0.297 mW/g

Reference Value = 14.4 V/m

Power Drift = -0.2 dB

Maximum value of SAR = 0.638 mW/g

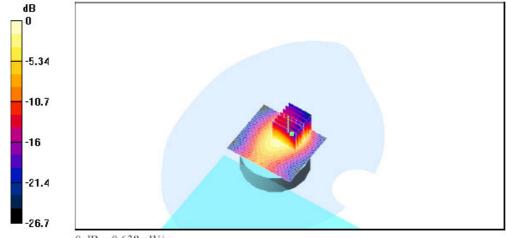

0 dB = 0.638 mW/g

Date/Time: 04/26/04 16:42:24

Test Laboratory: SPORTON

NB BTM Touch CH 06

DUT: AMIGO; Type: USB Dongle Program Name: NB BTM Touch

Communication System: 802.11b; Frequency: 2437 MHz; Duty Cycle: 1:1 Medium: MSL2450 (σ = 1.9496 mho/m, ε_r = 52.6733, ρ = 1000 kg/m³)

Phantom section: Flat Section; Ambient Temp=21~23C; Liquid Temp=21.5C; Liquid height=15.2cm

DASY4 Configuration:

- Probe: ET3DV6 SN1788; ConvF(4.5, 4.5, 4.5); Calibrated; 8/29/2003
- Sensor-Surface: 4mm (Mechanical Surface Detection)
- Electronics: DAE3 Sn577; Calibrated: 11/21/2003
- Phantom: SAM 12; Type: QD 000 P40 C; Serial: TP-1150
- Measurement SW: DASY4, V4.1 Build 47; Postprocessing SW: SEMCAD, V1.6 Build 116

Channel 6 2437MHz/Area Scan (81x71x1): Measurement grid: dx=10mm, dy=10mm

Reference Value = 16.4 V/m Power Drift = -0.1 dB

Maximum value of SAR = 0.821 mW/g

Channel 6 2437MHz/Zoom Scan (7x7x7)/Cube 0: Measurement grid: dx=5mm, dy=5mm, dz=5mm


Peak SAR (extrapolated) = 1.54 W/kg

SAR(1 g) = 0.706 mW/g; SAR(10 g) = 0.351 mW/g

Reference Value = 16.4 V/m

Power Drift = -0.1 dB

Maximum value of SAR = 0.763 mW/g

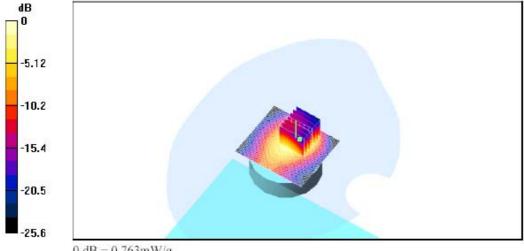

0 dB = 0.763 mW/g

Date/Time: 04/26/04 17:10:32

Test Laboratory: SPORTON

NB BTM Touch CH 11

DUT: AMIGO; Type: USB Dongle Program Name: NB BTM Touch

Communication System: 802.11b; Frequency: 2462 MHz; Duty Cycle: 1:1 Medium: MSL2450 (σ = 1.98739 mho/m, ϵ_r = 52.5473, ρ = 1000 kg/m³)

Phantom section: Flat Section; Ambient Temp=21~23C; Liquid Temp=21.5C; Liquid height=15.2cm

DASY4 Configuration:

- Probe: ET3DV6 SN1788; ConvF(4.5, 4.5, 4.5); Calibrated: 8/29/2003
- Sensor-Surface: 4mm (Mechanical Surface Detection)
- Electronics; DAE3 Sn577; Calibrated: 11/21/2003
- Phantom: SAM 12; Type: QD 000 P40 C; Serial: TP-1150
- Measurement SW: DASY4, V4.1 Build 47; Postprocessing SW: SEMCAD, V1.6 Build 116

Channel 11 2462MHz/Area Scan (81x71x1): Measurement grid: dx=10mm, dy=10mm

Reference Value = 16 V/m

Power Drift = -0.2 dB

Maximum value of SAR = 0.769 mW/g

Channel 11 2462MHz/Zoom Scan (7x7x7)/Cube 0: Measurement grid: dx=5mm, dy=5mm, dz=5mm


Peak SAR (extrapolated) = 1.44 W/kg

SAR(1 g) = 0.675 mW/g; SAR(10 g) = 0.337 mW/g

Reference Value = 16 V/m

Power Drift = -0.2 dB

Maximum value of SAR = 0.73 mW/g

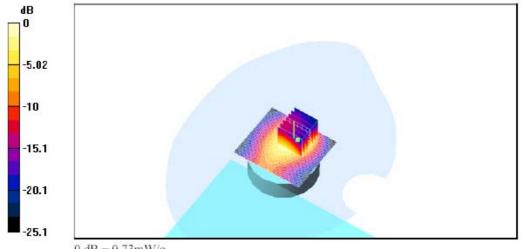

Date/Time: 04/26/04 18:44:44

Test Laboratory: SPORTON

NB BTM Touch CH 01

DUT: AMIGO; Type: USB Dongle Program Name: NB BTM Touch

Communication System: 802.11g ; Frequency: 2412 MHz;Duty Cycle: 1:1 Medium: MSL2450 (σ = 1.9206 mho/m, ϵ_r = 52.8945, ρ = 1000 kg/m³)

Phantom section: Flat Section; Ambient Temp=21~23C; Liquid Temp=21.5C; Liquid height=15.2cm

DASY4 Configuration:

- Probe: ET3DV6 SN1788; ConvF(4.5, 4.5, 4.5); Calibrated: 8/29/2003
- Sensor-Surface: 4mm (Mechanical Surface Detection)
- Electronics: DAE3 Sn577; Calibrated: 11/21/2003
- Phantom: SAM 12; Type: QD 000 P40 C; Serial: TP-1150
- Measurement SW: DASY4, V4.1 Build 47; Postprocessing SW: SEMCAD, V1.6 Build 116

Channel 1 2412MHz/Area Scan (81x71x1): Measurement grid: dx=10mm, dy=10mm

Reference Value = 9.49 V/m

Power Drift = 0.2 dB

Maximum value of SAR = 0.234 mW/g

Channel 1 2412MHz/Zoom Scan (7x7x7)/Cube 0: Measurement grid: dx=5mm, dy=5mm, dz=5mm


Peak SAR (extrapolated) = 0.447 W/kg

SAR(1 g) = 0.213 mW/g; SAR(10 g) = 0.107 mW/g

Reference Value = 9.49 V/m

Power Drift = 0.2 dB

Maximum value of SAR = 0.23 mW/g

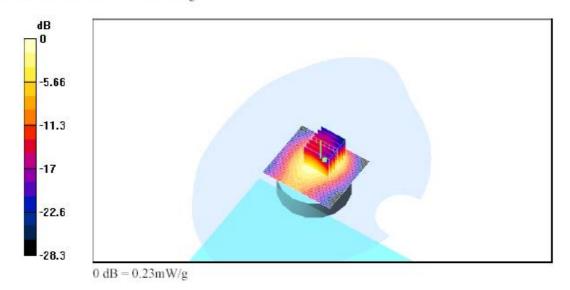

Date/Time: 04/26/04 19:07:00

Test Laboratory: SPORTON

NB BTM Touch CH 06

DUT: AMIGO; Type: USB Dongle Program Name: NB BTM Touch

Communication System: 802.11g; Frequency: 2437 MHz; Duty Cycle: 1:1 Medium: MSL2450 (σ = 1.9496 mho/m, ϵ_r = 52.6733, ρ = 1000 kg/m³)

Phantom section: Flat Section; Ambient Temp=21~23C; Liquid Temp=21.5C; Liquid height=15.2cm

DASY4 Configuration:

- Probe: ET3DV6 SN1788; ConvF(4.5, 4.5, 4.5); Calibrated: 8/29/2003
- Sensor-Surface: 4mm (Mechanical Surface Detection)
- Electronics: DAE3 Sn577; Calibrated: 11/21/2003
- Phantom: SAM 12; Type: QD 000 P40 C; Serial: TP-1150
- Measurement SW: DASY4, V4.1 Build 47; Postprocessing SW: SEMCAD, V1.6 Build 116

Channel 6 2437MHz/Area Scan (81x71x1): Measurement grid: dx=10mm, dy=10mm

Reference Value = 9.66 V/m

Power Drift = -0.1 dB

Maximum value of SAR = 0.33 mW/g

Channel 6 2437MHz/Zoom Scan (7x7x7)/Cube 0: Measurement grid: dx=5mm, dy=5mm, dz=5mm


Peak SAR (extrapolated) = 0.64 W/kg

SAR(1 g) = 0.294 mW/g; SAR(10 g) = 0.146 mW/g

Reference Value = 9.66 V/m

Power Drift = -0.1 dB

Maximum value of SAR = 0.316 mW/g

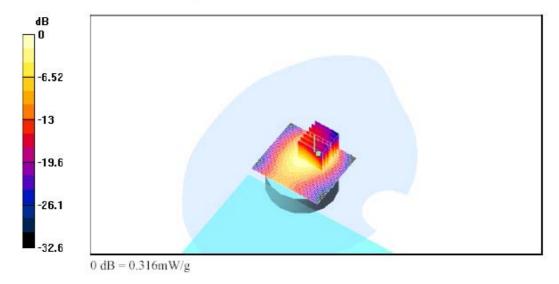

Date/Time: 04/26/04 19:55:48

Test Laboratory: SPORTON

NB BTM Touch CH 11

DUT: AMIGO; Type: USB Dongle Program Name: NB BTM Touch

Communication System: 802.11g; Frequency: 2462 MHz; Duty Cycle: 1:1 Medium: MSL2450 ($\sigma = 1.98739 \text{ mho/m}, \epsilon_r = 52.5473, \rho = 1000 \text{ kg/m}^3$)

Phantom section: Flat Section; Ambient Temp=21~23C; Liquid Temp=21.5C; Liquid height=15.2cm

DASY4 Configuration:

- Probe: ET3DV6 SN1788; ConvF(4.5, 4.5, 4.5); Calibrated: 8/29/2003
- Sensor-Surface: 4mm (Mechanical Surface Detection)
- Electronics: DAE3 Sn577; Calibrated: 11/21/2003
- Phantom: SAM 12; Type: QD 000 P40 C; Serial: TP-1150
- Measurement SW: DASY4, V4.1 Build 47; Postprocessing SW: SEMCAD, V1.6 Build 116

Channel 11 2462MHz/Area Scan (81x71x1): Measurement grid: dx=10mm, dy=10mm

Reference Value = 10.1 V/m

Power Drift = -0.2 dB

Maximum value of SAR = 0.331 mW/g

Channel 11 2462MHz/Zoom Scan (7x7x7)/Cube 0: Measurement grid: dx=5mm, dy=5mm, dz=5mm


Peak SAR (extrapolated) = 0.594 W/kg

SAR(1 g) = 0.286 mW/g; SAR(10 g) = 0.143 mW/g

Reference Value = 10.1 V/m

Power Drift = -0.2 dB

Maximum value of SAR = 0.311 mW/g

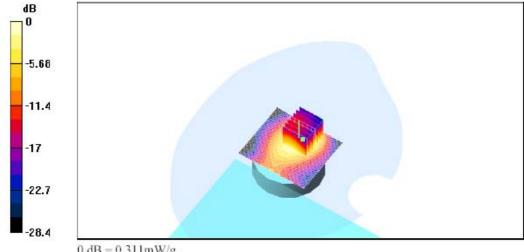

Date/Time: 04/26/04 16:42:24

Test Laboratory: SPORTON

NB BTM Touch CH 06

DUT: AMIGO; Type: USB Dongle Program Name: NB BTM Touch

Communication System: 802.11b; Frequency: 2437 MHz; Duty Cycle: 1:1 Medium: MSL2450 (σ = 1.9496 mho/m, ε_r = 52.6733, ρ = 1000 kg/m³)

Phantom section: Flat Section; Ambient Temp=21~23C; Liquid Temp=21.5C; Liquid height=15.2cm

DASY4 Configuration:

- Probe: ET3DV6 SN1788; ConvF(4.5, 4.5, 4.5); Calibrated: 8/29/2003
- Sensor-Surface: 4mm (Mechanical Surface Detection)
- Electronics: DAE3 Sn577; Calibrated: 11/21/2003
- Phantom: SAM 12; Type: QD 000 P40 C; Serial: TP-1150
- Measurement SW: DASY4, V4.1 Build 47; Postprocessing SW: SEMCAD, V1.6 Build 116

Channel 6 2437MHz/Area Scan (81x71x1): Measurement grid: dx=10mm, dy=10mm

Reference Value = 16.4 V/m

Power Drift = -0.1 dB

Maximum value of SAR = 0.821 mW/g

Channel 6 2437MHz/Zoom Scan (7x7x7)/Cube 0: Measurement grid: dx=5mm, dy=5mm, dz=5mm

Peak SAR (extrapolated) = 1.54 W/kg

SAR(1 g) = 0.706 mW/g; SAR(10 g) = 0.351 mW/g

Reference Value = 16.4 V/m

Power Drift = -0.1 dB

Maximum value of SAR = 0.763 mW/g





Page 1 (1)

Appendix C – Calibration Data

Calibration Laboratory of Schmid & Partner Engineering AG Zeughausstrasse 43, 8004 Zurich, Switzerland

Client

Auden > Sporton Int. Inc.

Object(s)	D2450V2 - SI	N:736	
Calibration procedure(s)	020000000000000000000000000000000000000	2 ocedure for dipole validation kits	
Calibration date:	August 27, 20	003	
Condition of the calibrated item	In Tolerance	(according to the specific calibration	on document)
17025 international standard.		E used in the calibration procedures and conformity tory facility: environment temperature 22 +/- 2 degree	
Calibration Equipment used (M&1	E critical for calibration)		
fodel Type	ID#	Cal Date (Calibrated by, Certificate No.)	Scheduled Calibration
	ID# 100698	Cal Date (Calibrated by, Certificate No.) 27-Mar-2002 (R&S, No. 20-92389)	Scheduled Calibration In house check: Mar-05
RF generator R&S SML-03			
RF generator R&S SML-03 Power sensor HP 8481A	100698	27-Mar-2002 (R&S, No. 20-92389)	In house check: Mar-05
RF generator R&S SML-03 Power sensor HP 8481A Power sensor HP 8481A	100698 MY41092317	27-Mar-2002 (R&S, No. 20-92389) 18-Oct-02 (Agilent, No. 20021018)	In house check: Mar-05 Oct-04
RF generator R&S SML-03 Power sensor HP 8481A Power sensor HP 8481A Power meter EPM E442	100698 MY41092317 US37292783	27-Mar-2002 (R&S, No. 20-92389) 18-Oct-02 (Agilent, No. 20021018) 30-Oct-02 (METAS, No. 252-0236)	In house check: Mar-05 Oct-04 Oct-03
Model Type RF generator R&S SML-03 Power sensor HP 8481A Power sensor HP 8481A Power meter EPM E442 Network Analyzer HP 8753E	100698 MY41092317 US37292783 GB37480704 US37390585	27-Mar-2002 (R&S, No. 20-92389) 18-Oct-02 (Agilent, No. 20021018) 30-Oct-02 (METAS, No. 252-0236) 30-Oct-02 (METAS, No. 252-0236) 18-Oct-01 (Agilent, No. 24BR1033101)	In house check: Mar-05 Oct-04 Oct-03 Oct-03 In house check: Oct 03
RF generator R&S SML-03 Power sensor HP 8481A Power sensor HP 8481A Power meter EPM E442	100698 MY41092317 US37292783 GB37480704 US37390585	27-Mar-2002 (R&S, No. 20-92389) 18-Oct-02 (Agilent, No. 20021018) 30-Oct-02 (METAS, No. 252-0236) 30-Oct-02 (METAS, No. 252-0236)	In house check: Mar-05 Oct-04 Oct-03 Oct-03
RF generator R&S SML-03 Power sensor HP 8481A Power sensor HP 8481A Power meter EPM E442 Network Analyzer HP 8753E	100698 MY41092317 US37292783 GB37480704 US37390585	27-Mar-2002 (R&S, No. 20-92389) 18-Oct-02 (Agilent, No. 20021018) 30-Oct-02 (METAS, No. 252-0236) 30-Oct-02 (METAS, No. 252-0236) 18-Oct-01 (Agilent, No. 24BR1033101) Function	In house check: Mar-05 Oct-04 Oct-03 Oct-03 In house check: Oct 03
RF generator R&S SML-03 Power sensor HP 8481A Power sensor HP 8481A Power meter EPM E442 Network Analyzer HP 8753E Calibrated by:	100698 MY41092317 US37292783 GB37480704 US37390585	27-Mar-2002 (R&S, No. 20-92389) 18-Oct-02 (Agilent, No. 20021018) 30-Oct-02 (METAS, No. 252-0236) 30-Oct-02 (METAS, No. 252-0236) 18-Oct-01 (Agilent, No. 24BR1033101) Function	In house check: Mar-05 Oct-04 Oct-03 Oct-03 In house check: Oct 03
RF generator R&S SML-03 Power sensor HP 8481A Power sensor HP 8481A Power meter EPM E442 Network Analyzer HP 8753E	100698 MY41092317 US37292783 GB37480704 US37390585 Name	27-Mar-2002 (R&S, No. 20-92389) 18-Oct-02 (Agilent, No. 20021018) 30-Oct-02 (METAS, No. 252-0236) 30-Oct-02 (METAS, No. 252-0236) 18-Oct-01 (Agilent, No. 24BR1033101) Function Technician	In house check: Mar-05 Oct-04 Oct-03 Oct-03 In house check: Oct 03
RF generator R&S SML-03 Power sensor HP 8481A Power sensor HP 8481A Power meter EPM E442 Network Analyzer HP 8753E Calibrated by:	100698 MY41092317 US37292783 GB37480704 US37390585 Name	27-Mar-2002 (R&S, No. 20-92389) 18-Oct-02 (Agilent, No. 20021018) 30-Oct-02 (METAS, No. 252-0236) 30-Oct-02 (METAS, No. 252-0236) 18-Oct-01 (Agilent, No. 24BR1033101) Function Technician	In house check: Mar-05 Oct-04 Oct-03 Oct-03 In house check: Oct 03 Signature Date issued: August 28, 2003

880-KP0301061-A



Schmid & Partner Engineering AG

s p e a q

Zeughausstrasse 43, 8004 Zurich, Switzerland Phone +41 1 245 9700, Fax +41 1 245 9779 info@speag.com, http://www.speag.com

DASY

Dipole Validation Kit

Type: D2450V2

Serial: 736

Manufactured: August 26, 2003 Calibrated: August 27, 2003

1. Measurement Conditions

The measurements were performed in the flat section of the SAM twin phantom filled with head simulating solution of the following electrical parameters at 2450 MHz:

Relative Dielectricity 38.2 \pm 5% Conductivity 1.89 mho/m \pm 5%

The DASY4 System with a dosimetric E-field probe ES3DV2 (SN:3013, Conversion factor 4.8 at 2450 MHz) was used for the measurements.

The dipole was mounted on the small tripod so that the dipole feedpoint was positioned below the center marking of the flat phantom section and the dipole was oriented parallel to the body axis (the long side of the phantom). The standard measuring distance was 10mm from dipole center to the solution surface. Lossless spacer was used during measurements for accurate distance positioning.

The coarse grid with a grid spacing of 15mm was aligned with the dipole. The 7x7x7 fine cube was chosen for cube integration.

The dipole input power (forward power) was $250mW \pm 3$ %. The results are normalized to 1W input power.

2. SAR Measurement with DASY4 System

Standard SAR-measurements were performed according to the measurement conditions described in section 1. The results (see figure supplied) have been normalized to a dipole input power of 1W (forward power). The resulting averaged SAR-values measured with the dosimetric probe ES3DV2 SN:3013 and applying the <u>advanced extrapolation</u> are:

averaged over 1 cm³ (1 g) of tissue: 55.6 mW/g \pm 16.8 % (k=2)¹

averaged over 10 cm³ (10 g) of tissue: 25.0 mW/g \pm 16.2 % (k=2)¹

1 validation uncertainty

3. Dipole Impedance and Return Loss

The impedance was measured at the SMA-connector with a network analyzer and numerically transformed to the dipole feedpoint. The transformation parameters from the SMA-connector to the dipole feedpoint are:

Electrical delay: 1.158 ns (one direction)

Transmission factor: 0.983 (voltage transmission, one direction)

The dipole was positioned at the flat phantom sections according to section 1 and the distance spacer was in place during impedance measurements.

Feedpoint impedance at 2450 MHz:

 $Re\{Z\} = 52.5 \Omega$

Im $\{Z\} = 3.6 \Omega$

Return Loss at 2450 MHz

-27.5 dB

4. Measurement Conditions

The measurements were performed in the flat section of the SAM twin phantom filled with body simulating solution of the following electrical parameters at 2450 MHz:

Relative Dielectricity

50.8

± 5%

Conductivity

2.03 mho/m ± 5%

The DASY4 System with a dosimetric E-field probe ES3DV2 (SN:3013, Conversion factor 4.2 at 2450 MHz) was used for the measurements.

The dipole was mounted on the small tripod so that the dipole feedpoint was positioned below the center marking of the flat phantom section and the dipole was oriented parallel to the body axis (the long side of the phantom). The standard measuring distance was 10mm from dipole center to the solution surface. Lossless spacer was used during measurements for accurate distance positioning.

The coarse grid with a grid spacing of 15mm was aligned with the dipole. The 7x7x7 fine cube was chosen for cube integration.

The dipole input power (forward power) was $250 \text{mW} \pm 3$ %. The results are normalized to 1W input power.

5. SAR Measurement with DASY4 System

Standard SAR-measurements were performed according to the measurement conditions described in section 4. The results (see figure supplied) have been normalized to a dipole input power of 1W (forward power). The resulting averaged SAR-values measured with the dosimetric probe ES3DV2 SN:3013 and applying the <u>advanced extrapolation</u> are:

averaged over 1 cm3 (1 g) of tissue:

56.0 mW/g \pm 16.8 % (k=2)²

averaged over 10 cm3 (10 g) of tissue:

25.8 mW/g \pm 16.2 % (k=2)²

Dipole Impedance and Return Loss

The dipole was positioned at the flat phantom sections according to section 4 and the distance spacer was in place during impedance measurements.

Feedpoint impedance at 2450 MHz:

 $Re{Z} = 48.7 \Omega$

Im $\{Z\} = 4.8 \Omega$

Return Loss at 2450 MHz

-25.8 dB

7. Handling

Do not apply excessive force to the dipole arms, because they might bend. Bending of the dipole arms stresses the soldered connections near the feedpoint leading to a damage of the dipole.

8. Design

The dipole is made of standard semirigid coaxial cable. The center conductor of the feeding line is directly connected to the second arm of the dipole. The antenna is therefore short-circuited for DC-signals.

Small end caps have been added to the dipole arms in order to improve matching when loaded according to the position as explained in Sections 1 and 4. The SAR data are not affected by this change. The overall dipole length is still according to the Standard.

Power Test

After long term use with 40W radiated power, only a slight warming of the dipole near the feedpoint can be measured.

² validation uncertainty

Page 1 of 1

Date/Time: 08/27/03 15:43:04

Test Laboratory: SPEAG, Zurich, Switzerland File Name: SN736 SN3013 M2450 270803.da4

DUT: Dipole 2450 MHz; Type: D2450V2; Serial: D2450V2 - SN736

Program: Dipole Calibration

Communication System: CW-2450; Frequency: 2450 MHz; Duty Cycle: 1:1 Medium: Muscle 2450 MHz ($\sigma = 2.03 \text{ mho/m}, \epsilon_r = 50.75, \rho = 1000 \text{ kg/m}^3$)

Phantom section: Flat Section

Measurement Standard: DASY4 (High Precision Assessment)

DASY4 Configuration:

- Probe: ES3DV2 SN3013; ConvF(4.2, 4.2, 4.2); Calibrated: 1/19/2003
- · Sensor-Surface: 4mm (Mechanical Surface Detection)
- Electronics: DAE3 SN411; Calibrated: 1/16/2003
- Phantom: SAM with CRP TP1006; Type: SAM 4.0; Serial: TP:1006
- Measurement SW: DASY4, V4.1 Build 47; Postprocessing SW: SEMCAD, V1.6 Build 115

Pin = 250 mW; d = 10 mm/Area Scan (81x81x1): Measurement grid: dx=15mm, dy=15mm.

Reference Value = 91 V/m

Power Drift = -0.02 dB

Maximum value of SAR = 15.7 mW/g

Pin = 250 mW; d = 10 mm/Zoom Scan (7x7x7)/Cube 0: Measurement grid: dx=5mm, dy=5mm,


dz=5mm


Peak SAR (extrapolated) = 27.8 W/kg

SAR(1 g) = 14 mW/g; SAR(10 g) = 6.46 mW/gReference Value = 91 V/m

Power Drift = -0.02 dB

Maximum value of SAR = 16 mW/g

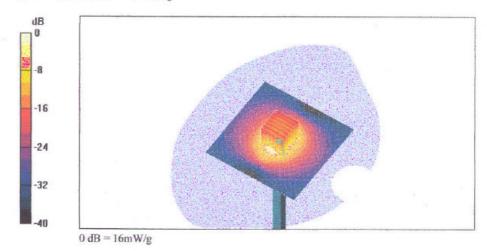

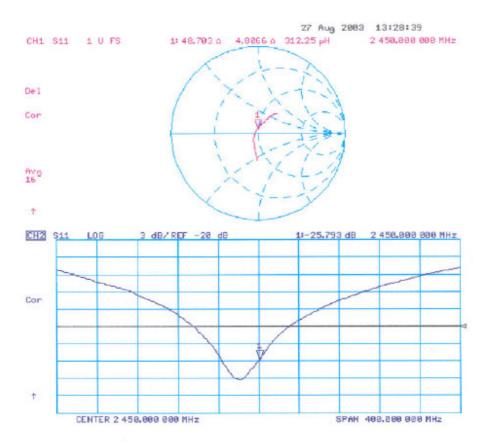

Page 1 of 1

Date/Time: 08/27/03 11:42:12

Test Laboratory: SPEAG, Zurich, Switzerland File Name: SN736_SN3013_HSL2450_270803.da4

DUT: Dipole 2450 MHz; Type: D2450V2; Serial: D2450V2 - SN736 Program: Dipole Calibration

Communication System: CW-2450; Frequency: 2450 MHz; Duty Cycle: 1:1 Medium: HSL 2450 MHz ($\sigma = 1.89 \text{ mho/m}$, $\epsilon_r = 38.19$, $\rho = 1000 \text{ kg/m}^3$)

Phantom section: Flat Section

Measurement Standard: DASY4 (High Precision Assessment)

DASY4 Configuration:

- Probe: ES3DV2 SN3013; ConvF(4.8, 4.8, 4.8); Calibrated: 1/19/2003
- · Sensor-Surface: 4mm (Mechanical Surface Detection)
- Electronics: DAE3 SN411; Calibrated: 1/16/2003
- Phantom: SAM with CRP TP1006; Type: SAM 4.0; Serial: TP:1006
- Measurement SW: DASY4, V4.1 Build 47; Postprocessing SW: SEMCAD, V1.6 Build 115

Pin = 250 mW; d = 10 mm/Area Scan (81x81x1): Measurement grid: dx=15mm, dy=15mm Reference Value = 91.5 V/m

Power Drift = -0.04 dB

Maximum value of SAR = 15.3 mW/g


Pin = 250 mW; d = 10 mm/Zoom Scan (7x7x7)/Cube 0: Measurement grid: dx=5mm, dy=5mm, dz=5mm


Peak SAR (extrapolated) = 30.2 W/kg

SAR(1 g) = 13.9 mW/g; SAR(10 g) = 6.25 mW/g Reference Value = 91.5 V/m

Power Drift = -0.04 dB

Maximum value of SAR = 15.5 mW/g

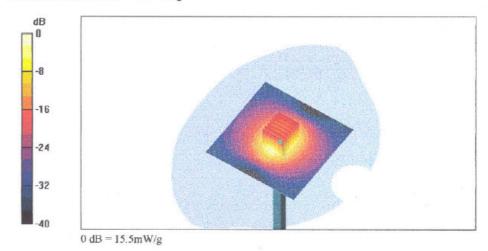

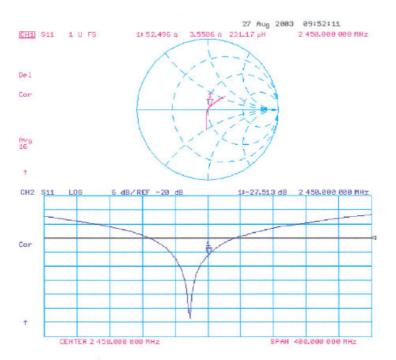



Calibration Laboratory of Schmid & Partner Engineering AG Zeughausstrasse 43, 8004 Zurich, Switzerland

Client

Auden > Sporton Int. Inc.

Object(s)	ET3DV6 - SN:	1788	
Calibration procedure(s)	QA CAL-01.v2		
	Calibration pro	ocedure for dosimetric E-field probe	es ·
Calibration date:	August 29, 20	03	
Condition of the calibrated item	In Tolerance (a	according to the specific calibration	n document)
his calibration statement documen 7025 international standard.	ts traceability of M&TE	used in the calibration procedures and conformity of	f the procedures with the ISO/IEC
Il calibrations have been conducte	d in the closed laborato	ry facility: environment temperature 22 +/- 2 degrees	s Celsius and humidity < 75%.
alibration Equipment used (M&TE	critical for calibration)		
Model Type	ID#	Cal Date (Calibrated by, Certificate No.)	Scheduled Calibration
	ID# US3642U01700	Cal Date (Calibrated by, Certificate No.) 4-Aug-99 (SPEAG, in house check Aug-02)	Scheduled Calibration In house check: Aug-05
RF generator HP 8684C			
RF generator HP 8684C Power sensor E4412A Power sensor HP 8481A	US3642U01700 MY41495277 MY41092180	4-Aug-99 (SPEAG, in house check Aug-02)	In house check: Aug-05
Model Type RF generator HP 8684C Power sensor E4412A Power sensor HP 8481A Power meter EPM E4419B	US3642U01700 MY41495277	4-Aug-99 (SPEAG, in house check Aug-02) 2-Apr-03 (METAS, No 252-0250)	In house check: Aug-05 Apr-04
RF generator HP 8684C Power sensor E4412A Power sensor HP 8481A Power meter EPM E4419B lietwork Analyzer HP 8753E	US3842U01700 MY41495277 MY41092180 GB41293874 US37390585	4-Aug-99 (SPEAG, in house check Aug-02) 2-Apr-03 (METAS, No 252-0250) 18-Sep-02 (Agilent, No. 20020918) 2-Apr-03 (METAS, No 252-0250) 18-Oct-01 (Agilent, No. 24BR1033101)	In house check: Aug-05 Apr-04 Sep-03 Apr-04 In house check: Oct 03
RF generator HP 8684C Power sensor E4412A Power sensor HP 8481A	US3642U01700 MY41495277 MY41092180 GB41293874	4-Aug-99 (SPEAG, in house check Aug-02) 2-Apr-03 (METAS, No 252-0250) 18-Sep-02 (Agilent, No. 20020918) 2-Apr-03 (METAS, No 252-0250)	In house check: Aug-05 Apr-04 Sep-03 Apr-04
RF generator HP 8684C Power sensor E4412A Power sensor HP 8481A Power meter EPM E4419B Network Analyzer HP 8753E	US3842U01700 MY41495277 MY41092180 GB41293874 US37390585	4-Aug-99 (SPEAG, in house check Aug-02) 2-Apr-03 (METAS, No 252-0250) 18-Sep-02 (Agilent, No. 20020918) 2-Apr-03 (METAS, No 252-0250) 18-Oct-01 (Agilent, No. 24BR1033101)	In house check: Aug-05 Apr-04 Sep-03 Apr-04 In house check: Oct 03
RF generator HP 8684C Power sensor E4412A Power sensor HP 8481A Power meter EPM E4419B Network Analyzer HP 8753E	US3642U01700 MY41495277 MY41092160 GB41293874 US37390585 SN: 6295803	4-Aug-99 (SPEAG, in house check Aug-02) 2-Apr-03 (METAS, No 252-0250) 18-Sep-02 (Agilent, No. 20020918) 2-Apr-03 (METAS, No 252-0250) 18-Oct-01 (Agilent, No. 24BR1033101) 3-Sep-01 (ELCAL, No.2360)	In house check: Aug-05 Apr-04 Sep-03 Apr-04 In house check: Oct 03 Sep-03
RF generator HP 8684C Power sensor E4412A Power sensor HP 8481A Power meter EPM E4419B Jetwork Analyzer HP 8753E Fluke Process Calibrator Type 702	US3842U01700 MY41495277 MY41092160 GB41293874 US37390585 SN: 6295803	4-Aug-99 (SPEAG, in house check Aug-02) 2-Apr-03 (METAS, No 252-0250) 18-Sep-02 (Agilent, No. 20020918) 2-Apr-03 (METAS, No 252-0250) 18-Oct-01 (Agilent, No. 24BR1033101) 3-Sep-01 (ELCAL, No.2360)	In house check: Aug-05 Apr-04 Sep-03 Apr-04 In house check: Oct 03 Sep-03
RF generator HP 8684C Power sensor E4412A Power sensor HP 8481A Power meter EPM E4419B Jetwork Analyzer HP 8753E Pluke Process Celibrator Type 702 Calibrated by:	US3642U01700 MY41495277 MY41092180 GB41293874 US37390585 SN: 6295803 Name	4-Aug-99 (SPEAG, in house check Aug-02) 2-Apr-03 (METAS, No 252-0250) 18-Sep-02 (Agilent, No. 20020918) 2-Apr-03 (METAS, No 252-0250) 18-Oct-01 (Agilent, No. 24BR1033101) 3-Sep-01 (ELCAL, No 2360) Function Technician	In house check: Aug-05 Apr-04 Sep-03 Apr-04 In house check: Oct 03 Sep-03
RF generator HP 8684C lower sensor E4412A lower sensor HP 8481A lower meter EPM E4419B letwork Analyzer HP 8753E sluke Process Calibrator Type 702 calibrated by:	US3842U01700 MY41495277 MY41092180 GB41293874 US37390585 SN: 6295803 Name Nico Vetters	4-Aug-99 (SPEAG, in house check Aug-02) 2-Apr-03 (METAS, No 252-0250) 18-Sep-02 (Agilent, No. 20020918) 2-Apr-03 (METAS, No 252-0250) 18-Oct-01 (Agilent, No. 24BR1033101) 3-Sep-01 (ELCAL, No 2360) Function Technician	In house check: Aug-05 Apr-04 Sep-03 Apr-04 In house check: Oct 03 Sep-03 Signature Date issued: August 28, 2003

880-KP0301061-A

Page 1 (1)



Schmid & Partner Engineering AG

s p e a g

Zeughausstrasse 43, 8004 Zurich, Switzerland Phone +41 1 245 9700, Fax +41 1 245 9779 info@speag.com, http://www.speag.com

Probe ET3DV6

SN:1788

Manufactured: Last calibration:

May 28, 2003 August 29, 2003

Calibrated for DASY Systems

(Note: non-compatible with DASY2 system!)

August 29, 2003 ET3DV6 SN:1788

DASY - Parameters of Probe: ET3DV6 SN:1788

Sensitiv	vity in Free	Spac	е		Diode	Compression	on	
	NormX		1.68 μV/	/(V/m) ²		DCP X	95	mV
	NormY		1.62 μV	/(V/m) ²		DCP Y	95	mV
	NormZ		1.71 μV	/(V/m) ²		DCP Z	95	mV
Sensitiv	rity in Tissue	Simu	lating Li	quid				
Head	90	0 MHz		ε _r = 41.5 :	£ 5%	$\sigma = 0.97 \pm 5\%$	mho/m	
Valid for f=	800-1000 MHz v	vith Head	Tissue Simu	ulating Liquid acc	cording to EN 5	0361, P1528-200	x	
	ConvF X		6.6 ±9	.5% (k=2)		Boundary e	ffect:	
	ConvF Y		6.6 ±9	.5% (k=2)		Alpha	0.34	
	ConvF Z		6.6 ±9	.5% (k=2)		Depth	2.48	
Head	180	0 MHz		ε _r = 40.0 :	± 5%	σ= 1.40 ± 5%	mho/m	
Valid for f=	1710-1910 MHz	with Hea	d Tissue Sin	nulating Liquid a	ccording to EN	50361, P1528-20	OX	
	ConvF X		5.3 ±9	.5% (k=2)		Boundary e	ffect:	
	ConvF Y		5.3 ±9	.5% (k=2)		Alpha	0.43	
	ConvF Z		5.3 ±9	.5% (k=2)		Depth	2.80	
Bounda	ry Effect							
Head	90	0 MHz	Тур	oical SAR gradi	ent: 5 % per n	nm		
	Probe Tip to	Boundar	y			1 mm	2 mm	
	SAR _{be} [%]	Withou	ut Correctio	n Algorithm		8.7	5.0	
	SAR _{be} [%]	With C	Correction A	lgorithm		0.3	0.5	
Head	180	0 MHz	Тур	oical SAR gradi	ent: 10 % per	mm		
	Probe Tip to	Boundar	v			1 mm	2 mm	
	SAR _{be} [%]			n Algorithm		12.8	8.9	
	SAR _{be} [%]	With C	Correction A	lgorithm		0.3	0.1	
Sensor	Offset							
an Factorisa de Falla	Probe Tip to	Sensor C	Center		2.7		mm	
	Optical Surfa	ce Detec	tion		1.6 ± 0	0.2	mm	

Page 2 of 10




ET3DV6 SN:1788

Test Report No : O432406-F

August 29, 2003


Receiving Pattern (ϕ), θ = 0°

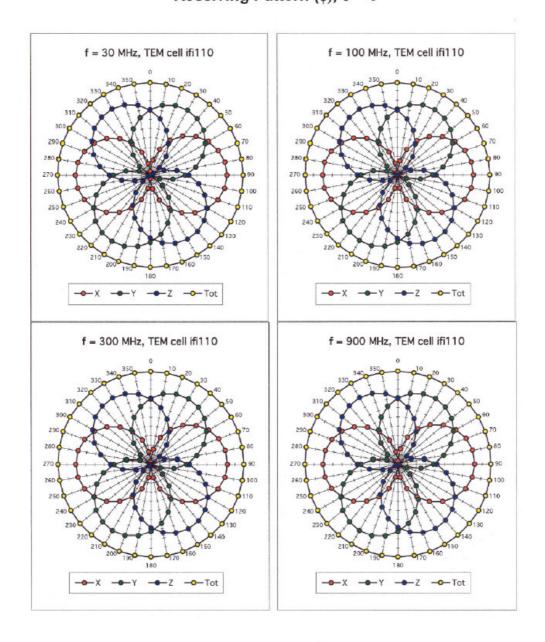


Page 3 of 10


ET3DV6 SN:1788

August 29, 2003





Isotropy Error (ϕ), $\theta = 0^{\circ}$

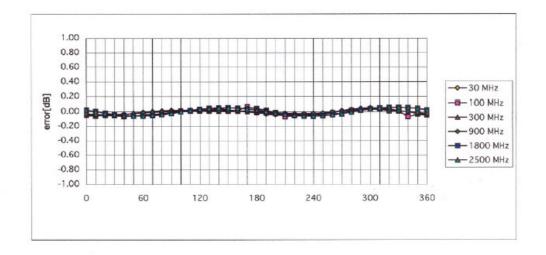

Page 4 of 10




ET3DV6 SN:1788

August 29, 2003

Frequency Response of E-Field

(TEM-Cell:ifi110, Waveguide R22)

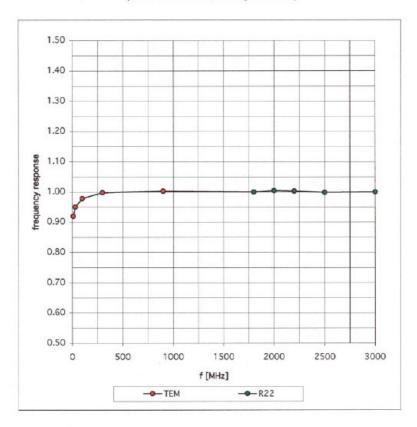



ET3DV6 SN:1788

August 29, 2003

Dynamic Range f(SAR_{brain})

(Waveguide R22)

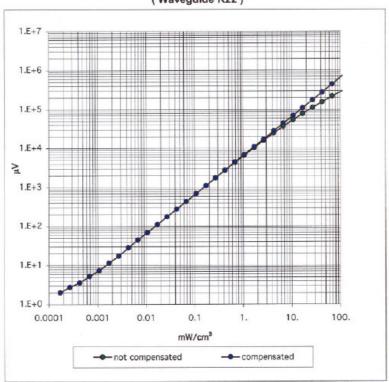

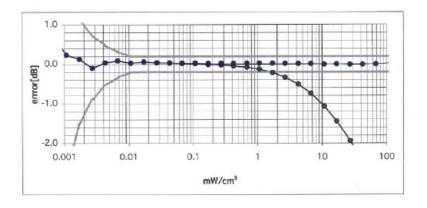



Page 6 of 10

ET3DV6 SN:1788

August 29, 2003

Conversion Factor Assessment

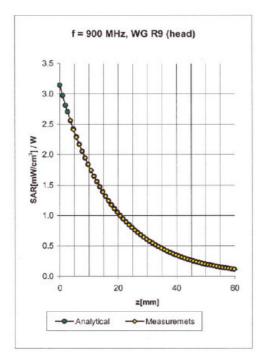

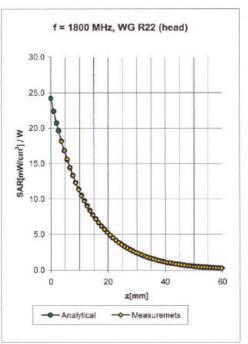


Head	900 MH	z	ε _τ = 41.5 ± 5%	σ = 0.97 ± 5% m	nho/m
Valid for f	=800-1000 MHz with H	ead Tissue Sir	nulating Liquid according to	EN 50361, P1528-200	X
	ConvF X	6.6 ±	9.5% (k=2)	Boundary effe	ct:
	ConvF Y	6.6 ±	9.5% (k=2)	Alpha	0.34
	ConvF Z	6.6 ±	9.5% (k=2)	Depth	2.48
Head	1800 MH	z	ϵ_r = 40.0 ± 5%	σ= 1.40 ± 5% n	nho/m
Valid for f	f=1710-1910 MHz with	Head Tissue S	imulating Liquid according	to EN 50361, P1528-20	OX
	ConvF X	5.3 ±9	9.5% (k=2)	Boundary effe	ct
	ConvF Y	5.3 ±	9.5% (k=2)	Alpha	0.43
	ConvF Z	5.3 ±9	9.5% (k=2)	Depth	2.80


Page 7 of 10

ET3DV6 SN:1788

August 29, 2003

Conversion Factor Assessment

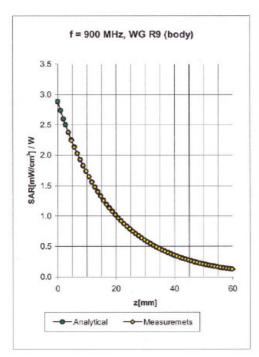

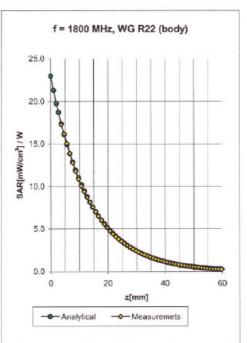


900 MHz		ε, = 55.0 ± 5%	σ=	1.05 ± 5% mho/r	n
0-1000 MHz with Body	Tissue	Simulating Liquid according to OE	T 65 5	Suppl. C	
ConvF X	6.5	± 9.5% (k=2)		Boundary effect:	
ConvF Y	6.5	± 9.5% (k=2)		Alpha	0.31
ConvF Z	6.5	± 9.5% (k=2)		Depth	2.92
1800 MHz		ϵ_r = 53.3 ± 5%	σ=	1.52 ± 5% mho/n	n
10-1910 MHz with Body	y Tiss	ue Simulating Liquid according to C	ET 65	Suppl. C	
ConvF X	5.0	± 9.5% (k=2)		Boundary effect:	
ConvF Y	5.0	± 9.5% (k=2)		Alpha	0.51
ConvF Z	5.0	± 9.5% (k=2)		Depth	2.78
	ConvF X ConvF Z 1800 MHz 10-1910 MHz with Bod ConvF X ConvF X	ConvF X 6.5 ConvF Z 6.5 ConvF Z 6.5 1800 MHz 10-1910 MHz with Body Tissu ConvF X 5.0 ConvF X 5.0	$\begin{array}{cccccccccccccccccccccccccccccccccccc$	$\begin{array}{cccccccccccccccccccccccccccccccccccc$	ConvF X 6.5 $\pm 9.5\%$ (k=2) Boundary effect: ConvF Z 6.5 $\pm 9.5\%$ (k=2) Depth 1800 MHz ϵ_r = 53.3 \pm 5% σ = 1.52 \pm 5% mho/m ConvF X 5.0 $\pm 9.5\%$ (k=2) Boundary effect: Alpha ConvF Z 6.5 $\pm 9.5\%$ (k=2) Depth


Page 8 of 10

ET3DV6 SN:1788

August 29, 2003

Conversion Factor Assessment

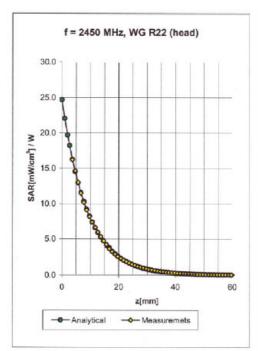

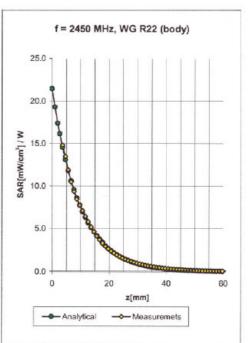

Head	2450 MHz		ϵ_r = 39.2 ± 5%	σ= 1.80	± 5% mho/m
Valid for f=2400	0-2500 MHz with He	ad Tiss	ue Simulating Liquid according t	o EN 50361, P1	1528-200X
С	onvF X	4.7	± 8.9% (k=2)	Boun	dary effect:
С	onvF Y	4.7	± 8.9% (k=2)	Alpha	0.99
С	onvF Z	4.7	± 8.9% (k=2)	Depth	1.81
Body	2450 MHz		ϵ_r = 52.7 ± 5%	σ= 1.95	± 5% mho/m
Valid for f=2400	0-2500 MHz with Bo	dy Tissi	ue Simulating Liquid according t	OET 65 Suppl	. c
С	onvF X	4.5	± 8.9% (k=2)	Boun	dary effect:
С	onvF Y	4.5	± 8.9% (k=2)	Alpha	1.01
С	onvF Z	4.5	± 8.9% (k=2)	Depth	1.74

Page 9 of 10



ET3DV6 SN:1788

August 29, 2003

Deviation from Isotropy in HSL

Error (θ,ϕ) , f = 900 MHz

