

Appendix A

Detailed System Check Results

1. System Performance Check
System Performance Check 750 MHz Head
System Performance Check 835 MHz Head
System Performance Check 1750 MHz Head
System Performance Check 1950 MHz Head
System Performance Check 2300 MHz Head
System Performance Check 2450 MHz Head
System Performance Check 2600 MHz Head
System Performance Check 3500 MHz Head
System Performance Check 3700 MHz Head
System Performance Check 3900 MHz Head
System Performance Check 5250 MHz Head
System Performance Check 5600 MHz Head
System Performance Check 5750 MHz Head
System Performance Check 6500 MHz Head

Measurement Report for Device, , , CW, Channel 0 (750.000 MHz)

Communication System: ; Frequency: 750.000

Medium: HSL. Medium parameters used: $f = 750.000$ MHz; $\sigma = 0.861$ S/m; $\epsilon_r = 42.7$

DASY8 Configuration:

- Probe: EX3DV4 - SN7735; ConvF(9.61, 9.61, 9.61); Calibrated: 2023-10-17
- Sensor-Surface: 1.4 mm
- Electronics: DAE4ip Sn1826; Calibrated: 2023-12-27
- Phantom: Twin-SAM V8.0 (30deg probe tilt); Serial: 2155
- Measurement Software: cDASY8 V16.2.0.1425


Area Scan (40.0 mm x 90.0 mm): Measurement Grid: 10.0 mm x 15.0 mm

SAR (1g) = 2.15 W/kg; SAR (10g) = 1.43 W/kg;

Zoom Scan (30.0 mm x 30.0 mm x 30.0 mm): Measurement Grid: 6.0 mm x 6.0 mm x 1.5 mm

Power Drift = 0.03 dB

SAR (1g) = 2.13 W/kg; SAR (10g) = 1.42 W/kg;

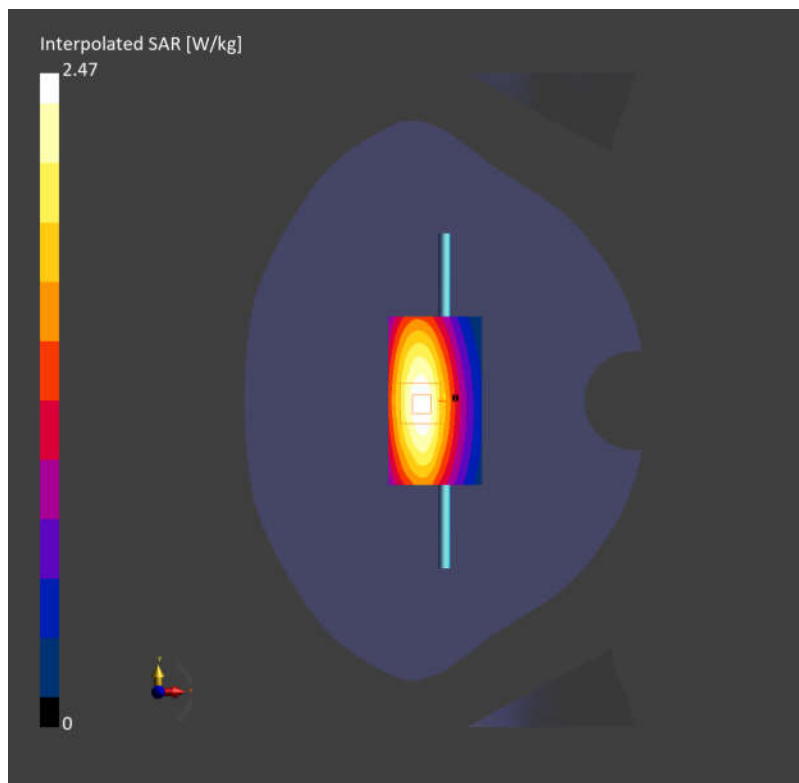

Test Laboratory: SGS-SAR Lab

System Performance Check 750 MHz Head

DUT: D750V3; Type: Dipole; Serial: 1214

Communication System: UID 0, CW (0); Frequency: 750 MHz; Duty Cycle: 1:1

Medium: HSL750; Medium parameters used: $f = 750 \text{ MHz}$; $\sigma = 0.888 \text{ S/m}$; $\epsilon_r = 42.094$; $\rho = 1000 \text{ kg/m}^3$

Phantom section: Flat Section

DASY 5 Configuration:

- Probe: EX3DV4 - SN7767; ConvF(10.54, 10.15, 10.87); Calibrated: 2023-10-26
- Sensor-Surface: 1.4mm (Mechanical Surface Detection)
- Electronics: DAE4 Sn1327; Calibrated: 2023-11-17
- Phantom: SAM 1; Type: QD000P40CD; Serial: TP:1769
- DASY52 52.10.4(1527); SEMCAD X 14.6.14(7483)

Body/d=15mm, Pin=250mW/Area Scan (7x13x1): Measurement grid: $dx=15\text{mm}$, $dy=15\text{mm}$
Maximum value of SAR (measured) = 2.66 W/kg


Body/d=15mm, Pin=250mW/Zoom Scan (5x5x7)/Cube 0: Measurement grid: $dx=8\text{mm}$, $dy=8\text{mm}$, $dz=5\text{mm}$

Reference Value = 44.73 V/m; Power Drift = 0.03 dB

Peak SAR (extrapolated) = 3.41 W/kg

SAR(1 g) = 2.14 W/kg; SAR(10 g) = 1.38 W/kg

Maximum value of SAR (measured) = 2.96 W/kg

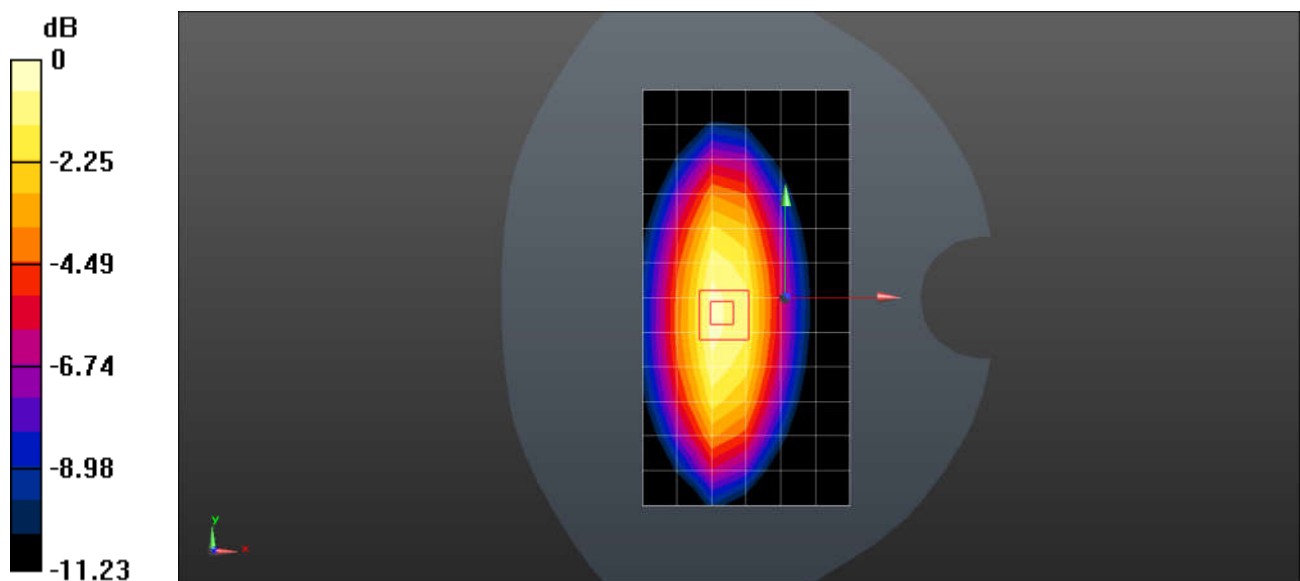

0 dB = 2.96 W/kg = 4.71 dBW/kg

Measurement Report for Device, , , CW, Channel 0 (835.000 MHz)

Communication System: ; Frequency: 835.000

Medium: HSL. Medium parameters used: $f = 835.000$ MHz; $\sigma = 0.908$ S/m; $\epsilon_r = 42.2$ **DASY8 Configuration:**

- Probe: EX3DV4 - SN7735; ConvF(9.2, 9.2, 9.2); Calibrated: 2023-10-17
- Sensor-Surface: 1.4 mm
- Electronics: DAE4ip Sn1826; Calibrated: 2023-12-27
- Phantom: Twin-SAM V8.0 (30deg probe tilt); Serial: 2155
- Measurement Software: cDASY8 V16.2.0.1425


Area Scan (40.0 mm x 90.0 mm): Measurement Grid: 10.0 mm x 15.0 mm

SAR (1g) = 2.39 W/kg; SAR (10g) = 1.59 W/kg;

Zoom Scan (30.0 mm x 30.0 mm x 30.0 mm): Measurement Grid: 6.0 mm x 6.0 mm x 1.5 mm

Power Drift = 0.01 dB

SAR (1g) = 2.38 W/kg; SAR (10g) = 1.58 W/kg;

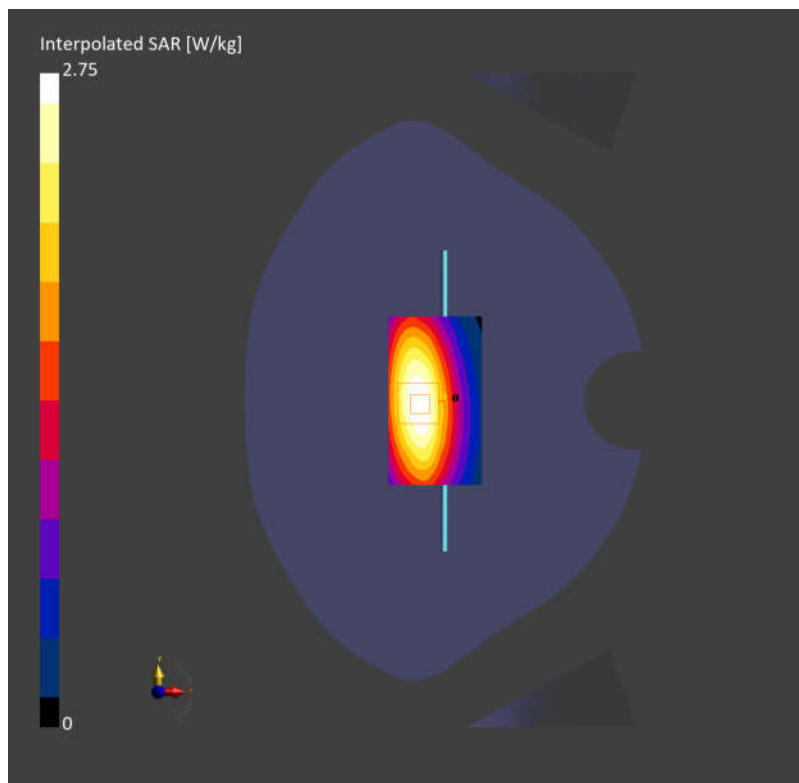

Test Laboratory: SGS-SAR Lab

System Performance Check 835 MHz Head

DUT: D835V2; Type: Dipole; Serial: 4d161

Communication System: UID 0, CW (0); Frequency: 835 MHz; Duty Cycle: 1:1

Medium: HSL835; Medium parameters used: $f = 835 \text{ MHz}$; $\sigma = 0.91 \text{ S/m}$; $\epsilon_r = 41.923$; $\rho = 1000 \text{ kg/m}^3$

Phantom section: Flat Section

DASY 5 Configuration:

- Probe: EX3DV4 - SN7767; ConvF(10.39, 9.86, 10); Calibrated: 2023-10-26
- Sensor-Surface: 1.4mm (Mechanical Surface Detection)
- Electronics: DAE4 Sn1327; Calibrated: 2023-11-17
- Phantom: SAM 1; Type: QD000P40CD; Serial: TP:1769
- DASY52 52.10.4(1527); SEMCAD X 14.6.14(7483)

Body/d=15mm, Pin=250mW/Area Scan (7x13x1): Measurement grid: $dx=15\text{mm}$, $dy=15\text{mm}$
Maximum value of SAR (measured) = 2.88 W/kg


Body/d=15mm, Pin=250mW/Zoom Scan (5x5x7)/Cube 0: Measurement grid: $dx=8\text{mm}$, $dy=8\text{mm}$, $dz=5\text{mm}$

Reference Value = 55.47 V/m ; Power Drift = -0.02 dB

Peak SAR (extrapolated) = 3.66 W/kg

SAR(1 g) = 2.43 W/kg ; SAR(10 g) = 1.59 W/kg

Maximum value of SAR (measured) = 3.10 W/kg

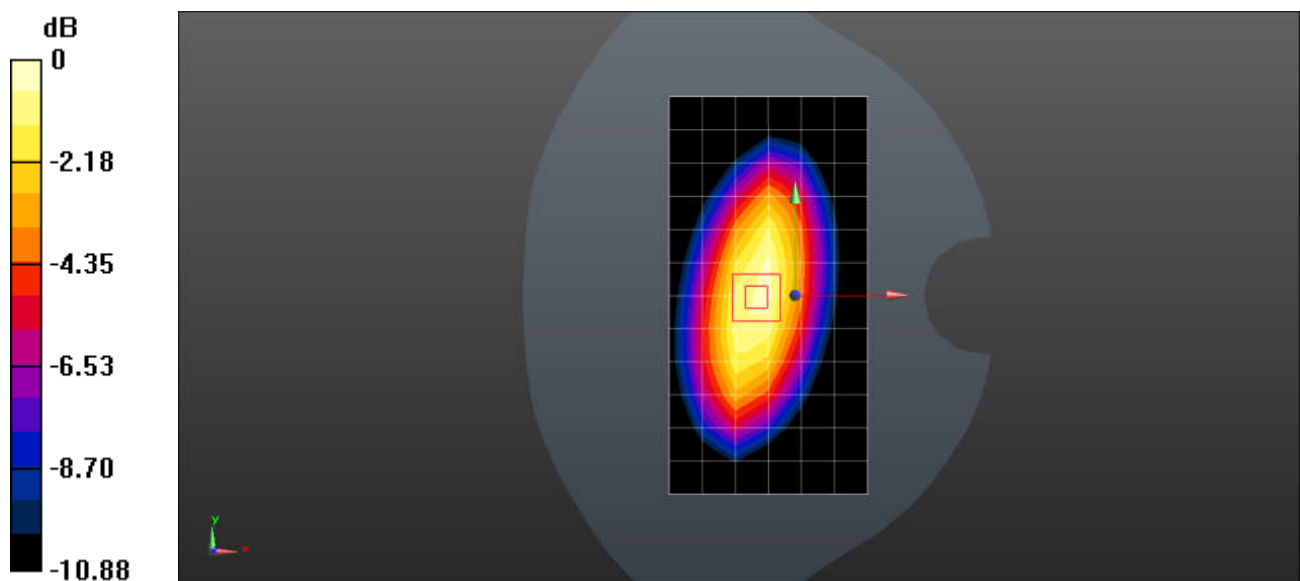

0 dB = 3.10 W/kg = 4.91 dBW/kg

Measurement Report for Device, , , CW, Channel 0 (1750.000 MHz)

Communication System: ; Frequency: 1750.000

Medium: HSL. Medium parameters used: $f = 1750.000$ MHz; $\sigma = 1.35$ S/m; $\epsilon_r = 41.0$ **DASY8 Configuration:**

- Probe: EX3DV4 - SN7735; ConvF(8.12, 8.12, 8.12); Calibrated: 2023-10-17
- Sensor-Surface: 1.4 mm
- Electronics: DAE4ip Sn1826; Calibrated: 2023-12-27
- Phantom: Twin-SAM V8.0 (30deg probe tilt); Serial: 2155
- Measurement Software: cDASY8 V16.2.0.1425


Area Scan (40.0 mm x 90.0 mm): Measurement Grid: 10.0 mm x 15.0 mm

SAR (1g) = 8.87 W/kg; SAR (10g) = 4.88 W/kg;

Zoom Scan (30.0 mm x 30.0 mm x 30.0 mm): Measurement Grid: 6.0 mm x 6.0 mm x 1.5 mm

Power Drift = -0.02 dB

SAR (1g) = 9.16 W/kg; SAR (10g) = 5.00 W/kg;

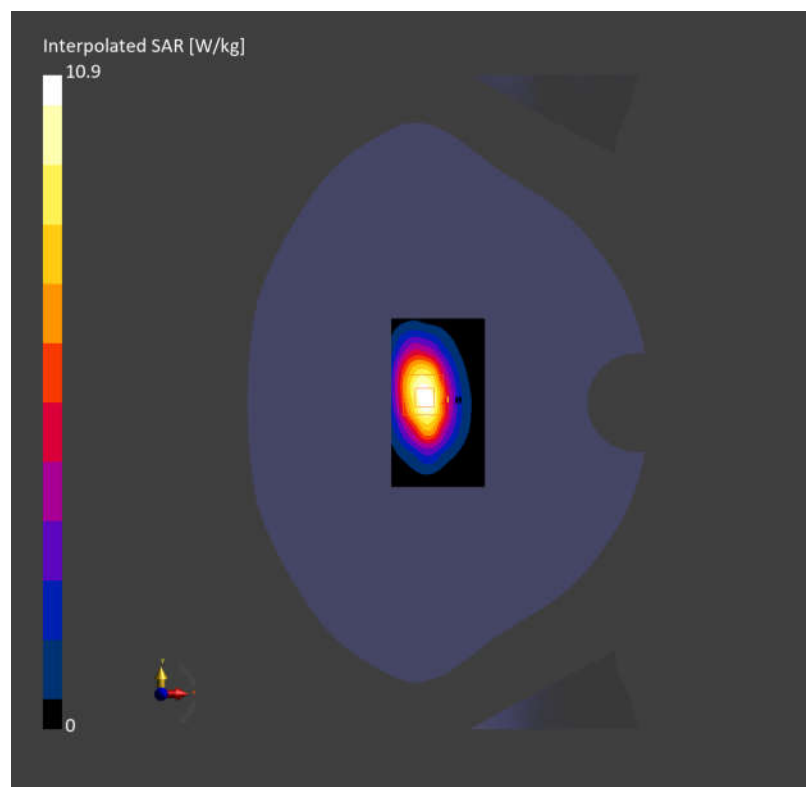

Test Laboratory: SGS-SAR Lab

System Performance Check 1750 MHz Head

DUT: D1750V2; Type: Dipole; Serial: 1038

Communication System: UID 0, CW (0); Frequency: 1750 MHz; Duty Cycle: 1:1

Medium: HSL1750; Medium parameters used: $f = 1750$ MHz; $\sigma = 1.369$ S/m; $\epsilon_r = 39.37$; $\rho = 1000$ kg/m³

Phantom section: Flat Section

DASY 5 Configuration:

- Probe: EX3DV4 - SN7767; ConvF(9.45, 8.73, 9.34); Calibrated: 2023-10-26
- Sensor-Surface: 1.4mm (Mechanical Surface Detection)
- Electronics: DAE4 Sn1327; Calibrated: 2023-11-17
- Phantom: SAM 1; Type: QD000P40CD; Serial: TP:1769
- DASY52 52.10.4(1527); SEMCAD X 14.6.14(7483)

Body/d=10mm, Pin=250mW/Area Scan (5x7x1): Measurement grid: dx=15mm, dy=15mm
Maximum value of SAR (measured) = 10.2 W/kg


Body/d=10mm, Pin=250mW/Zoom Scan (5x5x7)/Cube 0: Measurement grid: dx=8mm, dy=8mm, dz=5mm

Reference Value = 78.74 V/m; Power Drift = 0.03 dB

Peak SAR (extrapolated) = 16.0 W/kg

SAR(1 g) = 9.03 W/kg; SAR(10 g) = 4.84 W/kg

Maximum value of SAR (measured) = 12.9 W/kg

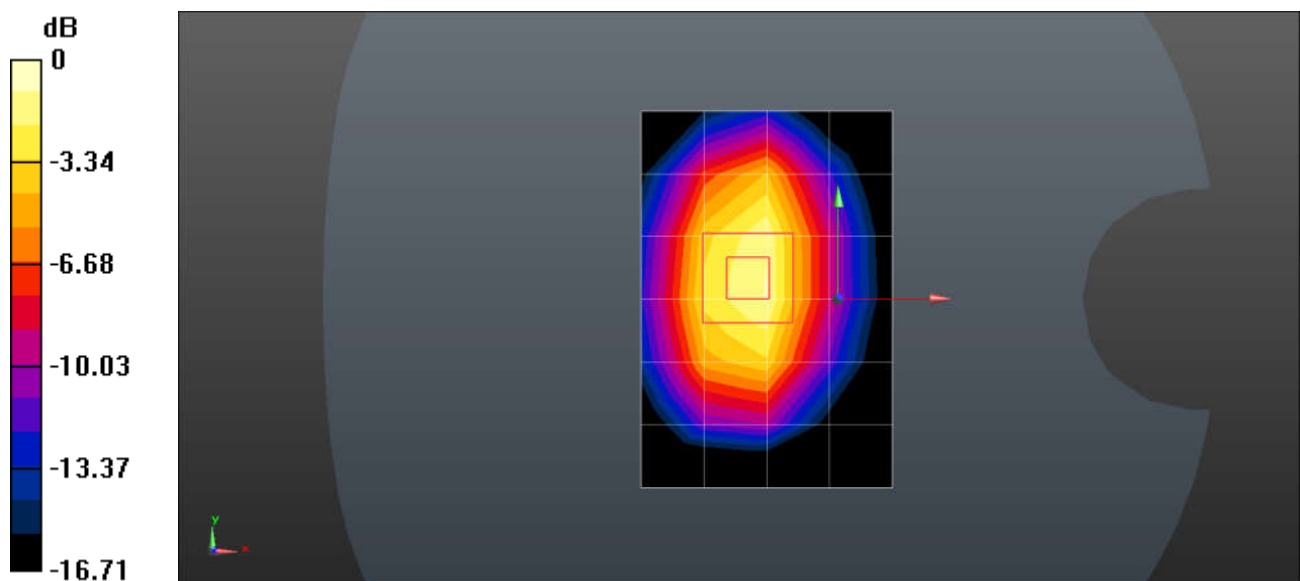

0 dB = 12.9 W/kg = 11.11 dBW/kg

Measurement Report for Device, , , CW, Channel 0 (1950.000 MHz)

Communication System: ; Frequency: 1950.000

Medium: HSL. Medium parameters used: $f = 1950.000$ MHz; $\sigma = 1.43$ S/m; $\epsilon_r = 40.4$ **DASY8 Configuration:**

- Probe: EX3DV4 - SN7735; ConvF(7.81, 7.81, 7.81); Calibrated: 2023-10-17
- Sensor-Surface: 1.4 mm
- Electronics: DAE4ip Sn1826; Calibrated: 2023-12-27
- Phantom: Twin-SAM V8.0 (30deg probe tilt); Serial: 2155
- Measurement Software: cDASY8 V16.2.0.1425


Area Scan (40.0 mm x 90.0 mm): Measurement Grid: 10.0 mm x 15.0 mm

SAR (1g) = 9.67 W/kg; SAR (10g) = 5.05 W/kg;

Zoom Scan (30.0 mm x 30.0 mm x 30.0 mm): Measurement Grid: 6.0 mm x 6.0 mm x 1.5 mm

Power Drift = -0.05 dB

SAR (1g) = 9.75 W/kg; SAR (10g) = 5.17 W/kg;

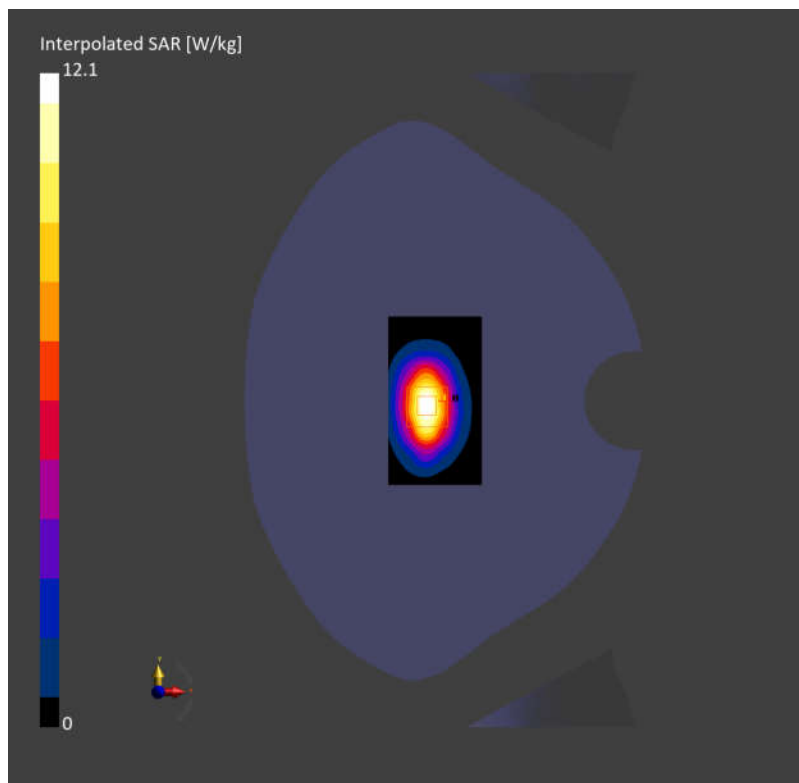

Test Laboratory: SGS-SAR Lab

System Performance Check 1950 MHz Head

DUT: D1950V3; Type: Dipole; Serial: 1218

Communication System: UID 0, CW (0); Frequency: 1950 MHz; Duty Cycle: 1:1

Medium: HSL1950; Medium parameters used: $f = 1950$ MHz; $\sigma = 1.419$ S/m; $\epsilon_r = 39.5$; $\rho = 1000$ kg/m³

Phantom section: Flat Section

DASY 5 Configuration:

- Probe: EX3DV4 - SN7767; ConvF(8.54, 7.96, 8.42); Calibrated: 2023-10-26
- Sensor-Surface: 1.4mm (Mechanical Surface Detection)
- Electronics: DAE4 Sn1327; Calibrated: 2023-11-17
- Phantom: SAM 1; Type: QD000P40CD; Serial: TP:1769
- DASY52 52.10.4(1527); SEMCAD X 14.6.14(7483)

Body/d=10mm, Pin=250mW/Area Scan (5x7x1): Measurement grid: dx=15mm, dy=15mm
Maximum value of SAR (measured) = 13.7 W/kg


Body/d=10mm, Pin=250mW/Zoom Scan (5x5x7)/Cube 0: Measurement grid: dx=8mm, dy=8mm, dz=5mm

Reference Value = 88.13 V/m; Power Drift = 0.12 dB

Peak SAR (extrapolated) = 18.3 W/kg

SAR(1 g) = 10.3 W/kg; SAR(10 g) = 5.41 W/kg

Maximum value of SAR (measured) = 14.5 W/kg

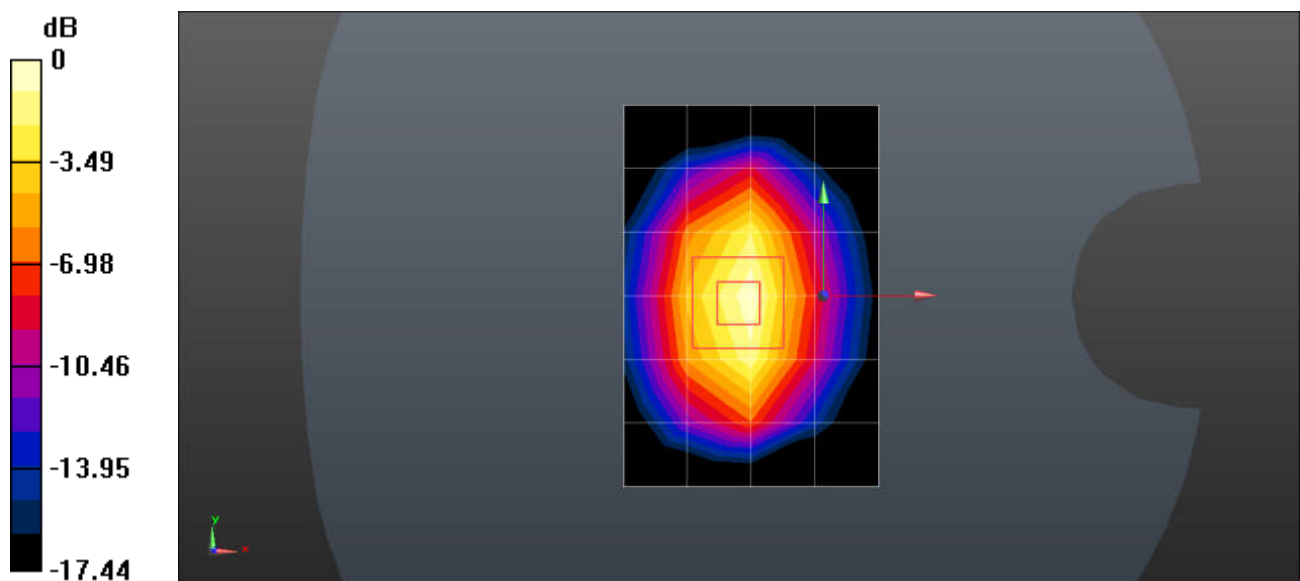

0 dB = 14.5 W/kg = 11.61 dBW/kg

Measurement Report for Device, , , CW, Channel 0 (2450.000 MHz)

Communication System: ; Frequency: 2450.000

Medium: HSL. Medium parameters used: $f = 2450.000$ MHz; $\sigma = 1.83$ S/m; $\epsilon_r = 39.3$ **DASY8 Configuration:**

- Probe: EX3DV4 - SN7735; ConvF(7.41, 7.41, 7.41); Calibrated: 2023-10-17
- Sensor-Surface: 1.4 mm
- Electronics: DAE4ip Sn1826; Calibrated: 2023-12-27
- Phantom: Twin-SAM V8.0 (30deg probe tilt); Serial: 2155
- Measurement Software: cDASY8 V16.2.0.1425


Area Scan (40.0 mm x 80.0 mm): Measurement Grid: 10.0 mm x 10.0 mm

SAR (1g) = 12.2 W/kg; SAR (10g) = 5.80 W/kg;

Zoom Scan (30.0 mm x 30.0 mm x 30.0 mm): Measurement Grid: 5.0 mm x 5.0 mm x 1.5 mm

Power Drift = -0.03 dB

SAR (1g) = 12.4 W/kg; SAR (10g) = 5.97 W/kg;

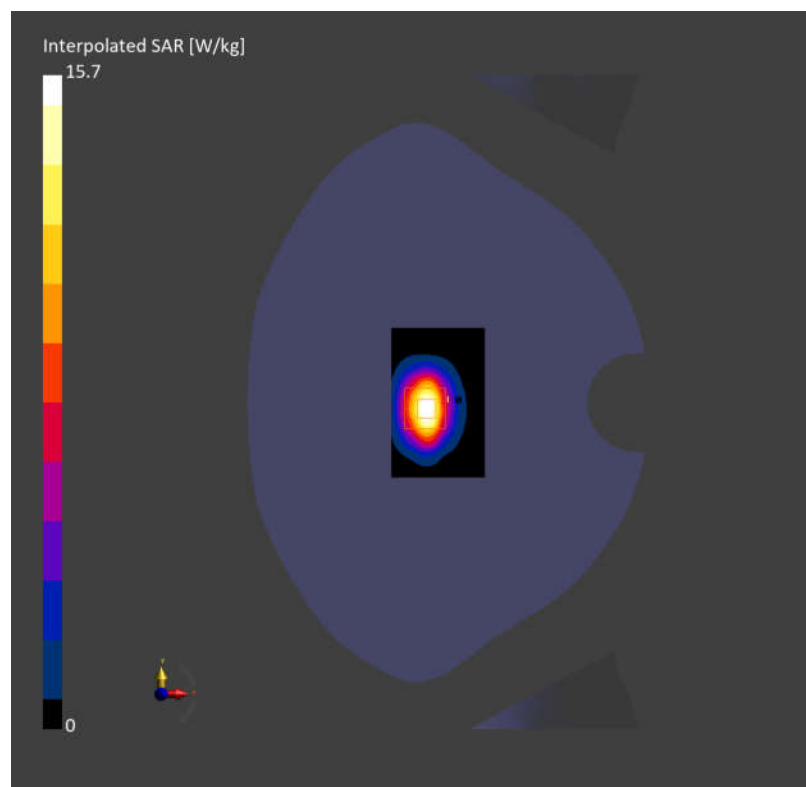

Measurement Report for Device, , , CW, Channel 0 (2600.000 MHz)

Communication System: ; Frequency: 2600.000

Medium: HSL. Medium parameters used: $f = 2600.000$ MHz; $\sigma = 1.98$ S/m; $\epsilon_r = 38.7$

DASY8 Configuration:

- Probe: EX3DV4 - SN7735; ConvF(7.16, 7.16, 7.16); Calibrated: 2023-10-17
- Sensor-Surface: 1.4 mm
- Electronics: DAE4ip Sn1826; Calibrated: 2023-12-27
- Phantom: Twin-SAM V8.0 (30deg probe tilt); Serial: 2155
- Measurement Software: cDASY8 V16.2.0.1425


Area Scan (40.0 mm x 80.0 mm): Measurement Grid: 10.0 mm x 10.0 mm

SAR (1g) = 13.6 W/kg; SAR (10g) = 6.34 W/kg;

Zoom Scan (30.0 mm x 30.0 mm x 30.0 mm): Measurement Grid: 5.0 mm x 5.0 mm x 1.5 mm

Power Drift = -0.01 dB

SAR (1g) = 14.2 W/kg; SAR (10g) = 6.51 W/kg;

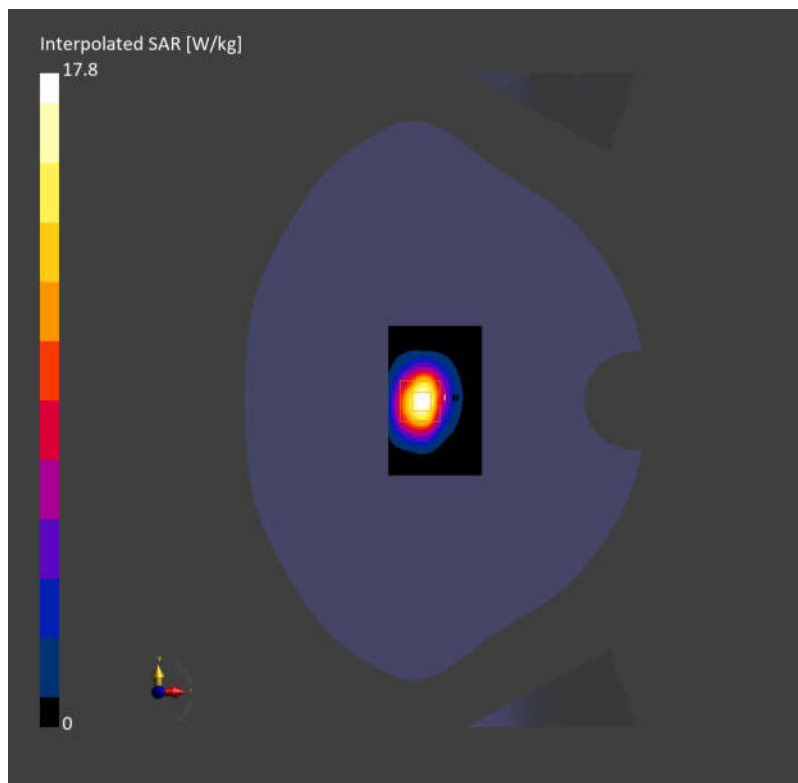

Test Laboratory: SGS-SAR Lab

System Performance Check 2600MHz Head

DUT: D2600V2; Type: Dipole; Serial: 1187

Communication System: UID 0, CW (0); Frequency: 2600 MHz; Duty Cycle: 1:1

Medium: HSL2600; Medium parameters used: $f = 2600$ MHz; $\sigma = 1.984$ S/m; $\epsilon_r = 37.972$; $\rho = 1000$ kg/m³

Phantom section: Flat Section

DASY 5 Configuration:

- Probe: EX3DV4 - SN7767; ConvF(8.01, 7.49, 7.95); Calibrated: 2023-10-26
- Sensor-Surface: 1.4mm (Mechanical Surface Detection)
- Electronics: DAE4 Sn1327; Calibrated: 2023-11-17
- Phantom: SAM 1; Type: QD000P40CD; Serial: TP:1769
- DASY52 52.10.4(1527); SEMCAD X 14.6.14(7483)

Body/d=10mm, Pin=250mW/Area Scan (6x9x1): Measurement grid: dx=12mm, dy=12mm
Maximum value of SAR (measured) = 22.1 W/kg


Body/d=10mm, Pin=250mW/Zoom Scan (7x7x7)/Cube 0: Measurement grid: dx=5mm, dy=5mm, dz=5mm

Reference Value = 87.42 V/m; Power Drift = 0.03 dB

Peak SAR (extrapolated) = 31.7 W/kg

SAR(1 g) = 14.7 W/kg; SAR(10 g) = 6.58 W/kg

Maximum value of SAR (measured) = 22.8 W/kg

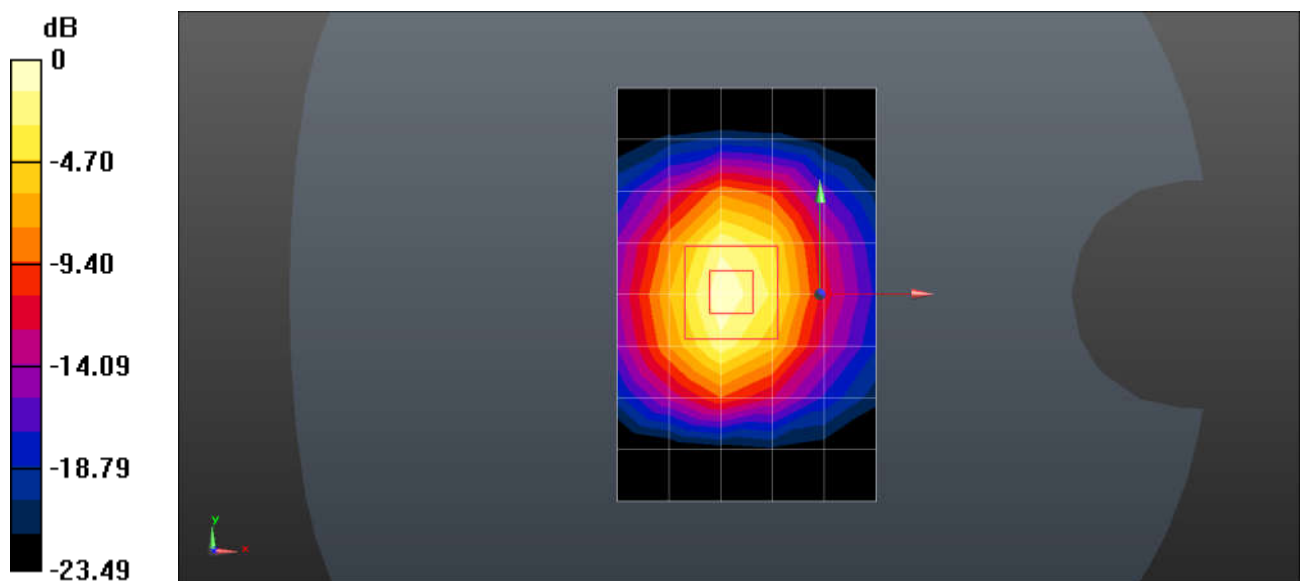

0 dB = 22.8 W/kg = 13.58 dBW/kg

Test Laboratory: SGS-SAR Lab

System Performance Check 3500MHz Head

DUT: D3500V2; Type: Dipole; Serial: 1133

Communication System: UID 0, CW (0); Frequency: 3500 MHz; Duty Cycle: 1:1

Medium: HSL3500; Medium parameters used: $f = 3500$ MHz; $\sigma = 3.001$ S/m; $\epsilon_r = 38.773$; $\rho = 1000$ kg/m³

Phantom section: Flat Section

DASY 5 Configuration:

- Probe: EX3DV4 - SN7767; ConvF(7.64, 7.02, 7.52); Calibrated: 2023-10-26
- Sensor-Surface: 1.4mm (Mechanical Surface Detection)
- Electronics: DAE4 Sn1327; Calibrated: 2023-11-17
- Phantom: SAM 1; Type: QD000P40CD; Serial: TP:1769
- DASY52 52.10.4(1527); SEMCAD X 14.6.14(7483)

Body/d=10mm, Pin=100mW/Area Scan (6x9x1): Measurement grid: dx=12mm, dy=12mm
Maximum value of SAR (measured) = 9.63 W/kg


Body/d=10mm, Pin=100mW/Zoom Scan (7x7x8)/Cube 0: Measurement grid: dx=5mm, dy=5mm, dz=5mm

Reference Value = 51.06 V/m; Power Drift = -0.03 dB

Peak SAR (extrapolated) = 16.7 W/kg

SAR(1 g) = 6.6 W/kg; SAR(10 g) = 2.49 W/kg

Maximum value of SAR (measured) = 12.7 W/kg

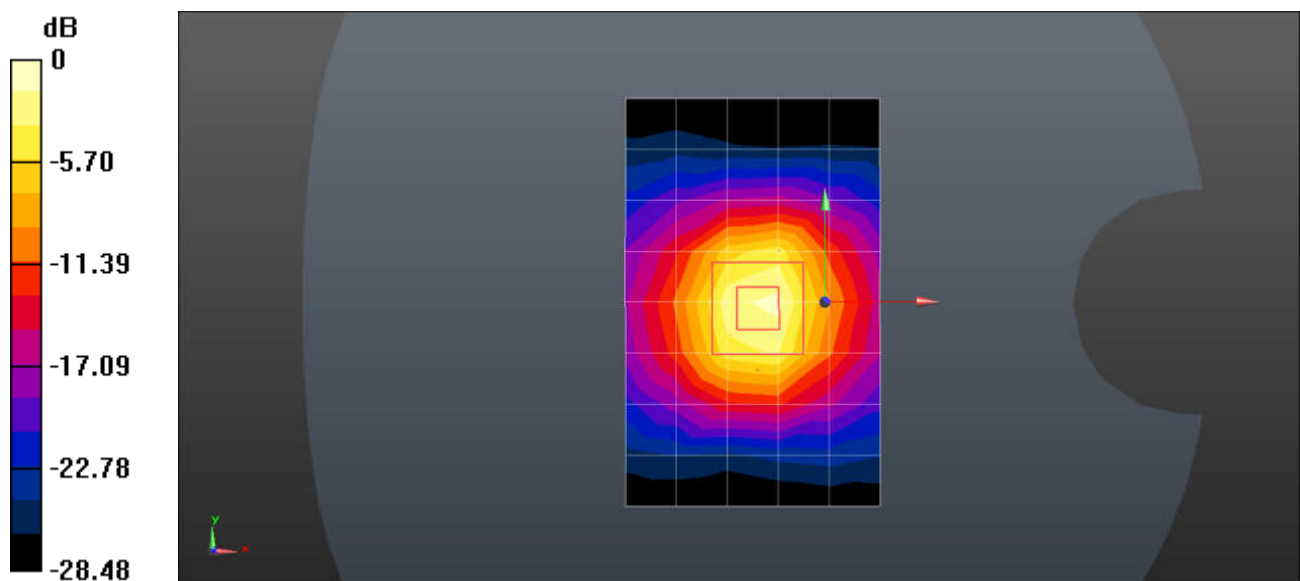

0 dB = 12.7 W/kg = 11.04 dBW/kg

Test Laboratory: SGS-SAR Lab

System Performance Check 3700MHz Head

DUT: D3700V2; Type: Dipole; Serial: 1108

Communication System: UID 0, CW (0); Frequency: 3700 MHz; Duty Cycle: 1:1

Medium: HSL3700; Medium parameters used: $f = 3700$ MHz; $\sigma = 3.115$ S/m; $\epsilon_r = 37.729$; $\rho = 1000$ kg/m³

Phantom section: Flat Section

DASY 5 Configuration:

- Probe: EX3DV4 - SN7767; ConvF(7.21, 6.62, 7.1); Calibrated: 2023-10-26
- Sensor-Surface: 1.4mm (Mechanical Surface Detection)
- Electronics: DAE4 Sn1327; Calibrated: 2023-11-17
- Phantom: SAM 1; Type: QD000P40CD; Serial: TP:1769
- DASY52 52.10.4(1527); SEMCAD X 14.6.14(7483)

Body/d=10mm, Pin=100mW/Area Scan (6x9x1): Measurement grid: dx=12mm, dy=12mm
Maximum value of SAR (measured) = 8.55 W/kg


Body/d=10mm, Pin=100mW/Zoom Scan (7x7x7)/Cube 0: Measurement grid: dx=5mm, dy=5mm, dz=5mm

Reference Value = 48.43 V/m; Power Drift = -0.11 dB

Peak SAR (extrapolated) = 16.8 W/kg

SAR(1 g) = 6.44 W/kg; SAR(10 g) = 2.34 W/kg

Maximum value of SAR (measured) = 12.4 W/kg

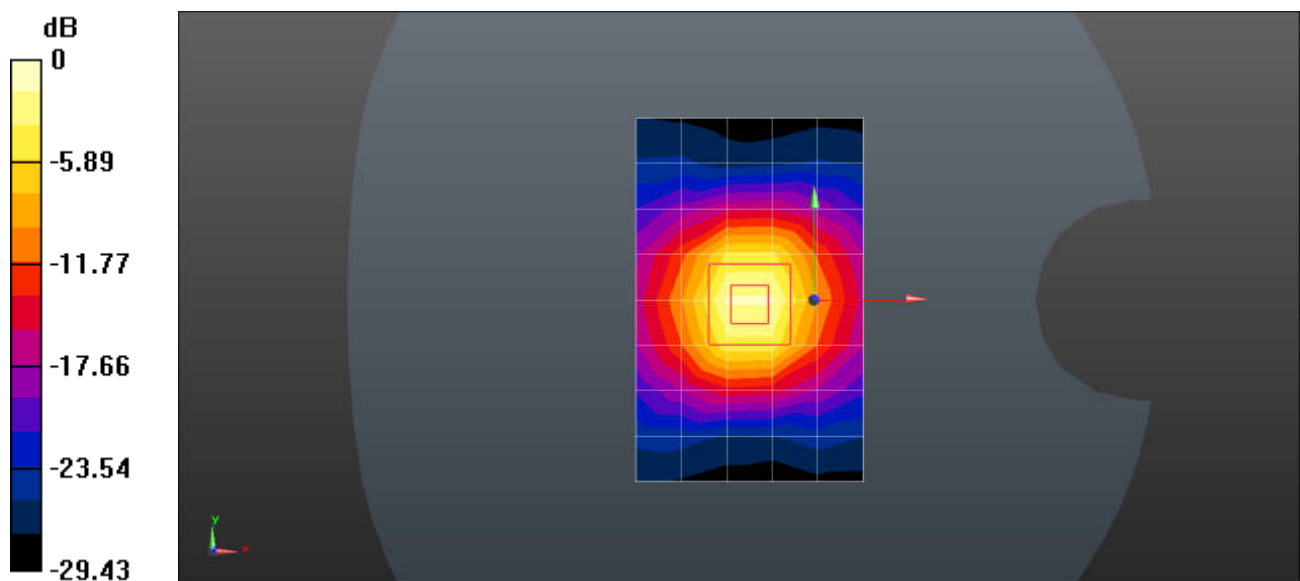

0 dB = 12.4 W/kg = 10.93 dBW/kg

Test Laboratory: SGS-SAR Lab

System Performance Check 3900MHz Head

DUT: D3900V2; Type: Dipole; Serial: 1174

Communication System: UID 0, CW (0); Frequency: 3900 MHz; Duty Cycle: 1:1

Medium: HSL3900; Medium parameters used: $f = 3900$ MHz; $\sigma = 3.473$ S/m; $\epsilon_r = 37.101$; $\rho = 1000$ kg/m³

Phantom section: Flat Section

DASY 5 Configuration:

- Probe: EX3DV4 - SN7767; ConvF(7.17, 6.59, 7.08); Calibrated: 2023-10-26
- Sensor-Surface: 1.4mm (Mechanical Surface Detection)
- Electronics: DAE4 Sn1327; Calibrated: 2023-11-17
- Phantom: SAM 1; Type: QD000P40CD; Serial: TP:1769
- DASY52 52.10.4(1527); SEMCAD X 14.6.14(7483)

Body/d=10mm, Pin=100mW/Area Scan (6x9x1): Measurement grid: dx=12mm, dy=12mm
Maximum value of SAR (measured) = 13.3 W/kg


Body/d=10mm, Pin=100mW/Zoom Scan (7x7x7)/Cube 0: Measurement grid: dx=5mm, dy=5mm, dz=5mm

Reference Value = 48.64 V/m; Power Drift = 0.08 dB

Peak SAR (extrapolated) = 19.2 W/kg

SAR(1 g) = 6.84 W/kg; SAR(10 g) = 2.37 W/kg

Maximum value of SAR (measured) = 14.6 W/kg

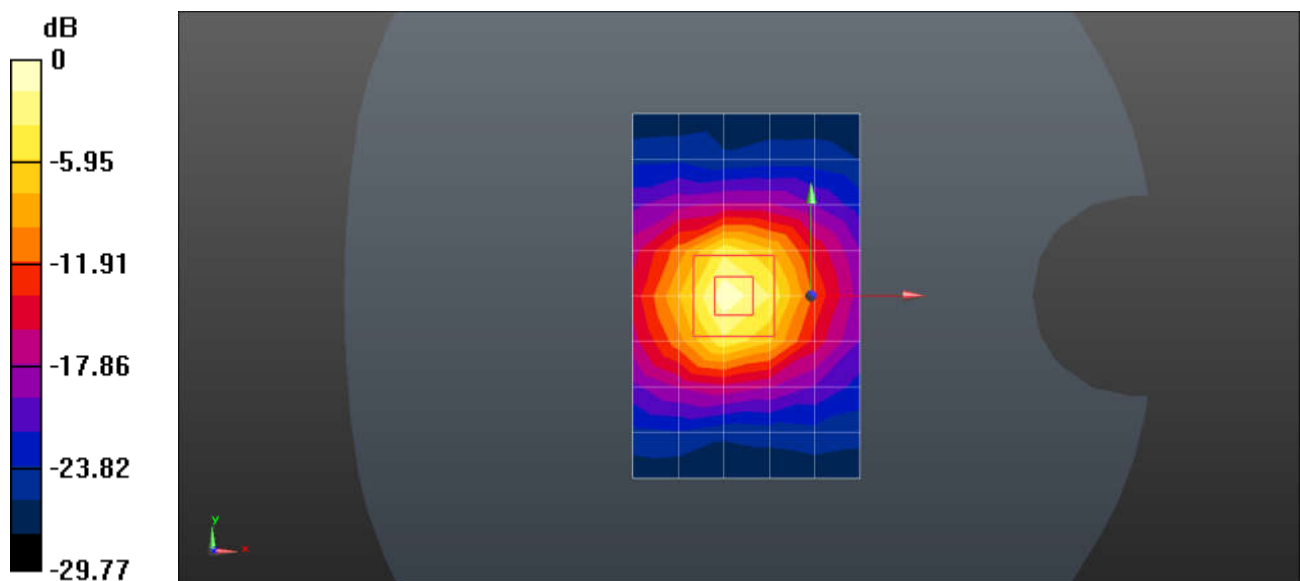

0 dB = 14.6 W/kg = 11.64 dBW/kg

Measurement Report for Device, , , CW, Channel 0 (5250.000 MHz)

Communication System: ; Frequency: 5250.000

Medium: HSL. Medium parameters used: $f = 5250.000$ MHz; $\sigma = 4.73$ S/m; $\epsilon_r = 36.1$ **DASY8 Configuration:**

- Probe: EX3DV4 - SN7735; ConvF(5.3, 5.3, 5.3); Calibrated: 2023-10-17
- Sensor-Surface: 1.4 mm
- Electronics: DAE4ip Sn1826; Calibrated: 2023-12-27
- Phantom: Twin-SAM V8.0 (30deg probe tilt); Serial: 2155
- Measurement Software: cDASY8 V16.2.0.1425


Area Scan (40.0 mm x 80.0 mm): Measurement Grid: 10.0 mm x 10.0 mm

SAR (1g) = 7.84 W/kg; SAR (10g) = 2.16 W/kg;

Zoom Scan (22.0 mm x 22.0 mm x 22.0 mm): Measurement Grid: 4.0 mm x 4.0 mm x 1.4 mm

Power Drift = 0.03 dB

SAR (1g) = 8.21 W/kg; SAR (10g) = 2.36 W/kg;

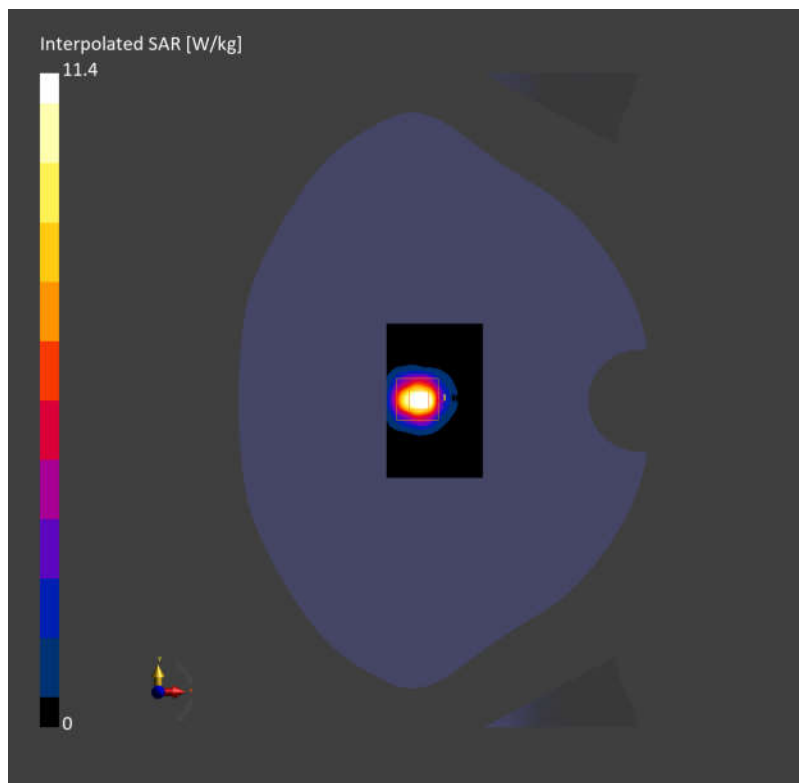

Measurement Report for Device, , , CW, Channel 0 (5600.000 MHz)

Communication System: ; Frequency: 5600.000

Medium: HSL. Medium parameters used: $f = 5600.000$ MHz; $\sigma = 5.12$ S/m; $\epsilon_r = 35.2$ **DASY8 Configuration:**

- Probe: EX3DV4 - SN7735; ConvF(4.71, 4.71, 4.71); Calibrated: 2023-10-17
- Sensor-Surface: 1.4 mm
- Electronics: DAE4ip Sn1826; Calibrated: 2023-12-27
- Phantom: Twin-SAM V8.0 (30deg probe tilt); Serial: 2155
- Measurement Software: cDASY8 V16.2.0.1425


Area Scan (40.0 mm x 80.0 mm): Measurement Grid: 10.0 mm x 10.0 mm

SAR (1g) = 7.86 W/kg; SAR (10g) = 2.12 W/kg;

Zoom Scan (22.0 mm x 22.0 mm x 22.0 mm): Measurement Grid: 4.0 mm x 4.0 mm x 1.4 mm

Power Drift = 0.04 dB

SAR (1g) = 8.33 W/kg; SAR (10g) = 2.39 W/kg;

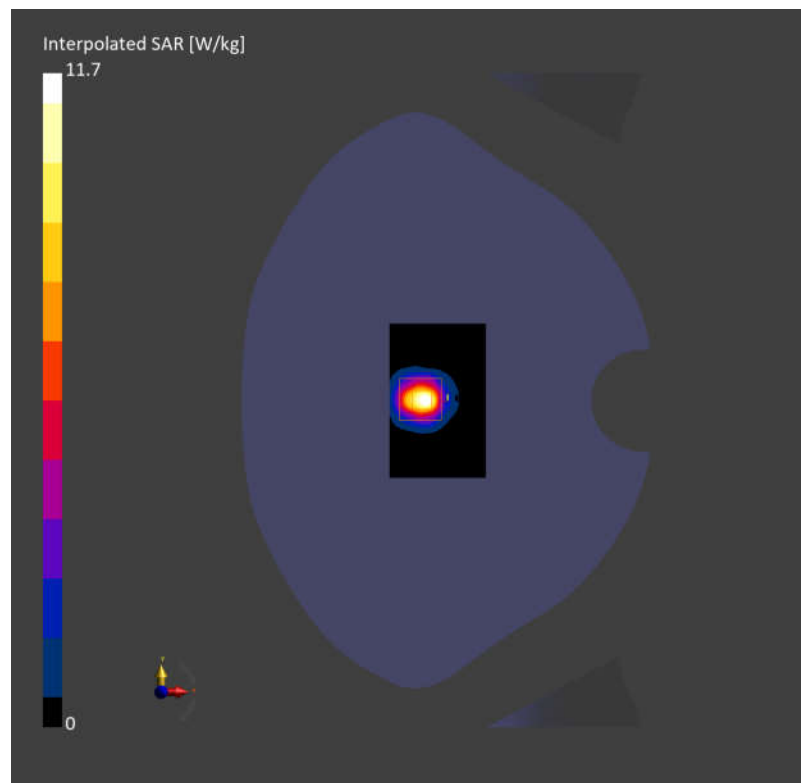

Measurement Report for Device, , , CW, Channel 0 (5750.000 MHz)

Communication System: ; Frequency: 5750.000

Medium: HSL. Medium parameters used: $f = 5750.000$ MHz; $\sigma = 5.29$ S/m; $\epsilon_r = 34.8$ **DASY8 Configuration:**

- Probe: EX3DV4 - SN7735; ConvF(4.79, 4.79, 4.79); Calibrated: 2023-10-17
- Sensor-Surface: 1.4 mm
- Electronics: DAE4ip Sn1826; Calibrated: 2023-12-27
- Phantom: Twin-SAM V8.0 (30deg probe tilt); Serial: 2155
- Measurement Software: cDASY8 V16.2.0.1425


Area Scan (40.0 mm x 80.0 mm): Measurement Grid: 10.0 mm x 10.0 mm

SAR (1g) = 7.04 W/kg; SAR (10g) = 2.07 W/kg;

Zoom Scan (22.0 mm x 22.0 mm x 22.0 mm): Measurement Grid: 4.0 mm x 4.0 mm x 1.4 mm

Power Drift = 0.04 dB

SAR (1g) = 7.59 W/kg; SAR (10g) = 2.19 W/kg;

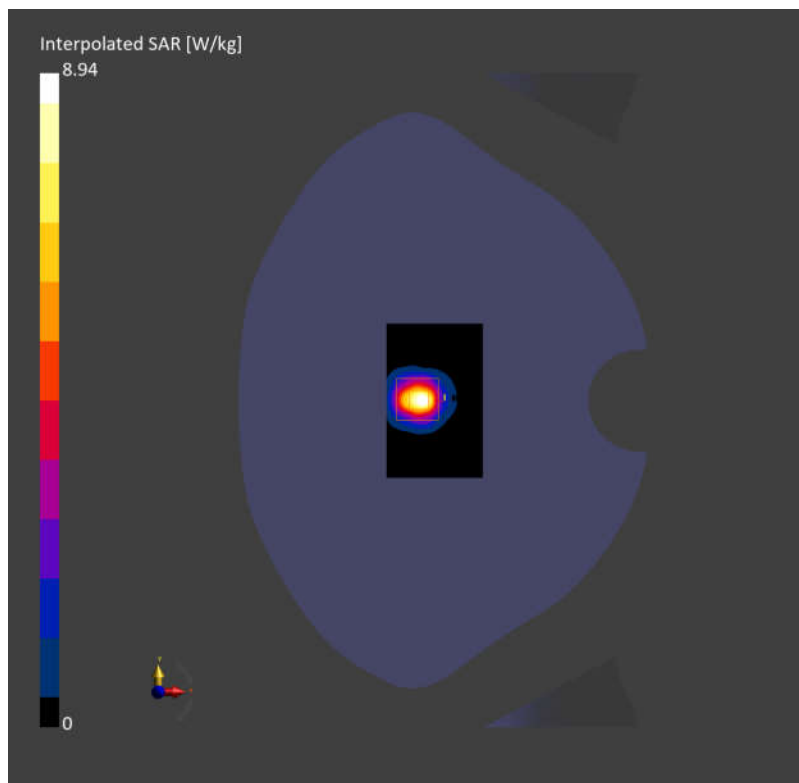

Measurement Report for Device, , , CW, Channel 0 (6500.000 MHz)

Communication System: ; Frequency: 6500.000

Medium: HSL. Medium parameters used: $f = 6500.000$ MHz; $\sigma = 6.18$ S/m; $\epsilon_r = 33.7$

DASY8 Configuration:

- Probe: EX3DV4 - SN7735; ConvF(5.11, 5.28, 5.08); Calibrated: 2023-12-19
- Sensor-Surface: 1.4 mm
- Electronics: DAE4ip Sn1826; Calibrated: 2023-12-27
- Phantom: Twin-SAM V8.0 (30deg probe tilt); Serial: 2155
- Measurement Software: cDASY8 V16.2.0.1425

Area Scan (51.0 mm x 51.0 mm): Measurement Grid: 8.5 mm x 8.5 mm

SAR (1g) = 26.4 W/kg; SAR (10g) = 5.13 W/kg;

Zoom Scan (22.0 mm x 22.0 mm x 22.0 mm): Measurement Grid: 3.4 mm x 3.4 mm x 1.4 mm

Power Drift = -0.06 dB

SAR (1g) = 31.0 W/kg; SAR (10g) = 5.65 W/kg;

