

## **Contents**

10. Photographs of Test Setup .....	54
11. Photographs of the EUT .....	56

## 10. Photographs of Test Setup

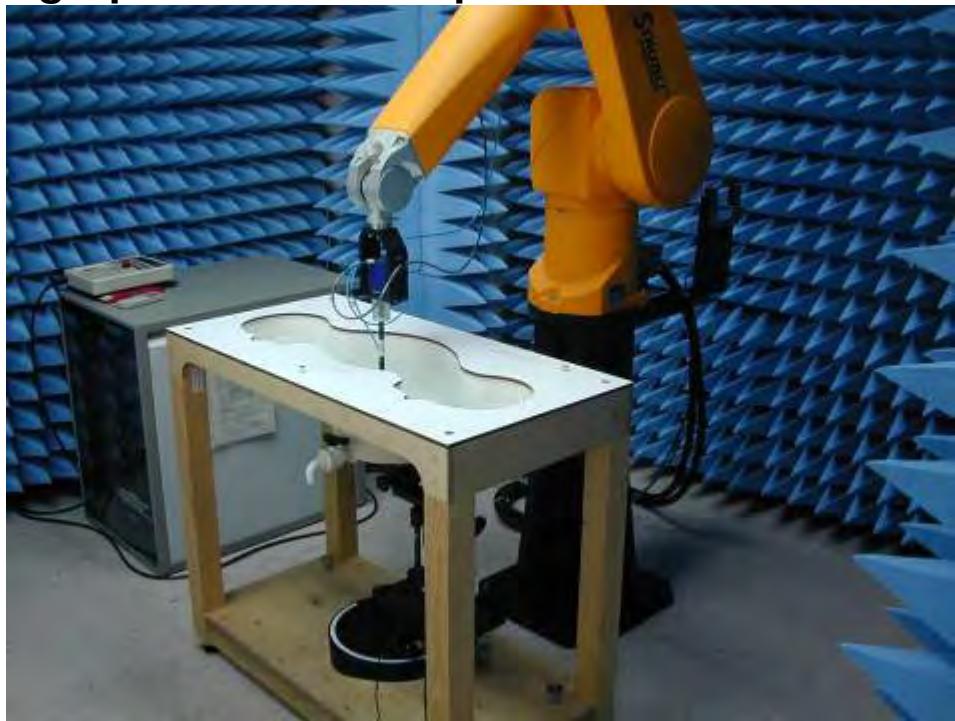


Fig.1 Photograph of the SAR measurement System

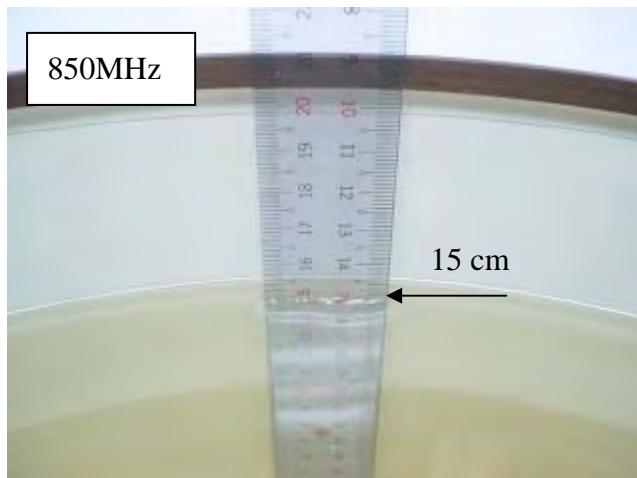


Fig.2.1 Photograph of the Tissue Simulant Fluid liquid depth 15cm for Flat (Body)

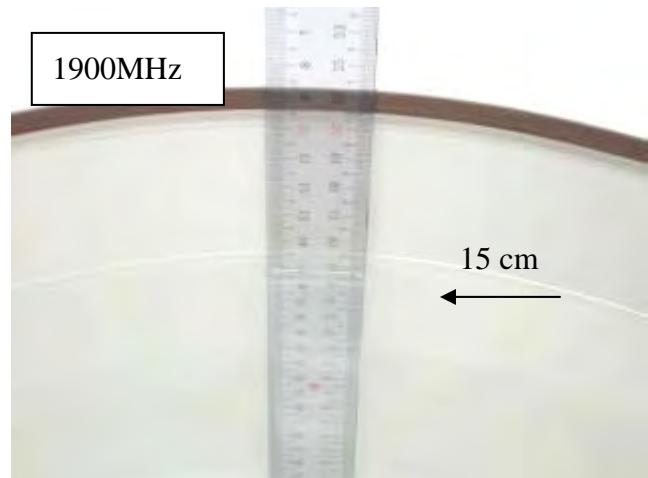


Fig.2.2 Photograph of the Tissue Simulant Fluid liquid depth 15cm for Flat (Body)



Fig.3 Put the EUT into holster and front side of EUT is paralleled with flat phantom, holster is paralleled and contacted with flat phantom.



Fig.4 Put the EUT into holster and back side of EUT is paralleled with flat phantom, holster is paralleled and contacted with flat phantom.

## 11. Photographs of the EUT



Fig.5 Front view of EUT



Fig.6 Back view of EUT



Fig.7 Holster

**End of Report**