



## Internal photo for MEGA2



Picture 1: Front view of the sample

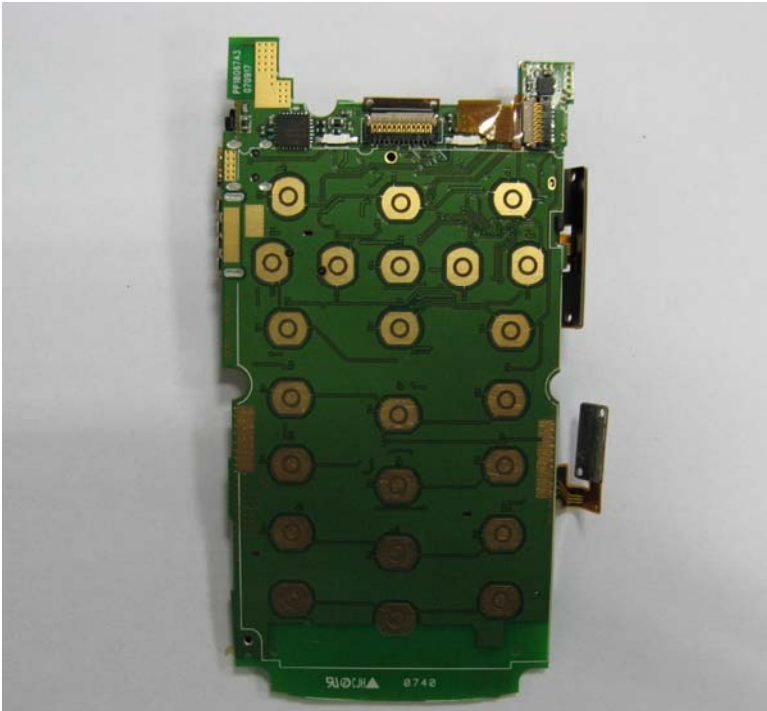

Picture 2: Back view of the sample-1

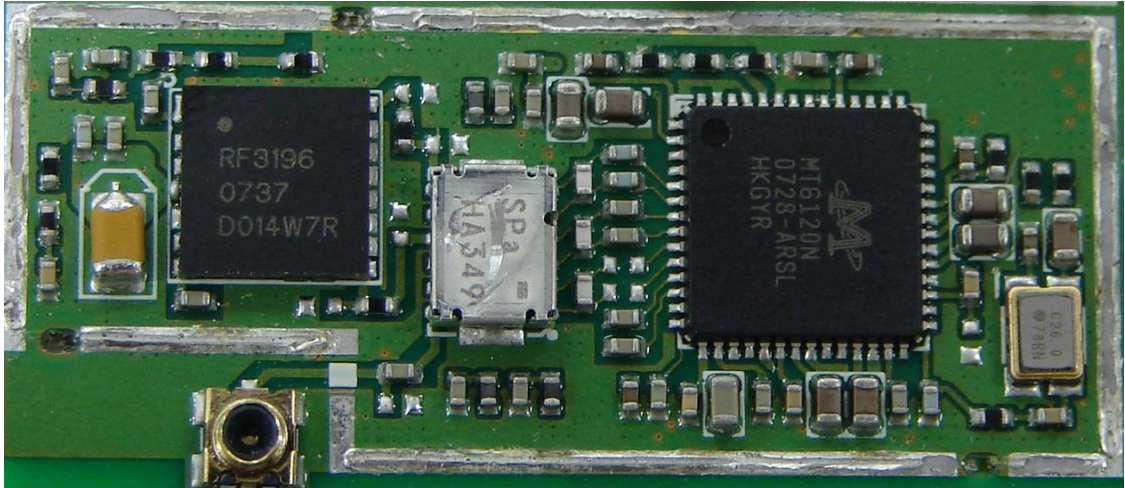

**Picture 3: Back view of the sample with the shielding cover removed**