## Calibration Laboratory of Schmid & Partner Engineering AG Zeughausstrasse 43, 8004 Zurich, Switzerland





S Schweizerischer Kalibrierdienst
Service suisse d'étalonnage
Servizio svizzero di taratura
Swiss Calibration Service

Accreditation No.: SCS 0108

Accredited by the Swiss Accreditation Service (SAS)

The Swiss Accreditation Service is one of the signatories to the EA

Multilateral Agreement for the recognition of calibration certificates

Glossary:

TSL

tissue simulating liquid

ConvF N/A sensitivity in TSL / NORM x,y,z not applicable or not measured

Calibration is Performed According to the Following Standards:

a) IEC/IEEE 62209-1528, "Measurement Procedure For The Assessment Of Specific Absorption Rate Of Human Exposure To Radio Frequency Fields From Hand-Held And Body-Worn Wireless Communication Devices - Part 1528: Human Models, Instrumentation And Procedures (Frequency Range of 4 MHz to 10 GHz)", October 2020.

#### Additional Documentation:

b) DASY System Handbook

#### Methods Applied and Interpretation of Parameters:

- Measurement Conditions: Further details are available from the Validation Report at the end of the certificate. All figures stated in the certificate are valid at the frequency indicated.
- Antenna Parameters with TSL: The dipole is mounted with the spacer to position its feed point exactly below the center marking of the flat phantom section, with the arms oriented parallel to the body axis.
- Feed Point Impedance and Return Loss: These parameters are measured with the dipole positioned under the liquid filled phantom. The impedance stated is transformed from the measurement at the SMA connector to the feed point. The Return Loss ensures low reflected power. No uncertainty required.
- SAR measured: SAR measured at the stated antenna input power.
- SAR normalized: SAR as measured, normalized to an input power of 1 W at the antenna connector.
- SAR for nominal TSL parameters: The measured TSL parameters are used to calculate the nominal SAR result.
- The absorbed power density (APD): The absorbed power density is evaluated according to Samaras T, Christ A, Kuster N, "Compliance assessment of the epithelial or absorbed power density above 6 GHz using SAR measurement systems", Bioelectromagnetics, 2021 (submitted). The additional evaluation uncertainty of 0.55 dB (rectangular distribution) is considered.

The reported uncertainty of measurement is stated as the standard uncertainty of measurement multiplied by the coverage factor k=2, which for a normal distribution corresponds to a coverage probability of approximately 95%.

Certificate No: D6.5GHzV2-1041\_Sep21

Page 2 of 6

## **Measurement Conditions**

DASY system configuration, as far as not given on page 1.

DASY Version	DASY6	V16.0	
Extrapolation	Advanced Extrapolation		
Phantom	Modular Flat Phantom		
Distance Dipole Center - TSL	5 mm	with Spacer	
Zoom Scan Resolution	dx, dy = 3.4  mm, dz = 1.4  mm	Graded Ratio = 1.4 (Z direction)	
Frequency	6500 MHz ± 1 MHz		

Head TSL parameters

The following parameters and calculations were applied.

	Temperature	Permittivity	Conductivity
Nominal Head TSL parameters	22.0 °C	34.5	6.07 mho/m
Measured Head TSL parameters	(22.0 ± 0.2) °C	33.6 ± 6 %	6.12 mho/m ± 6 %
Head TSL temperature change during test	< 0.5 °C		

# SAR result with Head TSL

SAR averaged over 1 cm <sup>3</sup> (1 g) of Head TSL	Condition	
SAR measured	100 mW input power	29.1 W/kg
SAR for nominal Head TSL parameters	normalized to 1W	289 W/kg ± 24.7 % (k=2)

SAR averaged over 10 cm <sup>3</sup> (10 g) of Head TSL	condition	
SAR measured	100 mW input power	5.34 W/kg
SAR for nominal Head TSL parameters	normalized to 1W	53.0 W/kg ± 24.4 % (k=2)

Certificate No: D6.5GHzV2-1041\_Sep21 Page 3 of 6

## **Appendix**

#### **Antenna Parameters with Head TSL**

Impedance, transformed to feed point	49.6 Ω - 1.5 jΩ
Return Loss	- 36.2 dB

## **APD (Absorbed Power Density)**

APD averaged over 1 cm <sup>2</sup>	Condition	
APD measured	100 mW input power	289 W/m²
APD measured	normalized to 1W	2890 W/m <sup>2</sup> ± 29.2 % (k=2)

APD averaged over 4 cm <sup>2</sup>	condition	
APD measured	100 mW input power	129 W/m²
APD measured	normalized to 1W	1290 W/m <sup>2</sup> ± 28.9 % (k=2)

# **General Antenna Parameters and Design**

After long term use with 100W radiated power, only a slight warming of the dipole near the feedpoint can be measured.

The dipole is made of standard semirigid coaxial cable. The center conductor of the feeding line is directly connected to the second arm of the dipole. The antenna is therefore short-circuited for DC-signals. On some of the dipoles, small end caps are added to the dipole arms in order to improve matching when loaded according to the position as explained in the "Measurement Conditions" paragraph. The SAR data are not affected by this change. The overall dipole length is still according to the Standard.

No excessive force must be applied to the dipole arms, because they might bend or the soldered connections near the feedpoint may be damaged.

#### **Additional EUT Data**

Manufactured by	SPEAG

# **DASY6 Validation Report for Head TSL**

Measurement Report for D6.5GHz-1041, UID 0 -, Channel 6500 (6500.0MHz)

Device under Test Properties	Device	under	Test	Pro	perties
------------------------------	--------	-------	------	-----	---------

Name, Manuf	acturer D	imensions	[mm]	IMEI	DUT Ty	pe	
D6.5GHz	1	6.0 x 6.0 x 3	300.0	SN: 1041	-		
Exposure Cond	ditions						
Phantom Section, TSL	Position, Test Distance [mm]	Band	Group, UID	Frequency [MHz]	Conversion Factor	TSL Cond. [S/m]	TSL Permittivity
Flat, HSL	5.00	Band	CW,	6500	5.75	6.12	33.6

Hardware Setup


Phantom	TSL	Probe, Calibration Date	DAE, Calibration Date
MFP V8.0 Center - 1182	HBBL600-10000V6	EX3DV4 - SN7405, 2020-12-30	DAE4 Sn908, 2021-06-24

#### Scan Setup

Scan Setup		Measurement Results	
	Zoom Scan		Zoom Scan
Grid Extents [mm]	22.0 x 22.0 x 22.0	Date	2021-09-02, 10:54
Grid Steps [mm]	3.4 x 3.4 x 1.4	psSAR1g [W/Kg]	29.1
Sensor Surface [mm]	1.4	psSAR10g [W/Kg]	5.34
Graded Grid	Yes	Power Drift [dB]	0.02
Grading Ratio	1.4	Power Scaling	Disabled
MAIA	N/A	Scaling Factor [dB]	
Surface Detection	VMS + 6p	TSL Correction	No correction
Scan Method	Measured	M2/M1 [%]	50.0
		Dist 3dB Peak [mm]	4.6



# Impedance Measurement Plot for Head TSL

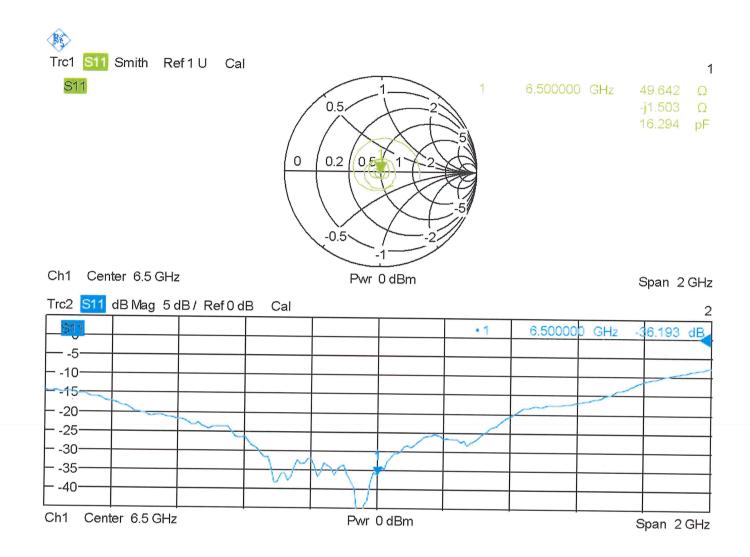

## Calibration Laboratory of Schmid & Partner Engineering AG Zeughausstrasse 43, 8004 Zurich, Switzerland





S Schweizerischer Kalibrierdienst
Service suisse d'étalonnage
Servizio svizzero di taratura
Swiss Calibration Service

Accreditation No.: SCS 0108

Issued: October 2, 2022

Accredited by the Swiss Accreditation Service (SAS)

The Swiss Accreditation Service is one of the signatories to the EA Multilateral Agreement for the recognition of calibration certificates

Client

BTL

Certificate No: 5G-Veri10-2011\_Sep22

	CERTIFICAT				
Object	5G Verification	Source 10 GHz - SN: 2011			
Calibration procedure(s)	QA CAL-45.v3 Calibration procedure for sources in air above 6 GHz				
Calibration date:	September 28,	, 2022			
he measurements and the u	ncertainties with confidenc	national standards, which realize the physical units of e probability are given on the following pages and ar atory facility: environment temperature $(22 \pm 3)^{\circ}$ C an	e part of the certificate.		
All calibrations have been con Calibration Equipment used (I			a mannary < 7070.		
Janistation Equipment used (I	1				
Primary Standards	) #	Cai Date (Certificate No.)			
-	ID # SN: 9374		Dec-22		
Reference Probe EUmmWV3		2021-12-21(No. EUmmWV3-9374_Dec21) 2022-06-27 (No. DAE4ip-1602_Jun22)			
Reference Probe EUmmWV3 DAE4ip	SN: 9374	2021-12-21(No. EUmmWV3-9374_Dec21)	Dec-22		
Reference Probe EUmmWV3 DAE4ip	SN: 9374 SN: 1602	2021-12-21(No. EUmmWV3-9374_Dec21) 2022-06-27 (No. DAE4ip-1602_Jun22)	Dec-22 Jun-23		
Reference Probe EUmmWV3 DAE4ip	SN: 9374 SN: 1602	2021-12-21(No. EUmmWV3-9374_Dec21) 2022-06-27 (No. DAE4ip-1602_Jun22)	Dec-22 Jun-23		
Reference Probe EUmmWV3 DAE4ip	SN: 9374 SN: 1602	2021-12-21(No. EUmmWV3-9374_Dec21) 2022-06-27 (No. DAE4ip-1602_Jun22)	Dec-22 Jun-23		
Primary Standards Reference Probe EUmmWV3 DAE4ip Secondary Standards	SN: 9374 SN: 1602	2021-12-21(No. EUmmWV3-9374_Dec21) 2022-06-27 (No. DAE4ip-1602_Jun22)	Dec-22 Jun-23		
Reference Probe EUmmWV3 DAE4ip	SN: 9374 SN: 1602	2021-12-21(No. EUmmWV3-9374_Dec21) 2022-06-27 (No. DAE4ip-1602_Jun22)  Check Date (in house)	Dec-22 Jun-23 Scheduled Check		
Reference Probe EUmmWV3 DAE4ip Secondary Standards	SN: 9374 SN: 1602	2021-12-21(No. EUmmWV3-9374_Dec21) 2022-06-27 (No. DAE4ip-1602_Jun22)  Check Date (in house)	Dec-22 Jun-23		
Reference Probe EUmmWV3 DAE4ip	SN: 9374 SN: 1602	2021-12-21(No. EUmmWV3-9374_Dec21) 2022-06-27 (No. DAE4ip-1602_Jun22)  Check Date (in house)	Dec-22 Jun-23 Scheduled Check		

This calibration certificate shall not be reproduced except in full without written approval of the laboratory.

## Calibration Laboratory of Schmid & Partner Engineering AG Zeughausstrasse 43, 8004 Zurich, Switzerland





S Schweizerischer Kalibrierdienst
S Service suisse d'étalonnage
Servizio svizzero di taratura
Swiss Calibration Service

Accreditation No.: SCS 0108

Accredited by the Swiss Accreditation Service (SAS)

The Swiss Accreditation Service is one of the signatories to the EA

Multilateral Agreement for the recognition of calibration certificates

Glossarv

CW

Continuous wave

## Calibration is Performed According to the Following Standards

- Internal procedure QA CAL-45-5Gsources
- IEC TR 63170 ED1, "Measurement procedure for the evaluation of power density related to human exposure to radio frequency fields from wireless communication devices operating between 6 GHz and 100 GHz", January 2018

## **Methods Applied and Interpretation of Parameters**

- Coordinate System: z-axis in the waveguide horn boresight, x-axis is in the direction of the E-field, y-axis normal to the others in the field scanning plane parallel to the horn flare and horn flange.
- Measurement Conditions: (1) 10 GHz: The radiated power is the forward power to the horn antenna minus ohmic and mismatch loss. The forward power is measured prior and after the measurement with a power sensor. During the measurements, the horn is directly connected to the cable and the antenna ohmic and mismatch losses are determined by farfield measurements. (2) 30, 45, 60 and 90 GHz: The verification sources are switched on for at least 30 minutes. Absorbers are used around the probe cub and at the ceiling to minimize reflections.
- Horn Positioning: The waveguide horn is mounted vertically on the flange of the waveguide source to allow vertical positioning of the EUmmW probe during the scan. The plane is parallel to the phantom surface. Probe distance is verified using mechanical gauges positioned on the flare of the horn.
- *E- field distribution:* E field is measured in two x-y-plane (10mm, 10mm +  $\lambda$ /4) with a vectorial E-field probe. The E-field value stated as calibration value represents the E-field-maxima and the averaged (1cm² and 4cm²) power density values at 10mm in front of the horn.
- Field polarization: Above the open horn, linear polarization of the field is expected. This is verified graphically in the field representation.

## **Calibrated Quantity**

Certificate No: 5G-Veri10-2011\_Sep22

 Local peak E-field (V/m) and average of peak spatial components of the poynting vector (W/m²) averaged over the surface area of 1 cm² and 4cm² at the nominal operational frequency of the verification source. Both square and circular averaging results are listed.

The reported uncertainty of measurement is stated as the standard uncertainty of measurement multiplied by the coverage factor k=2, which for a normal distribution corresponds to a coverage probability of approximately 95%.

#### **Measurement Conditions**

DASY system configuration, as far as not given on page 1.

DASY Version	cDASY6 Module mmWave	V3.0
Phantom	5G Phantom	
Distance Horn Aperture - plane	10 mm	
XY Scan Resolution	dx, dy = 7.5 mm	
Number of measured planes	2 (10mm, 10mm + λ/4)	
Frequency	10 GHz ± 10 MHz	

# Calibration Parameters, 10 GHz

**Circular Averaging** 

Distance Horn Aperture	Prad1	Max E-field	Uncertainty	Avg Powe	er Density	Uncertainty
to Measured Plane	(mW)	(V/m)	(k = 2)	Avg (psPDi	n+, psPDtot+,	(k = 2)
					mod+) /m²)	
				1 cm <sup>2</sup>	4 cm <sup>2</sup>	
10 mm	124	269	1.27 dB	188	152	1.28 dB

**Square Averaging** 

Distance Horn Aperture	Prad1	Max E-field	Uncertainty	Avg Powe	er Density	Uncertainty
to Measured Plane	(mW)	(V/m)	(k = 2)	Avg (psPDi	n+, psPDtot+,	(k = 2)
					mod+)	
				(W	/m²)	
				1 cm <sup>2</sup>	4 cm <sup>2</sup>	
10 mm	124	269	1.27 dB	190	153	1.28 dB

Certificate No: 5G-Veri10-2011\_Sep22

 $<sup>^{\</sup>rm 1}$  Assessed ohmic and mismatch loss plus numerical offset: 0.95 dB

# **DASY Report**

# Measurement Report for 5G Verification Source 10 GHz, UID 0 -, Channel 10000 (10000.0MHz)

#### **Device under Test Properties**

Name, Manufacturer	Dimensions [mm]	IMEI	DUT Type	
5G Verification Source 10 GHz	100.0 x 100.0 x 100.0	SN: 2011	-	


#### **Exposure Conditions**

Phantom Section	Position, Test Distance [mm]	Band	Group,	Frequency [MHz], Channel Number	Conversion Factor
5G -	10.0 mm	Validation band	CW	10000.0, 10000	1.0

#### **Hardware Setup**

Phantom	Medium	Probe, Calibration Date	DAE, Calibration Date
mmWave Phantom - 1002	Air	EUmmWV3 - SN9374_F1-55GHz, 2021-12-21	DAE4ip Sn1602, 2022-06-27

Scan Setup		Measurement Results	
•	5G Scan		5G Scan
Grid Extents [mm]	120.0 x 120.0	Date	2022-09-28, 19:23
Grid Steps [lambda]	0.25 x 0.25	Avg. Area [cm <sup>2</sup> ]	1.00
Sensor Surface [mm]	10.0	psPDn+ [W/m²]	188
MAIA	MAIA not used	psPDtot+ [W/m²]	188
		psPDmod+ [W/m²]	189
		E <sub>max</sub> [V/m]	269
		Power Drift [dB]	0.01

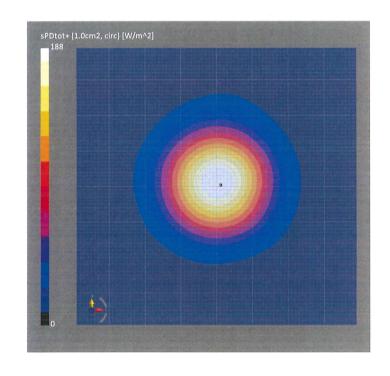

# **DASY Report**

# Measurement Report for 5G Verification Source 10 GHz, UID 0 -, Channel 10000 (10000.0MHz)

#### **Device under Test Properties**

Name, Manufacturer	Dimensions [mm]	IMEI	DUT Type
5G Verification Source 10 GHz	100.0 x 100.0 x 100.0	SN: 2011	

#### **Exposure Conditions**

Phantom Section	Position, Test Distance [mm]	Band	Group,	Frequency [MHz], Channel Number	Conversion Factor
5G -	10.0 mm	Validation band	CW	10000.0,	1.0

#### Hardware Setup

Trail attrail C occup			
Phantom	Medium	Probe, Calibration Date	DAE, Calibration Date
mmWave Phantom - 1002	Air	EUmmWV3 - SN9374_F1-55GHz, 2021-12-21	DAE4ip Sn1602, 2022-06-27

#### Scan Setup

Scan Setup		Measurement Results	
	5G Scan		5G Scan
Grid Extents [mm]	120.0 x 120.0	Date	2022-09-28, 19:23
Grid Steps [lambda]	0.25 x 0.25	Avg. Area [cm <sup>2</sup> ]	4.00
Sensor Surface [mm]	10.0	psPDn+ [W/m²]	151
MAIA	MAIA not used	psPDtot+ [W/m²]	151
		psPDmod+ [W/m²]	154
		$E_{max}[V/m]$	269
		Power Drift [dB]	0.01

