

ETL CLASSIFIED



Intertek

XXX



Mfg: 09-26-12
Rev A

FCC ID
RYM-LAL1001A

MODEL: LAL1001

100-240VAC, 50-60Hz
15Watts Max
IP24



SN: XXXXXXXX


FXI

Rose Tree Corporate Center II
1400 North Providence Road
Suite 2000
Media PA 19063-2076
800.355.3626



Medical Electrical Equipment
UL 60601-1, IEC 60601-2, CAN/CSA C22.2 No. 601.1

This device complies with Part 15 of the FCC Rules. Operation is subject to the following two conditions: 1) This device may not cause harmful interference, and 2) This device must accept any interference received, including interference that may cause undesired operation.

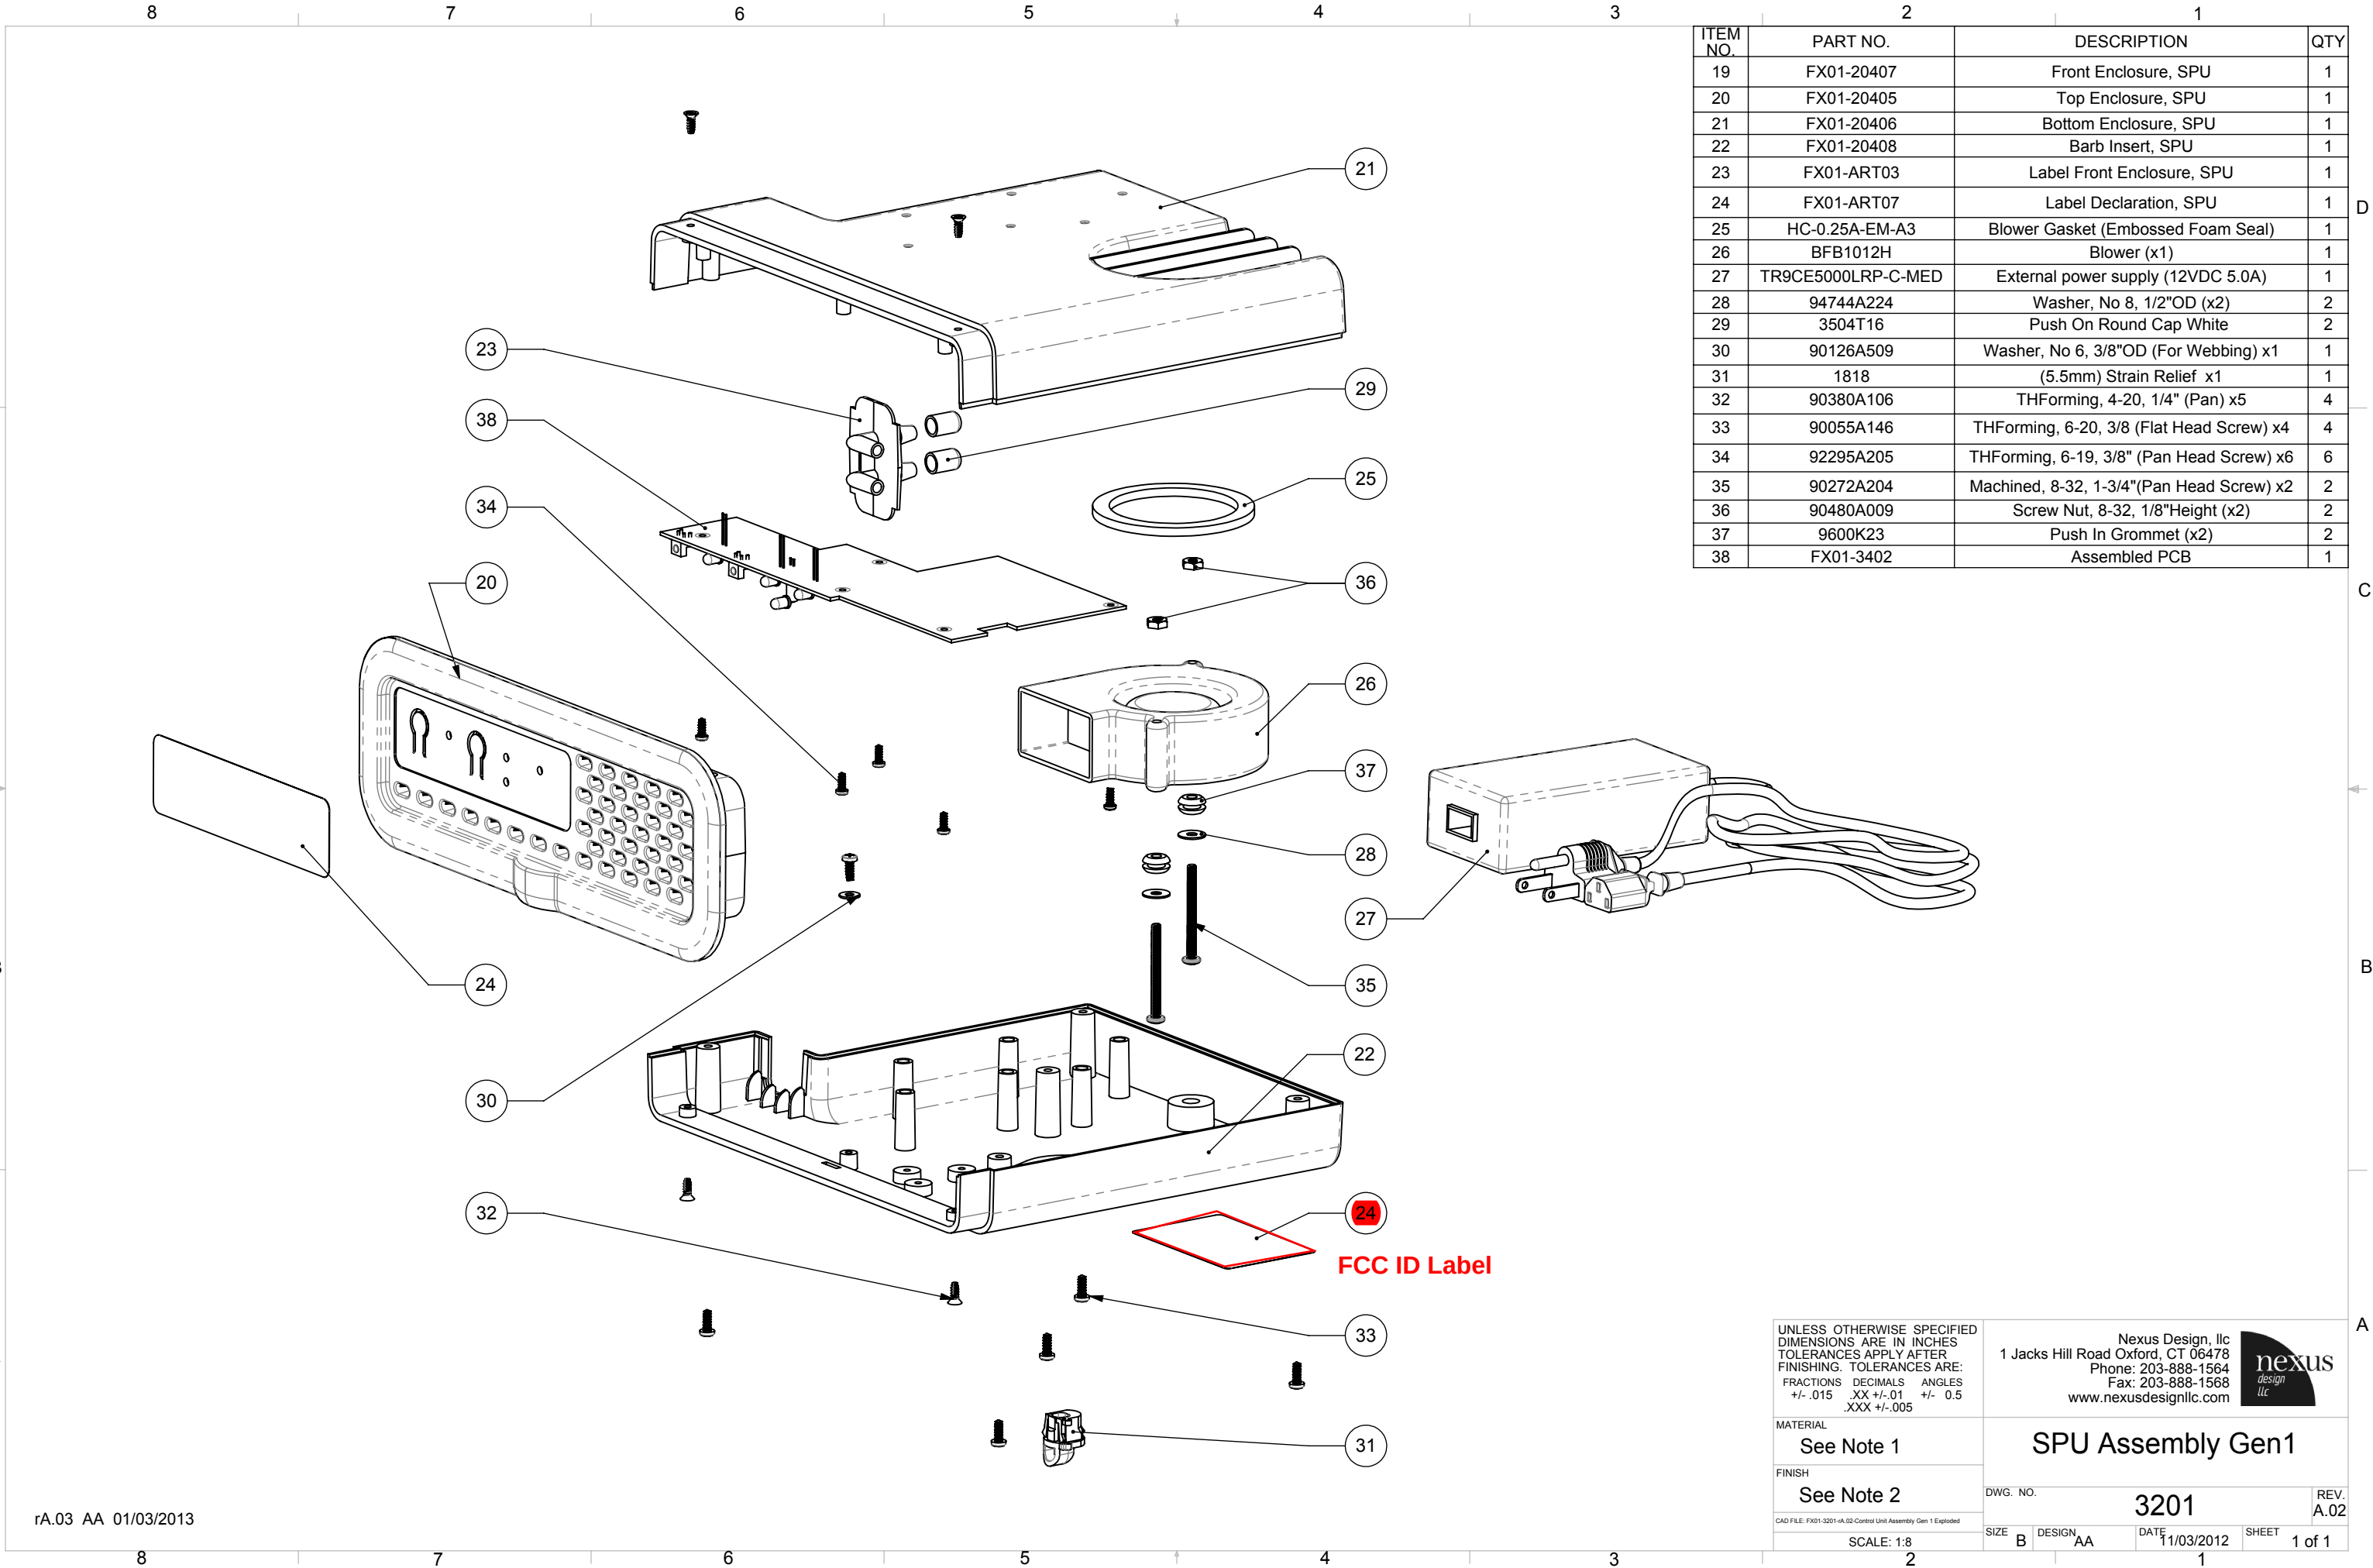

ITEM NO.	PART NO.	DESCRIPTION	QTY
19	FX01-20407	Front Enclosure, SPU	1
20	FX01-20405	Top Enclosure, SPU	1
21	FX01-20406	Bottom Enclosure, SPU	1
22	FX01-20408	Barb Insert, SPU	1
23	FX01-ART03	Label Front Enclosure, SPU	1
24	FX01-ART07	Label Declaration, SPU	1
25	HC-0.25A-EM-A3	Blower Gasket (Embossed Foam Seal)	1
26	BFB1012H	Blower (x1)	1
27	TR9CE5000LRP-C-MED	External power supply (12VDC 5.0A)	1
28	94744A224	Washer, No 8, 1/2"OD (x2)	2
29	3504T16	Push On Round Cap White	2
30	90126A509	Washer, No 6, 3/8"OD (For Webbing) x1	1
31	1818	(5.5mm) Strain Relief x1	1
32	90380A106	THForming, 4-20, 1/4" (Pan) x5	4
33	90055A146	THForming, 6-20, 3/8 (Flat Head Screw) x4	4
34	92295A205	THForming, 6-19, 3/8" (Pan Head Screw) x6	6
35	90272A204	Machined, 8-32, 1-3/4"(Pan Head Screw) x2	2
36	90480A009	Screw Nut, 8-32, 1/8"Height (x2)	2
37	9600K23	Push In Grommet (x2)	2
38	FX01-3402	Assembled PCB	1

UNLESS OTHERWISE SPECIFIED
DIMENSIONS ARE IN INCHES
TOLERANCES APPLY AFTER
FINISHING. TOLERANCES ARE:

FRACTIONS	DECIMALS	ANGLES
+/- .015	.XX +/- .01	+/- 0.5
	.XXX +/- .005	

Nexus Design, Inc
1 Jacks Hill Road Oxford, CT 06478
Phone: 203-888-1564
Fax: 203-888-1568
www.nexusdesignllc.com

nexus
design
llc

MATERIAL
See Note 1

FINISH
See Note 2

SCALE: 1:8

DWG. NO.
3201

DATE
11/03/2012

SHEET
1 of 1

REV.
A.02

SPU Assembly Gen1