

Pacific Bioscience Laboratories, Inc.

ADDENDUM TO TEST REPORT 99133-15

Smart Profile with Bluetooth

Tested To The Following Standards:

FCC Part 15 Subpart C Section(s)

**15.207 & 15.225
(13.110-14.010 MHz)**

Report No.: 99133-15A

Date of issue: March 3, 2017



This test report bears the accreditation symbol indicating that the testing performed herein meets the test and reporting requirements of ISO/IEC 17025 under the applicable scope of EMC testing for CKC Laboratories, Inc.

We strive to create long-term, trust based relationships by providing sound, adaptive, customer first testing services. We embrace each of our customers' unique EMC challenges, not as an interruption to set processes, but rather as the reason we are in business.

TABLE OF CONTENTS

Administrative Information	3
Test Report Information	3
Revision History	3
Report Authorization	3
Test Facility Information	4
Software Versions	4
Site Registration & Accreditation Information	4
Summary of Results	5
Modifications During Testing	5
Conditions During Testing	5
Equipment Under Test	6
General Product Information	6
FCC Part 15 Subpart C	7
15.215(c) Occupied Bandwidth (20dB BW)	7
15.225(a)-(c) Field Strength of Fundamental	11
15.225(e) Frequency Stability	16
15.225(d) Radiated Emissions & Band Edge	18
15.207. AC Conducted Emissions	27
Supplemental Information	34
Measurement Uncertainty	34
Emissions Test Details	34

ADMINISTRATIVE INFORMATION

Test Report Information

REPORT PREPARED FOR:

Pacific Bioscience Laboratories, Inc.
17275 NE 67th Ct
Redmond, WA 98052

REPORT PREPARED BY:

Terri Rayle
CKC Laboratories, Inc.
5046 Sierra Pines Drive
Mariposa, CA 95338

REPRESENTATIVE: Raj Shah
Customer Reference Number: 4200438589

Project Number: 99133

DATE OF EQUIPMENT RECEIPT:

November 16, 2016

DATE(S) OF TESTING:

November 16, 2016, February 2-6, 2017
and March 1, 2017

Revision History

Original: Testing of the Smart Profile with Bluetooth to FCC Part 15 Subpart C Section(s) 15.207 & 15.225 (13.110-14.010 MHz).

Addendum A: To add data for testing performed to 15.207 AC Conducted Emissions. Also added the Configuration used for the testing to the Equipment Under Test Section, the new testing dates and revised the Summary Table to reflect the result.

Report Authorization

The test data contained in this report documents the observed testing parameters pertaining to and are relevant for only the sample equipment tested in the agreed upon operational mode(s) and configuration(s) as identified herein. Compliance assessment remains the client's responsibility. This report may not be used to claim product endorsement by A2LA or any government agencies. This test report has been authorized for release under quality control from CKC Laboratories, Inc.



Steve Behm
Director of Quality Assurance & Engineering Services
CKC Laboratories, Inc.

Test Facility Information



Our laboratories are configured to effectively test a wide variety of product types. CKC utilizes first class test equipment, anechoic chambers, data acquisition and information services to create accurate, repeatable and affordable test results.

TEST LOCATION(S):
CKC Laboratories, Inc.
22116 23rd Drive S.E., Suite A
Canyon Park, Bothell, WA 98021

Software Versions

CKC Laboratories Proprietary Software	Version
EMITest Emissions	5.03.02

Site Registration & Accreditation Information

Location	CB #	TAIWAN	CANADA	FCC	JAPAN
Canyon Park, Bothell, WA	US0081	SL2-IN-E-1145R	3082C-1	US1022	A-0148

SUMMARY OF RESULTS

Standard / Specification: FCC Part 15 Subpart C - 15.225

Test Procedure	Description	Modifications	Results
15.215(c)	Occupied Bandwidth	NA	Pass
15.225(a)-(c)	Field Strength of Fundamental	NA	Pass
15.225(e)	Frequency Stability	NA	Pass
15.225(d)	Field Strength of Spurious Emissions	NA	Pass
15.207	AC Conducted Emissions	NA	Pass

NA = Not Applicable

Modifications During Testing

This list is a summary of the modifications made to the equipment during testing.

Summary of Conditions

No modifications were made during testing.

Modifications listed above must be incorporated into all production units.

Conditions During Testing

This list is a summary of the conditions noted to the equipment during testing.

Summary of Conditions

None

EQUIPMENT UNDER TEST (EUT)

During testing numerous configurations may have been utilized. The configurations listed below support compliance to the standard(s) listed in the Summary of Results section.

Configuration 1

Equipment Tested:

Device	Manufacturer	Model #	S/N
Smart Profile with Bluetooth	Pacific Bioscience Laboratories, Inc.	Smart Profile with Bluetooth	NA

Support Equipment:

Device	Manufacturer	Model #	S/N
None			

Configuration 3

Equipment Tested:

Device	Manufacturer	Model #	S/N
Smart Profile with Bluetooth	Pacific Bioscience Laboratories, Inc.	Smart Profile with Bluetooth	NA
Switching Power Supply	Clarisonic	PSM03A-050Q-3	NA
Smart Profile Charger	Pacific Bioscience Laboratories, Inc.	Smart Profile Charger	NA

Support Equipment:

Device	Manufacturer	Model #	S/N
None			

General Product Information:

Product Information	Manufacturer-Provided Details
Equipment Type:	Stand-Alone Equipment
Modulation Type(s):	ASK
Maximum Duty Cycle:	100%
Antenna Type(s) and Gain:	Loop -54.1dBi estimated
Antenna Connection Type:	Integral
Nominal Input Voltage:	2.4V DC Battery
Firmware / Software used for Test:	Iris_nRF52_EMCA_256K_v0.4

FCC Part 15 Subpart C

15.215(c) Occupied Bandwidth (20dB BW)

Test Setup/Conditions				
Test Location:	Bothell Lab C3	Test Engineer:	M. Atkinson	
Test Method:	ANSI C63.10 (2013)	Test Date(s):	2/6/2017	
Configuration:	1			
Test Setup:	Frequency tested: 13.56MHz Firmware power setting: Max Power EUT Firmware: Iris_nRF52 EMC_256K_v0.4 Protocol /MCS/Modulation: RFID Antenna type: Loop Duty Cycle: 100% Setup: The EUT is tested in X, Y & Z Axis. The EUT has a fresh battery installed. BLE transmitter is disabled. OBW is small enough that ratios in ANSI C63.10 (2013) can't be met.			


Environmental Conditions			
Temperature (°C)	21	Relative Humidity (%):	26

Test Equipment					
Asset#	Description	Manufacturer	Model	Cal Date	Cal Due
P05305	Cable	Andrews	ETSI-50T	2/15/2016	2/15/2018
00052	Loop Antenna	EMCO	6502	4/8/2016	4/8/2018
02872	Spectrum Analyzer	Agilent	E4440A	11/18/2015	11/18/2017
P06540	Cable	Andrews	Heliax	10/29/2015	10/29/2017

Test Data Summary

Frequency (MHz)	Antenna Port	Modulation	Measured (Hz)	Limit (Hz)	Results
13.56	1	ASK	29.7	None	NA

Plot

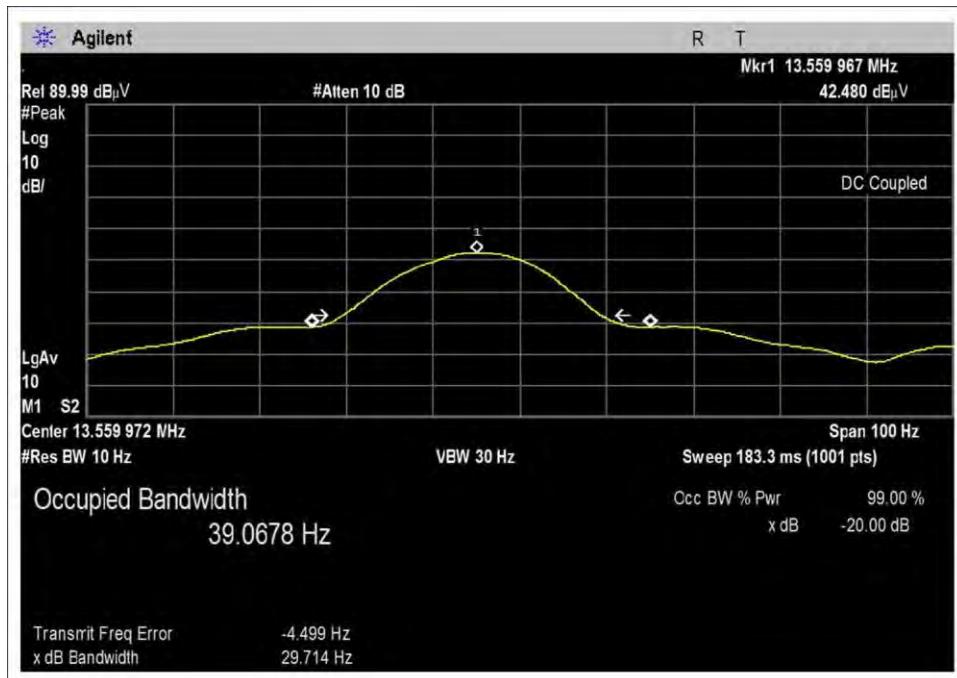

Test Setup Photos



Below 1GHz



X Axis



Y Axis



Z Axis

15.225(a)-(c) Field Strength of Fundamental

Test Setup / Conditions / Data

Test Location: CKC Laboratories, Inc. • 22116 23rd Drive SE • Bothell, WA 98021 • 1-800-500-4EMC (4362)
 Customer: **Pacific Bioscience Laboratories, Inc.**
 Specification: **15.225 Carrier and Spurious Emissions (13.110-14.010 MHz Transmitter)**
 Work Order #: **99133** Date: **2/6/2017**
 Test Type: **Maximized Emissions** Time: **10:25:33**
 Tested By: Steven Pittsford Sequence#: 2
 Software: EMITest 5.03.02

Equipment Tested:

Device	Manufacturer	Model #	S/N
Configuration 1			

Support Equipment:

Device	Manufacturer	Model #	S/N
Configuration 1			

Test Conditions / Notes:


Frequency tested: 13.56MHz
 Firmware power setting: Max Power
 EUT Firmware: Iris_nRF52 EMC_256K_v0.4
 Protocol /MCS/Modulation: RFID

Antenna type: Loop

Duty Cycle: 100%

Setup: The EUT is tested in X, Y & Z Axis.
 The EUT has a fresh battery installed.
 BLE transmitter is disabled.

Limit line in plots are corrected for system losses.

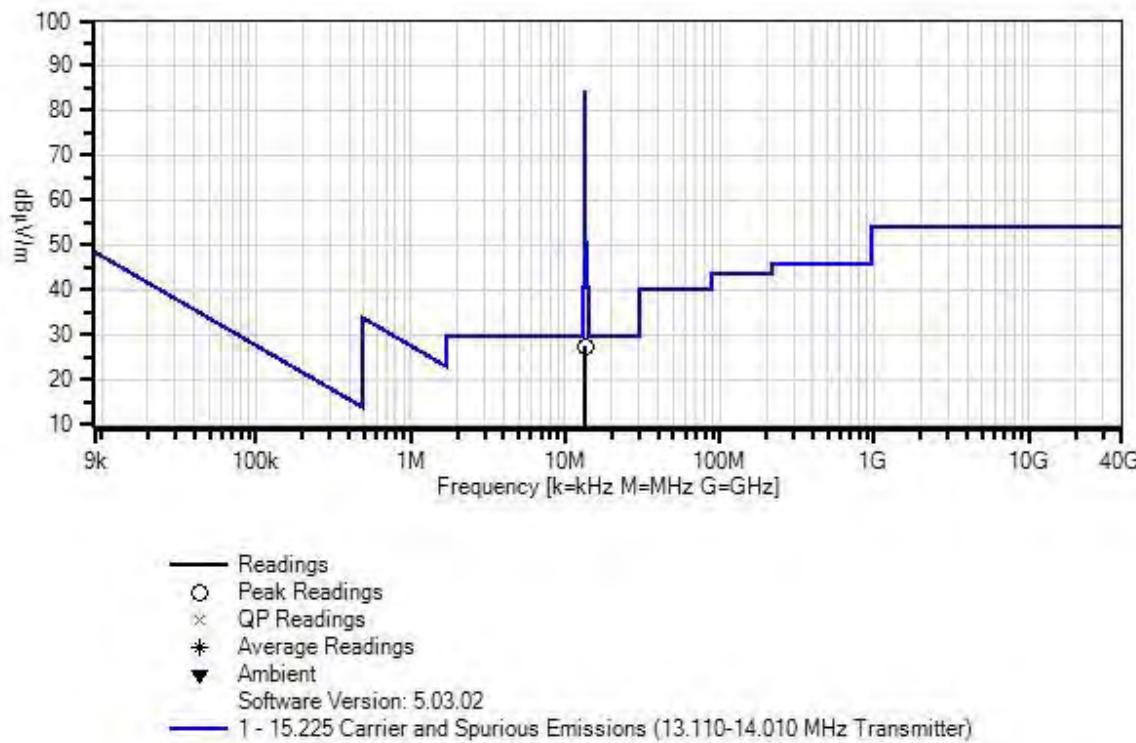Pacific Bioscience Laboratories, Inc. WO#: 99133 Sequence#: 2 Date: 2/6/2017
 15.225 Carrier and Spurious Emissions (13.110-14.010 MHz Transmitter) Test Distance: 3 Meters Para

Test Equipment:

ID	Asset #	Description	Model	Calibration Date	Cal Due Date
T1	ANP06540	Cable	Heliax	10/29/2015	10/29/2017
	AN02872	Spectrum Analyzer	E4440A	11/18/2015	11/18/2017
	ANP05963	Cable	RG-214	2/15/2016	2/15/2018
	ANP05360	Cable	RG214	11/30/2016	11/30/2018
	AN02307	Preamplifier	8447D	2/15/2016	2/15/2018
	AN01991	Biconilog Antenna	CBL6111C	3/11/2016	3/11/2018
	ANP05657	Attenuator	PE7004-6	12/22/2015	12/22/2017
T2	ANP05305	Cable	ETSI-50T	2/15/2016	2/15/2018
T3	AN00052	Loop Antenna	6502	4/8/2016	4/8/2018

Measurement Data:

Reading listed by margin.

Test Distance: 3 Meters

#	Freq MHz	Rdng dB μ V	T1 dB	T2 dB	T3 dB	Dist Table	Corr dB μ V/m	Spec dB μ V/m	Margin dB	Polar Ant
1	13.560M	58.5	+0.0	+0.2	+8.7	-40.0	27.4	84.0	-56.6	Para


Test Data Summary - Voltage Variations

This equipment is battery powered and manufacturer declares the equipment cannot operate while charging.
 Power output tests were performed using a fresh battery.

Test Data Summary – Radiated Field Strength Measurement

Frequency (MHz)	Modulation	Ant. Type	Measured (dB μ V/m @ 30m)	Limit (dB μ V/m @ 30m)	Results
13.56	ASK	Loop	27.4	≤84	Pass


Plot

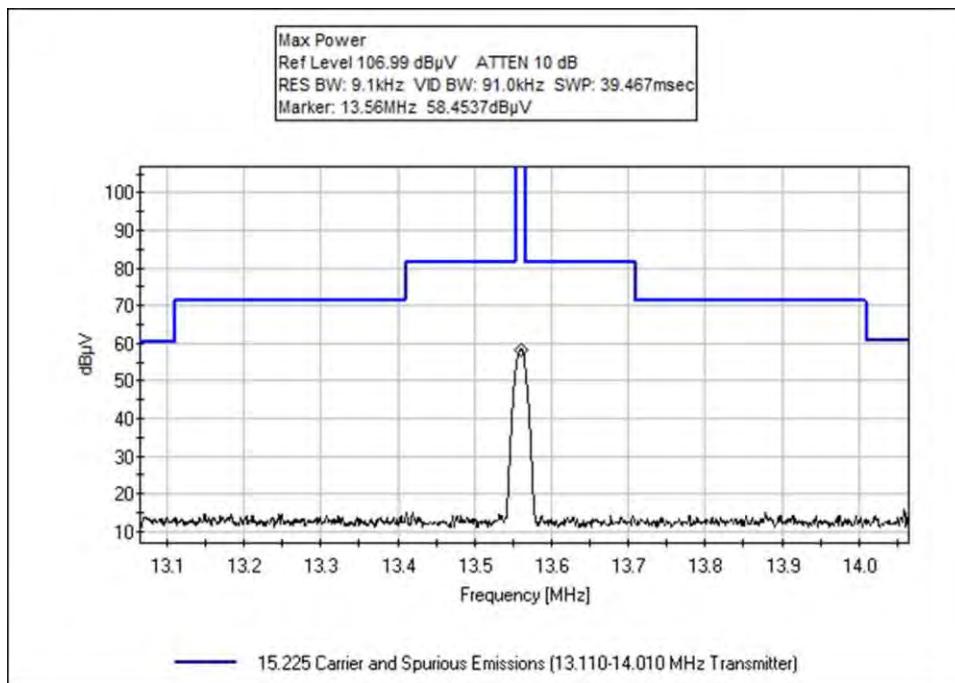

Test Setup Photos



Below 1GHz

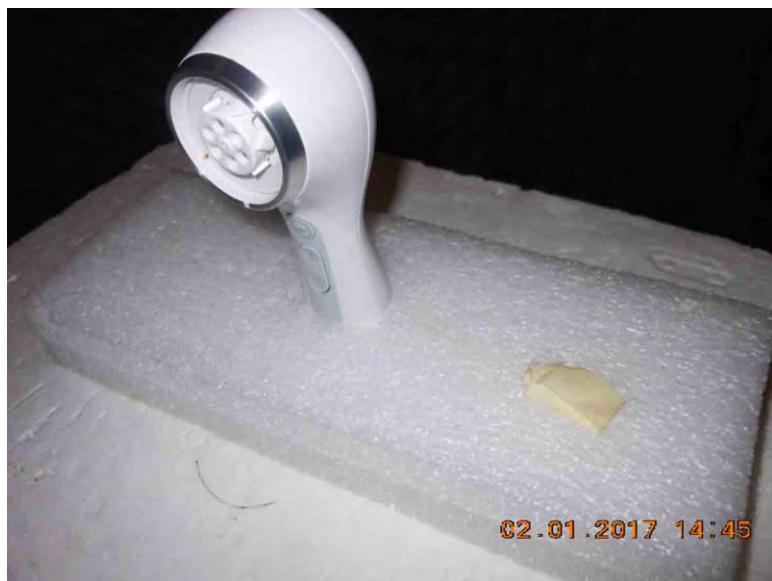

X Axis



Y Axis



Z Axis

15.225(e) Frequency Stability

Test Setup/Conditions			
Test Location:	Bothell Lab Bench	Test Engineer:	S. Pittsford
Test Method:	ANSI C63.10 (2013)	Test Date(s):	2/2/2017
Configuration:	1		
Test Setup:	Frequency tested: 13.56MHz Firmware power setting: Max Power EUT Firmware: Protocol / Modulation: Antenna type: Loop Duty Cycle: 100% Setup: The EUT's BLE radio is in standby The EUT is located inside the temperature chamber with a near field probe measuring the transmit frequency. The EUT is powered by a power supply set to maximum battery voltage rating.		

Environmental Conditions			
Temperature (°C)	22	Relative Humidity (%):	30

Test Equipment					
Asset#	Description	Manufacturer	Model	Cal Date	Cal Due
02757	Temperature Chamber	Bemco	F100/350-8	1/2/2017	1/2/2019
03029	Thermometer, Digital Infrared	Fluke	566	1/12/2017	1/12/2019
P06795	Spectrum Analyzer	HP	8560E	5/5/2015	5/5/2017

Test Data Summary					
Temperature (°C)	Voltage	Frequency (MHz)	Deviation (%)	Limit (%)	Results
-20	V _{Nominal}	13.560033	0.00024	±0.01	Pass
-10	V _{Nominal}	13.560042	0.00031	±0.01	
0	V _{Nominal}	13.560052	0.00038	±0.01	
10	V _{Nominal}	13.560050	0.00037	±0.01	
20	V _{Nominal}	13.560031	0.00023	±0.01	
30	V _{Nominal}	13.560008	0.00006	±0.01	
40	V _{Nominal}	13.559998	0.00001	±0.01	
50	V _{Nominal}	13.559996	0.00003	±0.01	
Nominal Frequency:		13.560000			

This equipment is battery powered and manufacturer declares the equipment cannot operate while charging.
 Power output tests were performed using a fresh battery.

Test Setup Photos



15.225(d) Radiated Emissions & Band Edge

Test Setup / Conditions / Data

Test Location: CKC Laboratories, Inc. • 22116 23rd Drive SE • Bothell, WA 98021 • 1-800-500-4EMC (4362)
 Customer: **Pacific Bioscience Laboratories, Inc.**
 Specification: **15.225 Carrier and Spurious Emissions (13.110-14.010 MHz Transmitter)**
 Work Order #: **99133** Date: **2/6/2017**
 Test Type: **Maximized Emissions** Time: **08:55:05**
 Tested By: Steven Pittsford Sequence#: 1
 Software: EMITest 5.03.02

Equipment Tested:

Device	Manufacturer	Model #	S/N
Configuration 1			

Support Equipment:

Device	Manufacturer	Model #	S/N
Configuration 1			

Test Conditions / Notes:


Frequency Range: 9k-1GHz
 Frequency tested: 13.56MHz
 Firmware power setting: Max Power
 EUT Firmware: Iris_nRF52_EMC_256K_v0.4
 Protocol /MCS/Modulation: RFID

Antenna type: Loop

Duty Cycle: 100%

Setup: The EUT is tested in X, Y & Z Axis.
 The EUT has a fresh battery installed.
 BLE transmitter is disabled.

Pacific Bioscience Laboratories, Inc. WO#: 99133 Sequence#: 1 Date: 2/6/2017
15.225 Carrier and Spurious Emissions (13.110-14.010 MHz Transmitter) Test Distance: 3 Meters Para

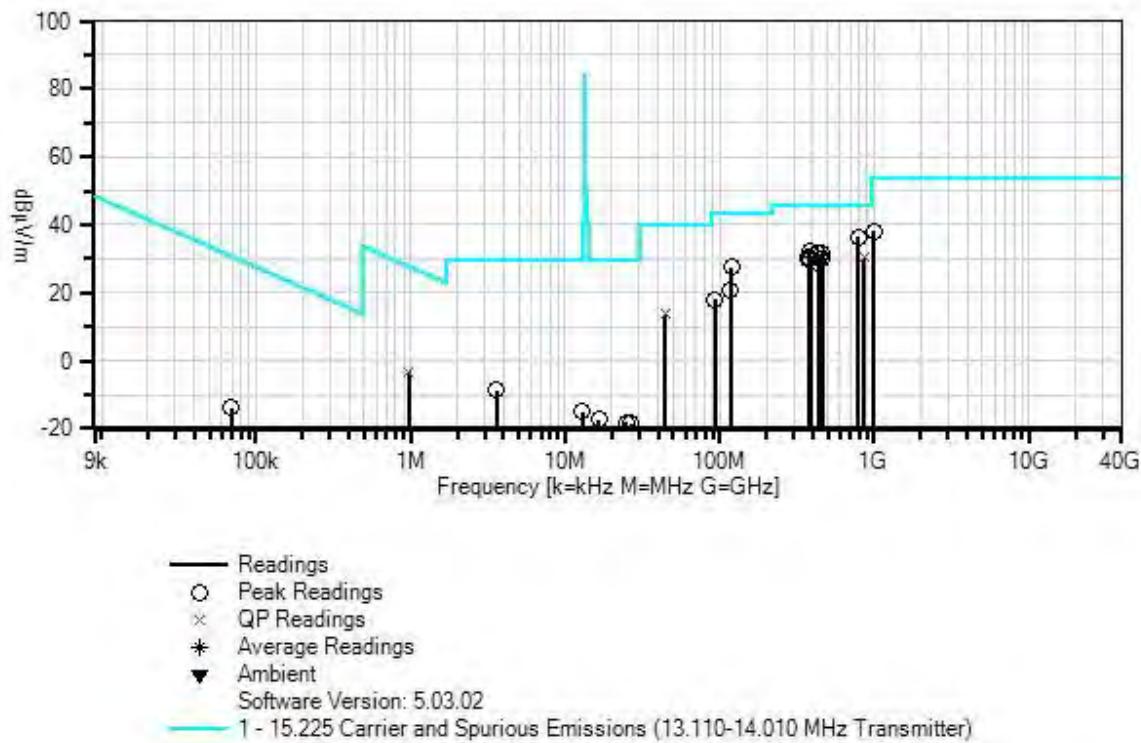

Test Equipment:

ID	Asset #	Description	Model	Calibration Date	Cal Due Date
T1	ANP06540	Cable	Heliax	10/29/2015	10/29/2017
T2	AN02872	Spectrum Analyzer	E4440A	11/18/2015	11/18/2017
T3	ANP05963	Cable	RG-214	2/15/2016	2/15/2018
T4	ANP05360	Cable	RG214	11/30/2016	11/30/2018
T5	AN02307	Preamp	8447D	2/15/2016	2/15/2018
T6	AN01991	Biconilog Antenna	CBL6111C	3/11/2016	3/11/2018
T7	ANP05657	Attenuator	PE7004-6	12/22/2015	12/22/2017
T8	ANP05305	Cable	ETSI-50T	2/15/2016	2/15/2018
T9	AN00052	Loop Antenna	6502	4/8/2016	4/8/2018

Measurement Data:

Reading listed by margin.

Test Distance: 3 Meters

#	Freq	Rdng	T1	T2	T3	T4	Dist	Corr	Spec	Margin	Polar
			T5	T6	T7	T8					
	MHz	dB μ V	dB	dB	dB	dB	Table	dB μ V/m	dB μ V/m	dB	Ant
1	789.800M	29.7	+0.3	+0.0	+2.3	+1.9	+0.0	36.5	46.0	-9.5	Horiz
			-27.8	+24.1	+6.0	+0.0					Y-Axis
			+0.0								
2	379.200M	34.6	+0.3	+0.0	+1.8	+1.2	+0.0	32.0	46.0	-14.0	Vert
			-27.5	+15.6	+6.0	+0.0					X-Axis
			+0.0								
3	461.600M	32.8	+0.3	+0.0	+1.9	+1.4	+0.0	31.8	46.0	-14.2	Vert
			-27.9	+17.3	+6.0	+0.0					X-Axis
			+0.0								
4	434.200M	33.2	+0.3	+0.0	+1.8	+1.3	+0.0	31.6	46.0	-14.4	Vert
			-27.8	+16.8	+6.0	+0.0					X-Axis
			+0.0								
5	861.000M	22.7	+0.3	+0.0	+2.3	+2.0	+0.0	30.5	46.0	-15.5	Horiz
	QP		-27.5	+24.7	+6.0	+0.0					Y-Axis
			+0.0								
^	861.000M	28.7	+0.3	+0.0	+2.3	+2.0	+0.0	36.5	46.0	-9.5	Horiz
			-27.5	+24.7	+6.0	+0.0					Y-Axis
			+0.0								
7	372.700M	33.0	+0.3	+0.0	+1.8	+1.2	+0.0	30.3	46.0	-15.7	Horiz
			-27.4	+15.4	+6.0	+0.0					Z-Axis
			+0.0								
8	118.900M	35.9	+0.1	+0.0	+1.2	+0.6	+0.0	27.6	43.5	-15.9	Horiz
			-27.6	+11.4	+6.0	+0.0					Y-Axis
			+0.0								
9	458.400M	31.1	+0.3	+0.0	+1.9	+1.4	+0.0	30.1	46.0	-15.9	Horiz
			-27.9	+17.3	+6.0	+0.0					Y-Axis
			+0.0								
10	991.900M	28.2	+0.4	+0.0	+2.5	+2.3	+0.0	38.1	54.0	-15.9	Vert
			-27.0	+25.6	+6.1	+0.0					X-Axis
			+0.0								
11	376.000M	32.8	+0.3	+0.0	+1.8	+1.2	+0.0	30.1	46.0	-15.9	Vert
			-27.5	+15.5	+6.0	+0.0					X-Axis
			+0.0								

12	384.000M	32.4	+0.3	+0.0	+1.8	+1.2	+0.0	29.9	46.0	-16.1	Horiz
			-27.5	+15.7	+6.0	+0.0				Y-Axis	
			+0.0								
13	434.200M	30.7	+0.3	+0.0	+1.8	+1.3	+0.0	29.1	46.0	-16.9	Vert
			-27.8	+16.8	+6.0	+0.0				X-Axis	
			+0.0								
14	117.300M	29.1	+0.1	+0.0	+1.2	+0.6	+0.0	20.7	43.5	-22.8	Vert
			-27.6	+11.3	+6.0	+0.0				Y-Axis	
			+0.0								
15	93.600M	28.8	+0.1	+0.0	+1.0	+0.6	+0.0	18.1	43.5	-25.4	Vert
			-27.7	+9.3	+6.0	+0.0				X-Axis	
			+0.0								
16	44.600M	23.5	+0.1	+0.0	+0.5	+0.4	+0.0	13.7	40.0	-26.3	Vert
QP			-27.9	+11.1	+6.0	+0.0				X-Axis	
			+0.0								
^	44.600M	34.5	+0.1	+0.0	+0.5	+0.4	+0.0	24.7	40.0	-15.3	Vert
			-27.9	+11.1	+6.0	+0.0				X-Axis	
			+0.0								
18	969.000k	26.8	+0.0	+0.0	+0.0	+0.0	-40.0	-3.3	27.8	-31.1	Para
QP			+0.0	+0.0	+0.0	+0.1				X-Axis	
			+9.8								
^	969.000k	32.8	+0.0	+0.0	+0.0	+0.0	-40.0	2.7	27.8	-25.1	Para
			+0.0	+0.0	+0.0	+0.1				X-Axis	
			+9.8								
20	3.578M	21.6	+0.0	+0.0	+0.0	+0.0	-40.0	-8.8	29.5	-38.3	Para
			+0.0	+0.0	+0.0	+0.1				X-Axis	
			+9.5								
21	12.965M	15.9	+0.0	+0.0	+0.0	+0.0	-40.0	-15.1	29.5	-44.6	Para
			+0.0	+0.0	+0.0	+0.2				X-Axis	
			+8.8								
22	69.000k	55.9	+0.0	+0.0	+0.0	+0.0	-80.0	-13.9	30.8	-44.7	Para
			+0.0	+0.0	+0.0	+0.0				X-Axis	
			+10.2								
23	123.451k	49.4	+0.0	+0.0	+0.0	+0.0	-80.0	-20.7	25.8	-46.5	Para
			+0.0	+0.0	+0.0	+0.0				X-Axis	
			+9.9								
24	16.594M	14.0	+0.0	+0.0	+0.0	+0.0	-40.0	-17.2	29.5	-46.7	Para
			+0.0	+0.0	+0.0	+0.3				X-Axis	
			+8.5								
25	24.812M	14.8	+0.0	+0.0	+0.0	+0.0	-40.0	-18.0	29.5	-47.5	Perp
			+0.0	+0.0	+0.0	+0.3					
			+6.9								
26	26.641M	14.6	+0.0	+0.0	+0.0	+0.0	-40.0	-18.6	29.5	-48.1	Para
			+0.0	+0.0	+0.0	+0.3				X-Axis	
			+6.5								

Band Edge

Band Edge Summary

Frequency (MHz)	Modulation	Ant. Type	Field Strength (dBuV/m @30m)	Limit (dBuV/m @30m)	Results
13.110	ASK	Loop	-17.8	≤29.5	Pass
14.010	ASK	Loop	-18.5	≤29.5	Pass

Test Setup / Conditions / Data

Test Location: CKC Laboratories, Inc. • 22116 23rd Drive SE • Bothell, WA 98021 • 1-800-500-4EMC (4362)
 Customer: **Pacific Bioscience Laboratories, Inc.**
 Specification: **15.225 Carrier and Spurious Emissions (13.110-14.010 MHz Transmitter)**
 Work Order #: **99133** Date: 2/6/2017
 Test Type: **Maximized Emissions** Time: 11:53:00
 Tested By: Steven Pittsford Sequence#: 2
 Software: EMITest 5.03.02

Equipment Tested:

Device	Manufacturer	Model #	S/N
Configuration 1			

Support Equipment:

Device	Manufacturer	Model #	S/N
Configuration 1			

Test Conditions / Notes:


Frequency Range: Band Edge
 Frequency tested: 13.56MHz
 Firmware power setting: Max Power
 EUT Firmware: Iris_nRF52 EMC_256K_v0.4
 Protocol /MCS/Modulation: RFID

Antenna type: Loop

Duty Cycle: 100%

Setup: The EUT is tested in X, Y & Z Axis.
 The EUT has a fresh battery installed.
 BLE transmitter is disabled.

Limit line in plots are corrected for system losses.

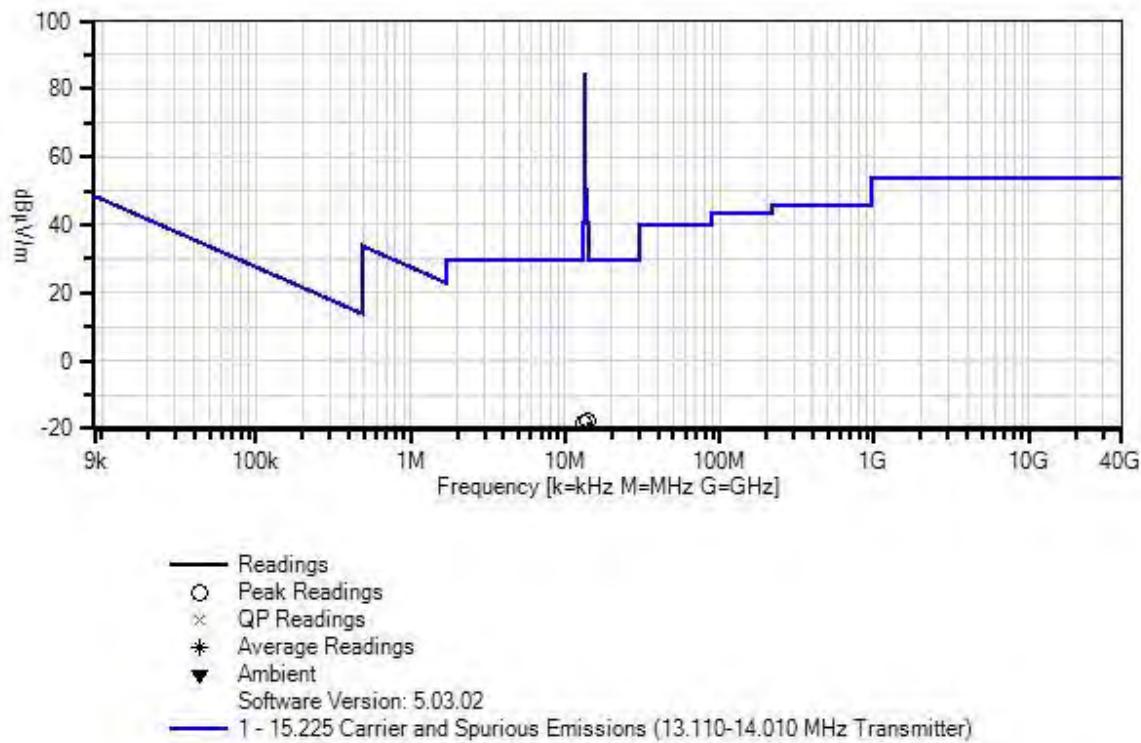Pacific Bioscience Laboratories, Inc. WO#: 99133 Sequence#: 2 Date: 2/6/2017
 15.225 Carrier and Spurious Emissions (13.110-14.010 MHz Transmitter) Test Distance: 3 Meters Para

Test Equipment:

ID	Asset #	Description	Model	Calibration Date	Cal Due Date
T1	ANP06540	Cable	Heliax	10/29/2015	10/29/2017
	AN02872	Spectrum Analyzer	E4440A	11/18/2015	11/18/2017
	ANP05963	Cable	RG-214	2/15/2016	2/15/2018
	ANP05360	Cable	RG214	11/30/2016	11/30/2018
	AN02307	Preamp	8447D	2/15/2016	2/15/2018
	AN01991	Biconilog Antenna	CBL6111C	3/11/2016	3/11/2018
	ANP05657	Attenuator	PE7004-6	12/22/2015	12/22/2017
T2	ANP05305	Cable	ETSI-50T	2/15/2016	2/15/2018
T3	AN00052	Loop Antenna	6502	4/8/2016	4/8/2018


Measurement Data:

Reading listed by margin.

Test Distance: 3 Meters

#	Freq MHz	Rdng dB μ V	T1 dB	T2 dB	T3 dB	Dist Table	Corr dB μ V/m	Spec dB μ V/m	Margin dB	Polar Ant
1	14.010M	13.3	+0.0	+0.2	+8.7	-40.0	-17.8	29.5	-47.3	Para
2	13.110M	12.5	+0.0	+0.2	+8.8	-40.0	-18.5	29.5	-48.0	Para

Band Edge Plot

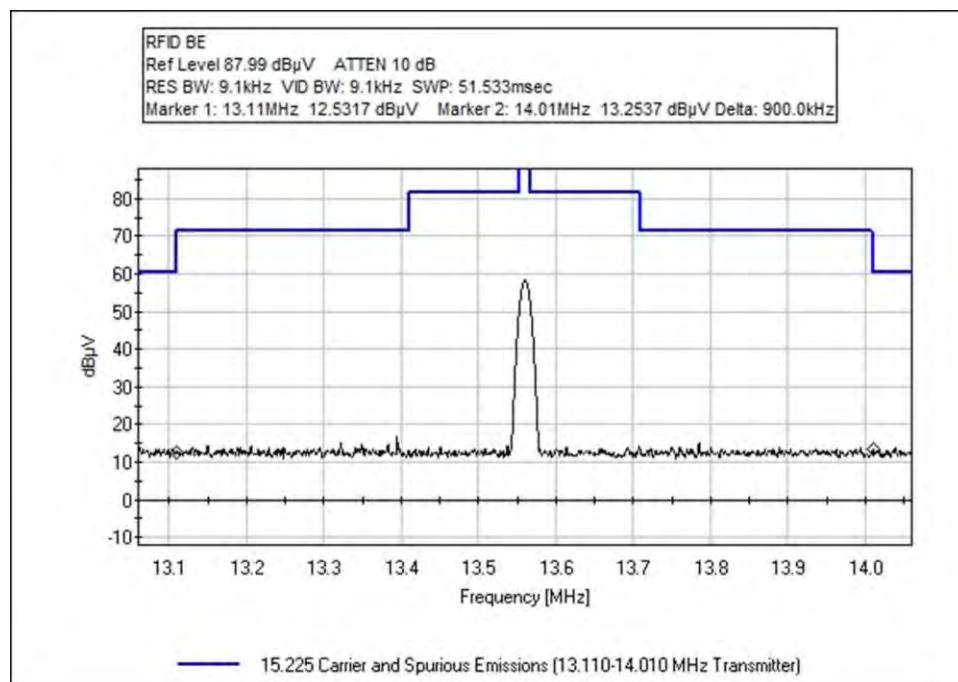

Test Setup Photos



Below 1GHz



X Axis



Y Axis



Z Axis

15.207 AC Conducted Emissions

Test Setup / Conditions / Data

Test Location: CKC Laboratories, Inc. • 22116 23rd Drive SE • Bothell, WA 98021 • 1-800-500-4EMC (4362)
 Customer: **Pacific Bioscience Laboratories, Inc.**
 Specification: **15.207 AC Mains - Average**
 Work Order #: **99133** Date: 3/1/2017
 Test Type: **Conducted Emissions** Time: 3:09:04 PM
 Tested By: Steven Pittsford Sequence#: 7
 Software: EMITest 5.03.02 115VAC 60Hz

Equipment Tested:

Device	Manufacturer	Model #	S/N
Configuration 3			

Support Equipment:

Device	Manufacturer	Model #	S/N
Configuration 3			


Test Conditions / Notes:

Temperature: 23°C
 Humidity: 28%
 Pressure: 102.2kPa
 Frequency: 0.15-30MHz

The EUT is charging, charger connected to AC mains. Transmitters are transmitting at 100% duty cycle.

Test Method: ANSI C63.10 (2013)

Pacific Bioscience Laboratories, Inc. WO#: 99133 Sequence#: 7 Date: 3/1/2017
 15.207 AC Mains - Average Test Lead: 115VAC 60Hz Line

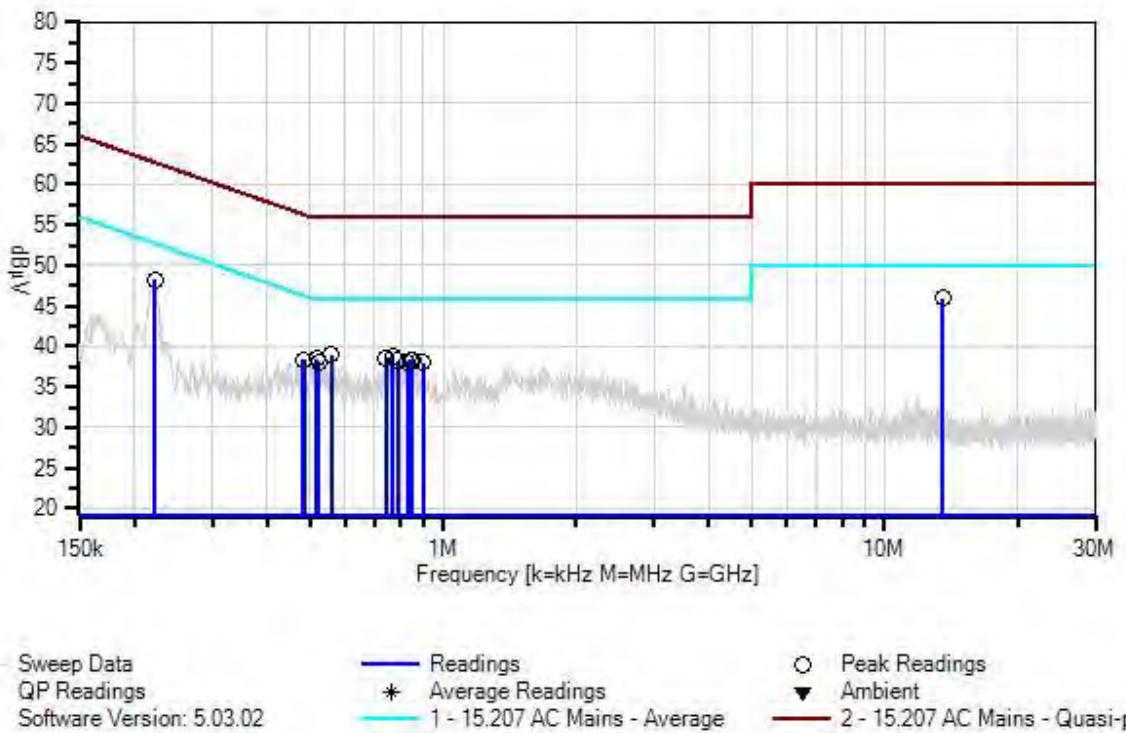

Test Equipment:

ID	Asset #	Description	Model	Calibration Date	Cal Due Date
	AN02872	Spectrum Analyzer	E4440A	11/18/2015	11/18/2017
T1	AN02611	High Pass Filter	HE9615-150K-50-720B	2/18/2016	2/18/2018
T2	ANP06540	Cable	Heliax	10/29/2015	10/29/2017
T3	ANP05305	Cable	ETSI-50T	2/15/2016	2/15/2018
T4	ANP06219	Attenuator	768-10	4/12/2016	4/12/2018
	AN01311	50uH LISN-Line1 (N)	3816/2	3/7/2016	3/7/2018
T5	AN01311	50uH LISN-Line2 (L)	3816/2	3/7/2016	3/7/2018

Measurement Data:

Reading listed by margin.

Test Lead: Line

#	Freq MHz	Rdng dB μ V	T1 dB	T2 dB	T3 dB	T4 dB	Dist Table	Corr dB μ V	Spec dB μ V	Margin dB	Polar
1	13.562M	36.5 +0.0	+0.1	+0.0	+0.2	+9.1	+0.0	45.9	50.0	-4.1	Line
2	222.720k	38.8 +0.1	+0.2	+0.0	+0.0	+9.1	+0.0	48.2	52.7	-4.5	Line
3	557.235k	29.7 +0.0	+0.2	+0.0	+0.0	+9.1	+0.0	39.0	46.0	-7.0	Line
4	767.397k	29.4 +0.0	+0.2	+0.0	+0.1	+9.1	+0.0	38.8	46.0	-7.2	Line
5	743.400k	29.2 +0.0	+0.2	+0.0	+0.1	+9.1	+0.0	38.6	46.0	-7.4	Line
6	518.693k	29.2 +0.0	+0.2	+0.0	+0.0	+9.1	+0.0	38.5	46.0	-7.5	Line
7	848.844k	29.0 +0.0	+0.2	+0.0	+0.1	+9.1	+0.0	38.4	46.0	-7.6	Line
8	852.480k	28.9 +0.0	+0.2	+0.0	+0.1	+9.1	+0.0	38.3	46.0	-7.7	Line
9	841.572k	28.9 +0.0	+0.2	+0.0	+0.1	+9.1	+0.0	38.3	46.0	-7.7	Line
10	789.941k	28.8 +0.0	+0.2	+0.0	+0.1	+9.1	+0.0	38.2	46.0	-7.8	Line
11	522.329k	28.8 +0.0	+0.2	+0.0	+0.0	+9.1	+0.0	38.1	46.0	-7.9	Line
12	829.210k	28.7 +0.0	+0.2	+0.0	+0.1	+9.1	+0.0	38.1	46.0	-7.9	Line
13	483.060k	29.0 +0.0	+0.2	+0.0	+0.0	+9.1	+0.0	38.3	46.3	-8.0	Line
14	484.514k	29.0 +0.0	+0.2	+0.0	+0.0	+9.1	+0.0	38.3	46.3	-8.0	Line
15	902.721k	28.6 +0.0	+0.2	+0.0	+0.1	+9.1	+0.0	38.0	46.0	-8.0	Line



Test Location: CKC Laboratories, Inc. • 22116 23rd Drive SE • Bothell, WA 98021 • 1-800-500-4EMC (4362)
Customer: **Pacific Bioscience Laboratories, Inc.**
Specification: **15.207 AC Mains - Average**
Work Order #: **99133** Date: 3/1/2017
Test Type: **Conducted Emissions** Time: 3:12:38 PM
Tested By: Steven Pittsford Sequence#: 8
Software: EMITest 5.03.02 115VAC 60Hz

Equipment Tested:

Device	Manufacturer	Model #	S/N
Configuration 3			

Support Equipment:

Device	Manufacturer	Model #	S/N
Configuration 3			

Test Conditions / Notes:

Temperature: 23°C


Humidity: 28%

Pressure: 102.2kPa

The EUT is charging, charger connected to AC mains. Transmitters are transmitting at 100% duty cycle.

Test Method: ANSI C63.10 (2013)

Pacific Bioscience Laboratories, Inc. WO#: 99133 Sequence#: 8 Date: 3/1/2017
 15.207 AC Mains - Average Test Lead: 115VAC 60Hz Neutral

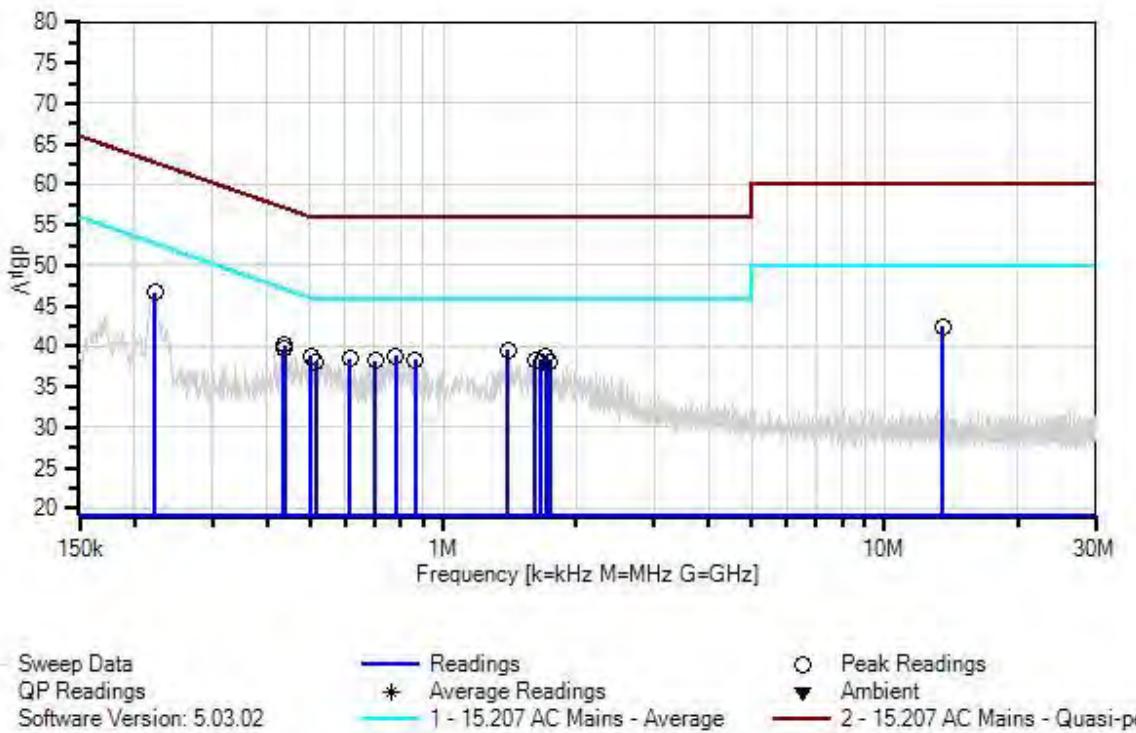

Test Equipment:

ID	Asset #	Description	Model	Calibration Date	Cal Due Date
	AN02872	Spectrum Analyzer	E4440A	11/18/2015	11/18/2017
T1	AN02611	High Pass Filter	HE9615-150K-50-720B	2/18/2016	2/18/2018
T2	ANP06540	Cable	Heliax	10/29/2015	10/29/2017
T3	ANP05305	Cable	ETSI-50T	2/15/2016	2/15/2018
T4	ANP06219	Attenuator	768-10	4/12/2016	4/12/2018
T5	AN01311	50uH LISN-Line1 (N)	3816/2	3/7/2016	3/7/2018
	AN01311	50uH LISN-Line2 (L)	3816/2	3/7/2016	3/7/2018

Measurement Data:

Reading listed by margin.

Test Lead: Neutral

#	Freq	Rdng	T1 T5	T2	T3	T4	Dist	Corr	Spec	Margin	Polar
	MHz	dB μ V	dB	dB	dB	dB	Table	dB μ V	dB μ V	dB	Ant
1	222.720k	37.4	+0.2 +0.0	+0.0	+0.0	+9.1	+0.0	46.7	52.7	-6.0	Neutr
2	1.405M	30.1	+0.2 +0.0	+0.0	+0.1	+9.1	+0.0	39.5	46.0	-6.5	Neutr
3	437.246k	30.9	+0.2 +0.0	+0.0	+0.0	+9.1	+0.0	40.2	47.1	-6.9	Neutr
4	782.669k	29.4	+0.2 +0.0	+0.0	+0.1	+9.1	+0.0	38.8	46.0	-7.2	Neutr
5	501.240k	29.4	+0.2 +0.0	+0.0	+0.0	+9.1	+0.0	38.7	46.0	-7.3	Neutr
6	1.706M	29.3	+0.2 +0.0	+0.0	+0.1	+9.1	+0.0	38.7	46.0	-7.3	Neutr
7	614.684k	29.1	+0.2 +0.0	+0.0	+0.1	+9.1	+0.0	38.5	46.0	-7.5	Neutr
8	435.064k	30.4	+0.2 +0.0	+0.0	+0.0	+9.1	+0.0	39.7	47.2	-7.5	Neutr
9	865.570k	29.0	+0.2 +0.0	+0.0	+0.1	+9.1	+0.0	38.4	46.0	-7.6	Neutr
10	13.562M	33.0	+0.1 +0.0	+0.0	+0.2	+9.1	+0.0	42.4	50.0	-7.6	Neutr
11	1.617M	28.9	+0.2 +0.0	+0.0	+0.1	+9.1	+0.0	38.3	46.0	-7.7	Neutr
12	700.494k	28.8	+0.2 +0.0	+0.0	+0.1	+9.1	+0.0	38.2	46.0	-7.8	Neutr
13	515.784k	28.8	+0.2 +0.0	+0.0	+0.0	+9.1	+0.0	38.1	46.0	-7.9	Neutr
14	1.664M	28.6	+0.2 +0.0	+0.0	+0.1	+9.1	+0.0	38.0	46.0	-8.0	Neutr
15	1.745M	28.6	+0.2 +0.0	+0.0	+0.1	+9.1	+0.0	38.0	46.0	-8.0	Neutr

Test Setup Photo



03.01.2017 15:04

SUPPLEMENTAL INFORMATION

Measurement Uncertainty

Uncertainty Value	Parameter
4.73 dB	Radiated Emissions
3.34 dB	Mains Conducted Emissions
3.30 dB	Disturbance Power

Reported uncertainties represent expanded uncertainties expressed at approximately the 95% confidence level using a coverage factor of $k=2$. Compliance is deemed to occur provided measurements are below the specified limits.

Emissions Test Details

TESTING PARAMETERS

Unless otherwise indicated, the following configuration parameters are used for equipment setup: The cables were routed consistent with the typical application by varying the configuration of the test sample. Interface cables were connected to the available ports of the test unit. The effect of varying the position of the cables was investigated to find the configuration that produced maximum emissions. Cables were of the type and length specified in the individual requirements. The length of cable that produced maximum emissions was selected.

The equipment under test (EUT) was set up in a manner that represented its normal use, as shown in the setup photographs. Any special conditions required for the EUT to operate normally are identified in the comments that accompany the emissions tables.

The emissions data was taken with a spectrum analyzer or receiver. Incorporating the applicable correction factors for distance, antenna, cable loss and amplifier gain, the data was reduced as shown in the table below. The corrected data was then compared to the applicable emission limits. Preliminary and final measurements were taken in order to ensure that all emissions from the EUT were found and maximized.

CORRECTION FACTORS

The basic spectrum analyzer reading was converted using correction factors as shown in the highest emissions readings in the tables. For radiated emissions in $\text{dB}\mu\text{V}/\text{m}$, the spectrum analyzer reading in $\text{dB}\mu\text{V}$ was corrected by using the following formula. This reading was then compared to the applicable specification limit. Individual measurements were compared with the displayed limit value in the margin column. The margin was calculated based on subtracting the limit value from the corrected measurement value; a positive margin represents a measurement exceeding the limit, while a negative margin represents a measurement less than the limit.

SAMPLE CALCULATIONS	
Meter reading	($\text{dB}\mu\text{V}$)
+ Antenna Factor	(dB/m)
+ Cable Loss	(dB)
- Distance Correction	(dB)
- Preamplifier Gain	(dB)
= Corrected Reading	($\text{dB}\mu\text{V}/\text{m}$)

TEST INSTRUMENTATION AND ANALYZER SETTINGS

The test instrumentation and equipment listed were used to collect the emissions data. A spectrum analyzer or receiver was used for all measurements. Unless otherwise specified, the following table shows the measuring equipment bandwidth settings that were used in designated frequency bands. For testing emissions, an appropriate reference level and a vertical scale size of 10 dB per division were used.

MEASURING EQUIPMENT BANDWIDTH SETTINGS PER FREQUENCY RANGE			
TEST	BEGINNING FREQUENCY	ENDING FREQUENCY	BANDWIDTH SETTING
CONDUCTED EMISSIONS	150 kHz	30 MHz	9 kHz
RADIATED EMISSIONS	9 kHz	150 kHz	200 Hz
RADIATED EMISSIONS	150 kHz	30 MHz	9 kHz
RADIATED EMISSIONS	30 MHz	1000 MHz	120 kHz
RADIATED EMISSIONS	1000 MHz	>1 GHz	1 MHz

SPECTRUM ANALYZER/RECEIVER DETECTOR FUNCTIONS

The notes that accompany the measurements contained in the emissions tables indicate the type of detector function used to obtain the given readings. Unless otherwise noted, all readings were made in the "positive peak" detector mode. Whenever a "quasi-peak" or "average" reading was recorded, the measurement was annotated with a "QP" or an "Ave" on the appropriate rows of the data sheets. In cases where quasi-peak or average limits were employed and data exists for multiple measurement types for the same frequency then the peak measurement was retained in the report for reference, however the numbering for the affected row was removed and an arrow or caret ("^") was placed in the far left-hand column indicating that the row above takes precedence for comparison to the limit. The following paragraphs describe in more detail the detector functions and when they were used to obtain the emissions data.

Peak

In this mode, the spectrum analyzer or receiver recorded all emissions at their peak value as the frequency band selected was scanned. By combining this function with another feature called "peak hold," the measurement device had the ability to measure intermittent or low duty cycle transient emission peak levels. In this mode the measuring device made a slow scan across the frequency band selected and measured the peak emission value found at each frequency across the band.

Quasi-Peak

Quasi-peak measurements were taken using the quasi-peak detector when the true peak values exceeded or were within 2 dB of a quasi-peak specification limit. Additional QP measurements may have been taken at the discretion of the operator.

Average

Average measurements were taken using the average detector when the true peak values exceeded or were within 2 dB of an average specification limit. Additional average measurements may have been taken at the discretion of the operator. If the specification or test procedure requires trace averaging, then the averaging was performed using 100 samples or as required by the specification. All other average measurements are performed using video bandwidth averaging. To make these measurements, the test engineer reduces the video bandwidth on the measuring device until the modulation of the signal is filtered out. At this point the measuring device is set into the linear mode and the scan time is reduced.