

Calibration Laboratory of
Schmid & Partner
Engineering AG
 Zeughausstrasse 43, 8004 Zurich, Switzerland

Client **H-CT (Dymstec)**

CALIBRATION CERTIFICATE																																			
Object(s)	ET3DV6 - SN:1609																																		
Calibration procedure(s)	QA CAL-01.v2 Calibration procedure for dosimetric E-field probes																																		
Calibration date:	September 2, 2004																																		
Condition of the calibrated item	In Tolerance (according to the specific calibration document)																																		
This calibration certificate documents the traceability to national standards, which realize the physical units of measurements (SI). The measurements and the uncertainties with confidence probability are given on the following pages and are part of the certificate. All calibrations have been conducted in the closed laboratory facility; environment temperature 22 +/- 2 degrees Celsius and humidity < 75%. Calibration Equipment used (M&TE critical for calibration) <table border="1"> <thead> <tr> <th>Model Type</th> <th>ID #</th> <th>Cal Date (Calibrated by, Certificate No.)</th> <th>Scheduled Calibration</th> </tr> </thead> <tbody> <tr> <td>Power meter EPM E4419B</td> <td>GB41263874</td> <td>5-May-04 (METAS, No 251-00368)</td> <td>May-05</td> </tr> <tr> <td>Power sensor E4412A</td> <td>MY41495277</td> <td>5-May-04 (METAS, No 251-00368)</td> <td>May-05</td> </tr> <tr> <td>Reference 20 dB Attenuator</td> <td>SN: 0086 (20b)</td> <td>3-May-04 (METAS, No 251-00369)</td> <td>May-05</td> </tr> <tr> <td>Fliuke Process Calibrator Type 702</td> <td>SN: 6295803</td> <td>8-Sep-03 (Sintrel SCS No. F030020)</td> <td>Sep-04</td> </tr> <tr> <td>Power sensor HP 8481A</td> <td>MY41092180</td> <td>18-Sep-02 (SPEAG, in house check Oct03)</td> <td>In house check: Oct 05</td> </tr> <tr> <td>RF generator HP 8684C</td> <td>US3642U01700</td> <td>4-Aug-99 (SPEAG, in house check Aug02)</td> <td>In house check: Aug05</td> </tr> <tr> <td>Network Analyzer HP 8753E</td> <td>US37390565</td> <td>18-Oct-01 (SPEAG, in house check Oct03)</td> <td>In house check: Oct 05</td> </tr> </tbody> </table>				Model Type	ID #	Cal Date (Calibrated by, Certificate No.)	Scheduled Calibration	Power meter EPM E4419B	GB41263874	5-May-04 (METAS, No 251-00368)	May-05	Power sensor E4412A	MY41495277	5-May-04 (METAS, No 251-00368)	May-05	Reference 20 dB Attenuator	SN: 0086 (20b)	3-May-04 (METAS, No 251-00369)	May-05	Fliuke Process Calibrator Type 702	SN: 6295803	8-Sep-03 (Sintrel SCS No. F030020)	Sep-04	Power sensor HP 8481A	MY41092180	18-Sep-02 (SPEAG, in house check Oct03)	In house check: Oct 05	RF generator HP 8684C	US3642U01700	4-Aug-99 (SPEAG, in house check Aug02)	In house check: Aug05	Network Analyzer HP 8753E	US37390565	18-Oct-01 (SPEAG, in house check Oct03)	In house check: Oct 05
Model Type	ID #	Cal Date (Calibrated by, Certificate No.)	Scheduled Calibration																																
Power meter EPM E4419B	GB41263874	5-May-04 (METAS, No 251-00368)	May-05																																
Power sensor E4412A	MY41495277	5-May-04 (METAS, No 251-00368)	May-05																																
Reference 20 dB Attenuator	SN: 0086 (20b)	3-May-04 (METAS, No 251-00369)	May-05																																
Fliuke Process Calibrator Type 702	SN: 6295803	8-Sep-03 (Sintrel SCS No. F030020)	Sep-04																																
Power sensor HP 8481A	MY41092180	18-Sep-02 (SPEAG, in house check Oct03)	In house check: Oct 05																																
RF generator HP 8684C	US3642U01700	4-Aug-99 (SPEAG, in house check Aug02)	In house check: Aug05																																
Network Analyzer HP 8753E	US37390565	18-Oct-01 (SPEAG, in house check Oct03)	In house check: Oct 05																																
Calibrated by:	Name Nico Vettari	Function Technician	Signature 																																
Approved by:	Name Kaša Polovic	Laboratory Director	Signature 																																
Date issued September 2, 2004																																			
This calibration certificate is issued as an intermediate solution until the accreditation process (based on ISO/IEC 17025 International Standard) for Calibration Laboratory of Schmid & Partner Engineering AG is completed.																																			

Probe ET3DV6

SN:1609

Manufactured:	July 27, 2001
Last calibrated:	January 22, 2004
Repaired:	August 18, 2004
Recalibrated:	September 2, 2004

Calibrated for DASY Systems

(Note: non-compatible with DASY2 system!)

ET3DV6 SN:1609

September 2, 2004

DASY - Parameters of Probe: ET3DV6 SN:1609

Sensitivity in Free Space

NomX	1.86 $\mu\text{V}/(\text{V}/\text{m})^2$
NormY	1.79 $\mu\text{V}/(\text{V}/\text{m})^2$
NormZ	1.78 $\mu\text{V}/(\text{V}/\text{m})^2$

Diode Compression^A

DCP X	96	mV
DCP Y	96	mV
DCP Z	96	mV

Sensitivity in Tissue Simulating Liquid (Conversion Factors)

Please see Page 7.

Boundary Effect

Head 900 MHz Typical SAR gradient: 5 % per mm

Sensor Center to Phantom Surface Distance		3.7 mm	4.7 mm
SAR _{cc} [%]	Without Correction Algorithm	8.8	4.3
SAR _{cc} [%]	With Correction Algorithm	0.0	0.1

Head 1800 MHz Typical SAR gradient: 10 % per mm

Sensor Center to Phantom Surface Distance		3.7 mm	4.7 mm
SAR _{cc} [%]	Without Correction Algorithm	13.6	9.0
SAR _{cc} [%]	With Correction Algorithm	0.2	0.0

Sensor Offset

Probe Tip to Sensor Center	2.7 mm
Optical Surface Detection	in tolerance

The reported uncertainty of measurement is stated as the standard uncertainty of measurement multiplied by the coverage factor k=2, which for a normal distribution corresponds to a coverage probability of approximately 95%.


^A numerical linearization parameter: uncertainty not required

ET3DV6 SN:1609

September 2, 2004

Frequency Response of E-Field




(TEM-Cell:ifi110, Waveguide R22)

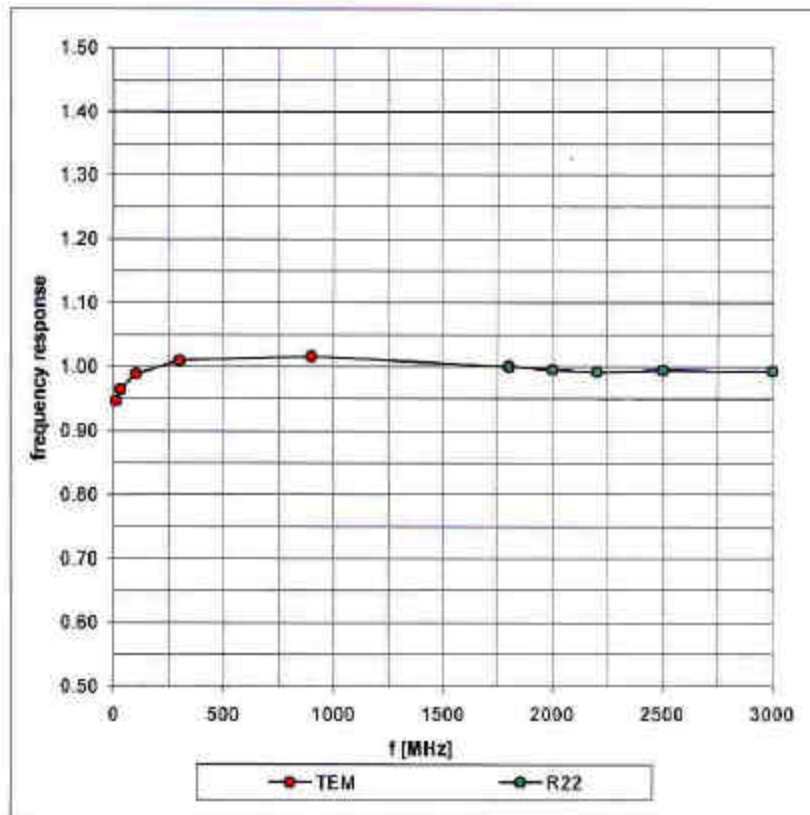

ET3DV6 SN:1609

September 2, 2004

Receiving Pattern (ϕ), $\theta = 0^\circ$

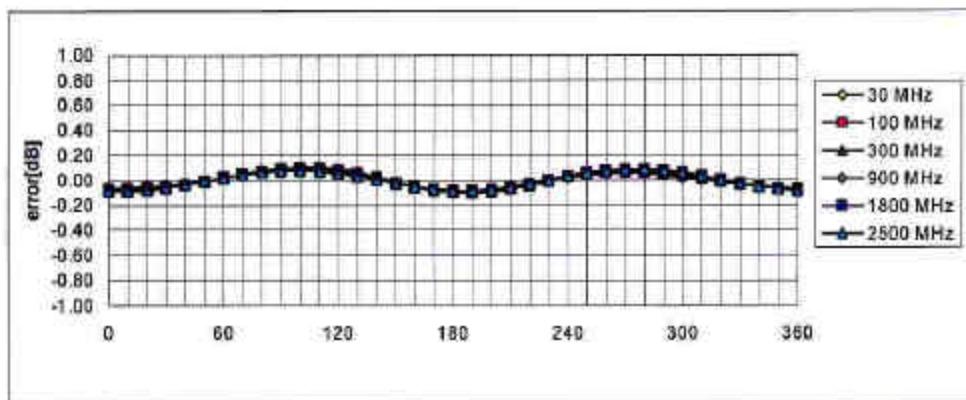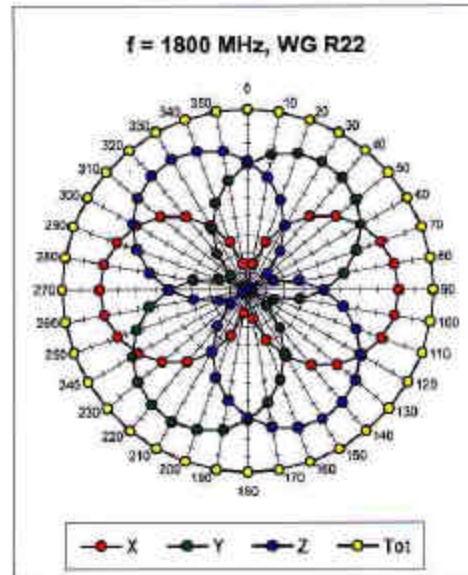
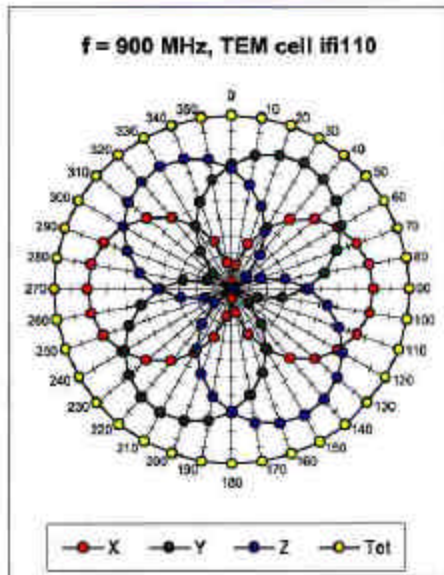


Axial Isotropy Error < ± 0.2 dB

ET3DV6 SN:1609

September 2, 2004



Dynamic Range $f(\text{SAR}_{\text{head}})$ (Waveguide R22)

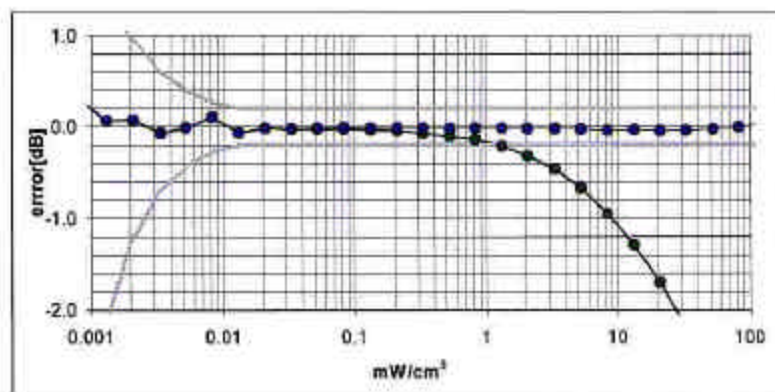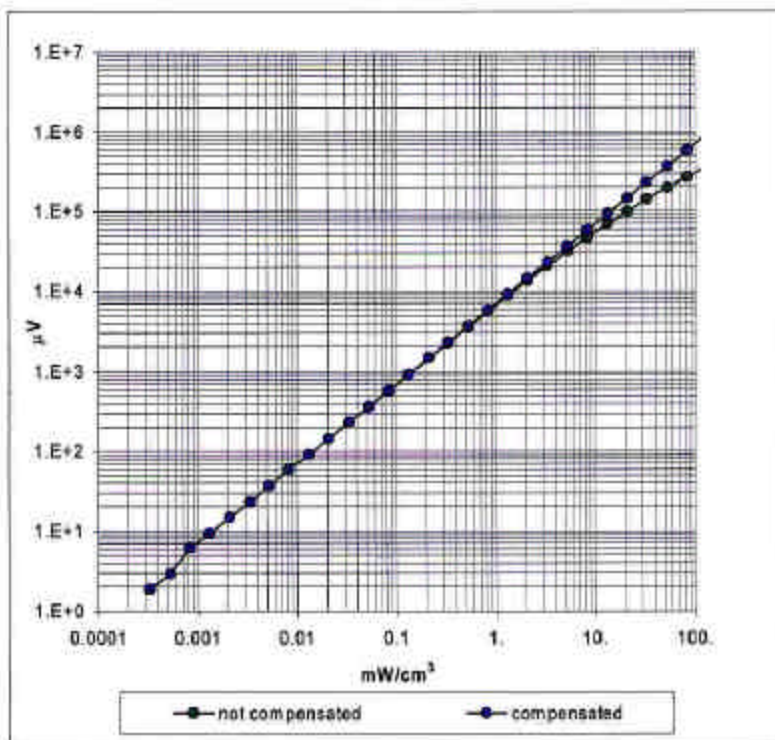
Probe Linearity Error $< \pm 0.2 \text{ dB}$

ET3DV6 SN:1609

September 2, 2004

Conversion Factor Assessment

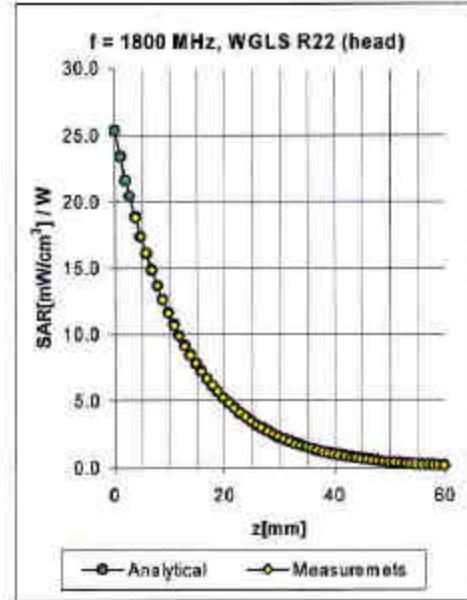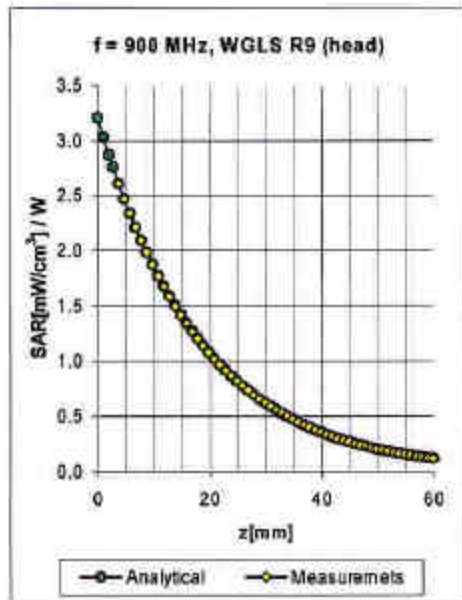


f [MHz]	Validity [MHz] ^a	Tissue	Permittivity	Conductivity	Alpha	Depth	ConvF Uncertainty
450	400-500	Head	$43.5 \pm 5\%$	$0.87 \pm 5\%$	0.19	2.72	$7.69 \pm 15.5\% (k=2)$
900	800-1000	Head	$41.5 \pm 5\%$	$0.97 \pm 5\%$	0.90	1.53	$6.63 \pm 11.3\% (k=2)$
1800	1710-1910	Head	$40.0 \pm 5\%$	$1.40 \pm 5\%$	0.50	2.61	$5.34 \pm 11.7\% (k=2)$
1950	1900-2000	Head	$40.0 \pm 5\%$	$1.40 \pm 5\%$	0.57	2.70	$4.89 \pm 9.7\% (k=2)$
2450	2400-2500	Head	$39.2 \pm 5\%$	$1.80 \pm 5\%$	0.99	1.92	$4.57 \pm 9.7\% (k=2)$
450	400-500	Body	$56.7 \pm 5\%$	$0.94 \pm 5\%$	0.14	2.69	$7.40 \pm 15.5\% (k=2)$
835	750-950	Body	$55.2 \pm 5\%$	$0.97 \pm 5\%$	0.58	1.95	$6.47 \pm 11.9\% (k=2)$
1900	1800-2000	Body	$53.3 \pm 5\%$	$1.52 \pm 5\%$	0.59	2.76	$4.60 \pm 11.3\% (k=2)$
2450	2400-2500	Body	$52.7 \pm 5\%$	$1.95 \pm 5\%$	1.21	1.63	$4.44 \pm 9.7\% (k=2)$

^a The total standard uncertainty is calculated as root-sum-square of standard uncertainty of the Conversion Factor at calibration frequency and the standard uncertainty for the indicated frequency band.

ET3DV6 SN:1609

September 2, 2004

Deviation from Isotropy in HSL

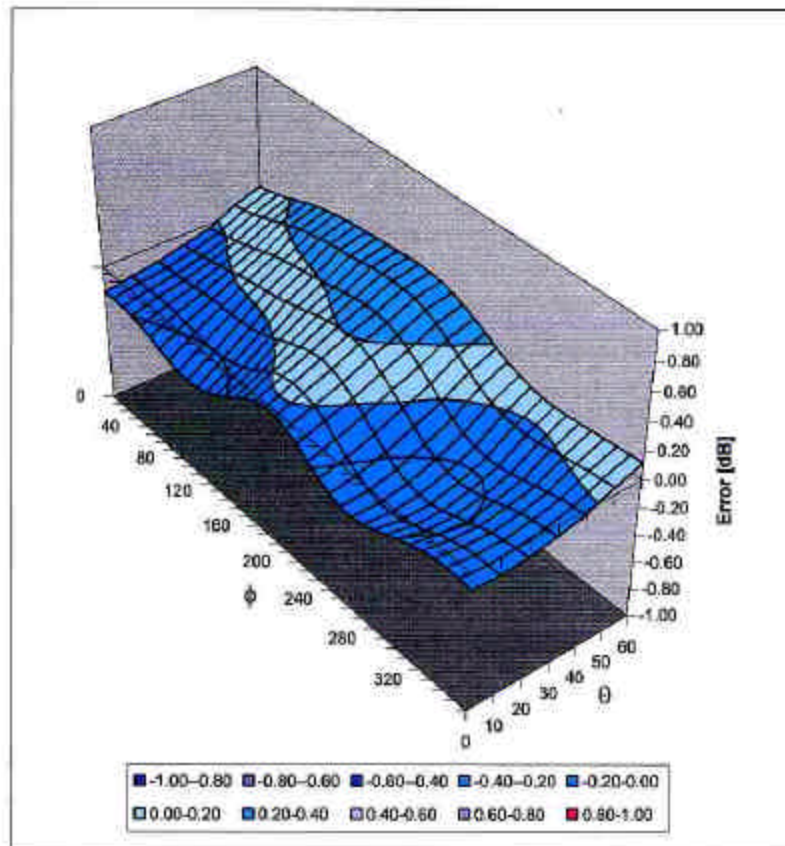Error (θ , ϕ), $f = 900$ MHz


Spherical Isotropy Error $< \pm 0.4$ dB

Schmid & Partner Engineering AG

s p e a g

Zeughausstrasse 43, 8004 Zurich, Switzerland
Phone +41 1 245 9700, Fax +41 1 245 9779
info@speag.com, <http://www.speag.com>

IMPORTANT NOTICE

USAGE OF PROBES IN ORGANIC SOLVENTS

Diethylene Glycol Monobutyl Ether (the basis for liquids above 1 GHz), as many other organic solvents, is a very effective softener for synthetic materials. These solvents can cause irreparable damage to certain SPEAG products, except those which are explicitly declared as compliant with organic solvents.

Compatible Probes:

- ET3DV6
- ET3DV6R
- ES3DVx
- ER3DV6
- H3DV6

Important Note for ET3DV6 Probes:

The ET3DV6 probes shall not be exposed to solvents longer than necessary for the measurements and shall be cleaned daily after use with warm water and stored dry.

s p e a g

Schmid & Partner Engineering AG
Zeughausstrasse 43, 8004 Zurich, Switzerland
Phone +41 1 245 9700, Fax +41 1 245 9779
info@speag.com, <http://www.speag.com>

Schmid & Partner Engineering AG

Technical Note 01.06.15-1

June 2002

Calibration Laboratory of
Schmid & Partner
Engineering AG
 Zauggstrasse 43, 8004 Zurich, Switzerland

Client **Harwha (Dymtec)**

CALIBRATION CERTIFICATE

Object(s) **ET3DV8 - SN:1807**

Calibration procedure(s) **QA CAL-01.v2
Calibration procedure for dosimetric E-field probes**

Calibration date: **April 28, 2004**

Condition of the calibrated item **In Tolerance (according to the specific calibration document)**

This calibration certificate documents the traceability to national standards, which realize the physical units of measurements (SI).
 The measurements and the uncertainties with confidence probability are given on the following pages and are part of the certificate.

All calibrations have been conducted in the closed laboratory facility: environment temperature 22 ± 2 degrees Celsius and humidity $< 75\%$.

Calibration Equipment used (M&E critical for calibration)

Model Type	ID #	Cal Date (Calibrated by, Certificate No.)	Scheduled Calibration
Power meter EPM E442	GB37480704	6-Nov-03 (METAS, No. 252-0254)	Nov-04
Power sensor HP 8481A	US37292783	6-Nov-03 (METAS, No. 252-0254)	Nov-04
Fluke Process Calibrator Type 702	SN 6295803	6-Sep-03 (Sintrel SCS No. E-030020)	Sep-04
Power sensor HP 8481A	MY41082100	18-Sep-02 (SPEAG, in house check Oct-03)	In house check: Oct-05
RF generator HP 8594C	US3642J01700	4-Aug-99 (SPEAG, in house check Aug-02)	In house check: Aug-05
Network Analyzer HP 8753E	US37390585	18-Oct-01 (SPEAG, in house check Oct-03)	In house check: Oct-05

	Name	Function	Signature
Calibrated by:	Nico Verbeek	Technician	
Approved by:	Katja Pokornic	Laboratory Director	

Date issued: April 28, 2004

This calibration certificate is issued as an intermediate solution until the accreditation process (based on ISO/IEC 17025 International Standard) for Calibration Laboratory of Schmid & Partner Engineering AG is completed.

Probe ET3DV6

SN:1607

Manufactured:	July 27, 2001
Last calibrated:	August 7, 2001
Recalibrated:	April 28, 2004

Calibrated for DASY Systems

(Note: non-compatible with DASY2 system!)

ET3DV6 SN:1607

April 28, 2004

DASY - Parameters of Probe: ET3DV6 SN:1607**Sensitivity in Free Space****Diode Compression^A**

NormX	$1.74 \mu\text{V}/(\text{V}/\text{m})^2$
NormY	$1.80 \mu\text{V}/(\text{V}/\text{m})^2$
NormZ	$1.74 \mu\text{V}/(\text{V}/\text{m})^2$

DCP X	90	mV
DCP Y	90	mV
DCP Z	90	mV

Sensitivity in Tissue Simulating Liquid (Conversion Factors)

Please see Page 7.

Boundary Effect**Head** **900 MHz** **Typical SAR gradient: 5 % per mm**

Sensor Center to Phantom Surface Distance		3.7 mm	4.7 mm
SAR _{oe} [%]	Without Correction Algorithm	8.8	4.4
SAR _{oe} [%]	With Correction Algorithm	0.0	0.1

Head **1800 MHz** **Typical SAR gradient: 10 % per mm**

Sensor Center to Phantom Surface Distance		3.7 mm	4.7 mm
SAR _{oe} [%]	Without Correction Algorithm	14.5	9.8
SAR _{oe} [%]	With Correction Algorithm	0.2	0.2

Sensor Offset

Probe Tip to Sensor Center	2.7 mm
Optical Surface Detection	in tolerance

The reported uncertainty of measurement is stated as the standard uncertainty of measurement multiplied by the coverage factor $k=2$, which for a normal distribution corresponds to a coverage probability of approximately 95%.


^A numerical linearization parameter: uncertainty not required

ET3DV6 SN:1607

April 28, 2004

Frequency Response of E-Field


(TEM-Cell:ifi110, Waveguide R22)

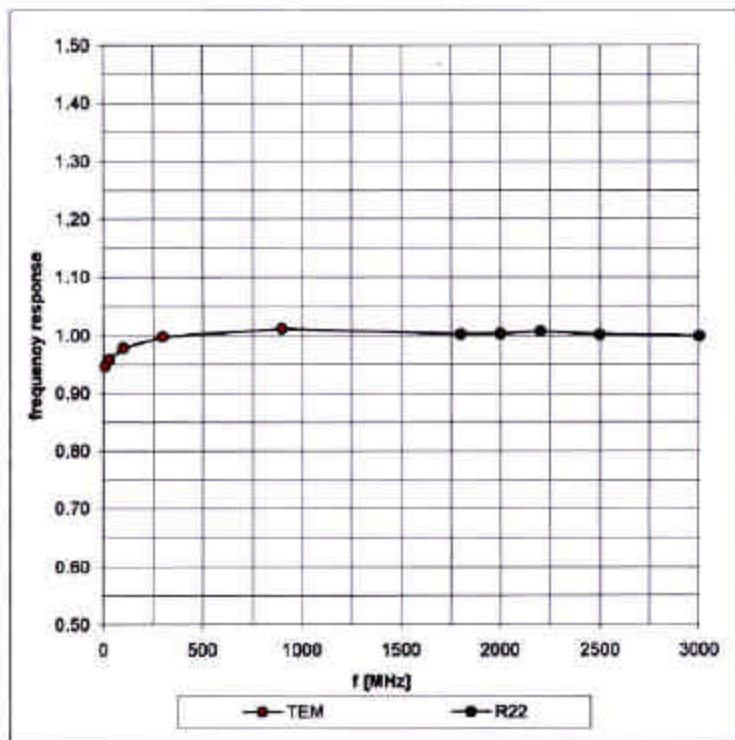

ET3DV6 SN:1607

April 28, 2004

Receiving Pattern (ϕ) , $\theta = 0^\circ$

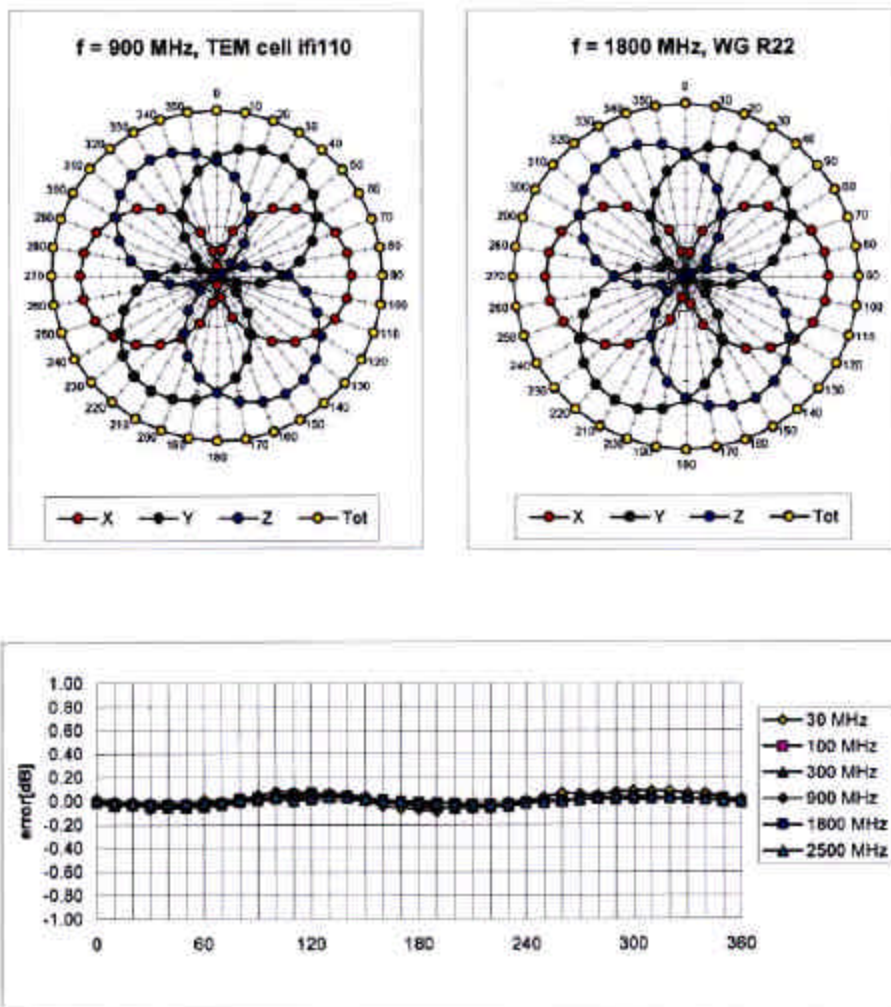


Axial Isotropy Error $< \pm 0.2 \text{ dB}$

ET3DV6 SN:1607

April 28, 2004


Dynamic Range f(SAR_{head}) (Waveguide R22)

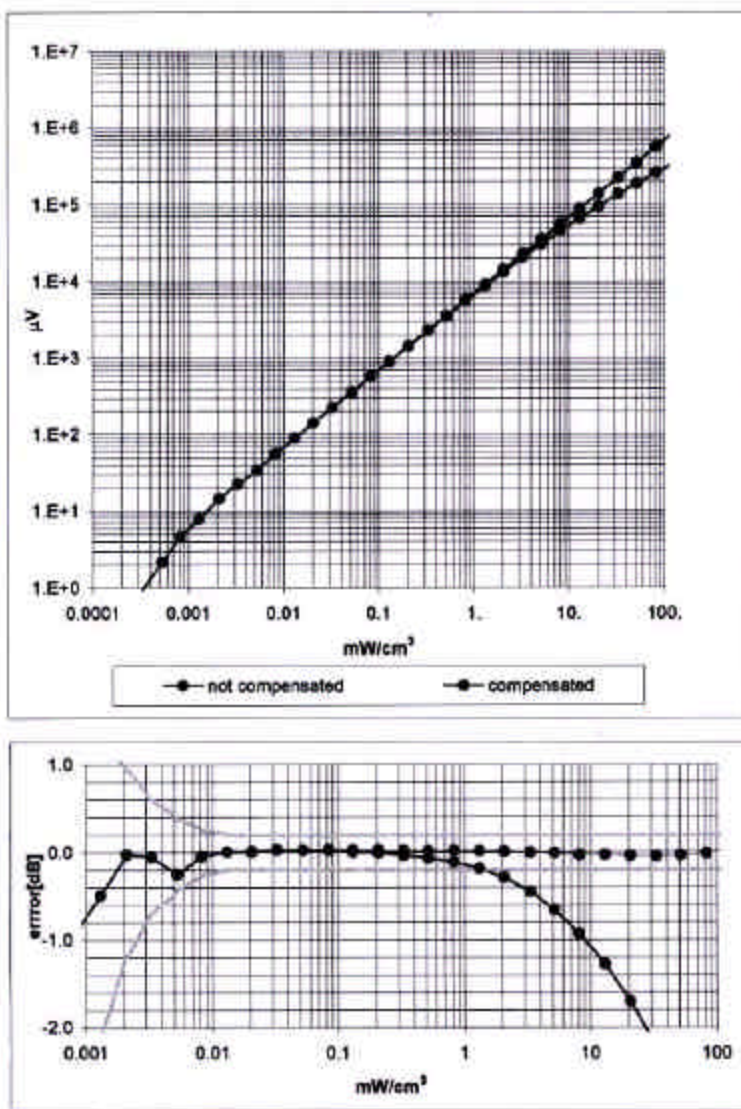
Probe Linearity < ± 0.2 dB

ET3DV6 SN:1607

April 28, 2004

Conversion Factor Assessment

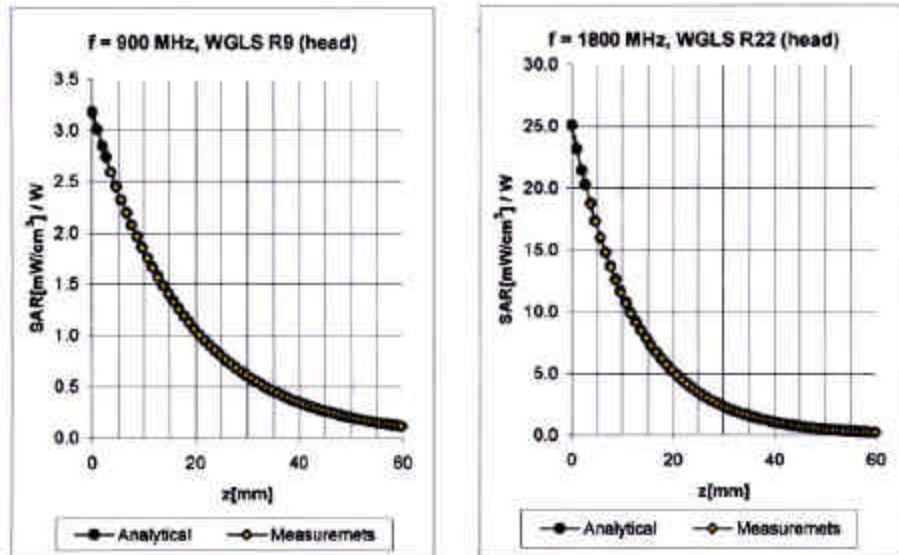

f [MHz]	Validity [MHz] ^a	Tissue	Permittivity	Conductivity	Alpha	Depth	ConvF Uncertainty
900	800-1000	Head	41.5 ± 5%	0.97 ± 5%	0.81	1.80	6.22 ± 11.3% (k=2)
1800	1710-1910	Head	40.0 ± 5%	1.40 ± 5%	0.53	2.80	5.10 ± 11.7% (k=2)
835	750-950	Body	55.2 ± 5%	0.97 ± 5%	0.62	1.90	8.26 ± 11.9% (k=2)
1900	1800-2000	Body	53.3 ± 5%	1.52 ± 5%	0.63	2.87	4.54 ± 11.3% (k=2)

^a The total standard uncertainty is calculated as root-sum-square of standard uncertainty of the Conversion Factor at calibration frequency and the standard uncertainty for the indicated frequency band.

Schmid & Partner Engineering AG

s p e a g

Zeughausstrasse 43, 8004 Zurich, Switzerland
Phone +41 1 245 9700, Fax +41 1 245 9779
info@speag.com, <http://www.speag.com>

Additional Conversion Factors

for Dosimetric E-Field Probe

Type:

ET3DV6

Serial Number:

1607

Place of Assessment:

Zurich

Date of Assessment:

May 1, 2004

Probe Calibration Date:

April 28, 2004

Schmid & Partner Engineering AG hereby certifies that conversion factor(s) of this probe have been evaluated on the date indicated above. The assessment was performed using the FDTD numerical code SEMCAD of Schmid & Partner Engineering AG. Since the evaluation is coupled with measured conversion factors, it has to be recalculated yearly, i.e., following the re-calibration schedule of the probe. The uncertainty of the numerical assessment is based on the extrapolation from measured value at 900 MHz or at 1800 MHz.

Assessed by:



ET3DV6-SN:1607

Page 1 of 2

May 1, 2004

Schmid & Partner Engineering AG

s p e a g

Zeughausstrasse 43, 8004 Zurich, Switzerland
Phone +41 1 245 9700, Fax +41 1 245 9779
info@speag.com, <http://www.speag.com>

Dosimetric E-Field Probe ET3DV6 SN:1607Conversion factor ($\pm$ standard deviation)450 MHz ConvF $7.3 \pm 8\%$ $\epsilon_r = 43.5 \pm 5\%$ $\sigma = 0.87 \pm 5\% \text{ mho/m}$

(head tissue)

450 MHz ConvF $7.1 \pm 8\%$ $\epsilon_r = 56.7 \pm 5\%$ $\sigma = 0.94 \pm 5\% \text{ mho/m}$

(body tissue)

Important Note:


For numerically assessed probe conversion factors, parameters Alpha and Delta in the DASY software must have the following entries: Alpha = 0 and Delta = 1.

Please see also Section 4.7 of the DASY4 Manual.

ET3DV6 SN:1607

April 28, 2004

Deviation from Isotropy in HSL

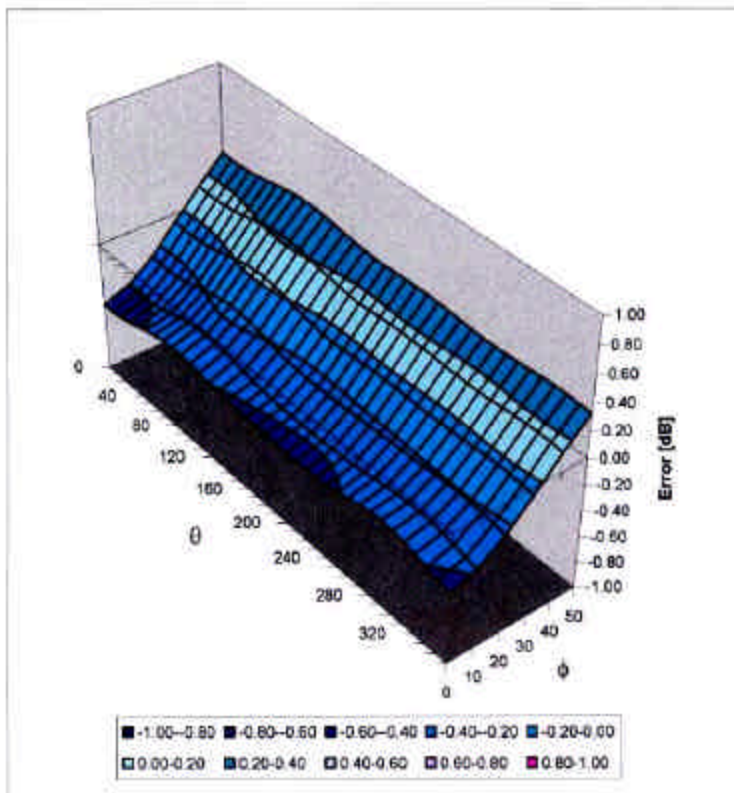Error (θ, ϕ), $f = 900$ MHz

Spherical Isotropy Error $< \pm 0.4$ dB