

SAR TEST REPORT

| | |
|----------------------|--|
| Equipment Under Test | : WLAN VoIP Phone |
| Model No. | : WPU-7800G |
| Applicant | : UniData Communication Systems, Inc. |
| Address of Applicant | : Bulim-Bldg, 837-6, Bangbae 4-dong, Seocho-gu, Seoul, Korea |
| FCC ID | : SQMWPU-7800G |
| Device Category | : Portable Device |
| Exposure Category | : General Population/Uncontrolled Exposure |
| Date of Receipt | : 2010-09-27 |
| Date of Test(s) | : 2010-10-14 ~ 2010-10-15 |
| Date of Issue | : 2010-10-25 |
| Max. SAR | : 0.127 W/kg (WLAN) |

Standards:

**FCC OET Bulletin 65 supplement C
IEEE 1528, 2003
ANSI/IEEE C95.1, C95.3**

In the configuration tested, the EUT complied with the standards specified above.

Remarks:

This report details the results of the testing carried out on one sample, the results contained in this test report do not relate to other samples of the same product. The manufacturer should ensure that all products in series production are in conformity with the product sample detailed in this report. This report may only be reproduced and distributed in full. If the product in this report is used in any configuration other than that detailed in the report, the manufacturer must ensure the new system complies with all relevant standards. Any mention of SGS Testing Korea Co., Ltd. or testing done by SGS Testing Korea Co., Ltd. in connection with distribution or use of the product described in this report must be approved by SGS Testing Korea Co., Ltd. in writing.

| | | | |
|-------------|---------------|---|------------|
| Tested by | : Fred Jeong |  | 2010-10-25 |
| Approved by | : Charles Kim |  | 2010-10-25 |

Contents

1. General Information

| | | |
|-----------|---|-----------|
| 1.1 | Testing Laboratory..... | 3 |
| 1.2 | Details of Applicant..... | 3 |
| 1.3 | Version of Report..... | 3 |
| 1.4 | Description of EUT(s)..... | 3 |
| 1.5 | Test Environment..... | 4 |
| 1.6 | Operation description..... | 4 |
| 1.7 | Evaluation procedures..... | 5 |
| 1.8 | The SAR Measurement System..... | 6 |
| 1.9 | System Components..... | 8 |
| 1.10 | SAR System Verification..... | 9 |
| 1.11 | Tissue Simulant Fluid for the Frequency Band..... | 11 |
| 1.12 | Test Standards and Limits..... | 12 |
| 2. | Instruments List..... | 14 |
| 3. | Summary of Results..... | 15 |

APPENDIX

- A. DASY4 SAR Report**
- B. Uncertainty Analysis**
- C. Calibration certificate**

1. General Information

1.1 Testing Laboratory

SGS Testing Korea Co., Ltd.
Wireless Div. 2FL, 18-34, Sanbon-dong, Gunpo-si, Gyeonggi-do, Korea 435-040
Telephone : +82 +31 428 5700
FAX : +82 +31 427 2371
Homepage : www.kr.sgs.com/ee

1.2 Details of Manufacturer

| | |
|----------------|--|
| Manufacturer | : UniData Communication Systems, Inc. |
| Address | : Bulim-Bldg, 837-6, Bangbae 4-dong, Seocho-gu, Seoul, Korea |
| Contact Person | : Jong Myung Kim |
| Phone No. | : 82-70-7544-3356 |

1.3 Version of Report

| Version Number | Date | Revision |
|----------------|------------|---------------|
| 00 | 2010-10-21 | Initial issue |
| 01 | 2010-10-25 | Revision 01 |

1.4 Description of EUT(s)

| | |
|----------------------------|------------------------------------|
| EUT Type | : WLAN VoIP Phone |
| Model | : WPU-7800G |
| Serial Number | : N/A |
| Mode of Operation | : WLAN |
| Duty Cycle | : 1(WLAN) |
| Body worn Accessory | : None |
| Tx Frequency Range | : 2412 MHz ~ 2462 MHz (WLAN) |
| Conducted Max Power | : 17.57 dBm(11b), 15.78 dBm(11g) |
| Battery Type | : 3.7 V d.c. (Lithium-ion Battery) |

1.5 Test Environment

| | |
|--------------------------|-----------------------|
| Ambient temperature | : (22 \pm 2) °C |
| Tissue Simulating Liquid | : (22 \pm 2) °C |
| Relative Humidity | : (55 \pm 5) % R.H. |

1.6 Operation Configuration

The client provided a special driver and test program which can control the frequency and power of the WLAN module. Measurements were performed at the lowest, middle and highest channels of the operating band. The EUT was set to maximum power level during all tests and at the beginning of each test the battery was fully charged.

The DASY4 system measures power drift during SAR testing by comparing e-field in the same location at the beginning and at the end of measurement.

1.7 EVALUATION PROCEDURES

- Power Reference Measurement Procedures

The Power Reference Measurement and Power Drift Measurements are for monitoring the power drift of the device under test in the batch process. The Minimum distance of probe sensors to surface determines the closest measurement point to phantom surface. The minimum distance of probe sensors to surface is 4 mm. This distance cannot be smaller than the Distance of sensor calibration points to probe tip as defined in the probe properties (for example, 2.7 mm for an ET3DV6 probe type).

- The entire evaluation of the spatial peak values is performed within the Post-processing engine (SEMCAD). The system always gives the maximum values for the 1 g and 10 g cubes. The algorithm to find the cube with highest averaged SAR is divided into the following stages:

1. The extraction of the measured data (grid and values) from the Zoom Scan.
2. The calculation of the SAR value at every measurement point based on all stored data (A/D values and measurement parameters)
3. The generation of a high-resolution mesh within the measured volume
4. The interpolation of all measured values from the measurement grid to the high-resolution grid
5. The extrapolation of the entire 3-D field distribution to the phantom surface over the distance from sensor to surface
6. The calculation of the averaged SAR within masses of 1 g and 10 g.

The probe is calibrated at the center of the dipole sensors that is located 1 mm to 2.7 mm away from the probe tip. During measurements, the probe stops shortly above the phantom surface, depending on the probe and the surface detecting system. Both distances are included as parameters in the probe configuration file. The software always knows exactly how far away the measured point is from the surface. As the probe cannot directly measure at the surface, the values between the deepest measured point and the surface must be extrapolated. The angle between the probe axis and the surface normal line is less than 30 degree.

In the Area Scan, the gradient of the interpolation function is evaluated to find all the extreme of the SAR distribution. The uncertainty on the locations of the extreme is less than 1/20 of the grid size. Only local maximum within -2 dB of the global maximum are searched and passed for the Cube Scan measurement. In the Cube Scan, the interpolation function is used to extrapolate the Peak SAR from the lowest measurement points to the inner phantom surface (the extrapolation distance). The uncertainty increases with the extrapolation distance. To keep the uncertainty within 1 % for the 1 g and 10 g cubes, the extrapolation distance should not be larger than 5 mm.

The maximum search is automatically performed after each area scan measurement. It is based on splines in two or three dimensions. The procedure can find the maximum for most SAR distributions even with

relatively large grid spacing. After the area scanning measurement, the probe is automatically moved to a position at the interpolated maximum. The following scan can directly use this position for reference, e.g., for a finer resolution grid or the cube evaluations. The 1 g and 10 g peak evaluations are only available for the predefined cube 7x7x7 scans. The routines are verified and optimized for the grid dimensions used in these cube measurements. The measured volume of 30x30x30mm contains about 30 g of tissue. The first procedure is an extrapolation (incl. Boundary correction) to get the points between the lowest measured plane and the surface. The next step uses 3D interpolation to get all points within the measured volume. In the last step, a 1 g cube is placed numerically into the volume and its averaged SAR is calculated. This cube is moved around until the highest averaged SAR is found. If the highest SAR is found at the edge of the measured volume, the system will issue a warning: higher SAR values might be found outside of the measured volume. In that case the cube measurement can be repeated, using the new interpolated maximum as the center.

1.8 The SAR Measurement System

A photograph of the SAR measurement System is given in Fig. a. This SAR Measurement System uses a Computer-controlled 3-D stepper motor system (Speag Dasy 4 professional system). A Model ET3DV6 1782 E-field probe is used to determine the internal electric fields. The SAR can be obtained from the equation $SAR = \sigma (|E|^2) / \rho$ where σ and ρ are the conductivity and mass density of the tissue-simulant. The DASY4 system for performing compliance tests consists of the following items:

- A standard high precision 6-axis robot (Staubli RX family) with controller, teach pendant and software. An arm extension for accommodating the data acquisition electronics (DAE).
- A dosimeter probe, i.e., an isotropic E-field probe optimized and calibrated for usage in tissue simulating liquid. The probe is equipped with an optical surface detector system.
- A data acquisition electronics (DAE) which performs the signal amplification, signal multiplexing, AD-conversion, offset measurements, mechanical surface detection, collision detection, etc. The unit is battery powered with standard or rechargeable batteries. The signal is optically transmitted to the EOC.

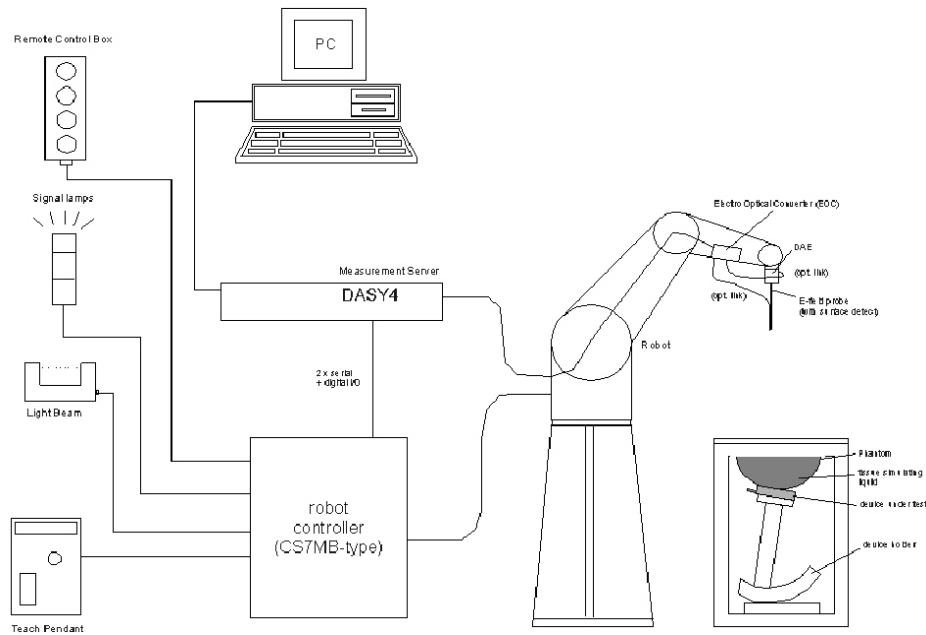


Fig a. The microwave circuit arrangement used for SAR system verification

- The Electro-optical converter (EOC) performs the conversion between optical and electrical of the signals for the digital communication to the DAE and for the analog signal from the optical surface detection. The EOC is connected to the measurement server.
- The function of the measurement server is to perform the time critical tasks such as signal filtering, control of the robot operation and fast movement interrupts.
- A probe alignment unit which improves the (absolute) accuracy of the probe positioning.
- A computer operating Windows 2000 or Windows XP.
- DASY4 software.
- Remote control with teach pendant and additional circuitry for robot safety such as warning lamps, etc.
- The SAM twin phantom enabling testing body usage.
- The device holder for flat phantom.
- Tissue simulating liquid mixed according to the given recipes.
- Validation dipole kits allowing to validate the proper functioning of the system.

1.9 System Components

ET3DV6 E-Field Probe

| | |
|----------------------|---|
| Construction | : Symmetrical design with triangular core Built-in shielding against static charges PEEK enclosure material (resistant to organic solvents, e.g. glycol). |
| Calibration | : In air from 10 MHz to 2.5 GHz In brain simulating tissue (accuracy $\pm 8\%$) |
| Frequency | : 10 MHz to >6 GHz; Linearity: ± 0.2 dB (30 MHz to 3 GHz) |
| Directivity | : ± 0.2 dB in brain tissue (rotation around probe axis) ± 0.4 dB in brain tissue (rotation normal to probe axis) |
| Dynamic Range | : 5 μ W/g to >100 mW/g; Linearity: ± 0.2 dB |
| Srfce. Detect | : ± 0.2 mm repeatability in air and clear liquids over diffuse reflecting surfaces |
| Dimensions | : Overall length: 330 mm Tip length: 16 mm Body diameter: 12 mm Tip diameter: 6.8 mm Distance from probe tip to dipole centers: 2.7 mm |
| Application | : General dosimetry up to 3 GHz Compliance tests of mobile phone |



ET3DV6 E-Field Probe

NOTE:

1. The Probe parameters have been calibrated by the SPEAG. Please reference "APPENDIX D" for the Calibration Certification Report.

SAM Phantom

Construction:

The SAM Phantom is constructed of a fiberglass shell integrated in a wooden table. The shape of the shell is based on data from an anatomical study designed to determine the maximum exposure in at least 90 % of all users. It enables the dosimetric evaluation of left and right hand phone usage as well as body mounted usage at the flat phantom region. A cover prevents the evaporation of the liquid. Reference markings on the Phantom allow the complete setup of all predefined phantom positions and measurement grids by manually teaching three points in the robot

Shell Thickness:

2.0 mm \pm 0.1 mm

Filling Volume:

Approx. 25 liters



SAM Phantom

DEVICE HOLDER

Construction

In combination with the Twin SAM PhantomV4.0/V4.0C or Twin SAM, the Mounting Device (made from POM) enables the rotation of the mounted transmitter in spherical coordinates, whereby the rotation point is the ear opening. The devices can be easily and accurately positioned according to IEC, IEEE, CENELEC, FCC or other specifications. The device holder can be locked at different phantom locations (left head, right head, flat phantom).



Device Holder

1.10 SAR System Verification

The microwave circuit arrangement for system verification is sketched in Fig. b. The daily system accuracy verification occurs within the flat section of the SAM phantom. A SAR measurement was performed to see if the measured SAR was within \pm 10 % from the target SAR value. This test was done at 2450 MHz. The test for EUT was conducted within 24 hours after validation. The obtained result from the system accuracy verification is displayed in the table 1. During the test, the ambient temperature of the laboratory was in the range (22 \pm 2) ° C, the relative humidity was in the range (55 \pm 5) % R.H. and the liquid depth above the ear reference points was above 15 cm in all the cases. It is seen that the system is operating within its specification, as the result is within acceptable tolerance of the reference value.

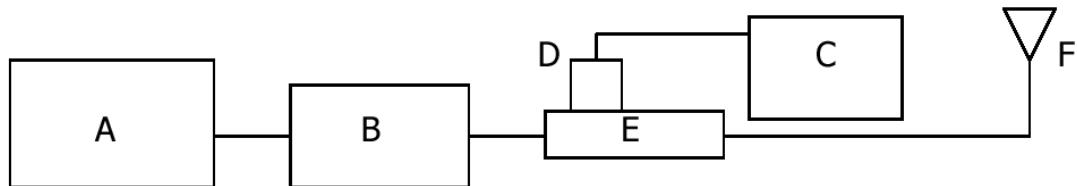


Fig b. The microwave circuit arrangement used for SAR system verification

- A. Agilent Model E4421B Signal Generator
- B. EMPOWER Model 2057-BBS3Q5KCK Amplifier
- C. Agilent Model E4419B Power Meter
- D. Agilent Model 9300H Power Sensor
- E. Agilent Model 777D/778D Dual directional coupling
- F. Reference dipole Antenna



Photo of the dipole Antenna

System Validation Results

| Validation Kit | Tissue | Target SAR 1 g from Calibration Certificate (Input Power : 250 mW) | Measured SAR 1 g (Input Power : 250 mW) | Deviation (%) | Date | Liquid Temp. (°C) |
|---------------------|-------------------|---|--|---------------|------------|-------------------|
| D2450V2 S/N: 734 | 2450 MHz Brain | 12.8 W/kg | 12.9 W/kg | 0.78 | 2010-10-14 | 22.3 |
| D2450V2 S/N: 734 | 2450 MHz Body | 13.4 W/kg | 13.7 W/kg | 2.24 | 2010-10-15 | 22.4 |

Table 1. Results system validation

1.11 Tissue Simulant Fluid for the Frequency Band

The dielectric properties for this simulant fluid were measured by using the Agilent Model 85070D Dielectric Probe (rates frequency band 200 MHz to 20 GHz) in conjunction with Agilent E5070B Network Analyzer(300 KHz - 3 GHz) by using a procedure detailed in Section V.

| f (MHz) | Tissue type | Limits / Measured | Dielectric Parameters | | |
|---------|-------------|-----------------------|-----------------------|--------------|--------------------------|
| | | | Permittivity | Conductivity | Simulated Tissue Temp() |
| 2450 | Head | Measured, 2010-010-14 | 38.2 | 1.84 | 22.3 |
| | | Recommended Limits | 39.2 | 1.80 | 21.0 ~ 23.0 |
| | | Deviation(%) | -2.55 | 2.22 | - |
| | Body | Measured, 2010-10-15 | 50.2 | 1.98 | 22.4 |
| | | Recommended Limits | 52.7 | 1.95 | 21.0 ~ 23.0 |
| | | Deviation(%) | -4.74 | 1.54 | - |

The composition of the brain tissue simulating liquid

The following tissue formulations are provided for reference only as some of the parameters have not been thoroughly verified. The composition of ingredients may be modified accordingly to achieve the desired target tissue parameters required for routine SAR evaluation.

| Ingredients (% by weight) | Frequency (MHz) | | | | | | | | | |
|------------------------------|-----------------|-------|-------|------|-------|-------|-------|------|------|------|
| | 450 | | 835 | | 915 | | 1900 | | 2450 | |
| Tissue Type | Head | Body | Head | Body | Head | Body | Head | Body | Head | Body |
| Water | 38.56 | 51.16 | 41.45 | 52.4 | 41.05 | 56.0 | 54.9 | 40.4 | 62.7 | 73.2 |
| Salt (NaCl) | 3.95 | 1.49 | 1.45 | 1.4 | 1.35 | 0.76 | 0.18 | 0.5 | 0.5 | 0.04 |
| Sugar | 56.32 | 46.78 | 56.0 | 45.0 | 56.5 | 41.76 | 0.0 | 58.0 | 0.0 | 0.0 |
| HEC | 0.98 | 0.52 | 1.0 | 1.0 | 1.0 | 1.21 | 0.0 | 1.0 | 0.0 | 0.0 |
| Bactericide | 0.19 | 0.05 | 0.1 | 0.1 | 0.1 | 0.27 | 0.0 | 0.1 | 0.0 | 0.0 |
| Triton X-100 | 0.0 | 0.0 | 0.0 | 0.0 | 0.0 | 0.0 | 0.0 | 0.0 | 36.8 | 0.0 |
| DGBE | 0.0 | 0.0 | 0.0 | 0.0 | 0.0 | 0.0 | 44.92 | 0.0 | 0.0 | 26.7 |
| Dielectric Constant | 43.42 | 58.0 | 42.54 | 56.1 | 42.0 | 56.8 | 39.9 | 54.0 | 39.8 | 52.5 |
| Conductivity (S/m) | 0.85 | 0.83 | 0.91 | 0.95 | 1.0 | 1.07 | 1.42 | 1.45 | 1.88 | 1.78 |

Salt: 99 ⁺% Pure Sodium Chloride

Sugar: 98 ⁺% Pure Sucrose

Water: De-ionized, 16 MΩ⁺ resistivity

HEC: Hydroxyethyl Cellulose

DGBE: 99 ⁺% Di(ethylene glycol) butyl ether, [2-(2-butoxyethoxy)ethanol]

Triton X-100 (ultra pure): Polyethylene glycol mono [4-(1,1,3,3-tetramethylbutyl)phenyl]ether

1.12 Test Standards and Limits

According to FCC 47CFR §2.1093(d) The limits to be used for evaluation are based generally on criteria published by the American National Standards Institute (ANSI) for localized specific absorption rate (“SAR”) in Section 4.2 of “IEEE Standard for Safety Levels with Respect to Human Exposure to Radio Frequency Electromagnetic Fields, 3 kHz to 300 GHz,” ANSI/IEEE C95.3–2003, Copyright 2003 by the Institute of Electrical and Electronics Engineers, Inc., New York, New York 10017. These criteria for SAR evaluation are similar to those recommended by the National Council on Radiation Protection and Measurements (NCRP) in “Biological Effects and Exposure Criteria for Radio frequency Electromagnetic Fields,” NCRP Report No. 86, Section 17.4.5. Copyright NCRP, 1986, Bethesda, Maryland 20814. SAR is a measure of the rate of energy absorption due to exposure to an RF transmitting source. SAR values have been related to threshold levels for potential biological hazards. The criteria to be used are specified in paragraphs (d)(1) and (d)(2) of this section and shall apply for portable devices transmitting in the

frequency range from 100 kHz to 6 GHz. Portable devices that transmit at frequencies above 6 GHz are to be evaluated in terms of the MPE limits specified in § 1.1310 of this chapter. Measurements and calculations to demonstrate compliance with MPE field strength or power density limits for devices operating above 6 GHz should be made at a minimum distance of 5 cm from the radiating source.

(1) Limits for Occupational/Controlled exposure: 0.4 W/kg as averaged over the whole-body and spatial peak SAR not exceeding 8 W/kg as averaged over any 1 gram of tissue (defined as a tissue volume in the shape of a cube). Exceptions are the hands, wrists, feet and ankles where the spatial peak SAR shall not exceed 20 W/kg, as averaged over an 10 grams of tissue (defined as a tissue volume in the shape of a cube). Occupational/Controlled limits apply when persons are exposed as a consequence of their employment provided these persons are fully aware of and exercise control over their exposure. Awareness of exposure can be accomplished by use of warning labels or by specific training or education through appropriate means, such as an RF safety program in a work environment.

(2) Limits for General Population/Uncontrolled exposure: 0.08 W/kg as averaged over the whole-body and spatial peak SAR not exceeding 1.6 W/kg as averaged over any 1 gram of tissue (defined as a tissue volume in the shape of a cube). Exceptions are the hands, wrists, feet and ankles where the spatial peak SAR shall not exceed 4 W/kg, as averaged over any 10 grams of tissue (defined as a tissue volume in the shape of a cube). General Population/Uncontrolled limits apply when the general public may be exposed, or when persons that are exposed as a consequence of their employment may not be fully aware of the potential for exposure or do not exercise control over their exposure. Warning labels placed on consumer devices such as cellular telephones will not be sufficient reason to allow these devices to be evaluated subject to limits for occupational/controlled exposure in paragraph (d)(1) of this section.(Table .4)

| Human Exposure | Uncontrolled Environment General Population | Controlled Environment Occupational |
|--|--|--|
| Partial Peak SAR (Partial) | 1.60 m W/g | 8.00 m W/g |
| Partial Average SAR (Whole Body) | 0.08 m W/g | 0.40 m W/g |
| Partial Peak SAR (Hands/Feet/Ankle/Wrist) | 4.00 m W/g | 20.00 m W/g |

Table .4 RF exposure limits

2. Instruments List

| Manufacturer | Device | Type | Serial Number | Due date of Calibration |
|--------------------------------|-----------------------------------|------------------|--------------------|-------------------------|
| Stäubli | Robot | RX90BL | F03/5W05A1/A/01 | N/A |
| Schmid& Partner Engineering AG | Dosimetric E-Field Probe | ET3DV6 | 1782 | April 28, 2011 |
| Schmid& Partner Engineering AG | 2450 MHz System Validation Dipole | D2450V2 | 734 | May 27, 2012 |
| Schmid& Partner Engineering AG | Data acquisition Electronics | DAE3 | 567 | December 09, 2010 |
| Schmid& Partner Engineering AG | Software | DASY 4 V4.7 | - | N/A |
| Schmid& Partner Engineering AG | Phantom | SAM Phantom V4.0 | TP-1299 TP-1300 | N/A |
| Agilent | Network Analyzer | E5070B | MY42100282 | March 31, 2011 |
| Agilent | Dielectric Probe Kit | 85070D | 2184 | N/A |
| Agilent | Power Meter | E4419B | GB43311126 | September 28, 2011 |
| Agilent | Power Sensor | E9300H | MY41495307 | October 01, 2011 |
| | | | MY41495308 | October 01, 2011 |
| Agilent | Signal Generator | E4421B | MY43350132 | September 28, 2011 |
| Empower RF Systems | Power Amplifier | 2001-BBS3Q7ECK | 1032 D/C 0336 | March 30, 2011 |
| Agilent | Dual Directional Coupler | 777D 778D | 50128 50454 | September 28, 2011 |
| Microlab | LP Filter | LA-15N LA-30N | N/A | October 01, 2011 |

3. Summary of Results

A. Conducted Power

1. Conducted Power Table.

- WLAN

| Mode (Data Rate) | Average Power(dBm) | | |
|------------------|--------------------|-------|-------|
| | Low | Mid | High |
| 11b (1 Mbps) | 17.17 | 17.45 | 17.57 |
| 11g (6 Mbps) | 15.64 | 15.78 | 15.72 |

** The data rate was set same as RF report.

2. Worst-case result was reported.

3. The EUT Position is based on normal operating condition.

B. SAR Evaluation Consideration

KDB 447498 -SAR evaluation

- output $60/f(\text{GHz})$: SAR not required
- output $> 60/f(\text{GHz})$: Stand-alone SAR required

| Frequency | P (dBm) | P (mW) | Stand-alone SAR |
|-----------|---------|--------|-----------------|
| 2462 MHz | 17.57 | 57.15 | Yes |

KDB 248227 <SAR Measurement Procedures for 802.11 a/b/g Transmitters>

- 802.11 b/g modes are tested on channels 1, 6 and 11. These channels are “default test channels”.

WLAN Head SAR

| | |
|--------------------------|------------|
| Ambient Temperature (°C) | 22.3 |
| Liquid Temperature (°C) | 22.3 |
| Date | 2010-10-14 |

| Head | Test Mode | EUT Position | Traffic Channel | | Power Drift(dB) | 1 g SAR (W/kg) | 1 g SAR Limits (W/kg) |
|-----------|-----------|--------------|-----------------|---------|-----------------|----------------|-----------------------|
| | | | Frequency (MHz) | Channel | | | |
| Left Ear | 11b | Cheek | 2437 | 6 | 0.006 | 0.055 | 1.6 |
| | 11b | Tilt | 2437 | 6 | 0.009 | 0.044 | |
| Right Ear | 11b | Cheek | 2437 | 6 | 0.122 | 0.078 | 1.6 |
| | 11b | Tilt | 2437 | 6 | -0.130 | 0.055 | |
| | 11g | Cheek | 2437 | 6 | 0.019 | 0.051 | |
| | 11b | Cheek | 2412 | 1 | -0.115 | 0.063 | |
| | 11b | Cheek | 2462 | 11 | -0.011 | 0.092 | |

<Note>

1. The test data reported are the worst-case SAR value with the position set in a typical configuration.
2. All modes of operation were investigated, and worst-case results are reported.
3. Battery is fully charged for all readings and the standard batteries are the only options.
4. Justification for reduced test configuration : Per FCC/OET Bulletin 65 Supplement C [July 2001], if the SAR measured at the middle channel for each test configuration (left, right, cheek, tilt) is at least 3.0 dB lower than the SAR limit, testing at the high and low channel is optional for such test configurations.
5. The default channels are 1, 6 and 11, so those channels were tested at worst position.

WLAN Body SAR

| | |
|--------------------------|------------|
| Ambient Temperature (°C) | 22.4 |
| Liquid Temperature (°C) | 22.4 |
| Date | 2010-10-15 |

| Body | Test Mode | EUT Position | Traffic Channel | | Power Drift(dB) | 1 g SAR (W/kg) | 1 g SAR Limits (W/kg) |
|-------------------|-----------|--------------|-----------------|---------|-----------------|----------------|-----------------------|
| | | | Frequency (MHz) | Channel | | | |
| Body | 11b | Front | 2437 | 6 | -0.176 | 0.021 | 1.6 |
| | 11b | Back | 2437 | 6 | -0.187 | 0.093 | |
| Body with Ear Set | 11b | Back | 2437 | 6 | 0.058 | 0.101 | |
| | 11g | Back | 2437 | 6 | -0.189 | 0.068 | |
| | 11b | Back | 2412 | 1 | 0.054 | 0.107 | |
| | 11b | Back | 2462 | 11 | -0.106 | 0.127 | |

<Note>

1. The test data reported are the worst-case SAR value with the position set in a typical configuration.
2. All modes of operation were investigated, and worst-case results are reported.
3. Battery is fully charged for all readings and the standard batteries are the only options.
4. Justification for reduced test configuration : Per FCC/OET Bulletin 65 Supplement C [July 2001], if the SAR measured at the middle channel for each test configuration (left, right, cheek, tilt) is at least 3.0 dB lower than the SAR limit, testing at the high and low channel is optional for such test configurations.
5. The distance from EUT to flat phantom for testing Body SAR is 15 mm.
(Please refer to the conduction power table Page 15)
6. The default channels are 1, 6 and 11, so those channels were tested at worst position.

Appendix

List

| | | |
|------------|---|---|
| Appendix A | DASY4 Report (Plots of the SAR Measurements) | - 2450 MHz Validation Test - WLAN Test |
| Appendix B | Uncertainty Analysis | |
| Appendix C | Calibration Certificate | - PROBE - DAE - DIPOLE |

Appendix A

Test Plot - DASY4 Report

2450 MHz Validation Test_Head

Date/Time: 2010-10-14 10:25:18

Test Laboratory: SGS Testing Korea
File Name: [Validation 2450_Head.dat](#)

DUT: Dipole 2450 MHz; Type: D2450V2; Serial: D2450V2 - SN:734
Program Name: Validation 2450 MHz_Head


Communication System: CW; Frequency: 2450 MHz; Duty Cycle: 1:1
Medium parameters used: $f = 2450$ MHz; $\sigma = 1.84$ mho/m; $\epsilon_r = 38.2$; $\rho = 1000$ kg/m³
Phantom section: Flat Section

DASY4 Configuration:


- Probe: ET3DV6 - SN1782; ConvF(4.48, 4.48, 4.48); Calibrated: 2010-04-28
- Sensor-Surface: 4mm (Mechanical Surface Detection)
- Electronics: DAE3 Sn567; Calibrated: 2009-12-09
- Phantom: SAM MIC #2000-93 with CRP; Type: SAM MIC #2000-93; Serial: TP-1299
- Measurement SW: DASY4, V4.7 Build 80; Postprocessing SW: SEMCAD, V1.8 Build 186

Validation 2450 MHz_Head/Area Scan (61x61x1): Measurement grid: dx=15mm, dy=15mm
Maximum value of SAR (interpolated) = 16.3 mW/g

Validation 2450 MHz_Head/Zoom Scan (7x7x7)/Cube 0: Measurement grid: dx=5mm, dy=5mm, dz=5mm
Reference Value = 86.4 V/m; Power Drift = -0.055 dB
Peak SAR (extrapolated) = 29.0 W/kg
SAR(1 g) = 12.9 mW/g; SAR(10 g) = 5.8 mW/g
Maximum value of SAR (measured) = 14.7 mW/g

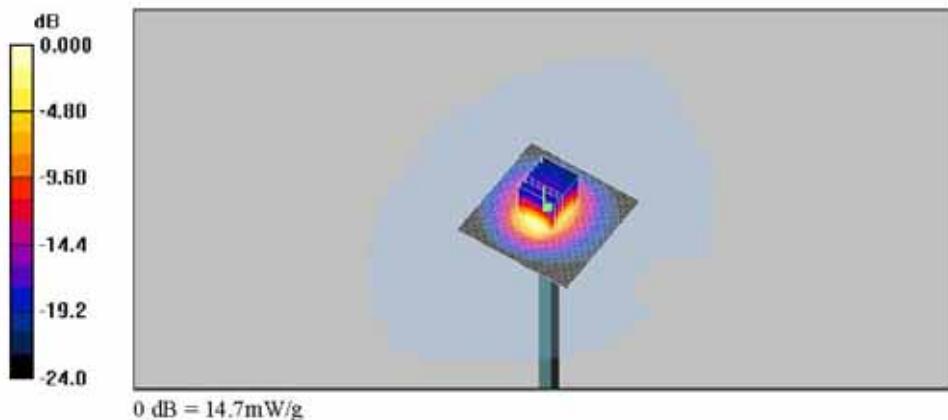

Z Scan

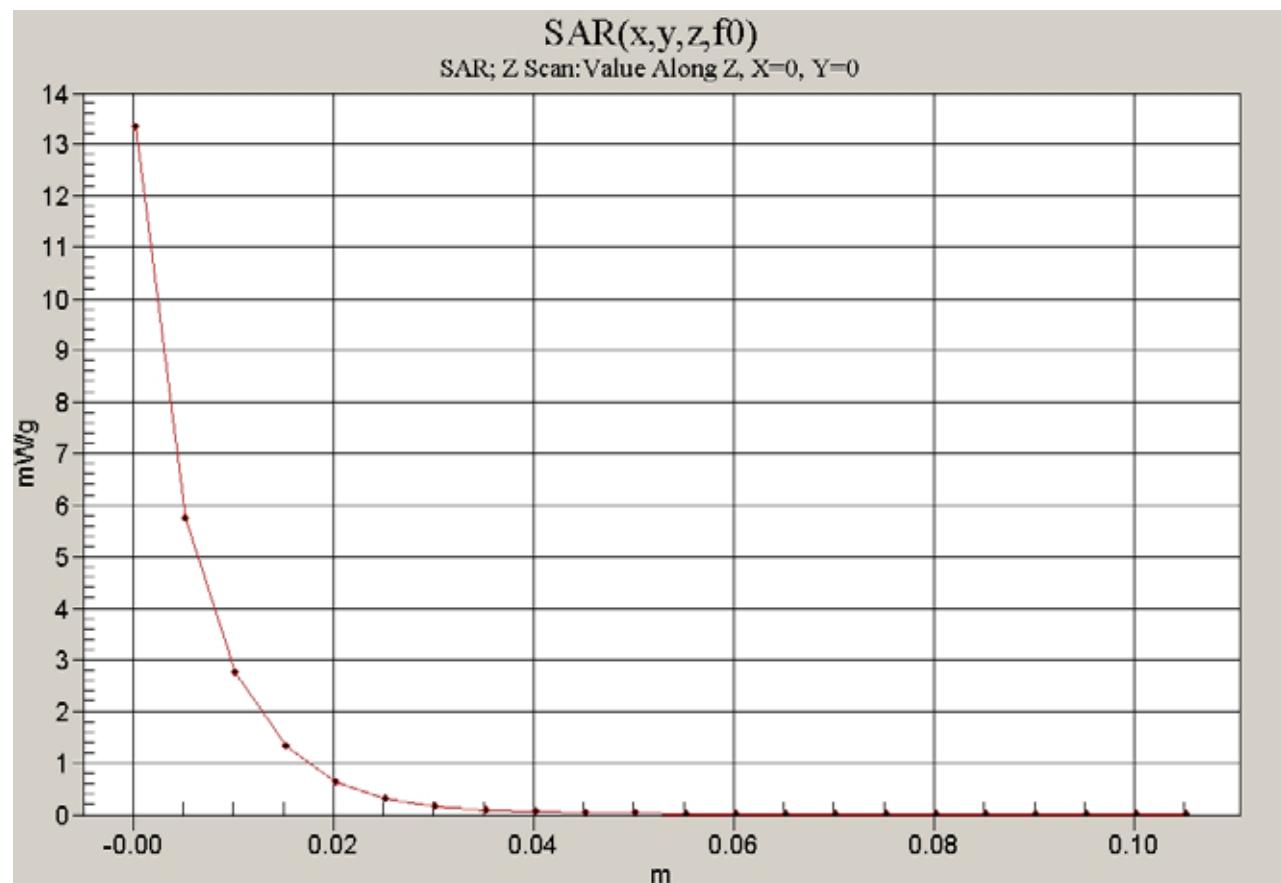

2450 MHz Validation Test_Body

Date/Time: 2010-10-15 9:51:39

Test Laboratory: SGS Testing Korea
File Name: [Validation 2450_Body.da4](#)

DUT: Dipole 2450 MHz; Type: D2450V2; Serial: D2450V2 - SN:734
Program Name: Validation 2450 MHz_Body


Communication System: CW; Frequency: 2450 MHz; Duty Cycle: 1:1
Medium parameters used: $f = 2450$ MHz; $\sigma = 1.98$ mho/m; $\epsilon_r = 50.2$; $\rho = 1000$ kg/m³
Phantom section: Flat Section

DASY4 Configuration:


- Probe: ET3DV6 - SN1782; ConvF(4.07, 4.07, 4.07); Calibrated: 2010-04-28
- Sensor-Surface: 4mm (Mechanical Surface Detection)
- Electronics: DAE3 Sn567; Calibrated: 2009-12-09
- Phantom: SAM MIC #2000-93 with CRP; Type: SAM MIC #2000-93; Serial: TP-1299
- Measurement SW: DASY4, V4.7 Build 80; Postprocessing SW: SEMCAD, V1.8 Build 186

Validation 2450 MHz_Body/Area Scan (61x61x1): Measurement grid: dx=15mm, dy=15mm
Maximum value of SAR (interpolated) = 16.2 mW/g

Validation 2450 MHz_Body/Zoom Scan (7x7x7)/Cube 0: Measurement grid: dx=5mm, dy=5mm, dz=5mm
Reference Value = 58.4 V/m; Power Drift = -0.006 dB
Peak SAR (extrapolated) = 33.5 W/kg
SAR(1 g) = 13.7 mW/g; SAR(10 g) = 6.05 mW/g
Maximum value of SAR (measured) = 15.0 mW/g

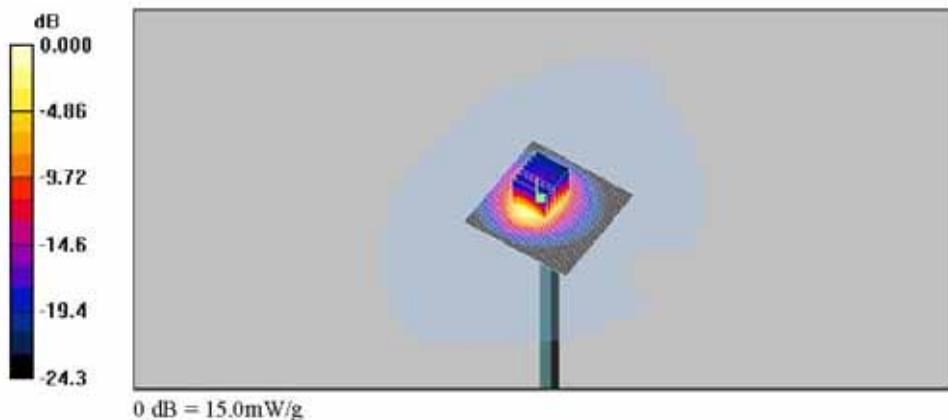

Z Scan

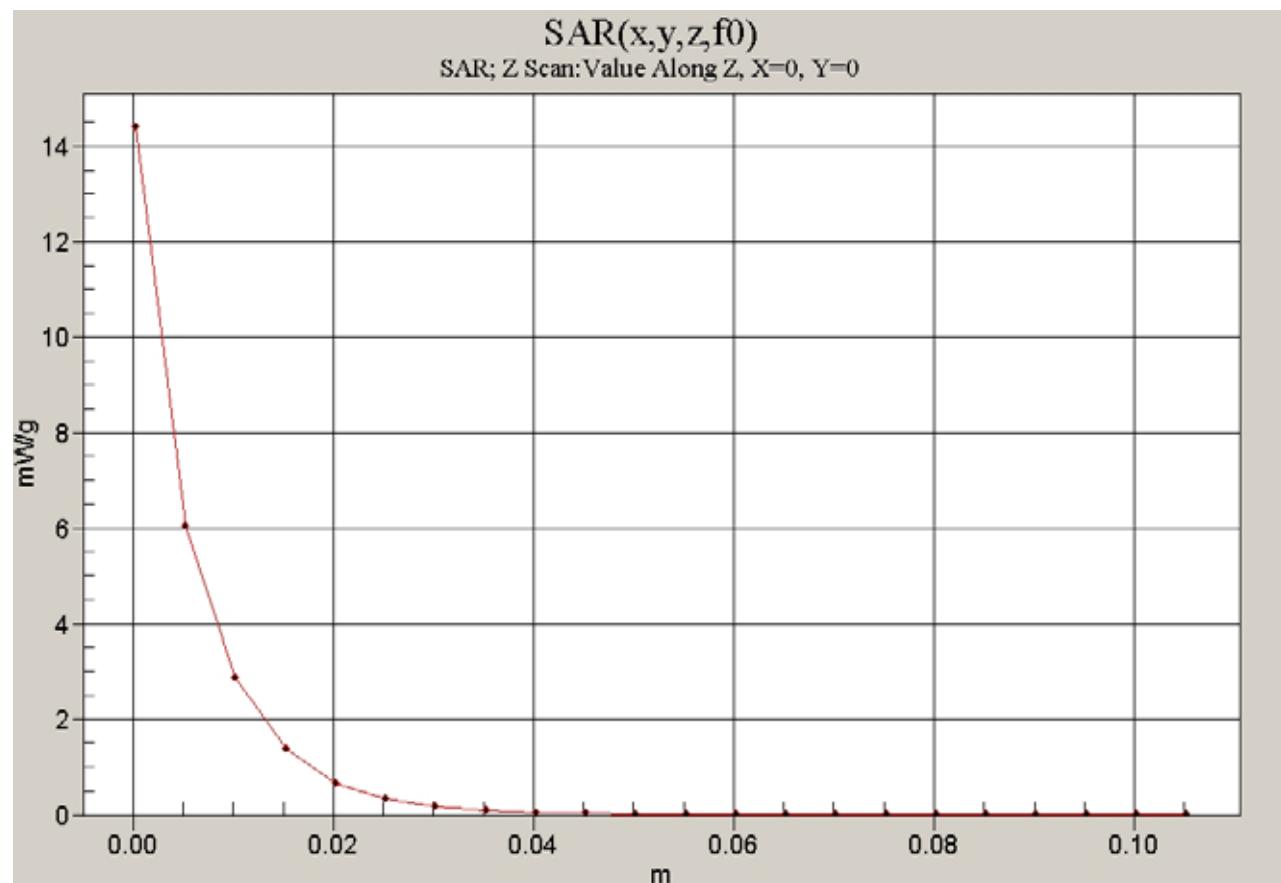

WLAN Head SAR Test

Date/Time: 2010-10-14 3:39:14

Test Laboratory: SGS Testing Korea
File Name: [WLAN LE.da4](#)

DUT: WPU-7800G; Type: Bar; Serial: -
Program Name: WLAN_Head


Communication System: WLAN; Frequency: 2437 MHz; Duty Cycle: 1:1
Medium parameters used: $f = 2437$ MHz; $\sigma = 1.8$ mho/m; $\epsilon_r = 38.2$; $\rho = 1000$ kg/m³
Phantom section: Left Section

DASY4 Configuration:

- Probe: ET3DV6 - SN1782; ConvF(4.48, 4.48, 4.48); Calibrated: 2010-04-28
- Sensor-Surface: 4mm (Mechanical Surface Detection)
- Electronics: DAE3 Sn567; Calibrated: 2009-12-09
- Phantom: SAM MIC #2000-93 with CRP; Type: SAM MIC #2000-93; Serial: TP-1299
- Measurement SW: DASY4, V4.7 Build 80; Postprocessing SW: SEMCAD, V1.8 Build 186

LE_11b_Mid_Cheek/Area Scan (61x71x1): Measurement grid: dx=15mm, dy=15mm
Maximum value of SAR (interpolated) = 0.065 mW/g

LE_11b_Mid_Cheek/Zoom Scan (7x7x7)/Cube 0: Measurement grid: dx=5mm, dy=5mm, dz=5mm
Reference Value = 5.51 V/m; Power Drift = 0.006 dB
Peak SAR (extrapolated) = 0.102 W/kg
 $SAR(1\text{ g}) = 0.055\text{ mW/g}$; $SAR(10\text{ g}) = 0.029\text{ mW/g}$
Maximum value of SAR (measured) = 0.061 mW/g

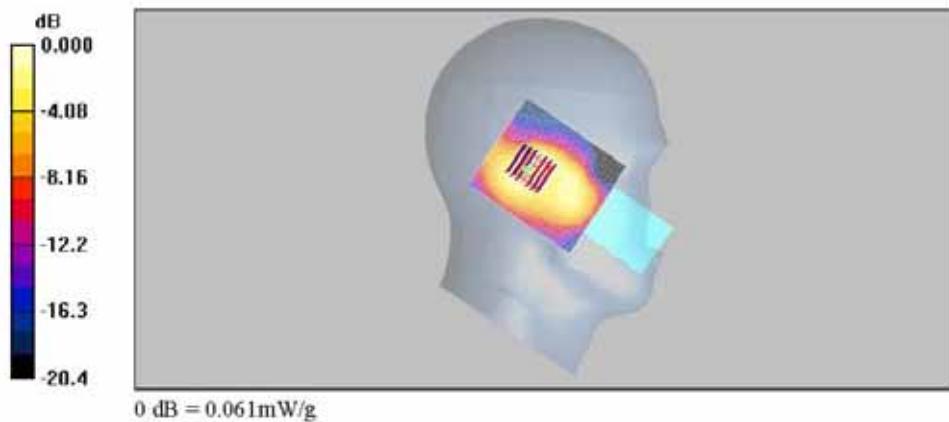

Date/Time: 2010-10-14 3:59:53

Test Laboratory: SGS Testing Korea
File Name: WLAN LE.da4

DUT: WPU-7800G; Type: Bar; Serial: -
Program Name: WLAN_Head


Communication System: WLAN; Frequency: 2437 MHz; Duty Cycle: 1:1
Medium parameters used: $f = 2437$ MHz; $\sigma = 1.8$ mho/m; $\epsilon_r = 38.2$; $\rho = 1000$ kg/m³
Phantom section: Left Section

DASY4 Configuration:

- Probe: ET3DV6 - SN1782; ConvF(4.48, 4.48, 4.48); Calibrated: 2010-04-28
- Sensor-Surface: 4mm (Mechanical Surface Detection)
- Electronics: DAE3 Sn567; Calibrated: 2009-12-09
- Phantom: SAM MIC #2000-93 with CRP; Type: SAM MIC #2000-93; Serial: TP-1299
- Measurement SW: DASY4, V4.7 Build 80; Postprocessing SW: SEMCAD, V1.8 Build 186

LE_11b_Mid_Tilt/Area Scan (61x71x1): Measurement grid: dx=15mm, dy=15mm
Maximum value of SAR (interpolated) = 0.052 mW/g

LE_11b_Mid_Tilt/Zoom Scan (7x7x7)/Cube 0: Measurement grid: dx=5mm, dy=5mm, dz=5mm
Reference Value = 5.23 V/m; Power Drift = 0.009 dB
Peak SAR (extrapolated) = 0.083 W/kg
SAR(1 g) = 0.044 mW/g; SAR(10 g) = 0.023 mW/g
Maximum value of SAR (measured) = 0.049 mW/g

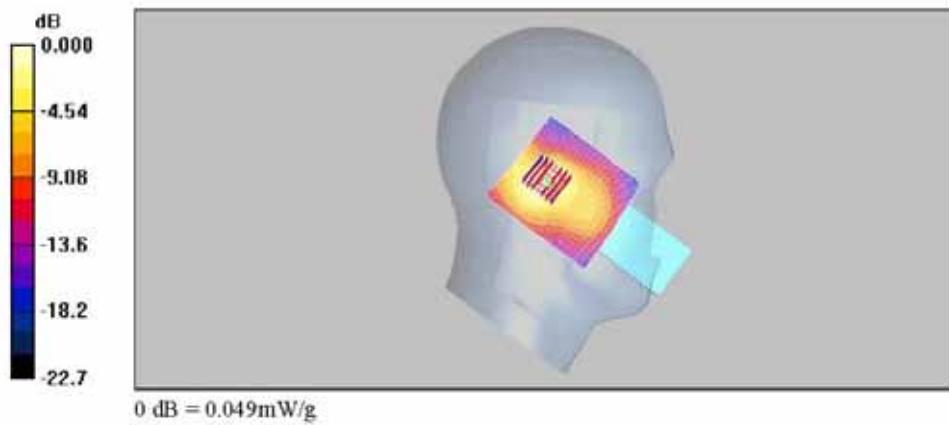

Date/Time: 2010-10-14 4:29:43

Test Laboratory: SGS Testing Korea
File Name: WLAN RE.da4

DUT: WPU-7800G; Type: Bar; Serial: -
Program Name: WLAN_Head


Communication System: WLAN; Frequency: 2437 MHz; Duty Cycle: 1:1
Medium parameters used: $f = 2437$ MHz; $\sigma = 1.8$ mho/m; $\epsilon_r = 38.2$; $\rho = 1000$ kg/m³
Phantom section: Right Section

DASY4 Configuration:

- Probe: ET3DV6 - SN1782; ConvF(4.48, 4.48, 4.48); Calibrated: 2010-04-28
- Sensor-Surface: 4mm (Mechanical Surface Detection)
- Electronics: DAE3 Sn567; Calibrated: 2009-12-09
- Phantom: SAM MIC #2000-93 with CRP; Type: SAM MIC #2000-93; Serial: TP-1299
- Measurement SW: DASY4, V4.7 Build 80; Postprocessing SW: SEMCAD, V1.8 Build 186

RE_11b_Mid_Cheek/Area Scan (61x71x1): Measurement grid: dx=15mm, dy=15mm
Maximum value of SAR (interpolated) = 0.083 mW/g

RE_11b_Mid_Cheek/Zoom Scan (7x7x7)/Cube 0: Measurement grid: dx=5mm, dy=5mm, dz=5mm
Reference Value = 6.54 V/m; Power Drift = 0.122 dB
Peak SAR (extrapolated) = 0.154 W/kg
SAR(1 g) = 0.078 mW/g; SAR(10 g) = 0.040 mW/g
Maximum value of SAR (measured) = 0.086 mW/g

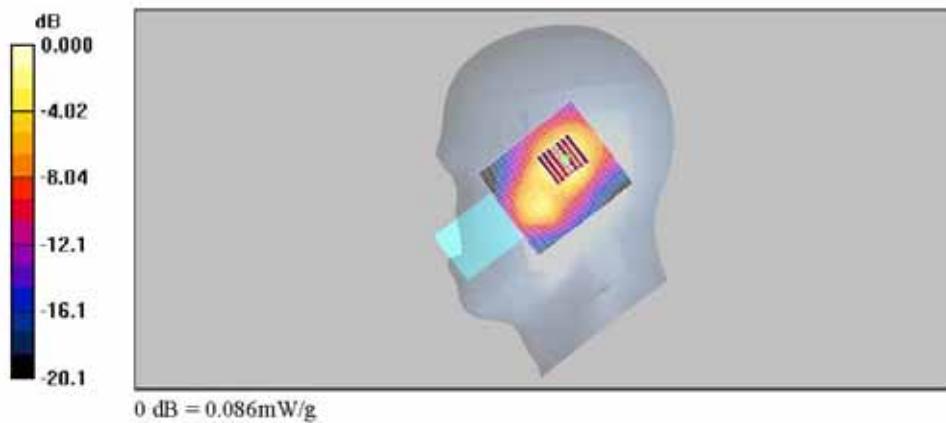

Date/Time: 2010-10-14 4:58:18

Test Laboratory: SGS Testing Korea
File Name: WLAN RE.da4

DUT: WPU-7800G; Type: Bar; Serial: -
Program Name: WLAN_Head


Communication System: WLAN; Frequency: 2437 MHz; Duty Cycle: 1:1
Medium parameters used: $f = 2437$ MHz; $\sigma = 1.8$ mho/m; $\epsilon_r = 38.2$; $\rho = 1000$ kg/m³
Phantom section: Right Section

DASY4 Configuration:

- Probe: ET3DV6 - SN1782; ConvF(4.48, 4.48, 4.48); Calibrated: 2010-04-28
- Sensor-Surface: 4mm (Mechanical Surface Detection)
- Electronics: DAE3 Sn567; Calibrated: 2009-12-09
- Phantom: SAM MIC #2000-93 with CRP; Type: SAM MIC #2000-93; Serial: TP-1299
- Measurement SW: DASY4, V4.7 Build 80; Postprocessing SW: SEMCAD, V1.8 Build 186

RE_11b_Mid_Tilt/Area Scan (61x71x1): Measurement grid: dx=15mm, dy=15mm
Maximum value of SAR (interpolated) = 0.061 mW/g

RE_11b_Mid_Tilt/Zoom Scan (7x7x7)/Cube 0: Measurement grid: dx=5mm, dy=5mm, dz=5mm
Reference Value = 6.01 V/m; Power Drift = -0.130 dB
Peak SAR (extrapolated) = 0.107 W/kg
SAR(1 g) = 0.055 mW/g; SAR(10 g) = 0.028 mW/g
Maximum value of SAR (measured) = 0.060 mW/g

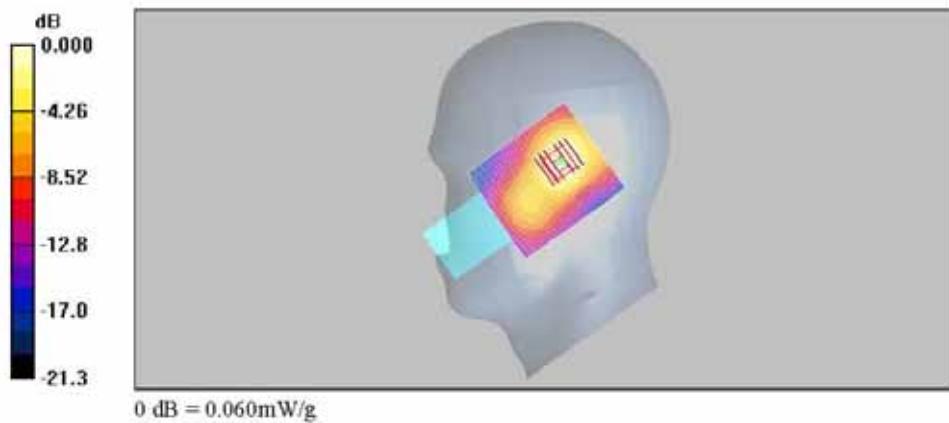

Date/Time: 2010-10-14 5:31:23

Test Laboratory: SGS Testing Korea
File Name: WLAN RE.da4

DUT: WPU-7800G; Type: Bar; Serial: -
Program Name: WLAN_Head


Communication System: WLAN; Frequency: 2437 MHz; Duty Cycle: 1:1
Medium parameters used: $f = 2437$ MHz; $\sigma = 1.8$ mho/m; $\epsilon_r = 38.2$; $\rho = 1000$ kg/m³
Phantom section: Right Section

DASY4 Configuration:

- Probe: ET3DV6 - SN1782; ConvF(4.48, 4.48, 4.48); Calibrated: 2010-04-28
- Sensor-Surface: 4mm (Mechanical Surface Detection)
- Electronics: DAE3 Sn567; Calibrated: 2009-12-09
- Phantom: SAM MIC #2000-93 with CRP; Type: SAM MIC #2000-93; Serial: TP-1299
- Measurement SW: DASY4, V4.7 Build 80; Postprocessing SW: SEMCAD, V1.8 Build 186

RE_11g_Mid_Cheek/Area Scan (61x71x1): Measurement grid: dx=15mm, dy=15mm
Maximum value of SAR (interpolated) = 0.058 mW/g

RE_11g_Mid_Cheek/Zoom Scan (7x7x7)/Cube 0: Measurement grid: dx=5mm, dy=5mm, dz=5mm
Reference Value = 5.37 V/m; Power Drift = 0.019 dB
Peak SAR (extrapolated) = 0.102 W/kg
SAR(1 g) = 0.051 mW/g; SAR(10 g) = 0.026 mW/g
Maximum value of SAR (measured) = 0.056 mW/g

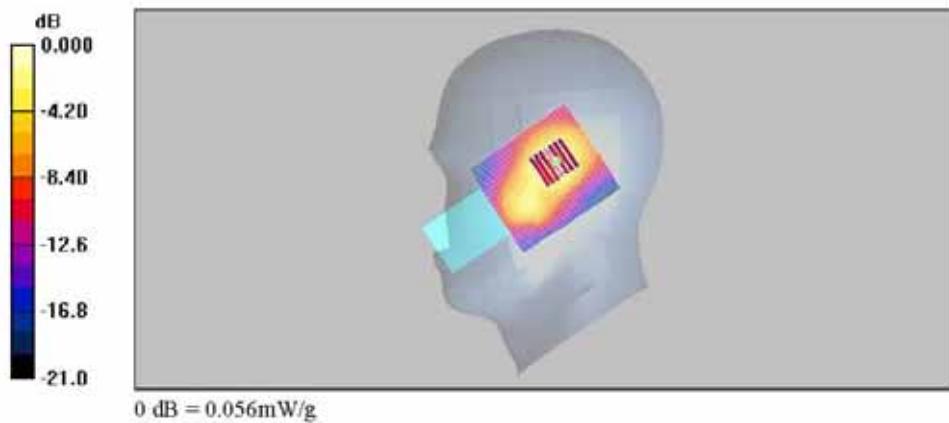

Date/Time: 2010-10-14 6:08:52

Test Laboratory: SGS Testing Korea
File Name: WLAN RE.da4

DUT: WPU-7800G; Type: Bar; Serial: -
Program Name: WLAN_Head


Communication System: WLAN; Frequency: 2412 MHz; Duty Cycle: 1:1
Medium parameters used: $f = 2412$ MHz; $\sigma = 1.73$ mho/m; $\epsilon_r = 38.5$; $\rho = 1000$ kg/m³
Phantom section: Right Section

DASY4 Configuration:

- Probe: ET3DV6 - SN1782; ConvF(4.48, 4.48, 4.48); Calibrated: 2010-04-28
- Sensor-Surface: 4mm (Mechanical Surface Detection)
- Electronics: DAE3 Sn567; Calibrated: 2009-12-09
- Phantom: SAM MIC #2000-93 with CRP; Type: SAM MIC #2000-93; Serial: TP-1299
- Measurement SW: DASY4, V4.7 Build 80; Postprocessing SW: SEMCAD, V1.8 Build 186

RE_11b_Low_Cheek/Area Scan (61x71x1): Measurement grid: dx=15mm, dy=15mm
Maximum value of SAR (interpolated) = 0.072 mW/g

RE_11b_Low_Cheek/Zoom Scan (7x7x7)/Cube 0: Measurement grid: dx=5mm, dy=5mm, dz=5mm
Reference Value = 6.06 V/m; Power Drift = -0.115 dB
Peak SAR (extrapolated) = 0.131 W/kg
SAR(1 g) = 0.063 mW/g; SAR(10 g) = 0.032 mW/g
Maximum value of SAR (measured) = 0.069 mW/g

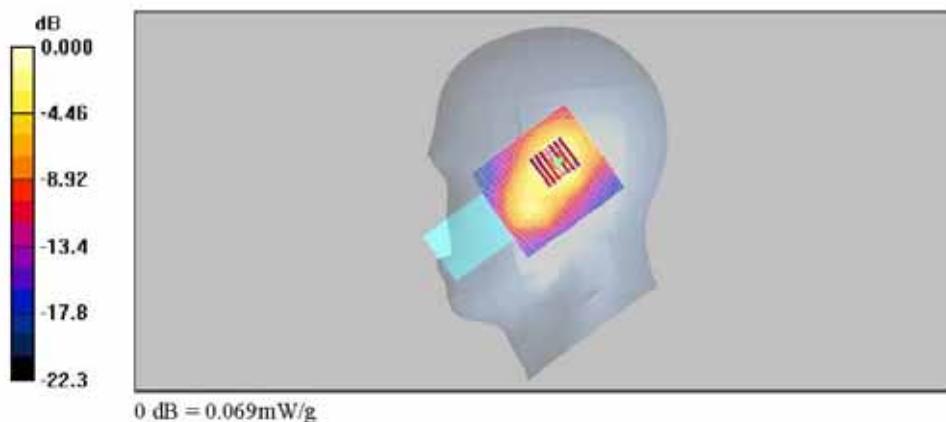

Date/Time: 2010-10-14 6:42:39

Test Laboratory: SGS Testing Korea
File Name: WLAN RE.da4

DUT: WPU-7800G; Type: Bar; Serial: -
Program Name: WLAN_Head


Communication System: WLAN; Frequency: 2462 MHz; Duty Cycle: 1:1
Medium parameters used: $f = 2462$ MHz; $\sigma = 1.86$ mho/m; $\epsilon_r = 38.3$; $\rho = 1000$ kg/m³
Phantom section: Right Section

DASY4 Configuration:

- Probe: ET3DV6 - SN1782; ConvF(4.48, 4.48, 4.48); Calibrated: 2010-04-28
- Sensor-Surface: 4mm (Mechanical Surface Detection)
- Electronics: DAE3 Sn567; Calibrated: 2009-12-09
- Phantom: SAM MIC #2000-93 with CRP; Type: SAM MIC #2000-93; Serial: TP-1299
- Measurement SW: DASY4, V4.7 Build 80; Postprocessing SW: SEMCAD, V1.8 Build 186

RE_11b_High_Cheek/Area Scan (61x71x1): Measurement grid: dx=15mm, dy=15mm
Maximum value of SAR (interpolated) = 0.108 mW/g

RE_11b_High_Cheek/Zoom Scan (7x7x7)/Cube 0: Measurement grid: dx=5mm, dy=5mm, dz=5mm
Reference Value = 7.08 V/m; Power Drift = -0.011 dB
Peak SAR (extrapolated) = 0.189 W/kg
SAR(1 g) = 0.092 mW/g; SAR(10 g) = 0.046 mW/g
Maximum value of SAR (measured) = 0.101 mW/g

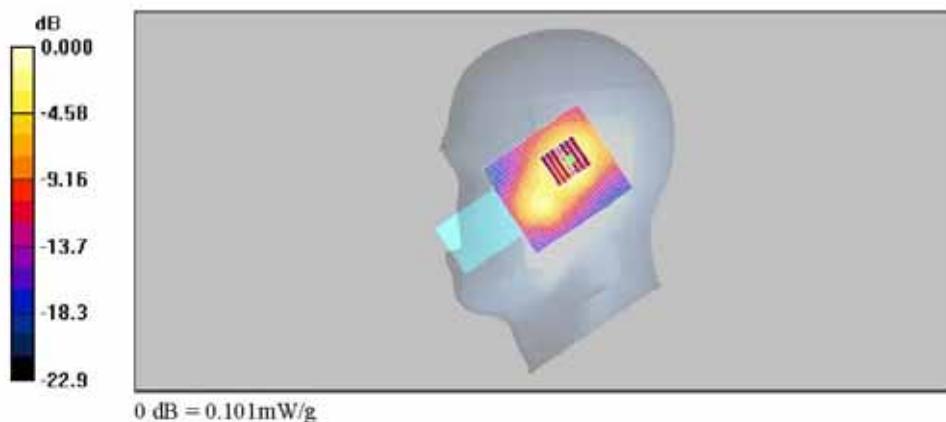

WLAN Body SAR Test

Date/Time: 2010-10-15 10:37:07

Test Laboratory: SGS Testing Korea
File Name: [WLAN_Body.da4](#)

DUT: WPU-7800G; Type: Bar; Serial: -
Program Name: WLAN_Body


Communication System: WLAN; Frequency: 2437 MHz; Duty Cycle: 1:1
Medium parameters used: $f = 2437$ MHz; $\sigma = 1.95$ mho/m; $\epsilon_r = 50.2$; $\rho = 1000$ kg/m³
Phantom section: Flat Section

DASY4 Configuration:

- Probe: ET3DV6 - SN1782; ConvF(4.07, 4.07, 4.07); Calibrated: 2010-04-28
- Sensor-Surface: 4mm (Mechanical Surface Detection)
- Electronics: DAE3 Sn567; Calibrated: 2009-12-09
- Phantom: SAM MIC #2000-93 with CRP; Type: SAM MIC #2000-93; Serial: TP-1299
- Measurement SW: DASY4, V4.7 Build 80; Postprocessing SW: SEMCAD, V1.8 Build 186

Body_11b_Mid_Front/Area Scan (61x71x1): Measurement grid: dx=15mm, dy=15mm
Maximum value of SAR (interpolated) = 0.022 mW/g

Body_11b_Mid_Front/Zoom Scan (7x7x7)/Cube 0: Measurement grid: dx=5mm, dy=5mm, dz=5mm
Reference Value = 3.26 V/m; Power Drift = -0.176 dB
Peak SAR (extrapolated) = 0.044 W/kg
SAR(1 g) = 0.021 mW/g; SAR(10 g) = 0.011 mW/g
Maximum value of SAR (measured) = 0.022 mW/g

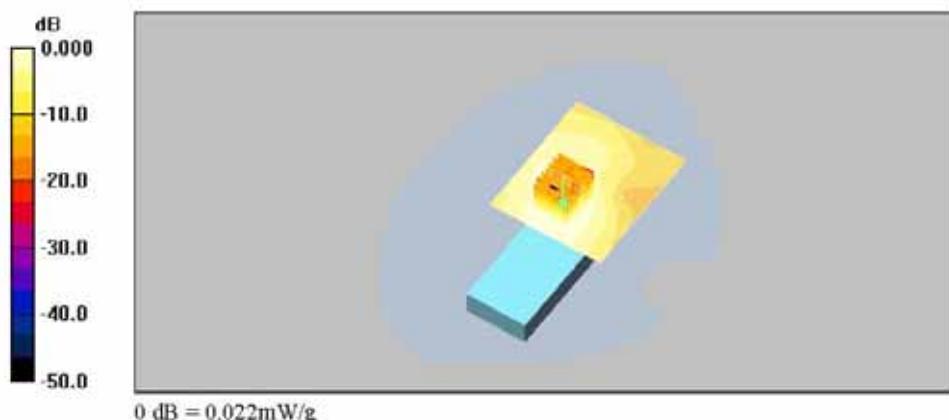

Date/Time: 2010-10-15 11:01:42

Test Laboratory: SGS Testing Korea
File Name: WLAN_Body.da4

DUT: WPU-7800G; Type: Bar; Serial: -
Program Name: WLAN_Body


Communication System: WLAN; Frequency: 2437 MHz; Duty Cycle: 1:1
Medium parameters used: $f = 2437$ MHz; $\sigma = 1.95$ mho/m; $\epsilon_r = 50.2$; $\rho = 1000$ kg/m³
Phantom section: Flat Section

DASY4 Configuration:

- Probe: ET3DV6 - SN1782; ConvF(4.07, 4.07, 4.07); Calibrated: 2010-04-28
- Sensor-Surface: 4mm (Mechanical Surface Detection)
- Electronics: DAE3 Sn567; Calibrated: 2009-12-09
- Phantom: SAM MIC #2000-93 with CRP; Type: SAM MIC #2000-93; Serial: TP-1299
- Measurement SW: DASY4, V4.7 Build 80; Postprocessing SW: SEMCAD, V1.8 Build 186

Body_11b_Mid_Back/Area Scan (61x71x1): Measurement grid: dx=15mm, dy=15mm
Maximum value of SAR (interpolated) = 0.104 mW/g

Body_11b_Mid_Back/Zoom Scan (7x7x7)/Cube 0: Measurement grid: dx=5mm, dy=5mm, dz=5mm
Reference Value = 1.77 V/m; Power Drift = -0.187 dB
Peak SAR (extrapolated) = 0.211 W/kg
SAR(1 g) = 0.093 mW/g; SAR(10 g) = 0.044 mW/g
Maximum value of SAR (measured) = 0.103 mW/g

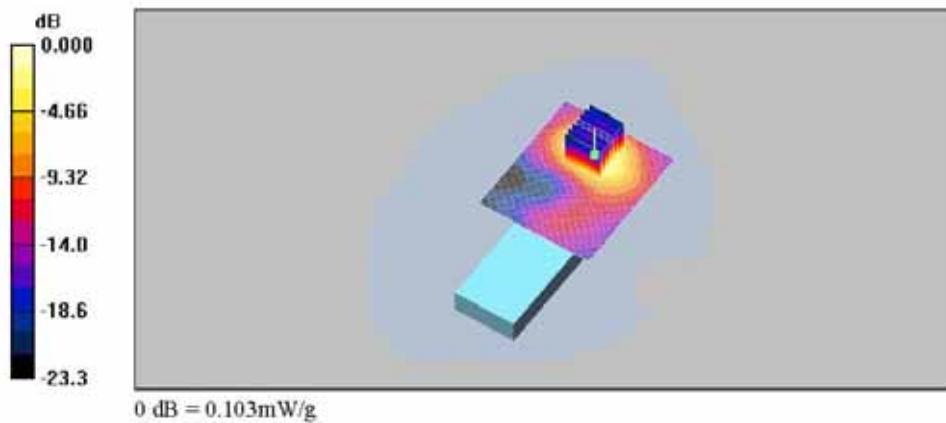

Date/Time: 2010-10-15 11:24:42

Test Laboratory: SGS Testing Korea
File Name: WLAN_Body.da4

DUT: WPU-7800G; Type: Bar; Serial: -
Program Name: WLAN_Body


Communication System: WLAN; Frequency: 2437 MHz; Duty Cycle: 1:1
Medium parameters used: $f = 2437$ MHz; $\sigma = 1.95$ mho/m; $\epsilon_r = 50.2$; $\rho = 1000$ kg/m³
Phantom section: Flat Section

DASY4 Configuration:

- Probe: ET3DV6 - SN1782; ConvF(4.07, 4.07, 4.07); Calibrated: 2010-04-28
- Sensor-Surface: 4mm (Mechanical Surface Detection)
- Electronics: DAE3 Sn567; Calibrated: 2009-12-09
- Phantom: SAM MIC #2000-93 with CRP; Type: SAM MIC #2000-93; Serial: TP-1299
- Measurement SW: DASY4, V4.7 Build 80; Postprocessing SW: SEMCAD, V1.8 Build 186

Body_11b_Mid_Back_Ear set/Area Scan (61x71x1): Measurement grid: dx=15mm, dy=15mm
Maximum value of SAR (interpolated) = 0.114 mW/g

Body_11b_Mid_Back_Ear set/Zoom Scan (7x7x7)/Cube 0: Measurement grid: dx=5mm, dy=5mm, dz=5mm
Reference Value = 1.65 V/m; Power Drift = 0.058 dB
Peak SAR (extrapolated) = 0.227 W/kg
SAR(1 g) = 0.101 mW/g; SAR(10 g) = 0.048 mW/g
Maximum value of SAR (measured) = 0.109 mW/g

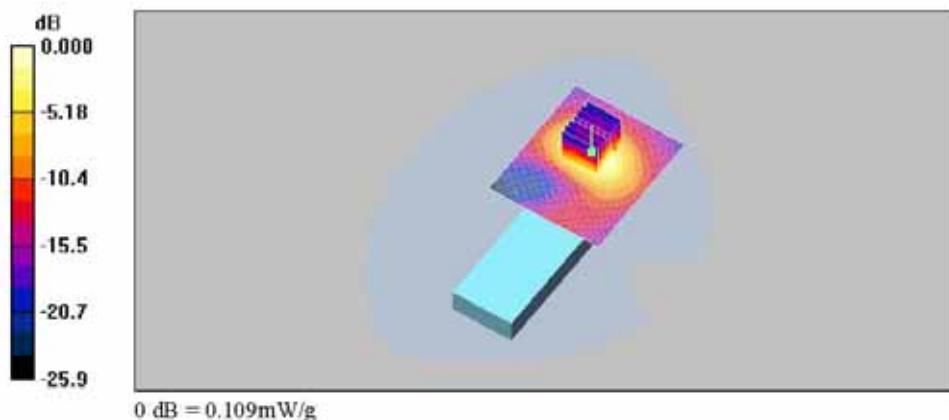

Date/Time: 2010-10-15 11:49:34

Test Laboratory: SGS Testing Korea
File Name: WLAN_Body.da4

DUT: WPU-7800G; Type: Bar; Serial: -
Program Name: WLAN_Body


Communication System: WLAN; Frequency: 2437 MHz; Duty Cycle: 1:1
Medium parameters used: $f = 2437$ MHz; $\sigma = 1.95$ mho/m; $\epsilon_r = 50.2$; $\rho = 1000$ kg/m³
Phantom section: Flat Section

DASY4 Configuration:

- Probe: ET3DV6 - SN1782; ConvF(4.07, 4.07, 4.07); Calibrated: 2010-04-28
- Sensor-Surface: 4mm (Mechanical Surface Detection)
- Electronics: DAE3 Sn567; Calibrated: 2009-12-09
- Phantom: SAM MIC #2000-93 with CRP; Type: SAM MIC #2000-93; Serial: TP-1299
- Measurement SW: DASY4, V4.7 Build 80; Postprocessing SW: SEMCAD, V1.8 Build 186

Body_11g_Mid_Back_Ear set/Area Scan (61x71x1): Measurement grid: dx=15mm, dy=15mm
Maximum value of SAR (interpolated) = 0.079 mW/g

Body_11g_Mid_Back_Ear set/Zoom Scan (7x7x7)/Cube 0: Measurement grid: dx=5mm, dy=5mm, dz=5mm
Reference Value = 1.50 V/m; Power Drift = -0.189 dB
Peak SAR (extrapolated) = 0.154 W/kg
SAR(1 g) = 0.068 mW/g; SAR(10 g) = 0.032 mW/g
Maximum value of SAR (measured) = 0.075 mW/g

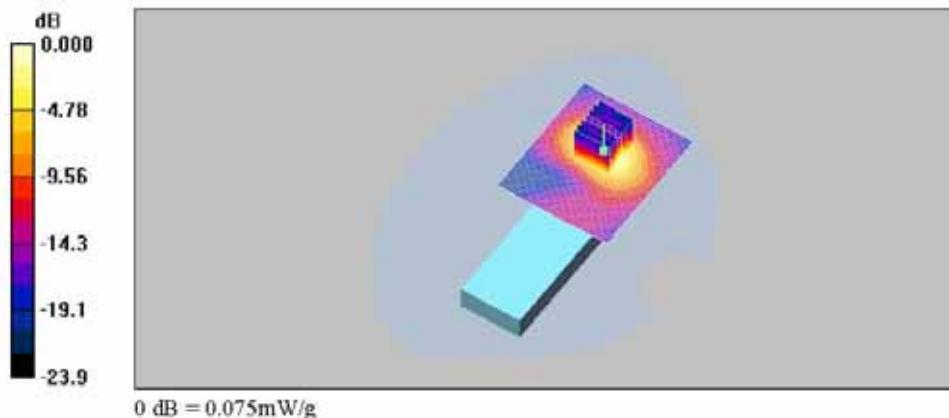

Date/Time: 2010-10-15 1:19:20

Test Laboratory: SGS Testing Korea
File Name: WLAN_Body.da4

DUT: WPU-7800G; Type: Bar; Serial: -
Program Name: WLAN_Body


Communication System: WLAN; Frequency: 2412 MHz; Duty Cycle: 1:1
Medium parameters used: $f = 2412$ MHz; $\sigma = 1.92$ mho/m; $\epsilon_r = 50.4$; $\rho = 1000$ kg/m³
Phantom section: Flat Section

DASY4 Configuration:

- Probe: ET3DV6 - SN1782; ConvF(4.07, 4.07, 4.07); Calibrated: 2010-04-28
- Sensor-Surface: 4mm (Mechanical Surface Detection)
- Electronics: DAE3 Sn567; Calibrated: 2009-12-09
- Phantom: SAM MIC #2000-93 with CRP; Type: SAM MIC #2000-93; Serial: TP-1299
- Measurement SW: DASY4, V4.7 Build 80; Postprocessing SW: SEMCAD, V1.8 Build 186

Body_11b_Low_Back_Ear set/Area Scan (61x71x1): Measurement grid: dx=15mm, dy=15mm
Maximum value of SAR (interpolated) = 0.123 mW/g

Body_11b_Low_Back_Ear set/Zoom Scan (7x7x7)/Cube 0: Measurement grid: dx=5mm, dy=5mm, dz=5mm
Reference Value = 1.79 V/m; Power Drift = 0.054 dB
Peak SAR (extrapolated) = 0.250 W/kg
SAR(1 g) = 0.107 mW/g; SAR(10 g) = 0.050 mW/g
Maximum value of SAR (measured) = 0.115 mW/g

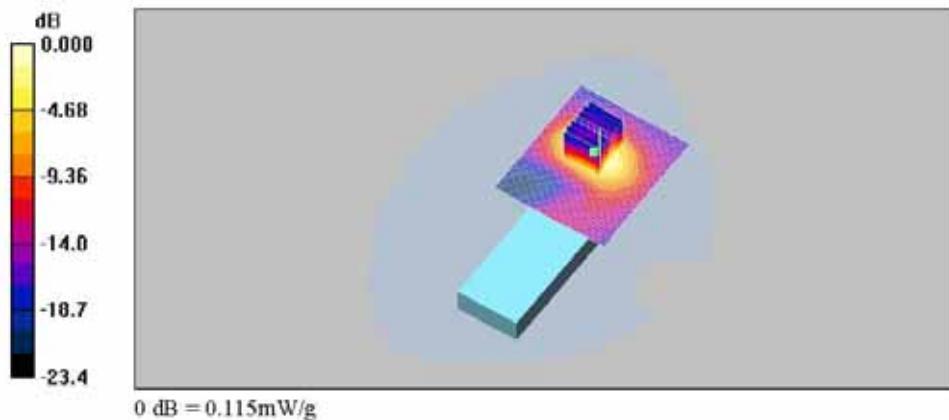

Date/Time: 2010-10-15 1:50:57

Test Laboratory: SGS Testing Korea
File Name: WLAN_Body.da4

DUT: WPU-7800G; Type: Bar; Serial: -
Program Name: WLAN_Body


Communication System: WLAN; Frequency: 2462 MHz; Duty Cycle: 1:1
Medium parameters used: $f = 2462$ MHz; $\sigma = 2$ mho/m; $\epsilon_r = 50.2$; $\rho = 1000$ kg/m³
Phantom section: Flat Section

DASY4 Configuration:


- Probe: ET3DV6 - SN1782; ConvF(4.07, 4.07, 4.07); Calibrated: 2010-04-28
- Sensor-Surface: 4mm (Mechanical Surface Detection)
- Electronics: DAE3 Sn567; Calibrated: 2009-12-09
- Phantom: SAM MIC #2000-93 with CRP; Type: SAM MIC #2000-93; Serial: TP-1299
- Measurement SW: DASY4, V4.7 Build 80; Postprocessing SW: SEMCAD, V1.8 Build 186

Body_11b_High_Back_Ear set/Area Scan (61x71x1): Measurement grid: dx=15mm, dy=15mm
Maximum value of SAR (interpolated) = 0.148 mW/g

Body_11b_High_Back_Ear set/Zoom Scan (7x7x7)/Cube 0: Measurement grid: dx=5mm, dy=5mm, dz=5mm
Reference Value = 2.14 V/m; Power Drift = -0.106 dB
Peak SAR (extrapolated) = 0.294 W/kg
SAR(1 g) = 0.127 mW/g; SAR(10 g) = 0.060 mW/g
Maximum value of SAR (measured) = 0.137 mW/g

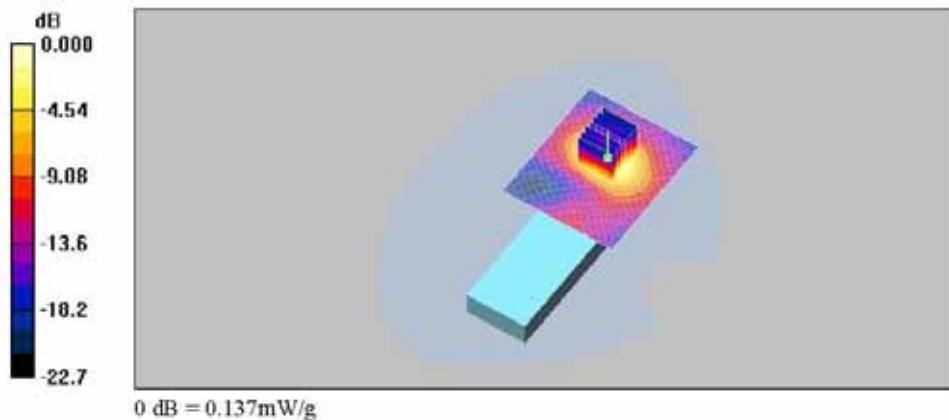

Z Scan

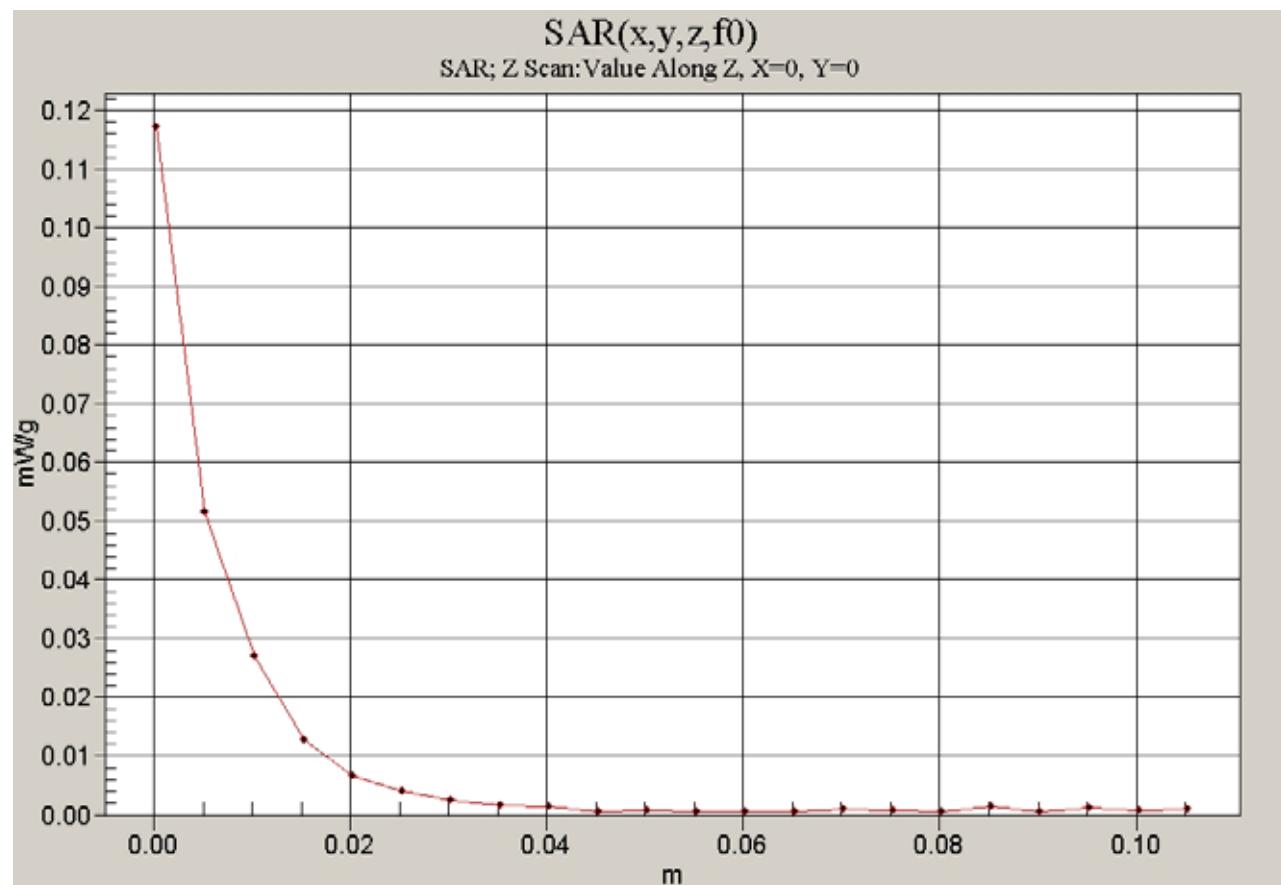

Appendix B

Uncertainty Analysis

| a | b | c | d | e = f(d,k) | g | i = cxg/e | k |
|--|------------------|---------|--------------|------------|---------|-----------|-----------|
| Uncertainty Component | Section in P1528 | Tol (%) | Prob . Dist. | Div. | Ci (1g) | 1g ui (%) | Vi (Veff) |
| Probe calibration | E.2.1 | 6.3 | N | 1 | 1 | 6.30 | |
| Axial isotropy | E.2.2 | 0.5 | R | 1.73 | 0.71 | 0.20 | |
| hemispherical isotropy | E.2.2 | 2.6 | R | 1.73 | 0.71 | 1.06 | |
| Boundary effect | E.2.3 | 0.8 | R | 1.73 | 1 | 0.46 | |
| Linearity | E.2.4 | 0.6 | R | 1.73 | 1 | 0.35 | |
| System detection limit | E.2.5 | 0.25 | R | 1.73 | 1 | 0.14 | |
| Readout electronics | E.2.6 | 0.3 | N | 1 | 1 | 0.30 | |
| Response time | E.2.7 | 0 | R | 1.73 | 1 | 0.00 | |
| Integration time | E.2.8 | 2.6 | R | 1.73 | 1 | 1.50 | |
| RF ambient Condition -Noise | E.6.1 | 3 | R | 1.73 | 1 | 1.73 | |
| RF ambient Condition - reflections | E.6.1 | 3 | R | 1.73 | 1 | 1.73 | |
| Probe positioning- mechanical tolerance | E.6.2 | 1.5 | R | 1.73 | 1 | 0.87 | |
| Probe positioning - with respect to phantom | E.6.3 | 2.9 | R | 1.73 | 1 | 1.67 | |
| Max. SAR evaluation | E.5.2 | 1 | R | 1.73 | 1 | 0.58 | |
| Test sample positioning | E.4.2 | 2.3 | N | 1 | 1 | 2.30 | 9 |
| Device holder uncertainty | E.4.1 | 3.6 | N | 1 | 1 | 3.60 | |
| Output power variation -SAR drift measurement | 6.62 | 5 | R | 1.73 | 1 | 2.89 | |
| Phantom uncertainty (shape and thickness tolerances) | E.3.1 | 4 | R | 1.73 | 1 | 2.31 | |
| Liquid conductivity - deviation from target values | E.3.2 | 5 | R | 1.73 | 0.64 | 1.85 | |
| Liquid conductivity - measurement uncertainty | E.3.2 | 1.2 | N | 1 | 0.64 | 0.77 | 5 |
| Liquid permittivity - deviation from target values | E.3.3 | 5 | R | 1.73 | 0.6 | 1.73 | |
| Liquid permittivity - measurement uncertainty | E.3.3 | 1.1 | N | 1 | 0.6 | 0.66 | 5 |
| Combined standard uncertainty | | | | RSS | | 9.63 | 2754 |
| Expanded uncertainty (95% CONFIDENCE INTERVAL) | | | | k=2 | | 19.27 | |

Appendix C

Calibration Certificate

- PROBE

- DAE

- 2450 MHz DIPOLE

- PROBE Calibration Certificate

Calibration Laboratory of
Schmid & Partner
Engineering AG
Zeughausstrasse 43, 8004 Zurich, Switzerland



S Schweizerischer Kalibrierdienst
C Service suisse d'étalementage
S Servizio svizzero di taratura
S Swiss Calibration Service

Accredited by the Swiss Accreditation Service (SAS)
The Swiss Accreditation Service is one of the signatories to the EA
Multilateral Agreement for the recognition of calibration certificates

Accreditation No.: SCS 108

Client SGS-KES (Dymstec)

Certificate No: ET3-1782_Apr10

CALIBRATION CERTIFICATE

| Object | ET3DV6 - SN:1782 | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | |
|---|--|-----------------------------------|------------------------|---------------------|------|----------------------------|-----------------------|-----------------------|----------------|----------------------------------|------------------------|---------------------------|------------|-----------------------------------|------------------------|---------------------|------------|--------------------------|--------|---------------------------|----------------|---------------------------|--------|----------------------------|-----------------|---------------------------|--------|----------------------------|-----------------|---------------------------|--------|------------------------|----------|--------------------------------|--------|------|---------|--------------------------------|--------|
| Calibration procedure(s) | QA CAL-01.v6, QA CAL-12.v6, QA CAL-23.v3 and QA CAL-25.v2 Calibration procedure for dosimetric E-field probes | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | |
| Calibration date: | April 28, 2010 | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | |
| <p>This calibration certificate documents the traceability to national standards, which realize the physical units of measurements (SI). The measurements and the uncertainties with confidence probability are given on the following pages and are part of the certificate.</p> <p>All calibrations have been conducted in the closed laboratory facility: environment temperature (22 ± 3)°C and humidity < 70%.</p> <p>Calibration Equipment used (M&TE critical for calibration)</p> | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | |
| <table><thead><tr><th>Primary Standards</th><th>ID #</th><th>Cal Date (Certificate No.)</th><th>Scheduled Calibration</th></tr></thead><tbody><tr><td>Power meter E4419B</td><td>GB41293874</td><td>1-Apr-10 (No. 217-01136)</td><td>Apr-11</td></tr><tr><td>Power sensor E4412A</td><td>MY41495277</td><td>1-Apr-10 (No. 217-01136)</td><td>Apr-11</td></tr><tr><td>Power sensor E4412A</td><td>MY41498587</td><td>1-Apr-10 (No. 217-01136)</td><td>Apr-11</td></tr><tr><td>Reference 3 dB Attenuator</td><td>SN: S5054 (3c)</td><td>30-Mar-10 (No. 217-01159)</td><td>Mar-11</td></tr><tr><td>Reference 20 dB Attenuator</td><td>SN: S5088 (20b)</td><td>30-Mar-10 (No. 217-01161)</td><td>Mar-11</td></tr><tr><td>Reference 30 dB Attenuator</td><td>SN: S5129 (30b)</td><td>30-Mar-10 (No. 217-01160)</td><td>Mar-11</td></tr><tr><td>Reference Probe ES3DV2</td><td>SN: 3013</td><td>30-Dec-09 (No. ES3-3013_Dec09)</td><td>Dec-10</td></tr><tr><td>DAE4</td><td>SN: 660</td><td>29-Sep-09 (No. DAE4-660_Sep09)</td><td>Sep-10</td></tr></tbody></table> | | | | Primary Standards | ID # | Cal Date (Certificate No.) | Scheduled Calibration | Power meter E4419B | GB41293874 | 1-Apr-10 (No. 217-01136) | Apr-11 | Power sensor E4412A | MY41495277 | 1-Apr-10 (No. 217-01136) | Apr-11 | Power sensor E4412A | MY41498587 | 1-Apr-10 (No. 217-01136) | Apr-11 | Reference 3 dB Attenuator | SN: S5054 (3c) | 30-Mar-10 (No. 217-01159) | Mar-11 | Reference 20 dB Attenuator | SN: S5088 (20b) | 30-Mar-10 (No. 217-01161) | Mar-11 | Reference 30 dB Attenuator | SN: S5129 (30b) | 30-Mar-10 (No. 217-01160) | Mar-11 | Reference Probe ES3DV2 | SN: 3013 | 30-Dec-09 (No. ES3-3013_Dec09) | Dec-10 | DAE4 | SN: 660 | 29-Sep-09 (No. DAE4-660_Sep09) | Sep-10 |
| Primary Standards | ID # | Cal Date (Certificate No.) | Scheduled Calibration | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | |
| Power meter E4419B | GB41293874 | 1-Apr-10 (No. 217-01136) | Apr-11 | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | |
| Power sensor E4412A | MY41495277 | 1-Apr-10 (No. 217-01136) | Apr-11 | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | |
| Power sensor E4412A | MY41498587 | 1-Apr-10 (No. 217-01136) | Apr-11 | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | |
| Reference 3 dB Attenuator | SN: S5054 (3c) | 30-Mar-10 (No. 217-01159) | Mar-11 | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | |
| Reference 20 dB Attenuator | SN: S5088 (20b) | 30-Mar-10 (No. 217-01161) | Mar-11 | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | |
| Reference 30 dB Attenuator | SN: S5129 (30b) | 30-Mar-10 (No. 217-01160) | Mar-11 | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | |
| Reference Probe ES3DV2 | SN: 3013 | 30-Dec-09 (No. ES3-3013_Dec09) | Dec-10 | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | |
| DAE4 | SN: 660 | 29-Sep-09 (No. DAE4-660_Sep09) | Sep-10 | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | |
| <table><thead><tr><th>Secondary Standards</th><th>ID #</th><th>Check Date (in house)</th><th>Scheduled Check</th></tr></thead><tbody><tr><td>RF generator HP 8648C</td><td>US3642U01700</td><td>4-Aug-99 (in house check Oct-09)</td><td>In house check: Oct-11</td></tr><tr><td>Network Analyzer HP 8753E</td><td>US37390585</td><td>18-Oct-01 (in house check Oct-09)</td><td>In house check: Oct-10</td></tr></tbody></table> | | | | Secondary Standards | ID # | Check Date (in house) | Scheduled Check | RF generator HP 8648C | US3642U01700 | 4-Aug-99 (in house check Oct-09) | In house check: Oct-11 | Network Analyzer HP 8753E | US37390585 | 18-Oct-01 (in house check Oct-09) | In house check: Oct-10 | | | | | | | | | | | | | | | | | | | | | | | | |
| Secondary Standards | ID # | Check Date (in house) | Scheduled Check | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | |
| RF generator HP 8648C | US3642U01700 | 4-Aug-99 (in house check Oct-09) | In house check: Oct-11 | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | |
| Network Analyzer HP 8753E | US37390585 | 18-Oct-01 (in house check Oct-09) | In house check: Oct-10 | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | |
| <table><thead><tr><th>Calibrated by:</th><th>Name</th><th>Function</th><th>Signature</th></tr></thead><tbody><tr><td></td><td>Jeton Kastrati</td><td>Laboratory Technician</td><td></td></tr></tbody></table> | | | | Calibrated by: | Name | Function | Signature | | Jeton Kastrati | Laboratory Technician | | | | | | | | | | | | | | | | | | | | | | | | | | | | | |
| Calibrated by: | Name | Function | Signature | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | |
| | Jeton Kastrati | Laboratory Technician | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | |
| <table><thead><tr><th>Approved by:</th><th>Name</th><th>Function</th><th>Signature</th></tr></thead><tbody><tr><td></td><td>Katja Pokovic</td><td>Technical Manager</td><td></td></tr></tbody></table> | | | | Approved by: | Name | Function | Signature | | Katja Pokovic | Technical Manager | | | | | | | | | | | | | | | | | | | | | | | | | | | | | |
| Approved by: | Name | Function | Signature | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | |
| | Katja Pokovic | Technical Manager | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | |
| Issued: April 28, 2010 | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | |
| This calibration certificate shall not be reproduced except in full without written approval of the laboratory | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | |

Calibration Laboratory of
Schmid & Partner
Engineering AG
Zeughausstrasse 43, 8004 Zurich, Switzerland



S Schweizerischer Kalibrierdienst
C Service suisse d'étalonnage
S Servizio svizzero di taratura
S Swiss Calibration Service

Accredited by the Swiss Accreditation Service (SAS)

The Swiss Accreditation Service is one of the signatories to the EA
Multilateral Agreement for the recognition of calibration certificates

Accreditation No.: SCS 108

Glossary:

| | |
|------------------------|---|
| TSL | tissue simulating liquid |
| NORM _{x,y,z} | sensitivity in free space |
| ConvF | sensitivity in TSL / NORM _{x,y,z} |
| DCP | diode compression point |
| CF | crest factor (1/duty_cycle) of the RF signal |
| A, B, C | modulation dependent linearization parameters |
| Polarization φ | φ rotation around probe axis |
| Polarization β | β rotation around an axis that is in the plane normal to probe axis (at measurement center), i.e., $\beta = 0$ is normal to probe axis |

Calibration is Performed According to the Following Standards:

- IEEE Std 1528-2003, "IEEE Recommended Practice for Determining the Peak Spatial-Averaged Specific Absorption Rate (SAR) in the Human Head from Wireless Communications Devices: Measurement Techniques", December 2003
- IEC 62209-1, "Procedure to measure the Specific Absorption Rate (SAR) for hand-held devices used in close proximity to the ear (frequency range of 300 MHz to 3 GHz)", February 2005

Methods Applied and Interpretation of Parameters:

- $NORM_{x,y,z}$: Assessed for E-field polarization $\beta = 0$ ($f \leq 900$ MHz in TEM-cell; $f > 1800$ MHz: R22 waveguide). $NORM_{x,y,z}$ are only intermediate values, i.e., the uncertainties of $NORM_{x,y,z}$ does not effect the E²-field uncertainty inside TSL (see below ConvF).
- $NORM(f)x,y,z = NORM_{x,y,z} * frequency_response$ (see Frequency Response Chart). This linearization is implemented in DASY4 software versions later than 4.2. The uncertainty of the frequency response is included in the stated uncertainty of ConvF.
- $DCPx,y,z$: DCP are numerical linearization parameters assessed based on the data of power sweep with CW signal (no uncertainty required). DCP does not depend on frequency nor media.
- Ax,y,z ; Bx,y,z ; Cx,y,z ; VRx,y,z ; A, B, C are numerical linearization parameters assessed based on the data of power sweep for specific modulation signal. The parameters do not depend on frequency nor media. VR is the maximum calibration range expressed in RMS voltage across the diode.
- ConvF and Boundary Effect Parameters*: Assessed in flat phantom using E-field (or Temperature Transfer Standard for $f \leq 800$ MHz) and inside waveguide using analytical field distributions based on power measurements for $f > 800$ MHz. The same setups are used for assessment of the parameters applied for boundary compensation (alpha, depth) of which typical uncertainty values are given. These parameters are used in DASY4 software to improve probe accuracy close to the boundary. The sensitivity in TSL corresponds to $NORM_{x,y,z} * ConvF$ whereby the uncertainty corresponds to that given for ConvF. A frequency dependent ConvF is used in DASY version 4.4 and higher which allows extending the validity from ± 50 MHz to ± 100 MHz.
- Spherical isotropy (3D deviation from isotropy)*: in a field of low gradients realized using a flat phantom exposed by a patch antenna.
- Sensor Offset*: The sensor offset corresponds to the offset of virtual measurement center from the probe tip (on probe axis). No tolerance required.

ET3DV6 SN:1782

April 28, 2010

Probe ET3DV6

SN:1782

| | |
|------------------|----------------|
| Manufactured: | April 15, 2003 |
| Last calibrated: | April 30, 2009 |
| Modified: | April 27, 2010 |
| Recalibrated: | April 28, 2010 |

Calibrated for DASY Systems

(Note: non-compatible with DASY2 system!)

ET3DV6 SN:1782

April 28, 2010

DASY - Parameters of Probe: ET3DV6 SN:1782

Basic Calibration Parameters

| | Sensor X | Sensor Y | Sensor Z | Unc (k=2) |
|--|----------|----------|----------|--------------|
| Norm (μ V/(V/m) ²) ^a | 2.01 | 1.74 | 1.86 | $\pm 10.1\%$ |
| DCP (mV) ^b | 93.9 | 96.4 | 91.2 | |

Modulation Calibration Parameters

| UID | Communication System Name | PAR | | A dB | B dBuV | C | VR mV | Unc ^c (k=2) |
|-------|---------------------------|------|-------------|----------------------|----------------------|----------------------|-------------------------|---------------------------|
| 10000 | CW | 0.00 | X Y Z | 0.00 0.00 0.00 | 0.00 0.00 0.00 | 1.00 1.00 1.00 | 300.0 300.0 300.0 | $\pm 1.5\%$ |

The reported uncertainty of measurement is stated as the standard uncertainty of measurement multiplied by the coverage factor k=2, which for a normal distribution corresponds to a coverage probability of approximately 95%.

^a The uncertainties of NormX,Y,Z do not affect the E²-field uncertainty inside TSL (see Pages 5 and 6).

^b Numerical linearization parameter: uncertainty not required.

^c Uncertainty is determined using the maximum deviation from linear response applying rectangular distribution and is expressed for the square of the field value.

ET3DV6 SN:1782

April 28, 2010

DASY - Parameters of Probe: ET3DV6 SN:1782

Calibration Parameter Determined in Head Tissue Simulating Media

| f [MHz] | Validity [MHz] ^c | Permittivity | Conductivity | ConvF X | ConvF Y | ConvF Z | Alpha | Depth Unc (k=2) |
|---------|-----------------------------|--------------|--------------|---------|---------|---------|-------|-----------------|
| 450 | ± 50 / ± 100 | 43.5 ± 5% | 0.87 ± 5% | 6.67 | 6.67 | 6.67 | 0.19 | 2.19 ± 13.3% |
| 835 | ± 50 / ± 100 | 41.9 ± 5% | 0.89 ± 5% | 6.26 | 6.26 | 6.26 | 0.51 | 2.05 ± 11.0% |
| 1750 | ± 50 / ± 100 | 40.1 ± 5% | 1.37 ± 5% | 5.30 | 5.30 | 5.30 | 0.53 | 2.60 ± 11.0% |
| 1900 | ± 50 / ± 100 | 40.0 ± 5% | 1.40 ± 5% | 5.04 | 5.04 | 5.04 | 0.69 | 2.24 ± 11.0% |
| 2450 | ± 50 / ± 100 | 39.2 ± 5% | 1.80 ± 5% | 4.48 | 4.48 | 4.48 | 0.99 | 1.71 ± 11.0% |

^c The validity of ± 100 MHz only applies for DASY v4.4 and higher (see Page 2). The uncertainty is the RSS of the ConvP uncertainty at calibration frequency and the uncertainty for the indicated frequency band.

ET3DV6 SN:1782

April 28, 2010

DASY - Parameters of Probe: ET3DV6 SN:1782

Calibration Parameter Determined in Body Tissue Simulating Media

| f [MHz] | Validity [MHz] ^c | Permittivity | Conductivity | ConvF X | ConvF Y | ConvF Z | Alpha | Depth Unc (k=2) |
|---------|-----------------------------|--------------|--------------|---------|---------|---------|-------|-----------------|
| 450 | ± 50 / ± 100 | 56.7 ± 5% | 0.94 ± 5% | 7.53 | 7.53 | 7.53 | 0.15 | 2.33 ± 13.3% |
| 635 | ± 50 / ± 100 | 55.2 ± 5% | 0.97 ± 5% | 6.11 | 6.11 | 6.11 | 0.42 | 2.40 ± 11.0% |
| 1750 | ± 50 / ± 100 | 53.4 ± 5% | 1.49 ± 5% | 4.68 | 4.68 | 4.68 | 0.63 | 3.03 ± 11.0% |
| 1900 | ± 50 / ± 100 | 53.3 ± 5% | 1.52 ± 5% | 4.46 | 4.46 | 4.46 | 0.85 | 2.44 ± 11.0% |
| 2450 | ± 50 / ± 100 | 52.7 ± 5% | 1.95 ± 5% | 4.07 | 4.07 | 4.07 | 0.99 | 1.40 ± 11.0% |


^c The validity of ± 100 MHz only applies for DASY v4.4 and higher (see Page 2). The uncertainty is the RSS of the ConvF uncertainty at calibration frequency and the uncertainty for the indicated frequency band.

ET3DV6 SN:1782

April 28, 2010

Frequency Response of E-Field

(TEM-Cell:ifi110 EXX, Waveguide: R22)


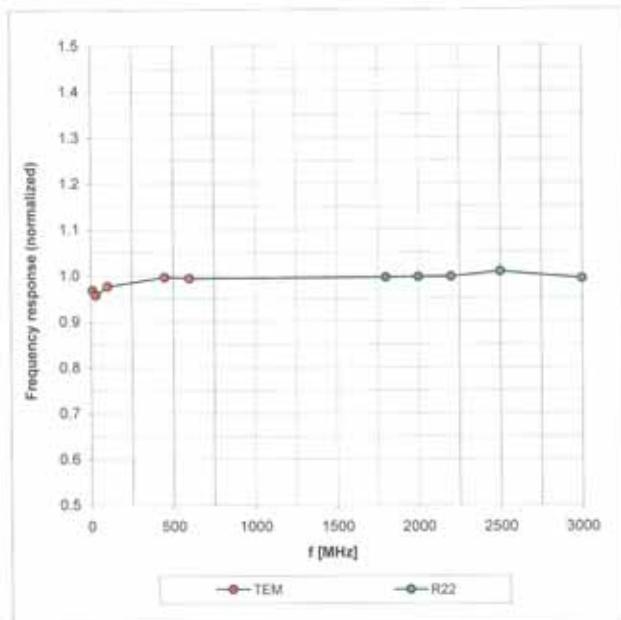


Uncertainty of Frequency Response of E-field: $\pm 6.3\%$ ($k=2$)

ET3DV6 SN:1782

April 28, 2010

Receiving Pattern (ϕ), $\theta = 0^\circ$

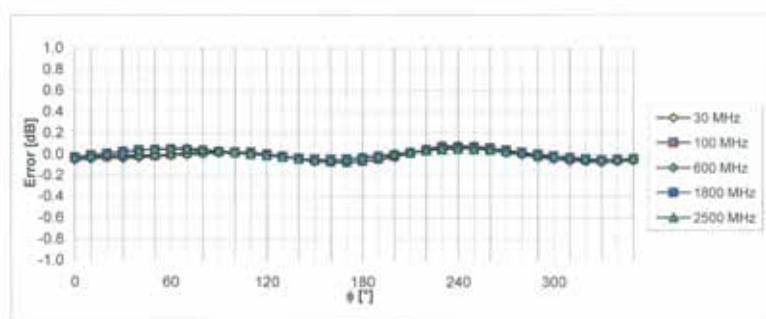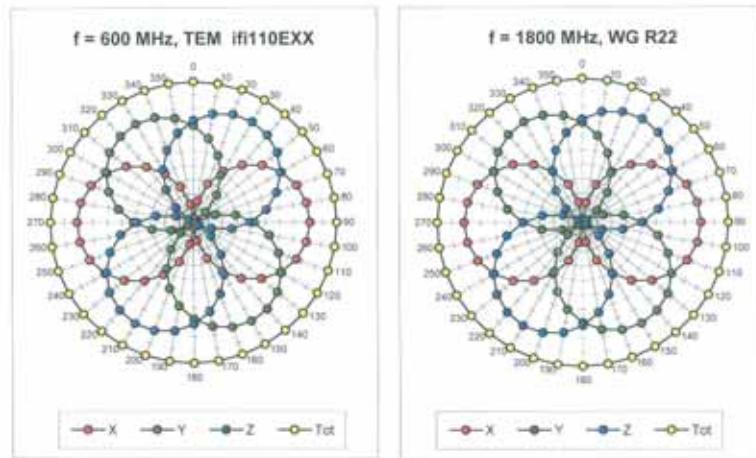


Uncertainty of Axial Isotropy Assessment: $\pm 0.5\%$ ($k=2$)

ET3DV6 SN:1782

April 28, 2010

Dynamic Range $f(\text{SAR}_{\text{head}})$
(Waveguide R22, $f = 1800$ MHz)

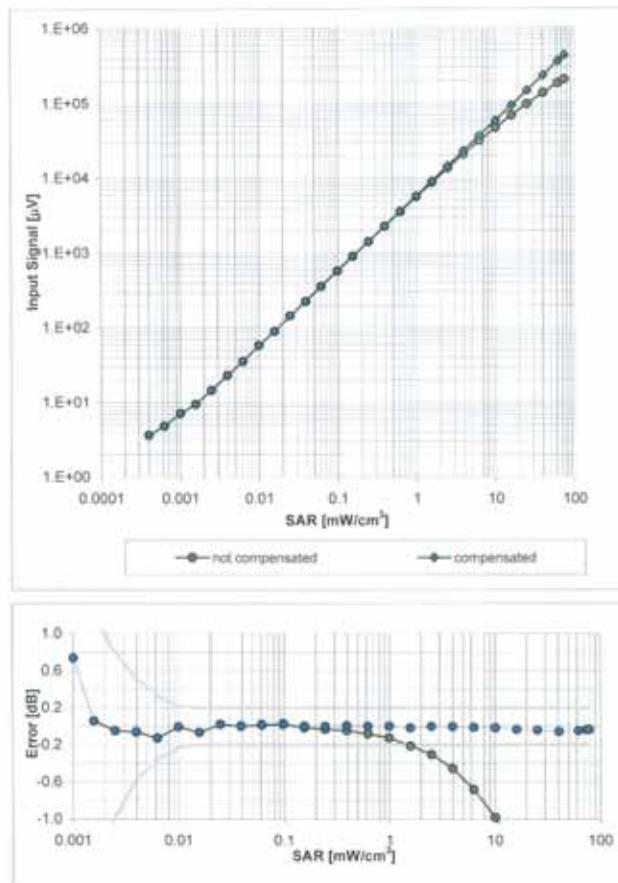


Uncertainty of Linearity Assessment: $\pm 0.6\%$ ($k=2$)


ET3DV6 SN:1782

April 28, 2010

Conversion Factor Assessment

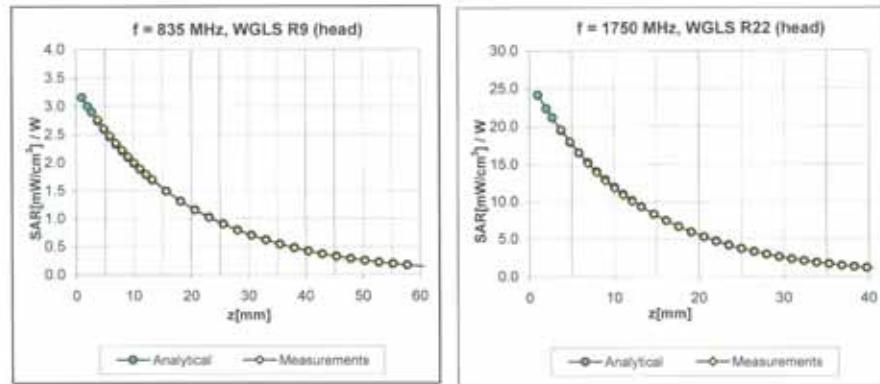

Deviation from Isotropy in HSL

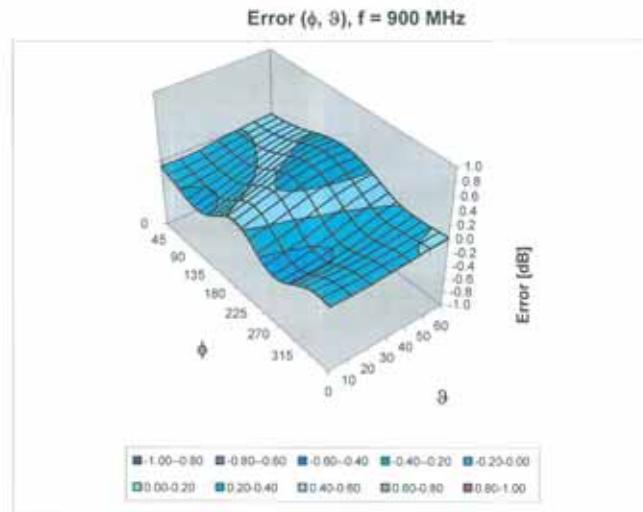

Uncertainty of Spherical Isotropy Assessment: $\pm 2.6\%$ ($k=2$)

ET3DV6 SN:1782

April 28, 2010

Other Probe Parameters

| | |
|---|----------------|
| Sensor Arrangement | Triangular |
| Connector Angle (") | Not applicable |
| Mechanical Surface Detection Mode | enabled |
| Optical Surface Detection Mode | disabled |
| Probe Overall Length | 337 mm |
| Probe Body Diameter | 10 mm |
| Tip Length | 10 mm |
| Tip Diameter | 6.8 mm |
| Probe Tip to Sensor X Calibration Point | 2.7 mm |
| Probe Tip to Sensor Y Calibration Point | 2.7 mm |
| Probe Tip to Sensor Z Calibration Point | 2.7 mm |
| Recommended Measurement Distance from Surface | 4 mm |

-DAE Calibration Certificate

Calibration Laboratory of
Schmid & Partner
Engineering AG
Zeughausstrasse 43, 8004 Zurich, Switzerland



S Schweizerischer Kalibrierdienst
C Service suisse d'étalonnage
S Servizio svizzero di taratura
S Swiss Calibration Service

Accredited by the Swiss Accreditation Service (SAS)
The Swiss Accreditation Service is one of the signatories to the EA
Multilateral Agreement for the recognition of calibration certificates

Accreditation No.: **SCS 108**Client **SGS KES**Certificate No: **DAE3-567_Dec09****CALIBRATION CERTIFICATE**Object: **DAE3 - SD 000 D03 AA - SN: 567**Calibration procedure(s): **QA CAL-06.v12**
Calibration procedure for the data acquisition electronics (DAE)Calibration date: **December 9, 2009**

This calibration certificate documents the traceability to national standards, which realize the physical units of measurements (SI).
The measurements and the uncertainties with confidence probability are given on the following pages and are part of the certificate.

All calibrations have been conducted in the closed laboratory facility; environment temperature (22 ± 3)°C and humidity < 70%.

Calibration Equipment used (M&TE critical for calibration)

| Primary Standards | ID # | Cal Date (Certificate No.) | Scheduled Calibration |
|-------------------------------|--------------------|----------------------------|------------------------|
| Keithley Multimeter Type 2001 | SN: 0810278 | 1-Oct-09 (No: 9055) | Oct-10 |
| Secondary Standards | ID # | Check Date (in house) | Scheduled Check |
| Calibrator Box V1.1 | SE UMS 006 AB 1004 | 05-Jun-09 (in house check) | In house check: Jun-10 |

| Calibrated by: | Name | Function | Signature |
|----------------|-------------------|--------------|-----------|
| | Dominique Steffen | Technician | |
| Approved by: | Fin Bomholt | R&D Director | |

Issued: December 9, 2009

This calibration certificate shall not be reproduced except in full without written approval of the laboratory.

Calibration Laboratory of
Schmid & Partner
Engineering AG
Zeughausstrasse 43, 8004 Zurich, Switzerland



S Schweizerischer Kalibrierdienst
C Service suisse d'étalonnage
S Servizio svizzero di taratura
S Swiss Calibration Service

Accredited by the Swiss Accreditation Service (SAS)

The Swiss Accreditation Service is one of the signatories to the EA
Multilateral Agreement for the recognition of calibration certificates

Accreditation No.: SCS 108

Glossary

| | |
|-----------------|---|
| DAE | data acquisition electronics |
| Connector angle | information used in DASY system to align probe sensor X to the robot coordinate system. |

Methods Applied and Interpretation of Parameters

- *DC Voltage Measurement*: Calibration Factor assessed for use in DASY system by comparison with a calibrated instrument traceable to national standards. The figure given corresponds to the full scale range of the voltmeter in the respective range.
- *Connector angle*: The angle of the connector is assessed measuring the angle mechanically by a tool inserted. Uncertainty is not required.
- The following parameters as documented in the Appendix contain technical information as a result from the performance test and require no uncertainty.
 - *DC Voltage Measurement Linearity*: Verification of the Linearity at +10% and -10% of the nominal calibration voltage. Influence of offset voltage is included in this measurement.
 - *Common mode sensitivity*: Influence of a positive or negative common mode voltage on the differential measurement.
 - *Channel separation*: Influence of a voltage on the neighbor channels not subject to an input voltage.
 - *AD Converter Values with inputs shorted*: Values on the internal AD converter corresponding to zero input voltage
 - *Input Offset Measurement*: Output voltage and statistical results over a large number of zero voltage measurements.
 - *Input Offset Current*: Typical value for information; Maximum channel input offset current, not considering the input resistance.
 - *Input resistance*: DAE input resistance at the connector, during internal auto-zeroing and during measurement.
 - *Low Battery Alarm Voltage*: Typical value for information. Below this voltage, a battery alarm signal is generated.
 - *Power consumption*: Typical value for information. Supply currents in various operating modes.

DC Voltage Measurement

A/D - Converter Resolution nominal

High Range: 1LSB = $6.1\mu\text{V}$, full range = $-100\ldots+300\text{ mV}$
Low Range: 1LSB = 61nV , full range = $-1\ldots+3\text{mV}$

DASY measurement parameters: Auto Zero Time: 3 sec; Measuring time: 3 sec

| Calibration Factors | X | Y | Z |
|---------------------|-----------------------------------|-----------------------------------|-----------------------------------|
| High Range | $404.546 \pm 0.1\% \text{ (k=2)}$ | $404.281 \pm 0.1\% \text{ (k=2)}$ | $404.334 \pm 0.1\% \text{ (k=2)}$ |
| Low Range | $3.96697 \pm 0.7\% \text{ (k=2)}$ | $3.97066 \pm 0.7\% \text{ (k=2)}$ | $3.95911 \pm 0.7\% \text{ (k=2)}$ |

Connector Angle

| | |
|---|-------------------------|
| Connector Angle to be used in DASY system | $7.5^\circ \pm 1^\circ$ |
|---|-------------------------|

Appendix

1. DC Voltage Linearity

| High Range | Reading (µV) | Difference (µV) | Error (%) |
|-------------------|--------------|-----------------|-----------|
| Channel X + Input | 200002.8 | -1.89 | -0.00 |
| Channel X + Input | 19998.11 | -1.59 | -0.01 |
| Channel X - Input | -19992.89 | 7.71 | -0.04 |
| Channel Y + Input | 199957.5 | -46.16 | -0.02 |
| Channel Y + Input | 19992.42 | -7.98 | -0.04 |
| Channel Y - Input | -19994.34 | 4.96 | -0.02 |
| Channel Z + Input | 199931.6 | -61.88 | -0.03 |
| Channel Z + Input | 19990.70 | -8.50 | -0.04 |
| Channel Z - Input | -19992.89 | -0.04 | -0.04 |

| Low Range | Reading (µV) | Difference (µV) | Error (%) |
|-------------------|--------------|-----------------|-----------|
| Channel X + Input | 2000.7 | 0.61 | 0.03 |
| Channel X + Input | 199.14 | -0.86 | -0.43 |
| Channel X - Input | -200.82 | -0.72 | 0.36 |
| Channel Y + Input | 2000.0 | -0.11 | -0.01 |
| Channel Y + Input | 198.97 | -1.13 | -0.56 |
| Channel Y - Input | -201.08 | -1.18 | 0.59 |
| Channel Z + Input | 1999.4 | -0.87 | -0.04 |
| Channel Z + Input | 198.62 | -1.48 | -0.74 |
| Channel Z - Input | -201.26 | -1.36 | 0.68 |

2. Common mode sensitivity

DASY measurement parameters: Auto Zero Time: 3 sec; Measuring time: 3 sec

| | Common mode Input Voltage (mV) | High Range Average Reading (µV) | Low Range Average Reading (µV) |
|-----------|-----------------------------------|------------------------------------|-----------------------------------|
| Channel X | 200 | 3.98 | 2.30 |
| | -200 | -0.74 | -2.83 |
| Channel Y | 200 | -0.27 | -0.39 |
| | -200 | -0.32 | -0.95 |
| Channel Z | 200 | 4.97 | 4.65 |
| | -200 | -6.07 | -6.68 |

3. Channel separation

DASY measurement parameters: Auto Zero Time: 3 sec; Measuring time: 3 sec

| | Input Voltage (mV) | Channel X (µV) | Channel Y (µV) | Channel Z (µV) |
|-----------|--------------------|----------------|----------------|----------------|
| Channel X | 200 | + | 1.57 | -1.52 |
| Channel Y | 200 | 3.06 | + | 3.39 |
| Channel Z | 200 | 3.26 | -0.28 | + |

4. AD-Converter Values with inputs shorted

DASY measurement parameters: Auto Zero Time: 3 sec; Measuring time: 3 sec

| | High Range (LSB) | Low Range (LSB) |
|-----------|------------------|-----------------|
| Channel X | 16355 | 16407 |
| Channel Y | 16166 | 16176 |
| Channel Z | 15925 | 16100 |

5. Input Offset Measurement

DASY measurement parameters: Auto Zero Time: 3 sec; Measuring time: 3 sec

input 10MΩ

| | Average (µV) | min. Offset (µV) | max. Offset (µV) | Std. Deviation (µV) |
|-----------|--------------|------------------|------------------|---------------------|
| Channel X | -0.19 | -1.19 | 0.58 | 0.37 |
| Channel Y | -0.59 | -1.52 | 0.73 | 0.36 |
| Channel Z | -1.05 | -2.18 | -0.05 | 0.34 |

6. Input Offset Current

Nominal Input circuitry offset current on all channels: <25fA

7. Input Resistance

| | Zeroing (MΩ) | Measuring (MΩ) |
|-----------|--------------|----------------|
| Channel X | 0.2000 | 203.2 |
| Channel Y | 0.1999 | 202.8 |
| Channel Z | 0.1999 | 201.0 |

8. Low Battery Alarm Voltage (verified during pre test)

| Typical values | Alarm Level (VDC) |
|----------------|-------------------|
| Supply (+ Vcc) | +7.9 |
| Supply (- Vcc) | -7.6 |

9. Power Consumption (verified during pre test)

| Typical values | Switched off (mA) | Stand by (mA) | Transmitting (mA) |
|----------------|-------------------|---------------|-------------------|
| Supply (+ Vcc) | +0.0 | +6 | +14 |
| Supply (- Vcc) | -0.01 | -8 | -9 |

- 2450 MHz Dipole Calibration Certificate

Calibration Laboratory of
Schmid & Partner
Engineering AG
Zeughausstrasse 43, 8004 Zurich, Switzerland



S Schweizerischer Kaliibrierdienst
C Service suisse d'étalonnage
S Servizio svizzero di taratura
S Swiss Calibration Service

Accredited by the Swiss Accreditation Service (SAS)
The Swiss Accreditation Service is one of the signatories to the EA
Multilateral Agreement for the recognition of calibration certificates

Accreditation No.: **SCS 108**Client **SGS (Dymstec)**Certificate No: **D2450V2-734_May10****CALIBRATION CERTIFICATE**Object **D2450V2 - SN: 734**Calibration procedure(s) **QA CAL-05.v7**
Calibration procedure for dipole validation kitsCalibration date: **May 27, 2010**

This calibration certificate documents the traceability to national standards, which realize the physical units of measurements (SI).
The measurements and the uncertainties with confidence probability are given on the following pages and are part of the certificate.

All calibrations have been conducted in the closed laboratory facility: environment temperature (22 ± 3)°C and humidity < 70%.

Calibration Equipment used (M&TE critical for calibration)

| Primary Standards | ID # | Cal Date (Certificate No.) | Scheduled Calibration |
|-----------------------------|--------------------|--------------------------------|-----------------------|
| Power meter EPM-442A | GB37480704 | 06-Oct-09 (No. 217-01086) | Oct-10 |
| Power sensor HP 8481A | US37292783 | 06-Oct-09 (No. 217-01086) | Oct-10 |
| Reference 20 dB Attenuator | SN: 5086 (20g) | 30-Mar-10 (No. 217-01158) | Mar-11 |
| Type-N mismatch combination | SN: 5047.2 / 06327 | 30-Mar-10 (No. 217-01162) | Mar-11 |
| Reference Probe ES3DV3 | SN: 3205 | 30-Apr-10 (No. ES3-3205_Apr10) | Apr-11 |
| DAE4 | SN: 601 | 02-Mar-10 (No. DAE4-601_Mar10) | Mar-11 |

| Secondary Standards | ID # | Check Date (in house) | Scheduled Check |
|---------------------------|------------------|-----------------------------------|------------------------|
| Power sensor HP 8481A | MY41092317 | 18-Oct-02 (in house check Oct-09) | In house check: Oct-11 |
| RF generator R&S SMT-06 | 100065 | 4-Aug-99 (in house check Oct-09) | In house check: Oct-11 |
| Network Analyzer HP 8753E | US37390585 S4206 | 18-Oct-01 (in house check Oct-09) | In house check: Oct-10 |

| Calibrated by: | Name | Function | Signature |
|----------------|-------------|-----------------------|-----------|
| | Dimce Iliev | Laboratory Technician | |

| Approved by: | Name | Function | Signature |
|--------------|---------------|-------------------|-----------|
| | Kalja Pokovic | Technical Manager | |

Issued: May 27, 2010

This calibration certificate shall not be reproduced except in full without written approval of the laboratory.

Calibration Laboratory of
Schmid & Partner
Engineering AG
Zeughausstrasse 43, 8004 Zurich, Switzerland



S Schweizerischer Kalibrierdienst
C Service suisse d'étalonnage
S Servizio svizzero di taratura
S Swiss Calibration Service

Accredited by the Swiss Accreditation Service (SAS)
The Swiss Accreditation Service is one of the signatories to the EA
Multilateral Agreement for the recognition of calibration certificates

Accreditation No.: SCS 108

Glossary:

| | |
|-------|---------------------------------|
| TSL | tissue simulating liquid |
| ConvF | sensitivity in TSL / NORM x,y,z |
| N/A | not applicable or not measured |

Calibration is Performed According to the Following Standards:

- a) IEEE Std 1528-2003, "IEEE Recommended Practice for Determining the Peak Spatial-Averaged Specific Absorption Rate (SAR) in the Human Head from Wireless Communications Devices: Measurement Techniques", December 2003
- b) IEC 62209-1, "Procedure to measure the Specific Absorption Rate (SAR) for hand-held devices used in close proximity to the ear (frequency range of 300 MHz to 3 GHz)", February 2005
- c) Federal Communications Commission Office of Engineering & Technology (FCC OET), "Evaluating Compliance with FCC Guidelines for Human Exposure to Radiofrequency Electromagnetic Fields; Additional Information for Evaluating Compliance of Mobile and Portable Devices with FCC Limits for Human Exposure to Radiofrequency Emissions", Supplement C (Edition 01-01) to Bulletin 65

Additional Documentation:

- d) DASY4/5 System Handbook

Methods Applied and Interpretation of Parameters:

- *Measurement Conditions:* Further details are available from the Validation Report at the end of the certificate. All figures stated in the certificate are valid at the frequency indicated.
- *Antenna Parameters with TSL:* The dipole is mounted with the spacer to position its feed point exactly below the center marking of the flat phantom section, with the arms oriented parallel to the body axis.
- *Feed Point Impedance and Return Loss:* These parameters are measured with the dipole positioned under the liquid filled phantom. The impedance stated is transformed from the measurement at the SMA connector to the feed point. The Return Loss ensures low reflected power. No uncertainty required.
- *Electrical Delay:* One-way delay between the SMA connector and the antenna feed point. No uncertainty required.
- *SAR measured:* SAR measured at the stated antenna input power.
- *SAR normalized:* SAR as measured, normalized to an input power of 1 W at the antenna connector.
- *SAR for nominal TSL parameters:* The measured TSL parameters are used to calculate the nominal SAR result.

Measurement Conditions

DASY system configuration, as far as not given on page 1.

| | | |
|------------------------------|---------------------------|-------------|
| DASY Version | DASY5 | V5.2 |
| Extrapolation | Advanced Extrapolation | |
| Phantom | Modular Flat Phantom V4.9 | |
| Distance Dipole Center - TSL | 10 mm | with Spacer |
| Zoom Scan Resolution | dx, dy, dz = 5 mm | |
| Frequency | 2450 MHz ± 1 MHz | |

Head TSL parameters

The following parameters and calculations were applied.

| | Temperature | Permittivity | Conductivity |
|----------------------------------|-----------------|--------------|------------------|
| Nominal Head TSL parameters | 22.0 °C | 39.2 | 1.80 mho/m |
| Measured Head TSL parameters | (22.0 ± 0.2) °C | 39.0 ± 6 % | 1.76 mho/m ± 6 % |
| Head TSL temperature during test | (21.5 ± 0.2) °C | ---- | ---- |

SAR result with Head TSL

| SAR averaged over 1 cm ³ (1 g) of Head TSL | Condition | |
|---|--------------------|---------------------------|
| SAR measured | 250 mW input power | 12.8 mW / g |
| SAR normalized | normalized to 1W | 51.2 mW / g |
| SAR for nominal Head TSL parameters | normalized to 1W | 51.7 mW /g ± 17.0 % (k=2) |

| SAR averaged over 10 cm ³ (10 g) of Head TSL | Condition | |
|---|--------------------|---------------------------|
| SAR measured | 250 mW input power | 6.03 mW / g |
| SAR normalized | normalized to 1W | 24.1 mW / g |
| SAR for nominal Head TSL parameters | normalized to 1W | 24.2 mW /g ± 16.5 % (k=2) |

Body TSL parameters

The following parameters and calculations were applied.

| | Temperature | Permittivity | Conductivity |
|----------------------------------|-----------------|--------------|------------------|
| Nominal Body TSL parameters | 22.0 °C | 52.7 | 1.95 mho/m |
| Measured Body TSL parameters | (22.0 ± 0.2) °C | 53.6 ± 6 % | 1.97 mho/m ± 6 % |
| Body TSL temperature during test | (21.8 ± 0.2) °C | ---- | ---- |

SAR result with Body TSL

| SAR averaged over 1 cm ³ (1 g) of Body TSL | Condition | |
|---|--------------------|----------------------------|
| SAR measured | 250 mW input power | 13.4 mW / g |
| SAR normalized | normalized to 1W | 53.6 mW / g |
| SAR for nominal Body TSL parameters | normalized to 1W | 53.5 mW / g ± 17.0 % (k=2) |

| SAR averaged over 10 cm ³ (10 g) of Body TSL | Condition | |
|---|--------------------|----------------------------|
| SAR measured | 250 mW input power | 6.31 mW / g |
| SAR normalized | normalized to 1W | 25.2 mW / g |
| SAR for nominal Body TSL parameters | normalized to 1W | 25.2 mW / g ± 16.5 % (k=2) |

Appendix

Antenna Parameters with Head TSL

| | |
|--------------------------------------|-----------------------------|
| Impedance, transformed to feed point | $53.8 \Omega + 3.2 j\Omega$ |
| Return Loss | - 26.4 dB |

Antenna Parameters with Body TSL

| | |
|--------------------------------------|-----------------------------|
| Impedance, transformed to feed point | $49.8 \Omega + 4.4 j\Omega$ |
| Return Loss | - 27.1 dB |

General Antenna Parameters and Design

| | |
|----------------------------------|----------|
| Electrical Delay (one direction) | 1.153 ns |
|----------------------------------|----------|

After long term use with 100W radiated power, only a slight warming of the dipole near the feedpoint can be measured.

The dipole is made of standard semirigid coaxial cable. The center conductor of the feeding line is directly connected to the second arm of the dipole. The antenna is therefore short-circuited for DC-signals.
No excessive force must be applied to the dipole arms, because they might bend or the soldered connections near the feedpoint may be damaged.

Additional EUT Data

| | |
|-----------------|--------------|
| Manufactured by | SPEAG |
| Manufactured on | May 07, 2003 |

DASY5 Validation Report for Head TSL

Date/Time: 25.05.2010 14:48:31

Test Laboratory: SPEAG, Zurich, Switzerland

DUT: Dipole 2450 MHz; Type: D2450V2; Serial: D2450V2 - SN:734

Communication System: CW; Frequency: 2450 MHz; Duty Cycle: 1:1

Medium: HSL U11 BB

Medium parameters used: $f = 2450$ MHz; $\sigma = 1.76$ mho/m; $\epsilon_r = 39$; $\rho = 1000$ kg/m³

Phantom section: Flat Section

Measurement Standard: DASY5 (IEEE/IEC/ANSI C63.19-2007)

DASY5 Configuration:

- Probe: ES3DV3 - SN3205; ConvF(4.53, 4.53, 4.53); Calibrated: 30.04.2010
- Sensor-Surface: 3mm (Mechanical Surface Detection)
- Electronics: DAE4 Sn601; Calibrated: 02.03.2010
- Phantom: Flat Phantom 5.0 (front); Type: QD000P50AA; Serial: 1001
- Measurement SW: DASY5, V5.2 Build 162; SEMCAD X Version 14.0 Build 61


Pin=250 mW /d=10mm, dist=3.0mm (ES-Probe)/Zoom Scan (7x7x7) /Cube 0: Measurement grid: dx=5mm, dy=5mm, dz=5mm

Reference Value = 101.2 V/m; Power Drift = 0.030 dB

Peak SAR (extrapolated) = 26.1 W/kg


SAR(1 g) = 12.8 mW/g; SAR(10 g) = 6.03 mW/g

Maximum value of SAR (measured) = 16.7 mW/g

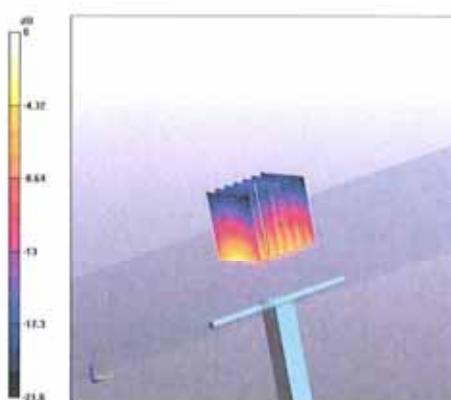

0 dB = 16.7mW/g

Impedance Measurement Plot for Head TSL

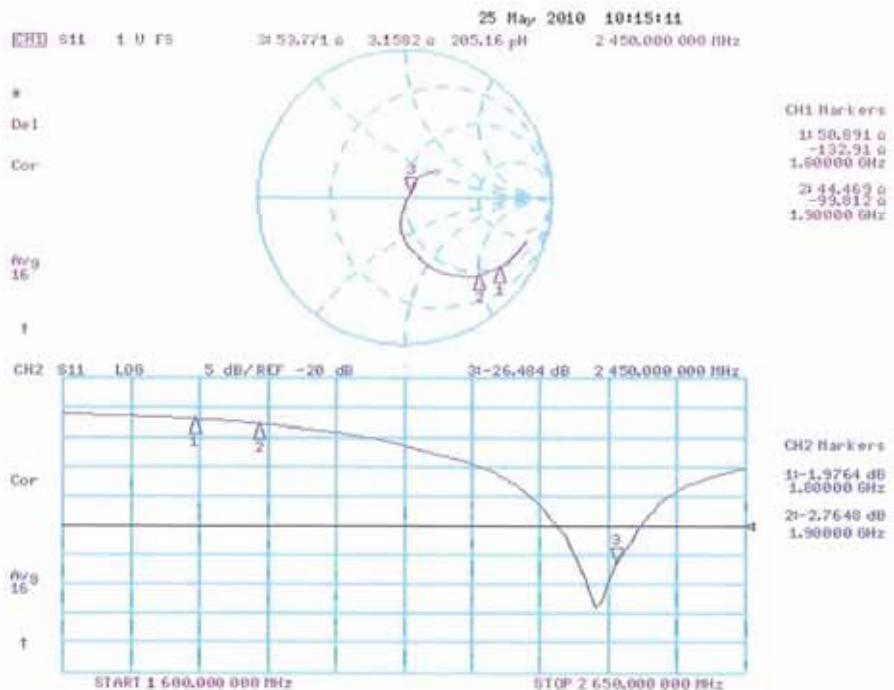

DASY5 Validation Report for Body

Date/Time: 27.05.2010 10:14:45

Test Laboratory: SPEAG, Zurich, Switzerland

DUT: Dipole 2450 MHz; Type: D2450V2; Serial: D2450V2 - SN:734

Communication System: CW; Frequency: 2450 MHz; Duty Cycle: 1:1

Medium: MSL U11 BB

Medium parameters used: $f = 2450$ MHz; $\sigma = 1.97$ mho/m; $\epsilon_r = 53.6$; $\rho = 1000$ kg/m³

Phantom section: Flat Section

Measurement Standard: DASY5 (IEEE/IEC/ANSI C63.19-2007)

DASY5 Configuration:

- Probe: ES3DV3 - SN3205; ConvF(4.31, 4.31, 4.31); Calibrated: 30.04.2010
- Sensor-Surface: 3mm (Mechanical Surface Detection)
- Electronics: DAE4 Sn601; Calibrated: 02.03.2010
- Phantom: Flat Phantom 5.0 (back); Type: QD000P50AA; Serial: 1002
- Measurement SW: DASY5, V5.2 Build 162; SEMCAD X Version 14.0 Build 61


Pin=250 mW /d=10mm, dist=3.0mm (ES-Probe)/Zoom Scan (7x7x7) /Cube 0: Measurement grid: dx=5mm, dy=5mm, dz=5mm

Reference Value = 96.7 V/m; Power Drift = -0.030 dB

Peak SAR (extrapolated) = 27.3 W/kg

SAR(1 g) = 13.4 mW/g; SAR(10 g) = 6.31 mW/g

Maximum value of SAR (measured) = 17.4 mW/g

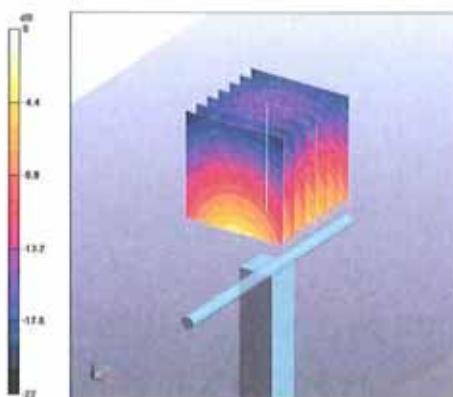

0 dB = 17.4mW/g

Impedance Measurement Plot for Body TSL

