

RF TEST REPORT



Report No.: FCC,IC_SAR_SL14031101-SLX-004 Rev1.0
Supersede Report No.: FCC,IC_SAR_SL14031101-SLX-004

Applicant	Hospira, Inc.
Product Name	SDIO Wireless Module
Model No.	SX-SDMAN
Test Standard	47CFR 2.1093, IEEE C95.1-1999 OET 65 C (Ed 01-01), RSS 102 Issue 4.0, IEEE 1528: 2003, IEC 62209-2: 2010
Test Method	IEEE 1528: 2003, IEC 62209-2: 2010 KDB 447498 D01 General RF Exposure Guidance v05r01 KDB 248227 SAR measurement procedures for 802.11 a/b/g TX KDB 865664 SAR Measurement Requirements for 3 to 6 GHz v05r01
Date of test	04/29/2014 - 05/01/2014
Issue Date	06/10/2014
Test Result	<u>Pass</u> Fail
Equipment complied with the specification	[x]
Equipment did not comply with the specification	[]
	
David Zhang	Nima Molaei
Test Engineer	Engineer Reviewer
This test report may be reproduced in full only Test result presented in this test report is applicable to the tested sample only	

Issued By:
SIEMIC Laboratories
775 Montague Expressway, Milpitas, 95035 CA



775 Montague Expressway, Milpitas, CA 95035, USA • Phone: (+1) 408 526 1188 • Facsimile (+1) 408 526 1088

Visit us at: www.siemic.com; Follow us at:



Laboratory Introduction

SIEMIC, headquartered in the heart of Silicon Valley, with superior facilities in US and Asia, is one of the leading independent testing and certification facilities providing customers with one-stop shop services for Compliance Testing and Global Certifications.



In addition to testing and certification, SIEMIC provides initial design reviews and compliance management throughout a project. Our extensive experience with China, Asia Pacific, North America, European, and International compliance requirements, assures the fastest, most cost effective way to attain regulatory compliance for the global markets.

Accreditations for Conformity Assessment

Country/Region	Accreditation Body	Scope
USA	FCC, A2LA	EMC , RF/Wireless , Telecom
Canada	IC, A2LA, NIST	EMC, RF/Wireless , Telecom
Taiwan	BSMI , NCC , NIST	EMC, RF, Telecom , Safety
Hong Kong	OFTA , NIST	RF/Wireless ,Telecom
Australia	NATA, NIST	EMC, RF, Telecom , Safety
Korea	KCC/RRR, NIST	EMI, EMS, RF , Telecom, Safety
Japan	VCCI, JATE, TELEC, RFT	EMI, RF/Wireless, Telecom
Mexico	NOM, COFETEL, Caniety	Safety, EMC , RF/Wireless, Telecom
Europe	A2LA, NIST	EMC, RF, Telecom , Safety

Accreditations for Product Certifications

Country	Accreditation Body	Scope
USA	FCC TCB, NIST	EMC , RF , Telecom
Canada	IC FCB , NIST	EMC , RF , Telecom
Singapore	iDA, NIST	EMC , RF , Telecom
EU	NB	EMC & R&TTE Directive
Japan	MIC (RCB 208)	RF , Telecom
HongKong	OFTA (US002)	RF , Telecom

Test report No.	FCC,IC_SAR_SL14031101-SLX-004 Rev1.0
Page	2 of 100
FCC ID	STJ-SDMAN
IC ID	5627A-SDMAN

CONTENTS

1	REPORT REVISION HISTORY	3
2	EXECUTIVE SUMMARY	4
3	CUSTOMER INFORMATION	4
4	TEST SITE INFORMATION	4
5	MODIFICATION	4
6	EUT INFORMATION	5
7	ACCESSORIES/SOFTWARE AND CABLING DESCRIPTION.....	8
8	EUT PHOTOS.....	9
9	KDB CONSIDERATION	11
10	TEST SUMMARY.....	15
11	SAR INTRODUCTION	16
12	SAR MEASUREMENT SETUP	17
13	MEASUREMENT UNCERTAINTY	25
14	LIQUID VALIDATION.....	27
15	SYSTEM VALIDATION AND SYSTEM VERIFICATION	29
16	MEASUREMENTS, EXAMINATION AND DERIVED RESULTS	32
	ANNEX A. TEST INSTRUMENT.....	37
	ANNEX B. USER MANUAL, BLOCK & CIRCUIT DIAGRAM	38
	ANNEX C. SIEMIC ACCREDITATION	39
	ANNEX D. CALIBRATION REPORT	42
	ANNEX E. SAR TEST PLOTS.....	81

Test report No.	FCC,IC_SAR_SL14031101-SLX-004 Rev1.0
Page	3 of 100
FCC ID	STJ-SDMAN
IC ID	5627A-SDMAN

1 Report Revision History

Report No.	Report Version	Description	Issue Date
FCC,IC_SAR_SL14031101-SLX-004	NONE	Original	05/02/2014
FCC,IC_SAR_SL14031101-SLX-004 Rev1.0	Rev1.0	Update applicant info and EUT photo	06/10/2014

Test report No.	FCC,IC_SAR_SL14031101-SLX-004 Rev1.0
Page	4 of 100
FCC ID	STJ-SDMAN
IC ID	5627A-SDMAN

2 Executive Summary

The purpose of this test programme was to demonstrate compliance of the FCC, IC certified radio module, SDIO Wireless Module (FCC ID: STJ-SDMAN, IC ID: 5627A-SDMAN), from Hospira, Inc., and Model: SX-SDMAN, to be installed inside portable host unit of Hospira, Inc., Wireless Infusion Pump, against the current Stipulated Standards. The SDIO Wireless Module to be installed inside portable host unit of Hospira, Inc., Wireless Infusion Pump, has demonstrated compliance with the 47 CFR Part 2 (2.1093), RSS 102 Issue 4.0, IEEE 1528: 2003 and IEC 62209-2: 2010, with 0cm separation distance to phantom.

3 Customer information

Applicant Name	:	Hospira, Inc.
Applicant Address	:	375 North Field Drive building H3, Lake Forest, IL. 60045
Manufacturer Name	:	Hospira, Inc.
Manufacturer Address	:	375 North Field Drive building H3, Lake Forest, IL. 60045

4 Test site information

Lab performing tests	:	SIEMIC Laboratories
Lab Address	:	775 Montague Expressway, Milpitas, CA 95035
FCC Test Site No.	:	881796
IC Test Site No.	:	4842D-2
VCCI Test Site No.	:	A0133

5 Modification

Index	Item	Description	Note
-	-	-	-

Test report No.	FCC,IC_SAR_SL14031101-SLX-004 Rev1.0
Page	5 of 100
FCC ID	STJ-SDMAN
IC ID	5627A-SDMAN

6 EUT Information

6.1 EUT Description

Product introduction				
This test report is for the Portable Module Approval of the SX-SDMAN with SAR for the Hospira, Inc., Wireless Infusion Pump. The module SX-SDMAN contains BT and WLAN function. It has 2 TX diversity antennas. It's to be installed into handheld host unit: Hospira, Inc., Wireless Infusion Pump. The Hospira, Inc., Wireless Infusion Pump is handheld device only; it's not designed to be worn onto human body. And there are no accessories or different battery options for it.				
Product Name	:	SDIO Wireless Module		
Model No.	:	SX-SDMAN		
Trade Name	:	Hospira		
Serial No.	:	20140203/3014322		
Input Power	:	3.3VDC		
Power Adapter Manu/Model	:	N/A		
Power Adapter SN	:	N/A		
Hardware version	:	N/A		
Software version	:	N/A		
Date of EUT received	:	Apr 27 th , 2014		
Equipment Class/ Category	:	DTS/UNII		
Clock Frequencies	:	26 MHz		
Port/Connectors	:	SDIO		
FCC ID	:	STJ-SDMAN		
IC ID	:	5627A-SDMAN		
Rated, Measured conducted RF output Power and SAR	:	Mode	Max Rated Power	Measured Max Power
	:	802.11b/g/n-2.4G	15dBm	13.25dBm
	:	802.11a	16dBm	15.35dBm
	:	802.11n	16dBm	16.88dBm
Wi-Fi Chipset	:	-		
Bluetooth Chipset	:	-		
IMEI	:	-		
Classification per Standard	:	Portable		
Co-located TX	:	N/A		

6.2 Radio Description

Radio Manu	Silex
Radio Model	SX-SDMAN
Radio Module SN	PW100125BA

Spec for Radio –

Radio Type	802.11b	802.11g	802.11a	802.11n-20M	802.11n-40M
Operating Frequency	2412-2462MHz	2412-2462MHz	5180-5320MHz 5470-5725MHz 5725-5825MHz	2412-2462MHz 5180-5320MHz 5470-5725MHz 5725-5825MHz	5190-5310MHz 5510-5670MHz 5755-5795MHz
Modulation	DSSS (CCK, DQPSK, DBPSK)	OFDM-CCK (BPSK, QPSK, 16QAM, 64QAM)	OFDM (BPSK, QPSK, 16QAM, 64QAM)	OFDM (BPSK, QPSK, 16QAM, 64QAM)	OFDM (BPSK, QPSK, 16QAM, 64QAM)
Channel Spacing	5MHz	5MHz	20MHz	5MHz(2.4GHz), 20MHz (5GHz)	40MHz
Number of Channels	11	11	21	11(2.4GH) 21 (5GHz)	14 (5GHz)
Antenna Type	Embedded PCB antenna				
Antenna Gain	4.2 dBi (2.4 GHz), 4.9 dBi (5 GHz)				
Antenna Connector Type	U.FL connector				

Channel list

Type		Channel No.	Frequency (MHz)	Available (Y/N)
802.11b/g/n-HT20	2412-2462	1	2412	Y
		2	2417	Y
		3	2422	Y
		4	2427	Y
		5	2432	Y
		6	2437	Y
		7	2442	Y
		8	2447	Y
		9	2452	Y
		10	2457	Y
		11	2462	Y
	2467-2472	12	2467	-
		13	2472	-
	2484	14	2484	-

Test report No.	FCC,IC_SAR_SL14031101-SLX-004 Rev1.0
Page	7 of 100
FCC ID	STJ-SDMAN
IC ID	5627A-SDMAN

Type		Channel No.	Frequency (MHz)	Available (Y/N)
802.11a/n-HT20	5150-5250MHz	36	5180	Y
		40	5200	Y
		44	5220	Y
		48	5240	Y
	5250-5350MHz	52	5260	Y
		56	5280	Y
		60	5300	Y
		64	5320	Y
	5470-5725MHz	100	5500	Y
		104	5520	Y
		108	5540	Y
		112	5560	Y
		116	5580	Y
		132	5660	Y
		136	5680	Y
		140	5700	Y
	5725-5825MHz	149	5745	Y
		153	5765	Y
		157	5785	Y
		161	5805	Y
		165	5825	Y

Type		Channel No.	Frequency (MHz)	Available (Y/N)
802.11n-HT40	5150-5250MHz	36,40	5190	Y
		40,44	5210	Y
		44,48	5230	Y
	5250-5350MHz	52,56	5270	Y
		56,60	5290	Y
		60,64	5310	Y
	5470-5725MHz	100,104	5510	Y
		104,108	5530	Y
		108,112	5550	Y
		112,116	5570	Y
		132,136	5670	Y
	5725-5825MHz	149,153	5755	Y
		153,157	5775	Y
		157,161	5795	Y

Test report No.	FCC,IC_SAR_SL14031101-SLX-004 Rev1.0
Page	8 of 100
FCC ID	STJ-SDMAN
IC ID	5627A-SDMAN

7 Accessories/Software and cabling Description

Accessories List

Index	Accessories Description	Model	Serial No.	Manu	Note
-	-	-	-	-	-

Battery options List

Index	Battery option Description	Model	Serial No.	Manu	Note
-	-	-	-	-	-

Test Software Description

Test Item	Software	Description
SAR	TTE test software	Set the EUT to different modulation and channel

Test report No.	FCC,IC_SAR_SL14031101-SLX-004 Rev1.0
Page	9 of 100
FCC ID	STJ-SDMAN
IC ID	5627A-SDMAN

8 EUT Photos

8.1 EUT Photos - External



Top Side View




Bottom Side View



Front Side View Side



Rear View Side

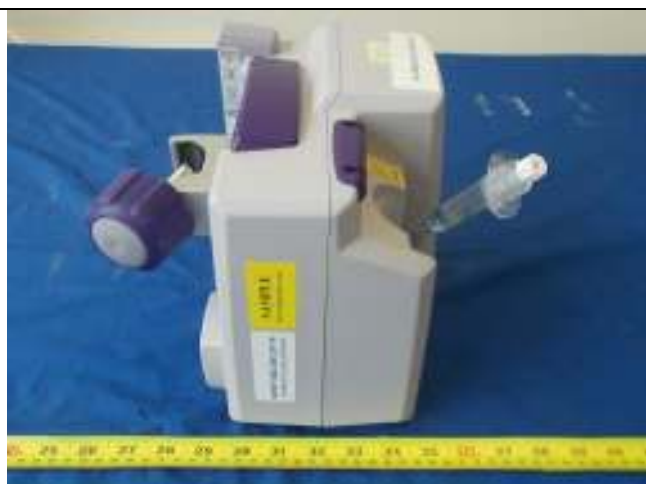




Left Side View



Right Side View

Test report No.	FCC,IC_SAR_SL14031101-SLX-004 Rev1.0
Page	10 of 100
FCC ID	STJ-SDMAN
IC ID	5627A-SDMAN

8.2 EUT Photos - Internal

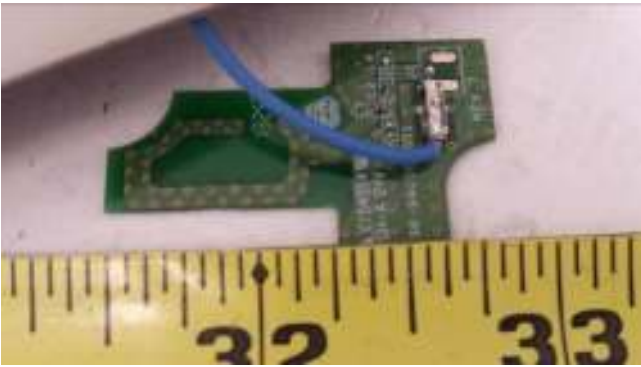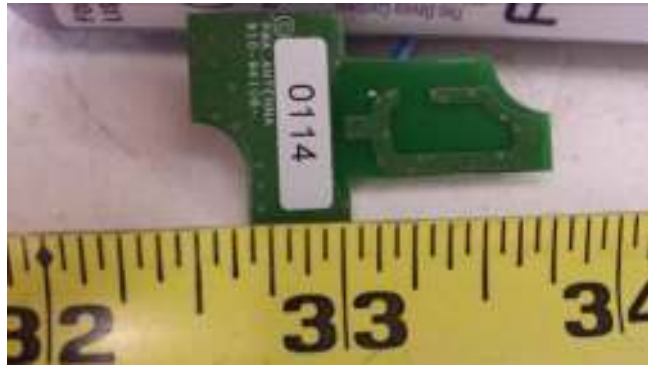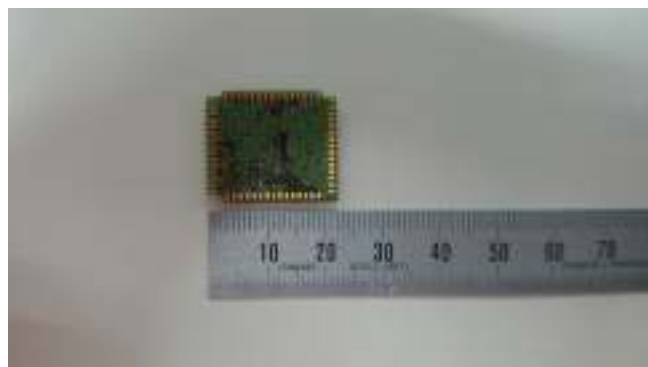	
Host Cover off view	Host Radio Board
	
Antenna Top View	Antenna Bottom View
	
Radio Module - Top zoom in view	Radio Module - Bottom zoom in view

Test report No.	FCC,IC_SAR_SL14031101-SLX-004 Rev1.0
Page	11 of 100
FCC ID	STJ-SDMAN
IC ID	5627A-SDMAN

9 KDB Consideration

Item	Applicable	Note
Applicable KDB	☒ 447498 D01 General RF Exposure Guidance v05r01	-
Exposure condition	☒ Portable ☐ Mobile ☐ Mixed Mobile & Portable	-
Exposure limit	☒ General/public ☐ Occupational	-
Operating Config	☒ Standalone ☐ Simultaneous Transmission	-
Enhanced Zoom Scan	☐ Yes ☒ No	-
Volume scan post-processing	☐ Yes ☒ No	-
Tune-up power	☒ Output power can't be more than 2dB lower than max tune-up power tolerance	-
Scale SAR to tune-up	☒ Scale SAR to the maximum tune-up tolerance limit	See SAR result table
Antenna variation	☐ Yes ☒ N/A	-
List of body-worn accessories	☐ Yes ☒ N/A	-

SAR Test exclusion

Testing of other required channels within the operating mode of a frequency band is not required when the reported 1-g or 10-g SAR for the mid-band or highest output power channel is:

transmission band is ≤ 100 MHz	☐ ≤ 0.8 W/kg or 2.0 W/kg, for 1-g or 10-g respectively
transmission band between 100 MHz-200 MHz	☐ ≤ 0.6 W/kg or 1.5 W/kg, for 1-g or 10-g respectively
transmission band is ≥ 200 MHz	☐ ≤ 0.4 W/kg or 1.0 W/kg, for 1-g or 10-g respectively

Not applicable for IC

Item	Applicable	Note
Applicable KDB	☒ 248227 SAR measurement procedures for 802.11 a/b/g TX	-
Power reduction	☐ Yes ☒ No	-
Test Reduction	☒ SAR is not required for 802.11g if maximum output power is less than $\frac{1}{4}$ dB higher than 802.11b.	802.11b has output 1/4dB higher than 802.11g/n-2.4GHz; 802.11a is not $\frac{1}{4}$ dB higher than 802.11n. So no testing for 802.11g and 802.11a.
BW selection	☐ Highest CH BW with highest output power. Lower BW is not required if power is $\frac{1}{4}$ dB less high.	20MHz and 40MHz BW were tested.
Data Rate	☒ Each CH should be tested at the lowest data rate. Higher data rate and higher order modulation is not required if power is $\frac{1}{4}$ dB less high.	See output power measurement result and SAR result
Duty Cycle scaling	☒ Yes ☐ No	See SAR result table
Switch diversity	☒ Yes ☐ No	-
	☒ Each antenna has 1g SAR < 1.2 W/kg, then the SAR only need to be measured with higher SAR antenna	-
MIMO	☐ Transmit simultaneously ☐ Each antenna is tested independently	Not applicable

Test report No.	FCC,IC_SAR_SL14031101-SLX-004 Rev1.0
Page	12 of 100
FCC ID	STJ-SDMAN
IC ID	5627A-SDMAN


Simultaneous SAR Evaluation

Test Case	TX Ant1	TX Ant2	Tx Ant3	The shortest distance between Ant & Ant2 (mm)
-	-	-	-	-
-	-	-	-	-
Remark:	N/A. EUT uses 2 TX diversity antennas, which won't transmit simultaneously.			

Radio & Antenna Location



Right Side View

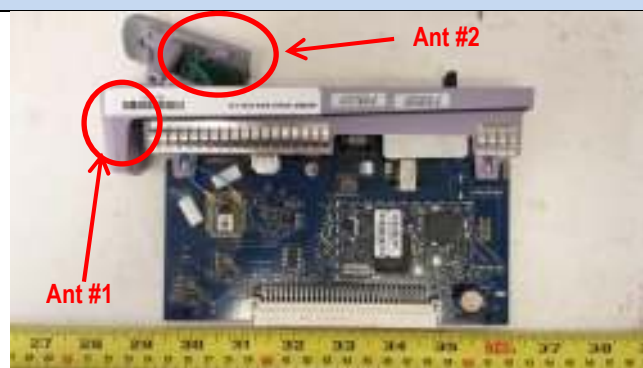

PCB containing Radio module & Antenna

Remark

1. EUT uses 2 TX diversity antennas, which won't transmit simultaneously.

Test report No.	FCC,IC_SAR_SL14031101-SLX-004 Rev1.0
Page	13 of 100
FCC ID	STJ-SDMAN
IC ID	5627A-SDMAN

EUT Test Position for SAR



Top position against flat phantom (Ant #1 location)
(separation distance – 0cm)



Right edge position against flat phantom (Ant #1 & #2 location)
(separation distance – 0cm)



Rear Position* (see Remark 3)

Remark:

- The Top, Right position was tested for SAR on following modes with higher output power,
- 802.11b
- 802.11n-HT40
The separation distance is 0cm.
- It's found that the top position is worst case. The low, mid and high channel of 802.11b mode, and 802.11n-HT40 mode were chosen for additional SAR measurement at this position.
- The Rear position was not tested because the handle provides enough separation for this position to be away from the human body when it's carried.

Test report No.	FCC,IC_SAR_SL14031101-SLX-004 Rev1.0
Page	14 of 100
FCC ID	STJ-SDMAN
IC ID	5627A-SDMAN

EUT Test Setup Photos



SAR Test System



Test setup – Top Position



Test setup – Right Position

Test report No.	FCC,IC_SAR_SL14031101-SLX-004 Rev1.0
Page	15 of 100
FCC ID	STJ-SDMAN
IC ID	5627A-SDMAN

10 Test Summary

Test Item	Test standard	Test Method/Procedure	Pass / Fail
SAR	47CFR 2.1093 IEEE C95.1-1999 OET 65 C (Ed 01-01)	IEEE 1528 – 2003 IEC 62209-2: 2010 KDB 447498 D01 General RF Exposure Guidance v05r01 KDB 248227 SAR measurement procedures for 802.11 a/b/g TX	☒ Pass ☐ N/A

11 SAR Introduction

Introduction

SAR is related to the rate at which energy is absorbed per unit mass in an object exposed to a radio field. The SAR distribution in a biological body is complicated and is usually carried out by experimental techniques or numerical modeling. The standard recommends limits for two tiers of groups, occupational/controlled and general population/uncontrolled, based on a person's awareness and ability to exercise control over his or her exposure. In general, occupational/controlled exposure limits are higher than the limits for general population/uncontrolled.

SAR Definition

Specific Absorption Rate is defined as the time derivative (rate) of the incremental energy (dW) absorbed by (dissipated in) an incremental mass (dm) contained in a volume element (dV) of a given density (ρ).

$$SAR = \frac{d}{dt} \left(\frac{dW}{dm} \right) = \frac{d}{dt} \left(\frac{dW}{\rho dV} \right)$$

SAR is expressed in units of watts per kilogram (W/kg). SAR can be related to the electric field at a point by

$$SAR = \frac{\sigma |E|^2}{\rho}$$

Where:

σ = conductivity of the tissue (S/m)
 ρ = mass density of the tissue (kg/m³)
 E = RMS electric field strength (V/m)


Test report No.	FCC,IC_SAR_SL14031101-SLX-004 Rev1.0
Page	17 of 100
FCC ID	STJ-SDMAN
IC ID	5627A-SDMAN

12 SAR Measurement Setup

Dosimetric Assessment System

These measurements were performed with the automated near-field scanning system OPENSAR from SATIMO. The system is based on a high precision robot (working range: 850 mm), which positions the probes with a positional repeatability of better than ± 0.02 mm. Special E- and H-field probes have been developed for measurements close to material discontinuity, the sensors of which are directly loaded with a Schottky diode and connected via highly resistive lines to the data acquisition unit.

Measurement System Diagram

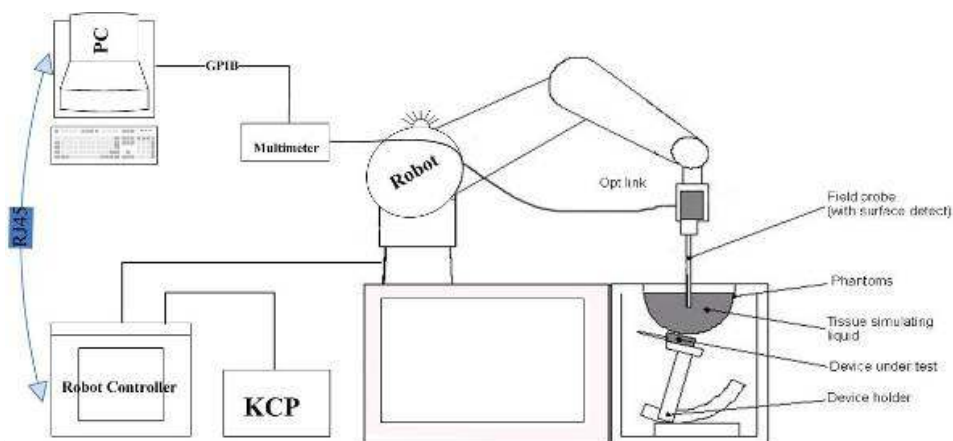

The OPENSAR

- A standard high precision 6-axis robot (KUKA) with controller and software.
- KUKA Control Panel (KCP).
- A dosimetric probe, i.e., an isotropic E-field probe optimized and calibrated for usage in tissue simulating liquid. The probe is equipped with an optical surface detector system.
- A computer operating Windows XP.
- OPENSAR software.
- Remote control with teaches pendant and additional circuitry for robot safety such as warning lamps, etc.
- The SAM phantom enabling testing left-hand right-hand and body usage.
- The Position device for handheld EUT.
- Tissue simulating liquid mixed according to the given recipes.
- System validation dipoles to validate the proper functioning of the system.

EP100 Probe

The SAR measurements were conducted with dosimetric probe (manufactured by SATIMO), designed in the classical triangular configuration and optimized for dosimetric evaluation. The probe has been calibrated according to the procedure described in SAR standard with accuracy of better than $\pm 10\%$.



It is connected to the KRC box on the robot arm and provides an automatic detection of the phantom surface. The 3D file of the phantom is include in OpenSAR software. The Video Positioning System allow the system to take the automatic reference and to move the probe safely and accurately on the phantom.

Parameter	Description
Frequency Range	100 MHz to 6 GHz
Linearity	0.25 dB (100 MHz to 6 GHz)
Directivity	0.25 dB in brain tissue (rotation around probe axis) 0.5 dB in brain tissue (rotation normal probe axis)
Dynamic	0.001W/kg to > 100W/kg
Range Linearity	0.25 dB
Surface	0.2 mm repeatability in air and liquids
Dimensions Overall length	330 mm
Tip length	16 mm
Body diameter	8 mm
Tip diameter	2.6 mm
Distance from probe tip to dipole centers	<1.5 mm

E-Field Probe Calibration

Each probe is calibrated according to a dosimetric assessment procedure described in SAR standard with accuracy better than $\pm 10\%$. The spherical isotropy was evaluated with the procedure described in SAR standard and found to be better than $\pm 0.25\text{dB}$. The sensitivity parameters (NormX, NormY, NormZ), the diode compression parameter (DCP) and the conversion factor (ConvF) of the probe are tested.

The free space E-field from probe outputs is determined in a test chamber. This is performed in a TEM cell for frequencies bellow 0.8 GHz, and in a waveguide above 0.8 GHz for free space. For the free space calibration, the probe is placed in the volumetric center of the cavity and at the proper orientation with the field. E-field correlation calibration is performed in a flat phantom filled with the appropriate simulated brain tissue.

Test report No.	FCC,IC_SAR_SL14031101-SLX-004 Rev1.0
Page	19 of 100
FCC ID	STJ-SDMAN
IC ID	5627A-SDMAN

SAM Phantom

The SAM Phantom SAM29 is constructed of a fiberglass shell integrated in a wooden table. The shape of the shell is in compliance with the specification set in IEEE P1528 and CENELEC EN62209-1.

The phantom enables the dosimetric evaluation of left and right hand phone usage as well as body mounted usage at the flat phantom region.

A cover prevents the evaporation of the liquid.

Reference markings on the Phantom allow the complete setup of all predefined phantom positions and measurement grids by manually teaching three points in the robot.

Shell Thickness: 0.2 mm

Filling Volume: Approx. 25 liters

Dimensions (H x L x W): 810 x 1000 x 500 mm

Liquid is filled to at least 15mm from the bottom of Phantom.



Device Holder

In combination with the Generic Twin Phantom V3.0, the Mounting Device enables the rotation of the mounted transmitter in spherical coordinates whereby the rotation points is the ear opening. The devices can be easily, accurately, and repeatedly positioned according to the FCC and CENELEC specifications. The device holder can be locked at different phantom locations (left head, right head, flat phantom).

Note: A simulating human hand is not used due to the complex anatomical and geometrical structure of the hand that may produce infinite number of configurations [10]. To produce the worst-case condition. (the hand absorbs antenna output power), the hand is omitted during the tests.



Test report No.	FCC,IC_SAR_SL14031101-SLX-004 Rev1.0
Page	20 of 100
FCC ID	STJ-SDMAN
IC ID	5627A-SDMAN

Data Evaluation

The OPENSAR software automatically executes the following procedure to calculate the field units from the microvolt readings at the probe connector. The parameters used in the valuation are stored in the configuration modules of the software:

Probe Parameters	- Sensitivity	Norm _i
	- Conversion factor	ConvFi
	- Diode compression point	Dcpi
Device Parameter	- Frequency	f
	- Crest factor	cf
Media Parameters	- Conductivity	σ
	- Density	ρ

These parameters must be set correctly in the software. They can either be found in the component documents or are imported into the software from the configuration files issued for the OPENSAR components.

The first step of the evaluation is a linearization of the filtered input signal to account for the compression characteristics of the detector diode. The compensation depends on the input signal, the diode type and the DC-transmission factor from the diode to the evaluation electronics. If the exciting field is pulsed, the crest factor of the signal must be known to correctly compensate for peak power. The formula for each channel can be given as

$$V_i = U_i - U_i^3 \cdot \frac{cf}{dcp_i}$$

Where V_i = Compensated signal of channel i ($i = x, y, z$)

U_i = Input signal of channel i ($i = x, y, z$)

cf = Crest factor of exciting field (DASY parameter)

dcp_i = Diode compression point (DASY parameter)

From the compensated input signals the primary field data for each channel can be evaluated:

$$E_i = \frac{V_i}{\sqrt{Norm_i \cdot ConvF}}$$

$$H_i = \sqrt{V_i} \cdot \frac{a_{0i} + a_{0i}f + a_{0i}f^2}{f}$$

Where V_i = Compensated signal of channel i ($i = x, y, z$)

$Norm_i$ = Sensor sensitivity of channel i ($i = x, y, z$)

$\mu V/(V/m)^2$ for E-field Probes

$ConvF$ = Sensitivity enhancement in solution

a_{0i} = Sensor sensitivity factors for H-field probes

f = Carrier frequency (GHz)

E_i = Electric field strength of channel i in V/m

H_i = Magnetic field strength of channel i in A/m

The RSS value of the field components gives the total field strength (Hermitian magnitude):

$$E_{tot} = \sqrt{E_x^2 + E_y^2 + E_z^2}$$

The primary field data are used to calculate the derived field units:

$$SAR = E_{tot}^2 \cdot \frac{\sigma}{\rho \cdot 1000}$$

where: SAR = local specific absorption rate in mW/kg

E_{tot} = total field strength in V/m

σ = conductivity in (mho/m) or (siemens/m)

ρ = equivalent tissue density in g/cm³

Note that the density is normally set to 1 (or 1.06), to account for actual brain density rather than the density of the simulation liquid.

The power flow density is calculated assuming the excitation field as a free space field:

$$P_{avg} = \frac{E_{tot}^2}{3770} \quad \text{or} \quad P_{avg} = H_{tot}^2 \cdot 37.7$$

where: P_{avg} = Equivalent power density of a plane wave in mW/cm²

E_{tot} = total electric field strength in V/m

H_{tot} = total magnetic field strength in A/m

Test report No.	FCC,IC_SAR_SL14031101-SLX-004 Rev1.0
Page	21 of 100
FCC ID	STJ-SDMAN
IC ID	5627A-SDMAN

SAR Evaluation – Peak Spatial - Average

The procedure for assessing the peak spatial-average SAR value consists of the following steps

- **Power Reference Measurement**

The reference and drift jobs are useful jobs for monitoring the power drift of the device under test in the batch process. Both jobs measure the field at a specified reference position, at a selectable distance from the phantom surface. The reference position can be either the selected section's grid reference point or a user point in this section. The reference job projects the selected point onto the phantom surface, orients the probe perpendicularly to the surface, and approaches the surface using the selected detection method.

- **Area Scan**

The area scan is used as a fast scan in two dimensions to find the area of high field values, before doing a finer measurement around the hot spot. The sophisticated interpolation routines implemented in OPENSAR software can find the maximum locations even in relatively coarse grids. The scan area is defined by an editable grid. This grid is anchored at the grid reference point of the selected section in the phantom. When the area scan's property sheet is brought-up, grid was at 15 mm by 15 mm and can be edited by a user.

- **Zoom Scan**

Zoom scans are used to assess the peak spatial SAR values within a cubic averaging volume containing 1 g and 10 g of simulated tissue. The default zoom scan measures 5 x 5 x 7 points within a cube whose base faces are centered on the maximum found in a preceding area scan job within the same procedure. If the preceding Area Scan job indicates more than one maximum, the number of Zoom Scans has to be enlarged accordingly (The default number inserted is 1).

- **Power Drift measurement**

The drift job measures the field at the same location as the most recent reference job within the same procedure, and with the same settings. The drift measurement gives the field difference in dB from the reading conducted within the last reference measurement. Several drift measurements are possible for one reference measurement. This allows a user to monitor the power drift of the device under test within a batch process. In the properties of the Drift job, the user can specify a limit for the drift and have OPENSAR software stop the measurements if this limit is exceeded.

SAR Evaluation – Peak SAR

The procedure for spatial peak SAR evaluation has been implemented according to the IEEE1529 standard. It can be conducted for 1 g and 10 g. The OPENSAR system allows evaluations that combine measured data and robot positions, such as:

- Maximum search
- Extrapolation
- Boundary correction
- Peak search for averaged SAR

During a maximum search, global and local maximum searches are automatically performed in 2-D after each Area Scan measurement with at least 6 measurement points. It is based on the evaluation of the local SAR gradient calculated by the Quadratic Shepard's method. The algorithm will find the global maximum and all local maxima within -2 dB of the global maxima for all SAR distributions.

Extrapolation

Extrapolation routines are used to obtain SAR values between the lowest measurement points and the inner phantom surface. The extrapolation distance is determined by the surface detection distance and the probe sensor offset. Several measurements at different distances are necessary for the extrapolation.


They are used in the Cube Scan to obtain SAR values between the lowest measurement points and the inner phantom surface. The routine uses the fourth order least square polynomial method for extrapolation. For a grid using 5x5x7 measurement points with 5mm resolution amounting to 343 measurement points, the uncertainty of the extrapolation routines is less than 1% for 1 g and 10 g cubes.

Device Reference Points


Definition of Reference Points

Ear Reference Point

Figure 6.2 shows the front, back and side views of the SAM Phantom. The point "M" is the reference point for the center of the mouth, "LE" is the left ear reference point (ERP), and "RE" is the right ERP. The ERPs are 15mm posterior to the entrance to the ear canal (EEC) along the B-M line (Back-Mouth), as shown in Figure 6.1. The plane passing through the two ear canals and M is defined as the Reference Plane. The line N-F (Neck-Front) is perpendicular to the reference plane and passing through the RE (or LE) is called the Reference Pivoting Line (see Figure 6.1). Line B-M is perpendicular to the N-F line. Both N-F and B-M lines are marked on the external phantom shell to facilitate handset positioning [5].

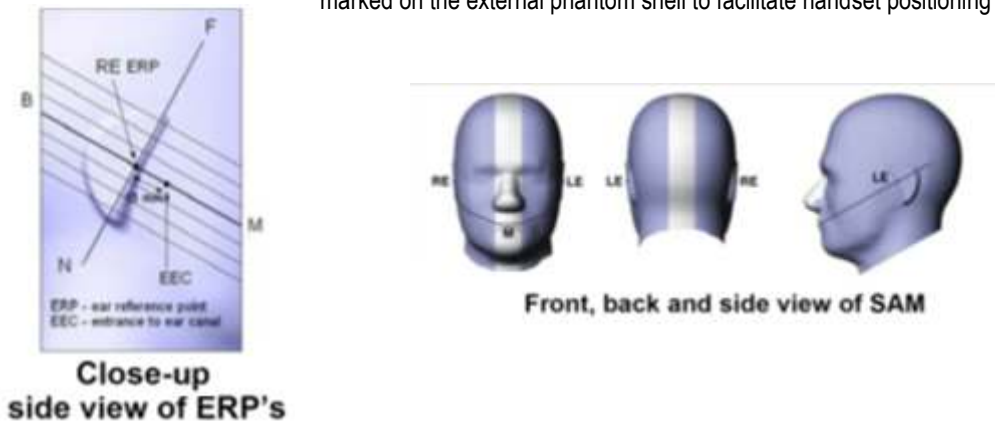

Two imaginary lines on the device need to be established: the vertical centerline and the horizontal line. The test device is placed in a normal operating position with the "test device reference point" located along the "vertical centerline" on the front of the device aligned to the "ear reference point" (See Fig. 6.3). The "test device reference point" is then located at the same level as the center of the ear reference point. The test device is positioned so that the "vertical centerline" is bisecting the front surface of the device at its top and bottom edges, positioning the "ear reference point" on the outer surface of both the left and right head phantoms on the ear reference point.

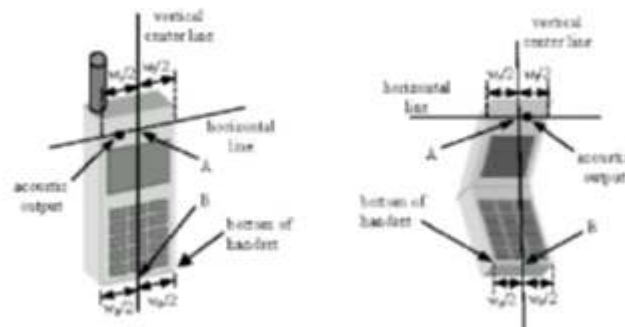

Test report No.	FCC,IC_SAR_SL14031101-SLX-004 Rev1.0
Page	23 of 100
FCC ID	STJ-SDMAN
IC ID	5627A-SDMAN


Test Configuration – Positioning for Cheek / Touch

1. Position the device close to the surface of the phantom such that point A is on the (virtual) extension of the line passing through points RE and LE on the phantom (see Figure below), such that the plane defined by the vertical center line and the horizontal line of the device is approximately parallel to the sagittal plane of the phantom



Front, Side and Top View of Cheek/Touch Position

2. Translate the device towards the phantom along the line passing through RE and LE until the device touches the ear.
3. While maintaining the device in this plane, rotate it around the LE-RE line until the vertical centerline is in the plane normal to MB-NF including the line MB (called the reference plane).
4. Rotate the device around the vertical centerline until the device (horizontal line) is symmetrical with respect to the line NF.
5. While maintaining the vertical centerline in the reference plane, keeping point A on the line passing through RE and LE and maintaining the device contact with the ear, rotate the device about the line NF until any point on the device is in contact with a phantom point below the ear (cheek). See Figure below.



Side view w/ relevant markings

Test report No.	FCC,IC_SAR_SL14031101-SLX-004 Rev1.0
Page	24 of 100
FCC ID	STJ-SDMAN
IC ID	5627A-SDMAN

Test Configuration – Positioning for Ear / 15° Tilt

With the test device aligned in the Cheek/Touch Position”:

1. While maintaining the orientation of the device, retracted the device parallel to the reference plane far enough to enable a rotation of the device by 15 degrees.
2. Rotate the device around the horizontal line by 15 degrees.
3. While maintaining the orientation of the device, move the device parallel to the reference plane until any part of the device touches the head. (In this position, point A is located on the line RE-LE). The tilted position is obtained when the contact is on the pinna. If the contact is at any location other than the pinna, the angle of the device shall be reduced. The tilted position is obtained when any part of the device is in contact with the ear as well as a second part of the device is in contact with the head (see Figure below).



Front, Side and Top View of Ear/15° Tilt Position

Test Position – Body Worn Configurations


Body-worn operating configurations are tested with the accessories attached to the device and positioned against a flat phantom in a normal use configuration. A device with a headset output is tested with a headset connected to the device. Body dielectric parameters are used.

Accessories for Body-worn operation configurations are divided into two categories: those that do not contain metallic components and those that do contain metallic components. When multiple accessories that do not contain metallic components are supplied with the device, the device is tested with only the accessory that dictates the closest spacing to the body. Then, when multiple accessories that contain metallic components are supplied with the device, the device is tested with each accessory that contains a unique metallic component. If multiple accessories share an identical metallic component (i.e. the same metallic belt-clip used with different holsters with no other metallic components) only the accessory that dictates the closest spacing to the body is tested.

Body-worn accessories may not always be supplied or available as options for some devices intended to be authorized for body-worn use. In this case, a test configuration where a separation distance between the back of the device and the flat phantom is used. All test position spacing are documented.

Transmitters that are designed to operate in front of a person's face, as in push-to-talk configurations, are tested for SAR compliance with the front of the device positioned to face the flat phantom. For devices that are carried next to the body such as a shoulder, waist or chest-worn transmitters, SAR compliance is tested with the accessory(ies), including headsets and microphones, attached to the device and positioned against a flat phantom in a normal use configuration.

In all cases SAR measurements are performed to investigate the worst-case positioning. Worst-case positioning is then documented and used to perform Body SAR testing.

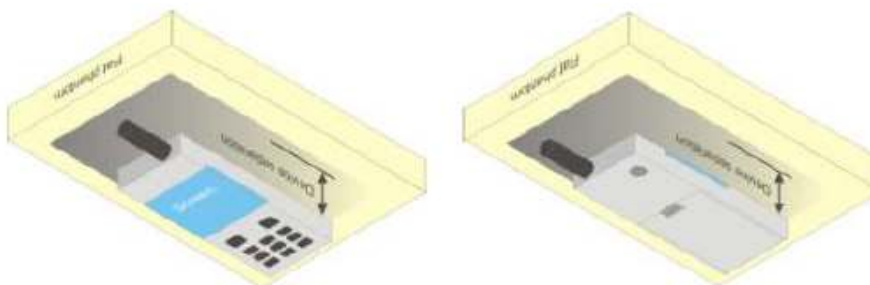

Test report No.	FCC,IC_SAR_SL14031101-SLX-004 Rev1.0
Page	25 of 100
FCC ID	STJ-SDMAN
IC ID	5627A-SDMAN

13 Measurement Uncertainty

The component of uncertainty may generally be categorized according to the methods used to evaluate them. The evaluation of uncertainty by the statistical analysis of a series of observations is termed a Type A evaluation of uncertainty. The evaluation of uncertainty by means other than the statistical analysis of a series of observation is termed a Type B evaluation of uncertainty. Each component of uncertainty, however evaluated, is represented by an estimated standard deviation, termed standard uncertainty, which is determined by the positive square root of the estimated variance

A Type A evaluation of standard uncertainty may be based on any valid statistical method for treating data. This includes calculating the standard deviation of the mean of a series of independent observations; using the method of least squares to fit a curve to the data in order to estimate the parameter of the curve and their standard deviations; or carrying out an analysis of variance in order to identify and quantify random effects in certain kinds of measurement.

A type B evaluation of standard uncertainty is typically based on scientific judgment using all of the relevant information available. These may include previous measurement data, experience and specification, data provided in calibration reports and uncertainties assigned to reference data taken from handbooks. Broadly speaking, the uncertainty is either obtained from an outdoor source or obtained from an assumed distribution, such as the normal distribution, rectangular or triangular distributions indicated in Table below :

Uncertainty Distribution	Normal	Rectangle	Triangular	U Shape
Multi-plying Factor ^(a)	1/k ^(b)	1 / $\sqrt{3}$	1 / $\sqrt{6}$	1 / $\sqrt{2}$

(a) standard uncertainty is determined as the product of the multiplying factor and the estimated range of variations in the measured quantity

(b) k is the coverage factor

Standard Uncertainty for Assumed Distribution

The combined standard uncertainty of the measurement result represents the estimated standard deviation of the result. It is obtained by combining the individual standard uncertainties of both Type A and Type -sum-by taking the positive square root of the estimated variances.

Expanded uncertainty is a measure of uncertainty that defines an interval about the measurement result within which the measured value is confidently believed to lie. It is obtained by multiplying the combined standard uncertainty by a coverage factor. Typically, the coverage factor ranges from 2 to 3. Using a coverage factor allows the true value of a measured quantity to be specified with a defined probability within the specified uncertainty range. For purpose of this document, a coverage factor two is used, which corresponds to confidence interval of about 95 %.

Test report No.	FCC,IC_SAR_SL14031101-SLX-004 Rev1.0
Page	26 of 100
FCC ID	STJ-SDMAN
IC ID	5627A-SDMAN

The COMOSAR Uncertainty Budget is show in below table:


Uncertainty Budget of COMOSAR for frequency range 300 MHz to 6 GHz

Uncertainty Component	Tolerances %	Probability Distribution	Divisor	Ci (1g)	Ci (10g)	Uncertainty 1g(%)	Uncertainty 10g(%)
Measurement System Related							
Probe Calibration	6	N	1	1	1	6	6
Axial Isotropy	3	R	$\sqrt{3}$	$\sqrt{1-C_p}$	$\sqrt{1-C_p}$	1.22474	1.22474
Hemispherical Isotropy	4	R	$\sqrt{3}$	$\sqrt{C_p}$	$\sqrt{C_p}$	1.63299	1.63299
Boundary Effect	1	R	$\sqrt{3}$	1	1	0.57735	0.57735
Linearity	5	R	$\sqrt{3}$	1	1	2.88675	2.88675
System Detection Limits	1	R	$\sqrt{3}$	1	1	0.57735	0.57735
Readout Electronics	0.5	N	1	1	1	0.5	0.5
Response Time	0.2	R	$\sqrt{3}$	1	1	0.11547	0.11547
Integration Time	2	R	$\sqrt{3}$	1	1	1.1547	1.1547
RF Ambient Conditions	3	R	$\sqrt{3}$	1	1	1.73205	1.73205
Probe Positioner Mechanical Tolerances	2	R	$\sqrt{3}$	1	1	1.1547	1.1547
Probe Positioning with respect to Phantom Shell	1	R	$\sqrt{3}$	1	1	0.57735	0.57735
Extrapolation, Interpolation and integration Algorithms for Max. SAR Evaluation.	1.5	R	$\sqrt{3}$	1	1	0.86603	0.86603
Test Sample Related							
Test Sample Positioning	1.5	N	1	1	1	1.5	1.5
Device Holder Uncertainty	5	N	1	1	1	5	5
Output Power Variation – SAR Drift measurement	3	R	$\sqrt{3}$	1	1	1.73205	1.73205
Phantom and Tissue Parameters Related							
Phantom Uncertainty (Shape and thickness Tolerances)	4	R	$\sqrt{3}$	1	1	2.3094	2.394
Liquid Conductivity – deviation from target value	5	R	$\sqrt{3}$	0.64	0.43	1.84752	1.2413
Liquid Conductivity – Measurement Uncertainty	2.5	N	1	0.64	0.43	1.6	1.075
Liquid Permittivity – deviation from target value	3	R	$\sqrt{3}$	0.6	0.49	1.03923	0.8487
Liquid Permittivity – Measurement Uncertainty	2.5	N	1	0.6	0.49	1.5	1.225
Combined Standard Uncertainty						9.66051 %	9.52428 %
Expanded Standard Uncertainty (K=2 , confidence 95%)						18.9346 %	18.6676 %

14 Liquid Validation

Liquid Validation

The dielectric parameters were checked prior to assessment using the HP85070C dielectric probe kit. The dielectric parameters measured are reported in each correspondent section.

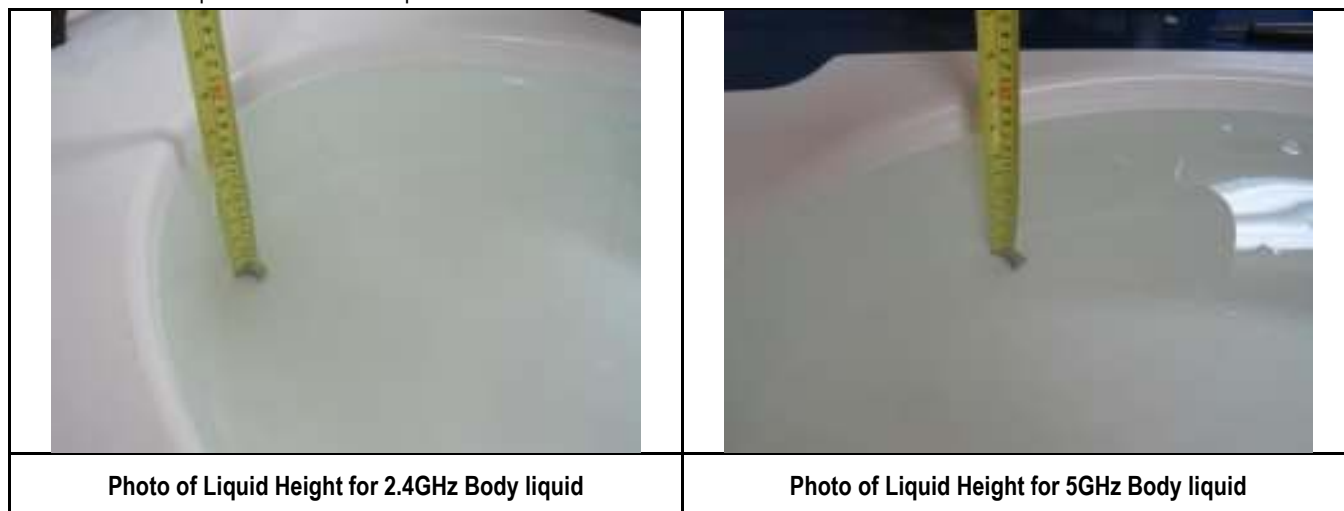

IEEE SCC-34/SC-2 P1528 recommended Tissue Dielectric Parameters

The head tissue dielectric parameters recommended by the IEEE SCC-34/SC-2 in P1528 have been incorporated in the following table. These head parameters are derived from planar layer models simulating the highest expected SAR for the dielectric properties and tissue thickness variations in a human head. Other head and body tissue parameters that have not been specified in P1528 are derived from the tissue dielectric parameters computed from the 4-Cole-Cole equations and extrapolated according to the head parameters specified in P1528

Target Frequency	Head		Body	
MHz	ϵ_r	σ (S/m)	ϵ_r	σ (S/m)
150	52.3	0.76	61.9	0.80
300	45.3	0.87	58.2	0.92
450	43.5	0.87	56.7	0.94
835	41.5	0.90	55.2	0.97
900	41.5	0.97	55.0	1.05
915	41.5	0.98	55.0	1.06
1450	40.5	1.20	54.0	1.30
1610	40.3	1.29	53.8	1.40
1800-2000	40.0	1.40	53.3	1.52
2450	39.2	1.80	52.7	1.95
3000	38.5	2.40	52.0	2.73
5800	35.3	5.27	48.2	6.00

Note: ϵ_r = relative permittivity, σ = conductivity and $\rho = 1000 \text{ kg/m}^3$

Test report No.	FCC,IC_SAR_SL14031101-SLX-004 Rev1.0
Page	28 of 100
FCC ID	STJ-SDMAN
IC ID	5627A-SDMAN

Liquid Confirmation Result:

Frequency (MHz)	Target Permittivity	Target Conductivity	Measured Permittivity	Measured Conductivity	Permittivity Deviation	Conductivity Deviation	Limit
2412	52.75	1.91	51.98	1.86	-1.47%	-2.58%	5
2437	52.72	1.94	51.63	1.94	-2.07%	0.01%	5
2450	52.7	1.95	51.21	1.93	-2.83%	-1.01%	5
2462	52.68	1.97	51.85	1.88	-1.58%	-4.54%	5
Remark	Measure Date Relative Humidity	04/29/2014 58%		Temperature Atmospheric Pressure		24oC 1009mbar	

Frequency (MHz)	Target Permittivity	Target Conductivity	Measured Permittivity	Measured Conductivity	Permittivity Deviation	Conductivity Deviation	Limit
5200	49.01	5.3	50.08	5.47	2.18%	3.25%	5
5230	48.97	5.33	50.03	5.49	2.16%	3.05%	5
5240	48.96	5.35	50.02	5.49	2.16%	2.66%	5
5270	48.92	5.38	49.97	5.52	2.15%	2.64%	5
5320	48.85	5.44	49.86	5.54	2.07%	1.88%	5
5500	48.61	5.65	49.06	5.61	0.93%	-0.68%	5
5580	48.5	5.74	48.81	5.70	0.64%	-0.67%	5
5680	48.36	5.86	48.60	5.76	0.50%	-1.69%	5
5670	48.38	5.85	48.62	5.76	0.50%	-1.52%	5
5700	48.34	5.88	48.56	5.77	0.46%	-1.85%	5
5745	48.27	5.94	48.40	5.73	0.28%	-3.52%	5
5755	48.26	5.95	48.37	5.72	0.23%	-3.84%	5
5800	48.2	6	48.20	5.72	0.01%	-4.72%	5
Remark	Measure Date Relative Humidity	04/29/2014 58%		Temperature Atmospheric Pressure		24oC 1009mbar	

15 System Validation and System Verification

15.1 System Validation

The system validation procedure evaluates the system against reference SAR values and the performance of the probe, readout electronics, and software. The test setup utilizes a flat phantom and a reference dipole.

Thus, the system validation process does not include data scatter due to the use of anthropomorphic phantoms or uncertainty due to handset positioning variability. System validation should be performed annually, or when a new system is put into operation, or whenever modifications have been made to the system, such as a new software release, different readout electronics or different types of probes. The probe used in the test system to be validated should be properly calibrated.

System validation provides a means of system-level validation. The test system utilizes a flat phantom and a reference dipole. Thus, system validation verifies the system accuracy against its specifications but does not include the uncertainty due to the use of anthropomorphic phantoms, nor does it include the uncertainty due to handset positioning variability. This test is performed annually (e.g., after probe calibration), before measurements related to inter laboratory comparison and every time modifications have been made to the system, such as a new software release, different readout electronics, and for different types of probes.

System Validation procedure is at below,

- a) **SAR evaluation:** A complete 1 g or 10 g averaged SAR measurement is performed. The reference dipole input power is adjusted to produce a 1 g averaged SAR value falling in the range of 0.4–10 W/kg. The 1 g or 10 g averaged SAR is measured at frequencies in reference table within the range to be used in compliance tests. The results are normalized to 1 W forward input power and compared with the reference SAR values shown in reference value. The differences from the reference values should be less than the tolerance specified for the SAR measurement system by the manufacturer or designer, i.e., within the expanded uncertainty for the system validation.
- b) **Extrapolation routine:** Local SAR values are measured along a vertical axis directly above the reference dipole feed-point using the same test grid-point spacing as used for handset SAR evaluations. This measurement is repeated along another vertical axis with a 2 cm transverse offset from the reference dipole feed-point. SAR values at the phantom surface are extrapolated and compared with the numerical values given in reference table. The difference from the reference values should be less than the tolerance specified for the SAR measurement system by the manufacturer or designer, i.e., within the expanded uncertainty for system validation.
- c) **Probe linearity:** The measurement in step a) is repeated using different reference dipole input power levels. The power levels are selected for each frequency to produce 1 g averaged SAR values of approximately 10 W/kg, 2 W/kg, and 0.4 W/kg. The measured SAR values are normalized to 1 W forward input power and compared with the 1 W normalized value from step a). The difference between these values should be less than the tolerance specified for the SAR measurement system by the manufacturer or designer, i.e., within the expanded uncertainty for the linearity component.
- d) **Modulation response:** The measurements in step a) are repeated with pulse-modulated signals having a duty factor of 0.1 and pulse repetition rate of 10 Hz. The power is adjusted to produce a 1 g-averaged SAR of approximately 8 W/kg with the pulse modulated signal (corresponding to a peak spatial-average SAR of approximately 80 W/kg). The measured SAR values are normalized to 1 W forward input power and duty factor of 1, and compared with the 1 W normalized values from step a). The difference between these values should be less than the tolerance specified for the SAR measurement system by the manufacturer or designer, i.e., within the expanded uncertainty for system validation.
- e) **System offset:** The measurements in step a) are repeated with a reference dipole input forward power that produces a 1 g or 10 g averaged SAR of approximately 0.05 W/kg. The measured SAR values are normalized to 1 W forward input power and compared with the 1 W normalized values from step a). The difference between these values should be less than the tolerance specified for the SAR measurement system by the manufacturer or designer, i.e., within the expanded uncertainty for system validation.
- f) **Probe axial isotropy:** The center point of the probe's sensors is placed directly above the reference dipole center at a measurement distance of approximately 5–10 mm from the phantom inner surface. The probe (or reference dipole, if precise rotations are supported by the dipole fixture) is rotated around its axis $\pm 180^\circ$ in steps no larger than 15° . The maximum and minimum SAR readings are recorded. The difference between these values should be less than the tolerance specified for the SAR measurement system by the manufacturer or designer, i.e., within the expanded uncertainty for the axial isotropy component.

Test report No.	FCC,IC_SAR_SL14031101-SLX-004 Rev1.0
Page	30 of 100
FCC ID	STJ-SDMAN
IC ID	5627A-SDMAN

Numerical reference SAR values (W/kg) for reference dipole and flat phantom

Frequency (MHz)	1 g SAR	10 g SAR	Local SAR at surface (above feed-point)	Local SAR at surface (y = 2 cm offset from feed-point) ^a
300	3.0	2.0	4.4	2.1
450	4.9	3.3	7.2	3.2
835	9.5	6.2	4.1	4.9
900	10.8	6.9	16.4	5.4
1450	29.0	16.0	50.2	6.5
1800	38.1	19.8	69.5	6.8
1900	39.7	20.5	72.1	6.6
2000	41.1	21.1	74.6	6.5
2450	52.4	24.0	104.2	7.7
3000	63.8	25.7	140.2	9.5

Target and measurement SAR after Normalized


System Validation Status

Frequency (MHz)	Temp (oC)	Humidity (%)	Validation Date	Probe SN	Validation Cycle	Validation Due
835	23	58	Oct 23rd, 2013	09/13 EPG176	1 year	Oct 23rd, 2014
900	23	58	Oct 23rd, 2013	09/13 EPG176	1 year	Oct 23rd, 2014
1800	23	58	Oct 23rd, 2013	09/13 EPG176	1 year	Oct 23rd, 2014
1900	23	58	Oct 23rd, 2013	09/13 EPG176	1 year	Oct 23rd, 2014
2000	23	58	Oct 23rd, 2013	09/13 EPG176	1 year	Oct 23rd, 2014
2450	23	58	Oct 23rd, 2013	09/13 EPG176	1 year	Oct 23rd, 2014
5200	23	58	Oct 23rd, 2013	09/13 EPG176	1 year	Oct 23rd, 2014
5500	23	58	Oct 23rd, 2013	09/13 EPG176	1 year	Oct 23rd, 2014
5800	23	58	Oct 23rd, 2013	09/13 EPG176	1 year	Oct 23rd, 2014

15.2 System Verification

The system performance check verifies that the system operates within its specifications. System and operator errors can be detected and corrected. It is recommended that the system performance check be performed prior to any usage of the system in order to guarantee reproducible results. The system performance check uses normal SAR measurements in a simplified setup with a well characterized source. This setup was selected to give a high sensitivity to all parameters that might fail or vary over time. The system check does not intend to replace the calibration of the components, but indicates situations where the system uncertainty is exceeded due to drift or failure.

In the simplified setup for system evaluation, the DUT is replaced by a calibrated dipole and the power source is replaced by a continuous wave that comes from a signal generator. The calibrated dipole must be placed beneath the flat phantom section of the SAM twin phantom with the correct distance holder. The distance holder should touch the phantom surface with a light pressure at the reference marking and be oriented parallel to the long side of the phantom. The equipment setup is shown below:

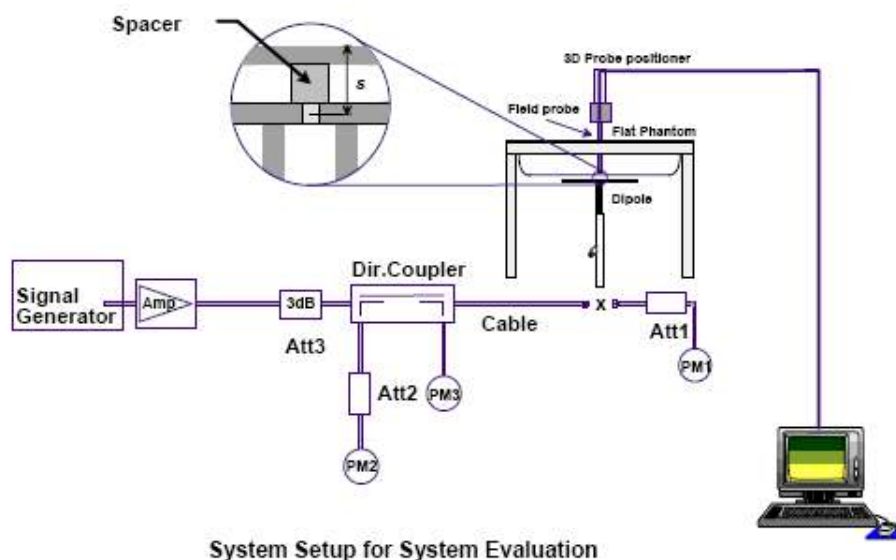

System Setup for System Evaluation

Note: Equipment description

1. Signal Generator
2. Amplifier
3. Directional Coupler
4. Power Meter
5. Calibrated Dipole

System Verification Results

Measurement Date	Temp (oC)	Humidity (%)	Frequency (MHz)	Phantom/Liquid	Target SAR1g (W/kg)	Input Power (dBm)	Measured SAR1g (W/kg)	1W Normalized SAR1g (W/kg)	Deviation (%)
Apr 29th, 2014	23	58	2450	Body	55.61	15	1.83	57.88	4.09
Apr 29th, 2014	23	58	5200	Body	162.43	15	4.99	157.79	-2.85
Apr 29th, 2014	23	58	5500	Body	173.99	15	5.61	177.55	2.05
Apr 29th, 2014	23	58	5800	Body	184.02	15	5.89	186.30	1.24

Test report No.	FCC,IC_SAR_SL14031101-SLX-004 Rev1.0
Page	32 of 100
FCC ID	STJ-SDMAN
IC ID	5627A-SDMAN

16 Measurements, Examination and Derived Results

16.1 Output Power Measurement Result

Requirement(s):

Spec	Item	Requirement	Applicable
-	-	Time averaged conducted output power to be measured	☒
Test Setup			
Test Procedure	FCC UNII Method SA-1 (trace averaging with the EUT transmitting at full power throughout each sweep)		
Test Date	04/29/2014 - 05/01/2014	Environmental condition	Temperature 24oC Relative Humidity 58% Atmospheric Pressure 1008mbar
Remark	NONE		
Result	☒ Pass ☐ Fail		

Equipment Setting

TEST	RBW	VBW	SPAN	Detector	SWEEP	Trace	NOTES
PK output power	1MHz	≥3MHz	≥EBW or 99% OBW	RMS	Auto	Average on 100 traces	CH PW on 26 dB EBW or 99% OBW

Data Rate setting

Type	Data Rate (Mbps)
802.11b	1
802.11g	6
802.11a	6
802.11n-HT20	6.5
802.11n-HT40	13.5

Test Data ☒ Yes ☐ N/A

Test report No.	FCC,IC_SAR_SL14031101-SLX-004 Rev1.0
Page	33 of 100
FCC ID	STJ-SDMAN
IC ID	5627A-SDMAN

Output Power measurement result

2.4GHz band- 802.11b/g/n

Ant Port	Data Rates (Mbps)	CH (MHz)	802.11b PW (dBm)	Rated Power for 802.11b (dBm)
Port1	1(802.11b) 6(802.11g) 6.5(802.11n)	2437	13.25*	13+2/-2.5
		2412	13.05	13+2/-2.5
		2462	13.23	13+2/-2.5
Port2		2437	13.13*	13+2/-2.5
		2412	13.04	13+2/-2.5
		2462	13.01	13+2/-2.5
Remark	1. Per KDB 248227 SAR measurement procedures for 802.11 a/b/g, the initial test configuration is chosen as 802.11b with the maximum output power channel. And if the specified output power of 11g/n is not ¼ dB higher than and not 1 dB higher than specified 11b power, and the measured SAR of 11b is not higher than 0.8w/kg, than the measurement on 11g/n and other channel on 11b is not required. 2. Per KDB 248227 SAR measurement procedures for 802.11 a/b/g TX, since output power of 802.11g and 802.11n are not ¼ dB higher than 802.11b, than 802.11b mode will be tested to represent 2.4GHz band. 3. Per KDB 248227, the lowest data rate mode was tested. 4. Port1 and Port2 are TX diversity; their antennas are installed along different edge position. Both of them will be tested separately. 5. Please help to see separate Power tolerant document for power setting for all configuration.			

5GHz Band- 802.11n-HT40

Ant Port	Data Rates (Mbps)	Band	CH (MHz)	802.11n-HT40PW (dBm)	Rated Power (dBm)
Port1	13.5(802.11n)	5.2GHz	5230	16.63*	14.0+2/-2.5
		5.3GHz	5270	16.88*	14.0+2/-2.5
		5.6GHz	5510	15.71	14.0+2/-2.5
		5.6GHz	5550	16.06	14.0+2/-2.5
		5.6GHz	5670	16.86*	14.0+2/-2.5
		5.8GHz	5755	15.78*	14.0+2/-2.5
Port2	13.5(802.11n)	5.2GHz	5230	16.27*	14.0+2/-2.5
		5.3GHz	5270	16.52*	14.0+2/-2.5
		5.6GHz	5510	15.39	14.0+2/-2.5
		5.6GHz	5550	15.57	14.0+2/-2.5
		5.6GHz	5670	16.54*	14.0+2/-2.5
		5.8GHz	5755	15.46*	13.0+2/-2.5
Remark	- Per KDB 248227 SAR measurement procedures for 802.11 a/n/ac, the initial test configuration is chosen with the specified maximum output power channel in each band with largest channel bandwidth, which is HT40. And if the specified output power of other configuration is less than ½ dB lower than specified 11n-HT40 power and the measured SAR of 11n-HT40 is not higher than 0.8w/kg, than the measurement on 11a/11n-20 and other channels in HT-40 is not required. - The channel with "*" are highest output power channel, which will be tested to find out worst SAR configuration. - Per KDB 248227, the lowest data rate mode was tested. - Port1 and Port2 are TX diversity; their antennas are installed along different edge position. Both of them will be tested separately. - Please help to see separate Power tolerant document for power setting for all configuration.				

Test report No.	FCC,IC_SAR_SL14031101-SLX-004 Rev1.0
Page	34 of 100
FCC ID	STJ-SDMAN
IC ID	5627A-SDMAN

Duty Cycle measurement

Type	ON time (uS)	Cycle time (uS)	Duty cycle	Crest factor
802.11b-1M	165.731	184.849	89.66%	1.115
802.11g-6M	303.687	334.348	90.83%	1.101
802.11a-6M	361.563	385.331	93.83%	1.066
802.11n-HT20-6.5M	300.641	332.024	90.55%	1.104
802.11n-HT40-13.5M	267.134	292.425	91.35%	1.095

Test report No.	FCC,IC_SAR_SL14031101-SLX-004 Rev1.0
Page	35 of 100
FCC ID	STJ-SDMAN
IC ID	5627A-SDMAN

16.2 SAR Measurement Result

Requirement(s):

Spec	Item	Requirement	Applicable
RSS-102 Issue 4-SAR	1	SAR limit for devices used by the General public (Uncontrolled Environment) in localized Head and Trunk is 1.6 W/kg	☒
	2	SAR limit for Controlled Use Devices (Controlled Environment) in localized Head and Trunk is 8 W/kg	☐
Test Method	IEEE 1528: 2003 IEC 62209-2: 2010 447498 D01 General RF Exposure Guidance v05r01 248227 SAR measurement procedures for 802.11 a/b/g TX KDB 865664 SAR Measurement Requirements for 3 to 6 GHz v05r01		
Test Setup	Refer to Section 6: SAR Measurement Setup		
Test Procedure	Steps: 1. Use client test software to set EUT transmit RF power in cont-TX mode in the highest power channel 2. Measure output power through spectrum analyzer 3. Place the DUT in the positions selected 4. Set scan area, grid size and other setting on the SATIMO software 5. Make SAR measurement for the selected highest output power channel at each testing position 6. Find out the position with highest SAR result 7. Measure additional SAR for other modes at the highest SAR position SAR measurement system will proceed the following basic steps: 1. Initial power reference measurement 2. Area Scan 3. Zoom Scan 4. Power drift measurement		
Test Date	04/29/2014	Environmental condition	Temperature 23oC Relative Humidity 58% Atmospheric Pressure 1008mbar
Remark	1. The testing in current report is to be performed at 0 cm separation distance. 2. For top position, the Ant #1 is enabled; for right position, the Ant #2 is enabled.		
Result	☒ Pass ☐ Fail		

Test Data ☒ Yes ☐ N/A

Test Plot ☒ Yes (Refer to Annex E) ☐ N/A

Test report No.	FCC,IC_SAR_SL14031101-SLX-004 Rev1.0
Page	36 of 100
FCC ID	STJ-SDMAN
IC ID	5627A-SDMAN

SAR Measurement result to determine the worst case position configuration

SAR Type		Body SAR							
Freq Band	Freq (MHz)	Position	Rated Max Power (dBm)	Measured Output Power (dBm)	Raw SAR 1g (W/kg)	Crest factor	Power Drift (%)	Scaled SAR (Tune-up & Duty Cycle)	1g SAR Limit (W/kg)
802.11b	2437	Top	15	13.25	0.303	1.115	-3.79	0.505	1.6
802.11n-HT40-5.2G	5230	Top	16	16.63	0.283	1.095	1.80	0.268	1.6
802.11n-HT40-5.3G	5270	Top	16	16.88	0.267	1.095	1.76	0.239	1.6
802.11n-HT40-5.6G	5670	Top	16	16.86	0.328	1.095	3.81	0.295	1.6
802.11n-HT40-5.8G	5755	Top	15	15.78	0.302	1.095	-3.12	0.276	1.6
802.11b	2437	Right	15	13.25	0.272	1.115	4.01	0.454	1.6
802.11n-HT40-5.2G	5230	Right	16	16.63	0.261	1.095	-2.84	0.247	1.6
802.11n-HT40-5.3G	5270	Right	16	16.88	0.275	1.095	-1.83	0.246	1.6
802.11n-HT40-5.6G	5670	Right	16	16.86	0.243	1.095	-2.10	0.218	1.6
802.11n-HT40-5.8G	5755	Right	15	15.78	0.261	1.095	-1.93	0.239	1.6
Note:		1. Separation distance : See page 14 (EUT position for SAR measurement) 2. The worst case configuration is Top position.							

Additional SAR measurement on worst case position configuration

SAR Type		Body SAR							
Freq Band	Freq (MHz)	Position	Rated Max Power (dBm)	Measured Output Power (dBm)	Raw SAR 1g (W/kg)	Crest Factor	Power Drift (%)	Scaled SAR (Tune-up & Duty Cycle)	1g SAR Limit (W/kg)
802.11b	2412	Top	15	13.15	0.235	1.115	3.71	0.401	1.6
802.11b	2437	Top	15	13.25	0.303	1.115	-3.79	0.505	1.6
802.11b	2462	Top	15	13.23	0.269	1.115	-3.81	0.451	1.6
802.11-HT40-5.6G	5510	Top	16	15.71	0.305	1.095	-3.01	0.357	1.6
802.11-HT40-5.6G	5550	Top	16	15.89	0.297	1.095	2.98	0.334	1.6
802.11-HT40-5.6G	5670	Top	16	16.86	0.328	1.095	3.81	0.295	1.6
Note:		1. Separation distance : 0cm							

Note:

Per KDB 248227, Since the initial test configuration reported SAR value for all Initial test position is less than 0.8W/kg. and the Max output power of other configuration is less than initial test configuration. There SAR testing for other configurations is not required.

Test report No.	FCC,IC_SAR_SL14031101-SLX-004 Rev1.0
Page	37 of 100
FCC ID	STJ-SDMAN
IC ID	5627A-SDMAN

Annex A. TEST INSTRUMENT

Instrument	Model	Serial #	Cal Date	Cal Cycle	Cal Due	In use
SAR						
P C	PV 3.06GHz	375052-AA1	N/A	N/A	N/A	☒
Signal Generator	8665B-008	3744A01304	05/17/2013	1 Year	05/17/2014	☒
Multi-meter	Multi-meter 2000	1259033	08/13/2013	1 Year	08/13/2014	☒
S-Parameter Network Analyzer	8753ES	US38161019	05/11/2013	1 Year	05/11/2014	☒
Power Meter	437B	3038A03648	04/25/2014	1 Year	04/25/2015	☐
E-field PROBE	EPG176	SN09/13 EPG176	05/01/2013	1 Year	05/01/2014	☒
DIPOLE 2450	DIPOLE 2450MHz	SN 31/10 DIPJ138	06/13/2013	1 Year	06/13/2014	☒
WaveGuide 5/6 GHz	Wave Guide 5/6GHz	SN 31/10 DIPWGA13	06/13/2013	1 Year	06/13/2014	☒
COMOSAR Open Coaxial Probe	OCP36	SN 31/10 OCP36	06/13/2013	1 Year	06/13/2014	☒
Communication Antenna	ANTA30	SN 31/10 ANTA30	N/A	N/A	N/A	☒
Laptop POSITIONING DEVICE	LSH63	SN 31/10 LSH13	N/A	N/A	N/A	☒
Mobile Phone POSITIONING DEVICE	MSH63	SN 31/10 MSH63	N/A	N/A	N/A	☒
DUMMY PROBE	None	SN 31/10	N/A	N/A	N/A	☐
SAM PHANTOM	SAM77	SN 31/10 SAM77	N/A	N/A	N/A	☐
Elliptic Phantom	ELLI17	SN 31-10 ELLI17	N/A	N/A	N/A	☒
PHANTOM TABLE	N/A	N/A	N/A	N/A	N/A	☒
6 AXIS ROBOT	KR5	949319	N/A	N/A	N/A	☒
Medium Power Solid State Amplifier (0.8~4.2GHz)	S41-25	M629-0408	N/A	N/A	N/A	☒

Test report No.	FCC,IC_SAR_SL14031101-SLX-004 Rev1.0
Page	38 of 100
FCC ID	STJ-SDMAN
IC ID	5627A-SDMAN

Annex B. USER MANUAL, BLOCK & CIRCUIT DIAGRAM

Please see attachment

Test report No.	FCC,IC_SAR_SL14031101-SLX-004 Rev1.0
Page	39 of 100
FCC ID	STJ-SDMAN
IC ID	5627A-SDMAN

Annex C. SIEMIC Accreditation

Accreditations	Document	Scope / Remark
ISO 17025 (A2LA)		Please see the documents for the detailed scope
ISO Guide 65 (A2LA)		Please see the documents for the detailed scope
TCB Designation		A1 , A2 , A3 , A4 , B1 , B2 , B3 , B4 , C
FCC DoC Accreditation		FCC Declaration of Conformity Accreditation
FCC Site Registration		3 meter site
FCC Site Registration		10 meter site
IC Site Registration		3 meter site
IC Site Registration		10 meter site
EU NB		Radio & Telecommunications Terminal Equipment: EN45001 – EN ISO/IEC 17025
		Electromagnetic Compatibility: EN45001 – EN ISO/IEC 17025
Singapore iDA CB(Certification Body)	 	Phase I , Phase II
Vietnam MIC CAB Accreditation		Please see the document for the detailed scope
HongKong OFCA		(Phase II) OFCA Foreign Certification Body for Radio and Telecom
		(Phase I) Conformity Assessment Body for Radio and Telecom
Industry Canada CAB		Radio: Scope A – All Radio Standard Specification in Category I
		Telecom: CS-03 Part I, II, V, VI, VII, VIII

Test report No.	FCC,IC_SAR_SL14031101-SLX-004 Rev1.0
Page	40 of 100
FCC ID	STJ-SDMAN
IC ID	5627A-SDMAN

Japan Recognized Certification Body Designation		Radio : A1. Terminal equipment for purpose of calling Telecom : B1. Specified radio equipment specified in Article 38-2, Paragraph 1, Item 1 of the Radio Law
Korea CAB Accreditation		EMI: KCC Notice 2008-39, RRL Notice 2008-3: CA Procedures for EMI KN22: Test Method for EMI EMS: KCC Notice 2008-38, RRL Notice 2008-4: CA Procedures for EMS KN24, KN61000-4-2, -4-3, -4-4, -4-5, -4-6, -4-8, -4-11: Test Method for EMS Radio: RRL Notice 2008-26, RRL Notice 2008-2, RRL Notice 2008-10, RRL Notice 2007-49, RRL Notice 2007-20, RRL Notice 2007-21, RRL Notice 2007-80, RRL Notice 2004-68 Telecom: President Notice 20664, RRL Notice 2007-30, RRL Notice 2008-7 with attachments 1, 3, 5, 6; President Notice 20664, RRL Notice 2008-7 with attachment 4
Taiwan NCC CAB Recognition		LP0002, PSTN01, ADSL01, ID0002, IS6100, CNS14336, PLMN07, PLMN01, PLMN08
Taiwan BSMI CAB Recognition		CNS 13438
Japan VCCI		R-3083: Radiation 3 meter site C-3421: Main Ports Conducted Interference Measurement T-1597: Telecommunication Ports Conducted Interference Measurement
Australia CAB Recognition		EMC: AS/NZS CISPR 11, AS/NZS CISPR 14.1, AS/NZS CISPR22, AS/NZS 61000.6.3, AS/NZS 61000.6.4 Radiocommunications: AS/NZS 4281, AS/NZS 4268, AS/NZS 4280.1, AS/NZS 4280.2, AS/NZS 4295, AS/NZS 4582, AS/NZS 4583, AS/NZS 4769.1, AS/NZS 4769.2, AS/NZS 4770, AS/NZS 4771 Telecommunications: AS/ACIF S002:05, AS/ACIF S003:06, AS/ACIF S004:06, AS/ACIF S006:01, AS/ACIF S016:01, AS/ACIF S031:01, AS/ACIF S038:01, AS/ACIF S040:01, AS/ACIF S041:05, AS/ACIF S043.2:06, AS/ACIF S60950.1
Australia NATA Recognition		AS/ACIF S002, AS/ACIF S003, AS/ACIF S004, AS/ACIF S006, AS/ACIF S016, AS/ACIF S031, AS/ACIF S038, AS/ACIF S040, AS/ACIF S041, AS/ACIF S043.2

Test report No.	FCC,IC_SAR_SL14031101-SLX-004 Rev1.0
Page	41 of 100
FCC ID	STJ-SDMAN
IC ID	5627A-SDMAN

This page has been left blank intentionally.

Test report No.	FCC,IC_SAR_SL14031101-SLX-004 Rev1.0
Page	42 of 100
FCC ID	STJ-SDMAN
IC ID	5627A-SDMAN

Annex D. Calibration report



COMOSAR E-Field Probe Calibration Report

Ref : ACR.137.1.13.SATULA

SIEMIC TESTING AND CERTIFICATION SERVICES

SUITE 311, BUILDING 1, SECTION 30 ,NO.2 KEFA ROAD,
SCIENCE AND TECHNOLOGY PARK
NAN SHAN DISTRICT, SHENZHEN 518057 , GUANGDONG
P.R.C.

SATIMO COMOSAR DOSIMETRIC E-FIELD PROBE
SERIAL NO.: SN 09/13 EPG176

Calibrated at SATIMO US
2105 Barrett Park Dr. - Kennesaw, GA 30144



05/01/2013

Summary:

This document presents the method and results from an accredited COMOSAR Dosimetric E-Field Probe calibration performed in SATIMO USA using the CALISAR / CALIBAIR test bench, for use with a SATIMO COMOSAR system only. All calibration results are traceable to national metrology institutions.

Test report No.	FCC,IC_SAR_SL14031101-SLX-004 Rev1.0
Page	43 of 100
FCC ID	STJ-SDMAN
IC ID	5627A-SDMAN



COMOSAR E-FIELD PROBE CALIBRATION REPORT

Ref: ACTR137.1.11.SATU.A

	Name	Function	Date	Signature
Prepared by :	Jérôme LUC	Product Manager	5/17/2013	
Checked by :	Jérôme LUC	Product Manager	5/17/2013	
Approved by :	Kim RUTKOWSKI	Quality Manager	5/17/2013	

	Customer Name
Distribution :	SIEMIC Testing and Certification Services

Issue	Date	Modifications
A	5/17/2013	Initial release

Page: 2/10

This document shall not be reproduced, except in full or in part, without the written approval of SATIMO.
The information contained herein is to be used only for the purpose for which it is submitted and is not to be released in whole or part without written approval of SATIMO.

Test report No.	FCC,IC_SAR_SL14031101-SLX-004 Rev1.0
Page	44 of 100
FCC ID	STJ-SDMAN
IC ID	5627A-SDMAN



TABLE OF CONTENTS

1	Device Under Test	4
2	Product Description	4
2.1	General Information	4
3	Measurement Method	4
3.1	Linearity	4
3.2	Sensitivity	5
3.3	Lower Detection Limit	5
3.4	Isotropy	5
3.5	Boundary Effect	5
4	Measurement Uncertainty	5
5	Calibration Measurement Results	6
5.1	Sensitivity in air	6
5.2	Linearity	7
5.3	Sensitivity in liquid	7
5.4	Isotropy	8
6	List of Equipment	10

Test report No.	FCC,IC_SAR_SL14031101-SLX-004 Rev1.0
Page	45 of 100
FCC ID	STJ-SDMAN
IC ID	5627A-SDMAN



COMOSAR E-FIELD PROBE CALIBRATION REPORT

Ref: ACR-137.1.13.SATU.A

1 DEVICE UNDER TEST

Device Under Test	
Device Type	COMOSAR DOSIMETRIC E FIELD PROBE
Manufacturer	Satimo
Model	SSE2
Serial Number	SN 09/13 EPG176
Product Condition (new / used)	new
Frequency Range of Probe	0.7 GHz-6GHz
Resistance of Three Dipoles at Connector	Dipole 1: R1=0.225 MΩ Dipole 2: R2=0.209 MΩ Dipole 3: R3=0.238 MΩ

A yearly calibration interval is recommended.

2 PRODUCT DESCRIPTION

2.1 GENERAL INFORMATION

Satimo's COMOSAR E field Probes are built in accordance to the IEEE 1528, OET 65 Bulletin C and CEI/IEC 62209 standards.



Figure 1 – Satimo COMOSAR Dosimetric E field Dipole

Probe Length	330 mm
Length of Individual Dipoles	2 mm
Maximum external diameter	8 mm
Probe Tip External Diameter	2.5 mm
Distance between dipoles / probe extremity	1 mm

3 MEASUREMENT METHOD

The IEEE 1528, OET 65 Bulletin C, CENELEC EN50361 and CEI/IEC 62209 standards provide recommended practices for the probe calibrations, including the performance characteristics of interest and methods by which to assess their affect. All calibrations / measurements performed meet the fore mentioned standards.

3.1 LINEARITY

The evaluation of the linearity was done in free space using the waveguide, performing a power sweep to cover the SAR range 0.01W/kg to 100W/kg.

Page: 4/10

*This document shall not be reproduced, except in full or in part, without the written approval of SATIMO.
The information contained herein is to be used only for the purpose for which it is submitted and is not to be released in whole or part without written approval of SATIMO.*

Test report No.	FCC,IC_SAR_SL14031101-SLX-004 Rev1.0
Page	46 of 100
FCC ID	STJ-SDMAN
IC ID	5627A-SDMAN



3.2 SENSITIVITY

The sensitivity factors of the three dipoles were determined using a two step calibration method (air and tissue simulating liquid) using waveguides as outlined in the standards.

3.3 LOWER DETECTION LIMIT

The lower detection limit was assessed using the same measurement set up as used for the linearity measurement. The required lower detection limit is 10 mW/kg.

3.4 ISOTROPY

The axial isotropy was evaluated by exposing the probe to a reference wave from a standard dipole with the dipole mounted under the flat phantom in the test configuration suggested for system validations and checks. The probe was rotated along its main axis from 0 - 360 degrees in 15 degree steps. The hemispherical isotropy is determined by inserting the probe in a thin plastic box filled with tissue-equivalent liquid, with the plastic box illuminated with the fields from a half wave dipole. The dipole is rotated about its axis (0°-180°) in 15° increments. At each step the probe is rotated about its axis (0°-360°).

3.5 BOUNDARY EFFECT

The boundary effect is defined as the deviation between the SAR measured data and the expected exponential decay in the liquid when the probe is oriented normal to the interface. To evaluate this effect, the liquid filled flat phantom is exposed to fields from either a reference dipole or waveguide. With the probe normal to the phantom surface, the peak spatial average SAR is measured and compared to the analytical value at the surface.

4 MEASUREMENT UNCERTAINTY

The guidelines outlined in the IEEE 1528, OET 65 Bulletin C, CENELEC EN50361 and CEI/IEC 62209 standards were followed to generate the measurement uncertainty associated with an E-field probe calibration using the waveguide technique. All uncertainties listed below represent an expanded uncertainty expressed at approximately the 95% confidence level using a coverage factor of k=2, traceable to the Internationally Accepted Guides to Measurement Uncertainty.

Uncertainty analysis of the probe calibration in waveguide					
ERROR SOURCES	Uncertainty value (%)	Probability Distribution	Divisor	ci	Standard Uncertainty (%)
Incident or forward power	3.00%	Rectangular	$\sqrt{3}$	1	1.732%
Reflected power	3.00%	Rectangular	$\sqrt{3}$	1	1.732%
Liquid conductivity	5.00%	Rectangular	$\sqrt{3}$	1	2.887%
Liquid permittivity	4.00%	Rectangular	$\sqrt{3}$	1	2.309%
Field homogeneity	3.00%	Rectangular	$\sqrt{3}$	1	1.732%
Field probe positioning	5.00%	Rectangular	$\sqrt{3}$	1	2.887%
Field probe linearity	3.00%	Rectangular	$\sqrt{3}$	1	1.732%



COMOSAR E-FIELD PROBE CALIBRATION REPORT

Ref: ACR.137.1.13.SATU.A

Combined standard uncertainty					5.831%
Expanded uncertainty 95 % confidence level k = 2					12.0%

5 CALIBRATION MEASUREMENT RESULTS

Calibration Parameters	
Liquid Temperature	21 °C
Lab Temperature	21 °C
Lab Humidity	45 %


5.1 SENSITIVITY IN AIR

Normx dipole 1 ($\mu\text{V}/(\text{V}/\text{m})^2$)	Normy dipole 2 ($\mu\text{V}/(\text{V}/\text{m})^2$)	Normz dipole 3 ($\mu\text{V}/(\text{V}/\text{m})^2$)
0.62	0.61	0.52

DCP dipole 1 (mV)	DCP dipole 2 (mV)	DCP dipole 3 (mV)
101	95	92

Calibration curves $e_i=f(V)$ ($i=1,2,3$) allow to obtain H-field value using the formula:

$$E = \sqrt{E_1^2 + E_2^2 + E_3^2}$$

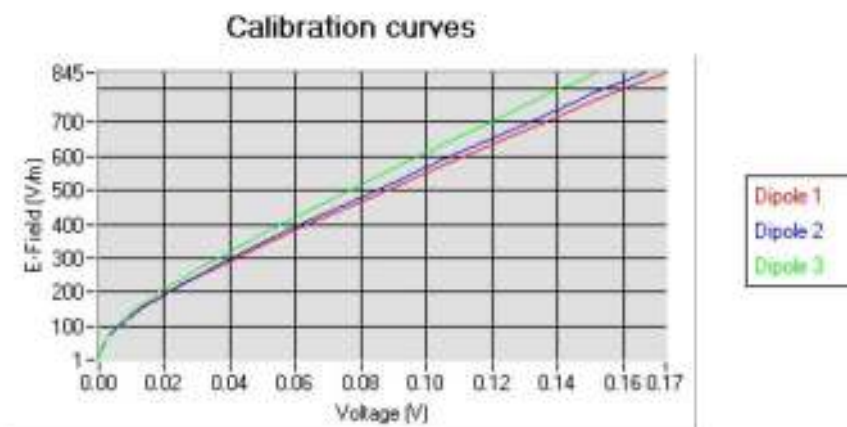

Page: 6/10


*This document shall not be reproduced, except in full or in part, without the written approval of SATIMO.
The information contained herein is to be used only for the purpose for which it is intended and is not to be released in whole or part without written approval of SATIMO.*



COMOSAR E-FIELD PROBE CALIBRATION REPORT

Ref: ACR-137.1.13.SATU.A

5.2 LINEARITY

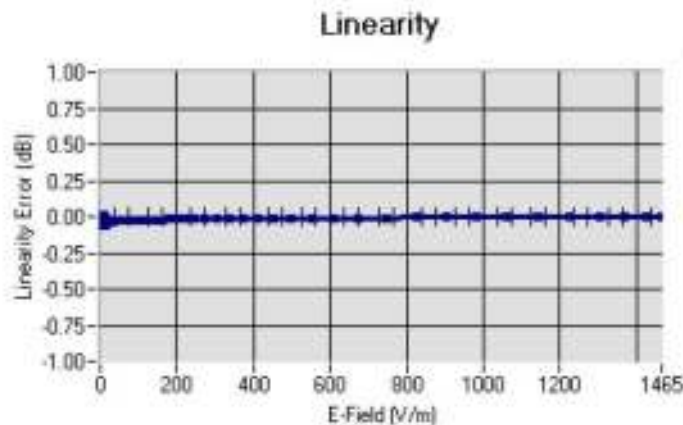

Linearity: $\pm 1.50\%$ ($\pm 0.07\text{dB}$)

5.3 SENSITIVITY IN LIQUID

Liquid	Frequency (MHz $\pm$ 100MHz)	Permittivity	Epsilon (S/m)	ConvF
HL850	835	42.56	0.88	3.49
BL850	835	55.26	0.96	3.59
HL900	900	41.79	0.96	3.40
BL900	900	55.98	1.04	3.53
HL1800	1750	40.17	1.38	3.95
BL1800	1750	52.05	1.48	4.04
HL1900	1880	39.80	1.43	4.53
BL1900	1880	52.55	1.50	4.68
HL2000	1950	38.93	1.44	4.08
BL2000	1950	53.12	1.51	4.22
HL2450	2450	38.64	1.82	4.31
BL2450	2450	52.02	1.94	4.43
HL3500	3500	36.42	3.07	4.55
BL3500	3500	51.56	3.24	4.72
HL5200	5200	36.11	4.81	4.95
BL5200	5200	49.87	4.99	5.11
HL5400	5400	36.61	5.08	5.35
BL5400	5400	49.09	5.64	5.54
HL5600	5600	35.97	5.37	5.25
BL5600	5600	48.64	5.99	5.41
HL5800	5800	35.33	5.59	5.65
BL5800	5800	47.76	6.21	5.80

LOWER DETECTION LIMIT: 7mW/kg

Page: 7/10

This document shall not be reproduced, except in full or in part, without the written approval of SATIMO. The information contained herein is to be used only for the purpose for which it is intended and is not to be released in whole or part without written approval of SATIMO.

Test report No.	FCC,IC_SAR_SL14031101-SLX-004 Rev1.0
Page	49 of 100
FCC ID	STJ-SDMAN
IC ID	5627A-SDMAN




COMOSAR E-FIELD PROBE CALIBRATION REPORT

Ref: ACR-137.1.13.SATU.A

5.4 ISOTROPY


HL 900 MHz

- Axial isotropy: 0.04 dB
- Hemispherical isotropy: 0.07 dB

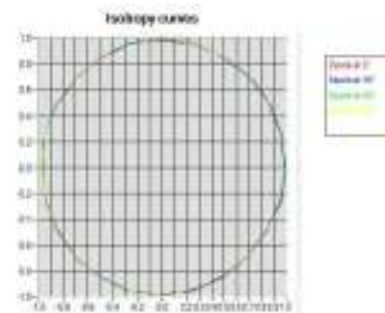

HL 1800 MHz

- Axial isotropy: 0.05 dB
- Hemispherical isotropy: 0.08 dB

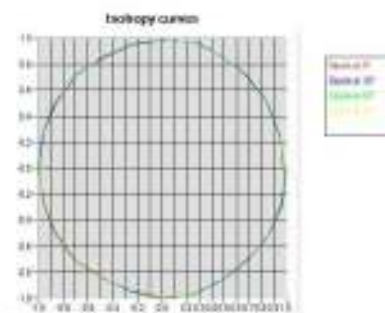

Page: 8/10

*This document shall not be reproduced, except in full or in part, without the written approval of SATIMO.
The information contained herein is to be used only for the purpose for which it is intended and is not to be released in whole or part without written approval of SATIMO.*

Test report No.	FCC,IC_SAR_SL14031101-SLX-004 Rev1.0
Page	50 of 100
FCC ID	STJ-SDMAN
IC ID	5627A-SDMAN




COMOSAR E-FIELD PROBE CALIBRATION REPORT

Ref: ACR-137.1.13.SATU.A


HL 2450 MHz

- Axial isotropy: 0.07 dB
- Hemispherical isotropy: 0.10 dB

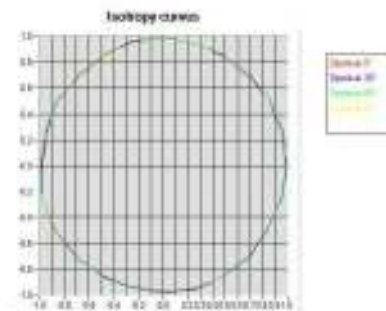

HL 5800 MHz

- Axial isotropy: 0.08 dB
- Hemispherical isotropy: 0.11 dB

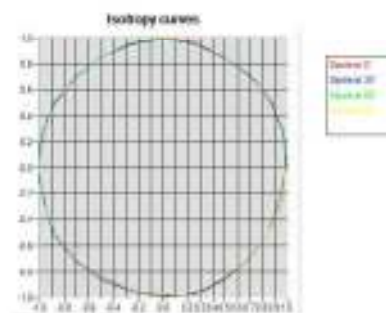

Page: 9/10

*This document shall not be reproduced, except in full or in part, without the written approval of SATIMO.
The information contained herein is to be used only for the purpose for which it is intended and is not to be released in whole or part without written approval of SATIMO.*

Test report No.	FCC,IC_SAR_SL14031101-SLX-004 Rev1.0
Page	51 of 100
FCC ID	STJ-SDMAN
IC ID	5627A-SDMAN



COMOSAR E-FIELD PROBE CALIBRATION REPORT

Ref: ACR-137.1.13.SATU.A

6 LIST OF EQUIPMENT

Equipment Summary Sheet				
Equipment Description	Manufacturer / Model	Identification No.	Current Calibration Date	Next Calibration Date
Flat Phantom	Satimo	SN-20/09-SAM71	Validated. No cal required.	Validated. No cal required.
COMOSAR Test Bench	Version 3	NA	Validated. No cal required.	Validated. No cal required.
Network Analyzer	Rhode & Schwarz ZVA	SN100132	02/2013	02/2016
Reference Probe	Satimo	EP 94 SN 37/08	Characterized prior to test. No cal required.	Characterized prior to test. No cal required.
Multimeter	Keithley 2000	1188656	11/2010	11/2013
Signal Generator	Agilent E4438C	MY49070581	12/2010	12/2013
Amplifier	Aethercomm	SN 046	Characterized prior to test. No cal required.	Characterized prior to test. No cal required.
Power Meter	HP E4418A	US38261498	11/2010	11/2013
Power Sensor	HP ECP-E26A	US37161460	11/2010	11/2013
Directional Coupler	Narda 4216-20	01386	Characterized prior to test. No cal required.	Characterized prior to test. No cal required.
Waveguide	Mega Industries	069Y7-158-13-712	Validated. No cal required.	Validated. No cal required.
Waveguide Transition	Mega Industries	069Y7-158-13-701	Validated. No cal required.	Validated. No cal required.
Waveguide Termination	Mega Industries	069Y7-158-13-701	Validated. No cal required.	Validated. No cal required.
Temperature / Humidity Sensor	Control Company	11-661-9	3/2012	3/2014

Page: 10/10

*This document shall not be reproduced, except in full or in part, without the written approval of SATIMO.
The information contained herein is to be used only for the purpose for which it is submitted and is not to be released in whole or part without written approval of SATIMO.*

Test report No.	FCC,IC_SAR_SL14031101-SLX-004 Rev1.0
Page	52 of 100
FCC ID	STJ-SDMAN
IC ID	5627A-SDMAN



SAR Reference Dipole Calibration Report

Ref : ACR.170.6.12.SATU.A

SIEMIC TESTING AND CERTIFICATION SERVICES

2206 RINGWOOD AVE.

SAN JOSE, CA 95131, USA

SATIMO COMOSAR REFERENCE DIPOLE

FREQUENCY: 2000 MHZ

SERIAL NO.: SN 31/10 DIPI137

Calibrated at SATIMO US

2105 Barrett Park Dr. - Kennesaw, GA 30144



06/13/2012

Summary:

This document presents the method and results from an accredited SAR reference dipole calibration performed in SATIMO USA using the COMOSAR test bench. All calibration results are traceable to national metrology institutions.

Test report No.	FCC,IC_SAR_SL14031101-SLX-004 Rev1.0
Page	53 of 100
FCC ID	STJ-SDMAN
IC ID	5627A-SDMAN



SAR REFERENCE DIPOLE CALIBRATION REPORT

Ref: ACR.170.6.12.SATU.A

	<i>Name</i>	<i>Function</i>	<i>Date</i>	<i>Signature</i>
<i>Prepared by :</i>	Jérôme LUC	Product Manager	6/18/2012	
<i>Checked by :</i>	Jérôme LUC	Product Manager	6/18/2012	
<i>Approved by :</i>	Kim RUTKOWSKI	Quality Manager	6/18/2012	

	<i>Customer Name</i>
<i>Distribution :</i>	SIEMIC Testing and Certification Services

<i>Issue</i>	<i>Date</i>	<i>Modifications</i>
A	6/18/2012	Initial release

Page: 29

*This document shall not be reproduced, except in full or in part, without the written approval of SATIMO.
The information contained herein is to be used only for the purpose for which it is submitted and is not to be released in whole or part without written approval of SATIMO.*

Test report No.	FCC,IC_SAR_SL14031101-SLX-004 Rev1.0
Page	54 of 100
FCC ID	STJ-SDMAN
IC ID	5627A-SDMAN



TABLE OF CONTENTS

1	Introduction.....	4
2	Device Under Test	4
3	Product Description	4
3.1	General Information	4
4	Measurement Method	5
4.1	Return Loss Requirements	5
4.2	Mechanical Requirements	5
5	Measurement Uncertainty	5
5.1	Return Loss	5
5.2	Dimension Measurement	5
5.3	Validation Measurement	5
6	Calibration Measurement Results	6
6.1	Return Loss	6
6.2	Mechanical Dimensions	6
7	Validation measurement	7
7.1	Measurement Condition	7
7.2	Head Liquid Measurement	7
7.3	Measurement Result	8
8	List of Equipment	8

Test report No.	FCC,IC_SAR_SL14031101-SLX-004 Rev1.0
Page	55 of 100
FCC ID	STJ-SDMAN
IC ID	5627A-SDMAN



SAR REFERENCE DIPOLE CALIBRATION REPORT

Ref: ACR.170.6.12.SATU.A

1 INTRODUCTION

This document contains a summary of the requirements set forth by the IEEE 1528, OET 65 Bulletin C and CEI/IEC 62209 standards for reference dipoles used for SAR measurement system validations and the measurements that were performed to verify that the product complies with the fore mentioned standards.

2 DEVICE UNDER TEST

Device Under Test	
Device Type	COMOSAR 2000 MHz REFERENCE DIPOLE
Manufacturer	Satimo
Model	SID2000
Serial Number	SN 31/10 DIP1137
Product Condition (new / used)	used

A yearly calibration interval is recommended.

3 PRODUCT DESCRIPTION

3.1 GENERAL INFORMATION

Satimo's COMOSAR Validation Dipoles are built in accordance to the IEEE 1528, OET 65 Bulletin C and CEI/IEC 62209 standards. The product is designed for use with the COMOSAR test bench only.



Figure 1 – Satimo COMOSAR Validation Dipole

Page: 4/9

This document shall not be reproduced, except in full or in part, without the written approval of SATIMO. The information contained herein is to be used only for the purpose for which it is submitted and is not to be released in whole or part without written approval of SATIMO.



4 MEASUREMENT METHOD

The IEEE 1528, OET 65 Bulletin C and CEI/IEC 62209 standards provide requirements for reference dipoles used for system validation measurements. The following measurements were performed to verify that the product complies with the fore mentioned standards.

4.1 RETURN LOSS REQUIREMENTS

The dipole used for SAR system validation measurements and checks must have a return loss of -20 dB or better. The return loss measurement shall be performed against a liquid filled flat phantom, with the phantom constructed as outlined in the fore mentioned standards.

4.2 MECHANICAL REQUIREMENTS

The IEEE Std. 1528 and CEI/IEC 62209 standards specify the mechanical components and dimensions of the validation dipoles, with the dimensions frequency and phantom shell thickness dependent. The COMOSAR test bench employs a 2 mm phantom shell thickness therefore the dipoles sold for use with the COMOSAR test bench comply with the requirements set forth for a 2 mm phantom shell thickness.

5 MEASUREMENT UNCERTAINTY

All uncertainties listed below represent an expanded uncertainty expressed at approximately the 95% confidence level using a coverage factor of $k=2$, traceable to the Internationally Accepted Guides to Measurement Uncertainty.

5.1 RETURN LOSS

The following uncertainties apply to the return loss measurement:

Frequency band	Expanded Uncertainty on Return Loss
400-6000MHz	0.1 dB

5.2 DIMENSION MEASUREMENT

The following uncertainties apply to the dimension measurements:

Length (mm)	Expanded Uncertainty on Length
3 - 300	0.05 mm

5.3 VALIDATION MEASUREMENT

The guidelines outlined in the IEEE 1528, OET 65 Bulletin C, CENELEC EN50361 and CEI/IEC 62209 standards were followed to generate the measurement uncertainty for validation measurements.

Scan Volume	Expanded Uncertainty
1 g	16.19 %
10 g	15.86 %

Page: 5/9

*This document shall not be reproduced, except in full or in part, without the written approval of SATIMO.
The information contained herein is to be used only for the purpose for which it is submitted and is not to be released in whole or part without written approval of SATIMO.*




SAR REFERENCE DIPOLE CALIBRATION REPORT

Ref: ACR.170.6.12.SATU.A

6 CALIBRATION MEASUREMENT RESULTS

6.1 RETURN LOSS

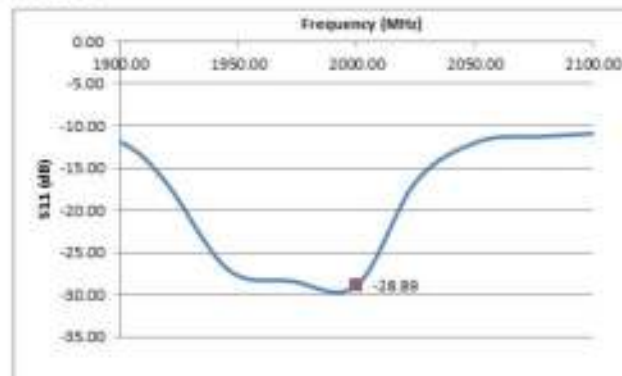

Frequency (MHz)	Return Loss (dB)	Requirement (dB)
2000	-28.89	-20

6.2 MECHANICAL DIMENSIONS

Frequency MHz	L mm		h mm		d mm	
	required	measured	required	measured	required	measured
300	420.0 ±1 %		250.0 ±1 %		6.35 ±1 %	
450	290.0 ±1 %		166.7 ±1 %		6.35 ±1 %	
750	176.0 ±1 %		100.0 ±1 %		6.35 ±1 %	
835	161.0 ±1 %		89.8 ±1 %		3.6 ±1 %	
900	149.0 ±1 %		83.3 ±1 %		3.6 ±1 %	
1450	89.1 ±1 %		51.7 ±1 %		3.6 ±1 %	
1500	80.5 ±1 %		50.0 ±1 %		3.6 ±1 %	
1640	79.0 ±1 %		45.7 ±1 %		3.6 ±1 %	
1750	75.2 ±1 %		42.9 ±1 %		3.6 ±1 %	
1800	72.0 ±1 %		41.7 ±1 %		3.6 ±1 %	
1900	68.0 ±1 %		39.5 ±1 %		3.6 ±1 %	
1950	66.3 ±1 %		38.5 ±1 %		3.6 ±1 %	
2000	64.5 ±1 %	PASS	37.5 ±1 %	PASS	3.6 ±1 %	PASS
2100	61.0 ±1 %		35.7 ±1 %		3.6 ±1 %	
2300	55.5 ±1 %		32.6 ±1 %		3.6 ±1 %	
2450	51.5 ±1 %		30.4 ±1 %		3.6 ±1 %	
2600	48.5 ±1 %		28.8 ±1 %		3.6 ±1 %	
3000	41.5 ±1 %		25.0 ±1 %		3.6 ±1 %	
3500	37.0 ±1 %		26.4 ±1 %		3.6 ±1 %	
3700	34.7 ±1 %		26.4 ±1 %		3.6 ±1 %	

Page: 6/9

*This document shall not be reproduced, except in full or in part, without the written approval of SATIMO.
The information contained herein is to be used only for the purpose for which it is intended and is not to be released in whole or part without written approval of SATIMO.*



7 VALIDATION MEASUREMENT

The IEEE Std. 1528, OET 65 Bulletin C and CEI/IEC 62209 standards state that the system validation measurements must be performed using a reference dipole meeting the fore mentioned return loss and mechanical dimension requirements. The validation measurement must be performed against a liquid filled flat phantom, with the phantom constructed as outlined in the fore mentioned standards. Per the standards, the dipole shall be positioned below the bottom of the phantom, with the dipole length centered and parallel to the longest dimension of the flat phantom, with the top surface of the dipole at the described distance from the bottom surface of the phantom.

7.1 MEASUREMENT CONDITION

Software	OPENSAR V4
Phantom	SN 20/09 SAM71
Probe	SN 18/11 EPG122
Liquid	Head Liquid Values: ϵ_{ps} : 39.5 σ : 1.43
Distance between dipole center and liquid	10.0 mm
Area scan resolution	$dx=8mm/dy=8mm$
Zoom Scan Resolution	$dx=8mm/dy=8mm/dz=5mm$
Frequency	2000 MHz
Input power	20 dBm
Liquid Temperature	21 °C
Lab Temperature	21 °C
Lab Humidity	45 %

7.2 HEAD LIQUID MEASUREMENT

Frequency MHz	Relative permittivity (ϵ_r)		Conductivity (σ) S/m	
	required	measured	required	measured
300	45.3 $\pm$ 5 %		0.87 $\pm$ 5 %	
450	43.5 $\pm$ 5 %		0.87 $\pm$ 5 %	
750	41.9 $\pm$ 5 %		0.89 $\pm$ 5 %	
835	41.5 $\pm$ 5 %		0.90 $\pm$ 5 %	
900	41.5 $\pm$ 5 %		0.97 $\pm$ 5 %	
1450	40.5 $\pm$ 5 %		1.20 $\pm$ 5 %	
1500	40.4 $\pm$ 5 %		1.23 $\pm$ 5 %	
1640	40.2 $\pm$ 5 %		1.31 $\pm$ 5 %	
1750	40.1 $\pm$ 5 %		1.37 $\pm$ 5 %	
1800	40.0 $\pm$ 5 %		1.40 $\pm$ 5 %	
1900	40.0 $\pm$ 5 %		1.40 $\pm$ 5 %	
1950	40.0 $\pm$ 5 %		1.40 $\pm$ 5 %	
2000	40.0 $\pm$ 5 %	PASS	1.40 $\pm$ 5 %	PASS
2100	39.8 $\pm$ 5 %		1.49 $\pm$ 5 %	
2300	39.5 $\pm$ 5 %		1.67 $\pm$ 5 %	
2450	39.2 $\pm$ 5 %		1.80 $\pm$ 5 %	
2600	39.0 $\pm$ 5 %		1.96 $\pm$ 5 %	
3000	38.5 $\pm$ 5 %		2.40 $\pm$ 5 %	
3500	37.9 $\pm$ 5 %		2.91 $\pm$ 5 %	

Page: 7/9

*This document shall not be reproduced, except in full or in part, without the written approval of SATIMO.
The information contained herein is to be used only for the purpose for which it is submitted and is not to be released in whole or part without written approval of SATIMO.*




SAR REFERENCE DIPOLE CALIBRATION REPORT

Ref: ACR.170.6.12.SATU.A

7.3 MEASUREMENT RESULT

The IEEE Std. 1528 and CEI/IEC 62209 standards state that the system validation measurements should produce the SAR values shown below (for phantom thickness of 2 mm), within the uncertainty for the system validation. All SAR values are normalized to 1 W forward power. In bracket, the measured SAR is given with the used input power.

Frequency MHz	1 g SAR (W/kg/W)		10 g SAR (W/kg/W)	
	required	measured	required	measured
300	2.85		1.94	
450	4.58		3.06	
750	8.49		5.55	
835	9.56		6.22	
900	10.9		6.99	
1450	29		16	
1500	30.5		16.8	
1640	34.2		18.4	
1750	36.4		19.3	
1800	38.4		20.1	
1900	39.7		20.5	
1950	40.5		20.9	
2000	41.1	43.67 (4.37)	21.1	21.32 (2.13)
2100	43.6		21.9	
2300	48.7		23.3	
2450	52.4		24	
2600	55.3		24.6	
3000	63.8		25.7	
3500	67.1		25	

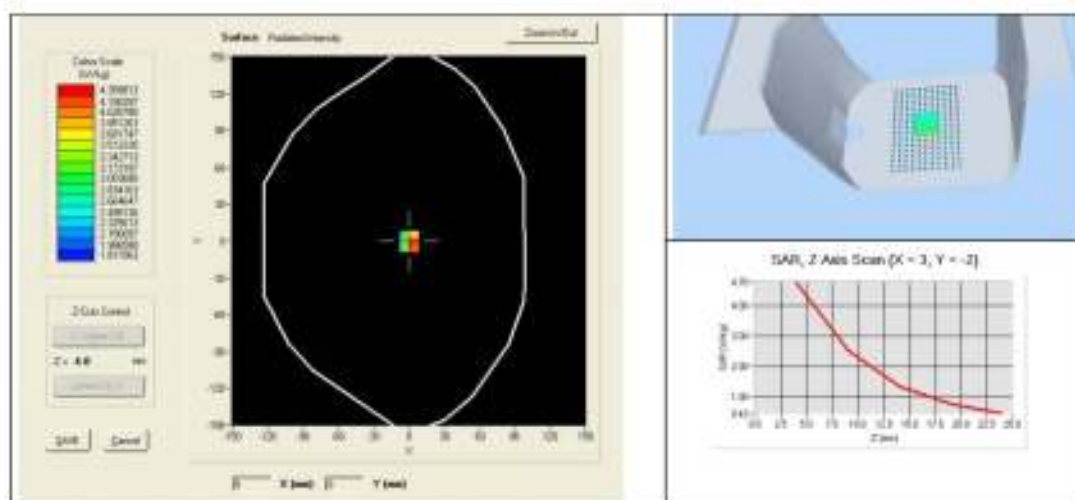

Page: 8/9

*This document shall not be reproduced, except in full or in part, without the written approval of SATIMO.
The information contained herein is to be used only for the purpose for which it is submitted and is not to be released in whole or part without written approval of SATIMO.*

Test report No.	FCC,IC_SAR_SL14031101-SLX-004 Rev1.0
Page	60 of 100
FCC ID	STJ-SDMAN
IC ID	5627A-SDMAN



SAR REFERENCE DIPOLE CALIBRATION REPORT

Ref: ACR.170.6.12.SATU.A

8 LIST OF EQUIPMENT

Equipment Summary Sheet				
Equipment Description	Manufacturer / Model	Identification No.	Current Calibration Date	Next Calibration Date
Flat Phantom	Satimo	SN-20/09-SAM71	Validated. No cal required.	Validated. No cal required.
COMOSAR Test Bench	Version 3	NA	Validated. No cal required.	Validated. No cal required.
Network Analyzer	Rhode & Schwarz ZVA	SN100132	02/2010	02/2013
Calipers	Camera	CALIPER-01	12/2010	12/2013
Reference Probe	Satimo	EPG122 SN 18/11	Characterized prior to test. No cal required.	Characterized prior to test. No cal required.
Multimeter	Keithley 2000	1188656	11/2010	11/2013
Signal Generator	Agilent E4438C	MY49070581	12/2010	12/2013
Amplifier	Aethercomm	SN 046	Characterized prior to test. No cal required.	Characterized prior to test. No cal required.
Power Meter	HP E4418A	US38261498	11/2010	11/2013
Power Sensor	HP ECP-E26A	US37181460	11/2010	11/2013
Directional Coupler	Narda 4216-20	01386	Characterized prior to test. No cal required.	Characterized prior to test. No cal required.
Temperature and Humidity Sensor	Control Company	11-661-9	3/2012	3/2014

Page: 9/9

*This document shall not be reproduced, except in full or in part, without the written approval of SATIMO.
The information contained herein is to be used only for the purpose for which it is intended and is not to be released in whole or part without written approval of SATIMO.*

Test report No.	FCC,IC_SAR_SL14031101-SLX-004 Rev1.0
Page	61 of 100
FCC ID	STJ-SDMAN
IC ID	5627A-SDMAN


SARTIMO Calibration Certificate-Extended Dipole Calibrations

According to KDB 450824 D02, Dipoles must be recalibrated at least once every three years; however, immediate re-calibration is required for following conditions. The test laboratory must ensure that the required supporting information and documentation have been included in the SAR report to qualify for extended 3-year calibration interval.

- 1) When the most recent return-loss, measured at least annually, deviates by more than 20% from the previous measurement (i.e. 0.2 of the dB value) or not meeting the required -20 dB return-loss specification
- 2) When the most recent measurement of the real or imaginary parts of the impedance, measured at least annually, deviates by more than 5 Ω from the previous measurement

Dipole Verification plot: SID2000

2000MHz for Head:

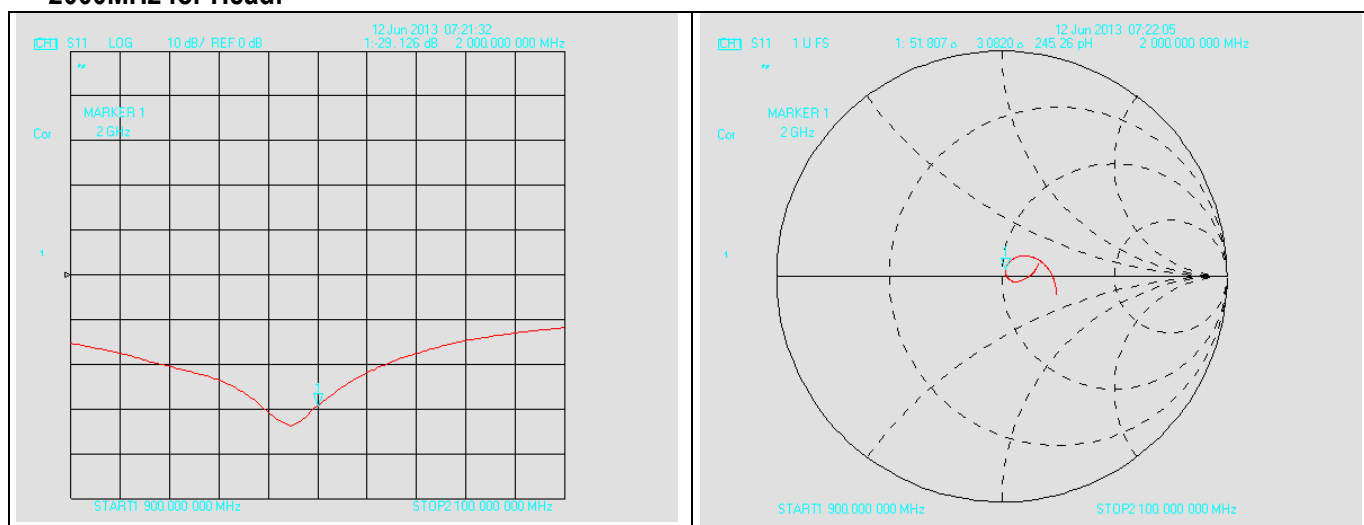

Summary results:

SID 2000					
Return- Loss (dB)	Deviate (dB)	Real Impedance (Ω)	Imaginary Impedance (Ω)	Deviate (Ω)	Calibrate Date
-28.89	-----	-----	50	-----	06/13/2013
-29.126	-0.236	51.807	50	1.807	06/12/2014

According to up table, the return loss is <-20dB, deviates by less than 20% from the previous measurement; the real Impedance are all within 5 Ω compared to the required Impedance (50 Ω).

Test report No.	FCC,IC_SAR_SL14031101-SLX-004 Rev1.0
Page	62 of 100
FCC ID	STJ-SDMAN
IC ID	5627A-SDMAN



SAR Reference Dipole Calibration Report

Ref : ACR.170.7.12.SATU.A

SIEMIC TESTING AND CERTIFICATION SERVICES

2206 RINGWOOD AVE.
SAN JOSE, CA 95131, USA

SATIMO COMOSAR REFERENCE DIPOLE

FREQUENCY: 2450 MHZ
SERIAL NO.: SN 31/10 DIPJ138

Calibrated at SATIMO US
2105 Barrett Park Dr. - Kennesaw, GA 30144



06/13/2012

Summary:

This document presents the method and results from an accredited SAR reference dipole calibration performed in SATIMO USA using the COMOSAR test bench. All calibration results are traceable to national metrology institutions.

Test report No.	FCC,IC_SAR_SL14031101-SLX-004 Rev1.0
Page	63 of 100
FCC ID	STJ-SDMAN
IC ID	5627A-SDMAN



SAR REFERENCE DIPOLE CALIBRATION REPORT

Ref: ACR.170.7.12.SATU.A

	<i>Name</i>	<i>Function</i>	<i>Date</i>	<i>Signature</i>
<i>Prepared by :</i>	Jérôme LUC	Product Manager	6/18/2012	
<i>Checked by :</i>	Jérôme LUC	Product Manager	6/18/2012	
<i>Approved by :</i>	Kim RUTKOWSKI	Quality Manager	6/18/2012	

	<i>Customer Name</i>
<i>Distribution :</i>	SIEMIC Testing and Certification Services

<i>Issue</i>	<i>Date</i>	<i>Modifications</i>
A	6/18/2012	Initial release

Page: 2/9

*This document shall not be reproduced, except in full or in part, without the written approval of SATIMO.
The information contained herein is to be used only for the purpose for which it is submitted and is not to be released in whole or part without written approval of SATIMO.*

Test report No.	FCC,IC_SAR_SL14031101-SLX-004 Rev1.0
Page	64 of 100
FCC ID	STJ-SDMAN
IC ID	5627A-SDMAN



SAR REFERENCE DIPOLE CALIBRATION REPORT

Ref: ACR.170.7.12.SATU.A

TABLE OF CONTENTS

1	Introduction.....	4
2	Device Under Test	4
3	Product Description	4
3.1	General Information	4
4	Measurement Method	5
4.1	Return Loss Requirements	5
4.2	Mechanical Requirements	5
5	Measurement Uncertainty	5
5.1	Return Loss	5
5.2	Dimension Measurement	5
5.3	Validation Measurement	5
6	Calibration Measurement Results	6
6.1	Return Loss	6
6.2	Mechanical Dimensions	6
7	Validation measurement	7
7.1	Measurement Condition	7
7.2	Head Liquid Measurement	7
7.3	Measurement Result	8
8	List of Equipment	8

Page: 3/9

*This document shall not be reproduced, except in full or in part, without the written approval of SATIMO.
The information contained herein is to be used only for the purpose for which it is submitted and is not to be released in whole or part without written approval of SATIMO.*



1 INTRODUCTION

This document contains a summary of the requirements set forth by the IEEE 1528, OET 65 Bulletin C and CEI/IEC 62209 standards for reference dipoles used for SAR measurement system validations and the measurements that were performed to verify that the product complies with the fore mentioned standards.

2 DEVICE UNDER TEST

Device Under Test	
Device Type	COMOSAR 2450 MHz REFERENCE DIPOLE
Manufacturer	Satimo
Model	SID2450
Serial Number	SN 31/10 DIPJ138
Product Condition (new / used)	used

A yearly calibration interval is recommended.

3 PRODUCT DESCRIPTION

3.1 GENERAL INFORMATION

Satimo's COMOSAR Validation Dipoles are built in accordance to the IEEE 1528, OET 65 Bulletin C and CEI/IEC 62209 standards. The product is designed for use with the COMOSAR test bench only.



Figure 1 – Satimo COMOSAR Validation Dipole

Test report No.	FCC,IC_SAR_SL14031101-SLX-004 Rev1.0
Page	66 of 100
FCC ID	STJ-SDMAN
IC ID	5627A-SDMAN



SAR REFERENCE DIPOLE CALIBRATION REPORT

Ref: ACR.170.7.12.SATU.A

4 MEASUREMENT METHOD

The IEEE 1528, OET 65 Bulletin C and CEI/IEC 62209 standards provide requirements for reference dipoles used for system validation measurements. The following measurements were performed to verify that the product complies with the fore mentioned standards.

4.1 RETURN LOSS REQUIREMENTS

The dipole used for SAR system validation measurements and checks must have a return loss of -20 dB or better. The return loss measurement shall be performed against a liquid filled flat phantom, with the phantom constructed as outlined in the fore mentioned standards.

4.2 MECHANICAL REQUIREMENTS

The IEEE Std. 1528 and CEI/IEC 62209 standards specify the mechanical components and dimensions of the validation dipoles, with the dimensions frequency and phantom shell thickness dependent. The COMOSAR test bench employs a 2 mm phantom shell thickness therefore the dipoles sold for use with the COMOSAR test bench comply with the requirements set forth for a 2 mm phantom shell thickness.

5 MEASUREMENT UNCERTAINTY

All uncertainties listed below represent an expanded uncertainty expressed at approximately the 95% confidence level using a coverage factor of $k=2$, traceable to the Internationally Accepted Guides to Measurement Uncertainty.

5.1 RETURN LOSS

The following uncertainties apply to the return loss measurement:

Frequency band	Expanded Uncertainty on Return Loss
400-6000MHz	0.1 dB

5.2 DIMENSION MEASUREMENT

The following uncertainties apply to the dimension measurements:

Length (mm)	Expanded Uncertainty on Length
3 - 300	0.05 mm

5.3 VALIDATION MEASUREMENT

The guidelines outlined in the IEEE 1528, OET 65 Bulletin C, CENELEC EN50361 and CEI/IEC 62209 standards were followed to generate the measurement uncertainty for validation measurements.

Scan Volume	Expanded Uncertainty
1 g	16.19 %
10 g	15.86 %

Page: 5/9

*This document shall not be reproduced, except in full or in part, without the written approval of SATIMO.
The information contained herein is to be used only for the purpose for which it is submitted and is not to be released in whole or part without written approval of SATIMO.*




SAR REFERENCE DIPOLE CALIBRATION REPORT

Ref: ACR.170.7.12.SATU.A

6 CALIBRATION MEASUREMENT RESULTS

6.1 RETURN LOSS

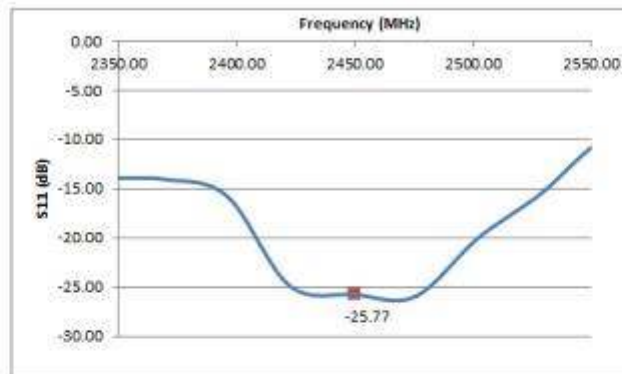

Frequency (MHz)	Return Loss (dB)	Requirement (dB)
2450	-25.77	-20

6.2 MECHANICAL DIMENSIONS

Frequency MHz	L mm		h mm		d mm	
	required	measured	required	measured	required	measured
300	420.0 ±1 %		250.0 ±1 %		6.35 ±1 %	
450	290.0 ±1 %		166.7 ±1 %		6.35 ±1 %	
750	176.0 ±1 %		100.0 ±1 %		6.35 ±1 %	
835	161.0 ±1 %		89.8 ±1 %		3.6 ±1 %	
900	149.0 ±1 %		83.3 ±1 %		3.6 ±1 %	
1450	89.1 ±1 %		51.7 ±1 %		3.6 ±1 %	
1500	80.5 ±1 %		50.0 ±1 %		3.6 ±1 %	
1640	79.0 ±1 %		45.7 ±1 %		3.6 ±1 %	
1750	75.2 ±1 %		42.9 ±1 %		3.6 ±1 %	
1800	72.0 ±1 %		41.7 ±1 %		3.6 ±1 %	
1900	68.0 ±1 %		39.5 ±1 %		3.6 ±1 %	
1950	66.3 ±1 %		38.5 ±1 %		3.6 ±1 %	
2000	64.5 ±1 %		37.5 ±1 %		3.6 ±1 %	
2100	61.0 ±1 %		35.7 ±1 %		3.6 ±1 %	
2300	55.5 ±1 %		32.6 ±1 %		3.6 ±1 %	
2450	51.5 ±1 %	PASS	30.4 ±1 %	PASS	3.6 ±1 %	PASS
2600	48.5 ±1 %		28.8 ±1 %		3.6 ±1 %	
3000	41.5 ±1 %		25.0 ±1 %		3.6 ±1 %	
3500	37.0 ±1 %		26.4 ±1 %		3.6 ±1 %	
3700	34.7 ±1 %		26.4 ±1 %		3.6 ±1 %	

Page: 6/9

*This document shall not be reproduced, except in full or in part, without the written approval of SATIMO.
The information contained herein is to be used only for the purpose for which it is submitted and is not to be released in whole or part without written approval of SATIMO.*



SAR REFERENCE DIPOLE CALIBRATION REPORT

Ref: ACR.170.7.12.SATU.A

7 VALIDATION MEASUREMENT

The IEEE Std. 1528, OET 65 Bulletin C and CEI/IEC 62209 standards state that the system validation measurements must be performed using a reference dipole meeting the fore mentioned return loss and mechanical dimension requirements. The validation measurement must be performed against a liquid filled flat phantom, with the phantom constructed as outlined in the fore mentioned standards. Per the standards, the dipole shall be positioned below the bottom of the phantom, with the dipole length centered and parallel to the longest dimension of the flat phantom, with the top surface of the dipole at the described distance from the bottom surface of the phantom.

7.1 MEASUREMENT CONDITION

Software	OPENSAR V4
Phantom	SN 20/09 SAM71
Probe	SN 18/11 EPG122
Liquid	Head Liquid Values: ϵ_p : 39.0 sigma : 1.88
Distance between dipole center and liquid	10.0 mm
Area scan resolution	dx=8mm/dy=8mm
Zoon Scan Resolution	dx=8mm/dy=8m/dz=5mm
Frequency	2450 MHz
Input power	20 dBm
Liquid Temperature	21 °C
Lab Temperature	21 °C
Lab Humidity	45 %

7.2 HEAD LIQUID MEASUREMENT

Frequency MHz	Relative permittivity (ϵ_r)		Conductivity (σ) S/m	
	required	measured	required	measured
300	45.3 $\pm$ 5 %		0.87 $\pm$ 5 %	
450	43.5 $\pm$ 5 %		0.87 $\pm$ 5 %	
750	41.9 $\pm$ 5 %		0.89 $\pm$ 5 %	
835	41.5 $\pm$ 5 %		0.90 $\pm$ 5 %	
900	41.5 $\pm$ 5 %		0.97 $\pm$ 5 %	
1450	40.5 $\pm$ 5 %		1.20 $\pm$ 5 %	
1500	40.4 $\pm$ 5 %		1.23 $\pm$ 5 %	
1640	40.2 $\pm$ 5 %		1.31 $\pm$ 5 %	
1750	40.1 $\pm$ 5 %		1.37 $\pm$ 5 %	
1800	40.0 $\pm$ 5 %		1.40 $\pm$ 5 %	
1900	40.0 $\pm$ 5 %		1.40 $\pm$ 5 %	
1950	40.0 $\pm$ 5 %		1.40 $\pm$ 5 %	
2000	40.0 $\pm$ 5 %		1.40 $\pm$ 5 %	
2100	39.8 $\pm$ 5 %		1.49 $\pm$ 5 %	
2300	39.5 $\pm$ 5 %		1.67 $\pm$ 5 %	
2450	39.2 $\pm$ 5 %	PASS	1.80 $\pm$ 5 %	PASS
2600	39.0 $\pm$ 5 %		1.96 $\pm$ 5 %	
3000	38.5 $\pm$ 5 %		2.40 $\pm$ 5 %	
3500	37.9 $\pm$ 5 %		2.91 $\pm$ 5 %	

Page: 7/9

This document shall not be reproduced, except in full or in part, without the written approval of SATIMO. The information contained herein is to be used only for the purpose for which it is submitted and is not to be released in whole or part without written approval of SATIMO.




SAR REFERENCE DIPOLE CALIBRATION REPORT

Ref: ACR.170.7.12.SATU.A

7.3 MEASUREMENT RESULT

The IEEE Std. 1528 and CEI/IEC 62209 standards state that the system validation measurements should produce the SAR values shown below (for phantom thickness of 2 mm), within the uncertainty for the system validation. All SAR values are normalized to 1 W forward power. In bracket, the measured SAR is given with the used input power.

Frequency MHz	1 g SAR (W/kg/W)		10 g SAR (W/kg/W)	
	required	measured	required	measured
300	2.85		1.94	
450	4.58		3.06	
750	8.49		5.55	
835	9.56		6.22	
900	10.9		6.99	
1450	29		16	
1500	30.5		16.8	
1640	34.2		18.4	
1750	36.4		19.3	
1800	38.4		20.1	
1900	39.7		20.5	
1950	40.5		20.9	
2000	41.1		21.1	
2100	43.6		21.9	
2300	48.7		23.3	
2450	52.4	54.82 (5.48)	24	24.50 (2.45)
2600	55.3		24.6	
3000	63.8		25.7	
3500	67.1		25	

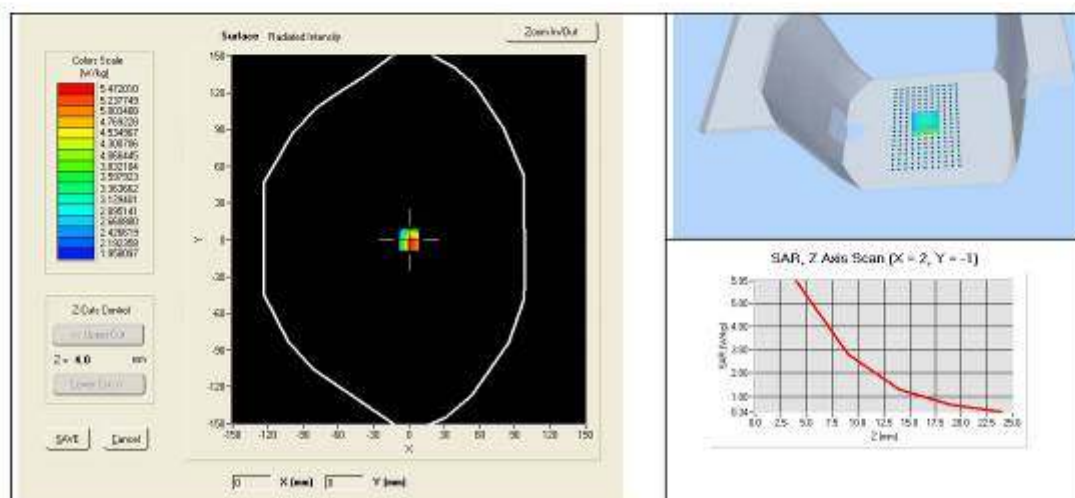

Page: 8/9

This document shall not be reproduced, except in full or in part, without the written approval of SATIMO.
The information contained herein is to be used only for the purpose for which it is submitted and is not to be released in whole or part without written approval of SATIMO.

Test report No.	FCC,IC_SAR_SL14031101-SLX-004 Rev1.0
Page	70 of 100
FCC ID	STJ-SDMAN
IC ID	5627A-SDMAN



SAR REFERENCE DIPOLE CALIBRATION REPORT

Ref: ACR.170.7.12.SATU.A

8 LIST OF EQUIPMENT

Equipment Summary Sheet				
Equipment Description	Manufacturer / Model	Identification No.	Current Calibration Date	Next Calibration Date
Flat Phantom	Satimo	SN-20/09-SAM71	Validated. No cal required.	Validated. No cal required.
COMOSAR Test Bench	Version 3	NA	Validated. No cal required.	Validated. No cal required.
Network Analyzer	Rhode & Schwarz ZVA	SN100132	02/2010	02/2013
Calipers	Carrera	CALIPER-01	12/2010	12/2013
Reference Probe	Satimo	EPG122 SN 18/11	Characterized prior to test. No cal required.	Characterized prior to test. No cal required.
Multimeter	Keithley 2000	1188656	11/2010	11/2013
Signal Generator	Agilent E4438C	MY49070581	12/2010	12/2013
Amplifier	Aethercomm	SN 046	Characterized prior to test. No cal required.	Characterized prior to test. No cal required.
Power Meter	HP E4418A	US38261498	11/2010	11/2013
Power Sensor	HP ECP-E26A	US37181460	11/2010	11/2013
Directional Coupler	Narda 4216-20	01386	Characterized prior to test. No cal required.	Characterized prior to test. No cal required.
Temperature and Humidity Sensor	Control Company	11-661-9	3/2012	3/2014

Page: 9/9


This document shall not be reproduced, except in full or in part, without the written approval of SATIMO. The information contained herein is to be used only for the purpose for which it is submitted and is not to be released in whole or part without written approval of SATIMO.

SARTIMO Calibration Certificate-Extended Dipole Calibrations

According to KDB 450824 D02, Dipoles must be recalibrated at least once every three years; however, immediate re-calibration is required for following conditions. The test laboratory must ensure that the required supporting information and documentation have been included in the SAR report to qualify for extended 3-year calibration interval.

- 3) When the most recent return-loss, measured at least annually, deviates by more than 20% from the previous measurement (i.e. 0.2 of the dB value) or not meeting the required -20 dB return-loss specification
- 4) When the most recent measurement of the real or imaginary parts of the impedance, measured at least annually, deviates by more than 5 Ω from the previous measurement

Dipole Verification plot: SID2450 2450MHz for Body:

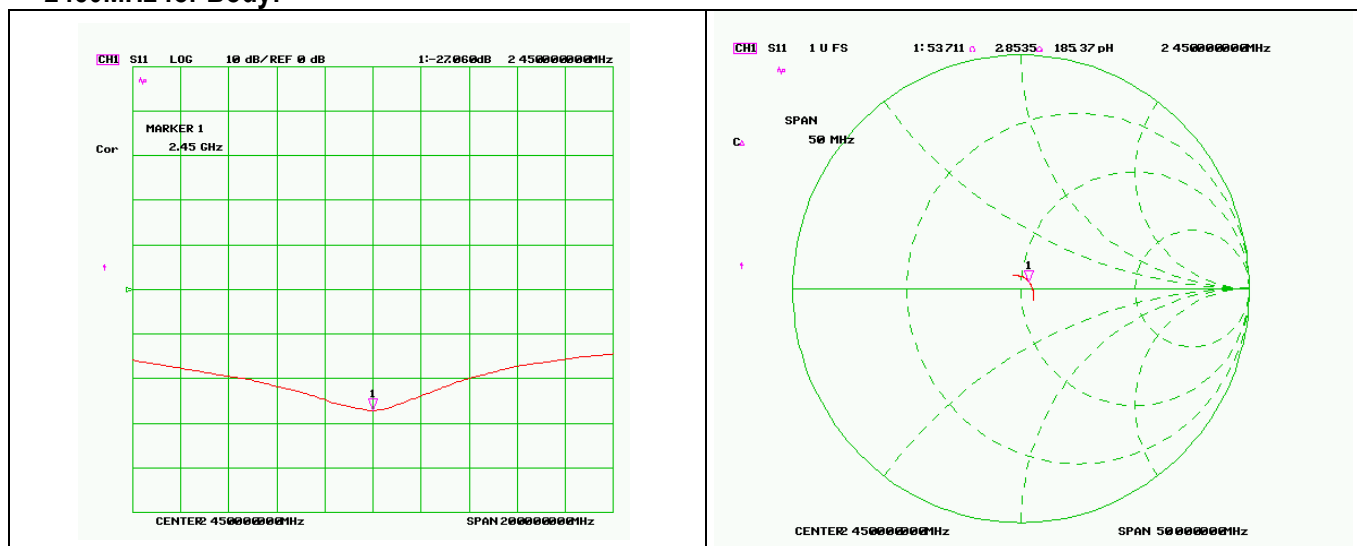

Summary results:

SID 2450					
Return- Loss (dB)	Deviate (dB)	Real Impedance (Ω)	Imaginary Impedance (Ω)	Deviate (Ω)	Calibrate Date
-26.80	-----	-----	50	-----	06/13/2013
-27.06	0.26	53.711	50	3.711	06/13/2014

According to up table, the return loss is <-20dB, deviates by less than 20% from the previous measurement; the real Impedance are all within 5 Ω compared to the required Impedance (50 Ω).

Test report No.	FCC,IC_SAR_SL14031101-SLX-004 Rev1.0
Page	72 of 100
FCC ID	STJ-SDMAN
IC ID	5627A-SDMAN



SAR Reference Waveguide Calibration Report

Ref : ACR.170.9.12.SATU.A

**SIEMIC TESTING AND CERTIFICATION
SERVICES**
2206 RINGWOOD AVE.
SAN JOSE, CA 95131, USA
SATIMO COMOSAR REFERENCE WAVEGUIDE
FREQUENCY: 5000-6000 MHZ
SERIAL NO.: SN 31/10 WGA13

Calibrated at SATIMO US
2105 Barrett Park Dr. - Kennesaw, GA 30144



06/13/2013

Summary:

This document presents the method and results from an accredited SAR reference waveguide calibration performed in SATIMO USA using the COMOSAR test bench. All calibration results are traceable to national metrology institutions.

Test report No.	FCC,IC_SAR_SL14031101-SLX-004 Rev1.0
Page	73 of 100
FCC ID	STJ-SDMAN
IC ID	5627A-SDMAN



SAR REFERENCE WAVEGUIDE CALIBRATION REPORT

Ref: ACR.170.9.12.SATU.A

	<i>Name</i>	<i>Function</i>	<i>Date</i>	<i>Signature</i>
<i>Prepared by :</i>	Jérôme LUC	Product Manager	6/18/2013	
<i>Checked by :</i>	Jérôme LUC	Product Manager	6/18/2013	
<i>Approved by :</i>	Kim RUTKOWSKI	Quality Manager	6/18/2013	

	<i>Customer Name</i>
<i>Distribution :</i>	SIEMIC Testing and Certification Services

<i>Issue</i>	<i>Date</i>	<i>Modifications</i>
A	6/18/2013	Initial release

Test report No.	FCC,IC_SAR_SL14031101-SLX-004 Rev1.0
Page	74 of 100
FCC ID	STJ-SDMAN
IC ID	5627A-SDMAN



TABLE OF CONTENTS

1	Introduction.....	4
2	Device Under Test	4
3	Product Description	4
3.1	General Information	4
4	Measurement Method	4
4.1	Return Loss Requirements	4
4.2	Mechanical Requirements	4
5	Measurement Uncertainty	5
5.1	Return Loss	5
5.2	Dimension Measurement	5
5.3	Validation Measurement	5
6	Calibration Measurement Results	5
6.1	Return Loss	5
6.2	Mechanical Dimensions	6
7	Validation measurement	6
7.1	Head Liquid Measurement	7
7.2	Measurement Result	7
8	List of Equipment	9

Test report No.	FCC,IC_SAR_SL14031101-SLX-004 Rev1.0
Page	75 of 100
FCC ID	STJ-SDMAN
IC ID	5627A-SDMAN



1 INTRODUCTION

This document contains a summary of the requirements set forth by the IEEE 1528 and CEI/IEC 62209 standards for reference waveguides used for SAR measurement system validations and the measurements that were performed to verify that the product complies with the fore mentioned standards.

2 DEVICE UNDER TEST

Device Under Test	
Device Type	COMOSAR 5000-6000 MHz REFERENCE WAVEGUIDE
Manufacturer	Satimo
Model	SWG5500
Serial Number	SN 31/10 WGA13
Product Condition (new / used)	used

A yearly calibration interval is recommended.

3 PRODUCT DESCRIPTION

3.1 GENERAL INFORMATION

Satimo's COMOSAR Validation Waveguides are built in accordance to the IEEE 1528 and CEI/IEC 62209 standards.

4 MEASUREMENT METHOD

The IEEE 1528 and CEI/IEC 62209 standards provide requirements for reference waveguides used for system validation measurements. The following measurements were performed to verify that the product complies with the fore mentioned standards.

4.1 RETURN LOSS REQUIREMENTS

The waveguide used for SAR system validation measurements and checks must have a return loss of -8 dB or better. The return loss measurement shall be performed with matching layer placed in the open end of the waveguide, with the waveguide and matching layer in direct contact with the phantom shell as outlined in the fore mentioned standards.

4.2 MECHANICAL REQUIREMENTS

The IEEE 1528 and CEI/IEC 62209 standards specify the mechanical dimensions of the validation waveguide, the specified dimensions are as shown in Section 6.2. Figure 1 shows how the dimensions relate to the physical construction of the waveguide.



5 MEASUREMENT UNCERTAINTY

All uncertainties listed below represent an expanded uncertainty expressed at approximately the 95% confidence level using a coverage factor of k=2, traceable to the Internationally Accepted Guides to Measurement Uncertainty.

5.1 RETURN LOSS

The following uncertainties apply to the return loss measurement:

Frequency band	Expanded Uncertainty on Return Loss
400-6000MHz	0.1 dB

5.2 DIMENSION MEASUREMENT

The following uncertainties apply to the dimension measurements:

Length (mm)	Expanded Uncertainty on Length
3 - 300	0.05 mm


5.3 VALIDATION MEASUREMENT

The guidelines outlined in the IEEE 1528 and CEI/IEC 62209 standards were followed to generate the measurement uncertainty for validation measurements.

Scan Volume	Expanded Uncertainty
1 g	16.19 %
10 g	15.86 %

6 CALIBRATION MEASUREMENT RESULTS

6.1 RETURN LOSS

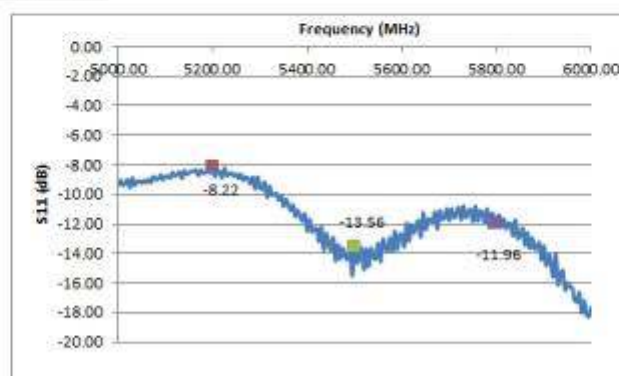

Frequency (MHz)	Return Loss (dB)	Requirement (dB)
5000-6000	< -8.00	-8

6.2 MECHANICAL DIMENSIONS

Frequency (MHz)	L (mm)		W (mm)		L _r (mm)		W _r (mm)		T (mm)	
	Require d	Measure d	Require d	Measure d	Require d	Measure d	Require d	Measure d	Require d	Measure d
5200	40.39 ± 0.13	PASS	20.19 ± 0.13	PASS	81.03 ± 0.13	PASS	61.98 ± 0.13	PASS	5.3*	PASS
5800	40.39 ± 0.13	PASS	20.19 ± 0.13	PASS	81.03 ± 0.13	PASS	61.98 ± 0.13	PASS	4.3*	PASS

* The tolerance for the matching layer is included in the return loss measurement.

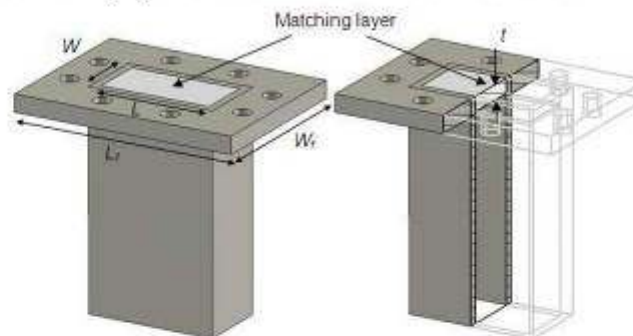


Figure 1: Validation Waveguide Dimensions

7 VALIDATION MEASUREMENT

The IEEE Std. 1528 and CEI/IEC 62209 standards state that the system validation measurements must be performed using a reference waveguide meeting the fore mentioned return loss and mechanical dimension requirements. The validation measurement must be performed with the matching layer placed in the open end of the waveguide, with the waveguide and matching layer in direct contact with the phantom shell.

Measurement Condition

Software	OPENSAR V4
Phantom	SN 20/09 SAM71
Probe	SN 18/11 EPG122
Liquid	Head Liquid Values 5200 MHz: eps' :37.0 sigma : 4.61 Head Liquid Values 5500 MHz: eps' :34.7 sigma : 4.96 Head Liquid Values 5800 MHz: eps' :33.7 sigma : 5.62
Distance between dipole waveguide and liquid	0 mm
Area scan resolution	dx=8mm/dy=8mm
Zoon Scan Resolution	dx=4mm/dy=4m/dz=2mm
Frequency	5200 MHz 5500 MHz 5800 MHz
Input power	20 dBm
Liquid Temperature	21 °C
Lab Temperature	21 °C
Lab Humidity	45 %



SAR REFERENCE WAVEGUIDE CALIBRATION REPORT

Ref: ACR.170.9.12.SATU.A

7.1 HEAD LIQUID MEASUREMENT


Frequency MHz	Relative permittivity (ϵ_r)		Conductivity (σ) S/m	
	required	measured	required	measured
5000	36.2 $\pm$ 10 %		4.45 $\pm$ 10 %	
5100	36.1 $\pm$ 10 %		4.56 $\pm$ 10 %	
5200	36.0 $\pm$ 10 %	PASS	4.66 $\pm$ 10 %	PASS
5300	35.9 $\pm$ 10 %		4.76 $\pm$ 10 %	
5400	35.8 $\pm$ 10 %		4.86 $\pm$ 10 %	
5500	35.6 $\pm$ 10 %	PASS	4.97 $\pm$ 10 %	PASS
5600	35.5 $\pm$ 10 %		5.07 $\pm$ 10 %	
5700	35.4 $\pm$ 10 %		5.17 $\pm$ 10 %	
5800	35.3 $\pm$ 10 %	PASS	5.27 $\pm$ 10 %	PASS
5900	35.2 $\pm$ 10 %		5.38 $\pm$ 10 %	
6000	35.1 $\pm$ 10 %		5.48 $\pm$ 10 %	

7.2 MEASUREMENT RESULT

At those frequencies, the target SAR value can not be generic. Hereunder is the target SAR value defined by Satimo, within the uncertainty for the system validation. All SAR values are normalized to 1 W net power. In bracket, the measured SAR is given with the used input power.

Frequency (MHz)	1 g SAR (W/kg)		10 g SAR (W/kg)	
	required	measured	required	measured
5200	159.00	161.46 (16.15)	56.90	54.83 (5.48)
5500	170.10	173.75 (17.37)	59.20	59.63 (5.96)
5800	181.20	183.99 (18.40)	61.50	59.17 (5.92)

SAR MEASUREMENT PLOTS @ 5200 MHz

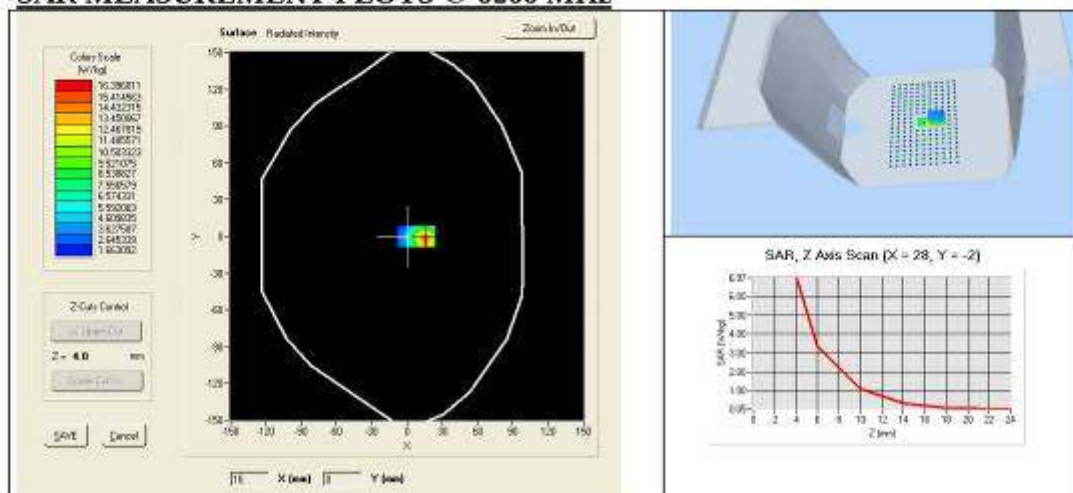

Page: 7/9

This document shall not be reproduced, except in full or in part, without the written approval of SATIMO. The information contained herein is to be used only for the purpose for which it is submitted and is not to be released in whole or part without written approval of SATIMO.


Test report No.	FCC,IC_SAR_SL14031101-SLX-004 Rev1.0
Page	79 of 100
FCC ID	STJ-SDMAN
IC ID	5627A-SDMAN




SAR REFERENCE WAVEGUIDE CALIBRATION REPORT

Ref: ACR.170.9.12.SATU.A

SAR MEASUREMENT PLOTS @ 5500 MHz

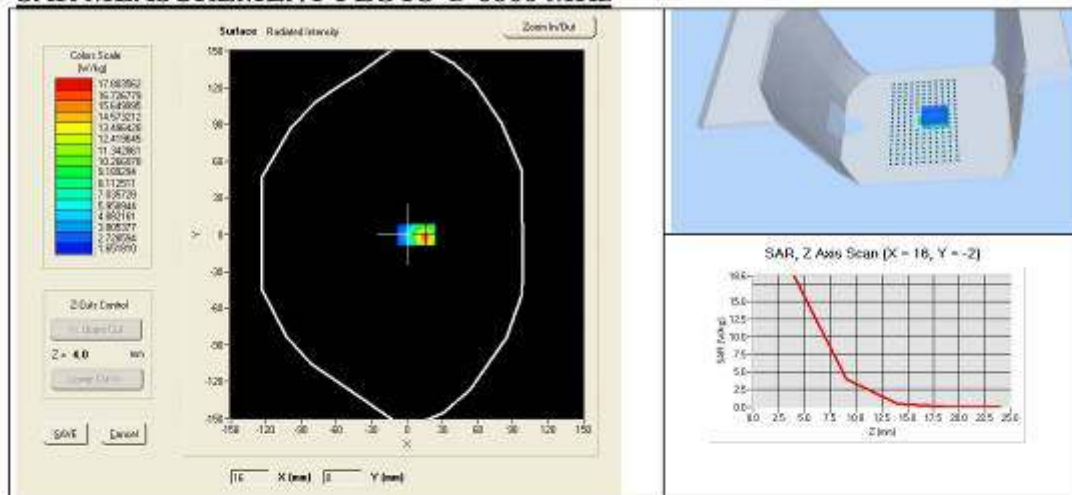

SAR MEASUREMENT PLOTS @ 5800 MHz

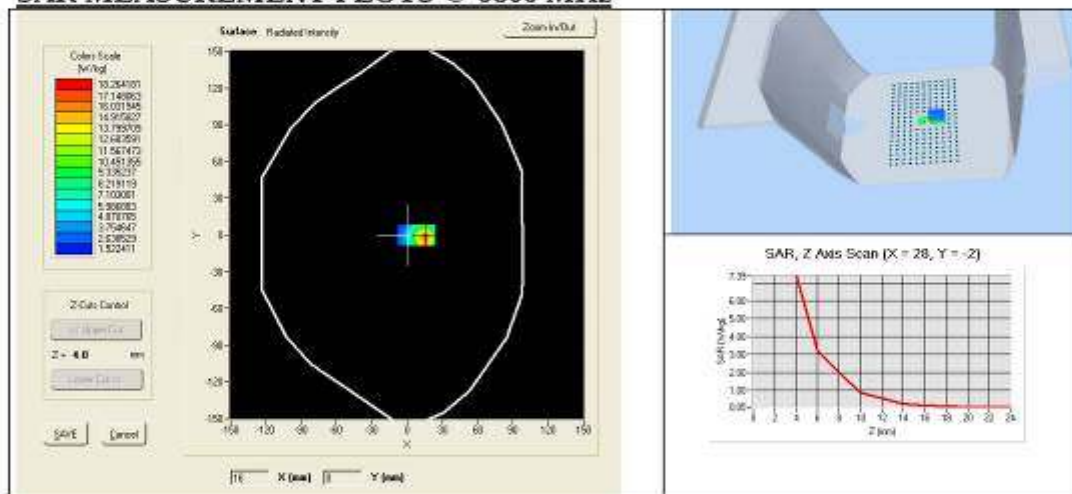

Page: 8/9

This document shall not be reproduced, except in full or in part, without the written approval of SATIMO. The information contained herein is to be used only for the purpose for which it is submitted and is not to be released in whole or part without written approval of SATIMO.

Test report No.	FCC,IC_SAR_SL14031101-SLX-004 Rev1.0
Page	80 of 100
FCC ID	STJ-SDMAN
IC ID	5627A-SDMAN



8 LIST OF EQUIPMENT

Equipment Summary Sheet				
Equipment Description	Manufacturer / Model	Identification No.	Current Calibration Date	Next Calibration Date
Flat Phantom	Satimo	SN-20/09-SAM71	Validated. No cal required.	Validated. No cal required.
COMOSAR Test Bench	Version 3	NA	Validated. No cal required.	Validated. No cal required.
Network Analyzer	Rhode & Schwarz ZVA	SN100132	02/2013	02/2016
Calipers	Carrera	CALIPER-01	12/2013	12/2016
Reference Probe	Satimo	EPG122 SN 18/11	Characterized prior to test. No cal required.	Characterized prior to test. No cal required.
Multimeter	Keithley 2000	1188656	11/2010	11/2013
Signal Generator	Agilent E4438C	MY49070581	12/2010	12/2013
Amplifier	Aethercomm	SN 046	Characterized prior to test. No cal required.	Characterized prior to test. No cal required.
Power Meter	HP E4418A	US38261498	11/2010	11/2013
Power Sensor	HP ECP-E26A	US37181460	11/2010	11/2013
Directional Coupler	Narda 4216-20	01386	Characterized prior to test. No cal required.	Characterized prior to test. No cal required.
Temperature and Humidity Sensor	Control Company	11-661-9	3/2012	3/2014

Page: 9/9

This document shall not be reproduced, except in full or in part, without the written approval of SATIMO. The information contained herein is to be used only for the purpose for which it is submitted and is not to be released in whole or part without written approval of SATIMO.

Test report No.	FCC,IC_SAR_SL14031101-SLX-004 Rev1.0
Page	81 of 100
FCC ID	STJ-SDMAN
IC ID	5627A-SDMAN


Annex E. SAR Test Plots

Test report No.	FCC,IC_SAR_SL14031101-SLX-004 Rev1.0
Page	82 of 100
FCC ID	STJ-SDMAN
IC ID	5627A-SDMAN


System Verification Plots

Test specification:	System Verification			
Environ Conditions:	Temp(oC):	23	Result:	Pass
	Humidity(%):	58		
	Atmospheric(mPa):	1009		
Mains Power:	3.3VDC			
Test Date:	04/29/2014			
Tested by:	David Zhang			
Remarks:	System Validation, dipole, CW signal, duty cycle =1			


Frequency (MHz)	2450.000000
Relative permittivity (real part)	51.21
Conductivity (S/m)	1.93
Transmission Duty Factor	1.00
Probe SN	09/13 EPG176
Conversion Factor (dB)	7.89
Area Scan Resolution	8 mm
Zoom Scan Resolution	dx=4mm, dy=4mm, dz=2mm
Zoom Scan Size	24x24x24 mm
Measurement Drifts (%)	2.84
Highest Extrapolated SAR (W/Kg)	3.242
SAR 1g (W/Kg)	1.81
Peak SAR Location	0mm(x),-18mm(y),4mm(z)

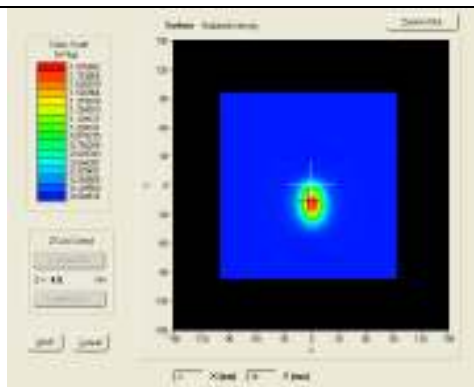

SURFACE SAR

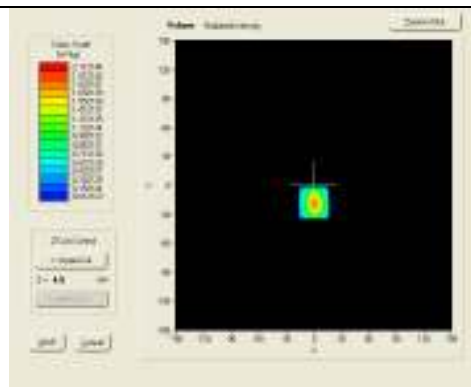

VOLUME SAR

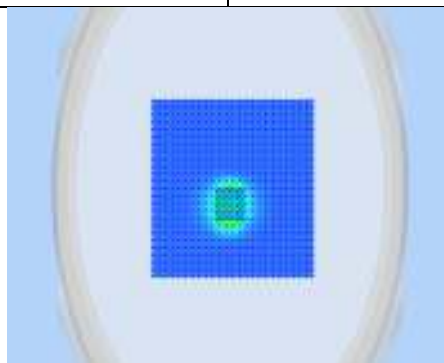


3D View


Test report No.	FCC,IC_SAR_SL14031101-SLX-004 Rev1.0
Page	83 of 100
FCC ID	STJ-SDMAN
IC ID	5627A-SDMAN

Test specification:	System Validation			
Environ Conditions:	Temp(oC):	23	Result:	Pass
	Humidity(%):	58		
	Atmospheric(mPa):	1009		
Mains Power:	3.3VDC			
Test Date:	04/29/2014			
Tested by:	David Zhang			
Remarks:	System Validation, dipole, CW signal, duty cycle =1			


Frequency (MHz)	5200.000000
Relative permittivity (real part)	50.08
Conductivity (S/m)	5.47
Transmission Duty Factor	1.00
Probe SN	09/13 EPG176
Conversion Factor (dB)	5.69
Area Scan Resolution	4 mm
Zoom Scan Resolution	dx=4mm, dy=4mm, dz=2mm
Zoom Scan Size	24x24x24 mm
Measurement Drifts (%)	3.74
Highest Extrapolated SAR (W/Kg)	9.41
SAR 1g (W/Kg)	4.99
Peak SAR Location	-2mm(x),0mm(y),4mm(z)

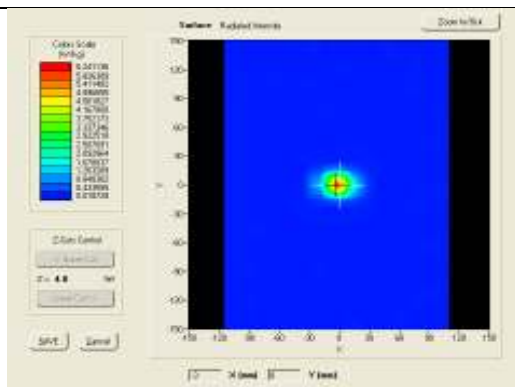

SURFACE SAR

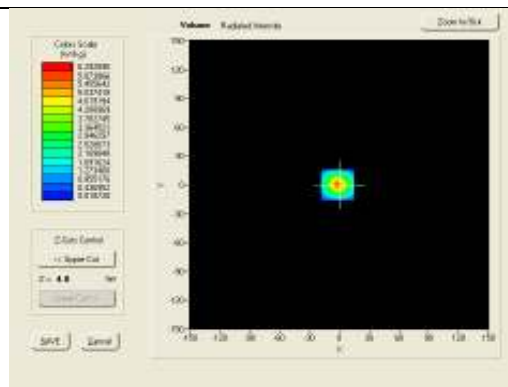

VOLUME SAR

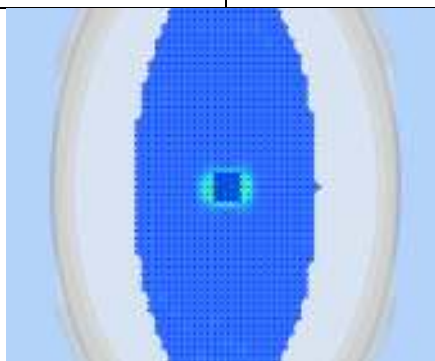


3D View


Test report No.	FCC,IC_SAR_SL14031101-SLX-004 Rev1.0
Page	84 of 100
FCC ID	STJ-SDMAN
IC ID	5627A-SDMAN

Test specification:	System Validation			
Environ Conditions:	Temp(oC):	23	Result:	Pass
	Humidity(%):	58		
	Atmospheric(mPa):	1009		
Mains Power:	3.3VDC			
Test Date:	04/29/2014			
Tested by:	David Zhang			
Remarks:	System Validation, dipole, CW signal, duty cycle =1			


Frequency (MHz)	5500.000000
Relative permittivity (real part)	49.06
Conductivity (S/m)	5.61
Transmission Duty Factor	1.00
Probe SN	09/13 EPG176
Conversion Factor (dB)	5.69
Area Scan Resolution	4 mm
Zoom Scan Resolution	dx=4mm, dy=4mm, dz=2mm
Zoom Scan Size	24x24x24 mm
Measurement Drifts (%)	-4.09
Highest Extrapolated SAR (W/Kg)	28.621
SAR 1g (W/Kg)	16.91
Peak SAR Location	21mm(x),22mm(y),4mm(z)

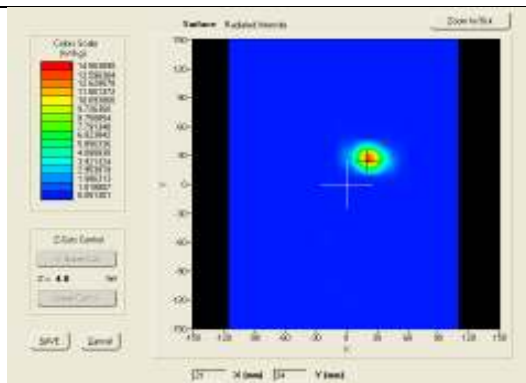

SURFACE SAR

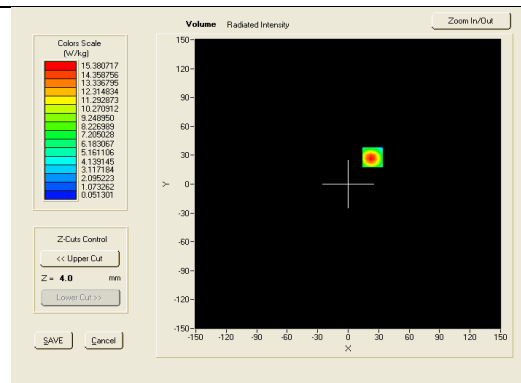

VOLUME SAR

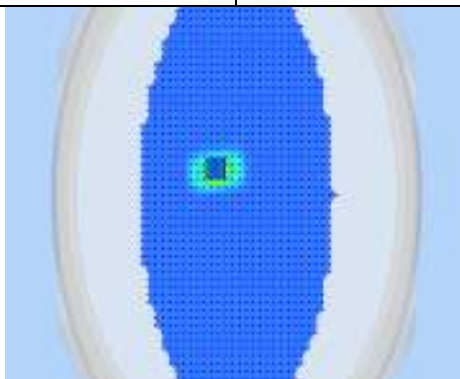


3D View


Test report No.	FCC,IC_SAR_SL14031101-SLX-004 Rev1.0
Page	85 of 100
FCC ID	STJ-SDMAN
IC ID	5627A-SDMAN

Test specification:	System Validation			
Environ Conditions:	Temp(oC):	23	Result:	Pass
	Humidity(%):	58		
	Atmospheric(mPa):	1009		
Mains Power:	3.3VDC			
Test Date:	04/29/2014			
Tested by:	David Zhang			
Remarks:	System Validation, dipole, CW signal, duty cycle =1			


Frequency (MHz)	5800.000000
Relative permittivity (real part)	48.20
Conductivity (S/m)	5.72
Transmission Duty Factor	1.00
Probe SN	09/13 EPG176
Conversion Factor (dB)	5.69
Area Scan Resolution	4 mm
Zoom Scan Resolution	dx=4mm, dy=4mm, dz=2mm
Zoom Scan Size	24x24x24 mm
Measurement Drifts (%)	2.93
Highest Extrapolated SAR (W/Kg)	33.182
SAR 1g (W/Kg)	17.89
Peak SAR Location	21mm(x),22mm(y),4mm(z)

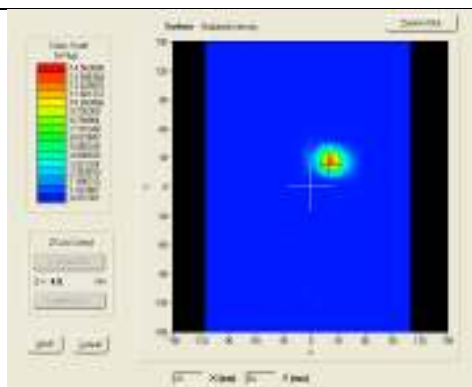

SURFACE SAR

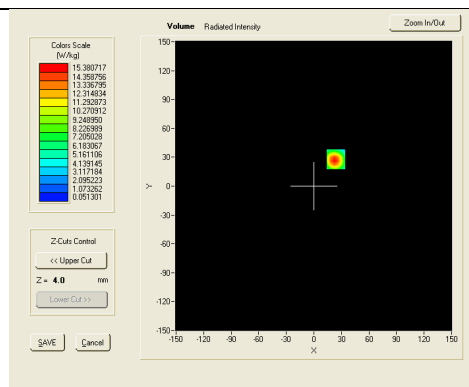

VOLUME SAR

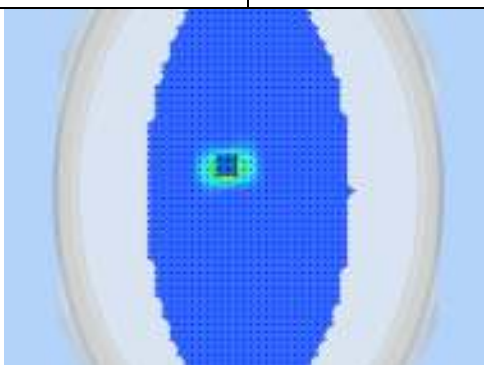


3D View

Test report No.	FCC,IC_SAR_SL14031101-SLX-004 Rev1.0
Page	86 of 100
FCC ID	STJ-SDMAN
IC ID	5627A-SDMAN


SAR Measurement Plots – Determine worst case configuraiton

Test specification:	802.11b-2437MHz-Body SAR-Top position			
Environ Conditions:	Temp(°C):	23	Result:	Pass
	Humidity(%):	58		
	Atmospheric(mPa):	1009		
Mains Power:	3.3VDC			
Test Date:	04/29/2014			
Tested by:	David Zhang			
Remarks:	-			


Frequency (MHz)	2437.000000
Relative permittivity (real part)	51.63
Conductivity (S/m)	1.94
Transmission Duty Factor	1.0
Probe SN	09/13 EPG176
Conversion Factor (dB)	7.46
Area Scan Resolution	8 mm
Zoom Scan Resolution	dx=5mm, dy=5mm, dz=4mm
Zoom Scan Size	24x24x24 mm
Measurement Drifts (%)	-3.79
Highest Extrapolated SAR (W/Kg)	1.301
SAR 1g (W/Kg)	0.303
Peak SAR Location	-7mm(x),18mm(y),4mm(z)

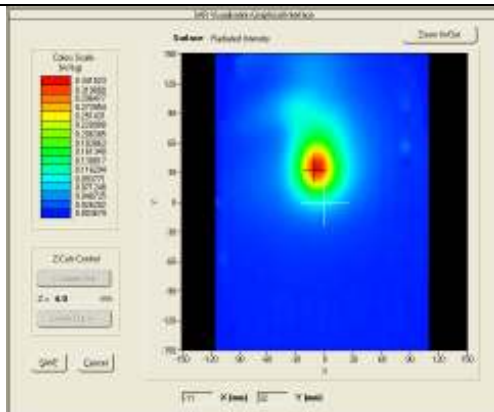

SURFACE SAR

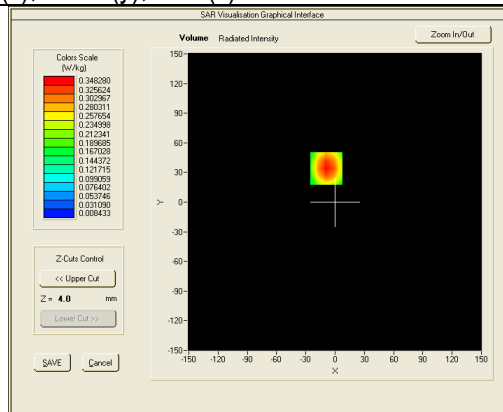

VOLUME SAR

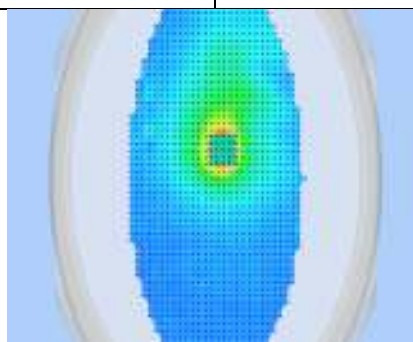


3D View Plot


Test report No.	FCC,IC_SAR_SL14031101-SLX-004 Rev1.0
Page	87 of 100
FCC ID	STJ-SDMAN
IC ID	5627A-SDMAN

Test specification:	802.11n-HT40-5230MHz-Body SAR-Top position			
Environ Conditions:	Temp(°C):	23	Result:	Pass
	Humidity(%):	58		
	Atmospheric(mPa):	1009		
Mains Power:	3.3VDC			
Test Date:	04/29/2014			
Tested by:	David Zhang			
Remarks:	-			


Frequency (MHz)	5230.000000
Relative permittivity (real part)	50.03
Conductivity (S/m)	5.49
Transmission Duty Factor	1.0
Probe SN	09/13 EPG176
Conversion Factor (dB)	5.69
Area Scan Resolution	8 mm
Zoom Scan Resolution	dx=4mm, dy=4mm, dz=2mm
Zoom Scan Size	24x24x24 mm
Measurement Drifts (%)	1.80
Highest Extrapolated SAR (W/Kg)	1.184
SAR 1g (W/Kg)	0.283
Peak SAR Location	4mm(x),0mm(y),4mm(z)

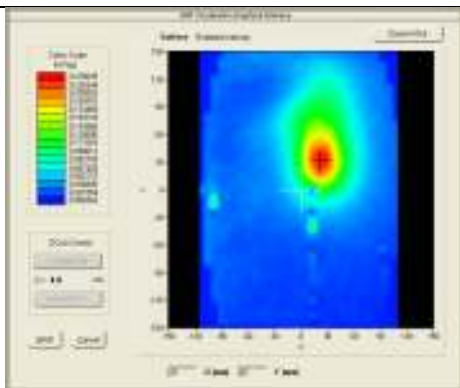

SURFACE SAR

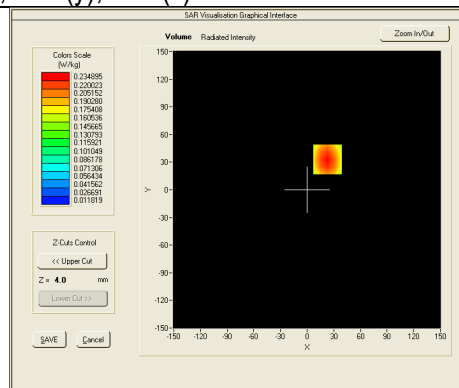

VOLUME SAR

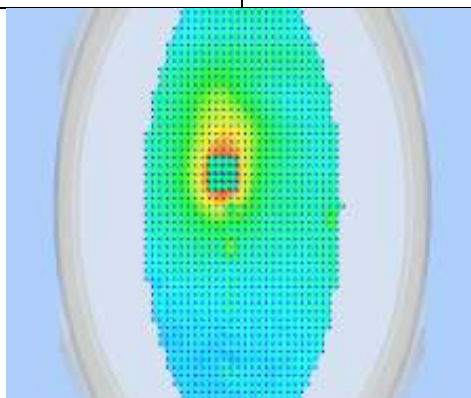


3D View Plot


Test report No.	FCC,IC_SAR_SL14031101-SLX-004 Rev1.0
Page	88 of 100
FCC ID	STJ-SDMAN
IC ID	5627A-SDMAN

Test specification:	802.11n-HT40-5270MHz-Body SAR-Top position			
Environ Conditions:	Temp(°C):	23	Result:	Pass
	Humidity(%):	58		
	Atmospheric(mPa):	1009		
Mains Power:	3.3VDC			
Test Date:	04/29/2014			
Tested by:	David Zhang			
Remarks:	-			


Frequency (MHz)	5270.000000
Relative permittivity (real part)	49.97
Conductivity (S/m)	5.52
Transmission Duty Factor	1.0
Probe SN	09/13 EPG176
Conversion Factor (dB)	5.69
Area Scan Resolution	8 mm
Zoom Scan Resolution	dx=4mm, dy=4mm, dz=2mm
Zoom Scan Size	24x24x24 mm
Measurement Drifts (%)	1.760
Highest Extrapolated SAR (W/Kg)	1.442
SAR 1g (W/Kg)	0.267
Peak SAR Location	-7mm(x),18mm(y),4mm(z)

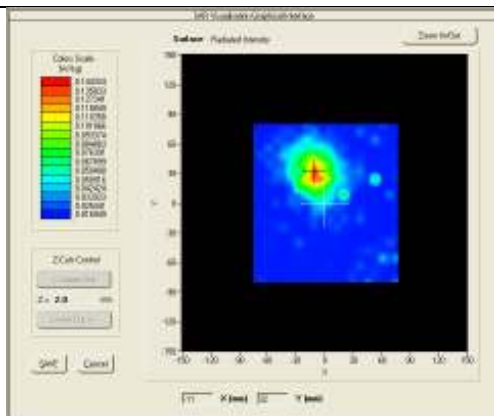

SURFACE SAR

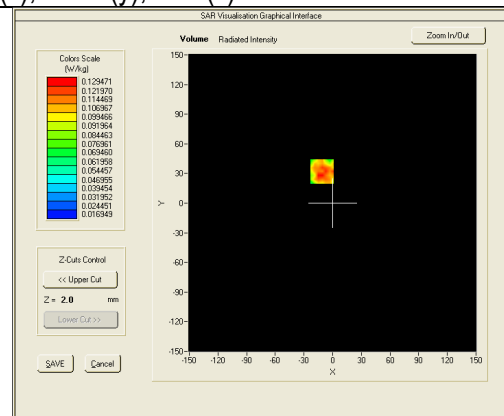

VOLUME SAR

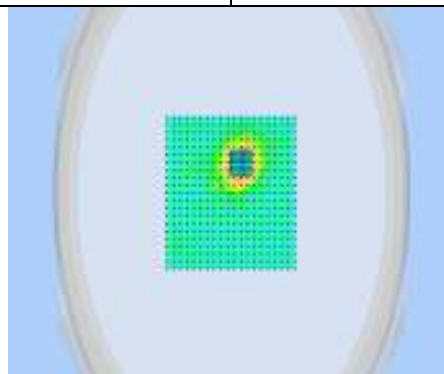


3D View Plot


Test report No.	FCC,IC_SAR_SL14031101-SLX-004 Rev1.0
Page	89 of 100
FCC ID	STJ-SDMAN
IC ID	5627A-SDMAN

Test specification:	802.11n-HT40-5670MHz-Body SAR-Top position			
Environ Conditions:	Temp(°C):	23	Result:	Pass
	Humidity(%):	58		
	Atmospheric(mPa):	1009		
Mains Power:	3.3VDC			
Test Date:	04/29/2014			
Tested by:	David Zhang			
Remarks:	-			


Frequency (MHz)	5670.000000
Relative permittivity (real part)	48.62
Conductivity (S/m)	5.76
Transmission Duty Factor	1.0
Probe SN	09/13 EPG176
Conversion Factor (dB)	5.69
Area Scan Resolution	8 mm
Zoom Scan Resolution	dx=4mm, dy=4mm, dz=2mm
Zoom Scan Size	24x24x24 mm
Measurement Drifts (%)	3.81
Highest Extrapolated SAR (W/Kg)	1.504
SAR 1g (W/Kg)	0.328
Peak SAR Location	-9mm(x),24mm(y),4mm(z)

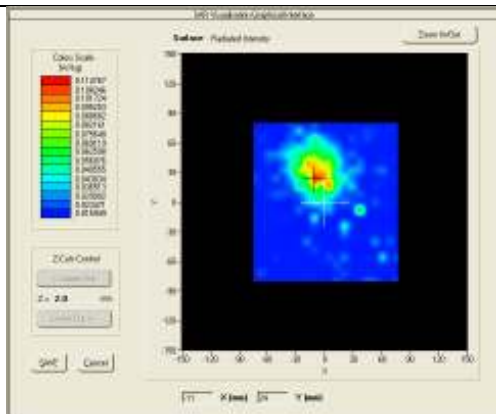

SURFACE SAR

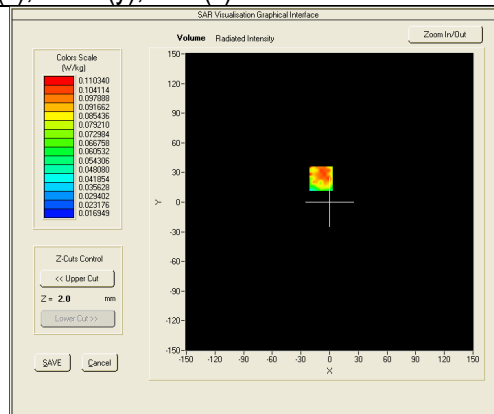

VOLUME SAR

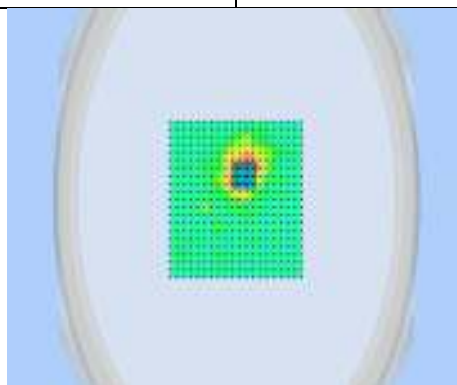


3D View Plot


Test report No.	FCC,IC_SAR_SL14031101-SLX-004 Rev1.0
Page	90 of 100
FCC ID	STJ-SDMAN
IC ID	5627A-SDMAN

Test specification:	802.11n-HT40-5755MHz-Body SAR-Top position			
Environ Conditions:	Temp(°C):	23	Result:	Pass
	Humidity(%):	58		
	Atmospheric(mPa):	1009		
Mains Power:	3.3VDC			
Test Date:	04/29/2014			
Tested by:	David Zhang			
Remarks:	-			


Frequency (MHz)	5755.000000
Relative permittivity (real part)	48.37
Conductivity (S/m)	5.72
Transmission Duty Factor	1.0
Probe SN	09/13 EPG176
Conversion Factor (dB)	5.69
Area Scan Resolution	8 mm
Zoom Scan Resolution	dx=4mm, dy=4mm, dz=2mm
Zoom Scan Size	24x24x24 mm
Measurement Drifts (%)	-3.12
Highest Extrapolated SAR (W/Kg)	1.305
SAR 1g (W/Kg)	0.302
Peak SAR Location	4mm(x),0mm(y),4mm(z)

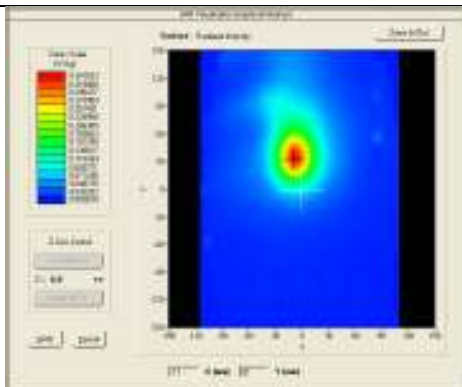

SURFACE SAR

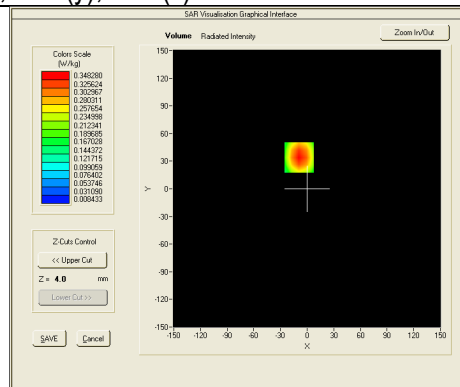

VOLUME SAR

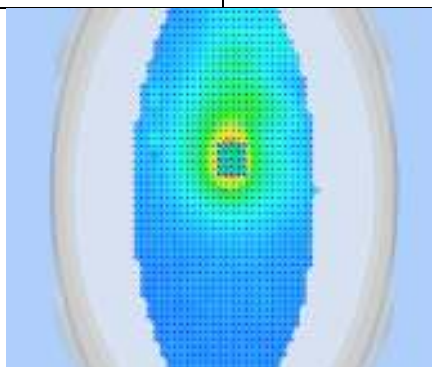


3D View Plot


Test report No.	FCC,IC_SAR_SL14031101-SLX-004 Rev1.0
Page	91 of 100
FCC ID	STJ-SDMAN
IC ID	5627A-SDMAN

Test specification:	802.11b-2437MHz-Body SAR-Right- position			
Environ Conditions:	Temp(°C):	23	Result:	Pass
	Humidity(%):	58		
	Atmospheric(mPa):	1009		
Mains Power:	3.3VDC			
Test Date:	04/29/2014			
Tested by:	David Zhang			
Remarks:	-			


Frequency (MHz)	2437.000000
Relative permittivity (real part)	51.63
Conductivity (S/m)	1.94
Transmission Duty Factor	1.0
Probe SN	09/13 EPG176
Conversion Factor (dB)	7.46
Area Scan Resolution	8 mm
Zoom Scan Resolution	dx=4mm, dy=4mm, dz=2mm
Zoom Scan Size	24x24x24 mm
Measurement Drifts (%)	4.01
Highest Extrapolated SAR (W/Kg)	1.045
SAR 1g (W/Kg)	0.272
Peak SAR Location	-7mm(x),18mm(y),4mm(z)

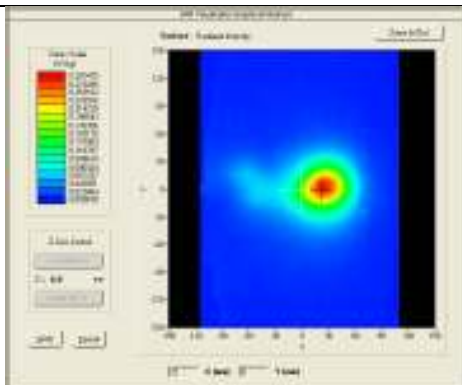

SURFACE SAR

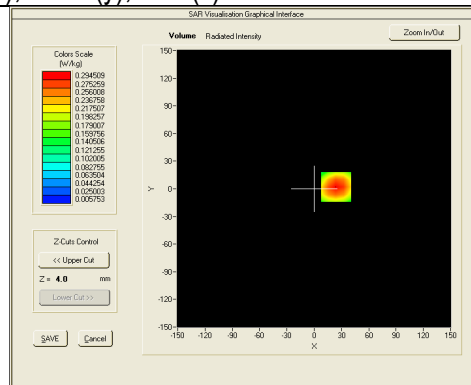

VOLUME SAR

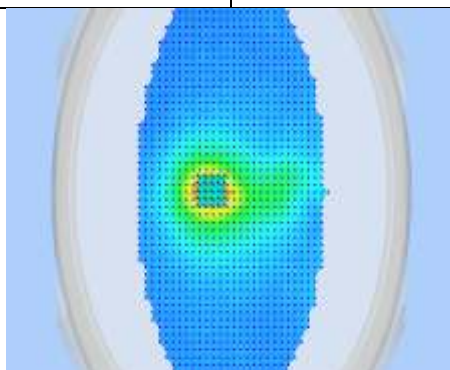


3D View Plot


Test report No.	FCC,IC_SAR_SL14031101-SLX-004 Rev1.0
Page	92 of 100
FCC ID	STJ-SDMAN
IC ID	5627A-SDMAN

Test specification:	802.11n-HT40-5230MHz-Body SAR-Right- position			
Environ Conditions:	Temp(°C):	23	Result:	Pass
	Humidity(%):	58		
	Atmospheric(mPa):	1009		
Mains Power:	3.3VDC			
Test Date:	04/29/2014			
Tested by:	David Zhang			
Remarks:	-			


Frequency (MHz)	5230.000000
Relative permittivity (real part)	50.03
Conductivity (S/m)	5.49
Transmission Duty Factor	1.0
Probe SN	09/13 EPG176
Conversion Factor (dB)	5.69
Area Scan Resolution	8 mm
Zoom Scan Resolution	dx=4mm, dy=4mm, dz=2mm
Zoom Scan Size	24x24x24 mm
Measurement Drifts (%)	-2.84
Highest Extrapolated SAR (W/Kg)	1.039
SAR 1g (W/Kg)	0.261
Peak SAR Location	4mm(x),0mm(y),4mm(z)

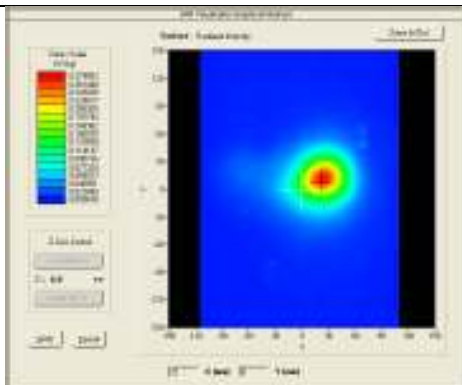

SURFACE SAR

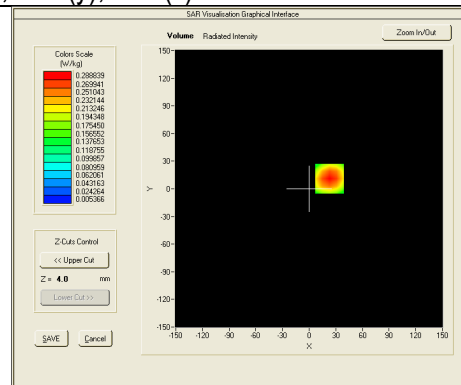

VOLUME SAR

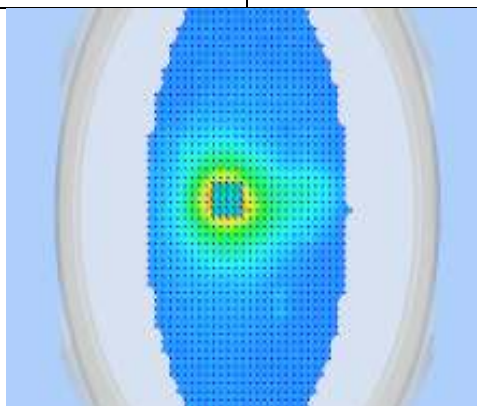


3D View Plot


Test report No.	FCC,IC_SAR_SL14031101-SLX-004 Rev1.0
Page	93 of 100
FCC ID	STJ-SDMAN
IC ID	5627A-SDMAN

Test specification:	802.11n-HT40-5270MHz-Body SAR-Right- position			
Environ Conditions:	Temp(°C):	23	Result:	Pass
	Humidity(%):	58		
	Atmospheric(mPa):	1009		
Mains Power:	3.3VDC			
Test Date:	04/29/2014			
Tested by:	David Zhang			
Remarks:	-			


Frequency (MHz)	5270.000000
Relative permittivity (real part)	49.97
Conductivity (S/m)	5.52
Transmission Duty Factor	1.0
Probe SN	09/13 EPG176
Conversion Factor (dB)	5.69
Area Scan Resolution	8 mm
Zoom Scan Resolution	dx=4mm, dy=4mm, dz=2mm
Zoom Scan Size	24x24x24 mm
Measurement Drifts (%)	-1.83
Highest Extrapolated SAR (W/Kg)	1.431
SAR 1g (W/Kg)	0.275
Peak SAR Location	4mm(x),0mm(y),4mm(z)

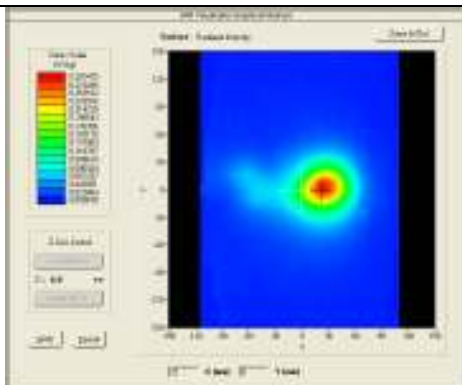

SURFACE SAR

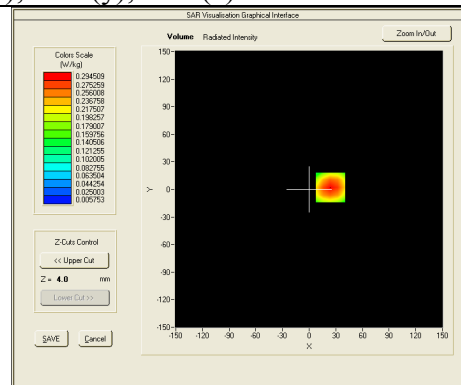

VOLUME SAR

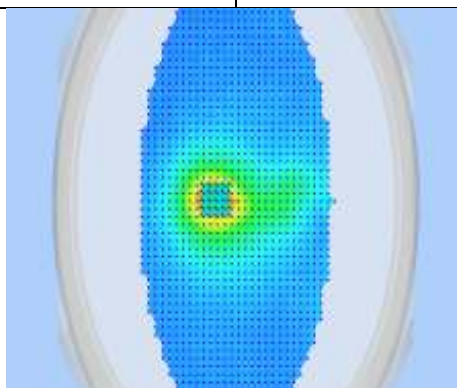


3D View Plot


Test report No.	FCC,IC_SAR_SL14031101-SLX-004 Rev1.0
Page	94 of 100
FCC ID	STJ-SDMAN
IC ID	5627A-SDMAN

Test specification:	802.11n-HT40-5670MHz-Body SAR-Right-position			
Environ Conditions:	Temp(°C):	23	Result:	Pass
	Humidity(%):	58		
	Atmospheric(mPa):	1009		
Mains Power:	3.3VDC			
Test Date:	04/29/2014			
Tested by:	David Zhang			
Remarks:	-			


Frequency (MHz)	5670.000000
Relative permittivity (real part)	48.62
Conductivity (S/m)	5.76
Transmission Duty Factor	1.0
Probe SN	09/13 EPG176
Conversion Factor (dB)	5.69
Area Scan Resolution	8 mm
Zoom Scan Resolution	dx=4mm, dy=4mm, dz=2mm
Zoom Scan Size	24x24x24 mm
Measurement Drifts (%)	-2.10
Highest Extrapolated SAR (W/Kg)	1.528
SAR 1g (W/Kg)	0.243
Peak SAR Location	4mm(x),0mm(y),4mm(z)

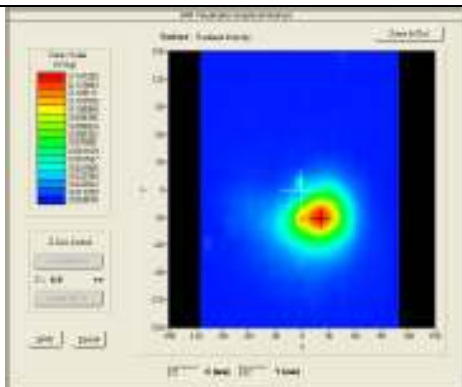

SURFACE SAR

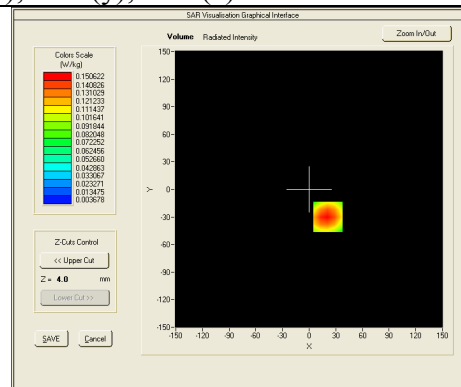

VOLUME SAR

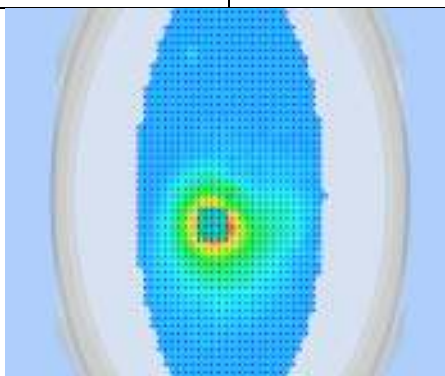


3D View Plot


Test report No.	FCC,IC_SAR_SL14031101-SLX-004 Rev1.0
Page	95 of 100
FCC ID	STJ-SDMAN
IC ID	5627A-SDMAN

Test specification:	802.11n-HT40-5755MHz-Body SAR-Right-position			
Environ Conditions:	Temp(°C):	23	Result:	Pass
	Humidity(%):	58		
	Atmospheric(mPa):	1009		
Mains Power:	3.3VDC			
Test Date:	04/29/2014			
Tested by:	David Zhang			
Remarks:	-			


Frequency (MHz)	5755.000000
Relative permittivity (real part)	48.37
Conductivity (S/m)	5.72
Transmission Duty Factor	1.0
Probe SN	09/13 EPG176
Conversion Factor (dB)	5.69
Area Scan Resolution	8 mm
Zoom Scan Resolution	dx=4mm, dy=4mm, dz=2mm
Zoom Scan Size	24x24x24 mm
Measurement Drifts (%)	-1.93
Highest Extrapolated SAR (W/Kg)	1.375
SAR 1g (W/Kg)	0.261
Peak SAR Location	4mm(x),-2mm(y),6mm(z)

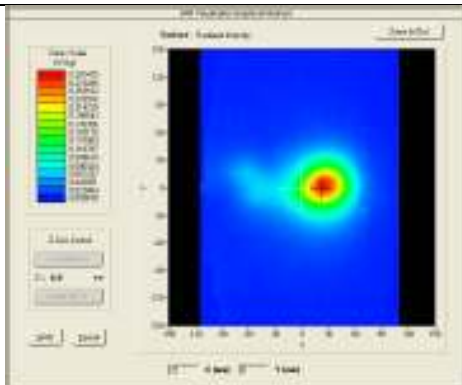

SURFACE SAR

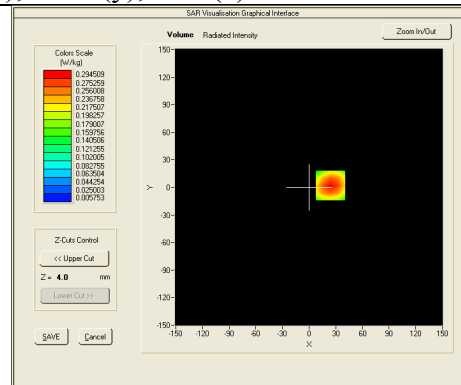

VOLUME SAR

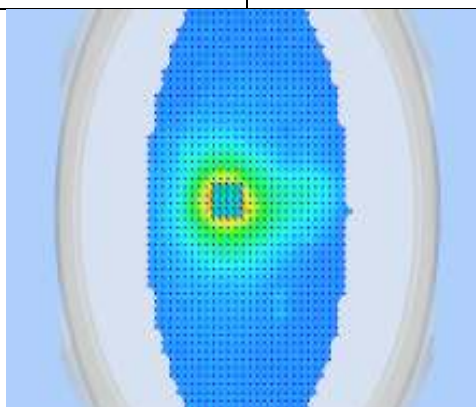


3D View Plot

Test report No.	FCC,IC_SAR_SL14031101-SLX-004 Rev1.0
Page	96 of 100
FCC ID	STJ-SDMAN
IC ID	5627A-SDMAN


SAR Measurement Plots – Additional measurement on worst configuration

Test specification:	802.11b-2412MHz-Body SAR-Top-position			
Environ Conditions:	Temp(°C):	23	Result:	Pass
	Humidity(%):	58		
	Atmospheric(mPa):	1009		
Mains Power:	3.3VDC			
Test Date:	04/29/2014			
Tested by:	David Zhang			
Remarks:	-			


Frequency (MHz)	2412.000000
Relative permittivity (real part)	51.98
Conductivity (S/m)	1.86
Transmission Duty Factor	1.0
Probe SN	09/13 EPG176
Conversion Factor (dB)	7.46
Area Scan Resolution	8 mm
Zoom Scan Resolution	dx=5mm, dy=5mm, dz=4mm
Zoom Scan Size	24x24x24 mm
Measurement Drifts (%)	3.71
Highest Extrapolated SAR (W/Kg)	0.982
SAR 1g (W/Kg)	0.235
Peak SAR Location	4mm(x),0mm(y),4mm(z)

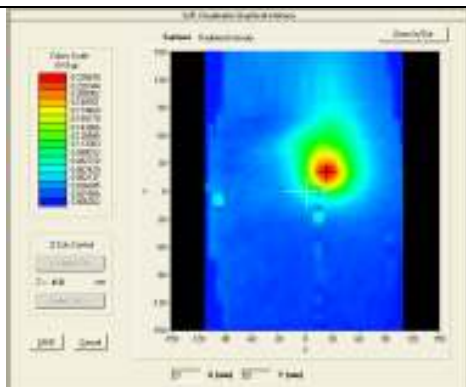

SURFACE SAR

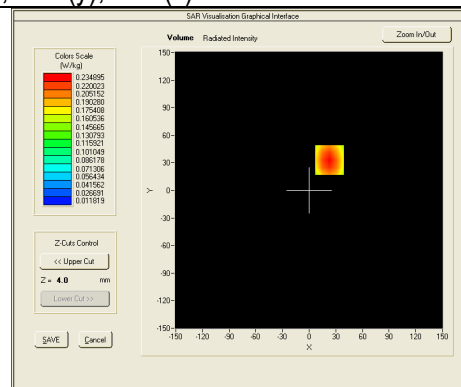

VOLUME SAR

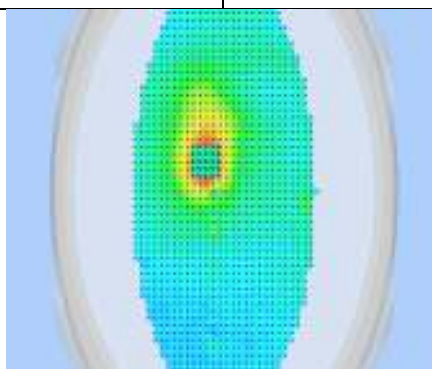


3D View Plot


Test report No.	FCC,IC_SAR_SL14031101-SLX-004 Rev1.0
Page	97 of 100
FCC ID	STJ-SDMAN
IC ID	5627A-SDMAN

Test specification:	802.11b-2462MHz-Body SAR-Top-position			
Environ Conditions:	Temp(°C):	23	Result:	Pass
	Humidity(%):	58		
	Atmospheric(mPa):	1009		
Mains Power:	3.3VDC			
Test Date:	04/29/2014			
Tested by:	David Zhang			
Remarks:	-			


Frequency (MHz)	2462.000000
Relative permittivity (real part)	51.85
Conductivity (S/m)	1.88
Transmission Duty Factor	1.0
Probe SN	09/13 EPG176
Conversion Factor (dB)	7.46
Area Scan Resolution	8 mm
Zoom Scan Resolution	dx=5mm, dy=5mm, dz=4mm
Zoom Scan Size	24x24x24 mm
Measurement Drifts (%)	-3.81
Highest Extrapolated SAR (W/Kg)	0.752
SAR 1g (W/Kg)	0.269
Peak SAR Location	5mm(x),2mm(y),4mm(z)

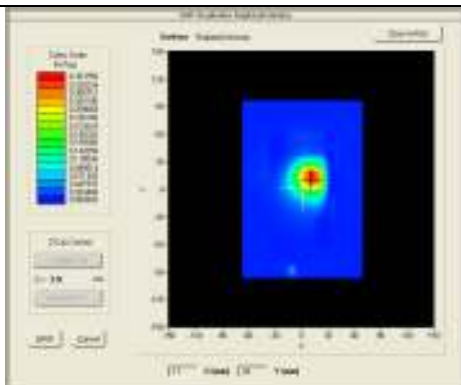

SURFACE SAR

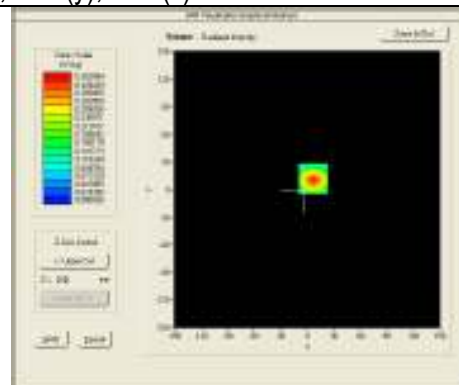

VOLUME SAR

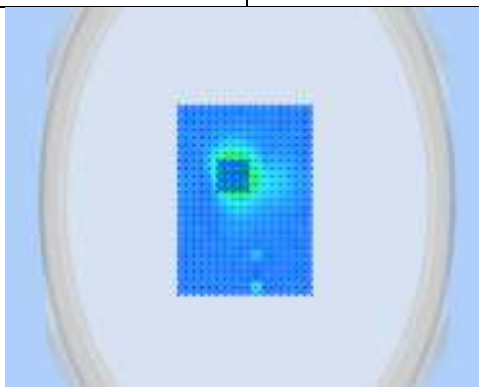


3D View Plot


Test report No.	FCC,IC_SAR_SL14031101-SLX-004 Rev1.0
Page	98 of 100
FCC ID	STJ-SDMAN
IC ID	5627A-SDMAN

Test specification:	802.11n-HT40-5510MHz-Body SAR-Top- position			
Environ Conditions:	Temp(°C):	23	Result:	Pass
	Humidity(%):	58		
	Atmospheric(mPa):	1009		
Mains Power:	3.3VDC			
Test Date:	04/29/2014			
Tested by:	David Zhang			
Remarks:	-			


Frequency (MHz)	5510.000000
Relative permittivity (real part)	49.06
Conductivity (S/m)	5.61
Transmission Duty Factor	1.0
Probe SN	09/13 EPG176
Conversion Factor (dB)	5.69
Area Scan Resolution	4 mm
Zoom Scan Resolution	dx=4mm, dy=4mm, dz=2mm
Zoom Scan Size	24x24x24 mm
Measurement Drifts (%)	-3.01
Highest Extrapolated SAR (W/Kg)	0.852
SAR 1g (W/Kg)	0.305
Peak SAR Location	7mm(x),2mm(y),4mm(z)

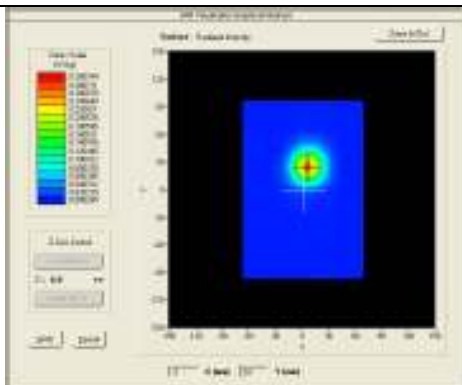

SURFACE SAR

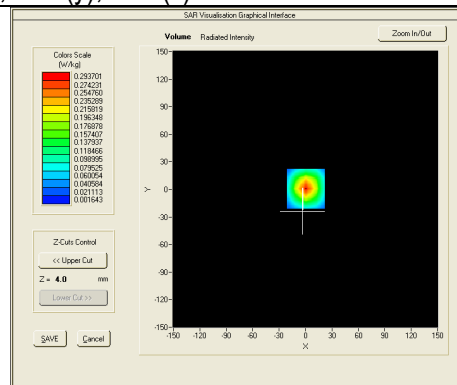

VOLUME SAR

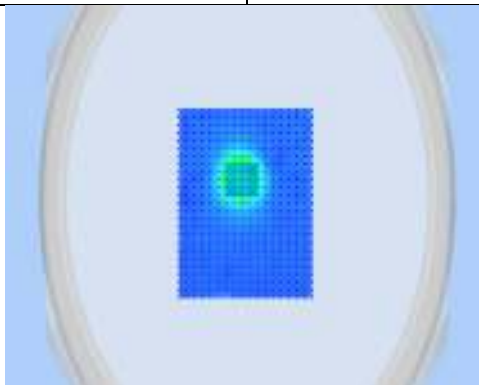


3D View Plot


Test report No.	FCC,IC_SAR_SL14031101-SLX-004 Rev1.0
Page	99 of 100
FCC ID	STJ-SDMAN
IC ID	5627A-SDMAN

Test specification:	802.11n-HT40-5550MHz-Body SAR-Top- position			
Environ Conditions:	Temp(°C):	23	Result:	Pass
	Humidity(%):	58		
	Atmospheric(mPa):	1009		
Mains Power:	3.3VDC			
Test Date:	04/29/2014			
Tested by:	David Zhang			
Remarks:	-			


Frequency (MHz)	5550.000000
Relative permittivity (real part)	48.81
Conductivity (S/m)	5.70
Transmission Duty Factor	1.0
Probe SN	09/13 EPG176
Conversion Factor (dB)	5.69
Area Scan Resolution	4 mm
Zoom Scan Resolution	dx=4mm, dy=4mm, dz=2mm
Zoom Scan Size	24x24x24 mm
Measurement Drifts (%)	2.98
Highest Extrapolated SAR (W/Kg)	0.798
SAR 1g (W/Kg)	0.297
Peak SAR Location	7mm(x),4mm(y),4mm(z)

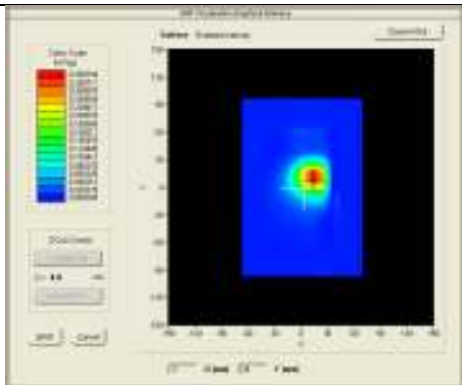

SURFACE SAR

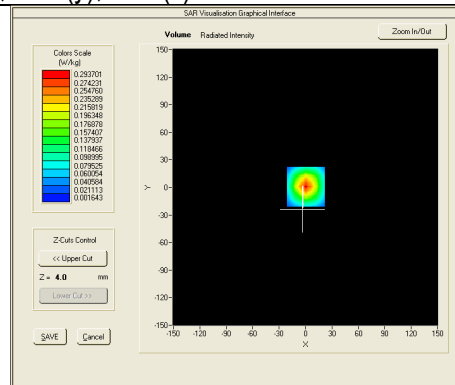

VOLUME SAR

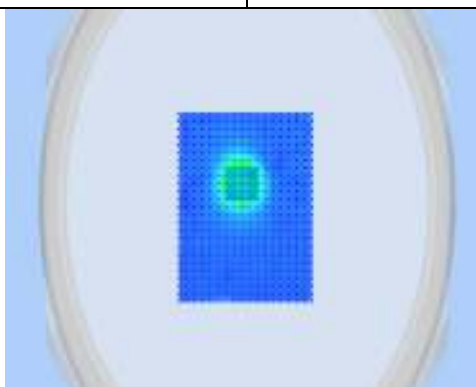

3D View Plot