



SAR Evaluation Report

IN ACCORDANCE WITH THE REQUIREMENTS OF
FCC OET BULLETIN 65 SUPPLEMENT C
IC RSS 102 ISSUE 1 : 1999

FOR

WIRELESS USB ADAPTER

MODEL: DWL-AG132

FCC ID: STJ80411396001
IC: 5627A-80411396001

REPORT NUMBER: 07U10885-5B

ISSUE DATE: MARCH 16, 2007

Prepared for

HOSPIRA, INC.
755 JARVIS DRIVE
MORGAN HILL, CA 95037

Prepared by

COMPLIANCE CERTIFICATION SERVICES
47173 BENICIA STREET,
FREMONT, CA 94538 USA

NVLAP®

NVLAP LAB CODE 200065-0

Revision History

Rev.	Issued date	Revisions	Revised By
--	March 6, 2006	Initial issue	HS
B	March 16, 2007	Additional test on 5.18 GHz	HS

CERTIFICATE OF COMPLIANCE (SAR EVALUATION)**DATES OF TEST:** March 1, 2, and 5, 2007

APPLICANT:	HOSPIRA, INC.
ADDRESS:	755 JARVIS DRIVE, MORGAN HILL, CA 95037
FCC ID:	STJ80411396001
MODEL:	DWL-AG132
DEVICE CATEGORY:	Portable Device
EXPOSURE CATEGORY:	Occupational/Controlled Exposure

Wireless USB Adapter is installed in medical unit DWL-AG132. The DWL-AG132 has been modified by replacing on-board chip antenna with an RF connector. A coaxial cable is used to connect the RF port to an external antenna assembly.

Test Sample is a:	Production unit	
Modulation type:	Direct Sequence Spread Spectrum (DSSS) for 802.11b Orthogonal Frequency Division Multiplexing (OFDM) for 802.11ag	
Rule Parts	Frequency Range [MHz]	The Highest SAR Values [1g_mW/g]
FCC 15.247	2412 - 2462	0.797
	5745 - 5825	0.826
FCC 15.401	5180 - 5320	1.458
	5500 - 5700	1.416

This wireless portable device has been shown to be capable of compliance for localized specific absorption rate (SAR) for General Population/Uncontrolled Exposure limits specified in ANSI/IEEE Std. C95.1-1992 and had been tested in accordance with the measurement procedures specified in FCC OET 65 Supplement C (Edition 01-01) and RSS 102.

Note: The results documented in this report apply only to the tested sample, under the conditions and modes of operation as described herein. This document may not be altered or revised in any way unless done so by Compliance Certification Services and all revisions are duly noted in the revisions section. Any alteration of this document not carried out by Compliance Certification Services will constitute fraud and shall nullify the document. No part of this report may be used to claim product certification, approval, or endorsement by NVLAP, NIST, or any government agency.

Approved & Released For CCS By:



Hsin Fu Shih
Engineering Supervisor
Compliance Certification Services

Tested By:



Ninous Davoudi
Compliance Certification Services

TABLE OF CONTENTS

1	DEVICE UNDER TEST (DUT) DESCRIPTION	5
2	FACILITIES AND ACCREDITATION	6
3	SYSTEM DESCRIPTION	7
3.1	COMPOSITION OF INGREDIENTS FOR TISSUE SIMULATING LIQUIDS	8
4	SIMULATING LIQUID PARAMETERS CHECK	9
4.1	SIMULATING LIQUID PARAMETER CHECK RESULT	11
5	SYSTEM PERFORMANCE CHECK	16
6	SAR MEASURMENT PROCEDURE	19
6.1	DASY4 SAR MEASURMENT PROCEDURE	20
7	PROCEDURE USED TO ESTABLISH TEST SIGNAL	21
8	SAR MEASURMENT RESULTS	22
8.1	2.4GHZ BAND	22
8.1.1	TOP POSITION	22
8.1.2	SIDE POSITION	23
8.2	5GHZ BAND	24
8.2.1	TOP POSITION	24
8.2.2	SIDE POSITION	25
9	MEASURMENT UNCERTAINTY	26
9.1	MEASURMENT UNCERTAINTY FOR 300 MHZ – 3000 MHZ	26
9.2	MEASURMENT UNCERTAINTY 3 GHZ – 6 GHZ	27
10	EQUIPMENT LIST AND CALIBRATION	28
11	PHOTOS	29
12	ATTACHMENTS	32

1 DEVICE UNDER TEST (DUT) DESCRIPTION

Wireless USB Adapter is installed in medical unit DWL-AG132. The DWL-AG132 has been modified by replacing on-board chip antenna with an RF connector. A coaxial cable is used to connect the RF port to an external antenna assembly.

Duty cycle:	100% for abg
Host Device(s):	DWL-AG132
Antenna(s)	Tyco, PN: 1513164-1
Power supply:	Power supplied through host device.

2 FACILITIES AND ACCREDITATION


The test sites and measurement facilities used to collect data are located at 47173 Benicia Street, Fremont, CA 94538 USA. The sites are constructed in conformance with the requirements of ANSI C63.4, ANSI C63.7 and CISPR Publication 22. All receiving equipment conforms to CISPR Publication 16-1, "Radio Interference Measuring Apparatus and Measurement Methods."



CCS is accredited by NVLAP, Laboratory Code 200065-0. The full scope of accreditation can be viewed at <http://www.ccsemc.com>.

No part of this report may be used to claim product certification, approval, or endorsement by NVLAP, NIST, or any government agency.

3 SYSTEM DESCRIPTION

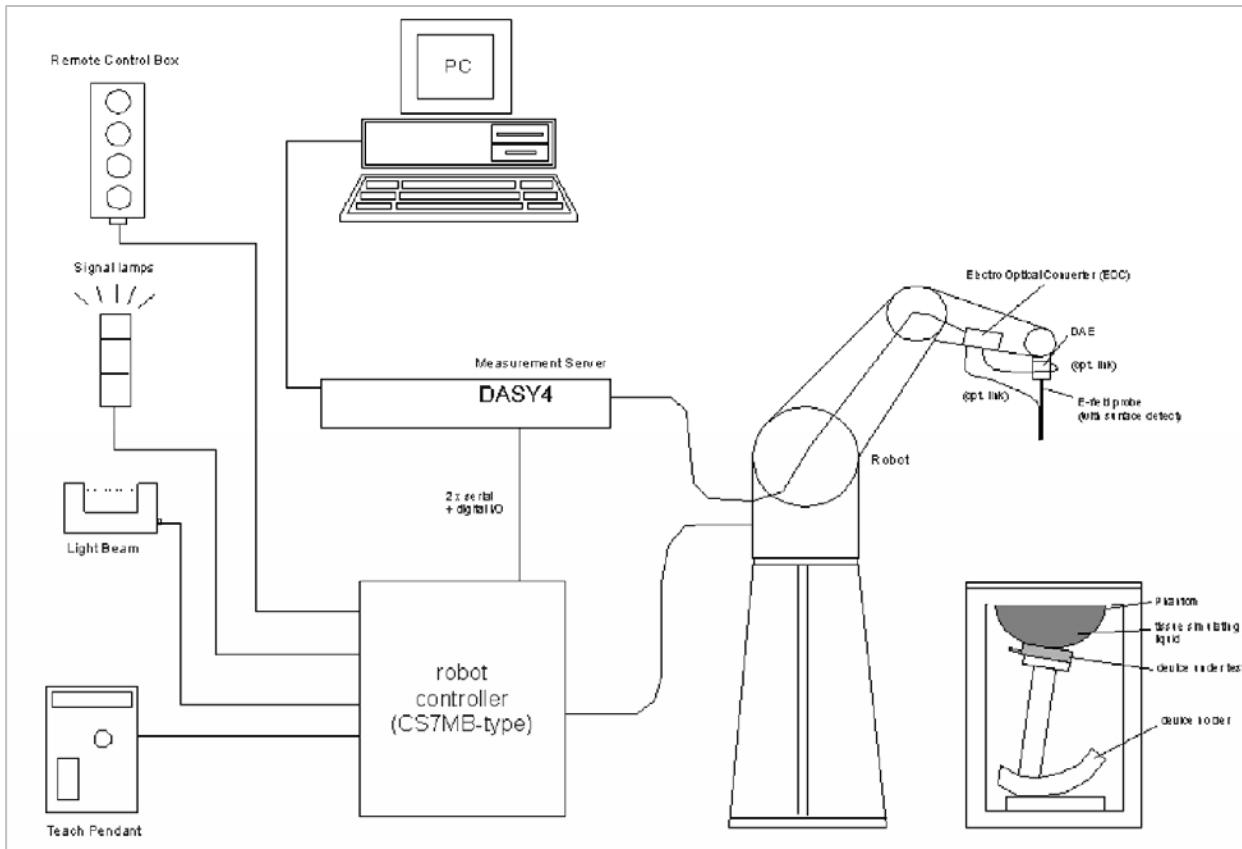

The DASY4 system for performing compliance tests consists of the following items:

- A standard high precision 6-axis robot (Stäubli RX family) with controller, teach pendant and software. An arm extension for accommodating the data acquisition electronics (DAE).
- A dosimetric probe, i.e., an isotropic E-field probe optimized and calibrated for usage in tissue simulating liquid. The probe is equipped with an optical surface detector system.
- A data acquisition electronics (DAE) which performs the signal amplification, signal multiplexing, AD-conversion, offset measurements, mechanical surface detection, collision detection, etc. The unit is battery powered with standard or rechargeable batteries. The signal is optically transmitted to the EOC.
- The function of the measurement server is to perform the time critical tasks such as signal filtering, control of the robot operation and fast movement interrupts.
- A probe alignment unit which improves the (absolute) accuracy of the probe positioning.
- A computer operating Windows 2000 or Windows XP.
- DASY4 software.
- Remote controls with teach pendant and additional circuitry for robot safety such as warning lamps, etc.
- The SAM twin phantom enabling testing left-hand and right-hand usage.
- The device holder for handheld mobile phones.
- Tissue simulating liquid mixed according to the given recipes.
- Validation dipole kits allowing to validate the proper functioning of the system.

3.1 COMPOSITION OF INGREDIENTS FOR TISSUE SIMULATING LIQUIDS

The following tissue formulations are provided for reference only as some of the parameters have not been thoroughly verified. The composition of ingredients may be modified accordingly to achieve the desired target tissue parameters required for routine SAR evaluation.

Ingredients (% by weight)	Frequency (MHz)									
	450		835		915		1900		2450	
Tissue Type	Head	Body	Head	Body	Head	Body	Head	Body	Head	Body
Water	38.56	51.16	41.45	52.4	41.05	56.0	54.9	40.4	62.7	73.2
Salt (NaCl)	3.95	1.49	1.45	1.4	1.35	0.76	0.18	0.5	0.5	0.04
Sugar	56.32	46.78	56.0	45.0	56.5	41.76	0.0	58.0	0.0	0.0
HEC	0.98	0.52	1.0	1.0	1.0	1.21	0.0	1.0	0.0	0.0
Bactericide	0.19	0.05	0.1	0.1	0.1	0.27	0.0	0.1	0.0	0.0
Triton X-100	0.0	0.0	0.0	0.0	0.0	0.0	0.0	0.0	36.8	0.0
DGBE	0.0	0.0	0.0	0.0	0.0	0.0	44.92	0.0	0.0	26.7
Dielectric Constant	43.42	58.0	42.54	56.1	42.0	56.8	39.9	54.0	39.8	52.5
Conductivity (S/m)	0.85	0.83	0.91	0.95	1.0	1.07	1.42	1.45	1.88	1.78

Salt: 99+% Pure Sodium Chloride

Sugar: 98+% Pure Sucrose

Water: De-ionized, 16 MΩ+ resistivity


HEC: Hydroxyethyl Cellulose

DGBE: 99+% Di(ethylene glycol) butyl ether, [2-(2-butoxyethoxy)ethanol]

Triton X-100 (ultra pure): Polyethylene glycol mono [4-(1,1,3,3-tetramethylbutyl)phenyl]ether

4 SIMULATING LIQUID PARAMETERS CHECK

The simulating liquids should be checked at the beginning of a series of SAR measurements to determine if the dielectric parameters are within the tolerances of the specified target values. The relative permittivity and conductivity of the tissue material should be within $\pm 5\%$ of the values given in the table below.

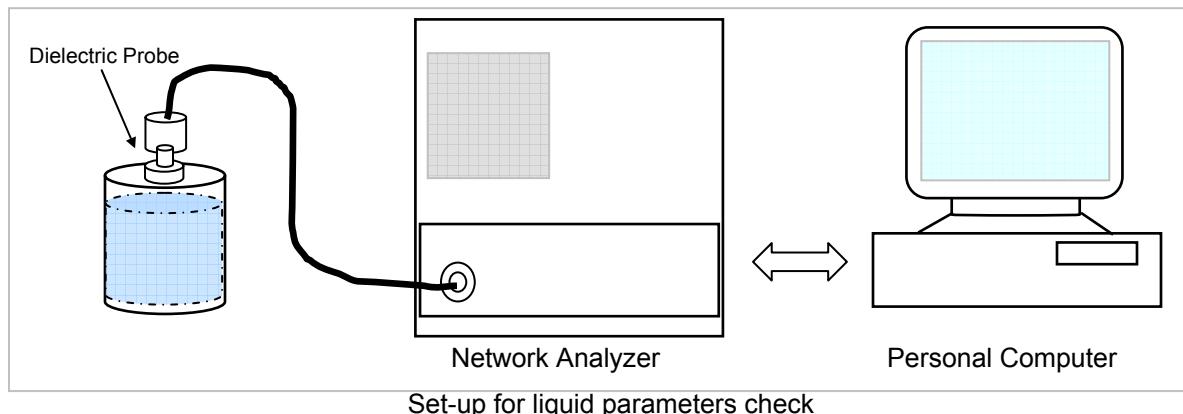

Reference Values of Tissue Dielectric Parameters for Head and Body Phantom (for 150 – 3000 MHz and 5800 MHz)

The head tissue dielectric parameters recommended by the IEEE SCC-34/SC-2 in IEEE Standard 1528 have been incorporated in the following table. These head parameters are derived from planar layer models simulating the highest expected SAR for the dielectric properties and tissue thickness variations in a human head. Other head and body tissue parameters that have not been specified in P1528 are derived from the tissue dielectric parameters computed from the 4-Cole-Cole equations and extrapolated according to the head parameters specified in IEEE Standard 1528.

Target Frequency (MHz)	Head		Body	
	ϵ_r	σ (S/m)	ϵ_r	σ (S/m)
150	52.3	0.76	61.9	0.80
300	45.3	0.87	58.2	0.92
450	43.5	0.87	56.7	0.94
835	41.5	0.90	55.2	0.97
900	41.5	0.97	55.0	1.05
915	41.5	0.98	55.0	1.06
1450	40.5	1.20	54.0	1.30
1610	40.3	1.29	53.8	1.40
1800 – 2000	40.0	1.40	53.3	1.52
2450	39.2	1.80	52.7	1.95
3000	38.5	2.40	52.0	2.73
5800	35.3	5.27	48.2	6.00

(ϵ_r = relative permittivity, σ = conductivity and $\rho = 1000 \text{ kg/m}^3$)

**Reference Values of Tissue Dielectric Parameters for Head and Body Phantom
(for 3000 MHz – 5800 MHz)**

In the current guidelines and draft standards for compliance testing of mobile phones (i.e., IEEE P1528, OET 65 Supplement C), the dielectric parameters suggested for head and body tissue simulating liquid are given only at 3.0 GHz and 5.8 GHz. As an intermediate solution, dielectric parameters for the frequencies between 5 to 5.8 GHz were obtained using linear interpolation (see table below).

SPEAG has developed suitable head and body tissue simulating liquids consisting of the following ingredients: de-ionized water, salt and a special composition including mineral oil and an emulgators. Dielectric parameters of these liquids were measured suing a HP 8570C Dielectric Probe Kit in conjunction with HP 8753ES Network Analyzer (30 kHz – 6G Hz). The differences with respect to the interpolated values were well within the desired $\pm 5\%$ for the whole 5 to 5.8 GHz range.

f (MHz)	Head Tissue		Body Tissue		Reference
	rel. permittivity	conductivity	rel. permittivity	conductivity	
3000	38.5	2.40	52.0	2.73	Standard
5800	35.3	5.27	48.2	6.00	Standard
5000	36.2	1.45	49.3	5.07	Interpolated
5100	36.1	4.55	49.1	5.18	Interpolated
5200	36.0	4.66	49.0	5.30	Interpolated
5300	35.9	4.76	48.9	5.42	Interpolated
5400	35.8	4.86	48.7	5.53	Interpolated
5500	35.6	4.96	48.6	5.65	Interpolated
5600	35.5	5.07	48.5	5.77	Interpolated
5700	35.4	5.17	48.3	5.88	Interpolated

(ϵ_r = relative permittivity, σ = conductivity and $\rho = 1000 \text{ kg/m}^3$)

4.1 SIMULATING LIQUID PARAMETER CHECK RESULT

Simulating Liquid Dielectric Parameter Check Result @ Muscle 2450 MHz

Room Ambient Temperature = 22°C; Relative humidity = 35% Measured by: Ninous Davoudi

Simulating Liquid			Parameters		Measured	Target	Deviation (%)	Limit (%)
f (MHz)	Temp. (°C)	Depth (cm)	e'	e" (ε _r)	Relative Permittivity (ε _r):	Conductivity (σ):		
2450	21	15	e'	52.5718	52.5718	1.97705	52.7	-0.24
			e"	14.5055	14.2532	1.95		1.39

Liquid Check

Ambient temperature: 22.0 deg. C; Liquid temperature: 21.0 deg C

March 01, 2007 09:10 AM

Frequency	e'	e"
2400000000.	52.8946	14.3011
2405000000.	52.8461	14.2532
2410000000.	52.8211	14.2443
2415000000.	52.7887	14.2414
2420000000.	52.7460	14.2481
2425000000.	52.7075	14.2726
2430000000.	52.6524	14.3226
2435000000.	52.6289	14.3818
2440000000.	52.6192	14.4159
2445000000.	52.5849	14.4513
2450000000.	52.5718	14.5055
2455000000.	52.5985	14.5929
2460000000.	52.6178	14.6477
2465000000.	52.6694	14.7146
2470000000.	52.6555	14.7903
2475000000.	52.6673	14.8554
2480000000.	52.6529	14.9091
2485000000.	52.6326	14.9433
2490000000.	52.6091	14.9394
2495000000.	52.5882	14.9050
2500000000.	52.5534	14.8659

The conductivity (σ) can be given as:

$$\sigma = \omega \epsilon_0 e'' = 2 \pi f \epsilon_0 e''$$

where $f = \text{target } f * 10^6$

$$\epsilon_0 = 8.854 * 10^{-12}$$

Simulating Liquid Parameter Check Result @ Muscle 5GHz

Room Ambient Temperature = 24°C; Relative humidity = 40%

Measured by: Ninous Davoudi

Simulating Liquid			Parameters		Measured	Target	Deviation (%)	Limit (%)
f (MHz)	Temp. (°C)	Depth (cm)	e'	Relative Permittivity (ϵ_r):				
5200	23	15	e'	49.3462	49.3462	49.0	0.71	± 10
			e''	18.8707	Conductivity (σ):	5.30	3.00	± 5

Liquid Check

Ambient temperature: 24.0 deg. C; Liquid temperature: 23.0 deg C

March 02, 2007 08:59 AM

Frequency	e'	e''
4600000000.	50.5013	17.4846
4650000000.	50.8297	17.8665
4700000000.	50.3391	17.5642
4750000000.	50.2305	18.0154
4800000000.	50.3408	17.8894
4850000000.	49.9083	18.0568
4900000000.	50.1342	18.2509
4950000000.	49.9138	18.1347
5000000000.	49.8871	18.5073
5050000000.	49.9230	18.2688
5100000000.	49.6642	18.6773
5150000000.	49.8165	18.7192
5200000000.	49.3462	18.8707
5250000000.	49.6065	18.9174
5300000000.	49.4059	18.8123
5350000000.	49.3898	18.9417
5400000000.	49.4909	18.8811
5450000000.	49.0001	18.8199
5500000000.	49.0884	18.9454
5550000000.	48.8375	18.9324
5600000000.	48.5919	19.0360
5650000000.	48.5605	19.0950
5700000000.	48.4951	19.2051
5750000000.	48.6183	19.3307
5800000000.	48.3014	19.1722
5850000000.	48.0864	19.5094
5900000000.	48.4708	19.4162
5950000000.	47.5970	19.3083
6000000000.	48.0330	20.0436

The conductivity (σ) can be given as:

$$\sigma = \omega \epsilon_0 e'' = 2 \pi f \epsilon_0 e''$$

where $f = \text{target } f * 10^6$

$$\epsilon_0 = 8.854 * 10^{-12}$$

Simulating Liquid Parameter Check Result @ Muscle 5GHz

Room Ambient Temperature = 24°C; Relative humidity = 40%

Measured by: Ninous Davoudi

Simulating Liquid			Parameters		Measured	Target	Deviation (%)	Limit (%)
f (MHz)	Temp. (°C)	Depth (cm)	e'	Relative Permittivity (ϵ_r):				
5500	23	15	e'	49.0884	49.0884	48.6	1.00	± 10
			e''	18.9454	5.79676	5.65	2.60	± 5

Liquid Check

Ambient temperature: 24.0 deg. C; Liquid temperature: 23.0 deg C

March 02, 2007 08:59 AM

Frequency	e'	e''
4600000000.	50.5013	17.4846
4650000000.	50.8297	17.8665
4700000000.	50.3391	17.5642
4750000000.	50.2305	18.0154
4800000000.	50.3408	17.8894
4850000000.	49.9083	18.0568
4900000000.	50.1342	18.2509
4950000000.	49.9138	18.1347
5000000000.	49.8871	18.5073
5050000000.	49.9230	18.2688
5100000000.	49.6642	18.6773
5150000000.	49.8165	18.7192
5200000000.	49.3462	18.8707
5250000000.	49.6065	18.9174
5300000000.	49.4059	18.8123
5350000000.	49.3898	18.9417
5400000000.	49.4909	18.8811
5450000000.	49.0001	18.8199
5500000000.	49.0884	18.9454
5550000000.	48.8375	18.9324
5600000000.	48.5919	19.0360
5650000000.	48.5605	19.0950
5700000000.	48.4951	19.2051
5750000000.	48.6183	19.3307
5800000000.	48.3014	19.1722
5850000000.	48.0864	19.5094
5900000000.	48.4708	19.4162
5950000000.	47.5970	19.3083
6000000000.	48.0330	20.0436

The conductivity (σ) can be given as:

$$\sigma = \omega \epsilon_0 e'' = 2 \pi f \epsilon_0 e''$$

where $f = \text{target } f * 10^6$

$$\epsilon_0 = 8.854 * 10^{-12}$$

Simulating Liquid Parameter Check Result @ Muscle 5GHz

Room Ambient Temperature = 24°C; Relative humidity = 40%

Measured by: Ninous Davoudi

Simulating Liquid			Parameters		Measured	Target	Deviation (%)	Limit (%)
f (MHz)	Temp. (°C)	Depth (cm)	e'	Relative Permittivity (ϵ_r):				
5800	23	15	e'	48.4728	48.4728	48.2	0.57	± 10
			e''	19.3582	6.24614	6.00	4.10	± 5

Liquid Check

Ambient temperature: 24.0 deg. C; Liquid temperature: 23.0 deg C

March 05, 2007 08:52 AM

Frequency	e'	e''
4600000000.	50.6788	17.6274
4650000000.	50.9264	17.8926
4700000000.	50.4557	17.7146
4750000000.	50.4754	18.0685
4800000000.	50.4211	17.9845
4850000000.	50.1883	18.1889
4900000000.	50.2528	18.3098
4950000000.	50.1268	18.3009
5000000000.	50.1107	18.5323
5050000000.	50.0238	18.4141
5100000000.	49.9293	18.7327
5150000000.	49.8870	18.7257
5200000000.	49.5801	18.9358
5250000000.	49.8280	18.9153
5300000000.	49.5690	18.8946
5350000000.	49.6860	19.0000
5400000000.	49.5896	18.9658
5450000000.	49.2900	18.9287
5500000000.	49.2400	19.0030
5550000000.	49.0038	18.9587
5600000000.	48.8079	19.1354
5650000000.	48.7200	19.1017
5700000000.	48.6700	19.3816
5750000000.	48.8130	19.3449
5800000000.	48.4728	19.3582
5850000000.	48.4707	19.6288
5900000000.	48.6700	19.5560
5950000000.	47.9720	19.5847
6000000000.	48.2947	20.1109

The conductivity (σ) can be given as:

$$\sigma = \omega \epsilon_0 e'' = 2 \pi f \epsilon_0 e''$$

where $f = \text{target } f * 10^6$

$$\epsilon_0 = 8.854 * 10^{-12}$$

Simulating Liquid Parameter Check Result @ Muscle 5GHz

Room Ambient Temperature = 24°C; Relative humidity = 45%

Measured by: Ninous Davoudi

Simulating Liquid			Parameters		Measured	Target	Deviation (%)	Limit (%)
f (MHz)	Temp. (°C)	Depth (cm)	e'	Relative Permittivity (ϵ_r):				
5200	23	15	e'	48.6697	48.6697	49.0	-0.67	± 10
			e''	18.4976	Conductivity (σ):	5.35103	5.30	0.96

Liquid Check

Ambient temperature: 24.0 deg. C; Liquid temperature: 23.0 deg C

March 16, 2007 11:03 AM

Frequency	e'	e''
4600000000.	49.4656	17.4232
4650000000.	49.5877	17.4130
4700000000.	49.1926	17.4848
4750000000.	49.2405	17.5887
4800000000.	49.1019	17.7024
4850000000.	49.1024	17.8093
4900000000.	48.9475	17.9557
4950000000.	48.9572	18.0290
5000000000.	48.9331	18.1328
5050000000.	48.8417	18.1801
5100000000.	48.8047	18.2405
5150000000.	48.5904	18.4285
5200000000.	48.6697	18.4976
5250000000.	48.5743	18.5649
5300000000.	48.5394	18.5897
5350000000.	48.4933	18.6199
5400000000.	48.5131	18.6941
5450000000.	48.2383	18.5700
5500000000.	48.0085	18.7030
5550000000.	47.9605	18.5848
5600000000.	47.7047	18.6776
5650000000.	47.6698	18.7293
5700000000.	47.5257	18.9914
5750000000.	47.7282	19.0209
5800000000.	47.4136	18.9409
5850000000.	47.4338	19.2562
5900000000.	47.6542	19.2036
5950000000.	47.0384	19.2219
6000000000.	47.2325	19.7012

The conductivity (σ) can be given as:

$$\sigma = \omega \epsilon_0 e'' = 2 \pi f \epsilon_0 e''$$

where $f = \text{target } f * 10^6$

$$\epsilon_0 = 8.854 * 10^{-12}$$

5 SYSTEM PERFORMANCE CHECK

The system performance check is performed prior to any usage of the system in order to guarantee reproducible results. The system performance check verifies that the system operates within its specifications of $\pm 10\%$.

System Performance Check Measurement Conditions

- The measurements were performed in the flat section of the SAM twin phantom filled with Body simulating liquid of the following parameters.
- The DASY4 system with an Isotropic E-Field Probe EX3DV3-SN: 3531 was used for the measurements.
- The dipole was mounted on the small tripod so that the dipole feed point was positioned below the center marking of the flat phantom section and the dipole was oriented parallel to the body axis (the long side of the phantom). The standard measuring distance was 10 mm (above 1 GHz) and 15 mm (below 1 GHz) from dipole center to the simulating liquid surface.
- The coarse grid with a grid spacing of 15 mm was aligned with the dipole.
For 5 GHz band - The coarse grid with a grid spacing of 10 mm was aligned with the dipole.
- Special 5 x 5 x 7 fine cube was chosen for cube integration($dx=dy=7.5\text{mm}$; $dz=5\text{mm}$).
For 5 GHz band - Special 8x8x8 fine cube was chosen for cube integration($dx=dy=4.3\text{mm}$; $dz=3\text{mm}$)
- Distance between probe sensors and phantom surface was set to 4 mm.
For 5 GHz band - Distance between probe sensors and phantom surface was set to 2.0mm
- The dipole input power (forward power) was $250\text{ mW}\pm 3\%$.
- The results are normalized to 1 W input power.

Reference SAR Values for body-tissue

In the table below, the numerical reference SAR values of a SPEAG validation dipoles placed below the flat phantom filled with body-tissue simulating liquid are given. The reference SAR values were calculated using the finite-difference time-domain method and the geometry parameters.

Dipole Type	Distance (mm)	Frequency (MHz)	SAR (1g) [W/kg]	SAR (10g) [W/kg]	SAR (peak) [W/kg]
D450V2	15	450	5.01	3.36	7.22
D835V2	15	835	9.71	6.38	14.1
D900V2	15	900	11.1	7.17	16.3
D1450V2	10	1450	29.6	16.6	49.8
D1800V2	10	1800	38.5	20.3	67.5
D1900V2	10	1900	39.8	20.8	69.6
D2000V2	10	2000	40.9	21.2	71.5
D2450V2	10	2450	51.2	23.7	97.6

Note: All SAR values normalized to 1 W forward power.

Reference SAR Values for body-tissue

In the table below, the numerical reference SAR values of a SPEAG validation dipoles placed below the flat phantom filled with body-tissue simulating liquid are given. The reference SAR values were calculated using finite-difference time-domain FDTD method (feed point-impedance set to 50 ohms) and the mechanical dimensions of the D5GHzV2 dipole (manufactured by SPEAG).

f (MHz)	Head Tissue		Body Tissue		
	SAR _{1g}	SAR _{10g}	SAR _{1g}	SAR _{10g}	SAR _{Peak}
5000	72.9	20.7	68.1	19.2	260.3
5100	74.6	21.1	78.8	19.6	272.3
5200	76.5	21.6	71.8	20.1	284.7
5500	83.3	23.4	79.1	22.0	326.3
5800	78.0	21.9	74.1	20.5	324.7

Note: All SAR values normalized to 1 W forward power.

System Validation Dipole: D2450V2 SN: 706

Date: March 1, 2007

Room Ambient Temperature = 22°C; Relative humidity = 35% Measured by: Ninous Davoudi

Body Simulating Liquid			SAR (mW/g)		Normalized to 1 W	Target	Deviation (%)	Limit (%)
f (MHz)	Temp. (°C)	Depth (cm)	1g	13.40	53.6	51.2	4.69	± 10
2450	21	15	1g	13.40	53.6	51.2	4.69	± 10
			10g	6.15	24.6	23.7	3.80	± 10

System Validation Dipole: D5GHzV2 SN 1003

Date: March 2, 2007

Room Ambient Temperature = 24°C; Relative humidity = 40% Measured by: Ninous Davoudi

Body Simulating Liquid			SAR (mW/g)		Normalized to 1 W	Target	Deviation (%)	Limit (%)
f (MHz)	Temp. (°C)	Depth (cm)	1g	19.60	78.4	71.8	9.19	± 10
5200	23	15	1g	19.60	78.4	71.8	9.19	± 10
			10g	5.46	21.84	20.1	8.66	± 10

System Validation Dipole: D5GHzV2 SN 1003

Date: March 2, 2007

Room Ambient Temperature = 24°C; Relative humidity = 40% Measured by: Ninous Davoudi

Body Simulating Liquid			SAR (mW/g)		Normalized to 1 W	Target	Deviation (%)	Limit (%)
f (MHz)	Temp. (°C)	Depth (cm)	1g	21.30	85.2	79.1	7.71	± 10
5500	23	15	1g	21.30	85.2	79.1	7.71	± 10
			10g	5.89	23.56	22.0	7.09	± 10

System Validation Dipole: D5GHzV2 SN 1003

Date: March 5, 2007

Room Ambient Temperature = 24°C; Relative humidity = 40% Measured by: Ninous Davoudi

Body Simulating Liquid			SAR (mW/g)		Normalized to 1 W	Target	Deviation (%)	Limit (%)
f (MHz)	Temp. (°C)	Depth (cm)	1g	18.80	75.2	74.1	1.48	± 10
5800	23	15	1g	18.80	75.2	74.1	1.48	± 10
			10g	5.27	21.08	20.5	2.83	± 10

System Validation Dipole: D5GHzV2 SN 1003

Date: March 16, 2007

Room Ambient Temperature = 24°C; Relative humidity = 45% Measured by: Ninous Davoudi

Body Simulating Liquid			SAR (mW/g)		Normalized to 1 W	Target	Deviation (%)	Limit (%)
f (MHz)	Temp. (°C)	Depth (cm)	1g	19.20	76.8	71.8	6.96	± 10
5200	23	15	1g	19.20	76.8	71.8	6.96	± 10
			10g	5.42	21.68	20.1	7.86	± 10

6 SAR MEASURMENT PROCEDURE

A summary of the procedure follows:

- a) A measurement of the SAR value at a fixed location is used as a reference value for assessing the power drop of the DUT. The SAR at this point is measured at the start of the test, and then again at the end of the test.
- b) The SAR distribution at the exposed flat section of the flat phantom is measured at a distance of 4 mm from the inner surface of the shell. The area covers the entire dimension of the DUT and the horizontal grid spacing is 15 mm x 15 mm. Based on this data, the area of the maximum absorption is determined by Spline interpolation. The first Area Scan covers the entire dimension of the DUT to ensure that the hotspot was correctly identified.

For 5 GHz band - The SAR distribution at the exposed flat section of the flat phantom is measured at a distance of 2.0 mm from the inner surface of the shell. The area covers the entire dimension of the DUT and the horizontal grid spacing is 10 mm x 10 mm. Based on this data, the area of the maximum absorption is determined by Spline interpolation. The first Area Scan covers the entire dimension of the DUT to ensure that the hotspot was correctly identified.

- c) Around this point, a volume of X=Y= 30 and Z=21 mm is assessed by measuring 5 x 5 x 7 mm points. On the basis of this data set, the spatial peak SAR value is evaluated with the following procedure:

For 5 GHz band - Around this point, a volume of X=Y=24 and Z=20 mm is assessed by measuring 7 x 7 x 9 mm points. On the basis of this data set, the spatial peak SAR value is evaluated with the following procedure:

- (i) The data at the surface are extrapolated, since the centre of the dipoles is 1.2 mm away from the tip of the probe and the distance between the surface and the lowest measuring point is 1.3 mm. The extrapolation is based on a least square algorithm. A polynomial of the fourth order is calculated through the points in z-axes. This polynomial is then used to evaluate the points between the surface and the probe tip.
- (ii) The maximum interpolated value is searched with a straightforward algorithm. Around this maximum the SAR values averaged over the spatial volumes (1 g and 10 g) are computed using the 3D-Spline interpolation algorithm. The 3D-Spline is composed of three one-dimensional splines with the "Not a knot"- condition (in x, y and z-direction). The volume is integrated with the trapezoidal – algorithm. One thousand points (10 x 10 x 10) are interpolated to calculate the averages.
- (iii) All neighbouring volumes are evaluated until no neighbouring volume with a higher average value is found.
- (iv) The SAR value at the same location as in Step (a) is again measured to evaluate the actual power drift.

6.1 DASY4 SAR MEASURMENT PROCEDURE

Step 1: Power Reference Measurement

The Power Reference Measurement and Power Drift Measurements are for monitoring the power drift of the device under test in the batch process. The Minimum distance of probe sensors to surface determines the closest measurement point to phantom surface. The minimum distance of probe sensors to surface is 2.1 mm. This distance cannot be smaller than the Distance of sensor calibration points to probe tip as defined in the probe properties (for example, 1.2 mm for an EX3DV3 probe type).

Step 2: Area Scan

The Area Scan is used as a fast scan in two dimensions to find the area of high field values, before doing a fine measurement around the hot spot. The sophisticated interpolation routines implemented in DASY4 software can find the maximum locations even in relatively coarse grids. When an Area Scan has measured all reachable points, it computes the field maximal found in the scanned area, within a range of the global maximum. The range (in dB) is specified in the standards for compliance testing. For example, a 2 dB range is required in IEEE Standard 1528, EN 50361 and IEC 62209 standards, whereby 3 dB is a requirement when compliance is assessed in accordance with the ARIB standard (Japan). If only one Zoom Scan follows the Area Scan, then only the absolute maximum will be taken as reference. For cases where multiple maximums are detected, the number of Zoom Scans has to be increased accordingly.

Step 3: Zoom Scan

Zoom Scans are used to assess the peak spatial SAR values within a cubic averaging volume containing 1 g and 10 g of simulated tissue. The Zoom Scan measures 5 x 5 x 7 points within a cube whose base faces are centered on the maxima found in a preceding area scan job within the same procedure. When the measurement is done, the Zoom Scan evaluates the averaged SAR for 1 g and 10 g and displays these values next to the job's label.

For 5 GHz band – Same as above except the Zoom Scan measures 7 x 7 x 9 points.

Step 4: Power drift measurement

The Power Drift Measurement measures the field at the same location as the most recent power reference measurement within the same procedure, and with the same settings. The Power Drift Measurement gives the field difference in dB from the reading conducted within the last Power Reference Measurement. This allows a user to monitor the power drift of the device under test within a batch process. The measurement procedure is the same as Step 1.

Step 5: Z-Scan

The Z Scan measures points along a vertical straight line. The line runs along the Z-axis of a one-dimensional grid. In order to get a reasonable extrapolation, the extrapolated distance should not be larger than the step size in Z-direction.

7 PROCEDURE USED TO ESTABLISH TEST SIGNAL

The following procedures had been used to prepare the EUT for the SAR test.

The client provided a special driver and program, ART version 5.3 build 22, which enable a user to control the frequency and output power of the module.

b mode

Channel	Frequency (MHz)	Power (dBm)
Low	2412	17.3
Middle	2437	17.5
High	2462	17.6

g mode

Channel	Frequency (MHz)	Power (dBm)
Low	2412	17.4
Middle	2437	17.3
High	2462	17.5

a mode

Channel	Frequency (MHz)	Power (dBm)
Low	5180	16.2
Low	5260	16.4
Middle	5280	16.1
High	5320	16.0

Channel	Frequency (MHz)	Power (dBm)
Low	5500	16.5
Middle	5600	16.6
High	5700	16.1

Channel	Frequency (MHz)	Power (dBm)
Low	5745	19.2
Middle	5785	18.5
High	5825	18.4

8 SAR MEASURMENT RESULTS

8.1 2.4GHZ BAND

8.1.1 TOP POSITION



802.11b (1Mbps)

Channel	f (MHz)	Measured SAR 1g (mW/g)	Power Drift (dB)	Extrapolated ¹⁾ SAR 1g (mW/g)
1	2412	0.685	0.000	0.685
6	2437	0.780	-0.093	0.797
11	2462	0.683	-0.062	0.693

802.11g (6 Mbps)

Channel	f (MHz)	Measured SAR 1g (mW/g)	Power Drift (dB)	Extrapolated ¹⁾ SAR 1g (mW/g)
1	2412			
6	2437	0.485	0.000	0.485
11	2462			

Notes:

- 1) The exact method of extrapolation is Measured SAR $\times 10^{(-\text{drift}/10)}$. The SAR reported at the end of the measurement process by the DASY4 system can be scaled up by the Power drift to determine the SAR at the beginning of the measurement process.
- 2) The SAR measured at the middle channel for this configuration is at least 3 dB lower (0.8 mW/g) than SAR limit (1.6 mW/g), thus testing at low & high channel is optional.
- 3) Please see attachments for the detailed measurement data and plots showing the maximum SAR location of the EUT.
- 4) For this position, the separation distance from the closest point on DUT to phantom is 5mm.

8.1.2 SIDE POSITION



802.11b (1Mbps)

Channel	f (MHz)	Measured SAR 1g (mW/g)	Power Drift (dB)	Extrapolated ¹⁾ SAR 1g (mW/g)
1	2412			
6	2437			
11	2462	0.146	-0.195	0.153

802.11g (6 Mbps)

Channel	f (MHz)	Measured SAR 1g (mW/g)	Power Drift (dB)	Extrapolated ¹⁾ SAR 1g (mW/g)
1	2412			
6	2437			
11	2462	0.107	0.000	0.107

Notes:

- 1) The exact method of extrapolation is Measured SAR $\times 10^{(-\text{drift}/10)}$. The SAR reported at the end of the measurement process by the DASY4 system can be scaled up by the Power drift to determine the SAR at the beginning of the measurement process.
- 2) The SAR measured at the middle channel for this configuration is at least 3 dB lower (0.8 mW/g) than SAR limit (1.6 mW/g), thus testing at low & high channel is optional.
- 3) Please see attachments for the detailed measurement data and plots showing the maximum SAR location of the EUT.

8.2 5GHz BAND

8.2.1 TOP POSITION



802.11a 5.2 GHz (6 Mbps)

Channel	f (MHz)	Measured SAR 1g (mW/g)	Power Drift (dB)	Extrapolated ¹⁾ SAR 1g (mW/g)
63	5180	0.916	-0.176	0.954
52	5260	0.853	-0.124	0.878
54	5280	1.030	0.000	1.030
64	5320	1.420	-0.115	1.458

802.11a 5.5 GHz (6 Mbps)

Channel	f (MHz)	Measured SAR 1g (mW/g)	Power Drift (dB)	Extrapolated ¹⁾ SAR 1g (mW/g)
100	5500	1.300	-0.043	1.313
120	5600	1.410	-0.017	1.416
140	5700	0.567	-0.174	0.590

802.11a 5.8 GHz (6 Mbps)

Channel	f (MHz)	Measured SAR 1g (mW/g)	Power Drift (dB)	Extrapolated ¹⁾ SAR 1g (mW/g)
149	5745	0.816	-0.055	0.826
157	5785	0.589	0.000	0.589
165	5825	0.628	-0.137	0.648

Notes:

- 1) The exact method of extrapolation is Measured SAR x 10^{-drift/10}. The SAR reported at the end of the measurement process by the DASY4 system can be scaled up by the Power drift to determine the SAR at the beginning of the measurement process.
- 2) The SAR measured at the middle channel for this configuration is at least 3 dB lower (0.8 mW/g) than SAR limit (1.6 mW/g), thus testing at low & high channel is optional.
- 3) Please see attachments for the detailed measurement data and plots showing the maximum SAR location of the EUT.
- 4) For this position, the separation distance from the closest point on DUT to phantom is 5mm.

8.2.2 SIDE POSITION



802.11a 5.2 GHz (6 Mbps)

Channel	f (MHz)	Measured SAR 1g (mW/g)	Power Drift (dB)	Extrapolated ¹⁾ SAR 1g (mW/g)
52	5260			
54	5280	0.174	0.000	0.174
64	5320			

802.11a 5.5 GHz (6 Mbps)

Channel	f (MHz)	Measured SAR 1g (mW/g)	Power Drift (dB)	Extrapolated ¹⁾ SAR 1g (mW/g)
100	5500			
120	5600	0.086	-0.143	0.089
140	5700			

802.11a 5.8 GHz (6 Mbps)

Channel	f (MHz)	Measured SAR 1g (mW/g)	Power Drift (dB)	Extrapolated ¹⁾ SAR 1g (mW/g)
149	5745			
157	5785	0.029	0.000	0.029
165	5825			

Notes:

- 1) The exact method of extrapolation is $\text{Measured SAR} \times 10^{(-\text{drift}/10)}$. The SAR reported at the end of the measurement process by the DASY4 system can be scaled up by the Power drift to determine the SAR at the beginning of the measurement process.
- 2) The SAR measured at the middle channel for this configuration is at least 3 dB lower (0.8 mW/g) than SAR limit (1.6 mW/g), thus testing at low & high channel is optional.
- 3) Please see attachments for the detailed measurement data and plots showing the maximum SAR location of the EUT.

9 MEASURMENT UNCERTAINTY

9.1 MEASURMENT UNCERTAINTY FOR 300 MHz – 3000 MHz

Uncertainty component	Tol. (±%)	Probe Dist.	Div.	Ci (1g)	Ci (10g)	Std. Unc.(±%)	
						Ui (1g)	Ui(10g)
Measurement System							
Probe Calibration	4.80	N	1	1	1	4.80	4.80
Axial Isotropy	4.70	R	1.732	0.707	0.707	1.92	1.92
Hemispherical Isotropy	9.60	R	1.732	0.707	0.707	3.92	3.92
Boundary Effects	1.00	R	1.732	1	1	0.58	0.58
Linearity	4.70	R	1.732	1	1	2.71	2.71
System Detection Limits	1.00	R	1.732	1	1	0.58	0.58
Readout Electronics	1.00	N	1	1	1	1.00	1.00
Response Time	0.80	R	1.732	1	1	0.46	0.46
Integration Time	2.60	R	1.732	1	1	1.50	1.50
RF Ambient Conditions - Noise	1.59	R	1.732	1	1	0.92	0.92
RF Ambient Conditions - Reflections	0.00	R	1.732	1	1	0.00	0.00
Probe Positioner Mechanical Tolerance	0.40	R	1.732	1	1	0.23	0.23
Probe Positioning With Respect to Phantom Shell	2.90	R	1.732	1	1	1.67	1.67
Extrapolation, interpolation, and integration algorithms for max. SAR evaluation	3.90	R	1.732	1	1	2.25	2.25
Test sample Related							
Test Sample Positioning	1.10	N	1	1	1	1.10	1.10
Device Holder Uncertainty	3.60	N	1	1	1	3.60	3.60
Power and SAR Drift Measurement	5.00	R	1.732	1	1	2.89	2.89
Phantom and Tissue Parameters							
Phantom Uncertainty	4.00	R	1.732	1	1	2.31	2.31
Liquid Conductivity - Target	5.00	R	1.732	0.64	0.43	1.85	1.24
Liquid Conductivity - Meas.	8.60	N	1	0.64	0.43	5.50	3.70
Liquid Permittivity - Target	5.00	R	1.732	0.6	0.49	1.73	1.41
Liquid Permittivity - Meas.	3.30	N	1	0.6	0.49	1.98	1.62
Combined Standard Uncertainty							
Expanded Uncertainty (95% Confidence Interval)							
RSS						11.44	10.49
K=2						22.87	20.98
Notes for table							
1. Tol. - tolerance in influence quality							
2. N - Nominal							
3. R - Rectangular							
4. Div. - Divisor used to obtain standard uncertainty							
5. Ci - is the sensitivity coefficient							

9.2 MEASURMENT UNCERTAINTY 3 GHz – 6 GHz

Uncertainty component	Tol. (±%)	Probe Dist.	Div.	Ci (1g)	Ci (10g)	Std. Unc.(±%)	
						Ui (1g)	Ui(10g)
Measurement System							
Probe Calibration	4.80	N	1	1	1	4.80	4.80
Axial Isotropy	4.70	R	1.732	0.707	0.707	1.92	1.92
Hemispherical Isotropy	9.60	R	1.732	0.707	0.707	3.92	3.92
Boundary Effects	1.00	R	1.732	1	1	0.58	0.58
Linearity	4.70	R	1.732	1	1	2.71	2.71
System Detection Limits	1.00	R	1.732	1	1	0.58	0.58
Readout Electronics	1.00	N	1	1	1	1.00	1.00
Response Time	0.80	R	1.732	1	1	0.46	0.46
Integration Time	2.60	R	1.732	1	1	1.50	1.50
RF Ambient Conditions - Noise	3.00	R	1.732	1	1	1.73	1.73
RF Ambient Conditions - Reflections	3.00	R	1.732	1	1	1.73	1.73
Probe Positioner Mechanical Tolerance	0.40	R	1.732	1	1	0.23	0.23
Probe Positioning With Respect to Phantom Shell	2.90	R	1.732	1	1	1.67	1.67
Extrapolation, interpolation, and integration algorithms for max. SAR evaluation	3.90	R	1.732	1	1	2.25	2.25
Test sample Related							
Test Sample Positioning	1.10	N	1	1	1	1.10	1.10
Device Holder Uncertainty	3.60	N	1	1	1	3.60	3.60
Power and SAR Drift Measurement	5.00	R	1.732	1	1	2.89	2.89
Phantom and Tissue Parameters							
Phantom Uncertainty	4.00	R	1.732	1	1	2.31	2.31
Liquid Conductivity - Target	5.00	R	1.732	0.64	0.43	1.85	1.24
Liquid Conductivity - Meas.	8.60	N	1	0.64	0.43	5.50	3.70
Liquid Permittivity - Target	5.00	R	1.732	0.6	0.49	1.73	1.41
Liquid Permittivity - Meas.	3.30	N	1	0.6	0.49	1.98	1.62
Combined Standard Uncertainty							
RSS							
K=2							
11.66							
23.32							
21.46							

Notes for table


1. Tol. - tolerance in influence quality
2. N - Nomal
3. R - Rectangular
4. Div. - Divisor used to obtain standard uncertainty
5. Ci - is the sensitivity coefficient

10 EQUIPMENT LIST AND CALIBRATION

Name of Equipment	Manufacturer	Type/Model	Serial Number	Cal. Due date		
				MM	DD	Year
Robot - Six Axes	Stäubli	RX90BL	N/A			N/A
Robot Remote Control	Stäubli	CS7MB	3403-91535			N/A
DASY4 Measurement Server	SPEAG	SEUMS001BA	1041			N/A
Probe Alignment Unit	SPEAG	LB (V2)	261			N/A
SAM Phantom (SAM1)	SPEAG	TP-1185	QD000P40CA			N/A
SAM Phantom (SAM2)	SPEAG	TP-1015	N/A			N/A
Electronic Probe kit	HP	85070C	N/A			N/A
S-Parameter Network Analyzer	Agilent	8753ES-6	US39173569	2	14	2008
E-Field Probe	SPEAG	EX3DV4	3552	5	30	2007
Thermometer	ERTCO	639-1S	1718	11	7	2007
Data Acquisition Electronics	SPEAG	DAE3 V1	427	11	16	2007
System Validation Dipole	SPEAG	D2450V2	706	4	27	2008
System Validation Dipole	SPEAG	D5GHzV2	1003	11	22	2007
Power Meter	HP	438A	3513U04320	9	4	2007
Amplifier	Mini-Circuits	ZVE-8G	360			N/A
Amplifier	Mini-Circuits	ZHL-42W	D072701-5			N/A
Radio Communication Tester	R & S	CMU 200	838114/032	3	21	2007
Simulating Liquid	CCS	M2450	N/A	Within 24 hrs of first test		
Simulating Liquid	SPEAG	M5200-5800	N/A	Within 24 hrs of first test		

11 PHOTOS


DUT

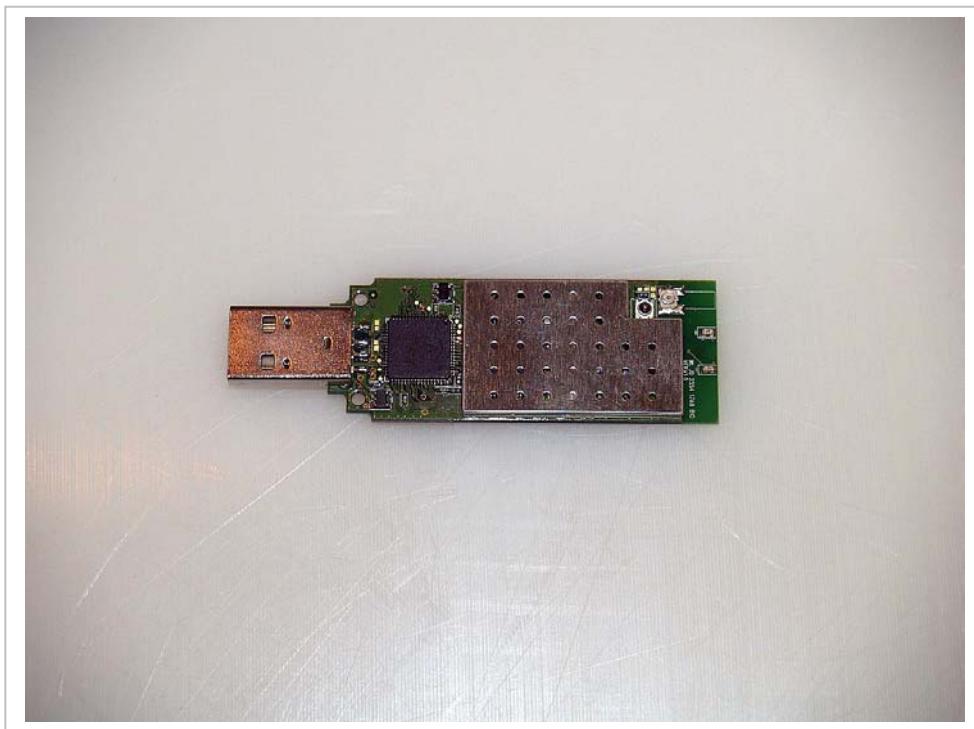


DWL-AG132



DUT location

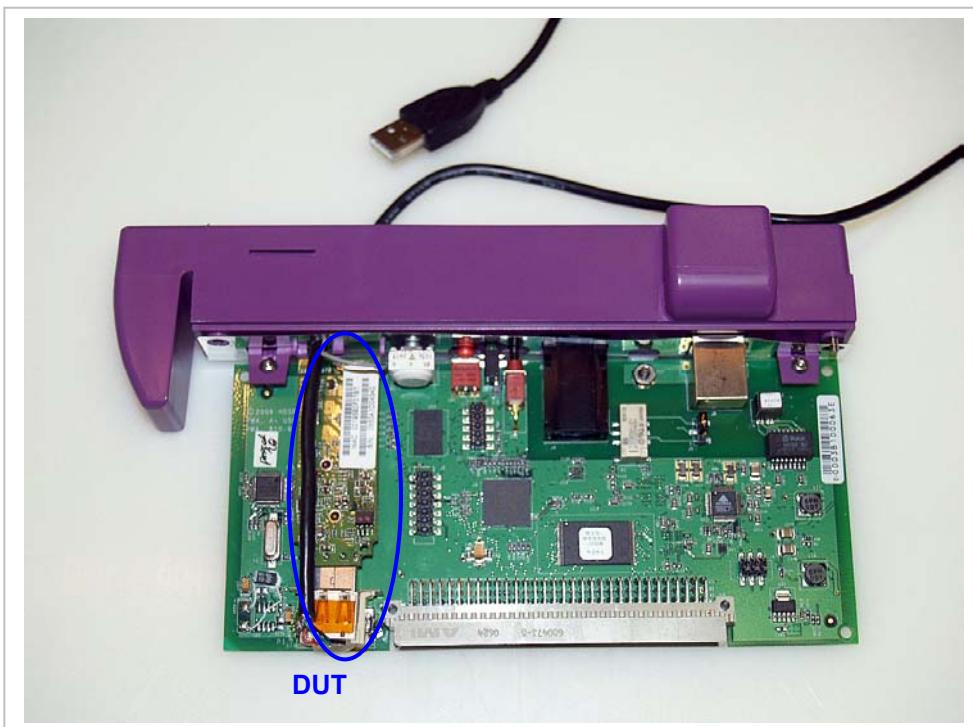

Antenna

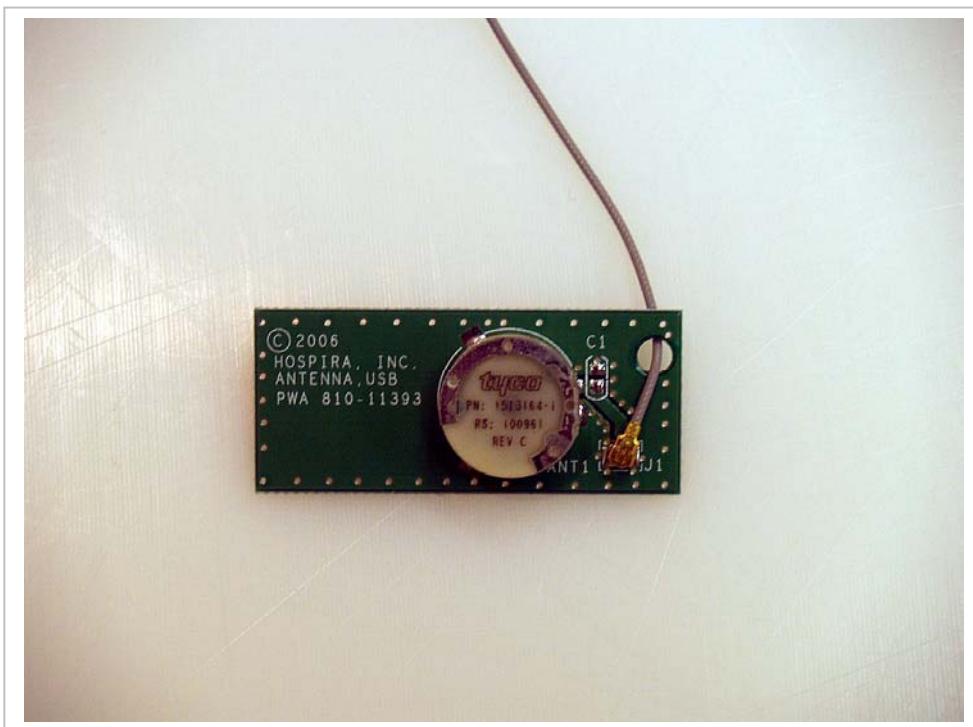

12 ATTACHMENTS

No.	Contents	No. Of Pages
1	System Performance Check Plots	8
2-1	SAR Test Plots - 2.4GHz	6
2-2	SAR Test Plots – 5GHz	14
3	Certificate of E-Field Probe - EXDV4SN3552	9
4	Certificate of System Validation Dipole - D2450 SN:706	9
5	Certificate of System Validation Dipole - D5GHzV2 SN:1003	10

END OF REPORT