



**PCTEST ENGINEERING LABORATORY, INC.**  
**6660 – B Dobbin Road • Columbia, MD 21045 • USA**  
**Telephone 410.290.6652 / Fax 410.290.6654**  
**<http://www.pctestlab.com> (email: randy@pctestlab.com)**



## **CERTIFICATE OF COMPLIANCE (SAR EVALUATION)**

### **APPLICANT NAME & ADDRESS:**

Simbex, LLC  
 10 Water Street, Suite 410  
 Lebanon, NH 03766

### **DATE & LOCATION OF TESTING:**

Dates of Tests: Jan. 28 - Feb. 4, 2005  
 Test Report S/N: SAR.0501210032.SUN  
 Test Site: PCTEST Lab, Columbia, MD USA

**FCC ID:**

**SUN-0226000**

**APPLICANT:**

**SIMBEX**

**EUT Type:**

**Head Impact Encoder**

**Tx Frequency:**

**902.24 – 927.82 MHz (FHSS)**

**Max. RF Output Power:**

**0.173 W (22.37 dBm) Conducted**

**Max. SAR Measurement:**

**1.27 W/kg Head SAR**

**Trade Name/Model(s):**

**SIMBEX MX ENCODER**

**FCC Classification:**

**Part 15 Spread Spectrum Transmitter (DSS)**

**FCC Rule Part(s):**

**§2.1093; FCC/OET Bulletin 65 Supplement C [July 2001]**

**Test Device Serial No.:**

**Identical Prototype [S/N: 121704-0067]**

This wireless device has been deemed portable by the applicant and has shown to be capable of compliance for localized specific absorption rate (SAR) for uncontrolled environment/general population exposure limits specified in ANSI/IEEE Std. C95.1-1992 and had been tested in accordance with the measurement procedures specified in FCC/OET Bulletin 65 Supplement C (2001), Industry Canada RSS-102 and IEEE Std. 1528-2003.

I attest to the accuracy of data. All measurements reported herein were performed by me or were made under my supervision and are correct to the best of my knowledge and belief. I assume full responsibility for the completeness of these measurements and vouch for the qualifications of all persons taking them.

*PCTEST certifies that no party to this application has been denied the FCC benefits pursuant to Section 5301 of the Anti-Drug Abuse Act of 1988, 21 U.S.C. 862.*

  
 Alfred Cirwithian

Vice President Engineering



### **PCTEST™ SAR TEST REPORT**



### **SAR MEASUREMENT REPORT**



Reviewed by:  
 Quality Manager

**Filename:**  
 SAR.0501210032.SUN

**Test Dates:**  
 Jan. 28 - Feb. 4, 2005

**EUT Type:** Head Impact Encoder

**FCC ID:**  
 SUN-0226000

Page 1 of 21

## TABLE OF CONTENTS

1. INTRODUCTION / SAR DEFINITION.....	3
2. SAR MEASUREMENT SETUP .....	4
3. ALIDX-500 E-FIELD PROBE SYSTEM .....	5
4. PROBE CALIBRATION PROCESS .....	6
5. PHANTOM & EQUIVALENT TISSUES .....	7
6. TEST SYSTEM SPECIFICATIONS .....	8
7. TEST CONFIGURATION POSITION.....	9
8. ANSI/IEEE C95.1 - 1992 RF EXPOSURE LIMITS .....	10
9. MEASUREMENT UNCERTAINTIES .....	11
10. SYSTEM VERIFICATION.....	12
11. SAR TEST DATA SUMMARY.....	13
12. SAR DATA SUMMARY.....	14
13. SAR TEST EQUIPMENT.....	15
14. CONCLUSION.....	16
15. REFERENCES .....	17

PCTEST™ SAR TEST REPORT		SAR MEASUREMENT REPORT		Sembex	Reviewed by: Quality Manager
Filename: SAR.0501210032.SUN		Test Dates: Jan. 28 - Feb. 4, 2005	EUT Type: Head Impact Encoder	FCC ID: SUN-0226000	Page 2 of 21

## 1. INTRODUCTION / SAR DEFINITION

The FCC has adopted the guidelines for evaluating the environmental effects of radiofrequency radiation in ET Docket 93-62 on Aug. 6, 1996 to protect the public and workers from the potential hazards of RF emissions due to FCC-regulated portable devices.[1]

The safety limits used for the environmental evaluation measurements are based on the criteria published by the American National Standards Institute (ANSI) for localized specific absorption rate (SAR) in *IEEE/ANSI C95.1-1992 Standard for Safety Levels with Respect to Human Exposure to Radio Frequency Electromagnetic Fields, 3 kHz to 300 GHz*. (c) 1992 by the Institute of Electrical and Electronics Engineers, Inc., New York, New York 10017.[2] The measurement procedure described in *IEEE/ANSI C95.3-1992 Recommended Practice for the Measurement of Potentially Hazardous Electromagnetic Fields - RF and Microwave*[3] is used for guidance in measuring SAR due to the RF radiation exposure from the Equipment Under Test (EUT). These criteria for SAR evaluation are similar to those recommended by the National Council on Radiation Protection and Measurements (NCRP) in *Biological Effects and Exposure Criteria for Radiofrequency Electromagnetic Fields*, NCRP Report No. 86 (c) NCRP, 1986, Bethesda, MD 20814.[6] SAR is a measure of the rate of energy absorption due to exposure to an RF transmitting source. SAR values have been related to threshold levels for potential biological hazards.

### SAR Definition

Specific Absorption Rate (SAR) is defined as the time derivative (rate) of the incremental energy ( $dU$ ) absorbed by (dissipated in) an incremental mass ( $dm$ ) contained in a volume element ( $dV$ ) of a given density ( $\rho$ ). It is also defined as the rate of RF energy absorption per unit mass at a point in an absorbing body (see Fig. 1.1).

$$SAR = \frac{d}{d t} \left( \frac{dU}{dm} \right) = \frac{d}{d t} \left( \frac{dU}{\rho dV} \right)$$

**Figure 1.1**  
**SAR Mathematical Equation**

**SAR is expressed in units of Watts per Kilogram (W/kg).**

$$SAR = \sigma E^2 / \rho$$

where:

- $\sigma$  = conductivity of the tissue-simulant material (S/m)
- $\rho$  = mass density of the tissue-simulant material (kg/m<sup>3</sup>)
- $E$  = Total RMS electric field strength (V/m)

NOTE: The primary factors that control rate of energy absorption were found to be the wavelength of the incident field in relations to the dimensions and geometry of the irradiated organism, the orientation of the organism in relation to the polarity of field vectors, the presence of reflecting surfaces, and whether conductive contact is made by the organism with a ground plane.[6]

PCTEST™ SAR TEST REPORT	SAR MEASUREMENT REPORT			Sumbex	Reviewed by: Quality Manager
Filename: SAR.0501210032.SUN	Test Dates: Jan. 28 - Feb. 4, 2005	EUT Type: Head Impact Encoder	FCC ID: SUN-0226000		Page 3 of 21

## 2. SAR MEASUREMENT SETUP


### Robotic System

Measurements are performed using the ALIDX-500 automated dosimetric assessment system. The ALIDX-500 is made by IDX Robotics, Inc. (IDX) in the United States and consists of high precision robotics system (CRS), robot controller, Pentium 4 computer, near-field probe, probe alignment sensor, and the Left and Right SAM phantoms containing the head/brain equivalent tissue, and the flat phantoms for body/muscle equivalent. The robot is a six-axis industrial robot performing precise movements to position the probe to the location (points) of maximum electromagnetic field (EMF) (see Fig. 2.1).

### System Hardware

The Robot table consists of the power supply, robot controller, safety computer, teach pendant (Joystick), six-axis robot arm, and the probe. The cell controller consists of DELL Dimension 4300 Pentium-4 1.6 GHz computer with Windows 2000 system and SAR Measurement software, National Instruments analog card, monitor, keyboard, and mouse. The robot controller is connected to the cell controller to communicate between the two computers. The probe data is connected to the cell controller via data acquisition cables.

### System Electronics

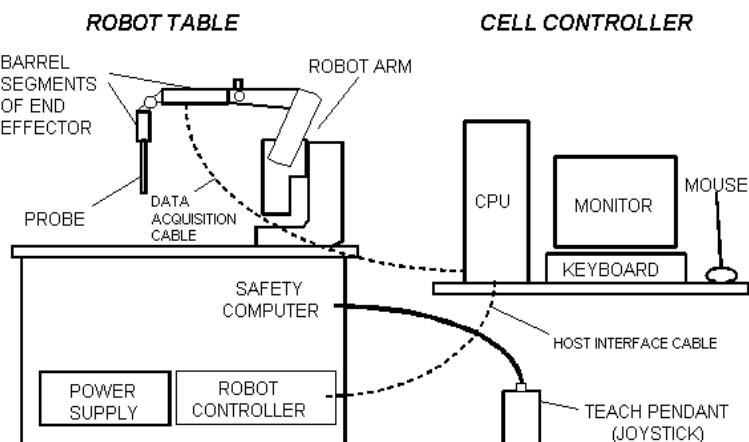

**Figure 2.1**  
**SAR Measurement System Setup**

When the Robot is in the home position, the Y-axis of the coordinate system parallels the line of intersection between the tabletop and the long axis of the Robot's Large Shoulder. The Teach Pendant may be used to establish the X,Y coordinate directions by depressing the 0-X and 0-Y MOTOR/AXIS switches while in axis mode.

The robot is first taught to position the probe sensor following a specific pattern of points. In the first sweep the sensor enclosure touches the inside of the phantom head. The SAR is measured on a defined grid of points that are concentrated on the surface of the head closest to the antenna of the transmitting device (EUT).

PCTEST™ SAR TEST REPORT	SAR MEASUREMENT REPORT			Simbex	Reviewed by: Quality Manager
Filename: SAR.0501210032.SUN	Test Dates: Jan. 28 - Feb. 4, 2005	EUT Type: Head Impact Encoder	FCC ID: SUN-0226000		Page 4 of 21

### 3. ALIDX-500 E-FIELD PROBE SYSTEM

#### Probe Measurement System




**Fig 3.1**  
IDX System


The near-field probe is an implantable isotropic E-field probe that measures the voltages proportional to the  $|E|^2$  (electric) or  $|H|^2$  (magnetic) fields. The probe is enclosed in a hollow glass protective cylinder 9-mm. outer diameter, 0.5 mm. thickness and 30 cm. in length. The E-probe contains three electrically small array of orthogonal dipoles strategically placed to provide greater accuracy and to compensate for near-field spatial gradients. The probe contains diodes that are placed over the gap of the dipoles to improve RF detection. The electrical signal detected by each diode is amplified by three DC amplifiers and are contained in a shielded container in the robot end effector so its performance is not affected by the presence of incident electromagnetic fields (see Fig. 3.1).

#### Probe Specifications

Frequency Range:	10 kHz – 6.0 GHz
Calibration:	In air from 10 MHz to 6.0 GHz
	In brain and muscle simulating tissue at Frequencies from 835 up to 2100MHz
Sensitivity:	3.5 mV/mW/cm <sup>2</sup> (air – typical)
DC Resistance:	300 kohm
Isotropic Response:	0.25 dB
Dynamic Range:	10 mW/kg – 100 W/kg
Resistance to Pull:	25 N
Probe Length:	290 mm
Probe Tip Material:	Ertalyte
Probe Tip Length:	60 mm
Probe Tip Diameter:	5 ± 0.2 mm
Application:	SAR Dosimetry Testing HAC (Hearing Aid Compatibility) Compliance tests of mobile phones



**Figure 3.2**  
Triangular Probe Configuration

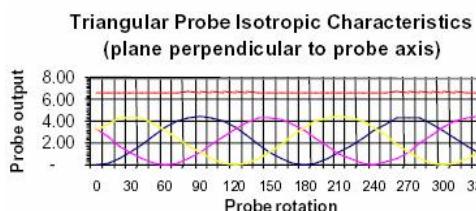

**Figure 3.3**  
Probe Characteristics

PCTEST™ SAR TEST REPORT	SAR MEASUREMENT REPORT			Simbex	Reviewed by: Quality Manager
Filename: SAR.0501210032.SUN	Test Dates: Jan. 28 - Feb. 4, 2005	EUT Type:	Head Impact Encoder	FCC ID: SUN-0226000	Page 5 of 21

## 4. PROBE CALIBRATION PROCESS

### Dosimetric Assessment Procedure

Each E-Probe/Probe amplifier combination has unique calibration parameters. A TEM calibration procedure is conducted to determine the proper amplifier settings to enter in the probe parameters. The amplifier settings are determined for a given frequency by subjecting the Probe to a known E-field density ( $1\text{mW/cm}^2$ ) using an RF Signal generator, TEM cell, and RF Power Meter. The SAR measurement software is used for Probe calibration.

### Free Space Assessment

The free space E-field from amplified probe outputs is determined in a test chamber. This calibration can be performed in a TEM cell if the frequency is below 1 GHz and in a waveguide or some other methodologies above 1 GHz for free space. For the free space calibration, we place the probe in the volumetric center of the cavity and at the proper orientation with the field. We then rotate the probe 360 degrees until the three channels show the maximum reading. The power density readings equates to  $1\text{mW/cm}^2$ .

### Temperature Assessment

E-field temperature correlation calibration is performed in a flat phantom filled with the appropriate simulated brain tissue. The measured free space E-field in the medium correlates to temperature rise in a dielectric medium. For temperature correlation calibration a RF transparent thermistor-based temperature probe is used in conjunction with the E-field probe.

$$\text{SAR} = C \frac{\Delta T}{\Delta t}$$

where:

$\Delta t$  = exposure time (30 seconds),

$C$  = heat capacity of tissue (brain or muscle),

$\Delta T$  = temperature in MX ENCODERase due to RF exposure.

$$\text{SAR} = \frac{|\mathbf{E}|^2 \cdot \sigma}{\rho}$$

where:

$\sigma$  = simulated tissue conductivity,

$\rho$  = Tissue density ( $1.25\text{ g/cm}^3$  for brain tissue)

SAR is proportional to  $\Delta T / \Delta t$ , the initial rate of tissue heating, before thermal diffusion takes place. Now it's possible to quantify the electric field in the simulated tissue by equating the thermally derived SAR to the E-field;

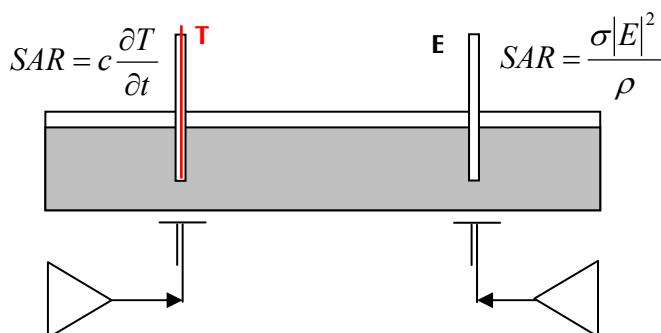


Figure 4.1 Temperature Assessment Test Configuration

PCTEST™ SAR TEST REPORT	SAR MEASUREMENT REPORT			Sumbex	Reviewed by: Quality Manager
Filename: SAR.0501210032.SUN	Test Dates: Jan. 28 - Feb. 4, 2005	EUT Type: Head Impact Encoder	FCC ID: SUN-0226000		Page 6 of 21

## 5. PHANTOM & EQUIVALENT TISSUES




**Figure 5.1**  
SAM Phantoms

The Left and Right SAM Phantoms are constructed of a vivac composite integrated in a corian stand. The shape of the shell is based on data from an anatomical study designed to determine the maximum exposure in at least 90% of all users [7][8]. It enables the dosimetric evaluation of left and right hand phone usage as well as body mounted usage at the flat phantom region. A cover prevents the evaporation of the liquid. Reference markings on the Phantom allow the complete setup of all predefined phantom positions and measurement grids by manually teaching three points in the robot. (see Fig. 5.1)



**Figure 5.2**  
Head Simulated  
Tissue



**Figure 5.3**  
Body/Muscle  
Simulated Tissue

### Brain & Muscle Simulating Mixture Characterization

The brain and muscle mixtures consist of a viscous gel using hydroxyethylcellulose (HEC) gelling agent and saline solution (see Table 6.1). Preservation with a bactericide is added and visual inspection is made to make sure air bubbles are not trapped during the mixing process. The mixture is calibrated to obtain proper dielectric constant (permittivity) and conductivity of the desired tissue. The head tissue dielectric parameters recommended by the IEEE SCC-34/SC-2 have been incorporated in the following table. Other head and body tissue parameters that have not been specified in 1528 are derived from the issue dielectric parameters computed from the 4-Cole-Cole equations. The mixture characterizations used for the brain and muscle tissue simulating liquids are according to the data by C. Gabriel and G. Hartsgrove [9].(see Table 5.1)

(% by weight)	Frequency (MHz)									
	450		835		915		1900		2450	
Tissue Type	Head	Body	Head	Body	Head	Body	Head	Body	Head	Body
Water	38.56	51.16	41.45	52.4	41.05	56.0	54.9	40.4	58.55	73.2
Salt (NAC1)	3.95	1.49	1.45	1.4	1.35	0.76	0.18	0.5	0.11	0.4
Sugar	56.32	46.78	56.0	45.0	56.0	41.76	0.0	58.0	0.0	0.0
HEC	0.98	0.52	1.0	1.0	1.0	1.21	0.0	1.0	0.0	0.0
Bacteride	0.19	0.05	0.1	0.1	0.27	0.0	0.1	0.0	0.0	0.0
Triton X-100	0.0	0.0	0.0	0.0	0.0	0.0	0.0	0.0	35.38	0.0
DGBE	0.0	0.0	0.0	0.0	0.0	0.0	44.92	0.0	6.96	26.7

**Table 5.1**  
Composition of the Brain & Muscle Tissue Equivalent Matter



**Figure 5.4**  
Device Positioner

### Device Holder

In combination with the SAM Phantom, the EUT Holder (see Fig. 5.4) enables the rotation of the mounted transmitter in spherical coordinates whereby the rotation point is the ear opening. Device positioning is accurate and repeatable according to the FCC and CENELEC specifications. The device holder can be locked at different phantom locations (left head, right head, flat phantom).

\* Note: A simulating human hand is not used due to the complex anatomical and geometrical structure of the hand that may produce infinite number of configurations [8]. To produce the worst-case condition (the hand absorbs antenna output power), the hand is omitted during the tests.

PCTEST™ SAR TEST REPORT	SAR MEASUREMENT REPORT			Sumbex	Reviewed by: Quality Manager
Filename: SAR.0501210032.SUN	Test Dates: Jan. 28 - Feb. 4, 2005	EUT Type: Head Impact Encoder	FCC ID: SUN-0226000		Page 7 of 21

## 6. TEST SYSTEM SPECIFICATIONS

### Automated Test System Specifications

#### Positioner

**Robot:** CRS Robotics, Inc. Robot Model: F3  
**Repeatability:**  $\pm 0.05$  mm (0.002 in.)  
**No. Of axes:** 6



#### Data Acquisition Electronic (DAE) System

##### Cell Controller

**Processor:** Pentium 4  
**Clock Speed:** 1.6 GHz  
**Operating System:** Windows 2000™ Professional  
**Data Card:** NI DAQ Card (in CPU)

##### Data Converter

**Software:** IDX Flexware  
**Connecting Lines:** Data Acquisition Cable  
 RS-232 Host Interface Cable  
**Sampling Rate:** 6000 samples/sec

**Figure 6.1**  
**ALIDX-500 Test System**

#### E-Field Probes

**Model:** E-020 S/N: PCT005  
**Construction:** Triangular core absolute encoder system  
**Frequency:** 10 MHz to 6.0 GHz

#### Phantom

**Phantom:** Planar Phantom  
**Shell Material:** Vivac Composite  
**Thickness:**  $2.0 \pm 0.2$  mm

PCTEST™ SAR TEST REPORT	SAR MEASUREMENT REPORT		Sumbex	Reviewed by: Quality Manager
Filename: SAR.0501210032.SUN	Test Dates: Jan. 28 - Feb. 4, 2005	EUT Type: Head Impact Encoder	FCC ID: SUN-0226000	Page 8 of 21

## 7. TEST CONFIGURATION POSITION

### Head-Worn Configurations

Head-Worn operating configurations are tested with the unit positioned against a head phantom in a user configuration (see Figure 7.1). Head dielectric parameters are used.

In all cases, the transmitting antenna is placed against the phantom to ensure worst-case positioning. This is documented and used to perform Head SAR testing.

This configuration represents a worst-case scenario when a player comes in contact with the antenna.



**Figure 7.1 Body-Worn Configuration**

PCTEST™ SAR TEST REPORT		SAR MEASUREMENT REPORT		Sumbex	Reviewed by: Quality Manager
Filename: SAR.0501210032.SUN		Test Dates: Jan. 28 - Feb. 4, 2005	EUT Type: Head Impact Encoder	FCC ID: SUN-0226000	Page 9 of 21

## 8. ANSI/IEEE C95.1 - 1992 RF EXPOSURE LIMITS

### Uncontrolled Environment

UNCONTROLLED ENVIRONMENTS are defined as locations where there is the exposure of individuals who have no knowledge or control of their exposure. The general population/uncontrolled exposure limits are applicable to situations in which the general public may be exposed or in which persons who are exposed as a consequence of their employment may not be made fully aware of the potential for exposure or cannot exercise control over their exposure. Members of the general public would come under this category when exposure is not employment-related; for example, in the case of a wireless transmitter that exposes persons in its vicinity.

### Controlled Environment

CONTROLLED ENVIRONMENTS are defined as locations where there is exposure that may be incurred by persons who are aware of the potential for exposure, (i.e. as a result of employment or occupation). In general, occupational/controlled exposure limits are applicable to situations in which persons are exposed as a consequence of their employment, who have been made fully aware of the potential for exposure and can exercise control over their exposure. This exposure category is also applicable when the exposure is of a transient nature due to incidental passage through a location where the exposure levels may be higher than the general population/uncontrolled limits, but the exposed person is fully aware of the potential for exposure and can exercise control over his or her exposure by leaving the area or by some other appropriate means.

**Table 10.1. Safety Limits for Partial Body Exposure [2]**

HUMAN EXPOSURE LIMITS		
	UNCONTROLLED ENVIRONMENT General Population (W/kg) or (mW/g)	CONTROLLED ENVIRONMENT General Population (W/kg) or (mW/g)
SPATIAL PEAK SAR 1 Brain	1.60	8.00
SPATIAL AVERAGE SAR 2 Whole Body	0.08	0.40
SPATIAL PEAK SAR 3 Hands, Feet, Ankles, Wrists	4.00	20.00

1 The Spatial Peak value of the SAR averaged over any 1 gram of tissue (defined as a tissue volume in the shape of a cube) and over the appropriate averaging time.

2 The Spatial Average value of the SAR averaged over the whole body.

3 The Spatial Peak value of the SAR averaged over any 10 grams of tissue (defined as a tissue volume in the shape of a cube) and over the appropriate averaging time.

PCTEST™ SAR TEST REPORT	 PCTEST Complete Wireless Lab™	SAR MEASUREMENT REPORT	 Sumbex	Reviewed by: Quality Manager
Filename: SAR.0501210032.SUN	Test Dates: Jan. 28 - Feb. 4, 2005	EUT Type: Head Impact Encoder	FCC ID: SUN-0226000	Page 10 of 21

## 9. MEASUREMENT UNCERTAINTIES

a	b	c	d	e = f(d,k)	f	g	h = cxg/e	i = cxg/e	k
Uncertainty Component	Sec.	Tol. (± %)	Prob. Dist.	Div.	c <sub>i</sub> (1 - g)	c <sub>i</sub> (10 - g)	1 - g u <sub>i</sub> (± %)	10 - g u <sub>i</sub> (± %)	v <sub>i</sub>
<b>Measurement System</b>									
Probe Calibration	E1.1	11.4	N	$\sqrt{3}$	1	1	6.6	6.6	$\infty$
Axial Isotropy	E1.2	3.4	R	$\sqrt{3}$	0.7	0.7	1.4	1.4	$\infty$
Hemispherical Isotropy	E1.2	5.2	R	$\sqrt{3}$	1	1	3.0	3.0	$\infty$
Boundary Effect	E1.3	4.7	R	$\sqrt{3}$	1	1	2.7	2.7	$\infty$
Linearity	E1.4	5.9	R	$\sqrt{3}$	1	1	3.4	3.4	$\infty$
System Detection Limits	E1.5	1.0	R	$\sqrt{3}$	1	1	0.6	0.6	$\infty$
Readout Electronics	E1.6	1.0	R	1	1	1	1.0	1.0	$\infty$
Response Time	E1.7	0.8	R	$\sqrt{3}$	1	1	0.5	0.5	$\infty$
Integration Time	E1.8	1.7	R	$\sqrt{3}$	1	1	1.0	1.0	$\infty$
RF Ambient Conditions	E5.1	1.2	R	$\sqrt{3}$	1	1	0.7	0.7	$\infty$
Probe Positioner Mechanical Tolerance	E5.2	0.4	R	$\sqrt{3}$	1	1	0.2	0.2	$\infty$
Probe Positioning w/ respect to Phantom Shell	E5.3	2.9	R	$\sqrt{3}$	1	1	1.7	1.7	$\infty$
Extrapolation, Interpolation & Integration Algorithms for Max. SAR Evaluation	E4.2	3.9	R	$\sqrt{3}$	1	1	2.3	2.3	$\infty$
<b>Test Sample Related</b>									
Test Sample Positioning	E3.2.1	10.6	R	$\sqrt{3}$	1	1	6.1	6.1	11
Device Holder Uncertainty	E3.1.1	8.7	R	$\sqrt{3}$	1	1	5.0	5.0	8
Output Power Variation - SAR drift measurement	5.6.2	5.0	R	$\sqrt{3}$	1	1	2.9	2.9	$\infty$
<b>Phantom &amp; Tissue Parameters</b>									
Phantom Uncertainty (Shape & Thickness tolerances)	E2.1	4.0	R	$\sqrt{3}$	1	1	2.3	2.3	$\infty$
Liquid Conductivity - deviation from target values	E2.2	5.0	R	$\sqrt{3}$	0.7	0.5	2.0	1.4	$\infty$
Liquid Conductivity - measurement uncertainty	E2.2	5.0	R	$\sqrt{3}$	0.7	0.5	2.0	1.4	$\infty$
Liquid Permittivity - deviation from target values	E2.2	5.0	R	$\sqrt{3}$	0.6	0.5	1.7	1.4	$\infty$
Liquid Permittivity - measurement uncertainty	E2.2	5.0	R	$\sqrt{3}$	0.6	0.5	1.7	1.4	$\infty$
<b>Combined Standard Uncertainty (k=1)</b>									
<b>Expanded Uncertainty (k=2)</b> (95% CONFIDENCE LEVEL)									
			RSS				13.2	13.0	
							26.6	26.2	

The above measurement uncertainties are according to IEEE Std. 1528-2003

PCTEST™ SAR TEST REPORT	 SAR MEASUREMENT REPORT		Reviewed by: Quality Manager
Filename: SAR.0501210032.SUN	Test Dates: Jan. 28 - Feb. 4, 2005	EUT Type: Head Impact Encoder	FCC ID: SUN-0226000

## 10. SYSTEM VERIFICATION

### Tissue Verification

Table 10.1 Simulated Tissue Verification

MEASURED TISSUE PARAMETERS					
Date(s)	1/28/05	835MHz Brain		915MHz Muscle	
Liquid Temperature (°C)	21.6	Target	Measured	Target	Measured
Dielectric Constant: $\epsilon$	41.50		40.81	55.00	N/A
Conductivity: $\sigma$	0.90		0.87	1.06	N/A

### Test System Verification

Prior to assessment, the system is verified to the  $\pm 10\%$  of the specifications at 835 MHz by using the system validation kits. (Graphic Plots Attached)

Table 10.2 System Verification

System Validation TARGET & MEASURED							
Date:	Amb. Temp (°C)	Liquid Temp (°C)	Input Power (W)	Tissue	Targeted SAR <sub>1g</sub> (mW/g)	Measured SAR <sub>1g</sub> (mW/g)	Deviation (%)
1/28/05	21.6	21.1	0.160	835MHz Brain	1.5	1.48	- 2.6 %

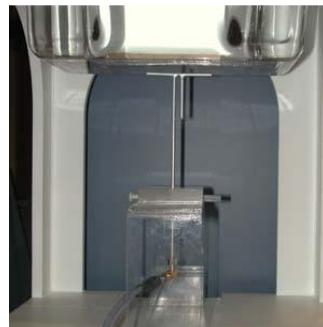


Figure 10.1 Dipole Validation Test Setup

PCTEST™ SAR TEST REPORT	SAR MEASUREMENT REPORT	Sumbex	Reviewed by: Quality Manager
Filename: SAR.0501210032.SUN	Test Dates: Jan. 28 - Feb. 4, 2005	EUT Type: Head Impact Encoder	FCC ID: SUN-0226000

## 11. SAR TEST DATA SUMMARY

### See Measurement Result Data Pages

#### Procedures Used To Establish Test Signal

The DUT was placed into continuous transmit mode set by the manufacturer, to maintain maximum output power. Such test signals offer a consistent means for testing SAR and are recommended for evaluating SAR [4].

#### Device Test Conditions

The DUT is powered through the battery. If a power deviation of more than 5% occurred, the test was repeated.

PCTEST™ SAR TEST REPORT		SAR MEASUREMENT REPORT		Symbex	Reviewed by: Quality Manager
Filename: SAR.0501210032.SUN		Test Dates: Jan. 28 - Feb. 4, 2005	EUT Type: Head Impact Encoder	FCC ID: SUN-0226000	Page 13 of 21

## 12. SAR DATA SUMMARY

Mixture Type: 915MHz Brain

12.1 MEASUREMENT RESULTS (Left Head SAR)							
FREQUENCY		Modulation	POWER (dBm)	Battery	Separation Distance (cm) **	Antenna	SAR (W/kg)
MHz	Ch.						
902.24	LOW	FHSS	22.37	Standard	TOUCH	Internal	0.65
914.95	MID	FHSS	22.37	Standard	TOUCH	Internal	1.27
927.82	HIGH	FHSS	22.37	Standard	TOUCH	Internal	0.90
ANSI / IEEE C95.1 1992 - SAFETY LIMIT Spatial Peak Uncontrolled Exposure/General Population				Brain 1.6 W/kg (mW/g) averaged over 1 gram			

**NOTES:**

1. The test data reported is the worst-case SAR value with the DUT set in a typical configuration. Test procedures used are according to FCC/OET Bulletin 65, Supp.C [July 2001].
2. All modes of operation were investigated, and worst-case results are reported.
3. <sup>\*</sup>Power Measured  Conducted  ERP  EIRP
4. SAR Measurement System  DASY3  IDX
5. SAR Configuration  Left Head  Flat Phantom  Left Head
6. Test Signal Call Mode  Head  Body  Hand
7.  Software  Base Station Simulator
8. Tissue parameters and temperatures are listed on the SAR plots.
9. Liquid tissue depth is 15 cm.  $\pm 0.1$
10. Right head SAR was evaluated during pretest and found to be negligible. This is due to the fact that the antenna and RF components are all located on the left side of the head.


  
 Alfred Cirwitzian  
 Vice President Engineering


Figure 12.1  
Head SAR Setup

PCTEST™ SAR TEST REPORT	SAR MEASUREMENT REPORT			Sumbex	Reviewed by: Quality Manager
Filename: SAR.0501210032.SUN	Test Dates: Jan. 28 - Feb. 4, 2005	EUT Type: Head Impact Encoder	FCC ID: SUN-0226000		Page 14 of 21

## 13. SAR TEST EQUIPMENT

### Equipment Calibration

Table 13.1 Test Equipment Calibration

EQUIPMENT SPECIFICATIONS		
Type	Calibration Date	Serial Number
CRS Robot F3	February 2004	RAF0134133
CRS C500C Motion Controller	February 2004	RCB0003303
CRS Teach Pendant (Joystick)	February 2004	STP0132231
DELL Computer, Pentium 4 1.6 GHz, Windows 2000™	February 2004	4PJZ111
E-Field Probe E-020	January 2005	PCT005
Right Ear SAM Phantom (P-SAM-R)	February 2004	94X-113
Left Ear SAM Phantom (P-SAM-L)	February 2004	94X-019
Flat SAM Phantom (P-SAM-FLAT)	February 2004	94X-097
IDX Robot End Effector (EE-103-C)	February 2004	07111223
IDX Probe Amplifier	February 2004	07111113
Validation Dipole D-2450	October 2004	PCT642
Brain Equivalent Matter (835MHz)	November 2004	PCTBEM301
Muscle Equivalent Matter (915MHz)	November 2004	PCTMEM901
Microwave Amp. Model: 5S1G4, (800MHz - 4.2GHz)	January 2005	22332
Gigatronics 8651A Power Meter	January 2005	1835299
HP-8648D (9kHz ~ 4GHz) Signal Generator	January 2005	PCT530
Amplifier Research 5S1G4 Power Amp	January 2005	PCT540
HP-8753E (30kHz ~ 3GHz) Network Analyzer	January 2005	PCT552
HP85070B Dielectric Probe Kit	January 2005	PCT501
Ambient Noise/Reflection, etc.	January 2005	Anechoic Room PCT01

NOTE:

Dipole Validation measurement was performed by PCTEST Lab before each test. The brain simulating material is calibrated by PCTEST using the dielectric probe system and network analyzer to determine the conductivity and permittivity (dielectric constant) of the brain-equivalent material.

PCTEST™ SAR TEST REPORT	SAR MEASUREMENT REPORT			Simbex	Reviewed by: Quality Manager
Filename: SAR.0501210032.SUN	Test Dates: Jan. 28 - Feb. 4, 2005	EUT Type: Head Impact Encoder	FCC ID: SUN-0226000		Page 15 of 21

## 14. CONCLUSION

### Measurement Conclusion

The SAR measurement indicates that the EUT complies with the RF radiation exposure limits of the FCC. These measurements are taken to simulate the RF effects exposure under worst-case conditions. Precise laboratory measures were taken to assure repeatability of the tests. The tested device complies with the requirements in respect to all parameters subject to the test. The test results and statements relate only to the item(s) tested.

Please note that the absorption and distribution of electromagnetic energy in the body are very complex phenomena that depend on the mass, shape, and size of the body, the orientation of the body with respect to the field vectors, and the electrical properties of both the body and the environment. Other variables that may play a substantial role in possible biological effects are those that characterize the environment (e.g. ambient temperature, air velocity, relative humidity, and body insulation) and those that characterize the individual (e.g. age, gender, activity level, debilitation, or disease). Because innumerable factors may interact to determine the specific biological outcome of an exposure to electromagnetic fields, any protection guide shall consider maximal amplification of biological effects as a result of field-body interactions, environmental conditions, and physiological variables.[3]

PCTEST™ SAR TEST REPORT		SAR MEASUREMENT REPORT			Sumbex	Reviewed by: Quality Manager
Filename: SAR.0501210032.SUN		Test Dates: Jan. 28 - Feb. 4, 2005	EUT Type: Head Impact Encoder	FCC ID: SUN-0226000		Page 16 of 21

## 15. REFERENCES

- [1] Federal Communications Commission, ET Docket 93-62, Guidelines for Evaluating the Environmental Effects of Radiofrequency Radiation, Aug. 1996.
- [2] ANSI/IEEE C95.1 - 1991, *American National Standard safety levels with respect to human exposure to radio frequency electromagnetic fields, 300kHz to 100GHz*, New York: IEEE, Aug. 1992.
- [3] ANSI/IEEE C95.3 - 1991, *IEEE Recommended Practice for the Measurement of Potentially Hazardous Electromagnetic Fields - RF and Microwave*, New York: IEEE, 1992.
- [4] Federal Communications Commission, OET Bulletin 65 (Edition 97-01), Supplement C (Edition 01-01), *Evaluating Compliance with FCC Guidelines for Human Exposure to Radiofrequency Electromagnetic Fields*, July 2001.
- [5] IEEE Standards Coordinating Committee 34 – IEEE Std. 1528 (Aug. 2003), *Recommended Practice for Determining the Peak Spatial-Average Specific Absorption Rate (SAR) in the Human Body Due to Wireless Communications Devices: Measurement Techniques*.
- [6] NCRP, National Council on Radiation Protection and Measurements, *Biological Effects and Exposure Criteria for RadioFrequency Electromagnetic Fields*, NCRP Report No. 86, 1986. Reprinted Feb. 1995.
- [7] V. Hombach, K. Meier, M. Burkhardt, E. Kuhn, N. Kuster, *The Dependence of EM Energy Absorption upon Human Head Modeling at 900 MHz*, IEEE Transaction on Microwave Theory and Techniques, vol. 44 no. 10, Oct. 1996, pp. 1865-1873.
- [8] N. Kuster and Q. Balzano, *Energy absorption mechanism by biological bodies in the near field of dipole antennas above 300MHz*, IEEE Transaction on Vehicular Technology, vol. 41, no. 1, Feb. 1992, pp. 17-23.
- [9] G. Hartsgrove, A. Kraszewski, A. Surowiec, *Simulated Biological Materials for Electromagnetic Radiation Absorption Studies*, University of Ottawa, Bioelectromagnetics, Canada: 1987, pp. 29-36.
- [10] Q. Balzano, O. Garay, T. Manning Jr., *Electromagnetic Energy Exposure of Simulated Users of Portable Cellular Telephones*, IEEE Transactions on Vehicular Technology, vol. 44, no.3, Aug. 1995.
- [11] W.H. Press, S.A. Teukolsky, W.T. Vetterling, and B.P. Flannery, *Numerical Receipes in C*, The Art of Scientific Computing, Second edition, Cambridge University Press, 1992.
- [12] Federal Communications Commission, OET Bulletin 65, Evaluating Compliance with FCC Guidelines for Human Exposure to Radiofrequency Electromagnetic Fields. Supplement C, Dec. 1997.
- [13] CENELEC CLC/SC111B, European Prestandard (prENV 50166-2), Human Exposure to Electromagnetic Fields High-frequency: 10kHz-300GHz, Jan. 1995.

PCTEST™ SAR TEST REPORT	SAR MEASUREMENT REPORT			Simbex	Reviewed by: Quality Manager
<b>Filename:</b> SAR.0501210032.SUN	<b>Test Dates:</b> Jan. 28 - Feb. 4, 2005	<b>EUT Type:</b> Head Impact Encoder	<b>FCC ID:</b> SUN-0226000	Page 17 of 21	

## EXHIBIT A – SAR TEST DATA

PCTEST™ SAR TEST REPORT		SAR MEASUREMENT REPORT		Sumbex	Reviewed by: Quality Manager
Filename: SAR.0501210032.SUN		Test Dates: Jan. 28 - Feb. 4, 2005	EUT Type: Head Impact Encoder	FCC ID: SUN-0226000	Page 18 of 21

SAR Data Report 05012831

Start : 28-Jan-05 03:34:08 pm  
End : 28-Jan-05 03:40:51 pm  
Code Version : 4.08  
Robot Version: 4.08

Product Data:

Type : SIMBEX  
Model Number : MX ENCODER  
Serial Number : 121704-0067  
Frequency : 915 MHz  
Transmit Pwr : 0.173 W  
Antenna Posn. : Fixed

Measurement Data:

Phantom Name : SAM-LEFT  
Phantom Type : Left Ear  
Tissue Type : Brain  
Tissue Dielectric : 40.810  
Tissue Conductivity : 0.870  
Tissue Density : 1.000  
Robot Name : CRS

Probe Data:

Probe Name : PCT005  
Probe Type : E Fld Triangle  
Frequency : 835 MHz  
Tissue Type : Brain  
Calibrated Dielectric : 40.810  
Calibrated Conductivity : 0.870  
Calibrated Density : 1.000  
Probe Offset : 1.560 mm  
Conversion Factor : 5.500  
Probe Sensitivity : 3.807 3.736 3.821 mV/(mW/cm<sup>2</sup>)  
Amplifier Gains : 20.00 20.00 20.00

Sample:

Rate: 6000 Samples/Sec  
Count: 1000 Samples  
NIDAQ Gain: 5

Comments:

Head SAR

CF=1; Amb. Temp= 21.6 'C; Liq. Temp=21.1 'C

Power Drop Test:

Reading @ start = 0.066  
Reading @ End = 0.067  
Power at End = 101.4%


Area Scan - Max Peak SAR Value at x=-15.0 y=37.0 = 1.31 W/kg

Zoom Scan - Max Peak SAR Value at x=-15.0 y=36.0 z=0.0 = 1.92 W/kg


Max 1g SAR at x=-13.0 y=37.0 z=0.0 = 1.27 W/kg


Max 10g SAR at x=-10.0 y=38.0 z=0.0 = 0.81 W/kg

SAR - Z Axis  
at Hotspot x:-15.0 y:36.0

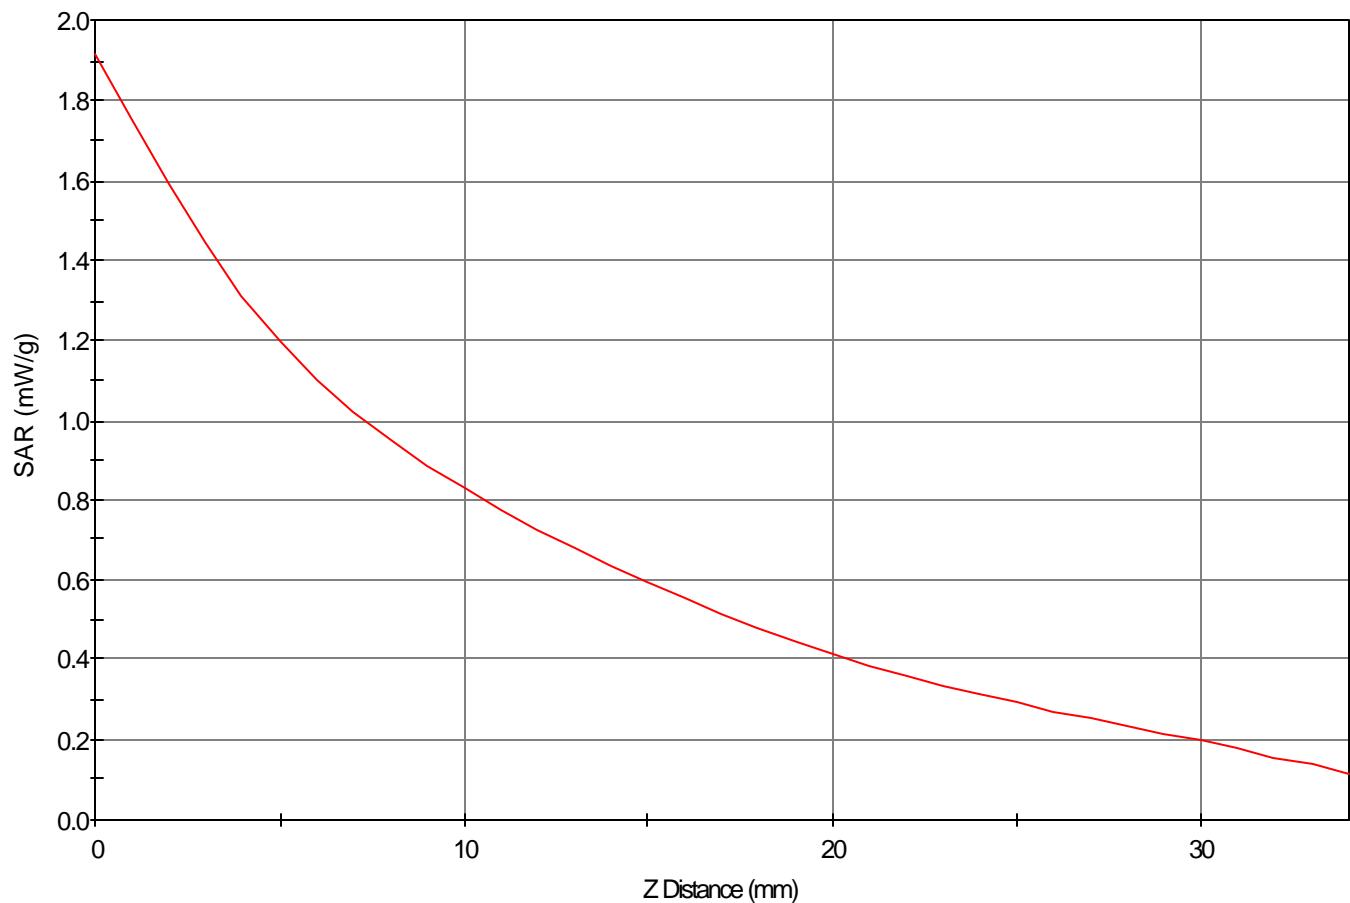

1g SAR Values

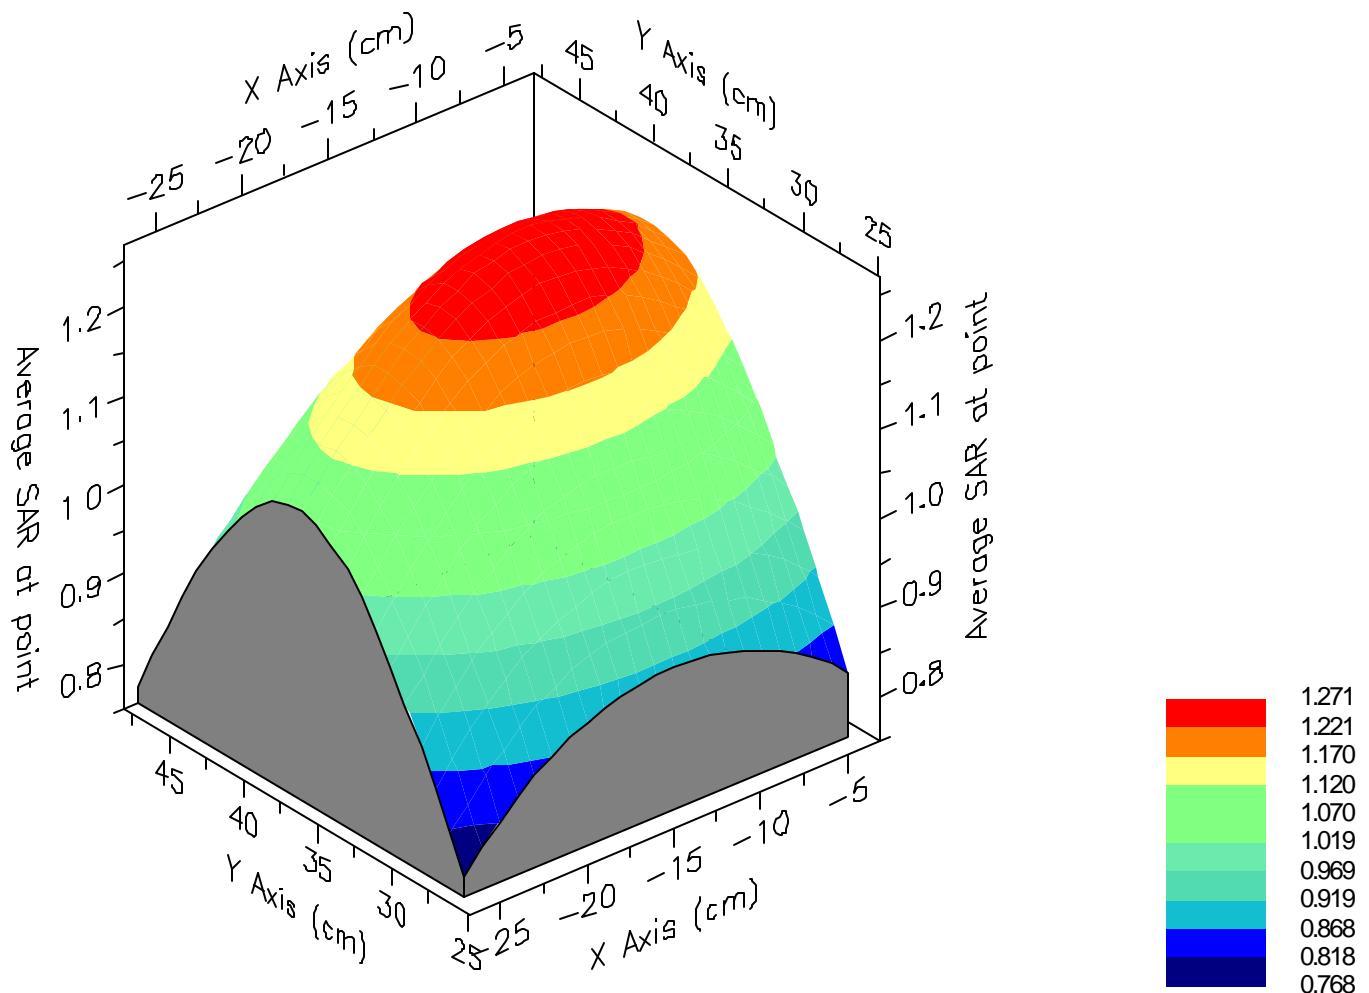

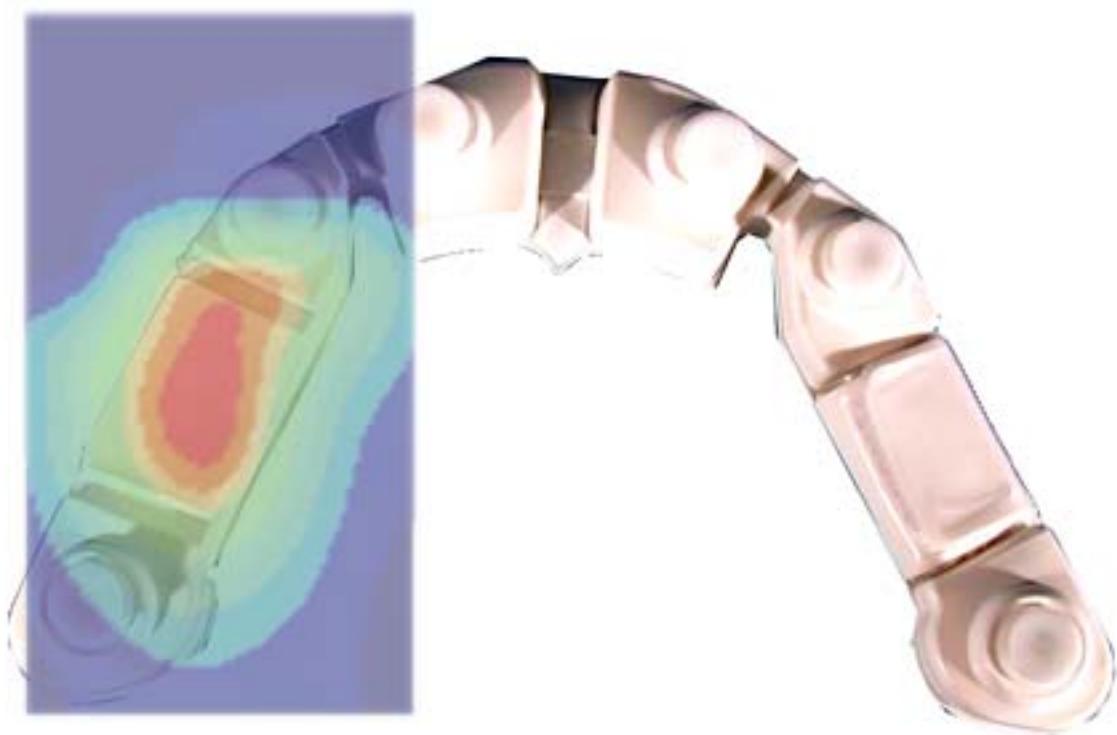

## EXHIBIT B – SAR TEST SETUP PHOTOGRAPHS


PCTEST™ SAR TEST REPORT		SAR MEASUREMENT REPORT			Reviewed by: Quality Manager
<b>Filename:</b> SAR.0501210032.SUN		<b>Test Dates:</b> Jan. 28 - Feb. 4, 2005	<b>EUT Type:</b> Head Impact Encoder	<b>FCC ID:</b> SUN-0226000	Page 19 of 21



 © 2005 PCTEST Lab.	SIMBEX FCC ID: SUN-0226000 Head Impact Encoder	EUT Photographs Model: MX ENCODER
---	---	--------------------------------------



 PCTEST <sup>®</sup> Dynamische Vibrations Lab <sup>®</sup>	SIMBEX FCC ID: SUN-0226000	EUT Photographs
© 2005 PCTEST Lab.	Head Impact Encoder	Model: MX ENCODER

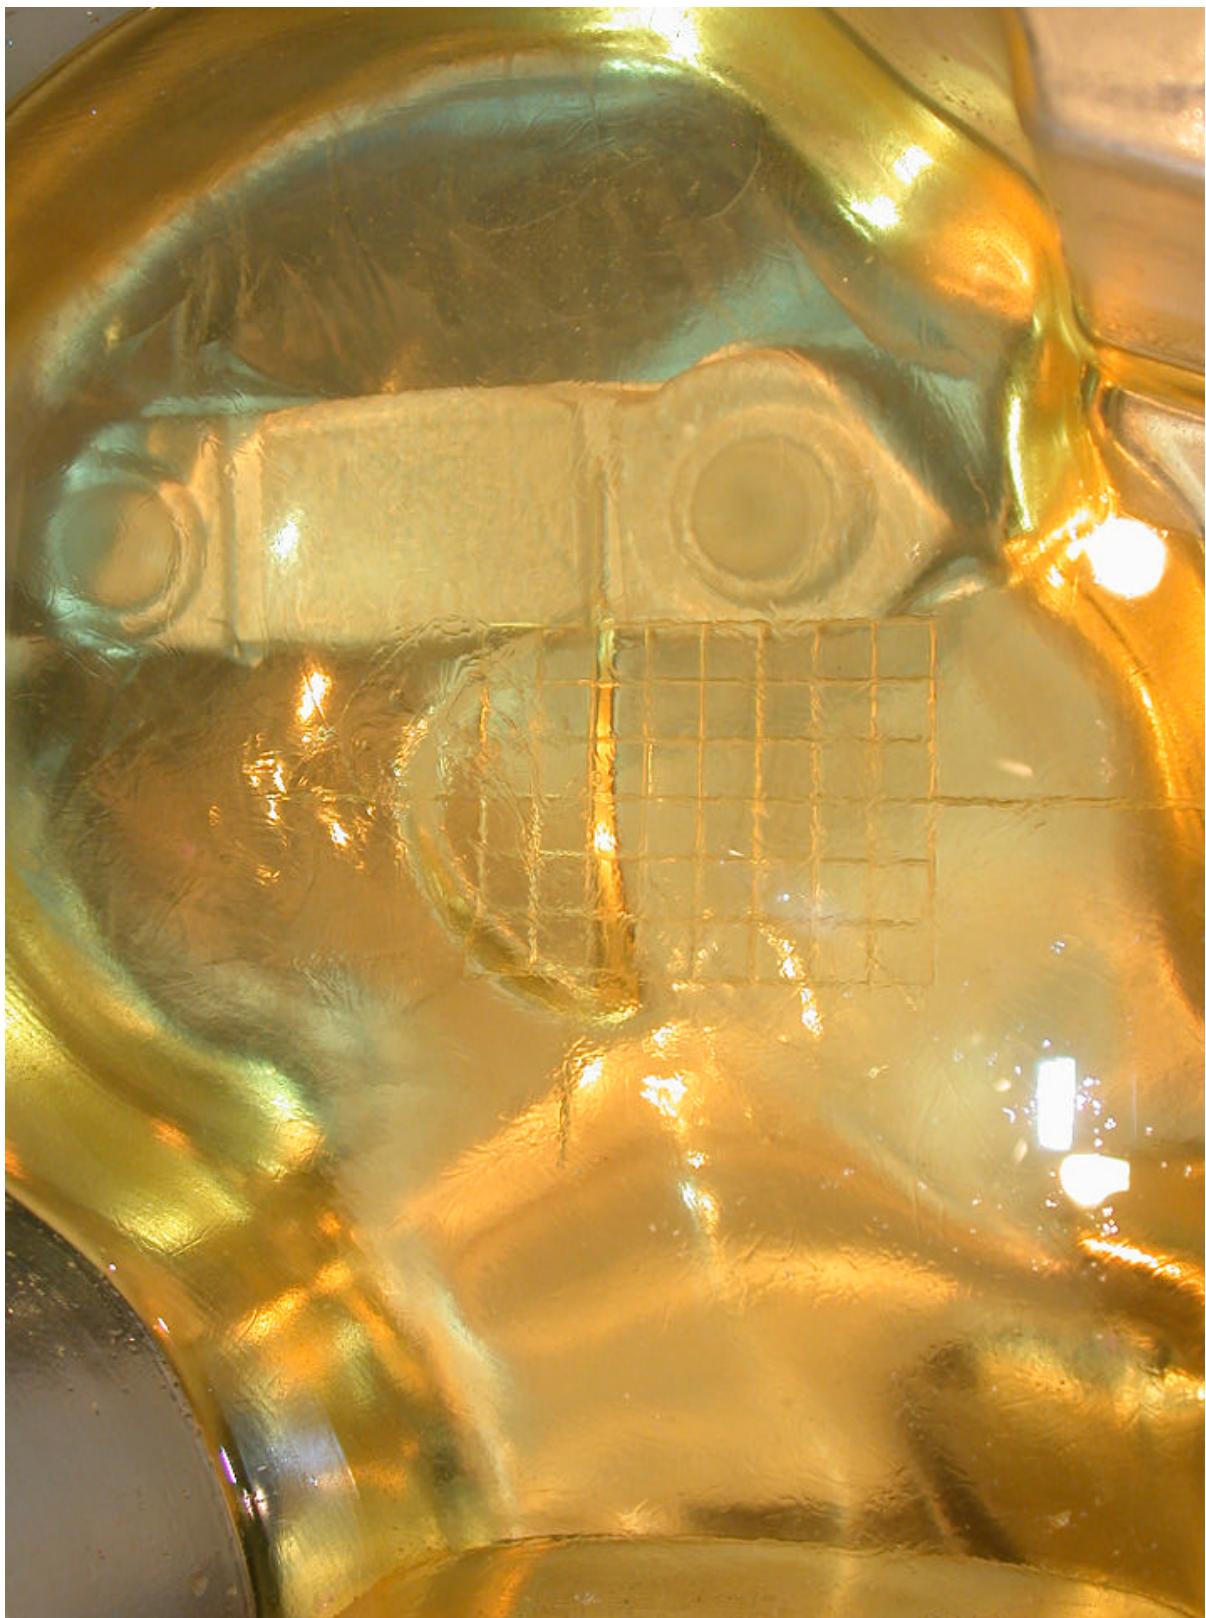

 PCTEST Polymerized Composite Test Systems	SIMBEX FCC ID: SUN-0226000	EUT Photographs
© 2005 PCTEST Lab.	Head Impact Encoder	Model: MX ENCODER

## EXHIBIT C – DIPOLE VALIDATION

PCTEST™ SAR TEST REPORT		SAR MEASUREMENT REPORT			Reviewed by: Quality Manager
<b>Filename:</b> SAR.0501210032.SUN		<b>Test Dates:</b> Jan. 28 - Feb. 4, 2005	<b>EUT Type:</b> Head Impact Encoder	<b>FCC ID:</b> SUN-0226000	Page 20 of 21

SAR Data Report 05012822

Start : 28-Jan-05 01:47:10 pm  
End : 28-Jan-05 01:54:27 pm  
Code Version : 4.08  
Robot Version: 4.08

Product Data:

Type : Verification  
Model Number : E-020  
Serial Number : PCT003  
Frequency : 835 MHz  
Transmit Pwr : 0.160 W  
Antenna Type : Dipole  
Antenna Posn. : Verification

Measurement Data:

Phantom Name : SAM-FLAT2  
Phantom Type : Uniphantom  
Tissue Type : Brain  
Tissue Dielectric : 40.810  
Tissue Conductivity : 0.870  
Tissue Density : 1.000  
Robot Name : CRS

Probe Data:

Probe Name : PCT005  
Probe Type : E Fld Triangle  
Frequency : 835 MHz  
Tissue Type : Brain  
Calibrated Dielectric : 40.810  
Calibrated Conductivity : 0.870  
Calibrated Density : 1.000  
Probe Offset : 1.600 mm  
Conversion Factor : 5.500  
Probe Sensitivity : 3.807 3.736 3.821 mV/(mW/cm^2)  
Amplifier Gains : 20.00 20.00 20.00

Sample:

Rate: 6000 Samples/Sec  
Count: 1000 Samples  
NIDAQ Gain: 5

Comments:

Verification

CF=1; Amb. Temp= 21.6 'C; Liq. Temp=21.1 'C

Power Drop Test:

Reading @ start = 2.078  
Reading @ End = 2.089  
Power at End = 100.5%

Area Scan - Max Peak SAR Value at x=-8.0 y=0.0 = 1.49 W/kg

Zoom Scan - Max Peak SAR Value at x=-8.0 y=0.0 z=0.0 = 2.22 W/kg


Max 1g SAR at x=-8.0 y=0.0 z=0.0 = 1.48 W/kg

Max 10g SAR at x=-7.0 y=0.0 z=0.0 = 0.95 W/kg


Validation Results at 0.16 W:


Peak Nominal = 2.3, Error: -1.78 %  
1g Nominal = 1.5, Error: -2.78 %

SAR - Z Axis  
at Hotspot x:-8.0 y:0.0

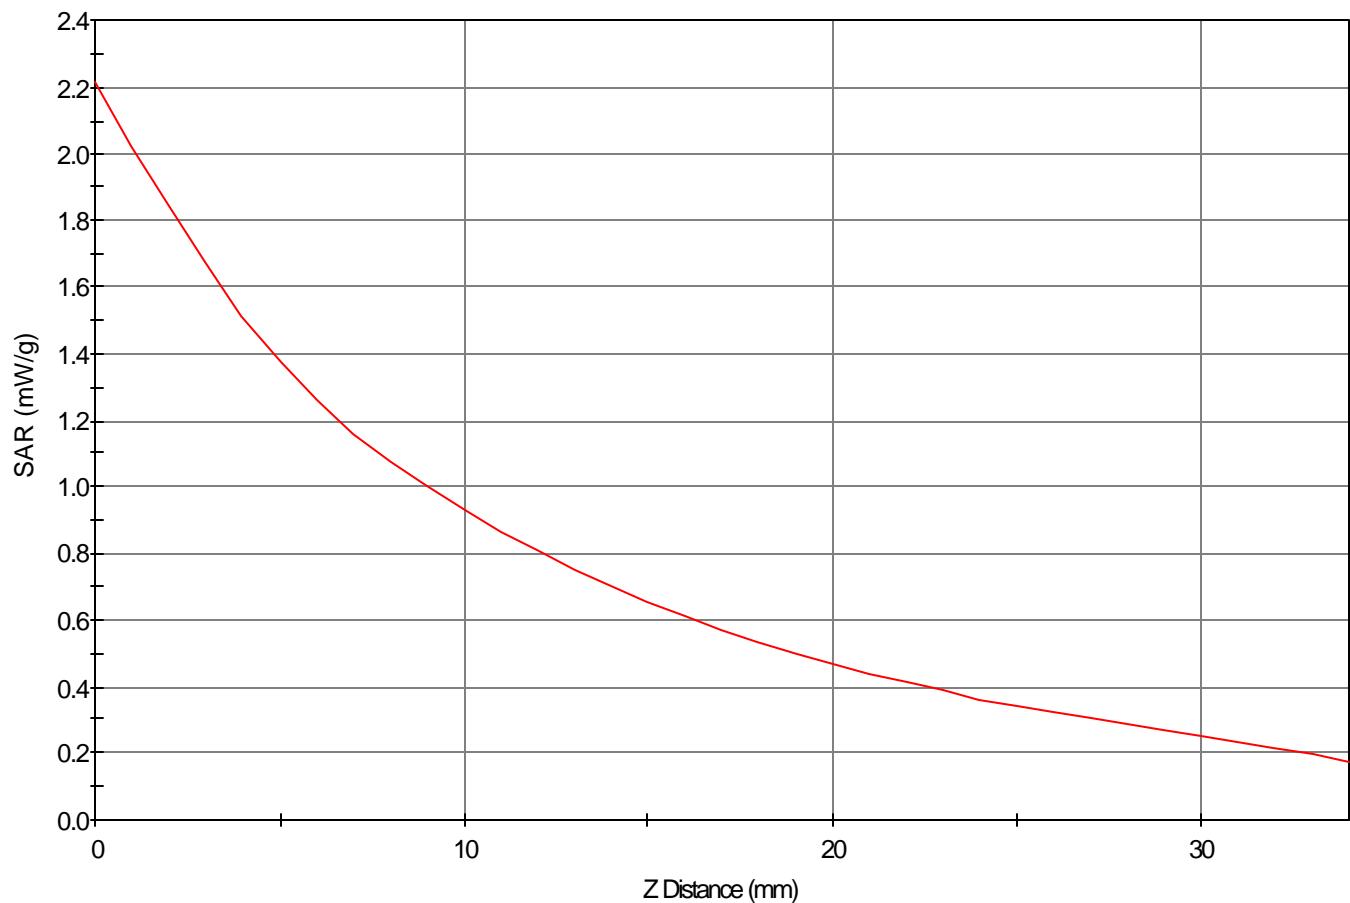

1g SAR Values

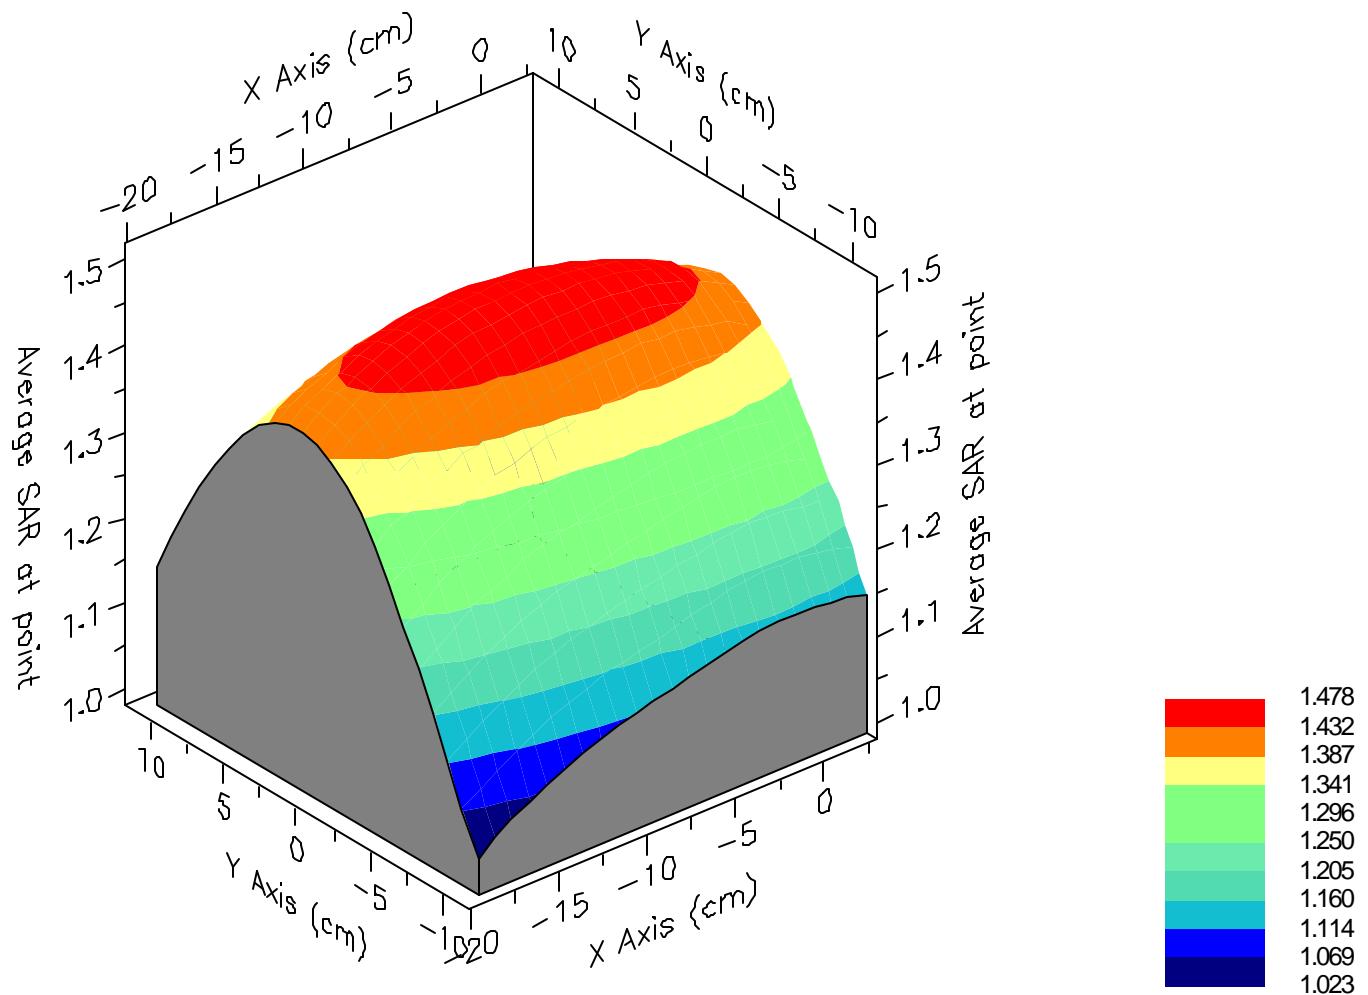

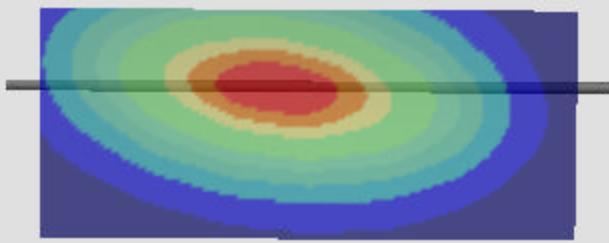

## EXHIBIT D – PROBE CALIBRATION

PCTEST™ SAR TEST REPORT		SAR MEASUREMENT REPORT		Sumbex	Reviewed by: Quality Manager
Filename: SAR.0501210032.SUN		Test Dates: Jan. 28 - Feb. 4, 2005	EUT Type: Head Impact Encoder	FCC ID: SUN-0226000	Page 21 of 21

# Probe E-020

**SN: PCT005**

Manufactured:

November 10, 2004


Calibrated:

January 17, 2005

Calibrated for the IDX System

PCTEST Calibration Laboratory

Approved By:



---

**Alfred Cirwitzian**  
**Vice President Engineering**

Calibration is performed according to IEEE Std. 1528 - 2003  
and all test equipment used is traceable to U.S. NIST.

## Calibration Summary

Model: E-020

S/N: PCT005

Tissue Type	Frequency (MHz)	Dielectric Constant $\epsilon_r$	Conductivity (S/m) $\sigma$	Conversion Factor $\gamma_x, \gamma_y, \gamma_z$
Brain	450	44.41	0.88	8.8
Brain	835	40.81	0.87	5.5
Brain	1900	39.02	1.37	5.4
Brain	2100	41.11	1.39	5.25
Muscle	450	57.70	0.96	9.24
Muscle	835	53.66	0.98	5.85
Muscle	1900	51.81	1.58	5.5
Muscle	2100	52.23	1.53	5.3

Frequency (MHz)	Isotropy	
	%	dB
450	1.23	0.05
835	2.12	0.09
1900	6.61	0.28
2100	7.61	0.32

**Boundary Effect** < 2%, 2.5 mm from probe tip to phantom

**Diode Compression Point:** 120 mV



**Environmental Conditions:**



Temperature: 22.6 °C


Relative Humidity: 41%

Barometer: 101.2 kPa

-----  
 This probe was calibrated under the IEEE Std 1309-1966, *IEEE Standard for Calibration of Electromagnetic Field Sensors and Probes, Excluding Antennas, from 9 kHz to 40 GHz*.

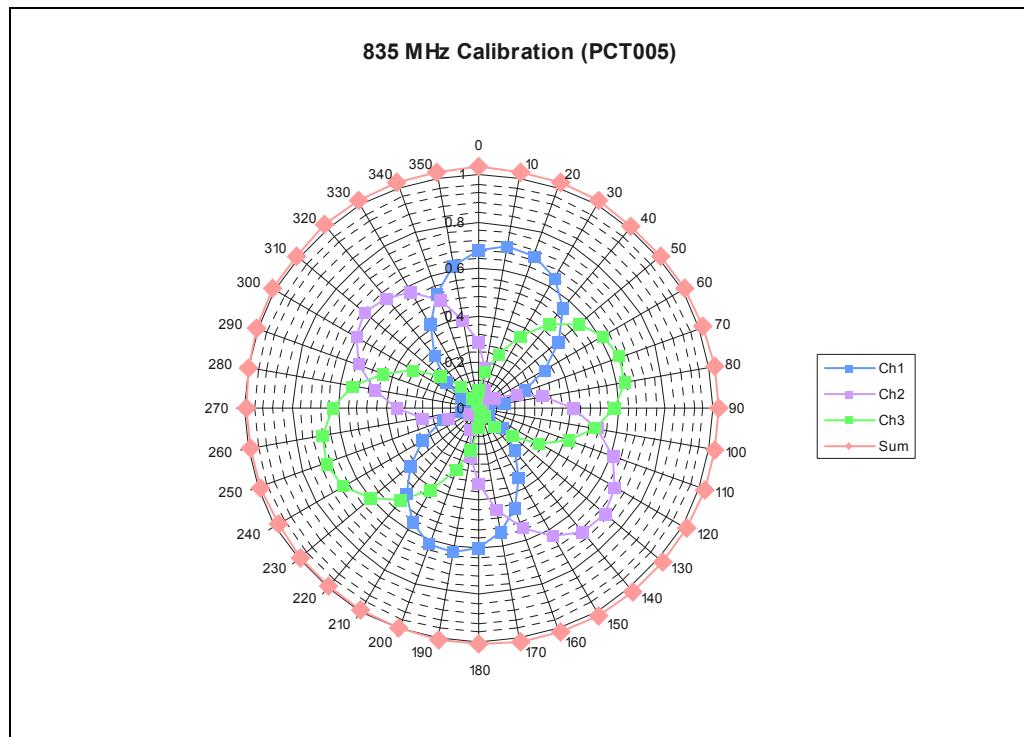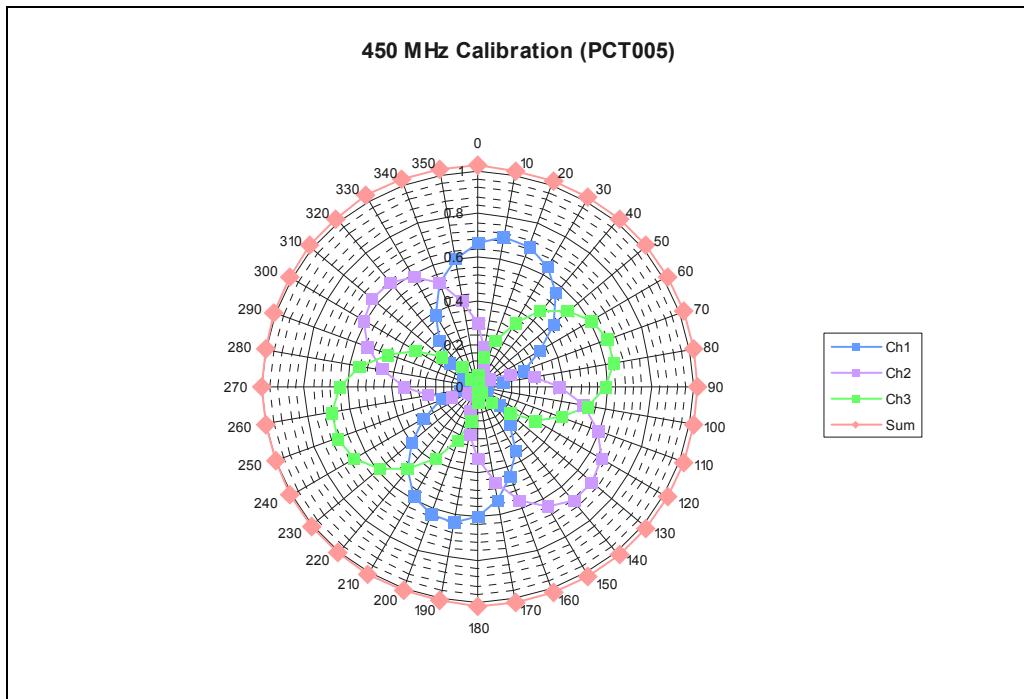


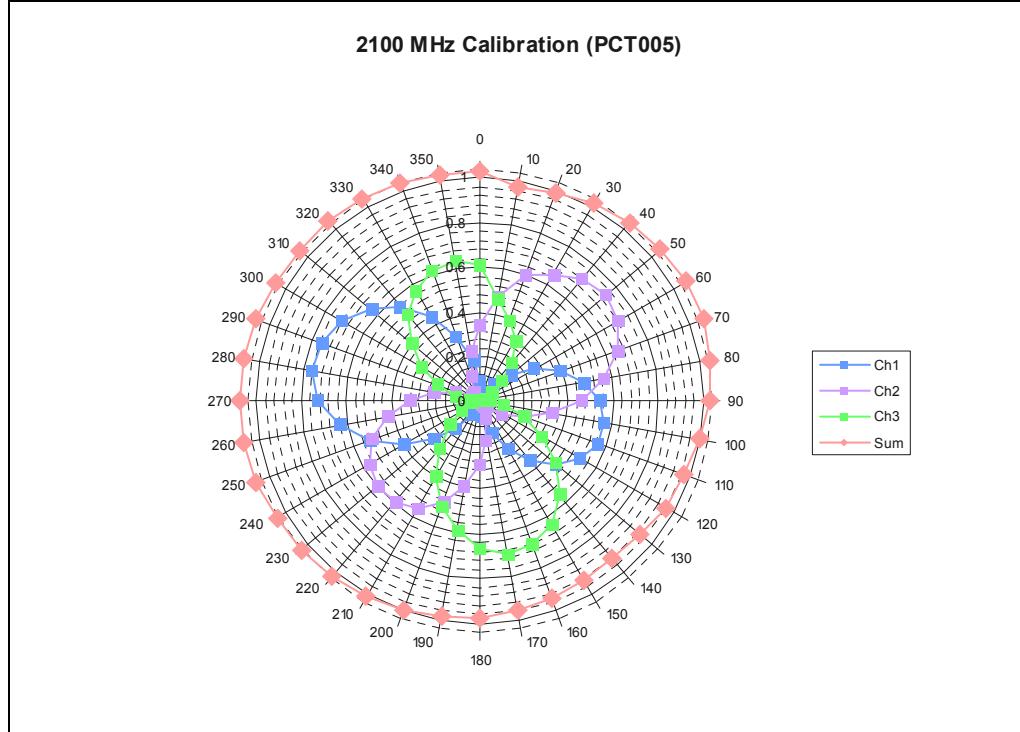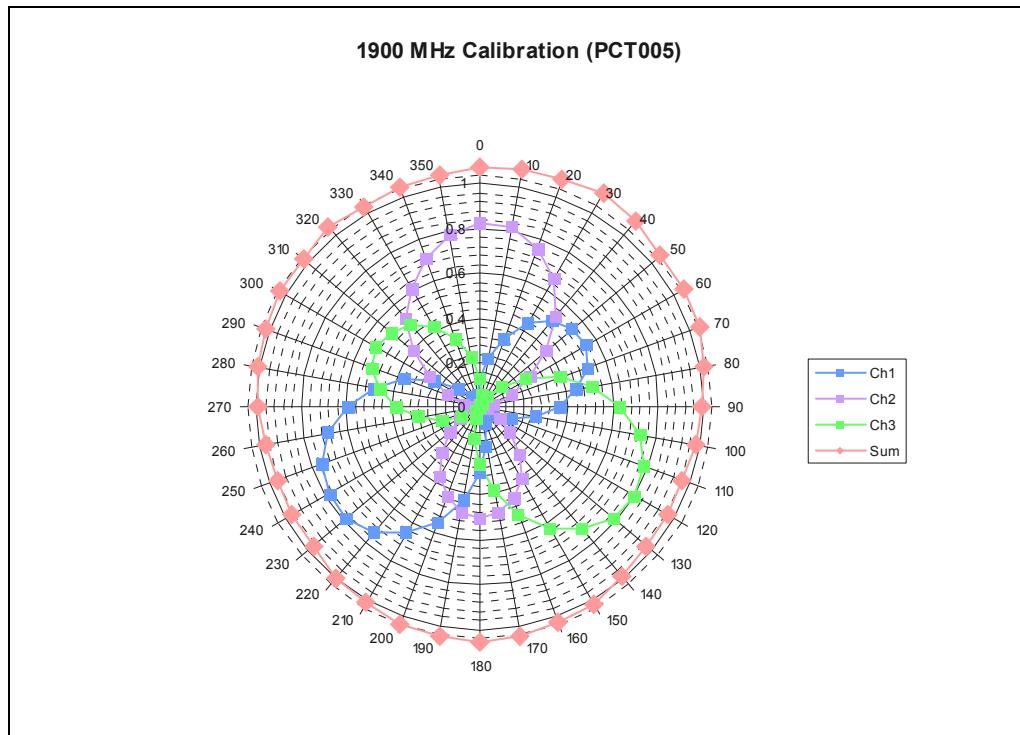

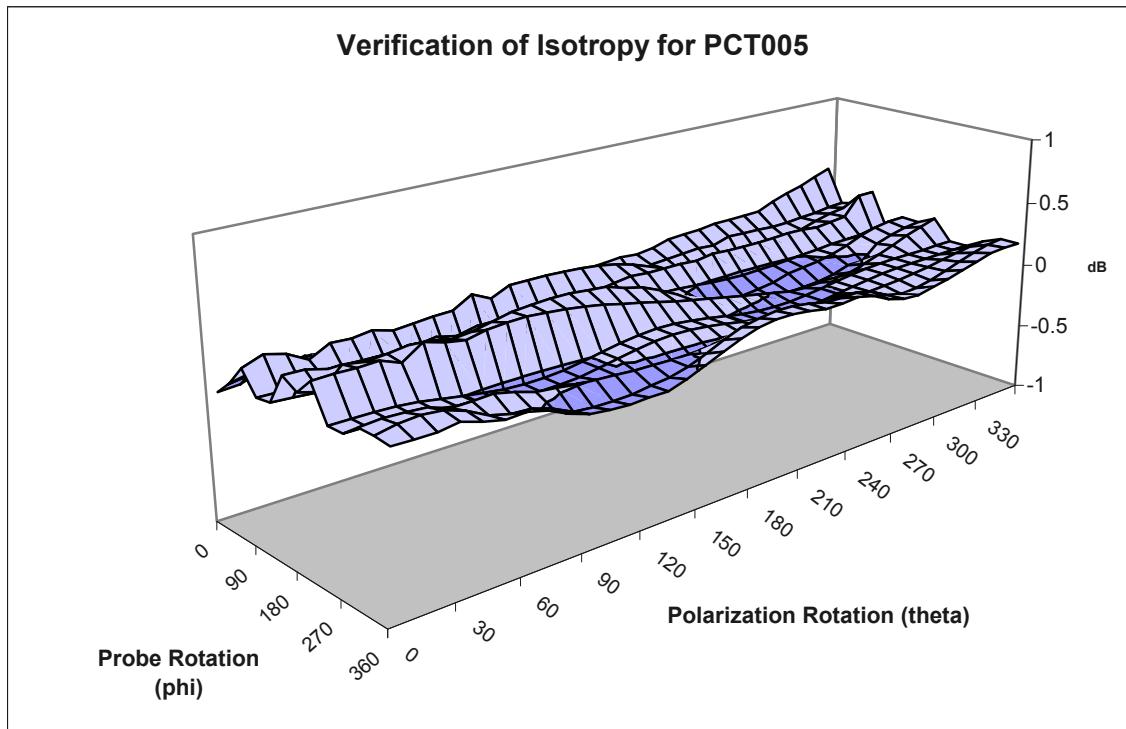


**PCTEST Calibration Laboratory**  
6660-B Dobbin Road  
Columbia, Maryland 21045 USA

TEM Calibration Plot  
Date: 13-Jan-05 04:03:28 pm  
Probe Name: PCT005  
Frequency: 450  
Sensitivity: Ch1: 3.320 Ch2: 3.289 Ch3: 3.267 mV/(mW/cm<sup>2</sup>)  
Isotropicity: 1.23% 0.05 db Min=0.993 Max=1.019

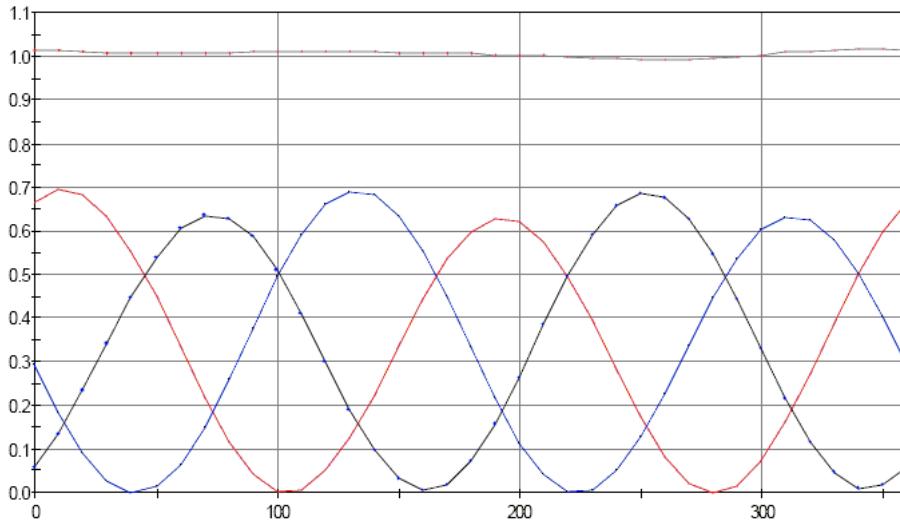


TEM Calibration Plot  
Date: 13-Jan-05 03:41:45 pm  
Probe Name: PCT005  
Frequency: 835  
Sensitivity: Ch1: 3.807 Ch2: 3.736 Ch3: 3.821 mV/(mW/cm<sup>2</sup>)  
Isotropicity: 2.12% 0.09 db Min=0.985 Max=1.028

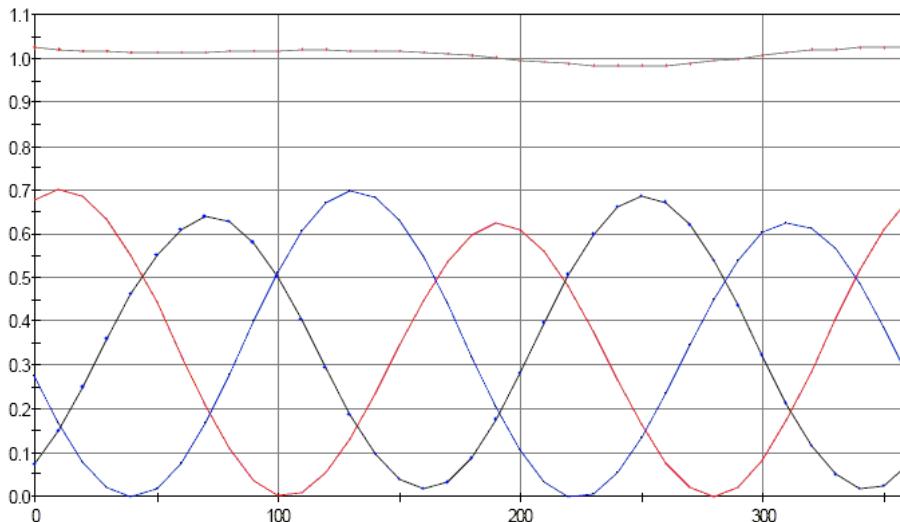



PCTEST Calibration Laboratory  
6660-B Dobbin Road  
Columbia, Maryland 21045 USA

TEM Calibration Plot  
Date: 14-Jan-05 11:08:15 am  
Probe Name: PCT005  
Frequency: 1900  
Sensitivity: Ch1: 5.115 Ch2: 4.969 Ch3: 4.453 mV/(mW/cm<sup>2</sup>)  
Isotropicity: 6.79% 0.29 db Min=0.961 Max=1.097

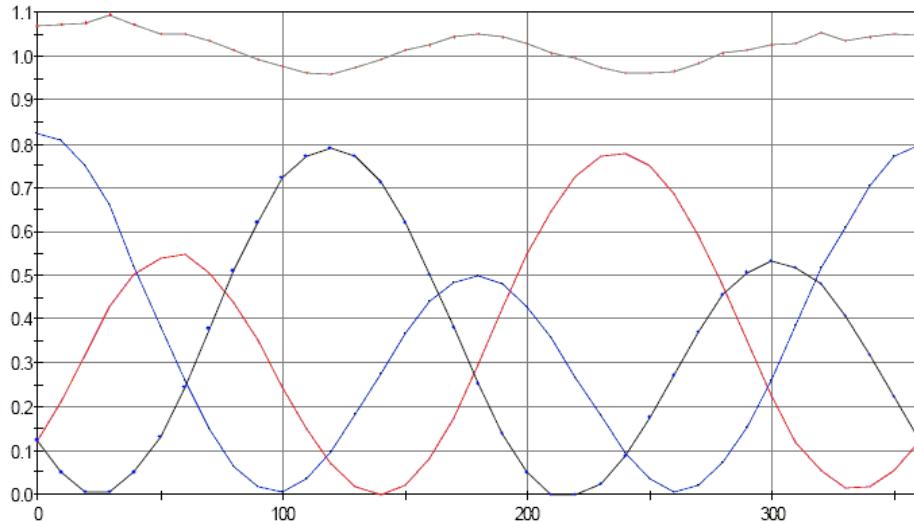

TEM Calibration Plot  
Date: 14-Jan-05 11:38:38 am  
Probe Name: PCT005  
Frequency: 2100  
Sensitivity: Ch1: 5.496 Ch2: 4.887 Ch3: 5.267 mV/(mW/cm<sup>2</sup>)  
Isotropicity: 7.61% 0.32 db Min=0.921 Max=1.074

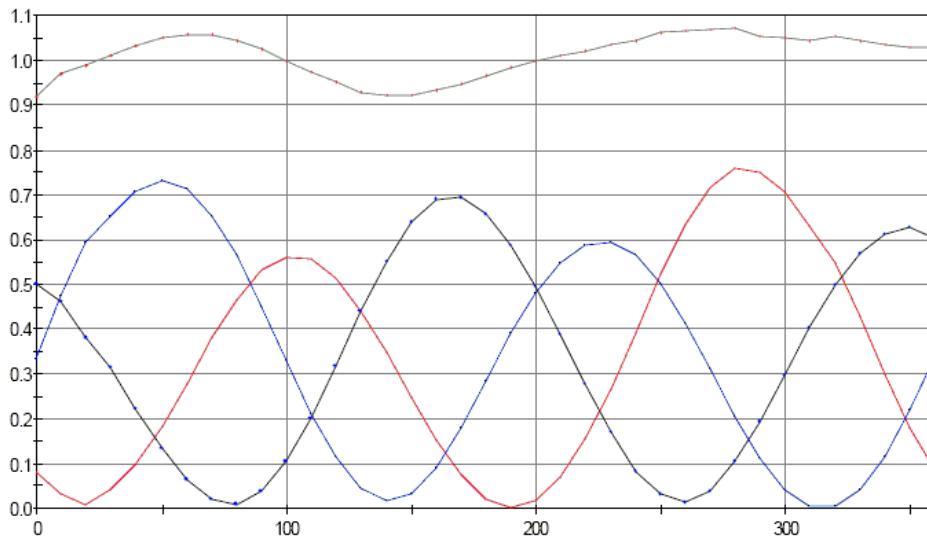

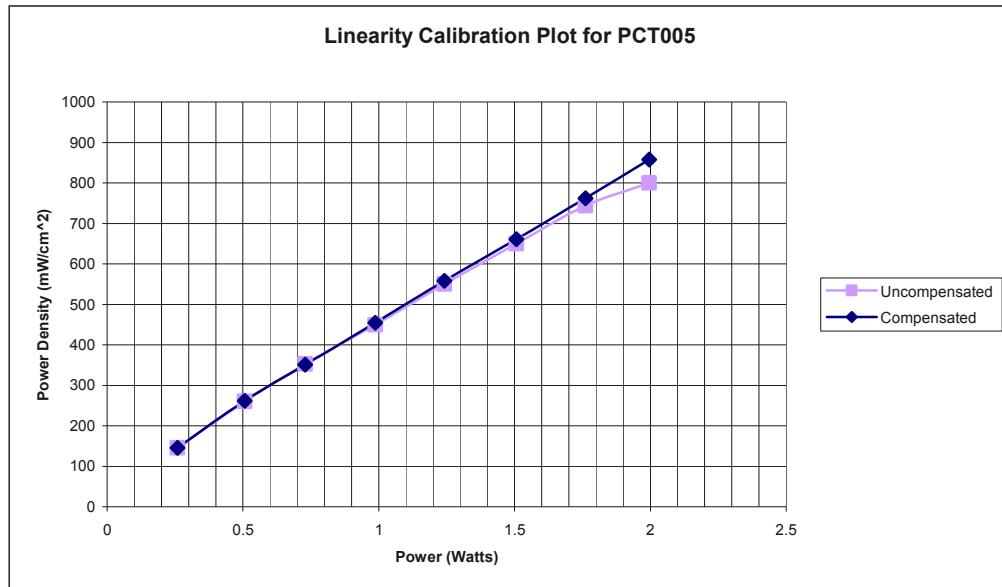

## Probe Physical Characteristics

Serial Number:	PCT005
Model:	E-020
Sensor Offset:	1.56 mm
Sensor Length:	2.5 mm
Tip Enclosure:	Ertalyte
Tip Diameter:	5 mm
Tip Length:	60 mm
Total Length:	290 mm

## Test Equipment

The test equipment used during the probe calibration are listed as follows:

EQUIPMENT SPECIFICATIONS		
Type	Calibration Due	Asset Number/ Serial Number
CRS Robot F3	February 2005	RAF0134133
CRS C500C Motion Controller	February 2005	RCB0003303
CRS Teach Pendant (Joystick)	February 2005	STP0132231
DELL Computer, Pentium 4 1.6 GHz, Windows 2000™	February 2005	4PJZ111
Flat SAM Phantom (P-SAM-FLAT)	February 2005	94X-097
IDX Robot End Effector (EE-103-C)	February 2005	07111223
IDX Probe Amplifier	February 2005	07111113
Validation Dipole D835V2	October 2005	PCT441
Validation Dipole D1900V2	February 2005	PCT512
Validation Dipole D2450V2	October 2005	PCT641
HP-778D Dual-Directional Coupler (0.1 ~ 2.0 GHz)	November 2005	PCT664
MicroCircuits Directional Coupler (4.0 ~ 8.0 GHz)	November 2005	PE2204-6
Amplifier Research 5S1G4 Power Amp	January 2005	PCT540
IFI T184-10 Power Amplifier (4.0 ~ 18.0 GHz)	December 2005	5957
HP-8241A (250kHz ~ 20 GHz) Signal Generator	December 2005	88934
HP-8753E (30kHz ~ 6GHz) Network Analyzer	January 2006	PCT552
Rohde & Schwarz Power Meter NRVS 1020.1809.02	January 2006	835360/079
Rohde & Schwarz Power Sensor NRV-Z53 858.0500.02	April 2005	846076/007
HP85070B Dielectric Probe Kit	January 2005	PCT501
IFI CC110EXX TEM Cell (DC to 2000 MHz)	January 2006	PCT498
EMCO 3115 Horn Antenna (2.0 ~ 18.0 GHz)	August 2005	PCT496
Guildline 5150 Precision Dual-Thermometer	November 2005	66145