NVLAP LAB CODE 200707-0

SAR EVALUATION REPORT

For

Cellon Communications Technology (Shenzhen) Co., Ltd.

13/F, Skyworth C Building, Gaoxin S.Ave1, Hi-Tech Industrial Park,

Nanshan, Shenzhen, Guangdong, 518057 China

FCC ID: T38UT2016

Report Type:	**Product Type:**
Original Report	GSM&GPRS Dual Band Mobile Phone

Test Engineer:	Eric Zhang
Report Number:	RSZ09031601-SAR
Report Date:	2009-04-09
Reviewed By:	William Chen EMC Engineer
Prepared By:	Bay Area Compliance Laboratories Corp. (Shenzhen) 6/F, the 3rd Phase of WanLi Industrial Building, ShiHua Road, FuTian Free Trade Zone Shenzhen, Guangdong, China Tel: +86-755-33320018 Fax: +86-755-33320008

Summary of Test Results	
Rule Part(s):	CFR 47 §2.1093
Test Procedure(s):	FCC OET Bulletin 65C IEEE 1528-2003
Device Type:	Portable device
Exposure Category	Population/Uncontrolled
Modulation:	GMSK
TX Frequency Range:	824-849 MHz (Cellular Band) 1850-1910 MHz (PCS Band)
Maximum Conducted Power Tested:	32.12 dBm (Cellular Band) 29.13 dBm(PCS Band)
Antenna Type(s):	Internal Antenna
Body-Worn Accessories:	Headset
Face-Head Accessories:	None
Max. SAR Level(s) Measured:	0.530W/Kg 1g Head Tissue (Cellular Band) 0.369W/Kg 1g Body Tissue (Cellular Band) 0.566W/Kg 1g Head Tissue (PCS Band) 0.308W/Kg 1g Body Tissue (PCS Band)

This wireless device has been shown to be capable of compliance for localized specific absorption rate (SAR) for General Population/Uncontrolled Exposure limits specified in ANSI/IEEE Standards and has been tested in accordance with the measurement procedures specified in FCC OET 65 Supplement C and IEEE 1528-2003.

The results and statements contained in this report pertain only to the device(s) evaluated.

EUT Photo

TABLE OF CONTENTS

REFERENCE, STANDARDS, AND GUILDELINES

FCC:

The Report and Order requires routine SAR evaluation prior to equipment authorization of portable transmitter devices, including portable telephones. For consumer products, the applicable limit is 1.6 mW/g as recommended by the ANSI/IEEE standard C95.1-1992 [6] for an uncontrolled environment (Paragraph 65). According to the Supplement C of OET Bulletin 65 “Evaluating Compliance with FCC Guide-lines for Human Exposure to Radio frequency Electromagnetic Fields", released on Jun 29, 2001 by the FCC, the device should be evaluated at maximum output power (radiated from the antenna) under “worst-case” conditions for normal or intended use, incorporating normal antenna operating positions, device peak performance frequencies and positions for maximum RF energy coupling.

This report describes the methodology and results of experiments performed on wireless data terminal. The objective was to determine if there is RF radiation and if radiation is found, what is the extent of radiation with respect to safety limits. SAR (Specific Absorption Rate) is the measure of RF exposure determined by the amount of RF energy absorbed by human body (or its parts) – to determine how the RF energy couples to the body or head which is a primary health concern for body worn devices. The limit below which the exposure to RF is considered safe by regulatory bodies in North America is 1.6 mW/g average over 1 gram of tissue mass.

CE:

The order requires routine SAR evaluation prior to equipment authorization of portable transmitter devices, including portable telephones. For consumer products, the applicable limit is 2 mW/g as recommended by the EN50360 for an uncontrolled environment. According to the Standard, the device should be evaluated at maximum output power (radiated from the antenna) under “worst-case” conditions for normal or intended use, incorporating normal antenna operating positions, device peak performance frequencies and positions for maximum RF energy coupling.

This report describes the methodology and results of experiments performed on wireless data terminal. The objective was to determine if there is RF radiation and if radiation is found, what is the extent of radiation with respect to safety limits. SAR (Specific Absorption Rate) is the measure of RF exposure determined by the amount of RF energy absorbed by human body (or its parts) – to determine how the RF energy couples to the body or head which is a primary health concern for body worn devices. The limit below which the exposure to RF is considered safe by regulatory bodies in Europe is 2 mW/g average over 10 gram of tissue mass.

The test configurations were laid out on a specially designed test fixture to ensure the reproducibility of measurements. Each configuration was scanned for SAR. Analysis of each scan was carried out to characterize the above effects in the device.

SAR Limits

FCC Limit (1g Tissue)

EXPOSURE LIMITS	SAR (W/kg)	
	(General Population / Uncontrolled Exposure Environment)	(Occupational / Controlled Exposure Environment)
Spatial Average (averaged over the whole body)	0.08	0.4
Spatial Peak (averaged over any 1 g of tissue)	1.60	8.0
Spatial Peak (hands/wrists/feet/ankles averaged over 10 g)	4.0	20.0

CE Limit (10g Tissue)

EXPOSURE LIMITS	SAR (W/kg)	
	(General Population / Uncontrolled Exposure Environment)	(Occupational / Controlled Exposure Environment)
Spatial Average (averaged over the whole body)	0.08	0.4
Spatial Peak (averaged over any 1 g of tissue)	2.0	10
Spatial Peak (hands/wrists/feet/ankles averaged over 10 g)	4.0	20.0

Population/Uncontrolled Environments are defined as locations where there is the exposure of individual who have no knowledge or control of their exposure.

Occupational/Controlled Environments are defined as locations where there is exposure that may be incurred by people who are aware of the potential for exposure (i.e. as a result of employment or occupation).

EUT DESCRIPTION

This Bay Area Compliance Laboratories Corp. test report has been prepared on behalf of Cellon Communications Technology(Shenzhen)Co., Ltd. and their product,C2016HW(FCC ID:T38UT2016) or the EUT (Equipment Under Test) as referred to in the rest of this report.

Technical Specification

Item	Content
Modulation	GMSK
Frequency Band	Cellular Band: 824-849 MHz 869-894 MHz PCS Band: 1850-1910 MHz 1930-1990 MHz
Dimensions (L*W*H)	109mm (L)× 48mm (W)× 11mm (H)
Weight	70 g
Power Source	3.7 Vdc/1800mAh Rechargeable Battery
Normal Operation	Head and Body-worn

EUT Photo

Model: C2016HW
Please refer to Appendix H

FACILITIES AND ACCREDITATION

The test site used by Bay Area Compliance Laboratories Corp. (Shenzhen) to collect data is located at

6/F, the 3rd Phase of WanLi Industrial Building,
Shi Hua Road, Fu Tian Free Trade Zone,
Shenzhen, Guangdong, P.R. of China

Additionally, Bay Area Compliance Laboratories Corp. (Shenzhen) is a National Institute of Standards and Technology (NIST) accredited laboratory, under the National Voluntary Laboratory Accredited Program (Lab Code 200707-0).

NVLAP LAB CODE 200707-0

The current scope of accreditations can be found at
http://ts.nist.gov/Standards/scopes/2007070.htm

DESCRIPTION OF TEST SYSTEM

These measurements were performed with ALSAS 10 Universal Integrated SAR Measurement system from APREL Laboratories.

ALSAS-10U System Description

ALSAS-10-U is fully compliant with the technical and scientific requirements of IEEE 1528, IEC 62209, CENELEC, ARIB, ACA, and the Federal Communications Commission. The system comprises of a six axes articulated robot which utilizes a dedicated controller.ALSAS-10U uses the latest methodologies. And FDTD modeling to provide a platform which is repeatable with minimum uncertainty.

Applications

Predefined measurement procedures compliant with the guidelines of CENELEC, IEEE, IEC, FCC, etc are utilized during the assessment for the device. Automatic detection for all SAR maxima are embedded within the core architecture for the system, ensuring that peak locations used for centering the zoom scan are within a 1mm resolution and a 0.05mm repeatable position. System operation range currently available up-to 6 GHz in simulated tissue.

Area Scans

Area scans are defined prior to the measurement process being executed with a user defined variable spacing between each measurement point (integral) allowing low uncertainty measurements to be conducted. Scans defined for FCC applications utilize a 10mm2 step integral, with 1mm interpolation used to locate the peak SAR area used for zoom scan assessments.
Where the system identifies multiple SAR peaks (which are within 25% of peak value) the system will provide the user with the option of assessing each peak location individually for zoom scan averaging.

Zoom Scan (Cube Scan Averaging)

The averaging zoom scan volume utilized in the ALSAS-10U software is in the shape of a cube and the side dimension of a 1 g or 10 g mass is dependent on the density of the liquid representing the simulated tissue. A density of 1000 kg/m3 is used to represent the head and body tissue density and not the phantom liquid density, in order to be consistent with the definition of the liquid dielectric properties, i.e. the side length of the 1 g cube is 10mm,with the side length of the 10 g cube 21,5mm.

When the cube intersects with the surface of the phantom, it is oriented so that 3 vertices touch the surface of the shell or the center of a face is tangent to the surface. The face of the cube closest to the surface is modified in order to conform to the tangent surface.

The zoom scan integer steps can be user defined so as to reduce uncertainty, but normal practice for typical test applications (including FCC) utilize a physical step of 5x5x8 (8mmx8mmx5mm) providing a volume of 32mm in the X & Y axis, and 35mm in the Z axis.

ALSAS-10U Interpolation and Extrapolation Uncertainty

The overall uncertainty for the methodology and algorithms the used during the SAR calculation was evaluated using the data from IEEE 1528 based on the example f3 algorithm:

$$f_3(x,y,z) = A\frac{a^2}{\frac{a^2}{4} + x'^2 + y'^2}\cdot\left(e^{-\frac{2z}{a}} + \frac{a^2}{2(a+2z)^2}\right)$$

Isotropic E-Field Probe

The isotropic E-Field probe has been fully calibrated and assessed for isotropicity, and boundary effect within a controlled environment. Depending on the frequency for which the probe is calibrated the method utilized for calibration will change.

The E-Field probe utilizes a triangular sensor arrangement as detailed in the diagram below:

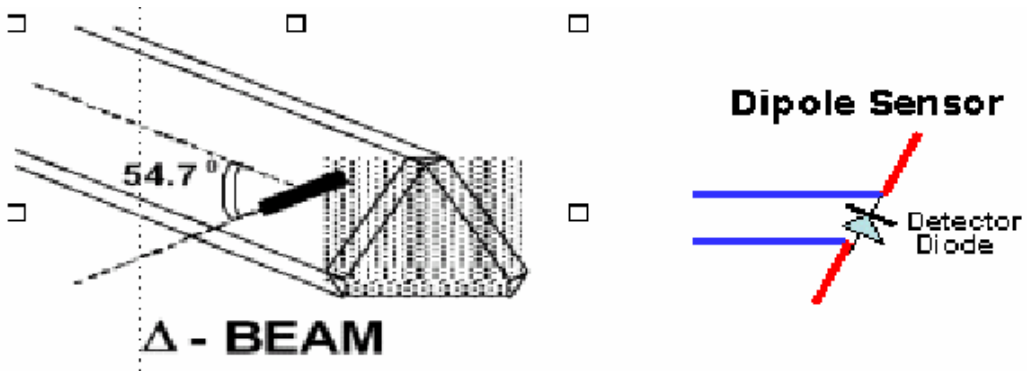

SAR is assessed with a calibrated probe which moves at a default height of 5mm from the center of the diode, which is mounted to the sensor, to the phantom surface (in the Z Axis). The 5mm offset height has been selected so as to minimize any resultant boundary effect due to the probe being in close proximity to the phantom surface.

The following algorithm is an example of the function used by the system for linearization of the output from the probe when measuring complex modulation schemes.

$$V_i = U_i + U_i^2 \cdot \frac{cf}{dcp_i}$$

Isotropic E-Field Probe Specification

Calibration in Air	Frequency Dependent Below 2 GHz Calibration in air performed in a TEM Cell Above 2 GHz Calibration in air performed in waveguide
Sensitivity	0.70 μV/(V/m)^2 to 0.85 μV/(V/m)^2
Dynamic Range	0.0005 W/kg to 100 W/kg
Isotropic Response	Better than 0.2 dB
Diode Compression Point (DCP)	Calibration for Specific Frequency
Probe Tip Radius	< 5 mm
Sensor Offset	1.56 (+/- 0.02 mm)
Probe Length	290 mm
Video Bandwidth	@ 500 Hz: 1 dB @ 1.02 kHz: 3 dB
Boundary Effect	Less than 2% for distance greater than 2.4 mm
Spatial Resolution	Diameter less than 5 mm Compliant with Standards

Boundary Detection Unit and Probe Mounting Device

ALSAS-10U incorporates a boundary detection unit with a sensitivity of 0.05mm for detecting all types of surfaces. The robust design allows for detection during probe tilt (probe normalize) exercises, and utilizes a second stage emergency stop. The signal electronics are fed directly into the robot controller for high accuracy surface detection in lateral and axial detection modes (X, Y, & Z).

The probe is mounted directly onto the Boundary Detection unit for accurate tooling and displacement calculations controlled by the robot kinematics. The probe is connect to an isolated probe interconnect where the output stage of the probe is fed directly into the amplifier stage of the Daq-Paq.

Daq-Paq (Analog to Digital Electronics)

ALSAS-10U incorporates a fully calibrated Daq-Paq (analog to digital conversion system) which has a 4 channel input stage, sent via a 2 stage auto-set amplifier module. The input signal is amplified accordingly so as to offer a dynamic range from 5μV to 800mV. Integration of the fields measured is carried out at board level utilizing a Co-Processor which then sends the measured fields down into the main computational module in digitized form via an RS232 communications port. Probe linearity and duty cycle compensation is carried out within the main Daq-Paq module.

ADC	12 Bit
Amplifier Range	20 mV to 200 mV and 150 mV to 800 mV
Field Integration	Local Co-Processor utilizing proprietary integration algorithms
Number of Input Channels	4 in total 3 dedicated and 1 spare
Communication	Packet data via RS232

Axis Articulated Robot

ALSAS-10U utilizes a six axis articulated robot, which is controlled using a Pentium based real-time movement controller. The movement kinematics engine utilizes proprietary (Thermo CRS) interpolation and extrapolation algorithms, which allow full freedom of movement for each of the six joints within the working envelope. Utilization of joint 6 allows for full probe rotation with a tolerance better than 0.05mm around the central axis.

Robot/Controller Manufacturer	Thermo CRS
Number of Axis	Six independently controlled axis
Positioning Repeatability	0.05 mm
Controller Type	Single phase Pentium based C500C
Robot Reach	710 mm
Communication	RS232 and LAN compatible

ALSAS Universal Workstation

ALSAS Universal workstation allows for repeatability and fast adaptability. It allows users to do calibration, testing and measurements using different types of phantoms with one set up, which significantly speeds up the measurement process.

Universal Device Positioner

The universal device positioner allows complete freedom of movement of the EUT. Developed to hold a EUT in a free-space scenario any additional loading attributable to the material used in the construction of the positioner has
been eliminated. Repeatability has been enhanced through the linear scales which form the design used to indicate positioning for any given test scenario in all
major axes. A 15° tilt indicator is included for the of aid cheek to tilt movements for head SAR analysis. Overall uncertainty for measurements have been reduced
due to the design of the Universal device positioner, which allows positioning of a device in as near to a free-space scenario as possible, and by providing the
means for complete repeatability.

Phantom Types

The ALSAS-10U allows the integration of multiple phantom types. SAM Phantoms fully compliant with IEEE 1528, Universal Phantom, and Universal Flat.

APREL SAM Phantoms

The SAM phantoms developed using the IEEE SAM CAD file. They are fully compliant with the requirements for both IEEE 1528 and FCC Supplement C. Both the left and right SAM phantoms are interchangeable, transparent and include the IEEE 1528 grid with visible NF and MB lines.

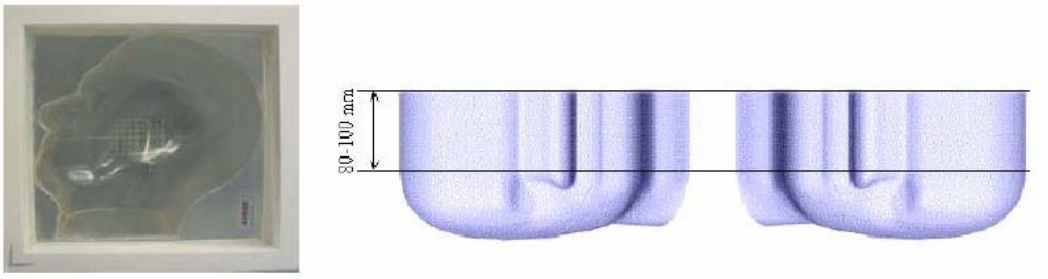

APREL Laboratories Universal Phantom

The Universal Phantom is used on the ALSAS-10U as a system validation phantom.The Universal Phantom has been fully validated both experimentally from 800MHz to 6GHz and numerically using XFDTD numerical software.
The shell thickness is 2mm overall, with a 4mm spacer located at the NF/MB intersection providing an overall thickness of 6mm in line with the requirements of
IEEE-1528.

The design allows for fast and accurate measurements, of handsets, by allowing the conservative SAR to be evaluated at on frequency for both left and right head experiments in one measurement.

Tissue Dielectric Parameters for Head and Body Phantoms

The head tissue dielectric parameters recommended by the IEEE SCC-34/SC-2 in P1528 have been incorporated in the following table. These head parameters are derived from planar layer models simulating the highest expected SAR for the dielectric properties and tissue thickness variations in a human head. Other head and body tissue parameters that have not been specified in P1528 are derived from the tissue dielectric parameters computed from the 4-Cole-Cole equations described in Reference [12] and extrapolated according to the head parameters specified in P1528.

Ingredients (% by weight)	Frequency (MHz)									
	450		835		915		1900		2450	
Tissue Type	Head	Body	Head	Body	Head	Body	Head	Body	Head	Body
Water	38.56	51.16	41.45	52.4	41.05	56.0	54.9	40.4	62.7	73.2
Salt (Nacl)	3.95	1.49	1.45	1.4	1.35	0.76	0.18	0.5	0.5	0.04
Sugar	56.32	46.78	56.0	45.0	56.5	41.76	0.0	58.0	0.0	0.0
HEC	0.98	0.52	1.0	1.0	1.0	1.21	0.0	1.0	0.0	0.0
Bactericide	0.19	0.05	0.1	0.1	0.1	0.27	0.0	0.1	0.0	0.0
Triton x-100	0.0	0.0	0.0	0.0	0.0	0.0	0.0	0.0	36.8	0.0
DGBE	0.0	0.0	0.0	0.0	0.0	0.0	44.92	0.0	0.0	26.7
Dielectric Constant	43.42	58.0	42.54	56.1	42.0	56.8	39.9	54.0	39.8	52.5
Conductivity (s/m)	0.85	0.83	0.91	0.95	1.0	1.07	1.42	1.45	1.88	1.78

IEEE SCC-34/SC-2 P1528 Recommended Tissue Dielectric Parameters

Frequency (MHz)	Head Tissue		Body Tissue	
	εr	Ơ (S/m)	εr	Ơ (S/m)
150	52.3	0.76	61.9	0.80
300	45.3	0.87	58.2	0.92
450	43.5	0.87	56.7	0.94
835	41.5	0.90	55.2	0.97
900	41.5	0.97	55.0	1.05
915	41.5	0.98	55.0	1.06
1450	40.5	1.20	54.0	1.30
1610	40.3	1.29	53.8	1.40
1800-2000	40.0	1.40	53.3	1.52
2450	39.2	1.80	52.7	1.95
3000	38.5	2.40	52.0	2.73
5800	35.3	5.27	48.2	6.00

EQUIPMENT LIST AND CALIBRATION

Equipments List & Calibration Info

Equipment	Model	Calibration Due Date	S/N:
CRS F3 robot	ALS-F3	N/A	RAF0805352
CRS F3 Software	ALS-F3-SW	N/A	N/A
CRS C500C controller	ALS-C500	N/A	RCF0805379
Probe mounting device & Boundary Detection Sensor System	ALS-PMDPS-3	N/A	120-00270
Universal Work Station	ALS-UWS	N/A	100-00157
Data Acquisition Package	ALS-DAQ-PAQ-3	N/A	110-00212
Miniature E-Field Probe	ALS-E-020	2009-08-01	273
Dipole, 835MHz	ALS-D-835-S-2	2009-08-01	180-00558
Dipole,1900MHz	ALS-D-1900-S-2	2009-08-01	210-00710
Dipole Spacer	ALS-DS-U	N/A	250-00907
R&S, universal Radio Communication Tester	CMU200	2008-06-21	1100.0008.02
Device holder/Positioner	ALS-H-E-SET-2	N/A	170-00510
Left ear SAM phantom	ALS-P-SAM-L	N/A	130-00311
Right ear SAM phantom	ALS-P-SAM-R	N/A	140-00359
UniPhantom	ALS-P-UP-1	N/A	150-00413
Simulated Tissue 835 MHz Head	ALS-T-835-1-H	Each Time	270-01002
Simulated Tissue 835 MHz Body	ALS-T-835-1-B	Each Time	270-02101
Simulated Tissue 1900 MHz Head	ALS-T-1900-1-H	Each Time	295-01103
Simulated Tissue 1900 MHz Body	ALS-T-1900-1-B	Each Time	295-02102
Signal Generator	HP8341B	2009-11-06	2624A00116
Power Amplifier	5S1G4	N/A	71377
Spectrum Analyzer	FSEM30	2009-05-08	849720/019

SAR MEASUREMENT SYSTEM VERIFICATION

Liquid Verification

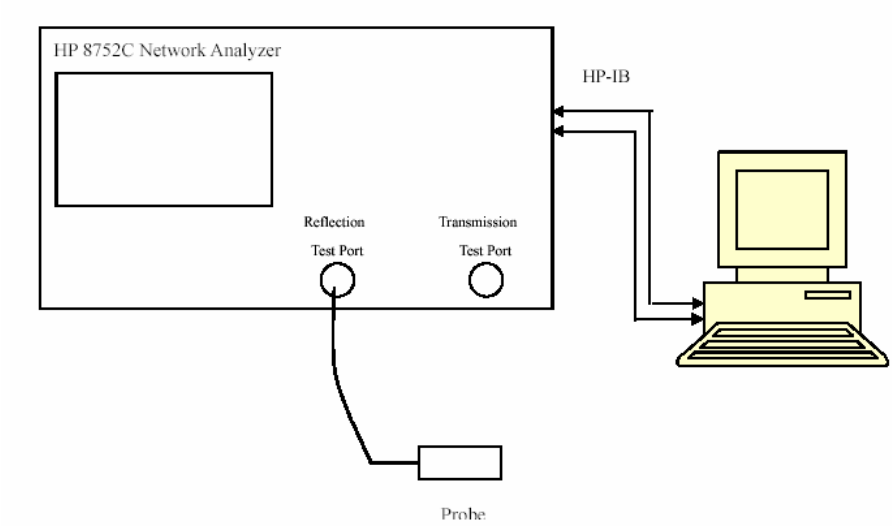

Liquid Verification Setup Block Diagram

Liquid Verification Results

Frequency (MHz)	Liquid Type	Liquid Parameter		Result
		εr	Ơ (S/m)	
850	Head	41.60	0.94	In Tolerance
850	Body	53.77	0.99	In Tolerance
1900	Head	39.30	1.43	In Tolerance
1900	Body	53.45	1.50	In Tolerance

Please refer to the following tables.

850 MHz Head				850 MHz Body		
Frequency	e'	e''		Frequency	e'	e''
824000000	41.559471	19.286859		824000000	53.848536	21.046323
824900000	41.626348	19.255343		824900000	53.836878	21.061756
825800000	41.574921	18.749347		825800000	53.912873	21.012184
826700000	41.495317	18.769255		826700000	53.866372	21.084608
827600000	41.524503	19.572751		827600000	53.877533	21.086146
828500000	41.453219	19.691251		828500000	53.871826	21.071617
829400000	41.474825	19.555821		829400000	53.877225	21.102917
830300000	41.540509	19.645248		830300000	53.871114	21.071928
831200000	41.528031	19.439698		831200000	53.889893	21.109305
832100000	41.529694	18.625416		832100000	53.890904	21.097009
833000000	41.451107	18.859946		833000000	53.813935	21.114849
833900000	41.505843	19.748819		833900000	53.815945	21.136105
834800000	41.548821	19.990147		834800000	53.837467	21.150323
835700000	41.577195	19.928789		835700000	53.831505	21.119378
836600000	41.562617	20.000158		836600000	53.825562	21.088466
837500000	41.565365	19.635072		837500000	53.847083	21.102551
838400000	41.551863	18.826912		838400000	53.777799	21.138862
839300000	41.518373	19.182774		839300000	53.844231	21.125409
840200000	41.545771	20.321049		840200000	53.819974	21.134238
841100000	41.625198	20.278847		841100000	53.808977	21.149140
842000000	41.644704	20.208828		842000000	53.822442	21.111184
842900000	41.611098	19.964607		842900000	53.782588	21.136709
843800000	41.567551	19.334881		843800000	53.770196	21.102855
844700000	41.492495	18.737412		844700000	53.752283	21.098440
845600000	41.595294	19.849752		845600000	53.780704	21.071480
846500000	41.716167	20.359021		846500000	53.735288	21.066359
847400000	41.761452	20.362395		847400000	53.759404	21.057366
848300000	41.748065	20.406468		848300000	53.754931	21.015368
849200000	41.701477	20.356443		849200000	53.815223	21.074627
850100000	41.603102	19.852319		850100000	53.773529	21.079109
851000000	41.530275	18.995781		851000000	53.719508	21.050097
851900000	41.640412	19.799573		851900000	53.811076	20.988771
852800000	41.785317	19.918771		852800000	53.758841	21.008161
853700000	41.820011	20.020379		853700000	53.775759	20.980049
854600000	41.833948	19.752405		854600000	53.774788	20.991163
855500000	41.755612	20.411683		855500000	53.743539	21.008146
856400000	41.701542	20.095651		856400000	53.768792	20.944475
857300000	41.565348	19.274689		857300000	53.782708	20.966214
858200000	41.626269	19.932137		858200000	53.704827	20.973672
859100000	41.904471	20.173105		859100000	53.706962	20.934978
860000000	41.931189	20.211592		860000000	53.756966	20.894565
860900000	41.874312	19.770067		860900000	53.710082	20.869027
861800000	41.810654	19.615594		861800000	53.679795	20.858803
862700000	41.611673	19.940681		862700000	53.782839	20.916826
863600000	41.590152	19.470003		863600000	53.695937	20.841984
864500000	41.800318	19.776664		864500000	53.743292	20.781077
865400000	41.881244	20.312102		865400000	53.721500	20.821493
866300000	41.032187	19.433891		866300000	53.734735	20.784253
867200000	41.967076	20.189665		867200000	53.688203	20.758977
868100000	40.895861	19.992624		868100000	53.689825	20.747634
869000000	40.794425	19.572079		869000000	53.659863	20.737600

1900 MHz Head				1900 MHz Body		
Frequency	e'	e''		Frequency	e'	e''
1850000000	39.515658	13.572314		1850000000	53.610099	13.990623
1851200000	39.515289	13.565529		1851200000	53.571643	13.969518
1852400000	39.534231	13.531715		1852400000	53.591382	14.016414
1853600000	39.519764	13.545747		1853600000	53.601427	13.984232
1854800000	39.502872	13.546224		1854800000	53.541049	13.942952
1856000000	39.497180	13.506712		1856000000	53.474739	13.866918
1857200000	39.500860	13.530467		1857200000	53.455789	13.802804
1858400000	39.474062	13.510156		1858400000	53.509401	13.862545
1859600000	39.494788	13.508248		1859600000	53.535671	13.892453
1860800000	39.438101	13.497654		1860800000	53.515867	13.927822
1862000000	39.453150	13.496261		1862000000	53.516868	13.925835
1863200000	39.447747	13.471730		1863200000	53.517987	13.879928
1864400000	39.432646	13.489195		1864400000	53.509250	13.971032
1865600000	39.444456	13.501814		1865600000	53.467224	13.906060
1866800000	39.430990	13.512279		1866800000	53.472851	13.932776
1868000000	39.430980	13.496352		1868000000	53.486695	13.944676
1869200000	39.406545	13.498728		1869200000	53.520130	13.989808
1870400000	39.396632	13.509950		1870400000	53.477556	13.984009
1871600000	39.393963	13.489747		1871600000	53.506378	14.004006
1872800000	39.410400	13.490464		1872800000	53.505101	14.015174
1874000000	39.409164	13.520195		1874000000	53.487669	14.048473
1875200000	39.396773	13.470258		1875200000	53.471347	14.055113
1876400000	39.394553	13.512516		1876400000	53.490980	14.068930
1877600000	39.388998	13.521024		1877600000	53.482507	14.072093
1878800000	39.370037	13.508110		1878800000	53.474685	14.012444
1880000000	39.362834	13.475894		1880000000	53.471632	14.025257
1881200000	39.356824	13.478749		1881200000	53.494337	14.058128
1882400000	39.359419	13.500034		1882400000	53.479498	14.03061
1883600000	39.326293	13.469313		1883600000	53.482734	13.979059
1884800000	39.373110	13.513351		1884800000	53.480697	14.016541
1886000000	39.376419	13.507375		1886000000	53.488158	14.001264
1887200000	39.357561	13.494509		1887200000	53.465653	14.028468
1888400000	39.340179	13.507513		1888400000	53.455706	14.124422
1889600000	39.319444	13.486927		1889600000	53.497573	14.154019
1890800000	39.311965	13.496670		1890800000	53.474272	14.152728
1892000000	39.314546	13.494114		1892000000	53.487210	14.146963
1893200000	39.301156	13.489781		1893200000	53.397435	13.995489
1894400000	39.311254	13.494353		1894400000	53.444571	14.041923
1895600000	39.296686	13.511587		1895600000	53.448325	14.026514
1896800000	39.268058	13.534731		1896800000	53.441965	14.086315
1898000000	39.280711	13.519834		1898000000	53.444669	14.101031
1899200000	39.281002	13.560333		1899200000	53.461806	14.138903
1900400000	39.295196	13.538512		1900400000	53.454226	14.236515
1901600000	39.331695	13.579749		1901600000	53.500872	14.298093
1902800000	39.314727	13.583670		1902800000	53.460710	14.353000
1904000000	39.325468	13.593681		1904000000	53.502438	14.338487
1905200000	39.325825	13.568739		1905200000	53.502035	14.341576
1906400000	39.303602	13.629451		1906400000	53.531387	14.360696
1907600000	39.323946	13.645180		1907600000	53.487790	14.411610
1908800000	39.327462	13.671673		1908800000	53.511743	14.421008
1910000000	39.321504	13.650727		1910000000	53.503154	14.384005

System Accuracy Verification

Prior to the assessment, the system validation kit was used to test whether the system was operating within its specifications of ±10%. The validation results are tabulated below. And also the corresponding SAR plot is attached as well in the SAR plots files.

System Verification Setup Block Diagram

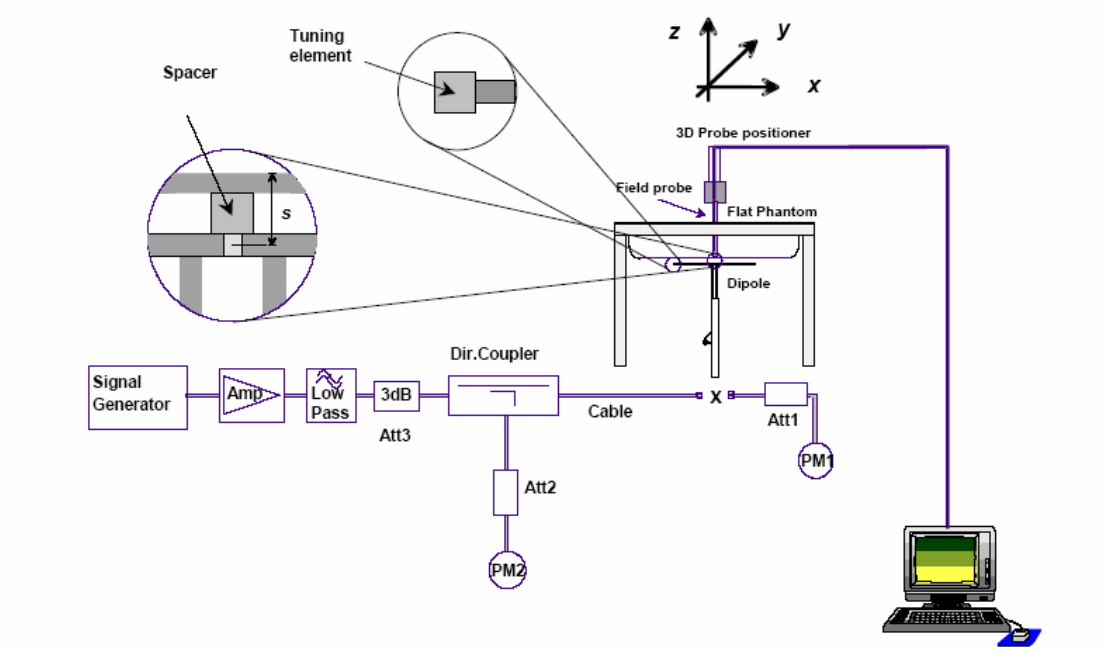

System Accuracy Check Results

Frequency (MHz)	1 g SAR (W/Kg)	10 g SAR (W/Kg)	Result
835	9.651	6.042	In Tolerance
1900	40.328	20.137	In Tolerance

* Note: All SAR values are normalized to 1 Watt forward power.

IEEE P1528 recommended reference value for Head Tissue

Frequency (MHz)	1 g SAR (W/Kg)	10 g SAR (W/Kg)	Local SAR at surface (above feed point)	Local SAR at surface (v=2cm offset from feed point)
300	3.0	2.0	4.4	2.1
450	4.9	3.3	7.2	3.2
835	9.5	6.2	14.1	4.9
900	10.8	6.9	16.4	5.4
1450	29.0	16.0	50.2	6.5
1800	38.1	19.8	69.5	6.8
1900	39.7	20.5	72.1	6.6
2000	41.1	21.1	74.6	6.5
2450	52.4	24.0	104.2	7.7
3000	63.8	25.7	140.2	9.5

EUT TEST STRATEGY AND METHODOLOGY

Test Positions for Device Operating Next to a Person's Ear

This category includes most wireless handsets with fixed, retractable or internal antennas located toward the top half of the device, with or without a foldout, sliding or similar keypad cover. The handset should have its earpiece located within the upper ¼ of the device, either along the centerline or off-centered, as perceived by its users. This type of handset should be positioned in a normal operating position with the "test device reference point" located along the "vertical centerline" on the front of the device aligned to the "ear reference point". The "test device reference point" should be located at the same level as the center of the earpiece region. The "vertical centerline" should bisect the front surface of the handset at its top and bottom edges. A "ear reference point" is located on the outer surface of the head phantom on each ear spacer. It is located 1.5 cm above the center of the ear canal entrance in the "phantom reference plane" defined by the three lines joining the center of each "ear reference point" (left and right) and the tip of the mouth.

A handset should be initially positioned with the earpiece region pressed against the ear spacer of a head phantom. For the SCC-34/SC-2 head phantom, the device should be positioned parallel to the "N-F" line defined along the base of the ear spacer that contains the "ear reference point". For interim head phantoms, the device should be positioned parallel to the cheek for maximum RF energy coupling. The "test device reference point" is aligned to the "ear reference point" on the head phantom and the "vertical centerline" is aligned to the "phantom reference plane". This is called the "initial ear position". While maintaining these three alignments, the body of the handset is gradually adjusted to each of the following positions for evaluating SAR:

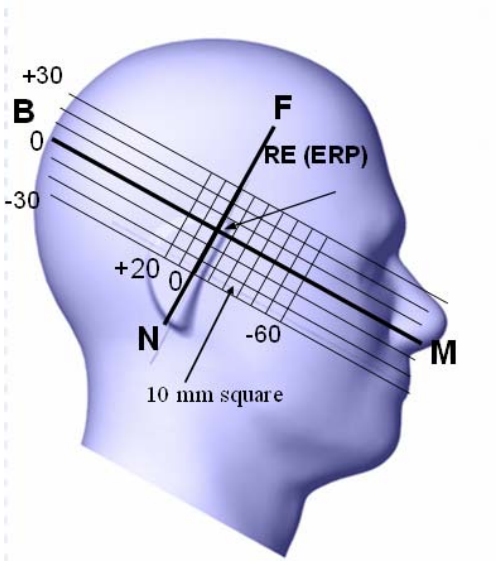

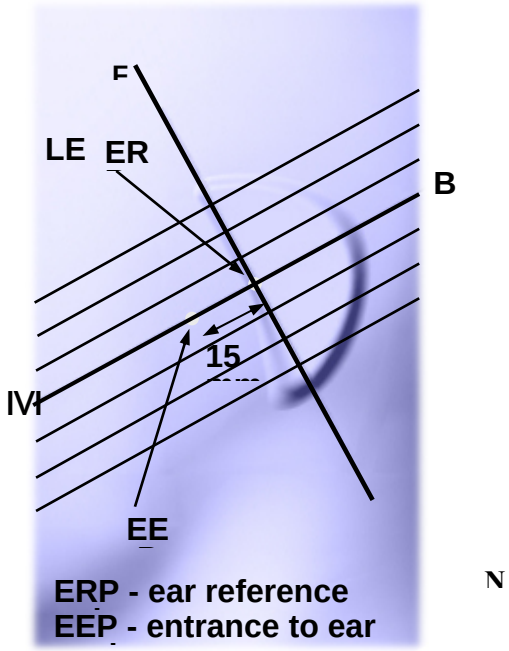

N

Cheek/Touch Position

The device is brought toward the mouth of the head phantom by pivoting against the "ear reference point" or along the "N-F" line for the SCC-34/SC-2 head phantom.

This test position is established:

- When any point on the display, keypad or mouthpiece portions of the handset is in contact with the phantom.
- (or) When any portion of a foldout, sliding or similar keypad cover opened to its intended self-adjusting normal use position is in contact with the cheek or mouth of the phantom.

For existing head phantoms – when the handset loses contact with the phantom at the pivoting point, rotation should continue until the device touches the cheek of the phantom or breaks its last contact from the ear spacer.

Check /Touch Position

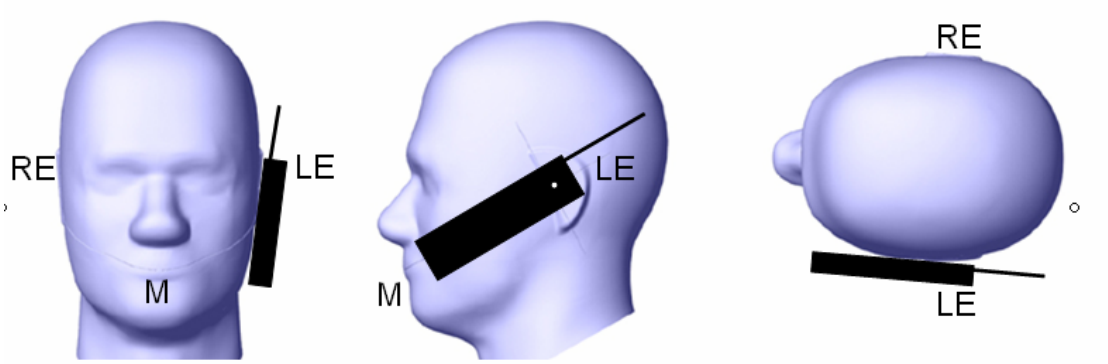

Ear/Tilt Position

With the handset aligned in the "Cheek/Touch Position":

1) If the earpiece of the handset is not in full contact with the phantom's ear spacer (in the "Cheek/Touch position") and the peak SAR location for the "Cheek/Touch" position is located at the ear spacer region or corresponds to the earpiece region of the handset, the device should be returned to the "initial ear position" by rotating it away from the mouth until the earpiece is in full contact with the ear spacer.

2) (otherwise) The handset should be moved (translated) away from the cheek perpendicular to the line passes through both "ear reference points" (note: one of these ear reference points may not physically exist on a split head model) for approximate 2-3 cm. While it is in this position, the device handset is tilted away from the mouth with respect to the "test device reference point" until the inside angle between the vertical centerline on the front surface of the phone and the horizontal line passing through the ear reference point isby 15 80°. After the tilt, it is then moved (translated) back toward the head perpendicular to the line passes through both "ear reference points" until the device touches the phantom or the ear spacer. If the antenna touches the head first, the positioning process should be repeated with a tilt angle less than 15° so that the device and its antenna would touch the phantom simultaneously. This test position may require a device holder or positioner to achieve the translation and tilting with acceptable positioning repeatability.

If a device is also designed to transmit with its keypad cover closed for operating in the head position, such positions should also be considered in the SAR evaluation. The device should be tested on the left and right side of the head phantom in the "Cheek/Touch" and "Ear/Tilt" positions. When applicable, each configuration should be tested with the antenna in its fully extended and fully retracted positions. These test configurations should be tested at the high, middle and low frequency channels of each operating mode; for example, AMPS, CDMA, and TDMA. If the SAR measured at the middle channel for each test configuration (left, right, Cheek/Touch, Tile/Ear, extended and retracted) is at least 2.0 dB lower than the SAR limit, testing at the high and low channels is optional for such test configuration(s). If the transmission band of the test device is less than 10 MHz, testing at the high and low frequency channels is optional.

Ear /Tilt 15^{o} Position

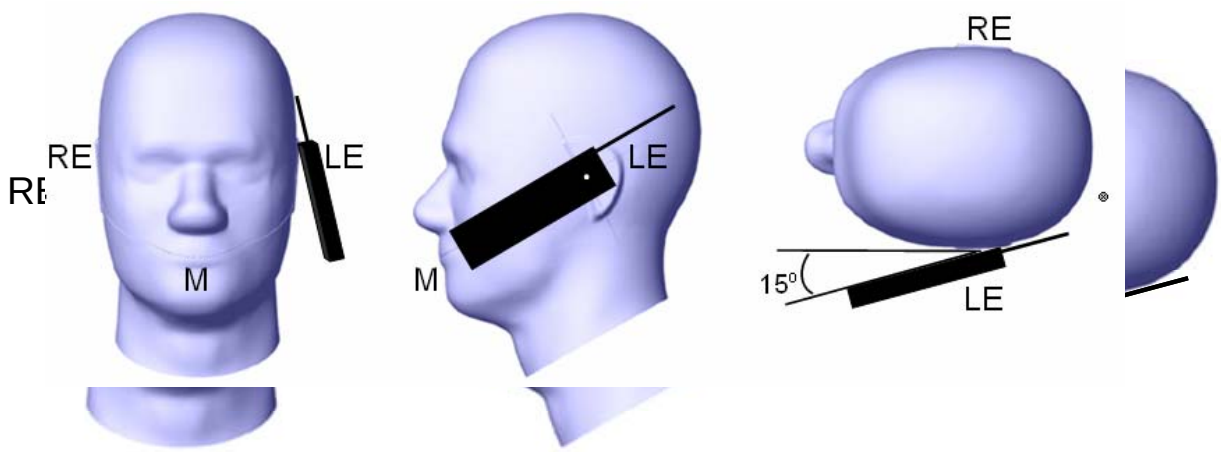

Test positions for body-worn and other configurations

Body-worn operating configurations should be tested with the belt-clips and holsters attached to the device and positioned against a flat phantom in normal use configurations. Devices with a headset output should be tested with a headset connected to the device. When multiple accessories that do not contain metallic components are supplied with the device, the device may be tested with only the accessory that dictates the closest spacing to the body. When multiple accessories that contain metallic components are supplied with the device, the device must be tested with each accessory that contains a unique metallic component. If multiple accessories share an identical metallic component (e.g., the same metallic belt-clip used with different holsters with no other metallic components), only the accessory that dictates the closest spacing to the body must be tested.

Body-worn accessories may not always be supplied or available as options for some devices that are intended to be authorized for body-worn use. A separation distance of 1.5 cm between the back of the device and a flat phantom is recommended for testing body-worn SAR compliance under such circumstances. Other separation distances may be used, but they should not exceed 2.5 cm. In these cases, the device may use body-worn accessories that provide a separation distance greater than that tested for the device provided however that the accessory contains no metallic components.

SAR Evaluation Procedure

The evaluation was performed with the following procedure:

Step 1: Measurement of the SAR value at a fixed location above the ear point or central position was used as a reference value for assessing the power drop. The SAR at this point is measured at the start of the test and then again at the end of the testing.

Step 2: The SAR distribution at the exposed side of the head was measured at a distance of 4 mm from the inner surface of the shell. The area covered the entire dimension of the head or EUT and the horizontal grid spacing was 15 mm x 15 mm. Based on these data, the area of the maximum absorption was determined by spline interpolation. The first Area Scan covers the entire dimension of the EUT to ensure that the hotspot was correctly identified.

Step 3: Around this point, a volume of 30 mm x 30 mm x 21 mm was assessed by measuring 5 x 5 x 7 points. On the basis of this data set, the spatial peak SAR value was evaluated under the following procedure:

1) The data at the surface were extrapolated, since the center of the dipoles is 1.2 mm away from the tip of the probe and the distance between the surface and the lowest measuring point is 1.3 mm. The extrapolation was based on a least square algorithm. A polynomial of the fourth order was calculated through the points in z-axes. This polynomial was then used to evaluate the points between the surface and the probe tip.

2) The maximum interpolated value was searched with a straightforward algorithm. Around this maximum the SAR values averaged over the spatial volumes (1 g or 10 g) were computed by the 3D-Spline interpolation algorithm. The 3D-Spline is composed of three one dimensional splines with the “Not a knot"-condition (in x, y and z-directions). The volume was integrated with the trapezoidal-algorithm. One thousand points (10 x 10 x 10) were interpolated to calculate the averages.

All neighboring volumes were evaluated until no neighboring volume with a higher average value was found.

Step 4: Re-measurement of the SAR value at the same location as in Step 1. If the value changed by more than 5%, the evaluation was repeated.

SAR MEASUREMENT RESULTS

This page summarizes the results of the performed dosimetric evaluation. The plots with the corresponding SAR distributions, which reveal information about the location of the maximum SAR with respect to the device, could be found in Appendix E.

SAR Test Data

Environmental Conditions

Temperature:	21° C
Relative Humidity:	54%
ATM Pressure:	1010 mbar

** Testing was performed by Eric Zhang on 2009-03-30.*

Cellular Band:

EUT Position	Frequency (MHz)	Test Type	Test Mode	Antenna Type	Liquid	Phantom	Accessories	1g SAR Value (W/Kg)	FCC Limit (W/Kg)	Ref. Plot #
Left Head Cheek	836.6	Head	GSM	Integral	Head	Left Head	-	0.432	1.6	1
Left Head Cheek	824.2	Head	GSM	Integral	Head	Left Head	-	0.530	1.6	2
Left Head Cheek	848.8	Head	GSM	Integral	Head	Left Head	-	0.450	1.6	3
Left Head Tilt	836.6	Head	GSM	Integral	Head	Left Head	-	0.149	1.6	4
Right Head Cheek	836.6	Head	GSM	Integral	Head	Right Head	-	0.343	1.6	5
Right Head Tilt	836.6	Head	GSM	Integral	Head	Right Head	-	0.135	1.6	6
Body-Worn Back	836.6	Body	GPRS	Integral	Body	Flat	Headset	0.369	1.6	7
Body-Worn Back	824.2	Body	GPRS	Integral	Body	Flat	Headset	0.349	1.6	8
Body-Worn Back	848.8	Body	GPRS	Integral	Body	Flat	Headset	0.331	1.6	9

PCS Band:

EUT Position	Frequency (MHz)	Test Type	Test Mode	Antenna Type	Liquid	Phantom	Accessories	1g SAR Value (W/Kg)	FCC Limit (W/Kg)	Ref. Plot #
Left Head Cheek	1880.0	Head	GSM	Integral	Head	Left Head	-	0.434	1.6	10
Left Head Tilt	1880.0	Head	GSM	Integral	Head	Left Head	-	0.145	1.6	11
Right Head Cheek	1880.0	Head	GSM	Integral	Head	Right Head	-	0.489	1.6	12
Right Head Cheek	1850.2	Head	GSM	Integral	Head	Right Head	-	0.566	1.6	13
Right Head Cheek	1909.8	Head	GSM	Integral	Head	Right Head	-	0.446	1.6	14
Right Head Tilt	1880.0	Head	GSM	Integral	Head	Right Head	-	0.228	1.6	15
Body-Worn Back	1880.0	Body	GPRS	Integral	Body	Flat	Headset	0.272	1.6	16
Body-Worn Back	1850.2	Body	GPRS	Integral	Body	Flat	Headset	0.308	1.6	17
Body-Worn Back	1909.8	Body	GPRS	Integral	Body	Flat	Headset	0.280	1.6	18

APPENDIX A – MEASUREMENT UNCERTAINTY

The uncertainty budget has been determined for the measurement system and is given in the following Table.

Exposure Assessment Measurement Uncertainty

Source of Uncertainty	Tolerance Value	Probability Distribution	Divisor	c_i^1 (1-g)	c_i^1 (10-g)	Standard Uncertainty (1-g) %	Standard Uncertainty (10-g) %
Measurement System							
Probe Calibration	3.5	normal	1	1	1	3.5	3.5
Axial Isotropy	3.7	rectangular	$\sqrt{3}$	$(1\text{-cp})^{1/2}$	$(1\text{-cp})^{1/2}$	1.5	1.5
Hemispherical Isotropy	10.9	rectangular	$\sqrt{3}$	$\sqrt{cp}$	$\sqrt{cp}$	4.4	4.4
Boundary Effect	1.0	rectangular	$\sqrt{3}$	1	1	0.6	0.6
Linearity	4.7	rectangular	$\sqrt{3}$	1	1	2.7	2.7
Detection Limit	1.0	rectangular	$\sqrt{3}$	1	1	0.6	0.6
Readout Electronics	1.0	normal	1	1	1	1.0	1.0
Response Time	0.8	rectangular	$\sqrt{3}$	1	1	0.5	0.5
Integration Time	1.7	rectangular	$\sqrt{3}$	1	1	1.0	1.0
RF Ambient Condition	3.0	rectangular	$\sqrt{3}$	1	1	1.7	1.7
Probe Positioner Mech.	0.4	rectangular	$\sqrt{3}$	1	1	0.2	0.2
Restriction							
Probe Positioning with respect to Phantom Shell	2.9	rectangular	$\sqrt{3}$	1	1	1.7	1.7
Extrapolation and Integration	3.7	rectangular	$\sqrt{3}$	1	1	2.1	2.1
Test Sample Positioning	4.0	normal	1	1	1	4.0	4.0
Device Holder Uncertainty	2.0	normal	1	1	1	2.0	2.0
Drift of Output Power	3.2	rectangular	$\sqrt{3}$	1	1	1.8	1.8
Phantom and Setup							
Phantom Uncertainty(shape & thickness tolerance)	3.4	rectangular	$\sqrt{3}$	1	1	2.0	2.0
Liquid Conductivity(target)	5.0	rectangular	$\sqrt{3}$	0.7	0.5	2.0	1.4
Liquid Conductivity(meas.)	0.0	normal	1	0.7	0.5	0.0	0.0
Liquid Permittivity(target)	5.0	rectangular	$\sqrt{3}$	0.6	0.5	1.7	1.4
Liquid Permittivity(meas.)	0.0	normal	1	0.6	0.5	0.0	0.0
Combined Uncertainty		RSS				9.4	9.2
Combined Uncertainty (coverage factor=2)		Normal(k=2)				18.8	18.5

APPENDIX B – PROBE CALIBRATION CERTIFICATES

NCL CALIBRATION LABORATORIES

Calibration File No.: CP-871

Client.: BACL

CERTIFICATE OF CALIBRATION

It is certified that the equipment identified below has been calibrated in the **NCL CALIBRATION LABORATORIES** by qualified personnel following recognized procedures and using transfer standards traceable to NRC/NIST.

Equipment: Miniature Isotropic RF Probe 835 MHz

Manufacturer: APREL Laboratories
Model No.: E-020
Serial No.: 273

Calibration Procedure: SSI/DRB-TP-D01-032-E020-V2
Project No: BACB-ALSAS10U-5323

Calibrated: 1st August 2008
Released on: 1st September 2008

This Calibration Certificate is Incomplete Unless Accompanied with the Calibration Results Summary

Released By: _____

NCL CALIBRATION LABORATORIES
51 SPECTRUM WAY
NEPEAN, ONTARIO
CANADA K2R 1E6
Division of APREL Lab.
TEL: (613) 820-4988
FAX: (613) 820-4161

NCL Calibration Laboratories
Division of APREL Laboratories.

Introduction

This Calibration Report reproduces the results of the calibration performed in line with the SSI/DRB-TP-D01-032-E020-V2 E-Field Probe Calibration Procedure. The results contained within this report are for APREL E-Field Probe E-020 273.

References

SSI/DRB-TP-D01-032-E020-V2 E-Field Probe Calibration Procedure
IEEE 1528 "Recommended Practice for Determining the Peak Spatial-Average Specific Absorption Rate (SAR) in the Human Body Due to Wireless Communications Devices: Experimental Techniques"
SSI-TP-011 Tissue Calibration Procedure

Conditions

Probe 273 was a new probe taken from stock prior to calibration.

Ambient Temperature of the Laboratory: 22 °C +/- 0.5°C
Temperature of the Tissue: 21 °C +/- 0.5°C

We the undersigned attest that to the best of our knowledge the calibration of this probe has been accurately conducted and that all information contained within this report has been reviewed for accuracy.

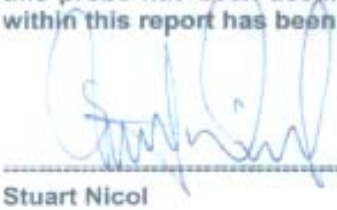

Stuart Nicol

Jesse Hones

NCL Calibration Laboratories
Division of APREL Laboratories.

Calibration Results Summary

Probe Type:	E-Field Probe E-020
Serial Number:	273
Frequency:	835 MHz
Sensor Offset:	1.56 mm
Sensor Length:	2.5 mm
Tip Enclosure:	Ertalyte*
Tip Diameter:	<5 mm
Tip Length:	60 mm
Total Length:	290 mm

*Resistive to recommended tissue recipes per IEEE-1528

Sensitivity in Air

Channel X:	1.2 $\mu V/(V/m)^2$
Channel Y:	1.2 $\mu V/(V/m)^2$
Channel Z:	1.2 $\mu V/(V/m)^2$
Diode Compression Point:	95 mV

Page 3 of 10
This page has been reviewed for content and attested to on Page 2 of this document.

Sensitivity in Head Tissue Measured

Frequency: 835 MHz

Epsilon: 41.24 (+/-5%) **Sigma:** 0.87 S/m (+/-5%)

ConvF

Channel X: 6.5

Channel Y: 6.5

Channel Z: 6.5

Tissue sensitivity values were calculated using the load impedance of the APREL Laboratories Daq-Paq.

Boundary Effect:

Uncertainty resulting from the boundary effect is less than 2% for the distance between the tip of the probe and the tissue boundary, when less than 2.44mm.

Spatial Resolution:

The measured probe tip diameter is 5 mm (+/- 0.01 mm) and therefore meets the requirements of SSI/DRB-TP-D01-032 for spatial resolution.

NCL Calibration Laboratories
Division of APREL Laboratories.

Receiving Pattern 835 MHz (Air)

This page has been reviewed for content and attested to on Page 2 of this document.

NCL Calibration Laboratories
Division of APREL Laboratories.

Isotropy Error 835 MHz (Air)

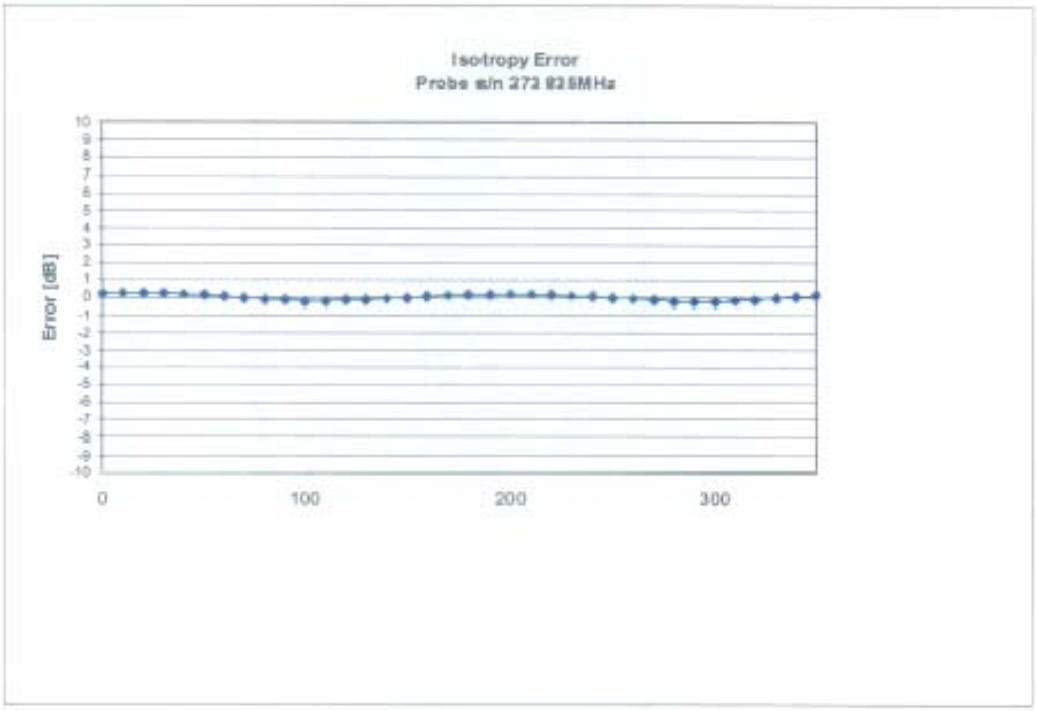

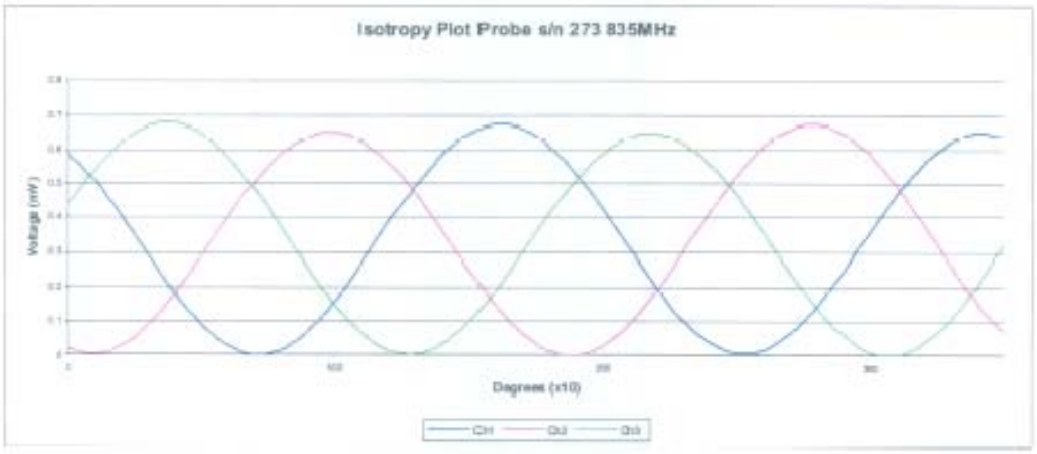

Isotropicity Tissue: 0.10 dB

NCL Calibration Laboratories
Division of APREL Laboratories.

Dynamic Range

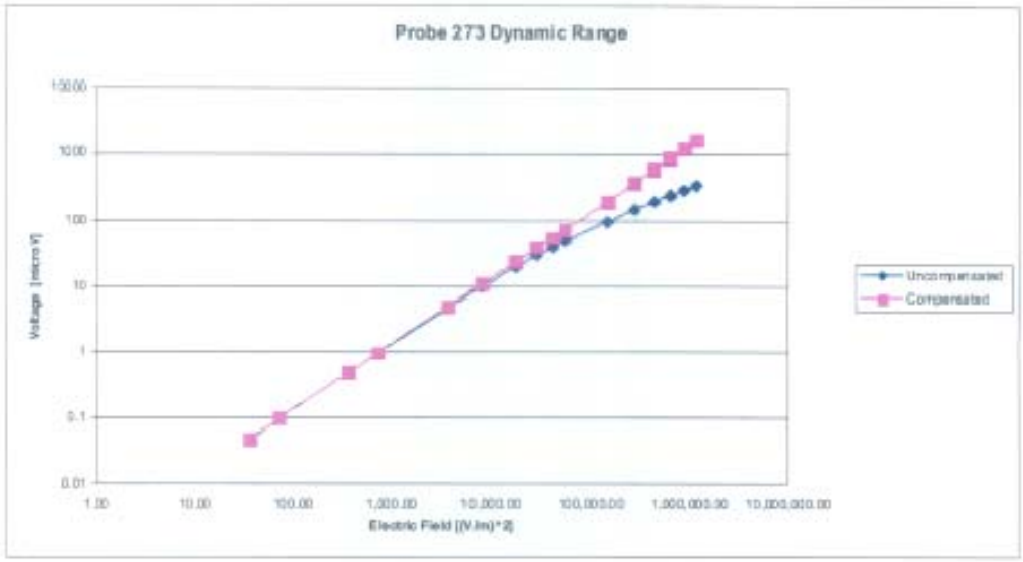

Video Bandwidth

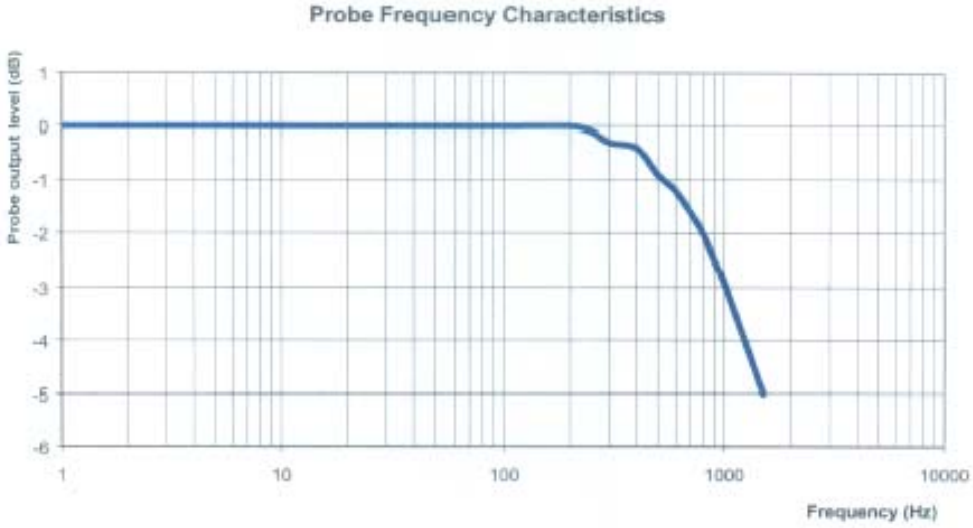

Video Bandwidth at 500 Hz 1 dB
Video Bandwidth at 1.02 KHz: 3 dB

NCL Calibration Laboratories
Division of APREL Laboratories.

Conversion Factor Uncertainty Assessment

Frequency:		835MHz	
Epsilon:	41.24 (+/-5%)	**Sigma:**	0.87 S/m (+/-5%)
ConvF			
Channel X:	6.5	7%(K=2)	
Channel Y:	6.5	7%(K=2)	
Channel Z:	6.5	7%(K=2)	

To minimize the uncertainty calculation all tissue sensitivity values were calculated using a load impedance of 5 MΩ.

Boundary Effect:

For a distance of 2.5mm the evaluated uncertainty (increase in the probe sensitivity) is less than 2%.

NCL Calibration Laboratories
Division of APREL Laboratories.

Test Equipment

The test equipment used during Probe Calibration, manufacturer, model number and, current calibration status are listed and located on the main APREL server R:\NCL\Calibration Equipment\Instrument List May 2008.

NCL CALIBRATION LABORATORIES

Calibration File No.: CP-872

Client.: BACL

CERTIFICATE OF CALIBRATION

It is certified that the equipment identified below has been calibrated in the **NCL CALIBRATION LABORATORIES** by qualified personnel following recognized procedures and using transfer standards traceable to NRC/NIST.

Equipment: Miniature Isotropic RF Probe 835 MHz

Manufacturer: APREL Laboratories
Model No.: E-020
Serial No.: 273

Calibration in Body Tissue

Calibration Procedure: SSI/DRB-TP-D01-032-E020-V2
Project No: BACL-ALSAS10U-5323

Calibrated: 1st September 2008
Released on: 1st September 2008

This Calibration Certificate is Incomplete Unless Accompanied with the Calibration Results Summary

Released By: _____

NCL CALIBRATION LABORATORIES

51 SPECTRUM WAY
NEPEAN, ONTARIO
CANADA K2R 1E6

Division of APREL Lab.
TEL: (613) 820-4988
FAX: (613) 820-4161

NCL Calibration Laboratories
Division of APREL Laboratories.

Introduction

This Calibration Report reproduces the results of the calibration performed in line with the SSI/DRB-TP-D01-032-E020-V2 E-Field Probe Calibration Procedure. The results contained within this report are for APREL E-Field Probe E-020 273.

References

SSI/DRB-TP-D01-032-E020-V2 E-Field Probe Calibration Procedure
IEEE 1528 "Recommended Practice for Determining the Peak Spatial-Average Specific Absorption Rate (SAR) in the Human Body Due to Wireless Communications Devices: Experimental Techniques"
SSI-TP-011 Tissue Calibration Procedure

Conditions

Probe 273 was a new probe taken from stock prior to calibration.

Ambient Temperature of the Laboratory:	22 °C +/- 0.5°C
Temperature of the Tissue:	21 °C +/- 0.5°C

We the undersigned attest that to the best of our knowledge the calibration of this probe has been accurately conducted and that all information contained within this report has been reviewed for accuracy.

Stuart Nicol

Jesse Hones

Page 2 of 10
This page has been reviewed for content and attested to on Page 2 of this document.

NCL Calibration Laboratories
Division of APREL Laboratories.

Calibration Results Summary

Probe Type:	E-Field Probe E-020
Serial Number:	273
Frequency:	835 MHz
Sensor Offset:	1.56 mm
Sensor Length:	2.5 mm
Tip Enclosure:	Ertalyte*
Tip Diameter:	<5 mm
Tip Length:	60 mm
Total Length:	290 mm

*Resistive to recommended tissue recipes per IEEE-1528

Sensitivity in Air

Channel X:	1.2 $\mu V/(V/m)^2$
Channel Y:	1.2 $\mu V/(V/m)^2$
Channel Z:	1.2 $\mu V/(V/m)^2$
Diode Compression Point:	95 mV

Page 3 of 10
This page has been reviewed for content and attested to on Page 2 of this document.

Sensitivity in Body Tissue Measured

Frequency: 835 MHz

Epsilon: 56.16 (+/-5%) **Sigma:** 0.99 S/m (+/-10%)

ConvF

Channel X: 6.7

Channel Y: 6.7

Channel Z: 6.7

Tissue sensitivity values were calculated using the load impedance of the APREL Laboratories Daq-Paq.

Boundary Effect:

Uncertainty resulting from the boundary effect is less than 2% for the distance between the tip of the probe and the tissue boundary, when less than 2.44mm.

Spatial Resolution:

The measured probe tip diameter is 5 mm (+/- 0.01 mm) and therefore meets the requirements of SSI/DRB-TP-D01-032 for spatial resolution.

NCL Calibration Laboratories
Division of APREL Laboratories.

Receiving Pattern 835 MHz (Air)

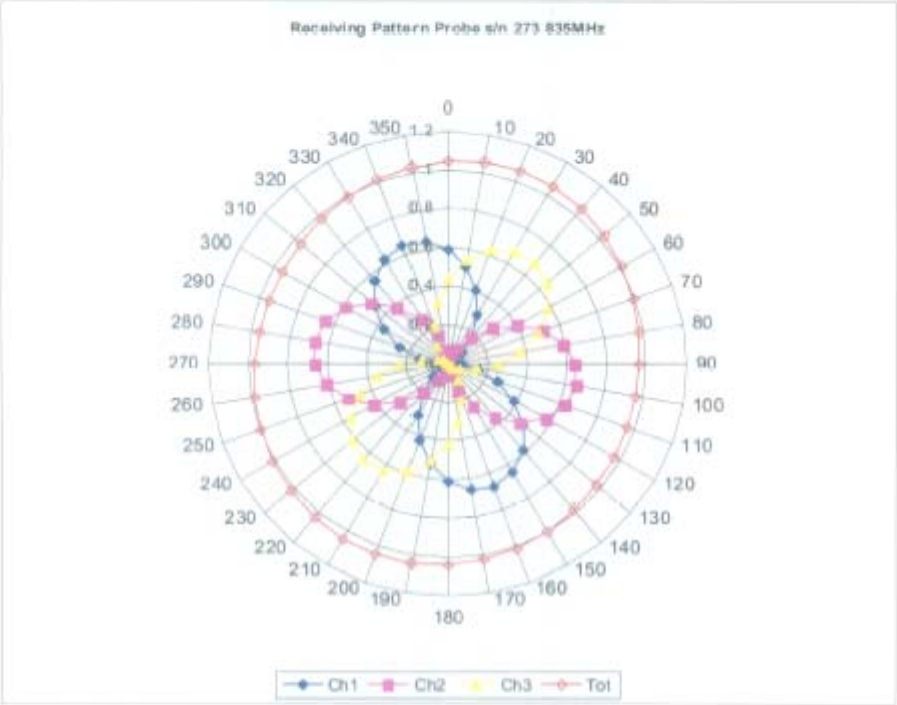

Page 5 of 10
This page has been reviewed for content and attested to on Page 2 of this document.

NCL Calibration Laboratories
Division of APREL Laboratories.

Isotropy Error 835 MHz (Air)

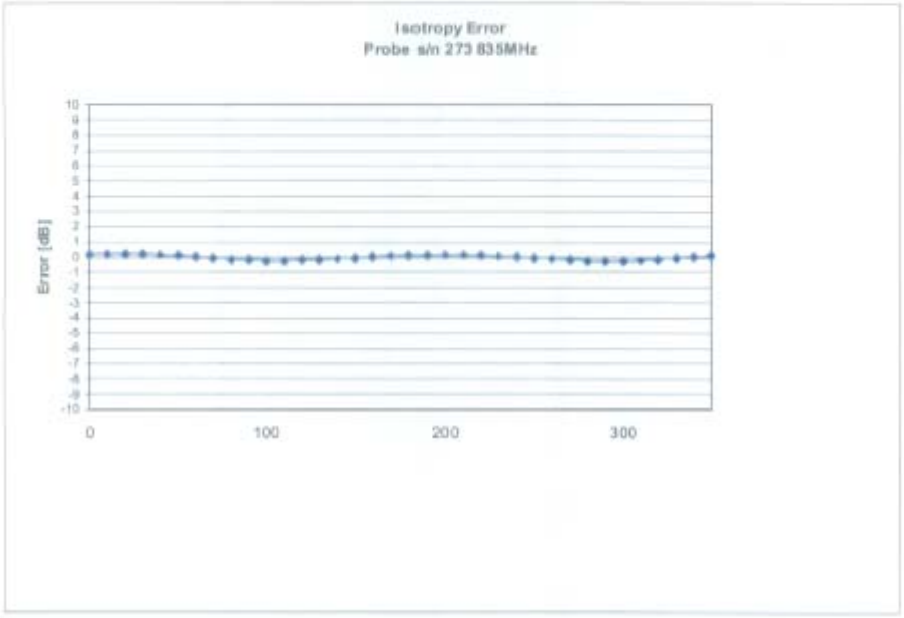

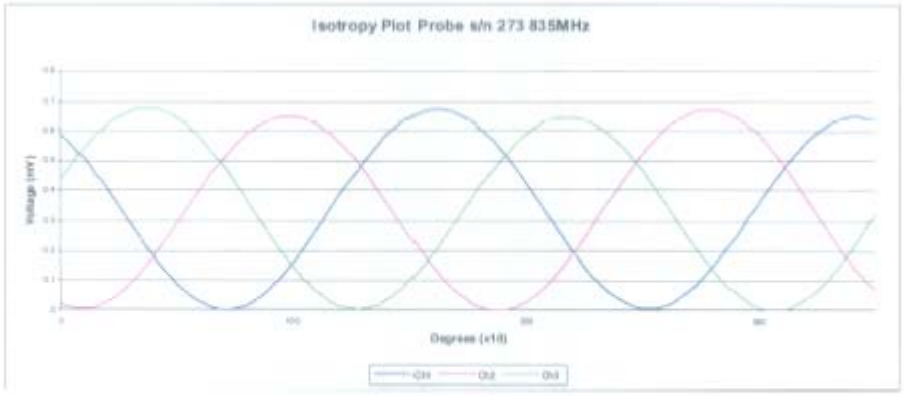

Isotropicity in Tissue: 0.10 dB

This page has been reviewed for content and attested to on Page 2 of this document.

NCL Calibration Laboratories
Division of APREL Laboratories.

Dynamic Range

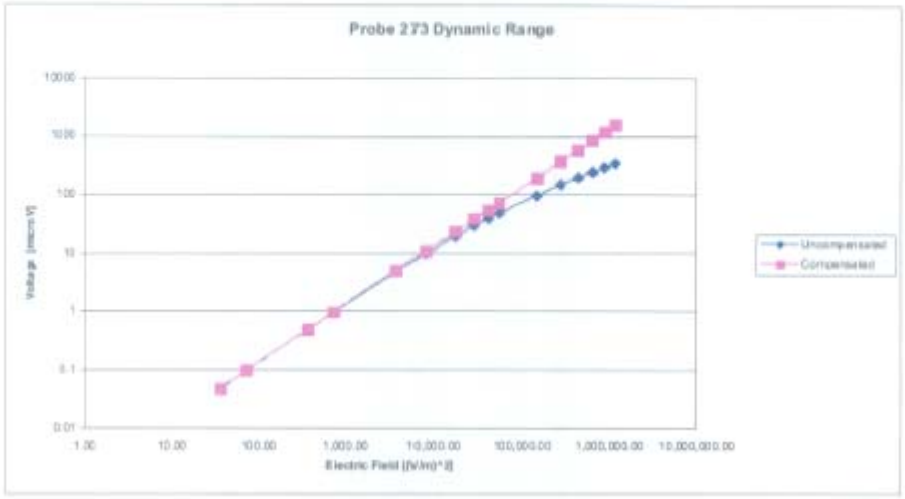

Page 7 of 10
This page has been reviewed for content and attested to on Page 2 of this document.

Video Bandwidth

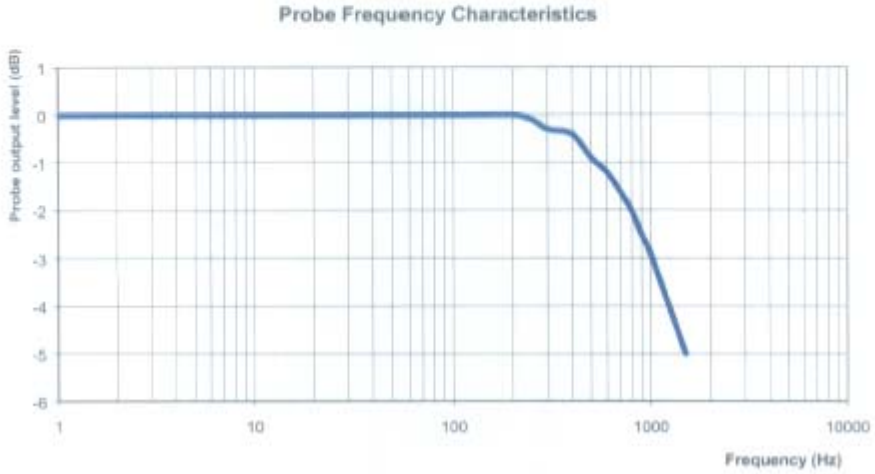

Video Bandwidth at 500 Hz 1 dB
Video Bandwidth at 1.02 KHz: 3 dB

NCL Calibration Laboratories
Division of APREL Laboratories.

Conversion Factor Uncertainty Assessment

Frequency:		835MHz	
Epsilon:	56.16 (+/-5%)	**Sigma:**	0.99 S/m (+/-10%)
ConvF			
Channel X:	6.7	7%(K=2)	
Channel Y:	6.7	7%(K=2)	
Channel Z:	6.7	7%(K=2)	

To minimize the uncertainty calculation all tissue sensitivity values were calculated using a load impedance of 5 MΩ.

Boundary Effect:

For a distance of 2.4mm the evaluated uncertainty (increase in the probe sensitivity) is less than 2%.

NCL Calibration Laboratories
Division of APREL Laboratories.

Test Equipment

The test equipment used during Probe Calibration, manufacturer, model number and, current calibration status are listed and located on the main APREL server R:\NCL\Calibration Equipment\Instrument List May 2008.

NCL CALIBRATION LABORATORIES

Calibration File No.: CP-877

Client.: BACL

CERTIFICATE OF CALIBRATION

It is certified that the equipment identified below has been calibrated in the **NCL CALIBRATION LABORATORIES** by qualified personnel following recognized procedures and using transfer standards traceable to NRC/NIST.

Equipment: Miniature Isotropic RF Probe 1900 MHz

Manufacturer: APREL Laboratories
Model No.: E-020
Serial No.: 273

Calibration Procedure: SSI/DRB-TP-D01-032-E020-V2
Project No: BACB-ALSAS10U-5323

Calibrated: 1st August 2008
Released on: 1st September 2008

This Calibration Certificate is Incomplete Unless Accompanied with the Calibration Results Summary

Released By:

NCL CALIBRATION LABORATORIES
51 SPECTRUM WAY
NEPEAN, ONTARIO
CANADA K2R 1E6
Division of APREL Lab.
TEL: (613) 820-4988
FAX: (613) 820-4161

NCL Calibration Laboratories
Division of APREL Laboratories.

Introduction

This Calibration Report reproduces the results of the calibration performed in line with the SSI/DRB-TP-D01-032-E020-V2 E-Field Probe Calibration Procedure. The results contained within this report are for APREL E-Field Probe E-020 273.

References

SSI/DRB-TP-D01-032-E020-V2 E-Field Probe Calibration Procedure
IEEE 1528 "Recommended Practice for Determining the Peak Spatial-Average Specific Absorption Rate (SAR) in the Human Body Due to Wireless Communications Devices: Experimental Techniques"
SSI-TP-011 Tissue Calibration Procedure

Conditions

Probe 273 was a new probe taken from stock prior to calibration.

Ambient Temperature of the Laboratory:	22 °C +/- 0.5°C
Temperature of the Tissue:	21 °C +/- 0.5°C

We the undersigned attest that to the best of our knowledge the calibration of this probe has been accurately conducted and that all information contained within this report has been reviewed for accuracy.

Stuart Nicol

Jesse Hones

NCL Calibration Laboratories
Division of APREL Laboratories.

Calibration Results Summary

Probe Type:	E-Field Probe E-020
Serial Number:	273
Frequency:	1900 MHz
Sensor Offset:	1.56 mm
Sensor Length:	2.5 mm
Tip Enclosure:	Ertalyte*
Tip Diameter:	<5 mm
Tip Length:	60 mm
Total Length:	290 mm

*Resistive to recommended tissue recipes per IEEE-1528

Sensitivity in Air

Channel X:	1.2 $\mu V/(V/m)^2$
Channel Y:	1.2 $\mu V/(V/m)^2$
Channel Z:	1.2 $\mu V/(V/m)^2$
Diode Compression Point:	95 mV

Page 3 of 10
This page has been reviewed for content and attested to on Page 2 of this document.

NCL Calibration Laboratories
Division of APREL Laboratories.

Sensitivity in Head Tissue Measured

Frequency: 1900 MHz

Epsilon: 38.50 (+/-5%) **Sigma:** 1.40 S/m (+/-5%)

ConvF

Channel X: 5.25

Channel Y: 5.25

Channel Z: 5.25

Tissue sensitivity values were calculated using the load impedance of the APREL Laboratories Daq-Paq.

Boundary Effect:

Uncertainty resulting from the boundary effect is less than 2% for the distance between the tip of the probe and the tissue boundary, when less than 2.44mm.

Spatial Resolution:

The measured probe tip diameter is 5 mm (+/- 0.01 mm) and therefore meets the requirements of SSI/DRB-TP-D01-032 for spatial resolution.

Page 4 of 10
This page has been reviewed for content and attested to on Page 2 of this document.

NCL Calibration Laboratories
Division of APREL Laboratories.

Receiving Pattern 1900 MHz (Air)

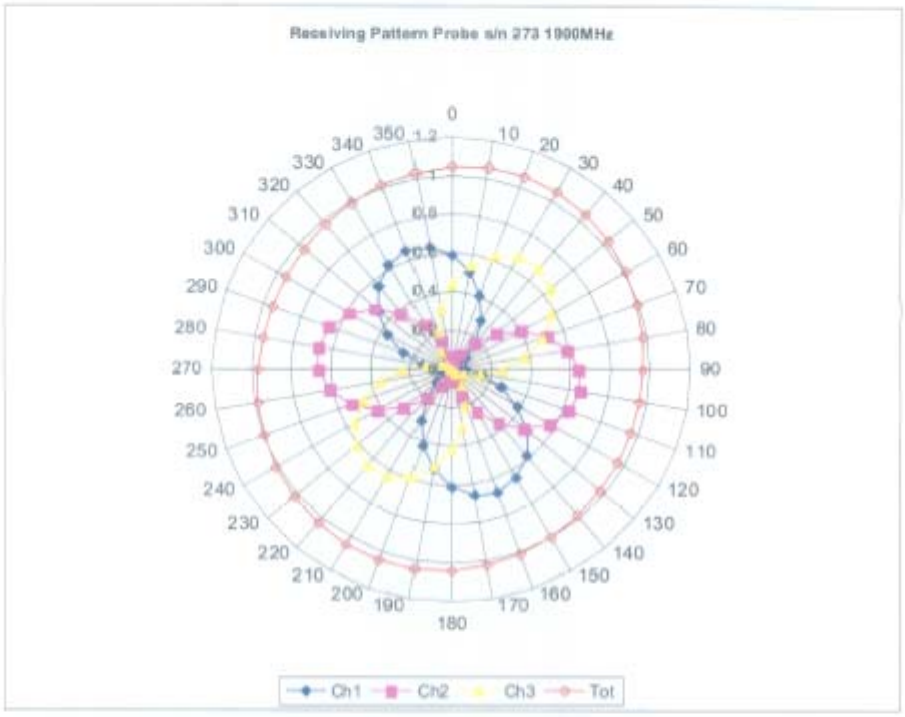

This page has been reviewed for content and attested to on Page 2 of this document.

Isotropy Error 1900 MHz (Air)

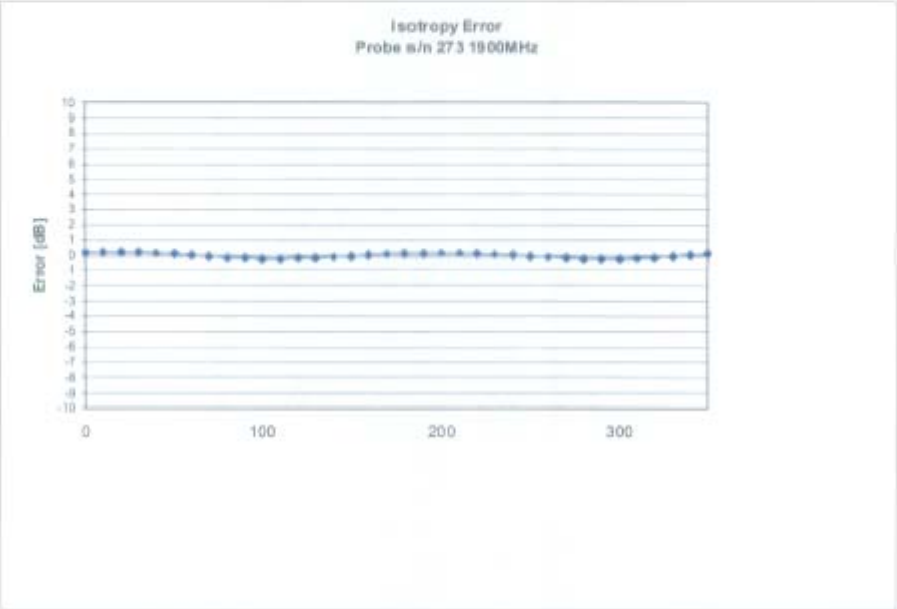

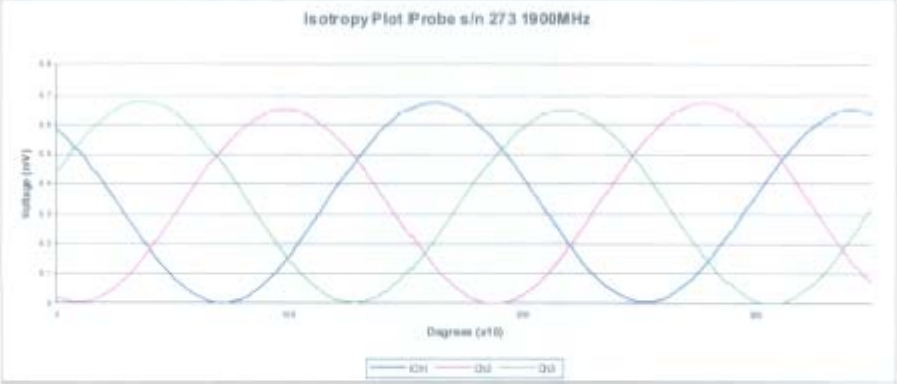

Isotropicity in Tissue: 0.10 dB

NCL Calibration Laboratories
Division of APREL Laboratories.

Dynamic Range

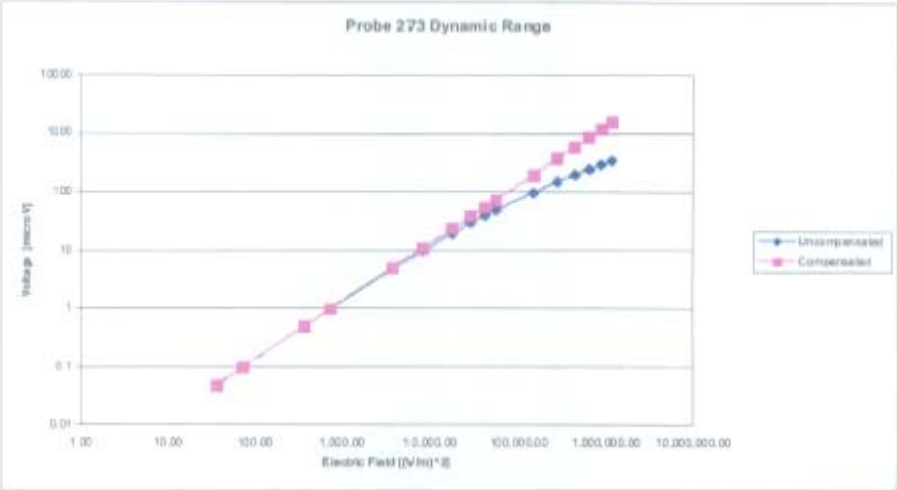

Page 7 of 10
This page has been reviewed for content and attested to on Page 2 of this document.

Video Bandwidth

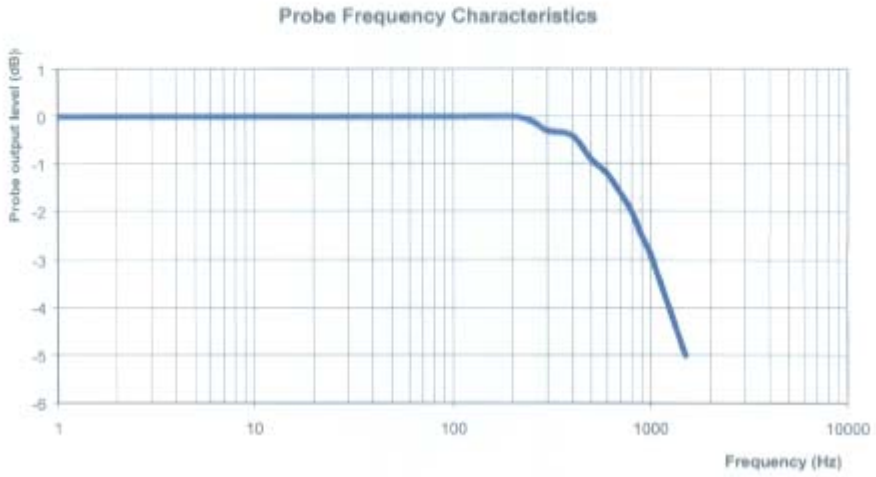

Video Bandwidth at 500 Hz 1 dB
Video Bandwidth at 1.02 KHz: 3 dB

NCL Calibration Laboratories
Division of APREL Laboratories.

Conversion Factor Uncertainty Assessment

Frequency:		1900MHz	
Epsilon:	38.50 (+/-5%)	**Sigma:**	1.40 S/m (+/-5%)
ConvF			
Channel X:	5.25	7%(K=2)	
Channel Y:	5.25	7%(K=2)	
Channel Z:	5.25	7%(K=2)	

To minimize the uncertainty calculation all tissue sensitivity values were calculated using a load impedance of 5 MΩ.

Boundary Effect:

For a distance of 2.4mm the evaluated uncertainty (increase in the probe sensitivity) is less than 2%.

Page 9 of 10
This page has been reviewed for content and attested to on Page 2 of this document.

NCL Calibration Laboratories
Division of APREL Laboratories.

Test Equipment

The test equipment used during Probe Calibration, manufacturer, model number and, current calibration status are listed and located on the main APREL server R:\NCL\Calibration Equipment\Instrument List May 2008.

NCL CALIBRATION LABORATORIES

Calibration File No.: CP-278

Client.: BACL

CERTIFICATE OF CALIBRATION

It is certified that the equipment identified below has been calibrated in the **NCL CALIBRATION LABORATORIES** by qualified personnel following recognized procedures and using transfer standards traceable to NRC/NIST.

Equipment: Miniature Isotropic RF Probe 1900 MHz

Manufacturer: APREL Laboratories
Model No.: E-020
Serial No.: 273

Calibration in Body Tissue

Calibration Procedure: SSI/DRB-TP-D01-032-E020-V2
Project No: BACB-ALSAS10U-5323

Calibrated: 1st August 2008
Released on: 1st September 2008

This Calibration Certificate is Incomplete Unless Accompanied with the Calibration Results Summary

Released By: _____

NCL CALIBRATION LABORATORIES
51 SPECTRUM WAY
NEPEAN, ONTARIO
CANADA K2R 1E6
Division of APREL Lab.
TEL: (613) 820-4988
FAX: (613) 820-4161

NCL Calibration Laboratories
Division of APREL Laboratories.

Introduction

This Calibration Report reproduces the results of the calibration performed in line with the SSI/DRB-TP-D01-032-E020-V2 E-Field Probe Calibration Procedure. The results contained within this report are for APREL E-Field Probe E-020 273.

References

SSI/DRB-TP-D01-032-E020-V2 E-Field Probe Calibration Procedure
IEEE 1528 "Recommended Practice for Determining the Peak Spatial-Average Specific Absorption Rate (SAR) in the Human Body Due to Wireless Communications Devices: Experimental Techniques"
SSI-TP-011 Tissue Calibration Procedure

Conditions

Probe 273 was a new probe taken from stock prior to calibration.

Ambient Temperature of the Laboratory:	22 °C +/- 0.5°C
Temperature of the Tissue:	21 °C +/- 0.5°C

We the undersigned attest that to the best of our knowledge the calibration of this probe has been accurately conducted and that all information contained within this report has been reviewed for accuracy.

Stuart Nicol

Jesse Hones

Page 2 of 10
This page has been reviewed for content and attested to on Page 2 of this document.

NCL Calibration Laboratories
Division of APREL Laboratories.

Calibration Results Summary

Probe Type:	E-Field Probe E-020
Serial Number:	273
Frequency:	1900 MHz
Sensor Offset:	1.56 mm
Sensor Length:	2.5 mm
Tip Enclosure:	Ertalyte*
Tip Diameter:	<5 mm
Tip Length:	60 mm
Total Length:	290 mm

*Resistive to recommended tissue recipes per IEEE-1528

Sensitivity in Air

Channel X:	1.2 $\mu V/(V/m)^2$
Channel Y:	1.2 $\mu V/(V/m)^2$
Channel Z:	1.2 $\mu V/(V/m)^2$
Diode Compression Point:	95 mV

Page 3 of 10
This page has been reviewed for content and attested to on Page 2 of this document.

Sensitivity in Body Tissue Measured

Frequency: 1900 MHz

Epsilon: 53.05 (+/-5%) **Sigma:** 1.58 S/m (+/-5%)

ConvF

Channel X: 5.15

Channel Y: 5.15

Channel Z: 5.15

Tissue sensitivity values were calculated using the load impedance of the APREL Laboratories Daq-Paq.

Boundary Effect:

Uncertainty resulting from the boundary effect is less than 2% for the distance between the tip of the probe and the tissue boundary, when less than 2.44mm.

Spatial Resolution:

The measured probe tip diameter is 5 mm (+/- 0.01 mm) and therefore meets the requirements of SSI/DRB-TP-D01-032 for spatial resolution.

NCL Calibration Laboratories
Division of APREL Laboratories.

Receiving Pattern 1900 MHz (Air)

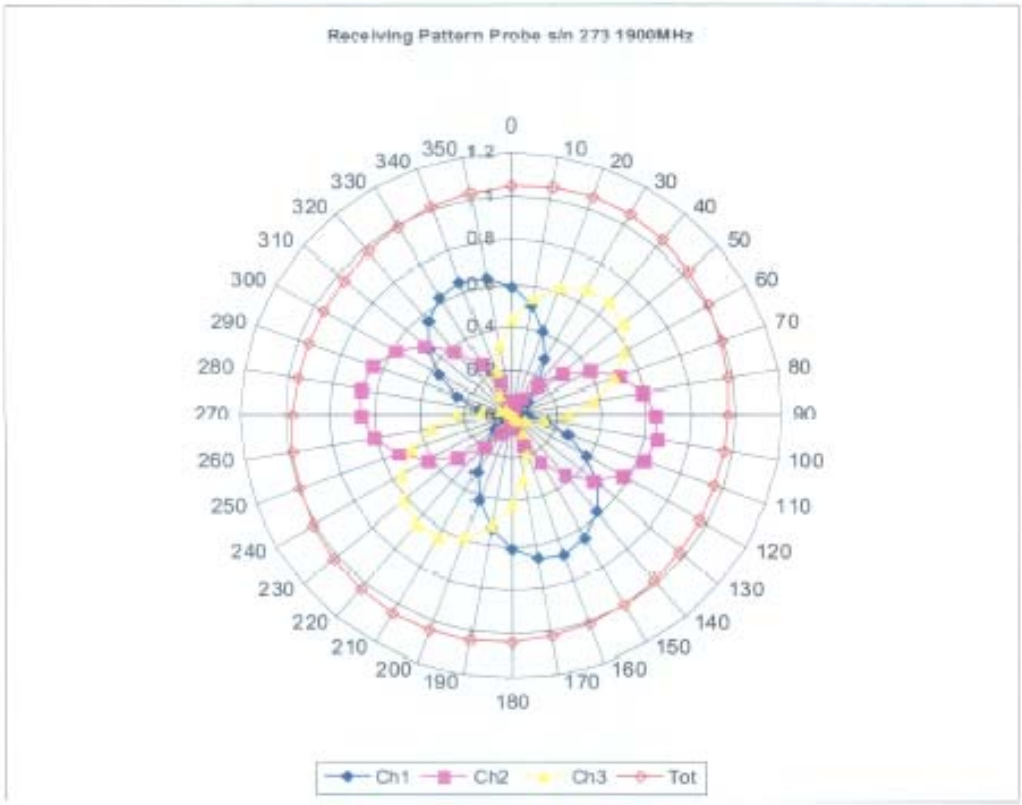

This page has been reviewed for content and attested to on Page 2 of this document.

NCL Calibration Laboratories
Division of APREL Laboratories.

Isotropy Error 1900 MHz (Air)

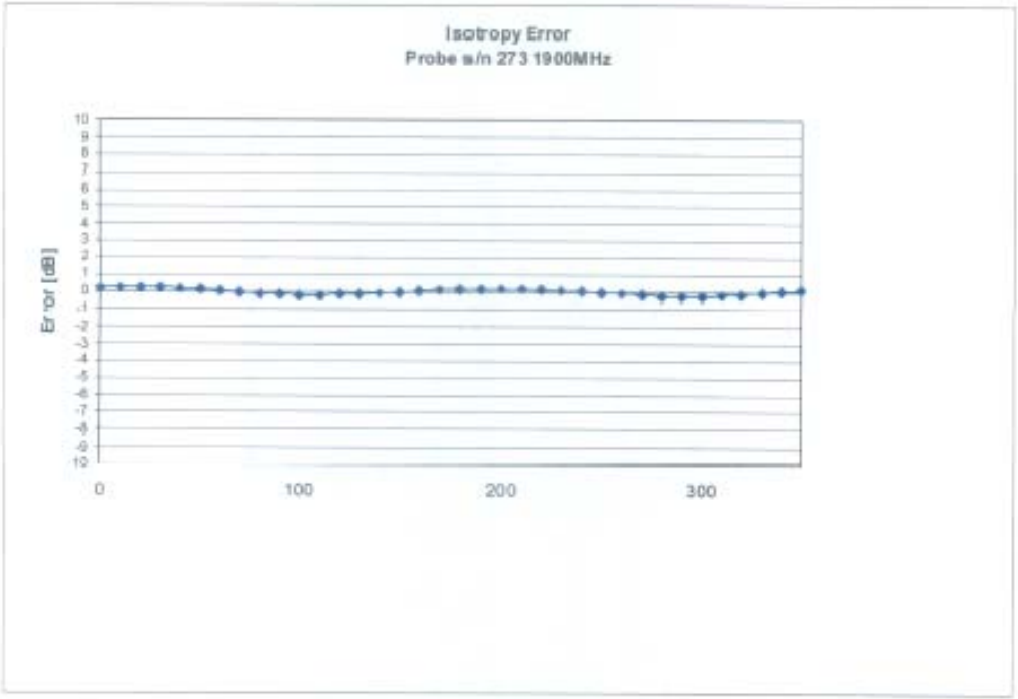

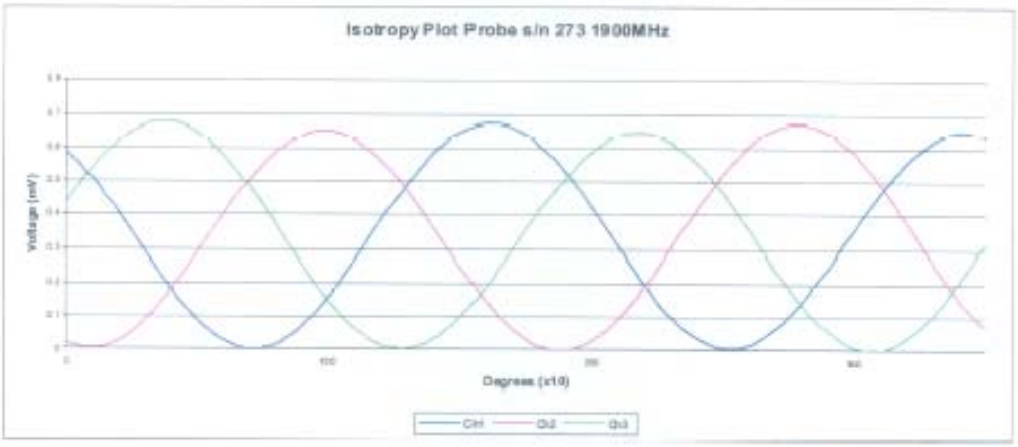

Isotropicity in Tissue: 0.10 dB

Page 6 of 10
This page has been reviewed for content and attested to on Page 2 of this document.

NCL Calibration Laboratories
Division of APREL Laboratories.

Dynamic Range

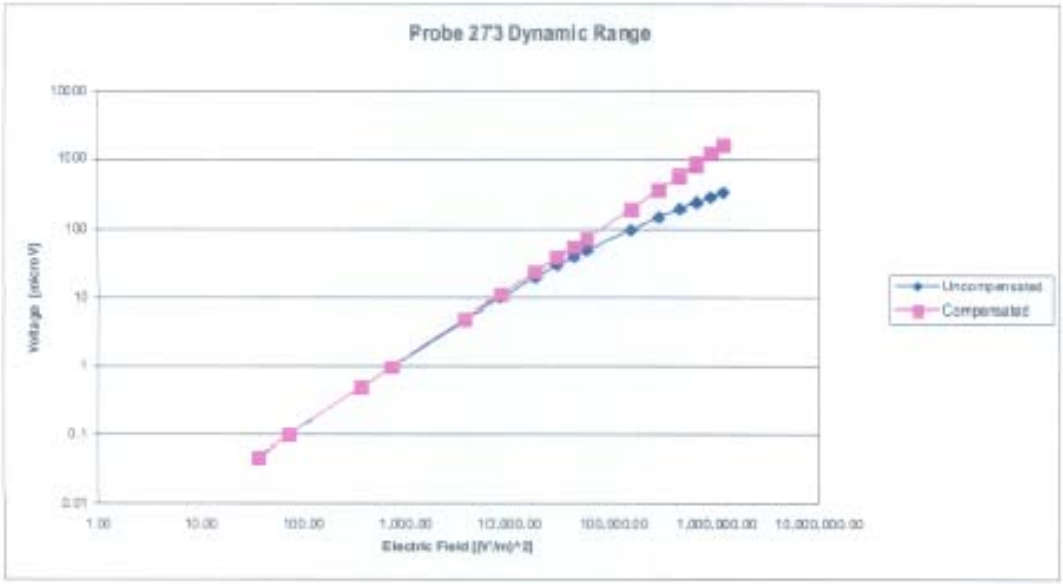

Video Bandwidth

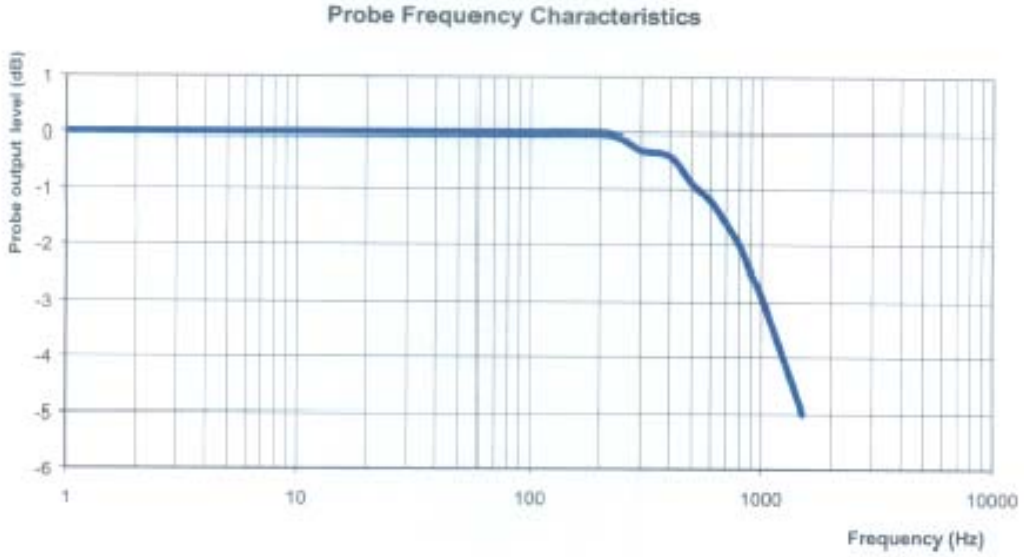

Video Bandwidth at 500 Hz 1 dB
Video Bandwidth at 1.02 KHz: 3 dB

NCL Calibration Laboratories
Division of APREL Laboratories.

Conversion Factor Uncertainty Assessment

Frequency:		1900MHz	
Epsilon:	53.05 (+/-5%)	**Sigma:**	1.58 S/m (+/-5%)
ConvF			
Channel X:	5.15	7%(K=2)	
Channel Y:	5.15	7%(K=2)	
Channel Z:	5.15	7%(K=2)	

To minimize the uncertainty calculation all tissue sensitivity values were calculated using a load impedance of 5 MΩ.

Boundary Effect:

For a distance of 2.4mm the evaluated uncertainty (increase in the probe sensitivity) is less than 2%.

Test Equipment

The test equipment used during Probe Calibration, manufacturer, model number and, current calibration status are listed and located on the main APREL server R:\NCL\Calibration Equipment\Instrument List May 2008.

APPENDIX C – DIPOLE CALIBRATION CERTIFICATES

NCL CALIBRATION LABORATORIES

Calibration File No: DC-917
Project Number: BACL-ALSAS10U-5323

CERTIFICATE OF CALIBRATION

It is certified that the equipment identified below has been calibrated in the **NCL CALIBRATION LABORATORIES** by qualified personnel following recognized procedures and using transfer standards traceable to NRC/NIST.

Validation Dipole

Manufacturer: APREL Laboratories
Part number: ALS-D-835-S-2
Frequency: 835 MHz
Serial No: 180-00558

Customer: Bay Area Compliance Laboratory

Calibrated: 1st September 2008
Released on: 1st September 2008

This Calibration Certificate is Incomplete Unless Accompanied with the Calibration Results Summary

Released By: _____

NCL CALIBRATION LABORATORIES

51 SPECTRUM WAY
NEPEAN, ONTARIO
CANADA K2R 1E6

Division of APREL Lab.
TEL: (613) 820-4988
FAX: (613) 820-4162

NCL Calibration Laboratories
Division of APREL Laboratories.

Conditions

Dipole 180-00558 was new and taken from stock prior to calibration.

Ambient Temperature of the Laboratory:	22 °C +/- 0.5°C
Temperature of the Tissue:	21 °C +/- 0.5°C

We the undersigned attest that to the best of our knowledge the calibration of this device has been accurately conducted and that all information contained within this report has been reviewed for accuracy.

Stuart Nicol

C. Teodorian

This page has been reviewed for content and attested to by signature within this document.

NCL Calibration Laboratories
Division of APREL Laboratories.

Calibration Results Summary

The following results relate the Calibrated Dipole and should be used as a quick reference for the user.

Mechanical Dimensions

Length: 162.2 mm
Height: 89.4 mm

Electrical Specification

SWR: 1.018 U
Return Loss: -41.371 dB
Impedance: 51.739 Ω

System Validation Results

Frequency	1 Gram	10 Gram	Peak
835 MHz	9.49	6.1	14.21

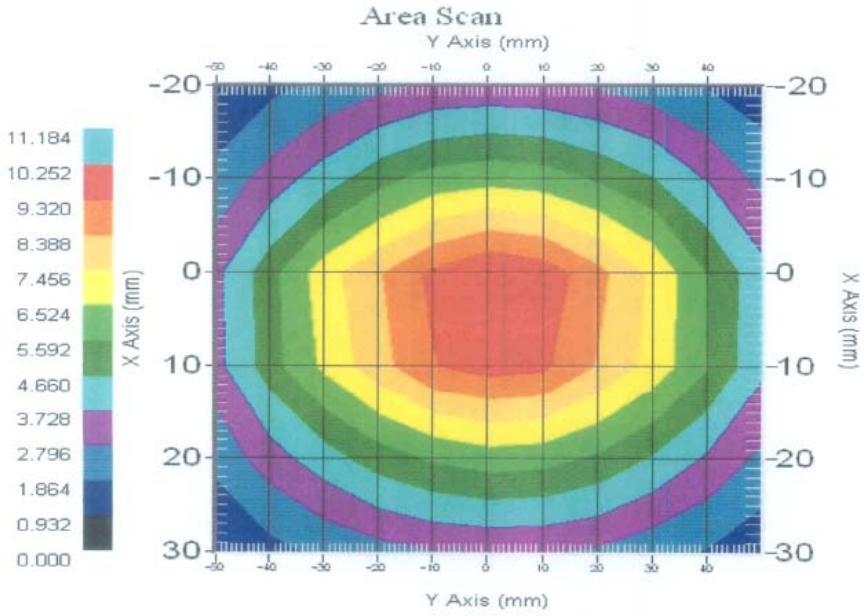

3

This page has been reviewed for content and attested to by signature within this document.

NCL Calibration Laboratories
Division of APREL Laboratories.

Introduction

This Calibration Report has been produced in line with the SSI Dipole Calibration Procedure SSI-TP-018-ALSAS. The results contained within this report are for Validation Dipole 180-00558. The calibration routine consisted of a three-step process. Step 1 was a mechanical verification of the dipole to ensure that it meets the mechanical specifications. Step 2 was an Electrical Calibration for the Validation Dipole, where the SWR, Impedance, and the Return loss were assessed. Step 3 involved a System Validation using the ALSAS-10U, along with APREL E-020 130 MHz to 26 GHz E-Field Probe Serial Number 212.

References

SSI-TP-018-ALSAS Dipole Calibration Procedure
SSI-TP-016 Tissue Calibration Procedure
IEEE 1528 "Recommended Practice for Determining the Peak Spatial-Average Specific Absorption Rate (SAR) in the Human Body Due to Wireless Communications Devices: Experimental Techniques"

Conditions

Dipole 180-00558 was new taken from stock.

Ambient Temperature of the Laboratory:	22 °C +/- 0.5°C
Temperature of the Tissue:	20 °C +/- 0.5°C

This page has been reviewed for content and attested to by signature within this document.

NCL Calibration Laboratories
Division of APREL Laboratories.

Dipole Calibration Results

Mechanical Verification

APREL Length	APREL Height	Measured Length	Measured Height
161.0 mm	89.8 mm	162.2 mm	89.4 mm

Tissue Validation

Head Tissue 835MHz	Measured
Dielectric constant, ε_r	41.12
Conductivity, σ [S/m]	0.92

5

This page has been reviewed for content and attested to by signature within this document.

NCL Calibration Laboratories
Division of APREL Laboratories.

Electrical Calibration

Test	Result
S11 RL	-41.371 dB
SWR	1.018 U
Impedance	51.739 Ω

The Following Graphs are the results as displayed on the Vector Network Analyzer.

S11 Parameter Return Loss

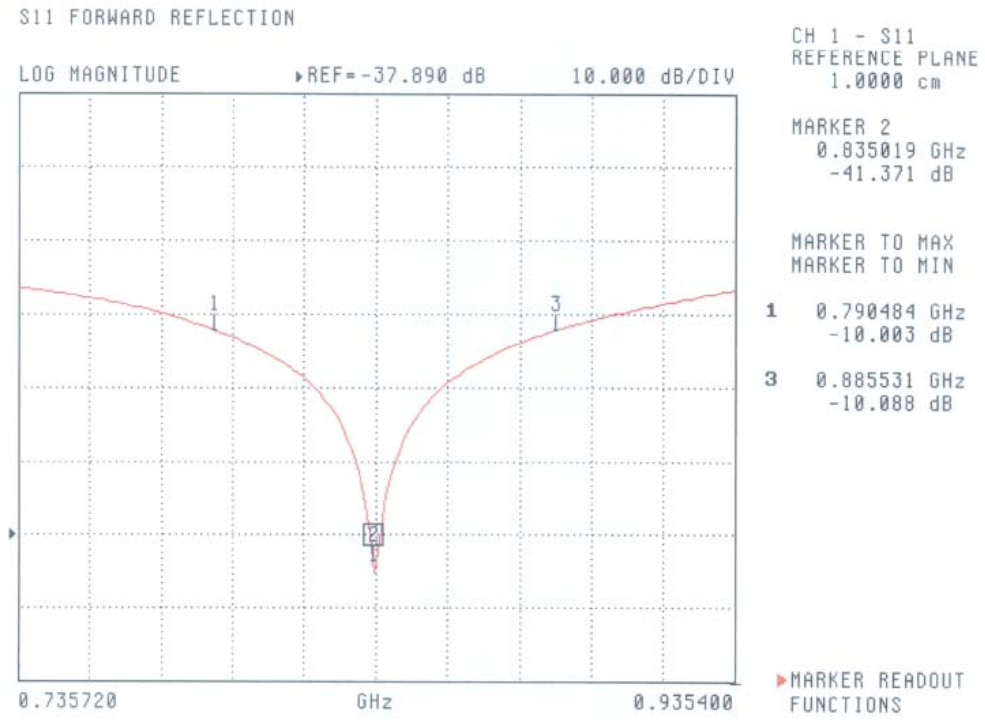

This page has been reviewed for content and attested to by signature within this document.

6

NCL Calibration Laboratories
Division of APREL Laboratories.

SWR

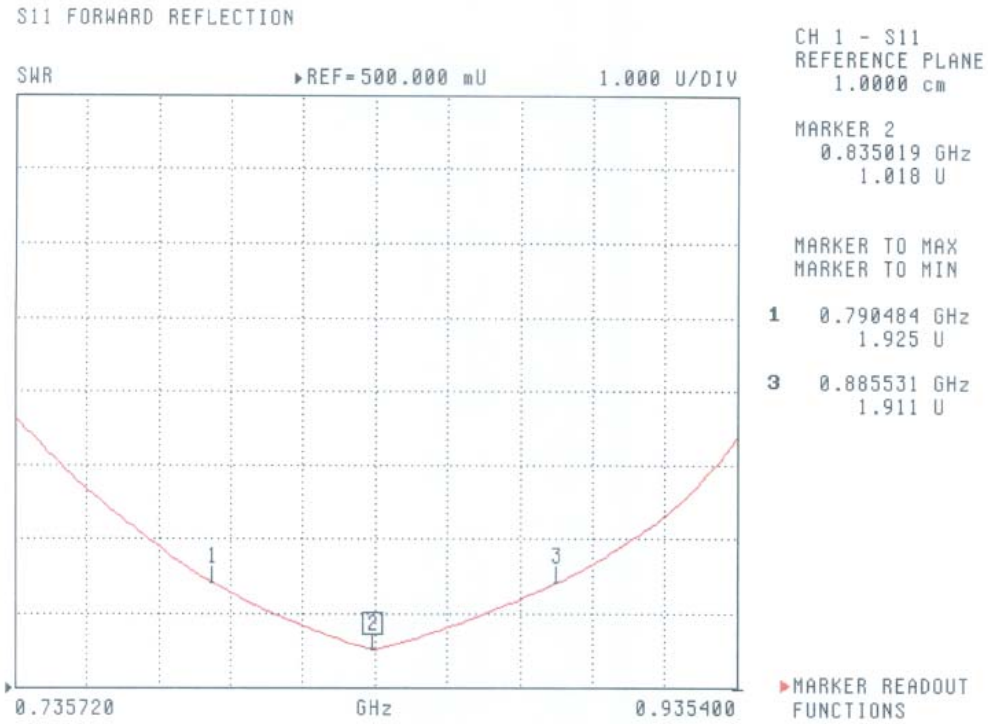

7

This page has been reviewed for content and attested to by signature within this document.

NCL Calibration Laboratories
Division of APREL Laboratories.

Smith Chart Dipole Impedance

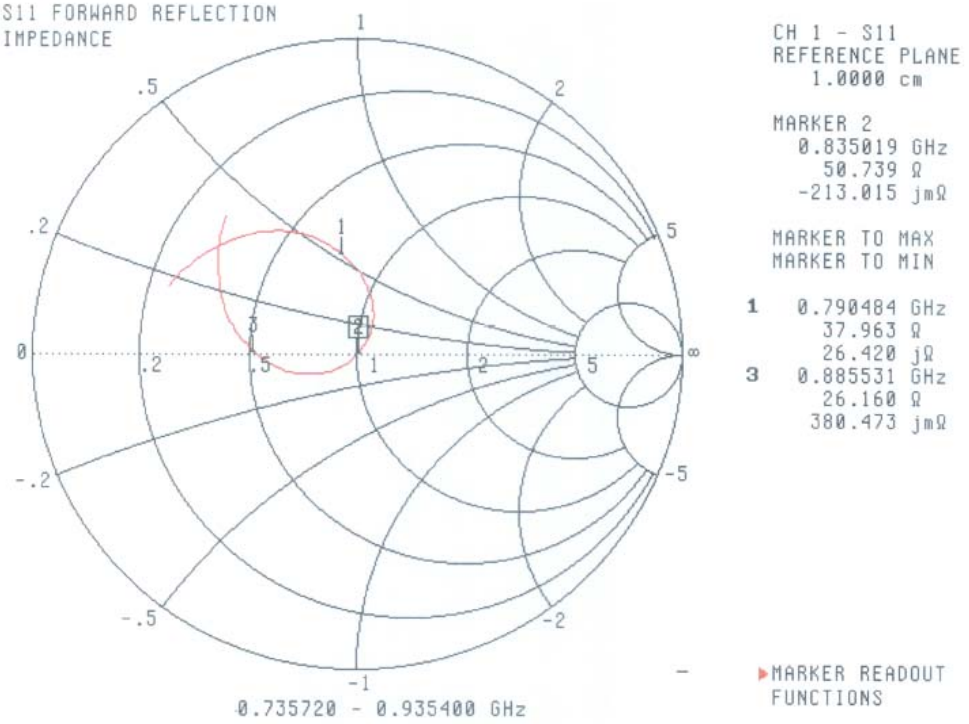

8

This page has been reviewed for content and attested to by signature within this document.

NCL Calibration Laboratories
Division of APREL Laboratories.

System Validation Results Using the Electrically Calibrated Dipole

Head Tissue Frequency	1 Gram	10 Gram	Peak Above Feed Point
835 MHz	9.49	6.1	14.21

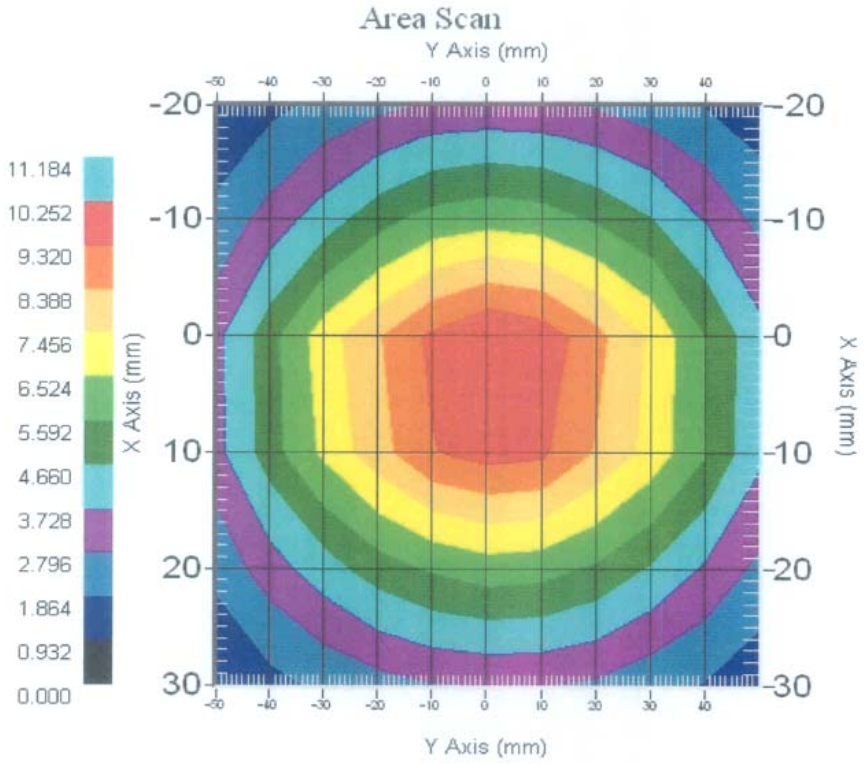

9

This page has been reviewed for content and attested to by signature within this document.

NCL Calibration Laboratories
Division of APREL Laboratories.

Test Equipment

The test equipment used during Probe Calibration, manufacturer, model number and, current calibration status are listed and located on the main APREL server R:\NCL\Calibration Equipment\Instrument List 2008.

This page has been reviewed for content and attested to by signature within this document.

NCL CALIBRATION LABORATORIES

Calibration File No: DC-920
Project Number: BACL-ALSAS10U-5323

CERTIFICATE OF CALIBRATION

It is certified that the equipment identified below has been calibrated in the **NCL CALIBRATION LABORATORIES** by qualified personnel following recognized procedures and using transfer standards traceable to NRC/NIST.

Validation Dipole

Manufacturer: APREL Laboratories
Part number: ALS-D-1900-S-2
Frequency: 1900 MHz
Serial No: 210-00710

Customer: Bay Area Compliance Laboratory

Calibrated: 1st September 2008
Released on: 1st September 2008

This Calibration Certificate is Incomplete Unless Accompanied with the Calibration Results Summary

Released By: _____

NCL CALIBRATION LABORATORIES
51 SPECTRUM WAY
NEPEAN, ONTARIO
CANADA K2R 1E6
Division of APREL Lab.
TEL: (613) 820-4988
FAX: (613) 820-4162

NCL Calibration Laboratories
Division of APREL Laboratories.

Conditions

Dipole 210-00710 was new and taken from stock prior to calibration.

Ambient Temperature of the Laboratory:	22 °C +/- 0.5°C
Temperature of the Tissue:	21 °C +/- 0.5°C

We the undersigned attest that to the best of our knowledge the calibration of this device has been accurately conducted and that all information contained within this report has been reviewed for accuracy.

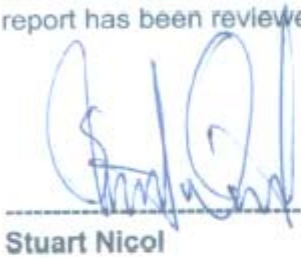

Stuart Nicol

C. Teodorian

This page has been reviewed for content and attested to by signature within this document.

NCL Calibration Laboratories
Division of APREL Laboratories.

Calibration Results Summary

The following results relate the Calibrated Dipole and should be used as a quick reference for the user.

Mechanical Dimensions

Length: 67.1 mm
Height: 38.9 mm

Electrical Specification

SWR: 1.059 U
Return Loss: -30.831 dB
Impedance: 50.914 Ω

System Validation Results

Frequency	1 Gram	10 Gram	Peak
1900 MHz	38.7	20.5	69.7

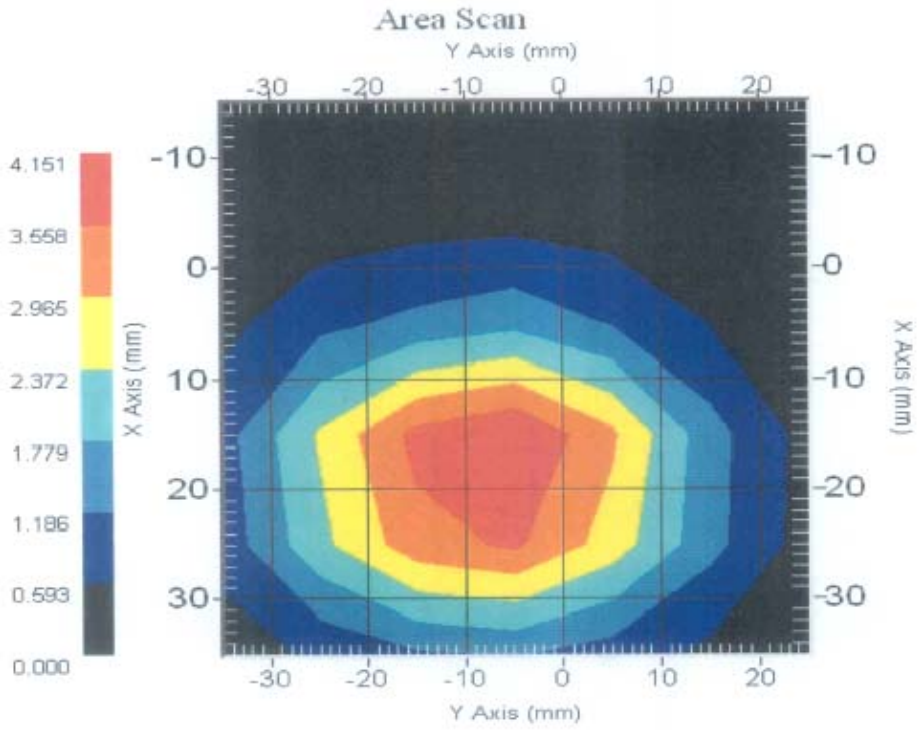

3

This page has been reviewed for content and attested to by signature within this document.

NCL Calibration Laboratories
Division of APREL Laboratories.

Introduction

This Calibration Report has been produced in line with the SSI Dipole Calibration Procedure SSI-TP-018-ALSAS. The results contained within this report are for Validation Dipole 210-00710. The calibration routine consisted of a three-step process. Step 1 was a mechanical verification of the dipole to ensure that it meets the mechanical specifications. Step 2 was an Electrical Calibration for the Validation Dipole, where the SWR, Impedance, and the Return loss were assessed. Step 3 involved a System Validation using the ALSAS-10U, along with APREL E-020 130 MHz to 26 GHz E-Field Probe Serial Number 212.

References

SSI-TP-018-ALSAS Dipole Calibration Procedure
SSI-TP-016 Tissue Calibration Procedure
IEEE 1528 "Recommended Practice for Determining the Peak Spatial-Average Specific Absorption Rate (SAR) in the Human Body Due to Wireless Communications Devices: Experimental Techniques"

Conditions

Dipole 210-00710 was new taken from stock.

Ambient Temperature of the Laboratory:	22 °C +/- 0.5°C
Temperature of the Tissue:	20 °C +/- 0.5°C

4

This page has been reviewed for content and attested to by signature within this document.

NCL Calibration Laboratories
Division of APREL Laboratories.

Dipole Calibration Results

Mechanical Verification

APREL Length	APREL Height	Measured Length	Measured Height
68.0 mm	39.5 mm	67.1mm	38.9 mm

Tissue Validation

Head Tissue 1900 MHz	Measured
Dielectric constant, ε_r	40.03
Conductivity, σ [S/m]	1.38

5

This page has been reviewed for content and attested to by signature within this document.

NCL Calibration Laboratories
Division of APREL Laboratories.

Electrical Calibration

Test	Result
S11 R/L	-30.831 dB
SWR	1.059 U
Impedance	50.914 Ω

The Following Graphs are the results as displayed on the Vector Network Analyzer.

S11 Parameter Return Loss

6

This page has been reviewed for content and attested to by signature within this document.

NCL Calibration Laboratories
Division of APREL Laboratories.

SWR

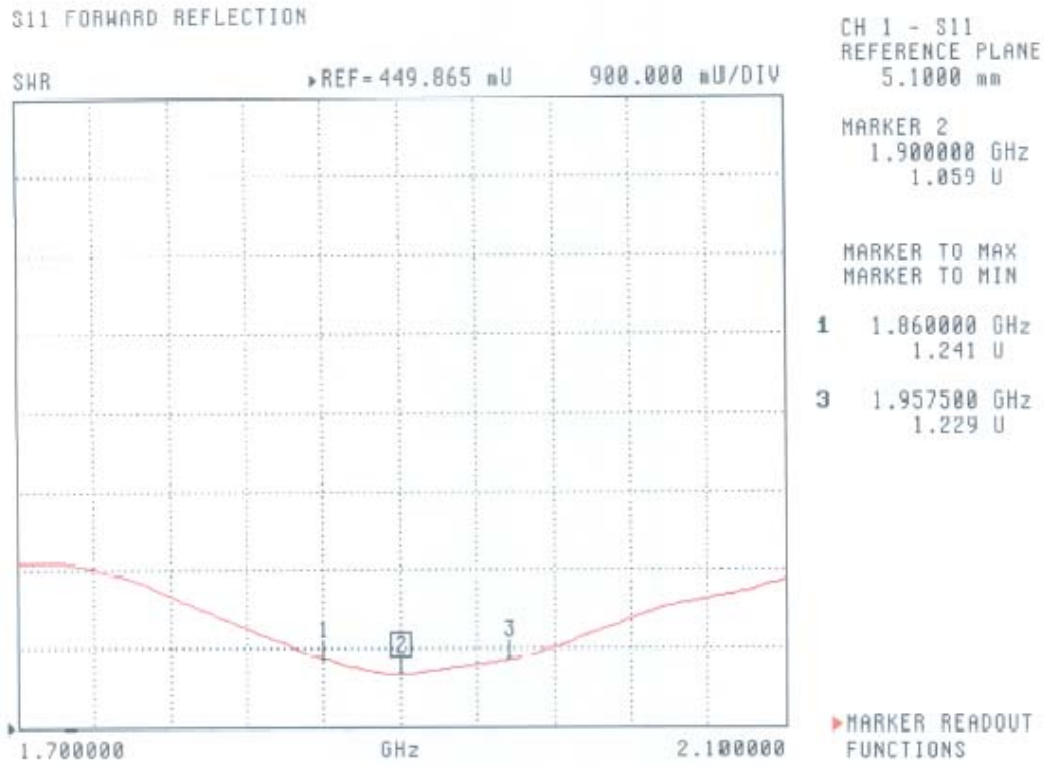

7

This page has been reviewed for content and attested to by signature within this document.

NCL Calibration Laboratories
Division of APREL Laboratories.

Smith Chart Dipole Impedance

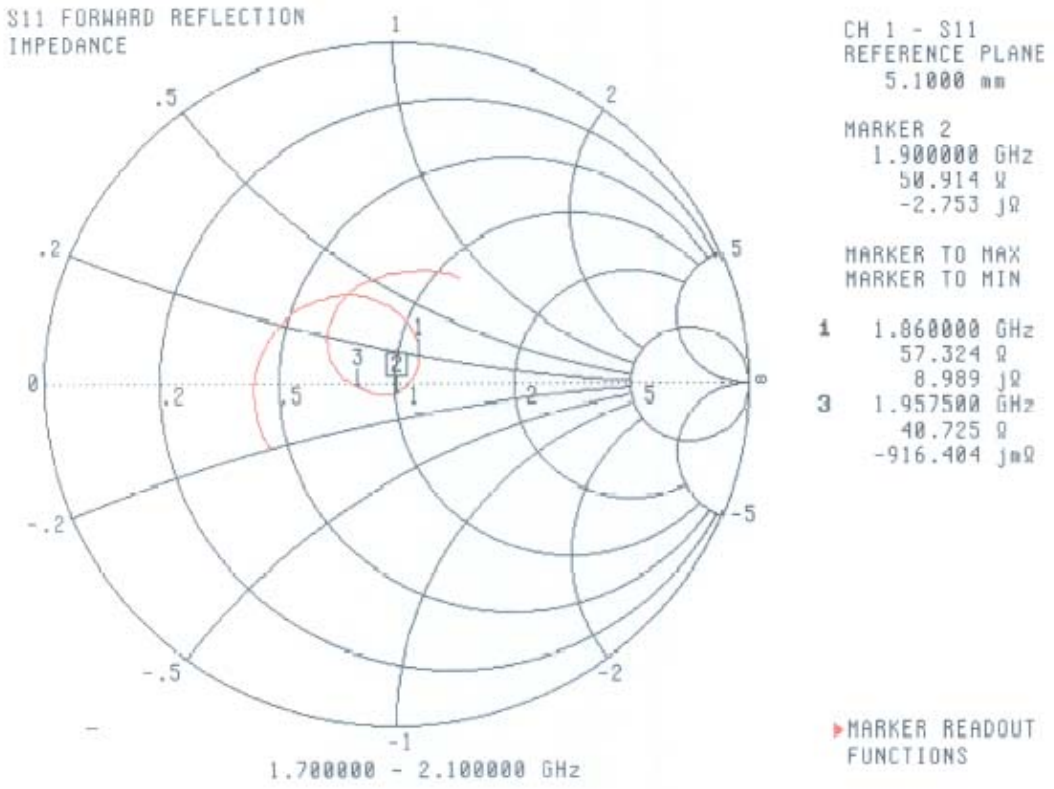

8

This page has been reviewed for content and attested to by signature within this document.

NCL Calibration Laboratories
Division of APREL Laboratories.

System Validation Results Using the Electrically Calibrated Dipole

Head Tissue Frequency	1 Gram	10 Gram	Peak Above Feed Point
1900 MHz	38.7	20.5	69.7

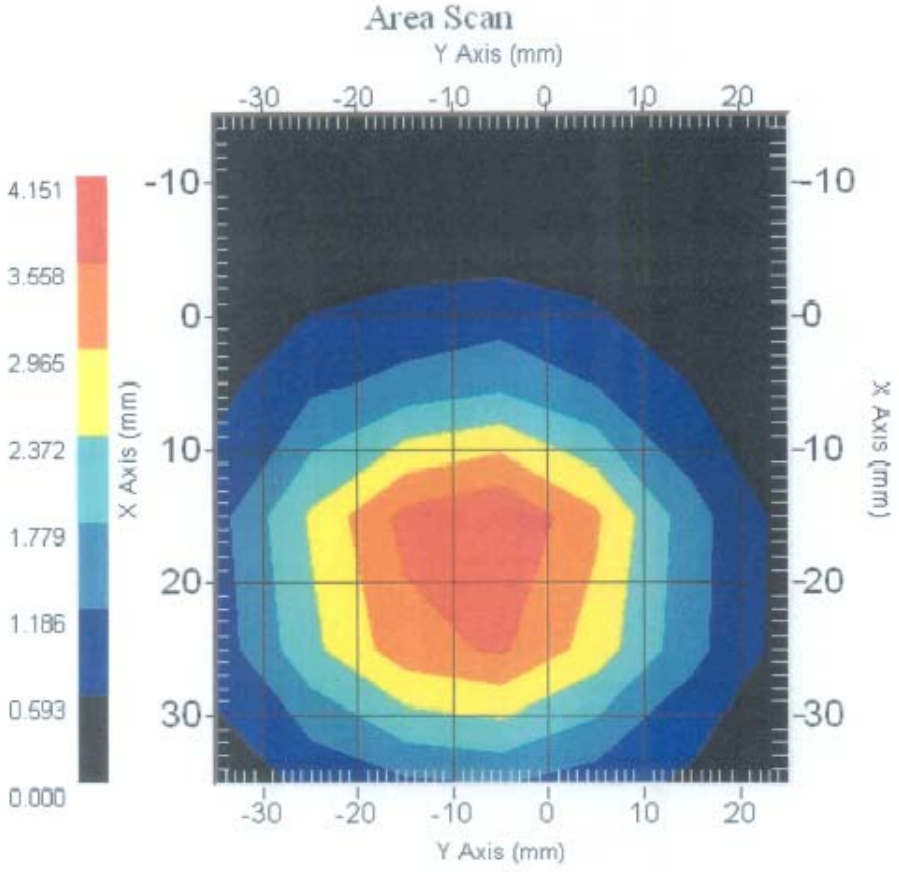

9

This page has been reviewed for content and attested to by signature within this document.

NCL Calibration Laboratories
Division of APREL Laboratories.

Test Equipment

The test equipment used during Probe Calibration, manufacturer, model number and, current calibration status are listed and located on the main APREL server R:\NCL\Calibration Equipment\Instrument List 2007.

10

This page has been reviewed for content and attested to by signature within this document.

APPENDIX D – SAR SYSTEM VALIDATION DATA

Test Laboratory: Bay Area Compliance Lab Corp. (Shenzhen)

System Performance Check 835MHz Head

Dipole 835 MHz; Type: ALS-D-835-S-2; S/N: 180-00558

Product Data
Device Name : Dipole 835 MHz
Serial No. : 180-00558
Type : Dipole
Model : ALS-D-835-S-2
Frequency : 835.00 MHz
Max. Transmit Pwr : 1 W
Drift Time : 3 min(s)
Power Drift-Start : 10.066 W/kg
Power Drift-Finish : 9.926 W/kg
Power Drift (%) : -1.391

Phantom Data
Name : APREL-Uni
Type : Uni-Phantom
Size (mm) : 280 x 280 x 200
Serial No. : System Default
Location : Center
Description : Default
Phantom Data

Tissue Data
Type : HEAD
Serial No. : 270-01002
Frequency : 835.00 MHz
Last Calib. Date : 15-Apr-2008
Temperature : 20.00 °C
Ambient Temp. : 20.00 °C
Humidity : 50.00 RH%
Epsilon : 41.50 F/m
Sigma : 0.90 S/m
Density : 1000.00 kg/cu. m

Probe Data
Name : E-Field
Model : E-020
Type : E-Field Triangle
Serial No. : 273
Last Calib. Date : 08-Jan-2008
Frequency : 835.00 MHz
Duty Cycle Factor : 1
Conversion Factor : 6.5
Probe Sensitivity : 1.20 1.20 1.20 μV/(V/m)2
Compression Point : 95.00 mV
Offset : 1.56 mm

Measurement Data
Crest Factor : 1
Scan Type : Complete
Tissue Temp. : 21.00 °C
Ambient Temp. : 21.00 °C
Area Scan : 7x9x1 : Measurement x=10mm, y=10mm, z=4mm
Zoom Scan : 7x7x7 : Measurement x=5mm, y=5mm, z=5mm

1 gram SAR value : 9.651 W/kg
10 gram SAR value : 6.042 W/kg
Area Scan Peak SAR : 10.936 W/kg
Zoom Scan Peak SAR : 15.013 W/kg

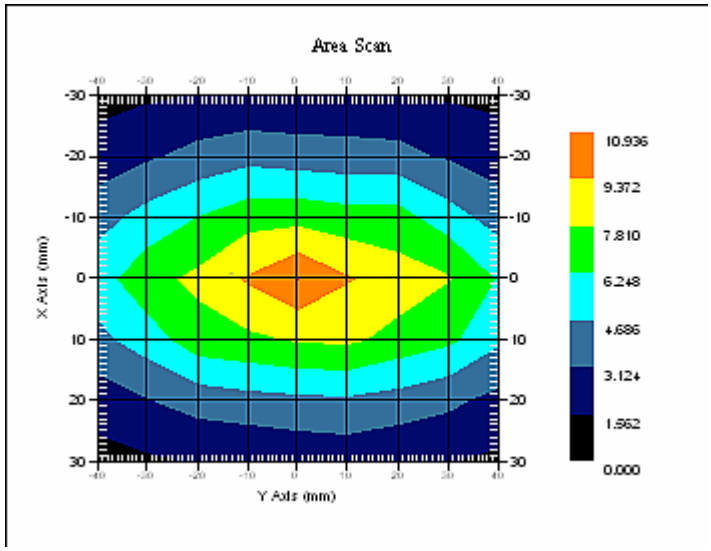

835 MHz System Validation

Test Laboratory: Bay Area Compliance Lab Corp. (Shenzhen)

System Performance Check 1900 Head

Dipole 1900 MHz; Type: ALS-D-1900-S-2; S/N: 210-00710

Product Data	
Device Name	: Dipole 1900MHz
Serial No.	: 210-00710
Type	: Dipole
Model	: ALS-D-1900-S-2
Frequency	: 1900.00 MHz
Max. Transmit Pwr	: 1 W
Drift Time	: 3 min(s)
Power Drift-Start	: 43.370 W/kg
Power Drift-Finish	: 41.609 W/kg
Power Drift (%)	: -4.059
Phantom Data	
Name	: APREL-Uni
Type	: Uni-Phantom
Size (mm)	: 280 x 280 x 200
Serial No.	: System Default
Location	: Center
Description	: Default
Tissue Data	
Type	: HEAD
Serial No.	: 295-01103
Frequency	: 1900.00 MHz
Last Calib. Date	: 16-Apr-2008
Temperature	: 20.00 °C
Ambient Temp.	: 20.00 °C
Humidity	: 56.00 RH%
Epsilon	: 40.00 F/m
Sigma	: 1.40 S/m
Density	: 1000.00 kg/cu. m
Probe Data	
Name	: E-Field
Model	: E-020
Type	: E-Field Triangle
Serial No.	: 273
Last Calib. Date	: 01-Aug-2008
Frequency	: 1900.00 MHz
Duty Cycle Factor	: 1
Conversion Factor	: 5.15
Probe Sensitivity	: 1.20 1.20 1.20 μV/(V/m)2
Compression Point	: 95.00 mV
Offset	: 1.56 mm
Measurement Data	
Crest Factor	: 1
Scan Type	: Complete
Tissue Temp.	: 20.00 °C
Ambient Temp.	: 20.00 °C
Area Scan	: 7x9x1 : Measurement x=10mm, y=10mm, z=4mm
Zoom Scan	: 7x7x7 : Measurement x=5mm, y=5mm, z=5mm

1 gram SAR value : 40.328 W/kg
10 gram SAR value : 20.137 W/kg
Area Scan Peak SAR : 44.786 W/kg
Zoom Scan Peak SAR : 75.567 W/kg

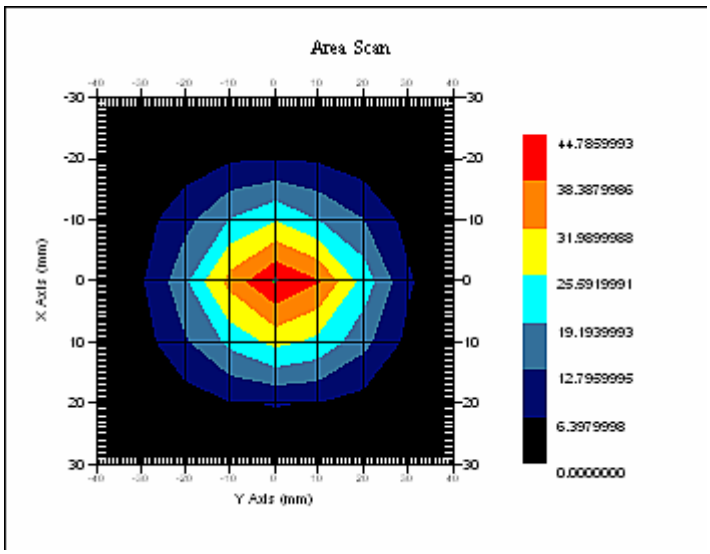

1900 MHz System Validation

APPENDIX E – EUT SCAN RESULTS

Test Laboratory: Bay Area Compliance Lab Corp. (Shenzhen)

Left Head Cheek (835 MHz Middle Channel)

Measurement Data	
Test mode	:GSM
Crest Factor	: 8
Scan Type	: Complete
Area Scan	: 11x7x1: Measurement x=10mm, y=10mm, z=4mm
Zoom Scan	: 7x7x7: Measurement x=5mm, y=5mm, z=5mm
Power Drift-Start	: 0.073 W/kg
Power Drift-Finish	: 0.071 W/kg
Power Drift (%)	: -2.7
Tissue Data	
Type	: HEAD
Frequency	: 835.00 MHz
Epsilon	: 41.60 F/m
Sigma	: 0.94 S/m
Density	: 1000.00 kg/cu. m
Probe Data	
Serial No.	: 273
Frequency	: 835.00 MHz
Duty Cycle Factor	: 8
Conversion Factor	: 6.5
Probe Sensitivity	: 1.20 1.20 1.20 μV/(V/m)2
Compression Point	: 95.00 mV
Offset	: 1.56 mm
1 gram SAR value	: 0.432 W/kg
10 gram SAR value	: 0.377 W/kg
Area Scan Peak SAR	: 0.443 W/kg
Zoom Scan Peak SAR	: 0.580 W/kg

Plot 1#

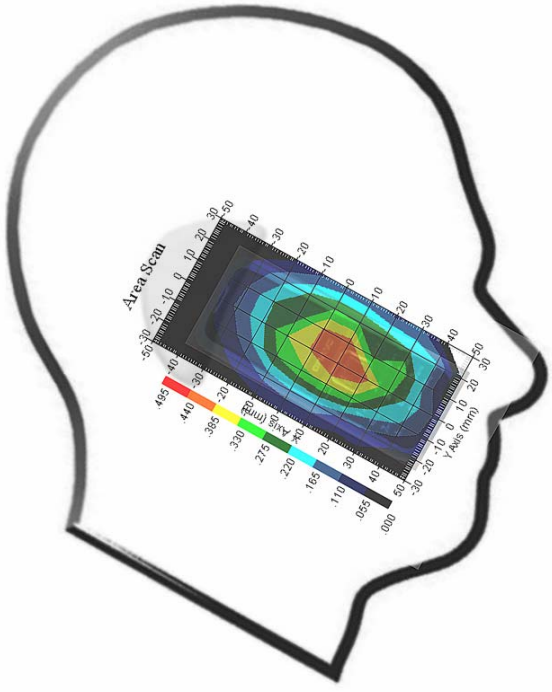

Test Laboratory: Bay Area Compliance Lab Corp. (Shenzhen)

Left Head Cheek (835 MHz Low Channel)

Measurement Data	
Test mode	:GSM
Crest Factor	: 8
Scan Type	: Complete
Area Scan	: 11x7x1 : Measurement x=10mm, y=10mm, z=4mm
Zoom Scan	: 7x7x7 : Measurement x=5mm, y=5mm, z=5mm
Power Drift-Start	: 0.091 W/kg
Power Drift-Finish	: 0.093 W/kg
Power Drift (%)	: 2.053
Tissue Data	
Type	: HEAD
Frequency	: 835.00 MHz
Epsilon	: 41.60 F/m
Sigma	: 0.94 S/m
Density	: 1000.00 kg/cu. m
Probe Data	
Serial No.	: 273
Frequency	: 835.00 MHz
Duty Cycle Factor	: 8
Conversion Factor	: 6.5
Probe Sensitivity	: 1.20 1.20 1.20 µV/(V/m)2
Compression Point	: 95.00 mV
Offset	: 1.56 mm
1 gram SAR value	: 0.530 W/kg
10 gram SAR value	: 0.509 W/kg
Area Scan Peak SAR	: 0.686 W/kg
Zoom Scan Peak SAR	: 1.211 W/kg

Plot 2#

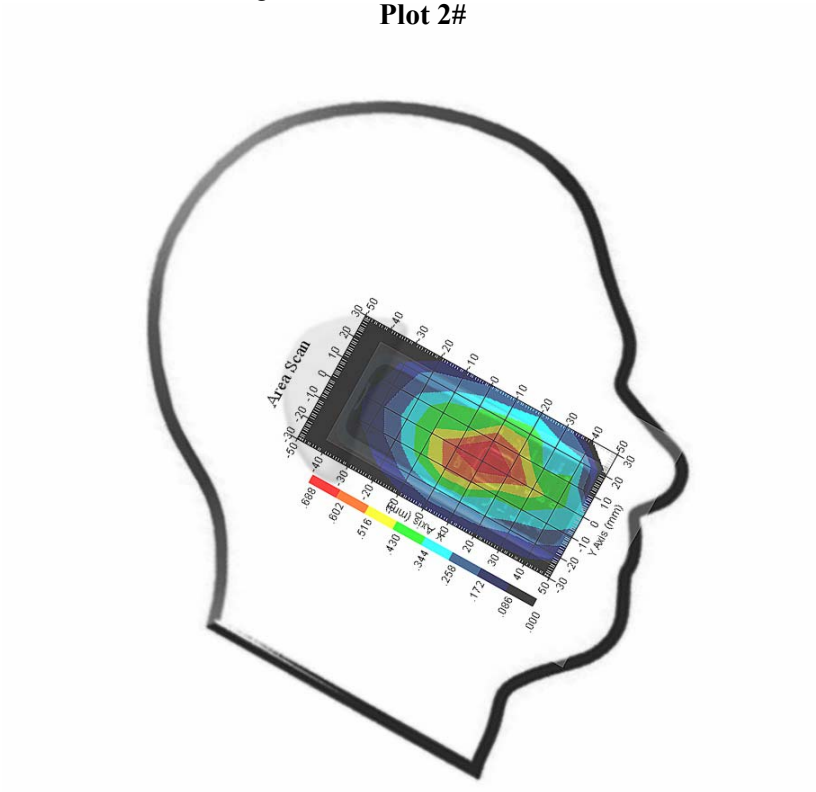

Test Laboratory: Bay Area Compliance Lab Corp. (Shenzhen)

Left Head Cheek (835 MHz High Channel)

Measurement Data	
Test mode	:GSM
Crest Factor	: 8
Scan Type	: Complete
Area Scan	: 11x7x1 : Measurement x=10mm, y=10mm, z=4mm
Zoom Scan	: 7x7x7 : Measurement x=5mm, y=5mm, z=5mm
Power Drift-Start	: 0.073 W/kg
Power Drift-Finish	: 0.068 W/kg
Power Drift (%)	: -0.068
Tissue Data	
Type	: HEAD
Frequency	: 835.00 MHz
Epsilon	: 41.60 F/m
Sigma	: 0.94 S/m
Density	: 1000.00 kg/cu. m
Probe Data	
Serial No.	: 273
Frequency	: 835.00 MHz
Duty Cycle Factor	: 8
Conversion Factor	: 6.5
Probe Sensitivity	: 1.20 1.20 1.20 μV/(V/m)2
Compression Point	: 95.00 mV
Offset	: 1.56 mm
1 gram SAR value	: 0.450 W/kg
10 gram SAR value	: 0.300 W/kg
Area Scan Peak SAR	: 0.456 W/kg
Zoom Scan Peak SAR	: 0.680 W/kg

Plot 3#

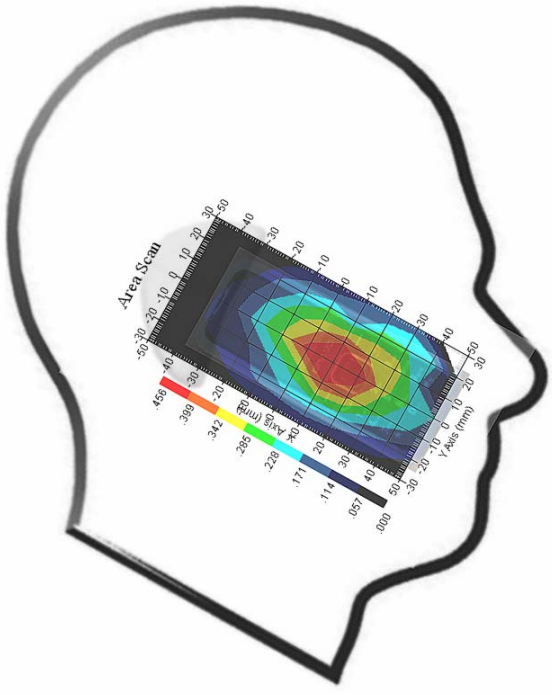

Test Laboratory: Bay Area Compliance Lab Corp. (Shenzhen)

Left Head Tilt (835 MHz Middle Channel)

Measurement Data	
Test mode	:GSM
Crest Factor	: 8
Scan Type	: Complete
Area Scan	: 11x7x1 : Measurement x=10mm, y=10mm, z=4mm
Zoom Scan	: 7x7x7 : Measurement x=5mm, y=5mm, z=5mm
Power Drift-Start	: 0.060 W/kg
Power Drift-Finish	: 0.062 W/kg
Power Drift (%)	: 2.989
Tissue Data	
Type	: HEAD
Frequency	: 835.00 MHz
Epsilon	: 41.60 F/m
Sigma	: 0.94 S/m
Density	: 1000.00 kg/cu. m
Probe Data	
Serial No.	: 273
Frequency	: 835.00 MHz
Duty Cycle Factor	: 8
Conversion Factor	: 6.5
Probe Sensitivity	: 1.20 1.20 1.20 μV/(V/m)2
Compression Point	: 95.00 mV
Offset	: 1.56 mm
1 gram SAR value	: 0.149 W/kg
10 gram SAR value	: 0.097 W/kg
Area Scan Peak SAR	: 0.150 W/kg
Zoom Scan Peak SAR	: 0.220 W/kg

Plot 4#

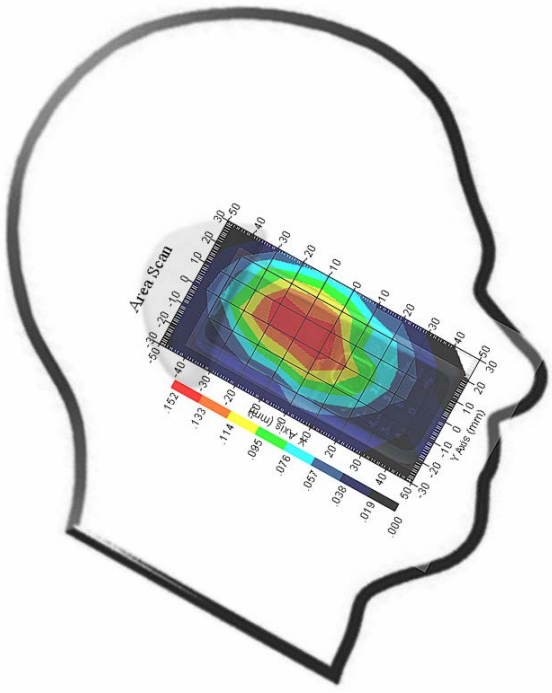

Test Laboratory: Bay Area Compliance Lab Corp. (Shenzhen)

Right Head Cheek (835 MHz Middle Channel)

Measurement Data	
Test mode	:GSM
Crest Factor	: 8
Scan Type：	: Complete
Area Scan	: 11x7x1 : Measurement x=10mm, y=10mm, z=4mm
Zoom Scan	: 7x7x7 : Measurement x=5mm, y=5mm, z=5mm
Power Drift-Start	: 0.077 W/kg
Power Drift-Finish	: 0.076 W/kg
Power Drift (%)	: -1.298
Tissue Data	
Type	: HEAD
Frequency	: 835.00 MHz
Epsilon	: 41.60 F/m
Sigma	: 0.94 S/m
Density	: 1000.00 kg/cu. m
Probe Data	
Serial No.	: 273
Frequency	: 835.00 MHz
Duty Cycle Factor	: 8
Conversion Factor	: 6.5
Probe Sensitivity	: 1.20 1.20 1.20 μV/(V/m)2
Compression Point	: 95.00 mV
Offset	: 1.56 mm
1 gram SAR value	: 0.343 W/kg
10 gram SAR value	: 0.216 W/kg
Area Scan Peak SAR	: 0.425 W/kg
Zoom Scan Peak SAR	: 0.640 W/kg

Plot 5#

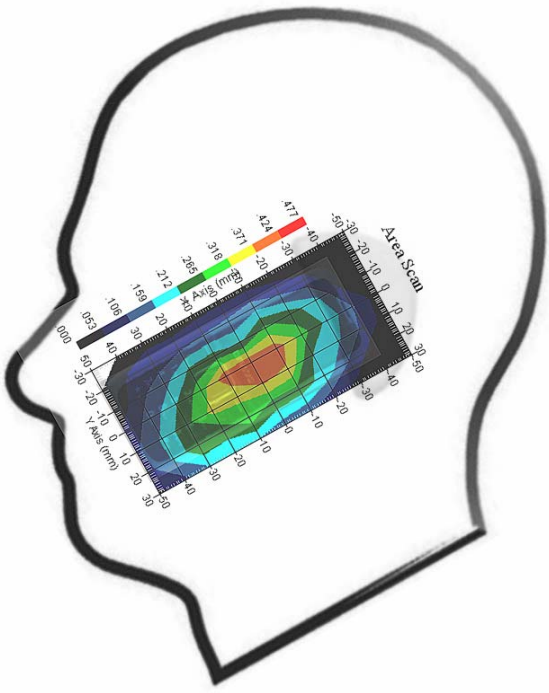

Test Laboratory: Bay Area Compliance Lab Corp. (Shenzhen)

Right Head Tilt (835 MHz Middle Channel)

Measurement Data	
Test mode	:GSM
Crest Factor	: 8
Scan Type：	: Complete
Area Scan	: 11x7x1 : Measurement x=10mm, y=10mm, z=4mm
Zoom Scan	: 7x7x7 : Measurement x=5mm, y=5mm, z=5mm
Power Drift-Start	: 0.130 W/kg
Power Drift-Finish	: 0.128 W/kg
Power Drift (%)	: -1.957
Tissue Data	
Type	: HEAD
Frequency	: 835.00 MHz
Epsilon	: 41.60 F/m
Sigma	: 0.94 S/m
Density	: 1000.00 kg/cu. m
Probe Data	
Serial No.	: 273
Frequency	: 835.00 MHz
Duty Cycle Factor	: 8
Conversion Factor	: 6.5
Probe Sensitivity	: 1.20 1.20 1.20 μV/(V/m)2
Compression Point	: 95.00 mV
Offset	: 1.56 mm
1 gram SAR value	: 0.135 W/kg
10 gram SAR value	: 0.078 W/kg
Area Scan Peak SAR	: 0.148 W/kg
Zoom Scan Peak SAR	: 0.220 W/kg

Plot 6#

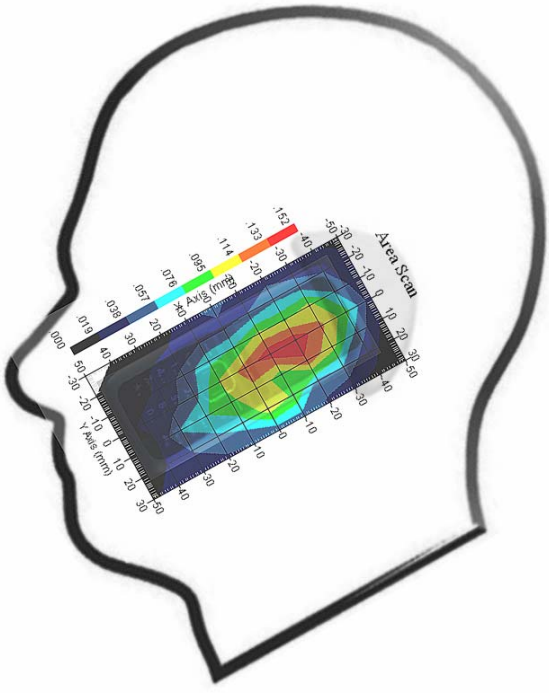

Test Laboratory: Bay Area Compliance Lab Corp. (Shenzhen)

Body- worn Back (835 MHz Middle Channel)

Measurement Data
Test mode :GPRS
Crest Factor : 8
Scan Type : Complete
Area Scan : 7x12x1 : Measurement x=10mm, y=10mm, z=4mm
Zoom Scan : 7x7x7 : Measurement x=5mm, y=5mm, z=5mm
Power Drift-Start : 0.124 W/kg
Power Drift-Finish : 0.129 W/kg
Power Drift (%) : 4.322

Tissue Data
Type : BODY
Frequency : 835.00 MHz
Epsilon : 53.77 F/m
Sigma : 0.99 S/m
Density : 1000.00 kg/cu. m

Probe Data
Serial No. : 273
Frequency : 835.00 MHz
Duty Cycle Factor : 8
Conversion Factor : 6.7
Probe Sensitivity : 1.20 1.20 1.20 μV/(V/m)2
Compression Point : 95.00 mV
Offset : 1.56 mm

1 gram SAR value : 0.369 W/kg
10 gram SAR value : 0.222 W/kg
Area Scan Peak SAR : 0.401 W/kg
Zoom Scan Peak SAR : 0.630 W/kg

Plot 7#

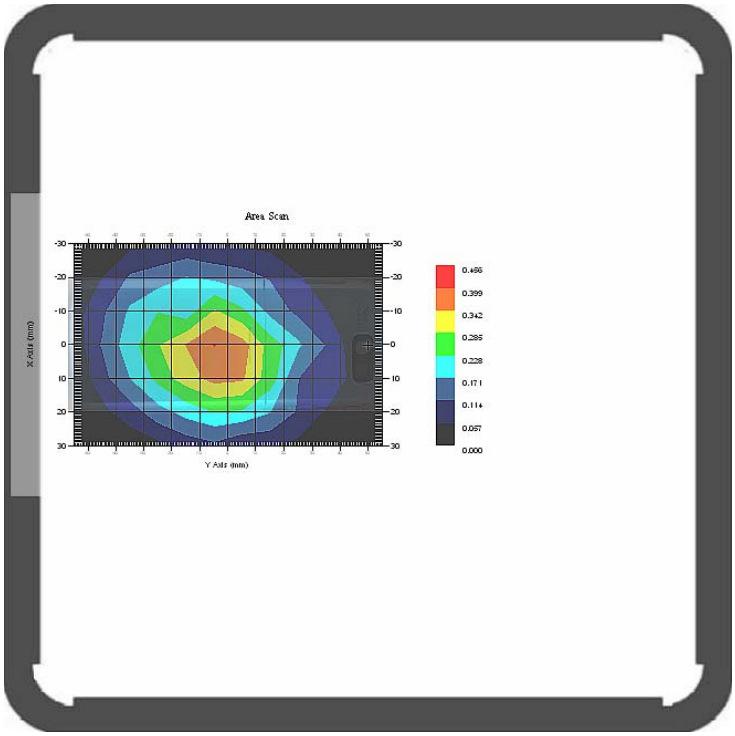

Test Laboratory: Bay Area Compliance Lab Corp. (Shenzhen)

Body- worn Back (835 MHz Low Channel)

Measurement Data
Test mode :GPRS
Crest Factor : 8
Scan Type : Complete
Area Scan : 7x12x1 : Measurement x=10mm, y=10mm, z=4mm
Zoom Scan : 7x7x7 : Measurement x=5mm, y=5mm, z=5mm
Power Drift-Start : 0.141 W/kg
Power Drift-Finish : 0.138 W/kg
Power Drift (%) : -2.127

Tissue Data
Type : BODY
Frequency : 835.00 MHz
Epsilon : 53.77 F/m
Sigma : 0.99 S/m
Density : 1000.00 kg/cu. m

Probe Data
Serial No. : 273
Frequency : 835.00 MHz
Duty Cycle Factor : 8
Conversion Factor : 6.7
Probe Sensitivity : 1.20 1.20 1.20 μV/(V/m)2
Compression Point : 95.00 mV
Offset : 1.56 mm

1 gram SAR value : 0.349 W/kg
10 gram SAR value : 0.217 W/kg
Area Scan Peak SAR : 0.368 W/kg
Zoom Scan Peak SAR : 0.580 W/kg

Plot 8#

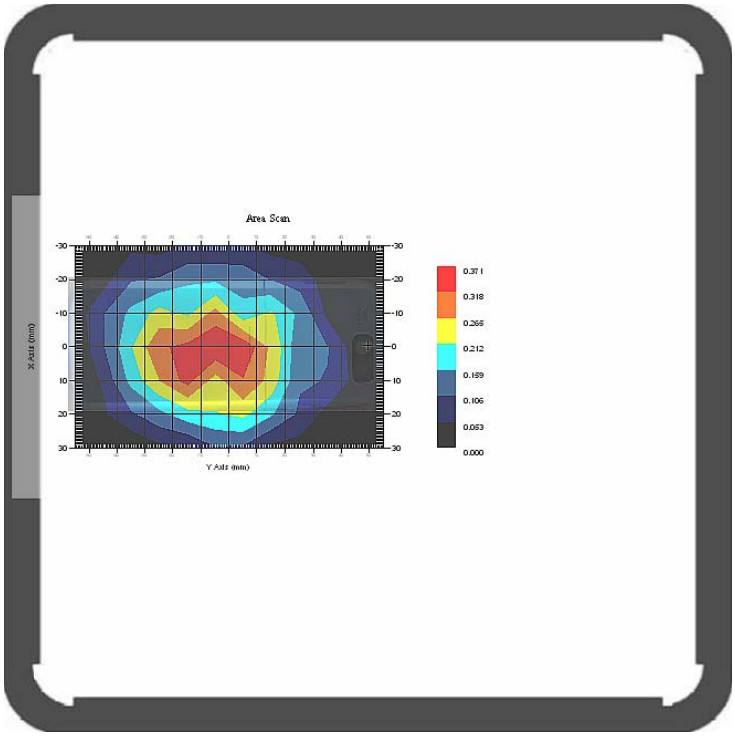

Test Laboratory: Bay Area Compliance Lab Corp. (Shenzhen)

Body- worn Back (835 MHz High Channel)

Measurement Data
Test mode :GPRS
Crest Factor : 8
Scan Type : Complete
Area Scan : 7x12x1 : Measurement x=10mm, y=10mm, z=4mm
Zoom Scan : 7x7x7 : Measurement x=5mm, y=5mm, z=5mm
Power Drift-Start : 0.157 W/kg
Power Drift-Finish : 0.155 W/kg
Power Drift (%) : -1.274

Tissue Data
Type : BODY
Frequency : 835.00 MHz
Epsilon : 53.77 F/m
Sigma : 0.99 S/m
Density : 1000.00 kg/cu. m

Probe Data
Serial No. : 273
Frequency : 835.00 MHz
Duty Cycle Factor : 8
Conversion Factor : 6.7
Probe Sensitivity : 1.20 1.20 1.20 μV/(V/m)2
Compression Point : 95.00 mV
Offset : 1.56 mm

1 gram SAR value : 0.331 W/kg
10 gram SAR value : 0.257 W/kg
Area Scan Peak SAR : 0.336 W/kg
Zoom Scan Peak SAR : 0.470 W/kg

Plot 9#

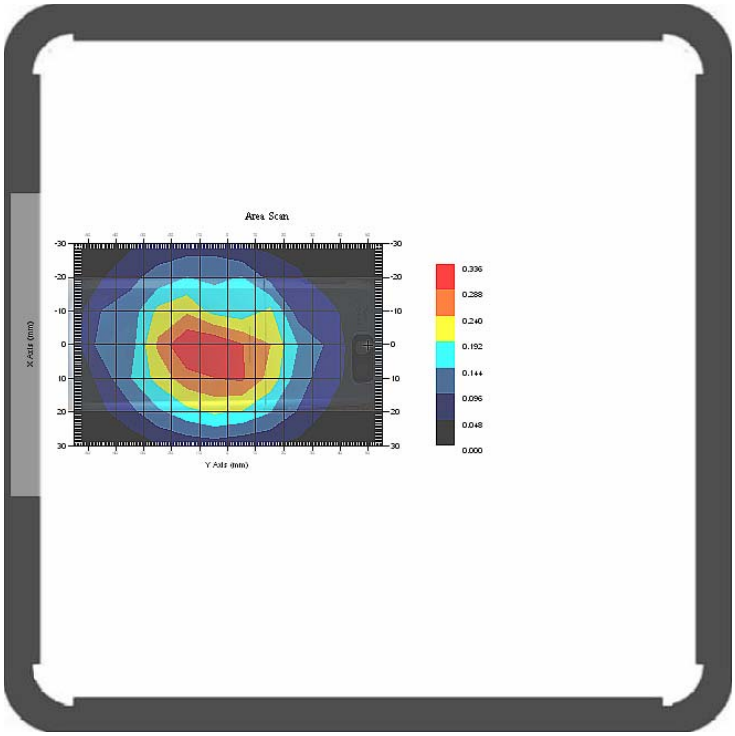

Test Laboratory: Bay Area Compliance Lab Corp. (Shenzhen)

Left Head Cheek (1900 MHz Middle Channel)

Measurement Data	
Test mode	:GSM
Crest Factor	: 8
Scan Type：	: Complete
Area Scan	: 11x7x1 : Measurement x=10mm, y=10mm, z=4mm
Zoom Scan	: 7x7x7 : Measurement x=5mm, y=5mm, z=5mm
Power Drift-Start	: 0.138 W/kg
Power Drift-Finish	: 0.136 W/kg
Power Drift (%)	: -1.449
Tissue Data	
Type	: HEAD
Frequency	: 1900.00 MHz
Epsilon	: 39.30 F/m
Sigma	: 1.43 S/m
Density	: 1000.00 kg/cu. m
Probe Data	
Serial No.	: 273
Frequency	: 1900.00 MHz
Duty Cycle Factor	: 8
Conversion Factor	: 5.25
Probe Sensitivity	: 1.20 1.20 1.20 μV/(V/m)2
Compression Point	: 95.00 mV
Offset	: 1.56 mm
1 gram SAR value	: 0.434 W/kg
10 gram SAR value	: 0.201 W/kg
Area Scan Peak SAR	: 0.553 W/kg
Zoom Scan Peak SAR	: 0.820 W/kg

Plot 10#

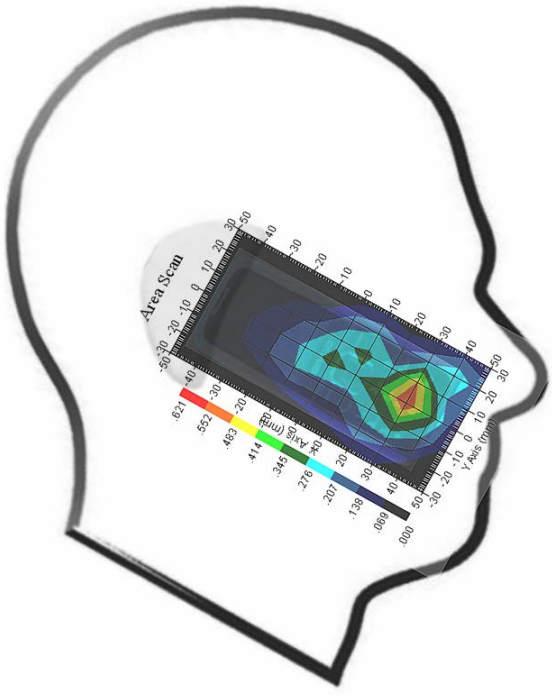

Test Laboratory: Bay Area Compliance Lab Corp. (Shenzhen)

Left Head Tilt (1900 MHz Middle Channel)

Measurement Data	
Test mode	:GSM
Crest Factor	: 8
Scan Type：	: Complete
Area Scan	: 11x7x1 : Measurement x=10mm, y=10mm, z=4mm
Zoom Scan	: 7x7x7 : Measurement x=5mm, y=5mm, z=5mm
Power Drift-Start	: 0.132 W/kg
Power Drift-Finish	: 0.130 W/kg
Power Drift (%)	: -1.515
Tissue Data	
Type	: HEAD
Frequency	: 1900.00 MHz
Epsilon	: 39.30 F/m
Sigma	: 1.43 S/m
Density	: 1000.00 kg/cu. m
Probe Data	
Serial No.	: 273
Frequency	: 1900.00 MHz
Duty Cycle Factor	: 8
Conversion Factor	: 5.25
Probe Sensitivity	: 1.20 1.20 1.20 μV/(V/m)2
Compression Point	: 95.00 mV
Offset	: 1.56 mm
1 gram SAR value	: 0.145 W/kg
10 gram SAR value	: 0.122 W/kg
Area Scan Peak SAR	: 0.149 W/kg
Zoom Scan Peak SAR	: 0.360 W/kg

Plot 11#

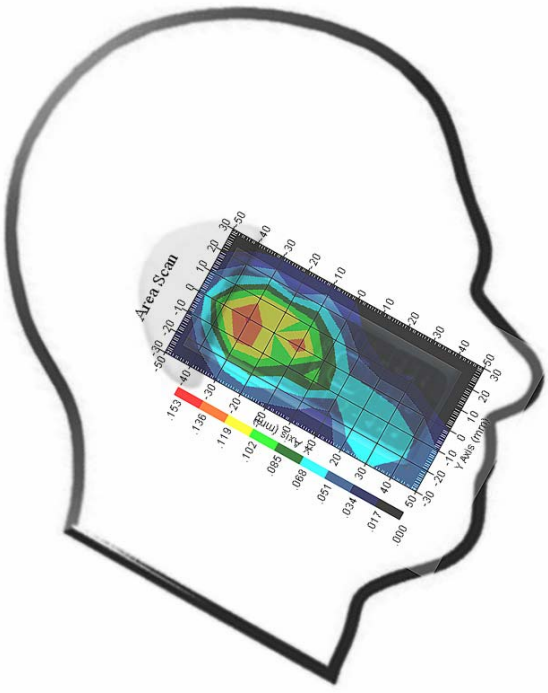

Test Laboratory: Bay Area Compliance Lab Corp. (Shenzhen)

Right Head Cheek (1900 MHz Middle Channel)

Measurement Data	
Test mode	:GSM
Crest Factor	: 8
Scan Type：	: Complete
Area Scan	: 11x7x1 : Measurement x=10mm, y=10mm, z=4mm
Zoom Scan	: 7x7x7 : Measurement x=5mm, y=5mm, z=5mm
Power Drift-Start	: 0.145 W/kg
Power Drift-Finish	: 0.141 W/kg
Power Drift (%)	: -2.758
Tissue Data	
Type	: HEAD
Frequency	: 1900.00 MHz
Epsilon	: 39.30 F/m
Sigma	: 1.43 S/m
Density	: 1000.00 kg/cu. m
Probe Data	
Serial No.	: 273
Frequency	: 1900.00 MHz
Duty Cycle Factor	: 8
Conversion Factor	: 5.25
Probe Sensitivity	: 1.20 1.20 1.20 μV/(V/m)2
Compression Point	: 95.00 mV
Offset	: 1.56 mm
1 gram SAR value	: 0.489 W/kg
10 gram SAR value	: 0.232 W/kg
Area Scan Peak SAR	: 0.800 W/kg
Zoom Scan Peak SAR	: 1.391 W/kg

Plot 12#

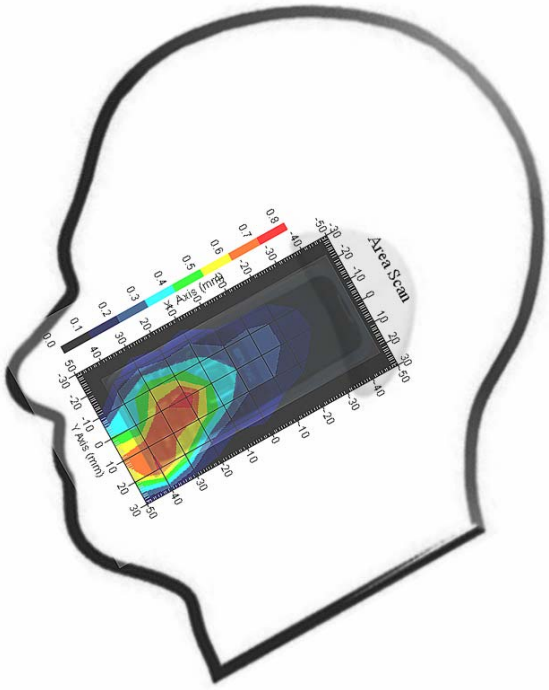

Test Laboratory: Bay Area Compliance Lab Corp. (Shenzhen)

Right Head Cheek (1900 MHz Low Channel)

Measurement Data	
Test mode	:GSM
Crest Factor	: 8
Scan Type：	: Complete
Area Scan	: 11x7x1 : Measurement x=10mm, y=10mm, z=4mm
Zoom Scan	: 7x7x7 : Measurement x=5mm, y=5mm, z=5mm
Power Drift-Start	: 0.124 W/kg
Power Drift-Finish	: 0.127 W/kg
Power Drift (%)	: 2.419
Tissue Data	
Type	: HEAD
Frequency	: 1900.00 MHz
Epsilon	: 39.30 F/m
Sigma	: 1.43 S/m
Density	: 1000.00 kg/cu. m
Probe Data	
Serial No.	: 273
Frequency	: 1900.00 MHz
Duty Cycle Factor	: 8
Conversion Factor	: 5.25
Probe Sensitivity	: 1.20 1.20 1.20 μV/(V/m)2
Compression Point	: 95.00 mV
Offset	: 1.56 mm
1 gram SAR value	: 0.566 W/kg
10 gram SAR value	: 0.343 W/kg
Area Scan Peak SAR	: 0.830 W/kg
Zoom Scan Peak SAR	: 1.241 W/kg

Plot 13#

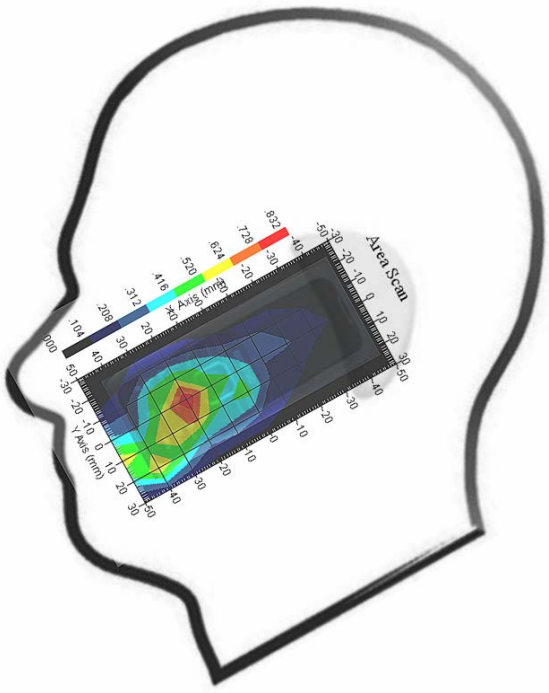

Test Laboratory: Bay Area Compliance Lab Corp. (Shenzhen)

Right Head Cheek (1900 MHz High Channel)

Measurement Data	
Test mode	:GSM
Crest Factor	: 8
Scan Type：	: Complete
Area Scan	: 11x7x1 : Measurement x=10mm, y=10mm, z=4mm
Zoom Scan	: 7x7x7 : Measurement x=5mm, y=5mm, z=5mm
Power Drift-Start	: 0.081 W/kg
Power Drift-Finish	: 0.084 W/kg
Power Drift (%)	: 3.704
Tissue Data	
Type	: HEAD
Frequency	: 1900.00 MHz
Epsilon	: 39.30 F/m
Sigma	: 1.43 S/m
Density	: 1000.00 kg/cu. m
Probe Data	
Serial No.	: 273
Frequency	: 1900.00 MHz
Duty Cycle Factor	: 8
Conversion Factor	: 5.25
Probe Sensitivity	: 1.20 1.20 1.20 μV/(V/m)2
Compression Point	: 95.00 mV
Offset	: 1.56 mm
1 gram SAR value	: 0.446 W/kg
10 gram SAR value	: 0.200 W/kg
Area Scan Peak SAR	: 0.648 W/kg
Zoom Scan Peak SAR	: 0.800 W/kg

Plot 14#

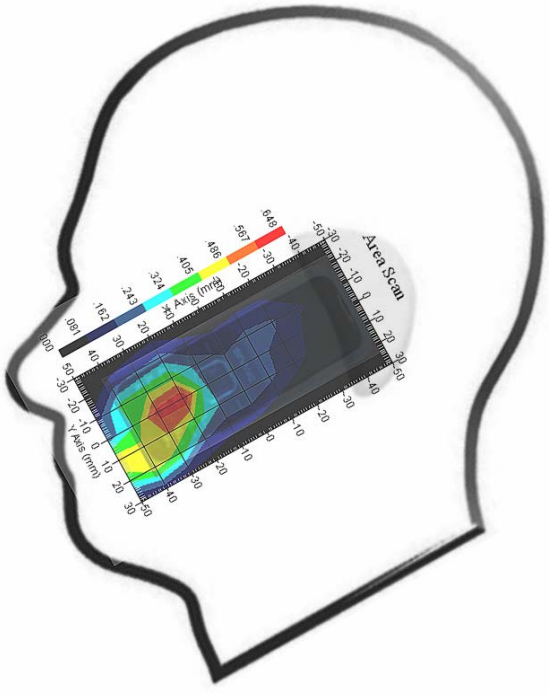

Test Laboratory: Bay Area Compliance Lab Corp. (Shenzhen)

Right Head Tilt (1900 MHz Middle Channel)

Measurement Data	
Test mode	:GSM
Crest Factor	: 8
Scan Type：	: Complete
Area Scan	: 11x7x1 : Measurement x=10mm, y=10mm, z=4mm
Zoom Scan	: 7x7x7 : Measurement x=5mm, y=5mm, z=5mm
Power Drift-Start	: 0.084 W/kg
Power Drift-Finish	: 0.083 W/kg
Power Drift (%)	: -1.190
Tissue Data	
Type	: HEAD
Frequency	: 1900.00 MHz
Epsilon	: 39.30 F/m
Sigma	: 1.43 S/m
Density	: 1000.00 kg/cu. m
Probe Data	
Serial No.	: 273
Frequency	: 1900.00 MHz
Duty Cycle Factor	: 8
Conversion Factor	: 5.25
Probe Sensitivity	: 1.20 1.20 1.20 μV/(V/m)2
Compression Point	: 95.00 mV
Offset	: 1.56 mm
1 gram SAR value	: 0.228 W/kg
10 gram SAR value	: 0.104 W/kg
Area Scan Peak SAR	: 0.232 W/kg
Zoom Scan Peak SAR	: 0.430 W/kg

Plot 15#

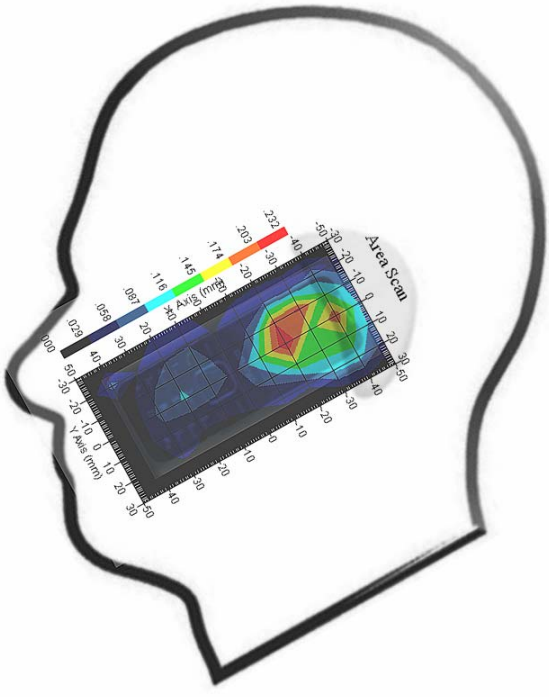

Test Laboratory: Bay Area Compliance Lab Corp. (Shenzhen)

Body- worn Back (1900 MHz Middle Channel)

Measurement Data
Test mode :GPRS
Crest Factor : 8
Scan Type : Complete
Area Scan : 7x12x1 : Measurement x=10mm, y=10mm, z=4mm
Zoom Scan : 7x7x7 : Measurement x=5mm, y=5mm, z=5mm
Power Drift-Start : 0.140 W/kg
Power Drift-Finish : 0.146 W/kg
Power Drift (%) : 4.285

Tissue Data
Type : BODY
Frequency : 1900.00 MHz
Epsilon : 53.45 F/m
Sigma : 1.50 S/m
Density : 1000.00 kg/cu. m

Probe Data
Serial No. : 273
Frequency : 1900.00 MHz
Duty Cycle Factor : 8
Conversion Factor : 5.15
Probe Sensitivity : 1.20 1.20 1.20 μV/(V/m)2
Compression Point : 95.00 mV
Offset : 1.56 mm

1 gram SAR value : 0.272 W/kg
10 gram SAR value : 0.137 W/kg
Area Scan Peak SAR : 0.308 W/kg
Zoom Scan Peak SAR : 0.550 W/kg

Plot 16#

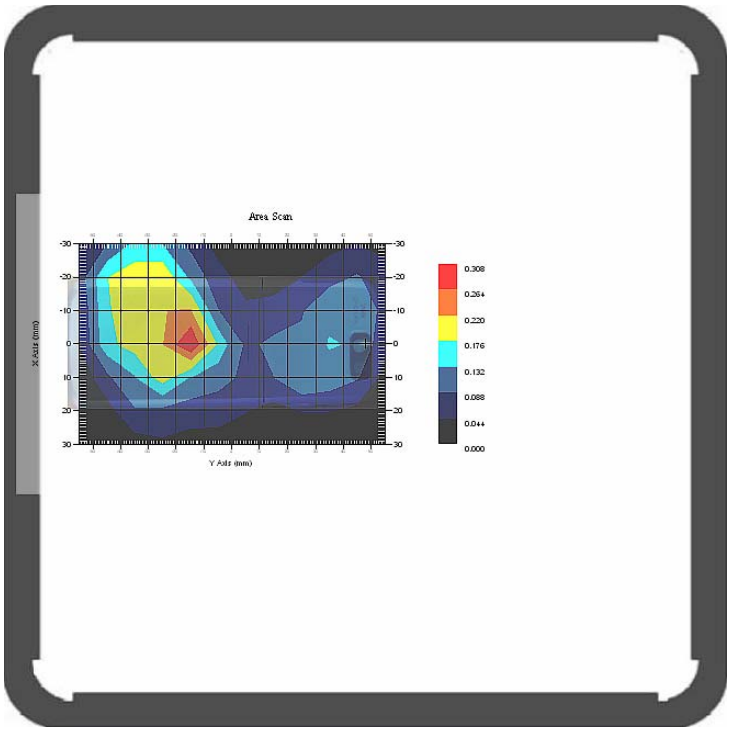

Test Laboratory: Bay Area Compliance Lab Corp. (Shenzhen)

Body- worn Back (1900 MHz Low Channel)

Measurement Data
Test mode :GPRS
Crest Factor : 8
Scan Type : Complete
Area Scan : 7x12x1 : Measurement x=10mm, y=10mm, z=4mm
Zoom Scan : 7x7x7 : Measurement x=5mm, y=5mm, z=5mm
Power Drift-Start : 0.136 W/kg
Power Drift-Finish : 0.134 W/kg
Power Drift (%) : -1.471

Tissue Data
Type : BODY
Frequency : 1900.00 MHz
Epsilon : 53.45 F/m
Sigma : 1.50 S/m
Density : 1000.00 kg/cu. m

Probe Data
Serial No. : 273
Frequency : 1900.00 MHz
Duty Cycle Factor : 8
Conversion Factor : 5.15
Probe Sensitivity : 1.20 1.20 1.20 μV/(V/m)2
Compression Point : 95.00 mV
Offset : 1.56 mm

1 gram SAR value : 0.308 W/kg
10 gram SAR value : 0.149 W/kg
Area Scan Peak SAR : 0.351 W/kg
Zoom Scan Peak SAR : 0.590 W/kg

Plot 17#

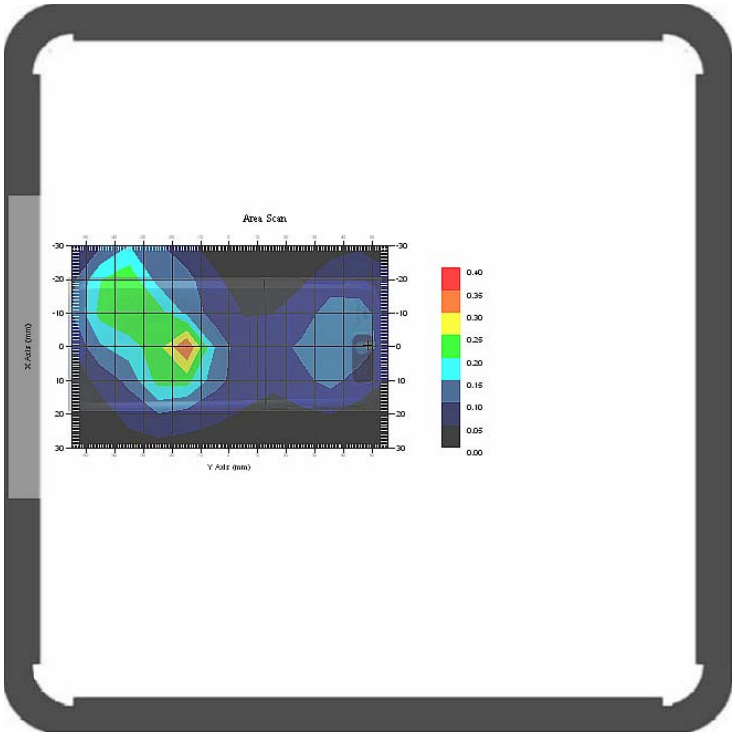

Test Laboratory: Bay Area Compliance Lab Corp. (Shenzhen)

Body- worn Back (1900 MHz High Channel)

Measurement Data
Test mode :GPRS
Crest Factor : 8
Scan Type : Complete
Area Scan : 7x12x1 : Measurement x=10mm, y=10mm, z=4mm
Zoom Scan : 7x7x7 : Measurement x=5mm, y=5mm, z=5mm
Power Drift-Start : 0.147 W/kg
Power Drift-Finish : 0.144 W/kg
Power Drift (%) : -2.041

Tissue Data
Type : BODY
Frequency : 1900.00 MHz
Epsilon : 53.45 F/m
Sigma : 1.50 S/m
Density : 1000.00 kg/cu. m

Probe Data
Serial No. : 273
Frequency : 1900.00 MHz
Duty Cycle Factor : 8
Conversion Factor : 5.15
Probe Sensitivity : 1.20 1.20 1.20 μV/(V/m)2
Compression Point : 95.00 mV
Offset : 1.56 mm

1 gram SAR value : 0.280 W/kg
10 gram SAR value : 0.133 W/kg
Area Scan Peak SAR : 0.274 W/kg
Zoom Scan Peak SAR : 0.730 W/kg

Plot 18#

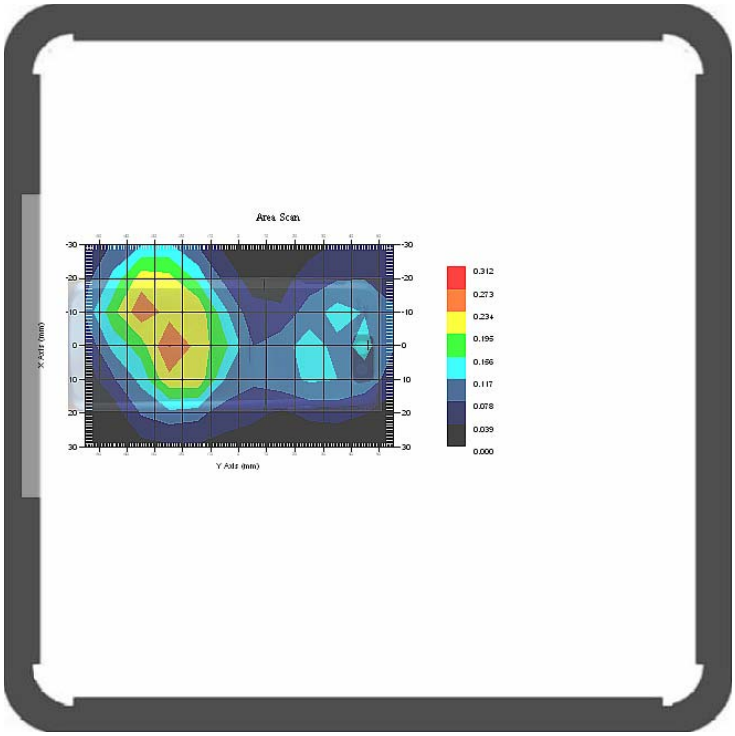

APPENDIX F – CONDUCTED OUTPUT POWER MEASUREMENT

Provision Applicable

The measured peak output power should be greater and within 5% than EMI measurement.

Test Procedure

The RF output of the transmitter was connected to the input of the spectrum analyzer through sufficient attenuation.

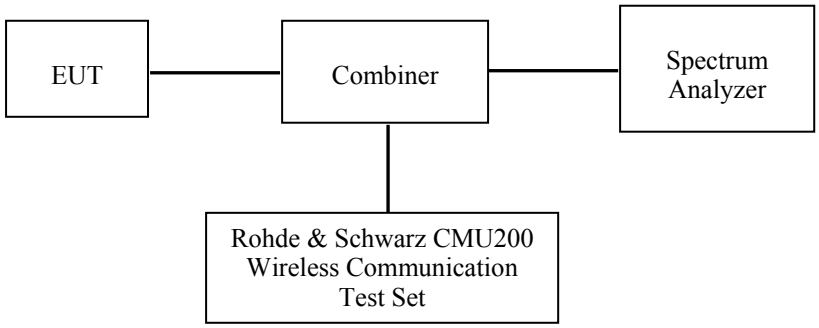

Test Equipment

Manufacturer	Equipment Description	Model No.	Serial No.	Calibration Date
Rohde & Schwarz	Communication Tester	CMU200	1100.0008.02	2008-06-21
Rohde & Schwarz	Spectrum Analyzer	FSEM30	849720/019	2008-05-09

Test Results

Band	Frequency (MHz)	Conducted Output Power（GSM Mode）	
		(dBm)	(Watt)
Cellular	824.2	32.12	1.629
	836.6	32.06	1.607
	848.8	32.09	1.618
PCS	1850.2	29.13	0.818
	1880.0	28.95	0.785
	1909.8	28.77	0.753

APPENDIX G – EUT TEST POSITION PHOTOS

1.5 cm Body-worn back Setup Photo

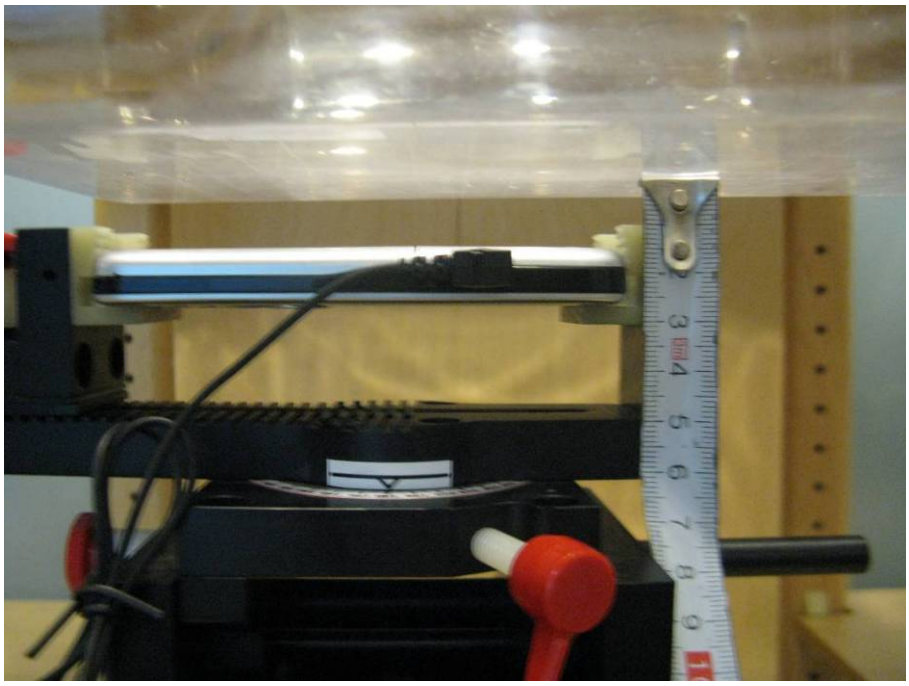

Left Head Touch Setup Photo

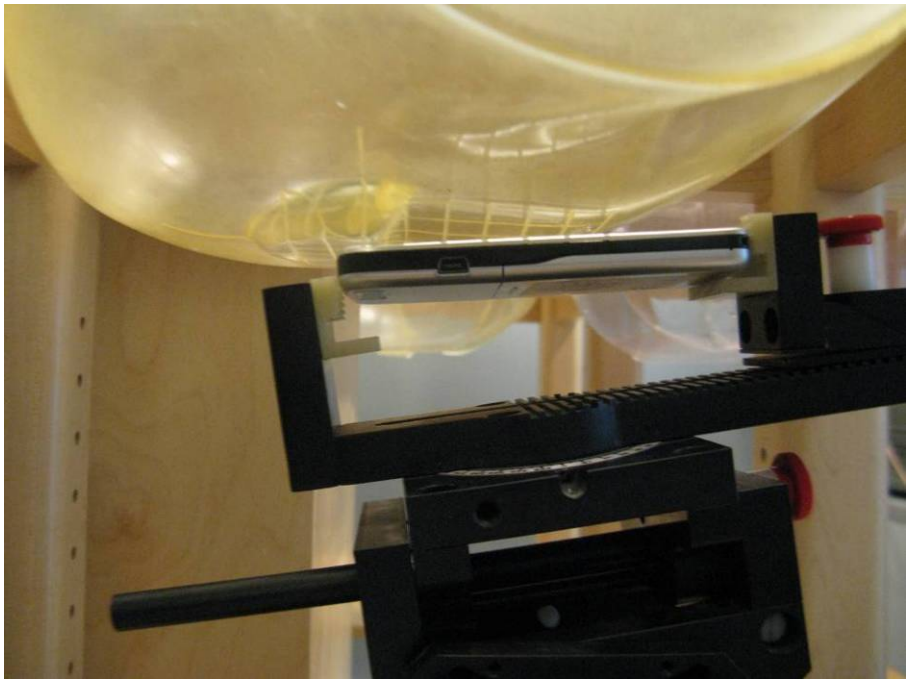

Left Head Tilt Setup Photo

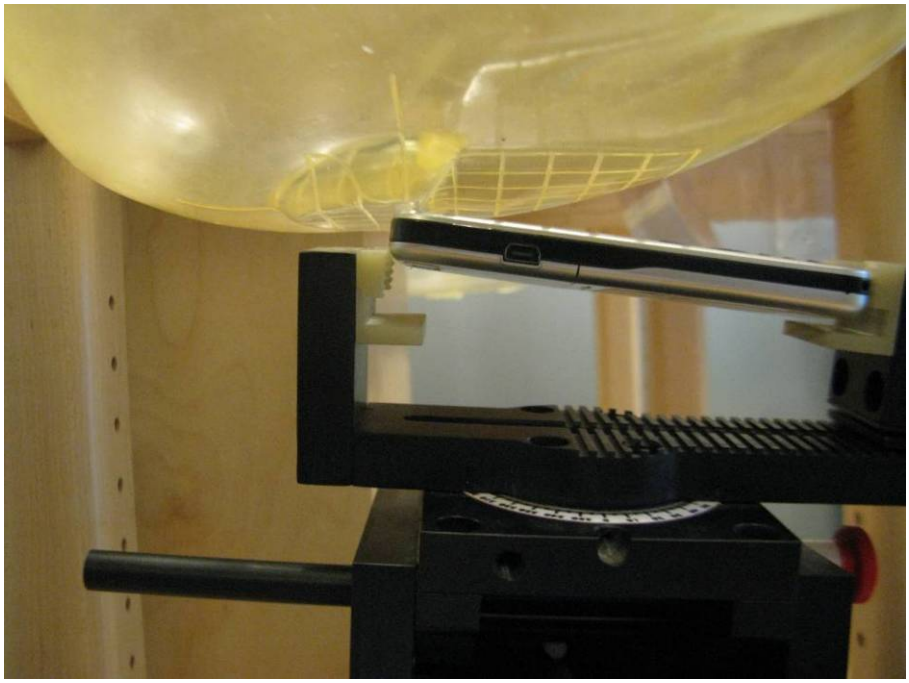

Right Head Touch Setup Photo

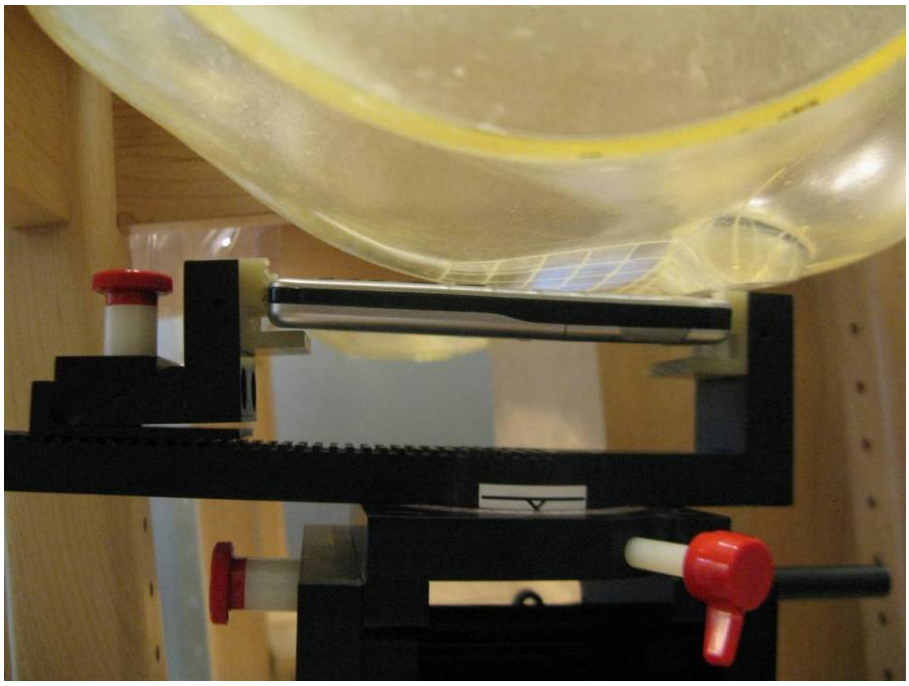

Right Head Tilt Setup Photo

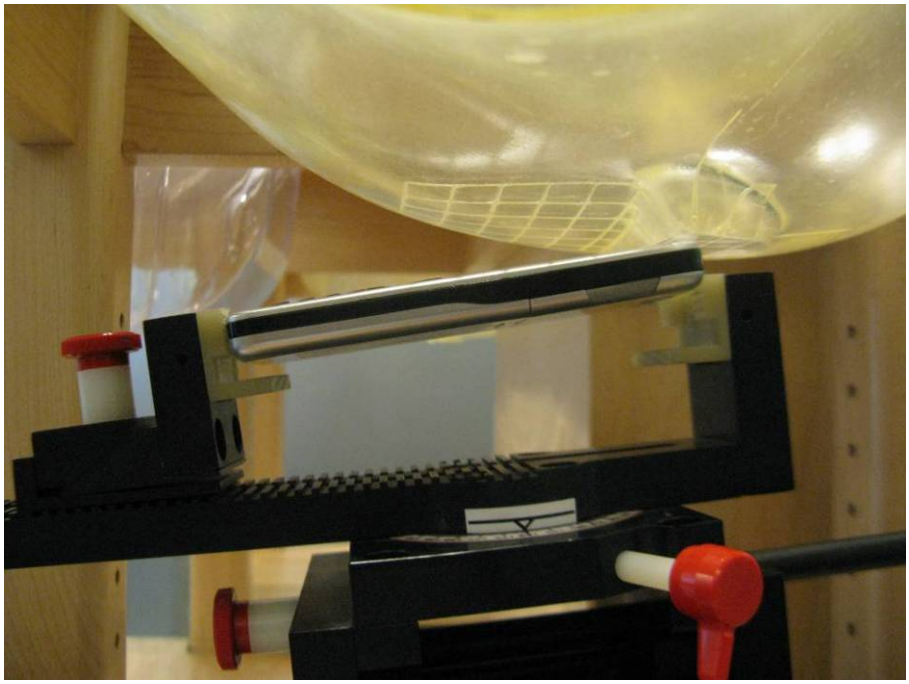

APPENDIX H – EUT PHOTOS

EUT - Top View

EUT - Bottom View

EUT- Uncovered View

EUT – Side View

EUT - Headset

APPENDIX I - INFORMATIVE REFERENCES

[1] Federal Communications Commission, \Report and order: Guidelines for evaluating the environmental effects of radiofrequency radiation", Tech. Rep. FCC 96-326, FCC, Washington, D.C. 20554, 1996.

[2] David L. Means Kwok Chan, Robert F. Cleveland, \Evaluating compliance with FCC guidelines for human exposure to radiofrequency electromagnetic fields", Tech. Rep., Federal Communication Commission, O_ce of Engineering & Technology, Washington, DC, 1997.

[3] Thomas Schmid, Oliver Egger, and Niels Kuster, \Automated E-_eld scanning system for dosimetric
assessments", IEEE Transactions on Microwave Theory and Techniques, vol. 44, pp. 105{113, Jan. 1996.

[4] Niels Kuster, Ralph K.astle, and Thomas Schmid, \Dosimetric evaluation of mobile communications
equipment with known precision", IEICE Transactions on Communications, vol. E80-B, no. 5, pp. 645{652, May 1997.

[5] CENELEC, \Considerations for evaluating of human exposure to electromagnetic fields (EMFs) from mobile telecommunication equipment (MTE) in the frequency range 30MHz - 6GHz", Tech. Rep., CENELEC, European Committee for Electrotechnical Standardization, Brussels, 1997.

[6] ANSI, ANSI/IEEE C95.1-1992: IEEE Standard for Safety Levels with Respect to Human Exposure to Radio Frequency Electromagnetic Fields, 3 kHz to 300 GHz, The Institute of Electrical and Electronics Engineers, Inc., New York, NY 10017, 1992.

[7] Katja Pokovic, Thomas Schmid, and Niels Kuster, \Robust setup for precise calibration of E-field probes in tissue simulating liquids at mobile communications frequencies", in ICECOM _ 97, Dubrovnik, October 15{17, 1997, pp. 120-24.

[8] Katja Pokovic, Thomas Schmid, and Niels Kuster, \E-field probe with improved isotropy in brain simulating liquids", in Proceedings of the ELMAR, Zadar, Croatia, 23{25 June, 1996, pp. 172-175.

[9] Volker Hombach, Klaus Meier, Michael Burkhardt, Eberhard K. uhn, and Niels Kuster, \The depen-dence of EM energy absorption upon human head modeling at 900 MHz", IEEE Transactions on Microwave Theory and Techniques, vol. 44, no. 10, pp. 1865-1873, Oct. 1996.

[10] Klaus Meier, Ralf Kastle, Volker Hombach, Roger Tay, and Niels Kuster, \The dependence of EM energy absorption upon human head modeling at 1800 MHz", IEEE Transactions on Microwave Theory and Techniques, Oct. 1997, in press.

[11] W. Gander, Computermathematik, Birkhaeuser, Basel, 1992.

[12] W. H. Press, S. A. Teukolsky,W. T. Vetterling, and B. P. Flannery, Numerical Recepies in C, The Art of Scientific Computing, Second Edition, Cambridge University Press, 1992.Dosimetric Evaluation of Sample device, month 1998 9

[13] NIS81 NAMAS, \The treatment of uncertainity in EMC measurement", Tech. Rep., NAMAS Executive, National Physical Laboratory, Teddington, Middlesex, England, 1994.

[14] Barry N. Taylor and Christ E. Kuyatt, \Guidelines for evaluating and expressing the uncertainty of NIST measurement results", Tech. Rep., National Institute of Standards and Technology, 1994. Dosimetric Evaluation of Sample device, month 1998 10.

******* END OF REPORT *******