



Annex A Test set-up photographs

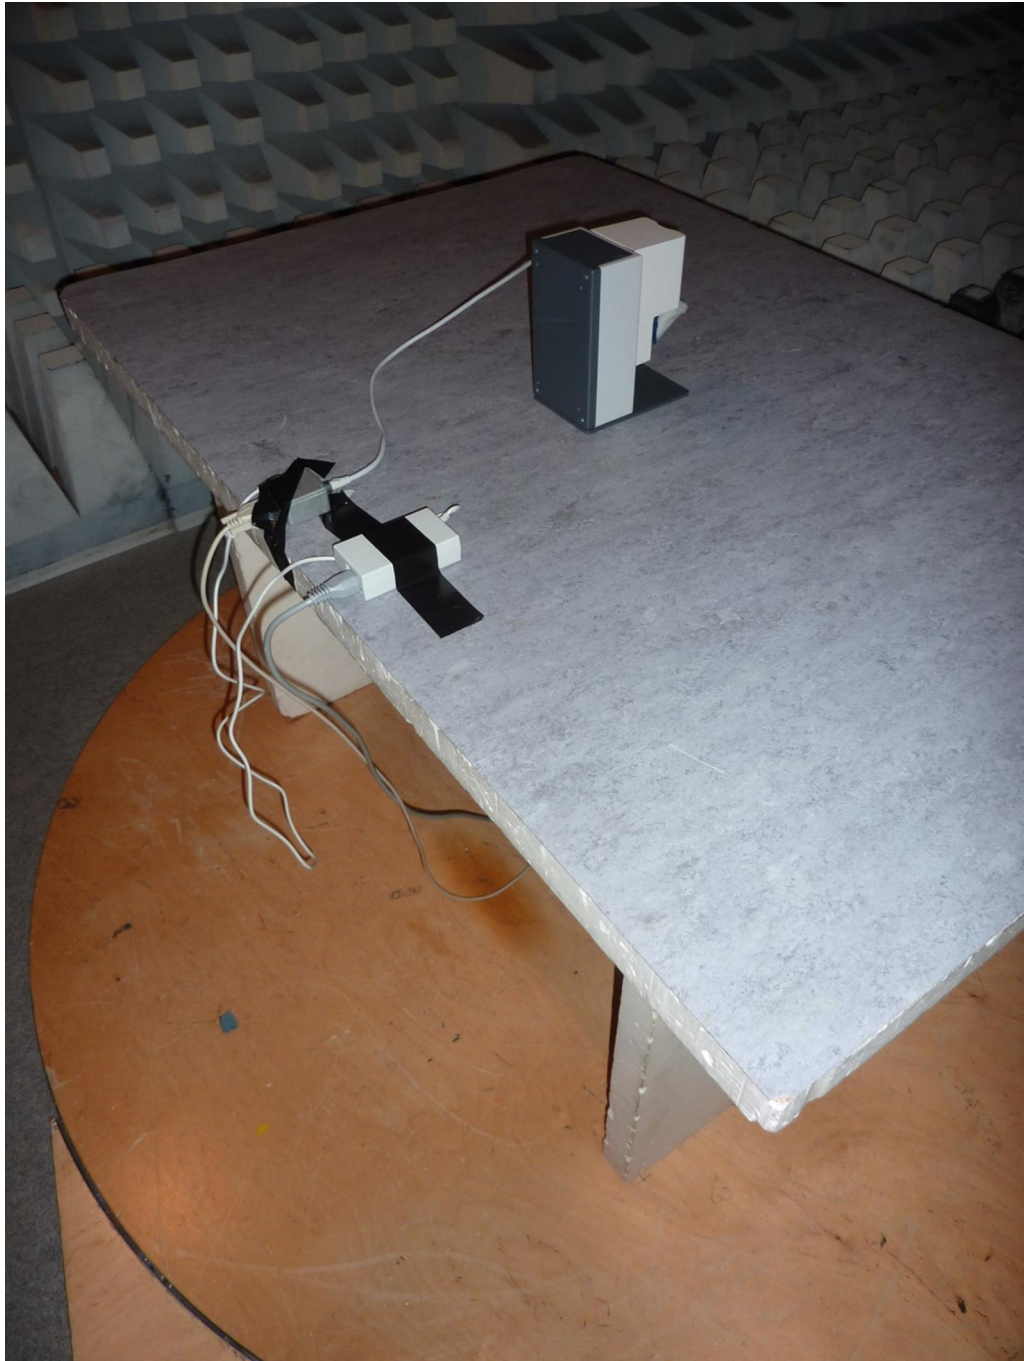


182314_g.jpg: dosing module, test setup fully anechoic chamber

Annex A Test set-up photographs

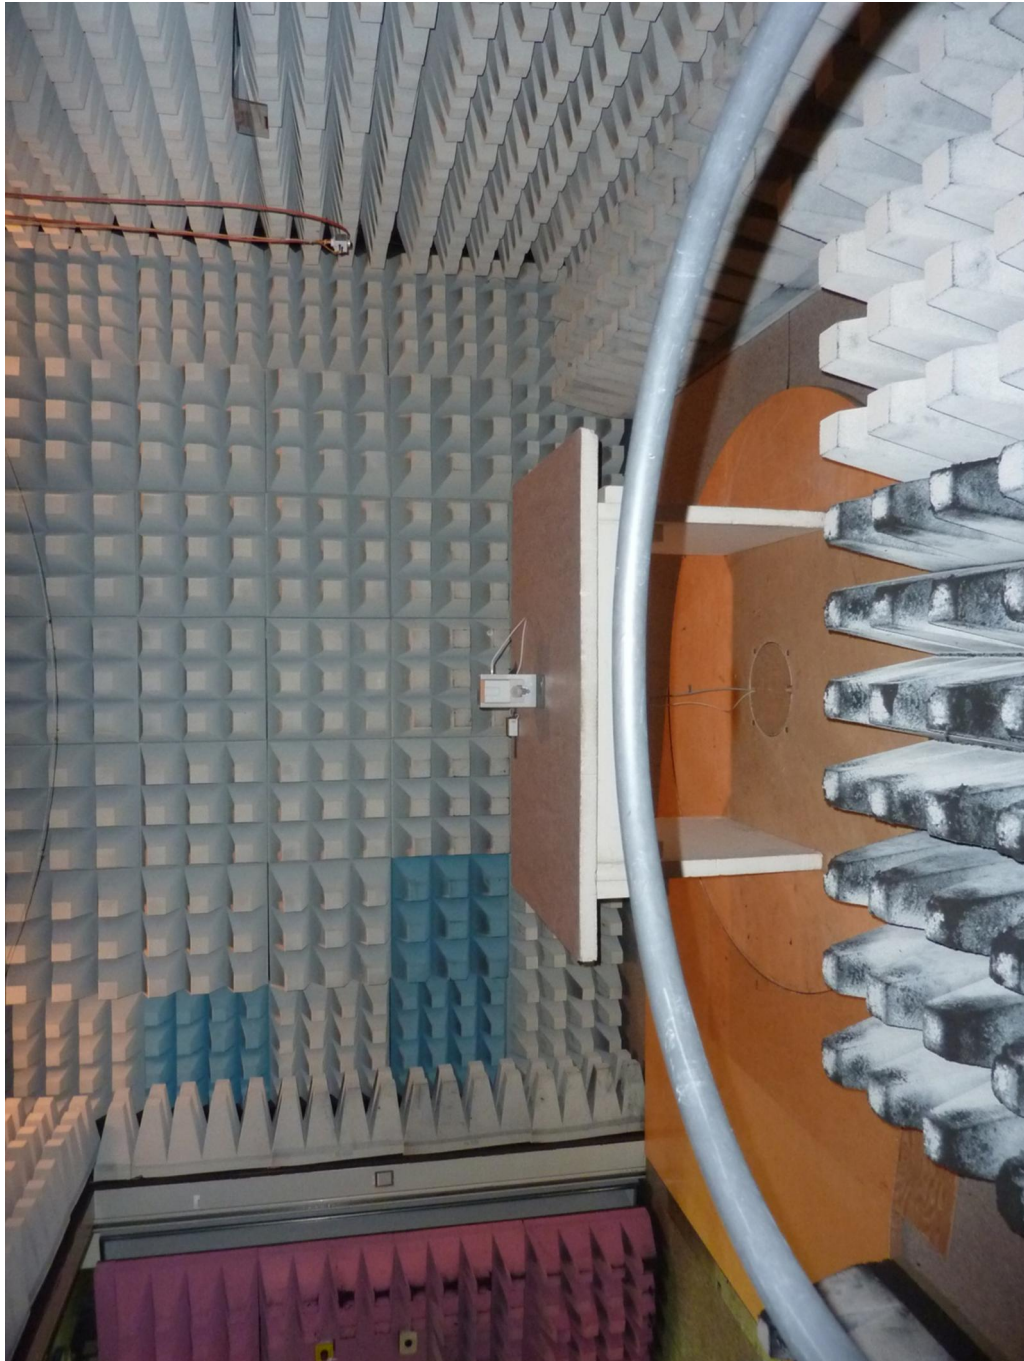

182314_i.jpg: dosing module, test setup fully anechoic chamber

Annex A Test set-up photographs

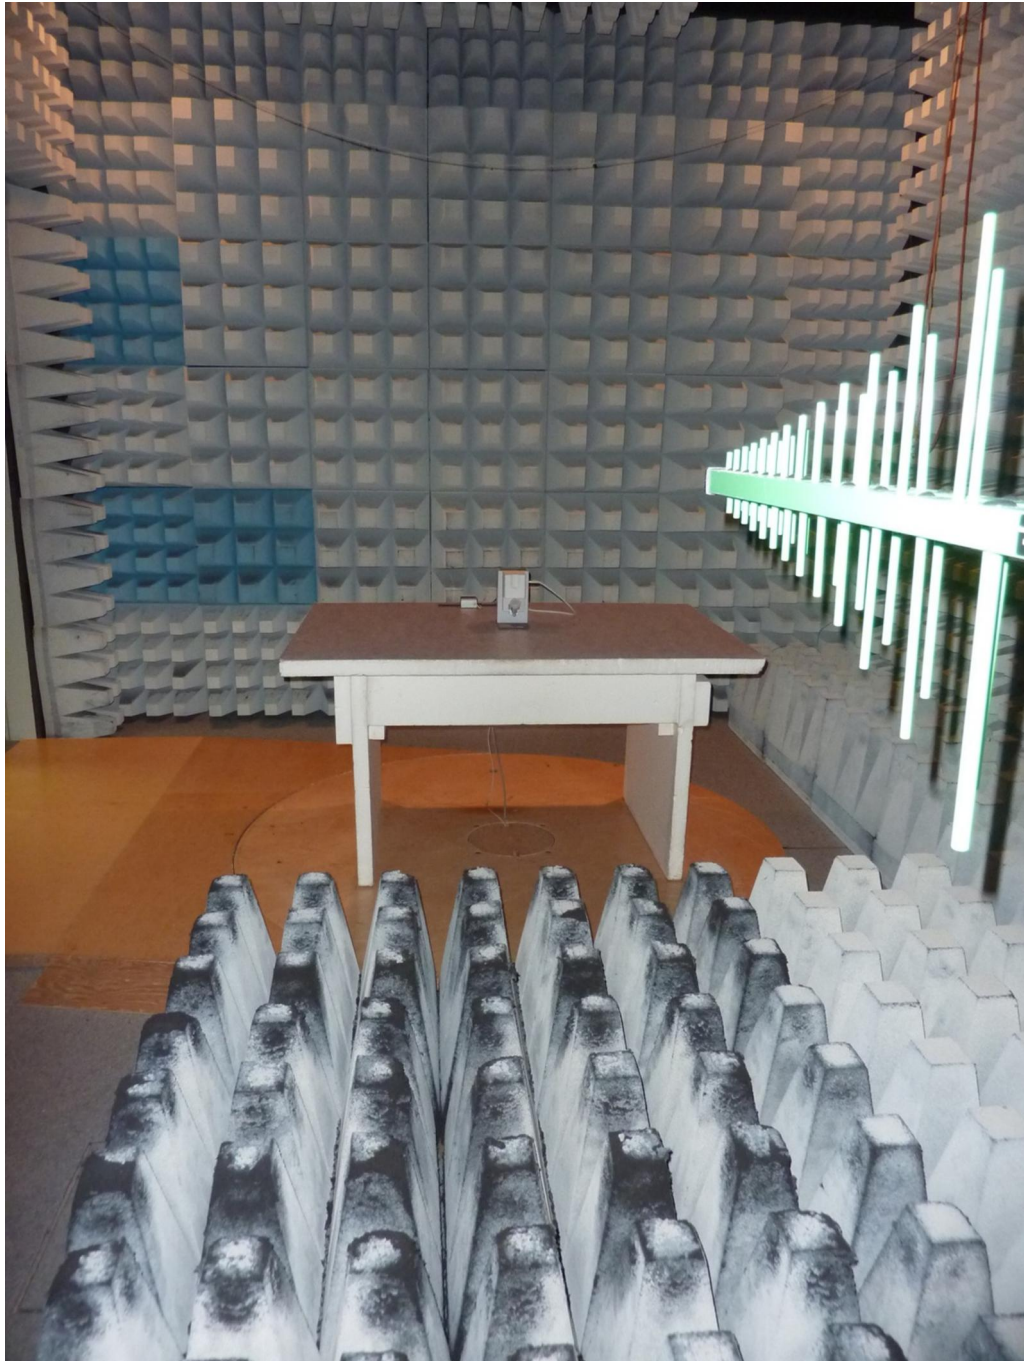


182314_h.jpg: dosing module, test setup fully anechoic chamber

Annex A Test set-up photographs



182314_l.jpg: dosing module, test setup outdoor test site

Annex A Test set-up photographs

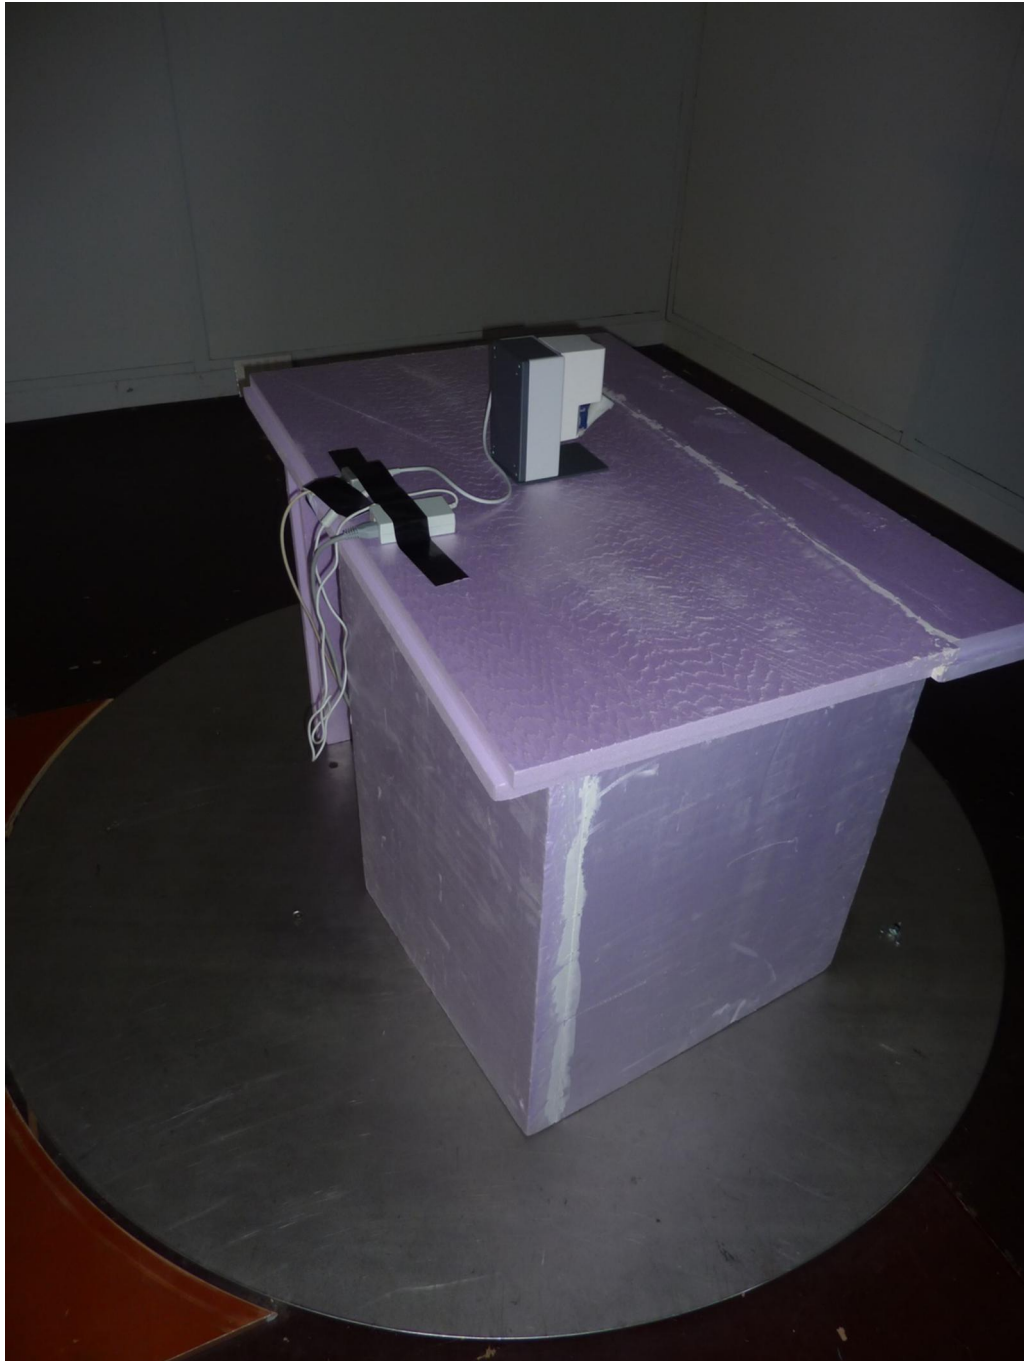

182314_n.jpg: dosing module, test setup open area test site

Annex A Test set-up photographs



182314_q.jpg: dosing module, test setup shielded chamber