

Appendix

Photographs of Test Setup

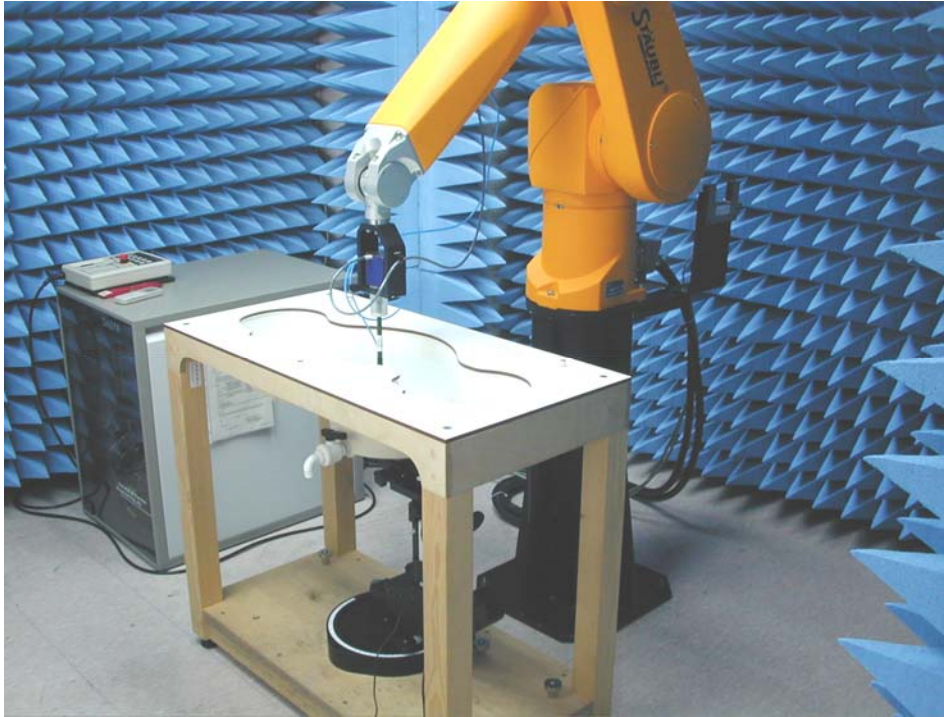


Fig.1 Photograph of the SAR measurement System

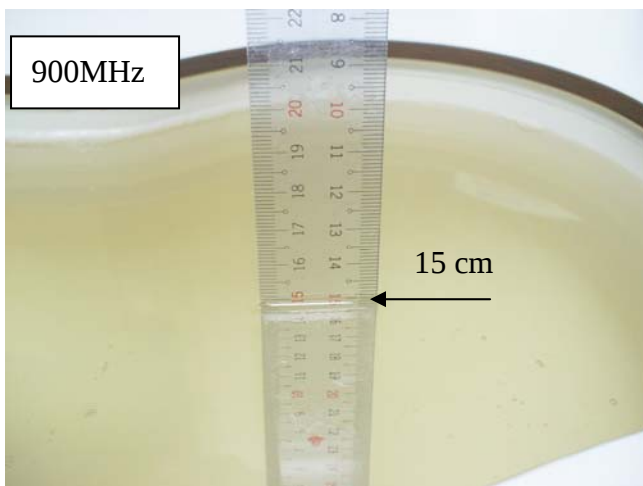


Fig.2.1 Photograph of the Tissue Simulant Fluid liquid depth 15cm for Left-head Side

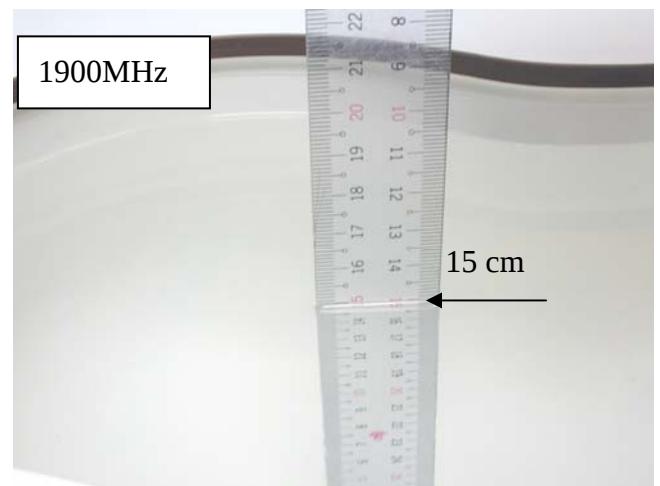


Fig.2.2 Photograph of the Tissue Simulant Fluid liquid depth 15cm for Right-head Side

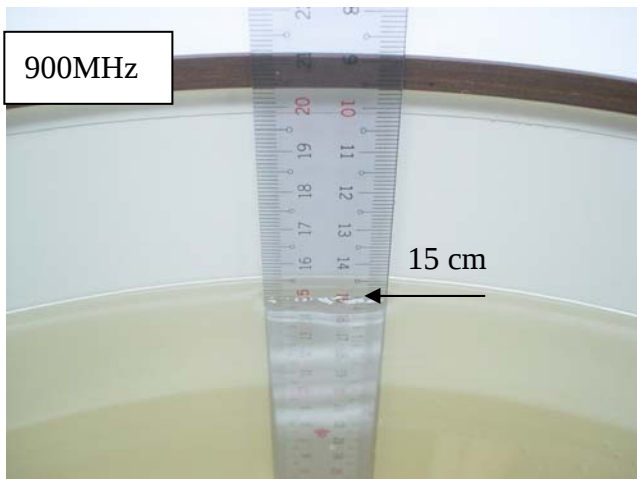


Fig.2-3 Photograph of the Tissue Simulant Fluid liquid depth 15cm for Flat (Body)

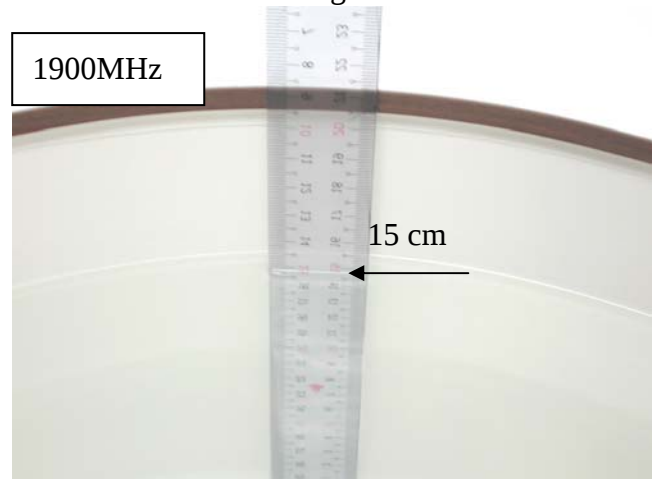


Fig.2-4 Photograph of the Tissue Simulant Fluid liquid depth 15cm for Flat (Body)

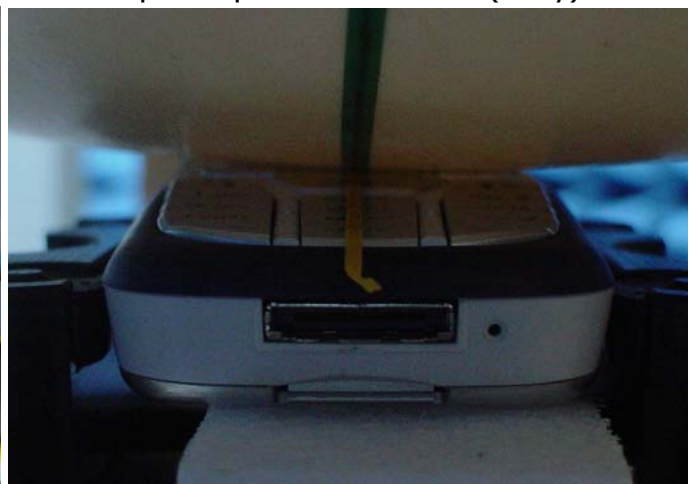
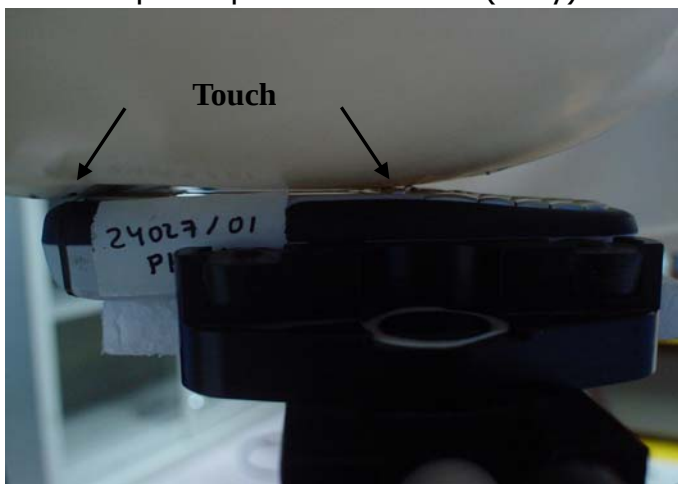


Fig.3 Right Head Section / Cheek-Touch Position

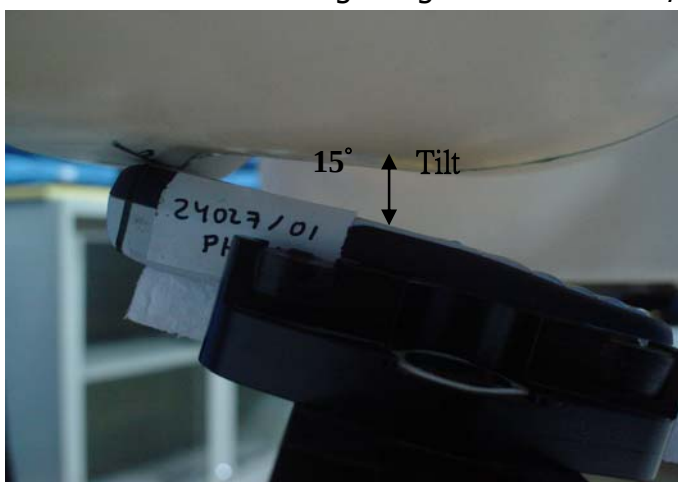


Fig.4 Right Head Section / Ear-Tilt Position(15°)

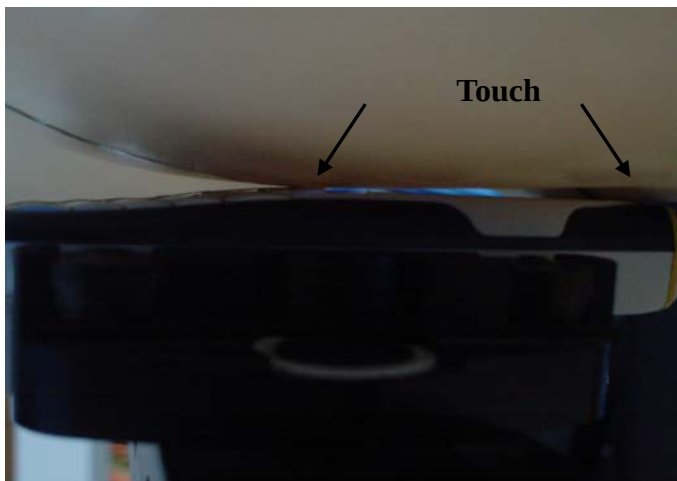


Fig.5 Left Head Section / Cheek-Touch Position

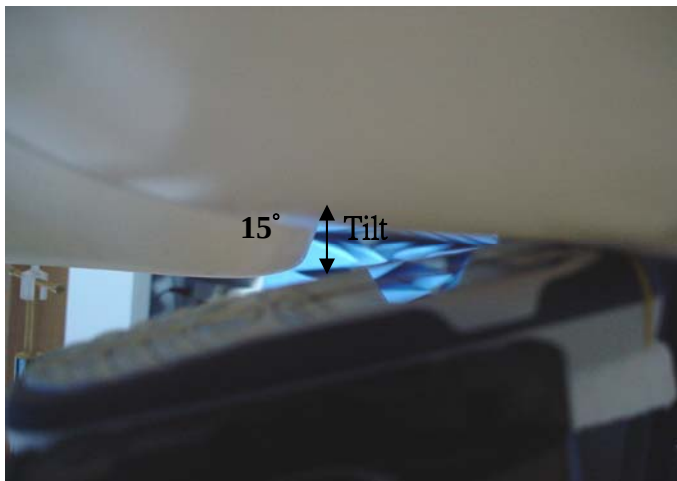


Fig.6 Left Head Section / Ear-Tilt Position(15°)

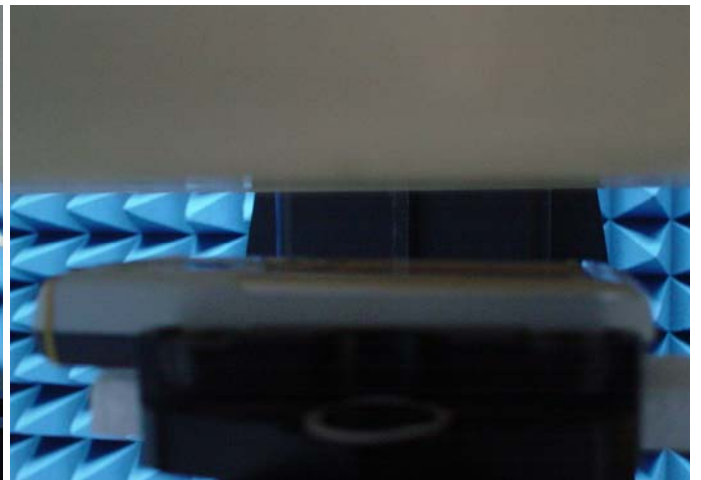
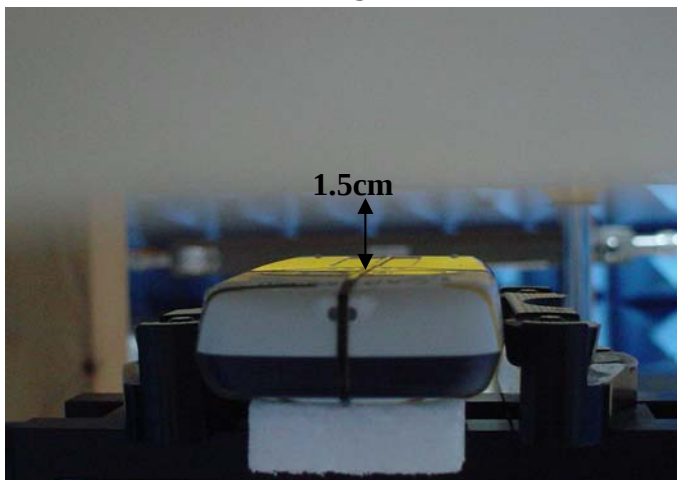


Fig.7 Body Section (test in EDGE&GPRS Mode)