

## Appendix Photographs of Test Setup



Fig.1 Photograph of the SAR measurement System

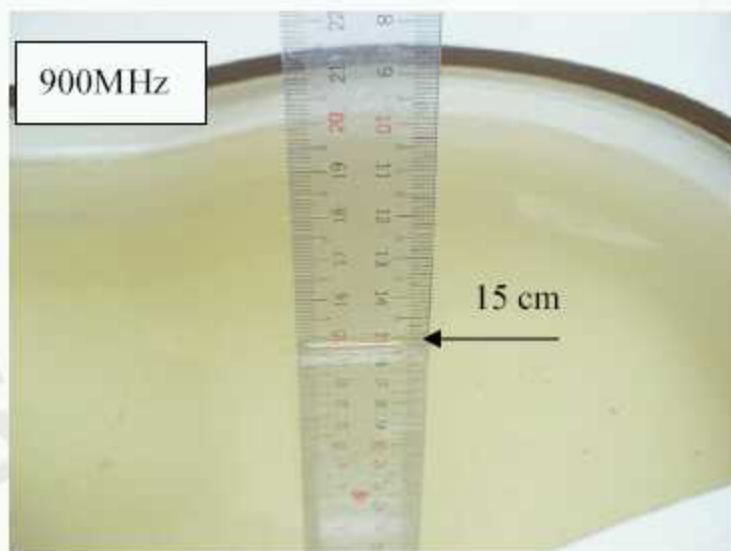


Fig.2.1 Photograph of the Tissue Simulant Fluid liquid depth 15cm for Left-head Side

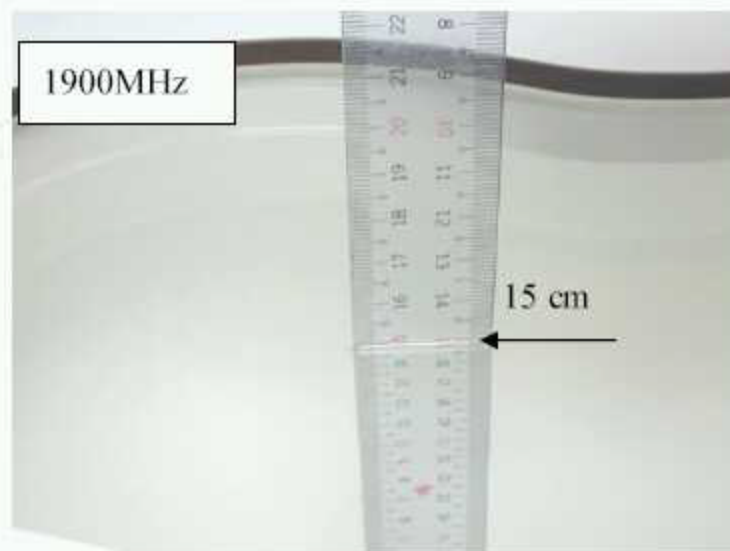


Fig.2.2 Photograph of the Tissue Simulant Fluid liquid depth 15cm for Right-head Side

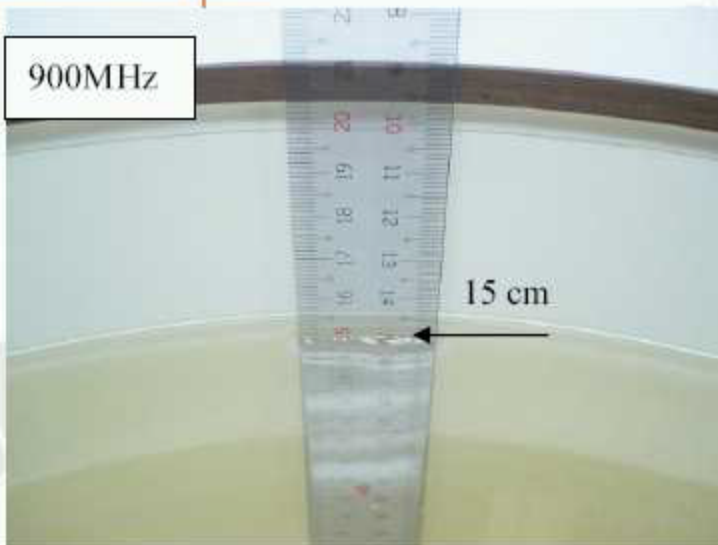


Fig.2.3 Photograph of the Tissue Simulant Fluid liquid depth 15cm for Flat (Body)

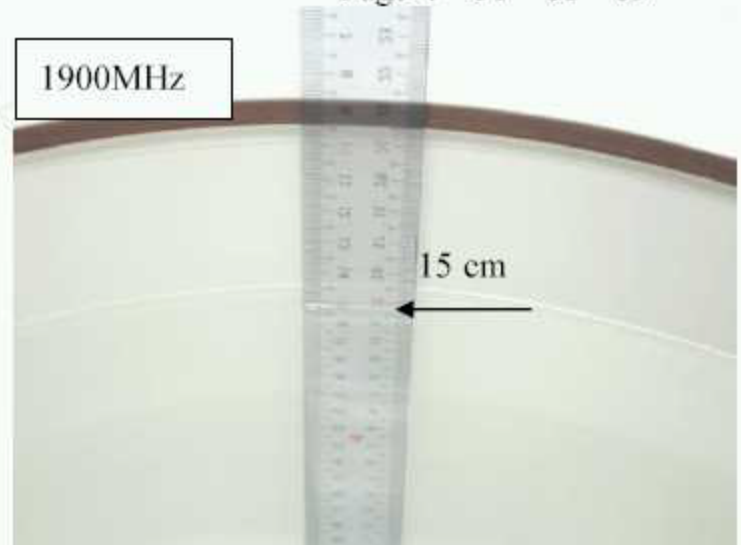


Fig.2.4 Photograph of the Tissue Simulant Fluid liquid depth 15cm for Flat (Body)

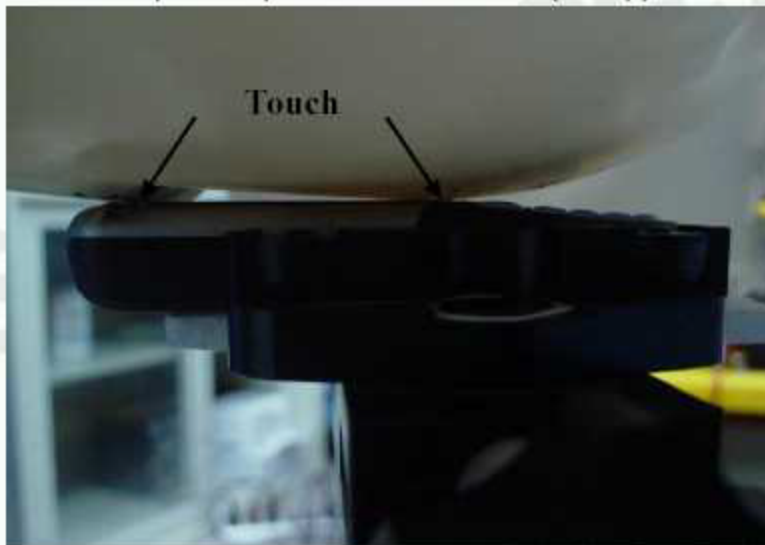


Fig.3 Right Head Section / Cheek-Touch Position

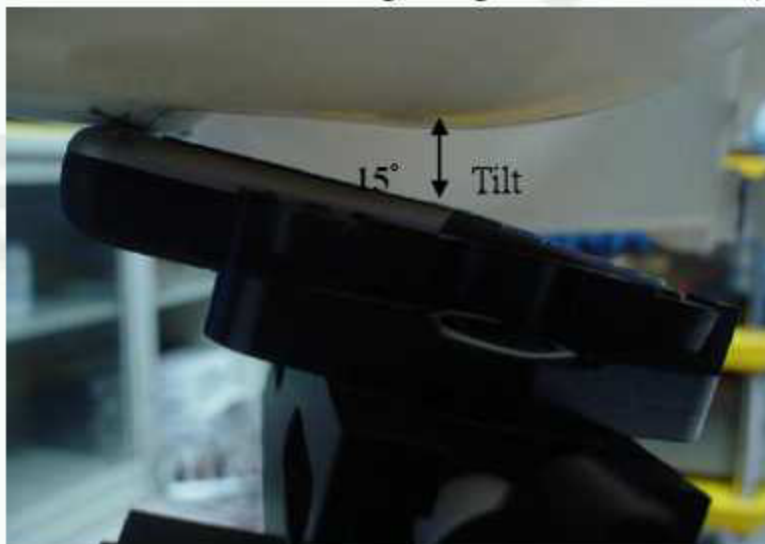


Fig.4 Right Head Section / Ear-Tilt Position(15°)



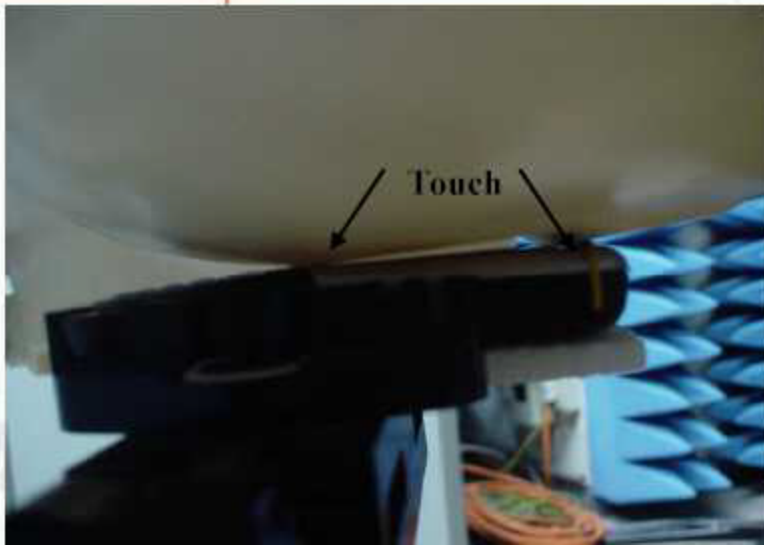


Fig.5 Left Head Section / Cheek-Touch Position



Fig.6 Left Head Section / Ear-Tilt Position(15°)

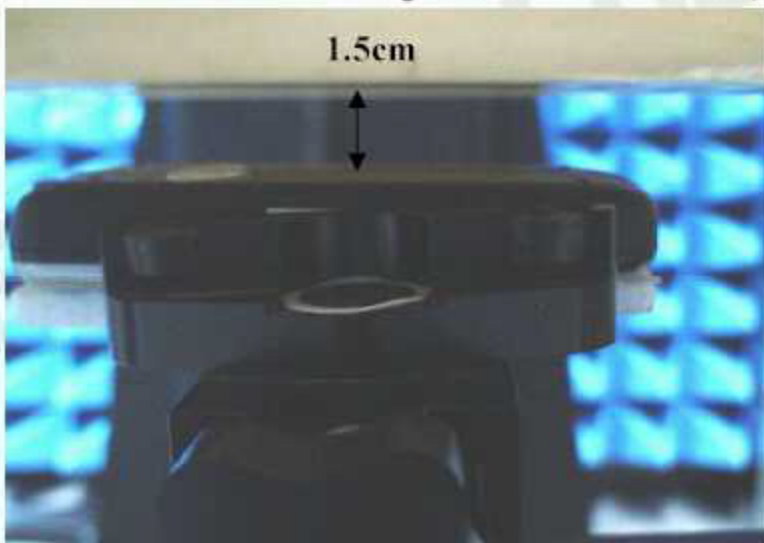


Fig.7 Body Section (test in EDGE&GPRS Mode)