

Appendix Photographs of Test Setup

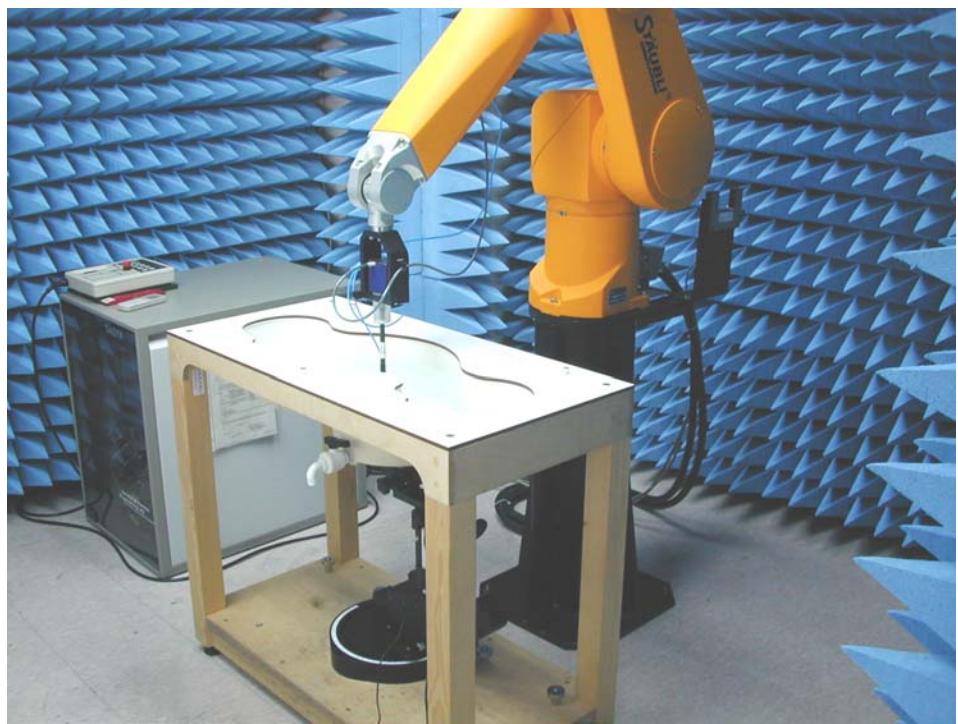


Fig.1 Photograph of the SAR measurement System

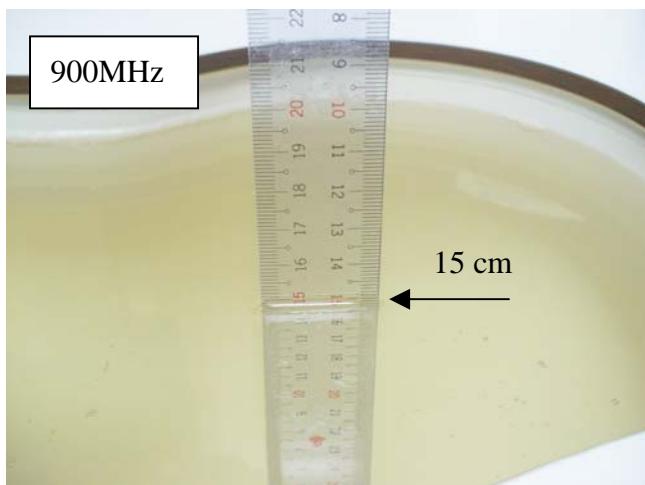


Fig.2.1 Photograph of the Tissue Simulant Fluid liquid depth 15cm for Left-head Side

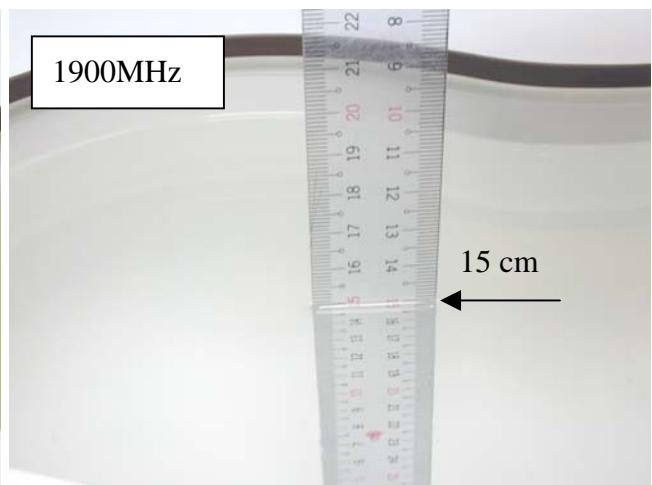


Fig.2.2 Photograph of the Tissue Simulant Fluid liquid depth 15cm for Right-head Side

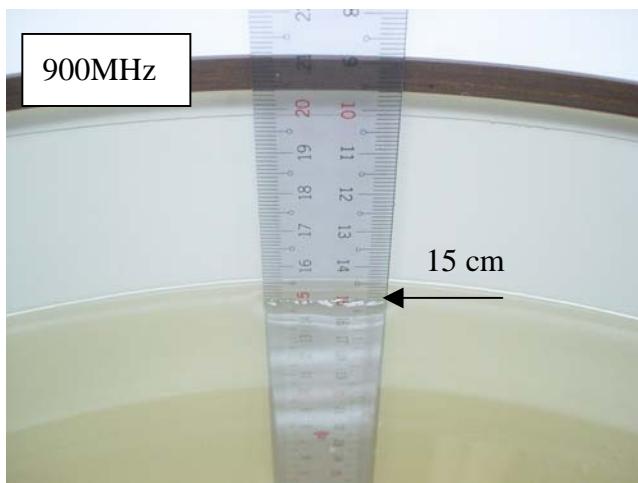


Fig.2-3 Photograph of the Tissue Simulant
Fluid liquid depth 15cm for Flat (Body)

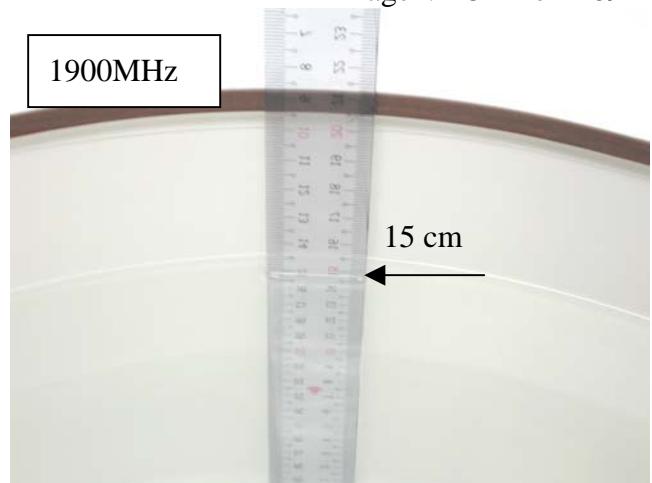


Fig.2-4 Photograph of the Tissue Simulant
Fluid liquid depth 15cm for Flat (Body)

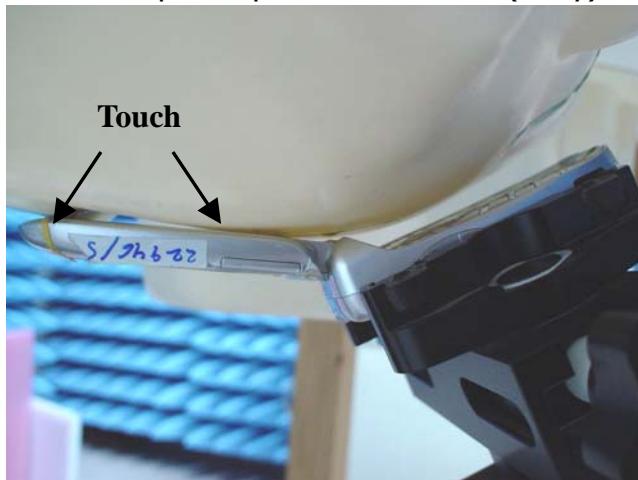


Fig.3 Right Head Section / Cheek-Touch Position

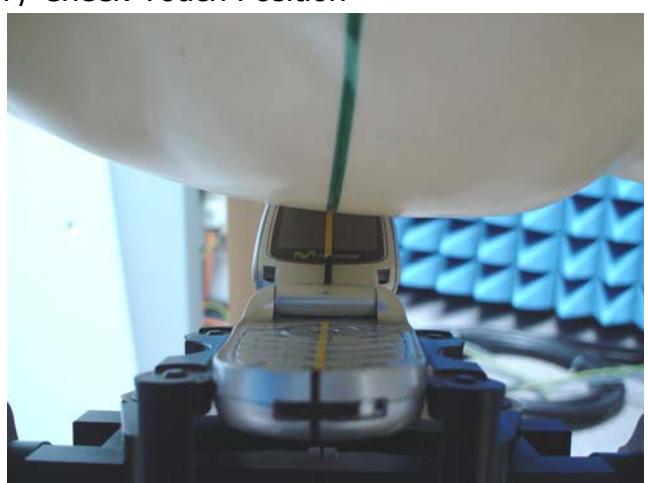
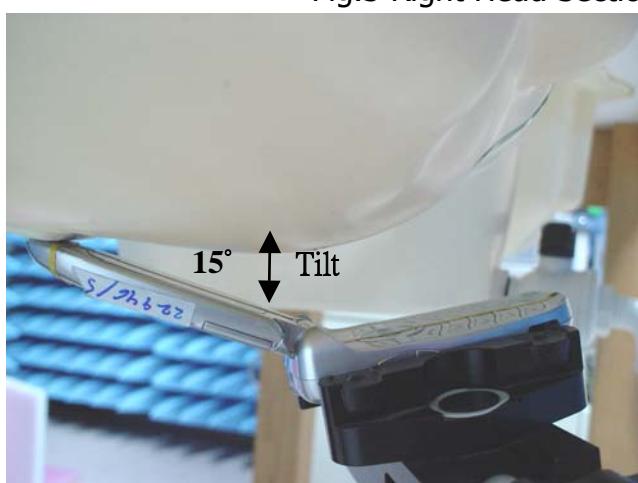


Fig.4 Right Head Section / Ear-Tilt Position(15°)

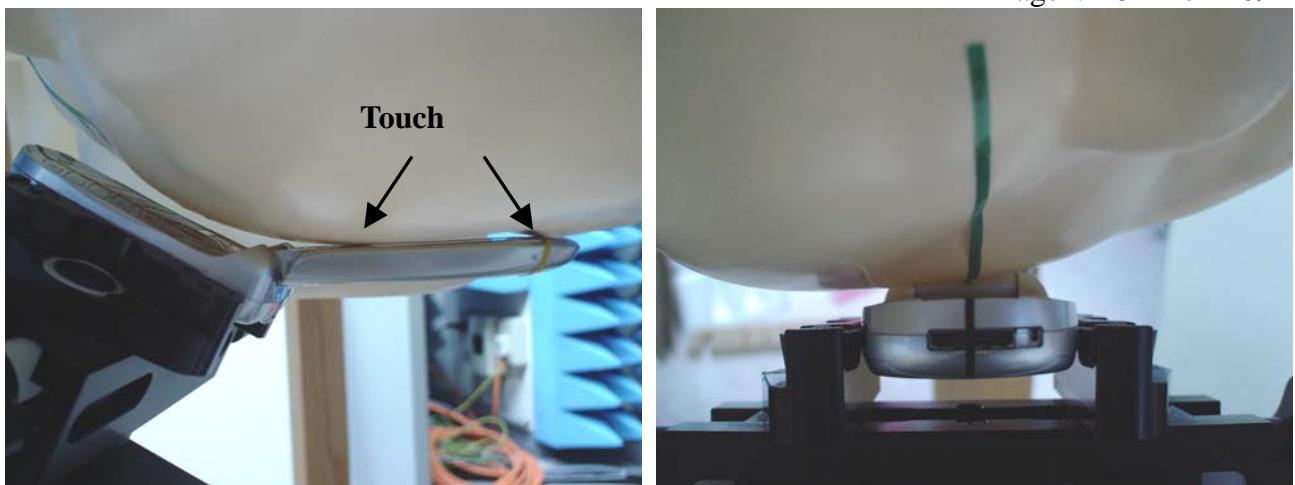


Fig.6 Left Head Section / Cheek-Touch Position

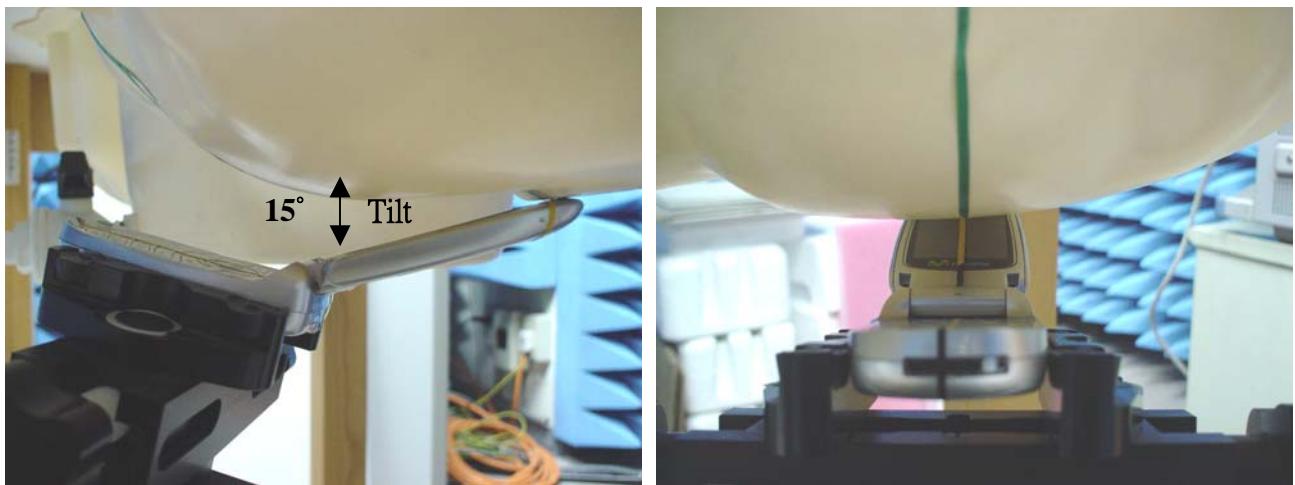


Fig.7 Left Head Section / Ear-Tilt Position(15°)



Fig.8 Body Section (Testing in GPRS Mode)

Photographs of the EUT



Fig.9 Front view of device



Fig.10 Back view of device



Fig.11 open view of device



Fig.12 Connected Charger

Photographs of the Battery



Fig.13 Front view of Battery



Fig.14 Black view of Battery